US00D1092771S

(12) **United States Design Patent**
Song et al.

(10) **Patent No.: US D1,092,771 S**
(45) **Date of Patent: ** Sep. 9, 2025**

(54) **BIOMETER BODY**

(71) Applicant: **Orange Biomed Co., Ltd**, Seoul (KR)

(72) Inventors: **Bong Kyu Song**, Seoul (KR); **Hui Gyu Kim**, Seoul (KR)

(73) Assignee: **Orange Biomed Co., Ltd**, Seoul (KR)

(**) Term: **15 Years**

(21) Appl. No.: **29/872,889**

(22) Filed: **Mar. 21, 2023**

(30) **Foreign Application Priority Data**

Oct. 11, 2022 (KR) 30-2022-0041392

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/216, 231, 232, 186, 187, 169, 107, D24/165, 167, 170, 130, 133; D10/75, D10/81
CPC A61B 5/14532; A61B 5/0002; A61M 5/1723; C12Q 1/006; G01N 33/492; G01N 33/48785; G16H 40/67
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D778,445	S	*	2/2017	Cadio	D24/169
D831,567	S	*	10/2018	Kim	D13/103
D884,903	S	*	5/2020	Cadio	D24/169
D897,536	S	*	9/2020	Mathers	D24/169
D921,904	S	*	6/2021	Cadio	D24/169
D1,004,778	S	*	11/2023	Lin	D24/169
D1,009,661	S	*	1/2024	Chang	D24/169
D1,011,533	S	*	1/2024	Xia	D24/169

FOREIGN PATENT DOCUMENTS

CN	305201608	*	6/2019
CN	307385859	*	6/2022
IN	254536	*	4/2014
KR	301132849.0000	*	10/2021

OTHER PUBLICATIONS

Rapid A1c Test Aims to Reduce Diabetes Diagnosis Inaccuracies, posted Apr. 19, 2023 [retrieved online Jan. 13, 2025]. Retrieved from internet, https://clpmag.com/disease-states/diabetes-metabolic/rapid-a1c-test-aims-to-reduce-diabetes-diagnosis-inaccuracies/ (Year: 2023).*

(Continued)

Primary Examiner — Justin M Jonaitis
Assistant Examiner — Samantha K Pollack
(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for a biometer body as shown and described.

DESCRIPTION

FIG. **1** is a perspective view of a biometer body showing our new design;
FIG. **2** is a front view thereof;
FIG. **3** is a rear view thereof;
FIG. **4** is a left side view thereof;
FIG. **5** is a right side view thereof;
FIG. **6** is a top view thereof;
FIG. **7** is a bottom view thereof;
FIG. **8** is a rear perspective view thereof; and,
FIG. **9** is a perspective view showing the biometer body in a state of use.
The broken lines shown in FIG. **9** depict portions of the biometer body that form no part of the claimed design.

1 Claim, 9 Drawing Sheets

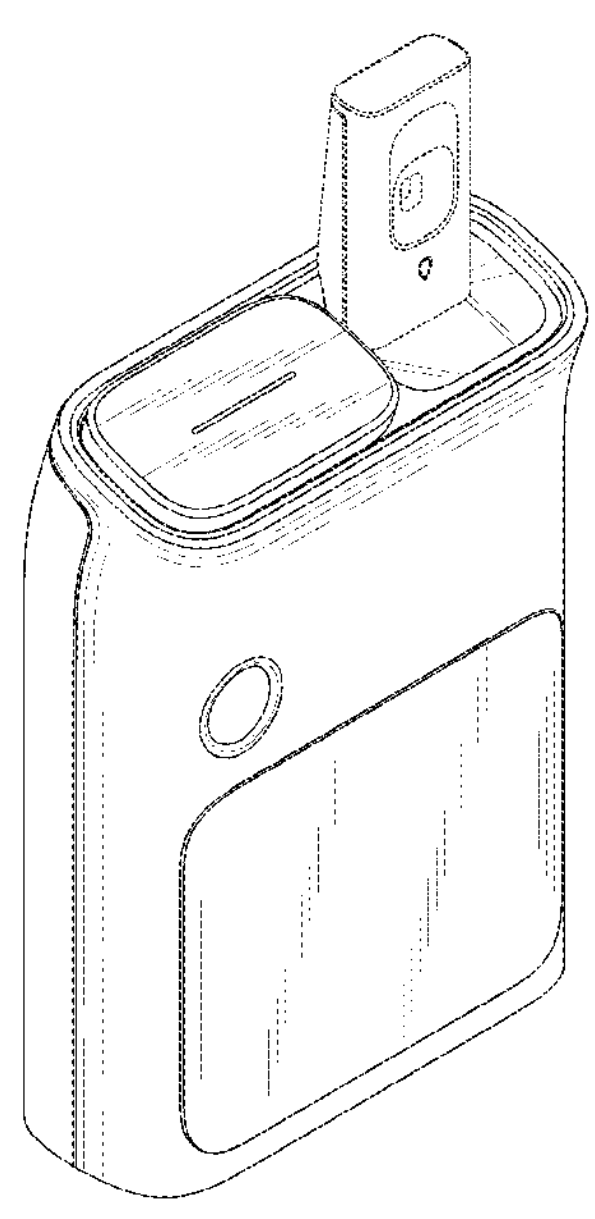

(56) **References Cited**

OTHER PUBLICATIONS

Orange Biomed | New At-Home A1C Test for Diabetes Management, posted date unavailable [retrieved online Jan. 13, 2025]. Retrieved from internet, https://orangebiomed.com (Year: 2025).*
Monitoring Your Diabetes At Home With OKRA Care Glucose Meter | OKRA Care Blog, posted Jun. 15, 2022 [retrieved online Jan. 13, 2025]. Retrieved from internet, https://okra.care/blogs/news/monitoring-your-diabetes-at-home-with-okra-care-glucose-meter (Year: 2022).*
Diabetic Outlet—FreeStyle Libre 2 Continuous Glucose Monitoring System, posted date unavailable [retrieved online Jan. 13, 2025]. Retrieved from internet, https://diabeticoutlet.com/product/freestyle-libre-2-continuous-glucose-monitoring-cgm/ (Year: 2025).*

* cited by examiner

FIG. 1

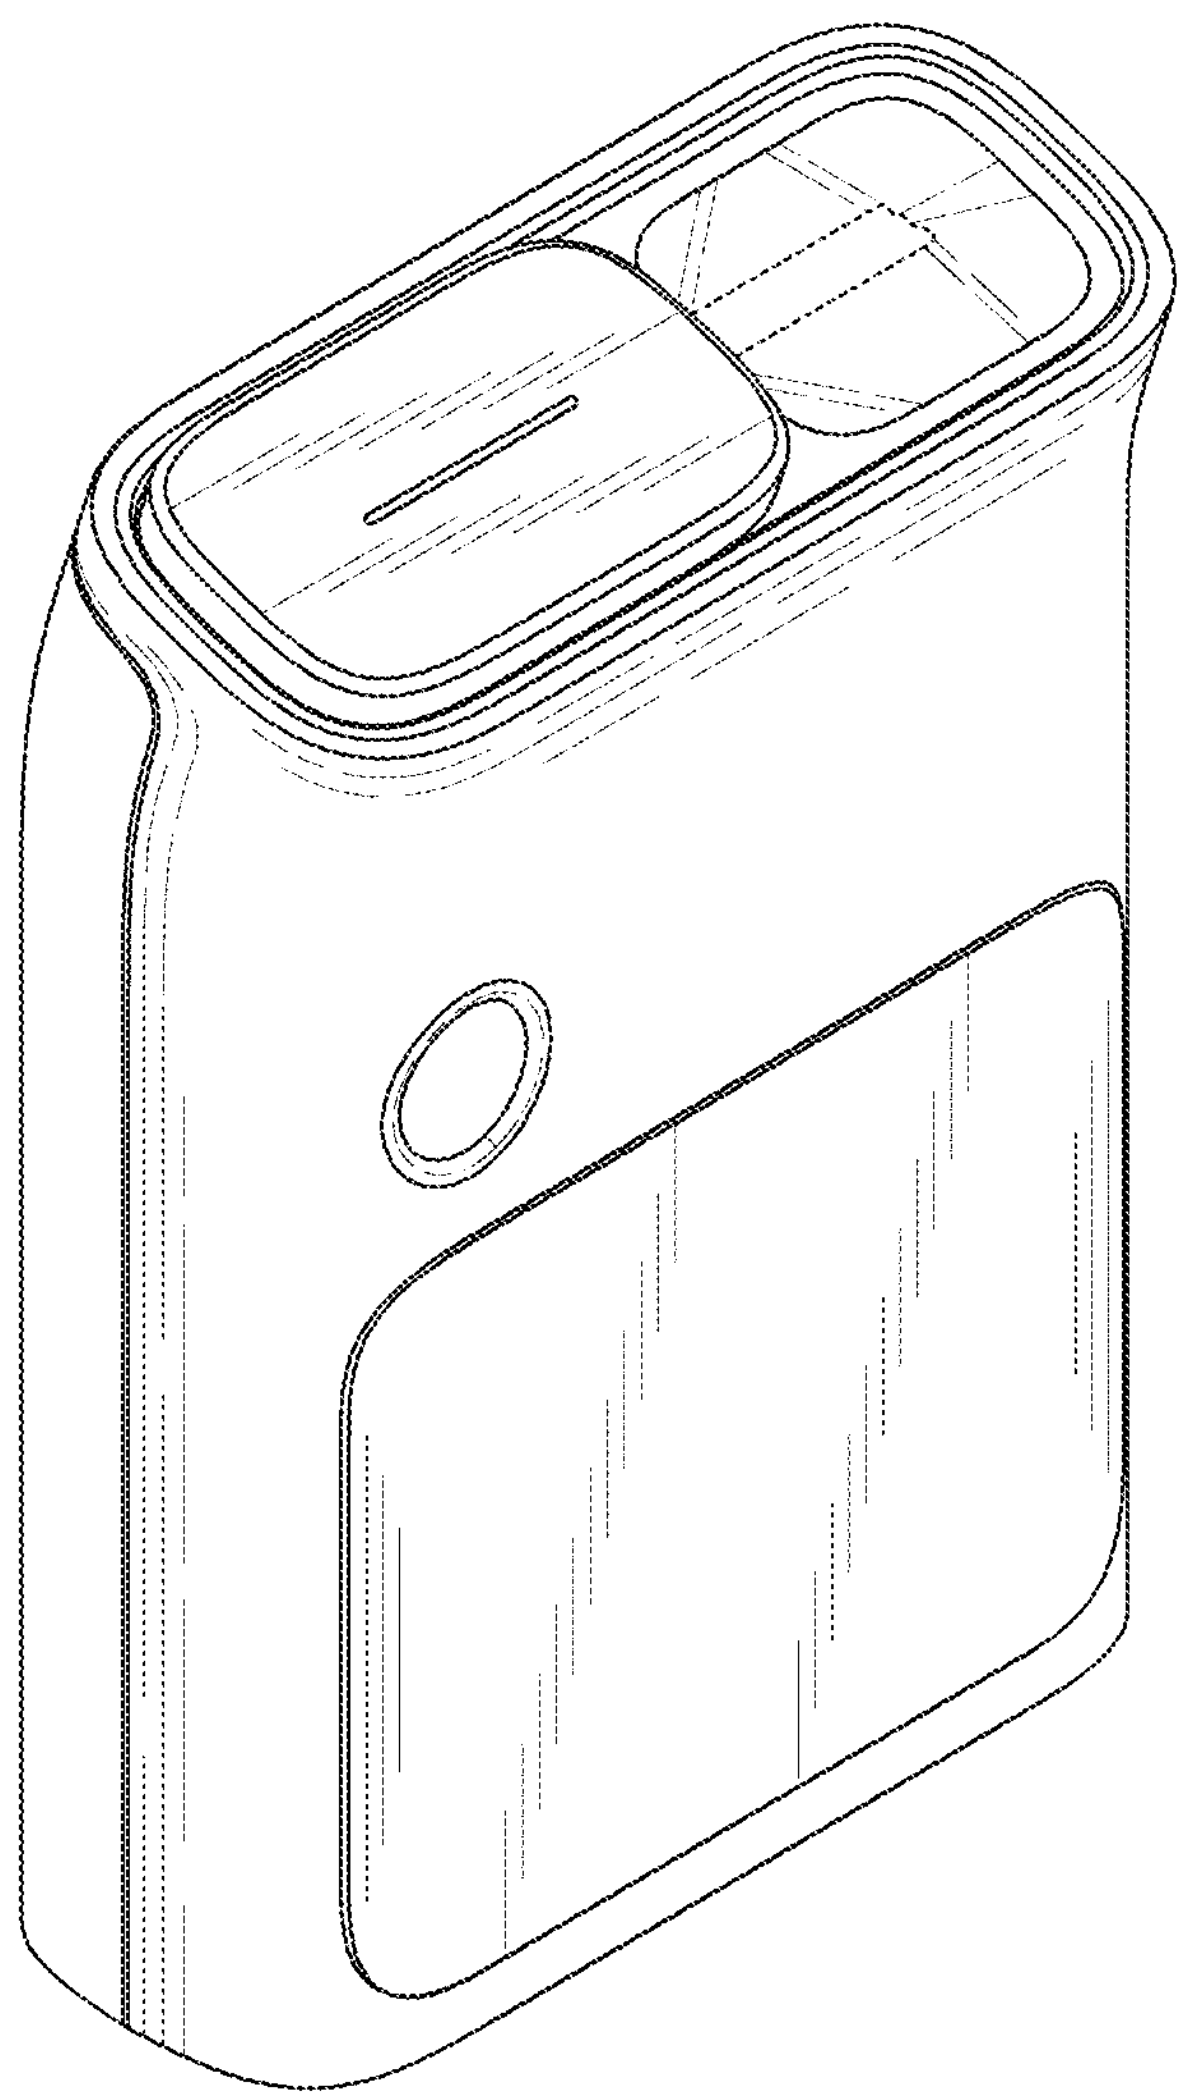

FIG. 2

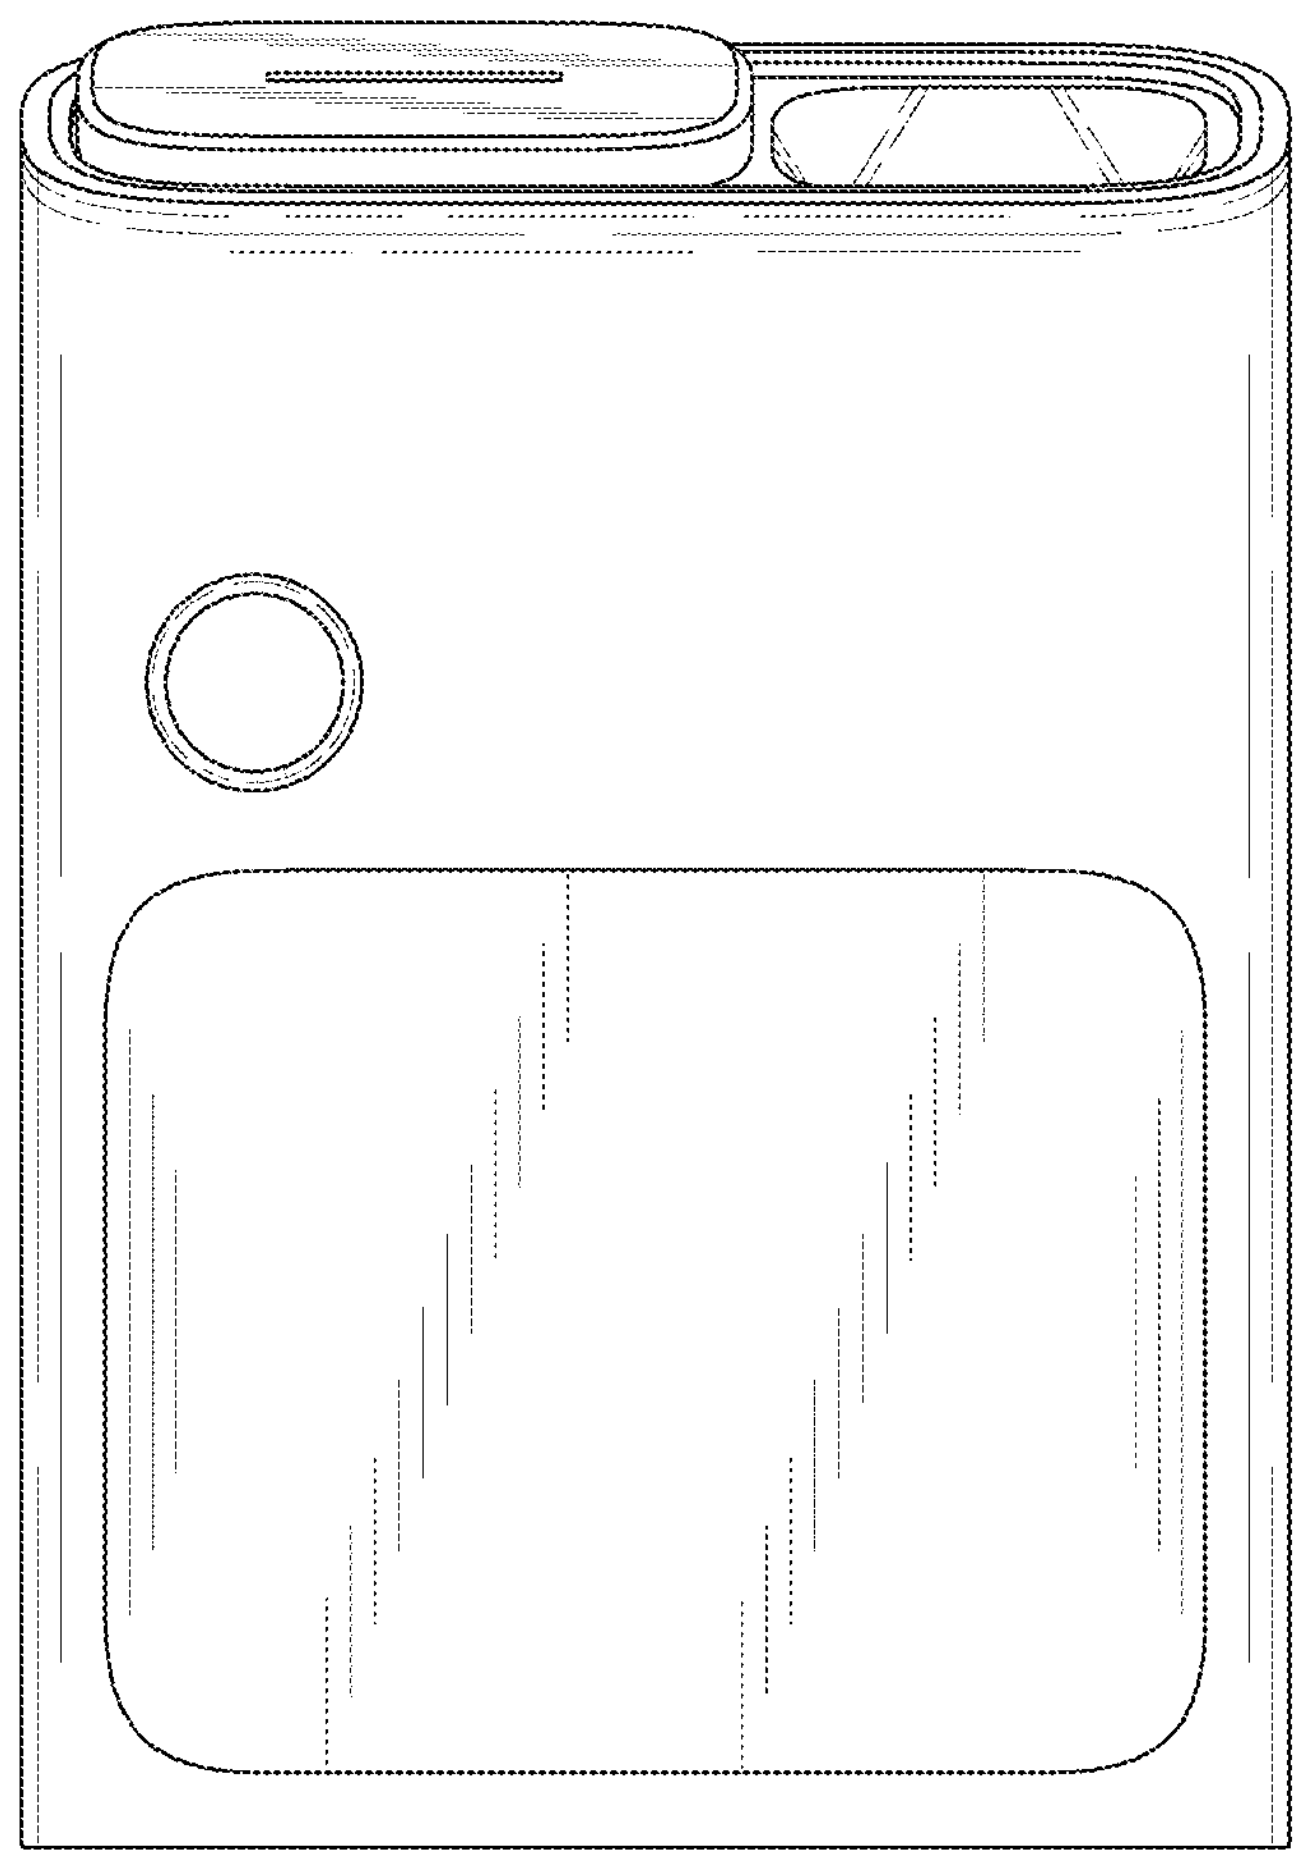

FIG. 3

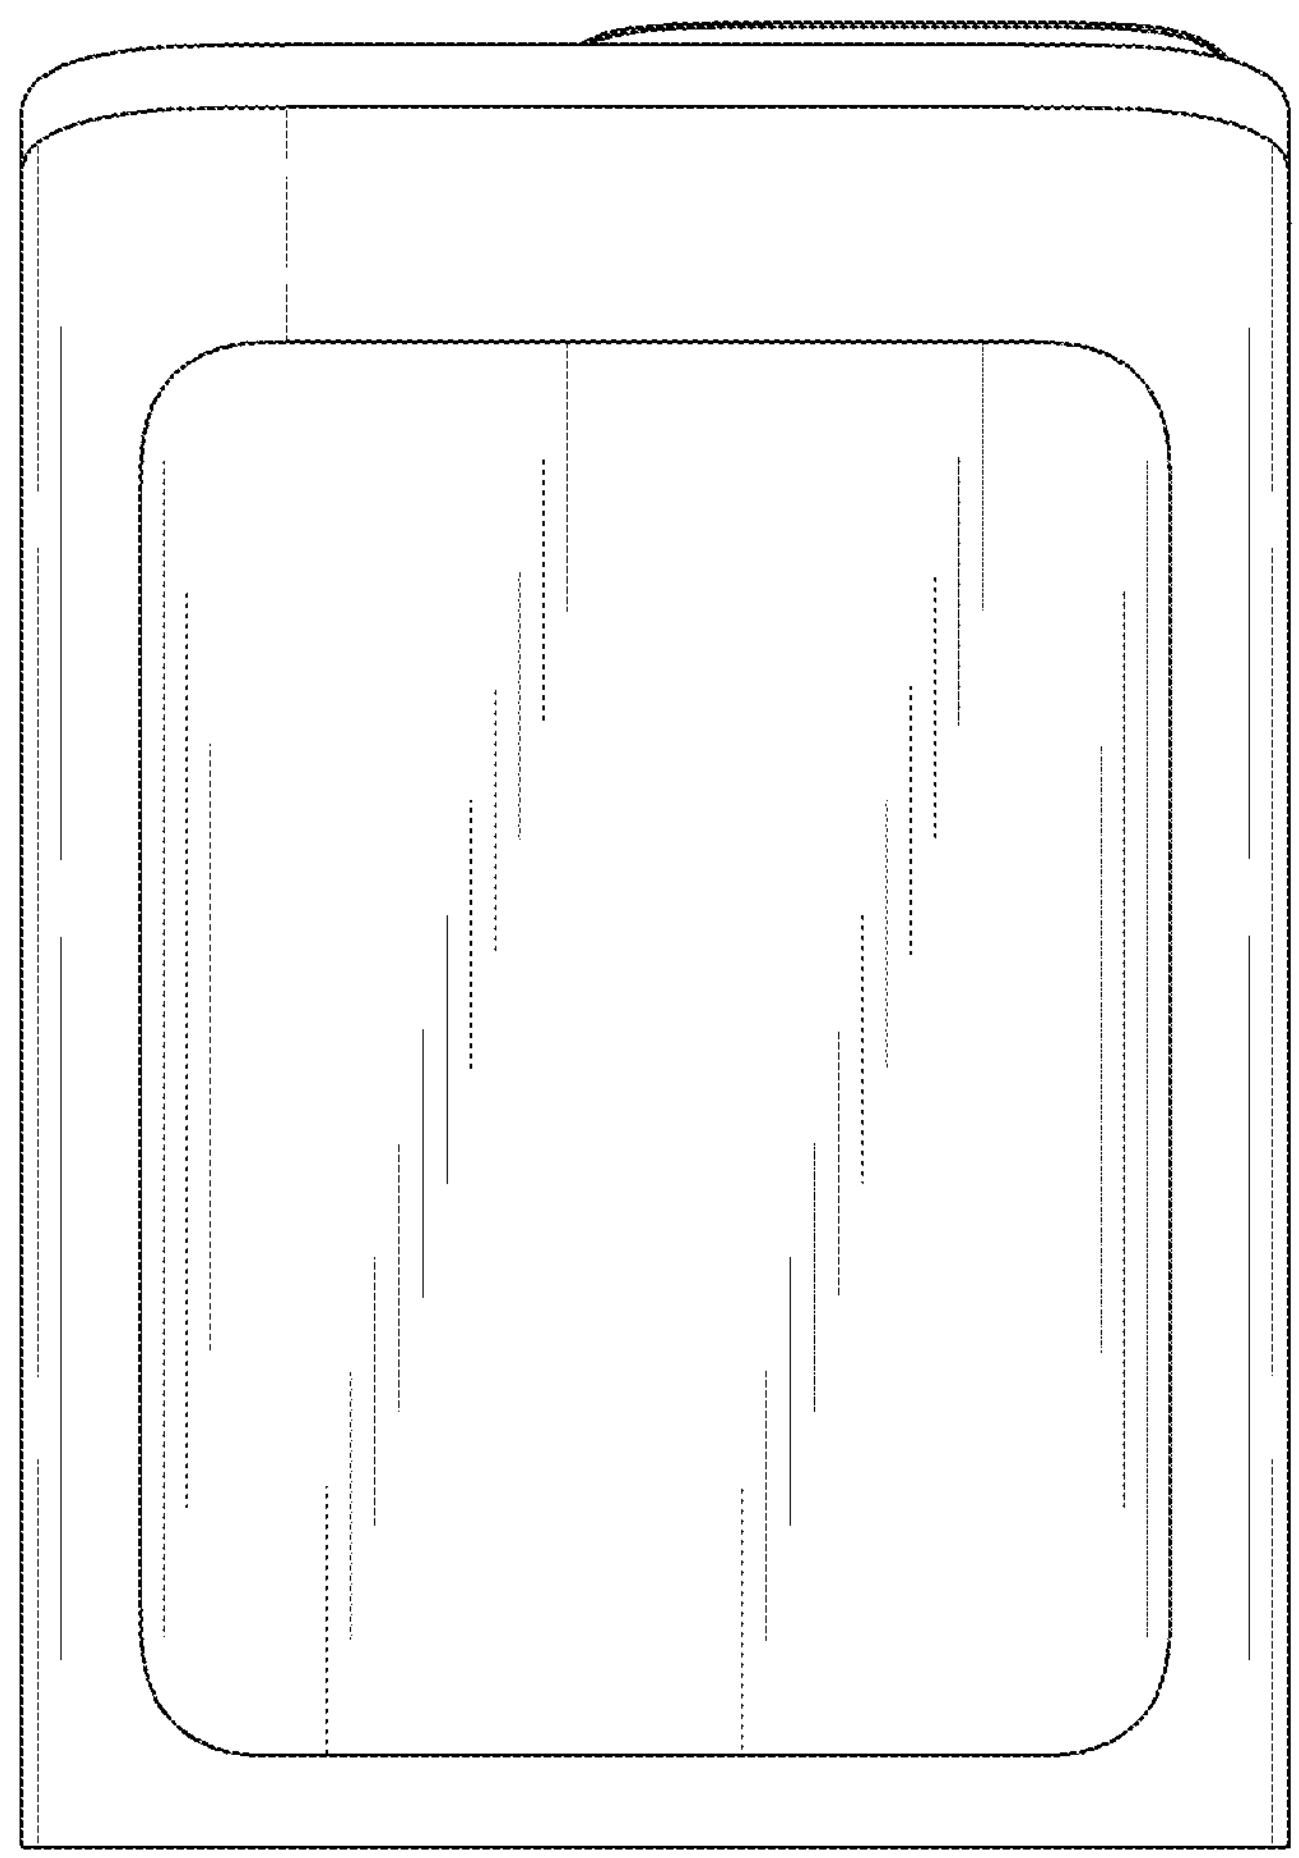

FIG. 4

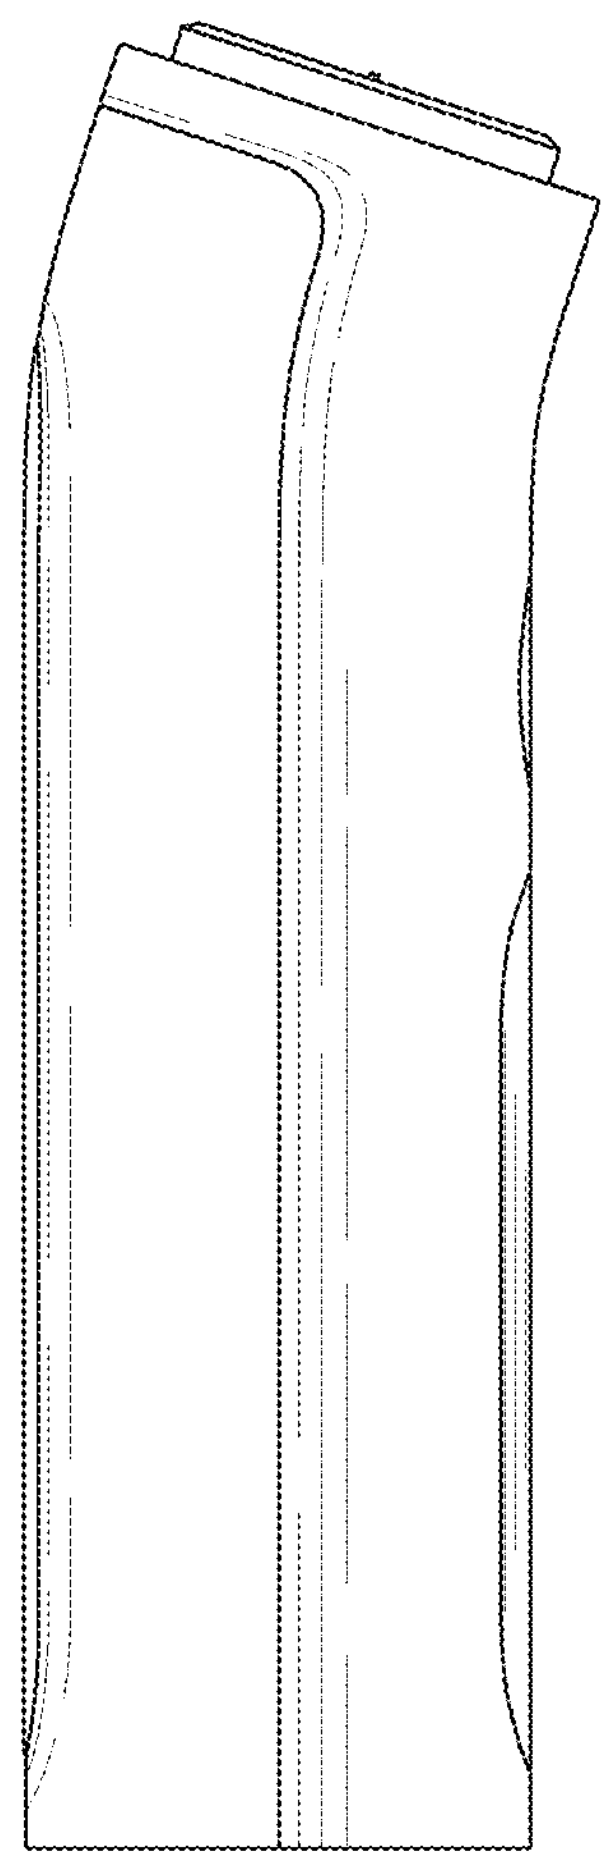

FIG. 5

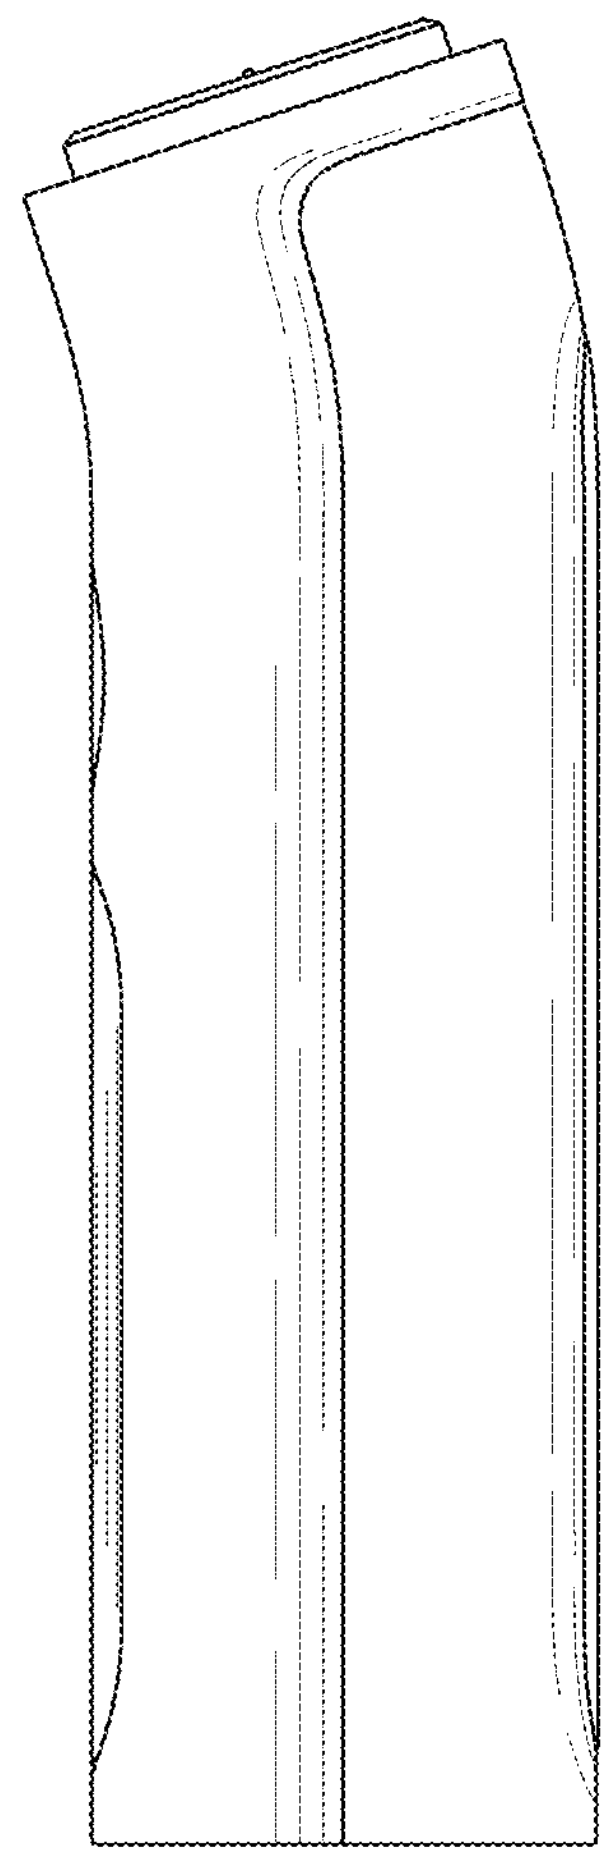

FIG. 6

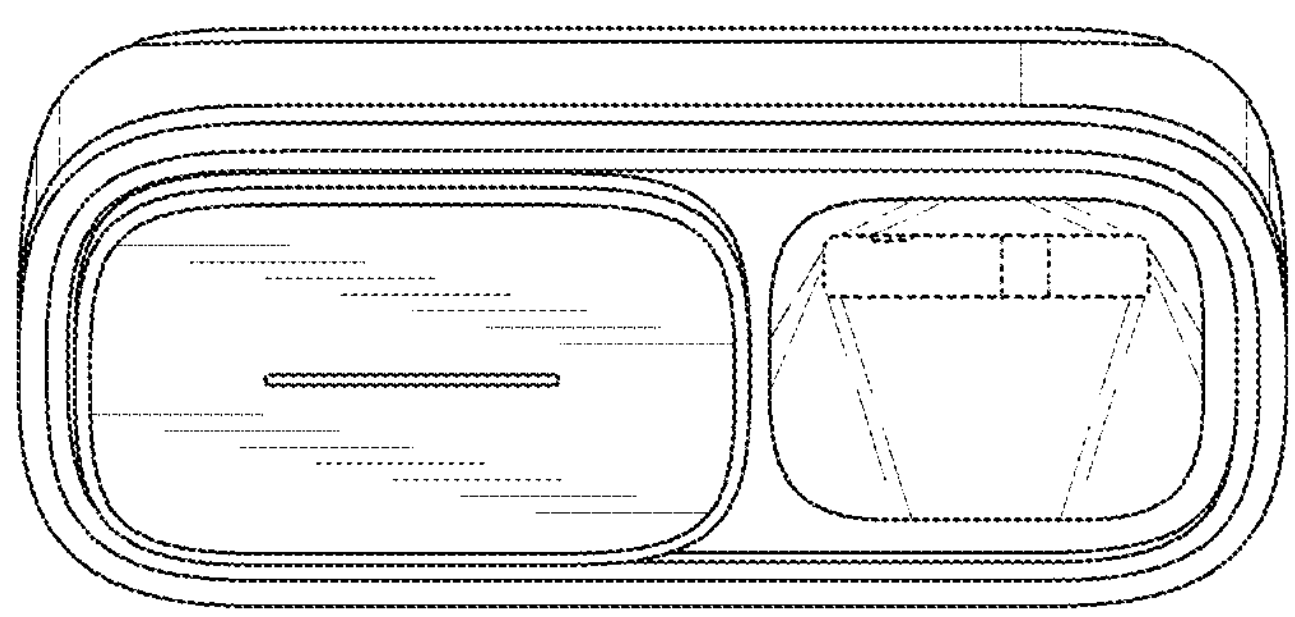

FIG. 7

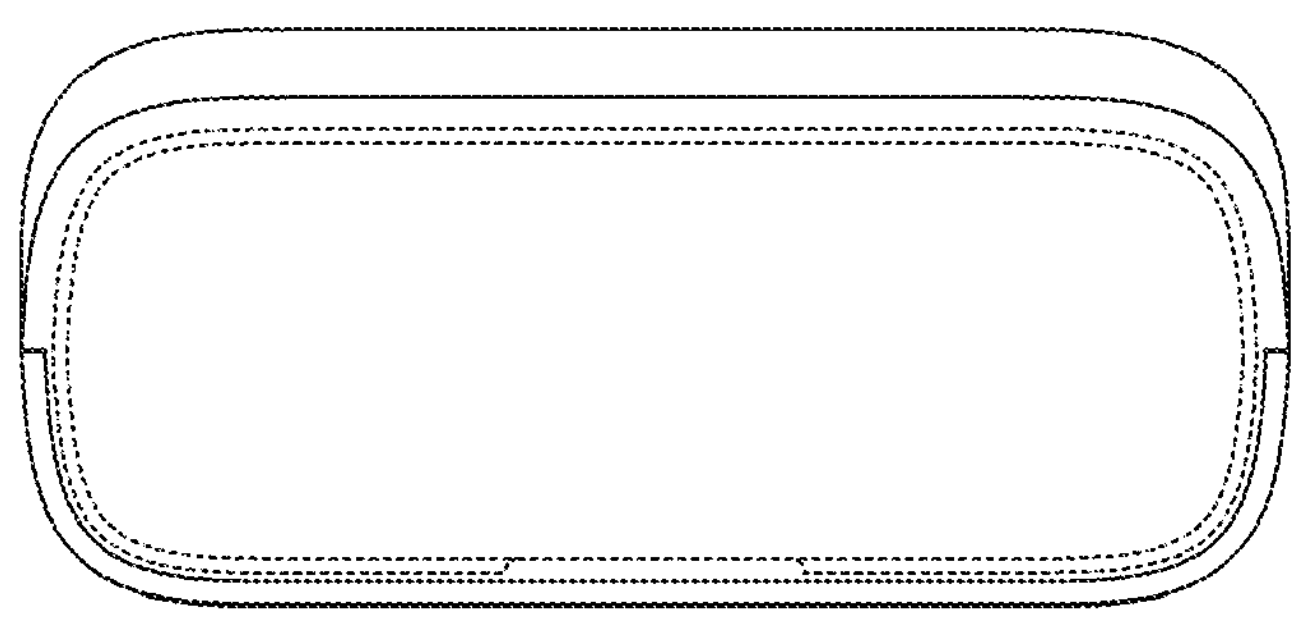

FIG. 8

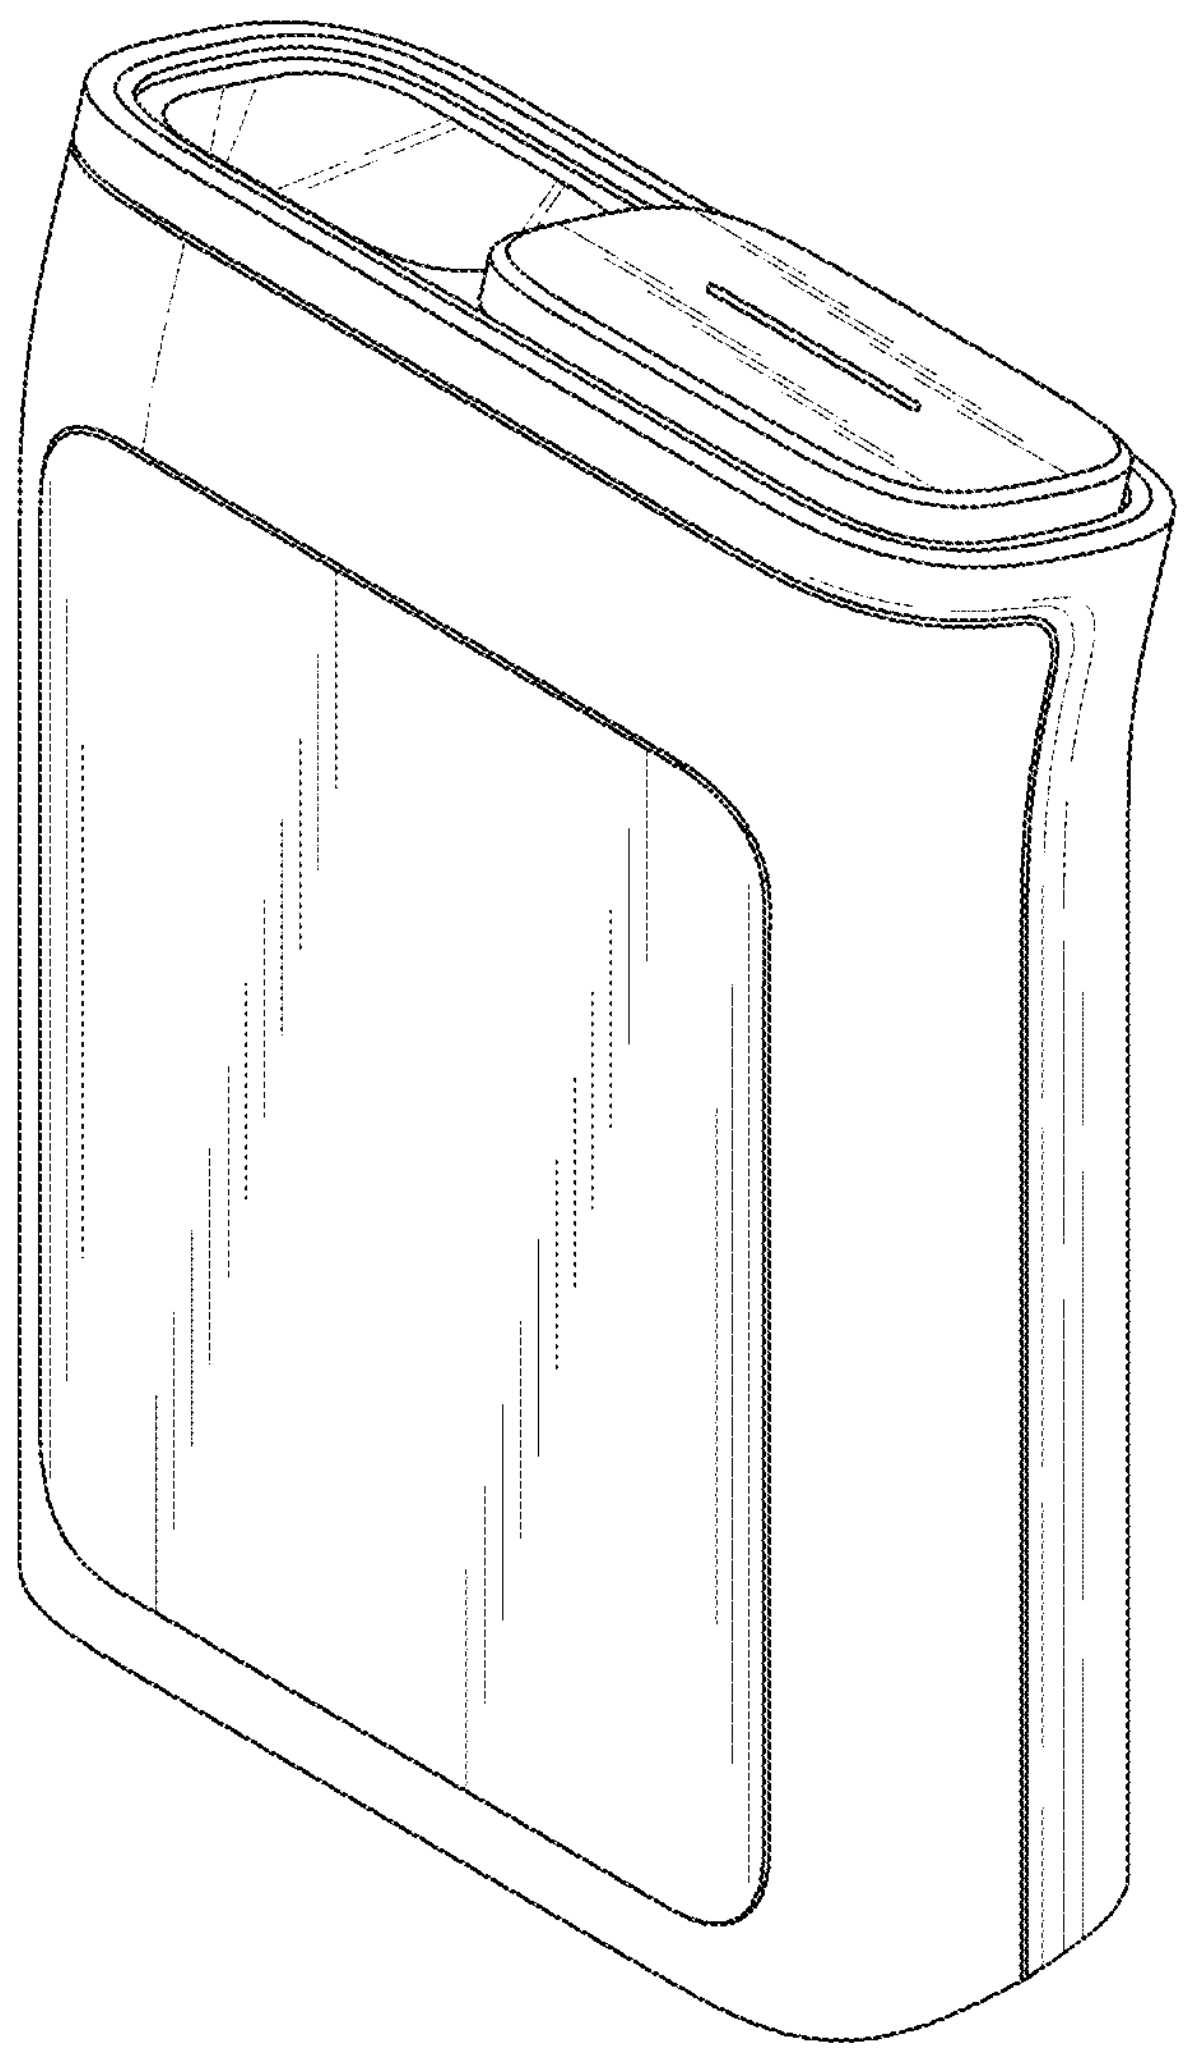

FIG. 9