



US 20250255576A1

(19) **United States**

(12) **Patent Application Publication**

Prince

(10) **Pub. No.: US 2025/0255576 A1**

(43) **Pub. Date: Aug. 14, 2025**

(54) **MINIMAL CATHETER LENGTH TOOL**

(71) Applicant: **Bard Access Systems, Inc.**, Salt Lake City, UT (US)

(72) Inventor: **Matthew J. Prince**, Herriman, UT (US)

(21) Appl. No.: **19/192,171**

(22) Filed: **Apr. 28, 2025**

Related U.S. Application Data

(63) Continuation of application No. 18/601,980, filed on Mar. 11, 2024, now Pat. No. 12,285,286, which is a continuation of application No. 17/485,035, filed on Sep. 24, 2021, now Pat. No. 11,925,505.

(60) Provisional application No. 63/083,684, filed on Sep. 25, 2020.

Publication Classification


(51) **Int. Cl.**
A61B 8/08 (2006.01)
A61B 8/00 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 8/085** (2013.01); **A61B 8/465** (2013.01); **A61B 8/469** (2013.01); **A61B 8/4472** (2013.01)

(57) **ABSTRACT**

A system and method including operations of generating an ultrasound image screen including an ultrasound image., the ultrasound image screen including a first user selection element configured to receive a first user input for selecting a blood vessel for display in the ultrasound image. The system and method can further include generating a parameter input screen. The parameter input screen can include a second user selection element configured to receive a second user input for selecting an angle of insertion of a medical device, a third user selection element configured to receive a third user input for increasing or decreasing a minimum dwell length of the medical device, and a graphical representation of the medical device depicting a selected angle of insertion and a selected minimum dwell length of the device.

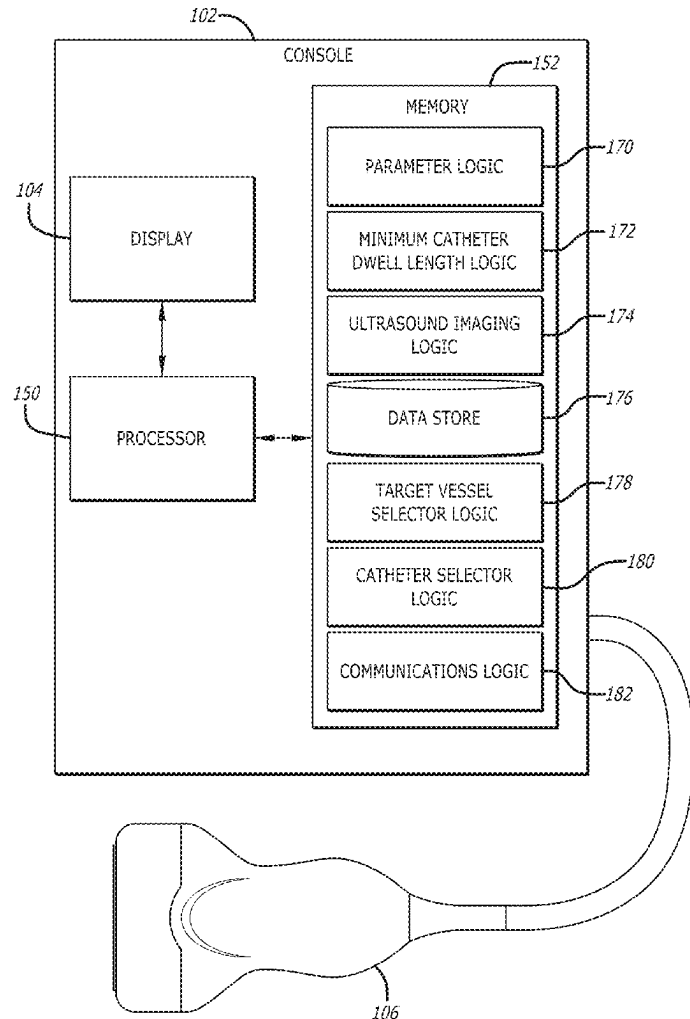

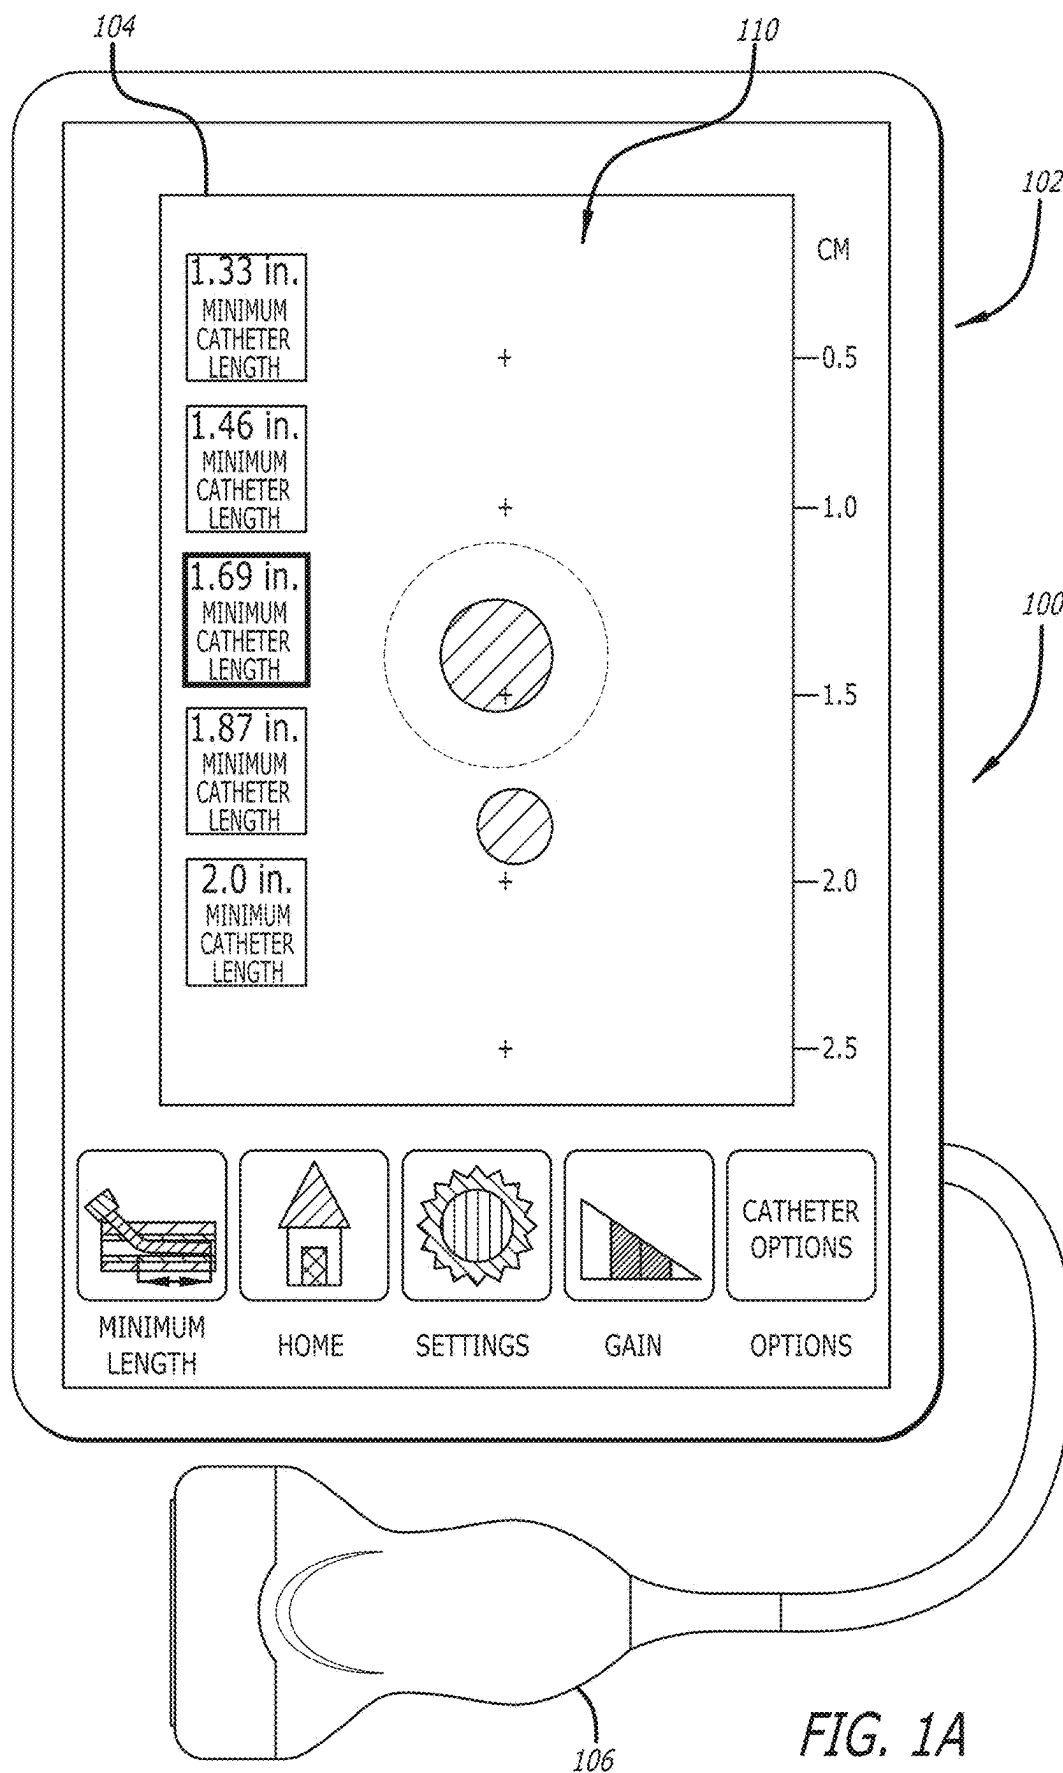


FIG. 1A

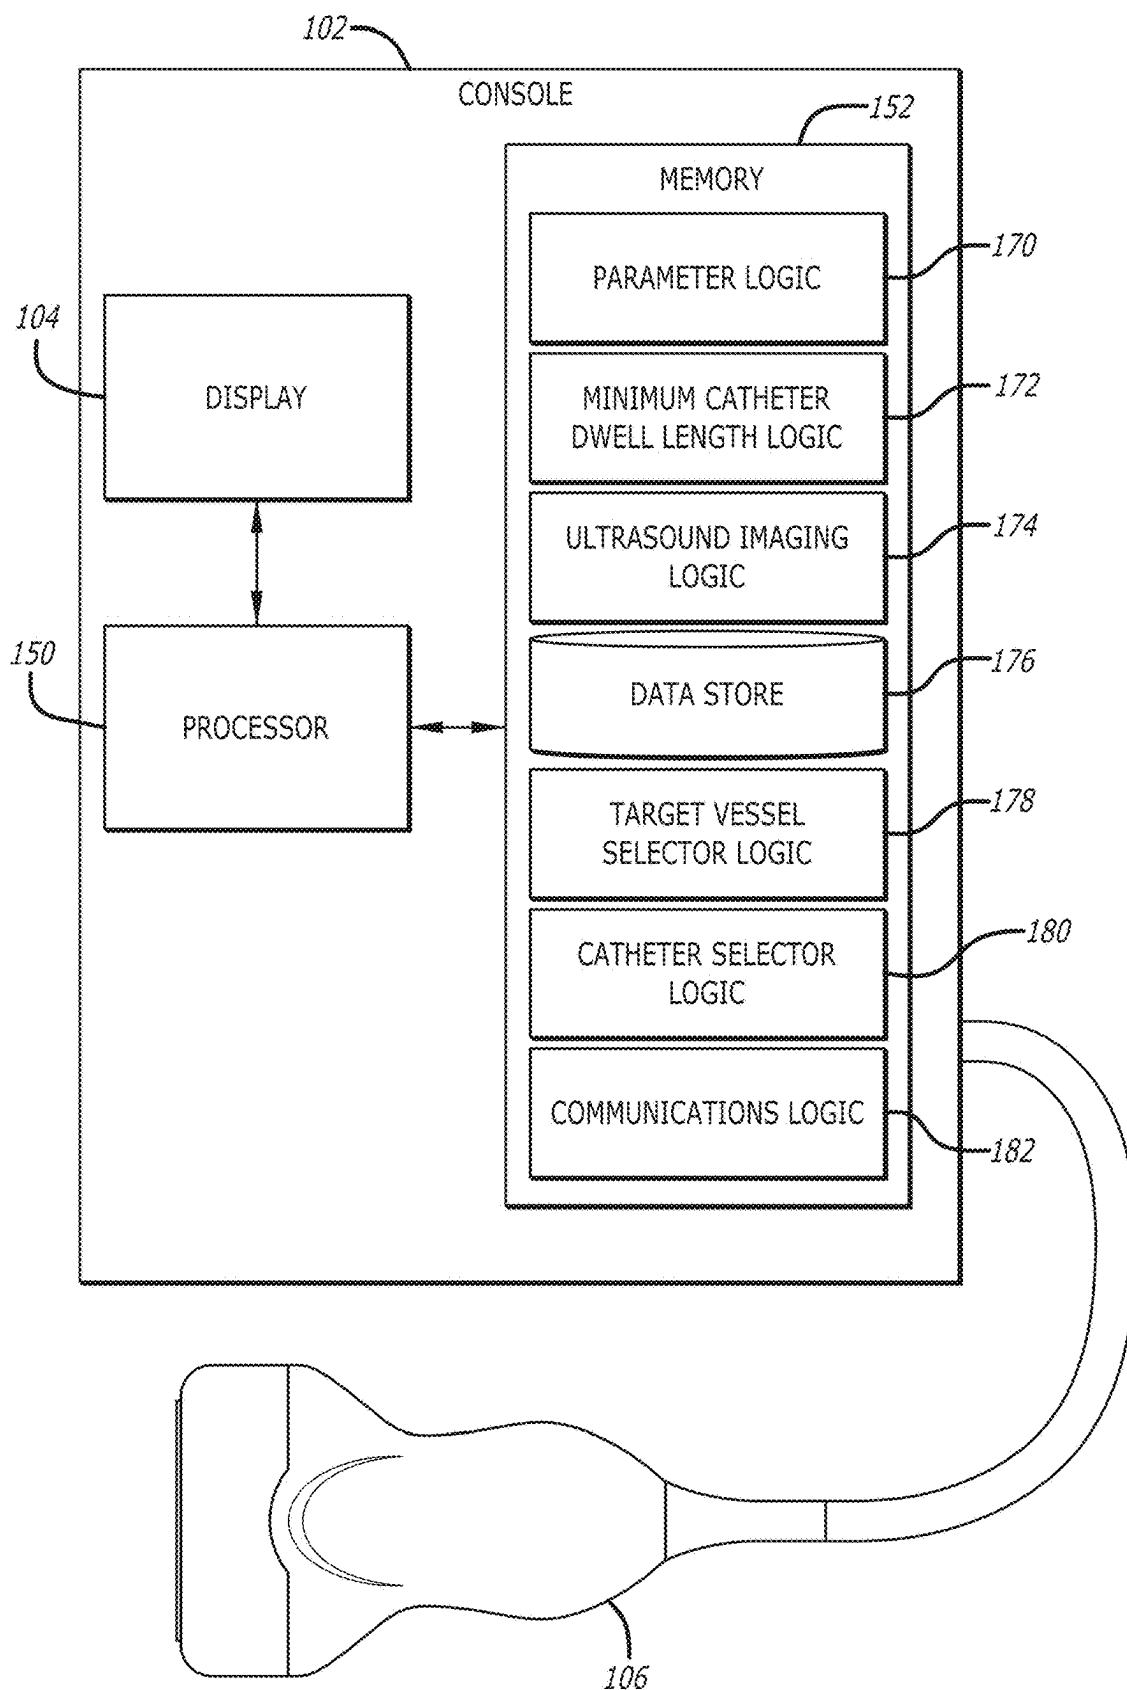
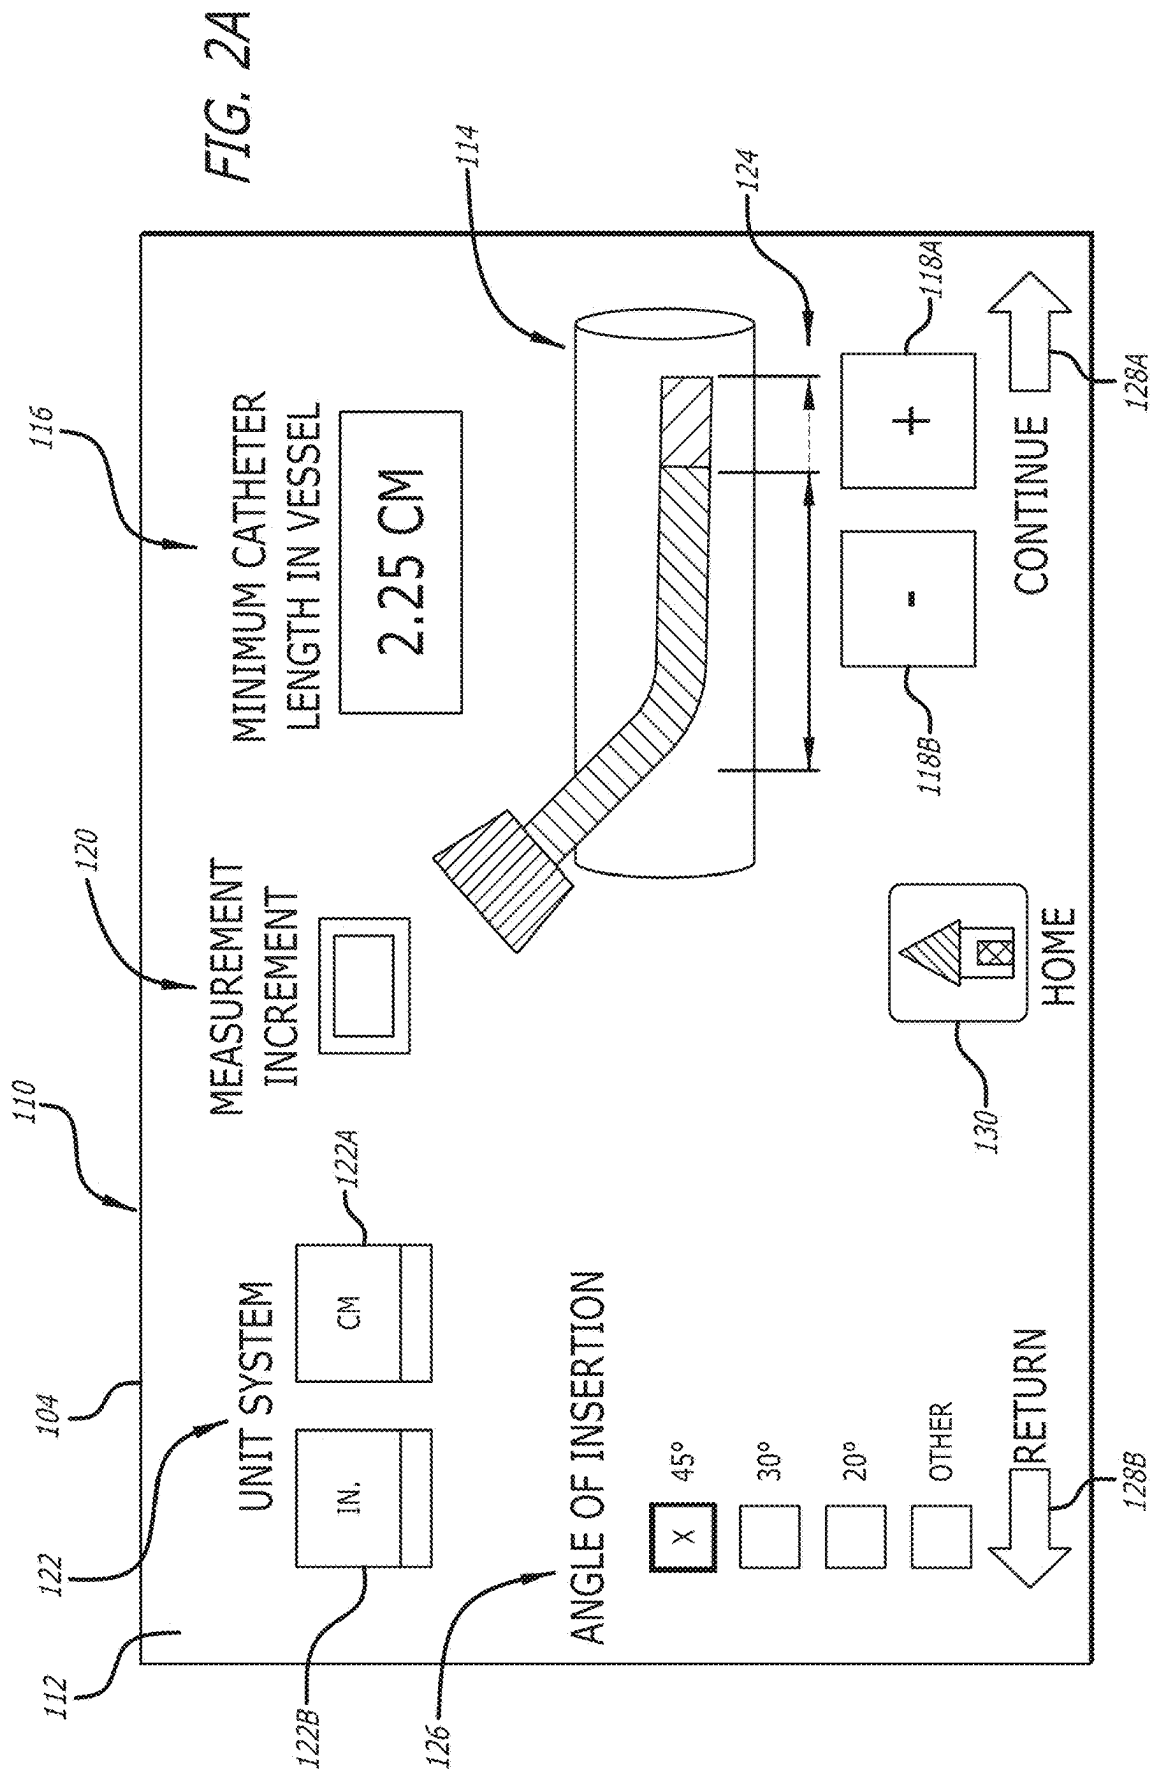


FIG. 1B



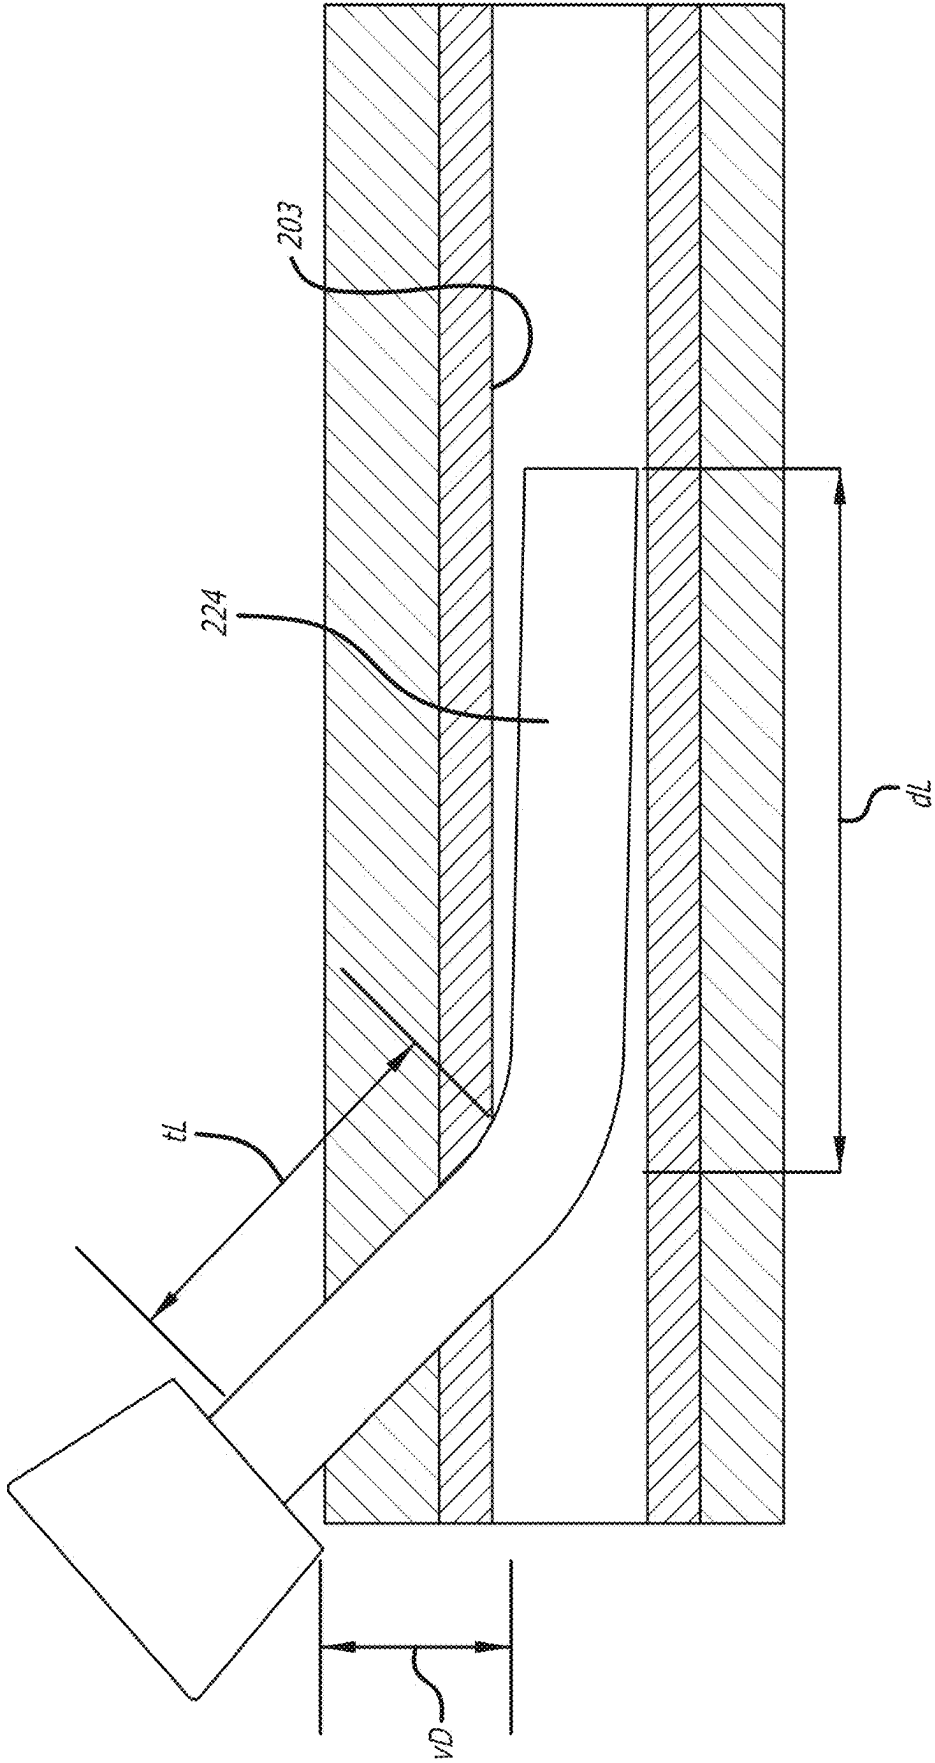


FIG. 2B

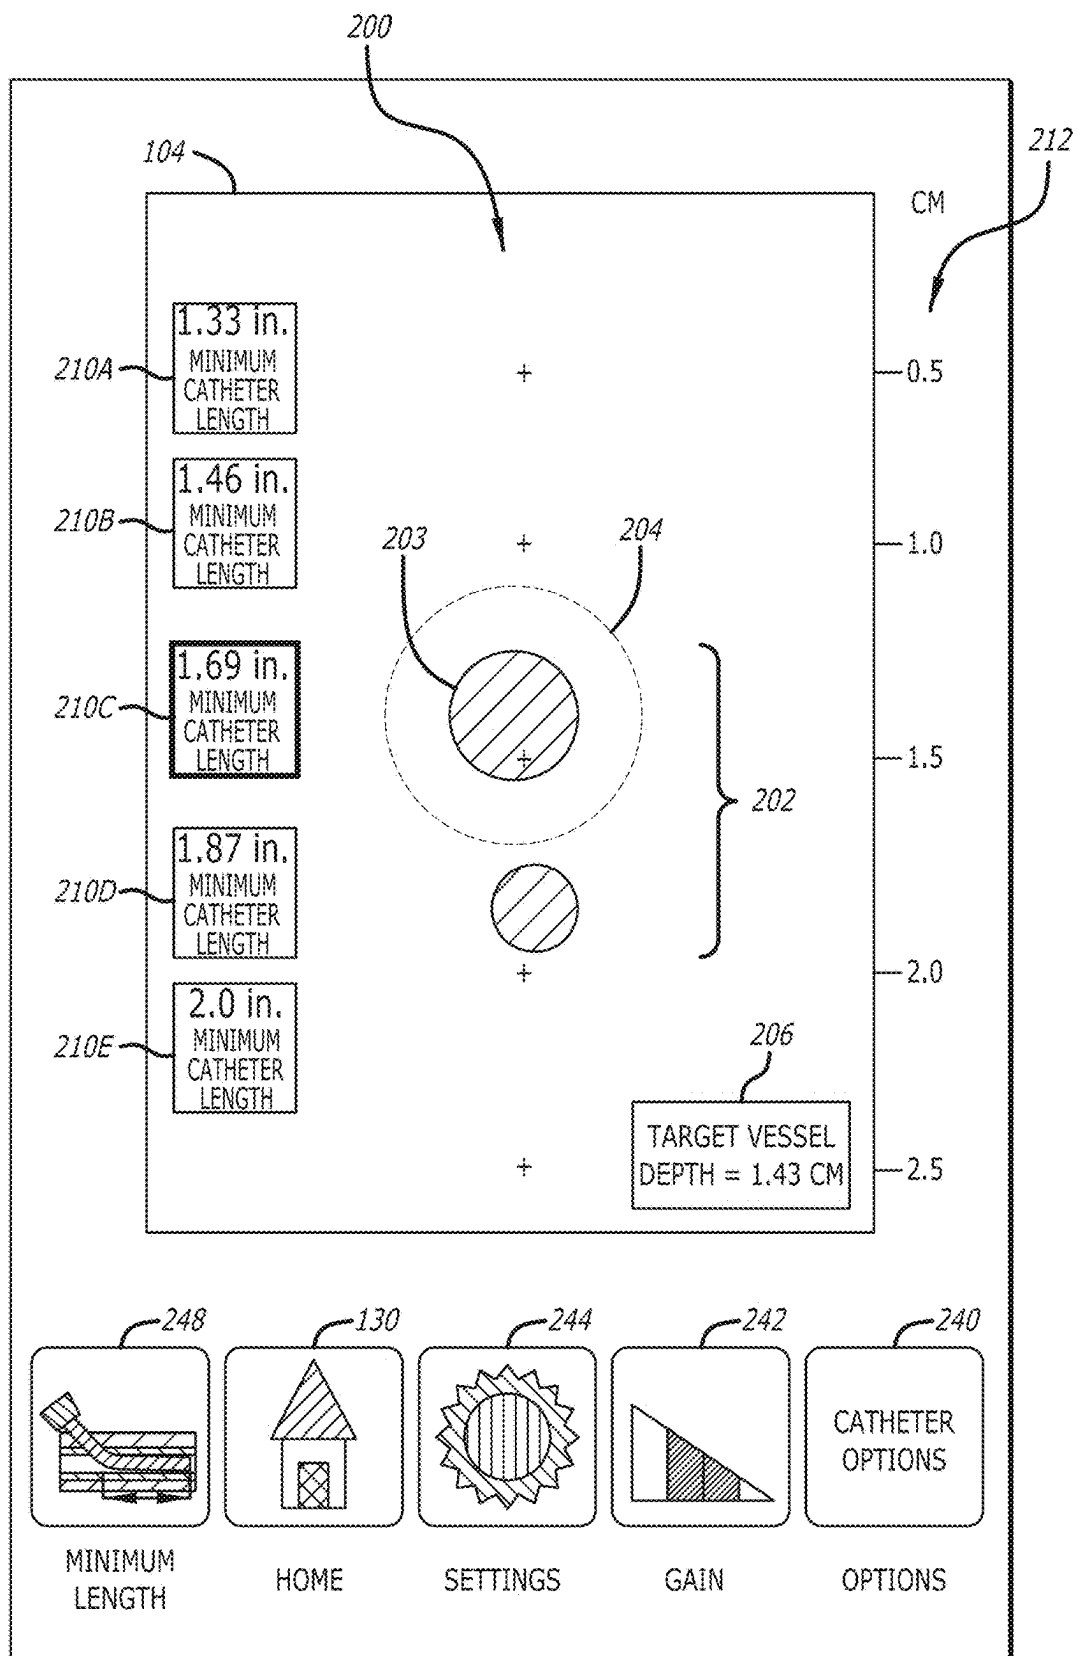


FIG. 3A

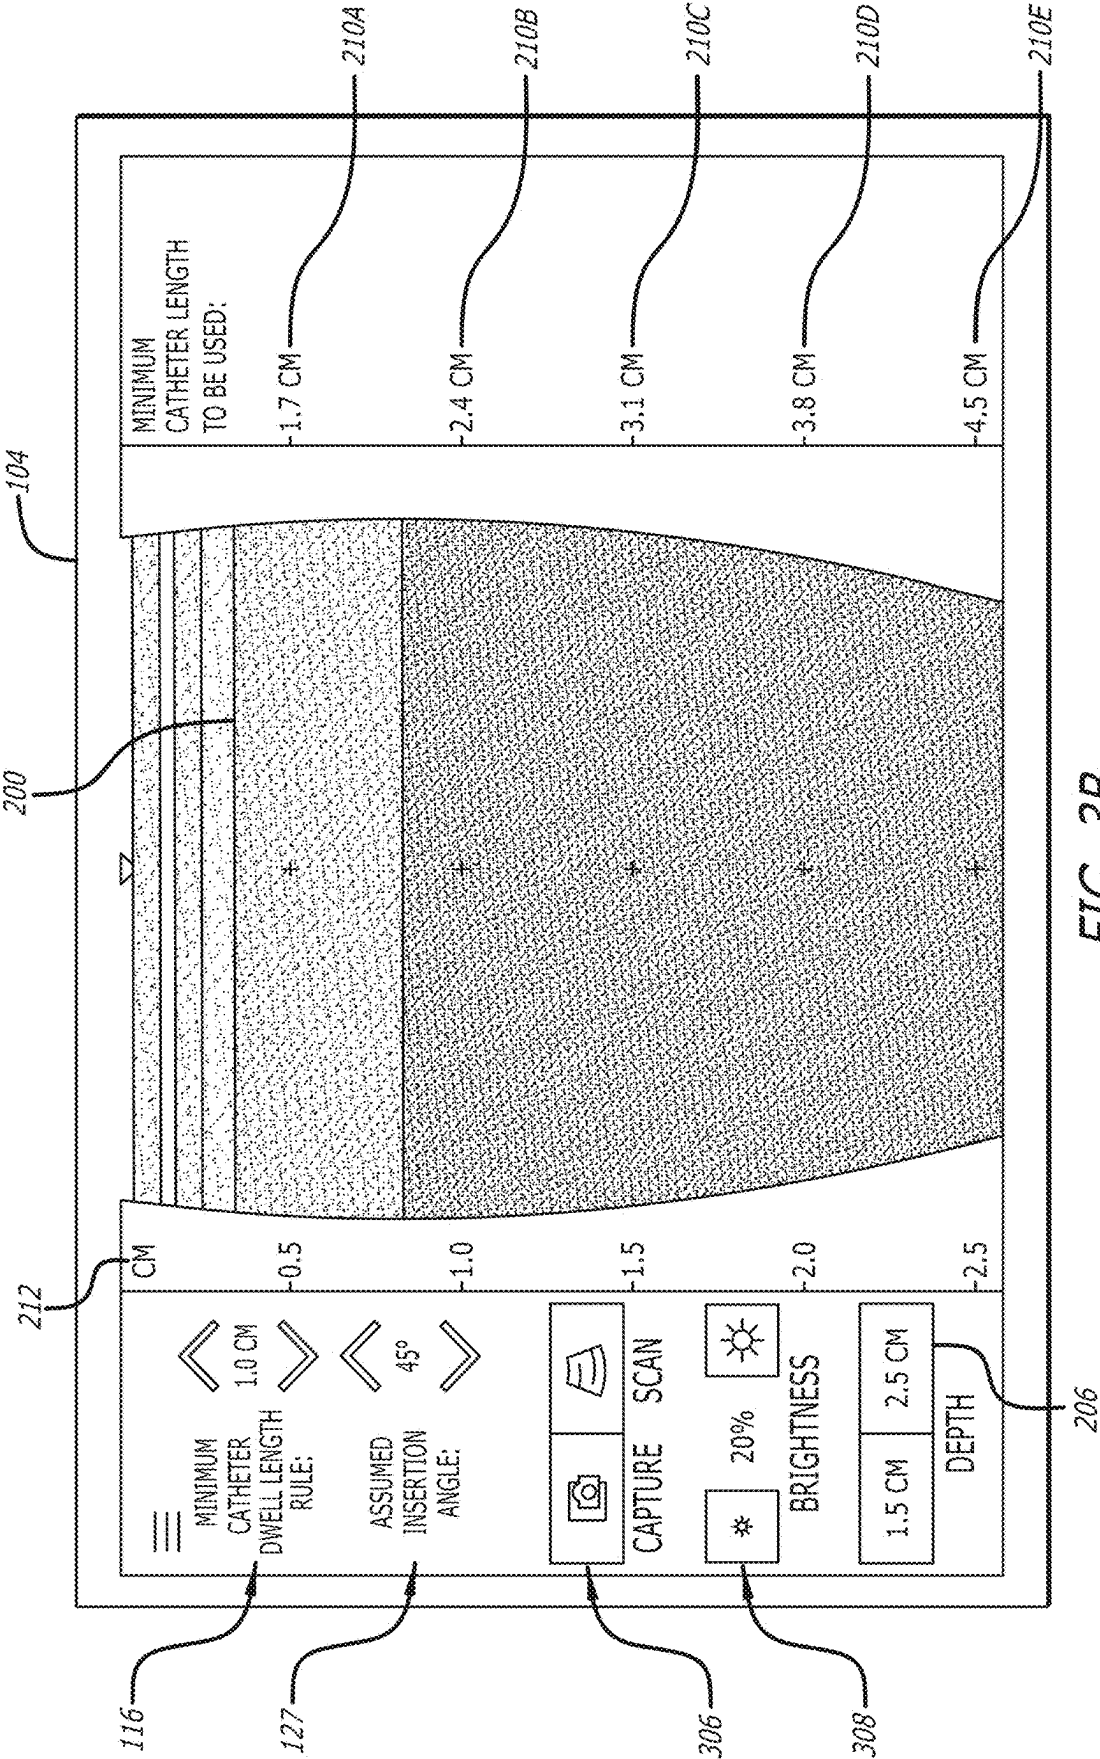


FIG. 3B

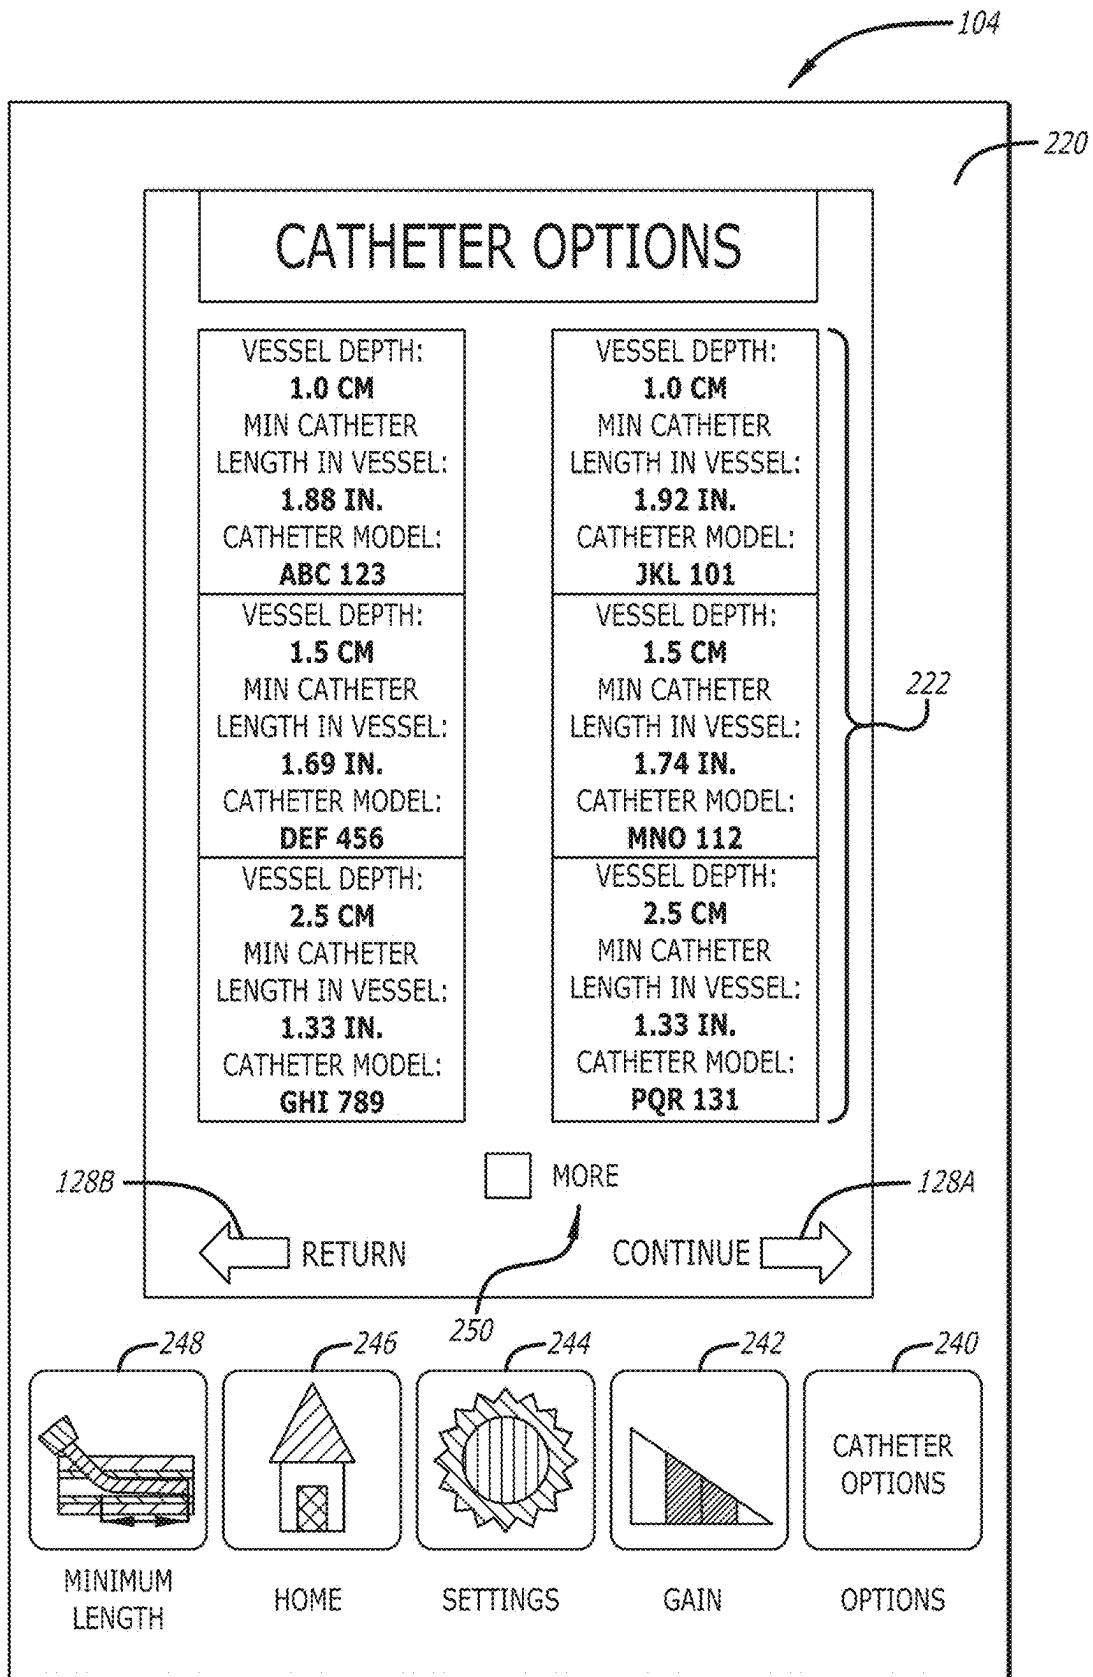


FIG. 4

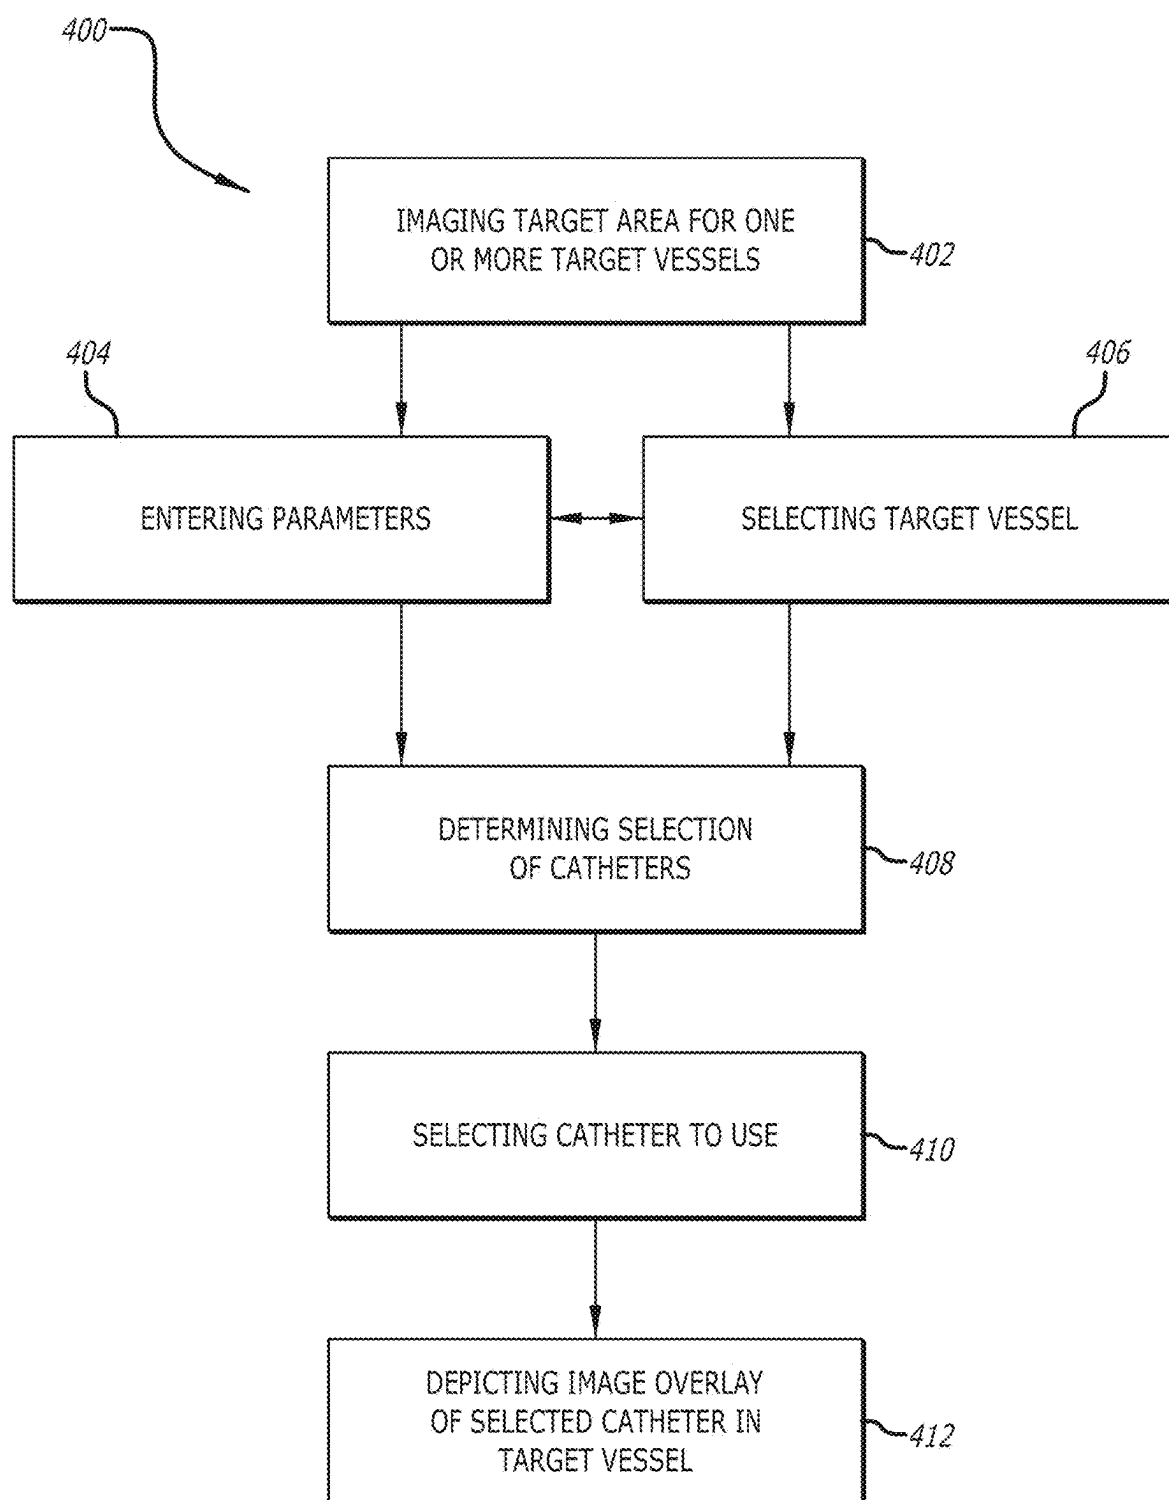


FIG. 5

MINIMAL CATHETER LENGTH TOOL**PRIORITY**

[0001] This application is a continuation of U.S. patent application Ser. No. 18/601,980, filed Mar. 11, 2024, now U.S. Pat. No. 12,285,286, which is a continuation of U.S. patent application Ser. No. 17/485,035, filed Sep. 24, 2021, now U.S. Pat. No. 11,925,505, which claims the benefit of priority to U.S. Provisional Application No. 63/083,684, filed Sep. 25, 2020, each of which is incorporated by reference in its entirety into this application.

BACKGROUND

[0002] When placing a vascular access device, clinicians must select a catheter based upon a number of different parameters. Current systems can force clinicians to select a vascular access device ("VAD") first, then use software and ultrasound imaging to evaluate if the vascular access device they selected would be appropriate. However, the clinicians' initial guess of vascular access device during pre-assessment may be incorrect, leaving clinicians to repeatedly guess until they finally arrive at the correct VAD. As such, clinicians would have to cycle through a selection of vascular access devices, evaluate the parameters of each VAD and use ultrasound imaging to confirm the VAD the clinicians selected would be the most appropriate for the target blood vessel. It would be beneficial to the patient, as well as time effective, for a tool that allows the clinicians to select a parameter (e.g., minimum catheter length in the vessel), image a vessel, display the vascular access device options that are most suitable and evaluate the vascular access device options in real time using ultrasound imaging. Disclosed herein is a system and method of use that addresses the foregoing.

[0003] Disclosed herein is a method for selecting a vascular access device for accessing a target blood vessel, including imaging one or more blood vessels, entering one or more parameter inputs including a minimum catheter dwell length or an angle of insertion, into a vascular access device selection tool, selecting a target blood vessel from the one or more blood vessels, determining a depth of the target blood vessel, and providing a selection of vascular access devices that are able to access the target blood vessel based on the one or more parameter inputs.

[0004] In some embodiments, the method includes using an ultrasound imaging system including a console communicatively coupled to an ultrasound probe and a display.

[0005] In some embodiments, the method includes where the vascular access device selection tool includes a parameter logic that is receiving the one or more parameter inputs from a user.

[0006] In some embodiments, the method includes where the vascular access device selection tool includes a target vessel selector logic that is determining a depth of the target blood vessel.

[0007] In some embodiments, the method includes where the vascular access device selection tool includes a catheter selection logic that is providing a selection of catheters capable of accessing the target blood vessel.

[0008] In some embodiments, the method includes where the vascular access device selection tool includes a minimum catheter length logic that is determining a selection of

catheters that are capable of accessing the target blood vessel, based on the parameter.

[0009] In some embodiments, the method includes where the vascular access device selection tool includes a data store that is storing a selection of catheters including information about each catheter length.

[0010] In some embodiments, the method includes where the vascular access device selection tool includes a communications logic that is updating the selection of catheters from a remote computing device.

[0011] In some embodiments, the method includes where the vascular access device selection tool includes an ultrasound imaging logic that is receiving input from an ultrasound probe and depicting one or more ultrasound images on a display.

[0012] In some embodiments, providing a selection of vascular access devices includes selecting a vascular access device to use, on a display.

[0013] In some embodiments, providing a selection of vascular access devices further includes depicting the ultrasound image overlay of the selected vascular access device in the target blood vessel on the display.

[0014] Also disclosed herein is an ultrasound imaging system including a console communicatively coupled to an ultrasound probe and a display, the console having a processor and a vascular access device selection tool configured to receive one or more of a minimum catheter dwell length parameter input or an angle of insertion parameter input.

[0015] In some embodiments, the ultrasound imaging system includes where the vascular access device selection tool includes one or more logic modules coupled to memory including a parameter logic, configured to receive the one or more minimum catheter dwell length parameter input or angle of insertion parameter input from a user, a target vessel selector logic, configured to determine a depth of the target vessel and a catheter selection logic, configured to provide a selection of catheters capable of accessing the target vessel.

[0016] In some embodiments, the ultrasound imaging system includes where the vascular access device selection tool includes a minimum catheter dwell length logic, configured to determine catheters that are capable of accessing the target vessel, given the one or more minimum catheter dwell length parameter input or the angle of insertion parameter input from the user.

[0017] In some embodiments, the ultrasound imaging system includes where the vascular access device selection tool includes a data store, configured to store a list of catheters including information about each catheter length.

[0018] In some embodiments, the ultrasound imaging system includes where the vascular access device selection tool further includes a communications logic, configured to update the selection of catheters from a remote computing device.

[0019] In some embodiments, the ultrasound imaging system includes where the vascular access device selection tool includes an ultrasound imaging logic, configured to receive an input transmitted from the ultrasound probe and provide an ultrasound image.

[0020] In some embodiments, the ultrasound imaging system includes where the display is wirelessly coupled to the console.

[0021] In some embodiments, the ultrasound imaging system includes where the display is touch screen.

[0022] Also disclosed herein is a vascular access device selection tool including one or more logic modules coupled to memory including a parameter logic, configured to receive one or more parameter inputs from a user, a target vessel selector logic, configured to determine a depth of a target blood vessel, and a catheter selection logic, configured to provide a selection of catheters capable of accessing the target vessel. The vascular access device selection tool includes a minimum catheter dwell length logic, configured to determine catheters that are capable of accessing the target blood vessel, given the one or more parameter inputs from the user, a data store, configured to store a selection of catheters including information about each catheter, a communications logic, configured to update the selection of catheters, and an ultrasound imaging logic, configured to depict one or more ultrasound images on a display.

[0023] In some embodiments, the vascular access device selection tool includes the one or more parameter inputs including a minimum catheter dwell length, angle of insertion or a combination of the minimum catheter dwell length and the angle of insertion.

[0024] These and other features of the concepts provided herein will become more apparent to those of skill in the art in view of the accompanying drawings and following description, which describe particular embodiments of such concepts in greater detail.

BRIEF DESCRIPTION OF DRAWINGS

[0025] A more particular description of the present disclosure will be rendered by reference to specific embodiments thereof that are illustrated in the appended drawings. It is appreciated that these drawings depict only typical embodiments of the invention and are therefore not to be considered limiting of its scope. Example embodiments of the invention will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

[0026] FIG. 1A illustrates a perspective view of an ultrasound imaging system including a minimum catheter length tool, in accordance with some embodiments.

[0027] FIG. 1B illustrates a block diagram depicting various components of an ultrasound imaging system including a minimum catheter length tool, in accordance with some embodiments.

[0028] FIG. 2A illustrates an exemplary parameter input screen of the minimum catheter length tool, in accordance with some embodiments.

[0029] FIG. 2B illustrates a method of identifying catheters by the minimum catheter length tool, in accordance with some embodiments.

[0030] FIG. 3A illustrates a depiction of a display of various components of the minimum catheter length tool, in accordance with some embodiments.

[0031] FIG. 3B illustrates an exemplary screenshot of an ultrasound imaging system including a minimum catheter length tool, in accordance with some embodiments.

[0032] FIG. 4 illustrates various components of the minimum catheter length tool, in accordance with some embodiments.

[0033] FIG. 5 illustrates a flow chart diagram of a method for selecting a vascular access device for accessing a target blood vessel, in accordance with some embodiments.

DESCRIPTION

[0034] Before some particular embodiments are disclosed in greater detail, it should be understood that the particular embodiments disclosed herein do not limit the scope of the concepts provided herein. It should also be understood that a particular embodiment disclosed herein can have features that can be readily separated from the particular embodiment and optionally combined with or substituted for features of any of a number of other embodiments disclosed herein.

[0035] Regarding terms used herein, it should also be understood the terms are for the purpose of describing some particular embodiments, and the terms do not limit the scope of the concepts provided herein. Ordinal numbers (e.g., first, second, third, etc.) are generally used to distinguish or identify different features or steps in a group of features or steps, and do not supply a serial or numerical limitation. For example, “first,” “second,” and “third” features or steps need not necessarily appear in that order, and the particular embodiments including such features or steps need not necessarily be limited to the three features or steps. Labels such as “left,” “right,” “top,” “bottom,” “front,” “back,” and the like are used for convenience and are not intended to imply, for example, any particular fixed location, orientation, or direction. Instead, such labels are used to reflect, for example, relative location, orientation, or directions. Singular forms of “a,” “an,” and “the” include plural references unless the context clearly dictates otherwise.

[0036] With respect to “proximal,” a “proximal portion” or a “proximal-end portion” of, for example, a catheter disclosed herein includes a portion of the catheter intended to be near a clinician when the catheter is used on a patient. Likewise, a “proximal length” of, for example, the catheter includes a length of the catheter intended to be near the clinician when the catheter is used on the patient. A “proximal end” of, for example, the catheter includes an end of the catheter intended to be near the clinician when the catheter is used on the patient. The proximal portion, the proximal-end portion, or the proximal length of the catheter can include the proximal end of the catheter; however, the proximal portion, the proximal-end portion, or the proximal length of the catheter need not include the proximal end of the catheter. That is, unless context suggests otherwise, the proximal portion, the proximal-end portion, or the proximal length of the catheter is not a terminal portion or terminal length of the catheter.

[0037] With respect to “distal,” a “distal portion” or a “distal-end portion” of, for example, a catheter disclosed herein includes a portion of the catheter intended to be near or in a patient when the catheter is used on the patient. Likewise, a “distal length” of, for example, the catheter includes a length of the catheter intended to be near or in the patient when the catheter is used on the patient. A “distal end” of, for example, the catheter includes an end of the catheter intended to be near or in the patient when the catheter is used on the patient. The distal portion, the distal-end portion, or the distal length of the catheter can include the distal end of the catheter; however, the distal portion, the distal-end portion, or the distal length of the catheter need not include the distal end of the catheter. That is, unless context suggests otherwise, the distal portion, the distal-end portion, or the distal length of the catheter is not a terminal portion or terminal length of the catheter.

[0038] The term “logic” may be representative of hardware, firmware or software that is configured to perform one

or more functions. As hardware, the term logic may refer to or include circuitry having data processing and/or storage functionality. Examples of such circuitry may include, but are not limited or restricted to a hardware processor (e.g., microprocessor, one or more processor cores, a digital signal processor, a programmable gate array, a microcontroller, an application specific integrated circuit “ASIC”, etc.), a semiconductor memory, or combinatorial elements.

[0039] Additionally, or in the alternative, the term logic may refer to or include software such as one or more processes, one or more instances, Application Programming Interface(s) (API), subroutine(s), function(s), applet(s), servlet(s), routine(s), source code, object code, shared library/dynamic link library (dll), or even one or more instructions. This software may be stored in any type of a suitable non-transitory storage medium, or transitory storage medium (e.g., electrical, optical, acoustical or other form of propagated signals such as carrier waves, infrared signals, or digital signals). Examples of a non-transitory storage medium may include, but are not limited or restricted to a programmable circuit; non-persistent storage such as volatile memory (e.g., any type of random access memory “RAM”); or persistent storage such as non-volatile memory (e.g., read-only memory “ROM”, power-backed RAM, flash memory, phase-change memory, etc.), a solid-state drive, hard disk drive, an optical disc drive, or a portable memory device. As firmware, the logic may be stored in persistent storage.

[0040] As used herein a “vascular access device” can include a catheter, peripherally inserted central catheter (“PICC”), peripheral intravenous line (“PIV”), central venous catheter (“CVC”), midline catheter, or the like etc.

[0041] Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by those of ordinary skill in the art.

[0042] FIG. 1A illustrates a perspective view of an ultrasound imaging system including a minimum catheter length tool, in accordance with some embodiments. In some embodiments, the ultrasound imaging system **100** includes an ultrasound probe **106** coupled to a console **102**. In some embodiments, the ultrasound probe **106** may be wired to the console **102** or in wirelessly communication with the console **102**. The ultrasound probe **106** may include transducer components for transmitting and receiving ultrasound signals that are transmitted to the console **102**. In some embodiments, the ultrasound imaging system **100** includes the console **102** coupled to a display **104**. In some embodiments, the console **102** may transmit ultrasound images to depict on the display **104**. In some embodiments, the display **104** may be a touch screen. In some embodiments, the display **104** may be wired, or in wirelessly communication with the console **102**. Exemplary wireless communication modalities can include WiFi, Bluetooth, Near Field Communications (NFC), cellular Global System for Mobile Communication (“GSM”), electromagnetic (EM), radio frequency (RF), combinations thereof, or the like.

[0043] In some embodiments, the ultrasound imaging system **100** includes a minimum catheter length tool (“tool”) **110** that may be configured to determine a selection of catheters that may achieve a minimum catheter dwell length based on the depth of a target vessel. As used herein, the minimum catheter dwell length is the length of a portion of a catheter that resides within the target vessel. The tool **110** can identify and depict on the display **104**, all the potential

catheters that fit the minimum catheter dwell length criteria for the given target vessel. The clinician can evaluate each potential catheter using the ultrasound imaging system **100** and chose a catheter, taking into account the results of the tool **110** along with other factors. When choosing a catheter, clinicians must evaluate a target vessel’s depth, the desired minimum catheter dwell length in the target vessel, the overall catheter length, and the preferred angle of insertion of the catheter into the target vessel among other factors.

[0044] FIG. 1B illustrates a block diagram depicting various components of an ultrasound imaging system including a minimum catheter length tool, in accordance with some embodiments. In some embodiments, the console **102** may include various components necessary for receiving, displaying and analyzing ultrasound images of the target blood vessel from the probe **106**. In some embodiments, the various components may include processor **150** and one or more logic modules coupled to memory **152** configured to perform at least one of the following: receive one or more parameter inputs from the user, calculate depth of a target blood vessel, provide a selection of catheters capable of accessing the target blood vessel, display one or more ultrasound images, determine catheters that are capable of accessing the target blood vessel given the user input, measure blood vessel area and blood vessel diameter, combinations thereof, or the like.

[0045] In some embodiments, the one or more logic modules may include a parameter logic **170**, a minimum catheter dwell length logic **172**, an ultrasound imaging logic **174**, a data store **176**, a target vessel selector logic **178**, a catheter selector logic **180**, a communications logic **182** or the like. In some embodiments, the parameter logic **170** may be configured to receive one or more parameter inputs (e.g., angle of insertion, desired minimum catheter dwell length in the blood vessel, or the like) from a user. In some embodiments, the minimum catheter dwell length logic **172** may be configured to determine a selection of catheters that are capable of accessing the target vessel, given the user input.

[0046] In some embodiments, the ultrasound imaging logic **174** may be configured to depict one or more ultrasound images on the display **104**. In some embodiments, the data store **176** may be configured to store one or more of: the ultrasound image data, catheters that are capable of accessing the target vessel data, user input data, a selection of all catheters including information about each catheter, or the like. In some embodiments, the target vessel selector logic **178** may be configured to calculate the target blood vessel depth from a skin surface. In some embodiments, the catheter selection logic **180** may be configured to provide a selection of catheters that are capable of accessing the target blood vessel. In some embodiments, the communications logic **182** may be configured to update the selection of catheters from a remote computing device. In some embodiments, a remote computing device may include a cloud network, an internet network, an intranet network, a server network or the like.

[0047] The minimum catheter length tool **110** can allow a clinician to select one or more target blood vessels using the ultrasound imaging system **100**, and provide the clinician a selection of suitable catheters to choose from, that meet various parameters including angle of insertion or minimum catheter dwell length, for the procedure. This contrasts with previous systems that require the clinician to choose a catheter first, then can advise if it is suitable, i.e. meets the

minimum catheter dwell length requirement. Advantageously, the minimum catheter length tool **110** avoids the clinician guessing as to which catheters might be suitable, and instead provides a selection of catheters that will be suitable.

[0048] The minimum catheter length tool **110** requires one or more parameter inputs provided by the user, the console **102** or a combination thereof. The one or more inputs can include parameter inputs including minimum catheter dwell length, catheter length, angle of insertion, depth of a target vessel, units of measurement or the like. In some embodiments, the one or more parameter inputs can be entered into the minimum catheter length tool **110** either qualitatively or quantitatively, or a combination thereof. As used herein, quantitative information can include entering numerical values, optionally within a range of predetermined values, or the like. As used herein, qualitative information can include selections of predetermined values, groupings, or the like.

[0049] FIG. 2A illustrates an exemplary parameter input screen of the minimum catheter length tool **110**, in accordance with some embodiments. In some embodiments, the minimum catheter length tool **110** can include a minimum catheter length tool parameter input screen (“parameter input screen”) **112** that depicts a plurality of icons on the display **104**. In some embodiments, the parameter input screen **112** can depict a catheter in a blood vessel icon **114**. In some embodiments, the icon **114** can include an indicator icon **116** that corresponds to the specified minimum catheter dwell length, in units of measurement, of a catheter in the blood vessel. The indicator icon **116** may be configured to be changed to match the user’s desired minimum catheter dwell length. In an embodiment, the minimum catheter dwell length can be selected by the clinician and entered to the tool **110** by way of the parameter input screen **112**. In an embodiment, the minimum catheter dwell length can be predetermined by the tool **110**.

[0050] In an embodiment, the clinician can adjust the minimum catheter dwell length. The indicator icon **116** may be configured to be increased or decreased by a standard unit of measurement with a positive icon **118A** or a negative icon **118B**. For example, selecting the positive icon **118A** will increase the dwell length of the catheter in the blood vessel icon **114** while selecting the negative icon **118B** will decrease the dwell length of the catheter in the blood vessel icon **114**. The standard unit of measure may be modified by the user by selecting a measurement increment icon **120**. The measurement increment icon **120** may be configured to allow the user to change the standard increment of the unit of measure depicted on the display **104**. For example, the unit of measure increment may be 0.5 in. and the user can change the unit of measure increment to be 1.0 in., 0.1 in., 0.01 in. or the like. However, it will be appreciated that greater or lesser increments are also contemplated.

[0051] In some embodiments, the parameter input screen **112** includes a unit system icon **122** that allows a user to select between imperial or metric measurement systems of the indicator icon **116**. In some embodiments, the user may select the desired units of measure displayed for the indicator icon **116**. For example, the indicator icon **116** may be configured to be displayed in metric by selecting the centimeter unit of the unit system icon **122A**. However, the user may select the inches unit of the unit system icon **122B** which would display the indicator icon **116** in imperial units. In some embodiments, the unit system icon **122** may be

configured to change the unit of measurement displayed on all user interfaces on the display **104**.

[0052] In some embodiments, the icon **114** can further include a catheter dwell length icon **124** indicating, e.g. by an arrow or similar graphical representation, the dwell length of the catheter in the blood vessel. In some embodiments, as the indicator icon **116** is increased or decreased by the positive icon **118A** or the negative icon **118B**, the catheter dwell length icon **124** may be modified to correspondingly increase or decrease in displayed length.

[0053] The parameter input screen **112** may include an angle of insertion selection panel **126** that includes a selection of predetermined angles of insertion, for example “45°”, “30°”, “20°” or the like. However, it will be appreciated that other predetermined angles are also contemplated. In an embodiment, the user can select a specified angle of insertion by selecting “other” and entering an angle of insertion. Optionally, the angle of insertion entered by the user may be limited to a predetermined range. As used herein, the angle of insertion can be defined as angle of the catheter relative to a surface of a patient’s skin at the point of insertion. In some embodiments, the “other” option may be configured to allow the user to specify the angle of insertion if the angle is not listed on the angle of insertion selection panel **126**.

[0054] In some embodiments, the parameter input screen **112** includes one or more arrow icons **128A/B** to help a user navigate through the user interface of the minimum catheter length tool **110**. In some embodiments, the one or more arrow icons **128A/B** can be indicated by text that includes “continue” or “return”. In some embodiments, the parameter input screen **112** may include a home icon **130** configured to return the user to a home screen, navigation page, a displayed ultrasound image screen **200**, or the like.

[0055] FIG. 2B illustrates a method of identifying catheters by the minimum catheter length tool, in accordance with some embodiments. In some embodiments, the minimum catheter length tool **110** may be configured to use various dimensions to identify catheters with overall catheter lengths that satisfy the desired minimum catheter dwell lengths in target vessels at various vessel depths. In some embodiments, the target blood vessel **203** has a vessel depth (“vD”). In some embodiments, a catheter **224** has a desired minimum catheter dwell length, (“dL”), and a travel length (“tL”), the length the catheter **224** travels to get to the target vessel at the specific angle of insertion. The minimum catheter length tool **110** will display only catheters that have a minimum overall catheter length of the desired minimum catheter dwell length, (dL)+the travel length (tL). For example, if a target vessel depth vD is 1.5 cm, the desired minimum catheter dwell length is 1.5 cm, the minimum catheter length tool **110** may be configured to calculate the travel length (tL) being 2.1 cm and will only display catheters that have a minimum overall catheter length of 3.6 cm. A catheter with a minimum overall catheter length of at least 3.6 cm is able to access a target vessel depth of 1.5 cm while allowing for least 1.5 cm of the catheter **224** to dwell in the target blood vessel **203**.

[0056] FIG. 3A illustrates an ultrasound image screen **200** of the minimum catheter length tool **110**, in accordance with some embodiments. In some embodiments, the ultrasound image screen **200** of the minimum catheter length tool **110** includes a dynamic ultrasound image of the one or more blood vessels **202**. In some embodiments, the ultrasound image screen **200** includes a static ultrasound image of the

one or more blood vessels **202**. The ultrasound image screen **200** can include vessel depth indicators **212** displaying segmented depth markers to indicate a depth of a target blood vessel **203**. The ultrasound image **200** includes a target vessel selector **204** used to select a target blood vessel **203** from the one or more blood vessel **202** on the display **104**. Using the target vessel selector **204** identifies a specific target vessel **203** from the one or more blood vessels **202** displayed. The tool **110** can then display a depth of the selected target vessel **203** as indicated by the target vessel depth icon **206**.

[0057] In some embodiments, the tool **110** can automatically determine a specified target vessel **203** from the one or more blood vessels **202** displayed. In an embodiment, a user can select a specified target vessel **203**, e.g. by selecting the target vessel **203** on the touch screen display, manipulating a cursor on the display, or the like. In some embodiments, selecting the target blood vessel **203** using the vessel selector **204** will bring up the parameter input screen **112** of FIG. 2A. In some embodiments, selecting the minimum length icon **248** will bring up the parameter input screen **112** of FIG. 2A.

[0058] In some embodiments, the tool **110** may be configured to display a plurality of “minimum catheter length” icons **210A-E** that depict the minimum catheter length needed to meet the minimum catheter dwell length in a vessel that resides at the respective vessel depth. The plurality of “minimum catheter length” icons **210A-E** may be configured to correspond to the vessel depth indicators **212** depicted on the display. In some embodiments, one of the plurality of “minimum catheter length” icons **210C** that corresponds with the targeted vessel depth as indicated by the vessel selector **204** may be configured to be highlighted. The user may select the highlighted “minimum catheter length” icon **210C** which may be configured to transition the user to a catheter options user interface **220** that will be described more detail herein.

[0059] In an embodiment, one of the depth icons **206** or the length icons **210** may be displayed proximate the selected target vessel **203** and dynamically update as the target vessel selector **204** is moved about the display **104**. In an embodiment, one of the depth icon **206** or the length icon **210** may be displayed proximate the target vessel **203** when the target vessel **203** is selected.

[0060] In an embodiment, the tool **110** may automatically navigate between different screens, e.g. the parameter input screen (FIG. 2A) or the ultrasound image screen (FIG. 3A) as the user selects different options, or as different inputs are required from the user. Optionally, the user can navigate between different screens using the arrows **128A/B** or similar icons.

[0061] In some embodiments, the catheter options screen **220** may be selected by a “catheter options” icon **240**. In some embodiments, the minimum catheter length tool **110** may include a “gain” icon **242** that may be configured to depict the strength of the received ultrasound signal. In some embodiments, the minimum catheter length tool **110** may include a “settings” icon **244** that may be configured to display and adjust the settings of all the components of the minimum length catheter tool **110**. In some embodiments, the minimum catheter length tool **110** may include the “home” icon **130** configured to return the user to a home screen, the ultrasound image screen **200**, or the like. It can be appreciated that other icons used in ultrasound imaging systems may be included.

[0062] FIG. 3B illustrates an exemplary screenshot of the ultrasound imaging system on the display **104** including the minimum catheter length tool **110**, in accordance with some embodiments. In some embodiments, the tool **110** can be configured to display the ultrasound image **200** including an angle of insertion icon **127** and the minimum catheter dwell length indicator icon **116**. The tool **110** can further be configured to display one or more of the plurality of “minimum catheter length” icons **210A-E**, target vessel depth icon **206** or the vessel depth indicators **212** as previously described. The tool **110** may further be configured to display a display selection icon **306**. In some embodiments, the display selection icon **306** may be configured to toggle between the static ultrasound image **200** and the dynamic ultrasound image **200**. The tool **110** may be configured to display a display adjustment icon **308**. In some embodiments, the display adjustment icon **308** may be configured to adjust the brightness of the display **104**.

[0063] FIG. 4. illustrates a catheter options screen **220** of the minimum catheter length tool on the display **104**, in accordance with some embodiments. Based on the inputs and information provided from the parameter input screen (FIG. 2A) and the ultrasound image screen (FIG. 3A), the catheter options screen **220** can display, a selection of catheters **222** that can be used to access the target vessel **203**. These catheters **222** fit the user selected criteria including catheter insertion angle and minimum catheter dwell length in target blood vessel when accessing the target blood vessel at the given depth. In some embodiments, each catheter option includes the specific information from the user selected criteria including one or more of the target vessel depth, the user selected minimum catheter length in the vessel or the catheter model. In some embodiments, selecting one of the catheter options may provide additional information, about the specific catheter including one of: catheter diameter, catheter cross sectional area, an indicator of whether the selected catheter will fit within the target blood vessel, vessel occupancy with that specific catheter, the procedures the catheter is used for, purchase price, current inventory, ordering information, combinations thereof, or the like. In some embodiments, the user can select additional catheter options not displayed on the catheter options user interface **220** or adjust the number of catheter options displayed on the catheter options user interface **220** by selecting a “more” icon **250**. Additionally, in some embodiments, a plurality of icons may be depicted including one or more of the “minimum length” icon **248**, the “home” icon **130**, the “settings” icon **244**, the “gain” icon **242** or the “catheter options” icon **240**, as described herein.

[0064] FIG. 5 illustrates a block diagram of a method for selecting a vascular access device for accessing a target blood vessel, in accordance with some embodiments. The method **400** includes imaging the target area for one or more blood vessels (block **402**). In some embodiments, imaging including using an ultrasound imaging system **100** having a console **102** communicatively coupled to an ultrasound probe **106** and a display **104**. In some embodiments, the console **102** may include a minimum catheter length tool **110**. In some embodiments, the minimum catheter length tool **110** may be configured to receive user parameter input to determine a selection of catheters that may be capable of accessing a target blood vessel at the prescribed depth. The method **400** further includes entering parameters (block **404**). In some embodiments, entering includes entering the

angle of insertion and the minimum catheter dwell length as parameters to use for choosing a catheter. In some embodiments, entering including entering the angle of insertion and the minimum catheter dwell length on a parameter input screen **112**. The method **400** includes selecting one or more target vessels (block **406**). In some embodiments, selecting includes selecting using a target vessel selector **204** on an ultrasound image screen **200**. The method **400** includes determining a selection of catheters **222** (block **408**). In some embodiments, determining a selection of catheters includes using the minimum length catheter tool **110** to determine the selection of catheters **222** that are capable of accessing the target vessel **203** based up the angle of insertion, the target vessel depth and the minimum catheter dwell length. The method **400** includes selecting a catheter to use (block **410**). In some embodiments, selecting the catheter to use includes selecting from the selection of catheters **222** generated by the minimum catheter length tool **110**. The method **400** includes depicting ultrasound image overlay of selected catheter in target vessel (block **412**). In some embodiments, the user can move between entering parameters (block **404**) and selecting one or more target vessels (block **406**) until the user is satisfied with the results. [0065] While some particular embodiments have been disclosed herein, and while the particular embodiments have been disclosed in some detail, it is not the intention for the particular embodiments to limit the scope of the concepts provided herein. Additional adaptations and/or modifications can appear to those of ordinary skill in the art, and, in broader aspects, these adaptations and/or modifications are encompassed as well. Accordingly, departures may be made from the particular embodiments disclosed herein without departing from the scope of the concepts provided herein.

What is claimed is:

1. A system comprising:

one or more logic modules stored within a non-transitory storage medium, the one or more logic modules, when executed by one or more processors, perform operations including:

generating an ultrasound image screen including an ultrasound image, the ultrasound image screen including a first user selection element configured to receive a first user input for selecting a blood vessel for display in the ultrasound image;

generating a parameter input screen, comprising:

a second user selection element configured to receive a second user input for selecting an angle of insertion of a medical device;

a third user selection element configured to receive a third user input for increasing or decreasing a minimum dwell length of the medical device; and
a graphical representation of the medical device depicting a selected angle of insertion and a selected minimum dwell length of the medical device;

determining a depth of a selected blood vessel; and
determining a selection of medical devices that satisfy conditions based on one or both of the selected angle of insertion and the selected minimum dwell length.

2. The system according to claim 1, wherein the system is configured to automatically toggle between the ultrasound image screen and the parameter input screen upon a selection of options by a user.

3. The system according to claim 1, wherein the ultrasound image screen and the parameter input screen include a toggle user selection element configured to navigate between the ultrasound image screen and the parameter input screen.

4. The system according to claim 1, wherein the operations further include generating a catheter options screen.

5. The system according to claim 1, wherein the medical device is a catheter, and wherein the selection of medical devices is a selection of catheters.

6. The system according to claim 5, wherein determining a selection of catheters comprises calculating a travel length of the catheter to a target vessel.

7. The system according to claim 6, wherein the operations further comprise depicting the catheter overlayed onto the target vessel in the ultrasound image.

8. The system according to claim 1, wherein the ultrasound image is a dynamic ultrasound image.

9. The system according to claim 1, wherein the ultrasound image screen is configured to display a depth of a selected blood vessel.

10. The system according to claim 1, wherein the graphical representation of the medical device is dynamically adjustable on the parameter input screen based on the third user input.

11. The system according to claim 1, wherein the ultrasound image screen and the parameter input screen are configured for display on a console operably connected to an ultrasound probe.

12. The system according to claim 1, wherein generating the ultrasound image screen comprises generating a plurality of minimum catheter length icons depicting a minimum catheter length necessary to satisfy a minimum catheter dwell length at a plurality of corresponding depths.

* * * * *