US0D1090829S

(12) United States Design Patent
Bazdanes et al.

(10) Patent No.: US D1,090,829 S
(45) Date of Patent: ** Aug. 26, 2025

(54) **MEDICAL DEVICE HOUSING**

(71) Applicant: **ABIOMED, Inc.**, Danvers, MA (US)

(72) Inventors: **Christopher Theodore Bazdanes**, Danvers, MA (US); **Robert Schaefer**, Danvers, MA (US); **Vincent Roy**, Danvers, MA (US)

(73) Assignee: **ABIOMED, INC.**, Danvers, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/946,144**

(22) Filed: **Jun. 6, 2024**

Related U.S. Application Data

(62) Division of application No. 29/893,659, filed on Jun. 1, 2023, now Pat. No. Des. 1,035,868, which is a division of application No. 29/813,991, filed on Nov. 2, 2021, now Pat. No. Des. 994,880.

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/133**

(58) **Field of Classification Search**
USPC D24/112–115, 127–130, 133
CPC A61M 25/0136; A61M 25/0097; A61M 2025/0098; A61M 25/0017
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D351,652	S	10/1994	Jackson et al.
D389,912	S	1/1998	Daniel et al.
D450,843	S	11/2001	McGuckin et al.
D494,270	S	8/2004	Reschke
D495,051	S	8/2004	Reschke
D564,093	S	3/2008	Marchand et al.
D597,668	S	8/2009	Woodruff et al.
D598,543	S	8/2009	Vogel et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CN	306163859		11/2020
CN	306177257	*	11/2020

(Continued)

OTHER PUBLICATIONS

Bi-Directional EP Catheter, RNDR Medical, [Post date: Jun. 26, 2022], [Site seen: Apr. 24, 2025], Seen at URL: https://www.rndrmedical.com/projects/bi-directional-ep-catheter/ (Year: 2022).*

(Continued)

Primary Examiner — Sandra Snapp
Assistant Examiner — Gilbert B Ford
(74) *Attorney, Agent, or Firm* — Botos Churchill IP Law LLP

(57) **CLAIM**

The ornamental design for a medical device housing, as shown and described.

DESCRIPTION

FIG. **1** is a top, front, left side perspective view of a medical device housing;
FIG. **2** is a front elevation view of FIG. **1**;
FIG. **3** is a rear elevation view of FIG. **1**;
FIG. **4** is a right side elevation view of FIG. **1**;
FIG. **5** is a left side elevation view of FIG. **1**;
FIG. **6** is a top plan view of FIG. **1**;
FIG. **7** is a bottom plan view of FIG. **1**; and,
FIG. **8** is a bottom, front, right side perspective view of FIG. **1**.
The dot-dash broken lines represent boundaries of the claimed design and form no part thereof. All other broken lines illustrate portions of the medical device housing that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

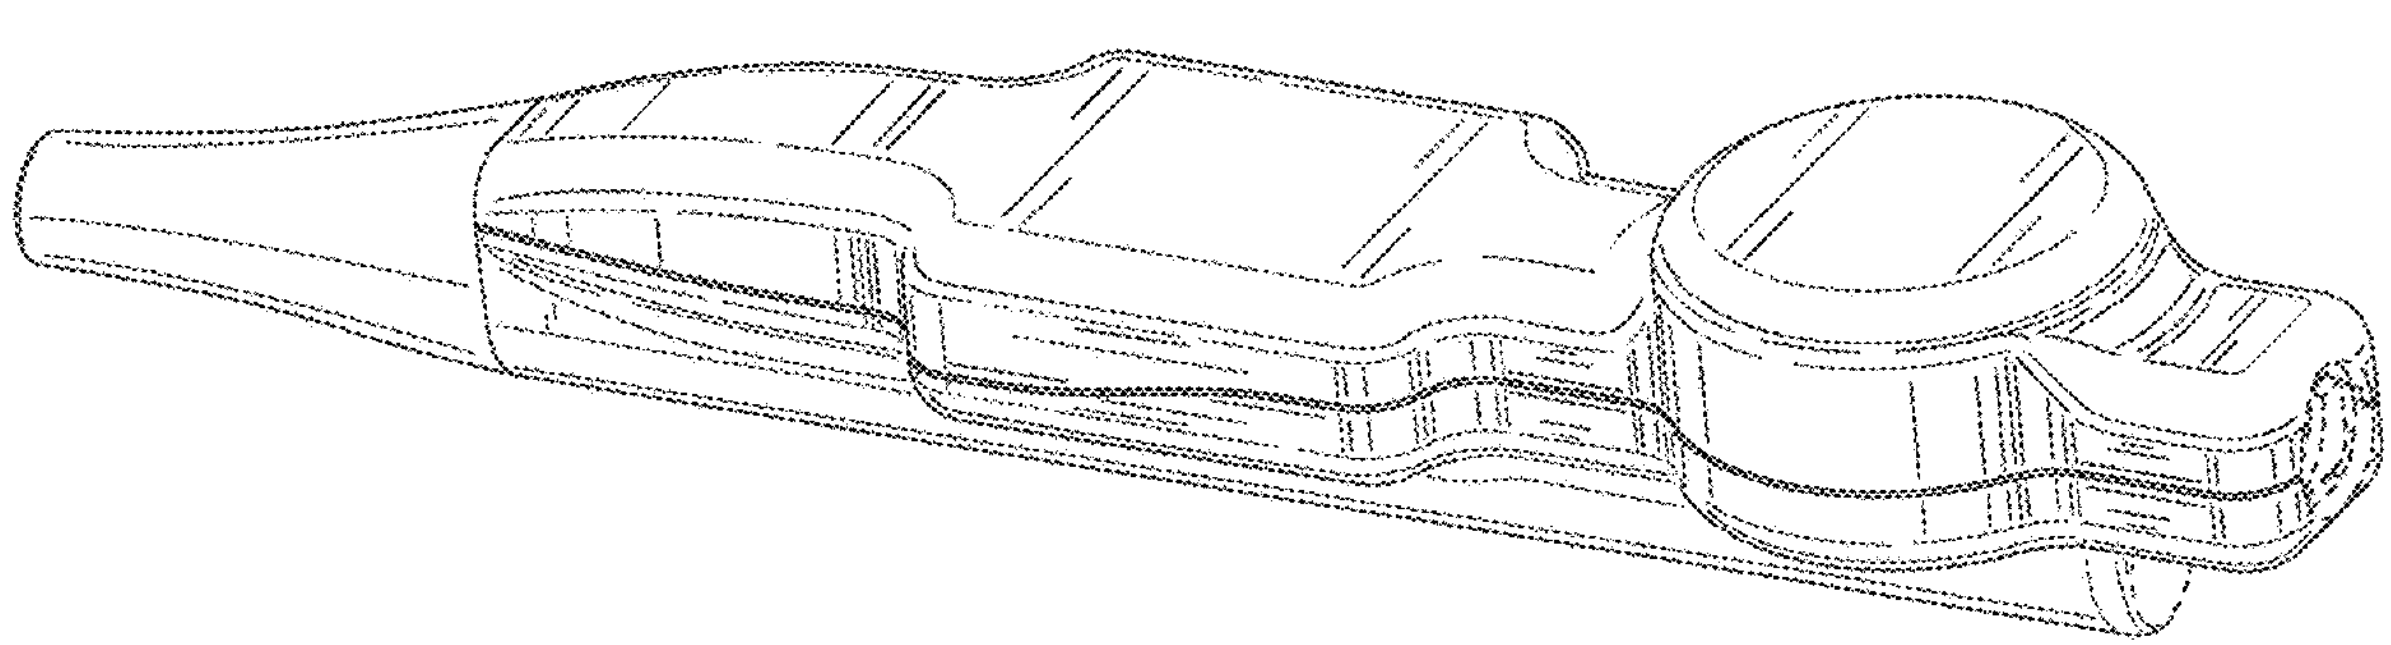

(56) **References Cited**

U.S. PATENT DOCUMENTS

D617,002	S		6/2010	Lundkvist	
D694,879	S		12/2013	Julian et al.	
D708,740	S		7/2014	Osypka et al.	
D715,429	S		10/2014	Yu et al.	
D715,430	S		10/2014	Yu et al.	
D717,427	S		11/2014	Kim et al.	
D718,437	S		11/2014	Osypka	
D726,908	S		4/2015	Yu et al.	
D733,874	S		7/2015	Yu et al.	
D734,457	S		7/2015	Yu et al.	
D747,801	S		1/2016	Kwon et al.	
D751,194	S		3/2016	Yu et al.	
D754,330	S		4/2016	Kim et al.	
D818,583	S		5/2018	Harlev et al.	
D818,584	S		5/2018	Lee et al.	
D827,818	S		9/2018	Hillukka et al.	
D828,548	S		9/2018	Bow	
D879,290	S		3/2020	Harman et al.	
D933,820	S		10/2021	Ota	
D940,889	S		1/2022	Hocking	
D943,092	S		2/2022	Buehrle et al.	
D944,396	S		2/2022	Harris et al.	
D947,375	S	*	3/2022	Norman	D24/112
D961,771	S	*	8/2022	Lee-Sepsick	D24/114
D963,841	S	*	9/2022	Copeland	D24/112
D964,559	S		9/2022	Fujii et al.	
D994,879	S	*	8/2023	Bazdanes	D24/133
D994,880	S	*	8/2023	Bazdanes	D24/133
D995,764	S	*	8/2023	Bazdanes	D24/133
D1,004,086	S	*	11/2023	Melkent	D24/133
D1,035,868	S	*	7/2024	Bazdanes	D24/133
D1,039,687	S	*	8/2024	Nelsen	D24/133
D1,040,341	S	*	8/2024	Kim	D24/133
2014/0276222	A1	*	9/2014	Tegg	A61M 25/0136 600/585
2015/0196736	A1	*	7/2015	Tegg	A61M 25/0136 604/95.04
2017/0049994	A1		2/2017	Truhler et al.	
2021/0046285	A1	*	2/2021	Maekubo	A61M 25/0147
2022/0062587	A1	*	3/2022	Furnish	A61M 25/0147
2023/0404661	A1	*	12/2023	Sakaki	A61B 18/1492

FOREIGN PATENT DOCUMENTS

IL	68679			5/2022
IL	68680	A		5/2022
IL	68681	A		5/2022
JP	D1498923			6/2014
JP	D1599365	S		3/2018
JP	D1612251			8/2018
JP	1671048	S		10/2020
KR	3010923210000			1/2021
TW	D199557			9/2019
TW	226134-0001		*	6/2023

OTHER PUBLICATIONS

The Advisor™ VL Mapping Catheter, Sensor Enabled™, Abbott, [post date unknown], [Site seen: Apr. 24, 2025], Seen at URL: https://www.cardiovascular.abbott/us/en/hcp/products/electrophysiology/diagnostic-catheters/advisor-vl-fl/about.html (Year: 2025).*

Thermedical® Ablation System , Thermomedical, thermodmedical .com, [Post date unknown], [Site seen Feb. 16, 2023], Seen at URL: https://www.thermedical.com/the-products (Year: 2023).

"Steerocath-Dx™ , Boston Scientific, [Post Date: unknown], [Site seen Nov. 14, 2023],", URL: https://www.watchman.com/content/dam/bostonscientific/ep/portfolio-group/catheters-diagnostic/Steerable%20Catheters/STEEROCA TH%20Dx/Resources/Spec%20Sheet%20-%20STEEROCATH%20DX%20. pdf (Year: 2023).

* cited by examiner

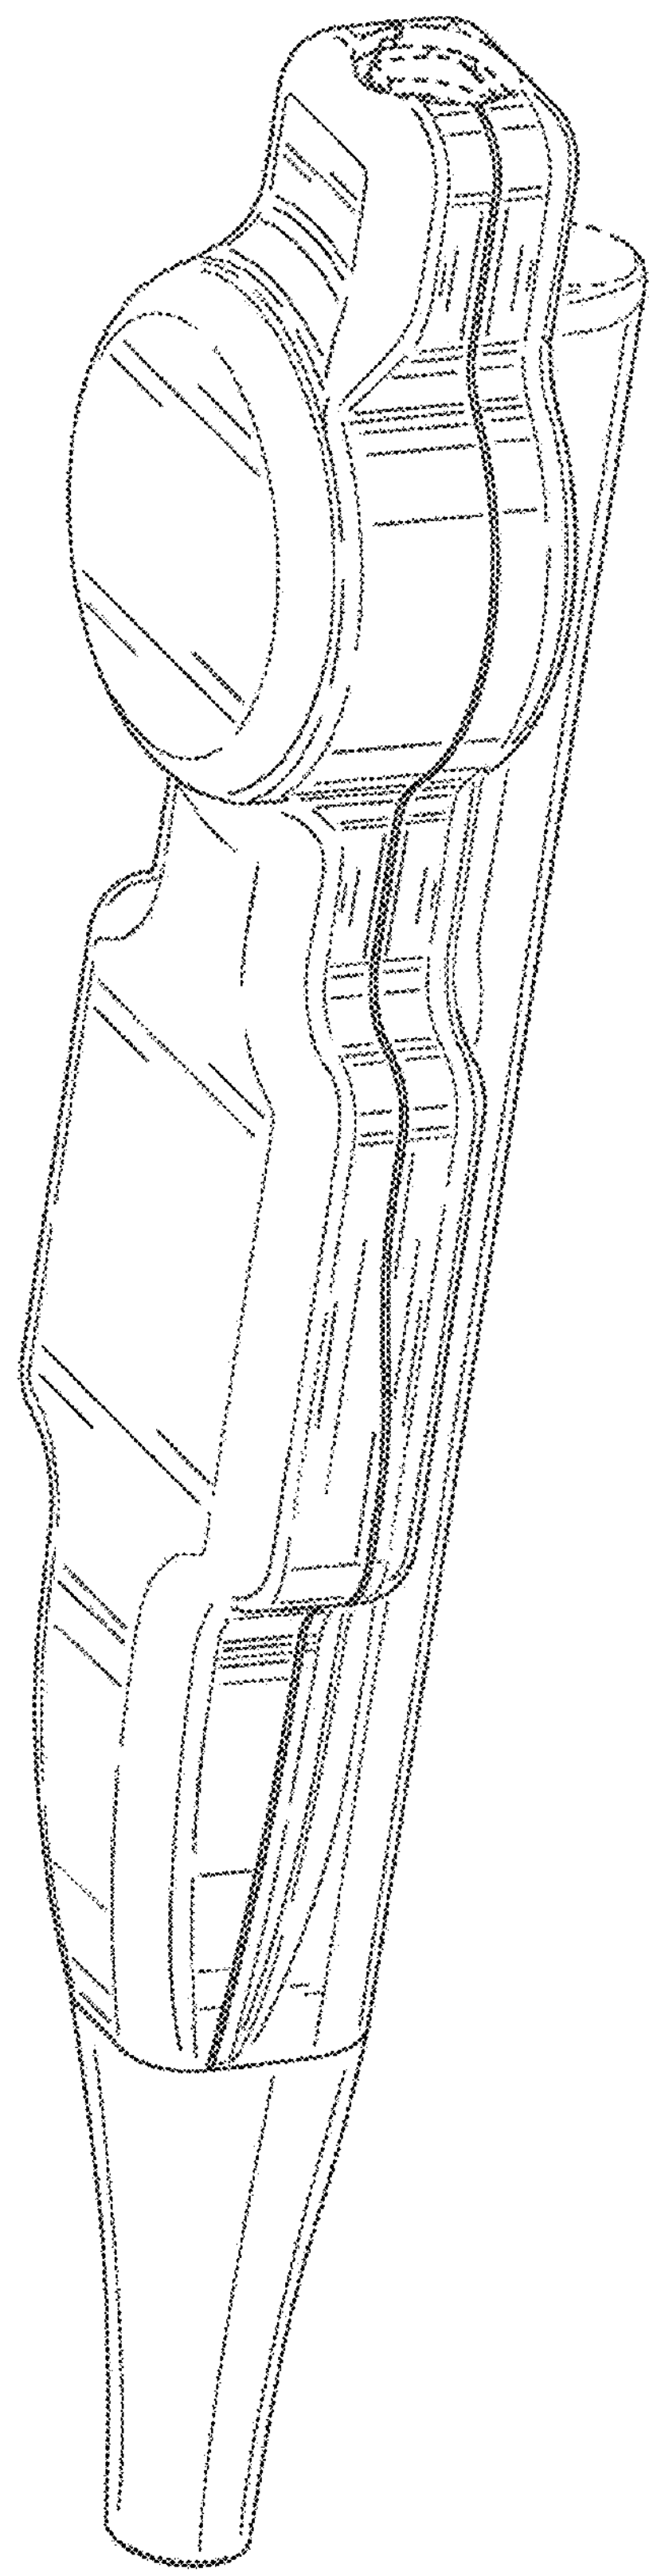

FIG. 1

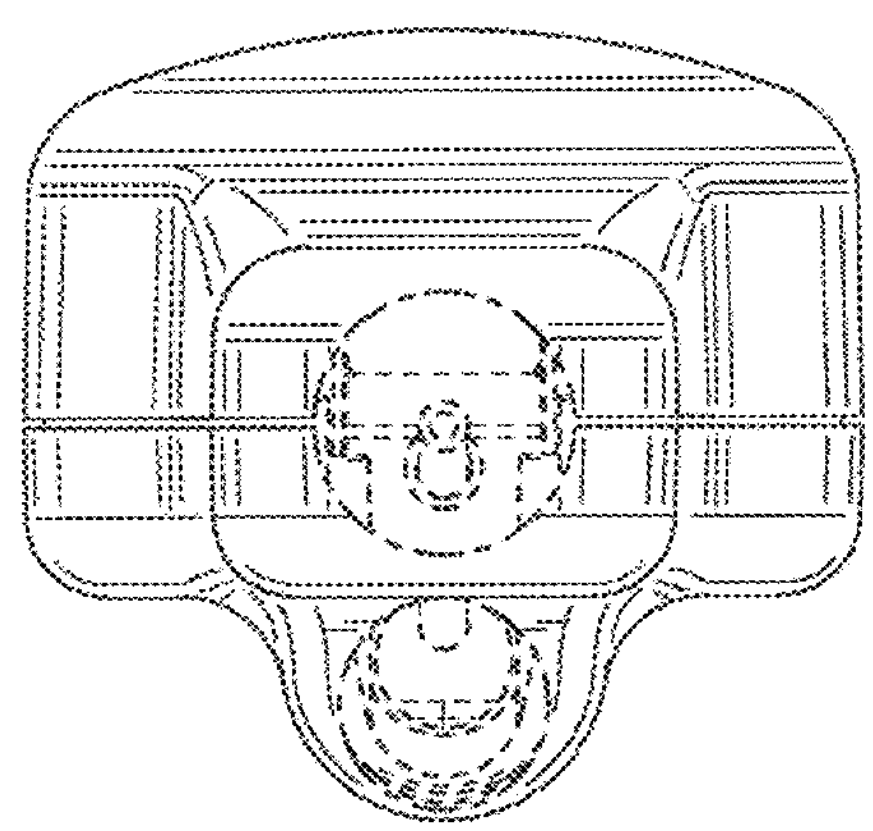

FIG. 2

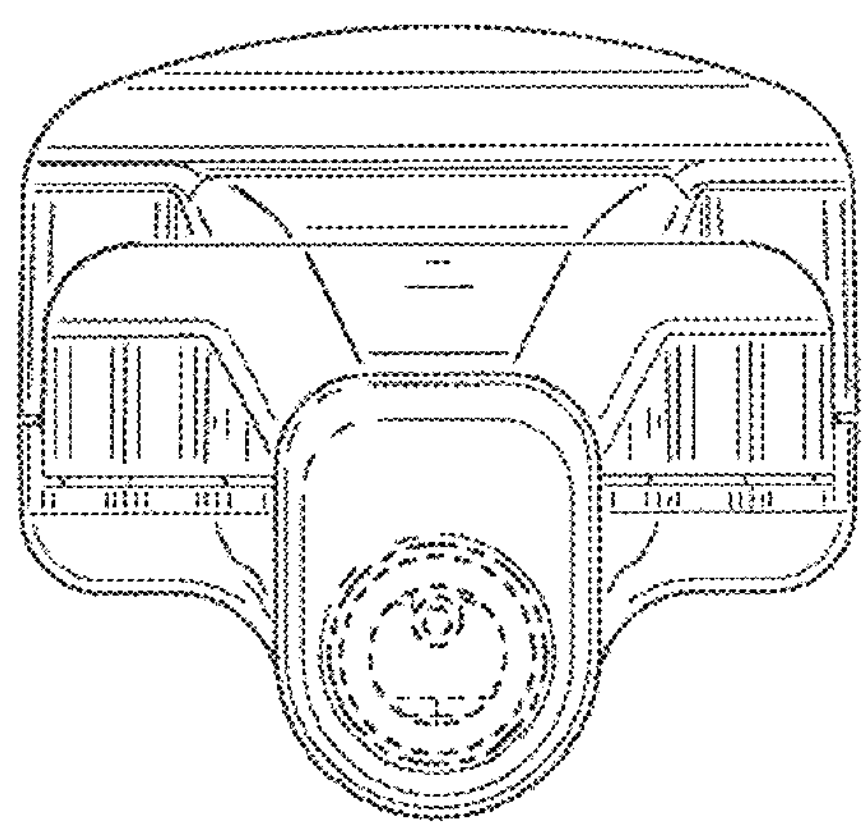

FIG. 3

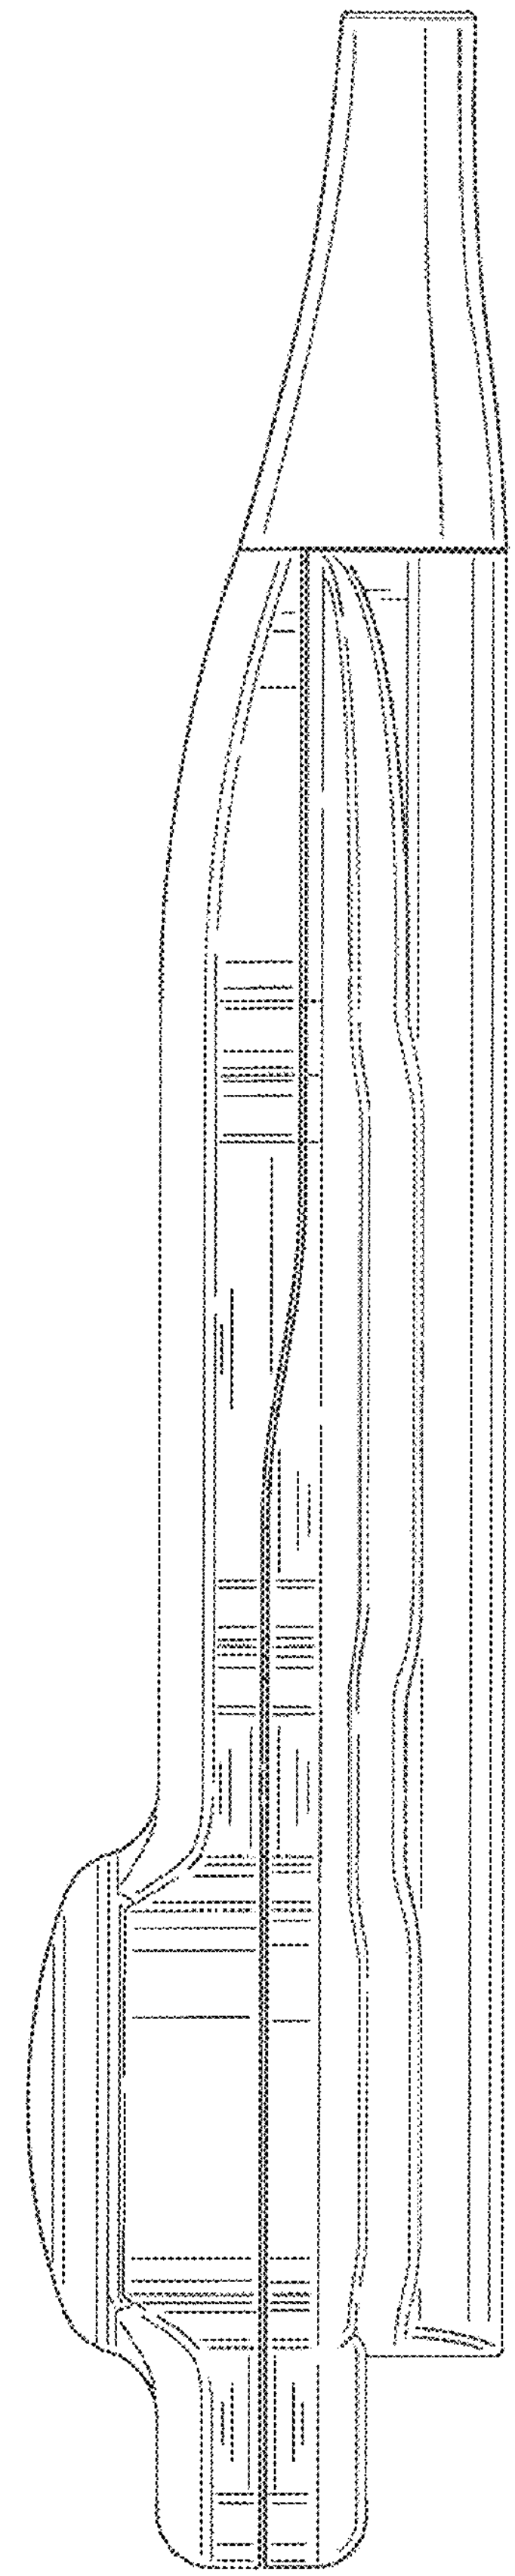

FIG. 4

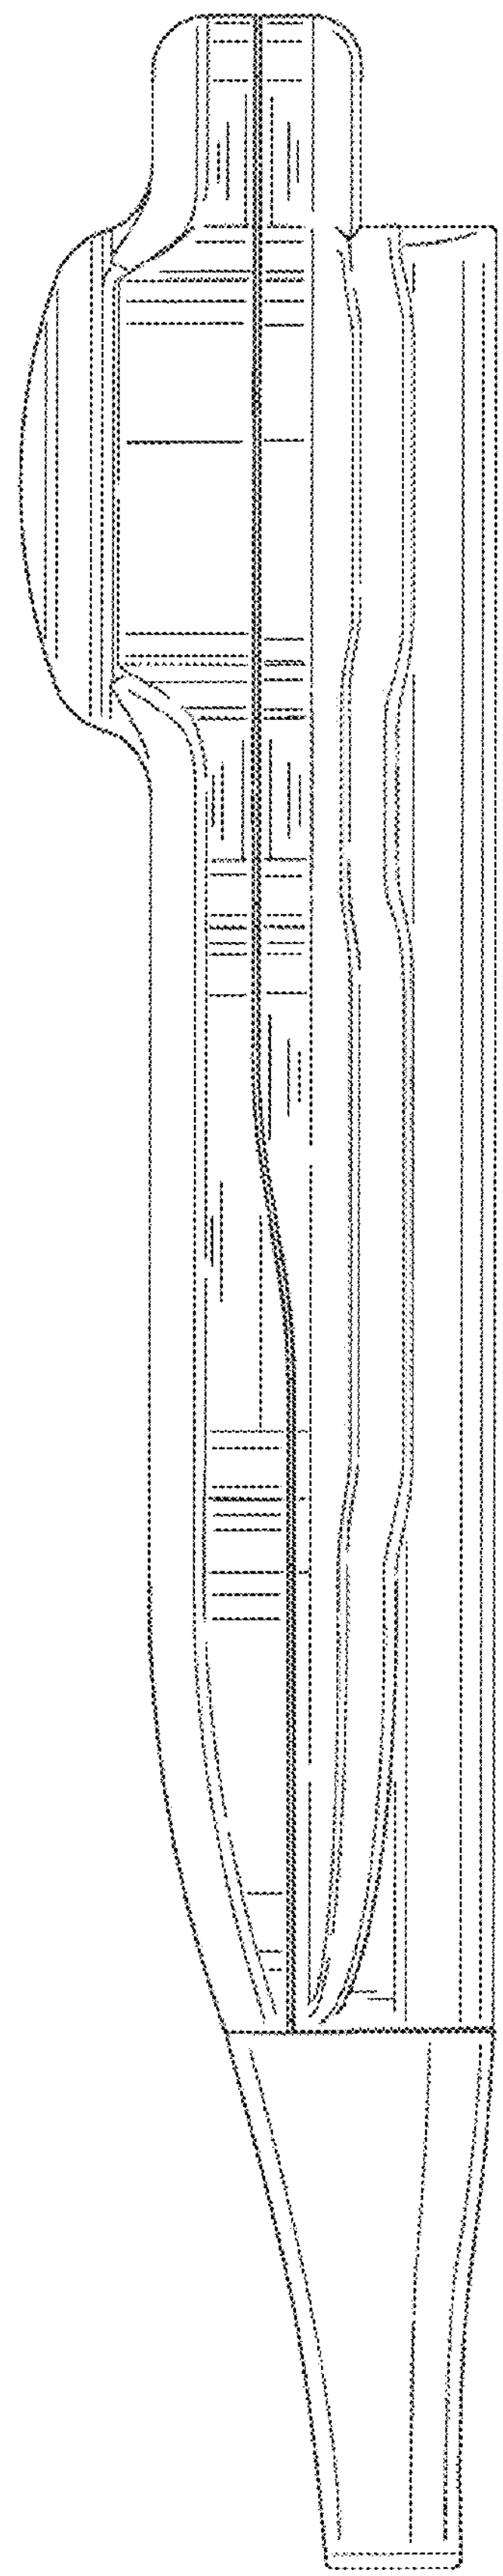

FIG. 5

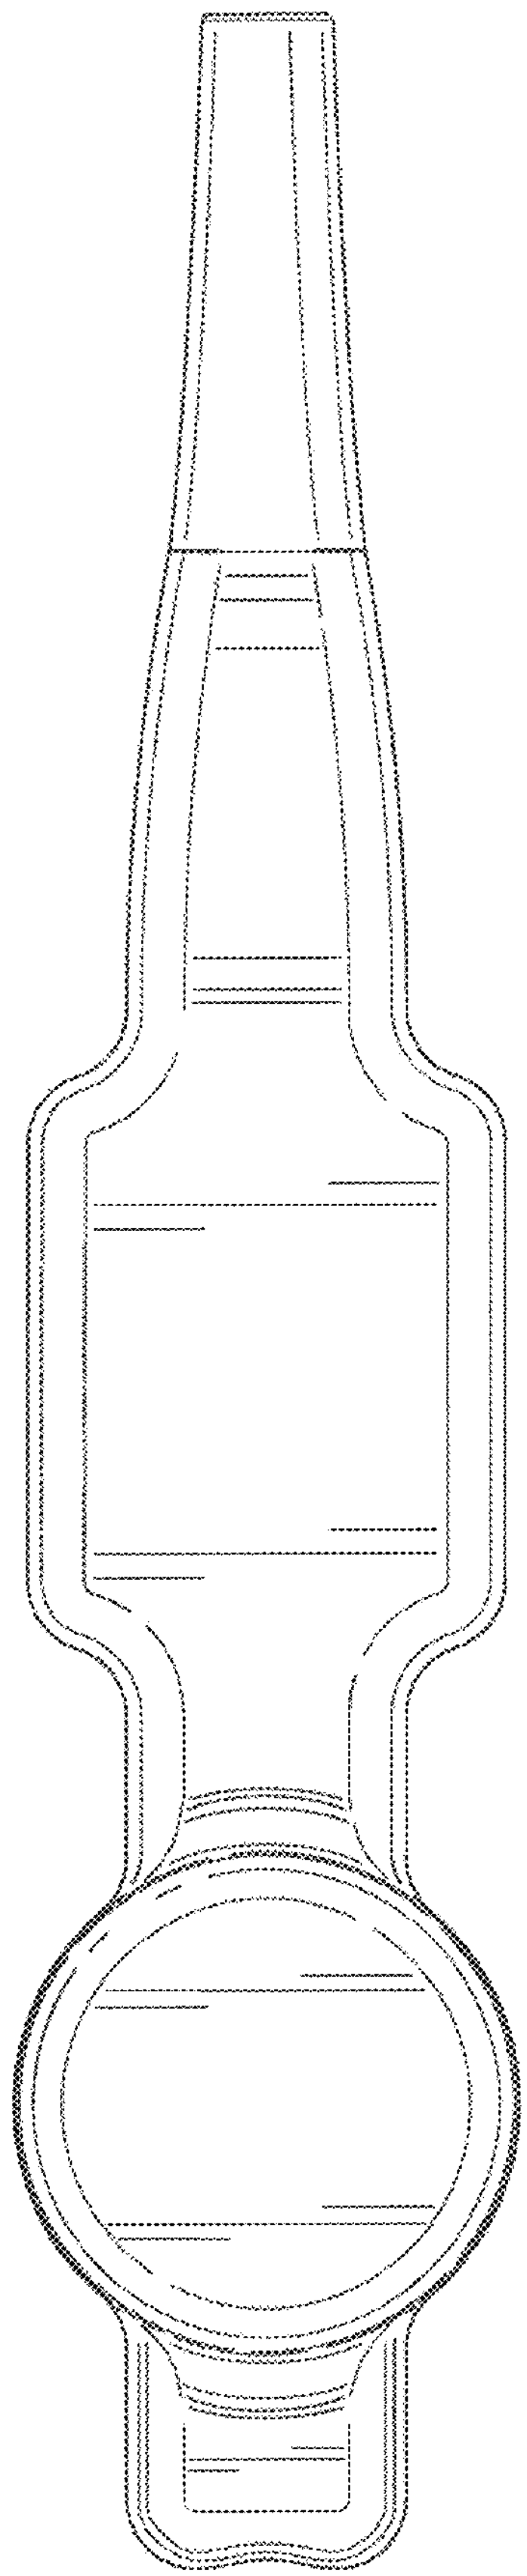

FIG. 6

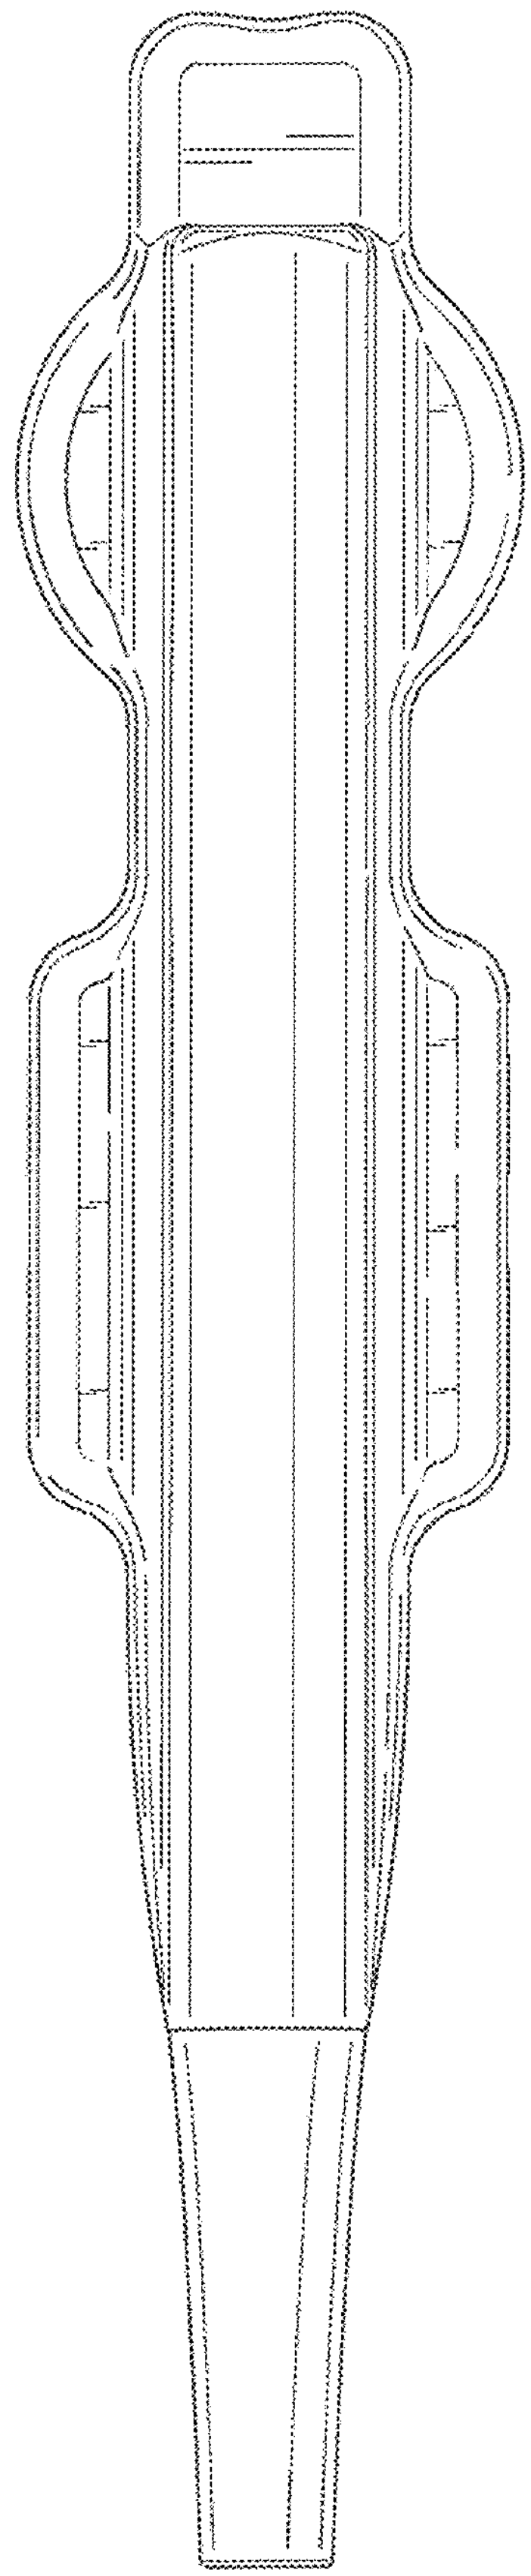

FIG. 7

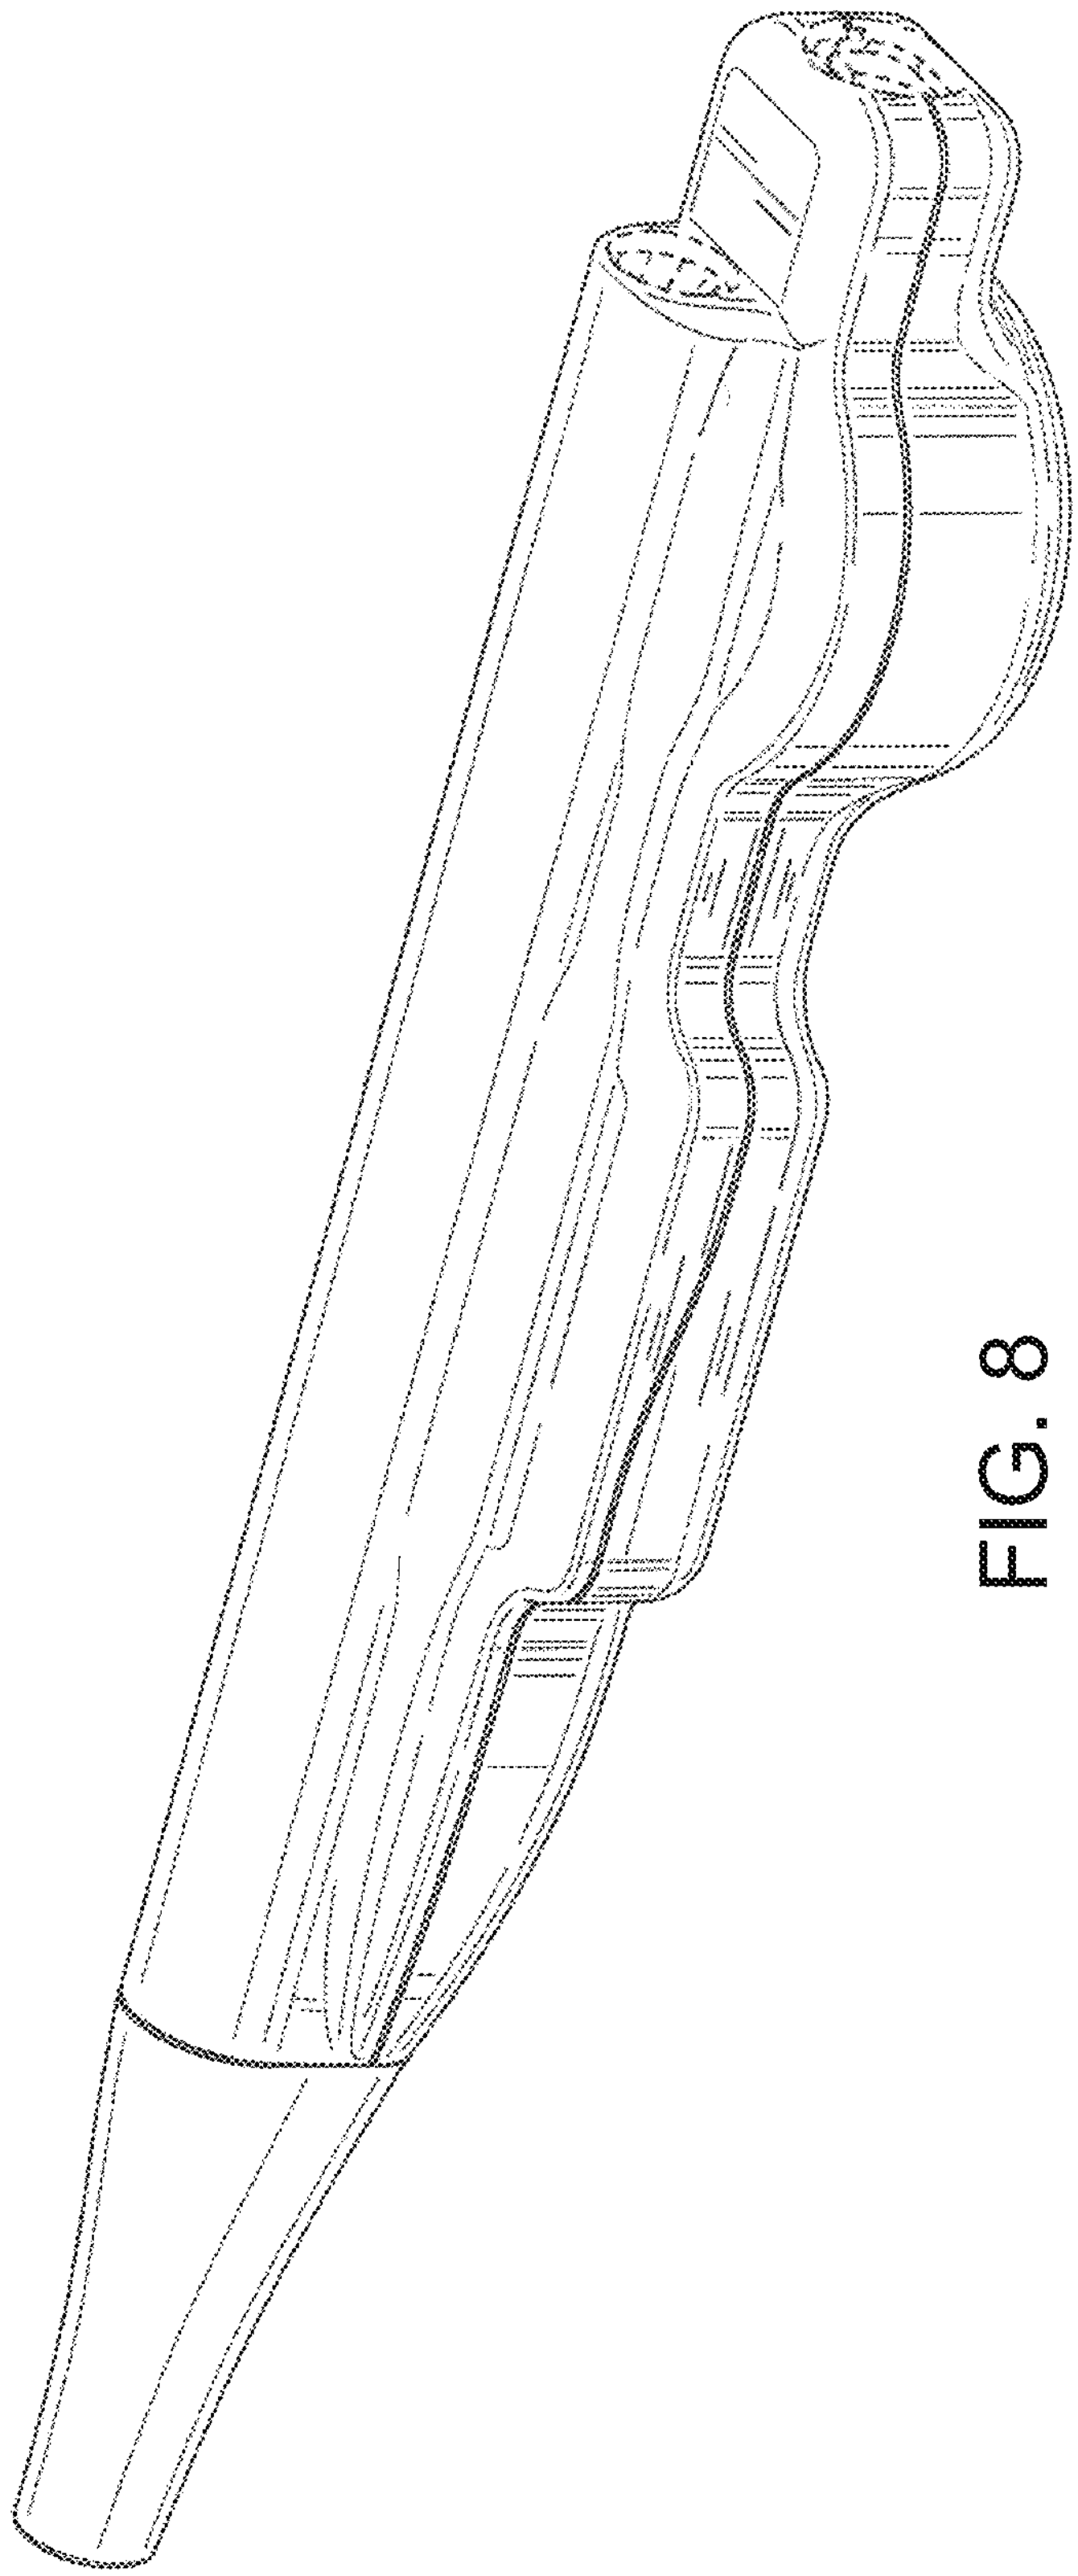

FIG. 8