US00D1090852S

(12) **United States Design Patent** (10) **Patent No.: US D1,090,852 S**

Karpowitz et al. (45) **Date of Patent: ** Aug. 26, 2025**

(54) **DENTAL KEYWAY DEVICE**

(71) Applicant: **MERIT CABOT, LLC**, Scottsdale, AZ (US)

(72) Inventors: **Cameron Karpowitz**, San Clemente, CA (US); **Dicken Smith**, Holladay, UT (US)

(73) Assignee: **MERIT CABOT, LLC**, Scottsdale, AZ (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/884,723**

(22) Filed: **Feb. 15, 2023**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/181**

(58) **Field of Classification Search**
USPC D24/152, 153, 154, 155, 156, 176, 178, D24/179, 180, 181, 182
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,906,186 A	*	3/1990	France, Jr.	A61C 13/1016 433/196
5,788,489 A		8/1998	Huffman	

(Continued)

FOREIGN PATENT DOCUMENTS

EM	015028275-0004	*	9/2023
KR	300961768		7/2018

OTHER PUBLICATIONS

Elos Medtech, "How Digital Dentistry Can Help Simplify The Digital Workflow", first available Jan. 18, 2016. (https://elosmedtech.com/how-digital-dentistry-can-help-simplify-the-digital-workflow/) (Year: 2016).*

(Continued)

Primary Examiner — Leanne Was-Englehart
Assistant Examiner — Justin A Johnson
(74) *Attorney, Agent, or Firm* — The Small Patent Law Group LLC; Christopher R. Carroll

(57) **CLAIM**

The ornamental design for a dental keyway device, as shown.

DESCRIPTION

FIG. **1** is a perspective view of a dental keyway device, showing our new design;
FIG. **2** is a top plan view of the dental keyway device shown in FIG. **1**;
FIG. **3** is a bottom plan view of the dental keyway device shown in FIG. **1**;
FIG. **4** is a first side elevation view of the dental keyway device shown in FIG. **1**;
FIG. **5** is a second side elevation view of the dental keyway device shown in FIG. **1**;
FIG. **6** is a front elevation view of the dental keyway device shown in FIG. **1**;
FIG. **7** is a rear elevation view of the dental keyway device shown in FIG. **1**;
FIG. **8** is a perspective view of a dental keyway device, showing our new design;
FIG. **9** is a top plan view of the dental keyway device shown in FIG. **8**;
FIG. **10** is a bottom plan view of the dental keyway device shown in FIG. **8**;
FIG. **11** is a first side elevation view of the dental keyway device shown in FIG. **8**;
FIG. **12** is a second side elevation view of the dental keyway device shown in FIG. **8**;
FIG. **13** is a front elevation view of the dental keyway device shown in FIG. **8**;
FIG. **14** is a rear elevation view of the dental keyway device shown in FIG. **8**;
FIG. **15** is a perspective view of a dental keyway device, showing our new design;

(Continued)

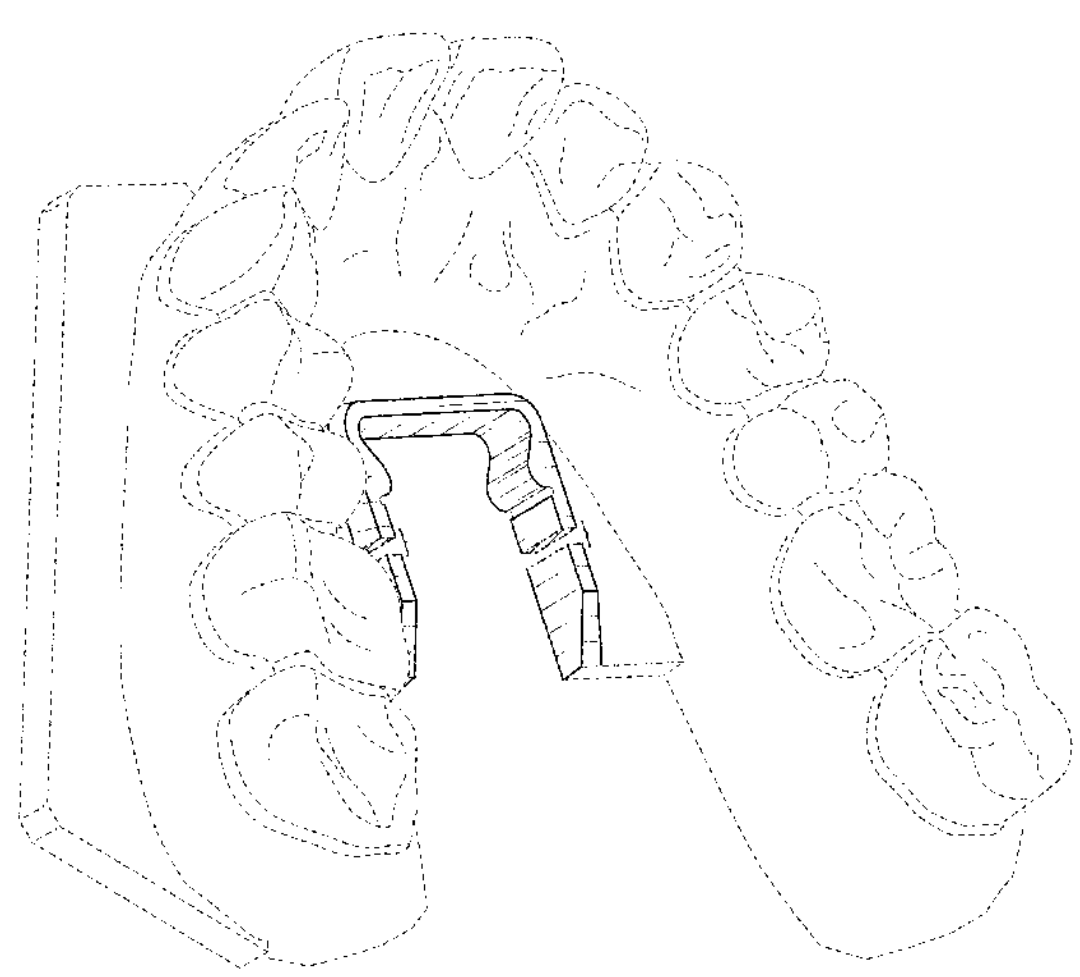

FIG. **16** is a top plan view of the dental keyway device shown in FIG. **15**;
FIG. **17** is a bottom plan view of the dental keyway device shown in FIG. **15**;
FIG. **18** is a first side elevation view of the dental keyway device shown in FIG. **15**;
FIG. **19** is a second side elevation view of the dental keyway device shown in FIG. **15**;
FIG. **20** is a front elevation view of the dental keyway device shown in FIG. **15**;
FIG. **21** is a rear elevation view of the dental keyway device shown in FIG. **15**;
FIG. **22** is a perspective view of a dental keyway device, showing our new design;
FIG. **23** is a top plan view of the dental keyway device shown in FIG. **22**;
FIG. **24** is a bottom plan view of the dental keyway device shown in FIG. **22**;
FIG. **25** is a first side elevation view of the dental keyway device shown in FIG. **22**;
FIG. **26** is a second side elevation view of the dental keyway device shown in FIG. **22**;
FIG. **27** is a front elevation view of the dental keyway device shown in FIG. **22**; and,
FIG. **28** is a rear elevation view of the dental keyway device shown in FIG. **22**.
The dash-dash broken lines represent environmental structure that is not part of the design sought to be patented. The drawings contain a symbolic break indicated by dot-dash-dot break lines. The portion between the break lines forms no part of the claimed design.

1 Claim, 20 Drawing Sheets

(58) **Field of Classification Search**
CPC .. A61C 1/00; A61C 1/08; A61C 1/084; A61C 1/16; A61C 3/00; A61C 3/08; A61C 5/00; A61C 5/007; A61C 5/20; A61C 5/30; A61C 5/70; A61C 7/00; A61C 8/0001; A61C 8/0054; A61C 8/008; A61C 8/0081; A61C 8/0083; A61C 2008/0084; A61C 8/0087; A61C 8/0089; A61C 8/0096; A61C 9/00; A61C 9/0006; A61C 19/008; A61C 19/02; A61C 7/002; A61C 7/08; A61C 9/004; A61K 6/00
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,788,490	A	8/1998	Huffman	
D399,319	S *	10/1998	Andrews	D24/181
6,497,574	B1 *	12/2002	Miller	A61C 9/0046 433/213
D582,558	S *	12/2008	Schulz	D24/181
8,360,772	B1 *	1/2013	McCarthy	A61C 9/0006 433/41
D951,458	S *	5/2022	Karpowitz	D24/181
2002/0164556	A1	11/2002	Huffman	
2004/0265769	A1 *	12/2004	Inman	A61C 7/00 433/21
2005/0106530	A1	5/2005	Huffman	
2006/0093992	A1	5/2006	Wen	
2006/0127851	A1	6/2006	Wen	
2006/0127853	A1	6/2006	Wen	
2006/0199153	A1	9/2006	Liu et al.	
2008/0318179	A1	12/2008	Liu	
2009/0286196	A1	11/2009	Wen et al.	
2010/0143855	A1 *	6/2010	Scheffler	A61C 7/00 433/6
2010/0279245	A1 *	11/2010	Navarro	A61C 7/08 433/10
2014/0024003	A1 *	1/2014	Iwaki	G09B 23/283 434/263
2014/0272797	A1 *	9/2014	Prestipino	A61C 8/0048 433/199.1
2019/0374305	A1 *	12/2019	Wang	A61C 1/084
2020/0352765	A1 *	11/2020	Lin	A63B 23/032
2021/0121270	A1	4/2021	Such Palacios	

OTHER PUBLICATIONS

Roland, "5-Axis Dental Mill", first available Feb. 2018. (https://public.rolanddga.com/brochures/products/dental/DWX-52D_Brochure.pdf) (Year: 2018).*
Youtube, "KeyMill High-Impact Denture Base Disc", first available Oct. 15, 2019. (youtube.com/watch?v=ZuXor-t-gGc) (Year: 2019).*
Digital Dental, "Mills", first available Aug. 5, 2020. (https://web.archive.org/web/20200805134555/https:/digitaldental.com/mills/) (Year: 2020).*
Youtube, "KeyMill High-Impact Denture Base Dise", first available Oct. 15, 2019. (youtube.com/watch?v=ZuXor-t-gGc) (Year: 2019).

* cited by examiner

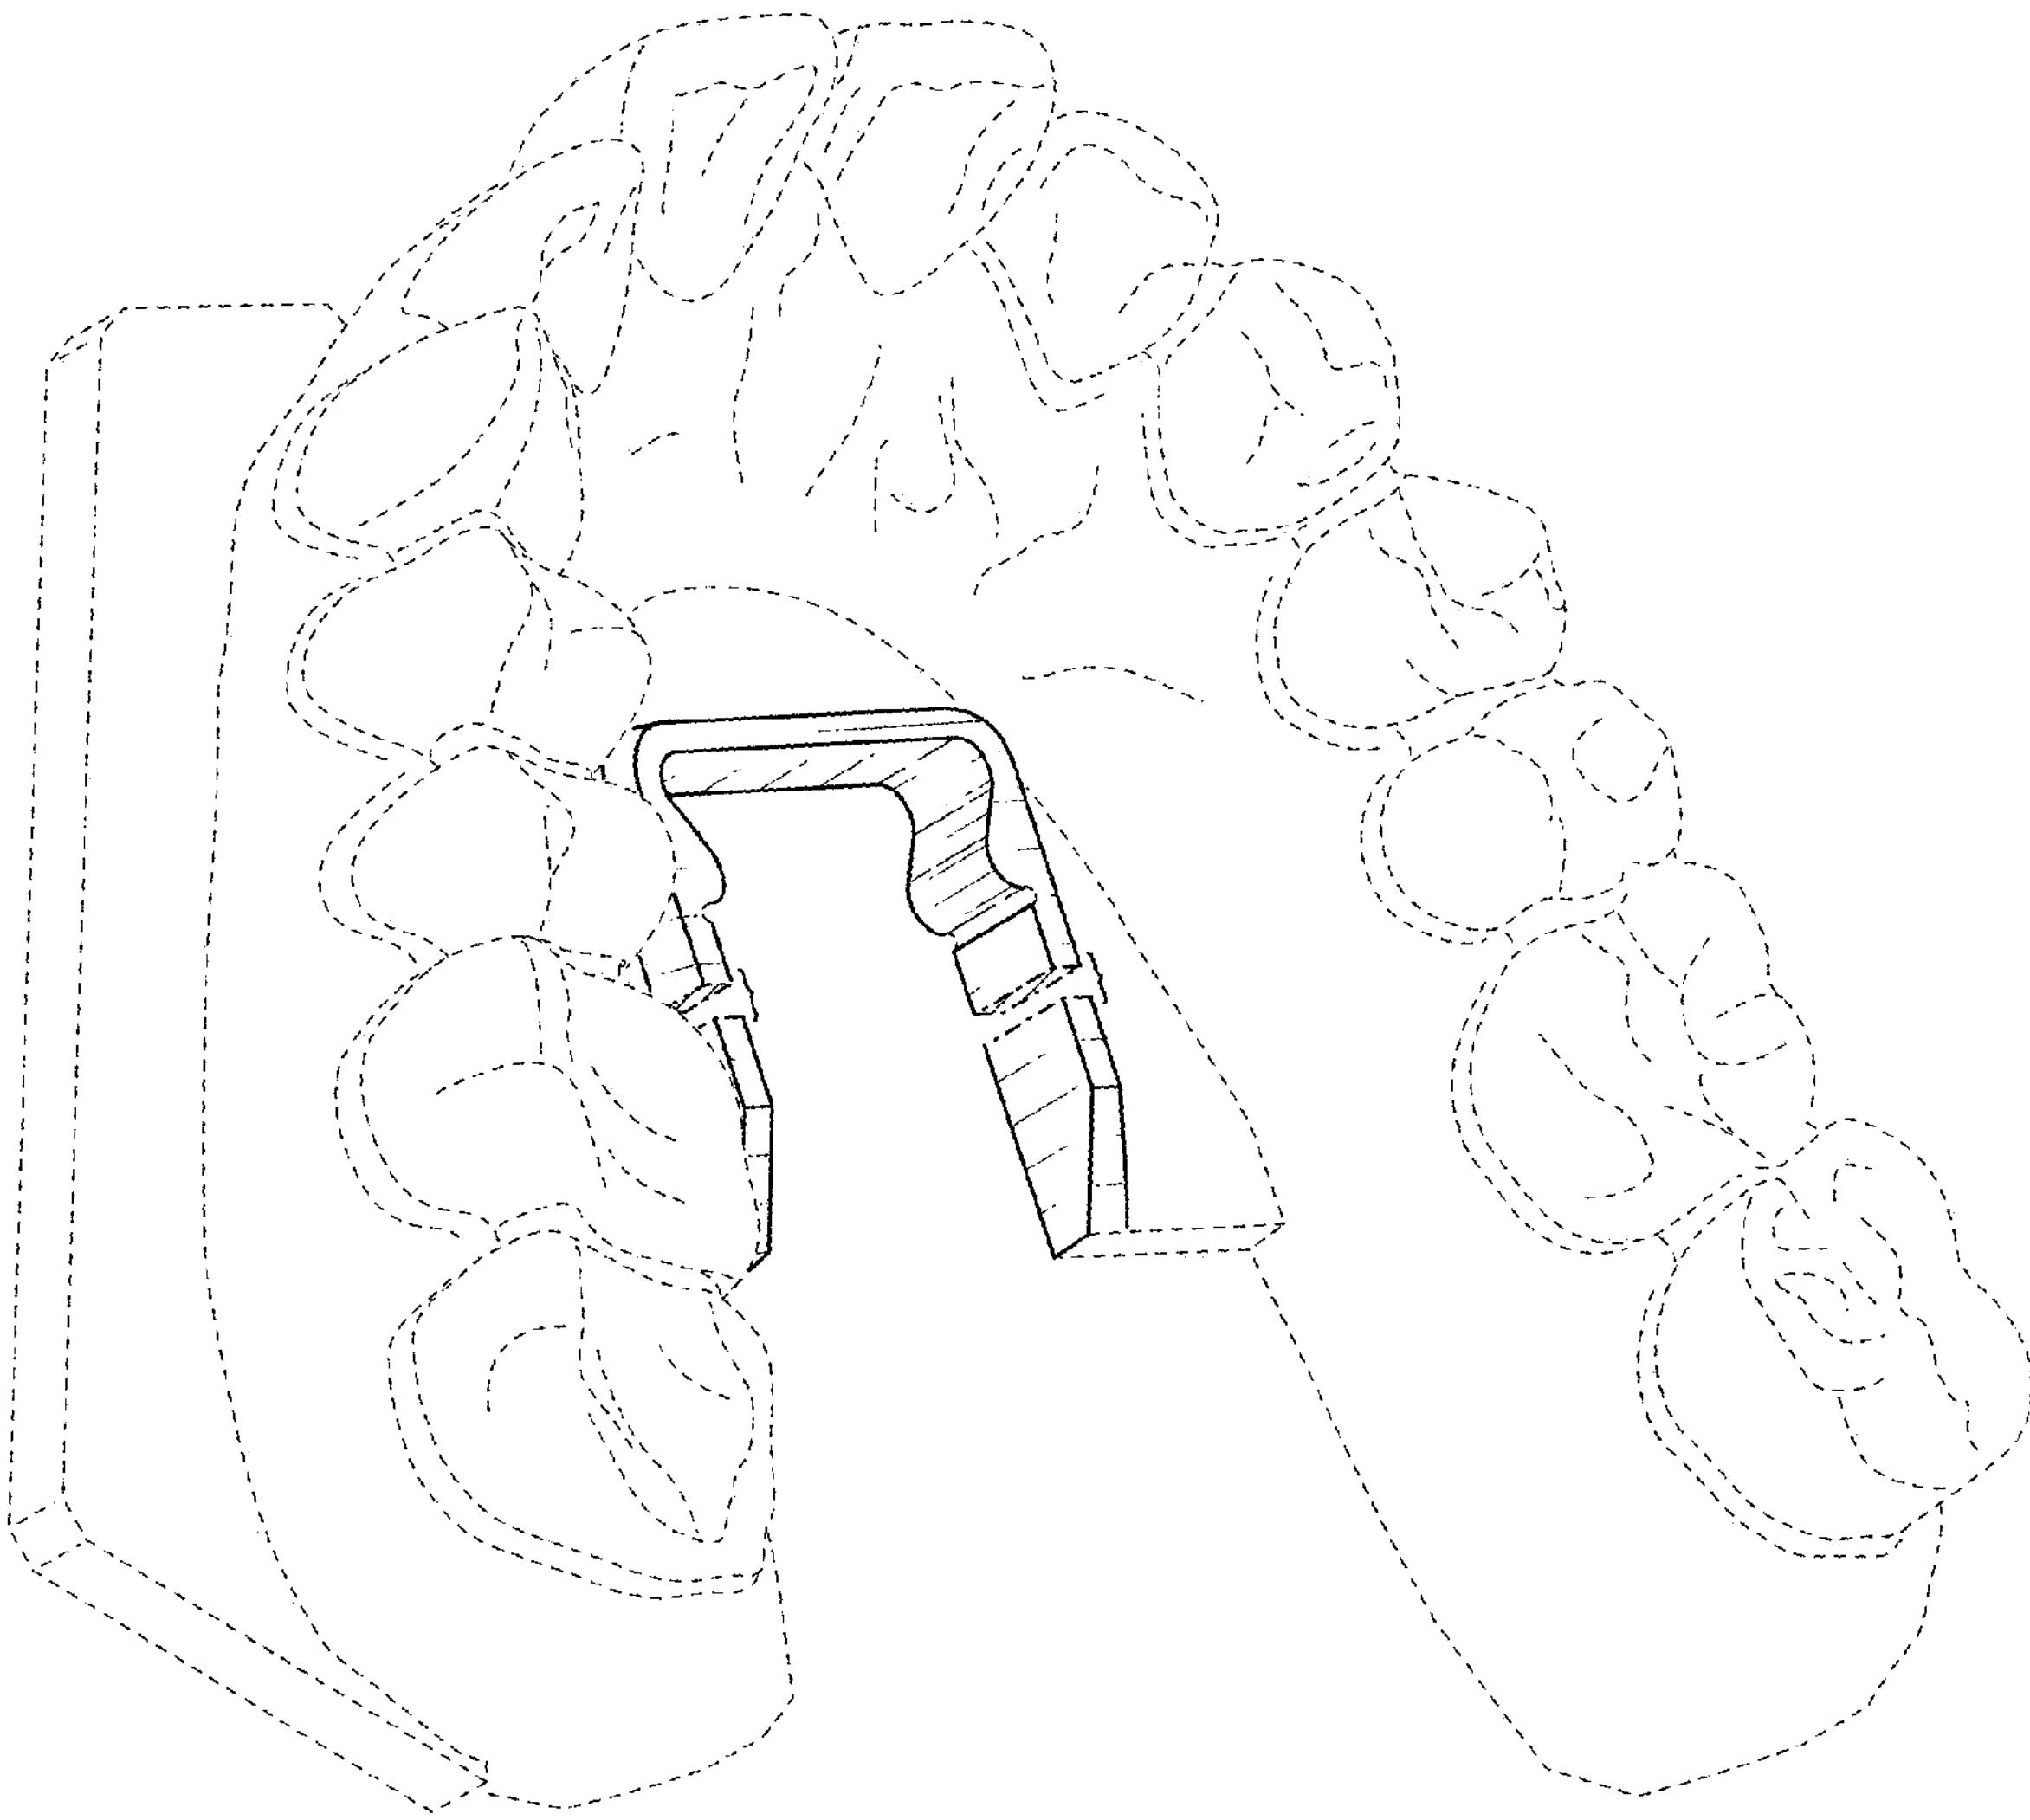

FIG. 1

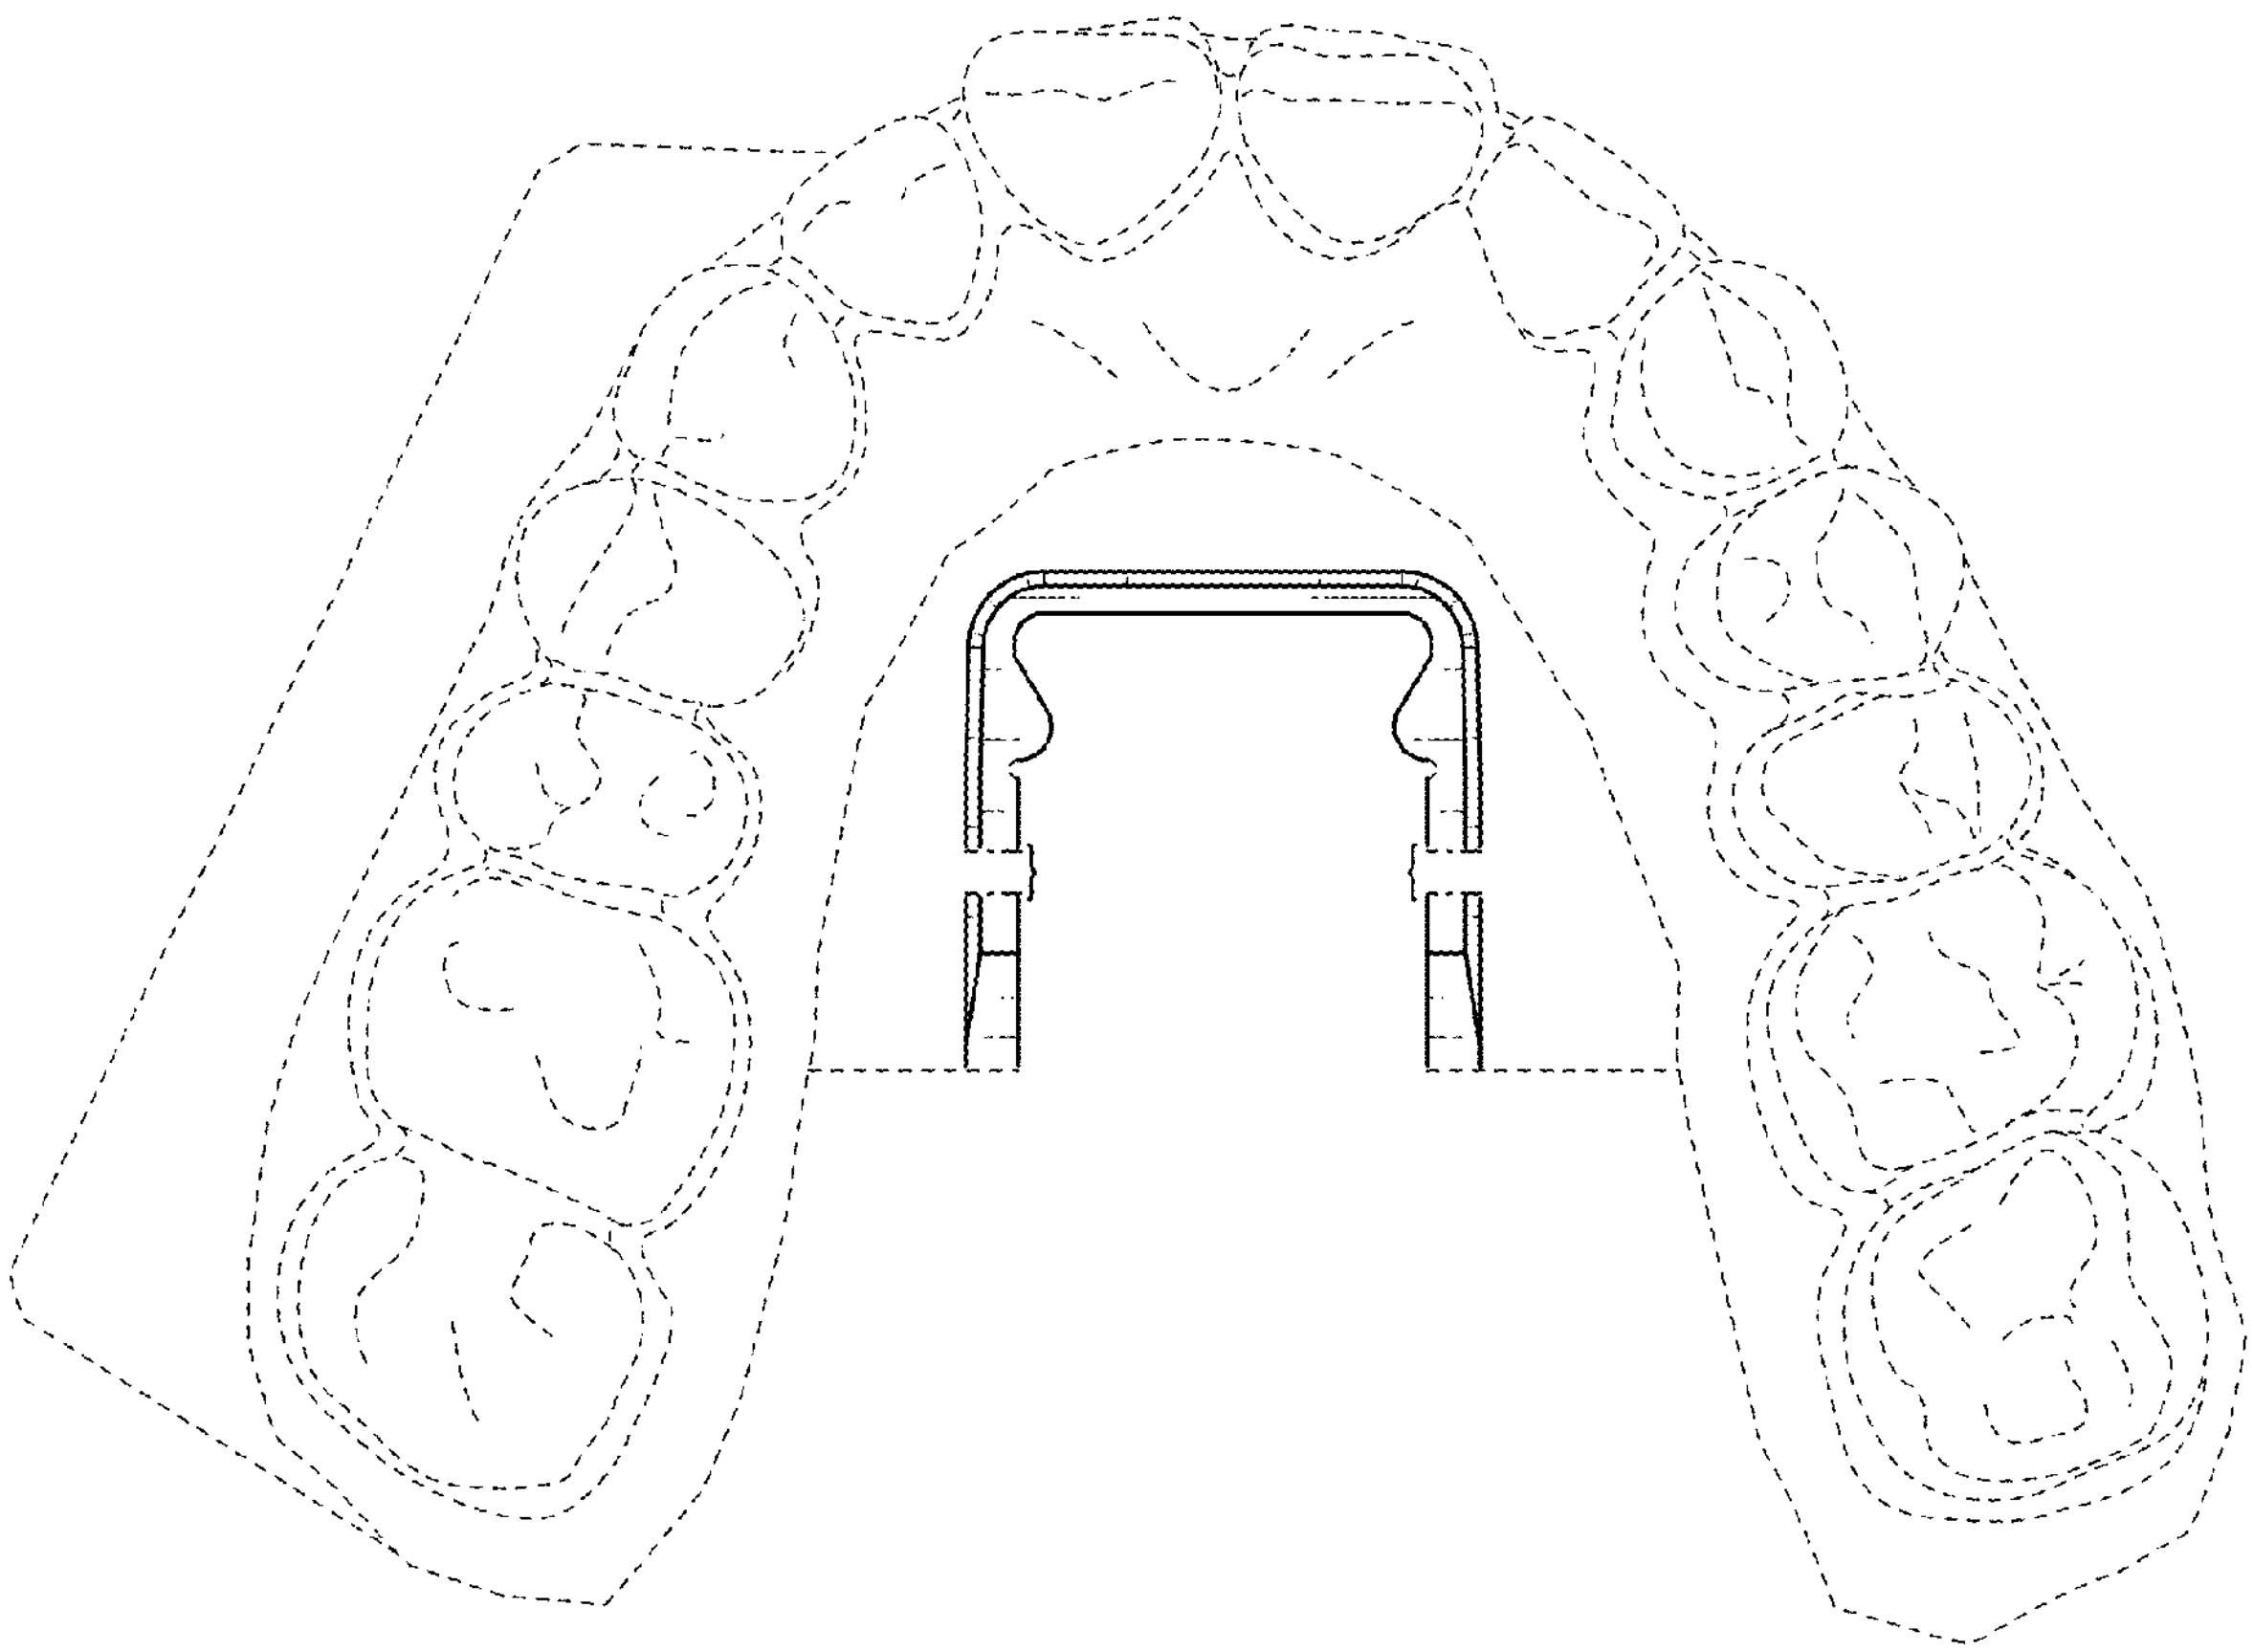

FIG. 2

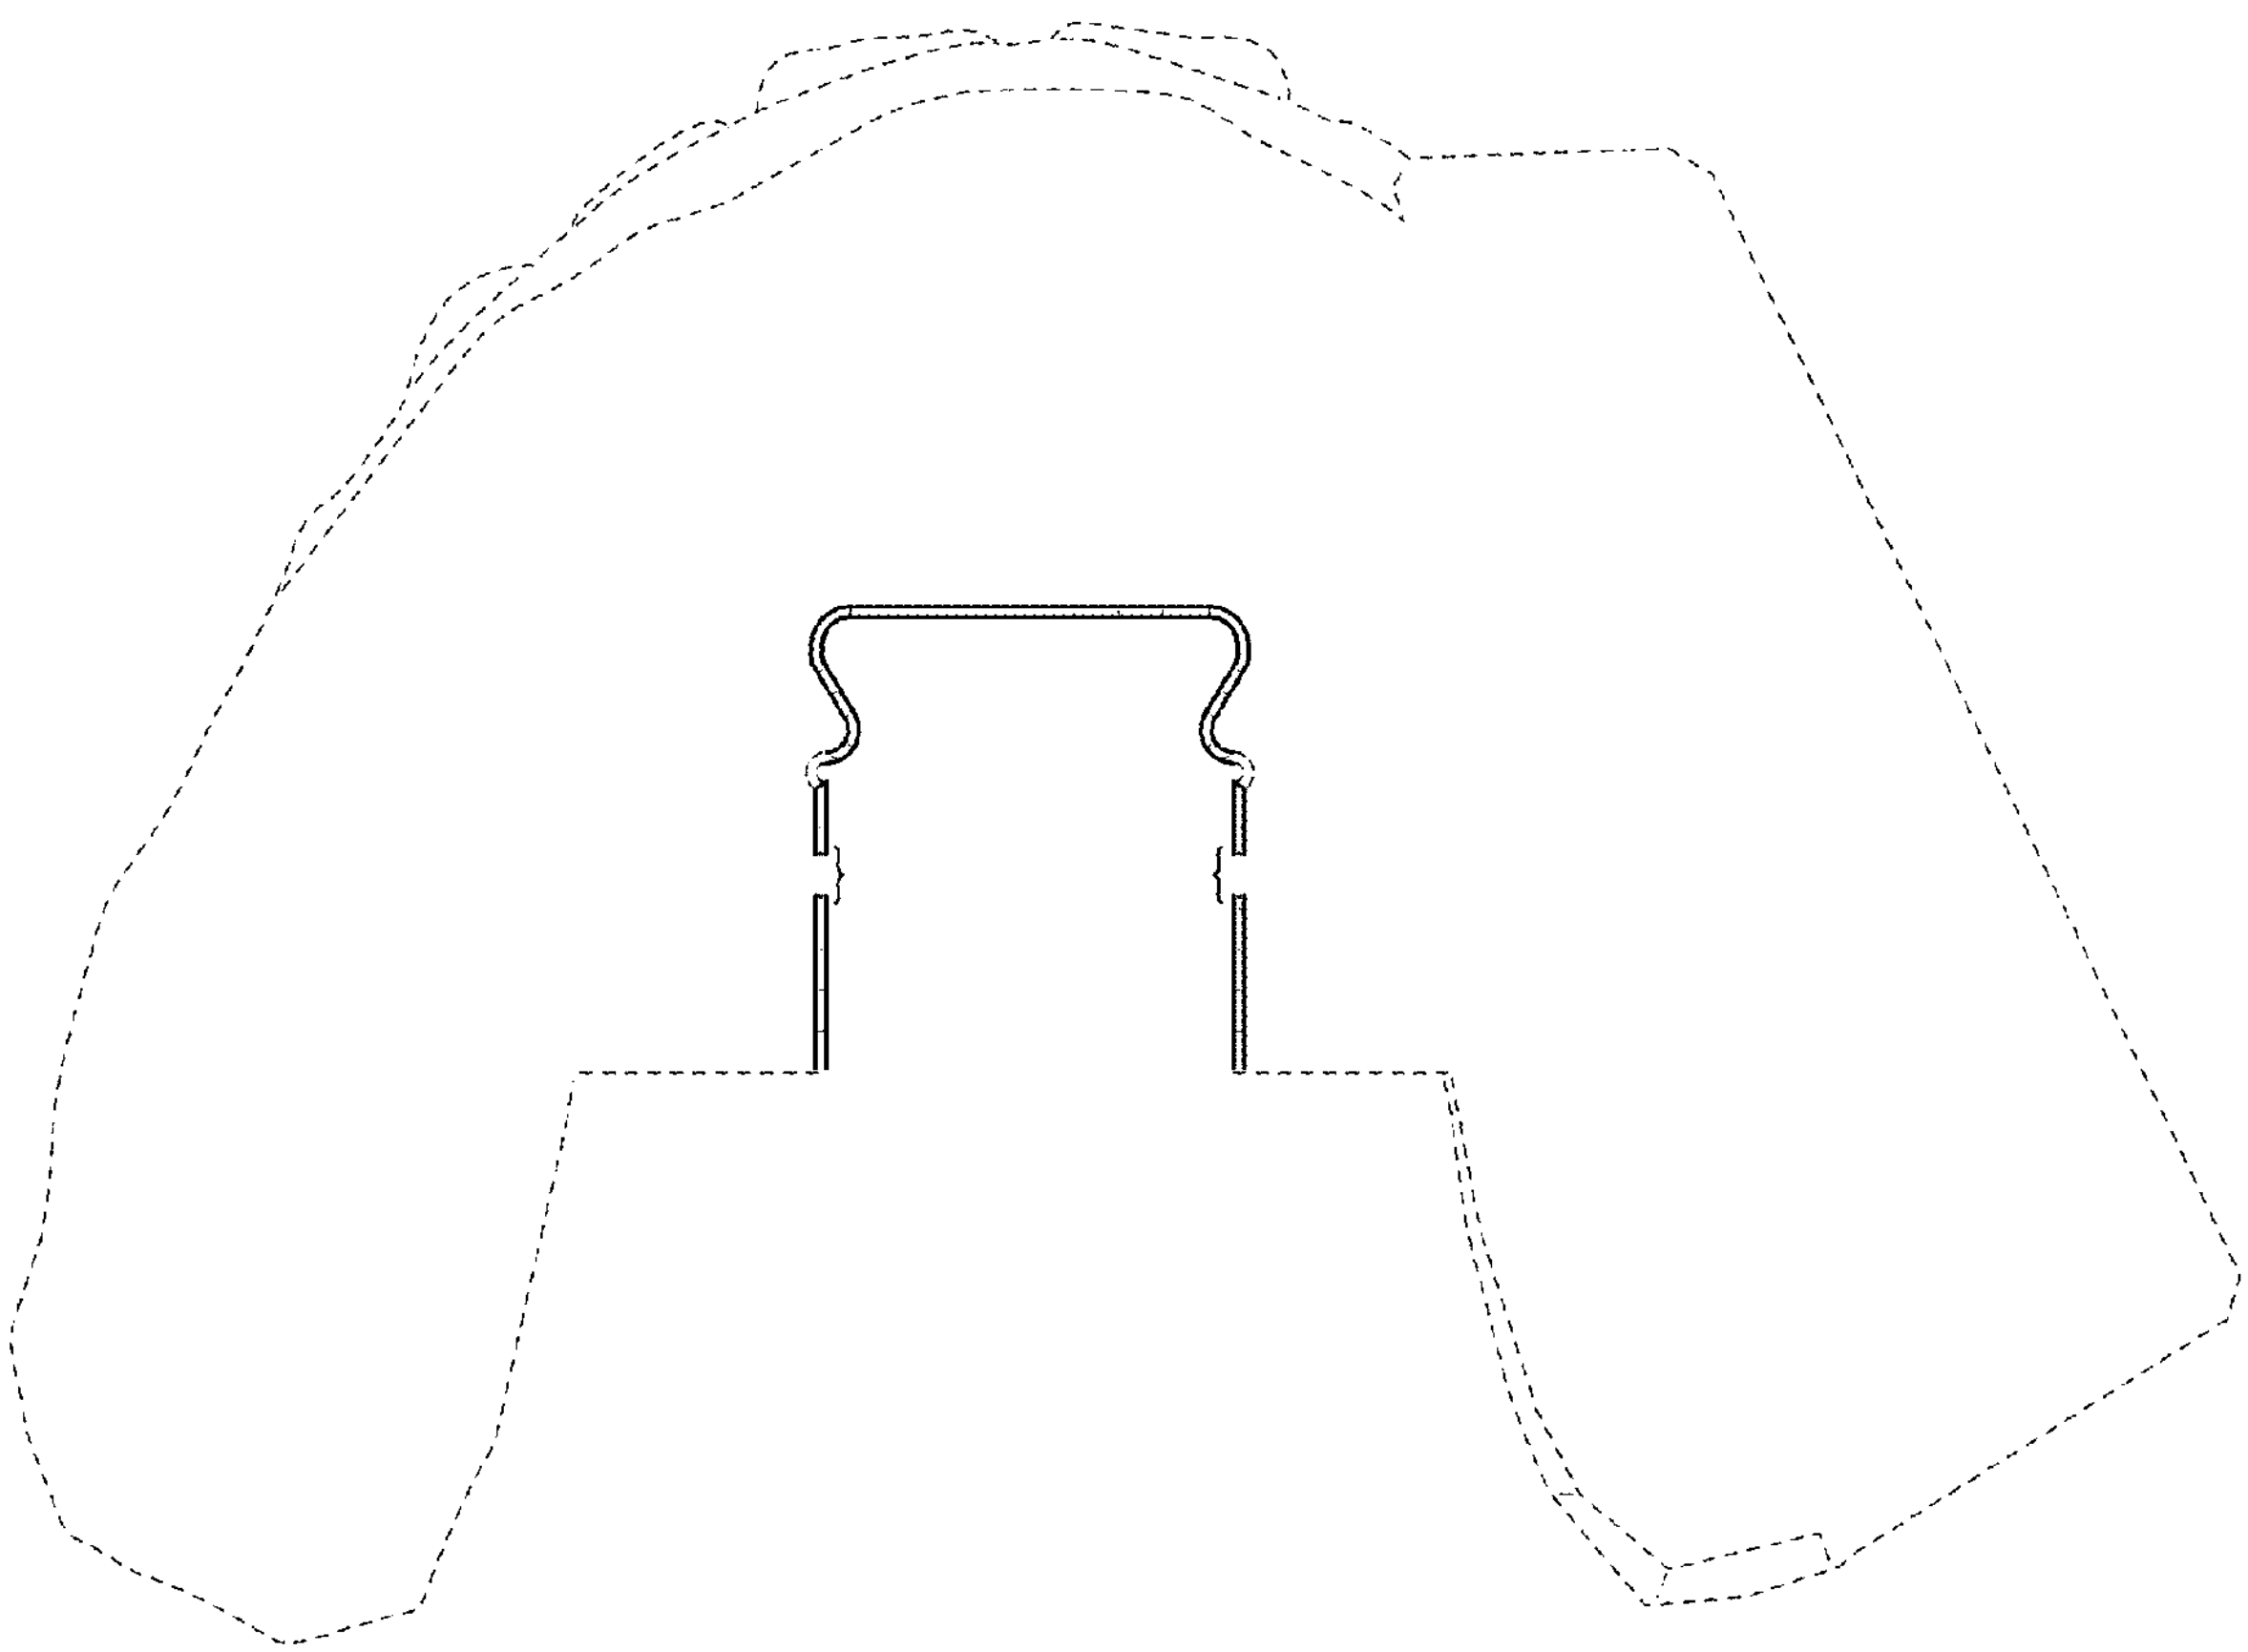

FIG. 3

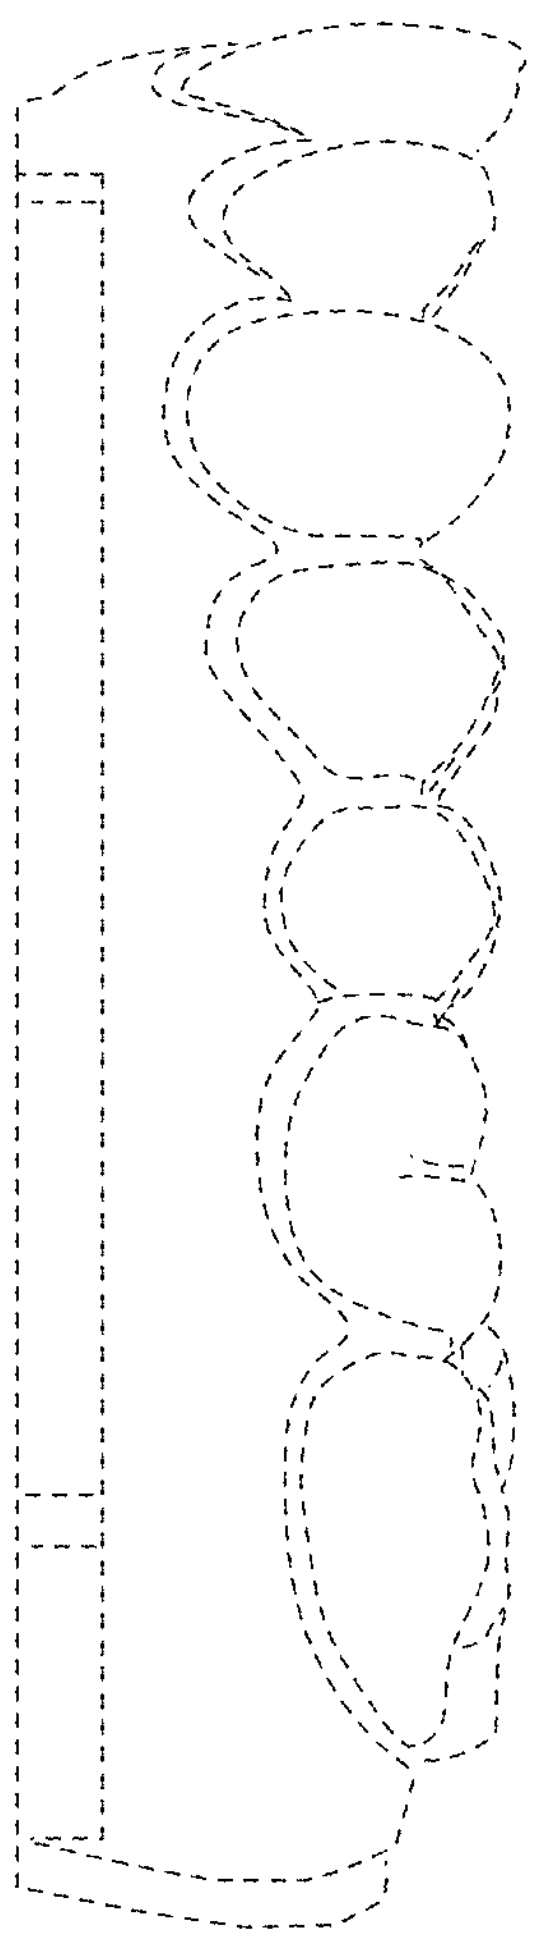

FIG. 4

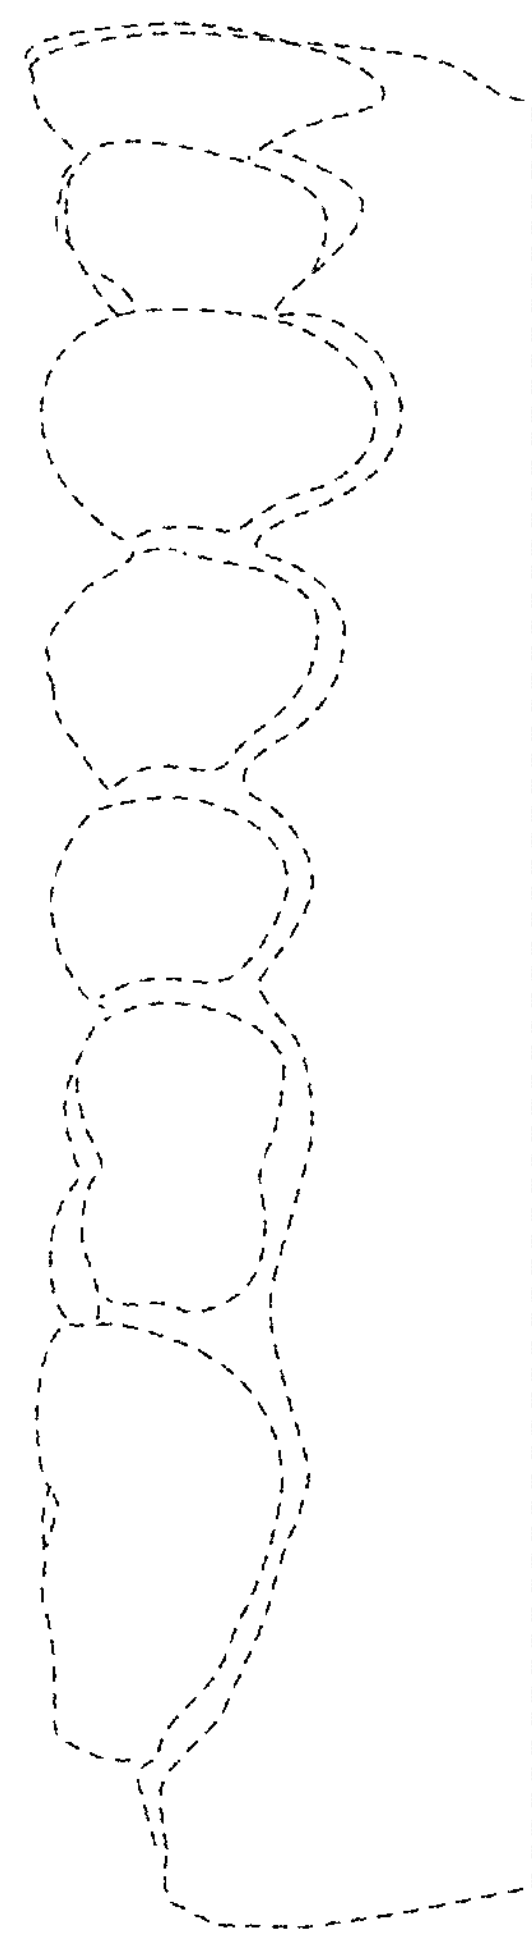

FIG. 5

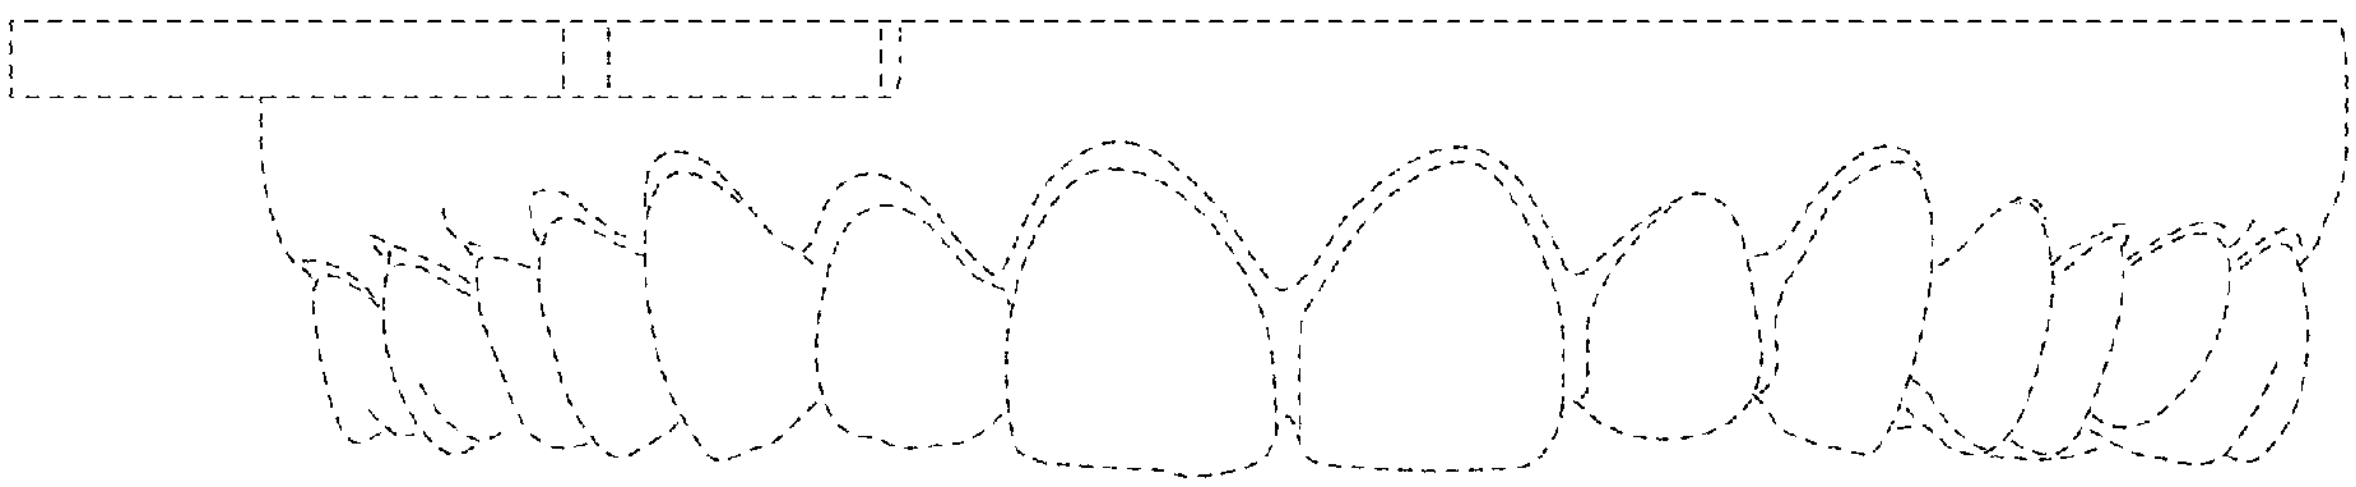

FIG. 6

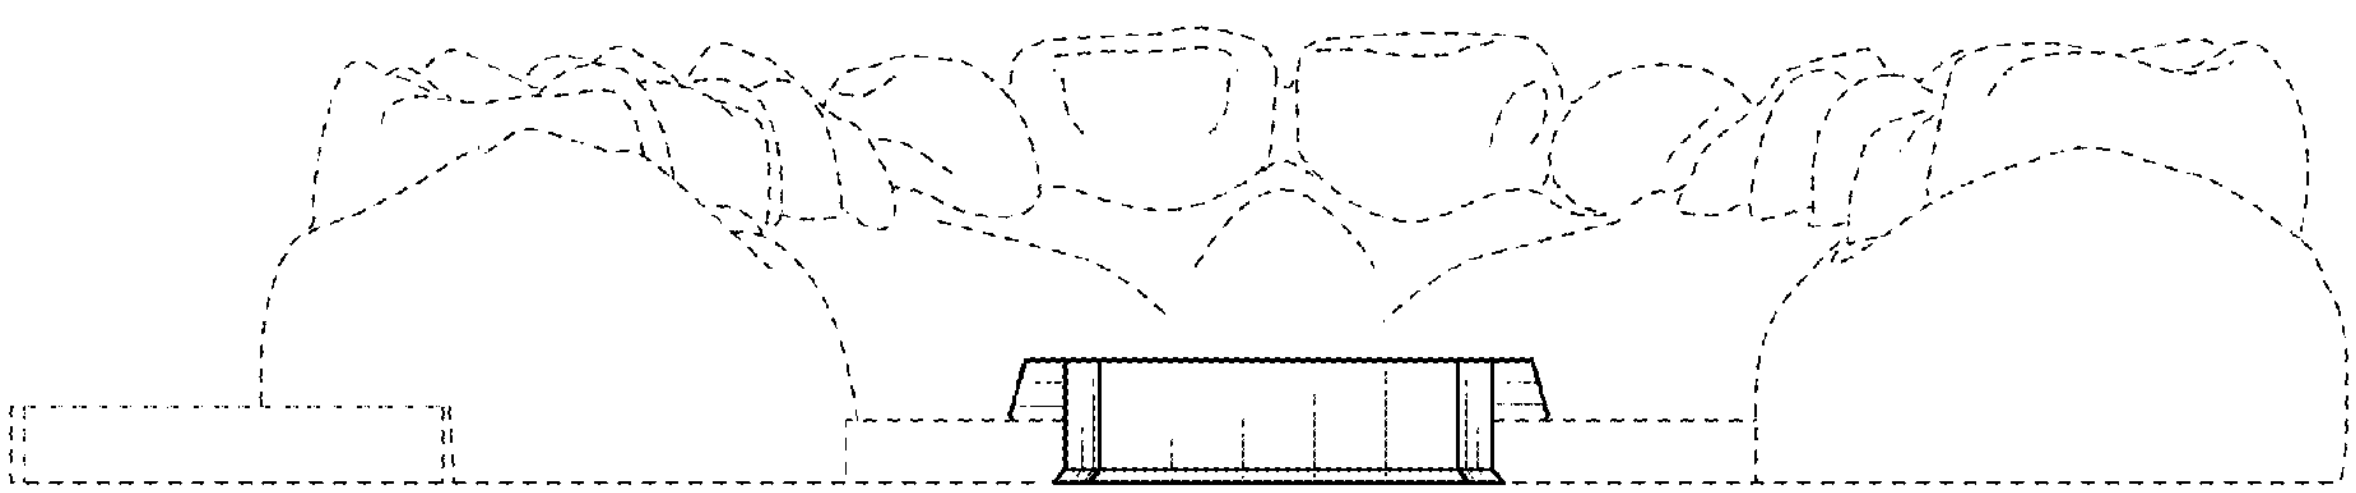

FIG. 7

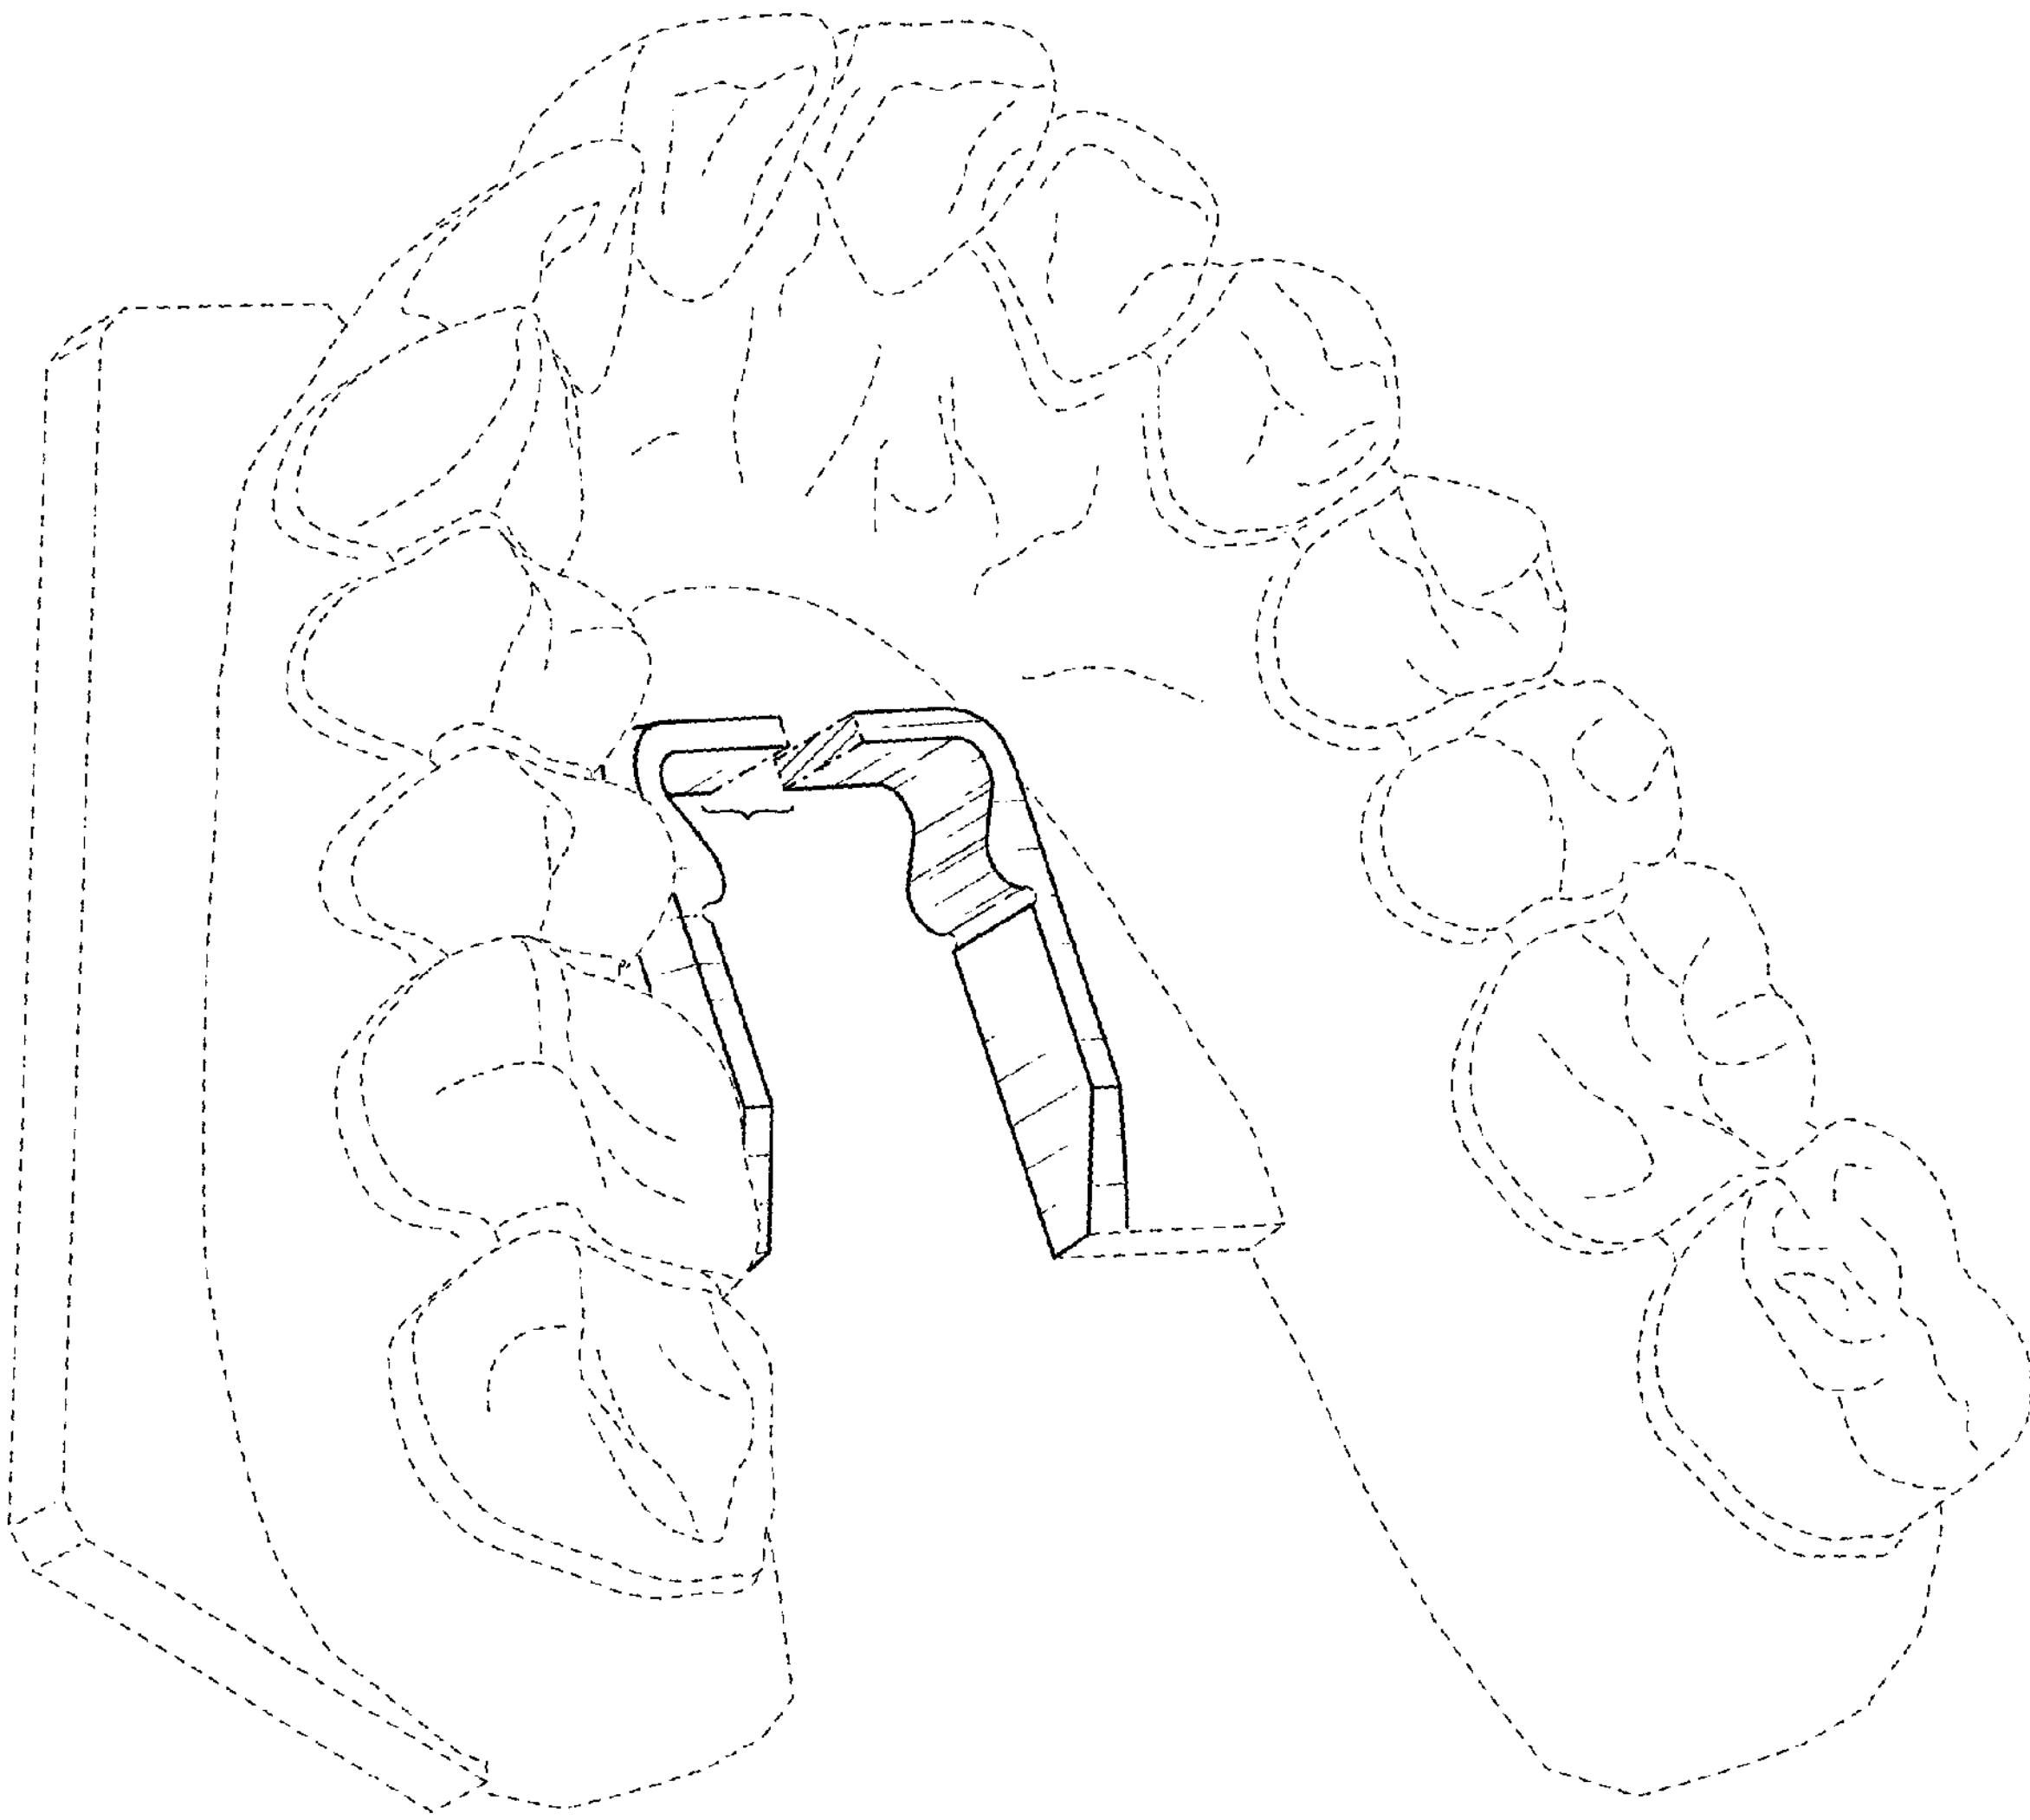

FIG. 8

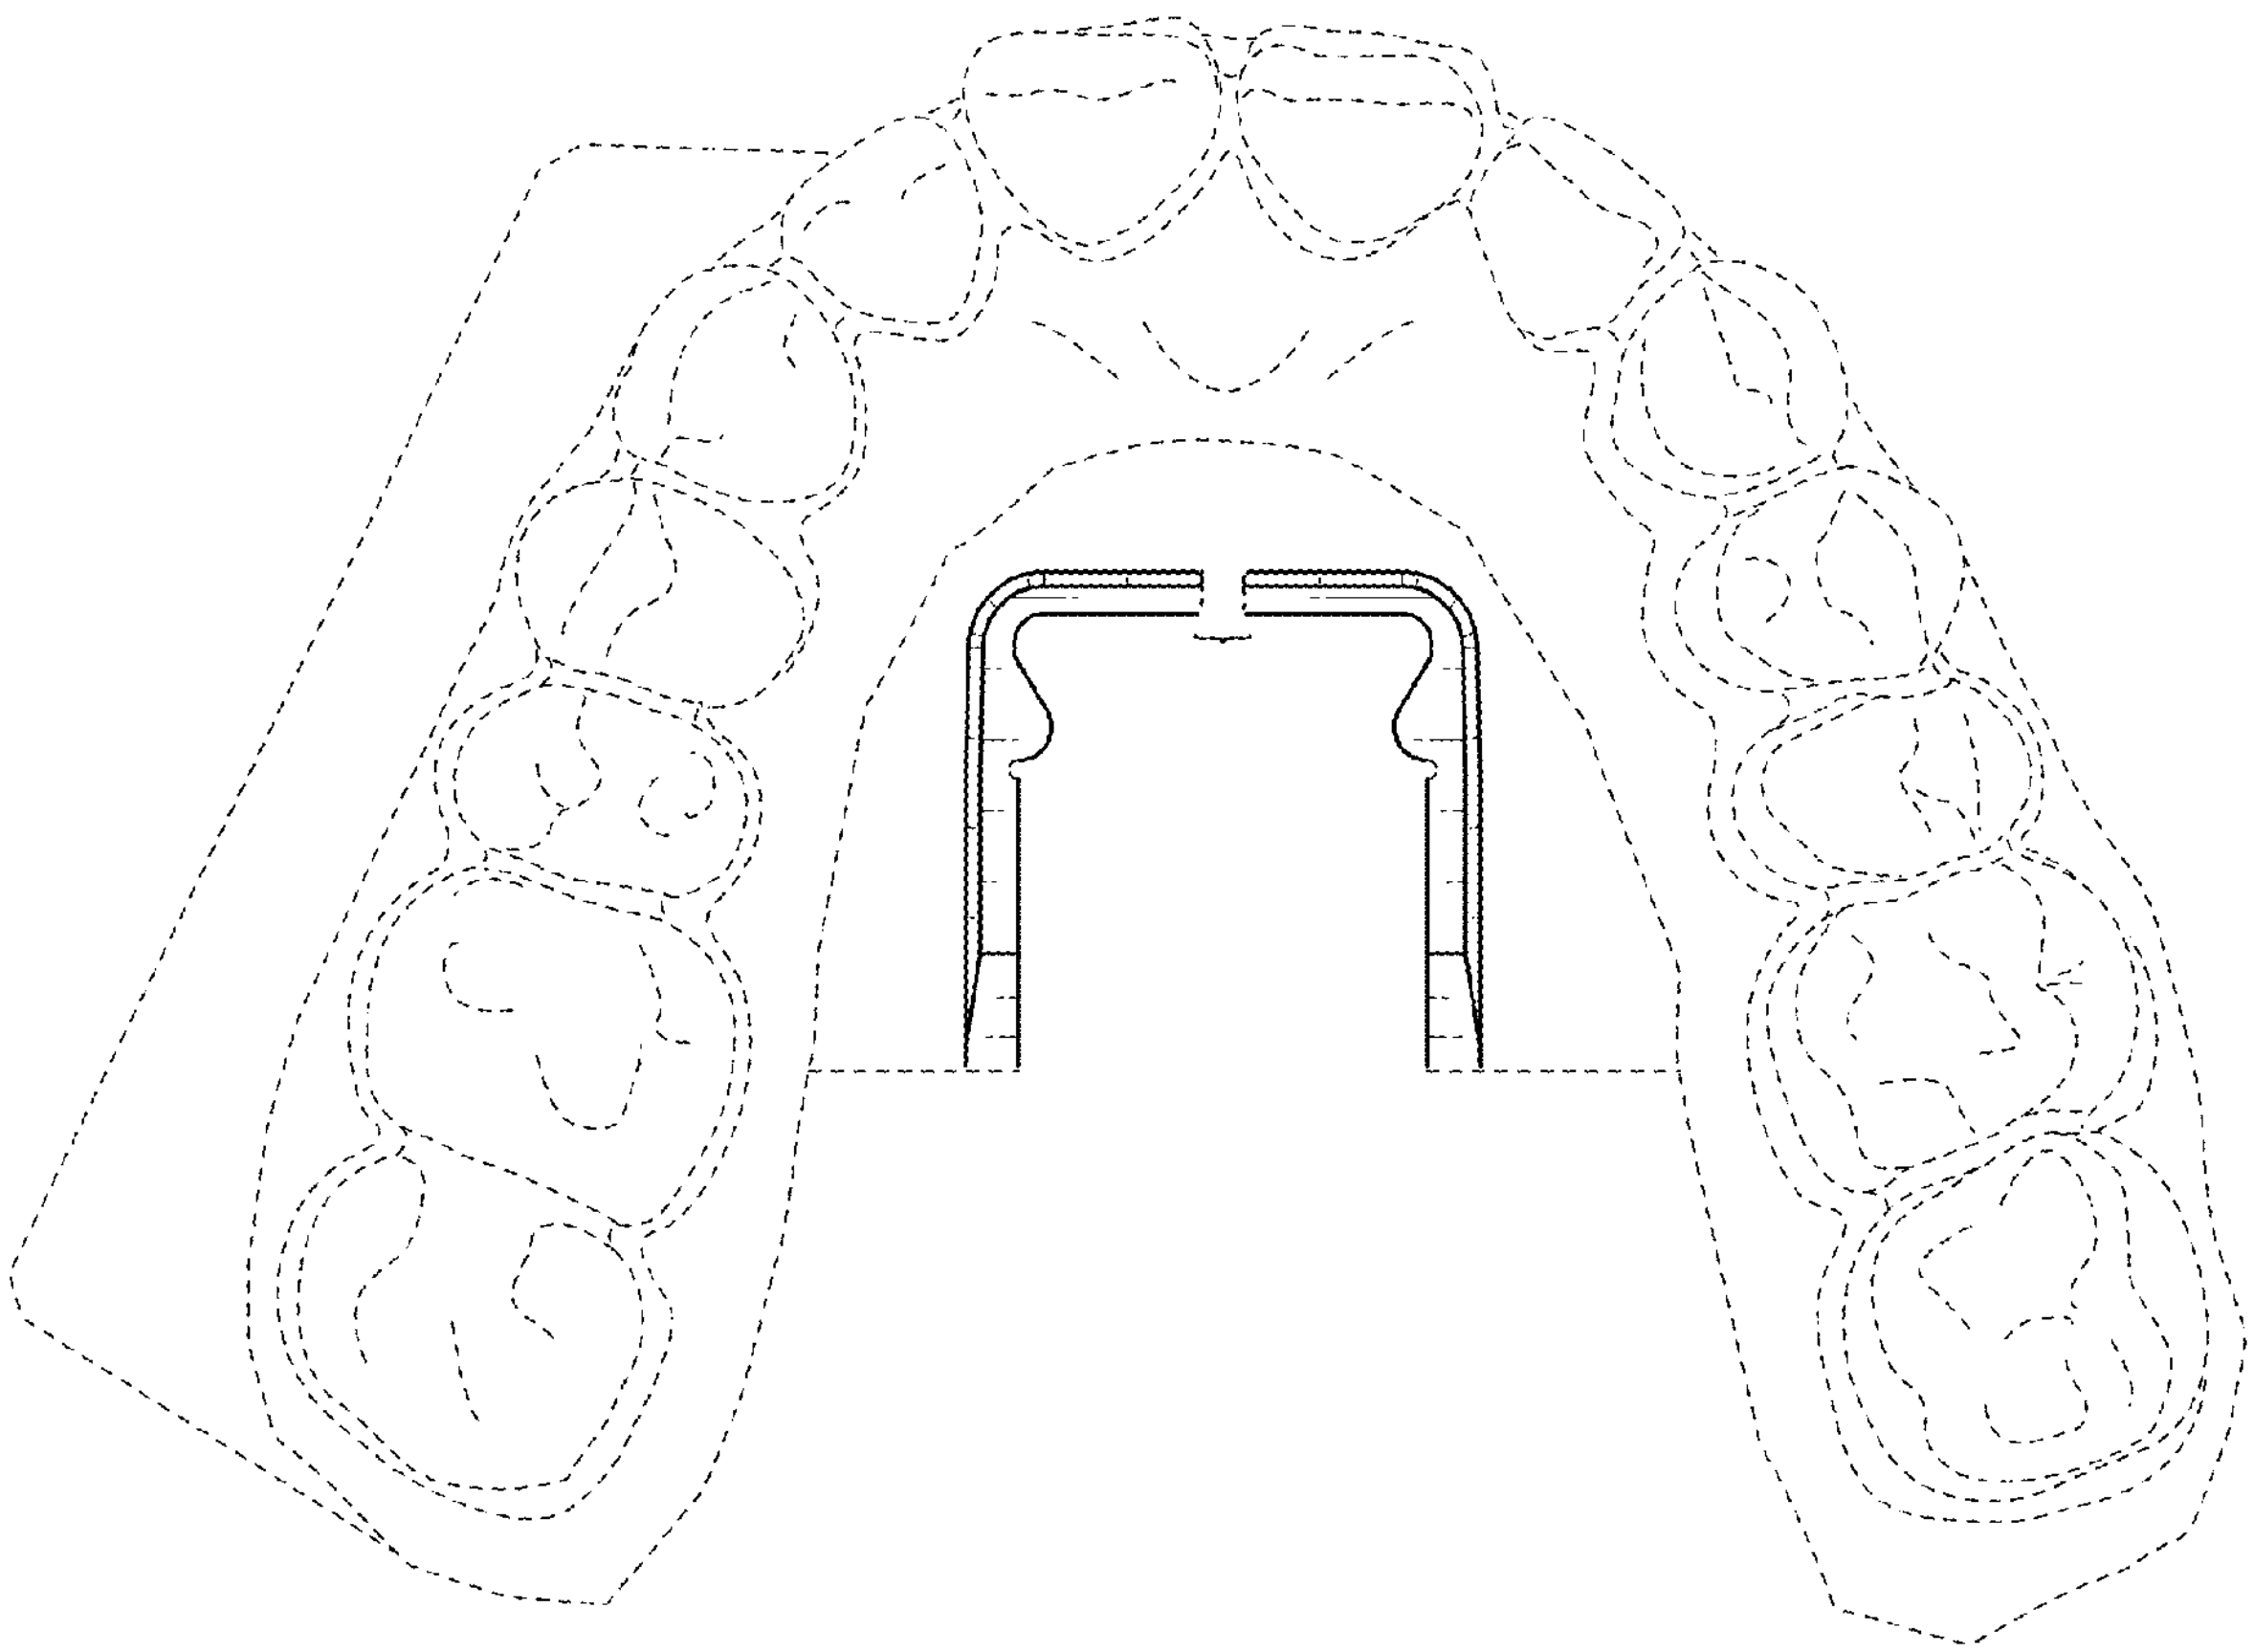

FIG. 9

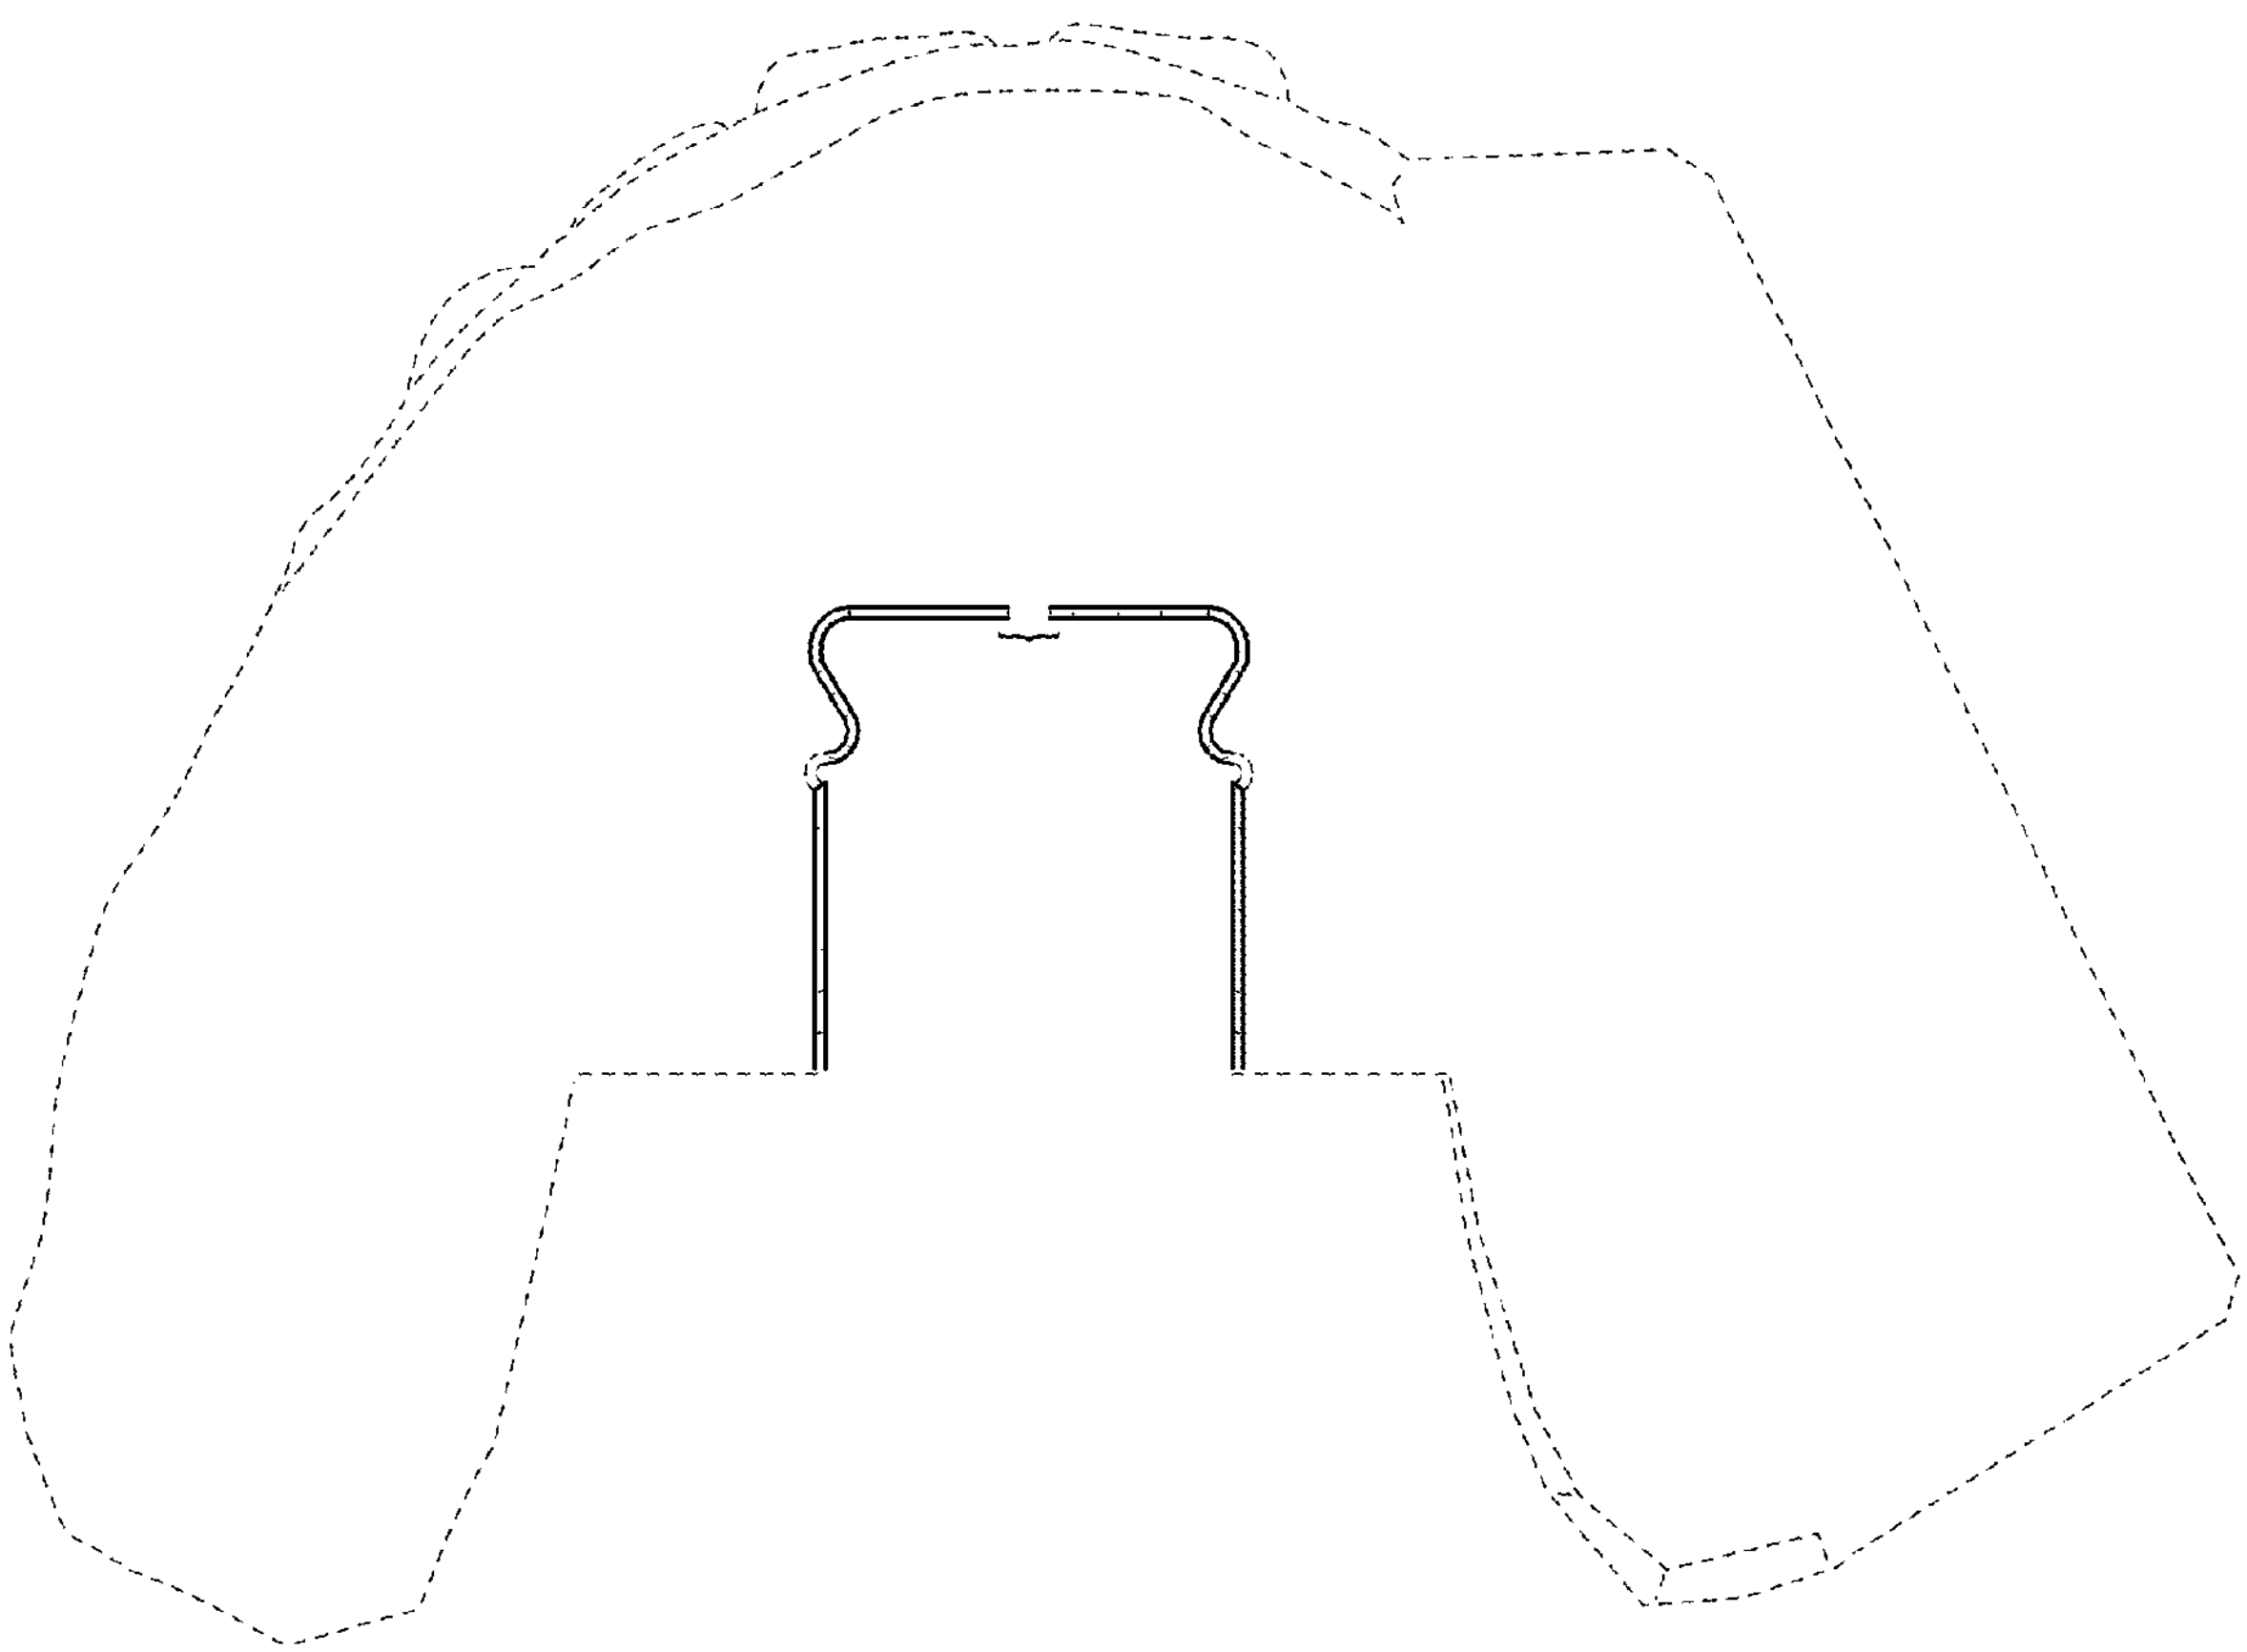

FIG. 10

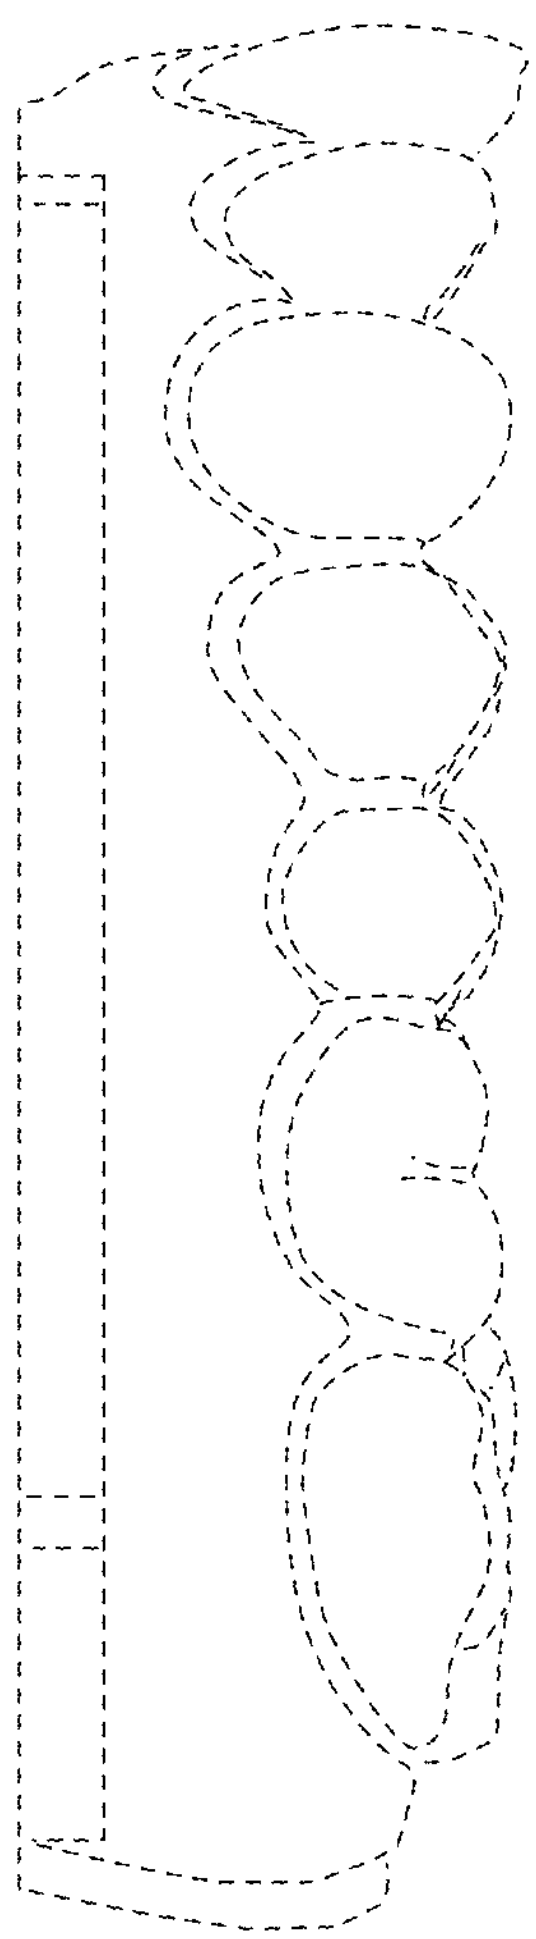

FIG. 11

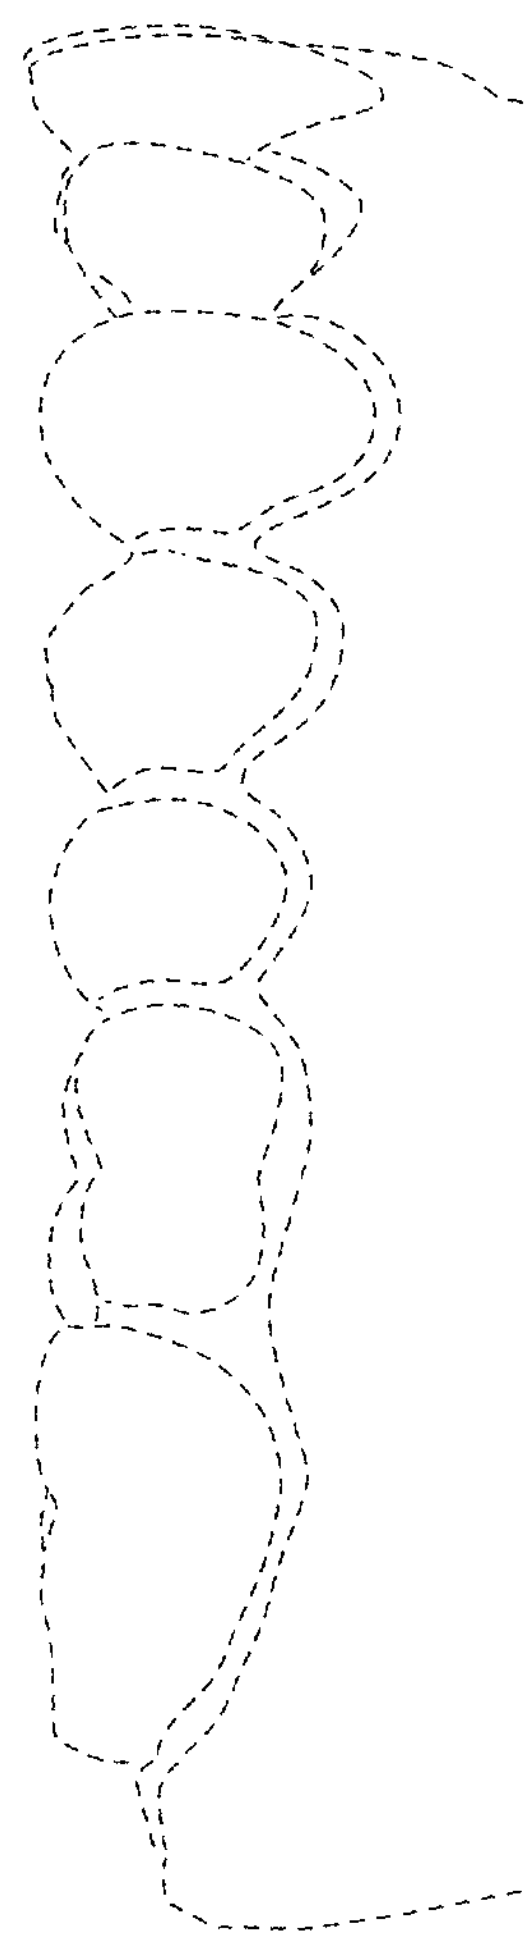

FIG. 12

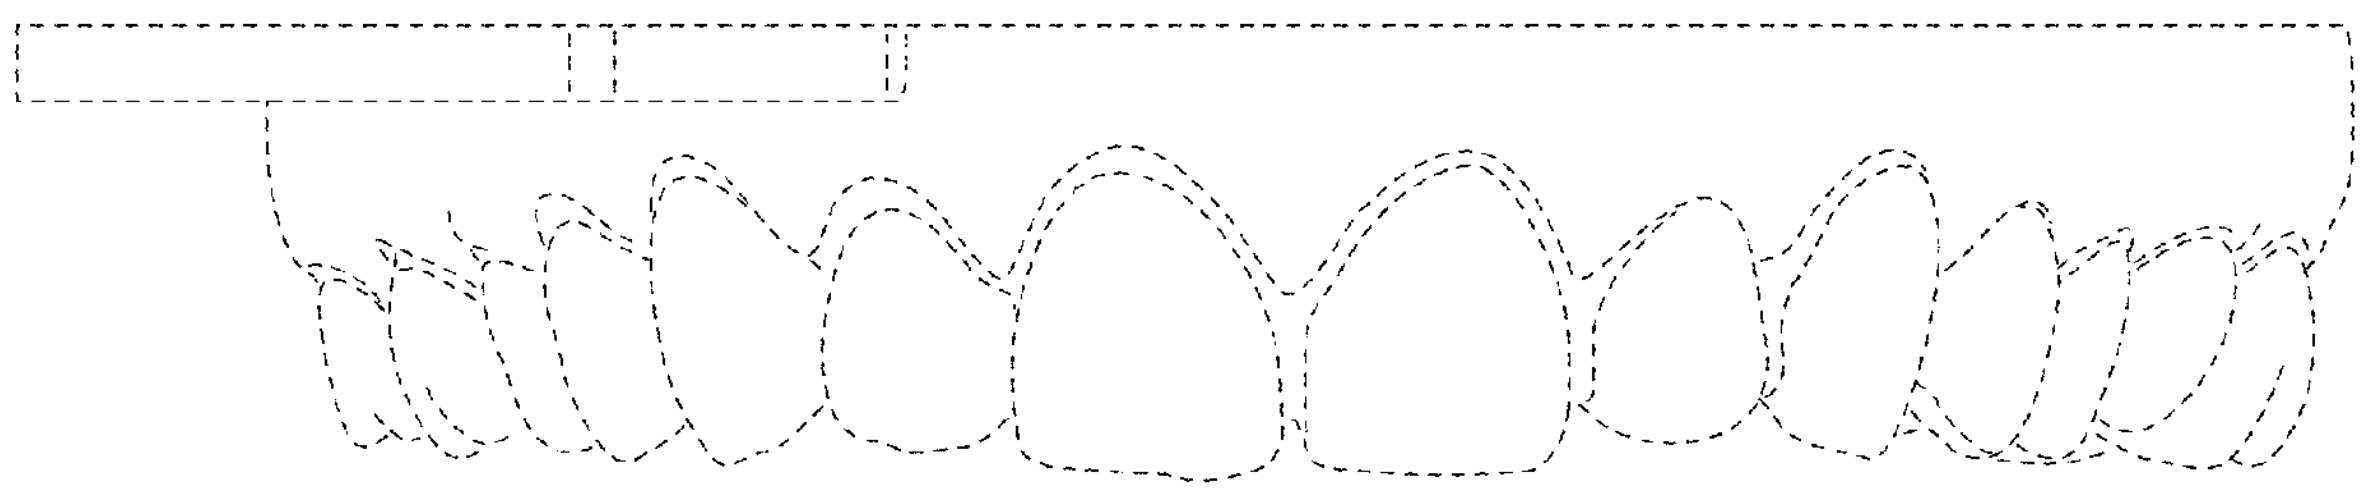

FIG. 13

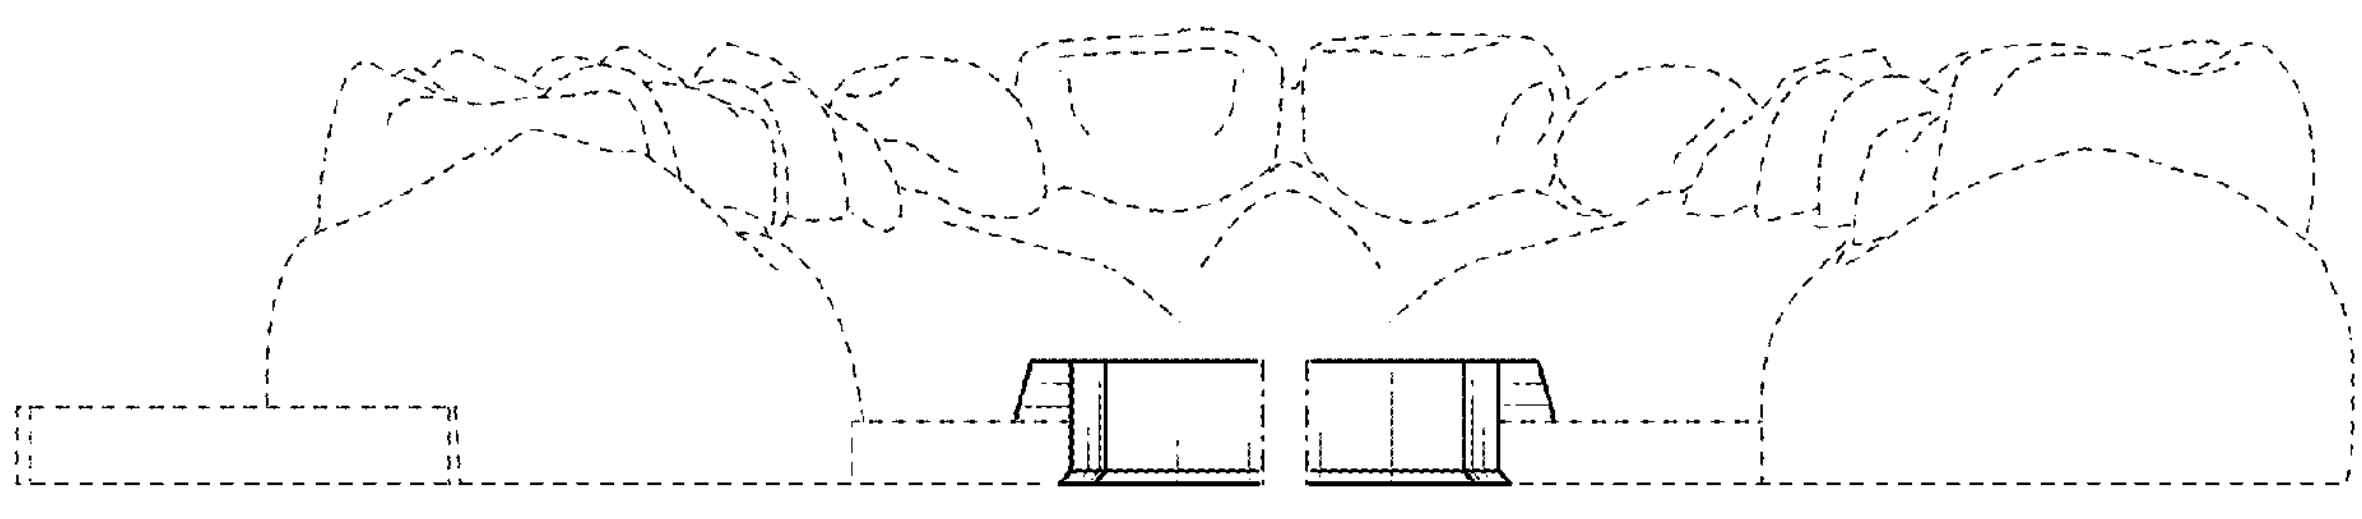

FIG. 14

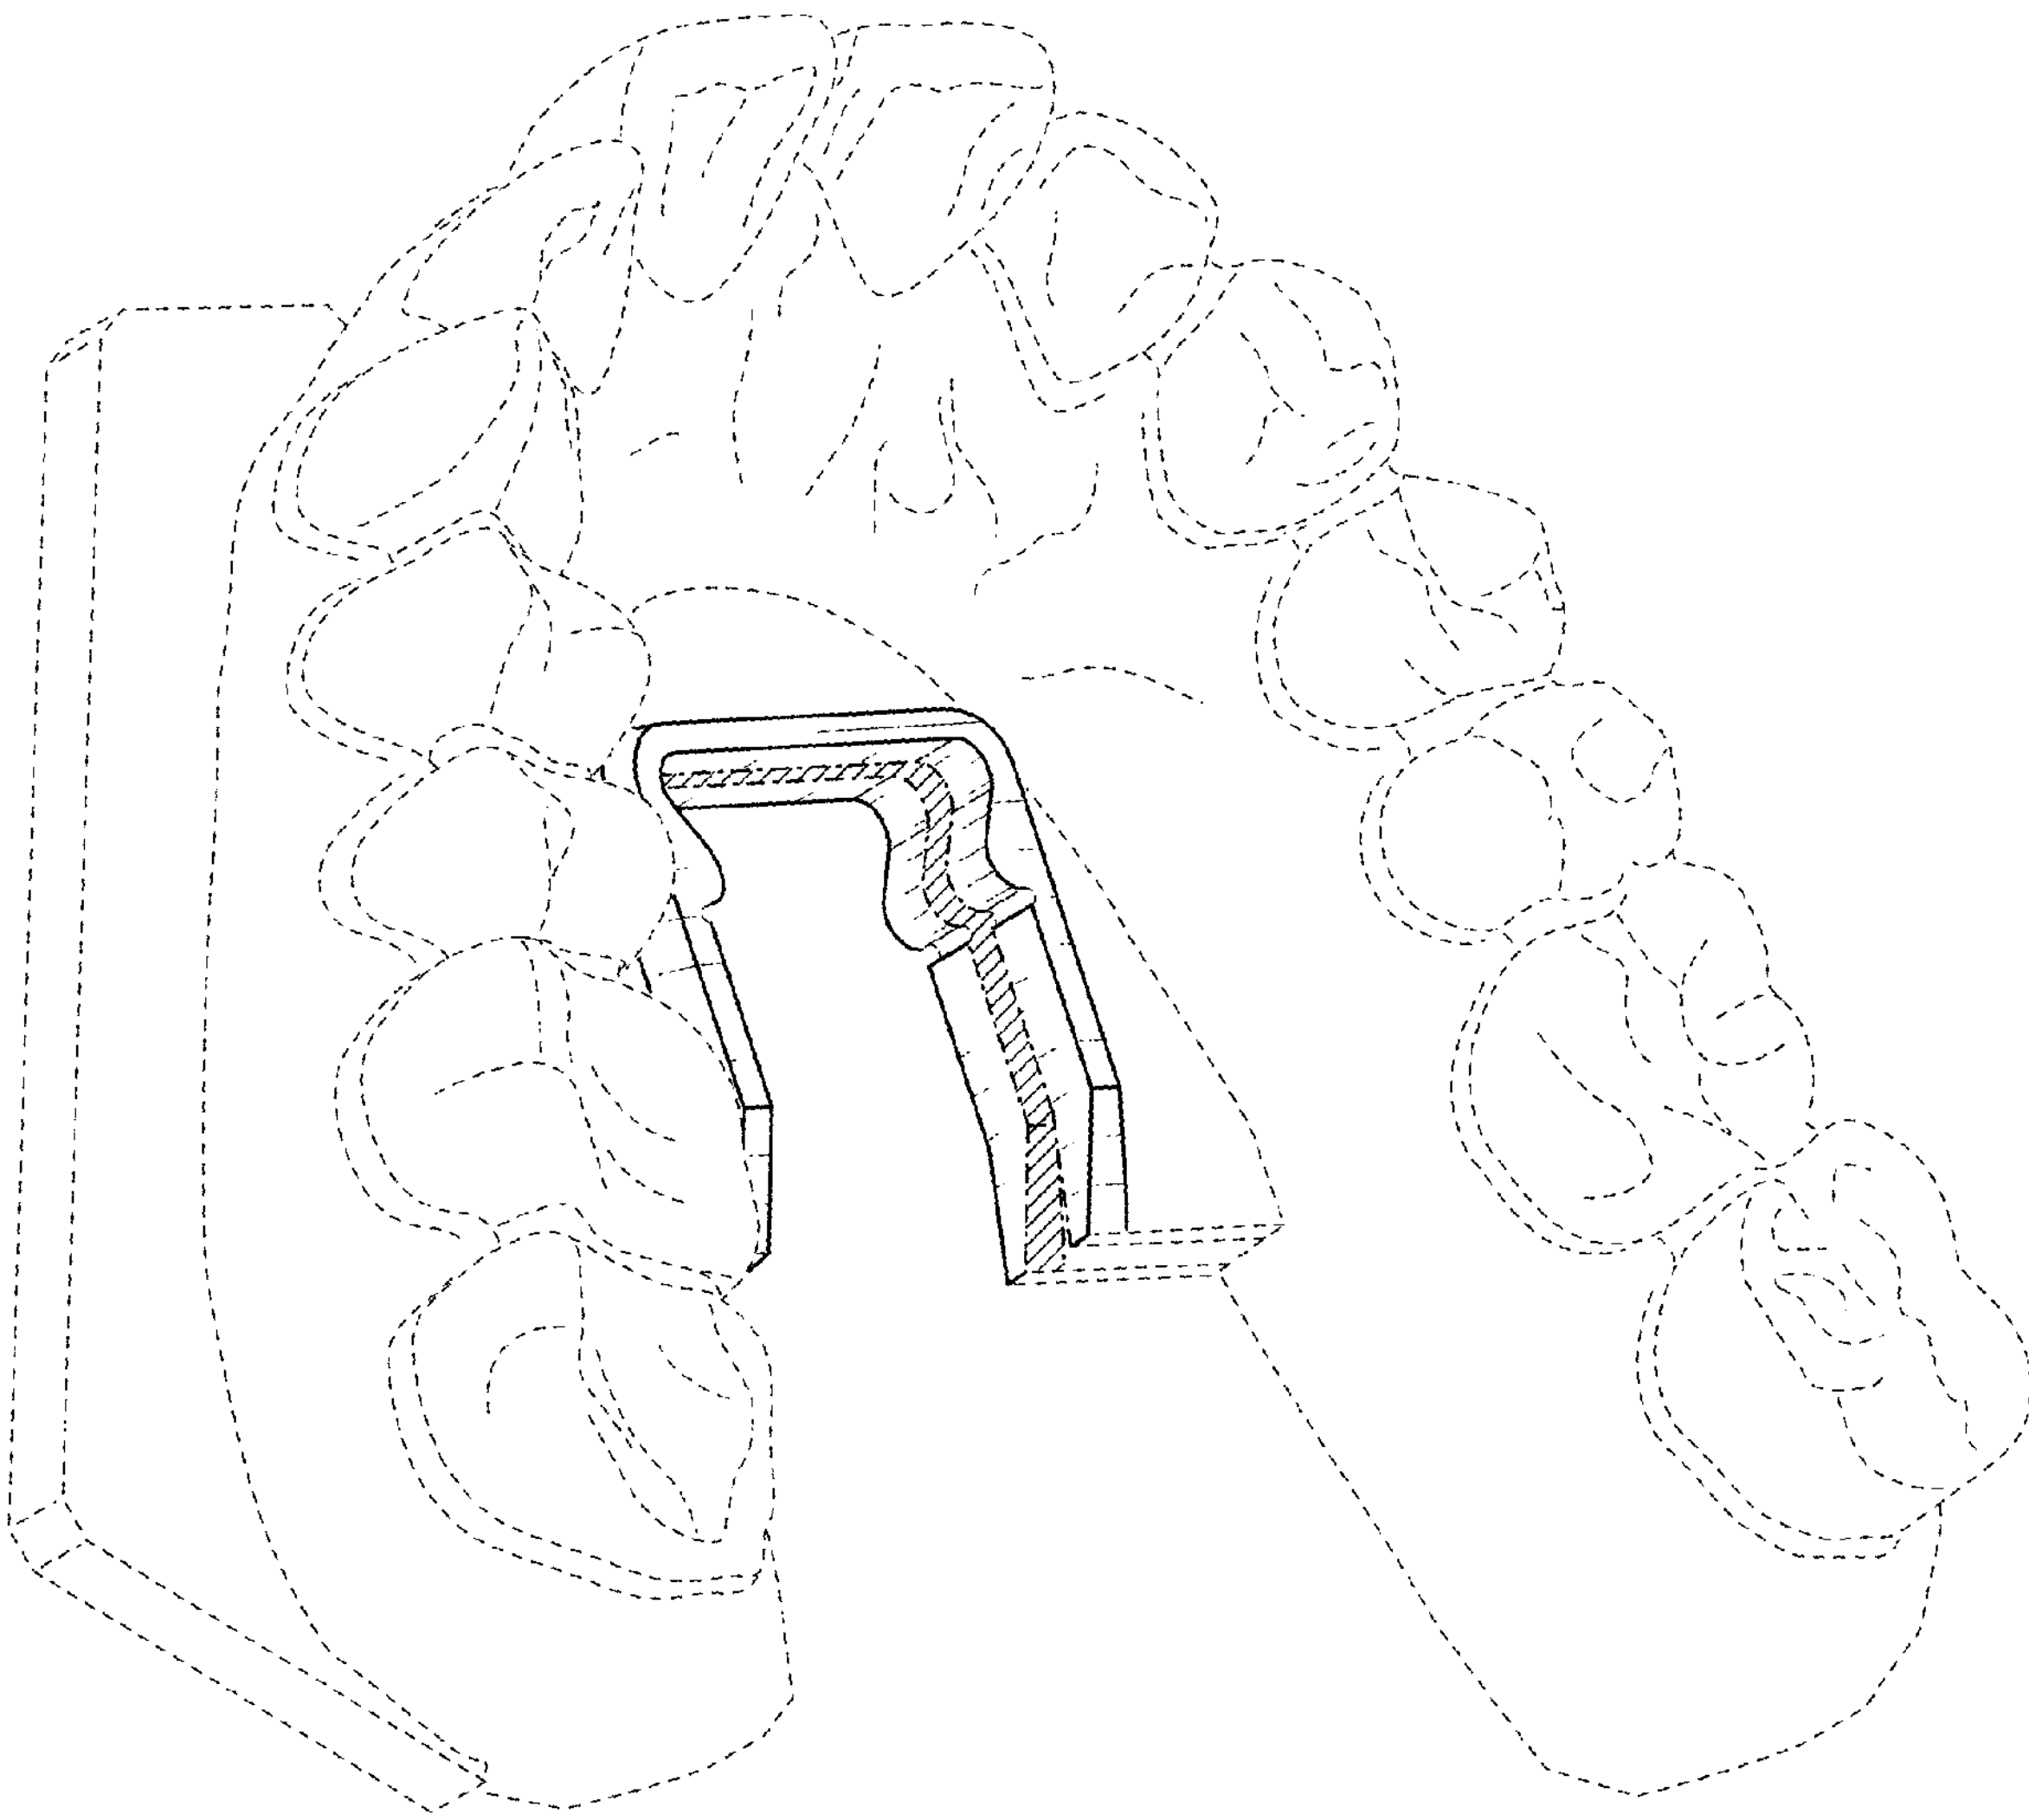

FIG. 15

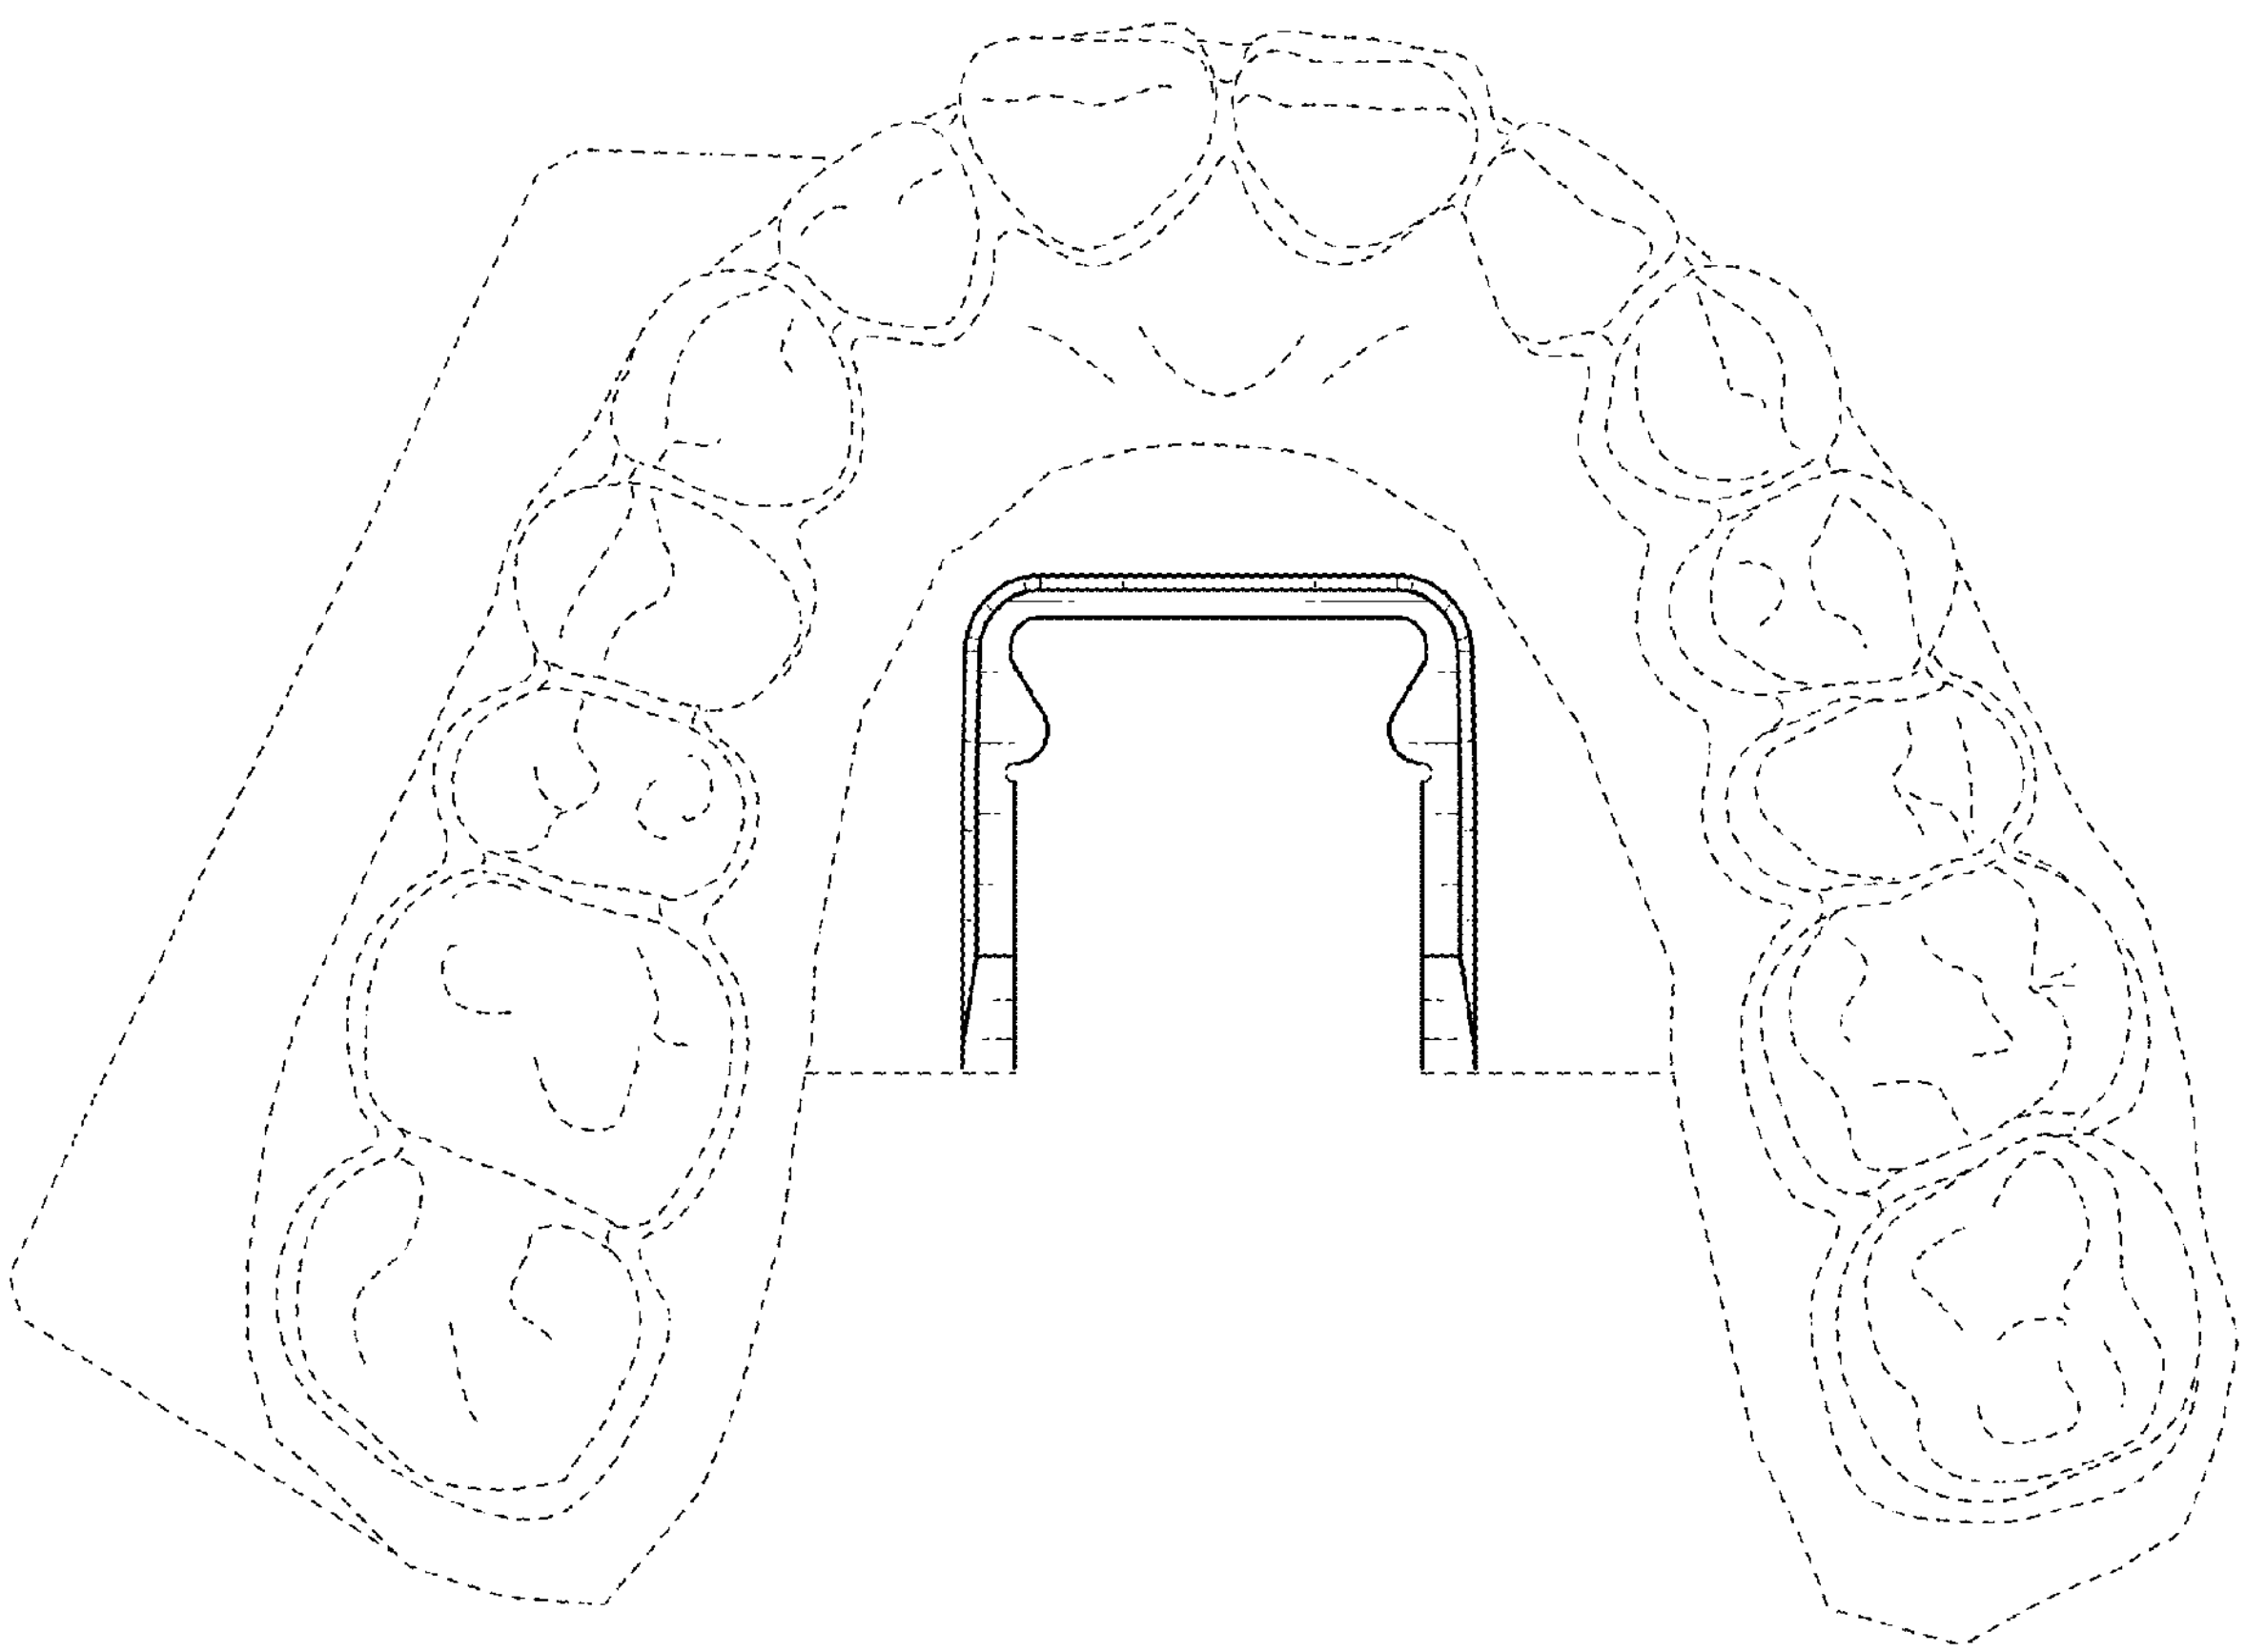

FIG. 16

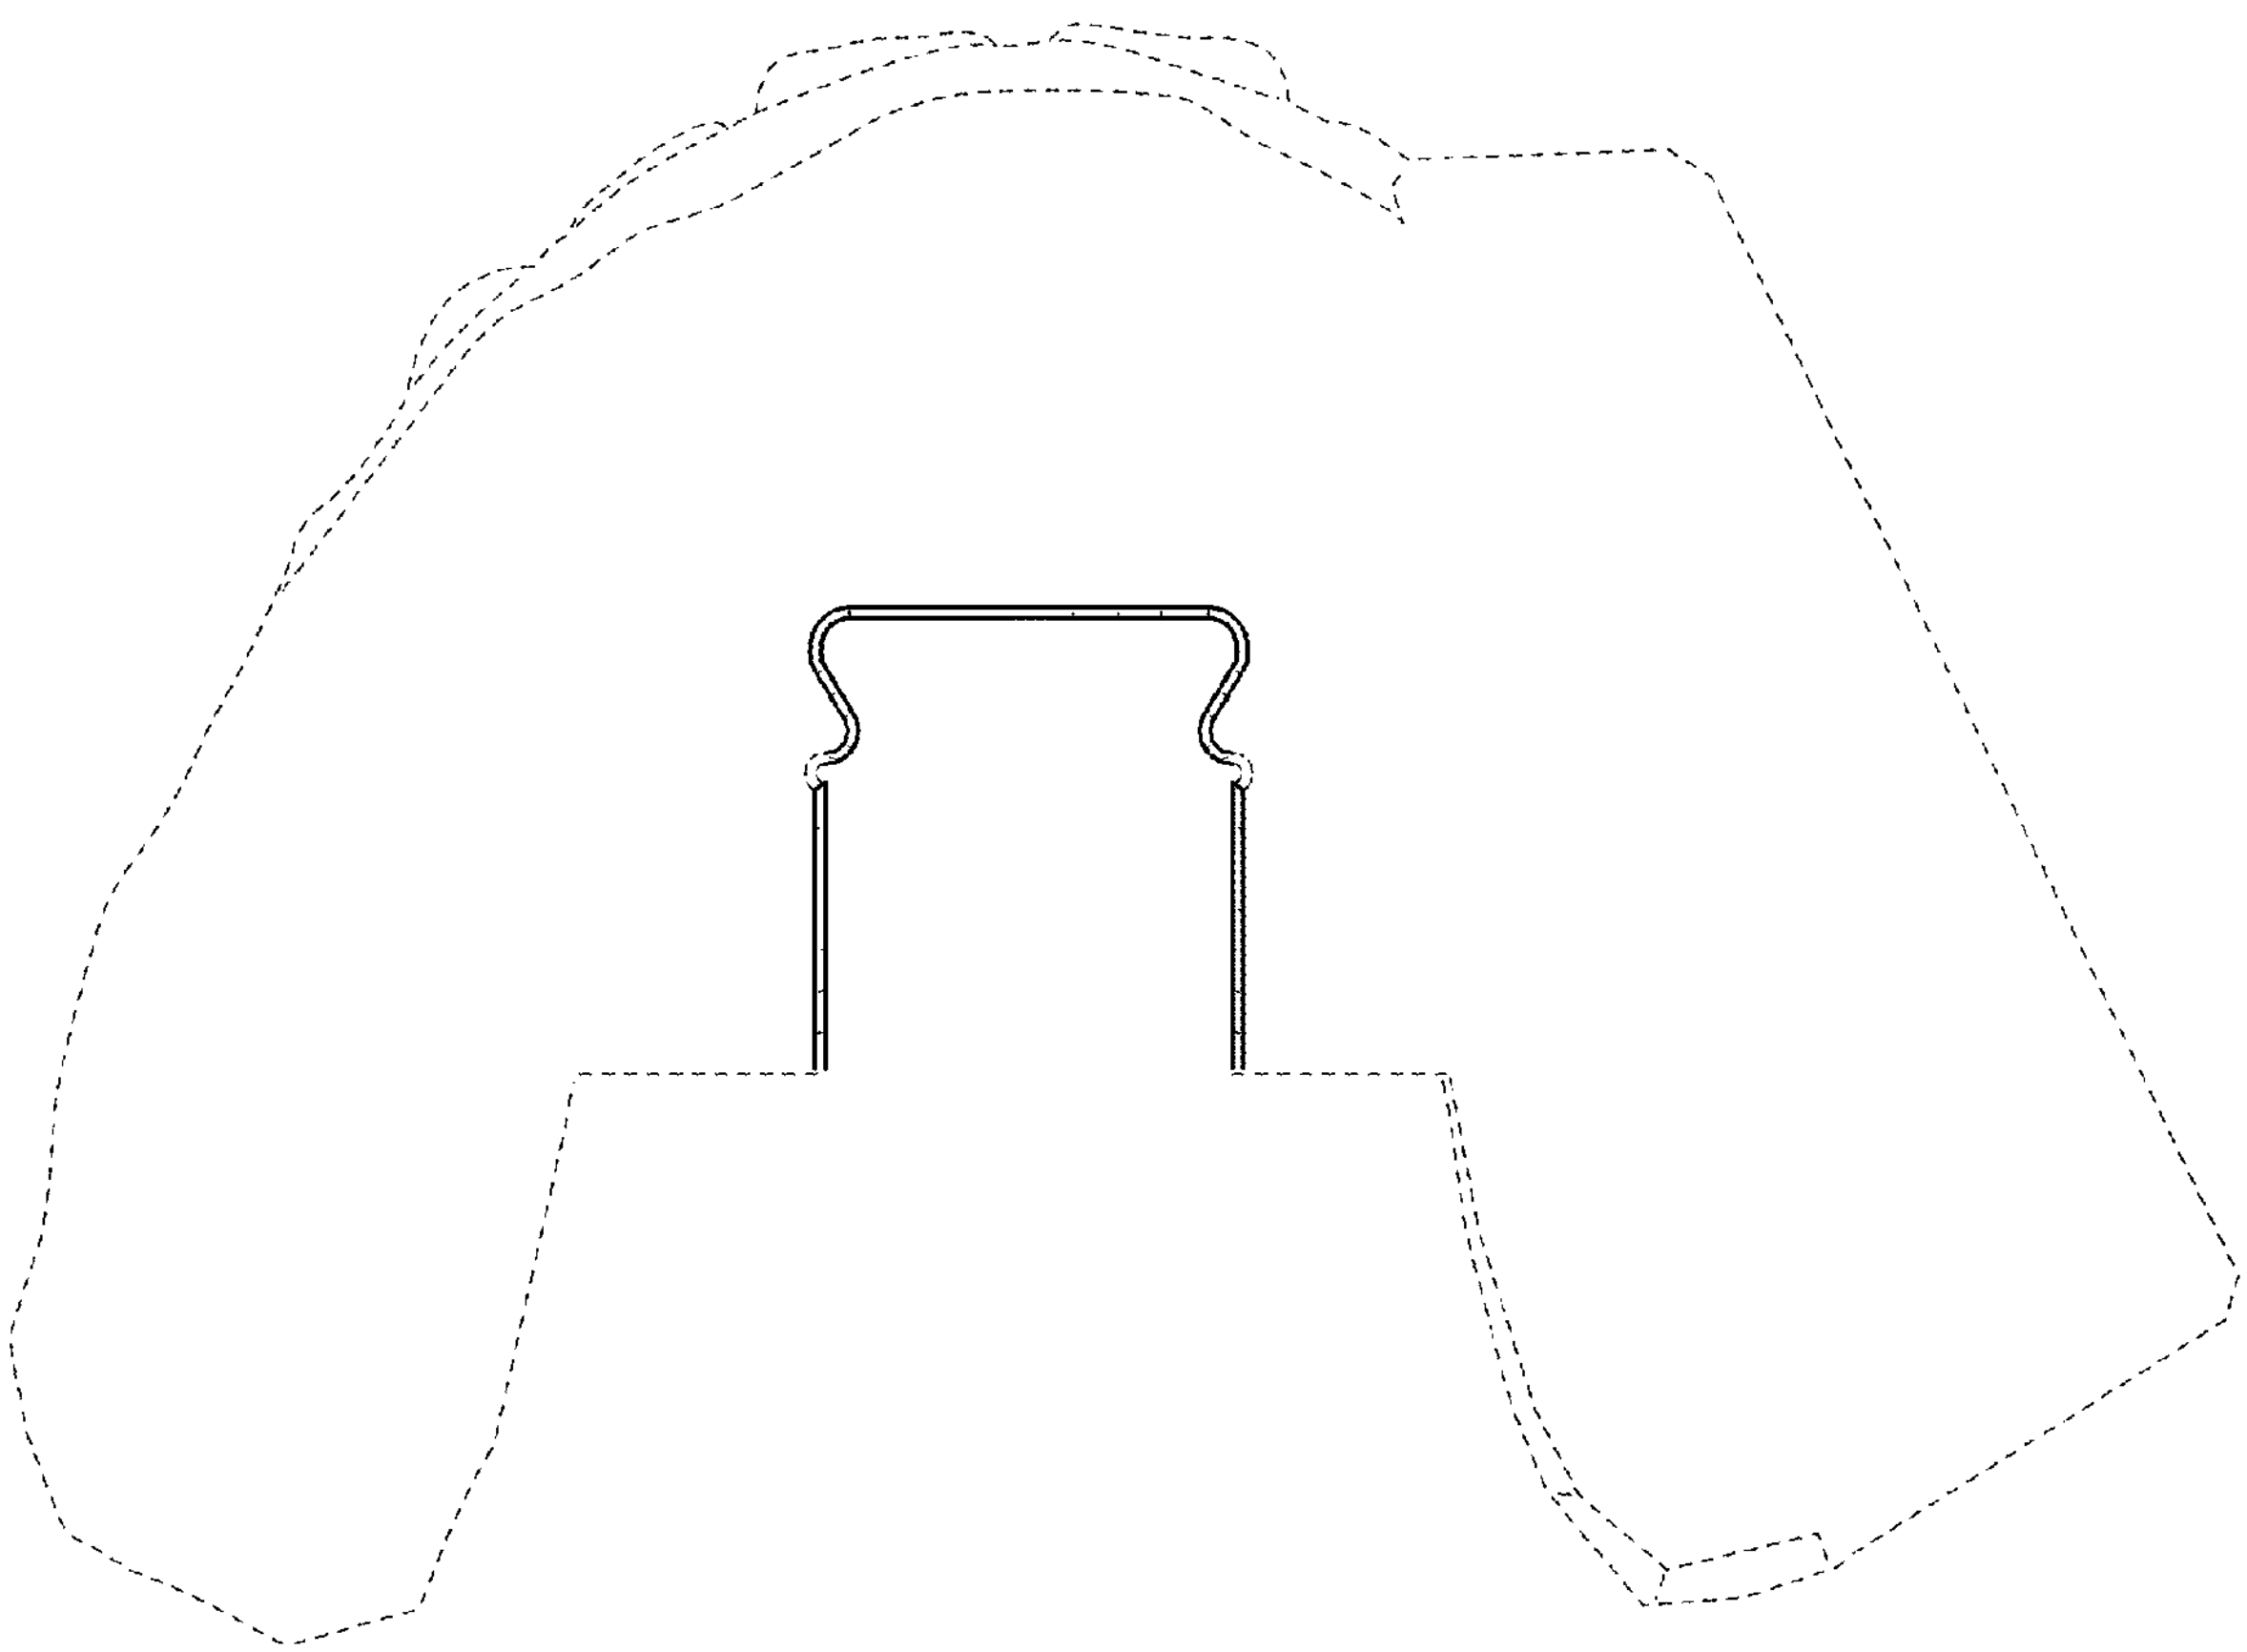

FIG. 17

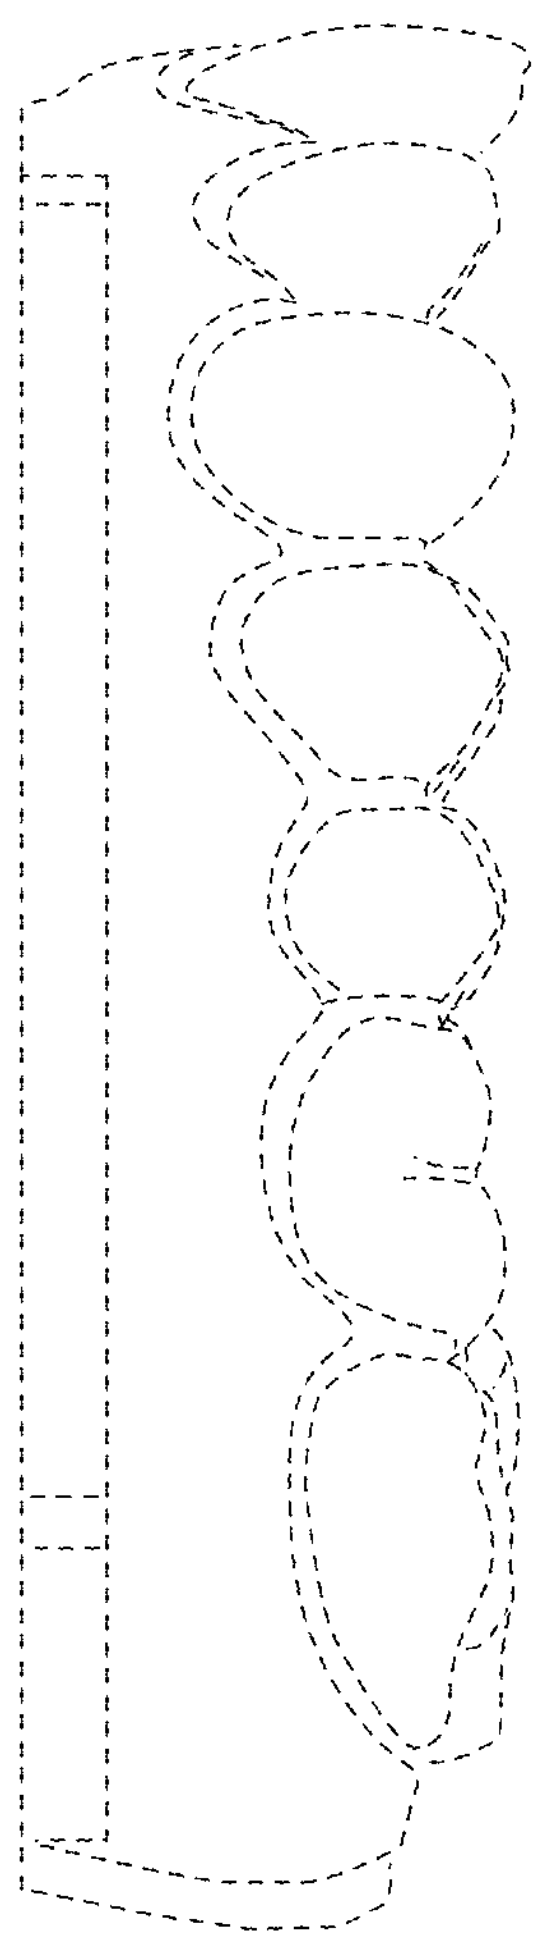

FIG. 18

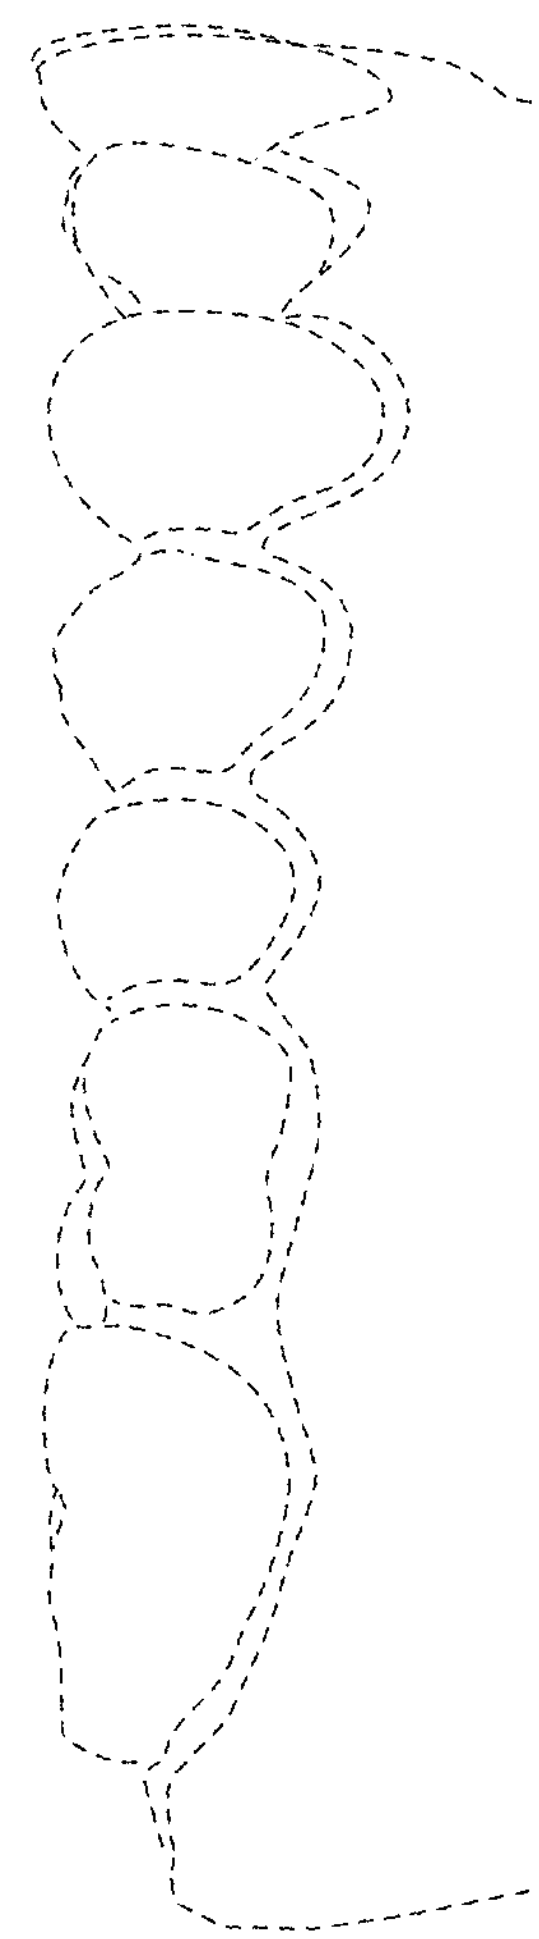

FIG. 19

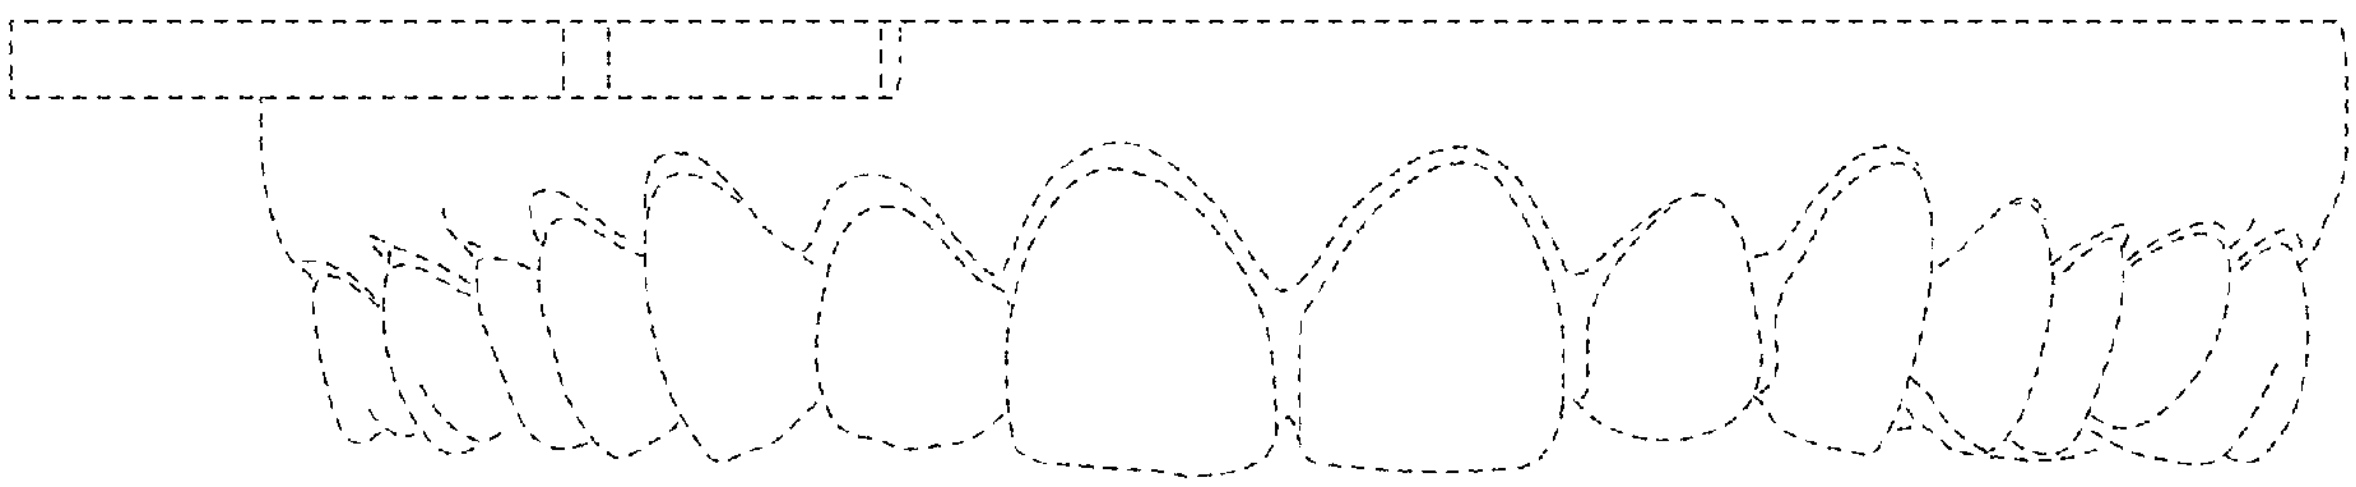

FIG. 20

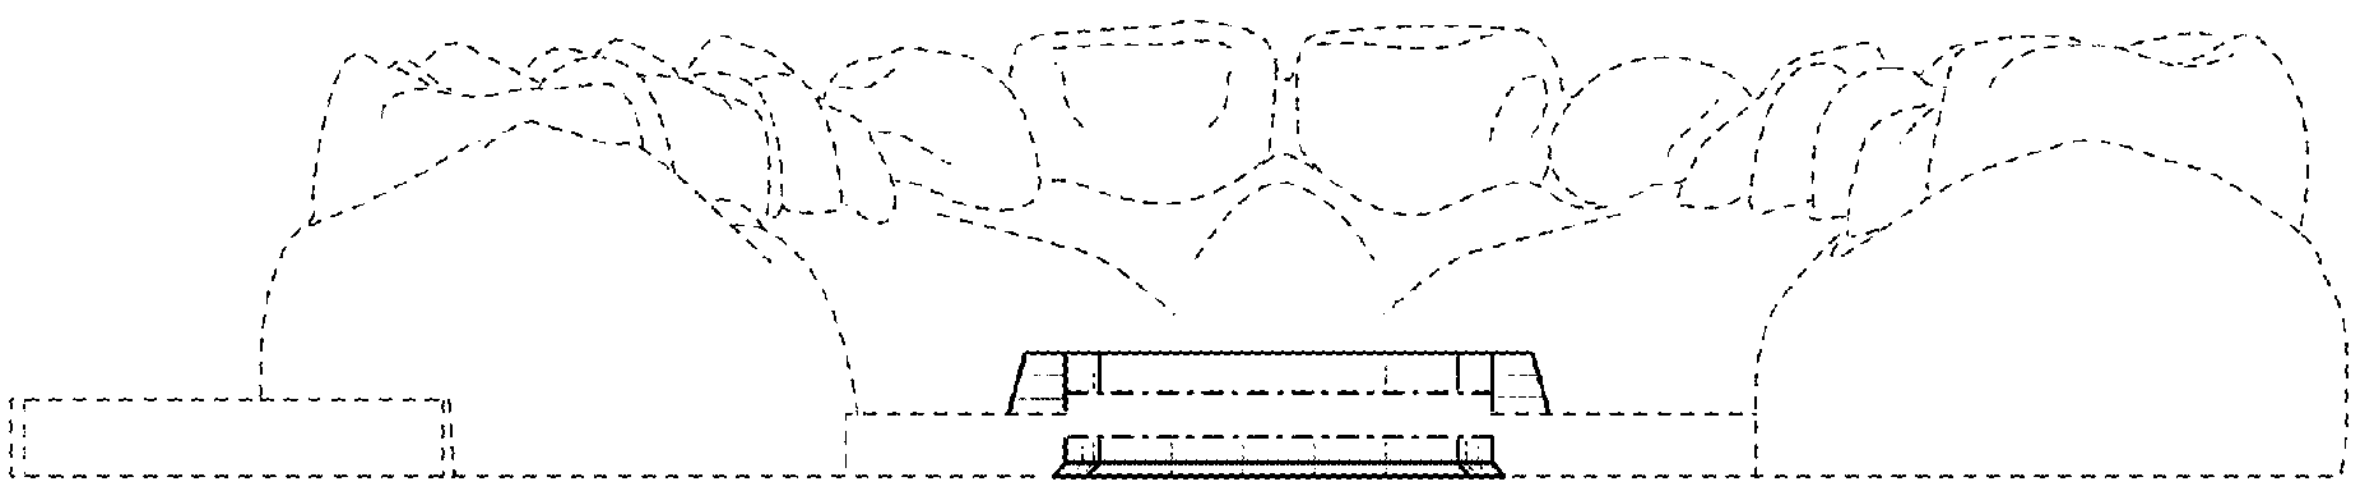

FIG. 21

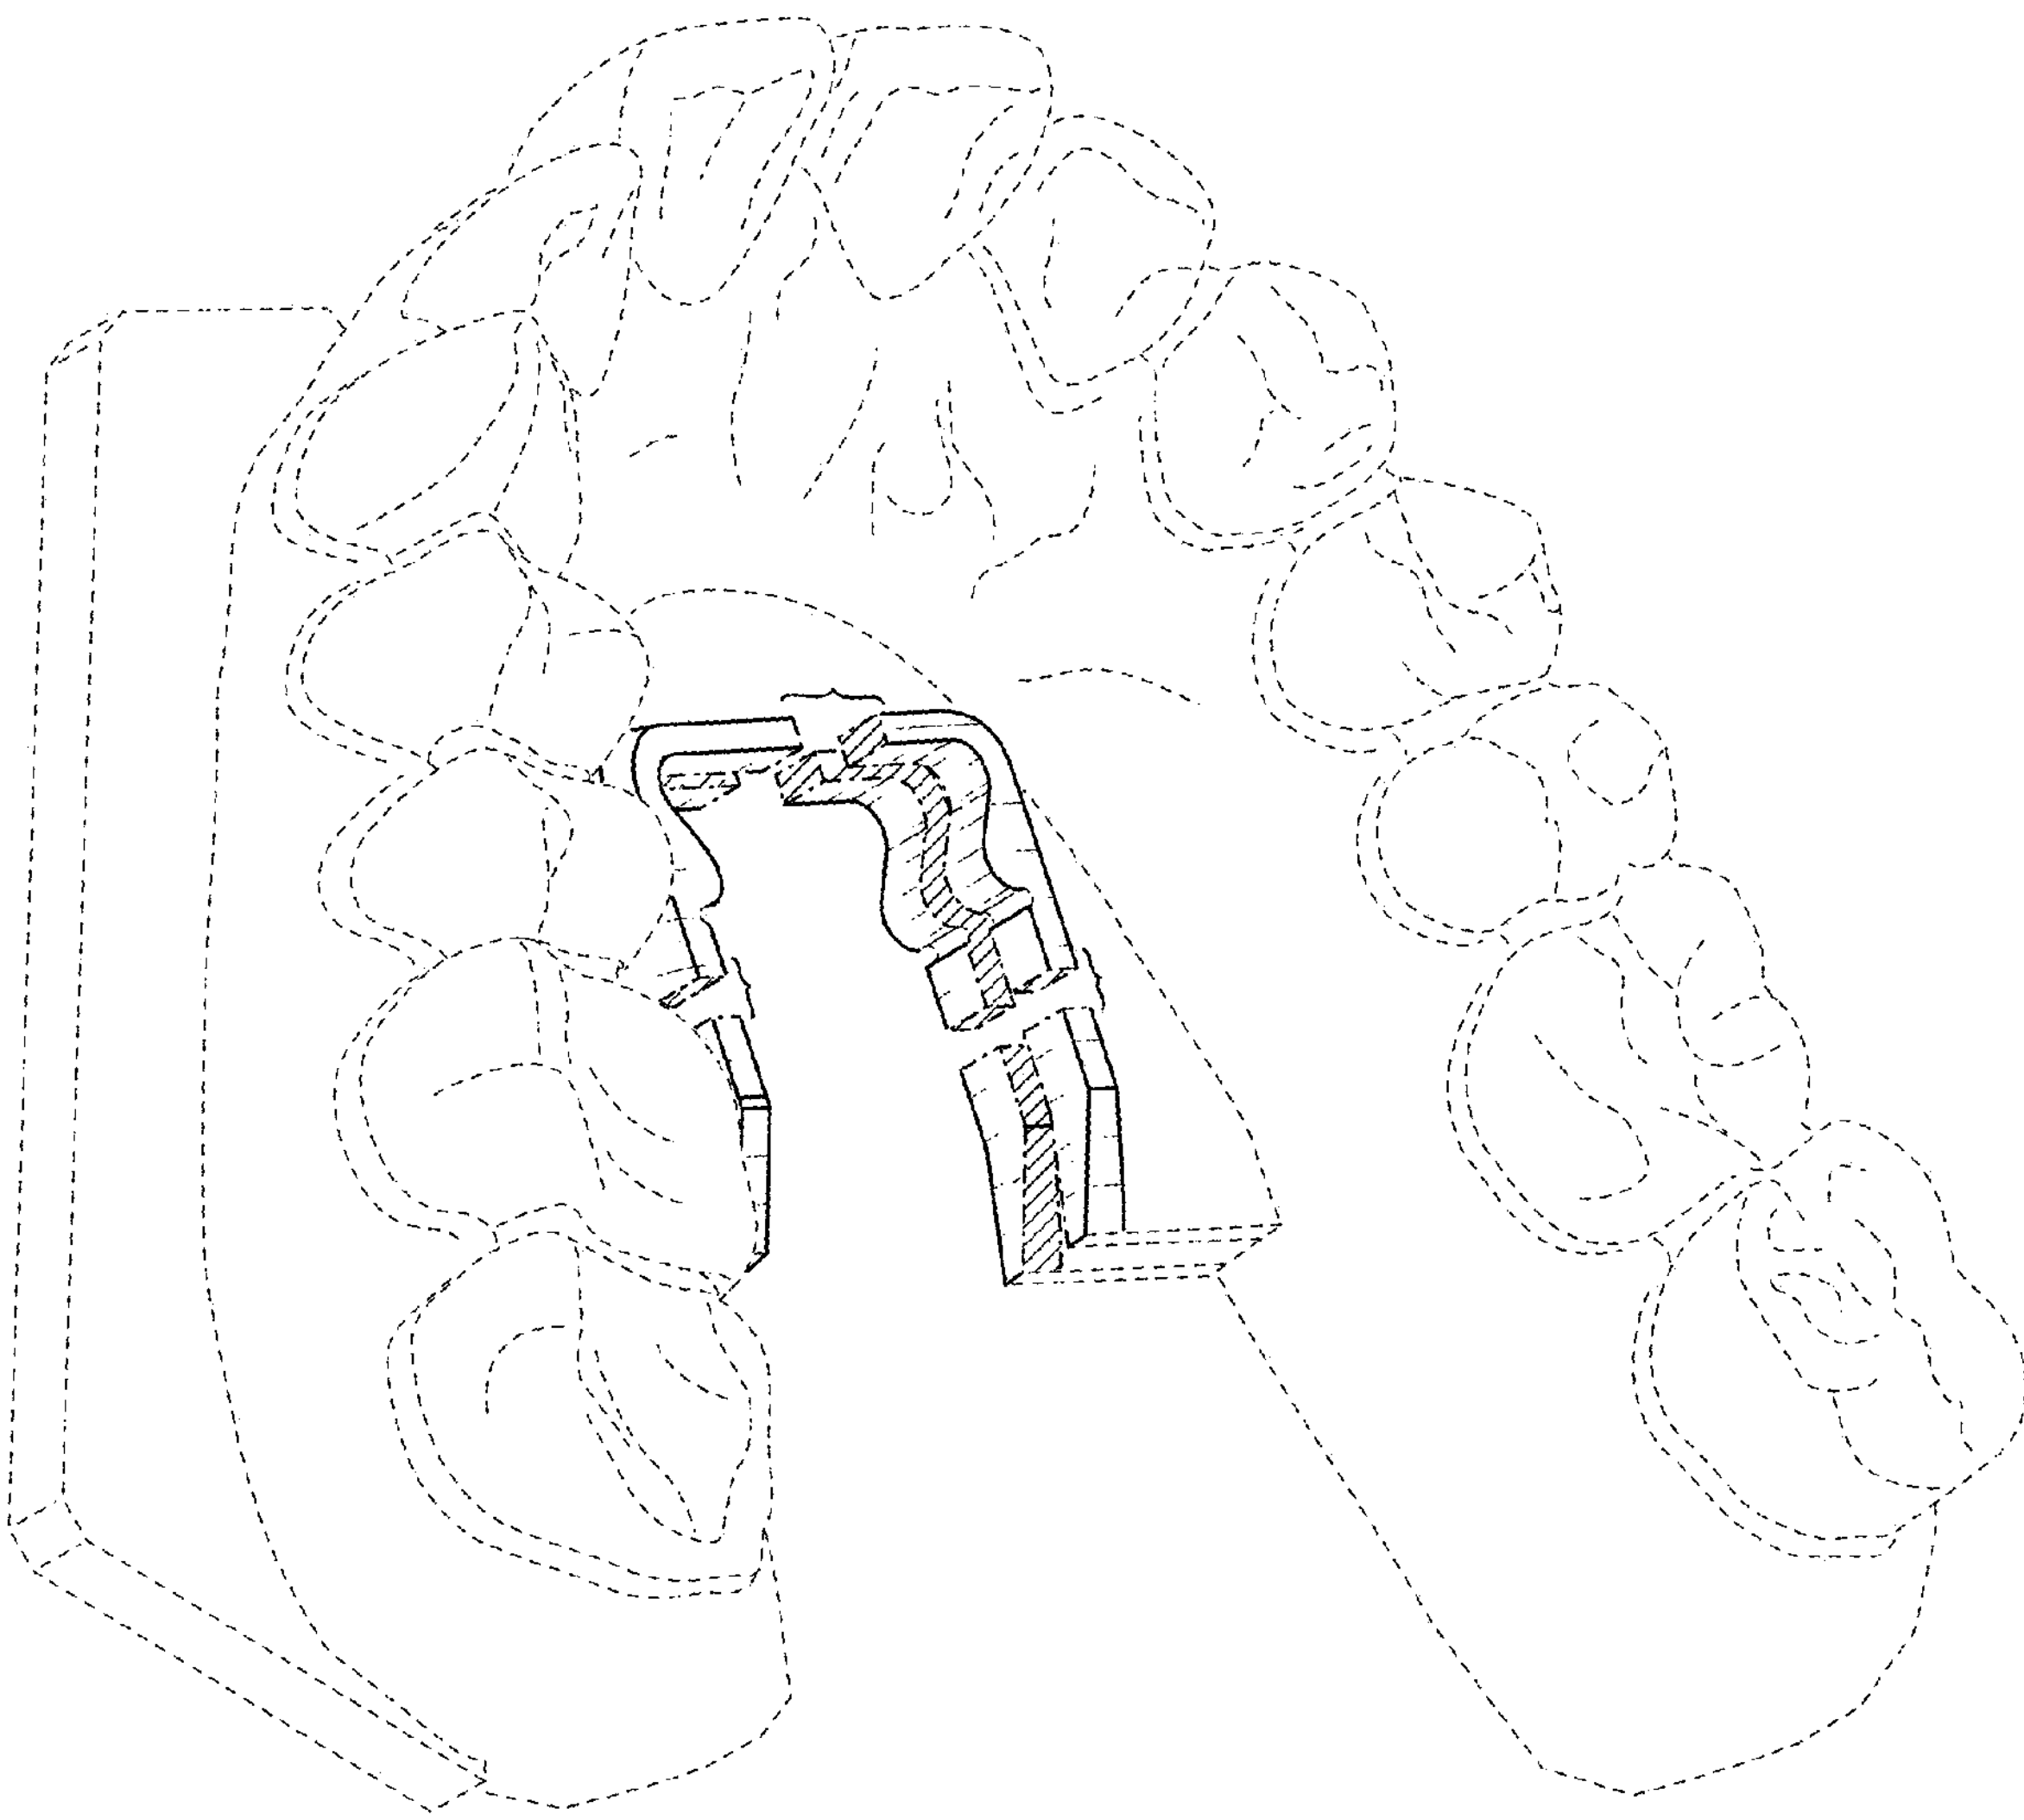

FIG. 22

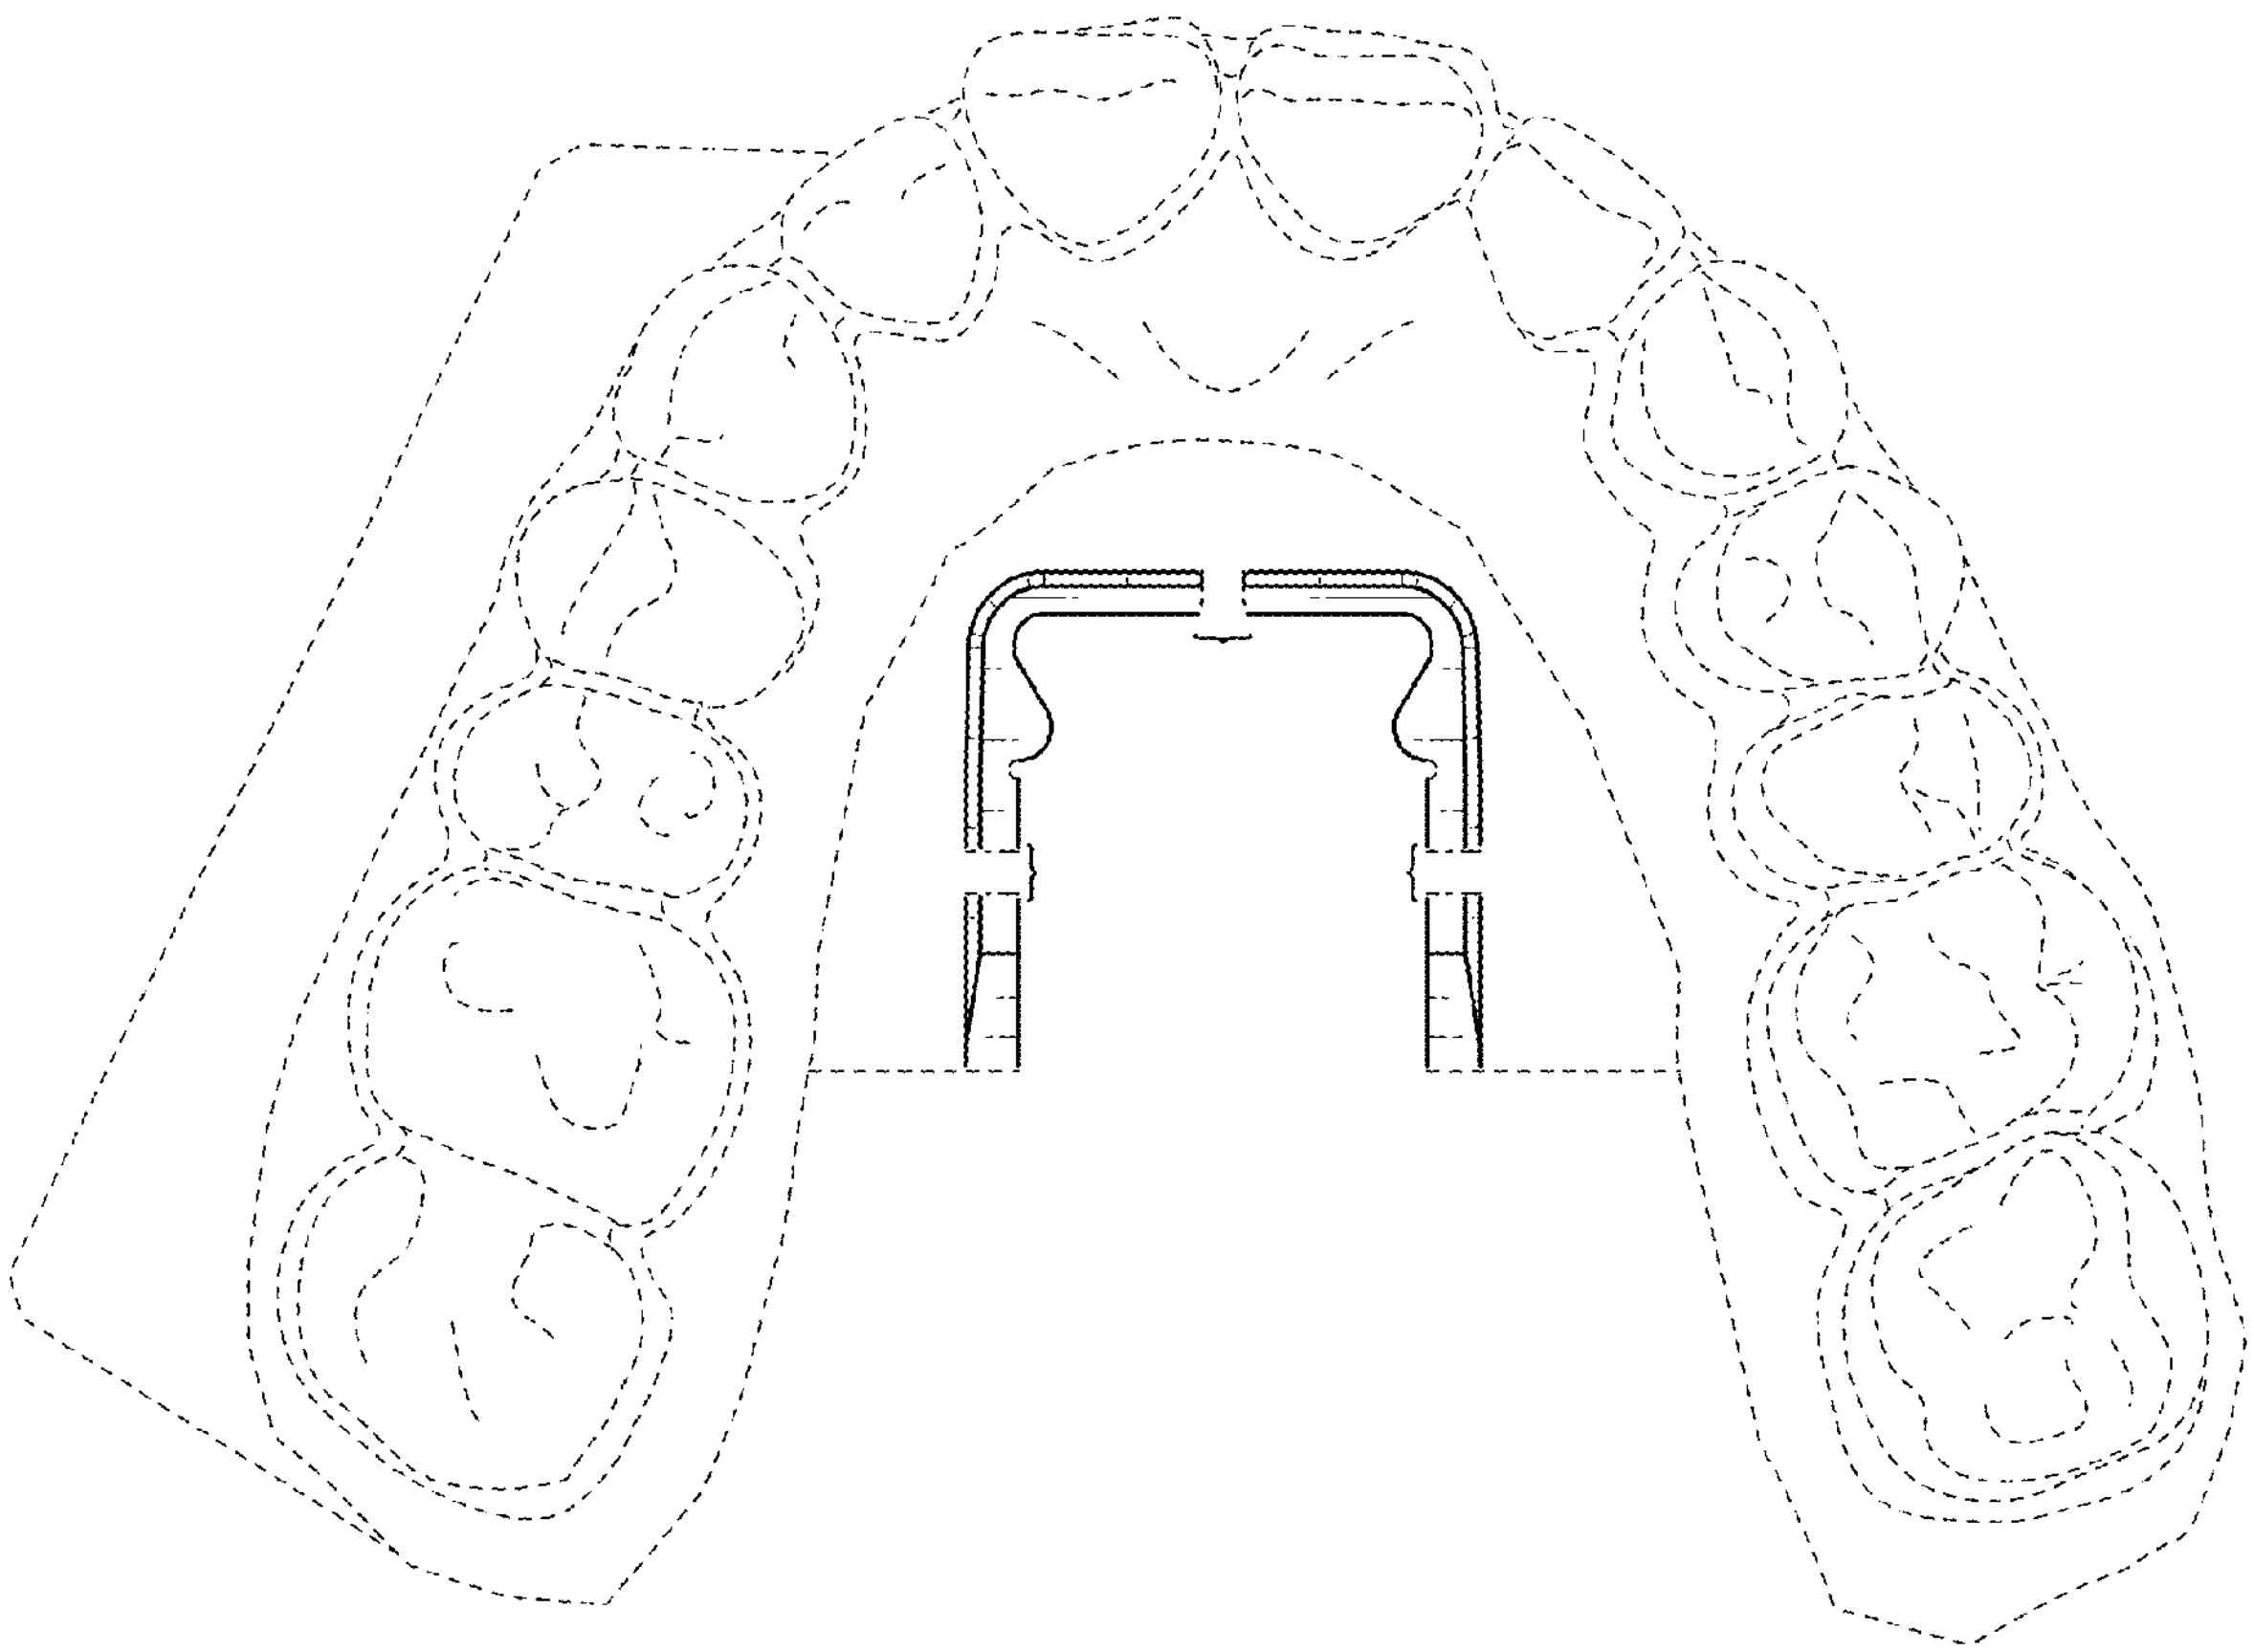

FIG. 23

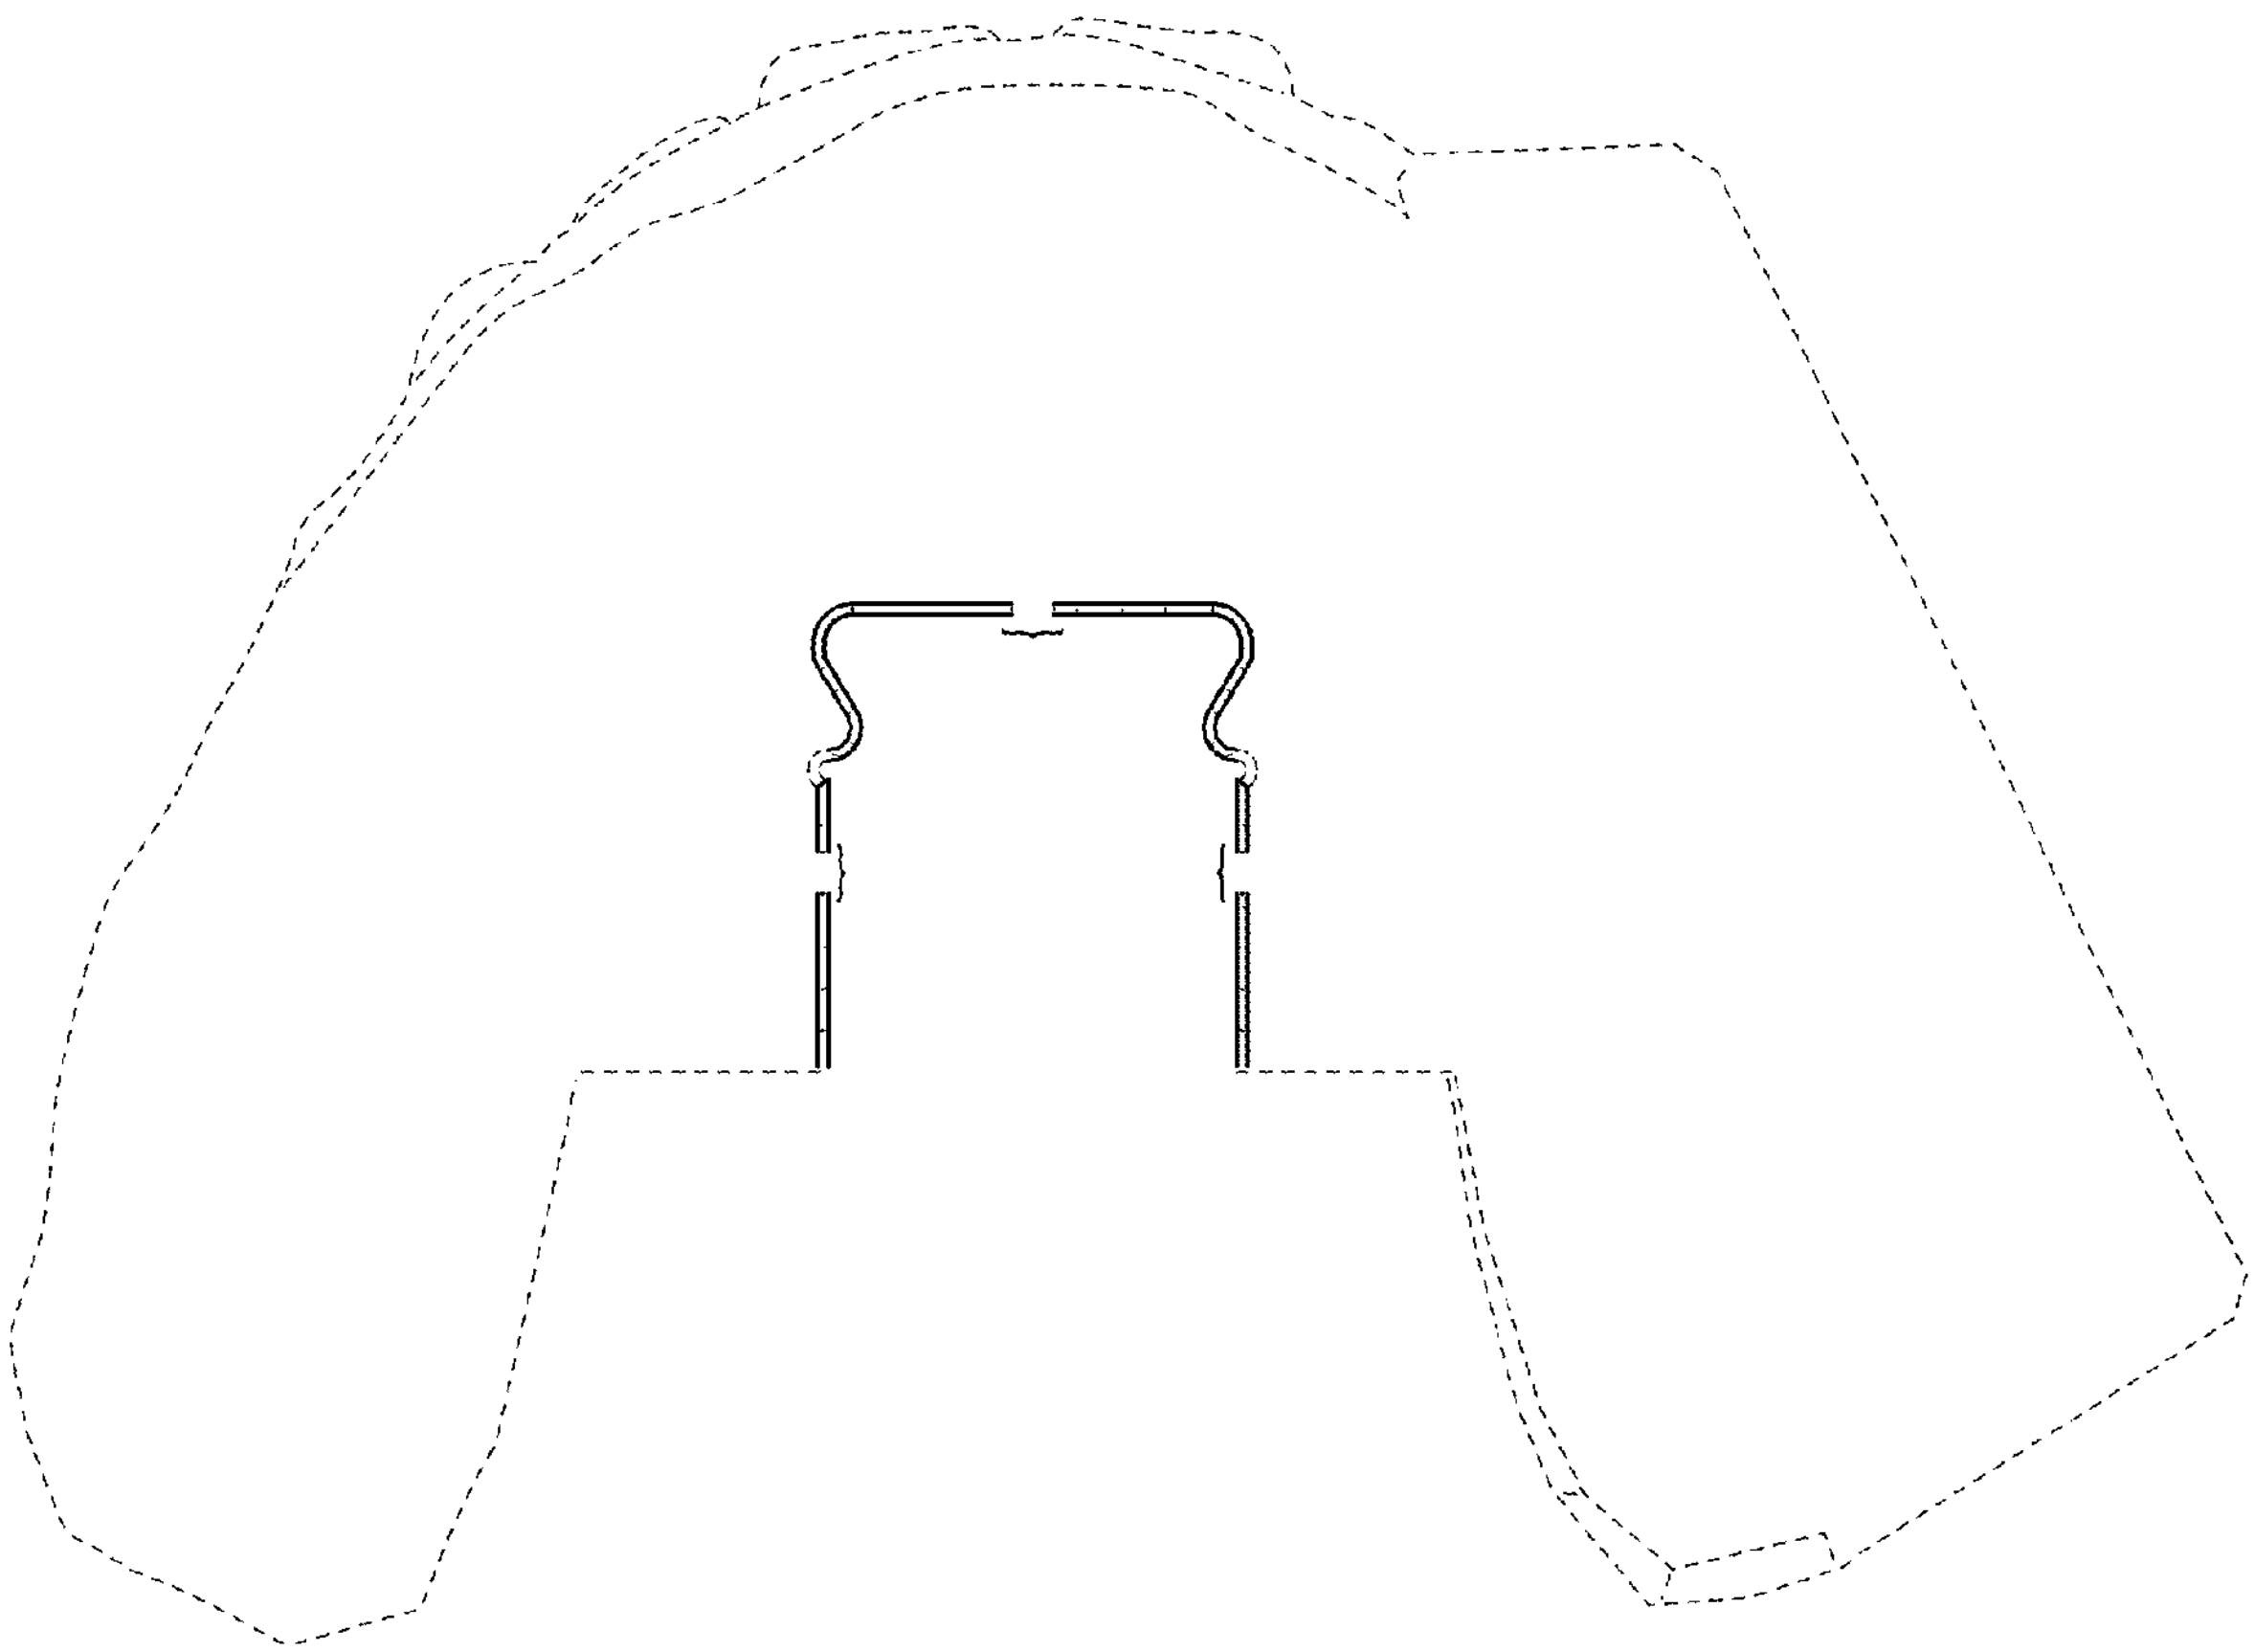

FIG. 24

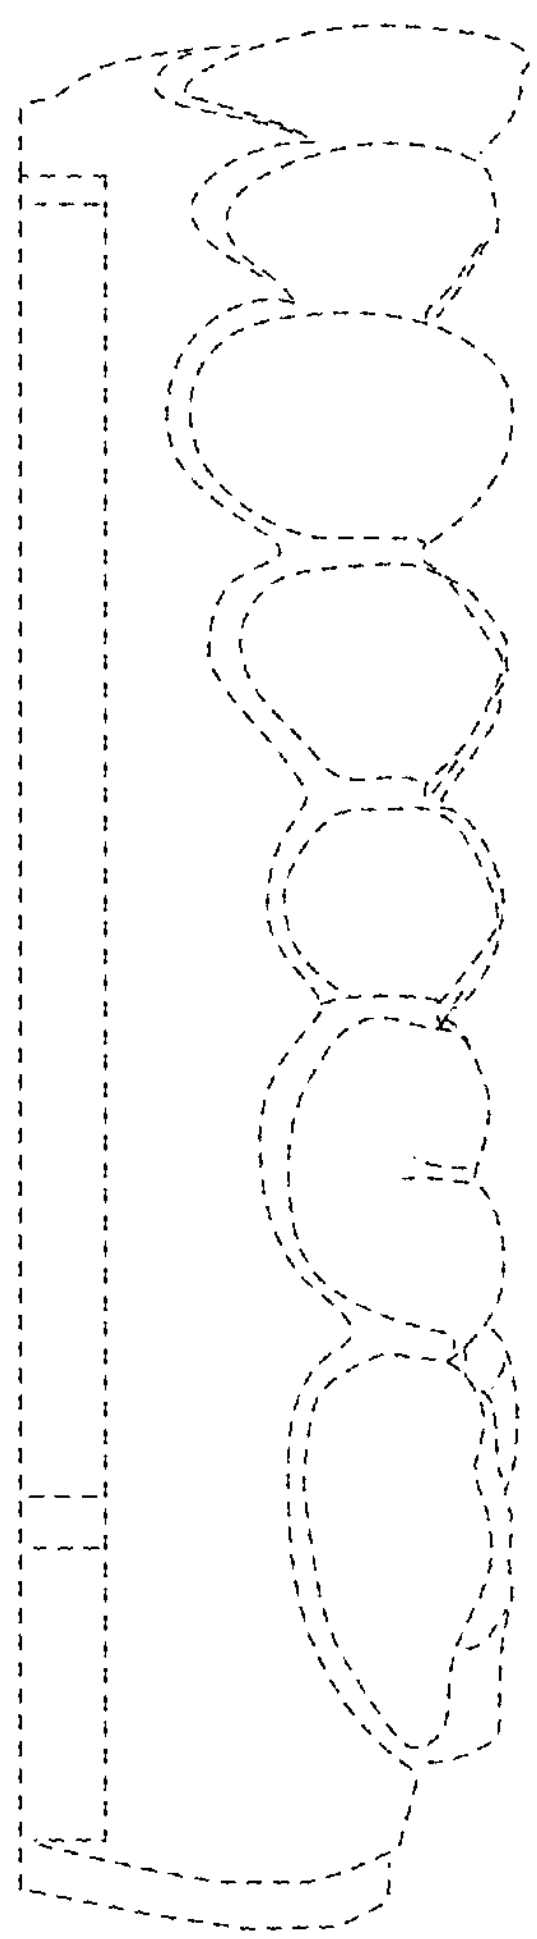

FIG. 25

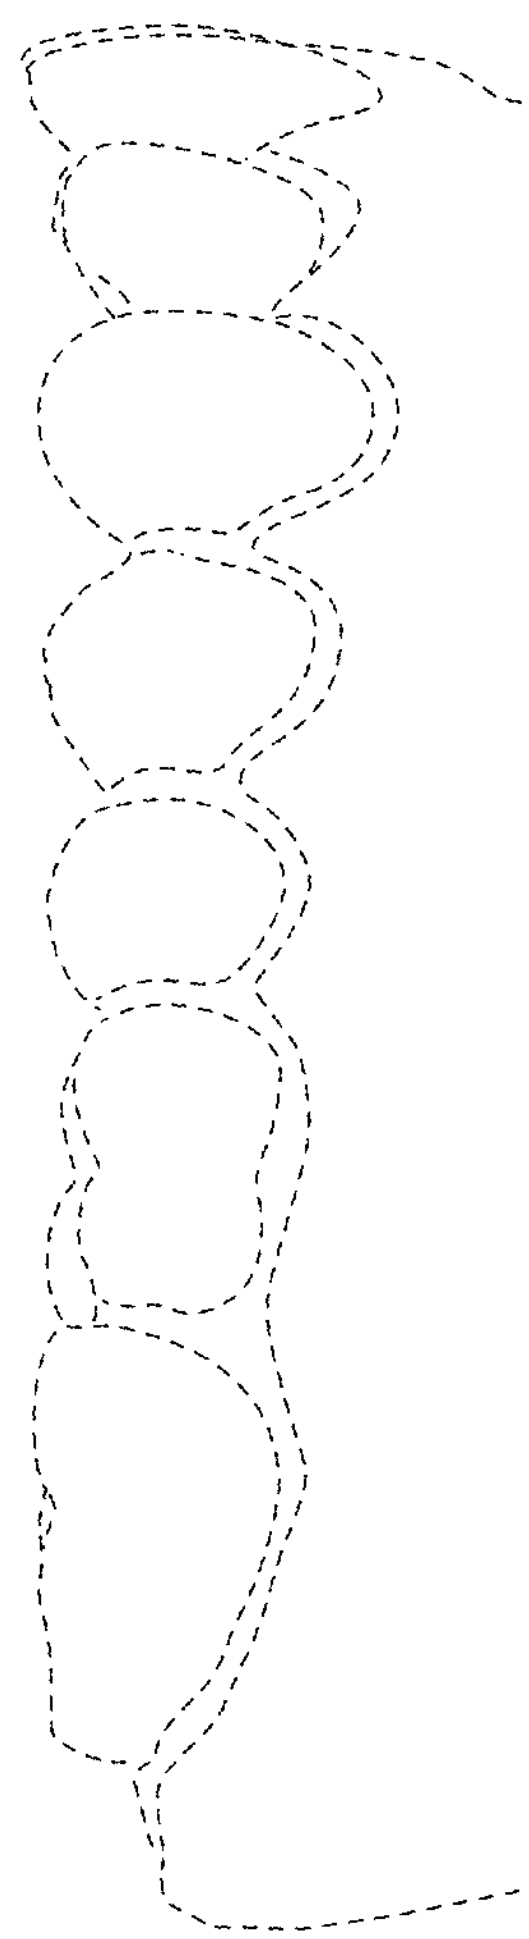

FIG. 26

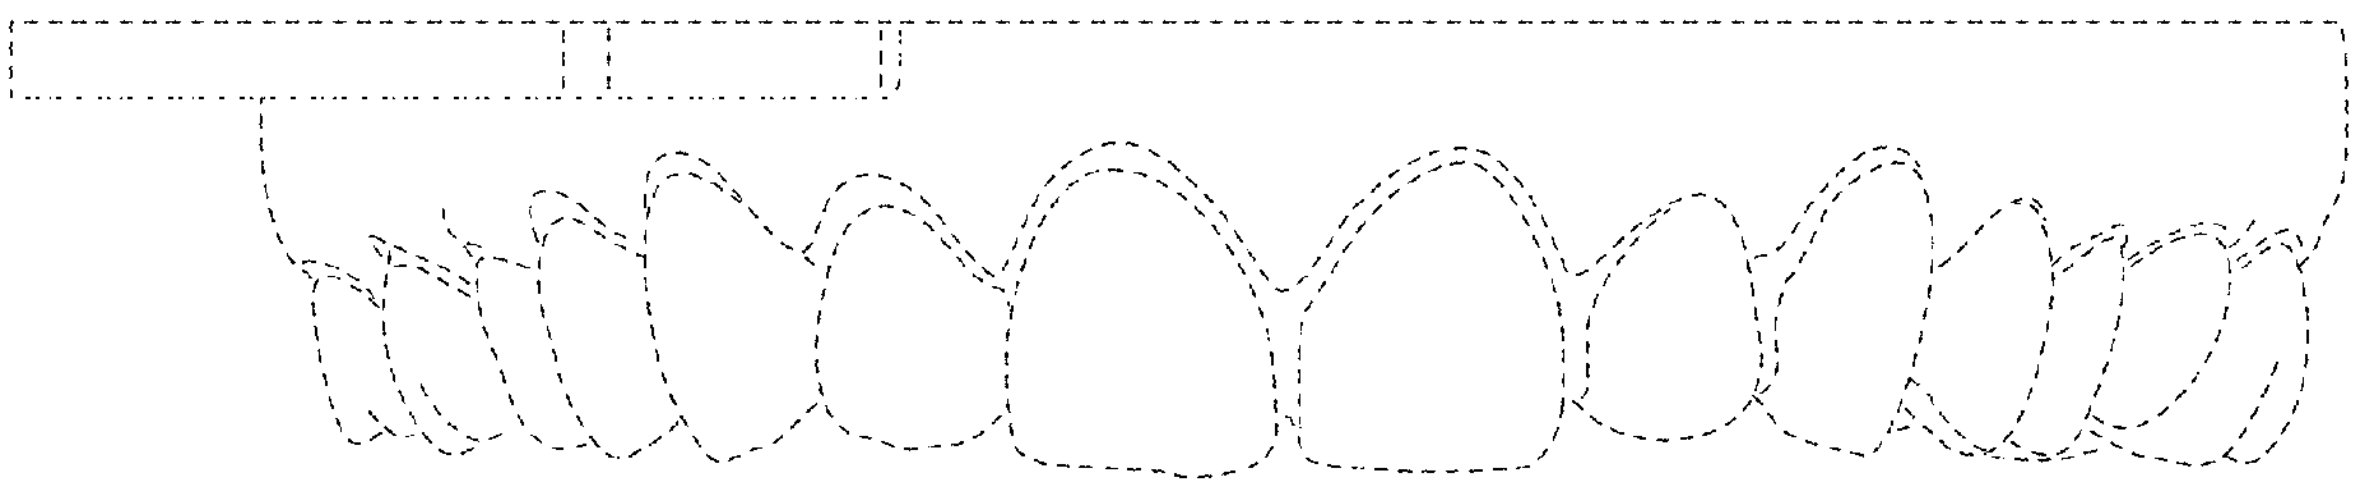

FIG. 27

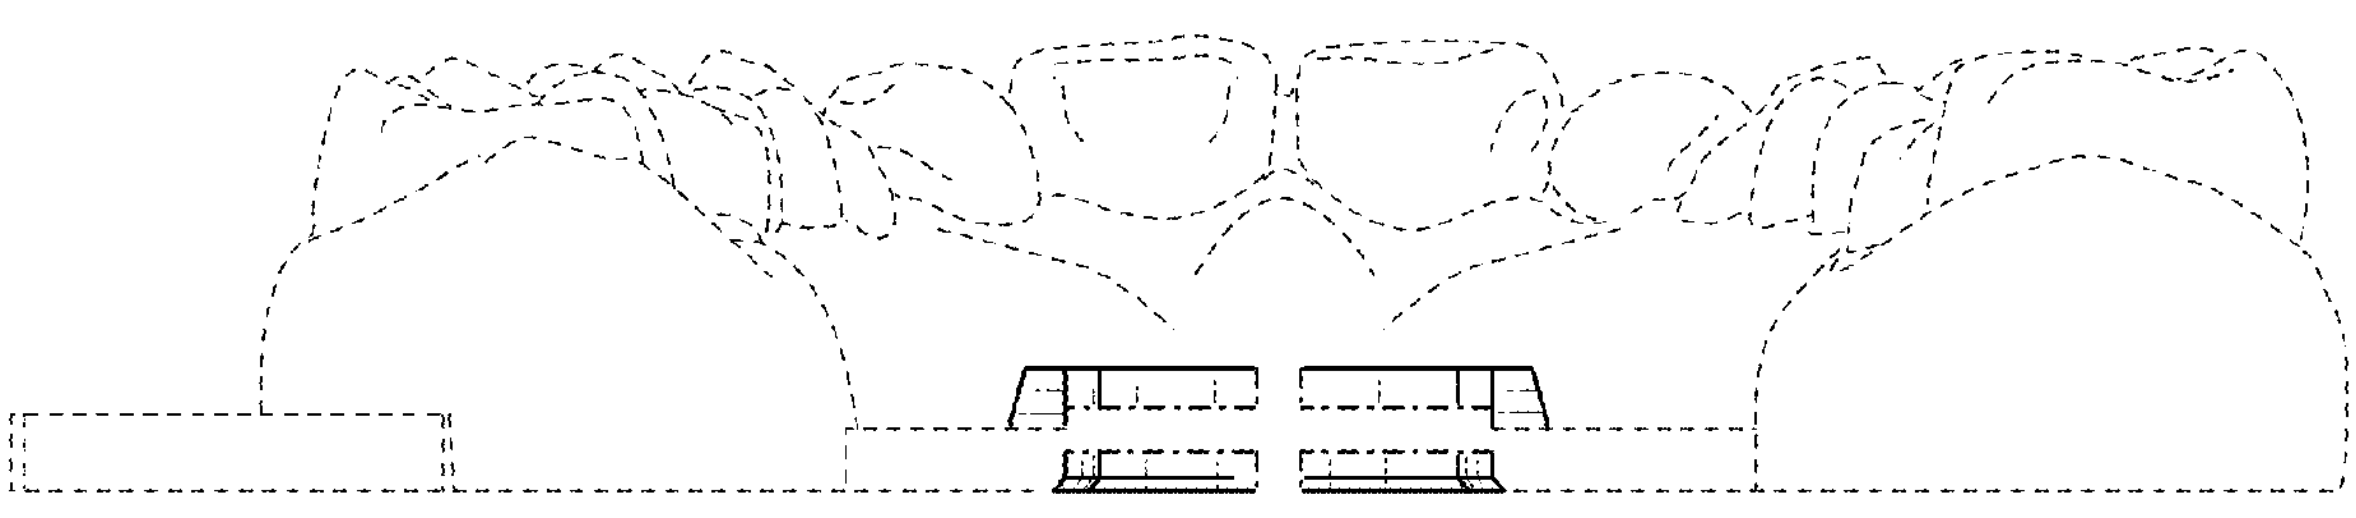

FIG. 28