US0D1092779S

(12) **United States Design Patent**
Ishizawa et al.

(10) **Patent No.: US D1,092,779 S**
(45) **Date of Patent: ** Sep. 9, 2025**

(54) **FLOW CHANNEL PLATE OF A CARTRIDGE FOR MEDICAL TESTING EQUIPMENT**

(71) Applicant: **Nikon Corporation**, Tokyo (JP)

(72) Inventors: **Naoya Ishizawa**, Saitama (JP); **Taro Ueno**, Tokyo (JP); **Ryo Kobayashi**, Kawasaki (JP)

(73) Assignee: **Nikon Corporation**, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/988,955**

(22) Filed: **Feb. 7, 2025**

Related U.S. Application Data

(62) Division of application No. 29/809,104, filed on Sep. 24, 2021, now Pat. No. Des. 1,066,733, which is a
(Continued)

(30) **Foreign Application Priority Data**

Mar. 22, 2018 (JP) 2018-006010
Mar. 22, 2018 (JP) 2018-006011
(Continued)

(51) **LOC (15) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/226**
(58) **Field of Classification Search**
USPC D24/107, 186, 216, 223–232; D10/81
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,983,038 A * 1/1991 Ohki G01N 15/1404
356/246
D371,749 S 7/1996 D'Orazio et al.
(Continued)

FOREIGN PATENT DOCUMENTS

JP D2020-13522 * 3/2021
KR 302015005.1181 10/2015

OTHER PUBLICATIONS

Fabrication of multilayered microfluidic 3D polymer packages. Online, published date Jul. 2005. Retrieved on Apr. 4, 2025 from URL: https://www.researchgate.net/figure/Polymer-based-disposable-microfluidic-cartridge-MycroLab_fig4_224614929.*
(Continued)

Primary Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

(57) **CLAIM**

The ornamental design for a flow channel plate of a cartridge for medical testing equipment, as shown and described.

DESCRIPTION

FIG. **1** is a perspective view of a flow channel plate of a cartridge for medical testing equipment showing our new design;
FIG. **2** is a front view thereof;
FIG. **3** is a top plan view thereof;
FIG. **4** is a right side view thereof;
FIG. **5** is an enlarged view of the portion defined by crop lines **5-5** in FIG. **1**; and,
FIG. **6** is an enlarged view of the portion defined by crop lines **6-6** in FIG. **2**.
The dashed lines depict portions of the flow channel plate of a cartridge for medical testing equipment that form no part of the claimed design. The dash-dotted lines depict the boundaries of the claimed design and form no part thereof.

1 Claim, 5 Drawing Sheets

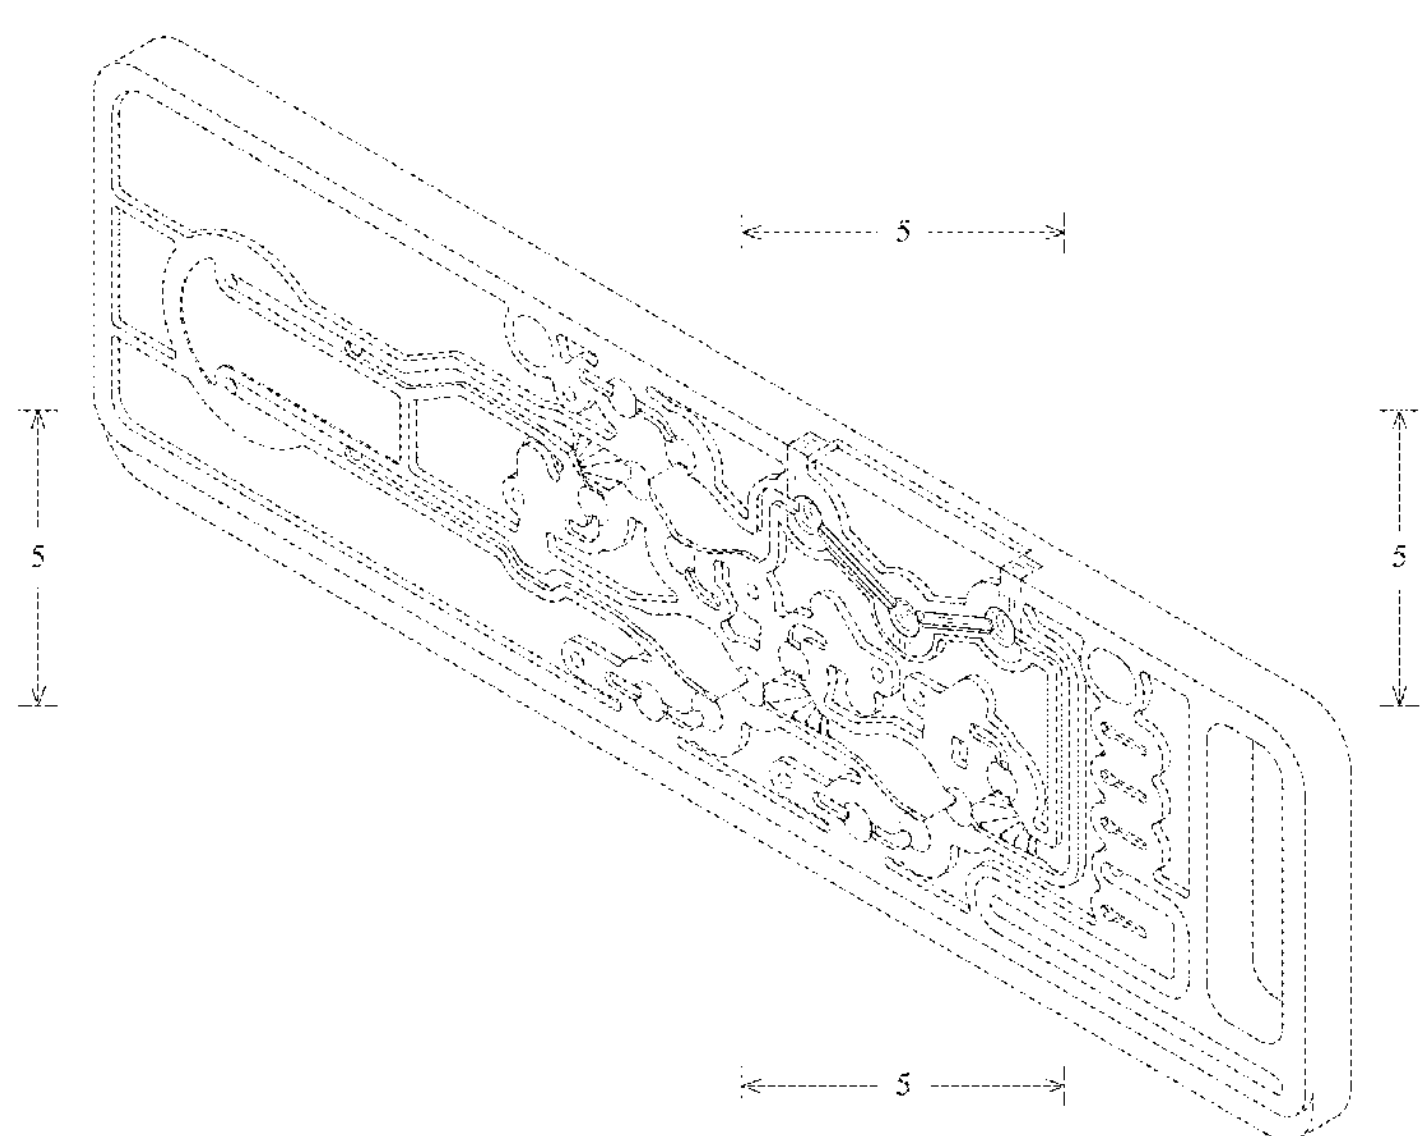

Related U.S. Application Data

division of application No. 29/664,120, filed on Sep. 21, 2018, now Pat. No. Des. 933,253.

(30) **Foreign Application Priority Data**

Mar. 22, 2018 (JP) 2018-006012
Mar. 22, 2018 (JP) 2018-006013
Mar. 22, 2018 (JP) 2018-006014

(58) **Field of Classification Search**
CPC B01L 3/50; B01L 3/545; B01L 3/502738; G01N 33/558
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D472,324 S 3/2003 Rumore et al.
D530,021 S 10/2006 Muraca
D621,060 S 8/2010 Handique
D669,594 S 10/2012 Cao et al.
8,440,149 B2 * 5/2013 Handique B01L 7/00 422/547
D732,186 S 6/2015 Burroughs et al.
D757,782 S 5/2016 Moriya
D767,782 S 9/2016 Cao et al.
D785,811 S 5/2017 Watts et al.
D794,817 S 8/2017 Yi et al.
D803,416 S 11/2017 Leaver et al.
D812,242 S 3/2018 Chang et al.
D812,766 S 3/2018 Levner et al.
D814,654 S 4/2018 Daines
D816,861 S 5/2018 Levner et al.
D843,009 S 3/2019 Watts et al.
D851,275 S 6/2019 Spuhler et al.
D887,999 S * 6/2020 Chen D13/182
10,835,898 B2 11/2020 Olsson et al.
D933,253 S 10/2021 Ishizawa et al.
D993,444 S 7/2023 Masuda
D1,004,128 S * 11/2023 George D24/225
D1,066,733 S * 3/2025 Ishizawa D24/226
2004/0184964 A1 * 9/2004 Watanabe B01F 25/4331 422/502
2007/0249062 A1 * 10/2007 Kageyama B01L 3/502746 436/514
2012/0267239 A1 * 10/2012 Chen B01L 3/502715 228/159
2015/0087079 A1 3/2015 Coffey et al.
2020/0249232 A1 * 8/2020 Konstantopoulos A61P 35/00
2020/0406263 A1 * 12/2020 Milgram B01L 3/502776
2021/0346887 A1 * 11/2021 Kobayashi B01L 3/502738
2021/0348992 A1 11/2021 Kobayashi et al.

OTHER PUBLICATIONS

[No Author Listed], Multi-Site Cartridge Carriers. Online, published date unknown. Retrieved on Jan. 12, 2020, from URL: https://www.testfixtures.com/cartridge-carrier-prototyping-test-sockets.
[No Author Listed], New Illumina Nexseq 500/550 Mid-Output Flowcell Cartridge Sequencing System. Online published date unknown. Retrieved on Nov. 1, 2024 from URL: https://spwindustrial.com/new-illumina-nexseq-500-550-mid-output-flowcell-cartridge-sequencing-system/.

* cited by examiner

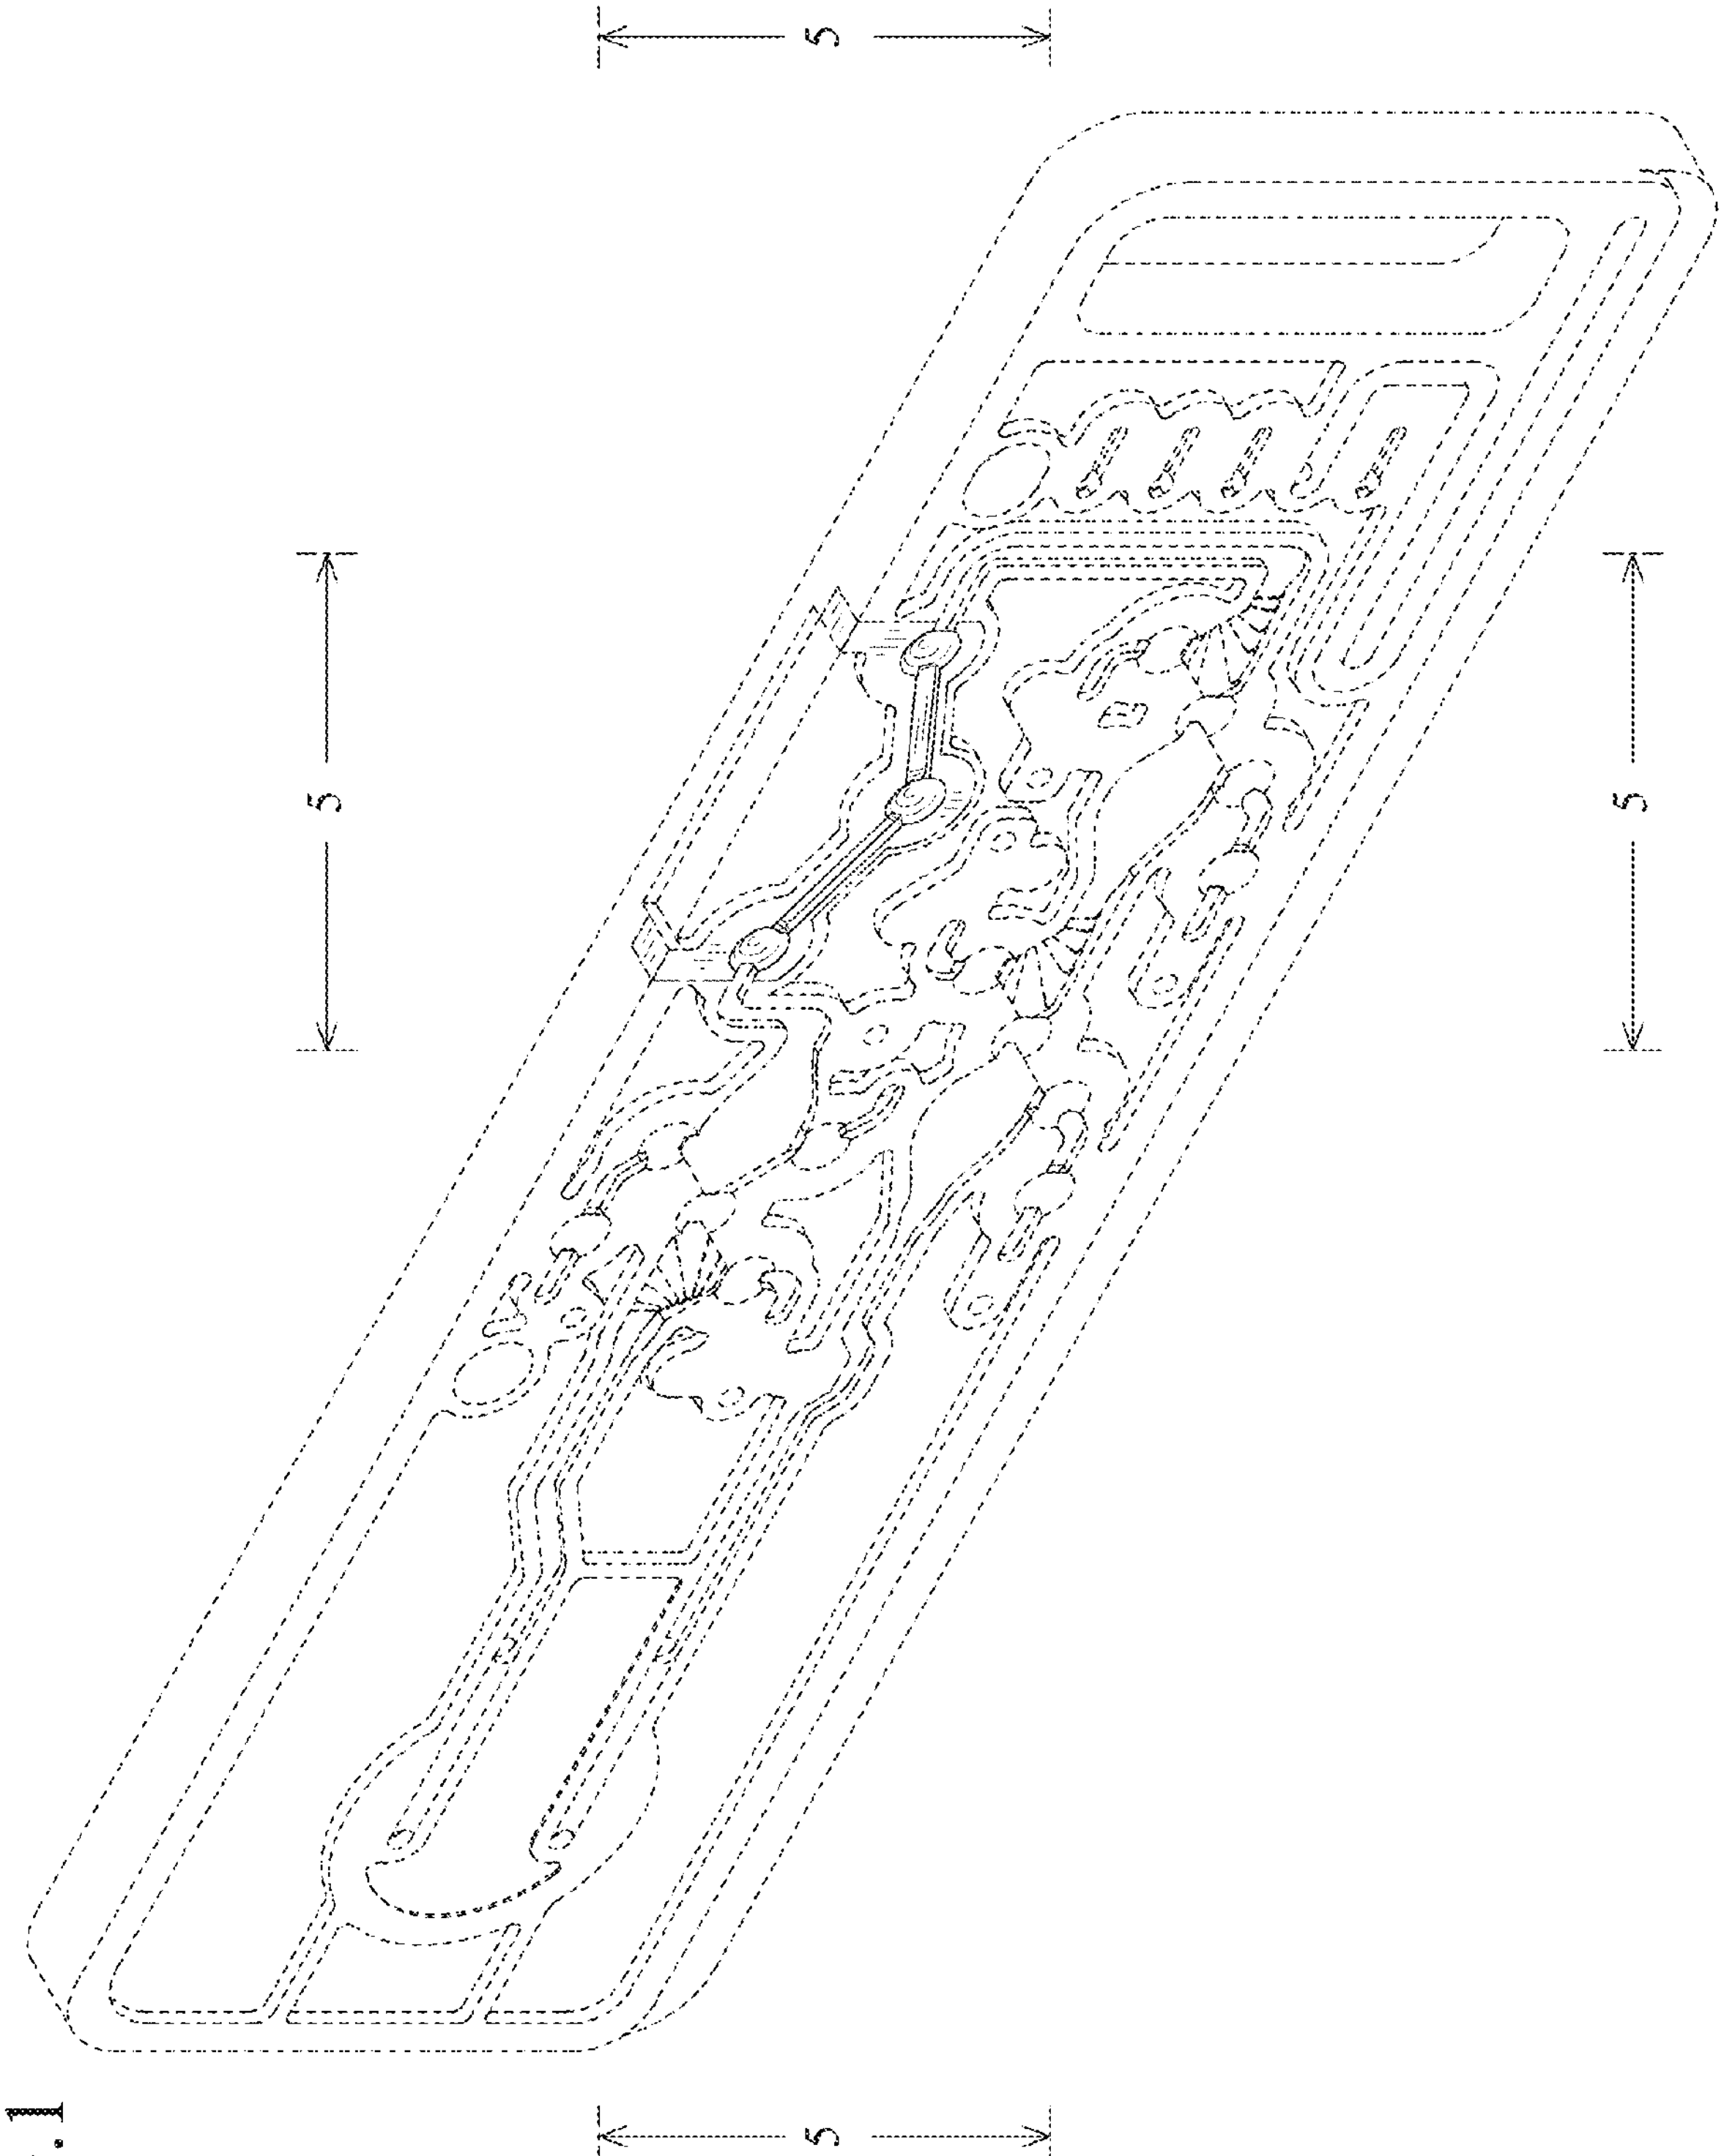

FIG.1

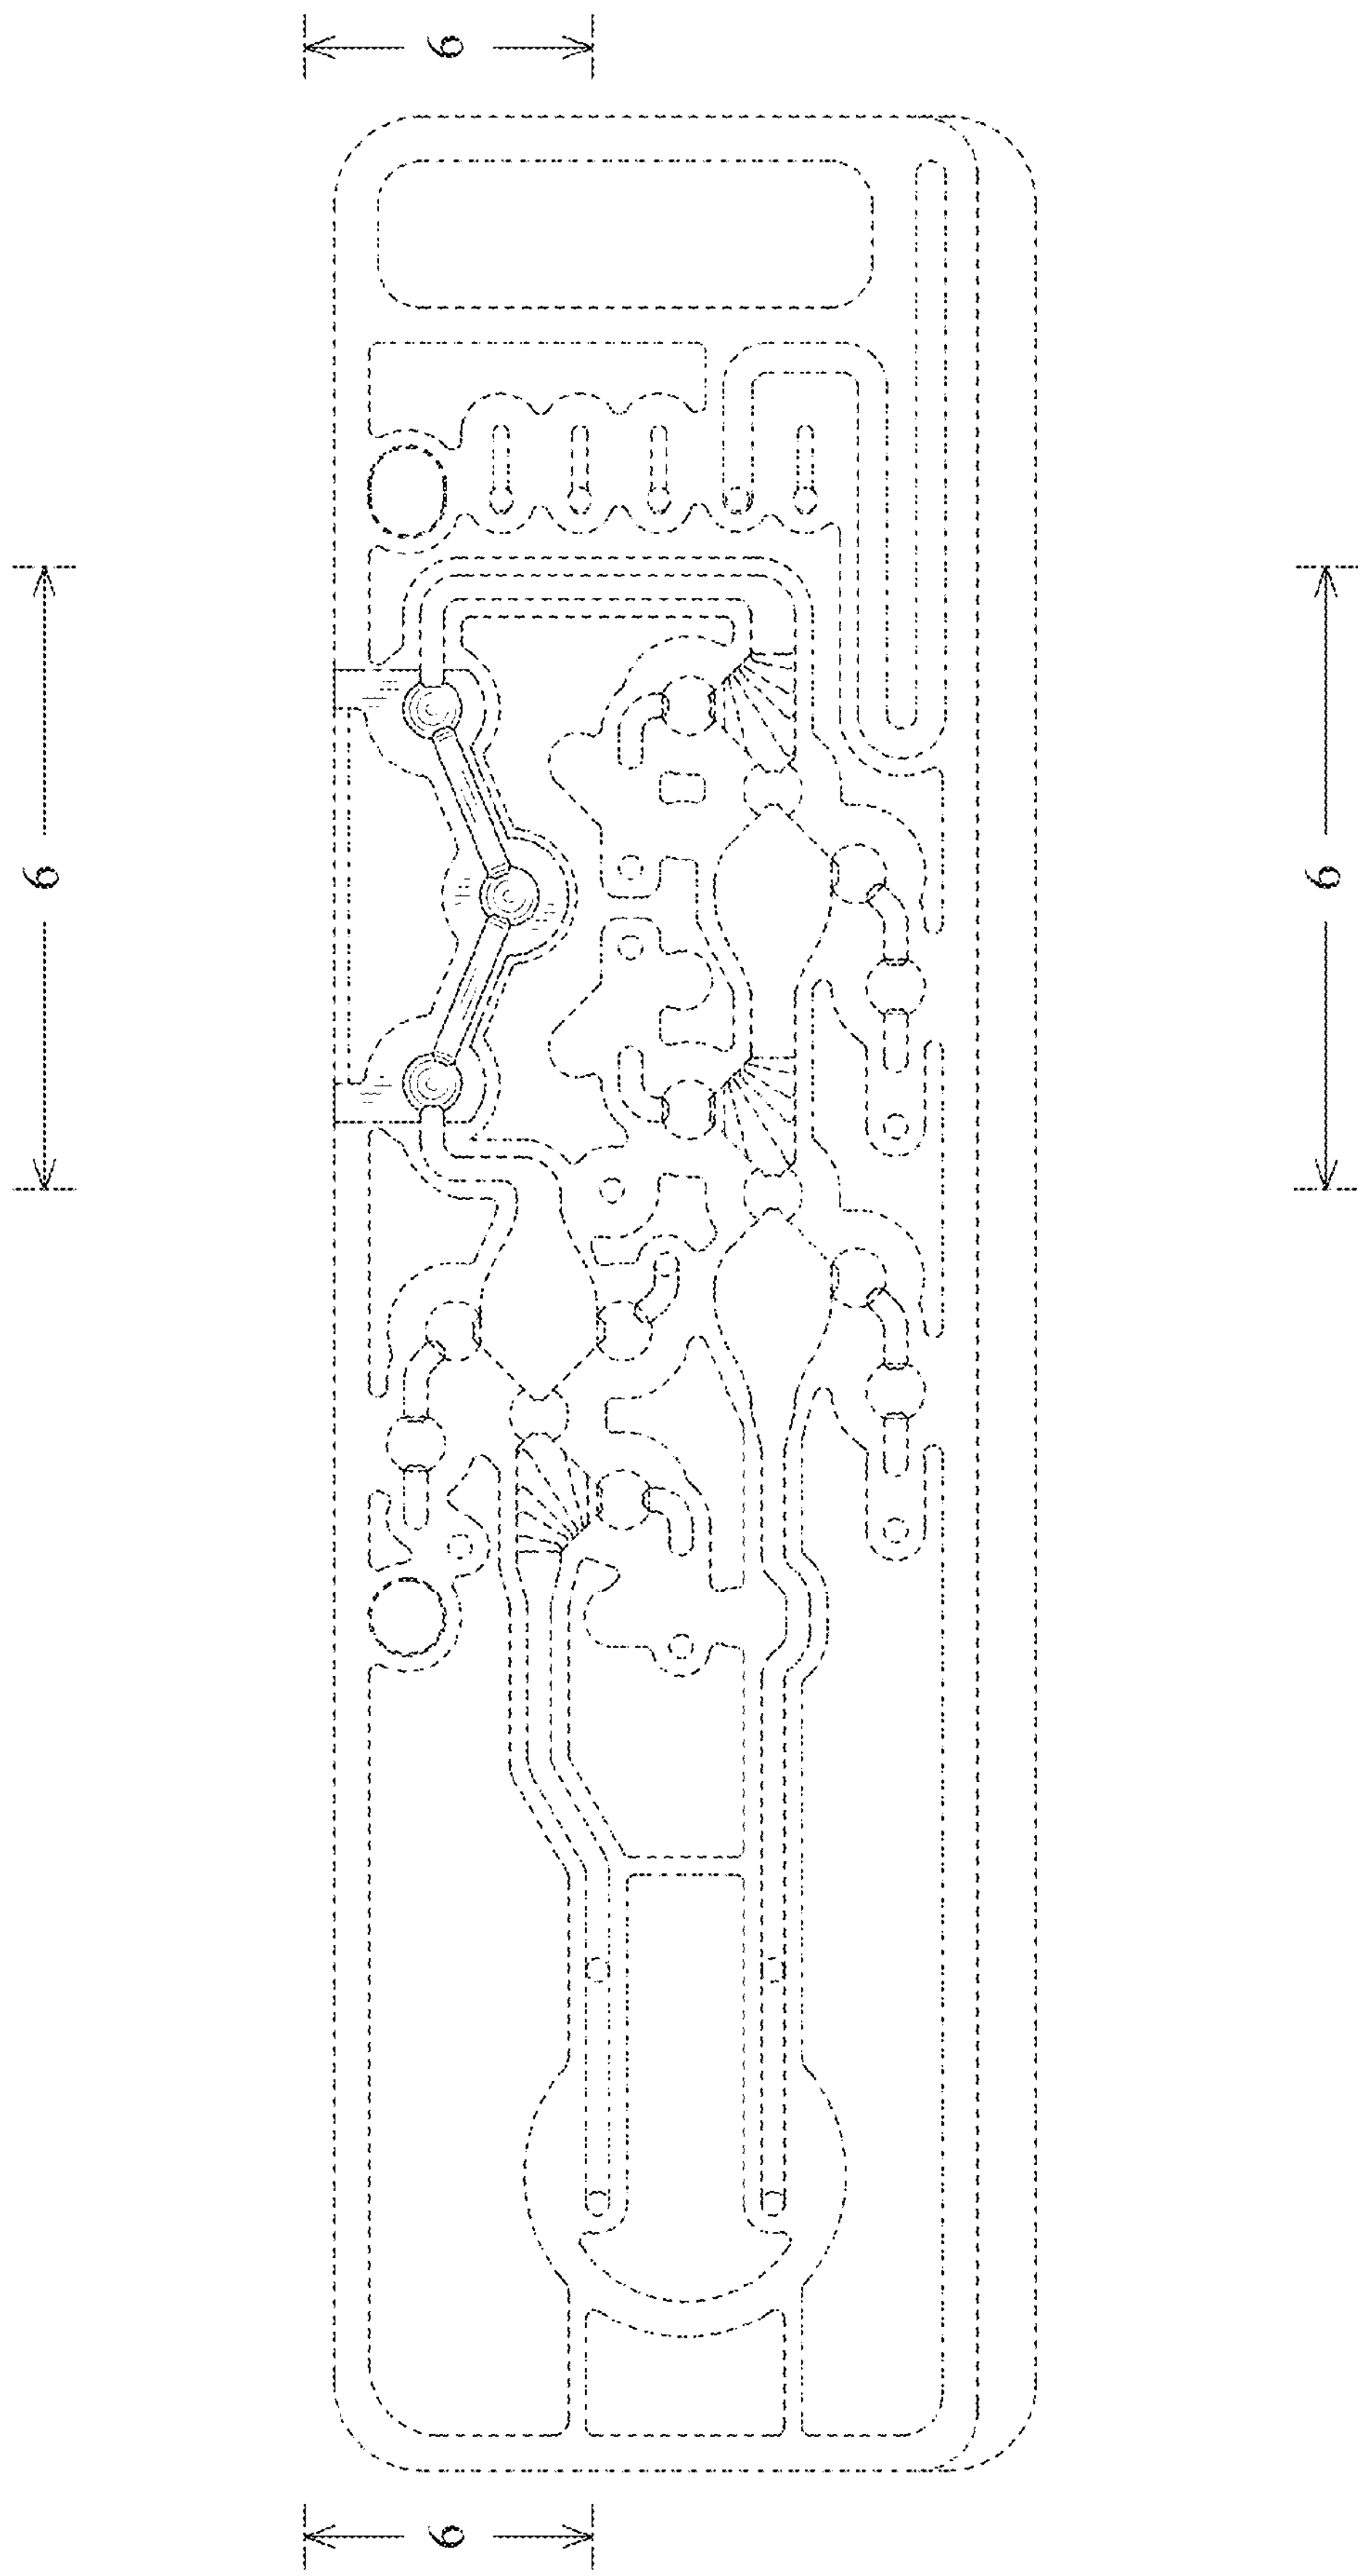

FIG.2



FIG.3



FIG.4

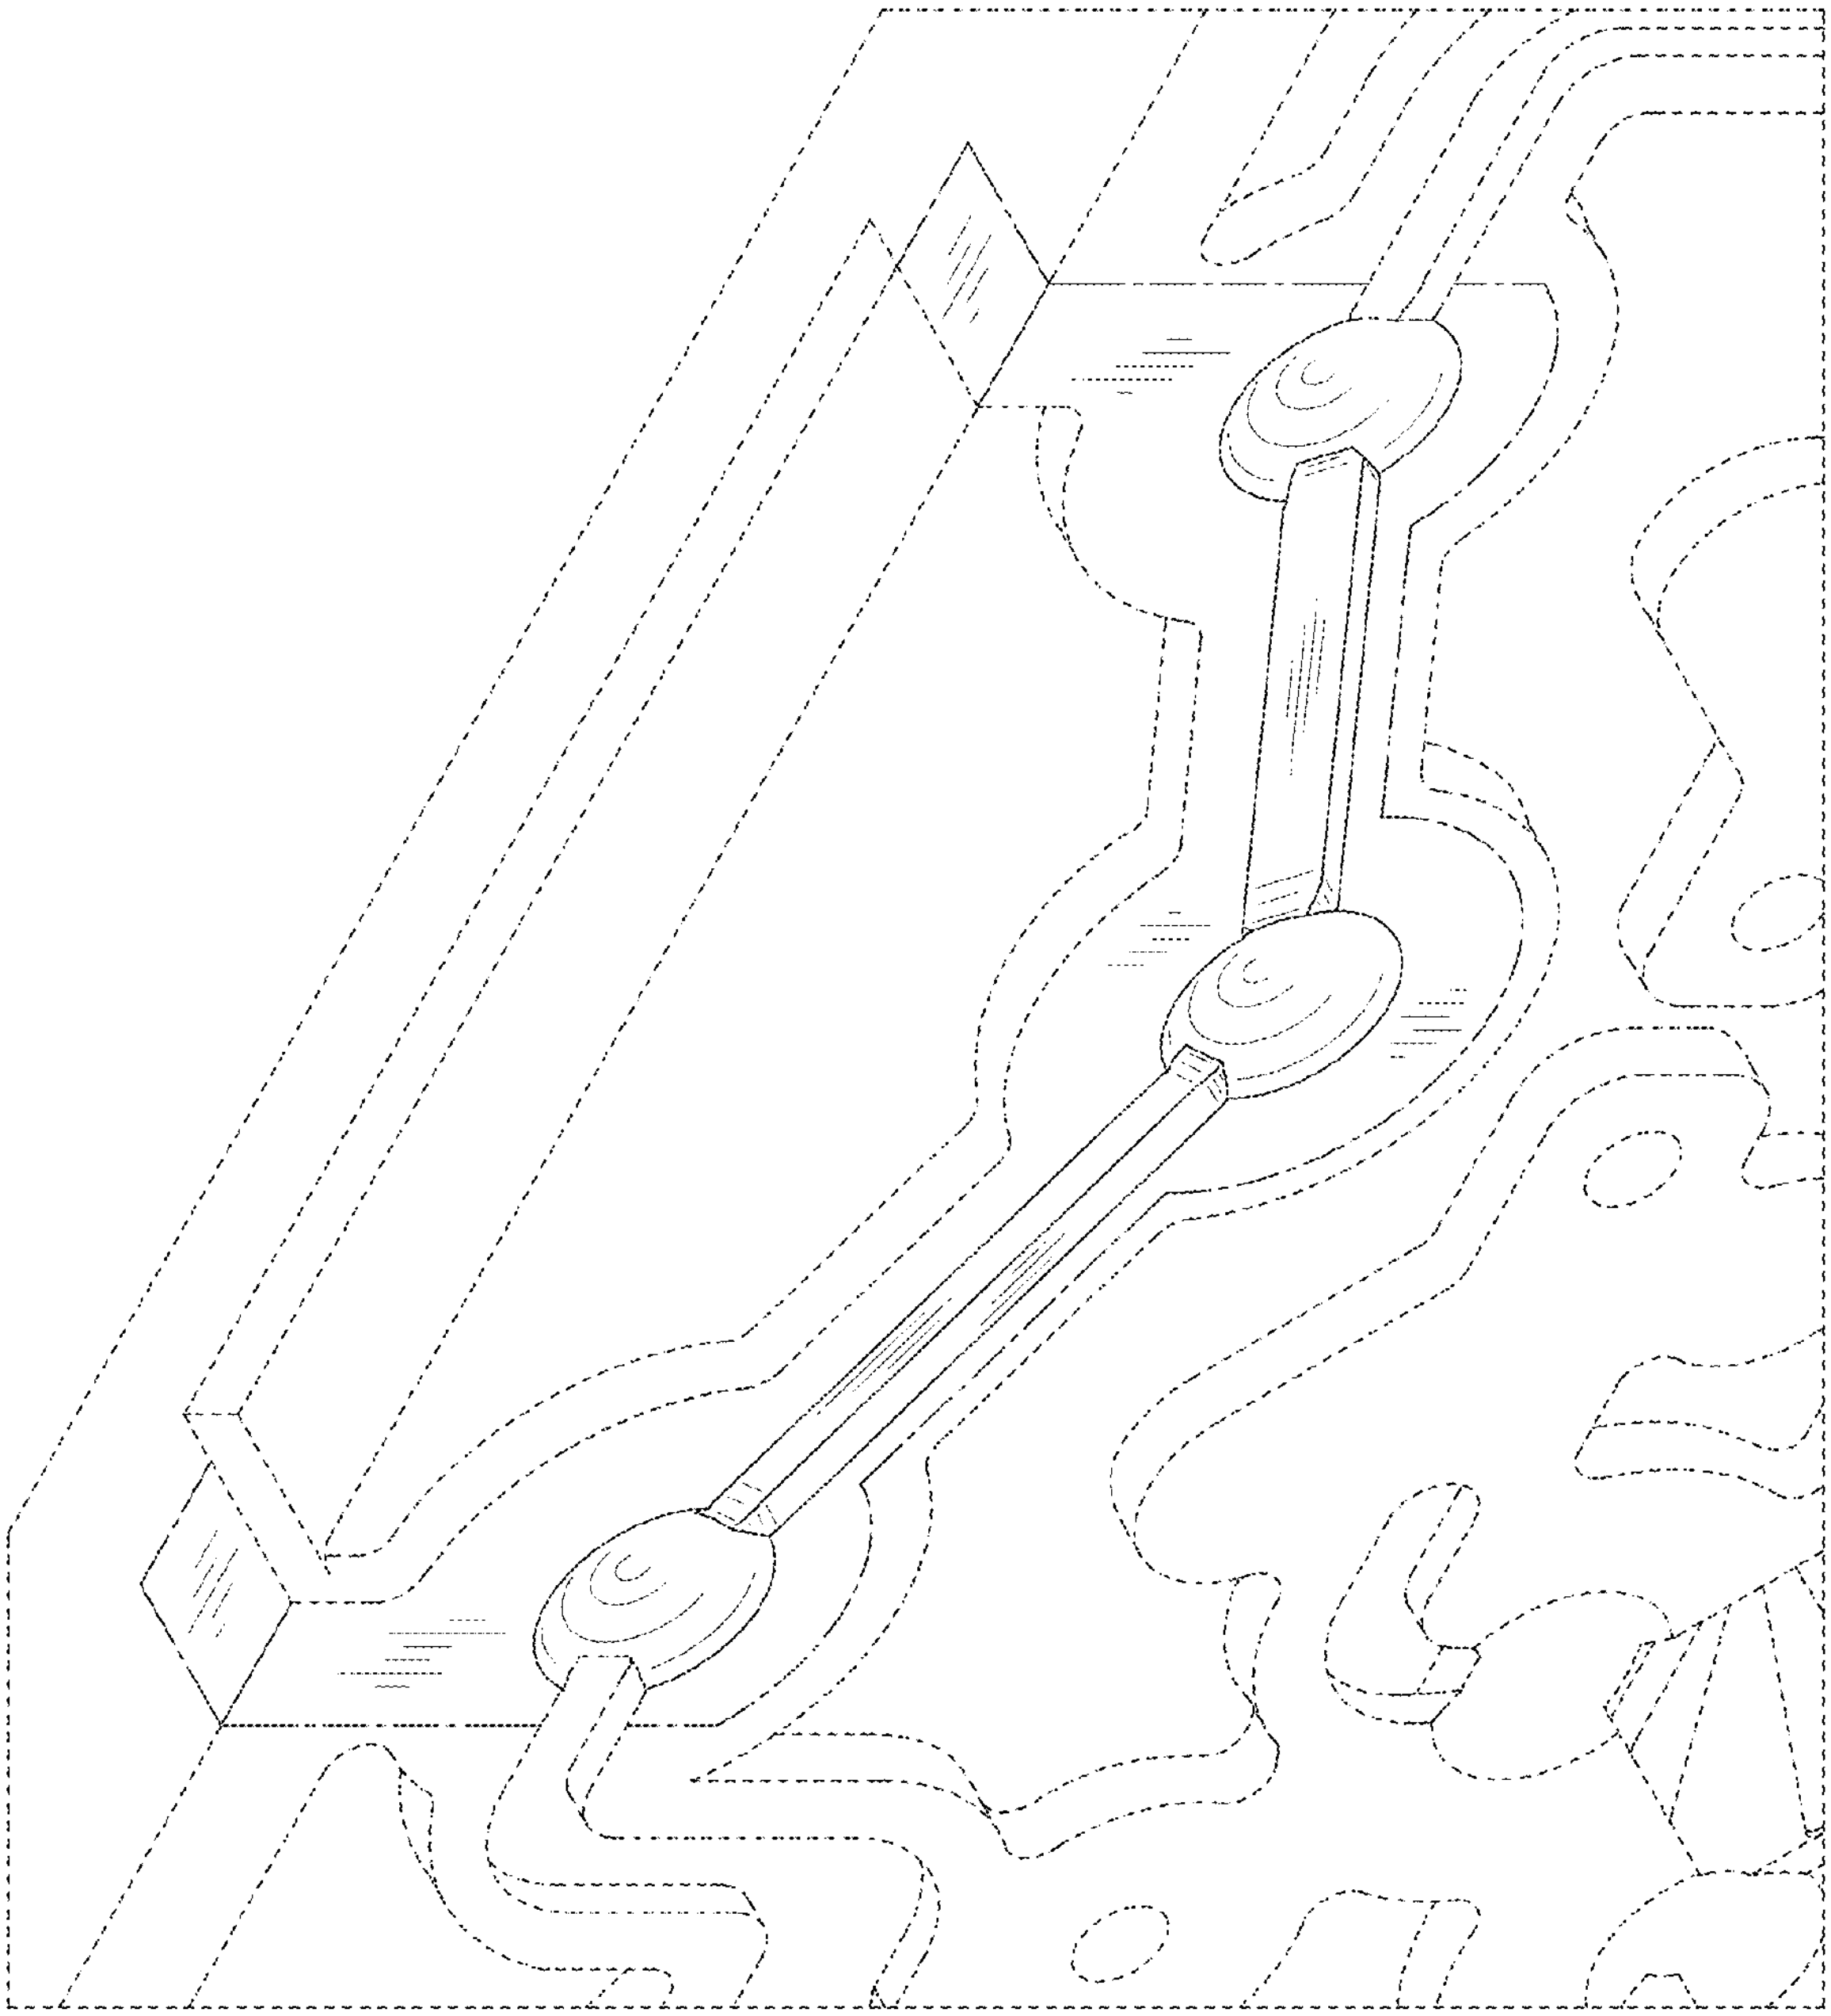

FIG.5

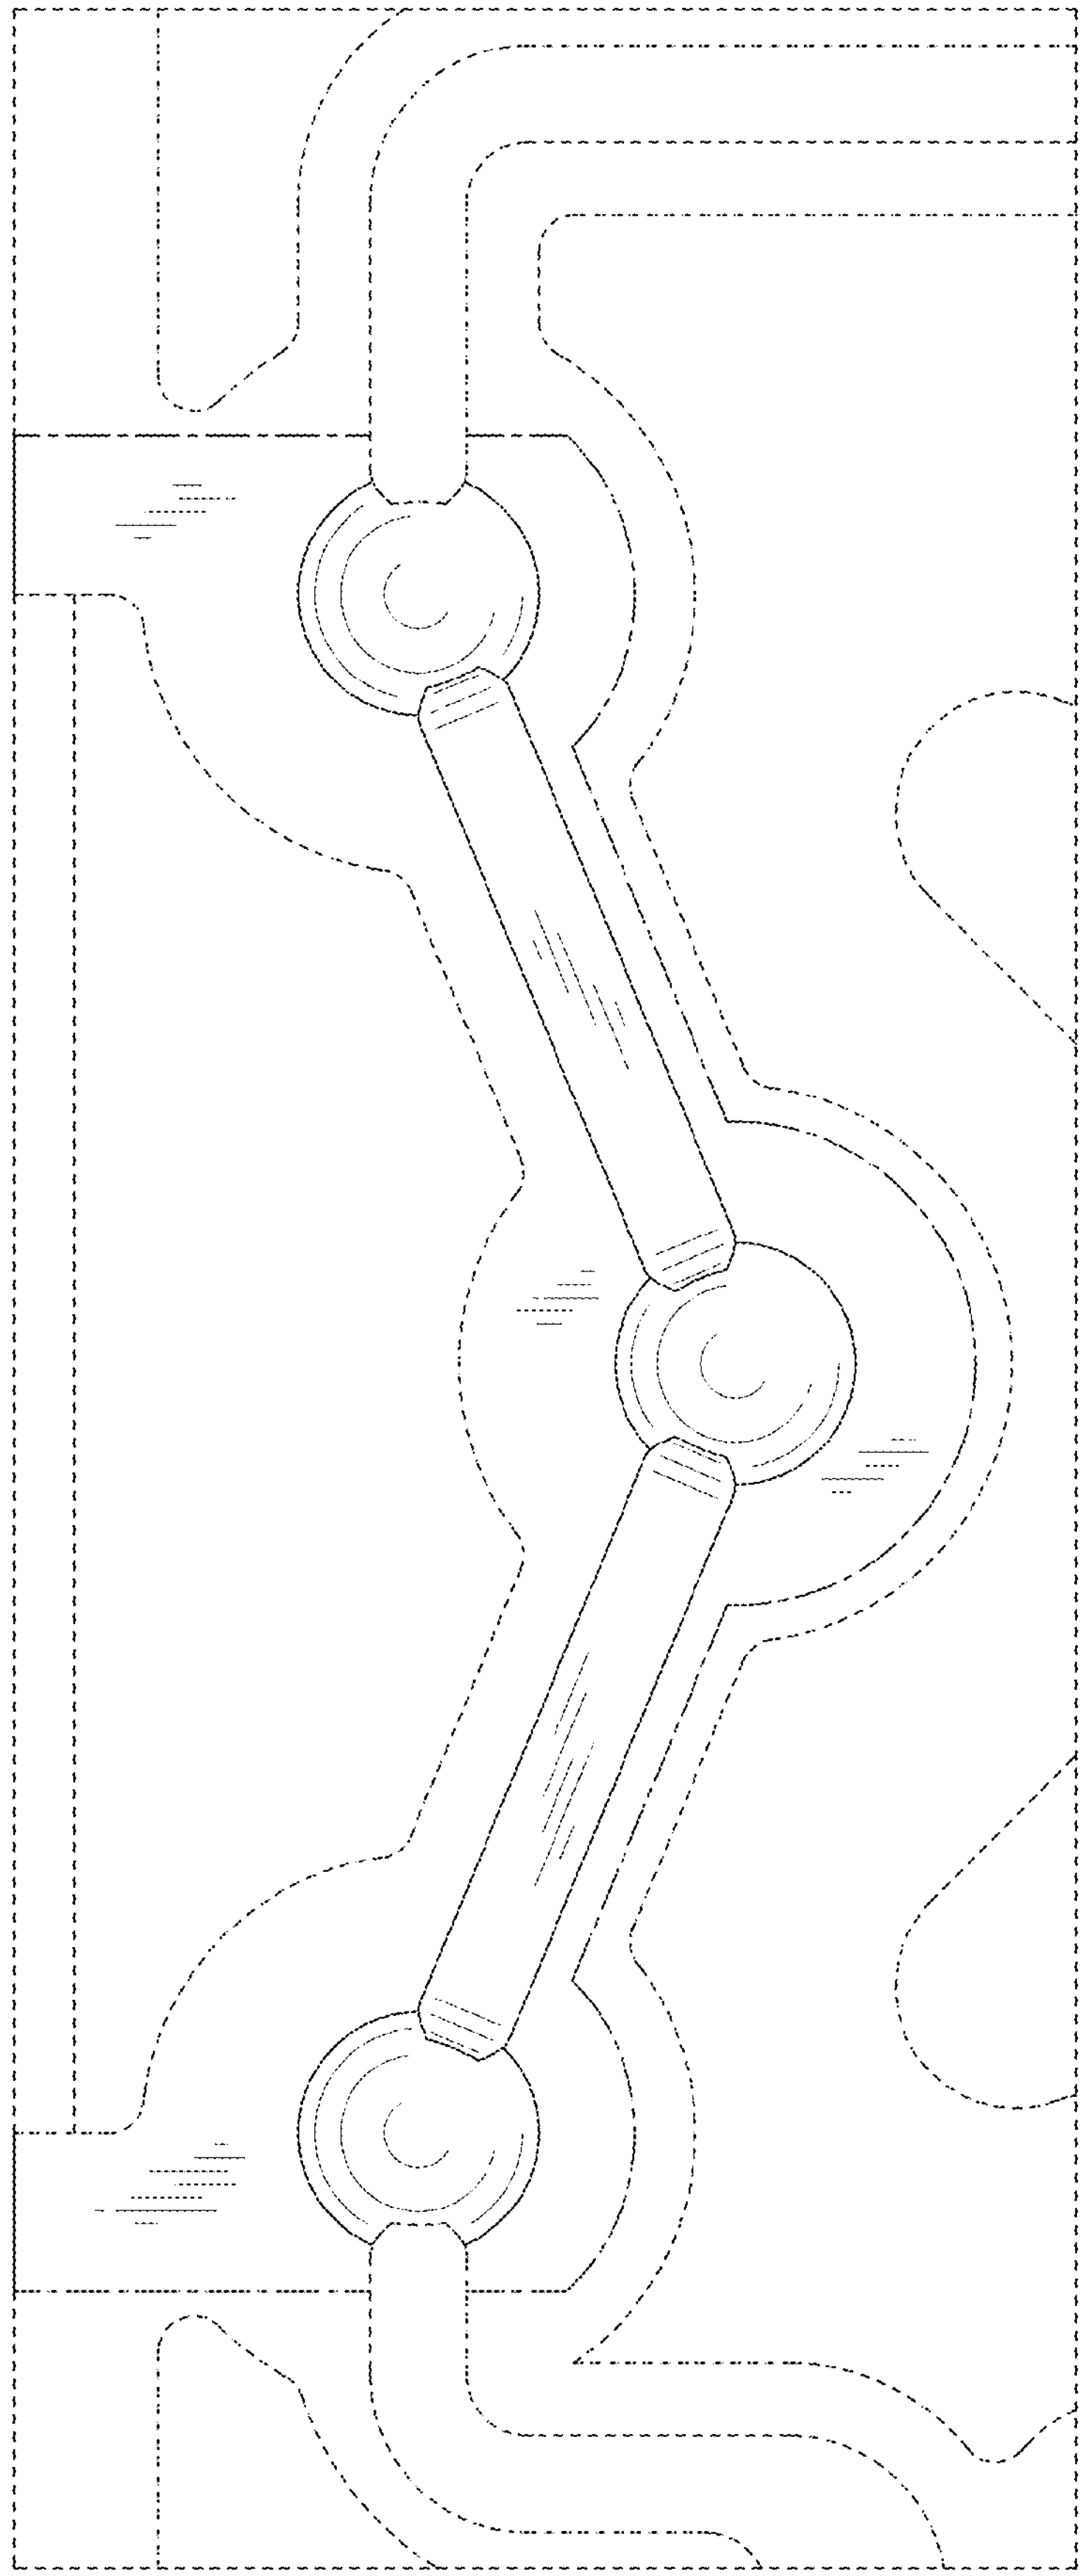

FIG.6