US0D1087801S

(12) **United States Design Patent**
Bathany et al.

(10) **Patent No.: US D1,087,801 S**
(45) **Date of Patent: ** Aug. 12, 2025**

(54) **SAMPLE COLLECTION DEVICE**

(71) Applicant: **Siro Diagnostics, Inc.**, San Diego, CA (US)

(72) Inventors: **Cedric Bathany**, Vista, CA (US); **Michael David Jacobson**, San Diego, CA (US); **Clint Sever**, San Diego, CA (US)

(73) Assignee: **Siro Diagnostics, Inc.**, San Diego, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/861,512**

(22) Filed: **Nov. 30, 2022**

(51) **LOC (15) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/224**; D24/216
(58) **Field of Classification Search**
USPC D24/107, 108, 115, 120–123, 130, 216, D24/224; D9/501, 519, 537, 549, 723, D9/724
CPC A61B 10/0045; A61B 5/14; A61B 5/15; A61B 10/0051; A61B 10/0048; A61B 10/0058; A61B 10/0064; A61B 10/0096; B01L 3/5023; B01L 3/50; B01L 3/505; B01L 3/508; B01L 3/52; B01L 3/523
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D115,326 S		6/1939	Chott	
D249,062 S		8/1978	Crafoord et al.	
D254,445 S	*	3/1980	Boghosian	D24/224
4,298,011 A		11/1981	Mangurten et al.	
D303,288 S		9/1989	Harboe et al.	
D306,067 S		2/1990	Bogdanoff et al.	
D307,052 S		4/1990	Baxter	
D331,625 S		12/1992	Price et al.	

(Continued)

FOREIGN PATENT DOCUMENTS

CN	306384884	3/2021
GB	2 430 032 A	3/2007

(Continued)

OTHER PUBLICATIONS

"Danrl: Inside the Cue Covid-19 Test Cartridge." Found online Sep. 6, 2024 at danrl.com. Reference dated Jan. 2022. Retrieved from https://danrl.com/cue19/.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton
Assistant Examiner — Elizabeth S Struble
(74) *Attorney, Agent, or Firm* — Foley & Lardner LLP

(57) **CLAIM**

The ornamental design for a sample collection device as shown and described.

DESCRIPTION

FIG. **1** is a top, front, right side perspective view of a sample collection device;
FIG. **2** is a bottom, rear, left side perspective view thereof;
FIG. **3** is a top plan view thereof;
FIG. **4** is a bottom plan view thereof;
FIG. **5** is a right side elevation view thereof;
FIG. **6** is a left side elevation view thereof;
FIG. **7** is a front elevation view thereof;
FIG. **8** is a rear elevation view thereof;
FIG. **9** is a cross-section view thereof taken along line **9-9** of FIG. **7**; and,
FIG. **10** is a cross-section view thereof taken along line **10-10** of FIG. **7**.
The broken lines in the drawings are for illustrative purposes only and form no part of the claimed design.

1 Claim, 6 Drawing Sheets

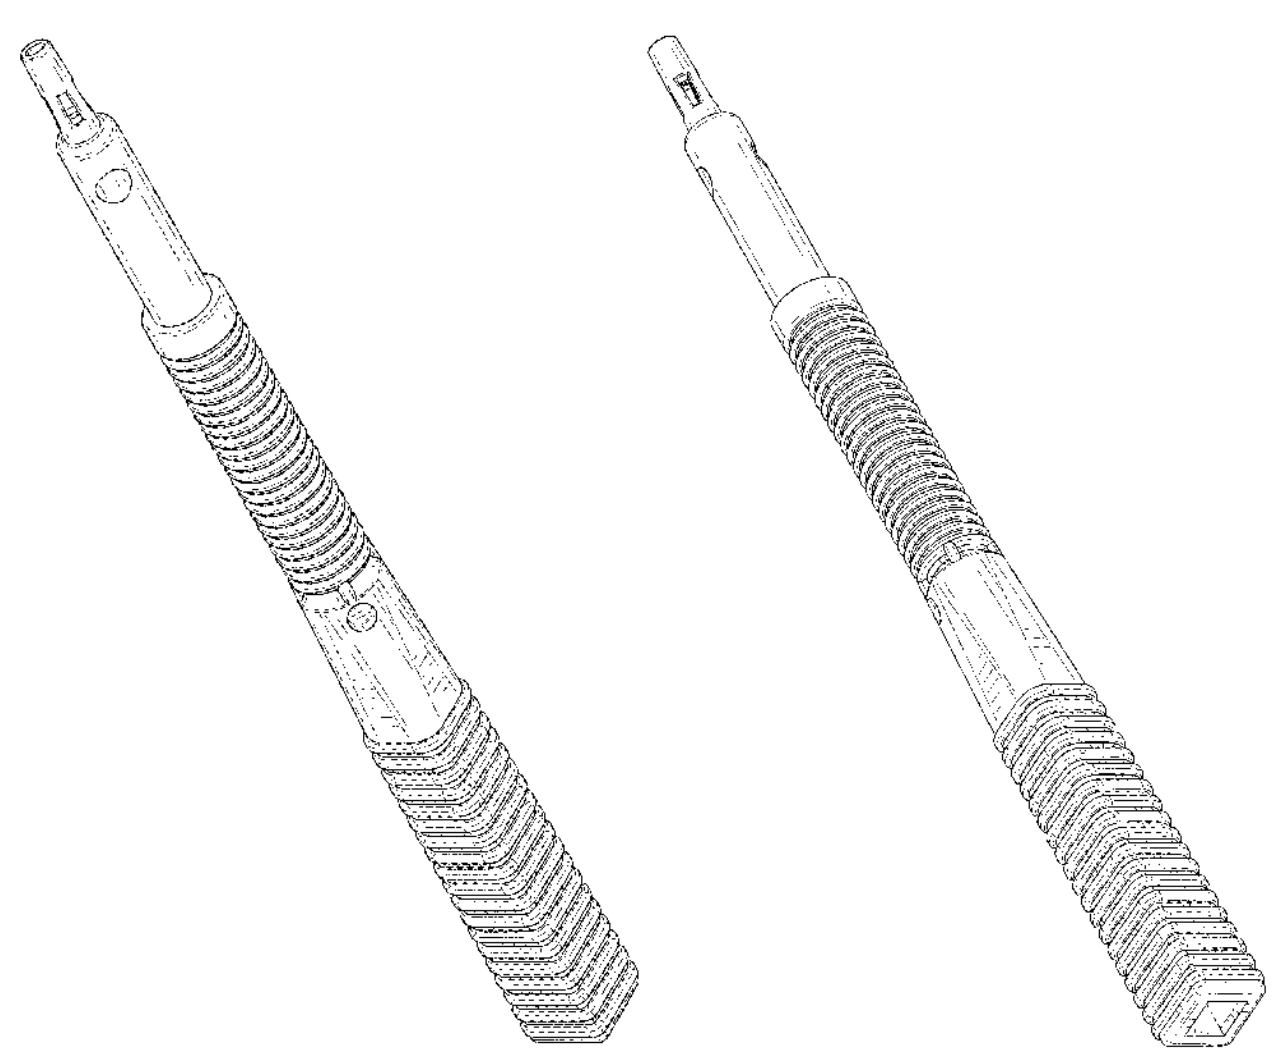

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,178,298	A	*	1/1993	Allina	B65D 83/0418 221/229
D336,957	S		6/1993	Koros et al.	
D343,679	S		1/1994	Wong	
D344,903	S		3/1994	Gampp, Jr. et al.	
D351,227	S		10/1994	Patton et al.	
D369,408	S		4/1996	Laun	
D372,311	S		7/1996	Koros et al.	
5,543,115	A		8/1996	Karakawa	
D373,634	S		9/1996	Brown	
D379,230	S		5/1997	Mark	
D381,418	S		7/1997	Erskine et al.	
D381,426	S		7/1997	Koros et al.	
D382,342	S		8/1997	Rosen	
D402,753	S		12/1998	White	
D407,488	S		3/1999	Injev	
D413,382	S		8/1999	Maissami	
D425,195	S		5/2000	Hellstrom et al.	
D425,625	S	*	5/2000	Niermann	D24/224
6,146,590	A		11/2000	Mazurek et al.	
D441,447	S		5/2001	Hjertman et al.	
D443,058	S		5/2001	Mulhauser et al.	
D443,930	S		6/2001	Nestenborg	
D444,885	S	*	7/2001	Conway	D24/224
D446,865	S		8/2001	Conway	
D448,086	S		9/2001	Conway	
D458,456	S		6/2002	Dragan et al.	
D465,283	S		11/2002	Lodge	
D466,214	S		11/2002	Otsuka	
D472,975	S	*	4/2003	Iori	D24/224
D475,482	S		6/2003	Angeletta	
D518,597	S		4/2006	Sommers	
D538,936	S		3/2007	Bohmel et al.	
7,225,689	B2		6/2007	Wickstead et al.	
D553,738	S		10/2007	Simonson	
D559,397	S	*	1/2008	Eriksson	D24/224
D581,534	S		11/2008	Liu et al.	
D585,989	S		2/2009	Leroy	
D588,888	S		3/2009	Yung-Kuan	
D589,618	S		3/2009	Hasebe	
D590,056	S		4/2009	McCrary et al.	
D593,202	S		5/2009	Petersen	
D601,252	S		9/2009	Ra	
D603,502	S		11/2009	Petersen	
D612,052	S		3/2010	McCollam et al.	
D613,873	S	*	4/2010	Jia	D24/224
D615,196	S		5/2010	Doll	
D619,707	S		7/2010	East	
D640,796	S		6/2011	Wilkinson	
D663,836	S		7/2012	Ruiz et al.	
D667,960	S		9/2012	Wilkinson	
D669,981	S		10/2012	Ruiz et al.	
D692,998	S		11/2013	Broberg et al.	
D698,036	S		1/2014	Dickinson	
D704,336	S		5/2014	Chon et al.	
D708,323	S		7/2014	Reyes et al.	
D720,070	S		12/2014	Khalaj	
D747,477	S		1/2016	Freigang et al.	
D749,725	S		2/2016	Sauer	
D750,270	S		2/2016	Ching et al.	
9,320,535	B2		4/2016	Zaretzka et al.	
D774,407	S		12/2016	Khattak et al.	
D779,059	S		2/2017	Nino et al.	
9,636,676	B2		5/2017	Sever et al.	
9,718,058	B2		8/2017	Khattak et al.	
9,724,691	B2		8/2017	Khattak et al.	
D798,446	S		9/2017	Nino et al.	
D809,138	S		1/2018	Khan et al.	
D810,273	S		2/2018	Maier et al.	
D821,602	S		6/2018	Sever et al.	
D825,772	S		8/2018	Sever et al.	
D831,210	S		10/2018	Nelson et al.	
D832,426	S		10/2018	Holton et al.	
D835,273	S		12/2018	Orr et al.	
D843,008	S		3/2019	Blaszcak et al.	
10,272,434	B2		4/2019	Khattak et al.	
D859,652	S		9/2019	Teufel	
D859,683	S		9/2019	Harding et al.	
D866,757	S		11/2019	Diluzio et al.	
D869,311	S		12/2019	Khattak et al.	
D873,433	S		1/2020	Hagiwara	
10,545,161	B2		1/2020	Khattak et al.	
D875,926	S		2/2020	Lee et al.	
D883,475	S		5/2020	Boyaval et al.	
D891,959	S		8/2020	Khattak et al.	
D909,600	S		2/2021	Sever et al.	
D921,196	S		6/2021	Wang	
D938,583	S		12/2021	Yan et al.	
D940,893	S		1/2022	Wisherd et al.	
D948,073	S		4/2022	Oishi	
D950,723	S		5/2022	Leibowitz	
D958,398	S		7/2022	O'Leary	
D971,431	S		11/2022	Best	
D971,432	S	*	11/2022	Best	D24/216
D975,847	S		1/2023	Goh et al.	
D978,376	S	*	2/2023	Ou	D24/224
D979,788	S	*	2/2023	Park	D24/216
D983,368	S		4/2023	Leibowitz	
D983,970	S		4/2023	Vaughan et al.	
D989,343	S		6/2023	Gao et al.	
D990,694	S	*	6/2023	Wu	D24/214
D1,006,991	S		12/2023	Vaughan et al.	
D1,009,258	S		12/2023	Leibowitz	
D1,009,259	S		12/2023	Leibowitz	
D1,009,260	S		12/2023	Leibowitz	
D1,014,750	S		2/2024	Shih	
D1,014,751	S		2/2024	Shih	
D1,017,031	S		3/2024	Ahn et al.	
D1,017,804	S		3/2024	Dubath et al.	
D1,022,196	S		4/2024	Ota et al.	
2002/0106809	A1		8/2002	Cesarczyk	
2002/0123048	A1	*	9/2002	Gau, Jr.	B01L 3/5088 435/7.1
2002/0182744	A1		12/2002	Tyrrell et al.	
2004/0082878	A1	*	4/2004	Baldwin	B01L 9/52 422/50
2004/0214200	A1		10/2004	Brown et al.	
2004/0245125	A1		12/2004	Trkulja	
2006/0074407	A1		4/2006	Padget et al.	
2007/0299364	A1		12/2007	Sangha	
2008/0166818	A1		7/2008	Ennis	
2008/0210619	A1		9/2008	Lapenna	
2013/0145591	A1		6/2013	Chen	
2014/0051178	A1		2/2014	Niggel et al.	
2014/0221987	A1		8/2014	Jeong et al.	
2015/0088151	A1		3/2015	Hatta	
2017/0043336	A1		2/2017	Khattak et al.	
2017/0045508	A1		2/2017	Khattak et al.	
2017/0241845	A1		8/2017	Hwang et al.	
2017/0350838	A1		12/2017	Katsumoto et al.	
2018/0021771	A1		1/2018	Tamir	
2018/0052096	A1		2/2018	Wan et al.	
2018/0141043	A1		5/2018	Malcolmson et al.	
2020/0116598	A1		4/2020	Ling	
2020/0268293	A1		8/2020	Gassler et al.	
2021/0085364	A1		3/2021	Wachli et al.	
2022/0257093	A1		8/2022	Tarke et al.	
2023/0129323	A1		4/2023	Bailey et al.	
2023/0143077	A1		5/2023	Higgins et al.	
2023/0172591	A1		6/2023	Robbins et al.	
2023/0339670	A1		10/2023	Brink et al.	

FOREIGN PATENT DOCUMENTS

IN	345026-001-0001			6/2023
IN	418118-001		*	7/2024
WO	WO-01/89933	A2		11/2001
WO	WO-2010/036808	A1		4/2010
WO	WO-2010/041231	A2		4/2010

(56) **References Cited**

FOREIGN PATENT DOCUMENTS

WO	WO-2014/164933 A1	10/2014
WO	WO-2017/015172 A1	1/2017

OTHER PUBLICATIONS

"X: Cue Health." Found online May 3, 2024 at twitter.com. Reference dated Apr. 8, 2024. Retrieved from https://twitter.com/CueHealth/status/1777441289438417055.*

"Pharmiweb: Vacuum Blood Collection Devices Market Set to Surpass US$4.7 Billion by 2033—RMI Projection." Found online May 3, 2024 at pharmiweb.com. Reference dated Dec. 8, 2023. Retrieved from https://www.pharmiweb.com/press-release/2023-12-08/vacuum-blood-collection-devices-market-set-to-surpass-us-47-billion-by-20.*

"PharmTech: Polymer Syringe for Infusion Therapy Devices." Found online May 3, 2024 at pharmtech.com. Reference dated Mar. 6, 2014. Retrieved from https://www.pharmtech.com/view/schott-introduces-prefillable-polymer-syringe-infusion-therapy-devices.*

Custom Candle Packaging Box, posted at everwinpack.en.made-in-china.com, site visited Feb. 6, 2024, available from the internet, URL: https://everwinpack.en.made-in-china.com/product/jmCRsNyxLSVa/China-Custom-Pink-Rigid-Cardboard-Paper-Candle-Packaging-Gift-Box-for-Three.html.

Facebook: "The Scientific Instrument Company" Found online at facebook.com. Jul. 17, 2023. Reference dated Jan. 9, 2021. Retrieved from: https://www.facebook.com/Thescientificinstrumentco/posts/extraction-tube-with-nozzle-cap-drop-size-35ul-for-using-in-covid-test-kitavaila/3949721501%E2%80%A6.

Manufacturing Chemist: "Bio-Rad introduces Ag Rapid Test with QC Kit." Found online at manufacturingchemist.com. Jul. 17, 2023. Reference dated Jun. 1, 2021. Retrieved from: https://www.manufacturingchemist.com/news/article_page/Bio-Rad_introduces_Coronavirus_Ag_Rapid_Test_with_QC_kit/176948.

"Ultechnovo: Plastic Specimen Cup" Found online at amazon.com. Jul. 17, 2023. Reference dated Jul. 11, 2019. Retrieved from https://www.amazon.com/ULTECHNOVO-10Pcs-25-30ml-Specimen-Container/dp/B07V3KDT6F/.

"Unitek College: Step-by-Step Guide to Specimen Collection" Found online at unitekcollege.com. Jul. 17, 2023. Reference dated Mar. 16, 2022. Retrieved from https://www.unitekcollege.edu/blog/a-step-by-step-guide-to-specimen-collection/.

"X: CueHealth." Found online May 8, 2025 at x.com. Reference dated Jan. 19, 2021. Retrieved from https://x.com/CueHealth/status/1351567401666531329/photo/1.

"X: CueHealth." Found online May 8, 2025 at x.com. Reference dated Jun. 12, 2023. Retrieved from https://x.com/CueHealth/status/1668386451837288450.

* cited by examiner

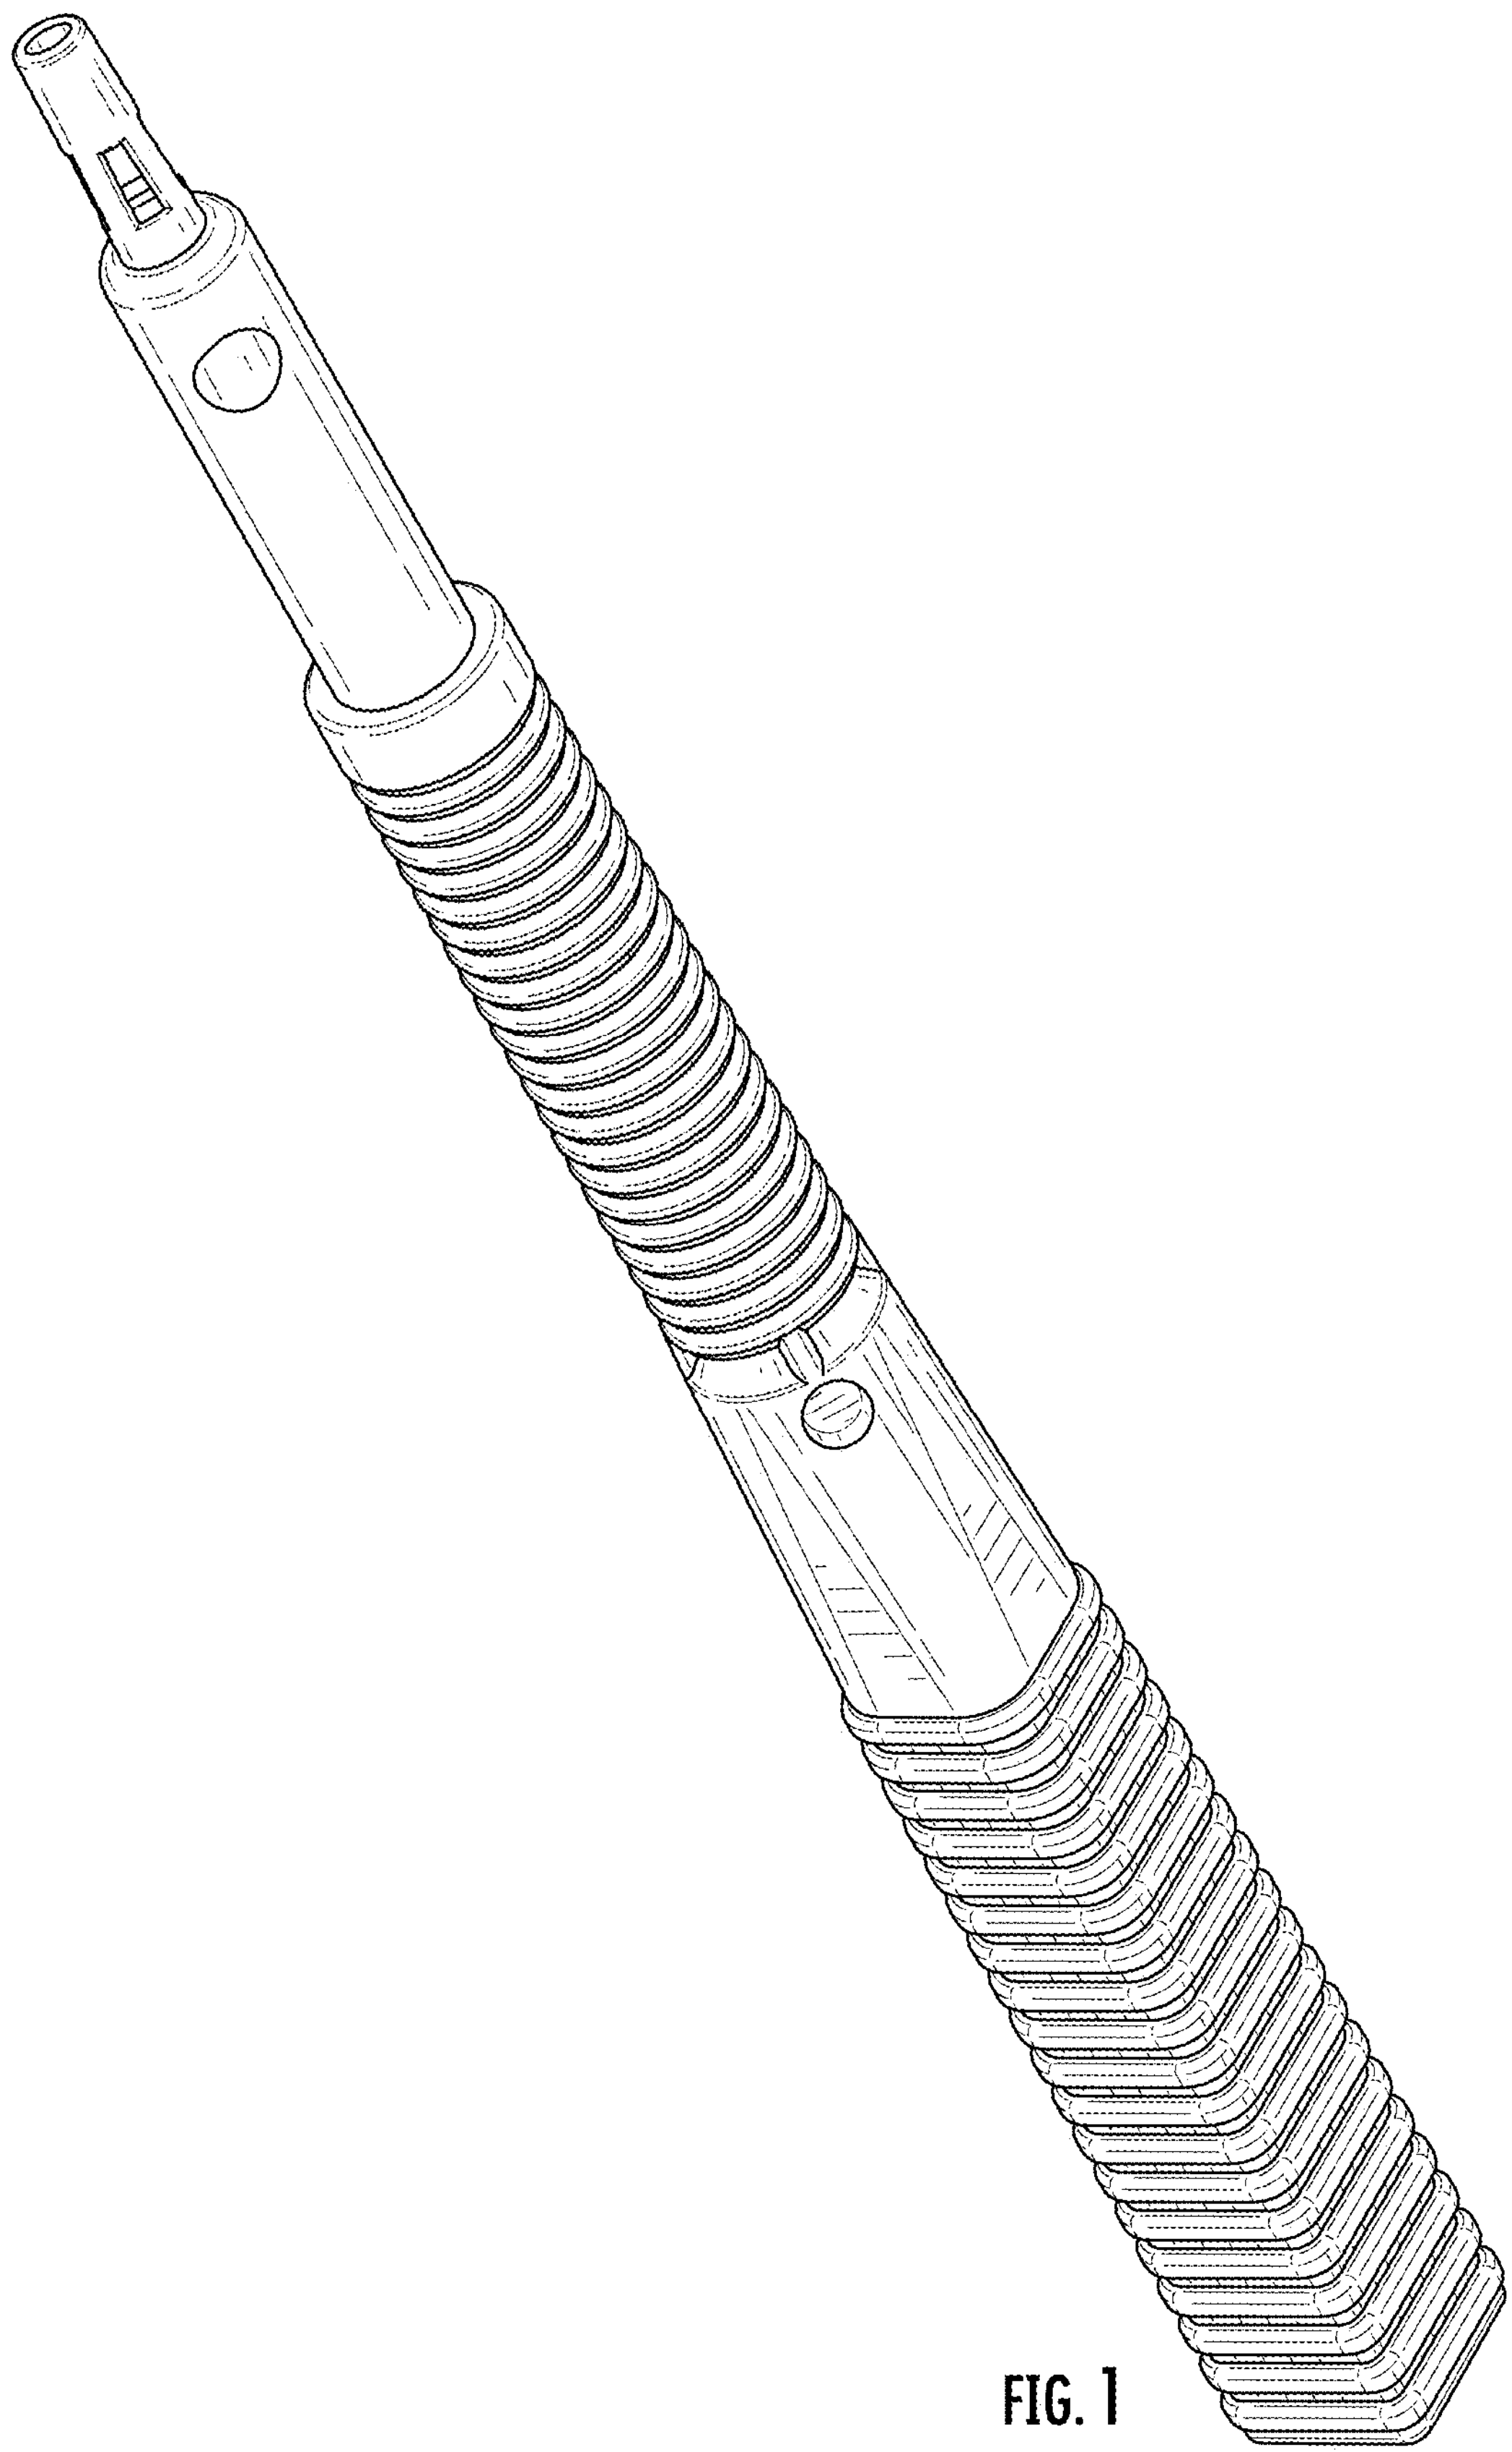

FIG. 1

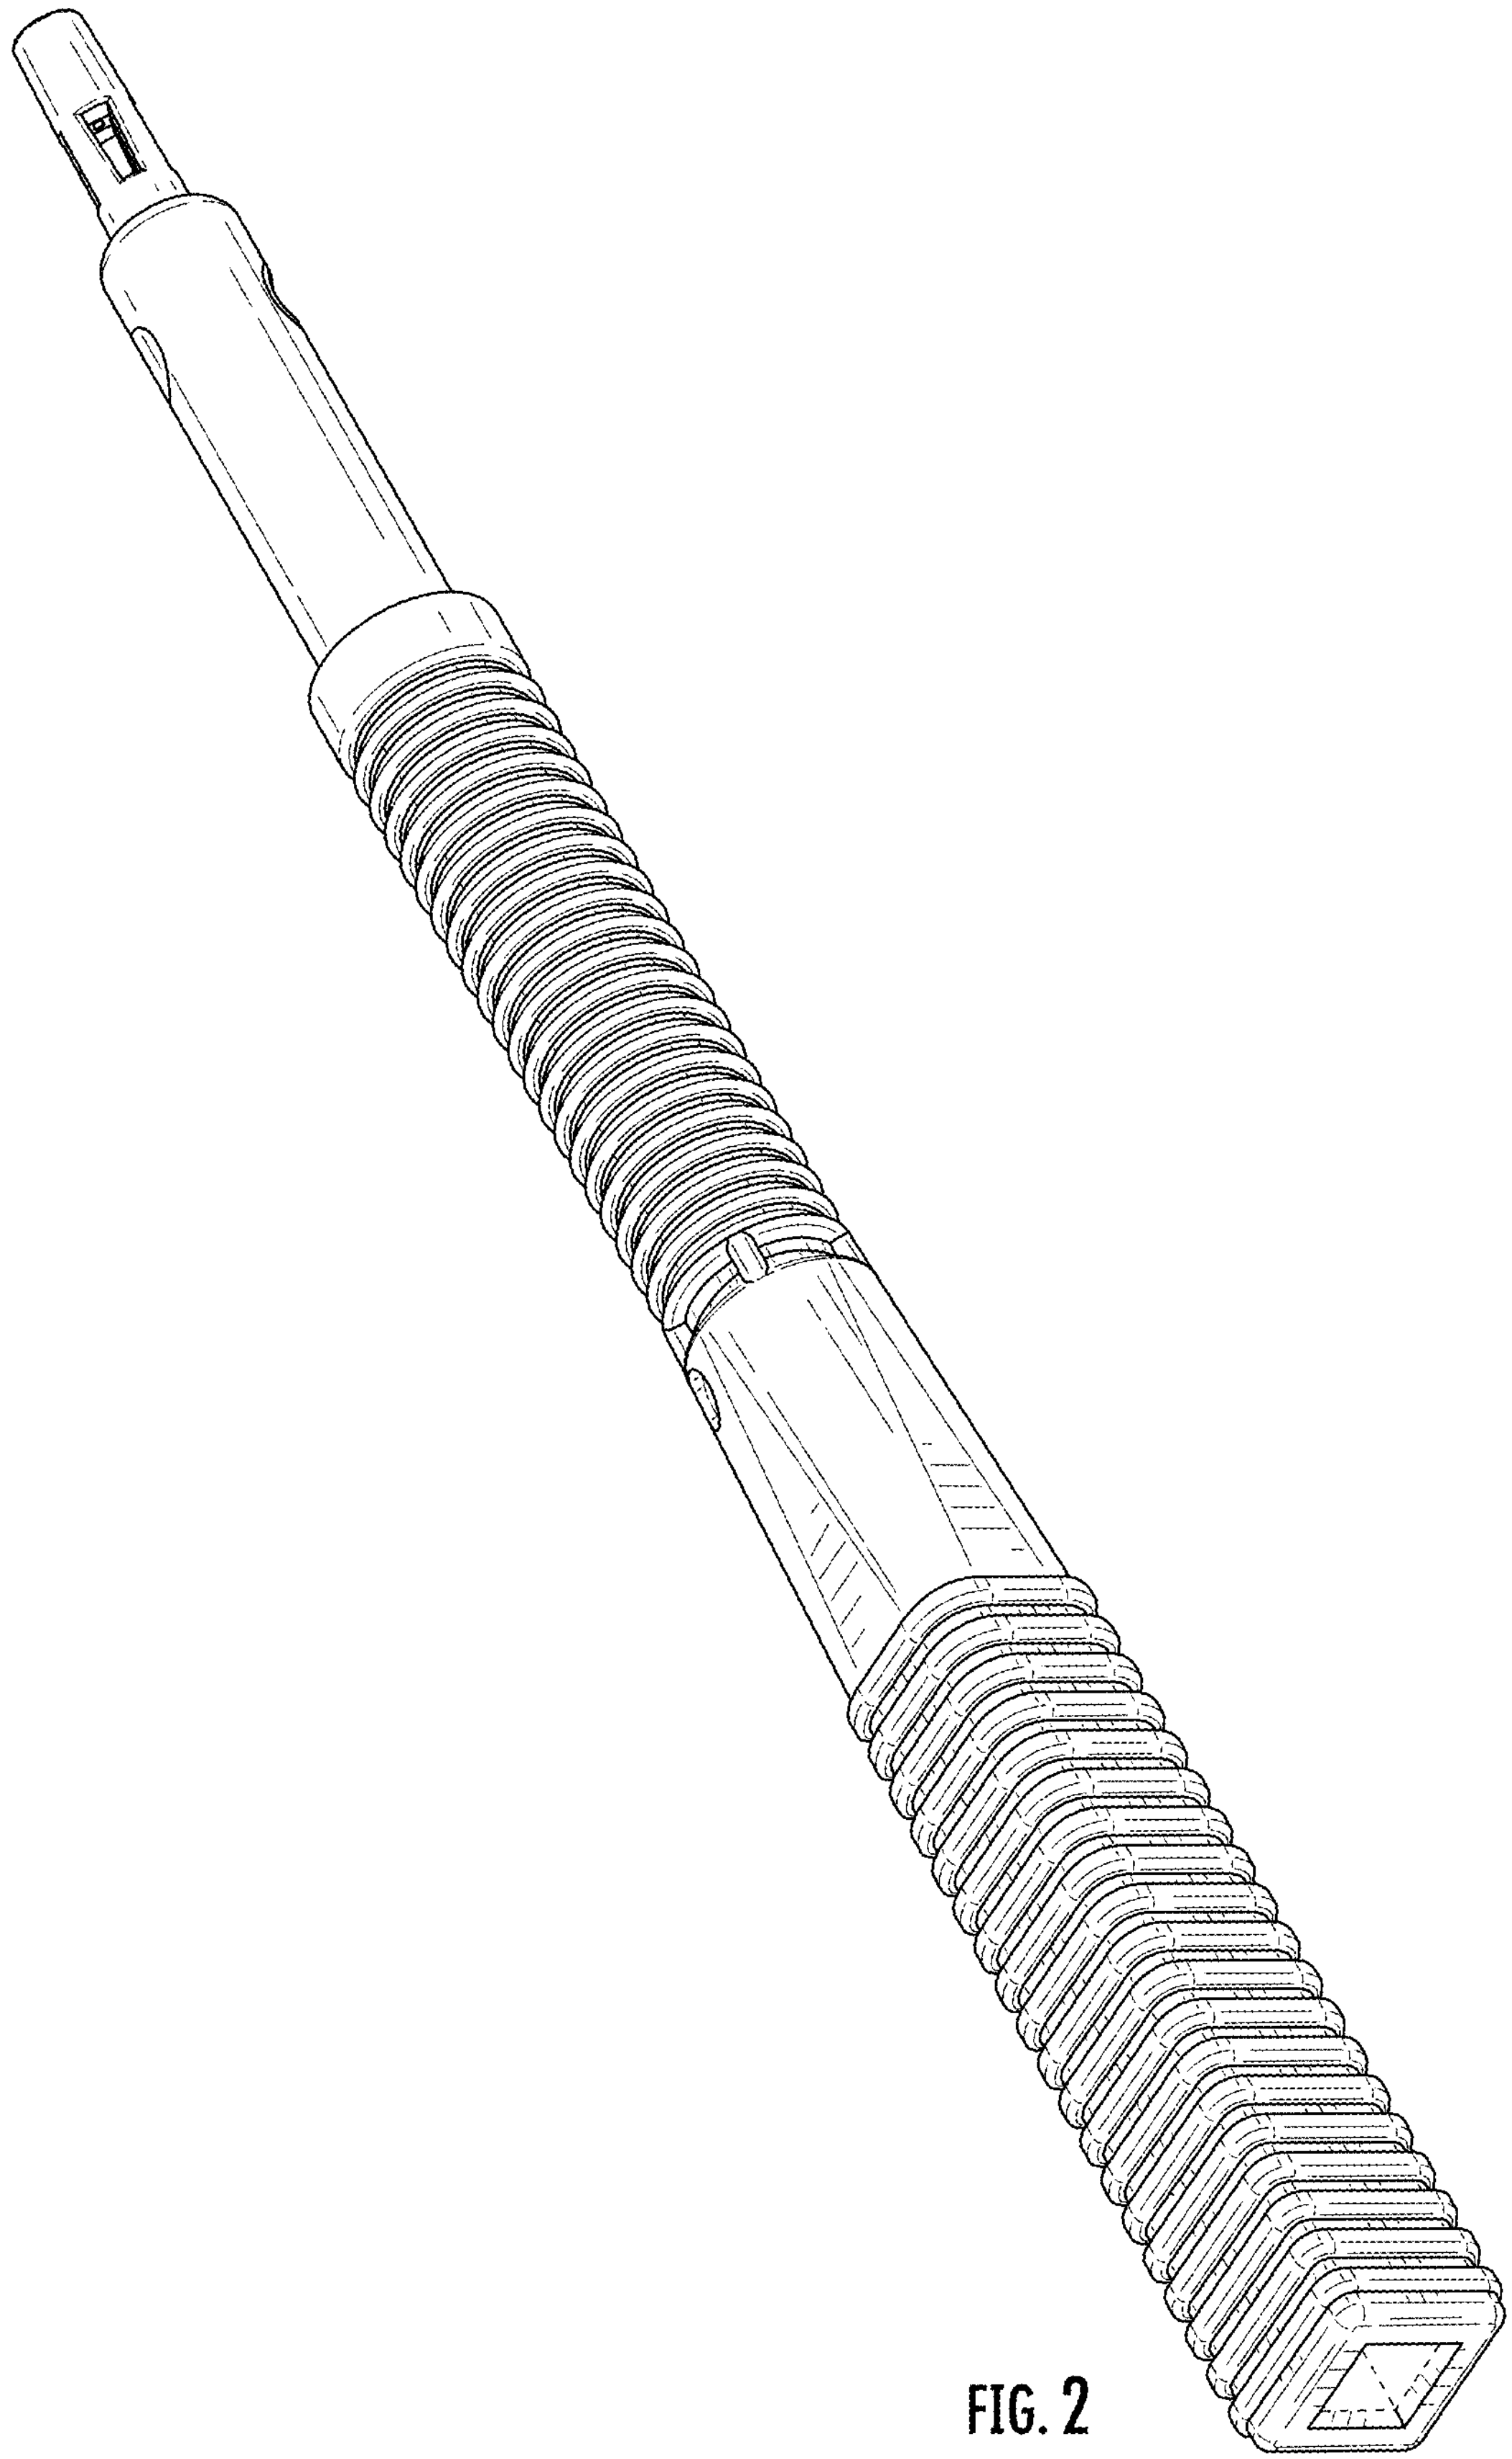

FIG. 2

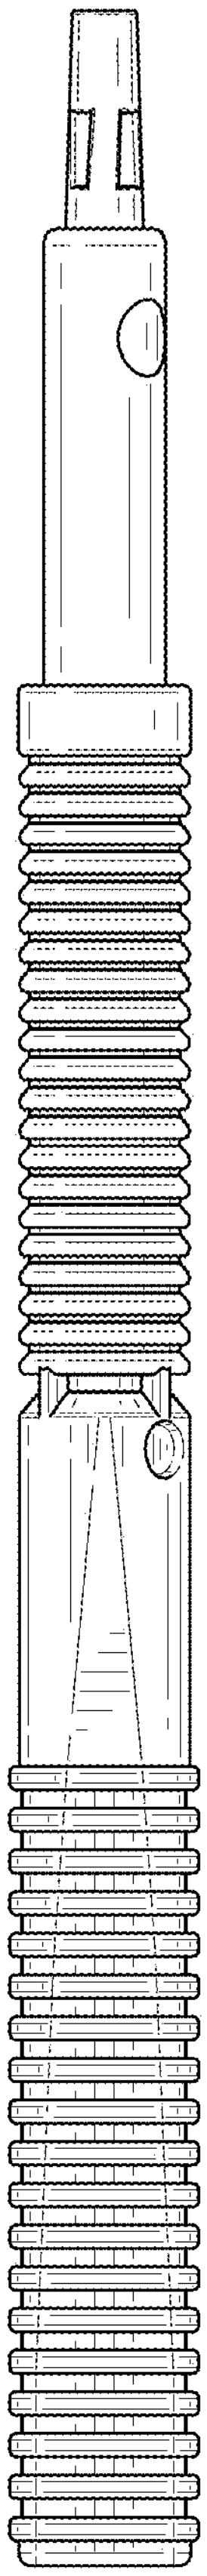

FIG. 3

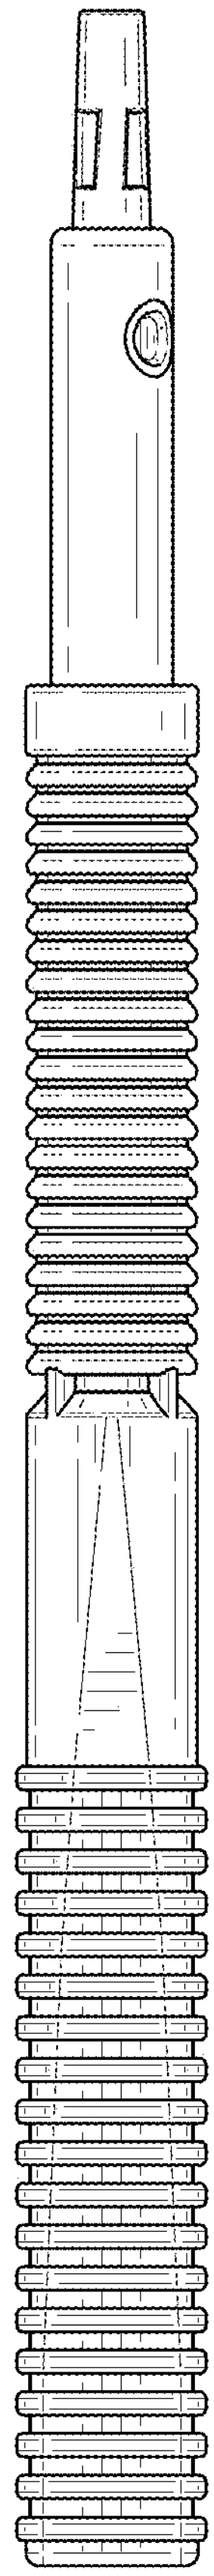

FIG. 4

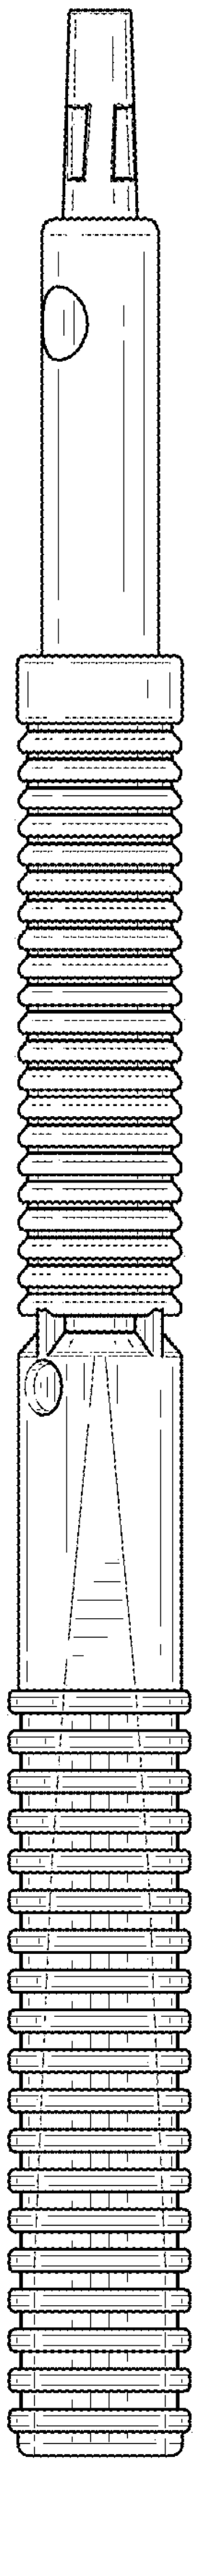

FIG. 5

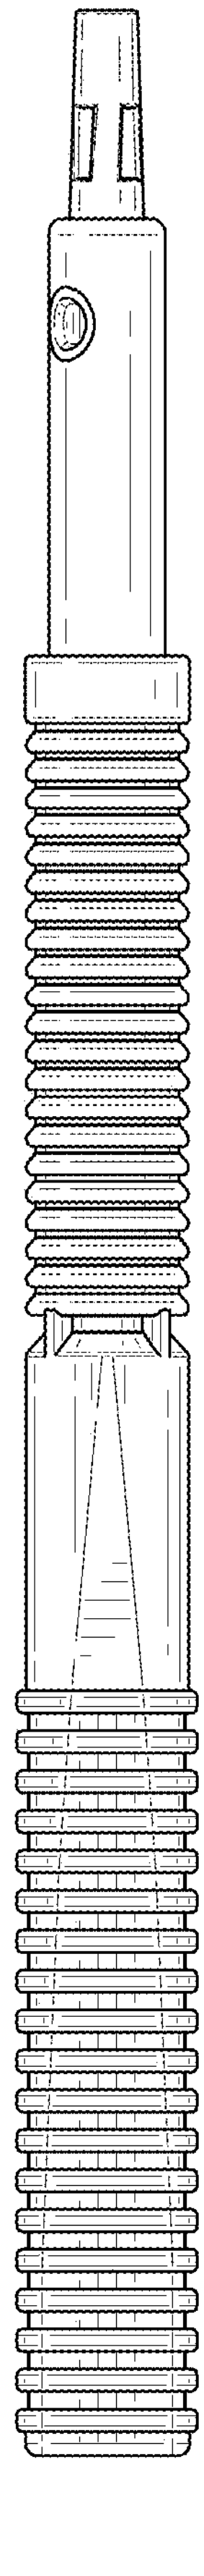

FIG. 6

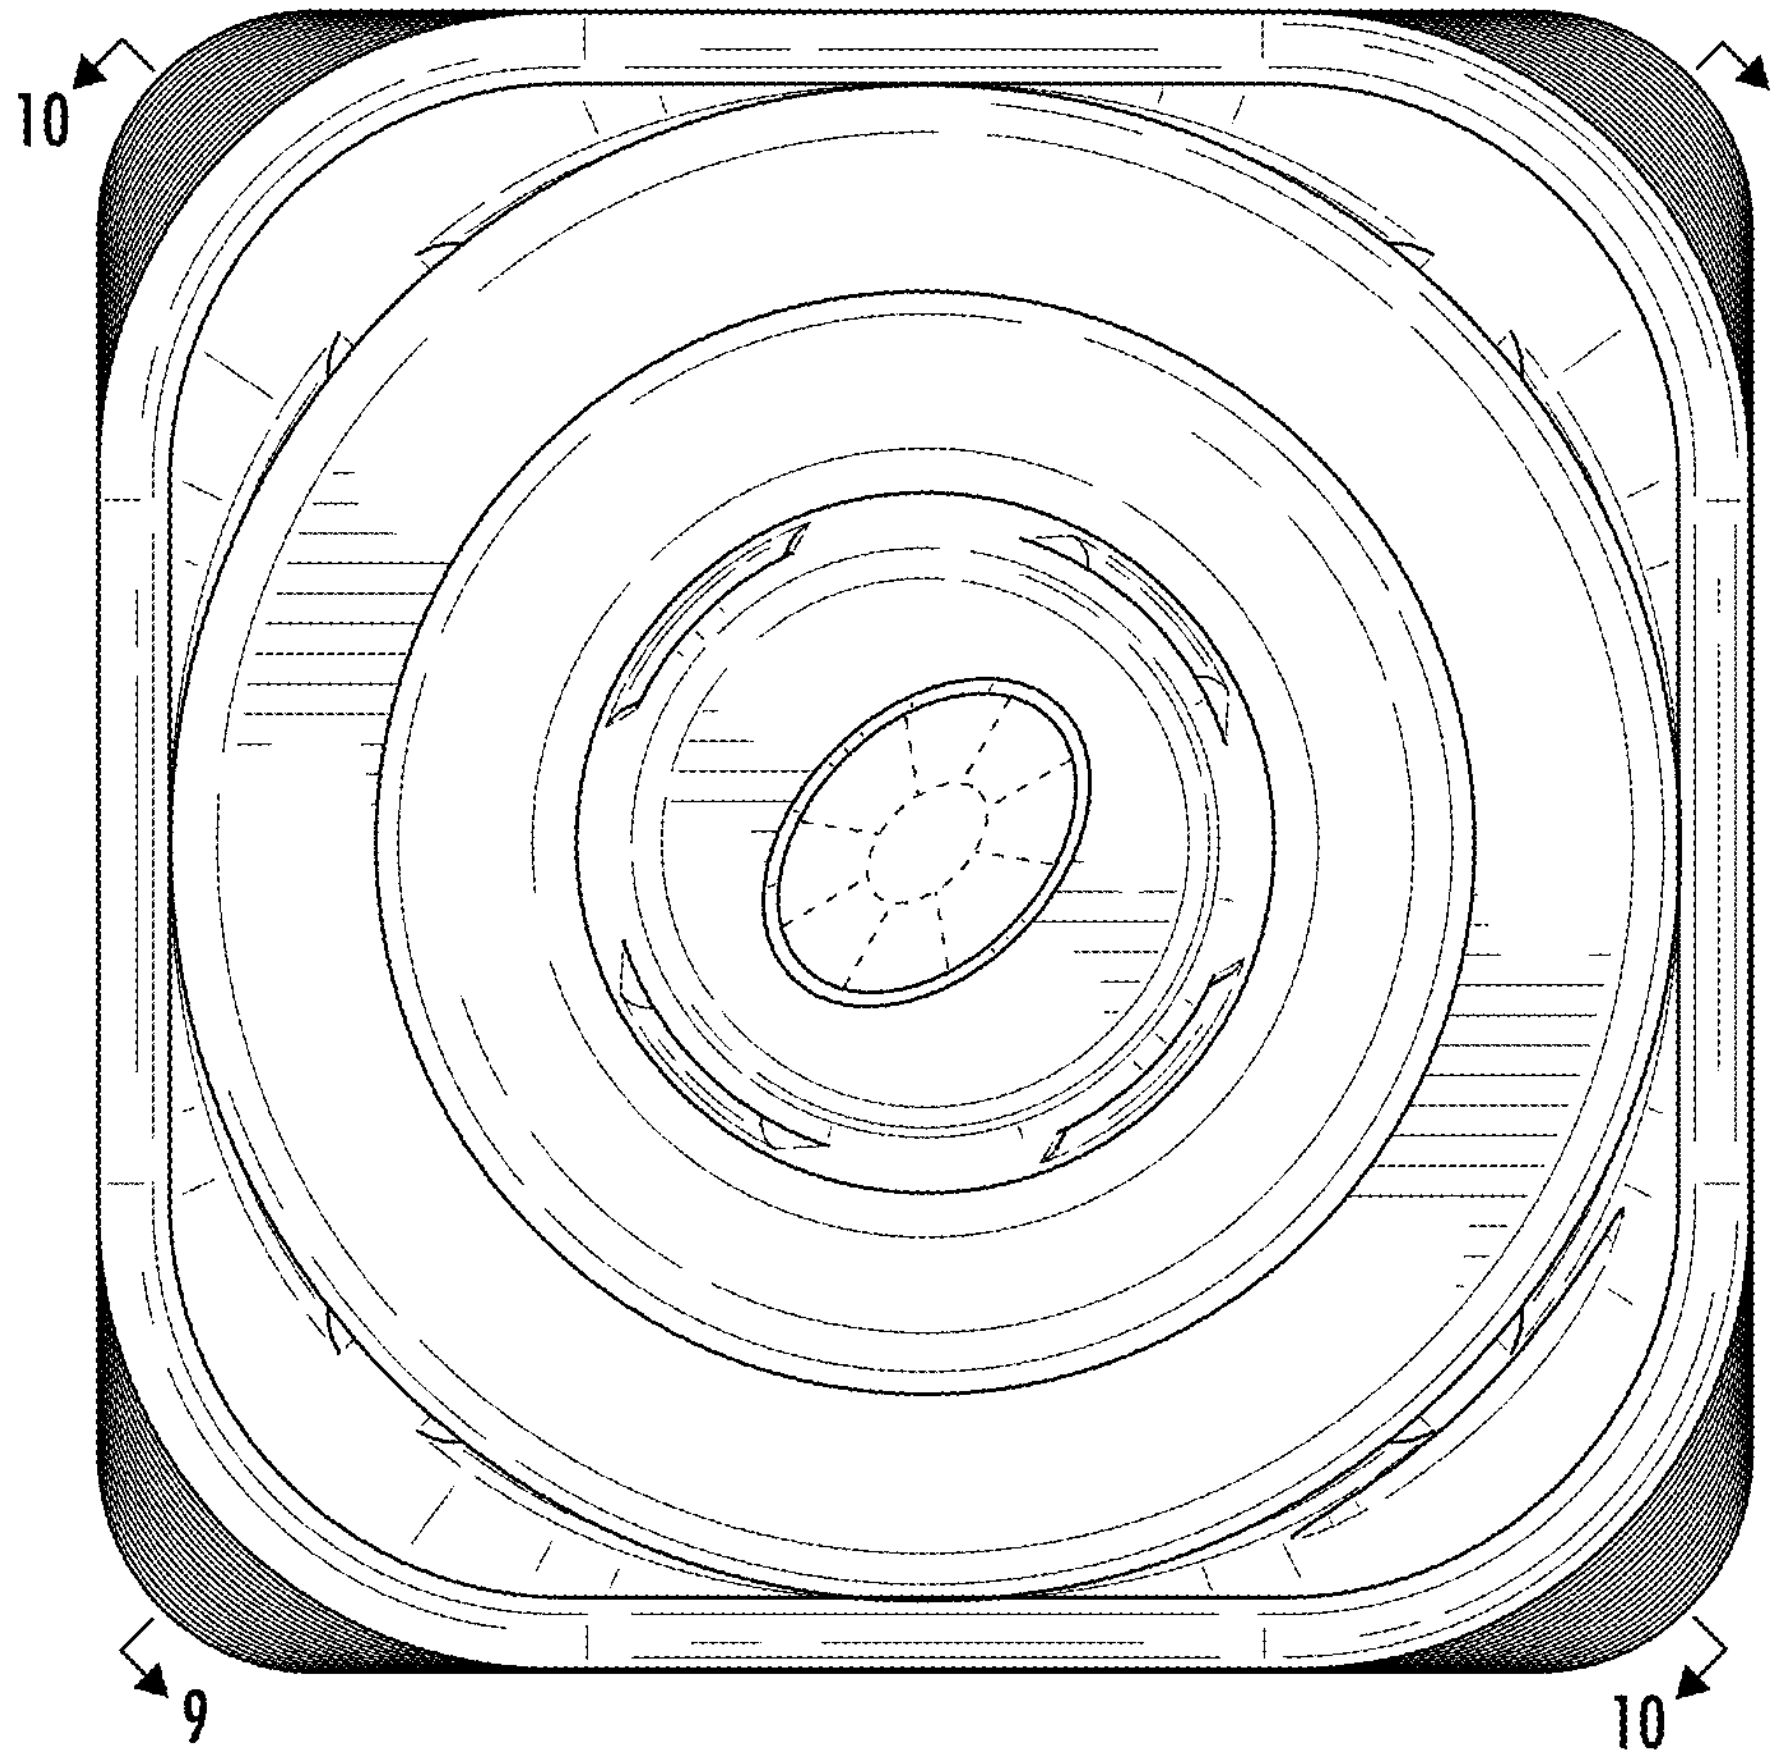

FIG. 7

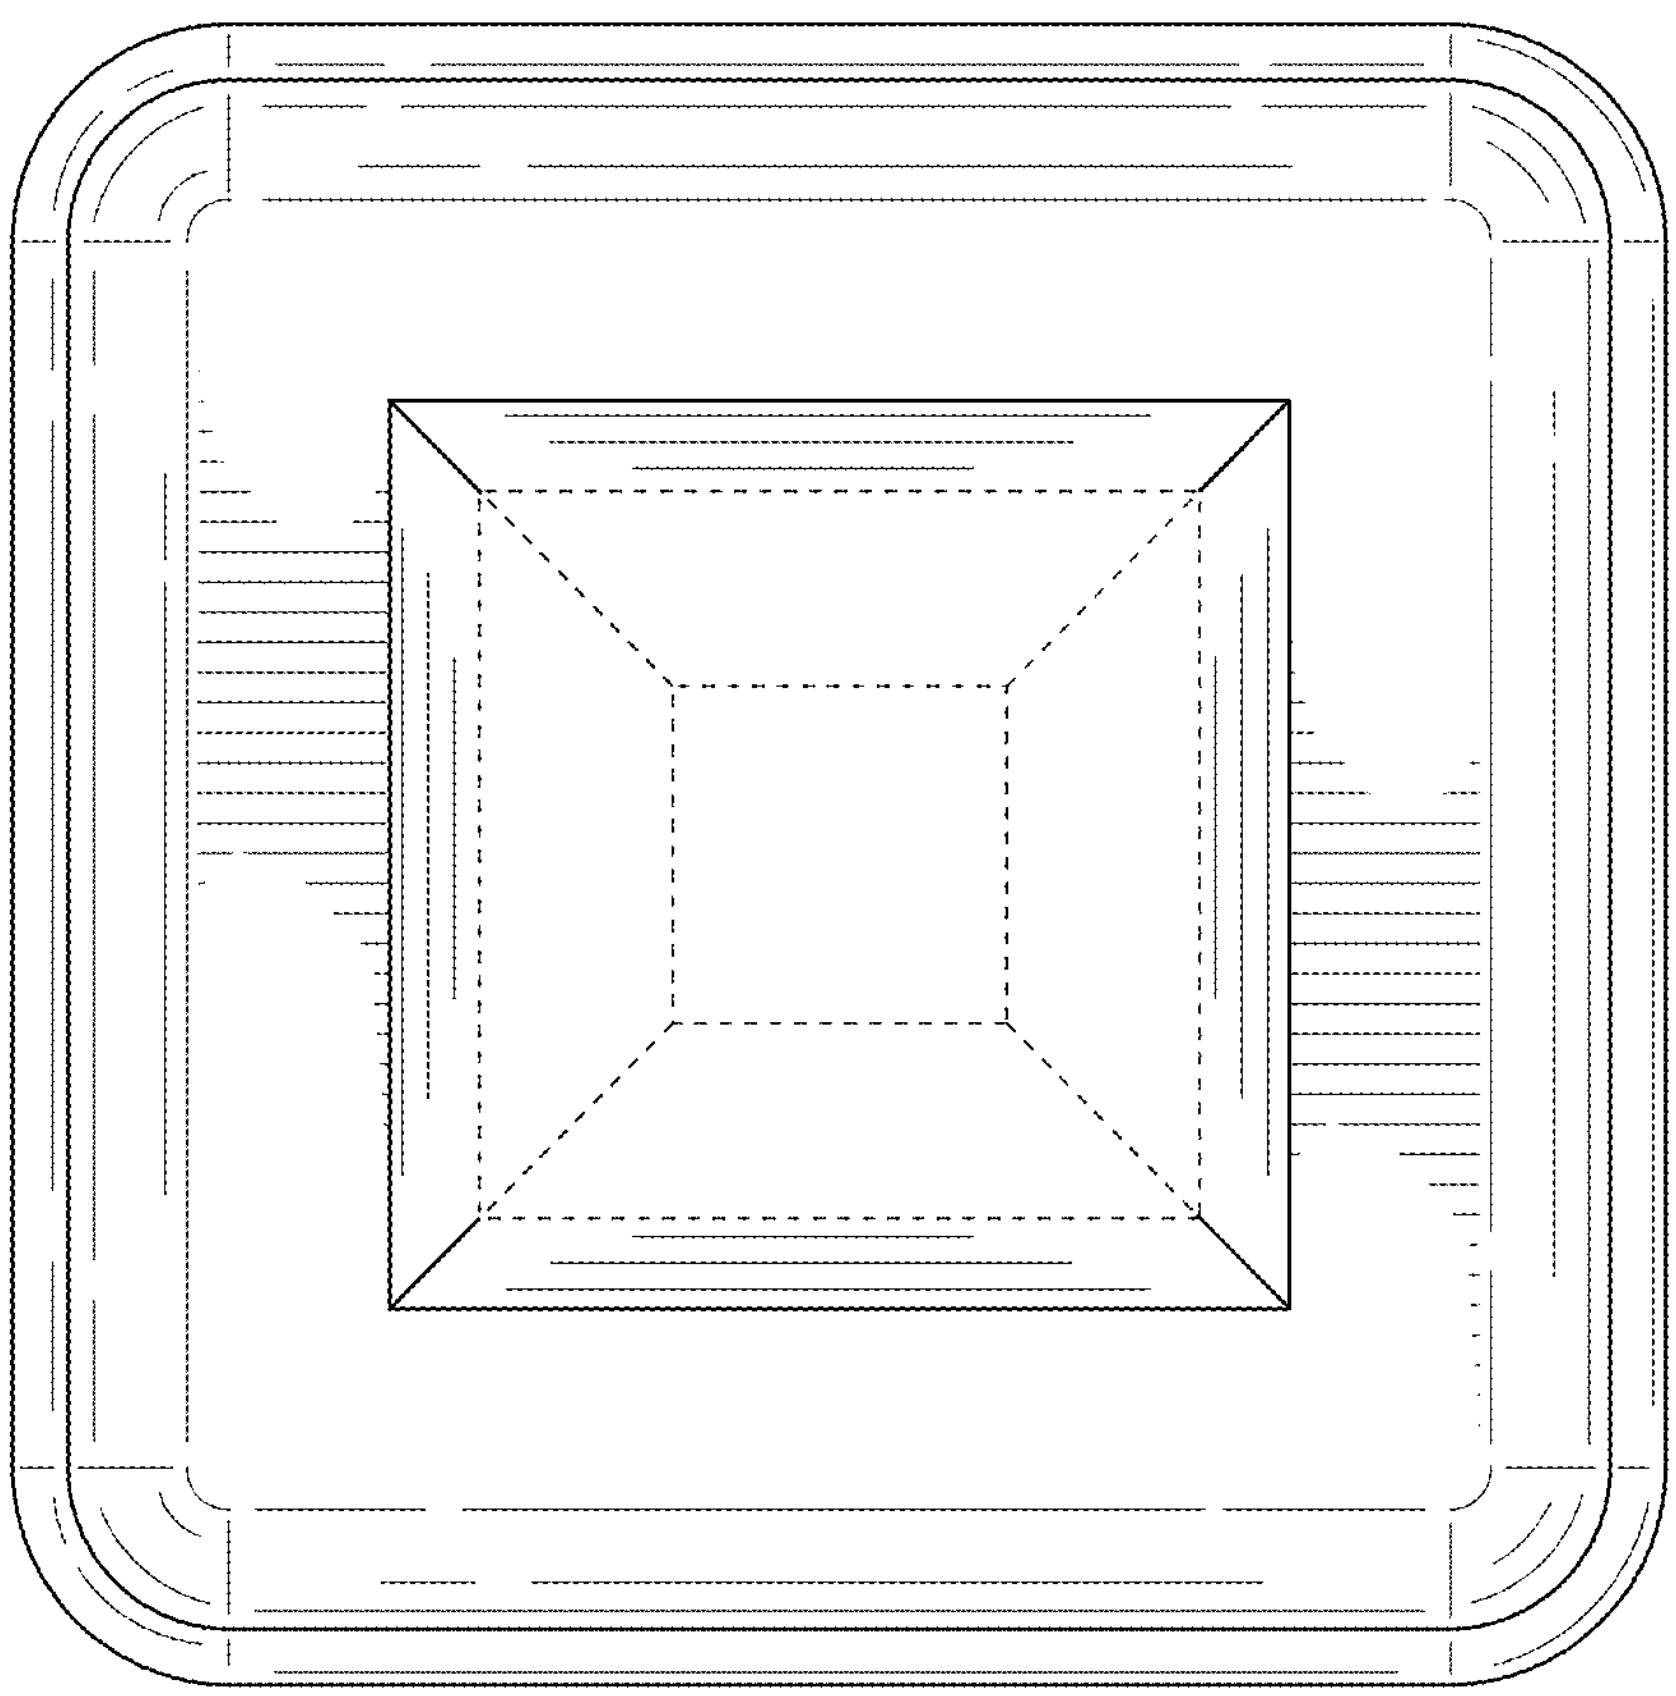

FIG. 8

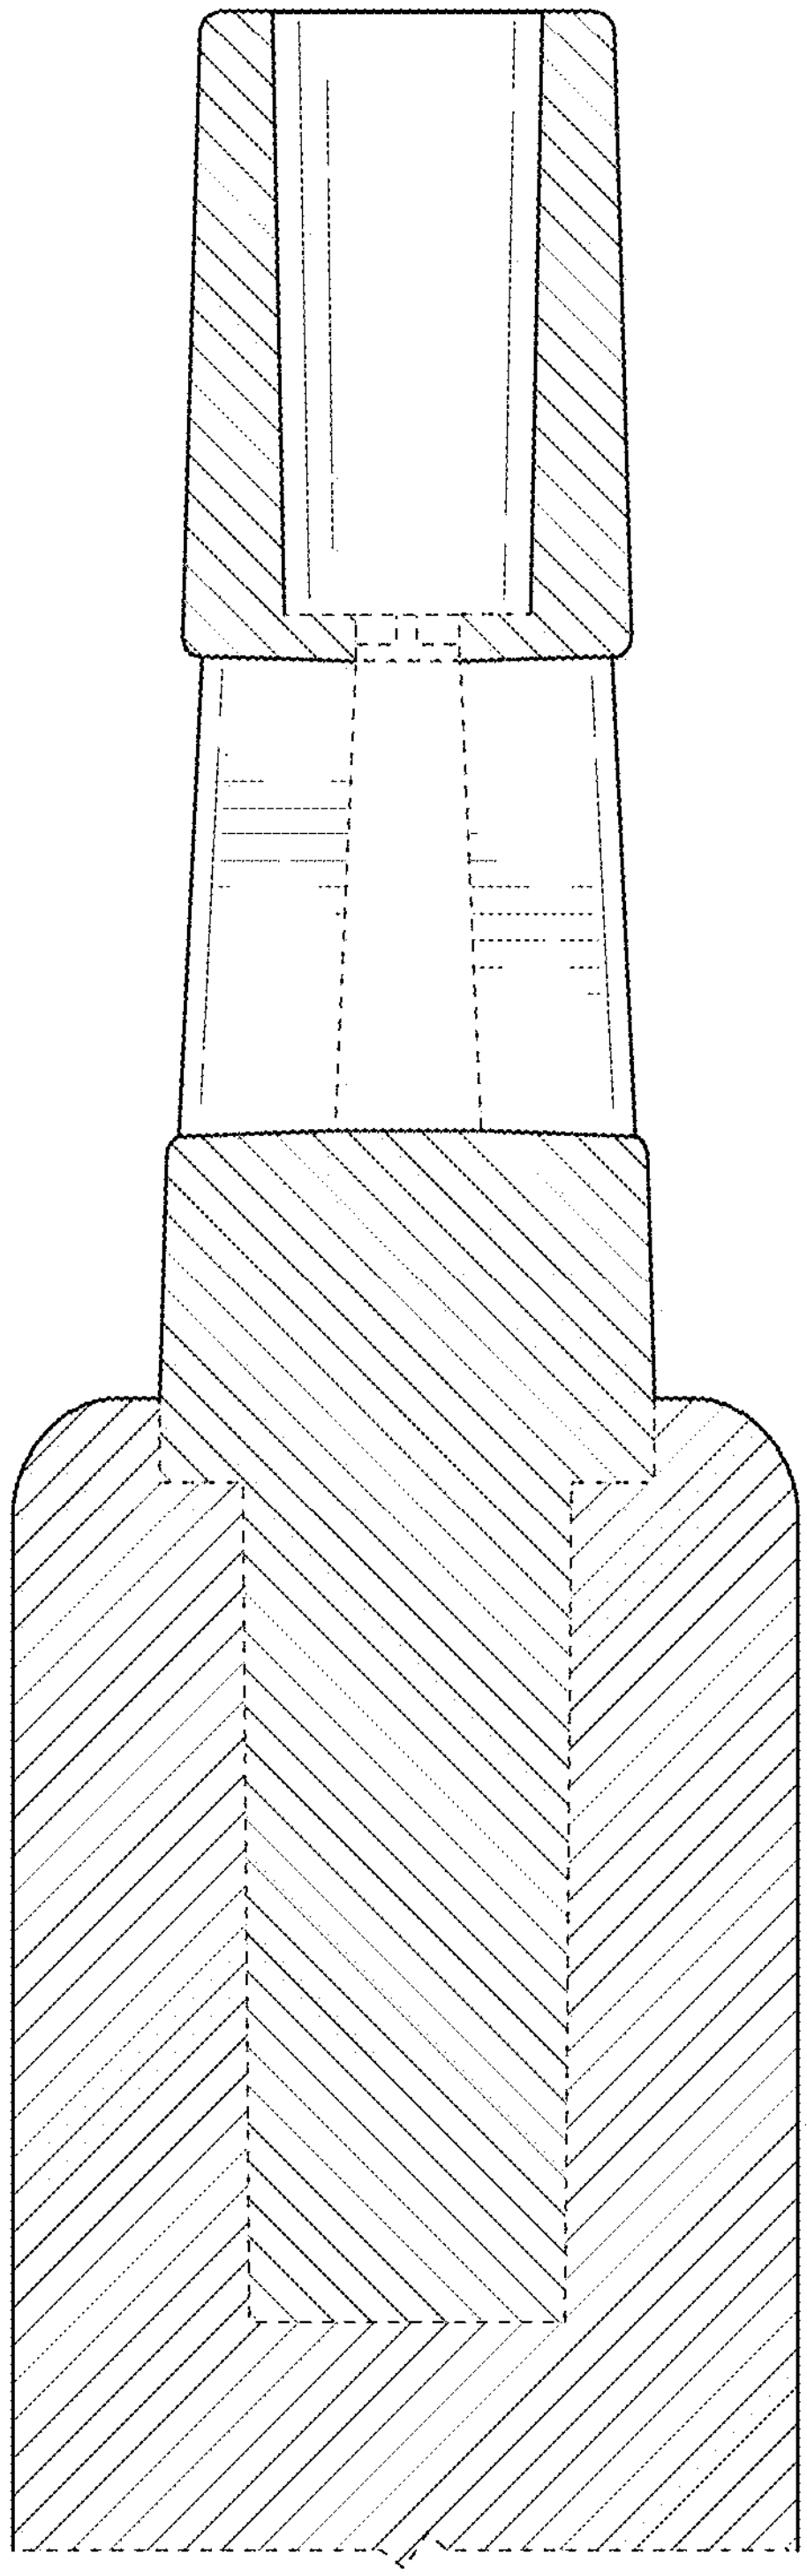

FIG. 9

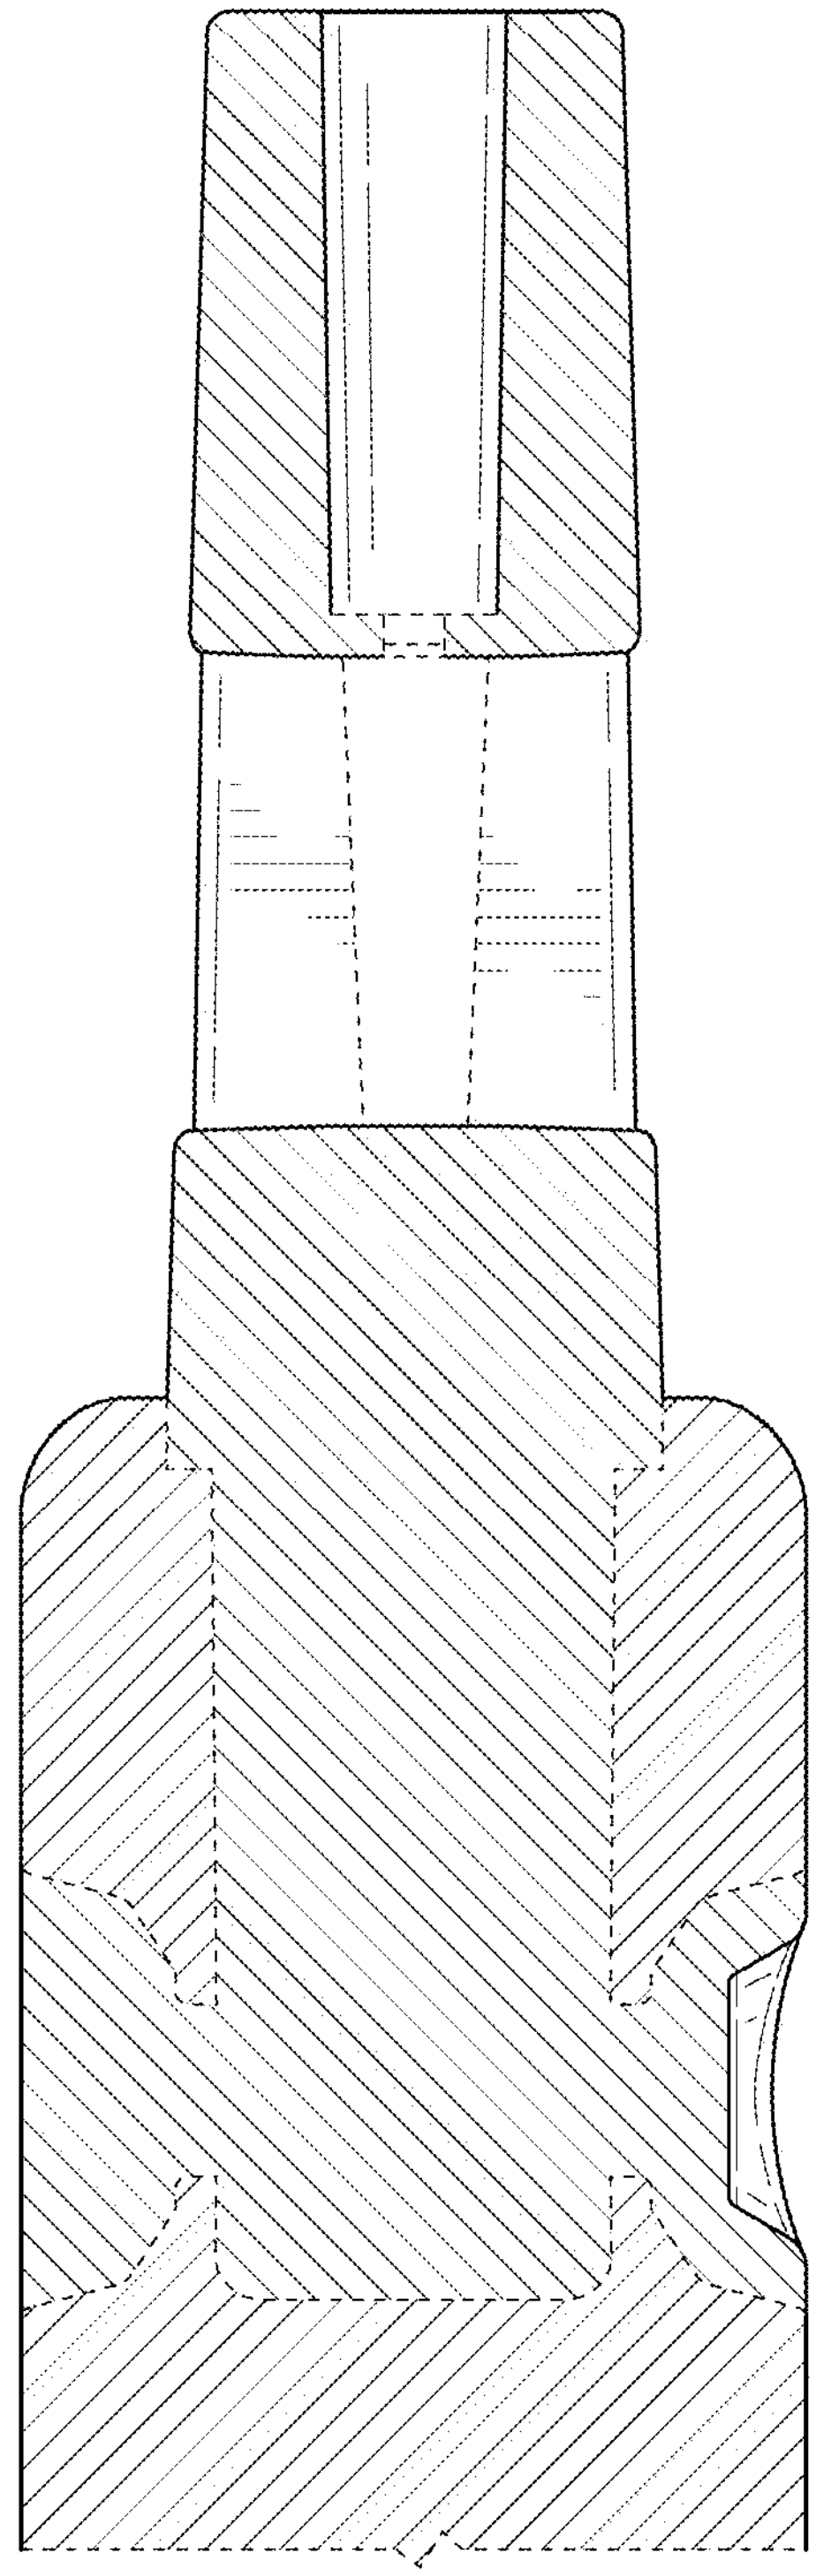

FIG. 10