



US0D1089638S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,089,638 S**  
**Perez et al.** (45) **Date of Patent:** **\*\* Aug. 19, 2025**

(54) **SWAB**

(71) Applicant: **CareFusion 2200, Inc.**, San Diego, CA  
(US)

(72) Inventors: **Katya Perez**, Huntley, IL (US);  
**Christopher McGinley**, Highland Park,  
IL (US); **Nathan Sieracki**, Deerfield, IL  
(US)

(73) Assignee: **CareFusion 2200, Inc.**, San Diego, CA  
(US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/883,497**

(22) Filed: **Jan. 30, 2023**

(51) **LOC (15) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/119**

(58) **Field of Classification Search**  
USPC ..... D24/119, 133, 146, 147, 151; D28/7  
CPC ..... A61B 10/0096; A61F 13/38  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,368,549 A \* 2/1968 Barr ..... A61B 10/0096  
600/572  
D269,811 S \* 7/1983 Kaufman ..... D24/119  
D270,762 S \* 9/1983 Kaufman ..... D24/119  
4,935,001 A \* 6/1990 George ..... A61F 13/38  
401/176  
D328,366 S \* 7/1992 Villani ..... D28/7  
5,439,643 A 8/1995 Liebert  
D405,175 S \* 2/1999 Stredic, III ..... D24/119  
D468,424 S \* 1/2003 Levesque ..... D24/119  
D656,609 S \* 3/2012 Perez ..... A61F 11/006  
D24/119  
D787,743 S \* 5/2017 Rosenthal ..... D28/7

D928,309 S \* 8/2021 Aagaard ..... D28/7  
D956,962 S \* 7/2022 Lyon ..... D24/119  
D970,723 S \* 11/2022 Qiu ..... D24/119

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 301396358 11/2010  
CN 103202827 A 7/2013

(Continued)

**OTHER PUBLICATIONS**

CHG Swab Stick, Chlorhexidine Gluconate Skin Prep Swab, publicaiton  
date May 20, 2022, [online] URL: <https://web.archive.org/web/20220520204237/https://www.chenyanglobal.com/fda-certified-disposable-chg-prep-swab-stick.html> (Year: 2022).\*

(Continued)

*Primary Examiner* — L. A. Grabenstetter

(74) *Attorney, Agent, or Firm* — Arent Fox LLP & Care  
Fusion

(57) **CLAIM**

The ornamental design for a swab as shown and described.

**DESCRIPTION**

FIG. 1 is a top front left perspective view of a swab showing  
our new design;

FIG. 2 is a left side view of the design shown of FIG. 1;

FIG. 3 is a right side view of the design shown of FIG. 1;

FIG. 4 is a front view of the design shown of FIG. 1;


FIG. 5 is a rear view of the design shown of FIG. 1;

FIG. 6 is a top view of the design shown of FIG. 1; and,

FIG. 7 is a bottom view of the design shown of FIG. 1.

The dash-dash broken line illustrating the distal end of the  
swab stick forms no part of the claimed design. The dot-dash  
line separating the claimed shaft of the swab from the  
unclaimed distal end represents a boundary to the claim and  
forms no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

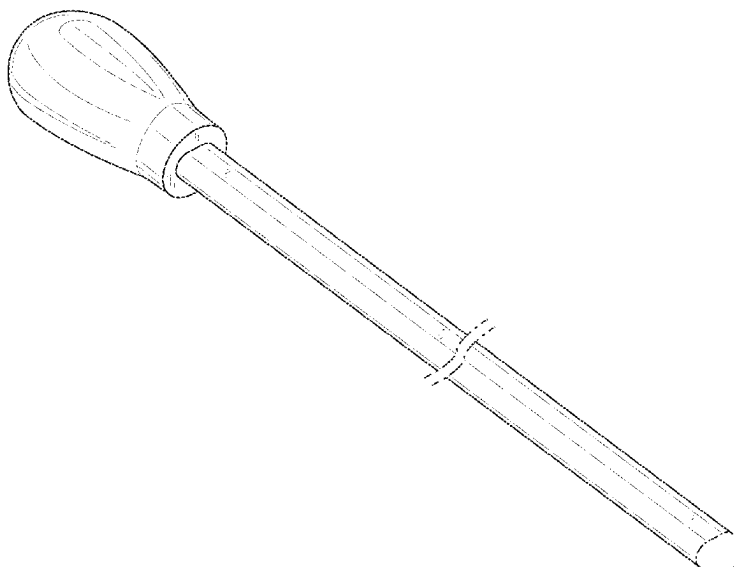

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

D983,448 S \* 4/2023 Matsuishi ..... D28/7  
D1,017,894 S \* 3/2024 Russo ..... D28/7  
D1,026,218 S \* 5/2024 Epstein ..... D24/119

## FOREIGN PATENT DOCUMENTS

CN 104922751 A 9/2015  
CN 303664016 5/2016  
CN 304922238 11/2018  
CN 304954372 12/2018  
CN 304954373 12/2018

## OTHER PUBLICATIONS

Impregnated Swabstick ChloraPrep™ One-Step 2% / 70% Strength  
CHG (Chlorhexidine Gluconate) / Isopropyl Alcohol NonSterile,

McKesson, Oct. 22, 2022, Retrieved from the Internet: <URL:https://mms.mckesson.com/product/526681/BD-260100>, 3 pages.

Bio-Equip, Skin Prep Chlorohexidine Gluconate SwabSticks, Mar. 15, 2018, Retrieved from the Internet: <URL: https://www.bio-equip.cn/ enshowlequip.pc.asp?equipid=II 1936&division=I 726>, 4 pages.

Cleanmo, Good quality ipa swabs Polyurethane Foam wholesale for Routine venipunctures, 2018, Retrieved from the Internet: <URL: https:// www.cleanmo.com/good-quality-ipa-swabs-polyurethane-foam-wholesale-for-routinevenipunctures>, 15 pages.

International Search Report received for PCT Patent Application No. PCT/US2024/013485, mailed on Apr. 12, 2024, 3 pages.

Office Action received for Canadian Patent Application No. 223162, mailed on Oct. 1, 2024, 3 Pages.

Swabstick Prep ChloraPrep CHG/Alc 3s 5.25mL 40/Bx, 10 BX/CA, https://www.surgicalsupplies.us/products/swabstick-prep-chloraprep-chg-alc-3s-5-25ml-40-bx-10-bx-ca, Sep. 21, 2021, 2 Pages.

\* cited by examiner

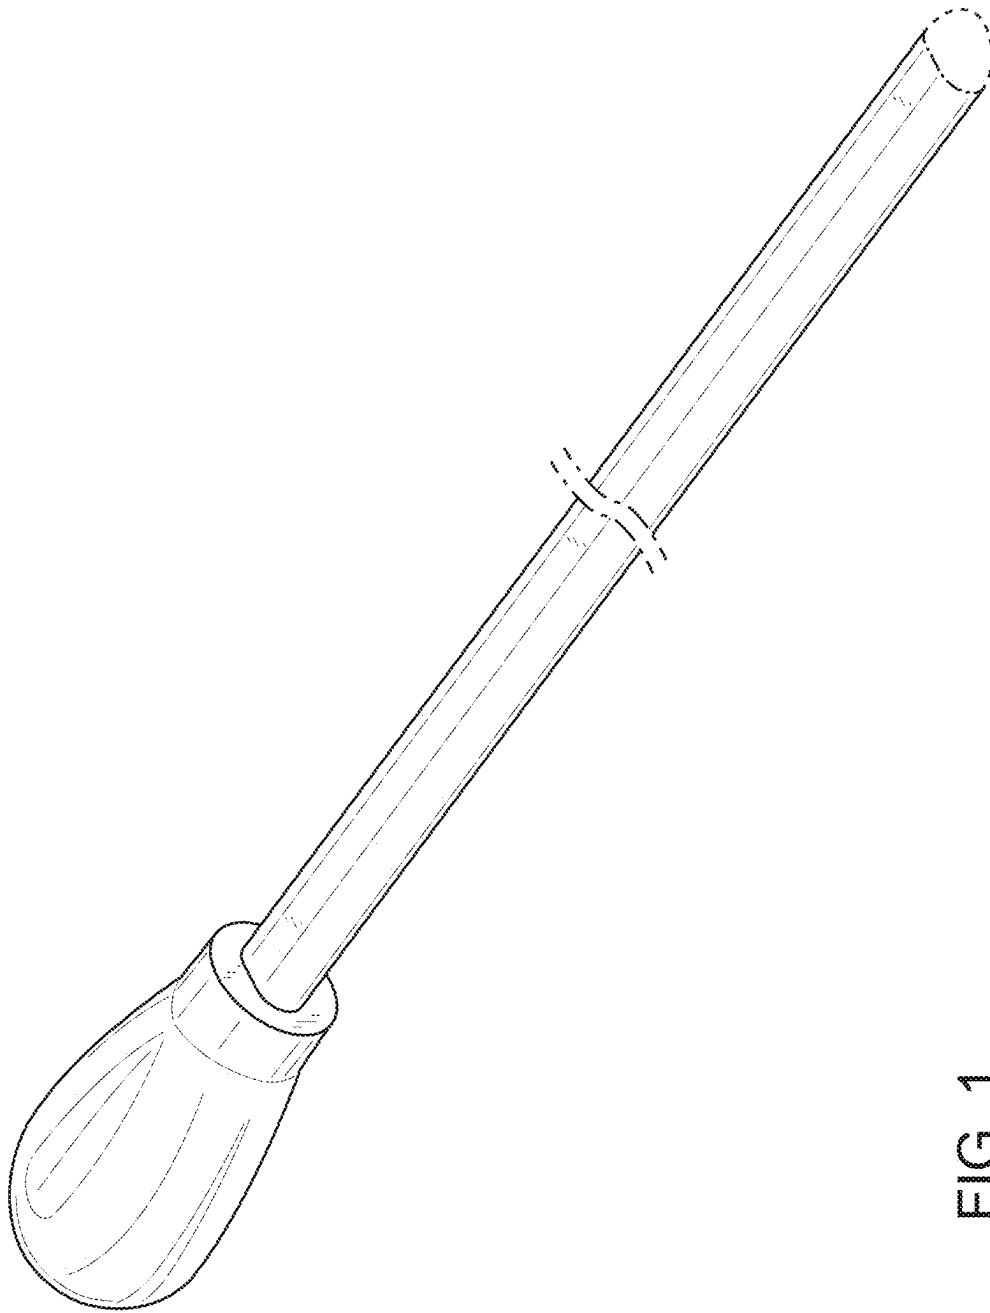


FIG. 1

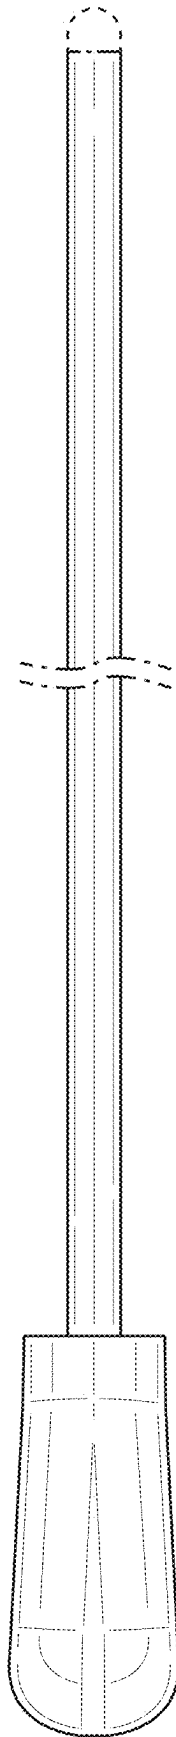


FIG. 2

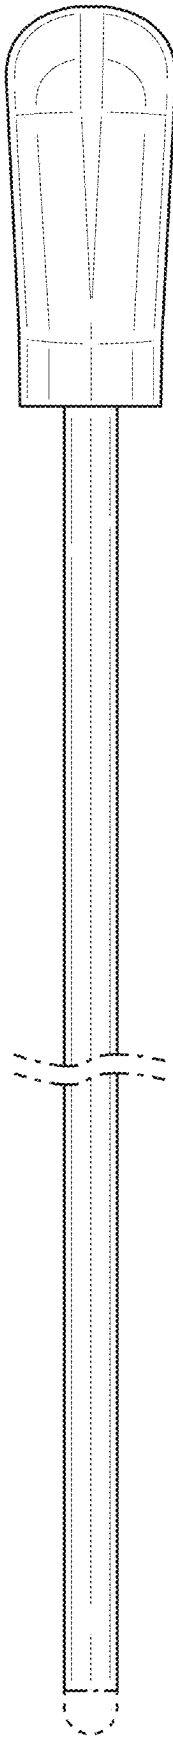


FIG. 3




FIG. 4




FIG. 5

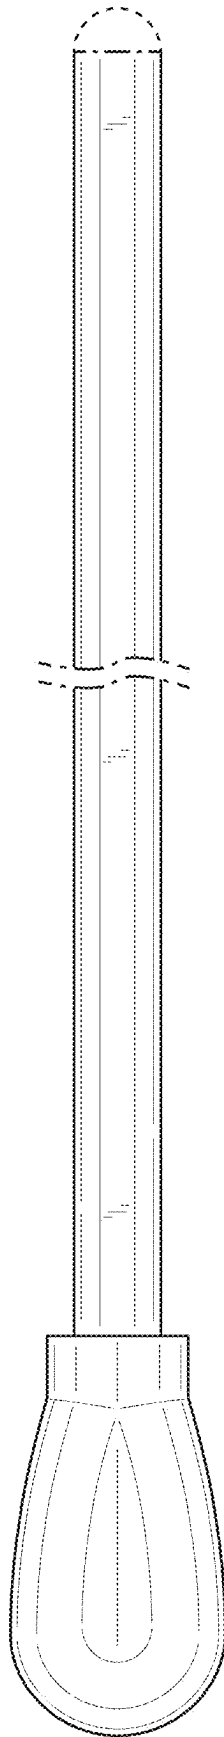


FIG. 6



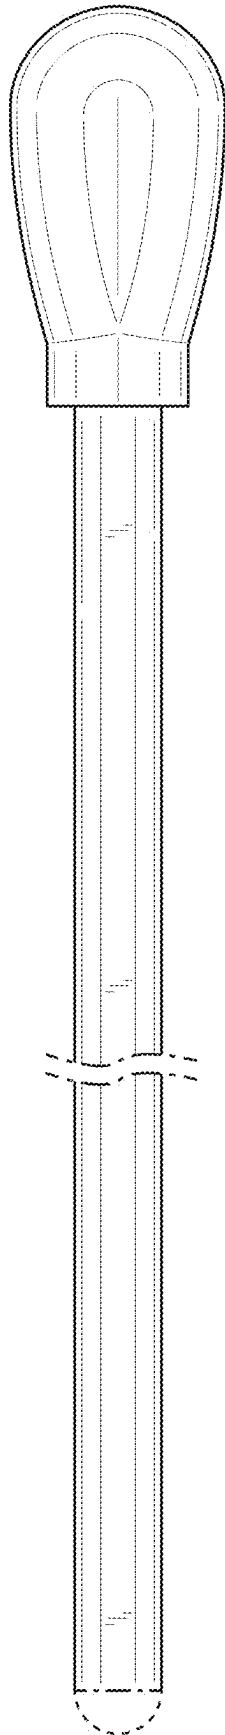


FIG. 7