

(12) **United States Patent**  
**Kusens et al.**

(10) **Patent No.:** **US 12,394,296 B2**  
(45) **Date of Patent:** **Aug. 19, 2025**

(54) **UTILIZING ARTIFICIAL INTELLIGENCE TO DETECT OBJECTS OR PATIENT SAFETY EVENTS IN A PATIENT ROOM**

(71) Applicant: **CERNER INNOVATION, INC.**,  
Kansas City, MO (US)

(72) Inventors: **Bruce Howard Kusens**, North Miami  
Beach, FL (US); **Michael Kusens**,  
Cooper City, FL (US)

(73) Assignee: **CERNER INNOVATION, INC.**,  
Kansas City, MO (US)

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 0 days.

(21) Appl. No.: **18/657,078**

(22) Filed: **May 7, 2024**

(65) **Prior Publication Data**  
US 2024/0290191 A1 Aug. 29, 2024

**Related U.S. Application Data**  
(63) Continuation of application No. 18/314,502, filed on  
May 9, 2023, now Pat. No. 12,008,880, which is a  
(Continued)

(51) **Int. Cl.**  
**G08B 29/18** (2006.01)  
**G06V 20/52** (2022.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **G08B 21/0476** (2013.01); **G06V 20/52**  
(2022.01); **G08B 29/185** (2013.01); **H04N**  
**13/204** (2018.05)

(58) **Field of Classification Search**  
None  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,669,263 A 6/1987 Sugiyama  
4,857,716 A 8/1989 Gombrich et al.  
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2014308590 A1 3/2016  
DE 19844918 A1 4/2000  
(Continued)

OTHER PUBLICATIONS


US 9,948,899 B1, 04/2018, Kusens (withdrawn)  
(Continued)

*Primary Examiner* — Eileen M Adams  
(74) *Attorney, Agent, or Firm* — Kilpatrick Townsend &  
Stockton LLP

(57) **ABSTRACT**

Methods and systems are provided for detecting objects or patient safety events in a patient room. Artificial intelligence is utilized to enhance safety issue recognition capabilities by the methods and systems. Sensors collect a series of images and depth data in a room of a patient. Data (corresponding to images and depth data of an object or patient safety event) is received from the sensors and compared to stored data to identify the object or patient safety event. The images are communicated to a central video monitoring system and a user may be prompted to confirm if the object requires learning or a patient safety event occurred (or identify the object or patient safety event) or to provide additional parameters or actions. A patient safety learning system analyzes the data and incorporates the user response to enhance safety issue recognition capabilities of the system and reduce false alerts.

**20 Claims, 6 Drawing Sheets**

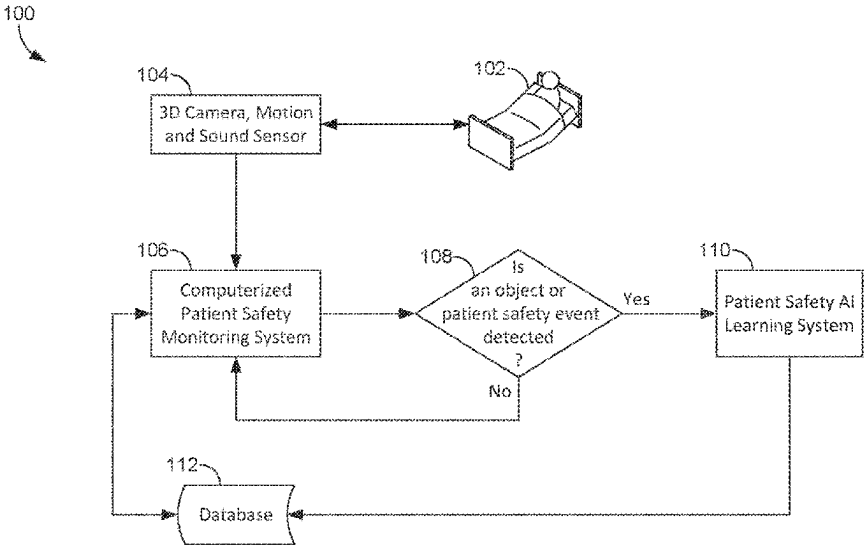

**Related U.S. Application Data**

continuation of application No. 17/646,942, filed on Jan. 4, 2022, now Pat. No. 11,721,190, which is a continuation of application No. 17/117,414, filed on Dec. 10, 2020, now Pat. No. 11,276,291, which is a continuation of application No. 16/832,790, filed on Mar. 27, 2020, now Pat. No. 10,922,946, which is a continuation of application No. 15/856,419, filed on Dec. 28, 2017, now Pat. No. 10,643,446.

(51) **Int. Cl.**

**G08B 21/04** (2006.01)

**H04N 13/204** (2018.01)

## (56)

**References Cited**

## U.S. PATENT DOCUMENTS

5,031,228 A	7/1991	Lu	8,769,153 B2	7/2014	Dziubinski
5,276,432 A	1/1994	Travis	8,890,937 B2	11/2014	Skubic et al.
5,448,221 A	9/1995	Weller	8,902,068 B2	12/2014	Bechtel et al.
5,482,050 A	1/1996	Smokoff et al.	8,917,186 B1	12/2014	Grant
5,592,153 A	1/1997	Welling et al.	8,953,886 B2	2/2015	King et al.
5,798,798 A	8/1998	Rector et al.	9,072,929 B1	7/2015	Rush et al.
5,838,223 A	11/1998	Gallant et al.	9,129,506 B1	9/2015	Kusens
5,915,379 A	6/1999	Wallace et al.	9,147,334 B2	9/2015	Long et al.
5,942,986 A	8/1999	Shabot et al.	9,159,215 B1	10/2015	Kusens
6,050,940 A	4/2000	Braun et al.	9,269,012 B2	2/2016	Fotland
6,095,984 A	8/2000	Amano et al.	9,292,089 B1	3/2016	Sadek
6,160,478 A	12/2000	Jacobsen et al.	9,305,191 B2	4/2016	Long et al.
6,174,283 B1	1/2001	Nevo et al.	9,367,270 B1	6/2016	Robertson
6,188,407 B1	2/2001	Smith et al.	9,408,561 B2	8/2016	Stone et al.
6,269,812 B1	8/2001	Wallace et al.	9,424,699 B2	8/2016	Kusens et al.
6,287,452 B1	9/2001	Allen et al.	9,466,163 B2	10/2016	Kusens et al.
6,322,502 B1	11/2001	Schoenberg et al.	9,489,820 B1	11/2016	Kusens
6,369,838 B1	4/2002	Wallace et al.	9,519,969 B1	12/2016	Kusens
6,429,869 B1	8/2002	Kamakura et al.	9,524,443 B1	12/2016	Kusens
6,614,349 B1	9/2003	Proctor et al.	9,536,310 B1	1/2017	Kusens
6,727,818 B1	4/2004	Wildman et al.	9,538,158 B1	1/2017	Rush et al.
6,804,656 B1	10/2004	Rosenfeld et al.	9,563,955 B1	2/2017	Kamarshi et al.
7,015,816 B2	3/2006	Wildman et al.	9,597,016 B2	3/2017	Stone et al.
7,122,005 B2	10/2006	Shusterman	9,691,206 B2	6/2017	Kusens et al.
7,154,397 B2	12/2006	Zerhusen et al.	9,729,833 B1	8/2017	Kusens
7,237,287 B2	7/2007	Weismiller et al.	9,741,227 B1	8/2017	Kusens
7,323,991 B1	1/2008	Eckert et al.	9,774,991 B2	9/2017	Kusens
7,408,470 B2	8/2008	Wildman et al.	9,838,849 B2	12/2017	Kusens
7,420,472 B2	9/2008	Tran	9,858,741 B2	1/2018	Kusens et al.
7,430,608 B2	9/2008	Noonan et al.	9,892,310 B2	2/2018	Kusens et al.
7,502,498 B2	3/2009	Wen et al.	9,892,311 B2	2/2018	Kusens et al.
7,612,679 B1	11/2009	Fackler et al.	9,892,611 B1	2/2018	Kusens
7,669,263 B2	3/2010	Menkedick et al.	9,905,113 B2	2/2018	Kusens
7,715,387 B2	5/2010	Schuman	9,934,427 B2	4/2018	Derenne et al.
7,724,147 B2	5/2010	Brown	9,984,521 B1	5/2018	Kusens et al.
7,756,723 B2	7/2010	Rosow et al.	9,997,001 B2	6/2018	Kusens et al.
7,890,349 B2	2/2011	Cole et al.	9,998,857 B2	6/2018	Kusens
7,893,842 B2	2/2011	Deutsch	10,013,831 B1	7/2018	Kusens et al.
7,895,055 B2	2/2011	Schneider et al.	10,055,961 B1	8/2018	Johnson et al.
7,908,153 B2	3/2011	Scherpbier et al.	10,068,116 B2	9/2018	Good et al.
7,945,457 B2	5/2011	Zaleski	10,078,956 B1	9/2018	Kusens
7,962,544 B2	6/2011	Torok et al.	10,090,068 B2	10/2018	Kusens et al.
7,972,140 B2	7/2011	Renaud	10,091,463 B1	10/2018	Kusens
8,108,036 B2	1/2012	Tran	10,096,223 B1	10/2018	Kusens
8,123,685 B2	2/2012	Brauers et al.	10,109,179 B2	10/2018	Kusens
8,128,596 B2	3/2012	Carter	10,115,253 B2	10/2018	Kusens et al.
8,190,447 B2	5/2012	Hungerford et al.	10,115,254 B1	10/2018	Kusens et al.
8,224,108 B2	7/2012	Steinberg et al.	10,121,299 B2	11/2018	Kusens et al.
8,237,558 B2	8/2012	Seyed Momen et al.	10,210,378 B2	2/2019	Kusens et al.
8,273,018 B1	9/2012	Fackler et al.	10,225,522 B1	3/2019	Kusens
8,432,263 B2	4/2013	Kunz	10,276,019 B2	4/2019	Johnson et al.
8,451,314 B1	5/2013	Cline et al.	10,303,924 B2	5/2019	Kusens et al.
8,529,448 B2	9/2013	McNair	10,342,478 B2	7/2019	Kusens
8,565,500 B2	10/2013	Neff	10,410,042 B2	9/2019	Kusens et al.
8,620,682 B2	12/2013	Bechtel et al.	10,524,722 B2	1/2020	Kusens et al.
8,655,680 B2	2/2014	Bechtel et al.	10,614,288 B2	4/2020	Kusens et al.
8,700,423 B2	4/2014	Eaton, Jr. et al.	10,643,061 B2	5/2020	Kusens et al.
8,727,981 B2	5/2014	Bechtel et al.	10,643,446 B2	5/2020	Kusens et al.
			10,878,220 B2	12/2020	Kusens
			10,922,936 B2	2/2021	Kusens et al.
			10,922,946 B2	2/2021	Kusens et al.
			11,241,169 B2	2/2022	Kusens et al.
			11,276,291 B2	3/2022	Kusens et al.
			11,721,190 B2	8/2023	Kusens et al.
			12,008,880 B2 *	6/2024	Kusens ..... G08B 21/0476
			2002/0015034 A1	2/2002	Malmberg
			2002/0038073 A1	3/2002	August
			2002/0077863 A1	6/2002	Rutledge et al.
			2002/0101349 A1	8/2002	Rojas, Jr.
			2002/0115905 A1	8/2002	August
			2002/0183976 A1	12/2002	Pearce
			2003/0037786 A1	2/2003	Biondi et al.
			2003/0070177 A1	4/2003	Kondo et al.
			2003/0092974 A1	5/2003	Santoso et al.
			2003/0095147 A1	5/2003	Daw
			2003/0108223 A1	6/2003	Prokoski
			2003/0135390 A1	7/2003	O'Brien et al.
			2003/0140928 A1	7/2003	Bui et al.
			2003/0227386 A1	12/2003	Pulkkinen et al.

(56)	<b>References Cited</b>				
	U.S. PATENT DOCUMENTS				
2004/0019900	A1	1/2004	Knightsbridge et al.	2011/0068930	A1 3/2011 Wildman et al.
2004/0052418	A1	3/2004	Delean	2011/0077965	A1 3/2011 Nolte et al.
2004/0054760	A1	3/2004	Ewing et al.	2011/0087079	A1 4/2011 Aarts
2004/0097227	A1	5/2004	Siegel	2011/0087125	A1 4/2011 Causevic
2004/0116804	A1	6/2004	Mostafavi	2011/0102133	A1 5/2011 Shaffer
2004/0193449	A1	9/2004	Wildman et al.	2011/0102181	A1 5/2011 Metz et al.
2005/0038326	A1	2/2005	Mathur	2011/0106560	A1 5/2011 Eaton, Jr. et al.
2005/0182305	A1	8/2005	Hendrich	2011/0106561	A1 5/2011 Eaton, Jr. et al.
2005/0231341	A1	10/2005	Shimizu	2011/0175809	A1 7/2011 Markovic et al.
2005/0249139	A1	11/2005	Nesbit	2011/0190593	A1 8/2011 McNair
2006/0004606	A1	1/2006	Wendl et al.	2011/0227740	A1 9/2011 Wohltjen
2006/0047538	A1	3/2006	Concurso et al.	2011/0245707	A1 10/2011 Castle et al.
2006/0049936	A1	3/2006	Collins, Jr. et al.	2011/0254682	A1 10/2011 Sigrist Christensen
2006/0058587	A1	3/2006	Heimbrock et al.	2011/0288811	A1 11/2011 Greene
2006/0089541	A1	4/2006	Braun et al.	2011/0295621	A1 12/2011 Farooq et al.
2006/0092043	A1	5/2006	Lagassey	2011/0301440	A1 12/2011 Riley et al.
2006/0107295	A1	5/2006	Margis et al.	2011/0313325	A1 12/2011 Cuddihy
2006/0145874	A1	7/2006	Fredriksson et al.	2012/0016295	A1 1/2012 Tsoukalis
2006/0261974	A1	11/2006	Albert et al.	2012/0025991	A1 2/2012 O'keefe et al.
2007/0033072	A1	2/2007	Bildirici	2012/0026308	A1 2/2012 Johnson et al.
2007/0083445	A1	4/2007	Garcia et al.	2012/0075464	A1 3/2012 Derenne et al.
2007/0085690	A1	4/2007	Tran	2012/0092162	A1 4/2012 Rosenberg
2007/0118054	A1	5/2007	Pinhas et al.	2012/0098918	A1 4/2012 Murphy
2007/0120689	A1	5/2007	Zerhusen et al.	2012/0140068	A1 6/2012 Monroe et al.
2007/0129983	A1	6/2007	Scherpbier et al.	2012/0154582	A1 6/2012 Johnson et al.
2007/0136102	A1	6/2007	Rodgers	2012/0212582	A1 8/2012 Deutsch
2007/0136218	A1	6/2007	Bauer et al.	2012/0259650	A1 10/2012 Mallon et al.
2007/0159332	A1	7/2007	Koblasz	2012/0314901	A1 12/2012 Hanson et al.
2007/0279219	A1	12/2007	Warriner	2012/0323090	A1 12/2012 Bechtel et al.
2007/0296600	A1	12/2007	Dixon et al.	2012/0323591	A1 12/2012 Bechtel et al.
2008/0001735	A1	1/2008	Tran	2012/0323592	A1 12/2012 Bechtel et al.
2008/0001763	A1	1/2008	Raja et al.	2013/0027199	A1 1/2013 Bonner
2008/0002860	A1	1/2008	Super et al.	2013/0028570	A1 1/2013 Suematsu et al.
2008/0004904	A1	1/2008	Tran	2013/0120120	A1 5/2013 Long et al.
2008/0009686	A1	1/2008	Hendrich	2013/0122807	A1 5/2013 Tenarvitz et al.
2008/0015903	A1	1/2008	Rodgers	2013/0127620	A1 5/2013 Siebers et al.
2008/0021731	A1	1/2008	Rodgers	2013/0184592	A1 7/2013 Venetianer et al.
2008/0071210	A1	3/2008	Moubayed et al.	2013/0265482	A1 10/2013 Funamoto
2008/0087719	A1	4/2008	Sahud	2013/0309128	A1 11/2013 Voegeli et al.
2008/0106374	A1	5/2008	Sharbaugh	2013/0324868	A1* 12/2013 Kaib ..... A61N 1/3937 600/510
2008/0126132	A1	5/2008	Warner et al.	2013/0332184	A1 12/2013 Burnham et al.
2008/0228045	A1	9/2008	Gao et al.	2014/0039351	A1 2/2014 Mix et al.
2008/0249376	A1	10/2008	Zaleski	2014/0070950	A1 3/2014 Snodgrass
2008/0267447	A1	10/2008	Kelusky et al.	2014/0081654	A1 3/2014 Bechtel et al.
2008/0277486	A1	11/2008	Seem et al.	2014/0085501	A1 3/2014 Tran
2008/0281638	A1	11/2008	Weatherly et al.	2014/0086450	A1 3/2014 Huang et al.
2009/0082829	A1	3/2009	Panken et al.	2014/0108041	A1 4/2014 Bechtel et al.
2009/0091458	A1	4/2009	Deutsch	2014/0155755	A1 6/2014 Pinter et al.
2009/0099480	A1	4/2009	Salgo et al.	2014/0168397	A1 6/2014 Greco et al.
2009/0112630	A1	4/2009	Collins, Jr. et al.	2014/0191861	A1 7/2014 Scherrer
2009/0119843	A1	5/2009	Rodgers et al.	2014/0191946	A1 7/2014 Cho et al.
2009/0177327	A1	7/2009	Turner et al.	2014/0213845	A1 7/2014 Bechtel et al.
2009/0196510	A1	8/2009	Gokturk et al.	2014/0267625	A1 9/2014 Clark et al.
2009/0224924	A1	9/2009	Thorp	2014/0267736	A1 9/2014 Delean
2009/0278934	A1	11/2009	Ecker et al.	2014/0309789	A1 10/2014 Ricci
2009/0322513	A1	12/2009	Hwang et al.	2014/0327545	A1 11/2014 Bolling et al.
2009/0326340	A1	12/2009	Wang et al.	2014/0328512	A1 11/2014 Gurwicz et al.
2010/0117836	A1	5/2010	Sayed Momen et al.	2014/0333744	A1 11/2014 Baym et al.
2010/0169114	A1	7/2010	Henderson et al.	2014/0333776	A1 11/2014 Dedeoglu et al.
2010/0169120	A1	7/2010	Herbst et al.	2014/0354436	A1 12/2014 Nix et al.
2010/0172567	A1	7/2010	Prokoski	2014/0365242	A1 12/2014 Neff
2010/0176952	A1	7/2010	Bajcsy et al.	2015/0057635	A1 2/2015 Bechtel et al.
2010/0188228	A1	7/2010	Hyland	2015/0061891	A1 3/2015 Oleson et al.
2010/0205771	A1	8/2010	Pietryga et al.	2015/0109442	A1 4/2015 Derenne et al.
2010/0245577	A1	9/2010	Yamamoto et al.	2015/0206415	A1 7/2015 Wegelin et al.
2010/0285771	A1	11/2010	Peabody	2015/0227680	A1 8/2015 Mainkar et al.
2010/0305466	A1	12/2010	Corn	2015/0269318	A1 9/2015 Neff
2011/0018709	A1	1/2011	Kornbluh	2015/0278456	A1 10/2015 Bermudez Rodriguez et al.
2011/0022981	A1	1/2011	Mahajan et al.	2015/0294143	A1 10/2015 Wells et al.
2011/0025493	A1	2/2011	Papadopoulos et al.	2016/0022218	A1 1/2016 Hayes et al.
2011/0025499	A1	2/2011	Hoy et al.	2016/0029160	A1 1/2016 Theurer et al.
2011/0035057	A1	2/2011	Receveur et al.	2016/0070869	A1 3/2016 Portnoy
2011/0035466	A1	2/2011	Panigrahi	2016/0093195	A1 3/2016 Ophardt
2011/0050411	A1	3/2011	Schuman et al.	2016/0098676	A1 4/2016 Kusens et al.
2011/0054936	A1	3/2011	Cowan et al.	2016/0127641	A1 5/2016 Gove
				2016/0180668	A1* 6/2016 Kusens ..... G16H 40/20 340/541
				2016/0183864	A1 6/2016 Kusens et al.

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

2016/0217347	A1	7/2016	Mineo	
2016/0253802	A1	9/2016	Venetianer et al.	
2016/0267327	A1	9/2016	Franz et al.	
2016/0285416	A1	9/2016	Tiwari et al.	
2016/0314258	A1	10/2016	Kusens	
2016/0324460	A1	11/2016	Kusens	
2016/0360970	A1	12/2016	Tzvieli et al.	
2017/0055917	A1	3/2017	Stone et al.	
2017/0084158	A1	3/2017	Kusens	
2017/0091562	A1	3/2017	Kusens	
2017/0109991	A1	4/2017	Kusens	
2017/0116473	A1	4/2017	Sashida et al.	
2017/0143240	A1	5/2017	Stone et al.	
2017/0163949	A1	6/2017	Suzuki	
2017/0193177	A1	7/2017	Kusens	
2017/0193279	A1	7/2017	Kusens et al.	
2017/0193772	A1	7/2017	Kusens et al.	
2017/0195637	A1	7/2017	Kusens et al.	
2017/0214902	A1	7/2017	Braune	
2017/0289503	A1	10/2017	Kusens	
2017/0337682	A1	11/2017	Liao et al.	
2018/0018864	A1	1/2018	Baker	
2018/0053071	A1 *	2/2018	Chen .....	G06N 20/10
2018/0068545	A1	3/2018	Kusens	
2018/0104409	A1	4/2018	Bechtel et al.	
2018/0114053	A1	4/2018	Kusens et al.	
2018/0116528	A1	5/2018	Tzvieli et al.	
2018/0137340	A1	5/2018	Kusens et al.	
2018/0144605	A1	5/2018	Kusens	
2018/0150683	A1 *	5/2018	Gordon .....	G06V 20/52
2018/0189946	A1	7/2018	Kusens et al.	
2018/0190098	A1	7/2018	Kusens	
2018/0357875	A1	12/2018	Kusens	
2019/0006046	A1	1/2019	Kusens et al.	
2019/0029528	A1	1/2019	Tzvieli et al.	
2019/0043192	A1	2/2019	Kusens et al.	
2019/0057592	A1	2/2019	Kusens	
2019/0122028	A1	4/2019	Kusens et al.	
2019/0205630	A1	7/2019	Kusens	
2019/0206218	A1	7/2019	Kusens et al.	
2019/0209022	A1	7/2019	Sobol et al.	
2019/0228866	A1	7/2019	Weffers-albu et al.	
2019/0253668	A1	8/2019	Kusens	
2019/0261915	A1	8/2019	Kusens	
2019/0307405	A1	10/2019	Terry et al.	
2019/0318149	A1	10/2019	Kusens et al.	
2019/0318478	A1	10/2019	Kusens et al.	
2020/0050844	A1	2/2020	Kusens	
2020/0210679	A1	7/2020	Kusens et al.	
2020/0226905	A1	7/2020	Kusens et al.	
2020/0335208	A1 *	10/2020	Talmor .....	G16H 40/60
2021/0090420	A1	3/2021	Kusens et al.	
2021/0202052	A1	7/2021	Bechtel et al.	

## FOREIGN PATENT DOCUMENTS

WO	2007081629	A2	7/2007
WO	2009018422	A1	2/2009
WO	2012122002	A1	9/2012
WO	2016126845	A1	8/2016
WO	2017058991	A1	4/2017
WO	2017124056	A1	7/2017
WO	2018218286	A1	12/2018

## OTHER PUBLICATIONS

Raheja, et al., Human Facial Expression Detection From Detected in Captured Image Using Back Propagation Neural Network, International Journal of Computer Science and Information Technology, vol. 2, No. 1, Feb. 2010, pp. 116-123.

U.S. Appl. No. 14/757,877, Final Office Action mailed on Sep. 29, 2017, 22 pages.

U.S. Appl. No. 14/757,877, Non-Final Office Action mailed on Feb. 23, 2017, 24 pages.

U.S. Appl. No. 14/757,877, Non-Final Office Action mailed on Mar. 14, 2018, 13 pages.

U.S. Appl. No. 15/134,189, Final Office Action mailed on Jul. 12, 2018, 23 pages.

U.S. Appl. No. 15/134,189, Final Office Action mailed on May 6, 2020, 31 pages.

U.S. Appl. No. 15/134,189, First Action Interview Office Action mailed on Feb. 22, 2018, 3 pages.

U.S. Appl. No. 15/134,189, First Action Interview Pre-Interview Communication mailed on Nov. 22, 2017, 5 pages.

U.S. Appl. No. 15/134,189, Non-Final Office Action mailed on May 9, 2019, 30 pages.

U.S. Appl. No. 15/148,151, Non-Final Office Action mailed on May 8, 2018, 5 pages.

U.S. Appl. No. 15/279,054, Corrected Notice of Allowability mailed on Jan. 18, 2018, 2 pages.

U.S. Appl. No. 15/279,054, Notice of Allowance mailed on Nov. 27, 2017, 2 pages.

U.S. Appl. No. 15/279,054, Notice of Allowance mailed on Oct. 20, 2017, 13 pages.

U.S. Appl. No. 15/285,416, Final Office Action mailed on Aug. 23, 2017, 16 pages.

U.S. Appl. No. 15/285,416, Final Office Action mailed on Jul. 5, 2018, 8 pages.

U.S. Appl. No. 15/285,416, Non-Final Office Action mailed on Apr. 11, 2017, 13 pages.

U.S. Appl. No. 15/285,416, Non-Final Office Action mailed on Mar. 12, 2018, 20 pages.

U.S. Appl. No. 15/395,243, Final Office Action mailed on Jun. 11, 2019, 18 pages.

U.S. Appl. No. 15/395,243, Non-Final Office Action mailed on Feb. 14, 2019, 14 pages.

U.S. Appl. No. 15/395,250, Non-Final Office Action mailed on May 8, 2017, 19 pages.

U.S. Appl. No. 15/395,250, Notice of Allowance mailed on Sep. 26, 2017, 12 pages.

U.S. Appl. No. 15/395,526, Non-Final Office Action mailed on Apr. 27, 2017, 16 pages.

U.S. Appl. No. 15/395,526, Notice of Allowance mailed on Sep. 21, 2017, 12 pages.

U.S. Appl. No. 15/395,716, First Action Interview Pilot Program Pre-Interview Communication mailed on Feb. 24, 2017, 5 pages.

U.S. Appl. No. 15/395,716, Notice of Allowance mailed on Apr. 19, 2017, 5 pages.

U.S. Appl. No. 15/395,716, Notice of Allowance mailed on Dec. 6, 2017, 5 pages.

U.S. Appl. No. 15/395,716, Notice of Allowance mailed on Jul. 24, 2017, 5 pages.

U.S. Appl. No. 15/395,716, Notice of Allowance mailed on Jun. 19, 2018, 2 pages.

U.S. Appl. No. 15/395,716, Notice of Allowance mailed on May 9, 2018, 5 pages.

U.S. Appl. No. 15/395,762, Non-Final Office Action mailed on May 1, 2019, 27 pages.

U.S. Appl. No. 15/395,762, Non-Final Office Action mailed on May 31, 2018, 24 pages.

U.S. Appl. No. 15/396,263, Final Office Action mailed on Oct. 18, 2017, 20 pages.

U.S. Appl. No. 15/396,263, Non-Final Office Action mailed on Apr. 14, 2017, 18 pages.

U.S. Appl. No. 15/396,263, Non-Final Office Action mailed on Feb. 7, 2018, 19 pages.

U.S. Appl. No. 15/396,263, Notice of Allowance mailed on Jul. 13, 2018, 9 pages.

U.S. Appl. No. 15/628,318, Non-Final Office Action mailed on Jun. 8, 2018, 9 pages.

U.S. Appl. No. 15/728,110, Non-Final Office Action mailed on May 2, 2018, 8 pages.

U.S. Appl. No. 15/728,110, Notice of Allowance mailed on Jul. 23, 2018, 15 pages.

(56)

**References Cited****OTHER PUBLICATIONS**

U.S. Appl. No. 15/848,621, Non-Final Office Action mailed on May 31, 2018, 23 pages.

U.S. Appl. No. 15/856,419, Non-Final Office Action mailed on May 2, 2019, 8 pages.

U.S. Appl. No. 15/856,419, Notice of Allowance mailed on Jan. 3, 2020, 6 pages.

U.S. Appl. No. 15/857,696, First Action Interview Pilot Program Pre-Interview Communication mailed on May 23, 2019, 14 pages.

U.S. Appl. No. 15/857,696, Notice of Allowance mailed on Jul. 16, 2019, 9 pages.

U.S. Appl. No. 15/910,632, Non-Final Office Action mailed on Aug. 15, 2018, 7 pages.

U.S. Appl. No. 15/910,645, First Action Interview Pre-Interview Communication mailed on May 21, 2018, 14 pages.

U.S. Appl. No. 16/107,567, Non-Final Office Action mailed on Mar. 29, 2019, 8 pages.

U.S. Appl. No. 16/181,897, First Action Interview Pilot Program Pre-Interview Communication mailed on May 11, 2020, 5 pages.

U.S. Appl. No. 16/181,897, Notice of Allowance mailed on Oct. 14, 2020, 9 pages.

U.S. Appl. No. 16/216,210, Non-Final Office Action mailed on Feb. 13, 2019, 29 pages.

U.S. Appl. No. 16/380,013, Notice of Allowance mailed on Jul. 10, 2019, 9 pages.

Camera System is Part of an Automated Hand Hygiene Monitoring System, Infection Control Today, Jul. 15, 2011, pp. 1-4.

Virtual Patient Observation: Centralize Monitoring of High-Risk Patients with Video-Cisco Video Surveillance Manager, Cisco, Available online at: [https://www.cisco.com/c/en/us/products/collateral/physical-security/video-surveillance-manager/white\\_paper\\_C11-715263.pdf](https://www.cisco.com/c/en/us/products/collateral/physical-security/video-surveillance-manager/white_paper_C11-715263.pdf), 2013, pp. 1-6.

U.S. Appl. No. 13/543,816, Final Office Action mailed on Jun. 17, 2014, 15 pages.

U.S. Appl. No. 13/543,816, Non-Final Office Action mailed on Dec. 1, 2014, 18 pages.

U.S. Appl. No. 13/543,816, Non-Final Office Action mailed on Dec. 30, 2013, 9 pages.

U.S. Appl. No. 13/543,816, Notice of Allowance mailed on Jun. 5, 2015, 5 pages.

U.S. Appl. No. 14/084,588, Final Office Action mailed on Dec. 19, 2014, 24 pages.

U.S. Appl. No. 14/084,588, Non-Final Office Action mailed on Jul. 16, 2014, 12 pages.

U.S. Appl. No. 14/339,397, Non-Final Office Action mailed on Oct. 7, 2015, 16 pages.

U.S. Appl. No. 14/575,850, Final Office Action mailed on Dec. 12, 2017, 10 pages.

U.S. Appl. No. 14/575,850, Non-Final Office Action mailed on Mar. 11, 2016, 10 pages.

U.S. Appl. No. 14/575,850, Notice of Allowance mailed on Jun. 13, 2018, 5 pages.

U.S. Appl. No. 14/575,850, Titled: Method and Process for Determining Whether an Individual Suffers a Fall Requiring Assistance filed Dec. 18, 2014, 37 pages.

U.S. Appl. No. 14/599,498, Final Office Action mailed on Oct. 12, 2017, 28 pages.

U.S. Appl. No. 14/599,498, Non-Final Office Action mailed on Feb. 22, 2018, 24 pages.

U.S. Appl. No. 14/599,498, Non-Final Office Action mailed on May 31, 2017, 24 pages.

U.S. Appl. No. 14/599,498, Notice of Allowance mailed on Jul. 18, 2018, 6 pages.

U.S. Appl. No. 14/599,498, Titled: Method and System for Determining Whether an Individual Takes Appropriate Measures To Prevent the Spread of Healthcare-Associated Infections, filed Jan. 17, 2015, 37 pages.

U.S. Appl. No. 14/611,363, Final Office Action mailed on Apr. 28, 2017, 20 pages.

U.S. Appl. No. 14/611,363, Non-Final Office Action mailed on Jan. 11, 2017, 19 pages.

U.S. Appl. No. 14/611,363, Non-Final Office Action mailed on May 7, 2018, 6 pages.

U.S. Appl. No. 14/611,363, Notice of Allowance mailed on Dec. 29, 2017, 11 pages.

U.S. Appl. No. 14/611,363, Titled: Method and System for Determining Whether an Individual Takes Appropriate Measures To Prevent the Spread of Healthcare-Associated Infections filed Feb. 2, 2015, 40 pages.

U.S. Appl. No. 14/613,866, Notice of Allowance mailed on Mar. 20, 2017, 11 pages.

U.S. Appl. No. 14/623,349, Final Office Action mailed on Oct. 4, 2017, 29 pages.

U.S. Appl. No. 14/623,349, Non-Final Office Action mailed on Apr. 5, 2017, 15 pages.

U.S. Appl. No. 14/623,349, Notice of Allowance mailed on Feb. 12, 2018, 11 pages.

U.S. Appl. No. 14/623,349, Notice of Allowance mailed on Jun. 18, 2018, 11 pages.

U.S. Appl. No. 14/724,969, Final Office Action mailed on Jul. 28, 2016, 26 pages.

U.S. Appl. No. 14/724,969, Non-Final Office Action mailed on Feb. 11, 2016, 14 pages.

U.S. Appl. No. 14/724,969, Notice of Allowance mailed on Apr. 21, 2017, 8 pages.

U.S. Appl. No. 14/724,969, Notice of Allowance mailed on Dec. 23, 2016, 5 pages.

U.S. Appl. No. 14/727,434, Non-Final Office Action mailed on Sep. 23, 2016, 9 pages.

U.S. Appl. No. 14/727,434, Notice of Allowance mailed on Apr. 25, 2017, 9 pages.

U.S. Appl. No. 14/727,434, Notice of Allowance mailed on Jul. 5, 2017, 9 pages.

U.S. Appl. No. 14/727,434, Notice of Allowance mailed on Oct. 10, 2017, 9 pages.

U.S. Appl. No. 14/728,762, Notice of Allowance mailed on Jun. 27, 2016, 13 pages.

U.S. Appl. No. 14/743,264, Notice of Allowance mailed on Jul. 18, 2016, 15 pages.

U.S. Appl. No. 14/743,264, Notice of Allowance mailed on Nov. 9, 2016, 14 pages.

U.S. Appl. No. 14/743,264, Notice of Allowance mailed on Oct. 14, 2016, 14 pages.

U.S. Appl. No. 14/743,447, Notice of Allowability mailed on Jun. 22, 2016, 4 pages.

U.S. Appl. No. 14/743,447, Notice of Allowance mailed on Aug. 26, 2016, 5 pages.

U.S. Appl. No. 14/743,447, Notice of Allowance mailed on May 31, 2016, 8 pages.

U.S. Appl. No. 14/743,447, Notice of Allowance mailed on Nov. 14, 2016, 5 pages.

U.S. Appl. No. 14/743,499, Non-Final Office Action mailed on May 23, 2016, 6 pages.

U.S. Appl. No. 14/743,499, Notice of Allowance mailed on Sep. 19, 2016, 5 pages.

U.S. Appl. No. 14/757,593, Final Office Action mailed on Feb. 16, 2018, 8 pages.

U.S. Appl. No. 14/757,593, Non-Final Office Action mailed on Apr. 21, 2017, 9 pages.

U.S. Appl. No. 14/757,593, Non-Final Office Action mailed on Aug. 16, 2017, 8 pages.

U.S. Appl. No. 14/757,593, Notice of Allowance mailed on Jun. 4, 2018, 5 pages.

Zarka, et al., Real-Time Human Motion Detection and Tracking, 3rd International Conference on Information and Communication Technologies: From Theory to Applications, Apr. 7-11, 2008, pp. 1-6.

U.S. Appl. No. 16/410,745, Non-Final Office Action mailed on May 21, 2021, 21 pages.

U.S. Appl. No. 16/410,745, Notice of Allowance mailed on Jan. 4, 2022, 10 pages.

U.S. Appl. No. 16/654,502, Notice of Allowance mailed on Feb. 17, 2021, 20 pages.

(56)

**References Cited**

## OTHER PUBLICATIONS

U.S. Appl. No. 16/731,274, First Action Interview Pilot Program Pre-Interview Communication mailed on Sep. 1, 2021, 12 pages.  
 U.S. Appl. No. 16/816,626, First Action Interview Pilot Program Pre-Interview Communication mailed on Dec. 22, 2020, 4 pages.  
 U.S. Appl. No. 16/816,626, Notice of Allowance mailed on Sep. 30, 2021, 9 pages.  
 U.S. Appl. No. 16/830,498, Non-Final Office Action mailed on Sep. 22, 2021, 29 pages.  
 U.S. Appl. No. 16/832,790, First Action Interview Pilot Program Pre-Interview Communication mailed on Aug. 25, 2020, 5 pages.  
 U.S. Appl. No. 16/832,790, Notice of Allowance mailed on Jan. 6, 2021, 2 pages.  
 U.S. Appl. No. 16/832,790, Notice of Allowance mailed on Oct. 27, 2020, 2 pages.  
 U.S. Appl. No. 16/832,790, Notice of Allowance mailed on Oct. 9, 2020, 10 pages.  
 U.S. Appl. No. 17/101,639, Non-Final Office Action mailed on Aug. 2, 2022, 13 pages.  
 U.S. Appl. No. 17/101,639, Non-Final Office Action mailed on Sep. 13, 2021, 13 pages.  
 U.S. Appl. No. 17/117,414, Non-Final Office Action mailed on Jul. 27, 2021, 12 pages.  
 U.S. Appl. No. 17/117,414, Notice of Allowance mailed on Jan. 31, 2022, 10 pages.  
 U.S. Appl. No. 17/117,414, Notice of Allowance mailed on Oct. 14, 2021, 2 pages.  
 U.S. Appl. No. 17/117,414, Notice of Allowance mailed on Sep. 27, 2021, 10 pages.  
 U.S. Appl. No. 17/152,403, Non-Final Office Action mailed on Mar. 15, 2022, 10 pages.  
 U.S. Appl. No. 17/318,521, Notice of Allowance mailed on Aug. 31, 2022, 9 pages.

U.S. Appl. No. 17/646,942, Non-Final Office Action mailed on Nov. 17, 2022, 11 pages.  
 U.S. Appl. No. 17/646,942, Notice of Allowance mailed on Jun. 7, 2023, 10 pages.  
 U.S. Appl. No. 17/646,942, Notice of Allowance mailed on Mar. 2, 2023, 10 pages.  
 U.S. Appl. No. 18/314,502, Final Office Action mailed on Mar. 1, 2024, 19 pages.  
 U.S. Appl. No. 18/314,502, Non-Final Office Action mailed on Dec. 13, 2023, 17 pages.  
 U.S. Appl. No. 18/314,502, Notice of Allowance mailed on Apr. 11, 2024, 10 pages.  
 Alotaibi, et al., The Impact of Health Information Technology on Patient Safety, Saudi Medical Journal, vol. 38, No. 12, Available online at: <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5787626/pdf/SaudiMedJ-38-1173.pdf>, Dec. 2017, pp. 1173-1180.  
 Conaire, et al., Fusion of Infrared and Visible Spectrum Video for Indoor Surveillance, Available Online at [https://doras.dcu.ie/382/1/wiamis\\_2005.pdf](https://doras.dcu.ie/382/1/wiamis_2005.pdf), Apr. 2005, 4 pages.  
 Hong, [WOHIT] Hand Hygiene Being Taught in Hospitals via Social Gaming, L'Atelier BNP Paribas, Apr. 2014, 6 pages.  
 Long, et al., Using Simulation to Teach Resuscitation: An Important Patient Safety Tool, Critical Care Nursing Clinics of North America, vol. 17, No. 1, Mar. 2005, pp. 1-8.  
 Mooney, Rhode Island ER First to Test Google Glass on Medical Conditions, EMS Technology, Mar. 10, 2014, 4 pages.  
 Otnasap, et al., Pre-Impact Fall Detection System Using Dynamic Threshold and 3D Bounding Box, Eighth International Conference on Graphic and Image Processing, Feb. 8, 2017, 5 pages.  
 Quan, et al., Facial Asymmetry Analysis Based on 3-D Dynamic Scans, Institute of Electrical and Electronics Engineers, International Conference on Systems, Man, and Cybernetics, Oct. 14-17, 2012, pp. 2676-2681.

\* cited by examiner

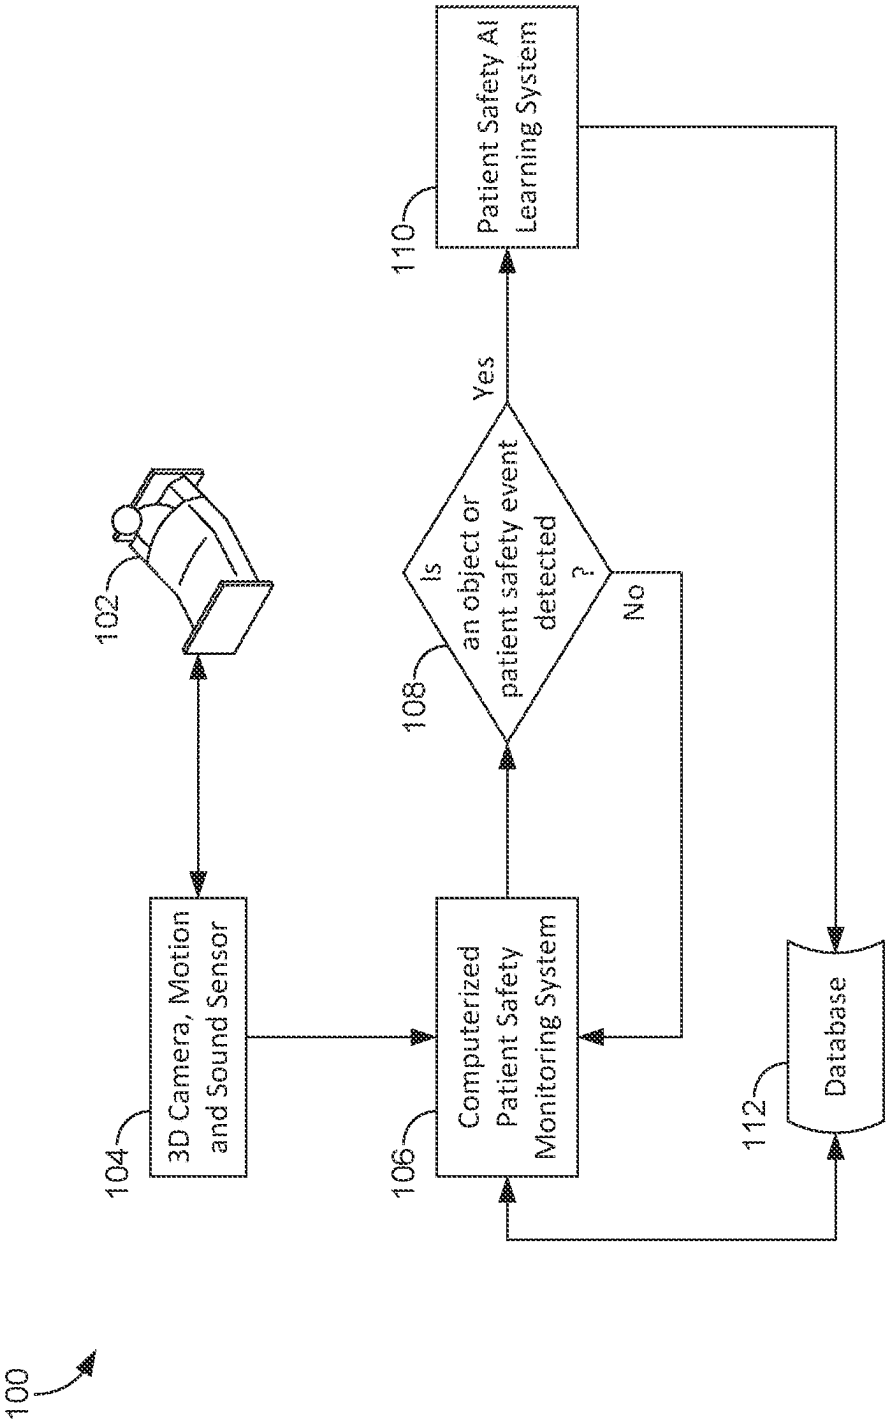


FIG. 1

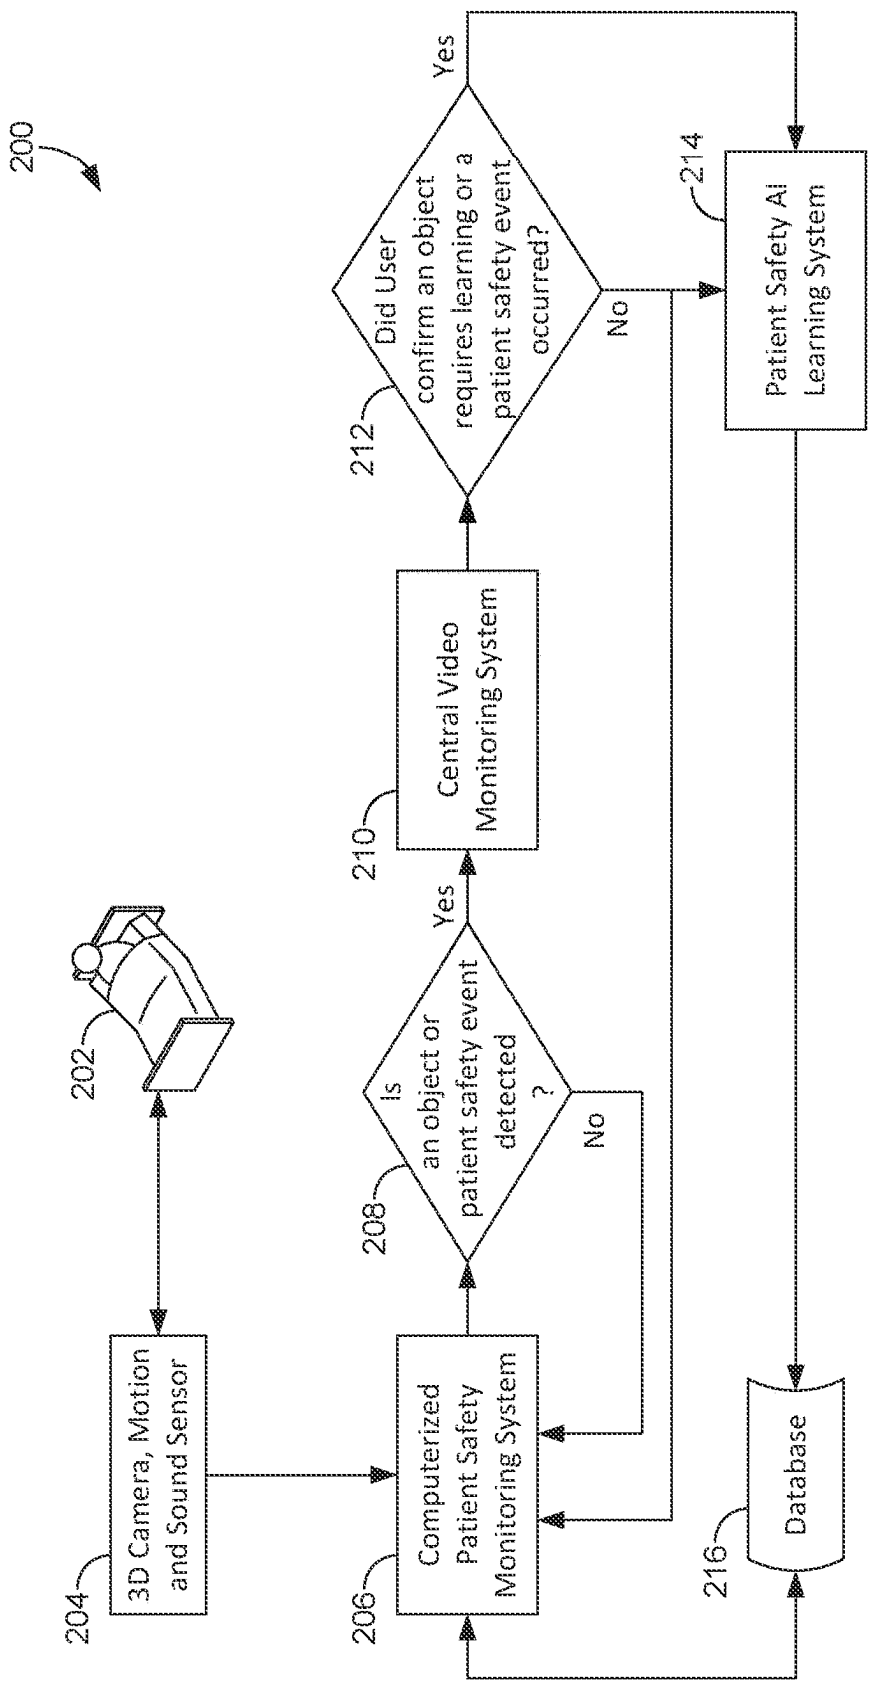


FIG. 2



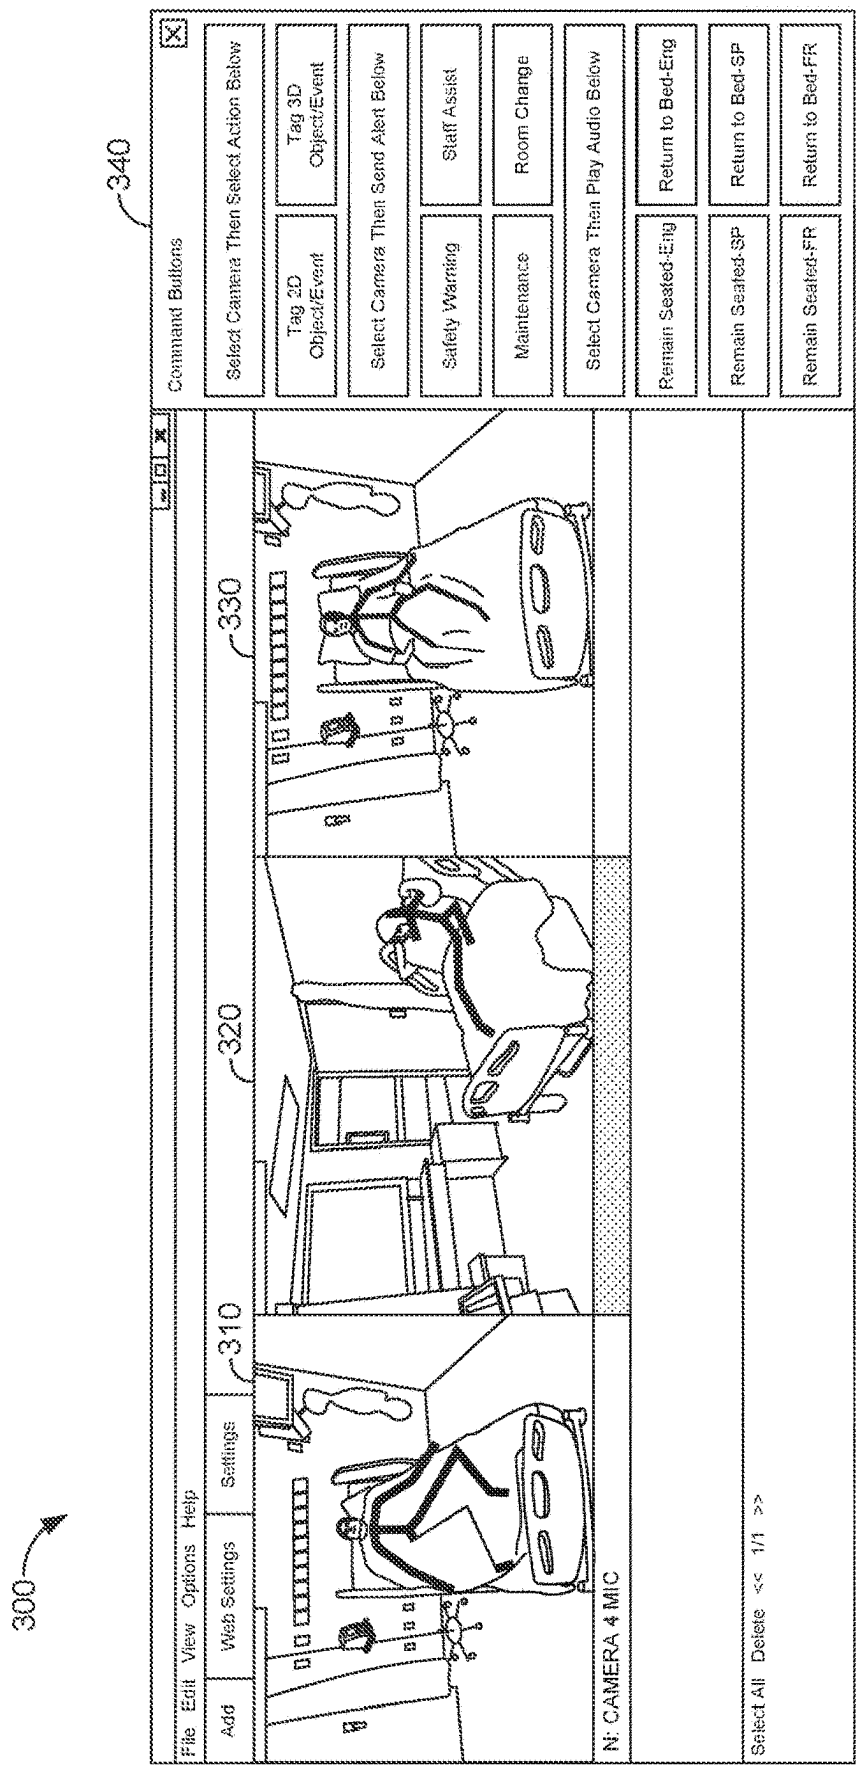


FIG. 3

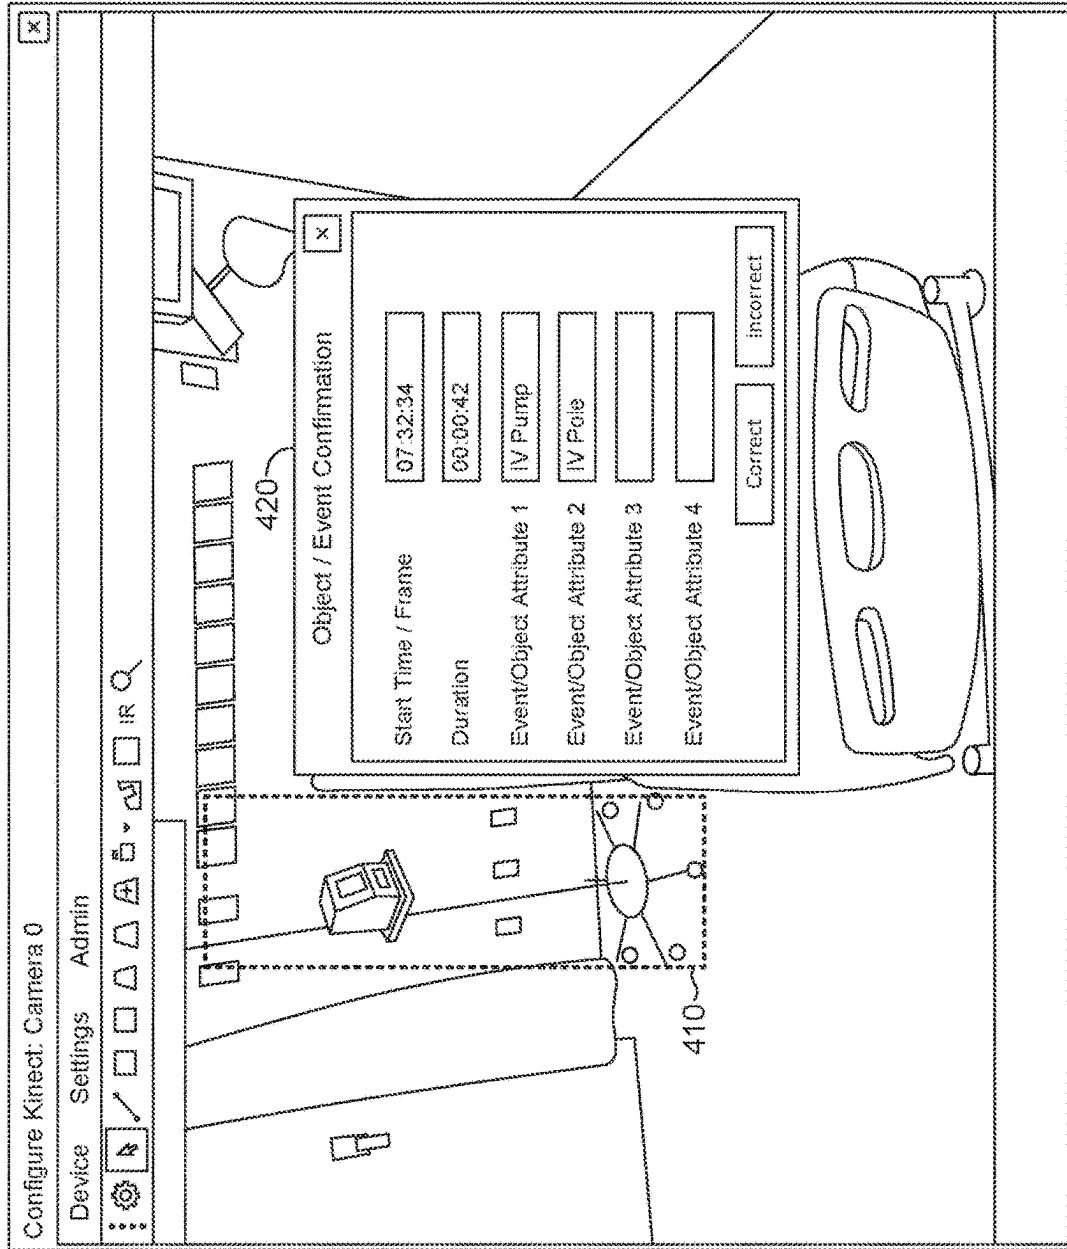


FIG. 4

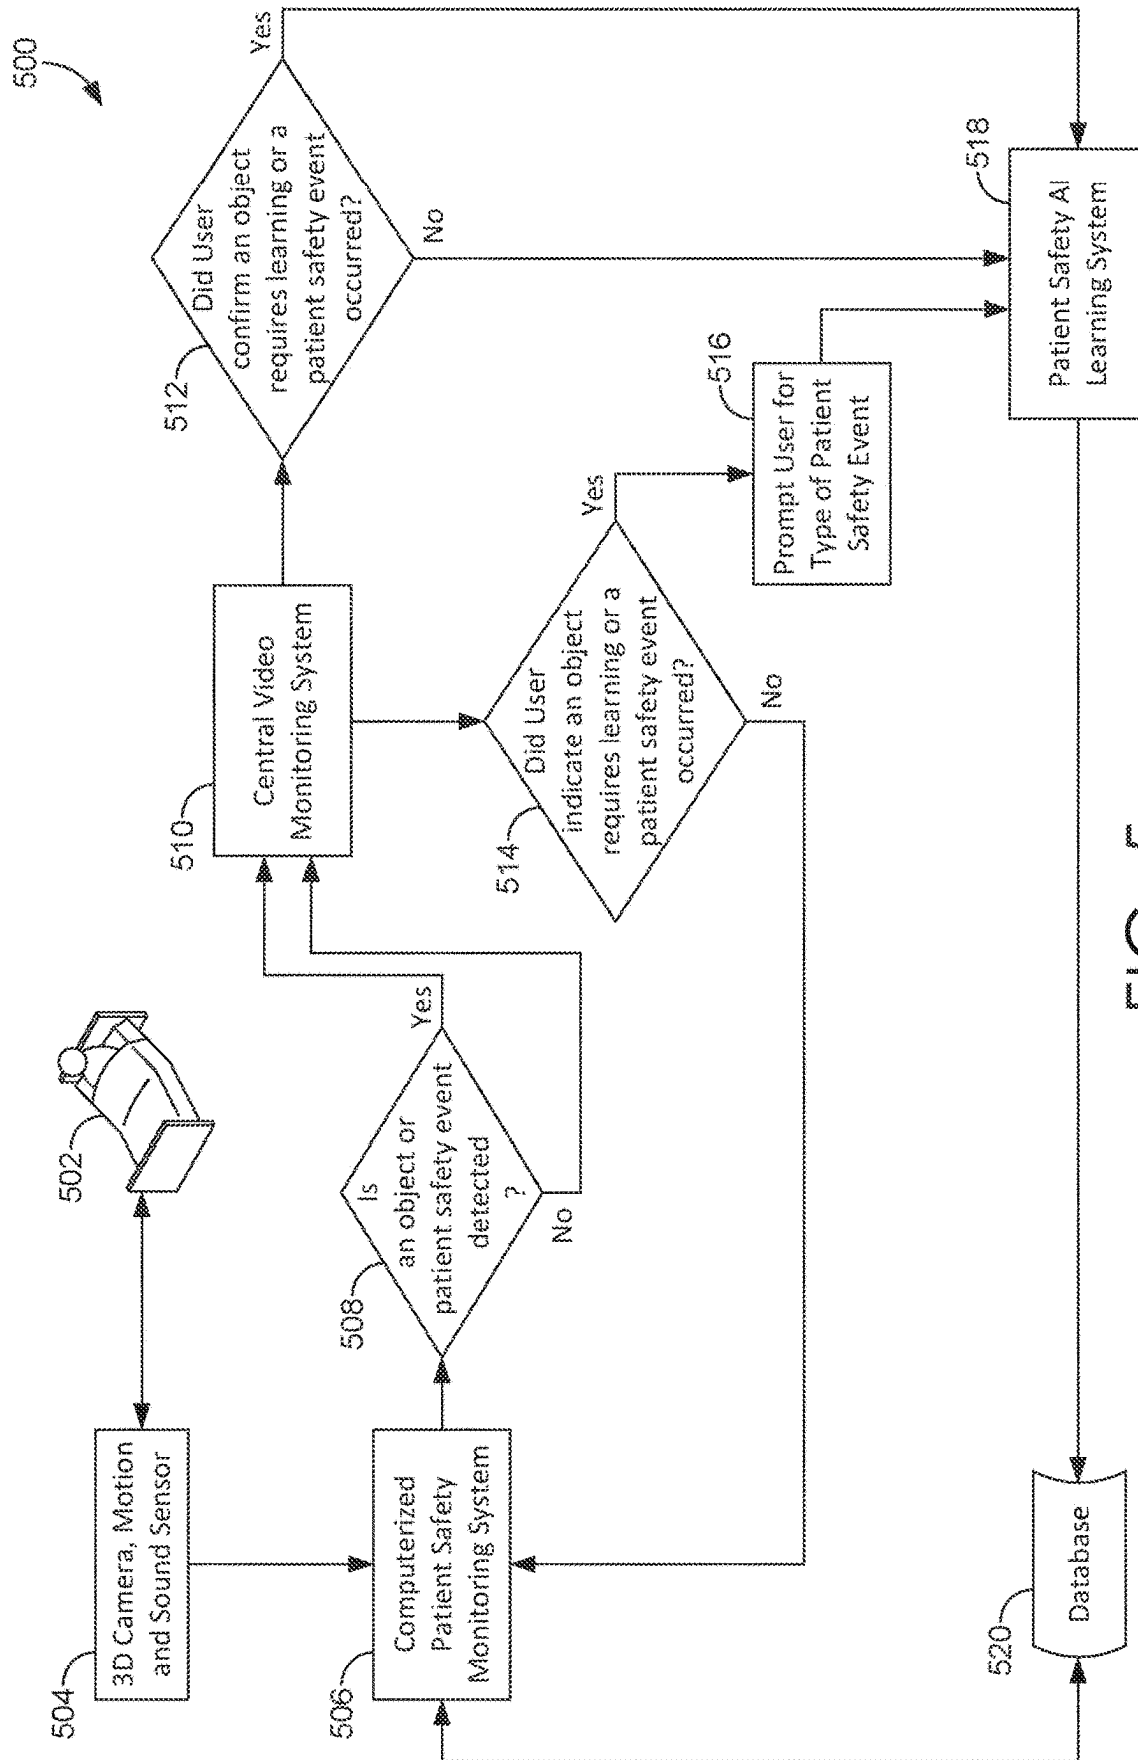


FIG. 5

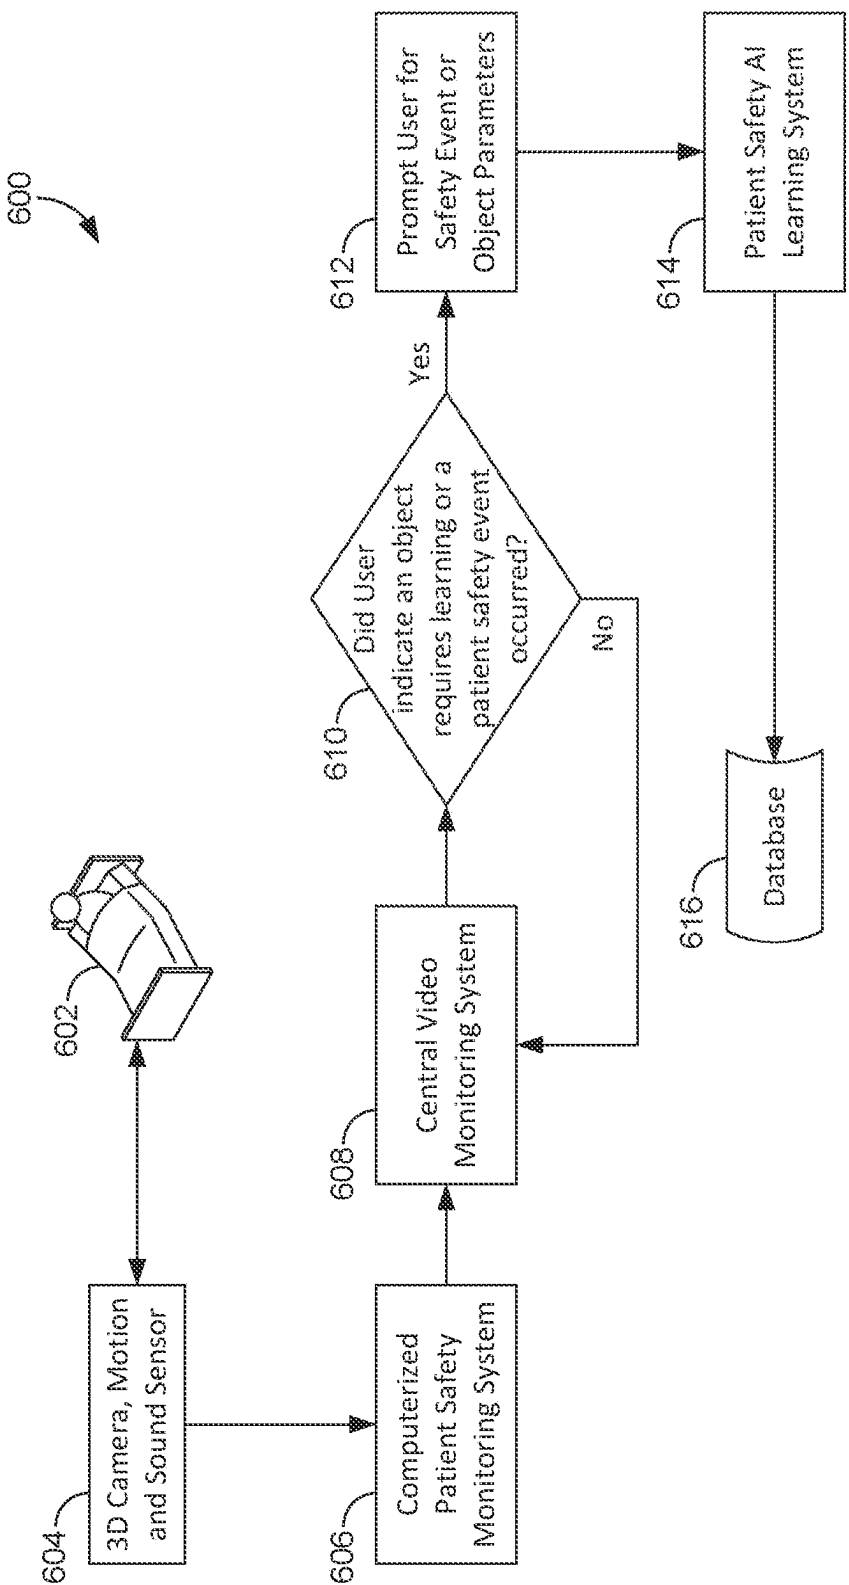


FIG. 6

1

# UTILIZING ARTIFICIAL INTELLIGENCE TO DETECT OBJECTS OR PATIENT SAFETY EVENTS IN A PATIENT ROOM

## CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 18/314,502, filed May 9, 2023, which is a continuation of U.S. patent application Ser. No. 17/646,942, filed Jan. 4, 2022, now U.S. Pat. No. 11,721,190, issued Aug. 8, 2023, which is a continuation of U.S. patent application Ser. No. 17/117,414, filed Dec. 10, 2020, now U.S. Pat. No. 11,276,291, issued Mar. 15, 2022, which is a continuation of U.S. patent application Ser. No. 16/832,790, filed Mar. 27, 2020, now U.S. Pat. No. 10,922,946, issued Feb. 16, 2021, which is a continuation of U.S. patent application Ser. No. 15/856,419, filed Dec. 28, 2017, now U.S. Pat. No. 10,643,446, issued May 5, 2020, the entire disclosures of which are incorporated by reference, for all purposes, as if fully set forth herein.

## BACKGROUND

Medical facilities, such as hospitals, face many challenges in addition to simply caring for patients. For example, securing patients and preventing safety events (e.g., stroke, seizure, getting out of bed, etc.) from occurring consumes many resources and current methods lack effectiveness. Although some medical facilities utilize cameras and/or sensors to monitor patients, current systems require subjective decision-making and are prone to error by the personnel monitoring the data received from the cameras and/or sensors. Additionally, in some situations, a patient may obtain an object the particular patient is not allowed (e.g., a gift from a visitor that might present health or safety risks to the patient) that the current methods are unable to automatically detect. Accordingly, overall security for patients and equipment suffers and the many resources currently being utilized are wasted.

## BRIEF SUMMARY

This brief summary is provided as a general overview of the more detailed disclosure which follows. It is not intended to identify key or essential elements of the disclosure, or to define the claim terms in isolation from the remainder of the disclosure, including the drawings.

This disclosure generally relates to methods and systems for detecting objects or patient safety events in a patient room. More particularly, artificial intelligence or machine learning is utilized to enhance safety issue recognition capabilities by the methods and systems. Generally, and without limitation, the sensors collect a series of images and depth data in a room of a patient. Data (corresponding to images and depth data of an object or patient safety event) is received from the sensors and compared to stored data to identify an object or patient safety event. The images of the object or patient safety event are communicated to a central video monitoring system and a user may be prompted to confirm if the object requires learning or a patient safety event occurred (or to identify the object or patient safety event so a patient safety learning system learns continuously). In some embodiments, the user may change the identification that the system originally produced if it is incorrect to further train the patient safety learning system. The patient safety learning system analyzes the data and

2

incorporates the user response to enhance safety issue recognition capabilities of the system and reduce false alerts.

In some aspects, this disclosure relates to a system for utilizing artificial intelligence to detect objects or patient safety events in a patient room. The system comprises: one or more motion sensors located to collect a series of images of a room of a patient; a computerized patient safety monitoring system communicatively coupled to the one or more motion sensors, the computerized monitoring system receiving data from the one or more motion sensors and comparing the data to stored data in a database to identify an object or patient safety event; and a central video monitoring system that receives images of the object or patient safety event from the computerized patient safety monitoring system and prompts a user to confirm the object requires learning or the patient safety event occurred; and a patient safety learning system that analyzes the data and incorporates whether the object requires learning or the patient safety event occurred to enhance safety issue recognition capabilities of the system and reduce false alerts.

In some aspects this disclosure relates to computer-readable storage media having embodied thereon computer-executable instructions. When executed by one or more computer processors, the instructions may cause the processors to: utilize one or more motion sensors to collect a series of images of a room of a patient; receive data from the one or more motion sensors at a computerized patient safety monitoring system, the computerized patient safety monitoring system communicatively coupled to the one or more motion sensors; compare the data to stored data in a database to identify an object or patient safety event; communicate, to a central video monitoring system, images of the object or patient safety event from the computerized patient safety monitoring system; and analyze, by a patient safety learning system, the data to enhance safety issue recognition capabilities of the system and reduce false alerts.

In some aspects, this disclosure relates to a method for utilizing artificial intelligence to detect objects or patient safety events in a patient room. The method comprises: utilizing one or more motion sensors to collect a series of images of a room of a patient; receiving data from the one or more motion sensors at a computerized patient safety monitoring system, the computerized patient safety monitoring system communicatively coupled to the one or more motion sensors; comparing the data to stored data in a database to identify an object or patient safety event; receiving, by a central video monitoring system, images of the object or patient safety event from the computerized patient safety monitoring system; prompting, at the central video monitoring system, a user to identify the object that requires learning or identify the patient safety event that occurred and to add additional parameters to the object or patient safety event; and analyzing, by a patient safety learning system, the data and incorporating the identification of the object that requires learning or the identification of the patient safety event that occurred to enhance safety issue recognition capabilities of the system and reduce false alerts.

Additional objects, advantages, and novel features of the disclosure will be set forth in part in the description which follows, and in part will become apparent to those skilled in the art upon examination of the following, or may be learned by practice of the disclosure.

## BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING

The description references the attached drawing figures, wherein:

3

FIG. 1 is an exemplary flowchart for an automated learning process to detect objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure;

FIG. 2 is an exemplary flowchart for a semi-automated learning process to detect objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure;

FIG. 3 is an exemplary display for object or patient safety event detection in a patient room, in accordance with embodiments of the present disclosure;

FIG. 4 is an exemplary display for object or patient safety event confirmation in a patient room, in accordance with embodiments of the present disclosure;

FIG. 5 is an exemplary flowchart for a semi-automated learning process to detect objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure; and

FIG. 6 is an exemplary flowchart for a manually initiated learning process to detect objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure.

#### DETAILED DESCRIPTION

As noted in the Background, medical facilities, such as hospitals, face many challenges in addition to simply caring for patients. For example, securing patients and preventing safety events (e.g., stroke, seizure, getting out of bed, etc.) from occurring consumes many resources and current methods lack effectiveness. Although some medical facilities utilize cameras and/or sensors to monitor patients, current systems require subjective decision-making and are prone to error by the personnel monitoring the data received from the cameras and/or sensors. Additionally, in some situations, a patient may obtain an object the particular patient is not allowed (e.g., a gift from a visitor that might present health or safety risks to the patient) that the current methods are unable to automatically detect. Accordingly, overall security for patients and equipment suffers and the many resources currently being utilized are wasted.

The subject matter of the present invention is described with specificity herein to meet statutory requirements. However, the description itself is not intended to limit the scope of this patent. Rather, the inventor has contemplated that the claimed subject matter might also be embodied in other ways, to include different steps or combinations of steps similar to the ones described in this document, in conjunction with other present or future technologies. Moreover, although the terms “step” and/or “block” may be used herein to connote different elements of methods employed, the terms should not be interpreted as implying any particular order among or between various steps herein disclosed unless and except when the order of individual steps is explicitly described.

Referring initially to FIG. 1, an automated learning process detects objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure. As shown in FIG. 1, a system 100 for utilizing artificial intelligence to detect objects or patient safety events in a patient room may include one or more 3D motion sensors 104. Although described as 3D motion sensors, it is contemplated that aspects of the present invention may be accomplished using 2D motion sensors rather than 3D motion sensors. A 3D motion sensor is an electronic device that contains one or more cameras capable of identifying individual objects, people and motion. The 3D motion

4

sensor may further contain one or more microphones to detect audio. The cameras can utilize technologies including but not limited to color RGB, CMOS sensors, lasers, infrared projectors and RF-modulated light. The 3D motion sensor may have one or more integrated microprocessors and/or image sensors to detect and process information both transmitted from and received by the various cameras. Exemplary 3D motion sensors include the Microsoft® Kinect® Camera, the Sony® PlayStation® Camera, the Intel® RealSense™ Camera, the Orbbec® Persee®, the Orbbec® Astra®, and the Asus® Ztion, each of which happens to include microphones, although sound capture is not essential to the practice of the disclosure. A user may be able to configure alerts based on data that is received from the 3D motion sensor 204 and interpreted by the computerized patient monitoring system 106. For example, a user can configure the computerized patient monitoring system 106 to provide alerts based on data the computerized patient monitoring system 106 has interpreted to detect objects or patient safety events.

As used herein, “a sensor” and “sensors” are used interchangeably in the singular and plural unless expressly described as a singular sensor or an array of sensors. A singular sensor may be used, or a sensor may comprise two or more cameras integrated into a single physical unit. Alternately, two or more physically distinct sensors may be used, or two or more physically distinct arrays of sensors may be used.

An “object” may be any object in the room of a patient being monitored that presents safety or medical issues to the patient. For example, the object may be a gift the patient received that heightens the risk for aggravating a condition that patient is being treated for. The “object” may also be medical equipment or devices in the room of the patient being monitored. For example, the object may be an infusion pump or a pole that supports the infusion pump and bag. The object may also include contraband, such as weapons or drugs.

A “patient safety event” may be any action (e.g., getting out of bed), activity, condition, symptom, or inferred diagnosis (e.g., stroke or seizure) that presents safety or medical issues to the patient.

As shown in FIG. 1, the system 100 may be utilized to collect a series of images in the room of a patient 102. For example, 3D motion sensor 104 may detect an object (e.g., medication, food, beverage, drug paraphernalia, tobacco products, and the like) in the room of the patient. Additionally, or alternatively, 3D motion sensor 104 may detect a patient safety event (e.g., the patient getting out of bed). Computerized patient safety monitoring system 106 is communicatively coupled to the 3D motion sensor 104 and receives data (i.e., the series of images relevant to the object or patient safety issue) from the 3D motion sensor 104. Features of the object or patient safety event may be analyzed by computerized patient safety monitoring system 106 and compared to stored data in a database 112 to identify known issues, patterns, and the like that can be used to detect an object or patient safety event.

If the object requires learning or the patient safety event occurred, as shown at 108, the data is communicated to a patient safety learning system 110. The patient safety learning system 110 analyzes the data (i.e., the video and depth data captured by the sensor 104) and stores new or modified issues, patterns, and the like that can be used to detect an object or patient safety event in database 112. This automated learning process enhances the safety issue recognition capabilities of the system and reduces false alerts. If, on the

5

other hand, no object or patient safety event is detected, no further action is taken and the computerized patient safety monitoring system **106** continues to wait for data received by the 3D sensor **104**.

In embodiments, the 3D motion sensor **104** may be co-located with a patient **102** to be monitored. The patient **102** to be monitored may be monitored in a variety of environments, including, without limitation, a hospital, a home, a hospice care facility, a nursing home, an assisted living facility, an outpatient medical care facility, and the like. The 3D motion sensor **104** may be positioned where it is likely to capture images of the face of the patient **102** to be monitored. For example, a 3D motion sensor **104** may be oriented to take images of a bed, chair, or other location where the patient **102** to be monitored may spend a significant amount of time. In some embodiments, the 3D motion sensor **104** may be oriented to take images of persons and/or objects entering and exiting the room of the patient **102** to be monitored. In some embodiments, the 3D motion sensor **104** may be oriented to take images of items or equipment (e.g., medical devices) that may be located in the room of the patient **102** to be monitored. The 3D motion sensor **104** may be permanently installed, or may be temporarily set up in a room as needed. The patient **102** to be monitored may be under immediate medical care, e.g., in a medical facility under the supervision of a medical professional, or may not be under immediate care, e.g., in a home or other environment, possibly with a caregiver. A caregiver may be a medical professional or paraprofessional, such as an orderly, nurse's aide, nurse, or the like. A caregiver may also be a friend, relative, individual, company, or facility that provides assistance with daily living activities and/or medical care for individuals, such as individuals who are disabled, ill, injured, elderly, or otherwise in need of temporary or long-term assistance. In some instances, the person to be monitored may be self-sufficient and not under the immediate care of any other person or service provider.

The 3D motion sensor **104** may communicate data (i.e., the video and depth data captured by the sensor **104**), such as images of the patient **102** being monitored or an object detected in the room, to a computerized patient safety monitoring system **106**. The computerized patient safety monitoring system **106** is a computer programmed to monitor transmissions of data from the 3D motion sensor **104**. The computerized patient safety monitoring system **106** may be integral to the 3D motion sensor **104** or a distinctly separate apparatus from the 3D motion sensor **104**, possibly in a remote location from 3D motion sensor **104** provided that the computerized patient safety monitoring system **106** can receive data from the 3D motion sensor **104**. The computerized patient safety monitoring system **106** may be located in the monitored person's room, such as a hospital room, bedroom, or living room. The computerized patient safety monitoring system **106** may be connected to a central video monitoring system (e.g., central video monitoring system **210** described below with respect to FIG. 2). The computerized patient safety monitoring system **106** and central video monitoring system may be remotely located at any physical locations so long as a data connection exists (USB, TCP/IP or comparable) between the computerized patient safety monitoring system **106**, the central video monitoring system, and the 3D motion sensor(s) **104**.

The computerized patient safety monitoring system **106** may receive data from 3D motion sensor **104** for a monitoring zone (i.e., the patient's room or area to be monitored). Computerized patient monitoring and object recognition system **106** may assign reference points to distinctive fea-

6

tures of a person or object. It should be understood that the selection of the reference points may vary with the individual and/or the configuration of the monitoring system **100**. Reference points may be configured automatically by the monitoring system **100**, may be configured automatically by the monitoring system **100** subject to confirmation and/or modification by a system user, or may be configured manually by a system user. The reference points corresponding to the object may be compared to a database comprising reference points of known or acceptable objects or patient safety events. As described below, various machine learning and/or object recognition techniques may additionally be utilized by patient safety learning system **110** to recognize the object or patient safety event.

As shown in FIG. 2, a semi-automated learning process detects objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure. The system **200** may be utilized to collect a series of images and depth data in the room of a patient **202**. For example, 3D motion sensor **204** may detect an object (e.g., medication, food, beverage, drug paraphernalia, tobacco products, and the like) in the room of the patient. Additionally, or alternatively, 3D motion sensor **204** may detect a patient safety event (e.g., the patient getting out of bed). Computerized patient safety monitoring system **206** is communicatively coupled to the 3D motion sensor **204** and receives data (i.e., the series of images relevant to the object or patient safety issue) from the 3D motion sensor **204**. Features of the object or patient safety event may be analyzed by computerized patient safety monitoring system **206** and compared to stored data in a database **216** to identify known issues, patterns, and the like that can be used to detect an object or patient safety event.

When an object or patient safety event is detected, images of the object or patient safety event are communicated, as shown at **208**, by the computerized patient safety monitoring system **206** to the central video monitoring system **210**. At the central video monitoring system **210**, a user is prompted, as shown at step **212**, to confirm the object requires learning (if not already known by the system **200**) or to confirm the patient safety event occurred. This process can occur in real-time or any time in the future. For example, the detected object or patient safety event's video and depth data may be recorded and displayed for a user at the central video monitoring system to be played back so the user can provide additional information or confirmation at any time. If the object requires learning or the patient safety event occurred, the data is communicated to a patient safety learning system **214**. The patient safety learning system **214** incorporates the response by the user so the object or patient safety event can be learned and stored in database **216**. This semi-automated learning process enhances the safety issue recognition capabilities of the system and reduces false alerts. If, on the other hand, the object does not require learning or the patient safety event did not occur, no further action is taken and the computerized patient safety monitoring system **206** continues to wait for data received by the 3D sensor **204**.

The 3D motion sensor **204** may communicate data, such as images of the patient **202** being monitored (e.g., via skeletal tracking or blob recognition) or an object detected in the room, to a computerized patient monitoring system **206**. The computerized patient monitoring system **206** is a computer programmed to monitor transmissions of data from the 3D motion sensor **204**. The computerized patient monitoring system **206** may be integral to the 3D motion sensor **204** or a distinctly separate apparatus from the 3D motion sensor **204**, possibly in a remote location from 3D

motion sensor **204** provided that the computerized patient monitoring system **206** can receive data from the 3D motion sensor **204**. The computerized patient monitoring system **206** may be located in the monitored person's room, such as a hospital room, bedroom, or living room. The computerized patient monitoring system **206** may be connected to a central video monitoring system **210**. The computerized patient monitoring system **206** and central video monitoring system **210** may be remotely located at any physical locations so long as a data connection exists (USB, TCP/IP or comparable) between the computerized patient monitoring system **206**, the central video monitoring system **210**, and the 3D motion sensor(s) **204**.

Computerized patient monitoring system **206** may assign reference points to identify the boundaries of an area to be monitored. For example, reference points may be assigned to a perimeter around the patient. It should be understood that the selection of the reference points may vary with the individual and/or the configuration of the monitoring system **200**. Reference points may be configured automatically by the system **200**, may be configured automatically by the system **200** subject to confirmation and/or modification by a system user, or may be configured manually by a system user.

Data associated with objects or patient safety events may be logged by computerized patient monitoring system **206** and/or central video monitoring system **210** in a database **216**. Data associated with the objects or patient safety events may include, without limitation, the telemetry data from 3D motion sensor **204** that triggered the object or patient safety event; buffered data preceding the telemetry data that triggered the object or patient safety event; telemetry data subsequent to the object or patient safety event; the number and substantive content of object or patient safety event; the individual(s) and/or groups to whom the object or patient safety event was addressed; the response, if any, received or observed following the object or patient safety event; and combinations thereof. In some embodiments, data associated with the object or patient safety event may include the video and/or pictures of the object or patient safety event.

FIG. 3 shows an exemplary view for central video monitoring system **300**, in accordance with embodiments of the present disclosure. More particularly, the central video monitoring system **300** displays patient safety event detection in a patient room. The view includes skeletal figures, which may be identified by central video monitoring system, and used to track or "lock on to" a patient. Although skeletal figures are shown in FIG. 3, alternate image analysis could be used, including, without limitation, blob recognition, bounding boxes, person masks, and facial recognition or object recognition. As illustrated, a user may be watching live or recorded video **310**, **320**, **330**. If the user sees an object or event that the user wants the system to learn, the user can select the appropriate button (e.g., Tag 2D Object/Event or Tag 3D Object/Event) to indicate to the system that the user wants to store the video immediately before and after the time the user hit the button to send to the patient safety learning system. The patient safety learning system is capable of buffering video and depth data for the user to enable this process. The user is additionally provided an opportunity to include additional information parameters about the object or safety event, as shown in FIG. 4, described below.

FIG. 4 shows an exemplary view for central video monitoring system **400**, in accordance with embodiments of the present disclosure. More particularly, the central video monitoring system **400** displays object detection in a patient

room (although illustrated in FIG. 4 and described with respect to object detection, the same process is used for patient safety events). As illustrated, an object **410** has been detected or identified by a user. Upon selecting the object **410**, a user can add additional parameters **420** corresponding to the object **410**. The objects and additional parameters are communicated to a patient safety learning system to enhance safety issue recognition capabilities of the system and reduce false alerts.

In FIG. 5, a semi-automated learning process detects objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure. The system **500** may be utilized to collect a series of images and depth data in the room of a patient **502**. For example, 3D motion sensor **504** may detect an object (e.g., medication, food, beverage, drug paraphernalia, tobacco products, and the like) in the room of the patient. Additionally, or alternatively, 3D motion sensor **504** may detect a patient safety event (e.g., the patient getting out of bed). Computerized patient safety monitoring system **506** is communicatively coupled to the 3D motion sensor **504** and receives data (i.e., the series of images relevant to the object or patient safety issue) from the 3D motion sensor **504**. Features of the object or patient safety event may be analyzed by computerized patient safety monitoring system **506** and compared to stored data in a database **520** to identify known issues, patterns, and the like that can be used to detect an object or patient safety event.

As shown at step **508**, images from the computerized patient safety monitoring system **506** are communicated for display on the central video monitoring system **510** regardless of whether an object or patient safety event is detected. However, when an object or patient safety event is detected, a user is prompted, as shown at step **512**, to confirm the object requires learning (if not already known by the system **500**) or to confirm the patient safety event occurred. Either way, the data is communicated to a patient safety learning system **518**. The patient safety learning system **518** incorporates the response by the user so the object or patient safety event can be learned and stored in database **520**. This semi-automated learning process enhances the safety issue recognition capabilities of the system and reduces false alerts. If, on the other hand, the object does not require learning or the patient safety event did not occur, no further action is taken and the computerized patient safety monitoring system **506** continues to wait for data received by the 3D sensor **504**.

Additionally, or alternatively, if the system does not detect an object or patient safety event, the user may indicate, as shown at step **514**, that an object requires learning (if not already known by the system **500**) or that a patient safety event occurred. If the user indicates that an object requires learning or that a patient safety event occurred, the user may be prompted, as shown at step **516**, to indicate parameters of the object or the type of patient safety event. This information, along with the data (which may include a recording prior (using data buffering), during, and after the object or patient safety event was detected), is communicated to a patient safety learning system **518**. The patient safety learning system **518** incorporates the parameters or type of event indicated by the user with the data so the object or patient safety event can be learned and stored in database **520**. This semi-automated learning process enhances the safety issue recognition capabilities of the system and reduces false alerts. If, on the other hand, the user indicates that the object does not require learning or the patient safety event did not occur, no further action is taken and the computerized



patient safety monitoring system 506 continues to wait for data received by the 3D sensor 504.

Referring now to FIG. 6, a manually initiated learning process detects objects or patient safety events in a patient room, in accordance with embodiments of the present disclosure. In FIG. 6, the system 600 may be utilized to collect a series of images and depth data in the room of a patient 602. For example, 3D motion sensor 604 may collect images of an object (e.g., medication, food, beverage, drug paraphernalia, tobacco products, and the like) in the room of the patient. Additionally, or alternatively, 3D motion sensor 604 may collect images of a patient safety event (e.g., the patient getting out of bed). Computerized patient safety monitoring system 606 is communicatively coupled to the 3D motion sensor 604 and receives data (i.e., the series of images relevant to the object or patient safety issue) from the 3D motion sensor 604. A constant stream of images is communicated by computerized patient safety monitoring system 606 for display on the central video monitoring system 610.

As shown at step 608, images from the computerized patient safety monitoring system 606 are communicated for display on the central video monitoring system 610. As shown at step 610, to indicate an object requires learning or to indicate a patient safety event occurred. If the user indicates that an object requires learning or that a patient safety event occurred, the user may be prompted, as shown at step 612, to indicate parameters of the object or the type of patient safety event. This information, along with the data (which may include a recording prior (using data buffering), during, and after the object or patient safety event was detected), is communicated to a patient safety learning system 614. The patient safety learning system 614 incorporates the parameters or type of event indicated by the user with the data so the object or patient safety event can be learned and stored in database 616. This semi-automated learning process enhances the safety issue recognition capabilities of the system and reduces false alerts. If, on the other hand, the user does not indicate that an object requires learning or that a patient safety event occurred, no further action is taken and the central video monitoring system 608 continues to display data received by the computerized patient safety monitoring system 606.

As noted, the patient safety learning system may utilize one or more machine learning algorithms to determine if an object or patient safety event is detected. For example, an ensemble of alternating decision trees can be used to determine if an object or patient safety event is detected. Each decision tree may be trained on a random subset of objects and patient safety events. In some embodiments, the number of decision trees used is based on the type of healthcare data received or specific information pertaining to the patient.

A generic decision tree is a decision support tool which arrives at a decision after following steps or rules along a tree-like path. While most decision trees are only concerned about the final destination along the decision path, alternating decision trees take into account every decision made along the path and may assign a score for every decision encountered. Once the decision path ends, the algorithm sum all of the incurred scores to determine a final classification (i.e., information that should be grouped and displayed together). In some embodiments, the alternating decision tree algorithm may be further customized. For example, the alternating decision tree algorithm may be modified by wrapping it in other algorithms.

A machine learning algorithm may use a generic cost matrix. The intuition behind the cost matrix is as follows. If the model predicts a member to be classified in group A, and

the member really should be in group A, no penalty is assigned. However, if this same member is predicted to be in group B, C, or D, a 1-point penalty will be assigned to the model for this misclassification, regardless of which group the member was predicted to be in. Thus, all misclassifications are penalized equally. However, by adjusting the cost matrix, penalties for specific misclassifications can be assigned. For example, where someone who was truly in group D was classified in group A, the model could increase the penalty in that section of the cost matrix. A cost matrix such as this may be adjusted as needed to help fine tune the model for different iterations, and may be based on the specific patient in some embodiments.

With regards to a multi-class classifier, some machine learning algorithms, such as alternating decision trees, generally only allow for the classification into two categories (e.g. a binary classification). In cases where it is desired to classify three or more categories, a multi-class classifier is used.

In order to assist the alternating decision tree in selecting best features for predictive modeling, an ensemble method called rotation forest may be used. The rotation forest algorithm randomly splits the dataset into a specified number of subsets and uses a clustering method called Principal Component Analysis to group features deemed useful. Each tree is then gathered (i.e., “bundled into a forest”) and evaluated to determine the features to be used by the base classifier.

Various alternative classifiers may be used to provide the medical and preventive healthcare personal assistant services. Indeed, there are thousands of machine learning algorithms, which could be used in place of, or in conjunction with, the alternating decision tree algorithm. For example, one set of alternative classifiers comprise ensemble methods.

Ensemble methods use multiple, and usually random, variations of learning algorithms to strengthen classification performance. Two of the most common ensemble methods are bagging and boosting. Bagging methods, short for “bootstrap aggregating” methods, develop multiple models from random subsets of features from the data (“bootstrapping”), assigns equal weight to each feature, and selects the best-performing attributes for the base classifier using the aggregated results. Boosting, on the other hand, learns from the data by incrementally building a model, thereby attempting to correct misclassifications from previous boosting iterations.

Regression models are frequently used to evaluate the relationship between different features in supervised learning, especially when trying to predict a value rather than a classification. However, regression methods are also used with other methods to develop regression trees. Some algorithms combine both classification and regression methods; algorithms that used both methods are often referred to as CART (Classification and Regression Trees) algorithms.

Bayesian statistical methods are used when the probability of some events happening are, in part, conditional to other circumstances occurring. When the exact probability of such events is not known, maximum likelihood methods are used to estimate the probability distributions. A textbook example of Bayesian learning is using weather conditions, and whether a sprinkler system has recently gone off, to determine whether a lawn will be wet. However, whether a homeowner will turn on their sprinkler system is influenced, in part, to the weather. Bayesian learning methods, then, build predictive models based on calculated prior probability distributions.

Another type of classifiers comprise artificial neural networks. While typical machine learning algorithms have a pre-determined starting node and organized decision paths, the structure of artificial neural networks are less structured. These algorithms of interconnected nodes are inspired by the neural paths of the brain. In particular, neural network methods are very effective in solving difficult machine learning tasks. Much of the computation occurs in “hidden” layers.

By way of example and not limitation, other classifiers and methods that may be utilized include (1) decision tree classifiers, such as: C4.5—a decision tree that first selects features by evaluating how relevant each attribute is, then using these attributes in the decision path development; Decision Stump—a decision tree that classifies two categories based on a single feature (think of a single swing of an axe); by itself, the decision stump is not very useful, but becomes more so paired with ensemble methods; LADTree—a multi-class alternating decision tree using a LogitBoost ensemble method; Logistic Model Tree (LMT)—a decision tree with logistic regression functions at the leaves; Naive Bayes Tree (NBTree)—a decision tree with naive Bayes classifiers at the leaves; Random Tree—a decision tree that considers a pre-determined number of randomly chosen attributes at each node of the decision tree; Random Forest—an ensemble of Random Trees; and Reduced-Error Pruning Tree (REPTree)—a fast decision tree learning that builds trees based on information gain, then prunes the tree using reduce-error pruning methods; (2) ensemble methods such as: AdaBoostM1—an adaptive boosting method; Bagging—develops models using bootstrapped random samples, then aggregates the results and votes for the most meaningful features to use in the base classifier; LogitBoost—a boosting method that uses additive logistic regression to develop the ensemble; MultiBoostAB—an advancement of the AdaBoost method; and Stacking—a method similar to boosting for evaluating several models at the same time; (3) regression methods, such as Logistic Regression—regression method for predicting classification; (4) Bayesian networks, such as BayesNet—Bayesian classification; and Naive-Bayes—Bayesian classification with strong independence assumptions; and (4) artificial neural networks such as MultiLayerPerception—a forward-based artificial neural network.

The various computerized systems and processors as described herein may include, individually or collectively, and without limitation, a processing unit, internal system memory, and a suitable system bus for coupling various system components, including database 118, with a control server. Computerized patient monitoring system 106 and/or central video monitoring system 116 may provide control server structure and/or function. The system bus may be any of several types of bus structures, including a memory bus or memory controller, a peripheral bus, and a local bus, using any of a variety of bus architectures. By way of example, and not limitation, such architectures include Industry Standard Architecture (ISA) bus, Micro Channel Architecture (MCA) bus, Enhanced ISA (EISA) bus, Video Electronic Standards Association (VESA) local bus, and Peripheral Component Interconnect (PCI) bus.

The computerized systems typically include therein, or have access to, a variety of computer-readable media, for instance, database 118. Computer-readable media can be any available media that may be accessed by the computerized system, and includes volatile and nonvolatile media, as well as removable and non-removable media. By way of example, and not limitation, computer-readable media may

include computer-storage media and communication media. Computer-readable storage media may include, without limitation, volatile and nonvolatile media, as well as removable and non-removable media implemented in any method or technology for storage of information, such as computer readable instructions, data structures, program modules, or other data. In this regard, computer-storage media may include, but is not limited to, RAM, ROM, EEPROM, flash memory or other memory technology, CD-ROM, digital versatile disks (DVDs) or other optical disk storage, magnetic cassettes, magnetic tape, magnetic disk storage, or other magnetic storage device, or any other medium which can be used to store the desired information and which may be accessed by the control server. Computer-readable storage media excludes signals per se.

Communication media typically embodies computer readable instructions, data structures, program modules, or other data in a modulated data signal, such as a carrier wave or other transport mechanism, and may include any information delivery media. As used herein, the term “modulated data signal” refers to a signal that has one or more of its attributes set or changed in such a manner as to encode information in the signal. By way of example, and not limitation, communication media includes wired media such as a wired network or direct-wired connection, and wireless media such as acoustic, RF, infrared, and other wireless media. Combinations of any of the above also may be included within the scope of computer-readable media. The computer-readable storage media discussed above, including database 118, provide storage of computer readable instructions, data structures, program modules, and other data for the computerized systems. Computer readable instructions embodied on computer-readable storage media may be accessible by prohibited object system 100 and/or component(s) thereof, and, when executed by a computer processor and/or server, may cause the system to function and/or perform the methods described herein.

The computerized systems may operate in a computer network using logical connections to one or more remote computers. Remote computers may be located at a variety of locations, for example, but not limited to, hospitals and other inpatient settings, veterinary environments, ambulatory settings, medical billing and financial offices, hospital administration settings, home health care environments, payer offices (e.g., insurance companies), home health care agencies, clinicians’ offices and the clinician’s home or the patient’s own home or over the Internet. Clinicians may include, but are not limited to, a treating physician or physicians, specialists such as surgeons, radiologists, cardiologists, and oncologists, emergency medical technicians, physicians’ assistants, nurse practitioners, nurses, nurses’ aides, pharmacists, dieticians, microbiologists, laboratory experts, laboratory technologists, genetic counselors, researchers, veterinarians, students, and the like. The remote computers may also be physically located in non-traditional medical care environments so that the entire health care community may be capable of integration on the network. The remote computers may be personal computers, servers, routers, network PCs, peer devices, other common network nodes, or the like, and may include some or all of the elements described above in relation to the control server. The devices can be personal digital assistants or other like devices.

Exemplary computer networks may include, without limitation, local area networks (LANs) and/or wide area networks (WANs). Such networking environments are commonplace in offices, enterprise-wide computer networks,

13

intranets, and the Internet. When utilized in a WAN networking environment, the control server may include a modem or other means for establishing communications over the WAN, such as the Internet. In a networked environment, program modules or portions thereof may be stored in the control server, in the database 118, or on any of the remote computers. For example, and not by way of limitation, various application programs may reside on the memory associated with any one or more of the remote computers. It will be appreciated by those of ordinary skill in the art that the network connections shown are exemplary and other means of establishing a communications link between the computers may be utilized.

In operation, a user may enter commands and information into the computerized system(s) using input devices, such as a keyboard, a pointing device (commonly referred to as a mouse), a trackball, a touch pad, a 3D Gesture recognition camera or motion sensor. Other input devices may include, without limitation, microphones, satellite dishes, scanners, or the like. In addition to or in lieu of a monitor, the computerized systems may include other peripheral output devices, such as speakers and a printer.

Many other internal components of the computerized system hardware are not shown because such components and their interconnection are well known. Accordingly, additional details concerning the internal construction of the computers that make up the computerized systems are not further disclosed herein.

Methods and systems of embodiments of the present disclosure may be implemented in a WINDOWS or LINUX operating system, operating in conjunction with an Internet-based delivery system, however, one of ordinary skill in the art will recognize that the described methods and systems can be implemented in any operating system suitable for supporting the disclosed processing and communications. As contemplated by the language above, the methods and systems of embodiments of the present invention may also be implemented on a stand-alone desktop, personal computer, cellular phone, smart phone, tablet computer, PDA, or any other computing device used in a healthcare environment or any of a number of other locations.

From the foregoing, it will be seen that this disclosure is well adapted to attain all the ends and objects hereinabove set forth together with other advantages which are obvious and which are inherent to the structure.

It will be understood that certain features and subcombinations are of utility and may be employed without reference to other features and subcombinations. This is contemplated by and is within the scope of the claims.

Since many possible embodiments may be made of the invention without departing from the scope thereof, it is to be understood that all matter herein set forth or shown in the accompanying drawings is to be interpreted as illustrative and not in a limiting sense.

The invention claimed is:

1. A method comprising:

collecting images of a scene including an object;  
detecting, based on the images, that an event involving the object has occurred in the scene, wherein the event is detected in-part by comparing one or more features of the object to one or more reference features;  
comparing the object to a database object to determine if the object is associated with a known object in a database, wherein, if the object is not determined to be associated with the known object, the database is updated with reference data associated with the object;

14

in response to detecting that the event has occurred within the scene, presenting at least one of the object and information associated with the event in a graphical user interface;

receiving an indication that the object or the event has been confirmed; and

in response to receiving the indication that the object or event has been confirmed, updating a machine learning model with i) the event, ii) the object, iii) the reference data associated with the object, or iv) combinations of i)-iii), wherein the machine learning model is configured to recognize objects and events occurring in the scene.

2. The method of claim 1, wherein the images are collected by an image capturing device located in the scene.

3. The method of claim 1, wherein the scene includes a medical patient and the event involves a motion of the medical patient.

4. The method of claim 1, wherein the object is a medical device and the event involves a medical patient manipulating the medical device.

5. The method of claim 1, wherein comparing the one or more features of the at least one object to one or more reference features comprises assigning one or more reference points to the one or more features of the at least one object.

6. The method of claim 1, wherein the images are first images and the event is a first event, the method further comprising:

collecting second images of the scene; and

predicting, using the machine learning model, that a second event involving the object has occurred in the scene.

7. The method of claim 6, further comprising:

in response to predicting that the second event has occurred in the scene, providing an alert.

8. A system comprising:

a processing system; and

one or more computer readable storage media storing instructions which, when executed by the processing system, cause the processing system to perform operations comprising:

collecting images of a scene including an object;

detecting, based on the images, that an event involving the object has occurred in the scene, wherein the event is detected in-part by comparing one or more features of the object to one or more reference features;

comparing the object to a database object to determine if the object is associated with a known object in a database, wherein, if the object is not determined to be associated with the known object, the database is updated with reference data associated with the object;

in response to detecting that the event has occurred within the scene, presenting at least one of the object and information associated with the event in a graphical user interface;

receiving an indication that the object or the event has been confirmed; and

in response to receiving the indication that the object or event has been confirmed, updating a machine learning model with i) the event, ii) the object, iii) the reference data associated with the object, or iv) combinations of i)-iii), wherein the machine learning model is configured to recognize objects and events occurring in the scene.

**15**

9. The system of claim 8, wherein the images are collected by an image capturing device located in the scene.

10. The system of claim 8, wherein the scene includes a medical patient and the event involves a motion of the medical patient.

11. The system of claim 8, wherein the object is a medical device and the event involves a medical patient manipulating the medical device.

12. The system of claim 8, wherein comparing the one or more features of the at least one object to one or more reference features comprises assigning one or more reference points to the one or more features of the at least one object.

13. The system of claim 8, wherein the images are first images and the event is a first event, the operations further comprising:

collecting second images of the scene; and  
predicting, using the machine learning model, that a second event involving the object has occurred in scene.

14. The system of claim 13, the operations further comprising:

in response to predicting that the second event has occurred in the scene, providing an alert.

15. One or more non-transitory computer-readable media storing computer-readable instructions that, when executed by a processing system, cause a system to perform operations comprising:

collecting images of a scene including an object;  
detecting, based on the images, that an event involving the object has occurred in the scene, wherein the event is detected in-part by comparing one or more features of the object to one or more reference features;  
comparing the object to a database object to determine if the object is associated with a known object in a database, wherein, if the object is not determined to be associated with the known object, the database is updated with reference data associated with the object;

**16**

in response to detecting that the event has occurred within the scene, presenting at least one of the object and information associated with the event in a graphical user interface;

receiving an indication that the object or the event has been confirmed; and

in response to receiving the indication that the object or event has been confirmed, updating a machine learning model with i) the event, ii) the object, iii) the reference data associated with the object, or iv) combinations of i)-iii), wherein the machine learning model is configured to recognize objects and events occurring in the scene.

16. The one or more non-transitory computer-readable media of claim 15, wherein the images are collected by an image capturing device located in the scene.

17. The one or more non-transitory computer-readable media of claim 15, wherein the scene includes a medical patient and the event involves a motion of the medical patient.

18. The one or more non-transitory computer-readable media of claim 15, wherein the object is a medical device and the event involves a medical patient manipulating the medical device.

19. The one or more non-transitory computer-readable media of claim 15, wherein comparing the one or more features of the at least one object to one or more reference features comprises assigning one or more reference points to the one or more features of the at least one object.

20. The one or more non-transitory computer-readable media of claim 15, wherein the images are first images and the event is a first event, the operations further comprising:  
collecting second images of the scene; and  
predicting, using the machine learning model, that a second event involving the object has occurred in scene.

\* \* \* \* \*