



US0D1091819S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,091,819 S**
Swick et al. (45) **Date of Patent:** **** Sep. 2, 2025**

(54) **BIOPSY DEVICE**

(71) Applicant: **HOLOGIC, INC.**, Marlborough, MA
(US)

(72) Inventors: **Zachary Stephen Swick**, Westborough,
MA (US); **David Sauvageau**, Westlake
Village, CA (US); **Rosario Friedman**,
Medford, MA (US); **Brett Haarala**,
Framingham, MA (US)

(73) Assignee: **hologic, inc.**, Marlborough, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/828,621**

(22) Filed: **Feb. 28, 2022**

Related U.S. Application Data

(60) Continuation of application No. 29/681,944, filed on
Feb. 28, 2019, now Pat. No. Des. 946,753, which is
a division of application No. 29/485,001, filed on
Mar. 14, 2014, now Pat. No. Des. 844,784.

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/133**

(58) **Field of Classification Search**

USPC D8/499; D16/100, 130, 309; D24/108,
D24/112, 113, 114, 115, 127, 128, 129,
D24/130, 133, 144, 146, 147, 170, 216,
D24/222, 231, 232

CPC A61B 17/00; A61B 2017/00349; A61B
10/00; A61B 10/02; A61B 2010/0208;
A61B 10/04; A61B 2010/045

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D239,026 S 3/1976 Knox
D255,990 S 7/1980 Lucas

D279,654 S 7/1985 Grip et al.
D329,592 S 9/1992 Crawford
D348,840 S 7/1994 Kuzma
D351,745 S 10/1994 Seifert

(Continued)

FOREIGN PATENT DOCUMENTS

GB 9002536623-0005 * 9/2014

OTHER PUBLICATIONS

Youtube, "Mammotome elite—Product Overview", first available
Sep. 2, 2015. (<https://www.youtube.com/watch?v=AFO3HLhOwM8&t=1s>) (Year: 2015).*

(Continued)

Primary Examiner — Leanne Was-Englehart

Assistant Examiner — Justin A Johnson

(74) *Attorney, Agent, or Firm* — Jones Robb, PLLC

(57) **CLAIM**

The ornamental design for a biopsy device, as shown and
described.

DESCRIPTION

FIG. 1 is a perspective view of a biopsy device, showing our
new design;

FIG. 2 is a right side elevational view of the biopsy device
of FIG. 1;

FIG. 3 is a left side elevational view of the biopsy device of
FIG. 1;

FIG. 4 is a top plan view of the biopsy device of FIG. 1;


FIG. 5 is a bottom plan view of the biopsy device of FIG. 1;

FIG. 6 is a front elevational view of the biopsy device of
FIG. 1; and,

FIG. 7 is a rear elevational view of the biopsy device of FIG.
1.

The broken lines in the drawings illustrate portions of the
biopsy device and form no part of the claimed design.

1 Claim, 6 Drawing Sheets

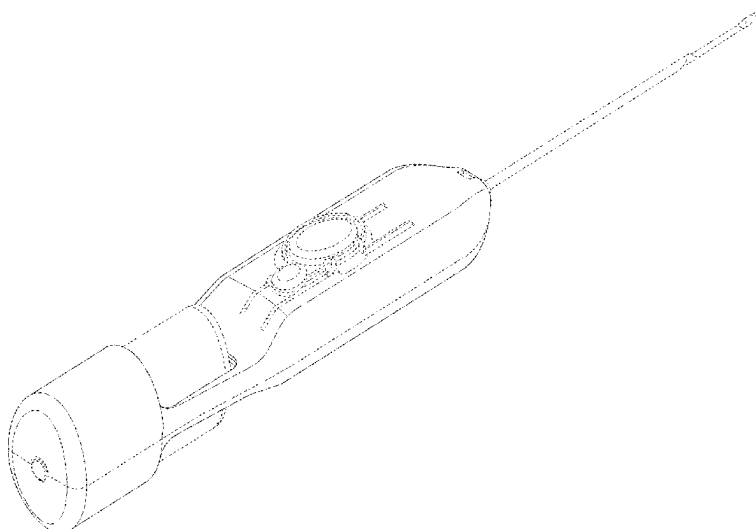

References Cited

2009/0024056	A1 *	1/2009	Bacon	A61B 10/0233 600/567
2012/0259287	A1	10/2012	Selvitelli et al.	
2015/0045828	A1 *	2/2015	McArthur	A61F 2/0108 606/200
2017/0131299	A1	5/2017	Holloway	
2019/0183463	A1 *	6/2019	Keller	A61B 10/0275
2020/0406020	A1	12/2020	Fangrow	

D369,097	S		4/1996	Dinand		
D372,676	S		8/1996	Desgrippes		
D379,312	S		5/1997	Crawford		
D381,899	S		8/1997	Crawford		
D413,263	S		8/1999	Pritchard et al.		
D541,155	S		4/2007	Battegazzore		
D590,942	S		4/2009	Petersen		
7,914,464	B2 *		3/2011	Burdorff		A61B 34/25
						600/568
D735,333	S *		7/2015	Allen		D24/147
D736,923	S *		8/2015	Snow		D24/146
D748,254	S *		1/2016	Freigang		D24/133
D751,199	S *		3/2016	Allen		D24/146
D771,249	S *		11/2016	Heath		D24/133
D772,411	S *		11/2016	Heath		D24/146
D779,062	S		2/2017	Evans et al.		
D782,693	S		3/2017	Brewer et al.		
D788,909	S *		6/2017	Ratjen		D24/113
D802,760	S		11/2017	Neby		
D837,375	S *		1/2019	Park		D24/146
D844,784	S *		4/2019	Swick		D24/147
D859,661	S		9/2019	Blackwell		
D893,716	S		8/2020	Siciliano		
D929,583	S		8/2021	Neimyy et al.		
D933,837	S *		10/2021	Tanghal		D24/187
D946,753	S *		3/2022	Swick		D24/133
2005/0054947	A1 *		3/2005	Goldenberg		A61B 10/0266
						600/567

Twitter, “Exclusive access to our Sertera™ Biopsy Device”, first available Dec. 2, 2015. (<https://twitter.com/hologic/status/672097947589337088>) (Year: 2015).*

Thingiverse, “Rounded Cylinder”, first available Oct. 11, 2015. (<https://www.thingiverse.com/thing:1065885>) (Year: 2015).

Twitter, “Exclusive access to our Sertera™ Biopsy Device”, first available Dec. 2, 2015. (<https://twitter.com/hologic/status/672097947589337088>) (Year: 2015).

Amazon, “Prescott Plastics 1½ Inch Round Black Vinyl End Cap”, first available Jun. 19, 2019. (<https://www.amazon.com/Prescott-Plastics-Round-Flexible-Rubber/dp/B07RLNPBCC>) (Year: 2019).

Specification and Drawings in U.S. Appl. No. 29/681,944, filed Feb. 28, 2019.

Office Action dated Jun. 23, 2021 in U.S. Appl. No. 29/681,944.

Notice of Allowance dated Nov. 12, 2021 in U.S. Appl. No. 29/681,944.

Notice of Allowance dated Nov. 9, 2018 in U.S. Appl. No. 29/485,001.

* cited by examiner

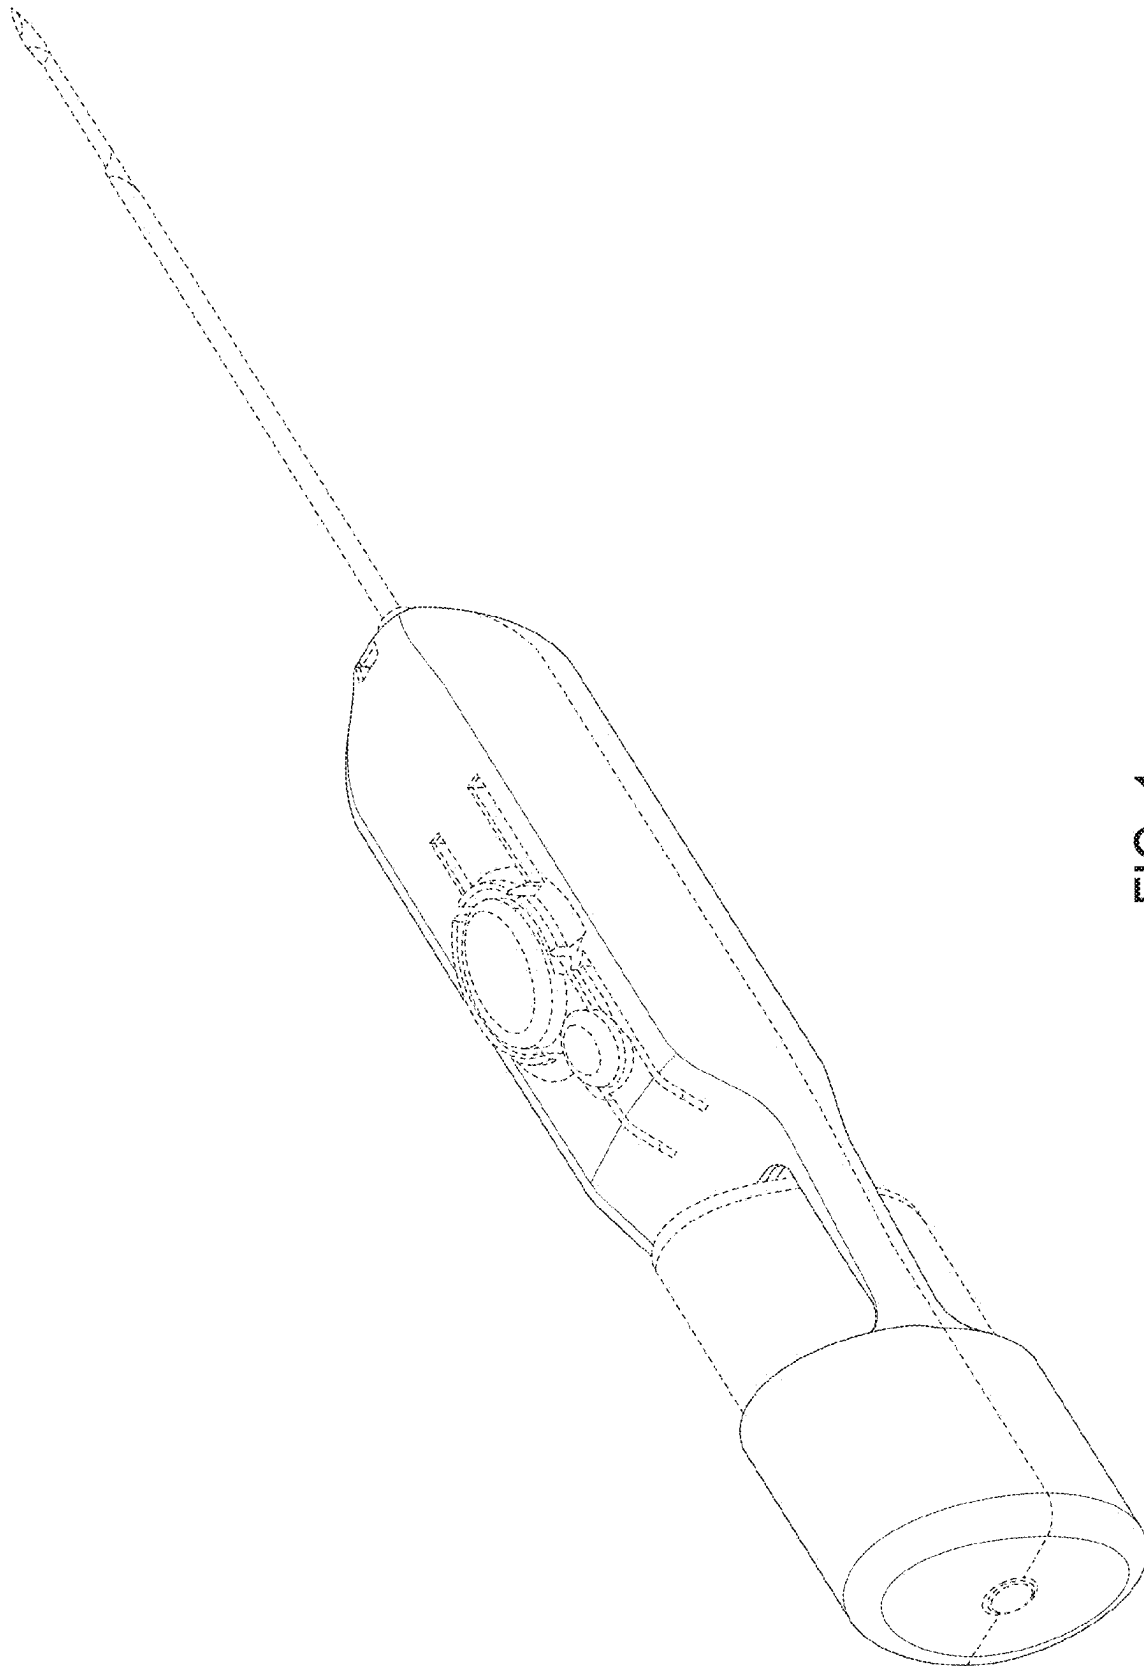


FIG. 1

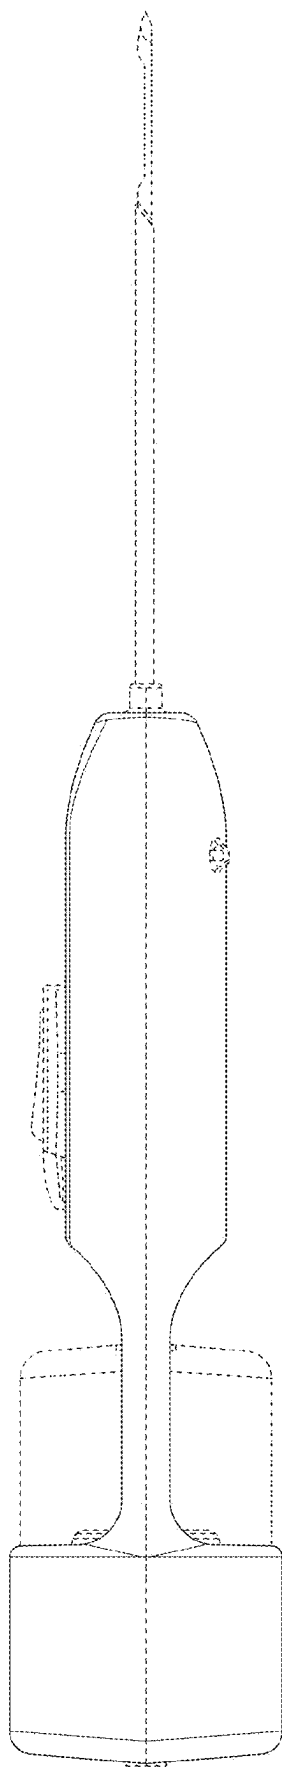


FIG. 2

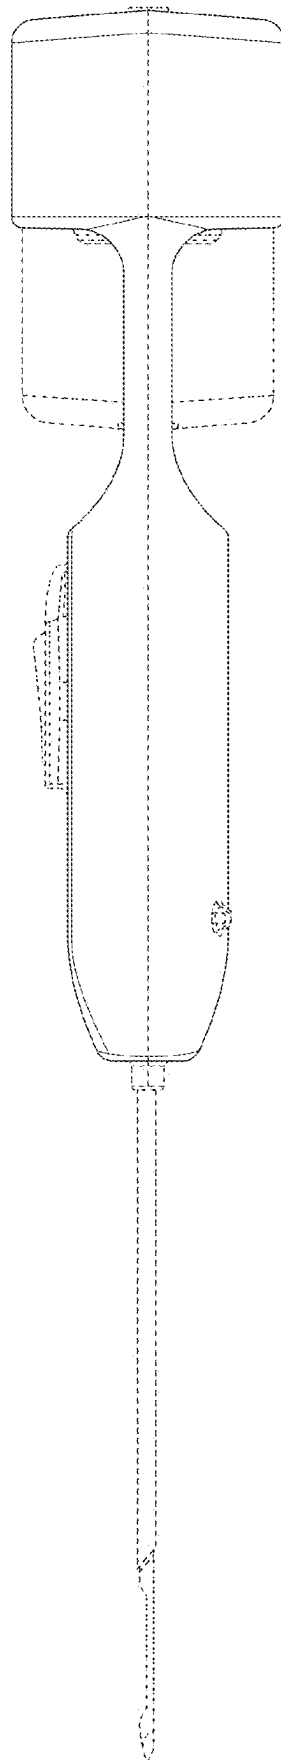


FIG. 3

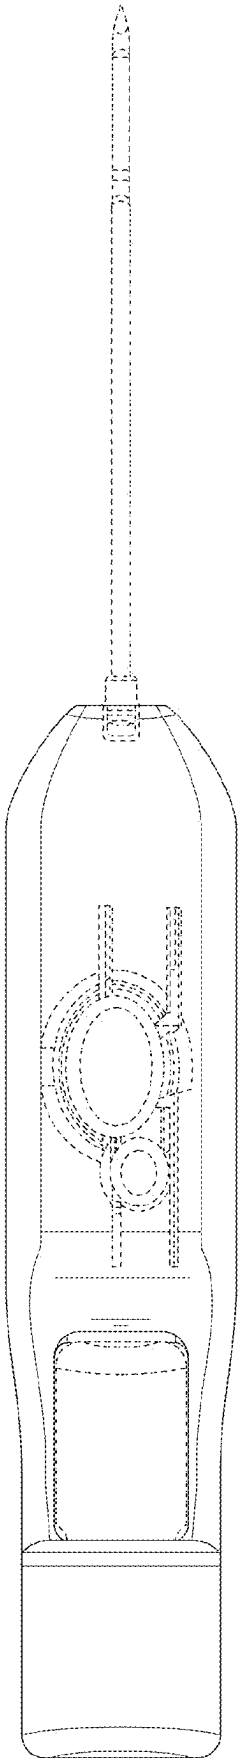


FIG. 4

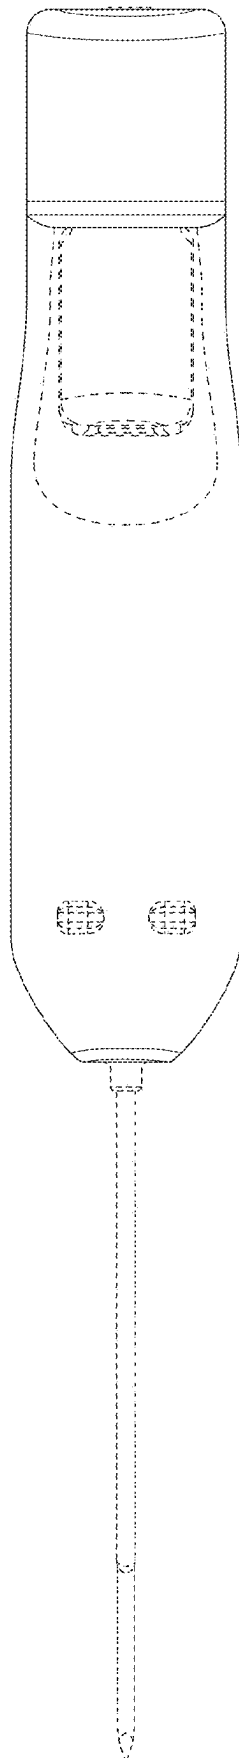


FIG. 5

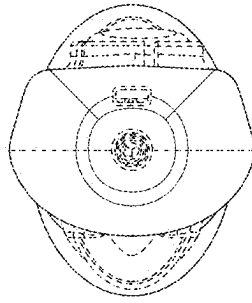


FIG. 6




FIG. 7