



US0D1092777S

(12) **United States Design Patent**
Lei et al.

(10) **Patent No.:** **US D1,092,777 S**

(45) **Date of Patent:** **** Sep. 9, 2025**

(54) **SAMPLE COLLECTION DETECTOR**

(71) Applicant: **Zhejiang Orient Gene Biotech Co., Ltd.**, Zhejiang (TW)

(72) Inventors: **Siyu Lei**, Zhejiang (TW); **Jianqiu Fang**, Zhejiang (TW); **Shaohua Fang**, Zhejiang (TW)

(73) Assignee: **Zhejiang Orient Gene Biotech Co., Ltd.**, Zhejiang (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/933,785**

(22) Filed: **Mar. 21, 2024**

(30) **Foreign Application Priority Data**

Oct. 27, 2023 (CN) 202330699205.3

(51) **LOC (15) CL.** **24-02**

(52) **U.S. CL.**
USPC **D24/224**

(58) **Field of Classification Search**

USPC D24/108, 121–123, 216, 217, 223–227,
D24/229, 230; D10/49–53, 57, 81, 93,
D10/125; D9/547, 550, 724, 732, 736
CPC G01N 2035/0436; G01N 33/5304; G01N
33/5302; G01N 35/00029; G01N 33/558;
G01N 2035/00148

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D256,786 S * 9/1980 Pedersen D10/81
D311,876 S * 11/1990 Kiegami D24/232
D594,131 S * 6/2009 Nguyen D24/216
D644,425 S * 9/2011 Gilmour D3/203.1
D664,258 S * 7/2012 Harkin D24/186
D720,070 S * 12/2014 Khalaj D24/144
D785,195 S * 4/2017 Owen D24/224

D845,504 S * 4/2019 Frezal D24/223
D864,774 S * 10/2019 Lei D24/186
D923,808 S * 6/2021 Lei D24/216
D965,788 S * 10/2022 Buess D24/164
D974,588 S * 1/2023 Lei D24/216
D980,448 S * 3/2023 Senda D24/216

(Continued)

FOREIGN PATENT DOCUMENTS

CN 202330231740.6 * 9/2023
JP D2022-26853 * 5/2023

OTHER PUBLICATIONS

UNC Fecal Test, Online, Published date Jun. 5, 2015, Retrieved on Apr. 30, 2025 from URL: <https://www.uncmedicalcenter.org/mclendon-clinical-laboratories/available-tests/fecal-immunochemical-test/> (Year: 2015).*

Primary Examiner — Justin C Dodson

Assistant Examiner — Eric Eldone Tormanen

(74) *Attorney, Agent, or Firm* — MUNCY, GEISSLER, OLDS & LOWE, P.C.


(57) **CLAIM**

The ornamental design for a sample collection detector as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right side perspective view of a sample collection detector showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof;
FIG. 8 is a bottom, front, left side perspective view thereof;
FIG. 9 is a top perspective view thereof; and,
FIG. 10 is a bottom perspective view thereof.

1 Claim, 10 Drawing Sheets

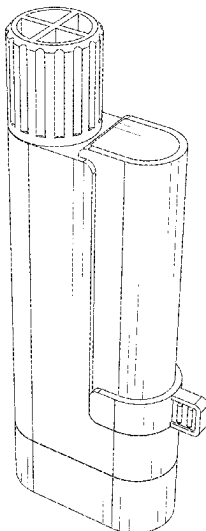

(56)

References Cited

U.S. PATENT DOCUMENTS

D1,021,130	S	*	4/2024	Thakor	D24/216
D1,044,022	S	*	9/2024	Hu	G01N 1/02
					D24/216
2014/0228769	A1	*	8/2014	Karlsson	A61M 5/31553
					604/197
2018/0235582	A1	*	8/2018	Dai	A61B 10/0038
2018/0333076	A1	*	11/2018	Kleinhappl	A61B 5/087
2022/0226804	A1	*	7/2022	Lei	B01L 3/523
2023/0129323	A1	*	4/2023	Bailey	B01L 3/5029
					422/420

* cited by examiner

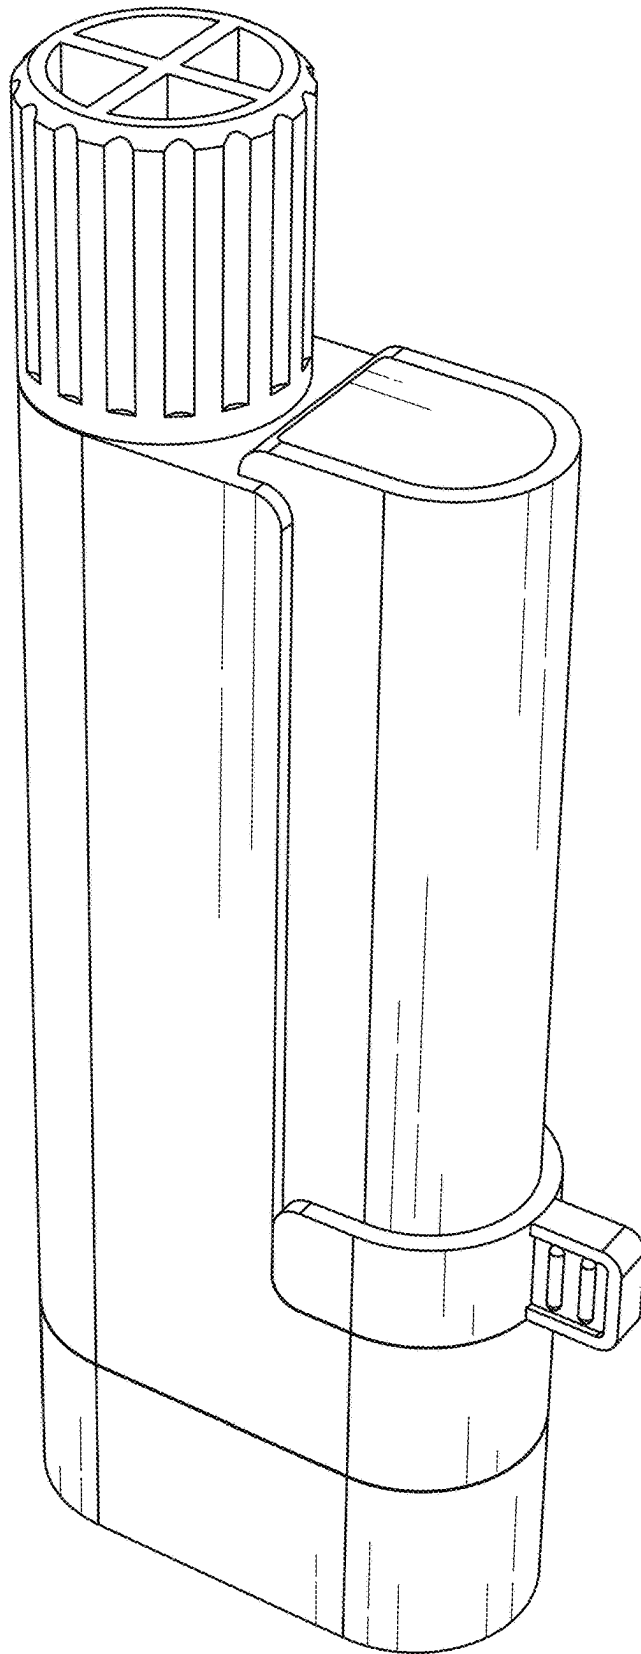


FIG. 1

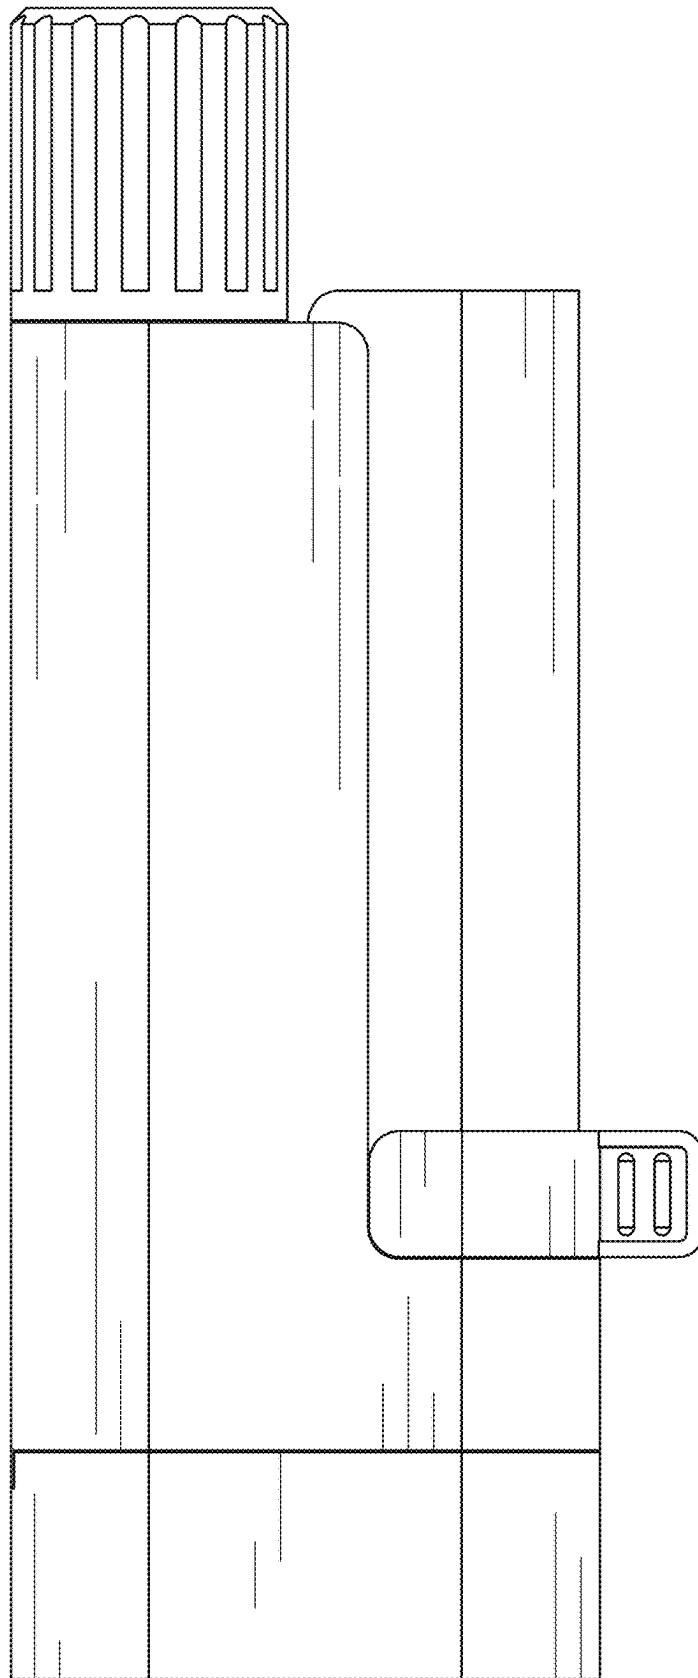


FIG. 2

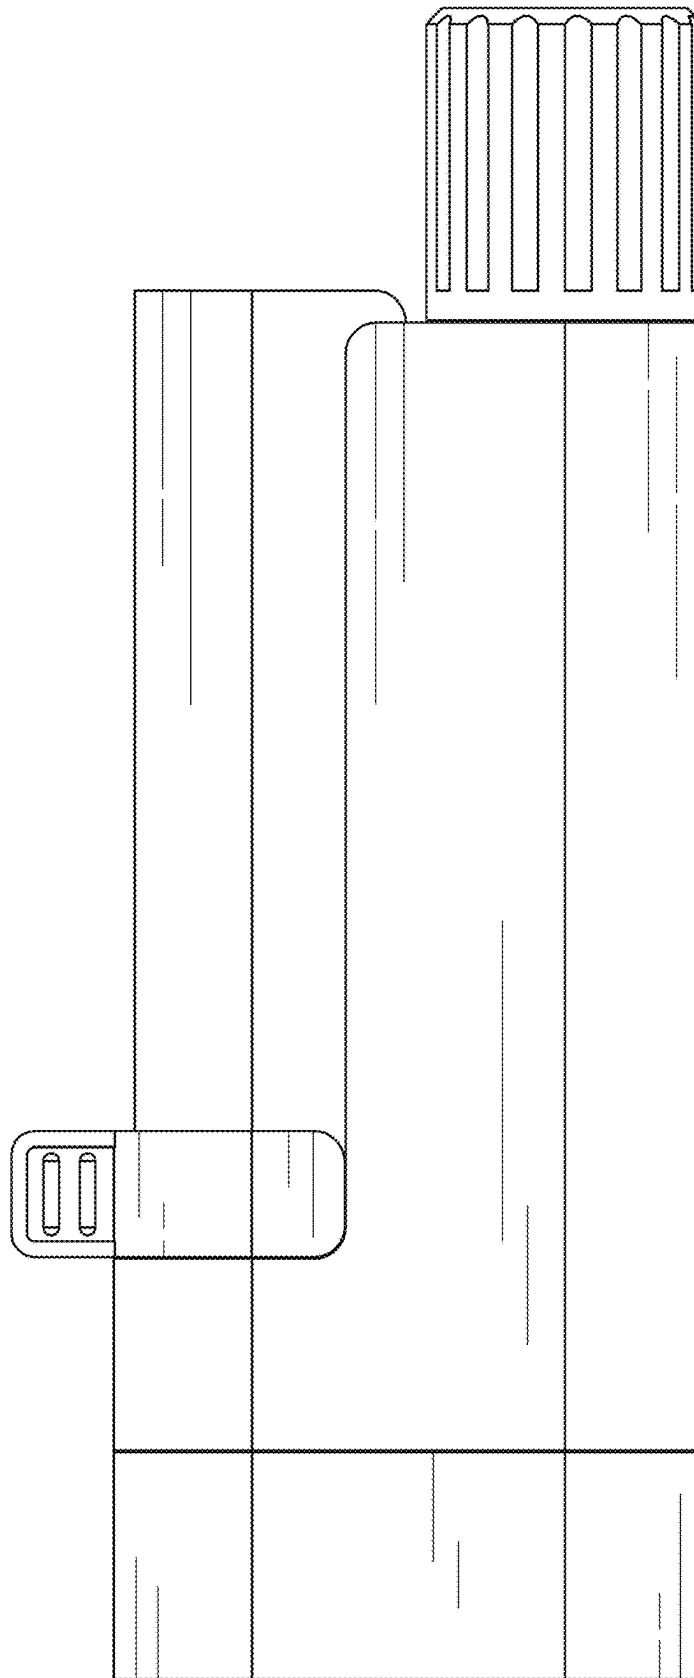


FIG. 3

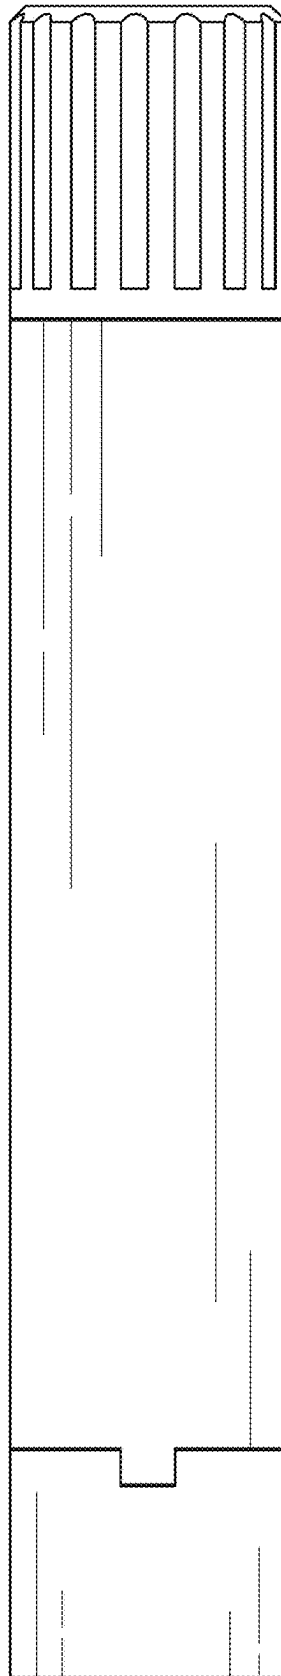


FIG. 4

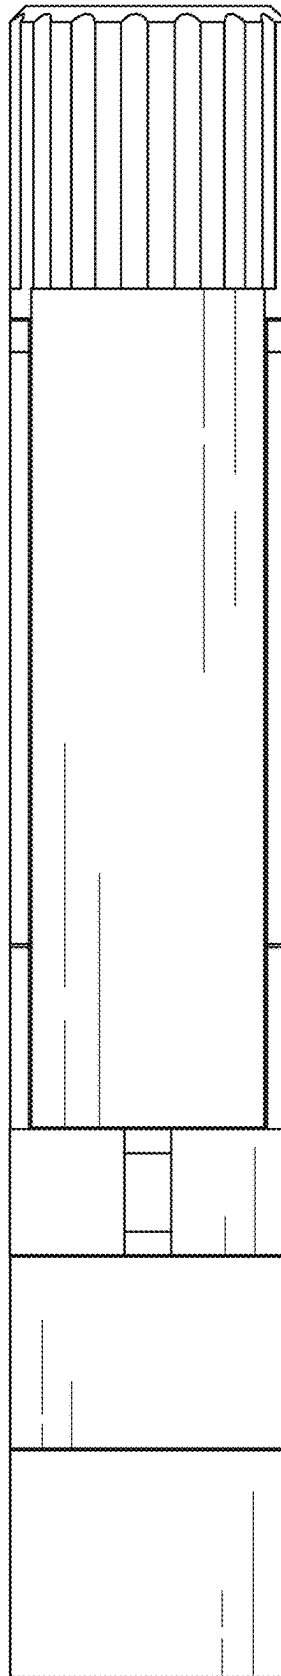


FIG. 5

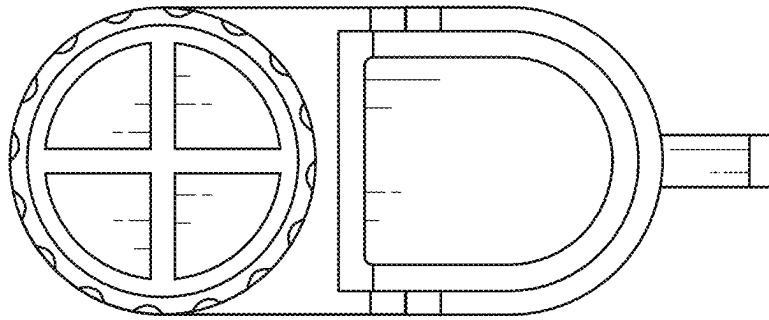


FIG. 6

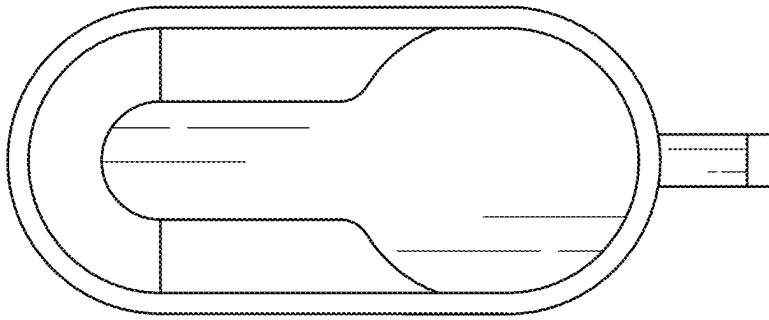


FIG. 7

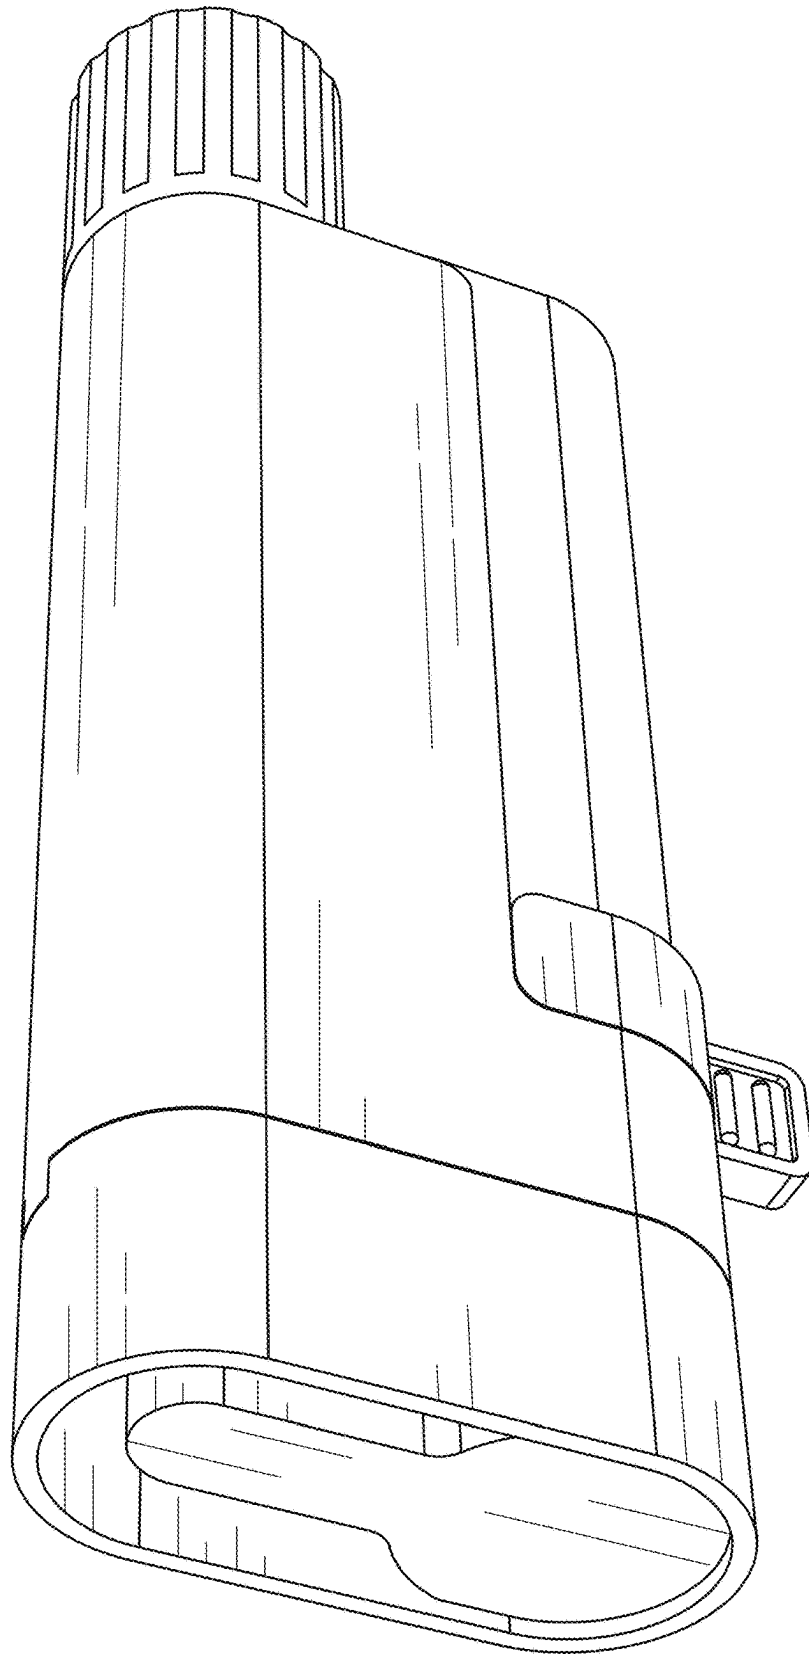


FIG. 8

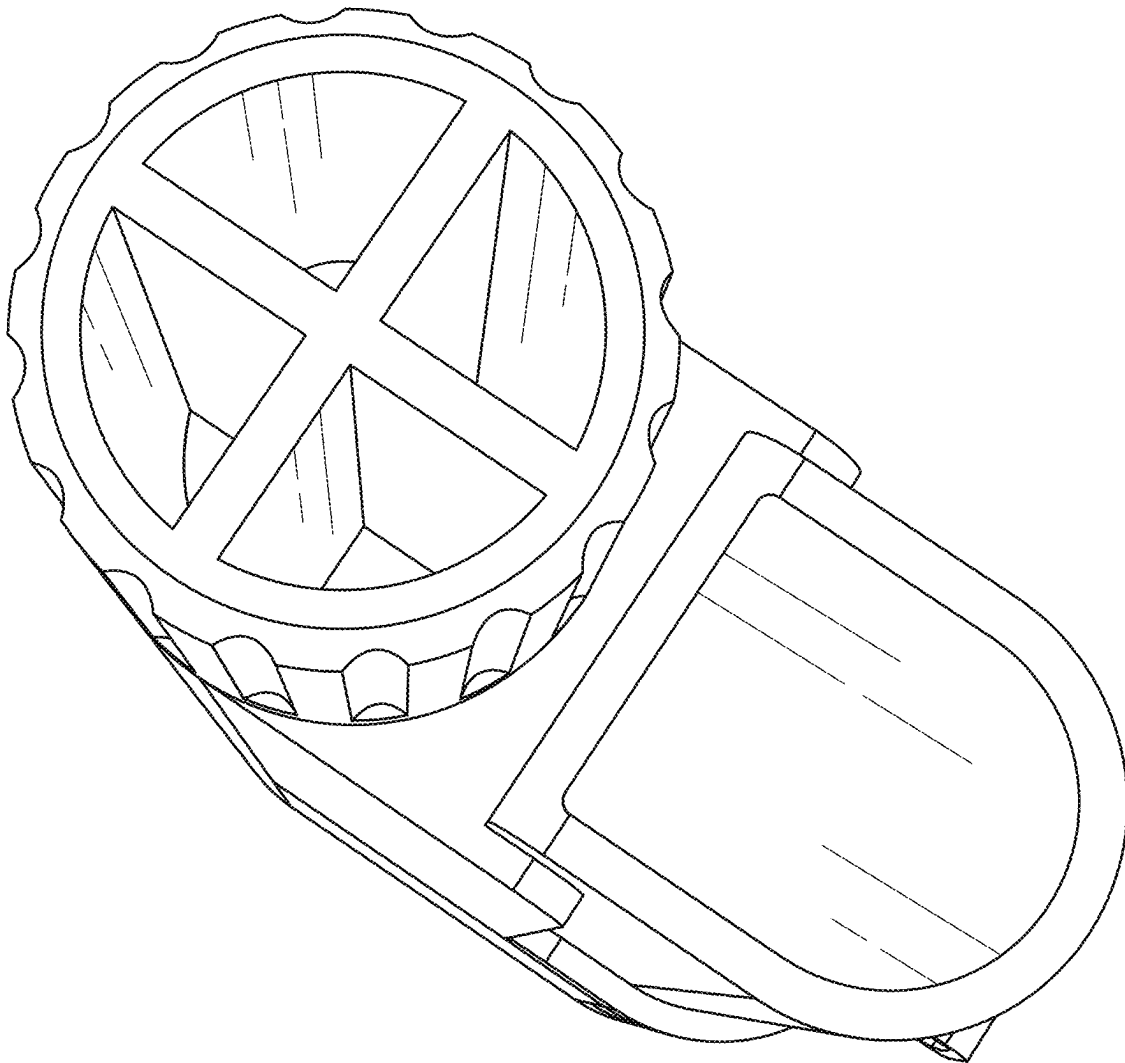


FIG. 9

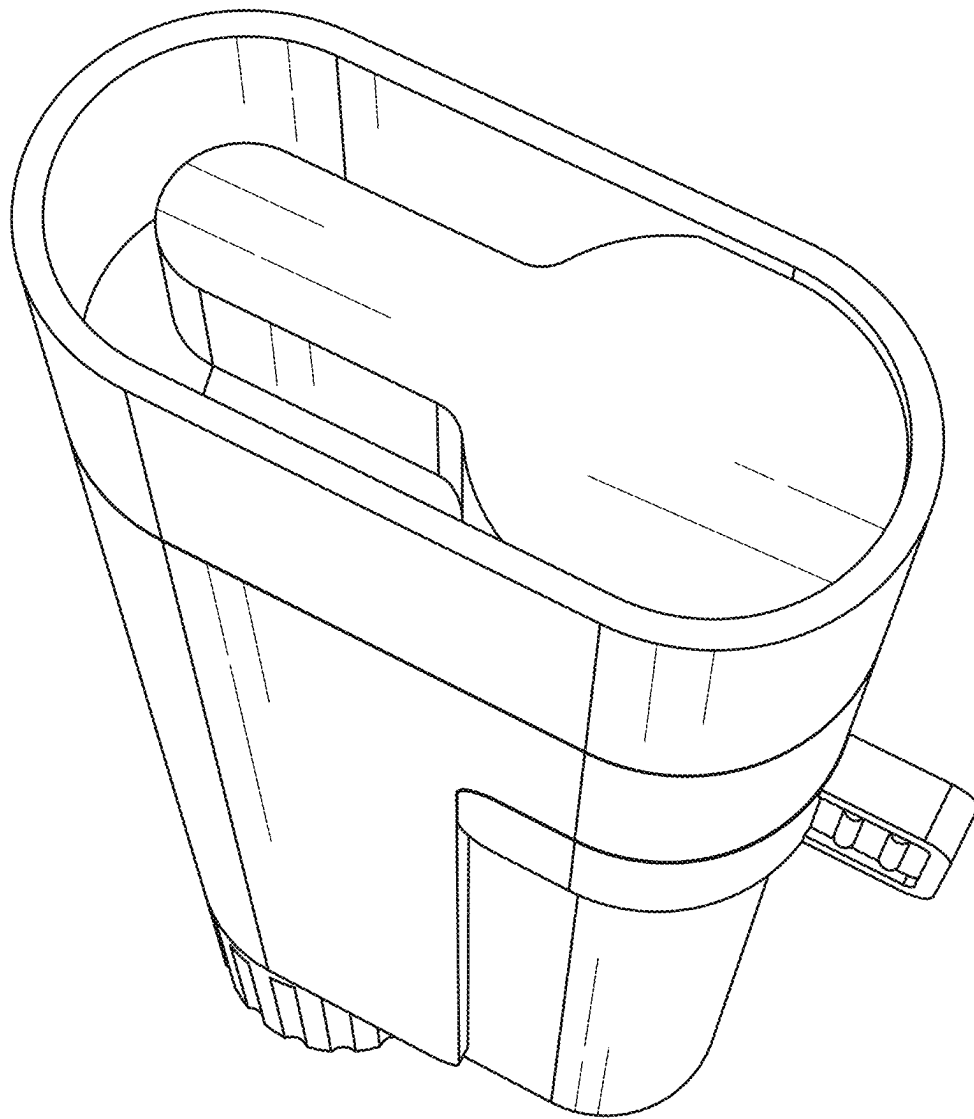


FIG. 10