



US0D1092740S

(12) **United States Design Patent**
Balathandayutham et al.

(10) **Patent No.:** **US D1,092,740 S**

(45) **Date of Patent:** **** Sep. 9, 2025**

(54) **X-RAY TUBE INSERT**

(71) Applicant: **GE Precision Healthcare LLC**,
Milwaukee, WI (US)

(72) Inventors: **Naren P Balathandayutham**,
Bangalore (IN); **Praveen Kvu**,
Bangalore (IN); **Vinod Kumar Y**,
Bangalore (IN); **Anup G**, Bangalore
(IN); **Manoj Kumar Mahala**,
Bangalore (IN); **Pratik Joshi**,
Bangalore (IN); **Anija M**, Bangalore
(IN)

(73) Assignee: **GE PRECISION HEALTHCARE
LLC**, Milwaukee, WI (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/776,791**

(22) Filed: **Mar. 31, 2021**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**

USPC D24/158, 159, 160, 161, 185, 186, 107;
D14/420, 421, 341
CPC G01N 2223/3307; G01N 2223/419; G01N
23/10; G01N 23/083; G01N 23/046;
G01V 5/0016; G01V 5/005; G01V
5/0025; G01V 5/0041; A61B 8/13; A61B
8/44; A61B 8/42; A61B 8/46; A61B 8/54;
A61N 2005/1061; A61N 5/10; A61N
5/1081; A61N 5/1048; A61N 5/1049

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,902,474 A * 3/1933 Ungelenk H05G 1/04
D24/158
D94,184 S * 1/1935 Brunst D16/242

D115,114 S * 6/1939 Horsley D24/158
D133,666 S * 9/1942 Goldfield D24/158
D153,789 S * 5/1949 Goldfield D24/158
2,670,443 A * 2/1954 Pennock G21F 5/02
378/150
D176,113 S * 11/1955 Graves D24/158
D177,540 S * 4/1956 Waggoner D24/158

(Continued)

FOREIGN PATENT DOCUMENTS

CN 308964067 * 11/2024

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) *Attorney, Agent, or Firm* — McCoy Russell LLP

(57) **CLAIM**

The ornamental design for an X-ray tube insert as shown and described.

DESCRIPTION

FIG. 1 is a top-left perspective view of an X-ray tube insert according to a first embodiment of the claimed design.

FIG. 2 is a top-right perspective view of the X-ray tube insert of FIG. 1.

FIG. 3 is a bottom-left perspective view of the X-ray tube insert of FIG. 1.

FIG. 4 is a bottom-right perspective view of the X-ray tube insert of FIG. 1.

FIG. 5 is a front view of the X-ray tube insert of FIG. 1.

FIG. 6 is a rear view of the X-ray tube insert of FIG. 1.


FIG. 7 is a right side view of the X-ray tube insert of FIG. 1.

FIG. 8 is a left side view of the X-ray tube insert of FIG. 1.

FIG. 9 is a top view of the X-ray tube insert of FIG. 1; and,

FIG. 10 is a bottom view of the X-ray tube insert of FIG. 1.

1 Claim, 10 Drawing Sheets

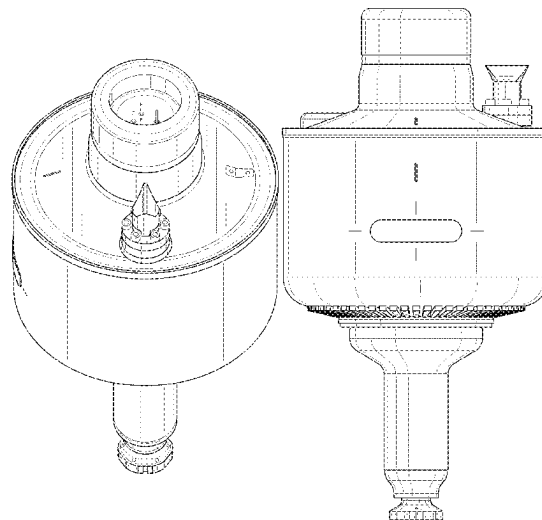

(56)

References Cited

U.S. PATENT DOCUMENTS

D192,167	S	*	2/1962	Noyes		D24/158	D755,386	S	*	5/2016	Kato		D24/158
D197,688	S	*	3/1964	Bastin		D24/158	D755,387	S	*	5/2016	Kato		D24/158
D217,078	S	*	3/1970	Vandervelden		D24/158	D755,388	S	*	5/2016	Kato		D24/158
D217,995	S	*	7/1970	Montgomery		D24/158	D755,389	S	*	5/2016	Kato		D24/158
D218,029	S	*	7/1970	Packin		D24/158	D767,141	S	*	9/2016	Mizumura		D24/158
D223,220	S	*	3/1972	Johnson		D24/158	D767,142	S	*	9/2016	Mizumura		D24/158
D234,544	S	*	3/1975	Bobov		D24/158	D767,143	S	*	9/2016	Mizumura		D24/158
D238,307	S	*	12/1975	Bobov		D24/158	D770,048	S	*	10/2016	Mizumura		D24/158
D242,171	S	*	11/1976	Warrikhoff		D24/158	D773,668	S	*	12/2016	Mizumura		D24/158
D306,577	S	*	3/1990	Matsutani		D24/158	D773,669	S	*	12/2016	Mizumura		D24/158
4,984,261	A	*	1/1991	Maldonado		H05G 1/06 378/127	D773,670	S	*	12/2016	Mizumura		D24/158
4,993,057	A	*	2/1991	Runnells		A61B 6/4423 378/197	D778,444	S	*	2/2017	Mizumura		D24/158
D363,349	S	*	10/1995	Dittert		D24/158	D793,558	S	*	8/2017	Mizumura		D24/158
5,795,207	A	*	8/1998	Blake et al.		D24/158	D794,198	S	*	8/2017	Mizumura		D24/158
D470,589	S	*	2/2003	Choi		D24/158	D794,199	S	*	8/2017	Mizumura		D24/158
D702,351	S	*	4/2014	Li		D24/158	D838,852	S	*	1/2019	Sottas		D24/158
D703,322	S	*	4/2014	Hayman		D24/158	D840,540	S		2/2019	Brogan et al.		
D726,920	S	*	4/2015	Ishihara		D24/158	D844,785	S		4/2019	Dayton et al.		
D726,921	S	*	4/2015	Ishihara		D24/158	D862,700	S		10/2019	Brogan et al.		
D726,922	S	*	4/2015	Ishihara		D24/158	D875,943	S		2/2020	Dayton et al.		
D727,507	S	*	4/2015	Ishihara		D24/158	D882,091	S	*	4/2020	Ishii		D24/158
D727,508	S	*	4/2015	Ishihara		D24/158	D902,154	S	*	11/2020	Hirabayashi		D13/112
D750,783	S	*	3/2016	Yasukawa		D24/158	D906,240	S	*	12/2020	Frank		D13/110
							D958,743	S	*	7/2022	Zhihua		D13/112
							D966,520	S	*	10/2022	Yan		D24/158
							2016/0287904	A1	*	10/2016	Liu		A61N 5/1049
							2019/0306964	A1	*	10/2019	Rogers		F04D 25/00

* cited by examiner

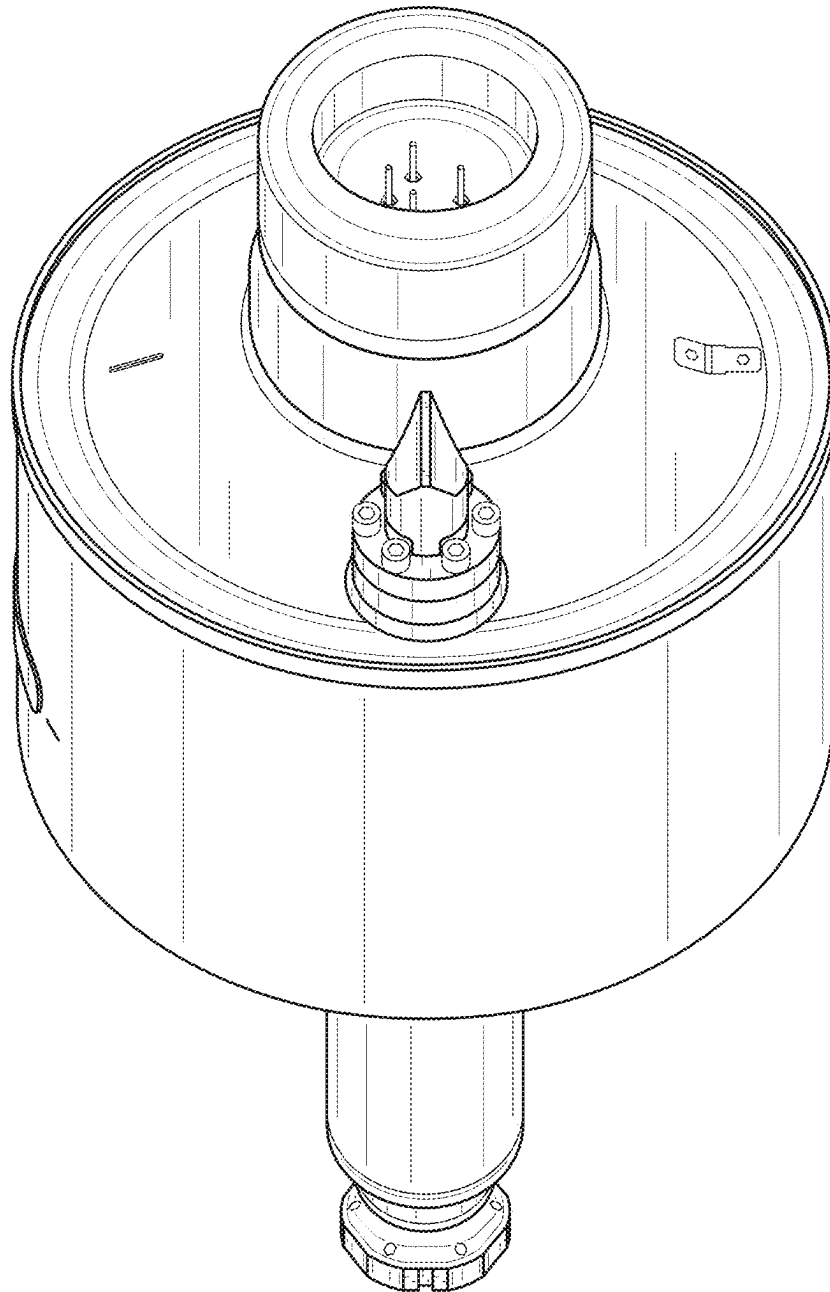


FIG. 1

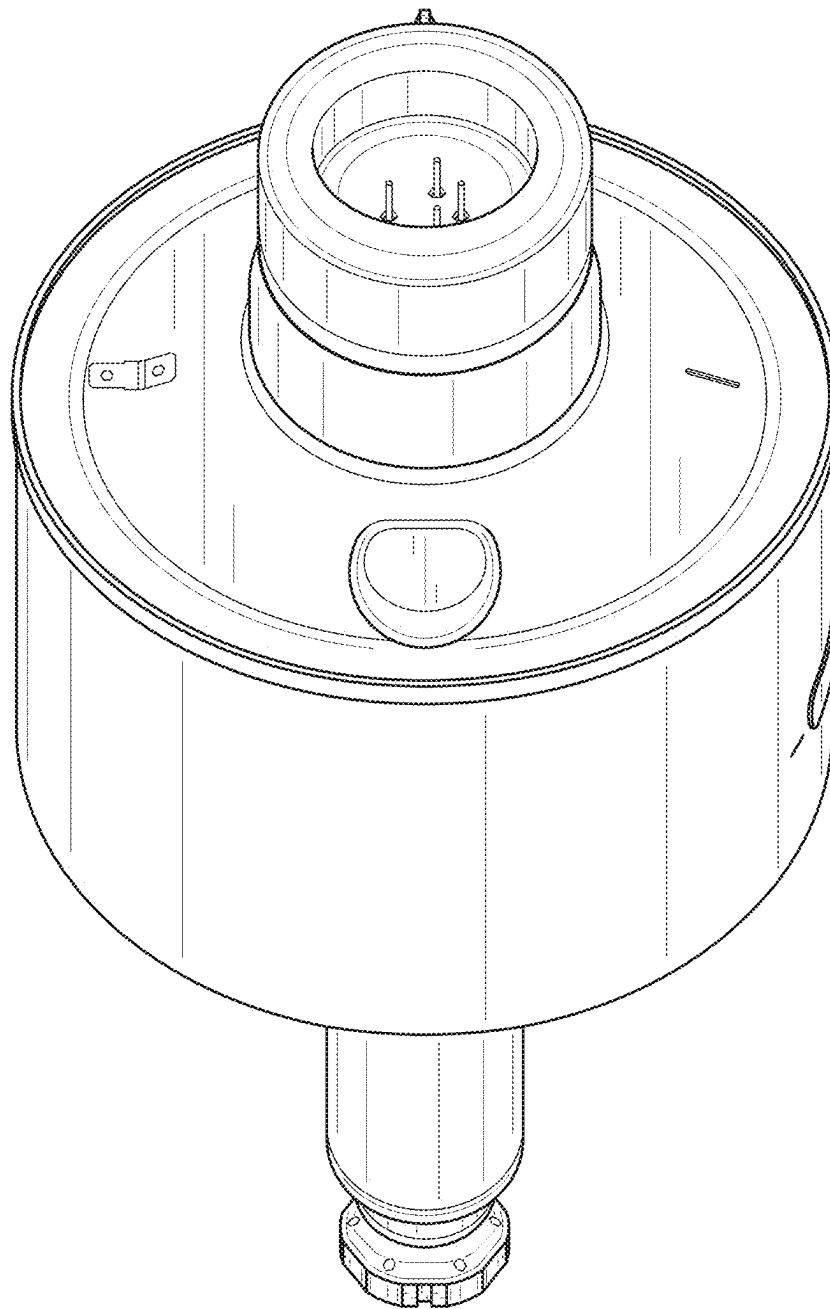


FIG. 2

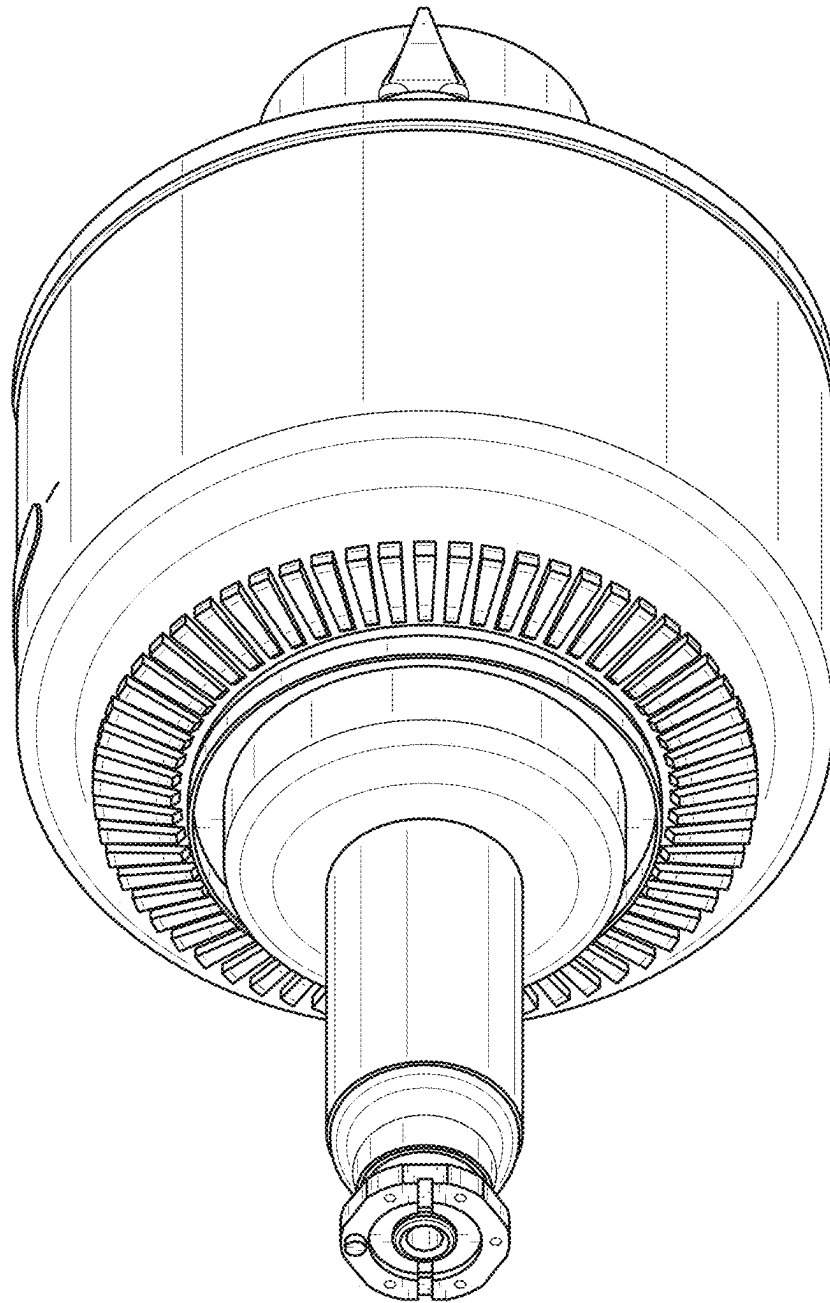


FIG. 3

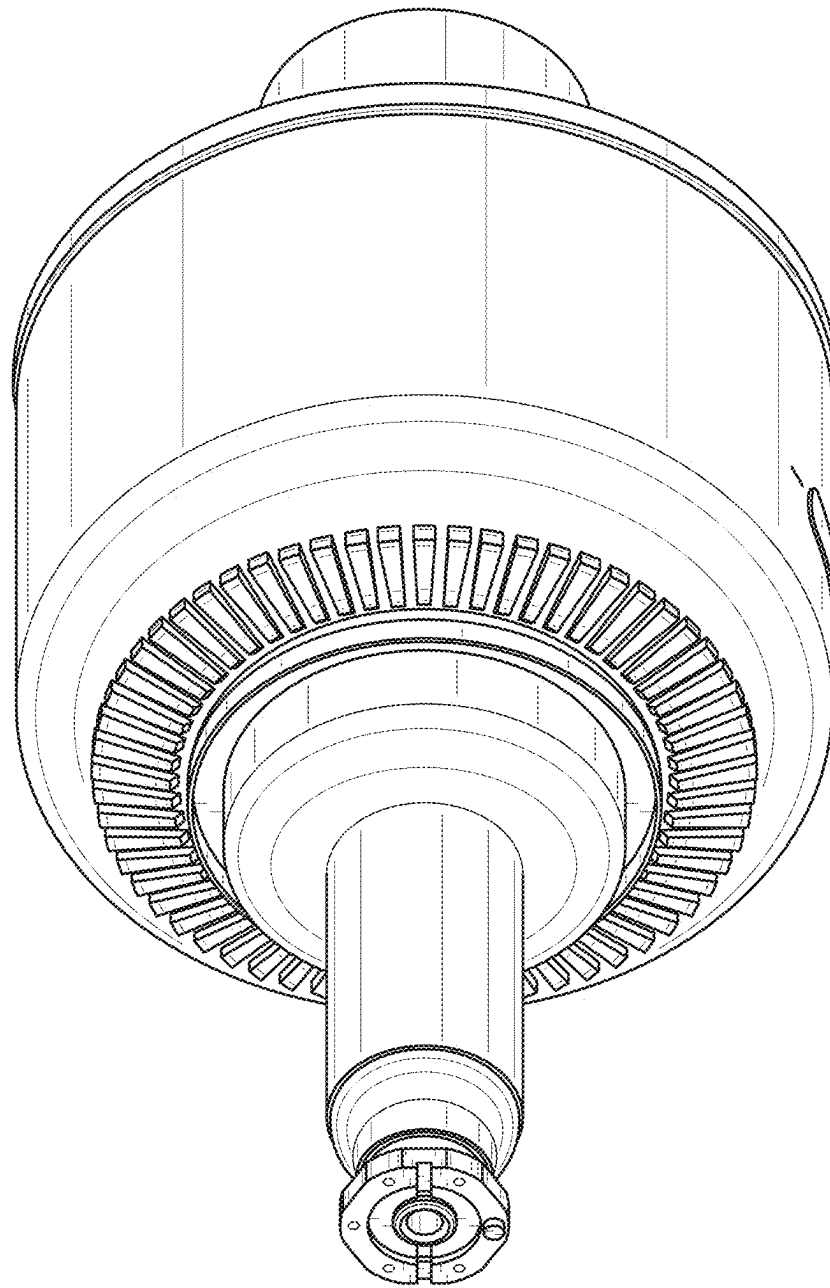


FIG. 4

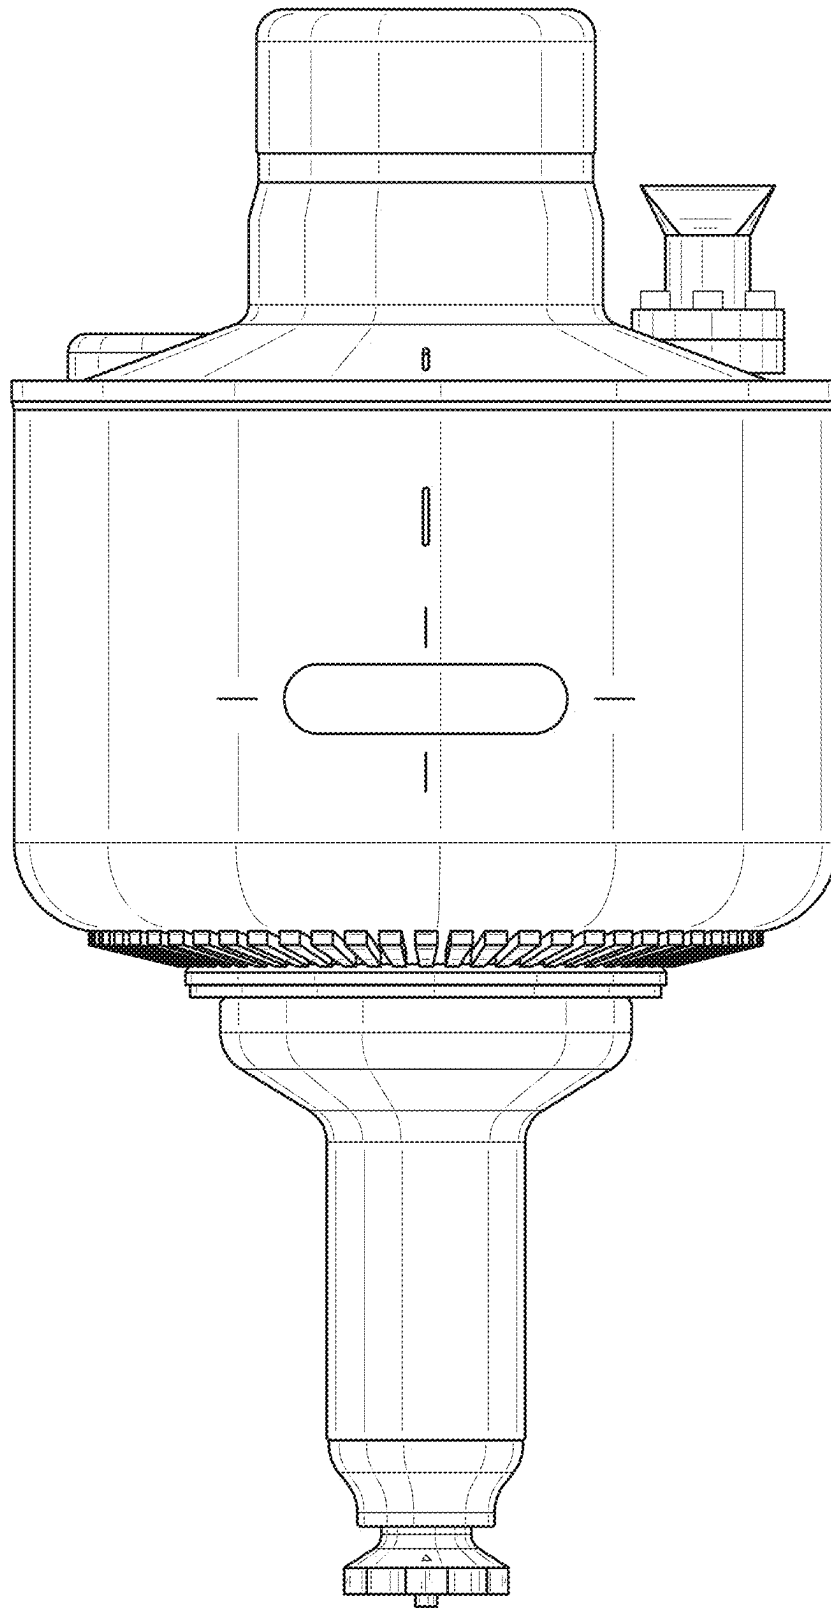


FIG. 5

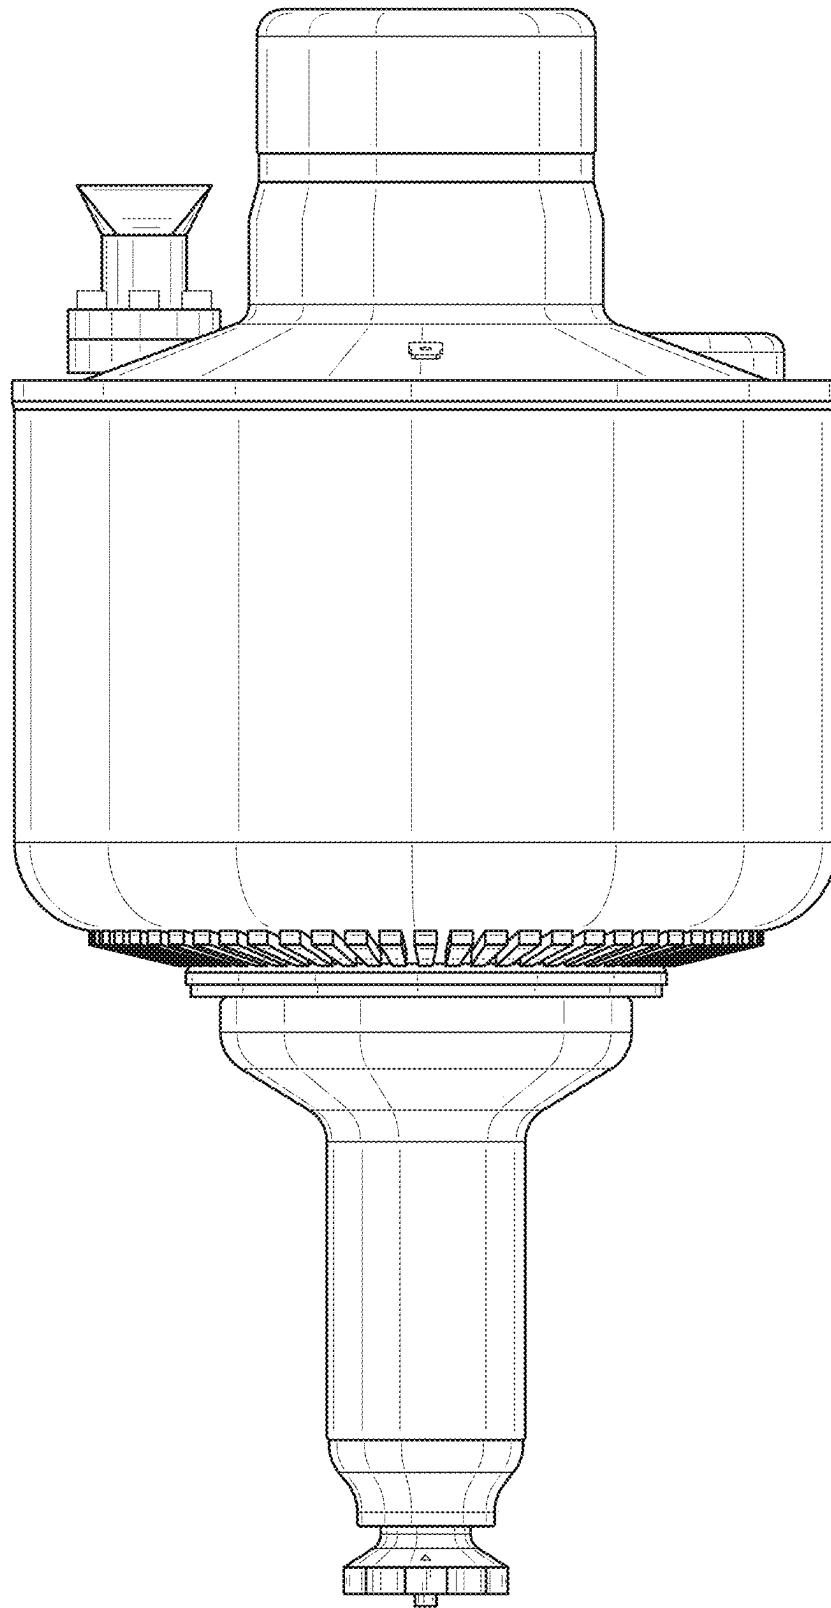


FIG. 6

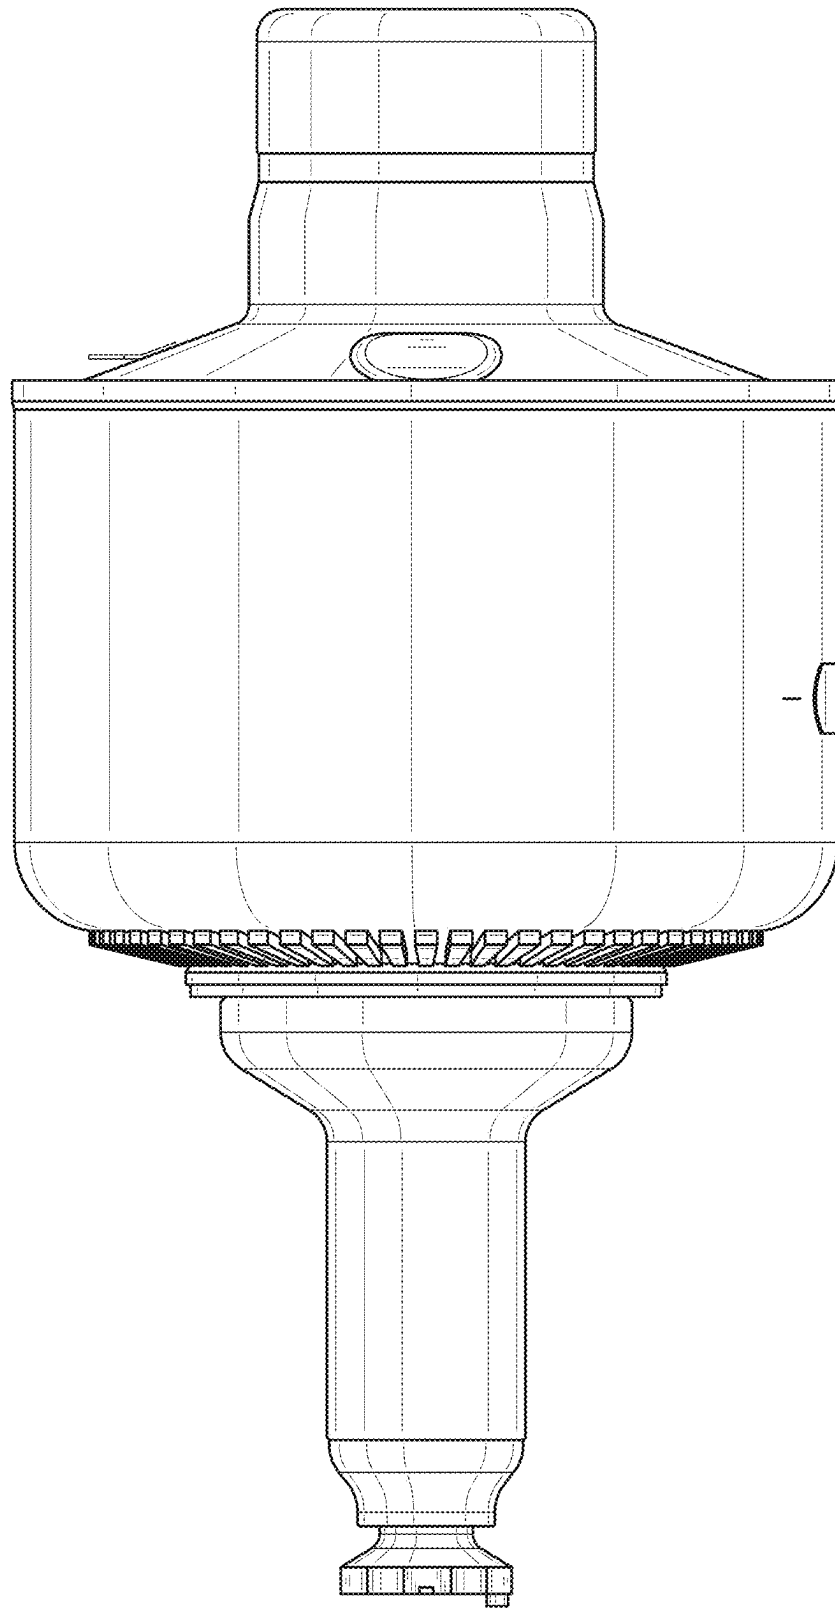


FIG. 7

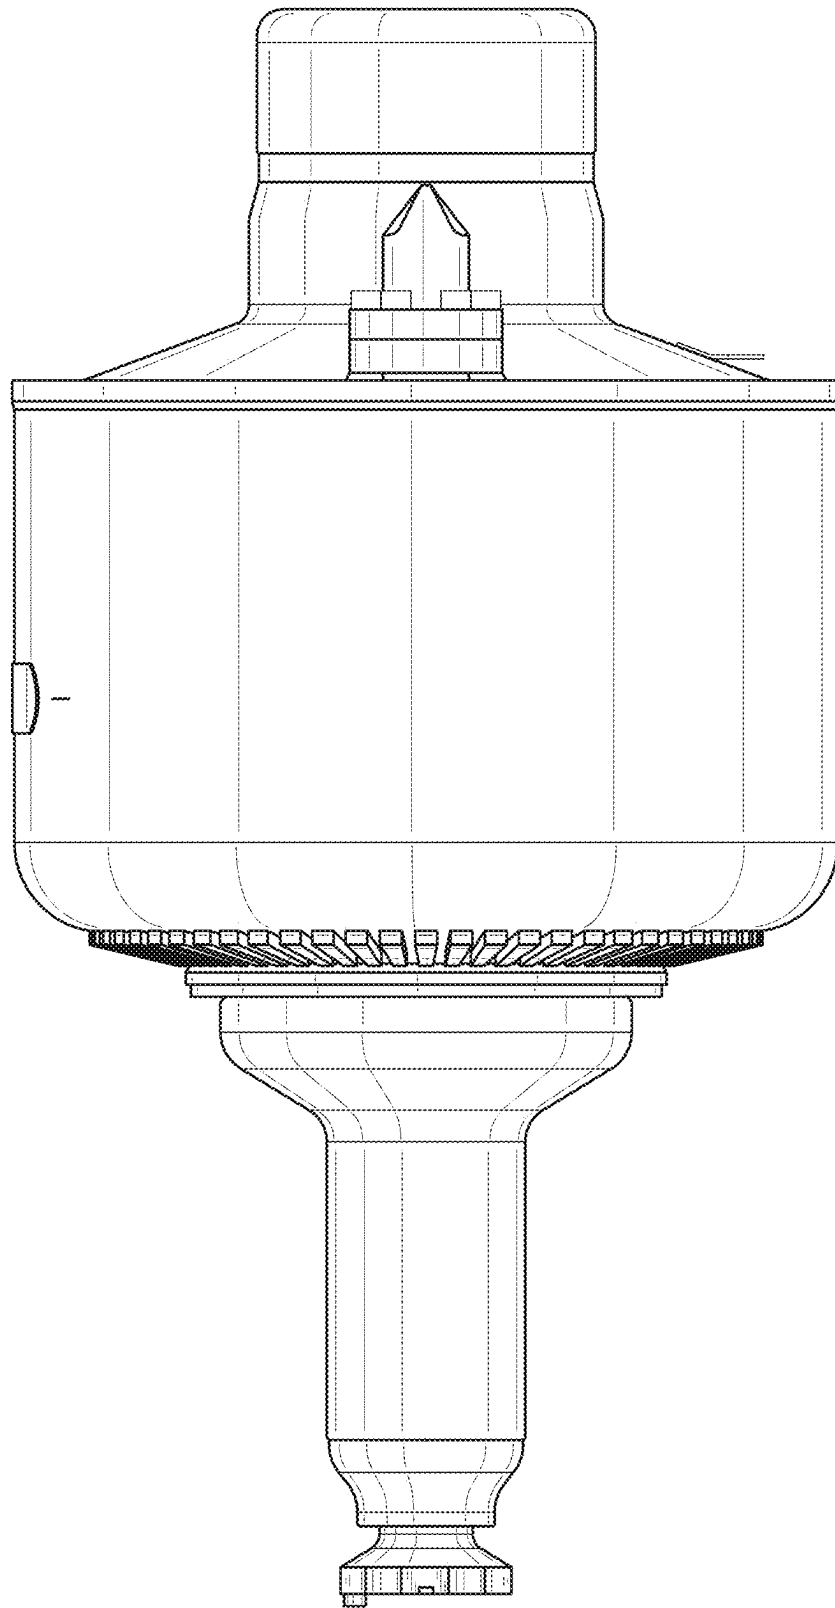


FIG. 8

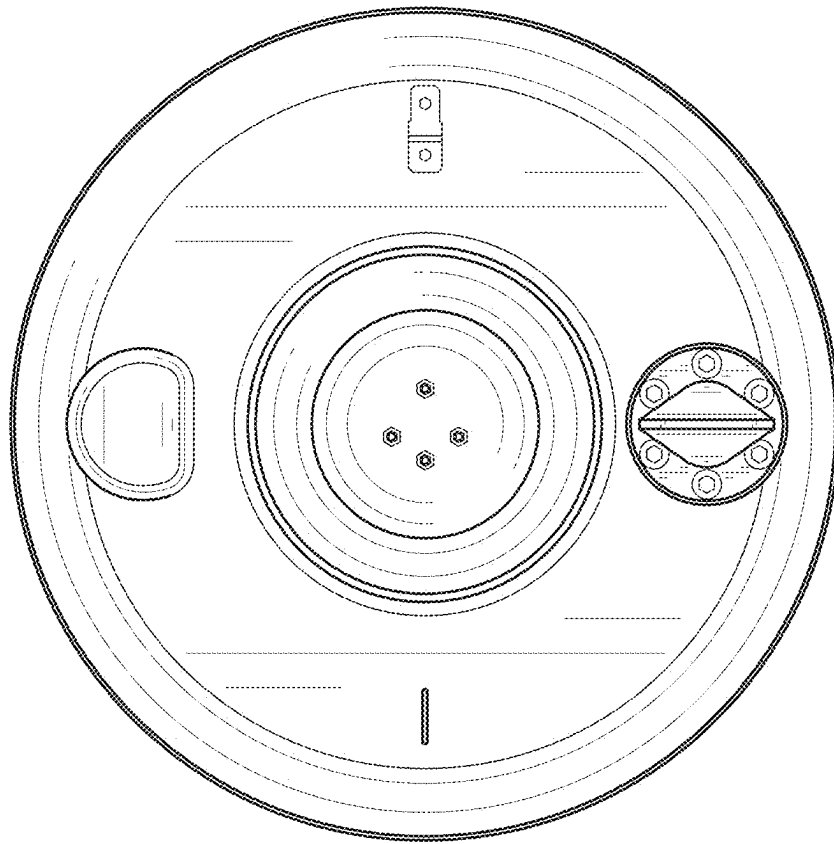


FIG. 9

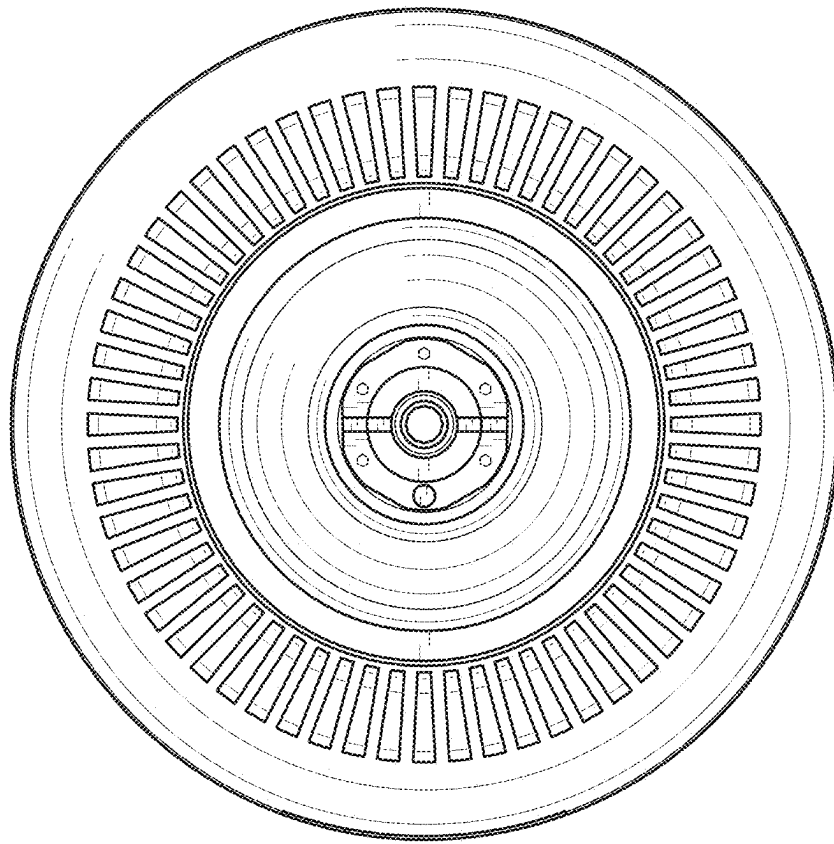


FIG. 10