

(12) **United States Patent**
Misener

(10) **Patent No.:** **US 12,403,288 B2**

(45) **Date of Patent:** **Sep. 2, 2025**

(54) **OPTICAL TIP-TRACKING SYSTEMS AND METHODS THEREOF**

(71) Applicant: **Bard Access Systems, Inc.**, Salt Lake City, UT (US)

(72) Inventor: **Anthony K. Misener**, Bountiful, UT (US)

(73) Assignee: **Bard Access Systems, Inc.**, Salt Lake City, UT (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **18/383,809**

(22) Filed: **Oct. 25, 2023**

(65) **Prior Publication Data**
US 2024/0050708 A1 Feb. 15, 2024

Related U.S. Application Data

(63) Continuation of application No. 17/105,310, filed on Nov. 25, 2020, now Pat. No. 11,850,338.
(Continued)

(51) **Int. Cl.**
A61B 34/20 (2016.01)
A61M 25/09 (2006.01)

(52) **U.S. Cl.**
CPC **A61M 25/09** (2013.01); **A61B 34/20** (2016.02); **A61B 2034/2055** (2016.02); **A61M 2025/09175** (2013.01)

(58) **Field of Classification Search**
CPC ... A61B 5/06; A61B 34/20; A61B 2034/2055; A61B 5/064; A61B 5/0059; A61M 2025/09175

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,813,429 A 3/1989 Eshel et al.
5,099,845 A 3/1992 Besz et al.
(Continued)

FOREIGN PATENT DOCUMENTS

CN 101132730 A 2/2008
CN 111265309 A 6/2020
(Continued)

OTHER PUBLICATIONS

Mayoral et al. Fiber Optic Sensors for Vital Signs Monitoring. A Review of Its Practicality in the Health Field. Biosensors (Basel). Feb. 23, 2021;11(2):58. doi: 10.3390/bios11020058.
(Continued)

Primary Examiner — Amal Aly Farag
(74) *Attorney, Agent, or Firm* — Rutan & Tucker LLP

(57) **ABSTRACT**

An optical tip-tracking system is disclosed including a light-emitting stylet, a light detector, and a console configured to operably connect to the light-emitting stylet and the light detector. The light-emitting stylet can be disposed in a lumen of a catheter. The light-emitting stylet can include a light source in a distal-end portion of the light-emitting stylet configured to emit light. The light detector can be placed over a patient. The light detector can include a plurality of photodetectors configured to detect the light emitted from the light source. The console can be configured to instantiate an optical tip-tracking process for optically tracking the distal-end portion of the light-emitting stylet while the light-emitting stylet is disposed in a vasculature of the patient, the light source is emitting light, the light detector is disposed over the light-emitting stylet, and the photodetectors are detecting the light emitted from the light source.

20 Claims, 7 Drawing Sheets

Related U.S. Application Data

- (60) Provisional application No. 62/940,107, filed on Nov. 25, 2019.

References Cited

U.S. PATENT DOCUMENTS

- | | | | | | |
|--------------|---------|-----------------------|-----------------|---------|--------------------|
| 5,163,935 A | 11/1992 | Black et al. | 9,060,687 B2 | 6/2015 | Yamanaka et al. |
| 5,207,672 A | 5/1993 | Roth et al. | 9,114,226 B1 | 8/2015 | Lash et al. |
| 5,211,165 A | 5/1993 | Dumoulin et al. | 9,206,309 B2 | 12/2015 | Appleby et al. |
| 5,275,151 A | 1/1994 | Shockey et al. | 9,360,630 B2 | 6/2016 | Jenner et al. |
| 5,280,786 A | 1/1994 | Włodarczyk et al. | 9,504,392 B2 | 11/2016 | Caron et al. |
| 5,423,321 A | 6/1995 | Fontenot | 9,560,954 B2 | 2/2017 | Jacobs et al. |
| 5,454,807 A | 10/1995 | Lennox et al. | 9,622,706 B2 | 4/2017 | Dick et al. |
| 5,460,182 A | 10/1995 | Goodman et al. | 9,678,275 B1 | 6/2017 | Griffin |
| 5,517,997 A | 5/1996 | Fontenot | 10,231,753 B2 | 3/2019 | Burnside et al. |
| 5,622,170 A | 4/1997 | Schulz | 10,258,240 B1 | 4/2019 | Eberle et al. |
| 5,740,808 A | 4/1998 | Panescu et al. | 10,327,830 B2 | 6/2019 | Grant et al. |
| 5,841,131 A | 11/1998 | Schroeder et al. | 10,349,890 B2 | 7/2019 | Misener et al. |
| 5,872,879 A | 2/1999 | Hamm | 10,492,876 B2 | 12/2019 | Anastassiou et al. |
| 5,873,842 A | 2/1999 | Brennen et al. | 10,568,586 B2 | 2/2020 | Begin et al. |
| 5,879,306 A | 3/1999 | Fontenot et al. | 10,631,718 B2 | 4/2020 | Petroff et al. |
| 5,906,579 A | 5/1999 | Vander Salm et al. | 10,992,078 B2 | 4/2021 | Thompson et al. |
| 6,069,698 A | 5/2000 | Ozawa et al. | 11,123,047 B2 | 9/2021 | Jaffer et al. |
| 6,081,741 A | 6/2000 | Hollis | 11,525,670 B2 | 12/2022 | Messerly et al. |
| 6,178,346 B1 | 1/2001 | Amundson et al. | 2001/0014793 A1 | 8/2001 | Brugger et al. |
| 6,208,887 B1 | 3/2001 | Clarke | 2002/0198457 A1 | 12/2002 | Tearney et al. |
| 6,245,103 B1 | 6/2001 | Stinson | 2003/0092995 A1 | 5/2003 | Thompson |
| 6,319,227 B1 | 11/2001 | Mansouri-Ruiz | 2004/0129555 A1 | 7/2004 | Marchitto et al. |
| 6,343,227 B1 | 1/2002 | Crowley | 2004/0161362 A1 | 8/2004 | Bogert |
| 6,398,721 B1 | 6/2002 | Nakamura et al. | 2004/0242995 A1 | 12/2004 | Maschke |
| 6,485,482 B1 | 11/2002 | Belef | 2005/0033264 A1 | 2/2005 | Redinger |
| 6,564,089 B2 | 5/2003 | Izatt et al. | 2005/0163424 A1 | 7/2005 | Chen |
| 6,593,884 B1 | 7/2003 | Gilboa et al. | 2005/0261598 A1 | 11/2005 | Banet et al. |
| 6,597,941 B2 | 7/2003 | Fontenot et al. | 2005/0278010 A1 | 12/2005 | Richardson |
| 6,650,923 B1 | 11/2003 | Esh et al. | 2006/0013523 A1 | 1/2006 | Childers et al. |
| 6,673,214 B1 | 1/2004 | Marchitto et al. | 2006/0015136 A1 | 1/2006 | Besselink |
| 6,685,666 B1 | 2/2004 | Fontenot | 2006/0036164 A1 | 2/2006 | Wilson et al. |
| 6,687,010 B1 | 2/2004 | Horii et al. | 2006/0189959 A1 | 8/2006 | Schneiter |
| 6,690,966 B1 | 2/2004 | Rava et al. | 2006/0200049 A1 | 9/2006 | Leo et al. |
| 6,701,181 B2 | 3/2004 | Tang et al. | 2006/0241395 A1 | 10/2006 | Kruger et al. |
| 6,711,426 B2 | 3/2004 | Benaron et al. | 2006/0241492 A1 | 10/2006 | Boese et al. |
| 6,816,743 B2 | 11/2004 | Moreno et al. | 2007/0156019 A1 | 7/2007 | Larkin et al. |
| 6,892,090 B2 | 5/2005 | Verard et al. | 2007/0201793 A1 | 8/2007 | Askins et al. |
| 6,895,267 B2 | 5/2005 | Panescu et al. | 2007/0287886 A1 | 12/2007 | Saadat |
| 7,132,645 B2 | 11/2006 | Korn | 2007/0287934 A1 | 12/2007 | Babaev |
| 7,273,056 B2 | 9/2007 | Wilson et al. | 2007/0299425 A1 | 12/2007 | Waner et al. |
| 7,344,533 B2 | 3/2008 | Pearson et al. | 2008/0039715 A1 | 2/2008 | Wilson et al. |
| 7,366,562 B2 | 4/2008 | Dukesherer et al. | 2008/0077225 A1 | 3/2008 | Carlin et al. |
| 7,366,563 B2 | 4/2008 | Kleen et al. | 2008/0082004 A1 | 4/2008 | Banet et al. |
| 7,396,354 B2 | 7/2008 | Rychnovsky et al. | 2008/0172119 A1 | 7/2008 | Yamasaki et al. |
| 7,406,346 B2 | 7/2008 | Kleen et al. | 2008/0183128 A1 | 7/2008 | Morriss et al. |
| 7,515,265 B2 | 4/2009 | Alfano et al. | 2008/0212082 A1 | 9/2008 | Froggatt et al. |
| 7,532,920 B1 | 5/2009 | Ainsworth et al. | 2008/0285909 A1 | 11/2008 | Younge et al. |
| 7,587,236 B2 | 9/2009 | Demos et al. | 2008/0319290 A1 | 12/2008 | Mao et al. |
| 7,603,166 B2 | 10/2009 | Casscells, III et al. | 2009/0054908 A1 | 2/2009 | Zand et al. |
| 7,729,735 B1 | 6/2010 | Burchman | 2009/0062634 A1 | 3/2009 | Say et al. |
| 7,757,695 B2 | 7/2010 | Wilson et al. | 2009/0118612 A1 | 5/2009 | Grunwald et al. |
| 7,758,499 B2 | 7/2010 | Adler | 2009/0137952 A1 | 5/2009 | Ramamurthy et al. |
| 7,840,253 B2 | 11/2010 | Tremblay et al. | 2009/0234328 A1 | 9/2009 | Cox et al. |
| 7,992,573 B2 | 8/2011 | Wilson et al. | 2009/0304582 A1 | 12/2009 | Rouso et al. |
| 8,032,200 B2 | 10/2011 | Tearney et al. | 2009/0314925 A1 | 12/2009 | Van Vorhis et al. |
| 8,054,469 B2 | 11/2011 | Nakabayashi et al. | 2010/0016729 A1 | 1/2010 | Futrell |
| 8,060,187 B2 | 11/2011 | Marshik-Geurts et al. | 2010/0030063 A1 | 2/2010 | Lee et al. |
| 8,073,517 B1 | 12/2011 | Burchman | 2010/0030132 A1 | 2/2010 | Niezgoda et al. |
| 8,078,261 B2 | 12/2011 | Imam | 2010/0063534 A1 | 3/2010 | Kugler et al. |
| 8,187,189 B2 | 5/2012 | Jung et al. | 2010/0114115 A1 | 5/2010 | Schlesinger et al. |
| 8,267,932 B2 | 9/2012 | Baxter et al. | 2010/0286531 A1 | 11/2010 | Ryan et al. |
| 8,369,932 B2 | 2/2013 | Cinbis et al. | 2010/0312095 A1 | 12/2010 | Jenkins et al. |
| 8,388,541 B2 | 3/2013 | Messerly et al. | 2011/0060229 A1 | 3/2011 | Hulvershorn et al. |
| 8,571,640 B2 | 10/2013 | Holman | 2011/0090486 A1 | 4/2011 | Udd |
| 8,597,315 B2 | 12/2013 | Snow et al. | 2011/0144481 A1 | 6/2011 | Feer et al. |
| 8,700,358 B1 | 4/2014 | Parker, Jr. | 2011/0166442 A1 | 7/2011 | Sarvazy |
| 8,781,555 B2 | 7/2014 | Burnside et al. | 2011/0172591 A1 | 7/2011 | Babaev |
| 8,798,721 B2 | 8/2014 | Dib | 2011/0172680 A1 | 7/2011 | Younge et al. |
| 8,968,331 B1 | 3/2015 | Sochor | 2011/0237958 A1 | 9/2011 | Onimura |
| 8,979,871 B2 | 3/2015 | Tyc et al. | 2011/0242532 A1 | 10/2011 | McKenna |
| | | | 2011/0245662 A1 | 10/2011 | Eggers et al. |
| | | | 2011/0288405 A1 | 11/2011 | Razavi et al. |
| | | | 2011/0295108 A1 | 12/2011 | Cox et al. |
| | | | 2011/0313280 A1 | 12/2011 | Govari et al. |
| | | | 2012/0046562 A1 | 2/2012 | Powers et al. |
| | | | 2012/0065481 A1 | 3/2012 | Hunter et al. |
| | | | 2012/0101413 A1 | 4/2012 | Beetel et al. |
| | | | 2012/0136242 A1 | 5/2012 | Qi et al. |
| | | | 2012/0143029 A1 | 6/2012 | Silverstein et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0184827	A1	7/2012	Shwartz et al.	2019/0110844	A1	4/2019	Misener et al.
2012/0184955	A1	7/2012	Pivotto et al.	2019/0231272	A1	8/2019	Yamaji
2012/0283747	A1	11/2012	Popovic	2019/0237902	A1	8/2019	Thompson et al.
2012/0289783	A1	11/2012	Duindam et al.	2019/0247132	A1	8/2019	Harks et al.
2012/0321243	A1	12/2012	Younge et al.	2019/0307331	A1	10/2019	Saadat et al.
2013/0028554	A1	1/2013	Wong et al.	2019/0321110	A1	10/2019	Grunwald et al.
2013/0072943	A1	3/2013	Parmar	2019/0343424	A1	11/2019	Blumenkranz et al.
2013/0096482	A1	4/2013	Bertrand et al.	2019/0343702	A1	11/2019	Smith
2013/0104884	A1	5/2013	Vazales et al.	2019/0357875	A1	11/2019	QI et al.
2013/0188855	A1	7/2013	Desjardins et al.	2019/0365199	A1	12/2019	Zhao et al.
2013/0204124	A1	8/2013	Duindam et al.	2019/0374130	A1	12/2019	Bydilon et al.
2013/0211246	A1	8/2013	Parasher	2020/0000526	A1	1/2020	Zhao
2013/0296693	A1	11/2013	Wenzel et al.	2020/0030575	A1	1/2020	Bogusky et al.
2013/0310668	A1	11/2013	Young	2020/0046434	A1	2/2020	Graetzel et al.
2013/0317372	A1	11/2013	Eberle et al.	2020/0054399	A1	2/2020	Duindam et al.
2013/0324840	A1	12/2013	Zhongping et al.	2020/0121482	A1	4/2020	Spector et al.
2014/0121468	A1	5/2014	Eichenholz	2020/0188036	A1	6/2020	Ding et al.
2014/0221829	A1	8/2014	Maitland et al.	2020/0297442	A1	9/2020	Adebar et al.
2014/0275997	A1	9/2014	Chopra et al.	2020/0305983	A1	10/2020	Yampolsky et al.
2015/0029511	A1	1/2015	Hooft et al.	2020/0315770	A1	10/2020	Dupont et al.
2015/0031987	A1	1/2015	Pameijer et al.	2020/0394789	A1	12/2020	Freund et al.
2015/0080688	A1	3/2015	Cinbis et al.	2021/0015470	A1	1/2021	Prisco et al.
2015/0099979	A1	4/2015	Caves et al.	2021/0023341	A1	1/2021	Decheek et al.
2015/0119700	A1	4/2015	Liang et al.	2021/0045814	A1	2/2021	Thompson et al.
2015/0124264	A1	5/2015	Ramachandran et al.	2021/0068911	A1	3/2021	Walker et al.
2015/0141854	A1	5/2015	Eberle et al.	2021/0100627	A1	4/2021	Soper et al.
2015/0164571	A1	6/2015	Saadat	2021/0244311	A1	8/2021	Zhao et al.
2015/0190221	A1	7/2015	Schaefer et al.	2021/0268229	A1	9/2021	Sowards et al.
2015/0209113	A1	7/2015	Burkholz et al.	2021/0271035	A1	9/2021	Sowards et al.
2015/0209117	A1	7/2015	Flexman et al.	2021/0275257	A1	9/2021	Prior et al.
2015/0254526	A1	9/2015	Denissen	2021/0298680	A1	9/2021	Sowards et al.
2015/0320977	A1	11/2015	Vitullo et al.	2021/0330399	A1	10/2021	Netravali et al.
2016/0018602	A1	1/2016	Govari et al.	2021/0401456	A1	12/2021	Cox et al.
2016/0067449	A1	3/2016	Misener et al.	2021/0401509	A1	12/2021	Misener et al.
2016/0102969	A1	4/2016	Verstege et al.	2021/0402144	A1	12/2021	Messerly
2016/0166326	A1	6/2016	Bakker et al.	2022/0011192	A1	1/2022	Misener et al.
2016/0166341	A1	6/2016	Iordachita et al.	2022/0034733	A1	2/2022	Misener et al.
2016/0184020	A1	6/2016	Kowalewski et al.	2022/0079683	A1	3/2022	Bydilon et al.
2016/0213432	A1	7/2016	Flexman et al.	2022/0096796	A1	3/2022	McLaughlin et al.
2016/0331461	A1*	11/2016	Cheatham, III	2022/0110508	A1	4/2022	Van Roosbroeck et al.
2016/0349044	A1	12/2016	Marell et al.	2022/0110695	A1	4/2022	Sowards et al.
2016/0354038	A1	12/2016	Demirtas et al.	2022/0151568	A1	5/2022	Yao et al.
2017/0020394	A1	1/2017	Harrington	2022/0152349	A1	5/2022	Sowards et al.
2017/0079681	A1	3/2017	Burnside et al.	2022/0160209	A1	5/2022	Sowards et al.
2017/0082806	A1	3/2017	Van Der Mark et al.	2022/0172354	A1	6/2022	Misener et al.
2017/0151027	A1	6/2017	Walker et al.	2022/0211442	A1	7/2022	McLaughlin et al.
2017/0173349	A1	6/2017	Pfleiderer et al.	2022/0233246	A1	7/2022	Misener et al.
2017/0196479	A1	7/2017	Liu et al.	2022/0369934	A1	11/2022	Sowards et al.
2017/0201036	A1	7/2017	Cohen et al.	2023/0081198	A1	3/2023	Sowards et al.
2017/0215973	A1	8/2017	Flexman et al.	2023/0097431	A1	3/2023	Sowards et al.
2017/0231699	A1	8/2017	Flexman et al.	2023/0101030	A1	3/2023	Misener et al.
2017/0273542	A1	9/2017	Au	2023/0108604	A1	4/2023	Messerly et al.
2017/0273565	A1	9/2017	Ma et al.	2023/0126813	A1	4/2023	Sowards et al.
2017/0273628	A1	9/2017	Ofek et al.	2023/0243715	A1	8/2023	Misener et al.
2017/0290563	A1	10/2017	Cole et al.	2023/0248444	A1	8/2023	Misener et al.
2017/0311901	A1	11/2017	Zhao et al.	2023/0251150	A1	8/2023	Misener et al.
2017/0319279	A1	11/2017	Fish et al.	2023/0337985	A1	10/2023	Sowards et al.
2018/0008443	A1	1/2018	Cole et al.	2023/0346479	A1	11/2023	Muller et al.
2018/0031493	A1	2/2018	Tojo et al.	2023/0414112	A1	12/2023	Misener et al.
2018/0095231	A1	4/2018	Lowell et al.	2024/0000515	A1	1/2024	Misener et al.
2018/0113038	A1	4/2018	Janabi-Sharifi et al.	2024/0099659	A1	3/2024	Sowards et al.
2018/0116551	A1	5/2018	Newman et al.	2024/0108856	A1	4/2024	Messerly
2018/0140170	A1	5/2018	Van Putten et al.	2024/0216077	A1	7/2024	Thompson et al.
2018/0235709	A1	8/2018	Donhowe et al.	2024/0335237	A1	10/2024	Sowards et al.
2018/0239124	A1	8/2018	Naruse et al.	2024/0353275	A1	10/2024	Misener et al.
2018/0240237	A1	8/2018	Donhowe et al.	2024/0383133	A1	11/2024	Bydilon et al.
2018/0250088	A1	9/2018	Brennan et al.	2024/0390644	A1	11/2024	McLaughlin et al.
2018/0264227	A1	9/2018	Flexman et al.	2025/0020453	A1	1/2025	Thompson et al.
2018/0279909	A1	10/2018	Noonan et al.	2025/0060266	A1	2/2025	Messerly
2018/0289390	A1	10/2018	Amorizzo et al.	2025/0186135	A1	6/2025	McLaughlin et al.
2018/0289927	A1	10/2018	Messerly				
2018/0339134	A1	11/2018	Leo				
2018/0360545	A1	12/2018	Cole et al.				
2019/0059743	A1	2/2019	Ramachandran et al.				
2019/0060003	A1	2/2019	Tuason				

FOREIGN PATENT DOCUMENTS

CN	113080937	A	7/2021
DE	102016109601	A1	11/2017
EP	2240111	A2	10/2010
EP	2907445	A1	8/2015
EP	3545849	A1	10/2019
EP	3705020	A1	9/2020

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	7366562	B2	10/2023
KR	20190098512	A	8/2019
WO	9964099	A1	12/1999
WO	2006113394	A2	10/2006
WO	2006122001	A2	11/2006
WO	2007002323	A2	1/2007
WO	2009155325	A2	12/2009
WO	2011121516	A2	10/2011
WO	2011141830	A1	11/2011
WO	2011150376	A1	12/2011
WO	2012064769	A2	5/2012
WO	2015044930	A1	4/2015
WO	2015074045	A2	5/2015
WO	2016038492	A1	3/2016
WO	2016051302	A1	4/2016
WO	2016061431	A1	4/2016
WO	2016149819	A1	9/2016
WO	2018096491	A1	5/2018
WO	2019037071	A1	2/2019
WO	2019046769	A1	3/2019
WO	2019070423	A1	4/2019
WO	2019230713	A1	12/2019
WO	2020182997	A1	9/2020
WO	2021030092	A1	2/2021
WO	2021108688	A1	6/2021
WO	2021108697	A1	6/2021
WO	2021138096	A1	7/2021
WO	2021216089	A1	10/2021
WO	2022031613	A1	2/2022
WO	2022081723	A1	4/2022
WO	2022150411	A1	7/2022
WO	2022164902	A1	8/2022
WO	2022245987	A1	11/2022
WO	2023043954	A1	3/2023
WO	2023049443	A1	3/2023
WO	2023055810	A1	4/2023
WO	2023076143	A1	5/2023
WO	2023211752	A1	11/2023
WO	2024006384	A1	1/2024
WO	2024006441	A1	1/2024
WO	2024064334	A1	3/2024
WO	2024215665	A1	10/2024

OTHER PUBLICATIONS

P.J. de Feyter, P. Kay, C. Disco, P.W. Serruys, "Reference chart derived from post-stent-implantation intravascular ultrasound predictors of 6-month expected restenosis on quantitative coronary angiography." *Circulation*. vol. 100, No. 17 (Year: 1999).

U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Advisory Action dated Nov. 6, 2024.

U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Final Office Action dated Aug. 27, 2024.

U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Non-Final Office Action dated Dec. 4, 2024.

U.S. Appl. No. 17/569,350, filed Jan. 5, 2022 Notice of Allowance dated Nov. 7, 2024.

U.S. Appl. No. 17/585,219, filed Jan. 26, 2022 Restriction Requirement dated Dec. 2, 2024.

U.S. Appl. No. 17/728,802, filed Apr. 25, 2022 Non-Final Office Action dated Aug. 28, 2024.

U.S. Appl. No. 17/852,138, filed Jun. 28, 2022 Non-Final Office Action dated Sep. 18, 2024.

U.S. Appl. No. 17/853,590, filed Jun. 29, 2022 Non-Final Office Action dated Oct. 17, 2024.

U.S. Appl. No. 17/955,019, filed Sep. 28, 2022 Non-Final Office Action dated Sep. 27, 2024.

U.S. Appl. No. 18/132,623, filed Apr. 10, 2023, Final Office Action dated Sep. 6, 2024.

U.S. Appl. No. 18/132,623, filed Apr. 10, 2023, Notice of Allowance dated Nov. 19, 2024.

U.S. Appl. No. 18/607,144, filed Mar. 15, 2024 Non-Final Office Action dated Sep. 24, 2024.

U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Notice of Allowance dated Jul. 16, 2024.

U.S. Appl. No. 17/569,350, filed Jan. 5, 2022 Advisory Action dated Jul. 12, 2024.

U.S. Appl. No. 17/747,903, filed May 18, 2022 Non-Final Office Action dated Aug. 15, 2024.

U.S. Appl. No. 17/747,903, filed May 18, 2022 Restriction Requirement dated May 28, 2024.

U.S. Appl. No. 17/955,019, filed Sep. 28, 2022 Restriction Requirement dated Jun. 6, 2024.

U.S. Appl. No. 18/079,653, filed Dec. 12, 2022 Notice of Allowance dated Jun. 4, 2024.

U.S. Appl. No. 18/132,231, filed Apr. 7, 2023 Non-Final Office Action dated Jul. 12, 2024.

U.S. Appl. No. 18/538,111, filed Dec. 13, 2023 Non-Final Office Action dated Aug. 9, 2024.

U.S. Appl. No. 17/569,350, filed Jan. 5, 2022 Non-Final Office Action dated Aug. 12, 2024.

U.S. Appl. No. 17/971,873, filed Oct. 24, 2022 Non-Final Office Action dated Jun. 6, 2024.

EP 20853352.1 filed Mar. 7, 2022 Extended European Search Report dated Jul. 27, 2023.

Fiber Optic RealShape (FORS) technology—research. Philips. (Oct. 18, 2018). Retrieved Feb. 28, 2023, from <https://www.philips.com/a-w/research/research-programs/fors.html> (Year: 2018).

Jackle Sonja et al. "Three-dimensional guidance including shape sensing of a stentgraft system for endovascular aneurysm repair." *International Journal of Computer Assisted Radiology and Surgery*, Springer DE. vol. 15, No. 6, May 7, 2020.

PCT/US2018/026493 filed Apr. 6, 2018 International Search Report and Written Opinion dated Jun. 22, 2018.

PCT/US2020/044801 filed Aug. 3, 2020 International Search Report and Written Opinion dated Oct. 26, 2020.

PCT/US2020/062396 filed Nov. 25, 2020 International Preliminary Report on Patentability dated Jan. 29, 2021.

PCT/US2020/062396 filed Nov. 25, 2020 International Search Report and Written Opinion dated Mar. 2, 2021.

PCT/US2020/062407 filed Nov. 25, 2020 International Preliminary Report on Patentability dated Jan. 25, 2021.

PCT/US2020/062407 filed Nov. 25, 2020 International Search Report and Written Opinion dated Mar. 11, 2021.

PCT/US2021/038899 filed Jun. 24, 2021 International Search Report and Written Opinion dated Oct. 6, 2021.

PCT/US2021/038954 filed Jun. 24, 2021 International Search Report and Written Opinion dated Oct. 28, 2021.

PCT/US2021/041128 filed Jul. 9, 2021 International Search Report and Written Opinion dated Oct. 25, 2021.

PCT/US2021/044216 filed Aug. 2, 2021 International Search Report and Written Opinion dated Nov. 18, 2021.

PCT/US2021/052046 filed Sep. 24, 2021 International Search Report and Written Opinion dated Jan. 11, 2022.

PCT/US2021/054802 filed Oct. 13, 2021 International Search Report and Written Opinion dated Feb. 2, 2022.

PCT/US2022/011347 filed Jan. 5, 2022 International Search Report and Written Opinion dated May 3, 2022.

PCT/US2022/013897 filed Jan. 26, 2022 International Search Report and Written Opinion dated May 11, 2022.

PCT/US2022/029894 filed May 18, 2022, International Search Report and Written Opinion dated Sep. 1, 2022.

PCT/US2022/043706 filed Sep. 16, 2022 International Search Report and Written Opinion dated Nov. 24, 2022.

PCT/US2022/044696 filed Sep. 26, 2022 International Search Report and Written Opinion dated Jan. 23, 2023.

PCT/US2022/045051 filed Sep. 28, 2022 International Search Report and Written Opinion dated Jan. 2, 2023.

PCT/US2022/047538 filed Oct. 24, 2022 International Search Report and Written Opinion dated Jan. 26, 2023.

PCT/US2023/019239 filed Apr. 20, 2023 International Search Report and Written Opinion dated Jul. 20, 2023.

PCT/US2023/026487 filed Jun. 28, 2023 International Search Report and Written Opinion dated Sep. 6, 2023.


(56)


References Cited**OTHER PUBLICATIONS**



U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Examiner's Answer dated November 28, 2022.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Final Office Action dated Apr. 22, 2022.
 U.S. Appl. No. 16/984,104, filed Aug. 3, 2020 Final Office Action dated Sep. 21, 2023.
 U.S. Appl. No. 16/984,104, filed Aug. 3, 2020 Non-Final Office Action dated Jun. 22, 2023.
 U.S. Appl. No. 16/984,104, filed Aug. 3, 2020 Restriction Requirement dated Mar. 13, 2023.
 U.S. Appl. No. 17/105,310, filed Nov. 25, 2020, Notice of Allowance dated Jul. 20, 2022.
 U.S. Appl. No. 17/105,310, filed Nov. 25, 2020 Non-Final Office Action dated Feb. 22, 2023.
 U.S. Appl. No. 17/105,310, filed Nov. 25, 2020 Notice of Allowance dated Aug. 2, 2023.
 U.S. Appl. No. 17/357,186, filed Jun. 24, 2021 Non Final Office Action dated May 30, 2023.
 U.S. Appl. No. 17/357,186, filed Jun. 24, 2021 Notice of Allowance dated Aug. 23, 2023.
 U.S. Appl. No. 17/357,186, filed Jun. 24, 2021 Restriction Requirement dated Mar. 7, 2023.
 U.S. Appl. No. 17/357,561, filed Jun. 24, 2021 Non-Final Office Action dated Aug. 11, 2022.
 U.S. Appl. No. 17/357,561, filed Jun. 24, 2021 Notice of Allowance dated Dec. 9, 2022.
 U.S. Appl. No. 17/371,993, filed Jul. 9, 2021 Non-Final Office Action dated Jul. 12, 2022.
 U.S. Appl. No. 17/371,993, filed Jul. 9, 2021 Notice of Allowance dated Nov. 3, 2022.
 U.S. Appl. No. 17/392,002, filed Aug. 2, 2021, Corrected Notice of Allowability dated Feb. 23, 2023.
 U.S. Appl. No. 17/392,002, filed Aug. 2, 2021, Non-Final Office Action dated Sep. 12, 2022.
 U.S. Appl. No. 17/392,002, filed Aug. 2, 2021, Notice of Allowance dated Jan. 19, 2023.
 U.S. Appl. No. 17/484,960, filed Sep. 24, 2021 Non-Final Office Action dated Oct. 5, 2023.
 U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Final Office Action dated Sep. 21, 2023.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Final Office Action dated Jun. 30, 2021.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Final Office Action dated Nov. 10, 2020.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Non-Final Office Action dated Mar. 12, 2021.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Non-Final Office Action dated May 29, 2020.
 U.S. Appl. No. 15/947,267, filed Apr. 6, 2018 Non-Final Office Action dated Oct. 13, 2021.
 U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Non-Final Office Action dated Mar. 15, 2023.
 Dziuda L et al: "Monitoring Respiration and Cardiac Activity Using Fiber Bragg Grating-Based Sensor", IEEE Transactions on Bio-medical Engineering vol. 59, No. 7, Jul. 2012 pp. 1934-1942.
 Dziuda L. et al: "Fiber-optic sensor for monitoring respiration and cardiac activity", 2011 IEEE Sensors Proceedings : Limerick, Ireland, Oct. 2011 pp. 413-416.
 EP 20893677.3 filed Jun. 22, 2022 Extended European Search Report dated Oct. 13, 2023.
 EP 20894633.5 filed Jun. 22, 2022 Extended European Search Report dated Oct. 16, 2023.
 PCT/US2023/026581 filed Jun. 29, 2023 International Search Report and Written Opinion dated Oct. 27, 2023.
 PCT/US2023/033471 filed Sep. 22, 2023 International Search Report and Written Opinion dated Dec. 21, 2023.

U.S. Appl. No. 16/984,104, filed Aug. 3, 2020 Notice of Allowance dated Nov. 21, 2023.
 U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Advisory Action dated Dec. 7, 2023.
 U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Non-Final Office Action dated Jan. 19, 2024.
 U.S. Appl. No. 18/135,337, filed Apr. 17, 2023 Non-Final Office Action dated Dec. 22, 2023.
 U.S. Appl. No. 17/569,350, filed Jan. 5, 2022 Non-Final Office Action dated Jan. 8, 2024.
 U.S. Appl. No. 17/484,960, filed Sep. 24, 2021 Notice of Allowance dated Apr. 12, 2024.
 U.S. Appl. No. 17/569,350, filed Jan. 5, 2022 Final Office Action dated Apr. 23, 2024.
 U.S. Appl. No. 18/079,653, filed Dec. 12, 2022 Non-Final Office Action dated Feb. 6, 2024.
 U.S. Appl. No. 18/132,623, filed Apr. 10, 2023, Non-Final Office Action dated May 3, 2024.
 U.S. Appl. No. 18/135,337, filed Apr. 17, 2023 Notice of Allowance dated Mar. 8, 2024.
 PCT/US2023/026581 filed Jun. 29, 2023 International Preliminary Report on Patentability dated Dec. 18, 2024.
 U.S. Appl. No. 17/585,219, filed Jan. 26, 2022 Non-Final Office Action dated Feb. 27, 2025.
 U.S. Appl. No. 17/728,802, filed Apr. 25, 2022 Final Office Action dated Jan. 17, 2025.
 U.S. Appl. No. 17/747,903, filed May 18, 2022 Final Office Action dated Jan. 27, 2025.
 U.S. Appl. No. 17/852,138, filed Jun. 28, 2022 Notice of Allowance dated Feb. 12, 2025.
 U.S. Appl. No. 17/853,590, filed Jun. 29, 2022 Notice of Allowance dated Mar. 5, 2025.
 U.S. Appl. No. 17/952,645, filed Sep. 26, 2022 Non-Final Office Action dated Feb. 28, 2025.
 U.S. Appl. No. 17/955,019, filed Sep. 28, 2022 Final Office Action dated Feb. 4, 2025.
 U.S. Appl. No. 17/971,873, filed Oct. 24, 2022 Non-Final Office Action dated Dec. 27, 2024.
 U.S. Appl. No. 18/132,231, filed Apr. 7, 2023 Final Office Action dated Jan. 31, 2025.
 U.S. Appl. No. 18/538,111, filed Dec. 13, 2023 Final Office Action dated Feb. 4, 2025.
 U.S. Appl. No. 18/607,144, filed Mar. 15, 2024 Final Office Action dated Feb. 19, 2025.
 Ogawa, K.; Koyama, S.; Ishizawa, H.; Fujiwara, S.; Fujimoto, K. Simultaneous Measurement of Heart Sound, PulseWave and Respiration with Single Fiber Bragg Grating Sensor. In Proceedings of the 2018 IEEE International Symposium on Medical Measurements and Applications (MeMeA), Rome, Italy, Jun. 11-13, 2018.
 U.S. Appl. No. 17/500,678, filed Oct. 13, 2021 Final Office Action dated Jun. 11, 2025.
 U.S. Appl. No. 17/728,802, filed Apr. 25, 2022 Advisory Action dated Apr. 4, 2025.
 U.S. Appl. No. 17/728,802, filed Apr. 25, 2022 Non-Final Office Action dated May 19, 2025.
 U.S. Appl. No. 17/747,903, filed May 18, 2022 Advisory Action dated Apr. 22, 2025.
 U.S. Appl. No. 17/955,019, filed Sep. 28, 2022 Advisory Action dated Apr. 16, 2025.
 U.S. Appl. No. 18/132,231, filed Apr. 7, 2023 Notice of Allowance dated Apr. 10, 2025.
 U.S. Appl. No. 18/132,891, filed Apr. 10, 2023 Restriction Requirement dated Jun. 2, 2025.
 U.S. Appl. No. 18/538,111, filed Dec. 13, 2023 Notice of Allowance dated Apr. 23, 2025.
 U.S. Appl. No. 18/607,144, filed Mar. 15, 2024 Notice of Allowance dated Apr. 5, 2025.

* cited by examiner

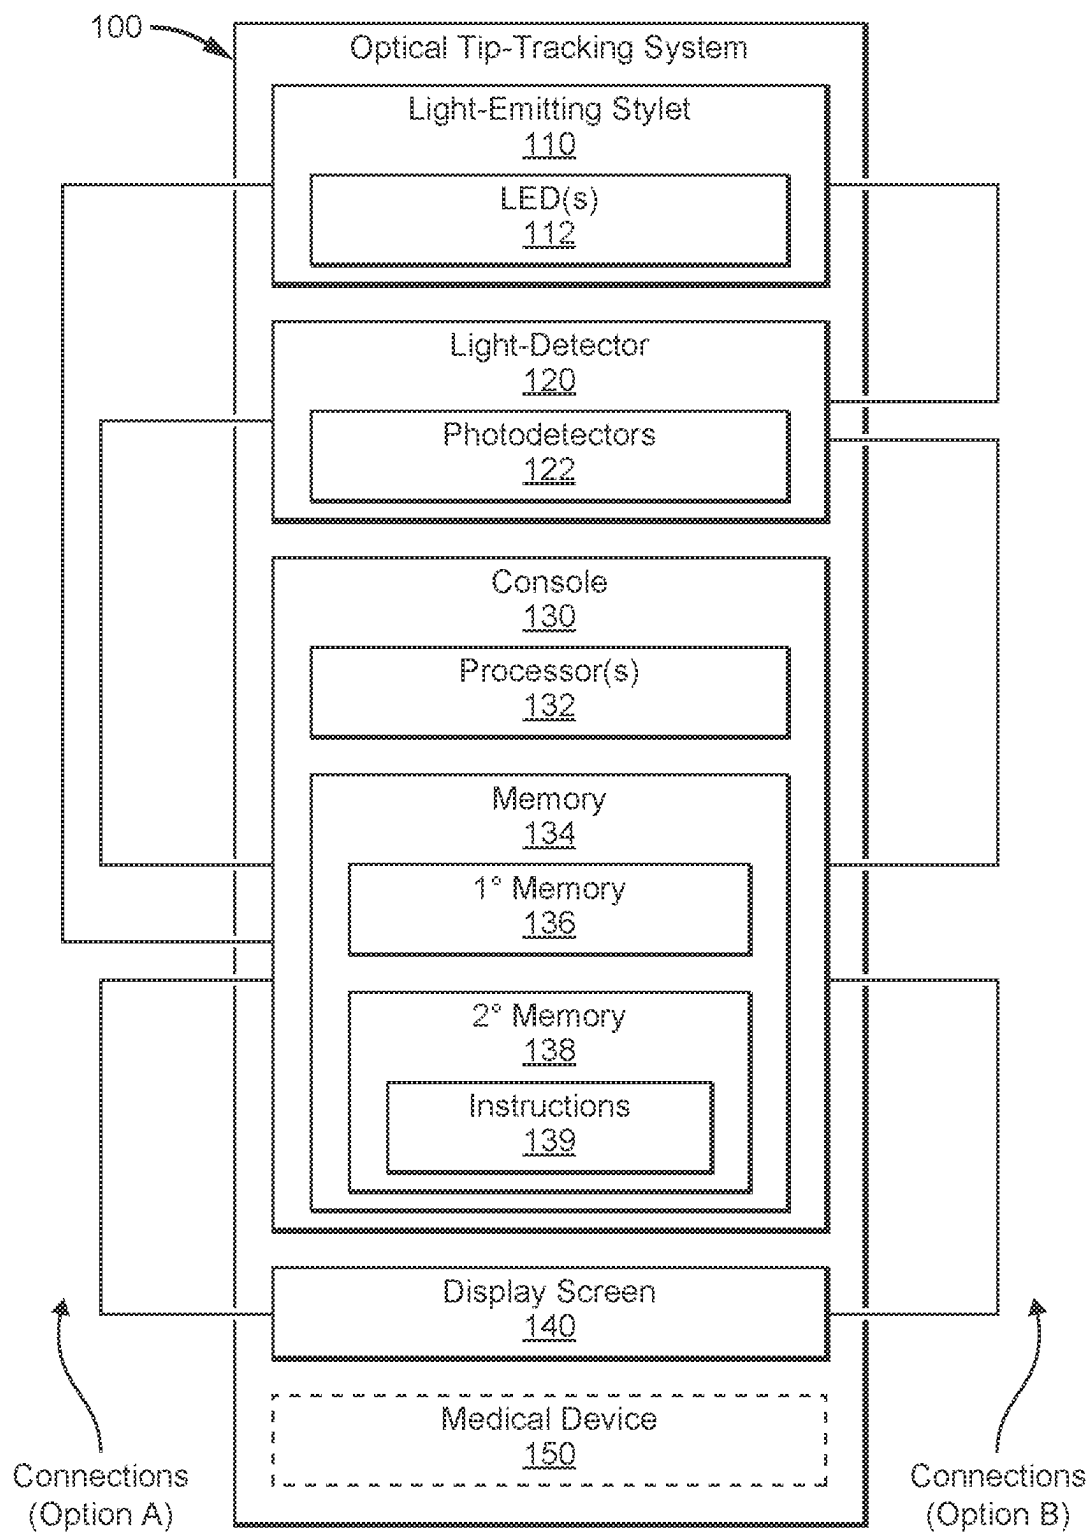*FIG. 1*

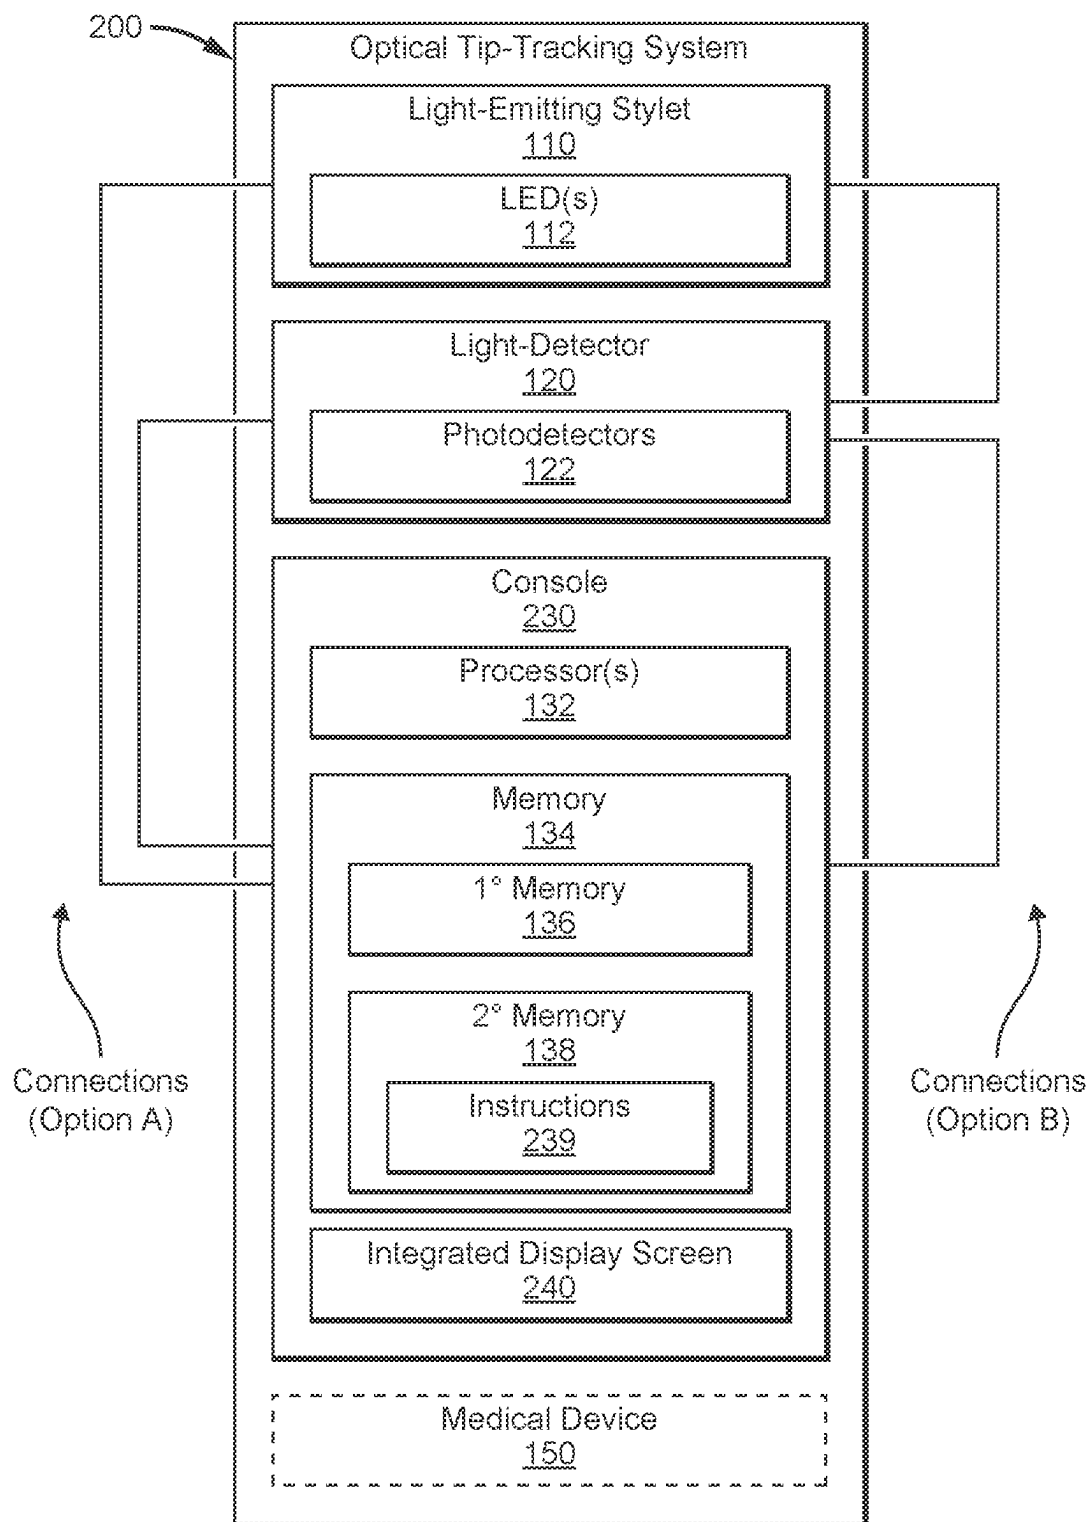**FIG. 2**

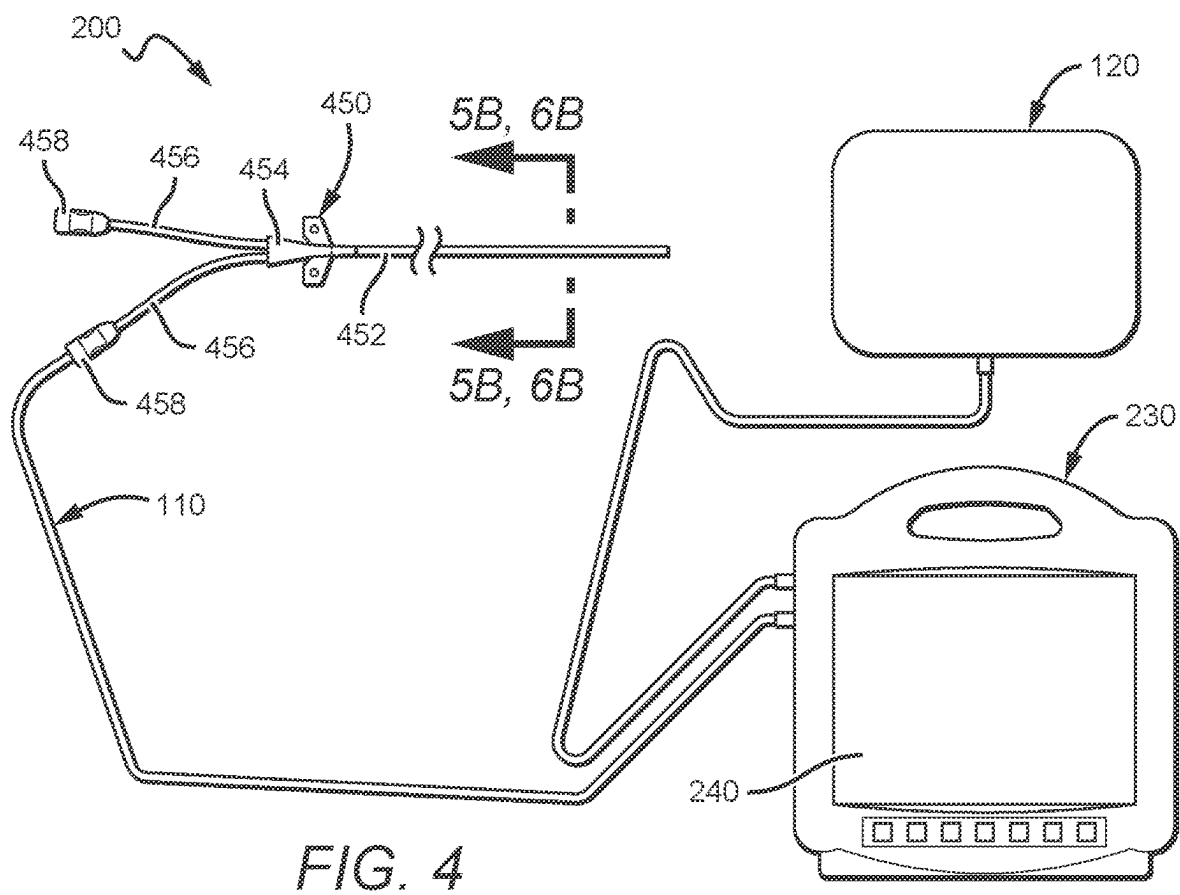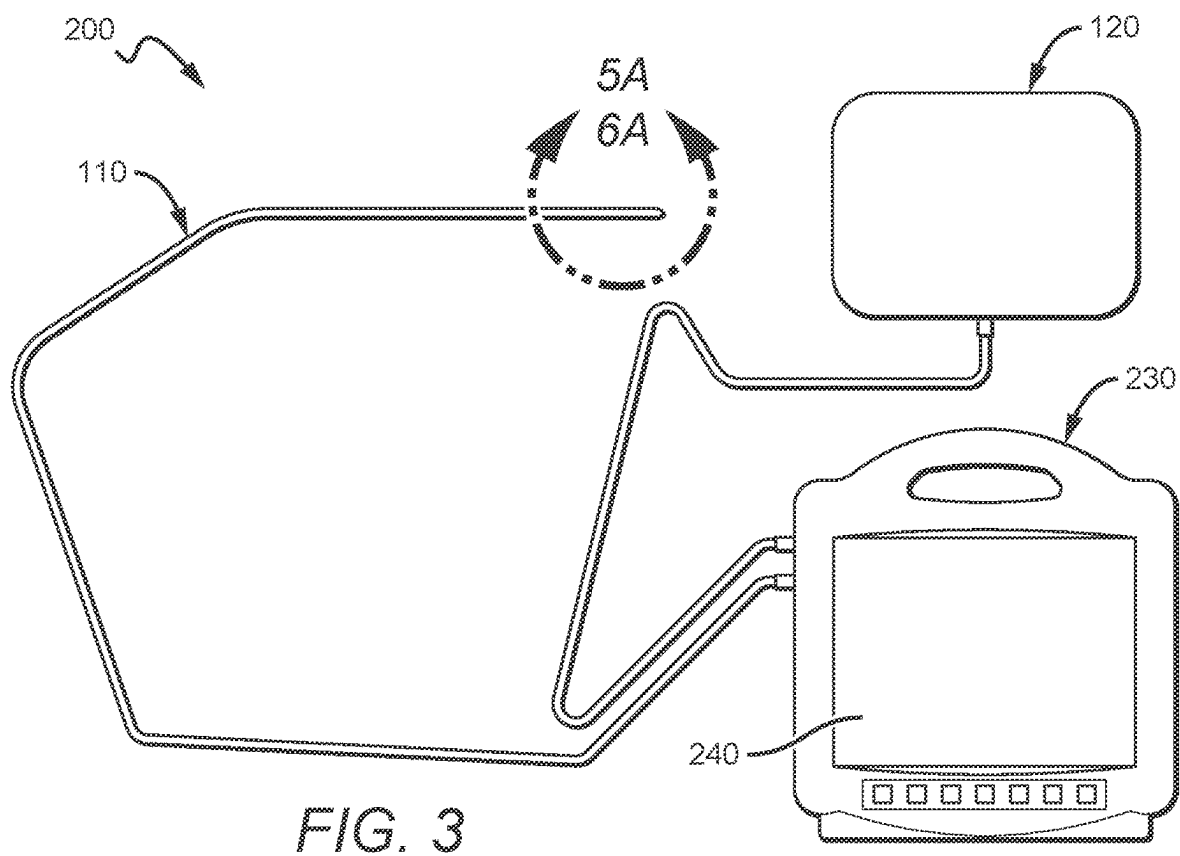

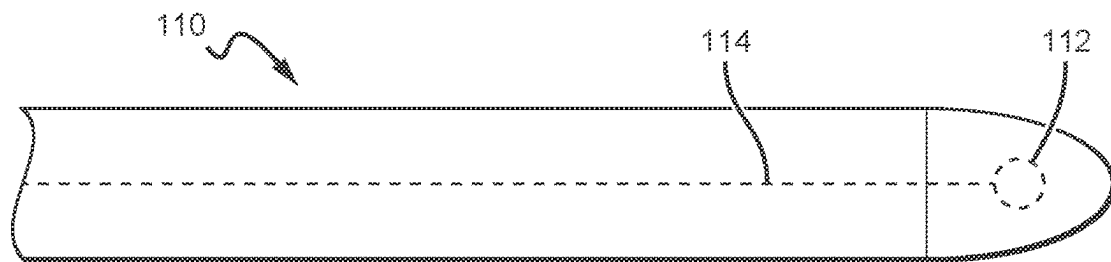


FIG. 5A

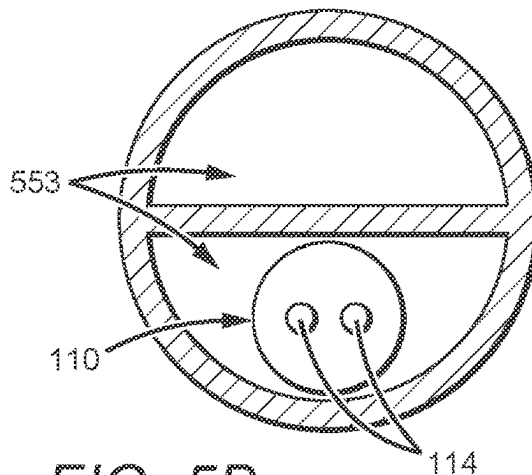


FIG. 5B

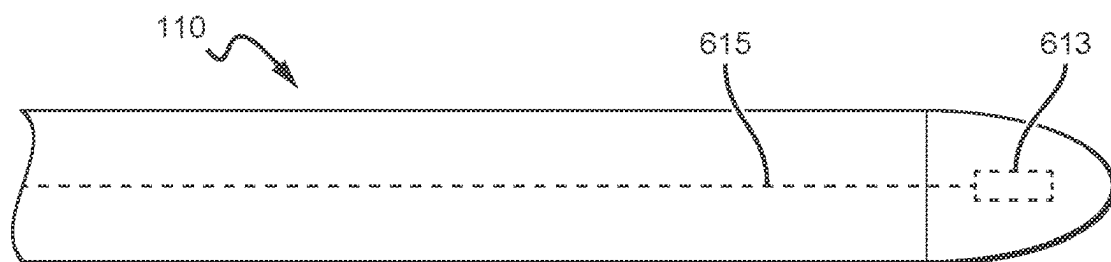


FIG. 6A

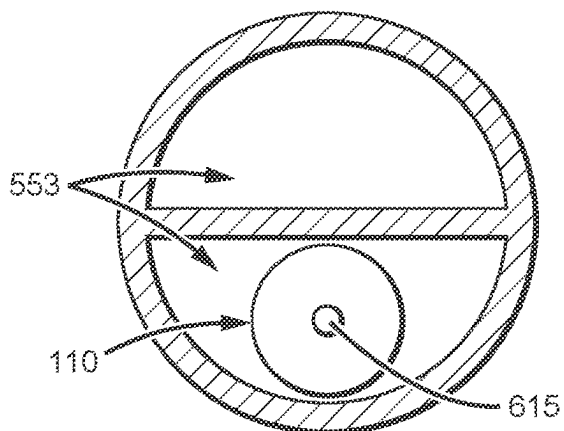


FIG. 6B

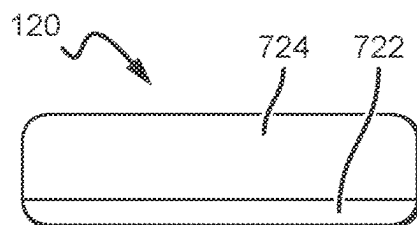


FIG. 7

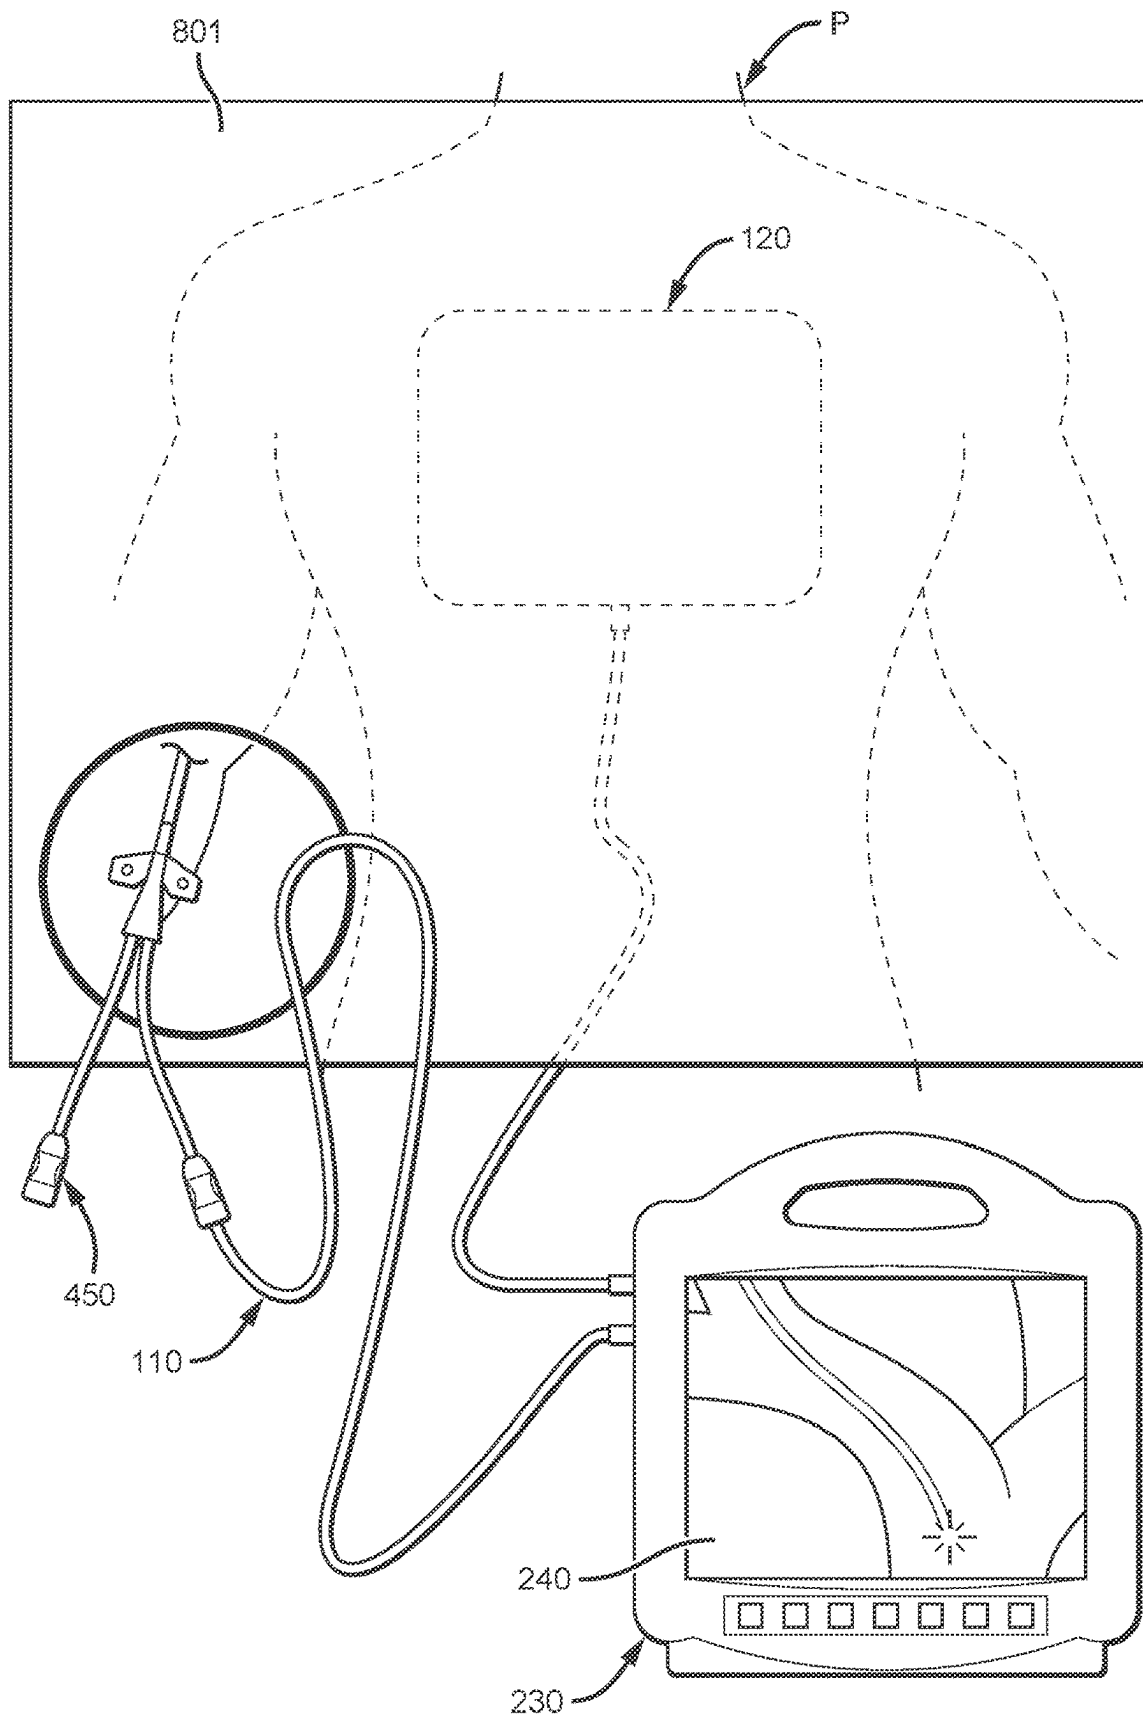


FIG. 8

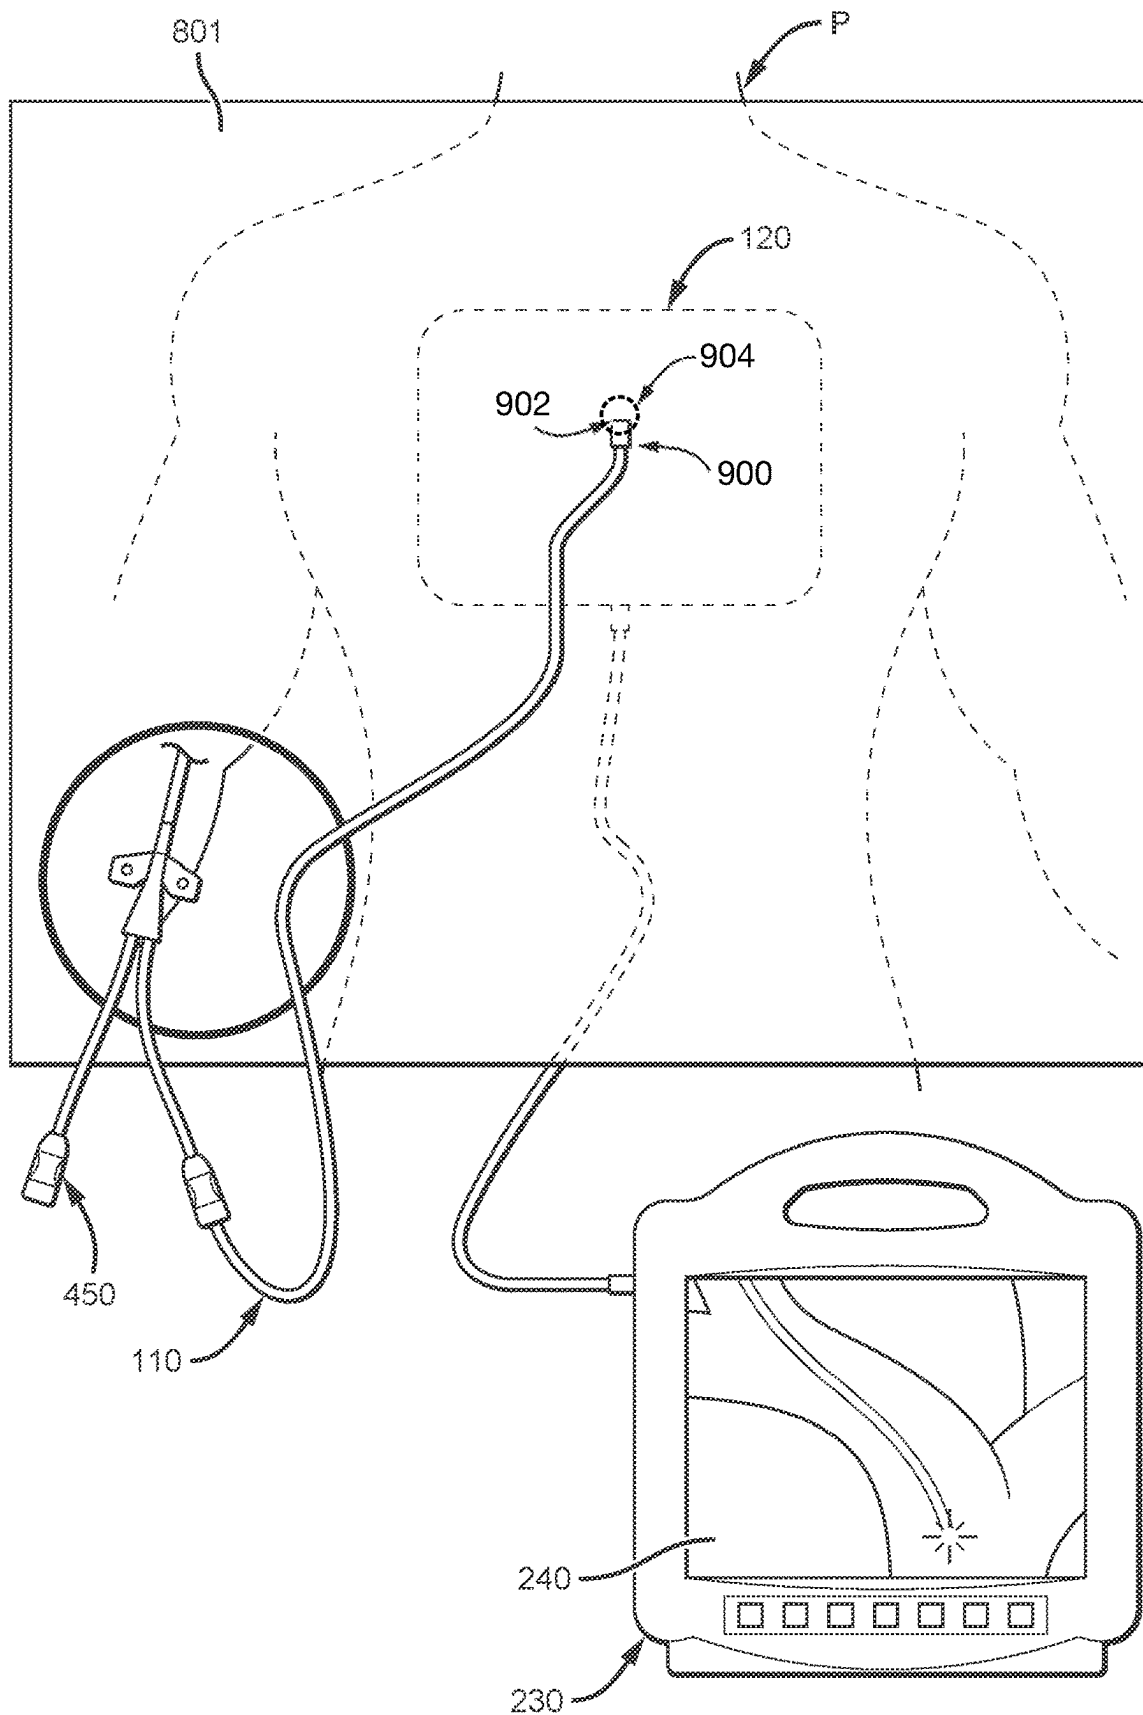


FIG. 9

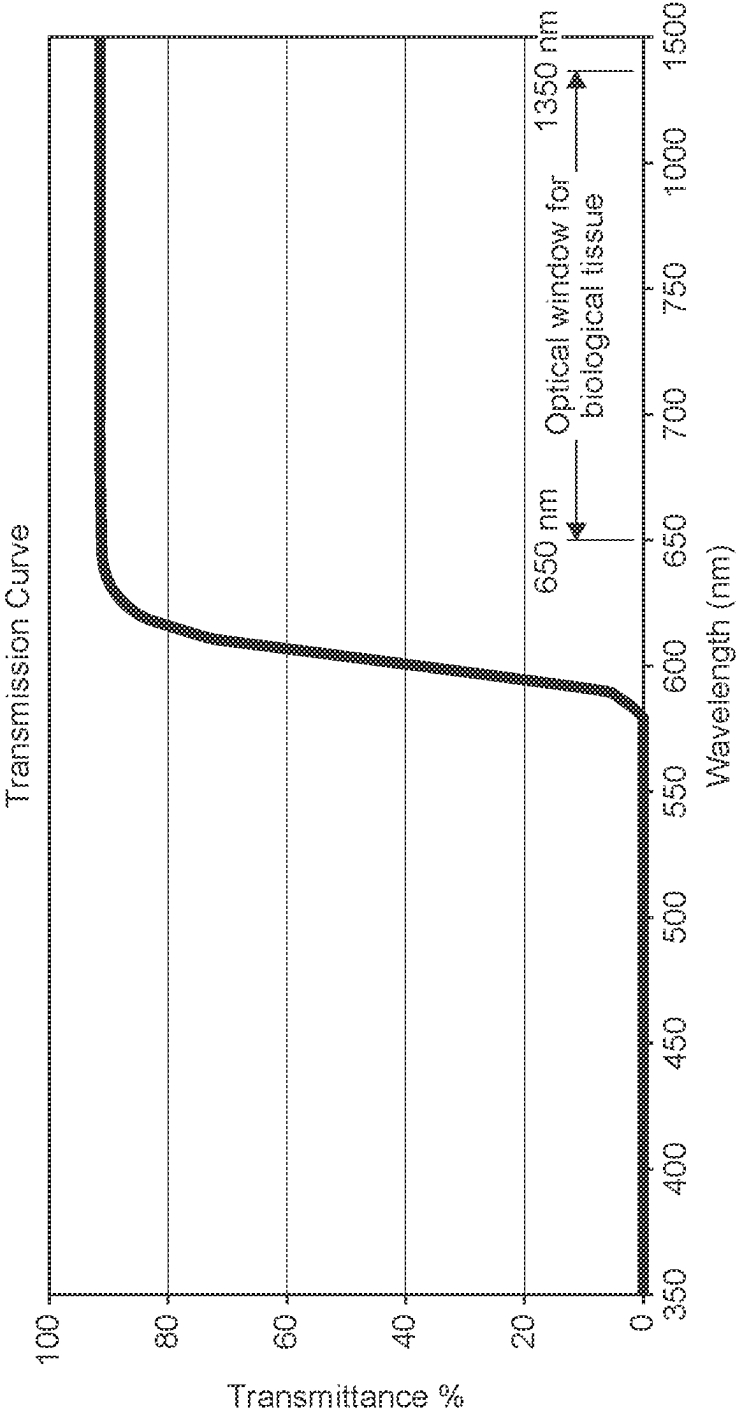


FIG. 10

1

OPTICAL TIP-TRACKING SYSTEMS AND METHODS THEREOF

PRIORITY

This application is a continuation of U.S. patent application Ser. No. 17/105,310, filed Nov. 25, 2020, now U.S. Pat. No. 11,850,338, which claims the benefit of priority to U.S. Patent Application No. 62/940,107 filed Nov. 25, 2019, each of which is incorporated by reference in its entirety into this application.

BACKGROUND

Intravascular guidance of medical devices such as guidewires and catheters typically requires fluoroscopic methods for tracking tips of the medical devices and determining whether the tips are appropriately localized in their target anatomical structures. Such fluoroscopic methods expose clinicians and patients alike to harmful X-ray radiation. In some cases, the patients are exposed to potentially harmful contrast media needed for the fluoroscopic methods. Magnetic and electromagnetic means for tracking the tips of the medical devices obviate some of the foregoing issues with respect to exposure to radiation and potentially harmful contrast media, but the magnetic and electromagnetic means for tracking the tips of the medical devices are prone to interference.

Disclosed herein are optical tip-tracking systems and methods thereof that address the foregoing.

SUMMARY

Disclosed herein is an optical tip-tracking system including, in some embodiments, a light-emitting stylet, a light detector, and a console configured to operably connect to the light-emitting stylet and the light detector. The light-emitting stylet is configured to be disposed in a lumen of a catheter. The light-emitting stylet includes a light source in a distal-end portion of the light-emitting stylet configured to emit light. The light detector is configured to be placed over a patient. The light detector includes a plurality of photodetectors configured to detect the light emitted from the light source. The console includes memory and a processor configured to instantiate an optical tip-tracking process for optically tracking the distal-end portion of the light-emitting stylet while the light-emitting stylet is disposed in a vasculature of the patient, the light source is emitting light, the light detector is disposed over the light-emitting stylet, and the photodetectors are detecting the light emitted from the light source.

In some embodiments, the light source is a light-emitting diode ("LED").

In some embodiments, the light emitted from the light source has a center wavelength between about 650 nm to 1350 nm.

In some embodiments, the light emitted from the light source has a center wavelength between about 650 nm to 950 nm.

In some embodiments, the distal-end portion of the light-emitting stylet is configured to directionally emit light in one or more chosen directions.

In some embodiments, the light detector includes a housing having a patient-facing portion of the housing configured to transmit at least a portion of the light emitted from the light source to the photodetectors.

2

In some embodiments, the housing has a light-blocking portion of the housing opposite the patient-facing portion configured to block ambient light from the photodetectors.

In some embodiments, the photodetectors are arranged in an array such that the light emitted from the light source remains detectable by at least one photodetector of the photodetectors even when the light emitted from the light source is anatomically blocked from another one or more photodetectors of the photodetectors.

In some embodiments, the optical tip-tracking process is configured to provide tracking information as input to a display server of the console for optically tracking the distal-end portion of the light-emitting stylet in a graphical user interface on a display.

In some embodiments, the light-emitting stylet is configured to directly connect to the console.

In some embodiments, the light-emitting stylet is configured to indirectly connect to the console through an intervening multi-use cable.

In some embodiments, the light-emitting stylet is configured to indirectly connect to the console through the light detector.

In some embodiments, the light detector is configured to be placed over the patient and under a sterile drape. The light-emitting stylet includes a drape-piercing connector having a piercing element configured to pierce the sterile drape and insert into a receptacle of a light-detector connector extending from the light detector under the drape.

Also disclosed herein is an optical tip-tracking system including, in some embodiments, a catheter, a light-emitting stylet for the catheter, a light detector, and a console configured to operably connect to the light-emitting stylet and the light detector. The catheter includes a lumen extending through the catheter. The light-emitting stylet is configured to be disposed in a lumen of a catheter. The light-emitting stylet includes a light-emitting diode ("LED") in a distal-end portion of the light-emitting stylet configured to emit light having a center wavelength between about 650 nm to 1350 nm. The light detector is configured to be placed over a patient. The light detector includes a plurality of photodetectors configured to detect the light emitted from the LED. The console includes memory and a processor configured to instantiate an optical tip-tracking process for optically tracking the distal-end portion of the light-emitting stylet in a graphical user interface on a display while the light-emitting stylet is disposed in a vasculature of the patient, the LED is emitting light, the light detector is disposed over the light-emitting stylet, and the photodetectors are detecting the light emitted from the LED.

In some embodiments, the light detector is configured to be placed over the patient and under a sterile drape. The light-emitting stylet includes a drape-piercing connector configured to pierce the sterile drape and connect with a light-detector connector extending from the light detector under the drape.

Also disclosed herein is an optical tip-tracking system including, in some embodiments, a light-emitting stylet, a light detector, and a console configured to operably connect to the light-emitting stylet and the light detector. The light-emitting stylet is configured to be disposed in a lumen of a catheter. The light-emitting stylet includes an optical fiber configured to convey light to a distal-end portion of the light-emitting stylet for emitting light therefrom. The light detector is configured to be placed over a patient. The light detector includes a plurality of photodetectors configured to detect the light emitted from the light source. The console includes a light source for the light emitting stylet and

3

memory and a processor. The memory and the processor are configured to instantiate an optical tip-tracking process for optically tracking the distal-end portion of the light-emitting stylet while the light-emitting stylet is disposed in a vasculature of the patient, the light source is emitting light, the light detector is disposed over the light-emitting stylet, and the photodetectors are detecting the light emitted from the light source.

Also disclosed herein is a method of an optical tip-tracking system including, in some embodiments, a disposing step of disposing a light-emitting stylet of the optical tip-tracking system in a lumen of a catheter. The light-emitting stylet includes a light source in a distal-end portion of the light-emitting stylet. The method also includes a placing step of placing a light detector of the optical tip-tracking system over a patient. The light detector includes a plurality of photodetectors. The method also includes an advancing step of advancing the catheter from an insertion site to a destination within a vasculature of the patient while emitting light from the light source and detecting the light with the photodetectors. The method also includes a viewing step of viewing a display screen of the optical tip-tracking system while the display screen graphically tracks the distal-end portion of the light-emitting stylet through the vasculature of the patient.

In some embodiments, the light source of the light-emitting stylet distally extends beyond a distal end of the catheter while advancing the catheter, thereby enabling the photodetectors of the light detector to detect the light emitted from the light source.

In some embodiments, the method also includes a placing step of placing a sterile drape over both the patient and the light detector. The method also includes a connecting step of connecting a drape-piercing connector of the light-emitting stylet with a light-detector connector extending from the light detector. The connecting step includes piercing the sterile drape with a piercing element of the drape-piercing connector before inserting the piercing element into a receptacle of the light-detector connector.

In some embodiments, the catheter is a central venous catheter ("CVC"). The advancing step includes advancing the CVC with the light-emitting stylet disposed therein through a right internal jugular vein, a right brachiocephalic vein, and into a superior vena cava ("SVC").

In some embodiments, the catheter is a peripherally inserted central catheter ("PICC"). The advancing step includes advancing the PICC with the light-emitting stylet disposed therein through a right basilic vein, a right axillary vein, a right subclavian vein, a right brachiocephalic vein, and into an SVC.

In some embodiments, the method also includes a ceasing step of ceasing to advance the catheter through the vasculature of the patient after determining the distal-end portion of light-emitting stylet is located at the destination by way of the display screen.

These and other features of the concepts provided herein will become more apparent to those of skill in the art in view of the accompanying drawings and following description, which describe particular embodiments of such concepts in greater detail.

DRAWINGS

FIG. 1 provides a block diagram of a first optical tip-tracking system in accordance with some embodiments.

FIG. 2 provides a block diagram of a second optical tip-tracking system in accordance with some embodiments.

4

FIG. 3 illustrates the first optical tip-tracking system in accordance with some embodiments.

FIG. 4 illustrates the first optical tip-tracking system including a catheter in accordance with some embodiments.

FIG. 5A illustrates a distal-end portion of a first light-emitting stylet of the first or second optical tip-tracking system in accordance with some embodiments.

FIG. 5B illustrates a transverse cross section of the first light-emitting stylet disposed in the catheter in accordance with some embodiments.

FIG. 6A illustrates a distal-end portion of a second light-emitting stylet of the first or second optical tip-tracking system in accordance with some embodiments.

FIG. 6B illustrates a transverse cross section of the second light-emitting stylet disposed in the catheter in accordance with some embodiments.

FIG. 7 illustrates a side view of a light detector of the first or second optical tip-tracking system in accordance with some embodiments.

FIG. 8 illustrate the first optical tip-tracking system in use in accordance with some embodiments.

FIG. 9 illustrate the second optical tip-tracking system in use in accordance with some embodiments.

FIG. 10 provides a transmission curve for optical window for biological tissue in accordance with some embodiments.

DESCRIPTION

Before some particular embodiments are disclosed in greater detail, it should be understood that the particular embodiments disclosed herein do not limit the scope of the concepts provided herein. It should also be understood that a particular embodiment disclosed herein can have features that can be readily separated from the particular embodiment and optionally combined with or substituted for features of any of a number of other embodiments disclosed herein.

Regarding terms used herein, it should also be understood the terms are for the purpose of describing some particular embodiments, and the terms do not limit the scope of the concepts provided herein. Ordinal numbers (e.g., first, second, third, etc.) are generally used to distinguish or identify different features or steps in a group of features or steps, and do not supply a serial or numerical limitation. For example, "first," "second," and "third" features or steps need not necessarily appear in that order, and the particular embodiments including such features or steps need not necessarily be limited to the three features or steps. Labels such as "left," "right," "top," "bottom," "front," "back," and the like are used for convenience and are not intended to imply, for example, any particular fixed location, orientation, or direction. Instead, such labels are used to reflect, for example, relative location, orientation, or directions. Singular forms of "a," "an," and "the" include plural references unless the context clearly dictates otherwise.

With respect to "proximal," a "proximal portion" or a "proximal-end portion" of, for example, a catheter disclosed herein includes a portion of the catheter intended to be near a clinician when the catheter is used on a patient. Likewise, a "proximal length" of, for example, the catheter includes a length of the catheter intended to be near the clinician when the catheter is used on the patient. A "proximal end" of, for example, the catheter includes an end of the catheter intended to be near the clinician when the catheter is used on the patient. The proximal portion, the proximal-end portion, or the proximal length of the catheter can include the proximal end of the catheter; however, the proximal portion, the proximal-end portion, or the proximal length of the

5

catheter need not include the proximal end of the catheter. That is, unless context suggests otherwise, the proximal portion, the proximal-end portion, or the proximal length of the catheter is not a terminal portion or terminal length of the catheter.

With respect to “distal,” a “distal portion” or a “distal-end portion” of, for example, a catheter disclosed herein includes a portion of the catheter intended to be near or in a patient when the catheter is used on the patient. Likewise, a “distal length” of, for example, the catheter includes a length of the catheter intended to be near or in the patient when the catheter is used on the patient. A “distal end” of, for example, the catheter includes an end of the catheter intended to be near or in the patient when the catheter is used on the patient. The distal portion, the distal-end portion, or the distal length of the catheter can include the distal end of the catheter; however, the distal portion, the distal-end portion, or the distal length of the catheter need not include the distal end of the catheter. That is, unless context suggests otherwise, the distal portion, the distal-end portion, or the distal length of the catheter is not a terminal portion or terminal length of the catheter.

Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by those of ordinary skill in the art.

Again, fluoroscopic methods typically used for tracking tips of medical devices such as guidewires and catheters expose clinicians and patients alike to harmful X-ray radiation. Magnetic and electromagnetic means for tracking the tips of the medical devices obviate some of the foregoing issues with respect to exposure to radiation, but the magnetic and electromagnetic means for tracking the tips of the medical devices are prone to interference.

Disclosed herein are optical tip-tracking systems and methods thereof that address the foregoing.

Optical Tip-Tracking Systems

FIG. 1 provides a block diagram of a first optical tip-tracking system 100, FIG. 3 illustrates the first optical tip-tracking system 100, FIG. 4 illustrates the first optical tip-tracking system 100 including a catheter 450, and FIG. 8 illustrates the first optical tip-tracking system 100 in use, in accordance with some embodiments. FIG. 2 provides a block diagram of a second optical tip-tracking system 200 and FIG. 9 illustrates the second optical tip-tracking system 200 in use, in accordance with some embodiments.

As shown, the optical tip-tracking system 100 or 200 includes a light-emitting stylet 110, a light detector 120, and a console 130 or 230 configured to operably connect to the light-emitting stylet 110 and the light detector 120. Each optical tip-tracking system of the optical tip-tracking systems 100 and 200 also includes a display screen; however, the optical tip-tracking system 100 includes a standalone display screen 140, whereas the optical tip-tracking system 200 includes an integrated display screen 240. Each optical tip-tracking system of the optical tip-tracking systems 100 and 200 can also include a medical device 150 such as the catheter 450 of FIG. 4.

Beginning with the consoles 130 and 230, the console 130 or 230 includes memory 134 such as primary memory 136 and secondary memory 138. The primary memory 136 includes random-access memory (“RAM”). The secondary memory 138 includes non-volatile memory such as read-only memory (“ROM”) including a set of instructions 139 or 239 for loading into the primary memory 136 at runtime of the console 130 or 230.

One or more processors 132 are configured to instantiate an optical tip-tracking process in accordance with the

6

instructions 139 or 239 for optically tracking a distal-end portion of the light-emitting stylet 110 while the light-emitting stylet 110 is disposed in a vasculature of a patient, a light source such as one or more LEDs 112 is emitting light, the light detector 120 is disposed over the light-emitting stylet 110, and a plurality of photodetectors of the light detector 120 such as photodetectors 122 are detecting the light emitted from the light source of the light-emitting stylet 110. The optical tip-tracking process is configured to provide tracking information as input to a display server of the console 130 or 230 for optically tracking the distal-end portion of the light-emitting stylet 110 in a graphical user interface on the display screen 140 or 240. Optically tracking the distal-end portion of the light-emitting stylet 110 can be animated on the display screen 140 or 240 as shown on the display screen 240 of the console 230 in FIGS. 8 and 9.

FIGS. 1 and 2 provide different connection options for connecting at least the light-emitting stylet 110 and the light detector 120 to the console 130 or 230.

The left-hand side of each figure of FIGS. 1 and 2 shows a connection option (“option A”) in which the light-emitting stylet 110 and the light detector 120 are independently connected to the console 130 or 230. For example, the console 130 or 230 and the light-emitting stylet 110 can be mutually configured such that the light-emitting stylet 110 directly connects to the console 130 or 230 or indirectly connects to the console 130 or 230 through an intervening multi-use cable having requisite conveying means for conveying electrical power (e.g., electrical leads), light (e.g., optical fiber), etc. Likewise, the console 130 or 230 and the light detector 120 can be mutually configured such that the light detector 120 directly connects to the console 130 or 230 or indirectly connects to the console 130 or 230 through an intervening multi-use cable.

The right-hand side of each figure of FIGS. 1 and 2 shows a connection option (“option B”) in which the light-emitting stylet 110 is connected to the light detector 120 and, in turn, the light detector 120 is connected to the console 130 or 230. A cable such as the intervening multi-use cable set forth above for connecting the light detector 120 to the console 130 or 230 includes the requisite conveying means for conveying electrical power (e.g., electrical leads), light (e.g., optical fiber), etc. The foregoing connection option is useful in that the light detector 120 is multi-use equipment configured to be placed over a patient P and under a sterile drape 801 outside a sterile field as shown in FIGS. 8 and 9. The light-emitting stylet 110 is single-use equipment intended for use within the foregoing sterile field. As shown in FIG. 9, the light-emitting stylet 110 can include a drape-piercing connector 900 in a proximal-end portion thereof having a piercing element 902 configured to both pierce the sterile drape 801 and insert into a receptacle 904 of a light-detector connector extending from the light detector 120 under the sterile drape 801. So configured, the intervening multi-use cable set forth above through which the light-emitting stylet 110 can be indirectly connected to the console 130 or 230 is not needed. For examples of drape-piercing connectors for the light-emitting stylet 110 and light-detector connectors for the light-detector 120 see U.S. Pat. No. 10,231,753 and children patents or patent applications thereof, each of which patents and patent application are incorporated herein by reference.

Both connection options of FIG. 1 show the display screen 140 connected to the console 130 in the optical tip-tracking system 100. FIG. 2 does not show connection options for connecting the integrated display screen 240 to the console 230 in the optical tip-tracking system 200. This

is because the integrated display screen **240** is integrated into the console **240** as shown in FIGS. **3**, **4**, **8**, and **9**.

In addition to FIGS. **1-4**, FIG. **7** illustrates a side view of the light detector **120** in accordance with some embodiments.

As set forth above, the light detector **120** is configured to be placed over a patient and under a sterile drape such as the sterile drape **801** of FIGS. **8** and **9**.

The light detector **120** includes the photodetectors **122** disposed within the light detector **120** configured to detect the light emitted from the light source of the light-emitting stylet **110**. The photodetectors **122** are arranged in an array such that the light emitted from the light source of the light-emitting stylet **110** remains detectable by at least one photodetector of the photodetectors **122** even when the light emitted from the light source of the light-emitting stylet **110** is anatomically blocked (e.g. by a rib) from another one or more photodetectors of the photodetectors **122**.

The light detector **120** includes a housing having a patient-facing portion **722** of the housing configured to transmit at least a portion of the light emitted from the light source of the light-emitting stylet **110** to the photodetectors **122** disposed within the light detector **120**. The housing also has a light-blocking portion **724** of the housing opposite the patient-facing portion **722** of the housing configured to block ambient light from the photodetectors **122** disposed within the light detector **120**. In addition to the light-blocking portion **724** of the housing of the light detector **120**, the sterile drape **801** also protects the photodetectors **122** from the ambient light while in use.

In addition to FIGS. **1-4**, FIG. **5A** illustrates the distal-end portion of the light-emitting stylet **110** and FIG. **5B** illustrates a transverse cross section of the light-emitting stylet **110** in accordance with some embodiments having the one-or-more LEDs **112** as the light source. FIG. **6A** illustrates the distal-end portion of the light-emitting stylet **110** and FIG. **6B** illustrates a transverse cross section of the light-emitting stylet **110** in accordance with some embodiments having an external light source.

As set forth in more detail below, the light-emitting stylet **110** is configured to be disposed in a lumen of a catheter.

With respect to the light-emitting stylet **110** having the one-or-more LEDs **112** as the light source, the light-emitting stylet **110** includes the one-or-more LEDs **112** in a distal-end portion (e.g., a tip) of the light-emitting stylet **110** configured to emit light. The light-emitting stylet **110** also includes at least a pair of electrical leads **114** configured to convey electrical power from the console **130** or **230** to power the one-or-more LEDs **112**. The distal-end portion of the light-emitting stylet **110** can be configured to directionally emit light from the one-or-more LEDs **112** in one or more chosen directions such as straight ahead in line with the light-emitting stylet **110**, radially outward such as toward an extracorporeal surface of a patient, or a combination thereof.

With respect to the light-emitting stylet **110** having the external light source, the light-emitting stylet **110** includes an optical fiber **615** configured to convey light from the external source, for example, a light within the console **130** or **230**, to the distal-end portion (e.g., the tip) of the light-emitting stylet **110** to emit light. A ferrule **613** disposed over a distal-end portion of the optical fiber **615** can be configured to directionally emit light from the optical fiber **615** in one or more chosen directions such as straight ahead in line with the light-emitting stylet **110**, radially outward such as toward an extracorporeal surface of a patient, or a combination thereof.

The light emitted from the light source can have a center wavelength between about 650 nm to 1350 nm including a center wavelength between about 650 nm to 950 nm or a center wavelength between about 1100 nm to 1350 nm. The light in the foregoing ranges of wavelengths is within an optical window for biological tissue in that such light penetrates biological tissue more deeply than light outside the foregoing ranges of wavelengths. (See FIG. **10** for the optical window for biological tissue.) Each LED of the one-or-more LEDs **112** can include aluminum gallium arsenide (AlGaAs) or gallium arsenide (GaAs) as a semiconductor material. In accordance with the semiconductor material and its composition, each LED of the one-or-more LEDs **112** can be configured to emit light at or within the following wavelengths: 660 nm, 680 nm, 800-850 nm, 850-940 nm, and 940 nm.

Adverting to FIG. **4**, the catheter **450** can be a peripherally inserted central catheter ("PICC"), as shown, or a central venous catheter ("CVC"). In an example of a diluminal catheter, the catheter **450** can include a catheter tube **452**, a bifurcated hub **454**, two extension legs **456**, and two Luer connectors **458** operably connected in the foregoing order. Notwithstanding the foregoing example, the catheter **450** can alternatively be a monoluminal catheter or a multi-luminal catheter including three or more lumens.

Continuing with the example of the diluminal catheter, the catheter **450** includes two lumens extending therethrough formed of adjoining lumen portions. Indeed, the catheter tube **452** includes two catheter-tube lumens **553**. (See FIGS. **5B** and **6B** for the two catheter-tube lumens **553**). The bifurcated hub **454** has two hub lumens correspondingly fluidly connected to the two catheter-tube lumens **553**. Each extension leg of the two extension legs **456** has an extension-leg lumen fluidly connected to a hub lumen of the two hub lumens. Either lumen extending through the catheter **450** can accommodate the light-emitting stylet **110** disposed therein.

Methods

A method of the optical tip-tracking system **100** or **200** includes a disposing step of disposing the light-emitting stylet **110** of the optical tip-tracking system **100** or **200** in a lumen of the catheter **450**.

The method also includes a placing step of placing the light detector **120** of the optical tip-tracking system **100** or **200** over the patient **P** as shown in FIGS. **8** and **9**.

The method also includes a placing step of placing the sterile drape **801** over both the patient **P** and the light detector **120**.

As shown in FIG. **8**, the method can also include a connecting step of connecting the drape-piercing connector of the light-emitting stylet **110** with the light-detector connector extending from the light detector **120**. Such a connecting step includes piercing the sterile drape **801** with the piercing element of the drape-piercing connector before inserting the piercing element into the receptacle of the light-detector connector.

The method also includes an advancing step of advancing the catheter **450** from an insertion site to a destination within a vasculature of the patient **P** while emitting light from the light source (e.g., the one-or-more LEDs **112**) and detecting the light with the photodetectors **122**. The light source of the light-emitting stylet **110** should distally extend beyond a distal end of the catheter **450** while advancing the catheter **450**, thereby enabling the photodetectors **122** of the light detector **120** to detect the light emitted from the light source of the light-emitting stylet **110**.

When the catheter 450 is a CVC, the advancing step includes advancing the CVC with the light-emitting stylet 110 disposed therein through a right internal jugular vein, a right brachiocephalic vein, and into an SVC.

When the catheter 450 is a PICC, the advancing step includes advancing the PICC with the light-emitting stylet 110 disposed therein through a right basilic vein, a right axillary vein, a right subclavian vein, a right brachiocephalic vein, and into an SVC.

The method also includes a viewing step of viewing the display screen 140 or 240 of the optical tip-tracking system 100 or 200 while the display screen 140 or 240 graphically tracks the distal-end portion of the light-emitting stylet 110 through the vasculature of the patient P.

The method also includes a ceasing step of ceasing to advance the catheter 450 through the vasculature of the patient P after determining the distal-end portion of the light-emitting stylet 110 is located at the destination by way of the display screen 140 or 240.

While some particular embodiments have been disclosed herein, and while the particular embodiments have been disclosed in some detail, it is not the intention for the particular embodiments to limit the scope of the concepts provided herein. Additional adaptations and/or modifications can appear to those of ordinary skill in the art, and, in broader aspects, these adaptations and/or modifications are encompassed as well. Accordingly, departures may be made from the particular embodiments disclosed herein without departing from the scope of the concepts provided herein.

What is claimed is:

1. A medical device tip-tracking system, comprising:
 - a light-emitting stylet configured to be disposed in a lumen of a medical device, the light-emitting stylet configured to emit light from a distal-end portion of the light-emitting stylet;
 - a light detector configured to be placed over and external to a patient, the light detector including a plurality of photodetectors configured to detect the light emitted from a light source, wherein the plurality of photodetectors are arranged in the light detector such that the plurality of photodetectors are configured to detect a remaining portion of the light when a first portion of the light is anatomically blocked by a bone of the patient; and
 - a console coupled to the light-emitting stylet and the light detector, the console including:
 - a processor; and
 - non-volatile memory storing instructions that, when executed by the processor, cause performance of operations including:
 - displaying tracking information in a graphical user interface on a display screen as the light-emitting stylet is advanced through a vasculature of the patient.
2. The medical device tip-tracking system of claim 1, wherein the light-emitting stylet is configured to directly connect to the light detector.
3. The medical device tip-tracking system of claim 1, wherein the light-emitting stylet is configured to directly connect to the console.
4. The medical device tip-tracking system of claim 1, wherein the light-emitting stylet includes the light source at the distal-end portion, wherein the light source is configured to emit the light.
5. The medical device tip-tracking system of claim 4, wherein the light-emitting stylet is configured to indirectly

connect to the console through the light detector such that electrical power passes from either the console to the light source or the light detector.

6. The medical device tip-tracking system of claim 1, wherein the light-emitting stylet includes an electrical lead configured to convey electrical power to the light source.

7. The medical device tip-tracking system of claim 1, wherein the light-emitting stylet includes an optical fiber configured to convey the light along a length of the light-emitting stylet, wherein the light is emitted from a distal-end portion of the optical fiber.

8. The medical device tip-tracking system of claim 7, wherein the light-emitting stylet includes a ferrule disposed over the distal-end portion of the optical fiber, and wherein the ferrule is configured to direct the light in one or more directions.

9. The medical device tip-tracking system of claim 1, wherein the instructions, when executed by the processor, cause performance of further operations including:

graphically tracking the distal-end portion of the light-emitting stylet through the vasculature of the patient.

10. The medical device tip-tracking system of claim 1, wherein the console further includes the display screen integrated into a housing of the console.

11. A method of deploying an optical tip-tracking system, comprising:

disposing a light-emitting stylet in a lumen of a medical device, the light-emitting stylet configured to emit light from a distal-end portion of the light-emitting stylet;

placing a light detector over and external to a patient, the light detector including a plurality of photodetectors configured to detect the light emitted from a light source, wherein the plurality of photodetectors are arranged in the light detector such that the plurality of photodetectors are configured to detect a remaining portion of the light when a first portion of the light is anatomically blocked by a bone of the patient;

advancing the light-emitting stylet through a vasculature of the patient; and

viewing tracking information on a graphical user interface on a display screen as the light-emitting stylet is advanced through the vasculature of the patient.

12. The method of claim 11, wherein the light-emitting stylet is configured to directly connect to the light detector.

13. The method of claim 11, wherein the light-emitting stylet is configured to directly connect to a console.

14. The method of claim 11, wherein the light-emitting stylet includes the light source at the distal-end portion, wherein the light source is configured to emit the light.

15. The method of claim 14, wherein the light-emitting stylet is configured to indirectly connect to a console through the light detector such that electrical power passes from either the console to the light source or to the light detector.

16. The method of claim 11, wherein the light-emitting stylet includes an electrical lead configured to convey electrical power to the light source.

17. The method of claim 11, wherein the light-emitting stylet includes an optical fiber configured to convey the light along a length of the light-emitting stylet, wherein the light is emitted from a distal-end portion of the optical fiber.

18. The method of claim 17, wherein the light-emitting stylet includes a ferrule disposed over the distal-end portion of the optical fiber, and wherein the ferrule is configured to direct the light in one or more directions.

11

19. The method of claim **11**, wherein instructions, when executed by a processor, cause performance of further operations including:

graphically tracking the distal-end portion of the light-emitting stylet through the vasculature of the patient. 5

20. The method of claim **11**, wherein a console further includes the display screen integrated into a housing of the console.

* * * * *

12