



US0D1088232S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,088,232 S**
Achleitner et al. (45) **Date of Patent:** **** Aug. 12, 2025**

(54) **ELECTROMEDICAL DEVICE**

(71) Applicant: **Siemens Healthineers AG**, Forchheim
(DE)

(72) Inventors: **Roman Achleitner**, Nuremberg (DE);
Stefanie Guegel-Wild,
Langensendelbach (DE); **Aurel Jensch**,
Eggolsheim (DE); **Xiao Yan Du**,
Shanghai (CN)

(73) Assignee: **Siemens Healthineers AG**, Erlangen
(DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/708,869**

(22) Filed: **Oct. 10, 2019**

(30) **Foreign Application Priority Data**

Apr. 12, 2019 (EM) 006377628

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/107, 158–161, 183–185, 231–232,
D24/234
CPC A61B 5/00; A61B 5/0033; A61B 5/05;
A61B 5/055; A61B 6/00; A61B 6/03;
A61B 6/032; A61B 6/035; A61B 6/0407;
A61B 8/00; A61B 8/13–15
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D683,023 S * 5/2013 Andersson D24/158
D715,943 S * 10/2014 Zhang D24/159
D716,948 S * 11/2014 Yokoyama D24/158
D746,465 S * 12/2015 Du D24/158

D785,799 S * 5/2017 Park D24/158
D794,799 S * 8/2017 Achleitner D24/158
D842,994 S * 3/2019 Avranches D24/158

(Continued)

FOREIGN PATENT DOCUMENTS

CN 305752138 * 5/2020
IN 291123 * 9/2018
JP D1582511 * 7/2017

OTHER PUBLICATIONS

Atrium Health, Siemens Healthineers, Atrium Health Enter Multi-Year Value Partnership to Improve Health Care Capabilities, Access and Equity, Published on: Nov. 28, 2022, atriumhealth.org, Retrieved from Internet: <https://atriumhealth.org/about-us/newsroom/news/2022/11/siemens-healthineers-atrium-health-enter-multi-year-value-partnership> (Year: 2022).*

(Continued)

Primary Examiner — John R Yeh

Assistant Examiner — Edward P Jones

(74) *Attorney, Agent, or Firm* — Banner & Witcoff Ltd.


(57) **CLAIM**

The ornamental design for an electromedical device as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of an electromedical device showing our new design;
FIG. 2 is a back elevational view thereof;
FIG. 3 is a top plan view thereof;
FIG. 4 is a bottom view thereof;
FIG. 5 is a right side elevational view thereof;
FIG. 6 is a left side elevational view thereof; and,
FIG. 7 is a perspective view taken generally from the top, front, right-hand side thereof.
The broken lines shown in the drawings represent portions of the electromedical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

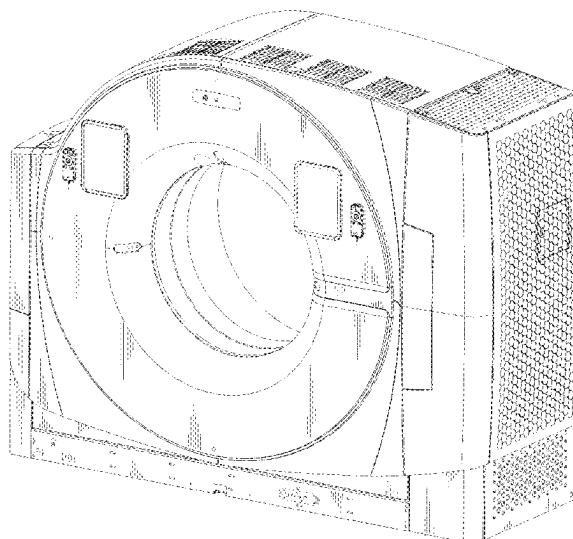

(56)

References Cited

U.S. PATENT DOCUMENTS

D843,578	S	*	3/2019	Avranches		D24/158
D931,463	S	*	9/2021	Achleitner		D24/158
D940,868	S	*	1/2022	Achleitner		D24/158
D982,161	S	*	3/2023	Achleitner		D24/158
11,730,440	B2	*	8/2023	Suehling		A61B 6/4275 378/205
D1,007,684	S	*	12/2023	Achleitner		D24/158
D1,011,531	S	*	1/2024	Achleitner		D24/158
D1,029,264	S	*	5/2024	von Zweigbergk		D24/159
D1,046,157	S	*	10/2024	Takano		D24/158
D1,050,441	S	*	11/2024	Gügel-Wild		D24/158
D1,050,442	S	*	11/2024	Sun		D24/158
D1,052,733	S	*	11/2024	Gügel-Wild		D24/158
D1,057,157	S	*	1/2025	Tasar		D24/159
2018/0271372	A1	*	9/2018	Lee		A61B 5/0035

OTHER PUBLICATIONS

Marty Stempniak, FDA clears PET/CT scanner from Siemens Healthineers, Published on: Nov. 27, 2023, [radiologybusiness.com](https://radiologybusiness.com/topics/medical-imaging/computed-tomography-ct/fda-clears-petct-scanner-siemens-healthineers), Retrieved from Internet: <https://radiologybusiness.com/topics/medical-imaging/computed-tomography-ct/fda-clears-petct-scanner-siemens-healthineers> (Year: 2023).*

itnonline.com, Siemens Healthineers Introduces Magnetom Vida MRI Scanner With BioMatrix Technology, Published on: Feb. 28, 2017, itnonline.com, Retrieved from Internet: [Siemens Healthineers Introduces Magnetom Vida MRI Scanner With BioMatrix Technology](https://itnonline.com) (Year: 2017).*

* cited by examiner

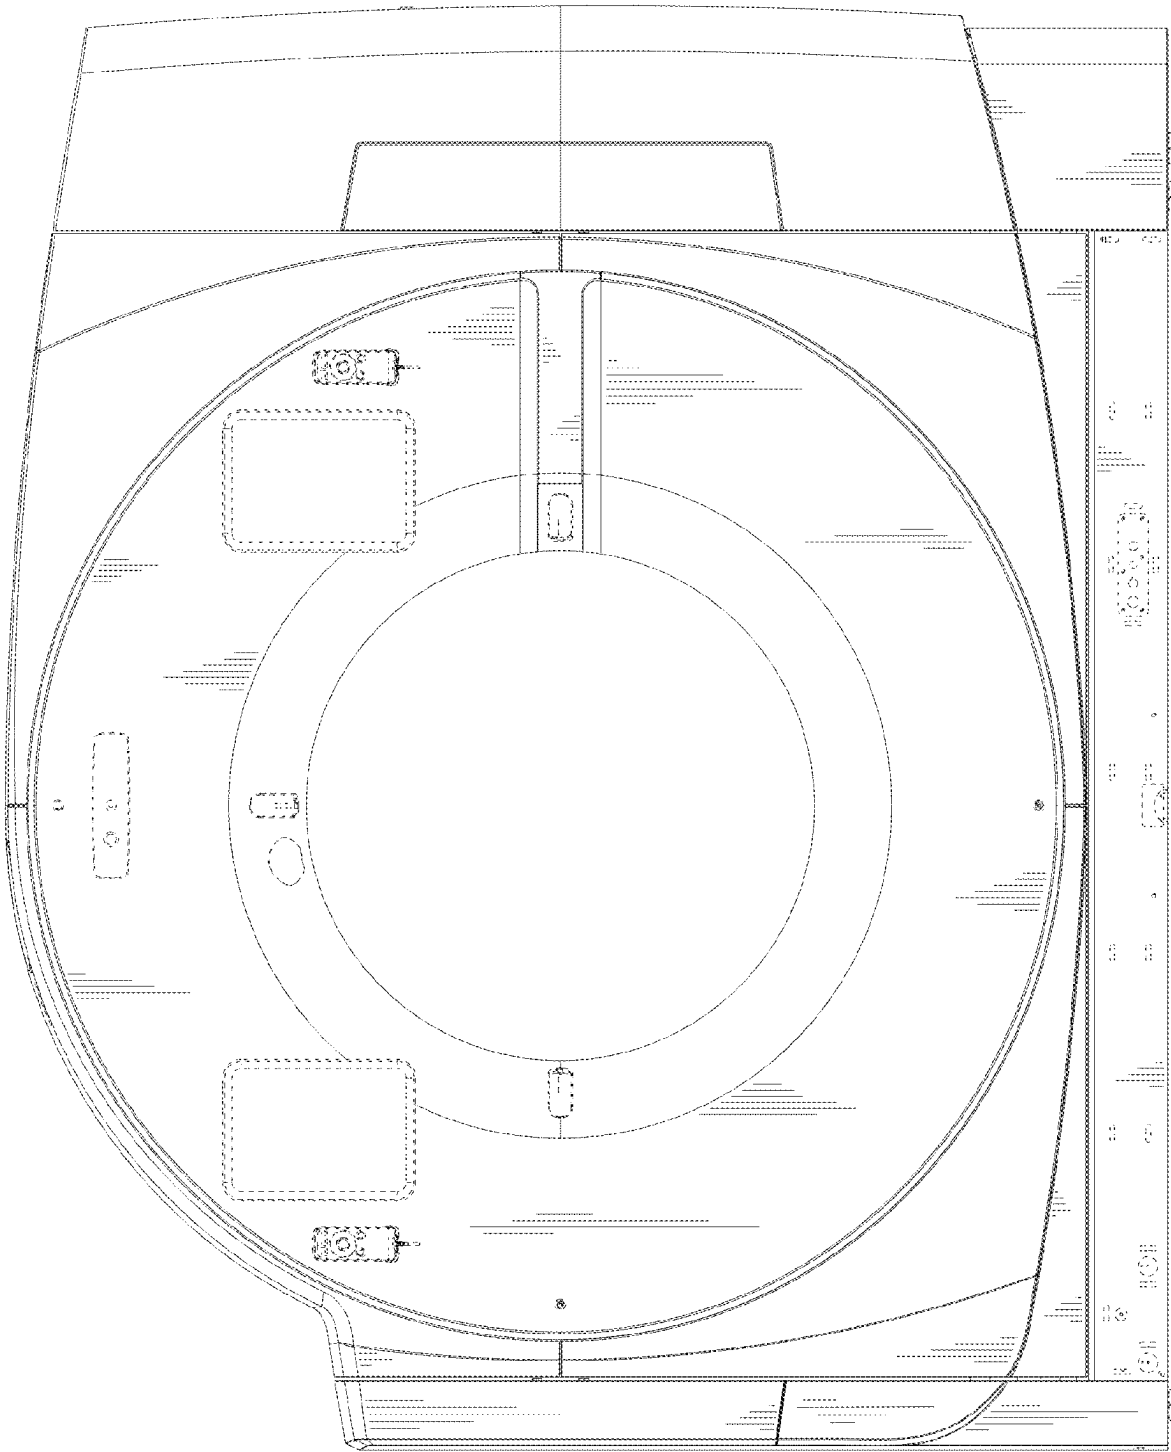


FIG. 1

FIG. 2

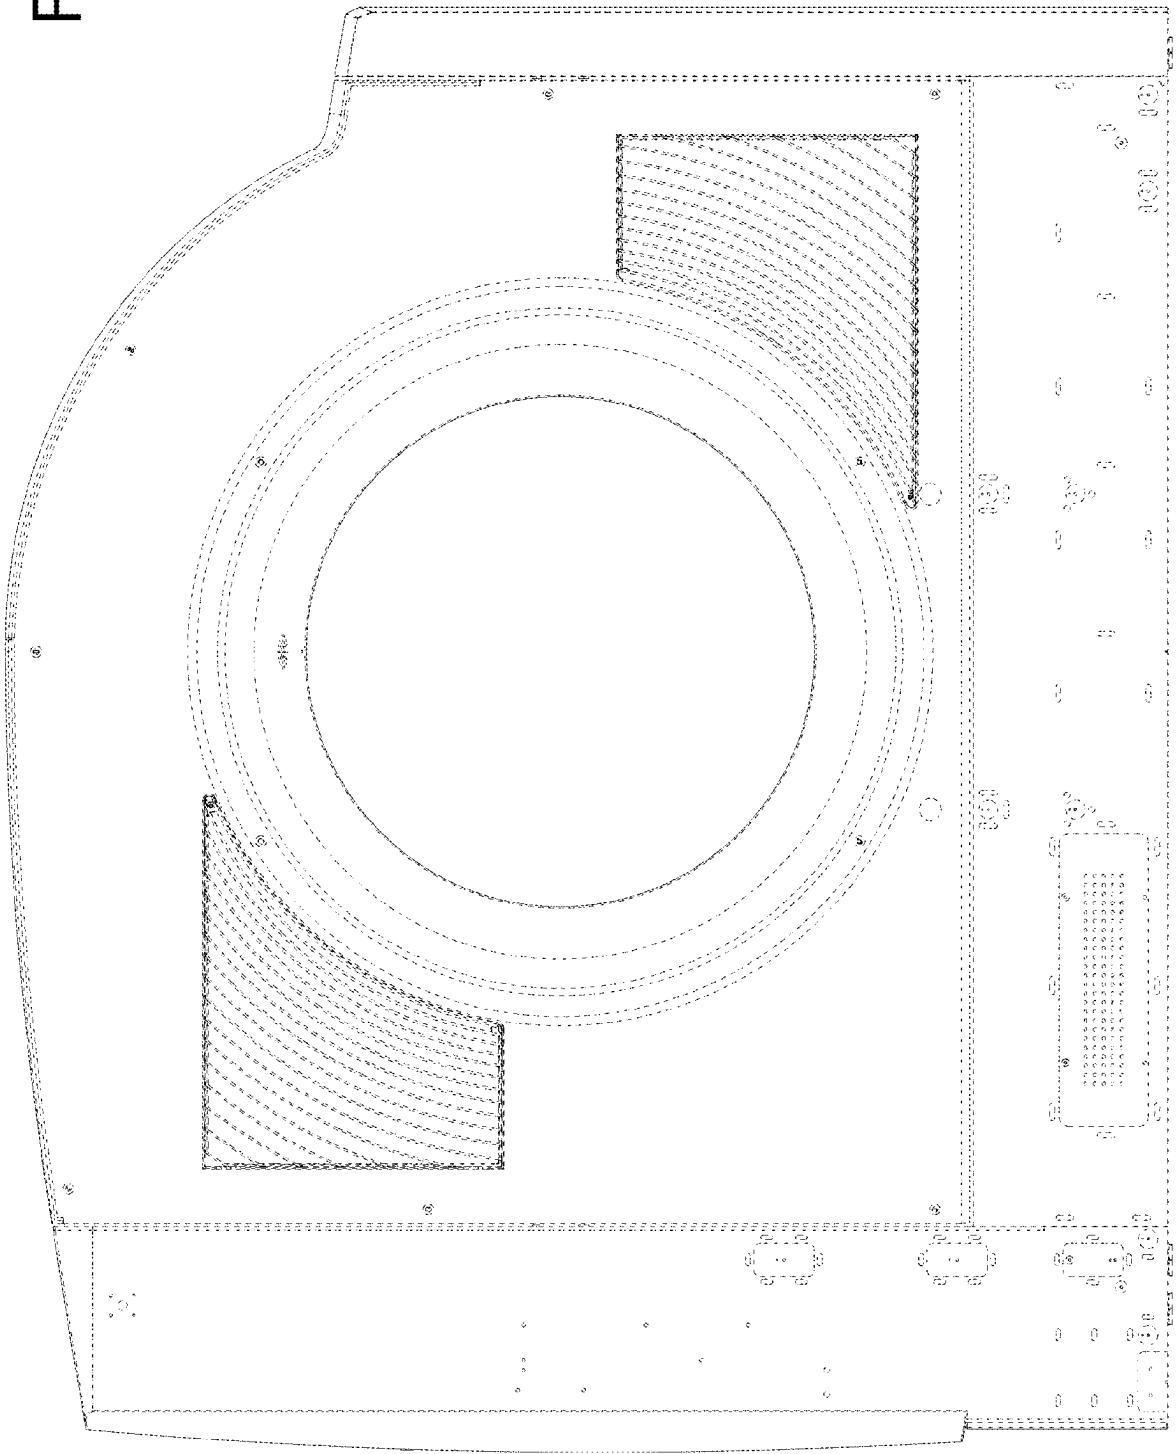


FIG. 3

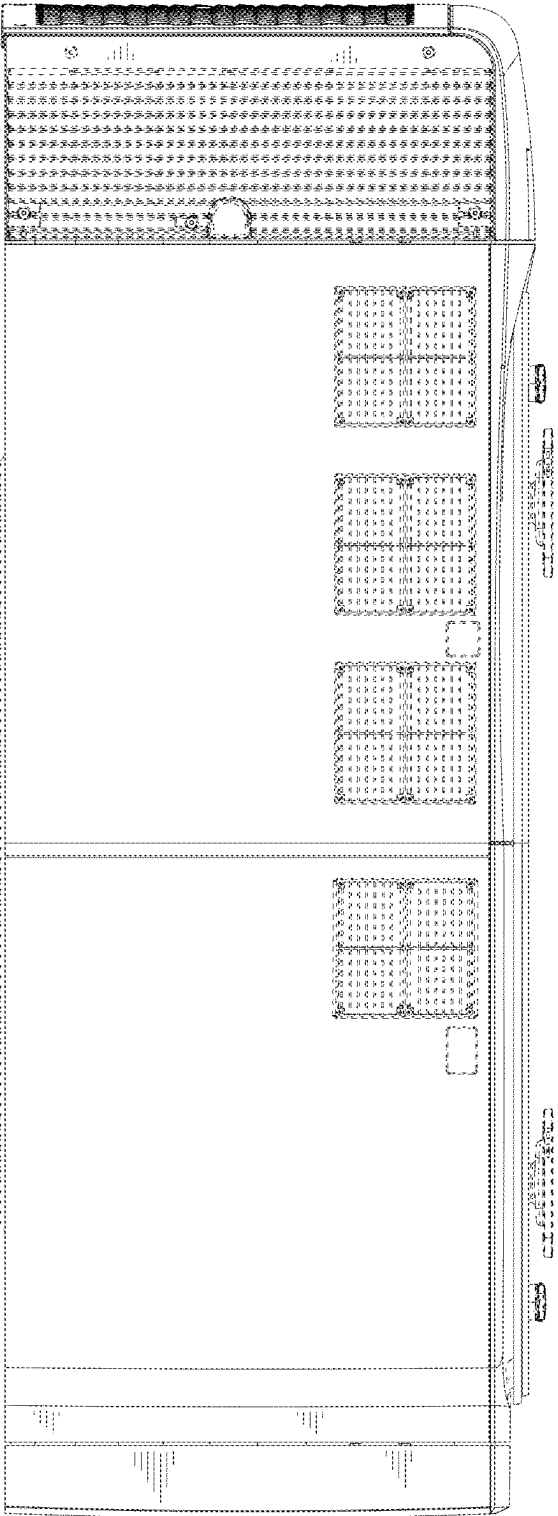


FIG. 4

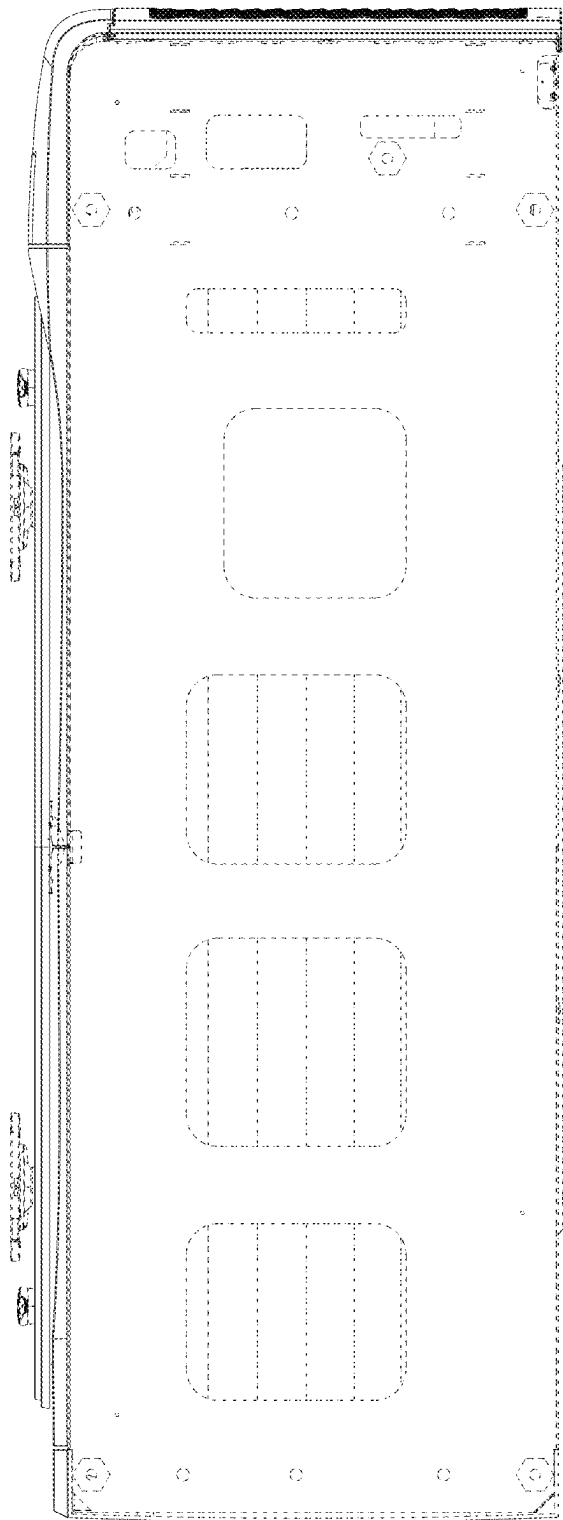


FIG. 5



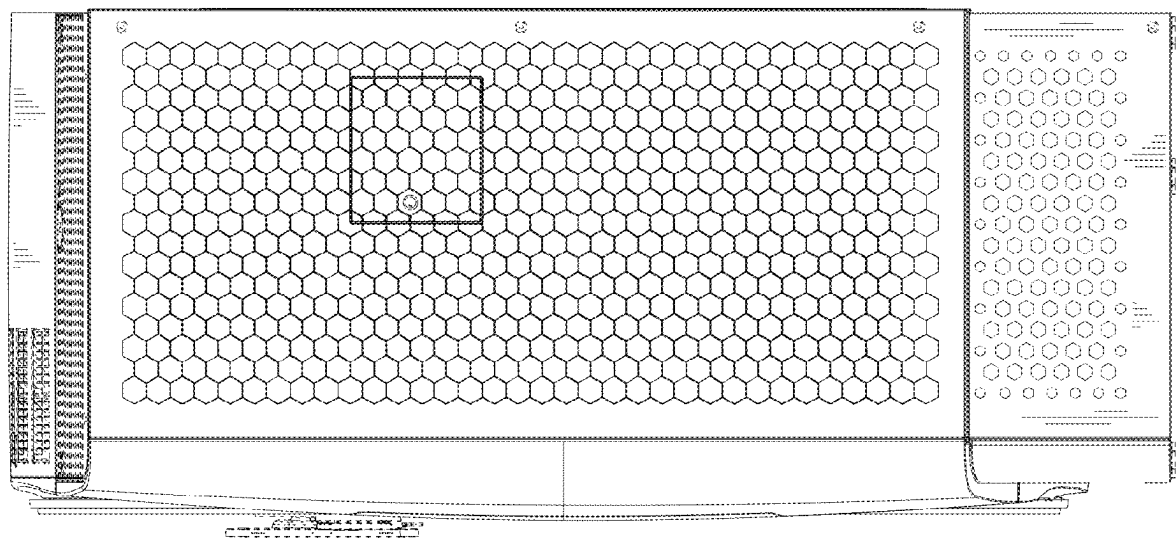


FIG. 6

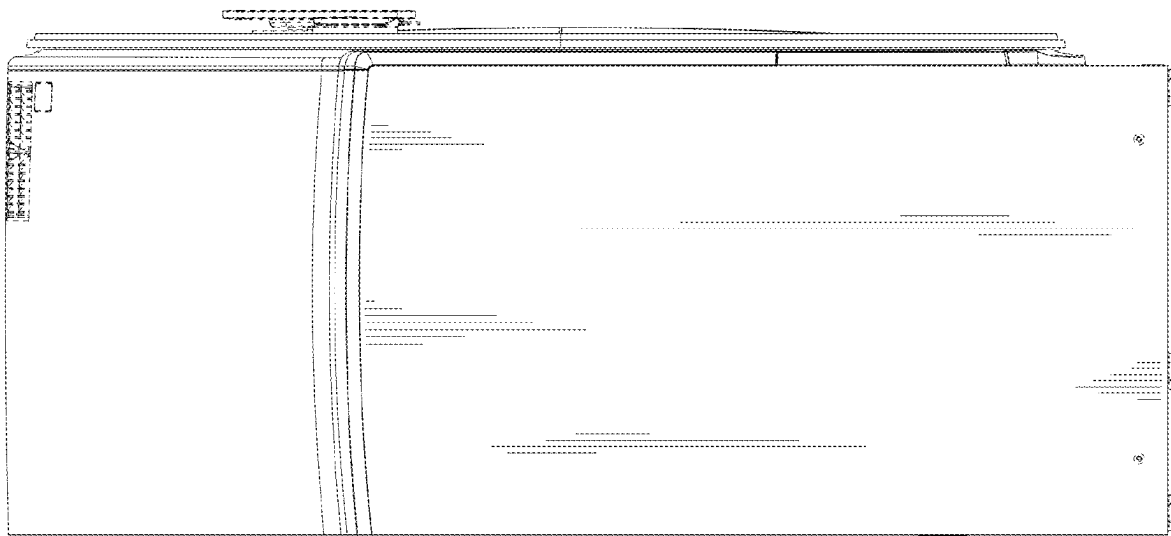

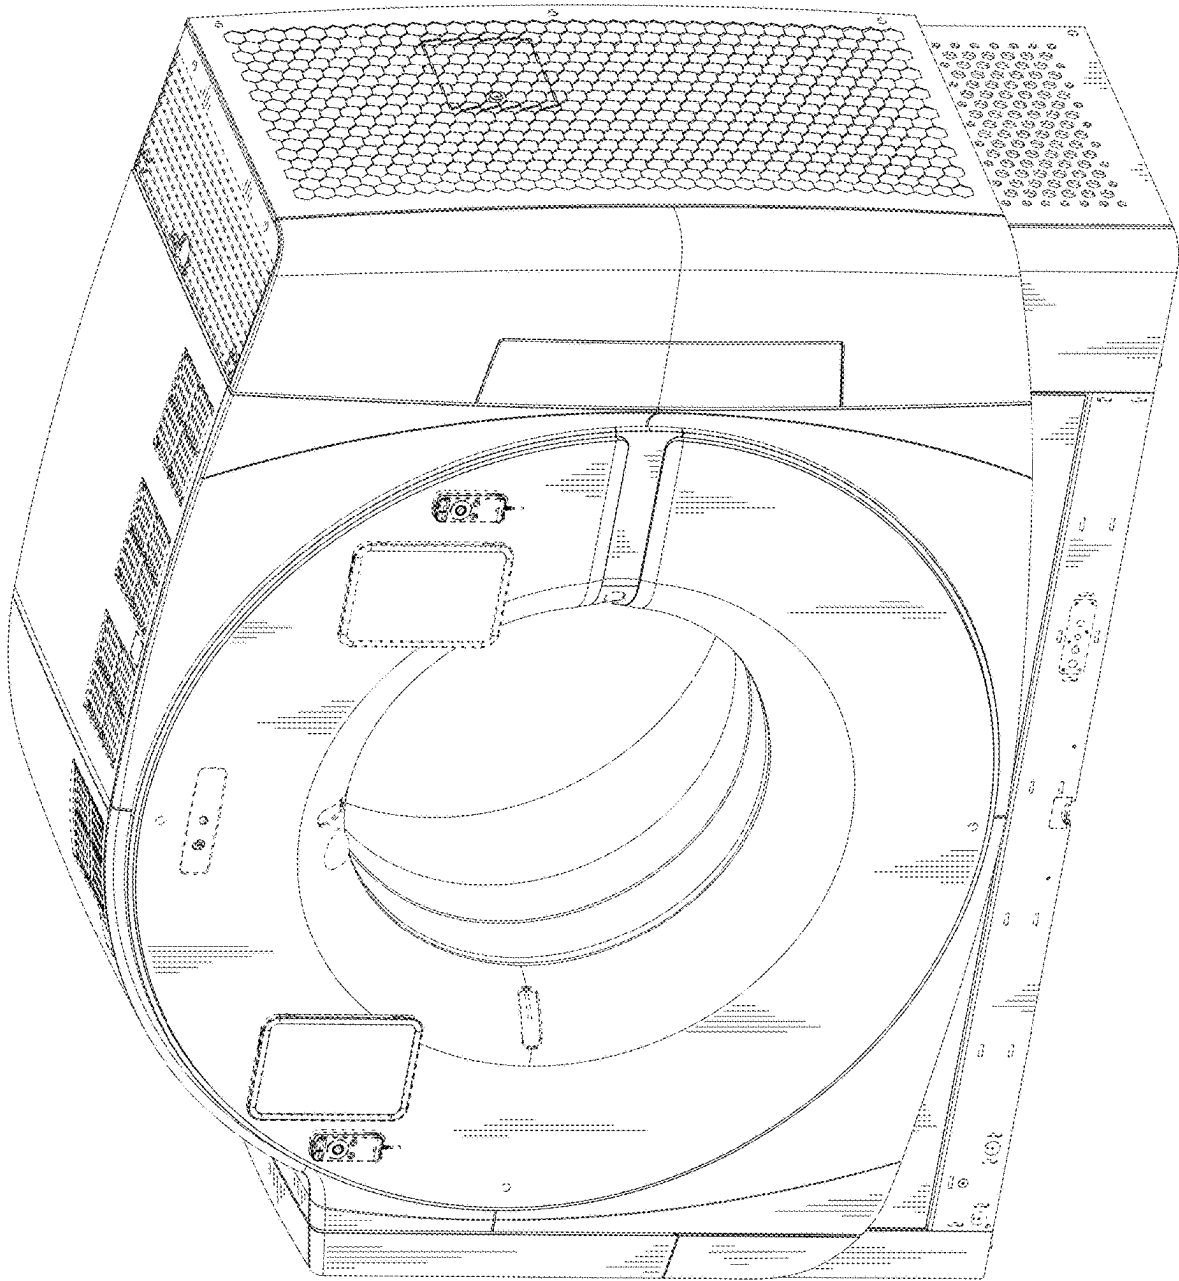

7
G.
F.