



US0D1088236S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,088,236 S**
Okada et al. (45) **Date of Patent:** **** Aug. 12, 2025**

(54) **EYE TESTING APPARATUS AND EQUIPMENT**

FOREIGN PATENT DOCUMENTS

JP D1752906 * 9/2023

(71) Applicant: **TOPCON CORPORATION**, Tokyo (JP)

OTHER PUBLICATIONS

(72) Inventors: **Hiroyuki Okada**, Tokyo (JP); **Takeo Aoki**, Tokyo (JP); **Yasuhisa Kaneda**, Tokyo (JP)

NW500 Non-Mydriatic Retinal Camera. 2023. Site visited Feb. 15, 2024. [chrome-extension://efaidnbmnnnibpcajpcglclefindmkaj/https://cdn.brandfolder.io/I6S47VV/at/5mhkhwjrzmsx6tksjzfzmm96/NW500_brochure.pdf] (Year: 2023).*

(73) Assignee: **TOPCON CORPORATION**, Tokyo (JP)

(Continued)

(**) Term: **15 Years**

Primary Examiner — Wendy L Arminio

Assistant Examiner — Maheen Khurshid

(21) Appl. No.: **29/827,178**

(74) *Attorney, Agent, or Firm* — Muncy, Geissler, Olds & Lowe, P.C.

(22) Filed: **Feb. 17, 2022**

(57) **CLAIM**

(51) **LOC (15) Cl.** **24-02**

The ornamental design for an eye testing apparatus and equipment as shown and described.

(52) **U.S. Cl.**

DESCRIPTION

USPC **D24/172**

(58) **Field of Classification Search**

USPC D24/170, 172, 185–187, 231, 232, 140, D24/158–160, 120, 184, 137; D15/199; D16/100, 130, 136, 200, 300

CPC A61B 3/024; A61B 3/113; A61B 3/028; A61B 3/112; A61B 3/14; A61B 3/00; A61B 3/0008; A61B 3/18; A61B 3/11; A61B 5/163; A61B 5/6821; G02B 27/0172; G02B 27/0025; G02B 27/0012; G02B 27/0093

See application file for complete search history.

FIG. 1 is a top, front, and right side perspective view of an eye testing apparatus and equipment showing our new design;

FIG. 2 is a bottom, front, and right side perspective view thereof;

FIG. 3 is a bottom, back, and left side perspective view thereof;

FIG. 4 is a front view thereof;

FIG. 5 is a back view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof;

FIG. 8 is a right side elevational view thereof;

FIG. 9 is a left side elevational view thereof; and,

FIG. 10 is a top, front, left side perspective view showing the eye testing apparatus and equipment in an alternate position. In the drawings, the broken lines depict portions of the eye testing apparatus and equipment that form no part of the claimed design.

(56) **References Cited**


U.S. PATENT DOCUMENTS

D341,541 S * 11/1993 Ichiyoshi D10/46
5,474,066 A * 12/1995 Grolman A61B 3/165
600/401

D390,662 S * 2/1998 Cooper D24/172
D394,505 S * 5/1998 Hayashi D24/172

(Continued)

1 Claim, 10 Drawing Sheets

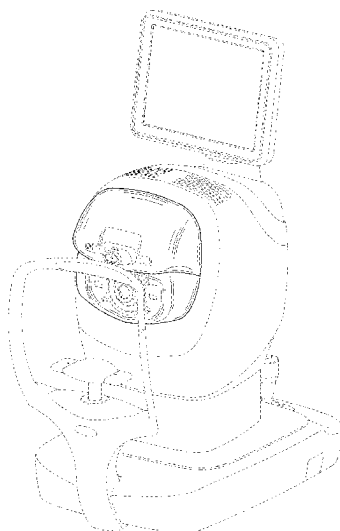

References Cited

D922,583	S *	6/2021	Kobayashi	D24/172
D935,619	S *	11/2021	Huber-Meznaric	D24/172
D936,834	S *	11/2021	Yamaoka	D24/172
D936,835	S *	11/2021	Yamaoka	D24/172
D971,037	S *	11/2022	Ishii	D10/66
2019/0380571	A1 *	12/2019	Kitamura	A61B 3/152

5,838,424	A	*	11/1998	Wawro	A61B 3/02
					351/200
D436,665	S	*	1/2001	Becker	D24/172
D472,637	S	*	4/2003	Cooper	D24/172
D552,736	S	*	10/2007	Yamaoka	D24/172
D589,622	S	*	3/2009	Koest	D10/46
D614,774	S	*	4/2010	Gausmann	D24/160
D694,890	S	*	12/2013	Bott	D24/172
D698,444	S	*	1/2014	Mensink	D24/172
D705,430	S	*	5/2014	Sekine	D24/172
D738,509	S	*	9/2015	van Elzakker	D24/172
D812,759	S	*	3/2018	Sekine	G01N 23/046
					D24/172
D827,833	S	*	9/2018	Brottier	A61F 9/008
					D24/172
D834,968	S	*	12/2018	Ishii	D10/66
10,278,587	B2	*	5/2019	Grenon	A61B 5/0077


Topcon NW500 Non-mydiatic Retinal Camera. Apr. 6, 2023. Site visited Feb. 15, 2024. [<https://www.youtube.com/watch?v=59rLGYc4p9c>] (Year: 2023).*

Kowa Nonmyd AF—Non-Mydriatic Retinal Camera. Jul. 23, 2020. Site visited Feb. 15, 2024. [<https://www.youtube.com/watch?v=YVt1YALF6qA>] (Year: 2020).*


TFC-1000 Non-Mydriatic Fundus Camera. Jun. 8, 2020. Site visited Feb. 15, 2024. [<https://www.youtube.com/watch?v=t6ILFvHvQFs>] (Year: 2020).*

* cited by examiner


F I G. 1

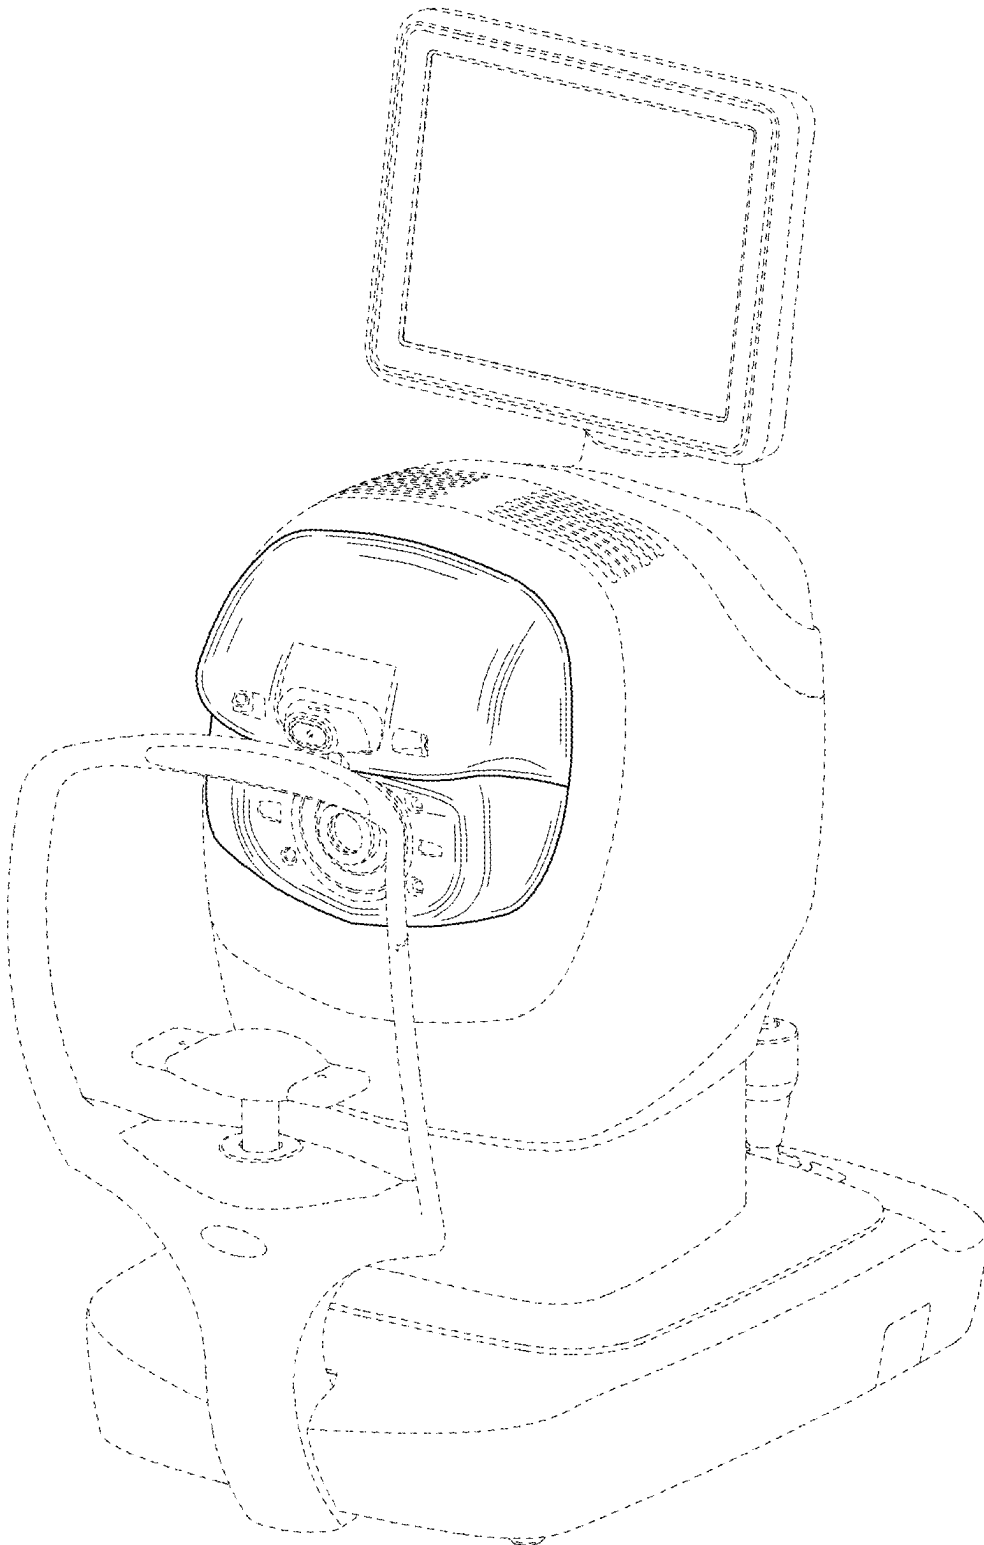


F I G. 2

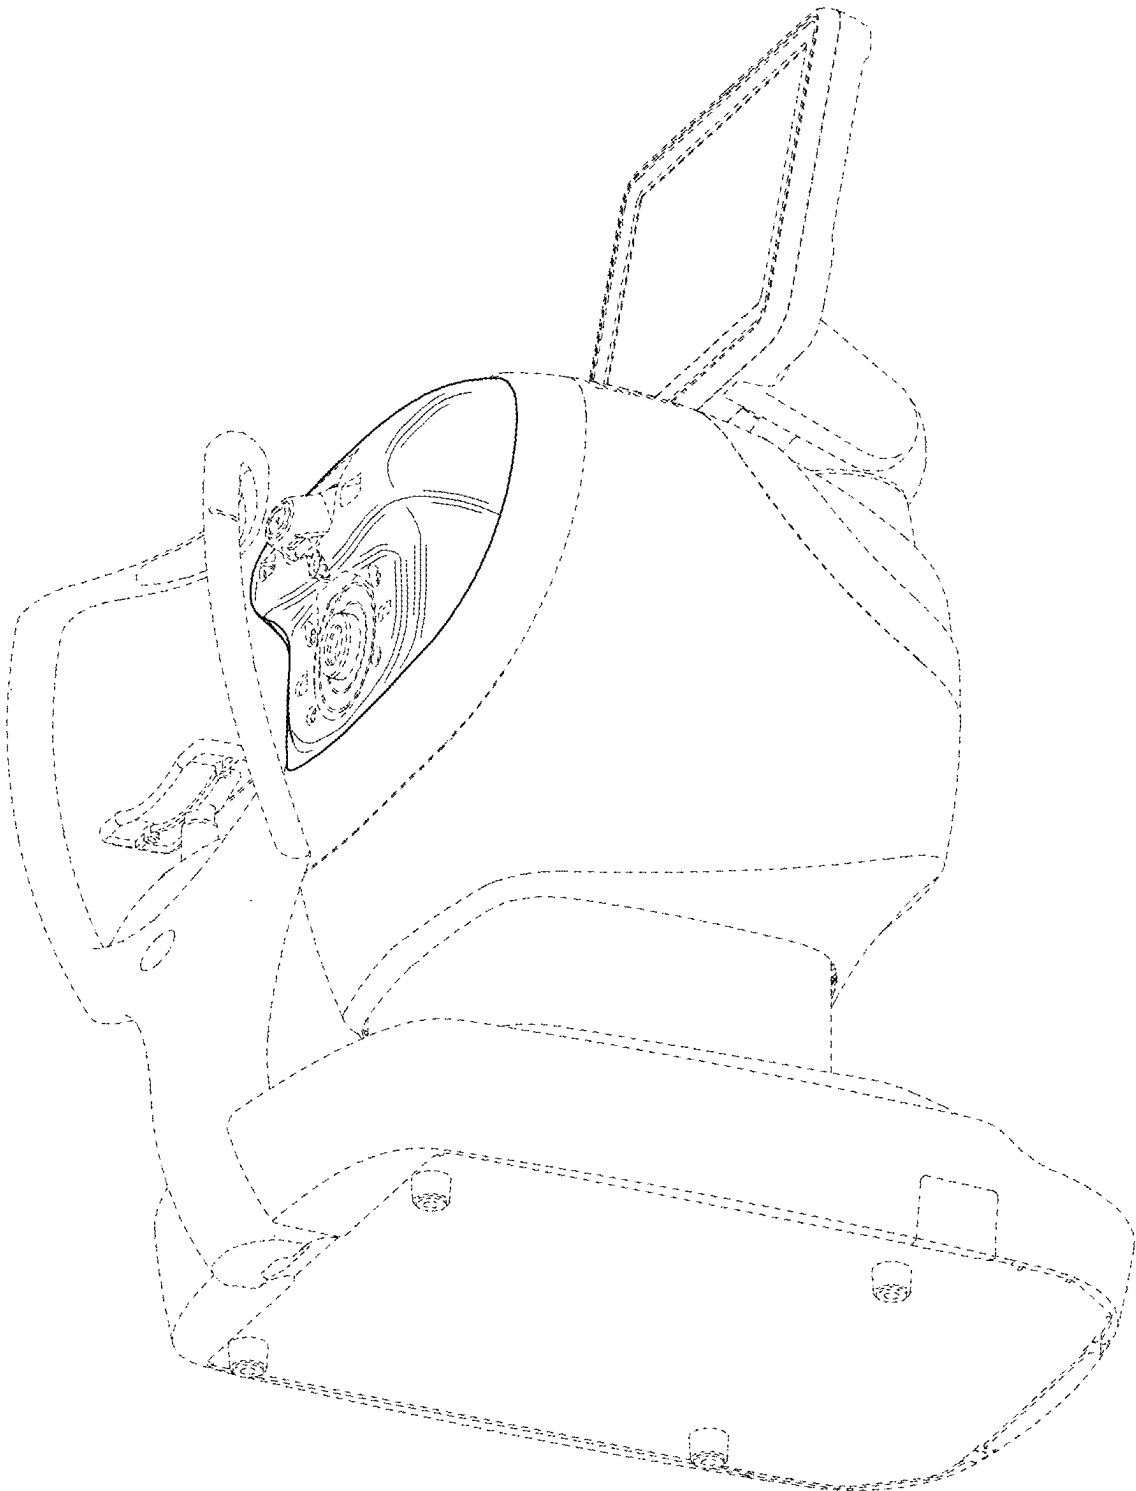


F I G. 3

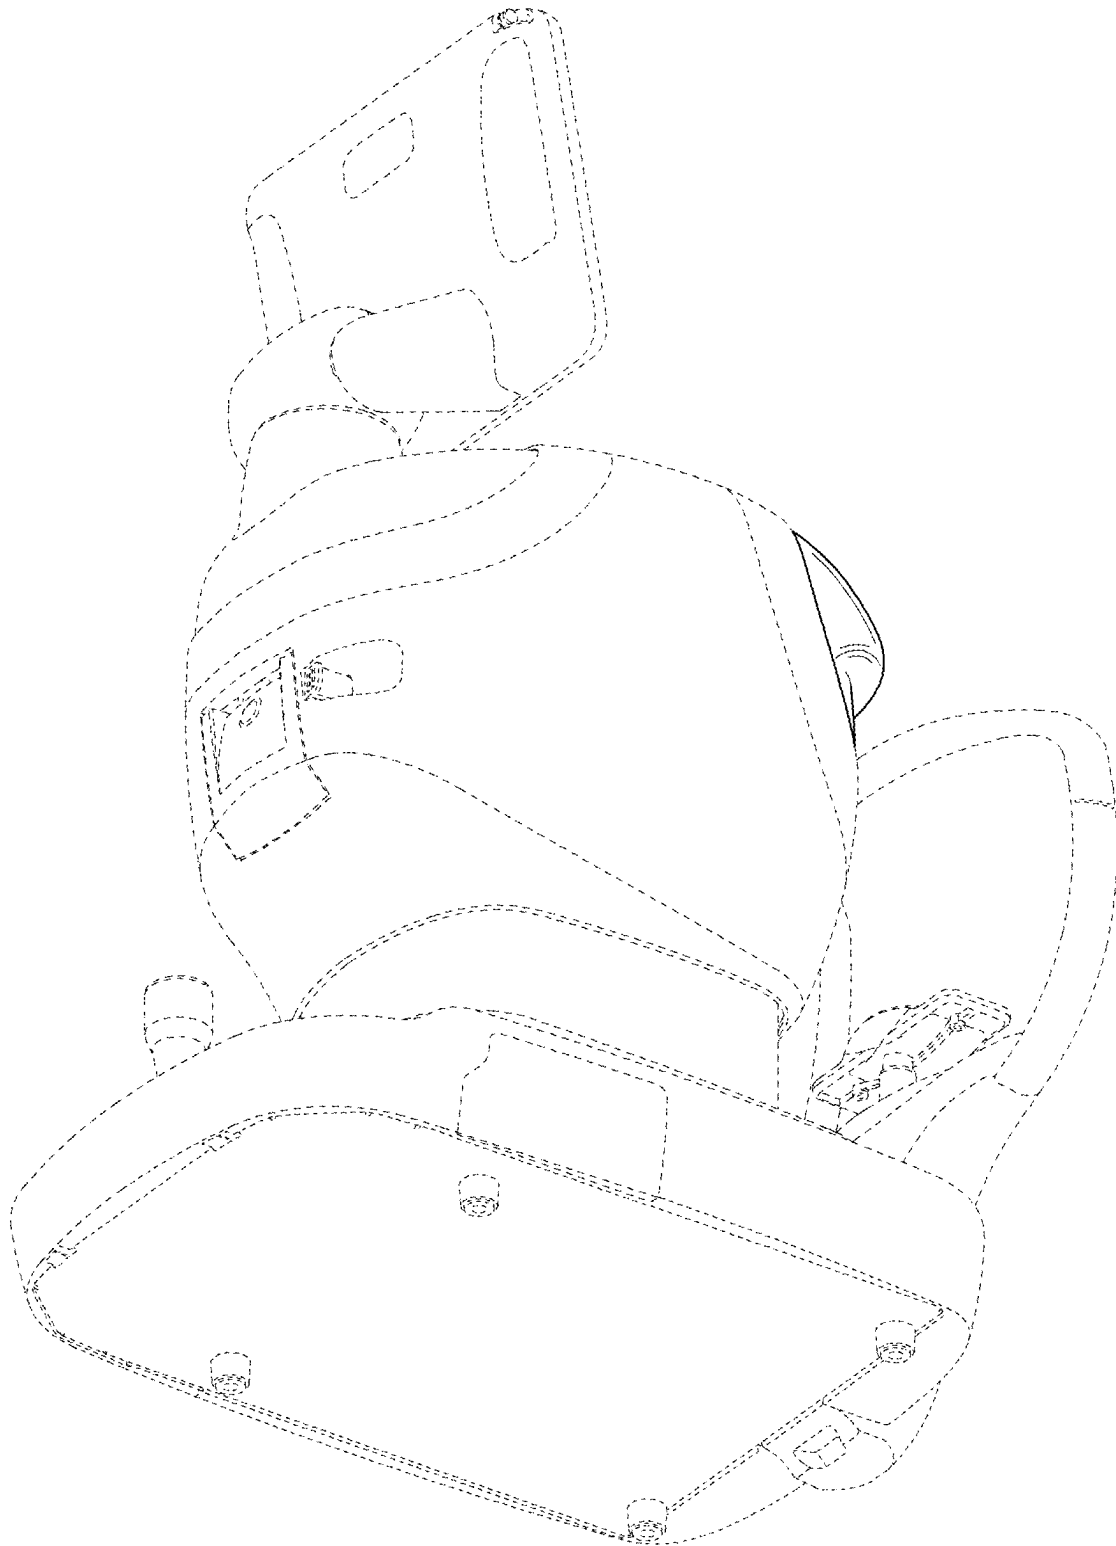


F I G. 4

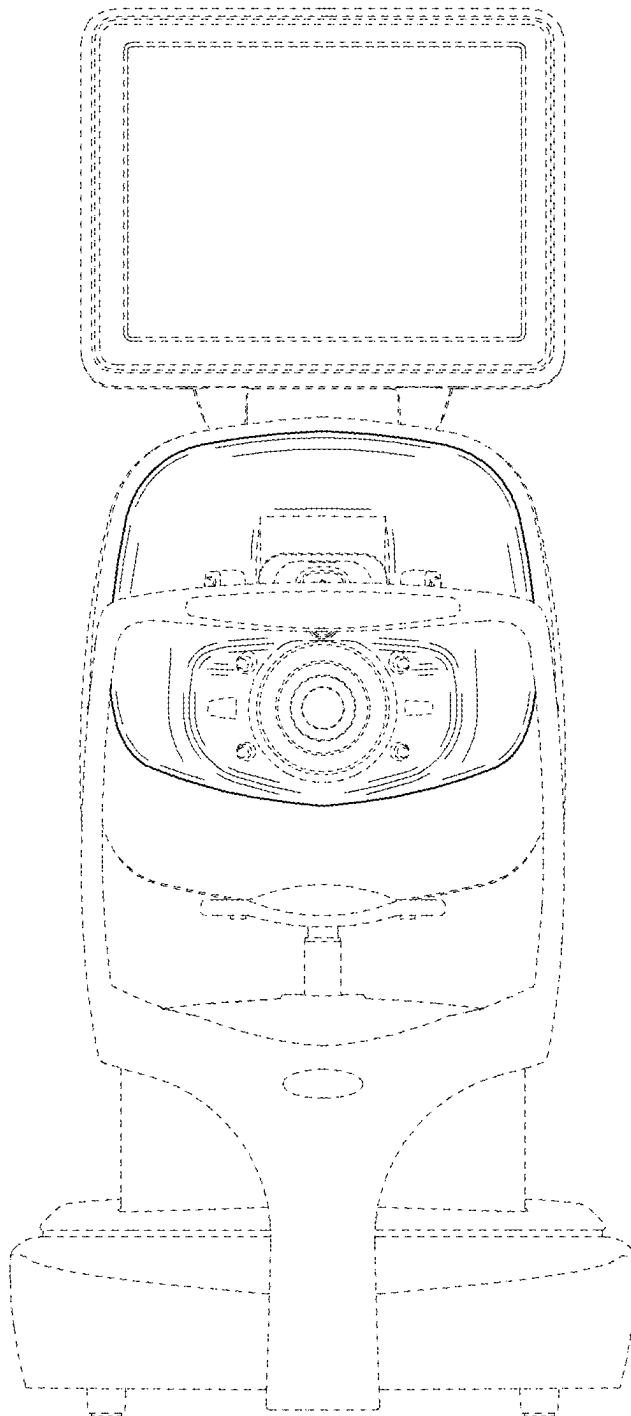


F I G. 5

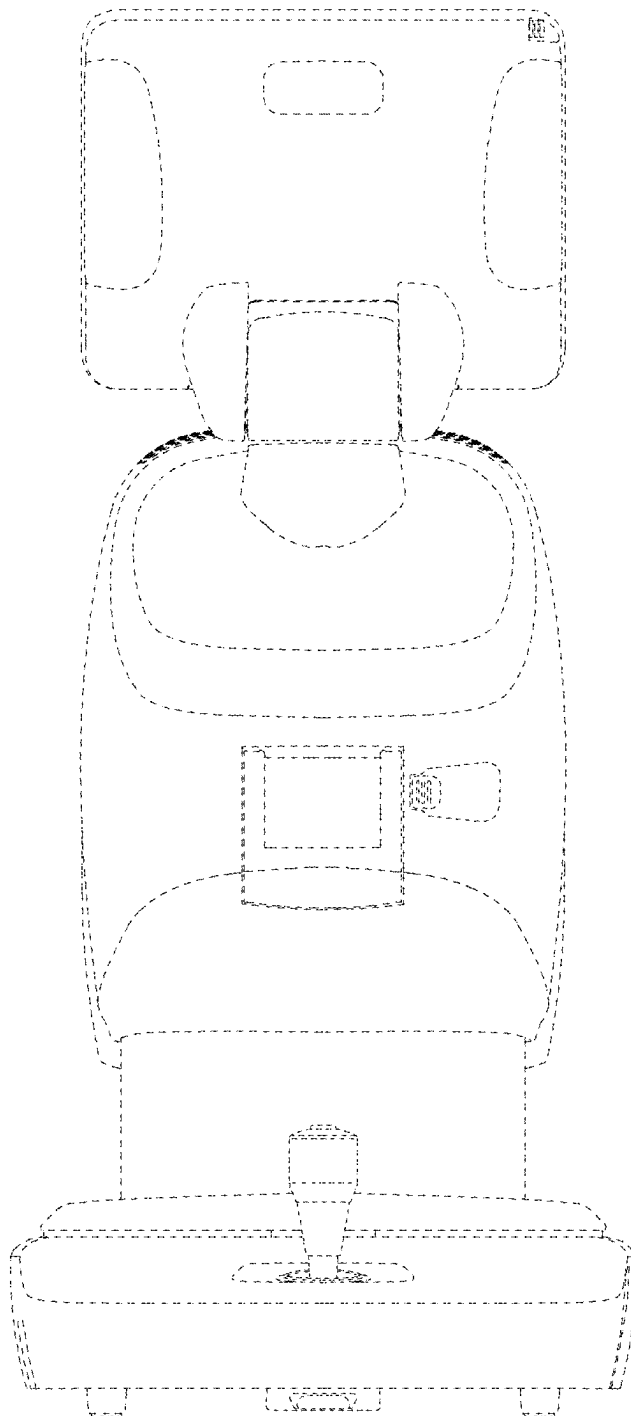


F I G. 6

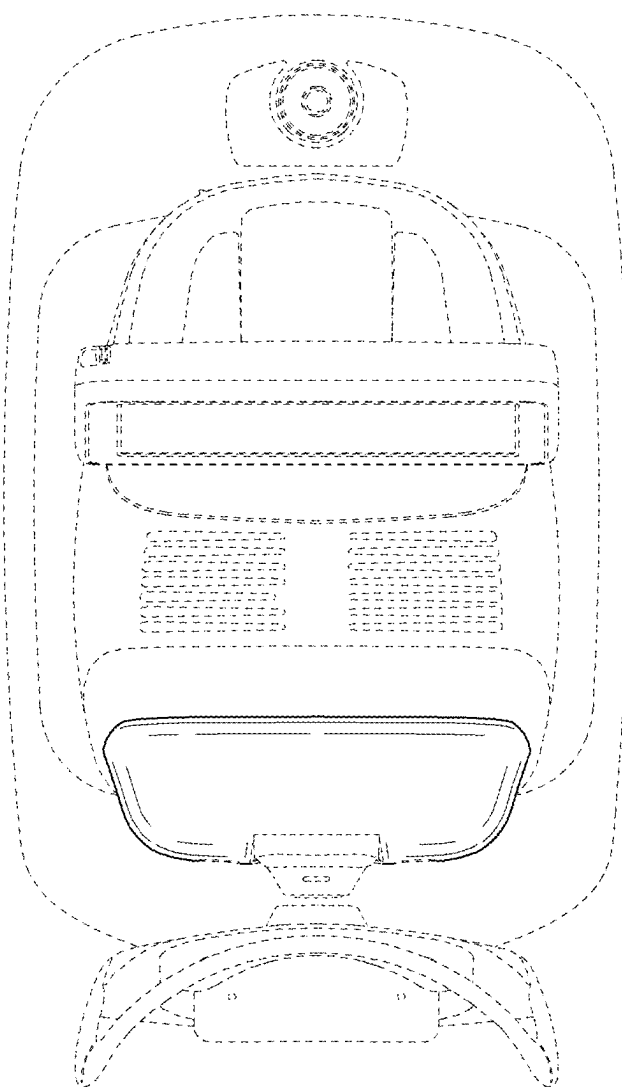


F I G. 7

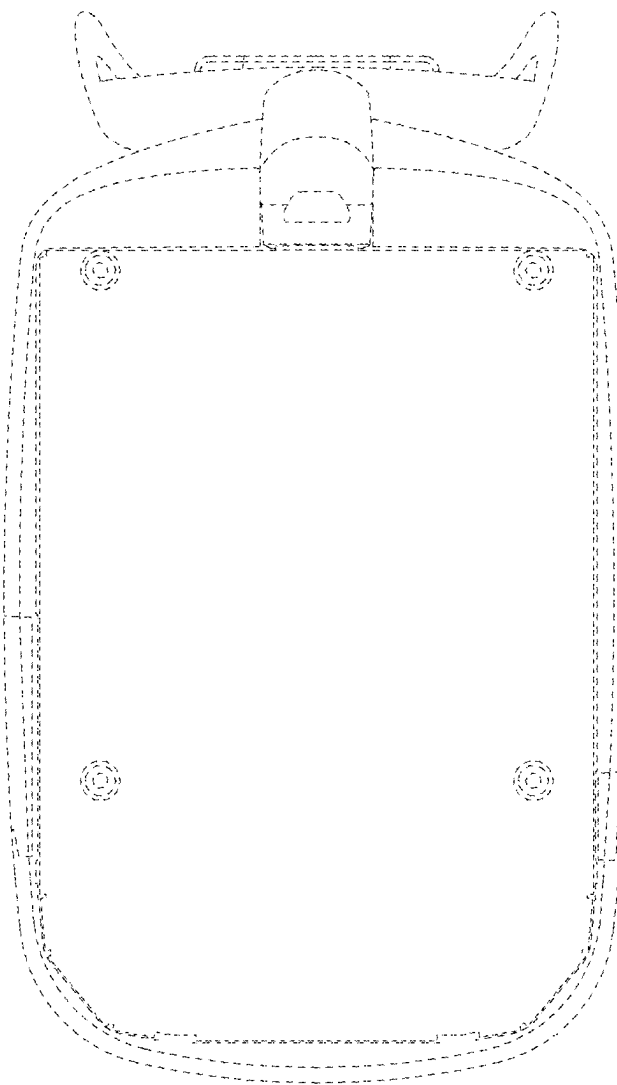

F I G. 8

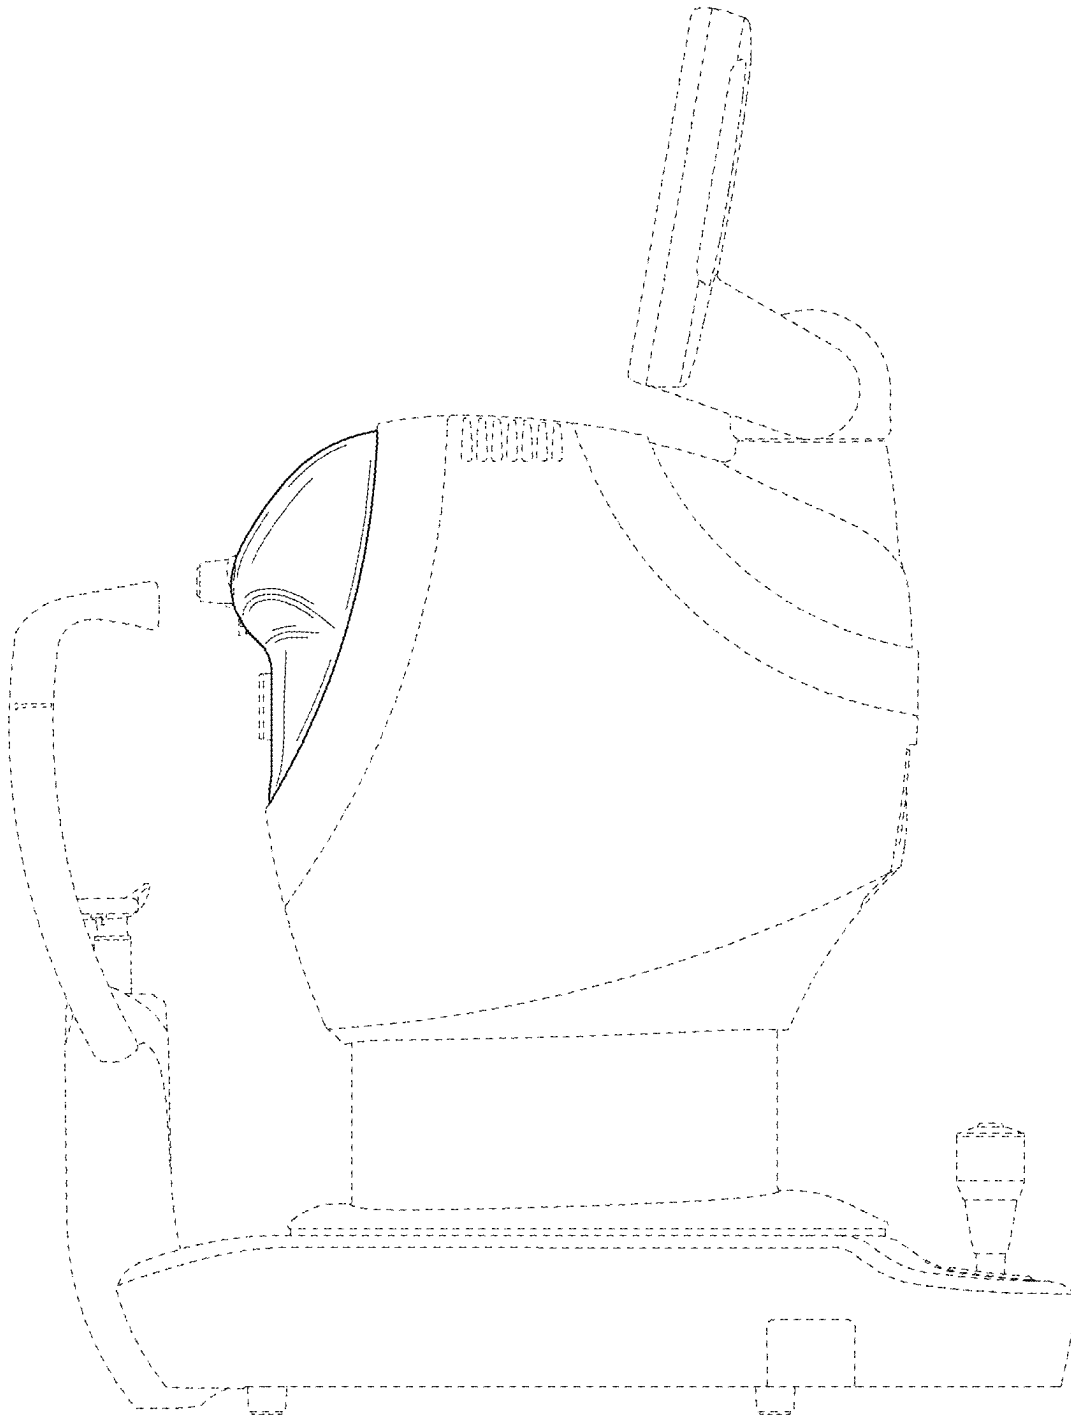

F I G. 9

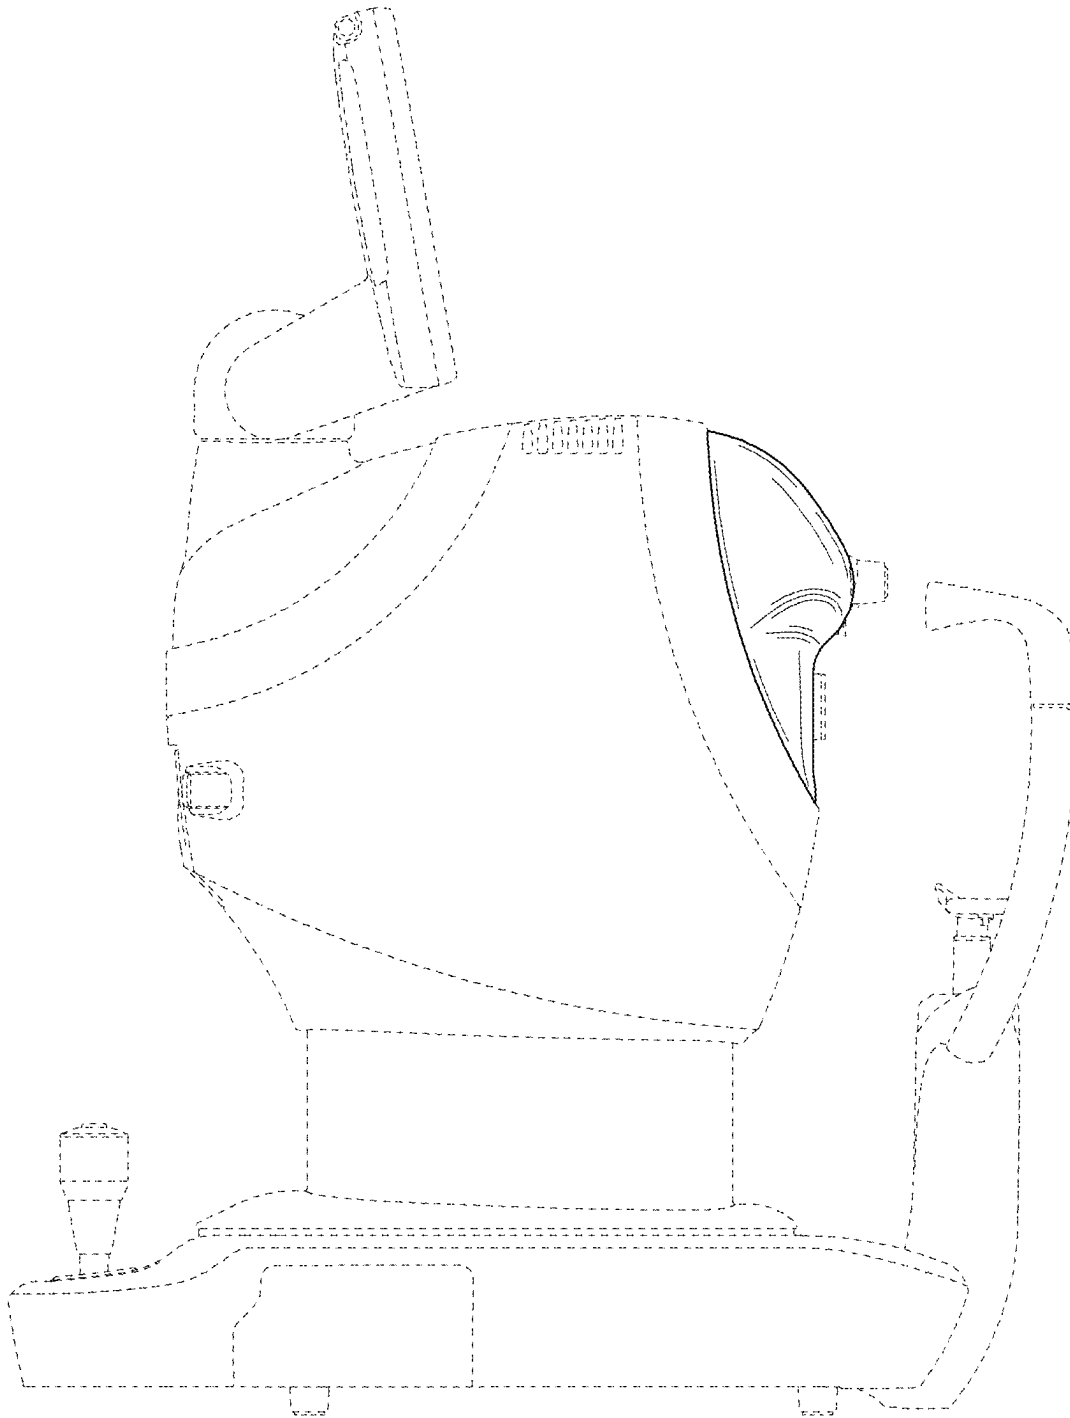

F I G. 10

