



US0D1090854S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,090,854 S**
Wappler et al. (45) **Date of Patent:** **** Aug. 26, 2025**

(54) **MEDICAL TROLLEY**

(71) Applicant: **AGILE ROBOTS SE**, Munich (DE)

(72) Inventors: **Fabian Wappler**, Munich (DE); **Daniel Dür**, Munich (DE)

(73) Assignee: **Agile Robots AG**, Munich (DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/944,183**

(22) Filed: **May 27, 2024**

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.** **D24/185**
USPC **D24/185**

(58) **Field of Classification Search**
USPC D24/185–187, 121–123
CPC A61B 5/0002; A61B 5/0013; A61B 5/002;
A61B 5/742

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D486,915	S	*	2/2004	Warschewske		D24/185
D808,533	S	*	1/2018	Verguldi		D24/185
D837,380	S	*	1/2019	Hulford		D24/185
D852,963	S	*	7/2019	Shuart		D24/185
D874,655	S	*	2/2020	Calef		D24/185
D879,967	S	*	3/2020	Verguldi		D24/185
D890,351	S	*	7/2020	Sung		D24/185
D936,230	S	*	11/2021	Prout		D24/185
D950,734	S	*	5/2022	Cho		D24/185
11,553,160	B1	*	1/2023	Schultz		A61B 50/13
D1,030,067	S	*	6/2024	Liao		D24/185

D1,046,160	S	*	10/2024	Matuschek		D24/185
D1,049,387	S	*	10/2024	Polasek		D24/185
D1,059,599	S	*	1/2025	Chen		D24/185
D1,066,681	S	*	3/2025	Chen		D24/185

OTHER PUBLICATIONS

Medical Rehabilitation System, Agile Robots SE, posted 2025, retrieved Jun. 4, 2025, online, URL: <https://ifdesign.com/en/winner-ranking/project/medical-rehabilitation-system/679261> (Year: 2025).*

* cited by examiner

Primary Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Sutton Magidoff
Barkume LLP


(57) **CLAIM**

The ornamental design for a medical trolley as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical trolley showing our new design;
FIG. 2 is a right view of the article of FIG. 1;
FIG. 3 is a left view of the article of FIG. 1;
FIG. 4 is a front view of the article of FIG. 1;
FIG. 5 is a rear view of the article of FIG. 1;
FIG. 6 is a top view of the article of FIG. 1;
FIG. 7 is a bottom view of the article of FIG. 1; and,
FIG. 8 is another perspective view of the article of FIG. 1.
The broken lines shown in FIGS. 1, 2, 3, 4, 5, 6, 7, and 8, illustrate portions of the medical trolley that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

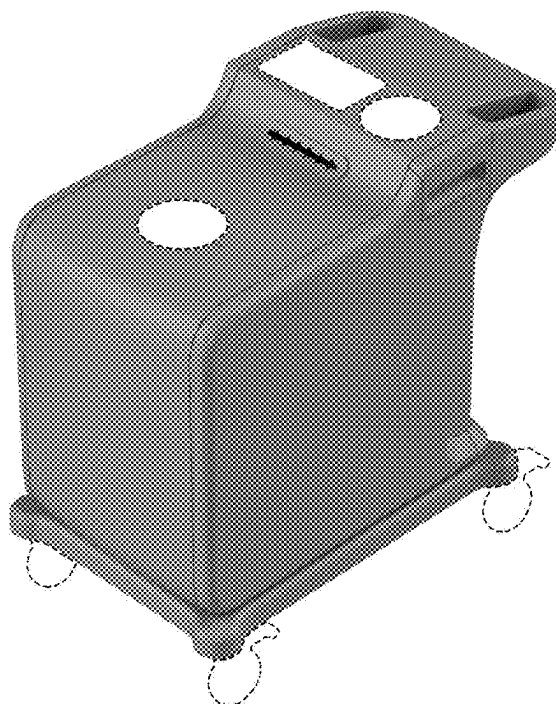

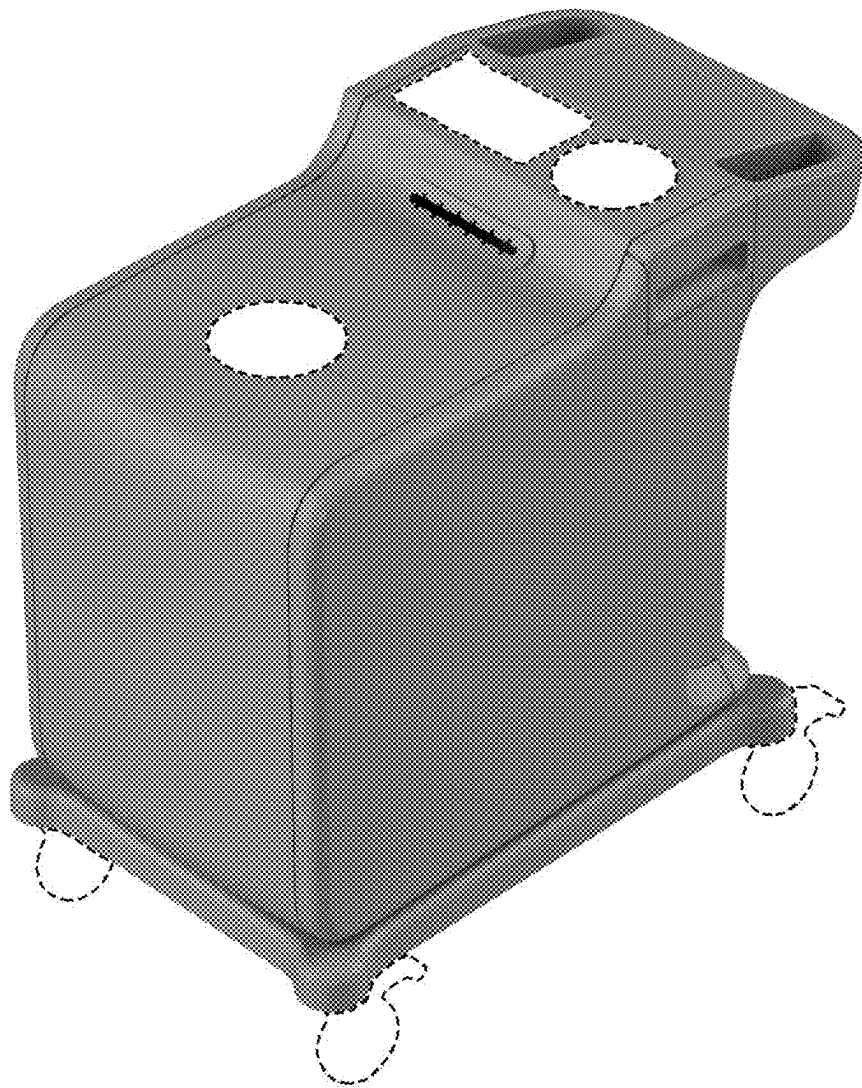


FIG. 1

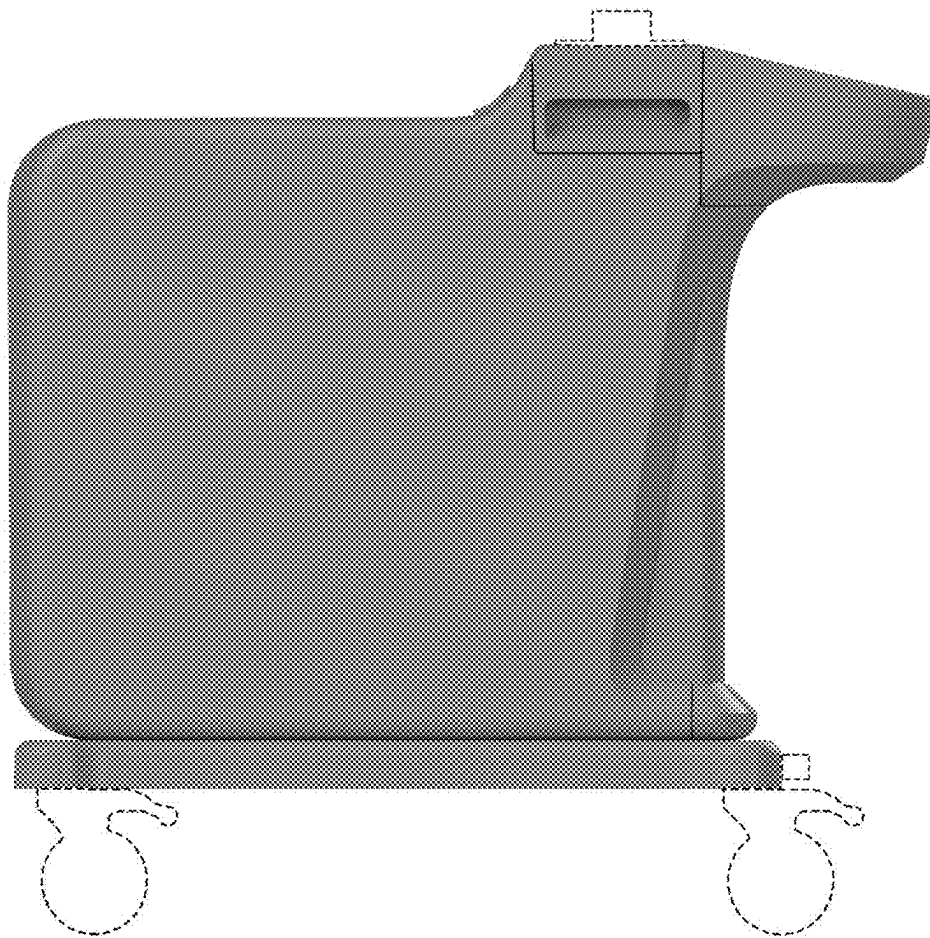


FIG. 2

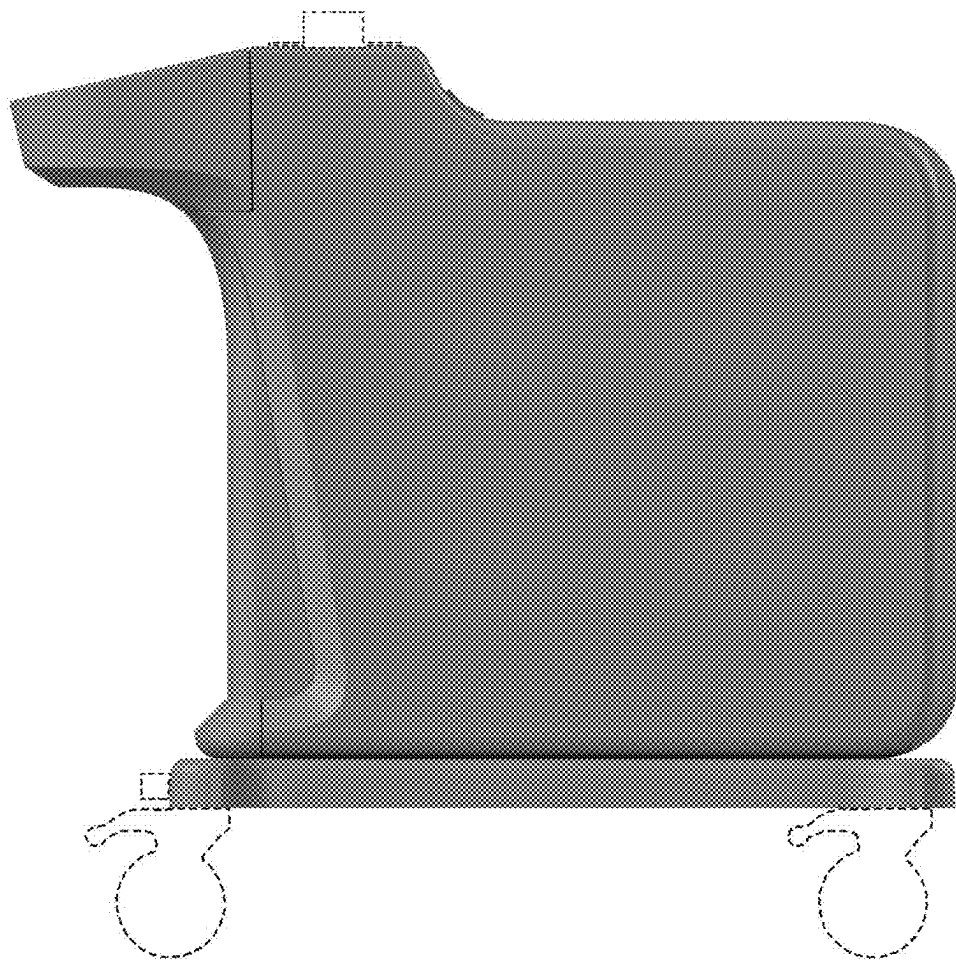


FIG. 3



FIG. 4



FIG. 5

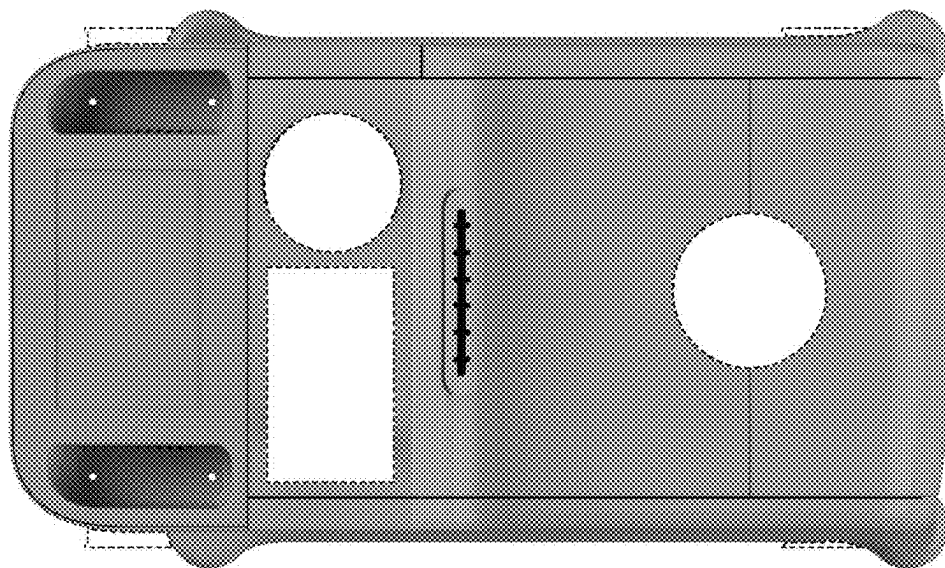


FIG. 6

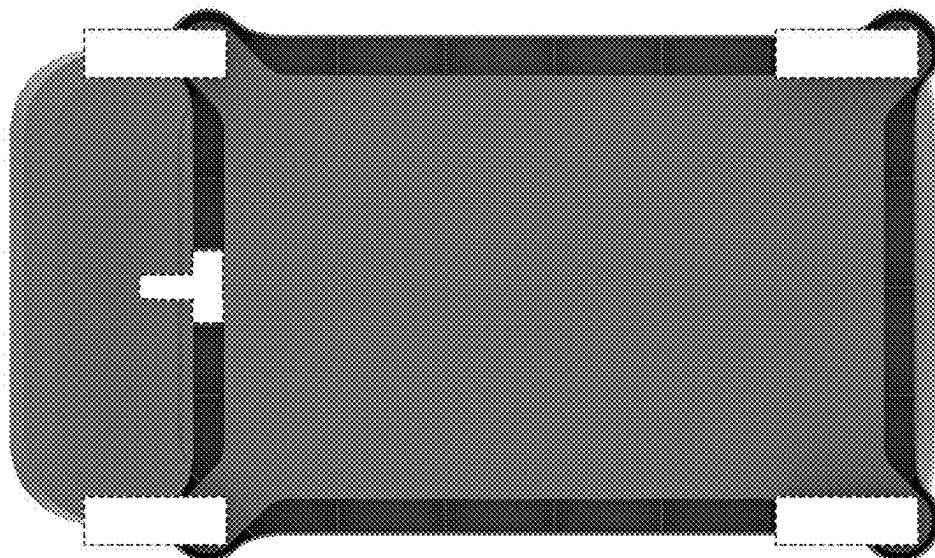


FIG. 7

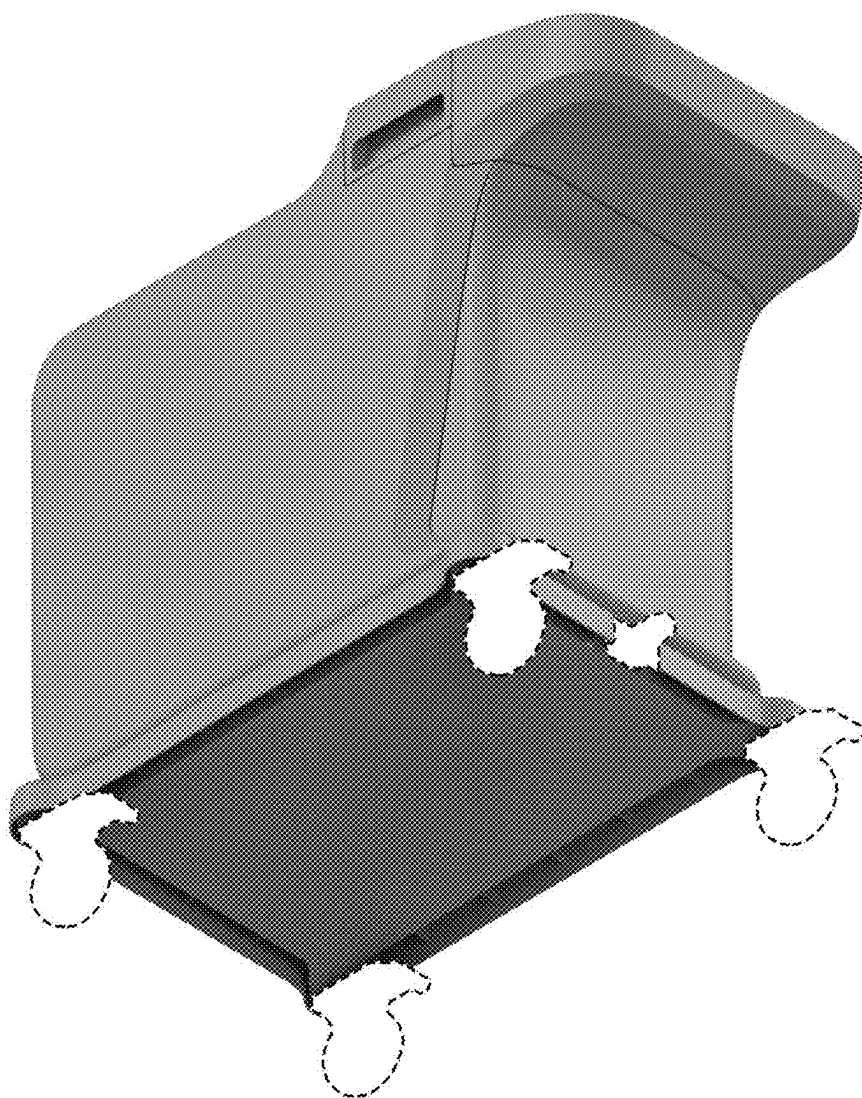


FIG. 8