



US0D1093609S

(12) **United States Design Patent**
Pittsford et al.

(10) **Patent No.:** **US D1,093,609 S**
(45) **Date of Patent:** **** Sep. 16, 2025**

(54) **TIP FOR A MEDICAL DEVICE**

(71) Applicant: **Solta Medical Ireland Limited**, Dublin
(IE)

(72) Inventors: **Jonathan Pittsford**, Everett, WA (US);
Roland Horth, Whangarei (NZ)

(73) Assignee: **Solta Medical Ireland Limited**, Dublin
(IE)

(**) Term: **15 Years**

(21) Appl. No.: **29/874,006**

(22) Filed: **Apr. 12, 2023**

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/209**

(58) **Field of Classification Search**

USPC D24/100, 107, 185, 186, 187, 188, 200,
D24/206, 209, 210, 211, 214; D28/44,
D28/45, 46, 47, 48, 49, 51, 52, 53, 54, 99
CPC B26B 19/00; B26B 19/02; B26B 19/04;
B26B 19/06; B26B 19/10; B26B 19/20;
B26B 19/22; B26B 19/38; B26B 19/3806;
B26B 21/00; B26B 21/22; B26B 21/40;
B26B 21/4012; B26B 21/4018; A61H
2039/005; A45D 2200/1054

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,405,439	B1 *	6/2002	Malobabic		B26B 19/06
					30/346.51
6,568,083	B1 *	5/2003	Taniguchi		B26B 19/10
					30/43.2
D567,444	S *	4/2008	Giannini		D28/54
D646,396	S *	10/2011	Seki		D24/209
D672,879	S *	12/2012	Hawkins		D24/200
D713,537	S *	9/2014	Ben-Haim		D24/200
D820,464	S *	6/2018	Gabriele		D24/209
D961,785	S *	8/2022	Hool		D24/200

(Continued)

FOREIGN PATENT DOCUMENTS

CN	303350932	S	8/2015
CN	304718364	*	7/2018

(Continued)

OTHER PUBLICATIONS

“PhxSkin Dermatology: Clear + Brilliant Touch Laser.” Found online Feb. 7, 2025 at youtube.com. Reference dated May 19, 2021. Retrieved from https://www.youtube.com/watch?v=EDmdSpNI_wY.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson,
Farabow, Garrett & Dunner, LLP

(57) **CLAIM**



The ornamental design for a tip for a medical device as shown and described.

DESCRIPTION

FIG. 1 is a front, left, bottom perspective view of a tip for a medical device showing the new design; FIG. 2 is a front elevation view thereof; FIG. 3 is a rear elevation view thereof; FIG. 4 is a right side view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a bottom plan view thereof; and, FIG. 7 is a top plan view thereof.

The dash-dot-dash broken lines illustrate the boundary of the claimed design and form no part thereof. The equal-length broken lines shown in the drawings illustrate portions of the tip for a medical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

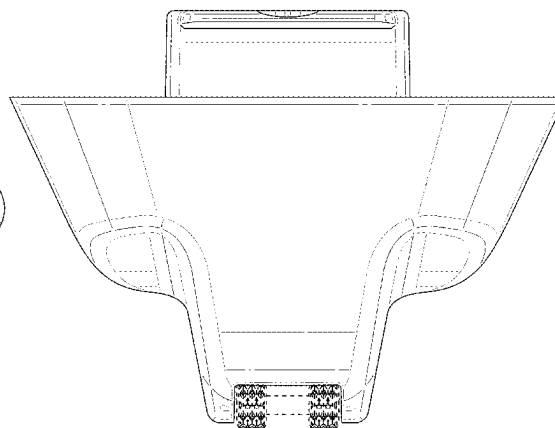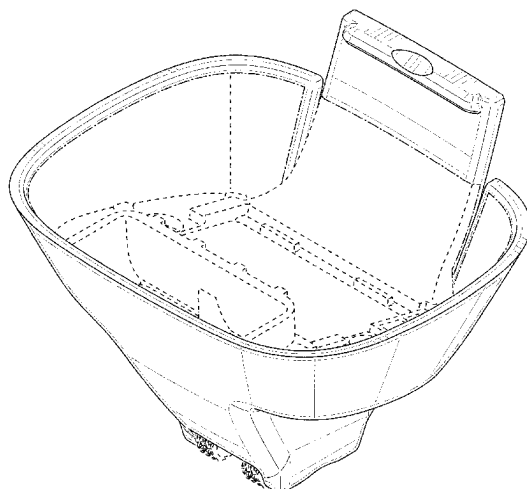

(56)

References Cited

U.S. PATENT DOCUMENTS

D970,741	S	*	11/2022	Holmberg		D24/209
D979,843	S	*	2/2023	Lyles		D28/51
D981,045	S	*	3/2023	Goeder		D28/54
D983,455	S	*	4/2023	Kulshreshtha		D28/51
D1,033,624	S	*	7/2024	Bradish, III		D24/107

FOREIGN PATENT DOCUMENTS

CN	304999619	*	1/2019
CN	305133445	S	4/2019
CN	305414141	S	11/2019
CN	306055755	S	9/2020
CN	306505709	S	4/2021
CN	306798410	S	8/2021
CN	307196831	S	3/2022
CN	307409765	S	6/2022
CN	308016420	S	5/2023
JP	D1637717	S	7/2019
JP	D1786416	*	12/2024
JP	D1786417	*	12/2024

OTHER PUBLICATIONS

“Severn River Medspa: Preparing for Your CO2 Laser Treatment: Essential Tips.” Found online Feb. 7, 2025 at [aaentmd.com](https://aaentmd.com/blog/preparing-for-your-co2-laser-treatment-essential-tips/). Reference dated Feb. 6, 2024. Retrieved from <https://aaentmd.com/blog/preparing-for-your-co2-laser-treatment-essential-tips/>.*

“Allure: Dermatologists Explain the Best Laser Treatments for Dark Skin Tones.” Found online Feb. 7, 2025 at [allure.com](https://www.allure.com/story/best-laser-treatments-for-dark-skin-at-dermatologist). Reference dated Apr. 19, 2018. Retrieved from <https://www.allure.com/story/best-laser-treatments-for-dark-skin-at-dermatologist>.*

“Teanna’s Channel: Vlog Clear + Brilliant Laser Treatment at Laser Away.” Found online.*

* cited by examiner

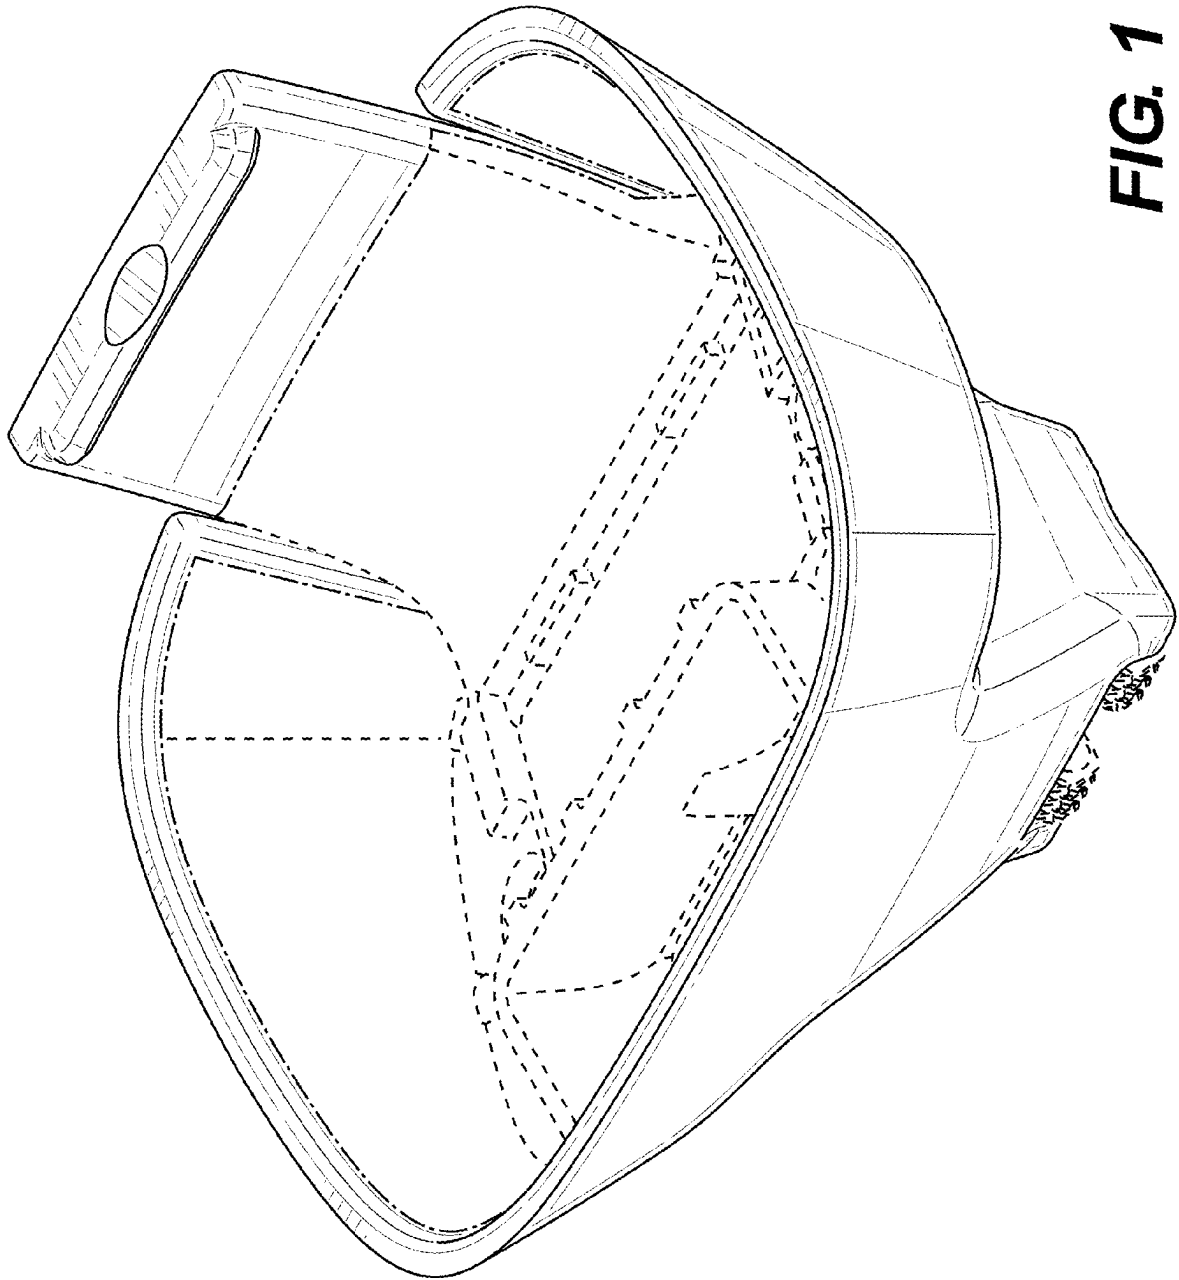


FIG. 1

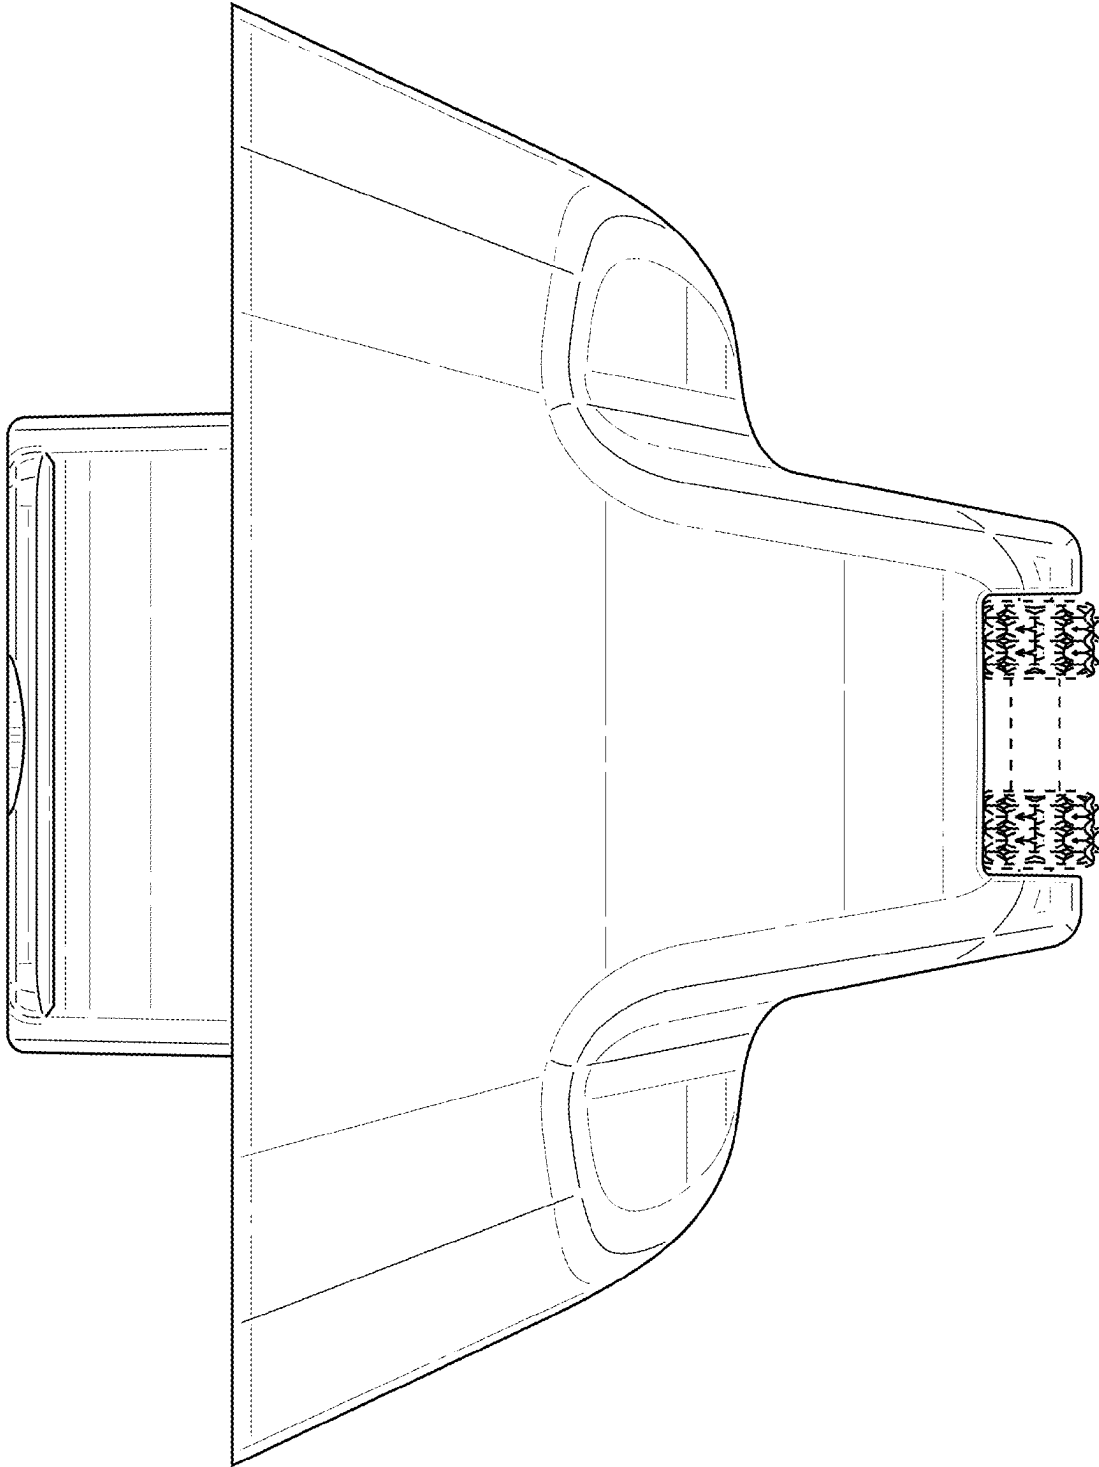


FIG. 2

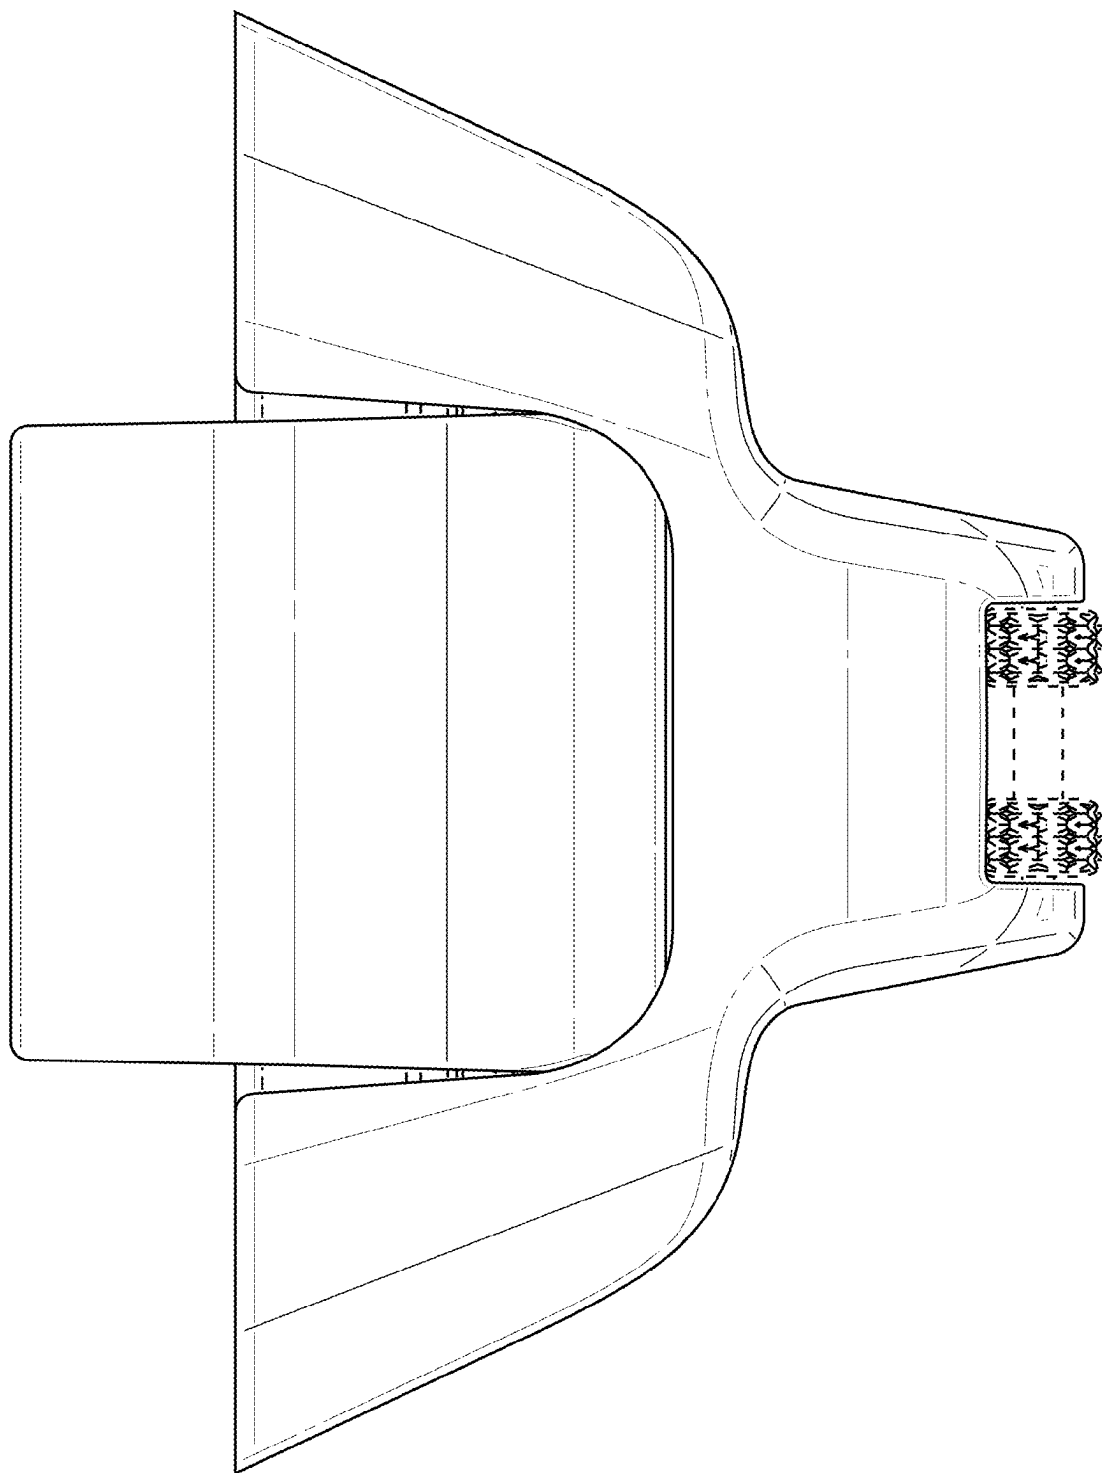


FIG. 3

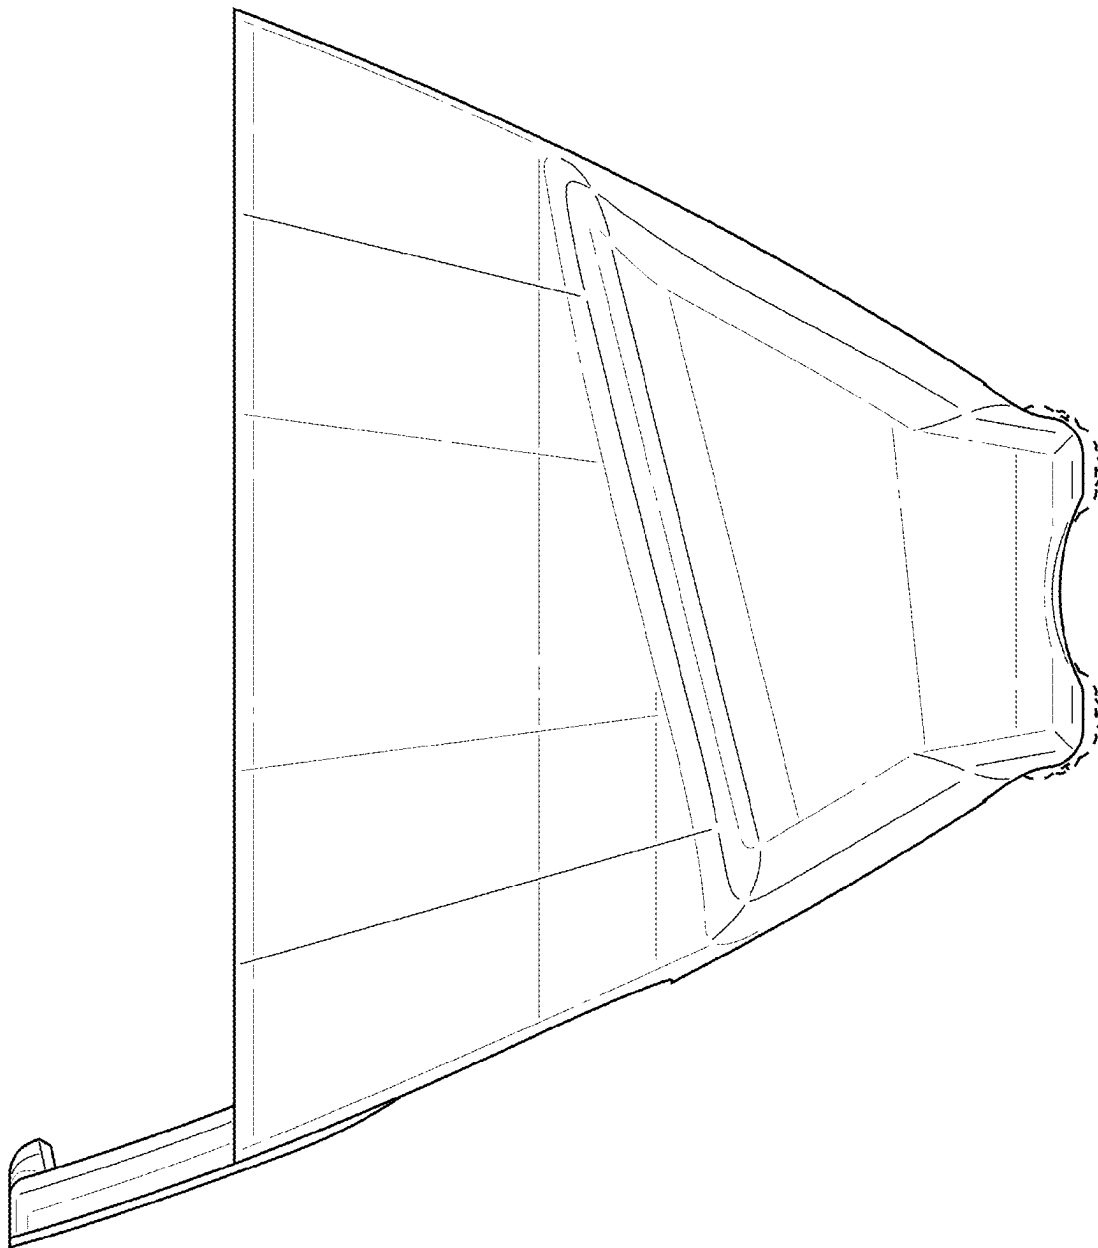


FIG. 4

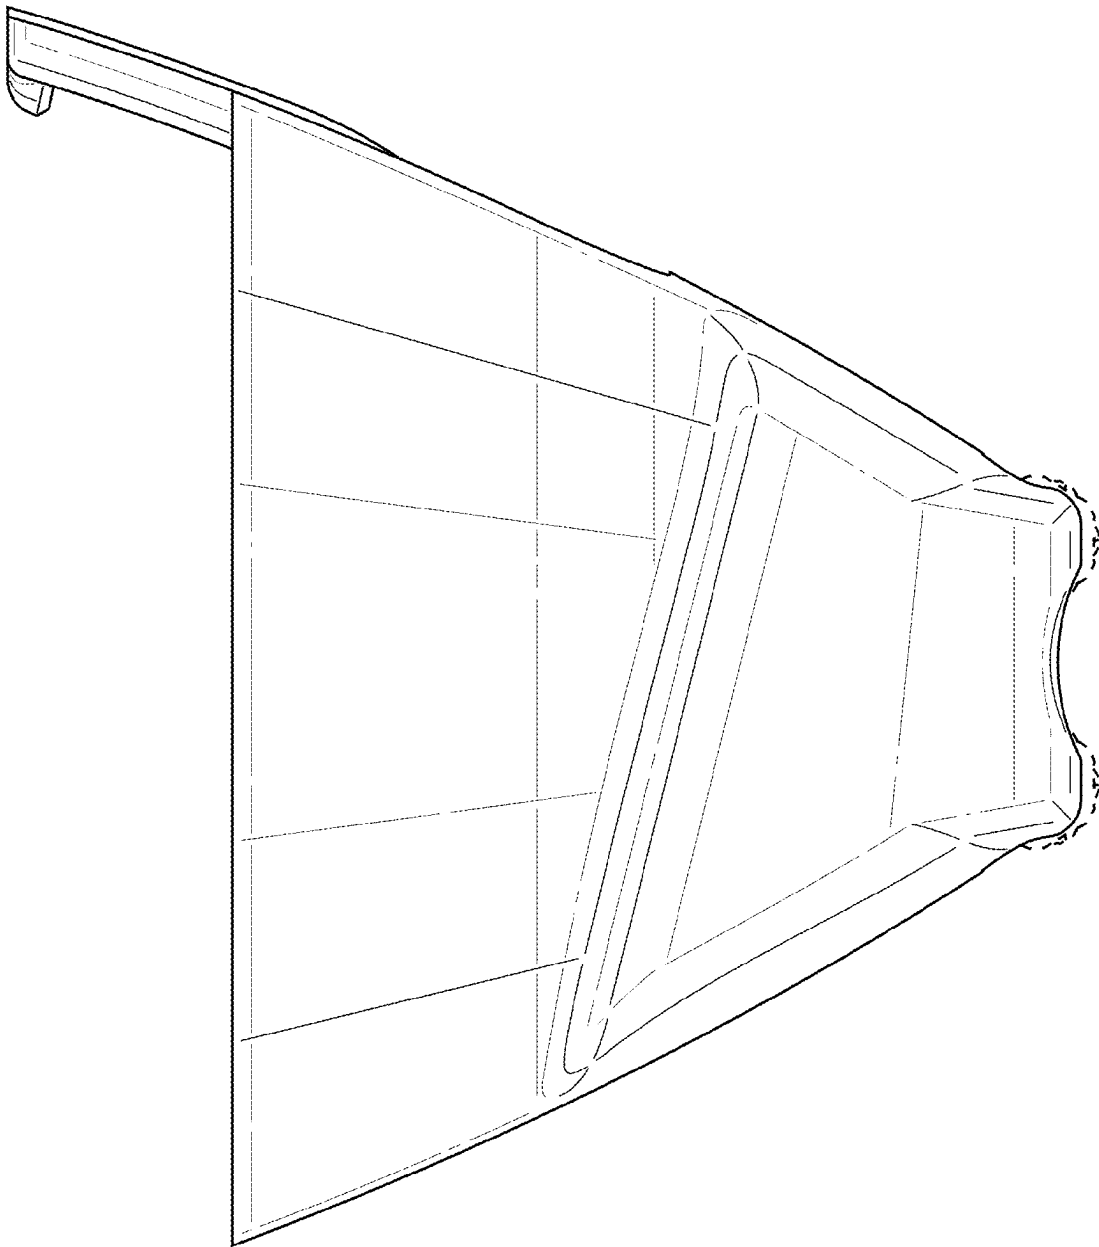


FIG. 5

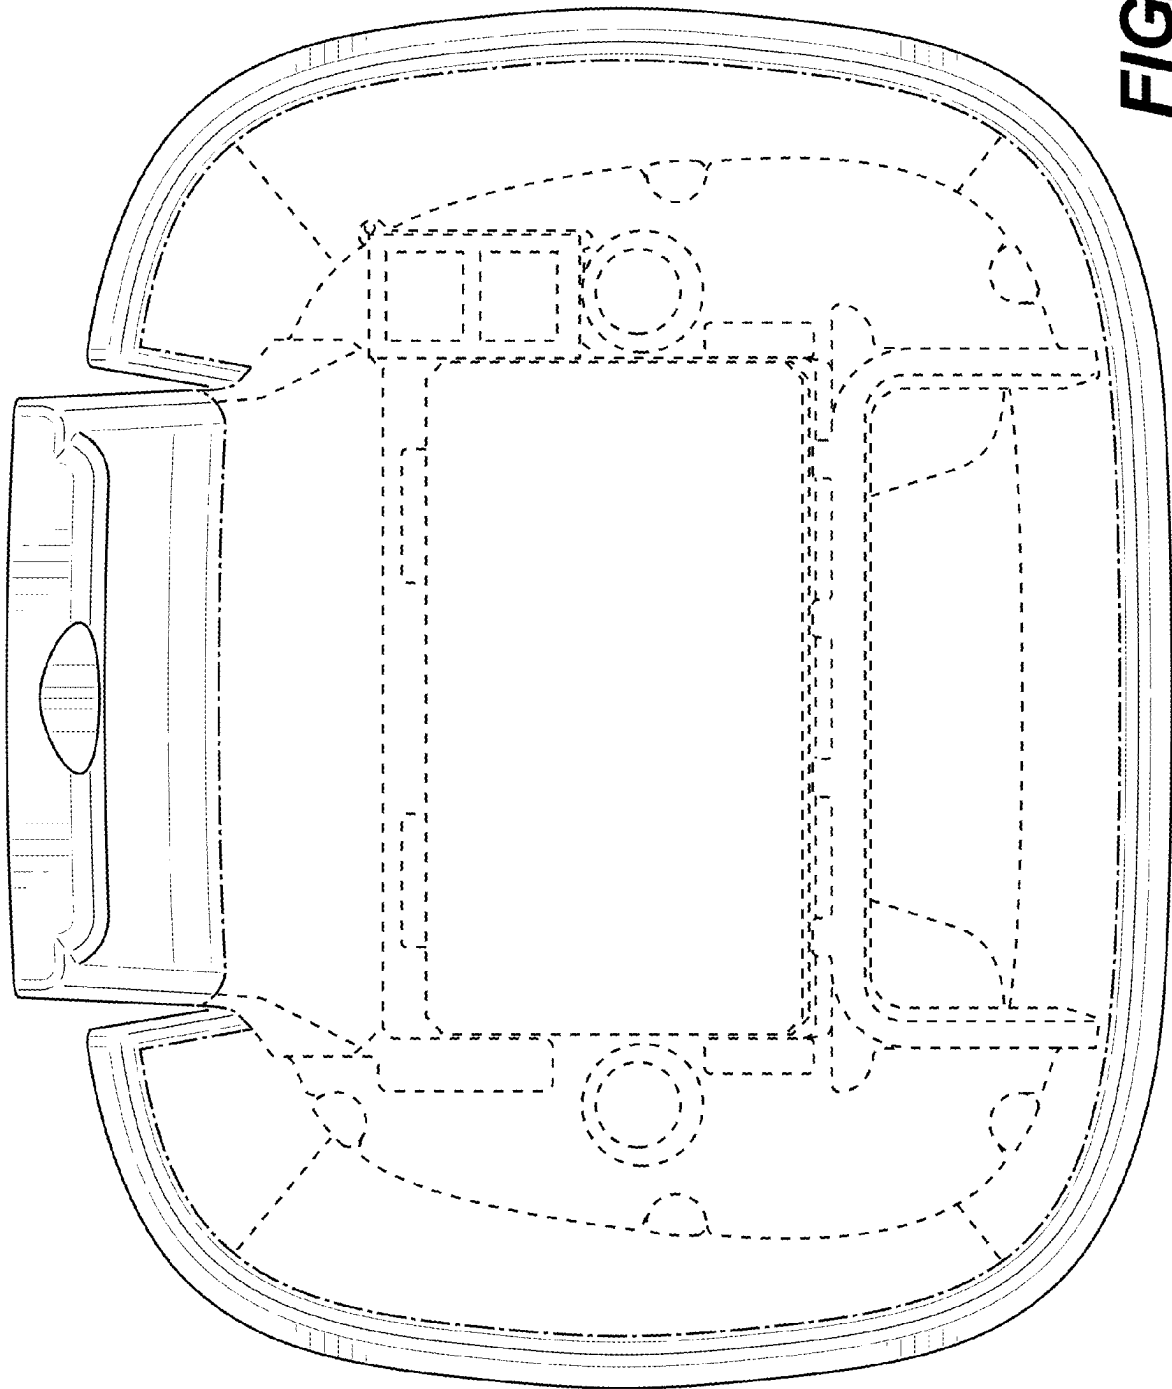


FIG. 6

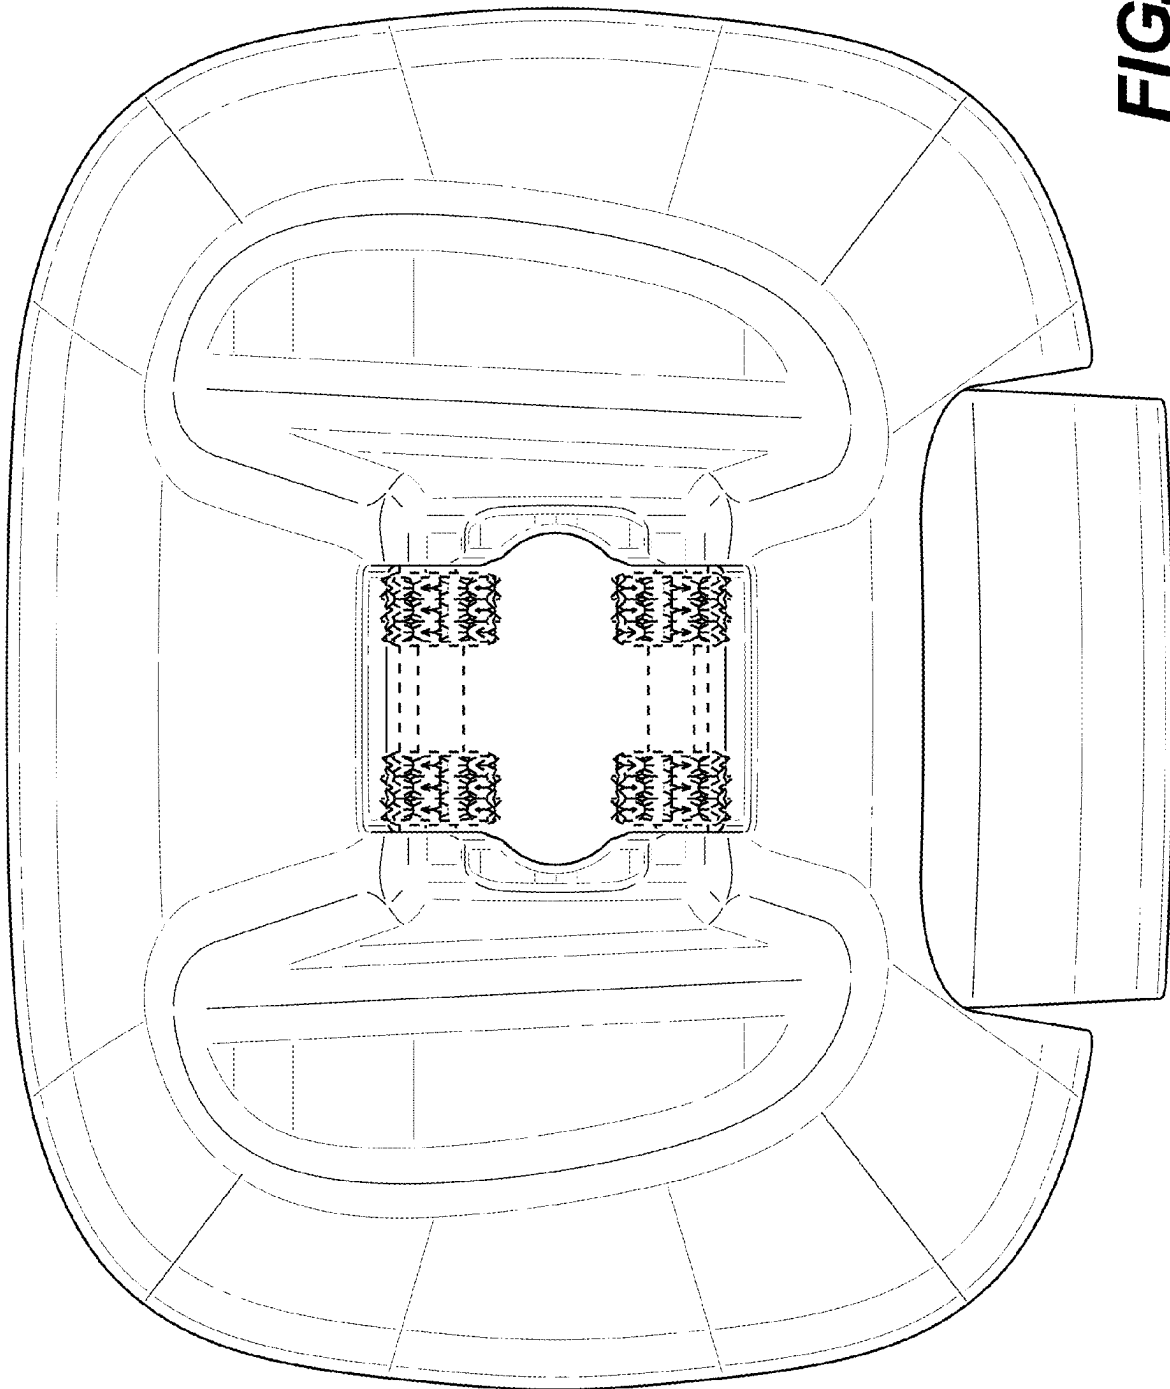


FIG. 7