



US0D1093615S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,093,615 S**
Ogi (45) **Date of Patent:** **** *Sep. 16, 2025**

(54) **X-RAY IRRADIATOR**

(71) Applicant: **FUJIFILM CORPORATION**, Tokyo (JP)

(72) Inventor: **Kazuyuki Ogi**, Kanagawa (JP)

(73) Assignee: **FUJIFILM CORPORATION**, Tokyo (JP)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

(21) Appl. No.: **29/878,516**

(22) Filed: **Jun. 23, 2023**

(30) **Foreign Application Priority Data**

Dec. 27, 2022 (JP) 2022-028038 D

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158; D16/206**

(58) **Field of Classification Search**
USPC D24/158, 160, 185, 186, 210, 231, 232;
D16/200, 204, 206, 202, 208, 203, 211,
D16/243; D14/125, 129, 134
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D331,590 S * 12/1992 Horiuchi D16/209
D657,875 S * 4/2012 Yanase D24/158
(Continued)

FOREIGN PATENT DOCUMENTS

CN 305047156 * 2/2019
CN 307487492 S 8/2022
(Continued)

OTHER PUBLICATIONS

Fujifilm Healthcare Asia Pacific, Facebook Post, Published: Aug. 27, 2024, Facebook.com, Retrieved from Internet: <https://www.facebook.com/FujifilmHealthcareAsiaPacific/posts/fujifilm-fdr-xair-portable-x-ray-device-is-revolutionizing-medical-imaging-with-/1016427113614728/> (Year: 2024).*

(Continued)

Primary Examiner — Jennifer L Rempfer

Assistant Examiner — Edward P Jones

(74) *Attorney, Agent, or Firm* — SOLARIS Intellectual Property Group, PLLC


(57) **CLAIM**

The ornamental design for an X-ray irradiator as shown and described.

DESCRIPTION

FIG. 1 is a front-side perspective view of an X-ray irradiator, showing the new design;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a bottom view thereof;
FIG. 6 is a right side view thereof;
FIG. 7 is a left side view thereof;
FIG. 8 is a left side view thereof in which a liquid crystal panel has been rotated 60°;
FIG. 9 is a left side view thereof in which a liquid crystal panel has been rotated 120°;
FIG. 10 is a rear-side perspective view thereof;
FIG. 11 is a rear-side perspective view thereof in which a liquid crystal panel has been rotated 60°;
FIG. 12 is a rear-side perspective view thereof in which a liquid crystal panel has been rotated 120°;
FIG. 13 is a rear-and-lower-side perspective view thereof;
FIG. 14 is a rear-and-lower-side perspective view thereof in which a liquid crystal panel has been rotated 60°; and,
FIG. 15 is a rear-and-lower-side perspective view thereof in which a liquid crystal panel has been rotated 120°.

(Continued)

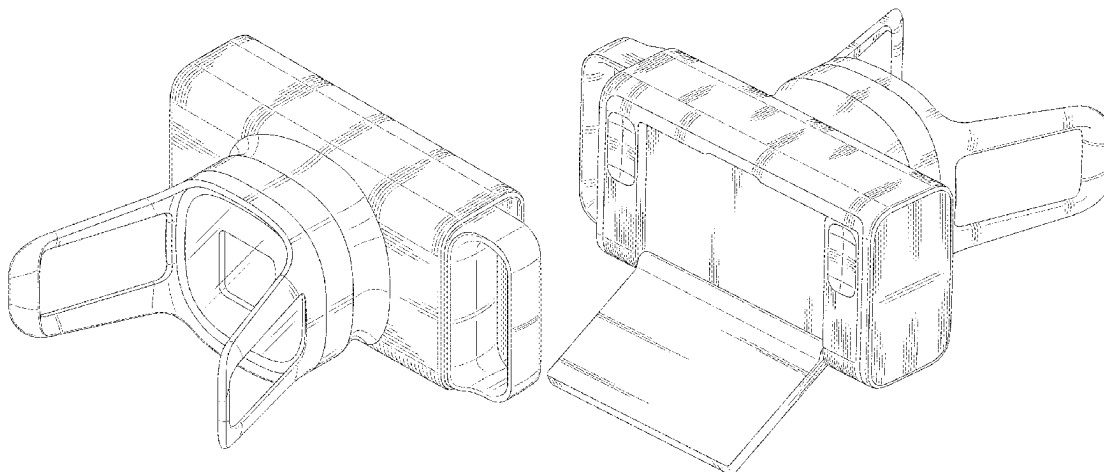

The present article is an X-ray irradiator that is used in radiography and that irradiates a medical examinee with X-rays.

1 Claim, 15 Drawing Sheets

(58) Field of Classification Search

CPC .. H05G 1/02; H05G 1/06; H05G 1/58; G21G 1/00; G21G 1/001; G21G 1/02; G21G 1/0005; G21G 1/10; G21K 5/08

See application file for complete search history.

(56)

References Cited

U.S. PATENT DOCUMENTS

D681,814 S *	5/2013	Nenoki	378/197
D700,230 S *	2/2014	Sul	D16/202
D715,441 S *	10/2014	Li	D24/158
D715,443 S *	10/2014	Sul	D24/158
D729,297 S *	5/2015	Ikegame	D16/202
D785,183 S *	4/2017	Ogura	D24/158
D806,877 S *	1/2018	Skeats	D24/158
D836,074 S *	12/2018	Sun	D14/125
D884,183 S *	5/2020	Takahashi	D24/158
D897,534 S *	9/2020	Hofmann	D24/158
D943,101 S *	2/2022	Takahashi	
D967,420 S *	10/2022	Sun	D16/202
D971,990 S *	12/2022	Mu	D16/202
D975,280 S *	1/2023	Byun	
D1,044,909 S *	10/2024	Hu	D16/218

D1,051,394 S *	11/2024	Viola	D24/158
D1,075,875 S *	5/2025	Sun	D16/202
D1,078,043 S *	6/2025	Sun	D24/138
D1,078,999 S *	6/2025	Chen	D24/138
2019/0089873 A1 *	3/2019	Misawa	H04N 23/51
2024/0210573 A1 *	6/2024	Ogi	G01T 1/16

FOREIGN PATENT DOCUMENTS

GB	6291557	*	6/2023
JP	D1457225	*	12/2012
JP	D1684557 S		5/2021
TW	D217228 S		2/2022

OTHER PUBLICATIONS

Fujifilm Healthcare UK, FDR Xair Portable X-Ray Is Here, Published: Nov. 11, 2020, YouTube.com, Retrieved from Internet: <https://www.youtube.com/watch?v=VFcCB46Wdhl> (Year: 2020).*

Puxiang, Fujifilm Portable X-ray Machine, Published: Dec. 15, 2022, puxiang.com, Retrieved from Internet: <https://www.puxiang.com/galleries/9d58928cf6202eb01a8a7e42c23e8e8c?favorite=true> (Year: 2022).*

Rad Magazine, Lightweight x-ray platform, Published: Jun. 21, 2021, Rad Magazine, Retrieved from Internet: <https://www.radmagazine.com/lightweight-x-ray-platform-puts-community-imaging-within-reach/> (Year: 2021).*

English language translation of the following: Office action dated Nov. 3, 2023 from the TIPO in a Taiwan patent application No. 112303116 corresponding to the instant patent application.

* cited by examiner

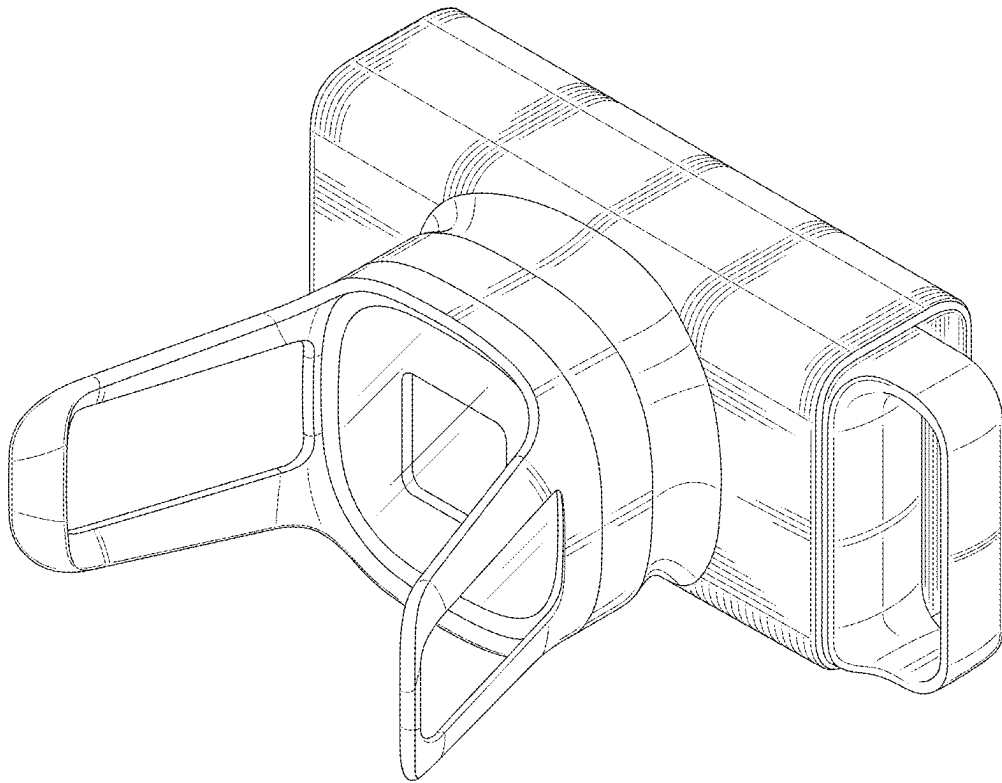


FIG.1

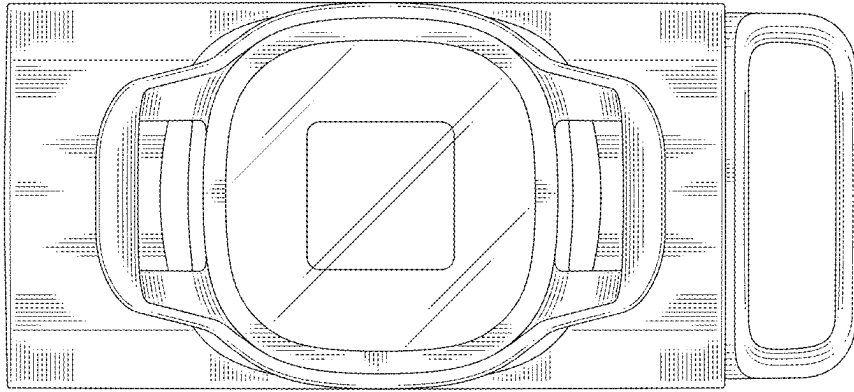


FIG.2

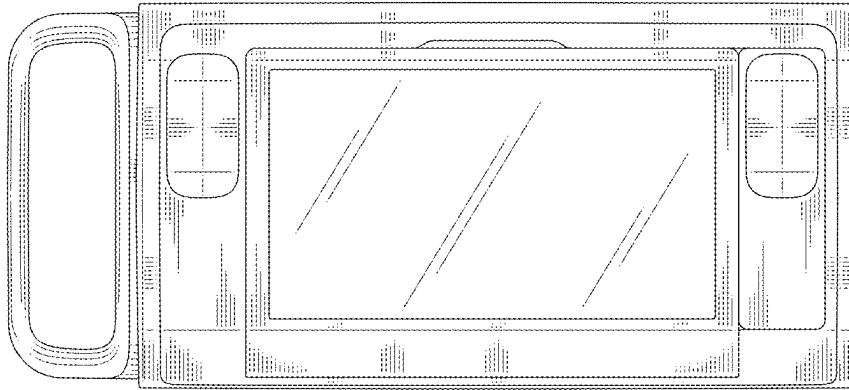


FIG.3

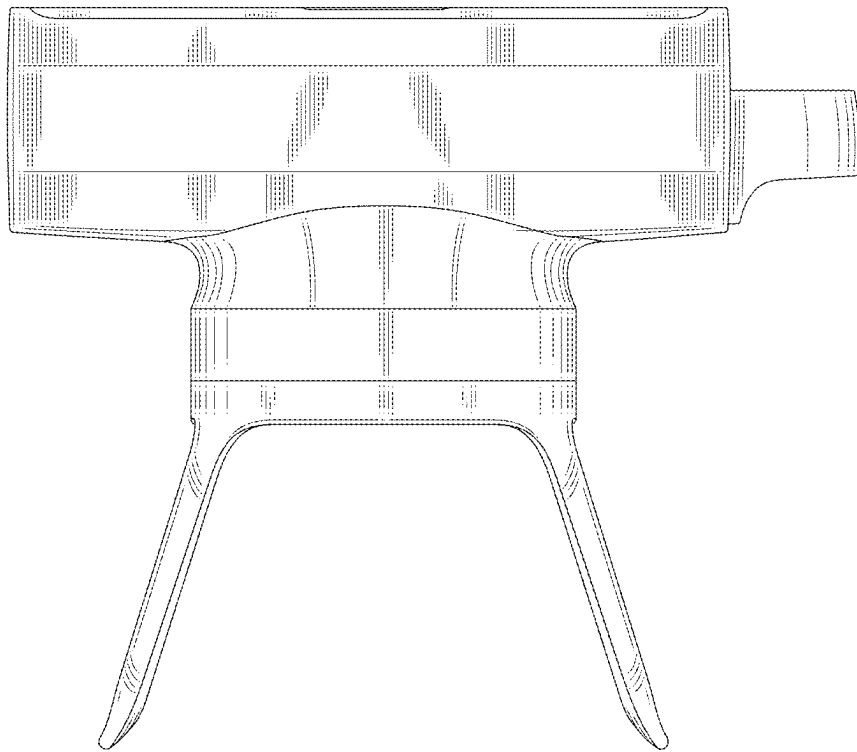


FIG.4

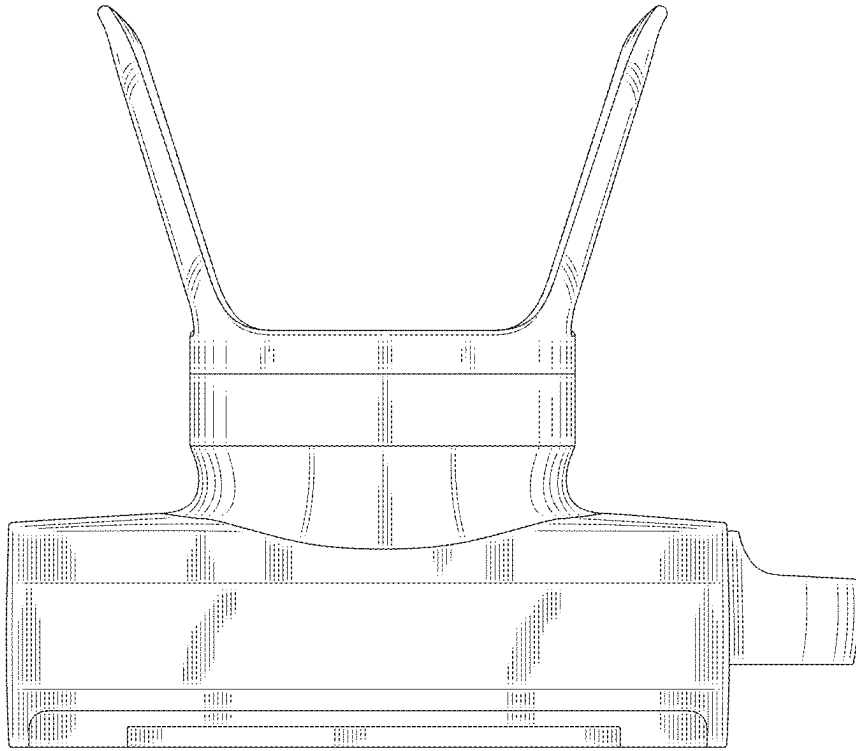


FIG.5

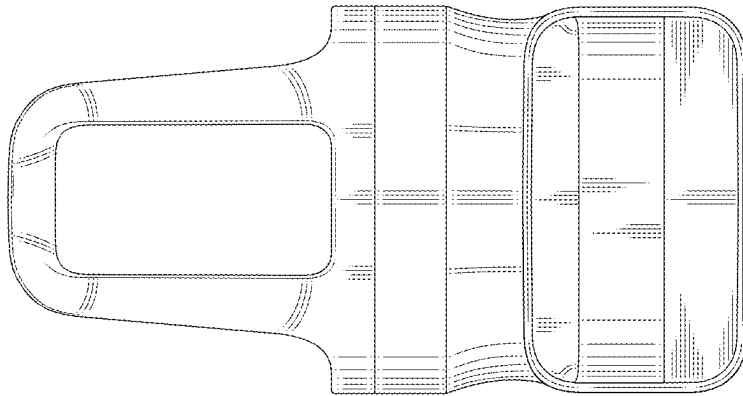


FIG.6

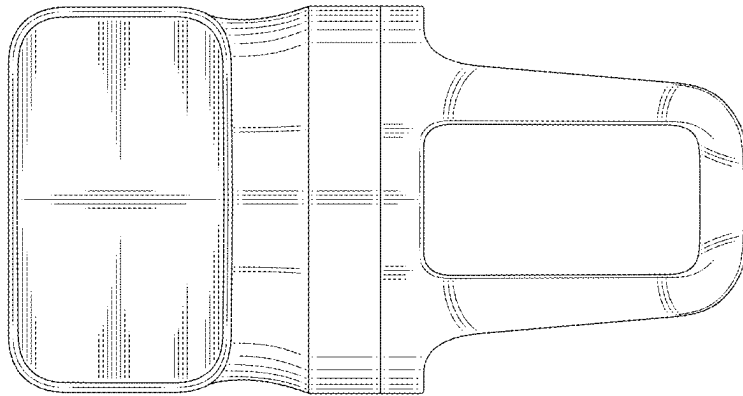


FIG.7

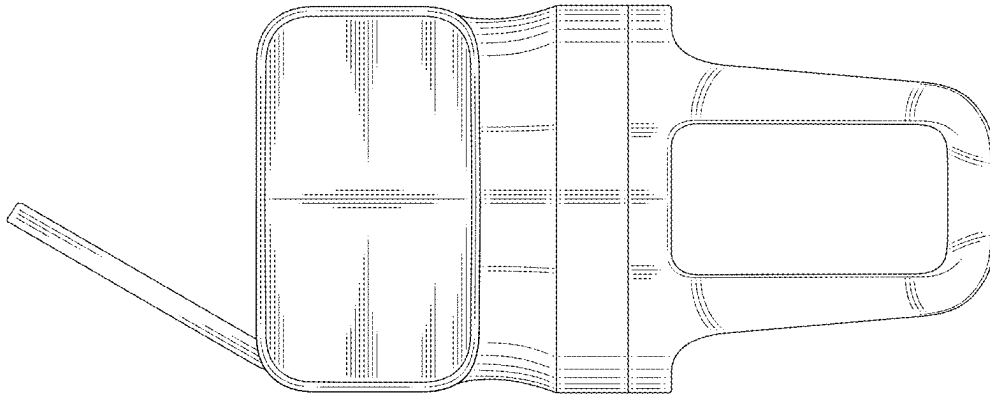


FIG.8

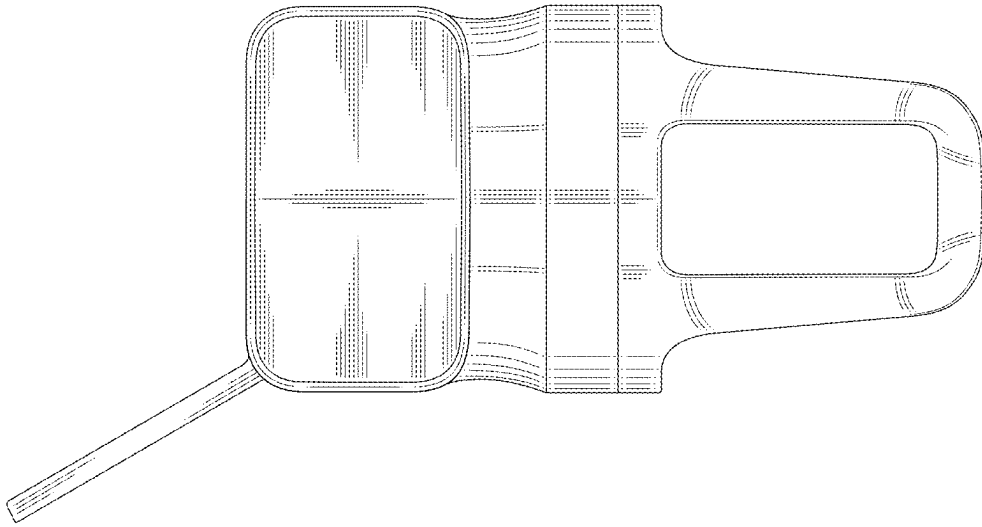


FIG.9

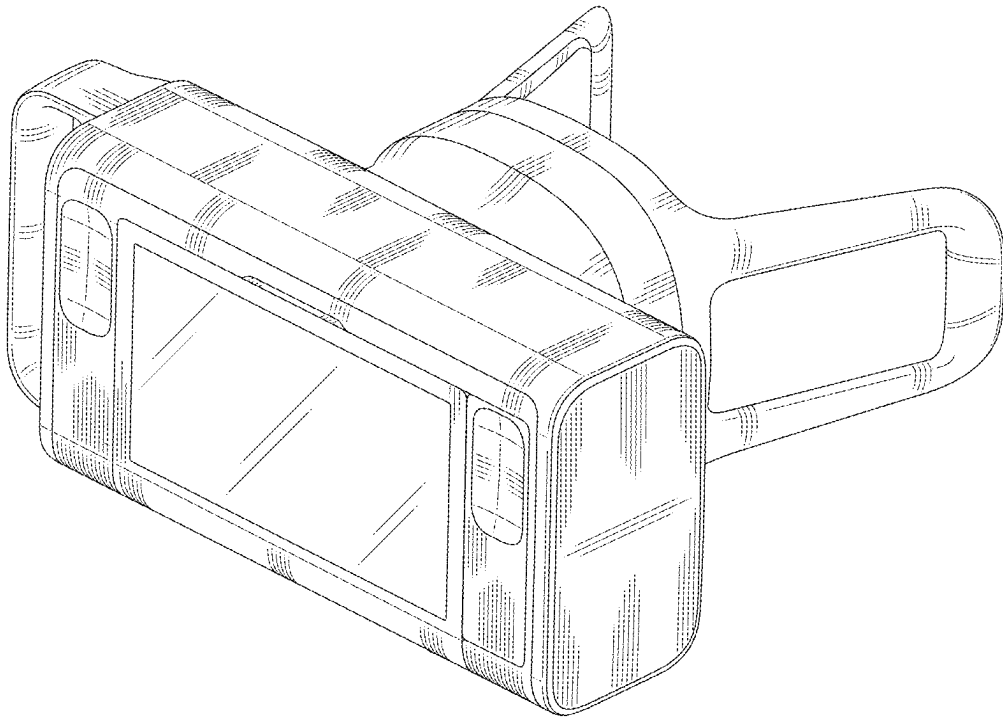


FIG.10

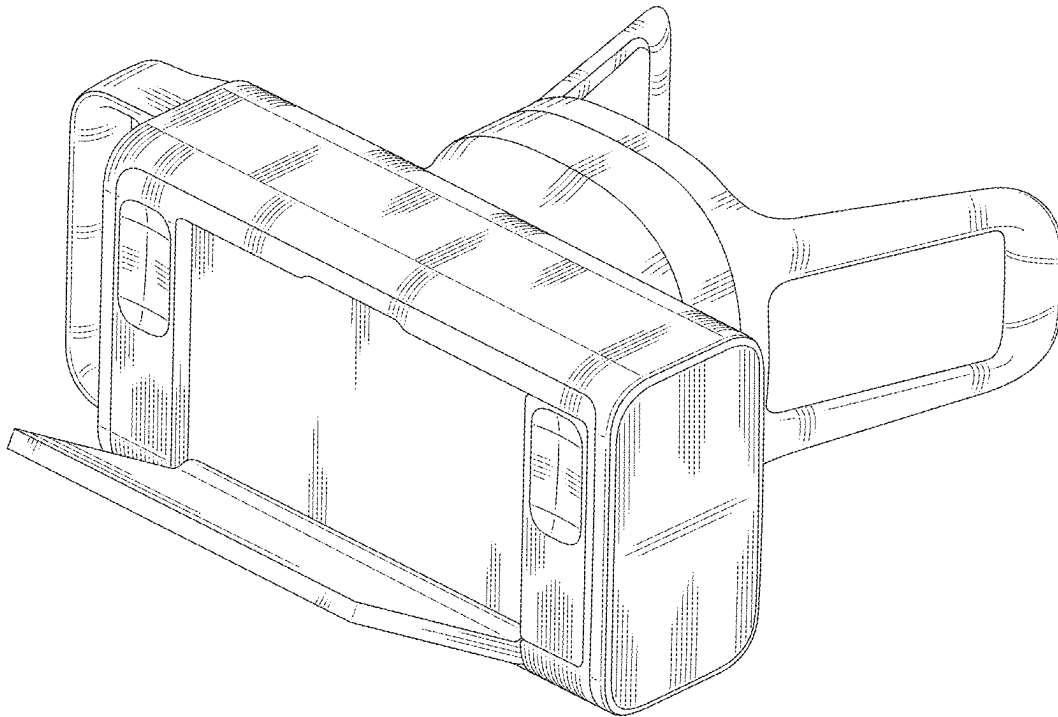


FIG.11

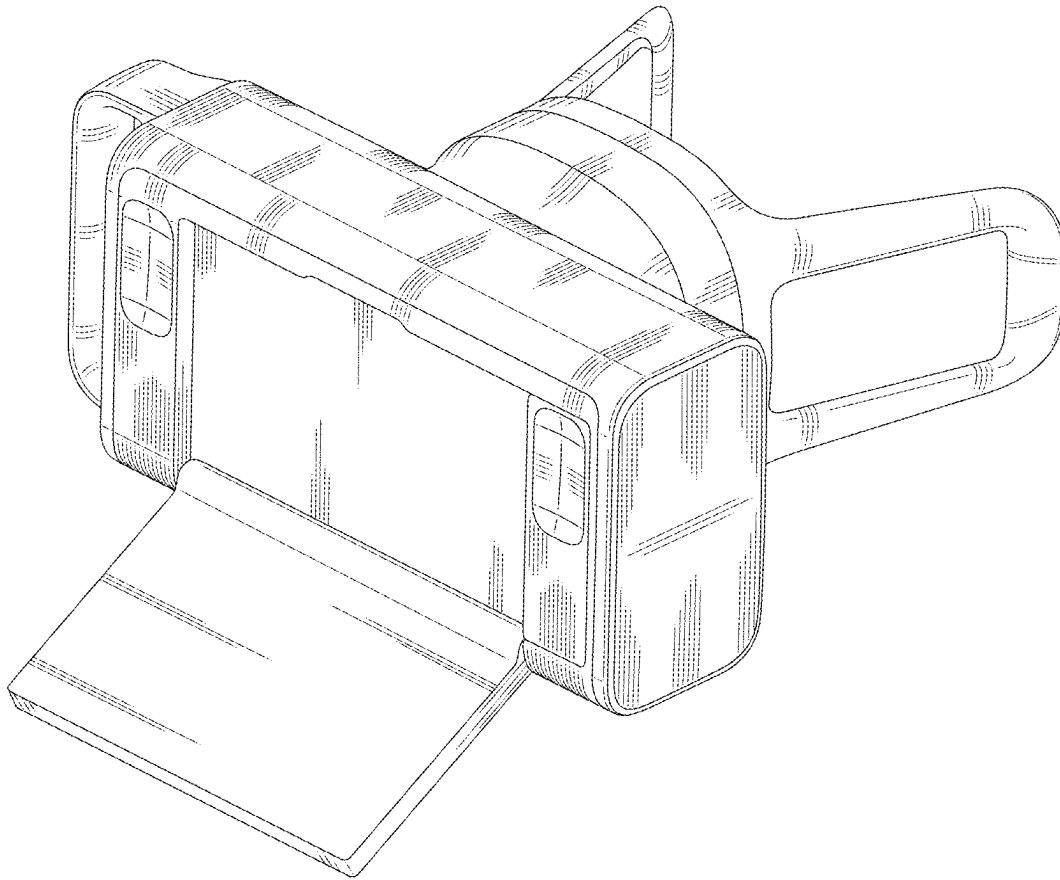


FIG.12

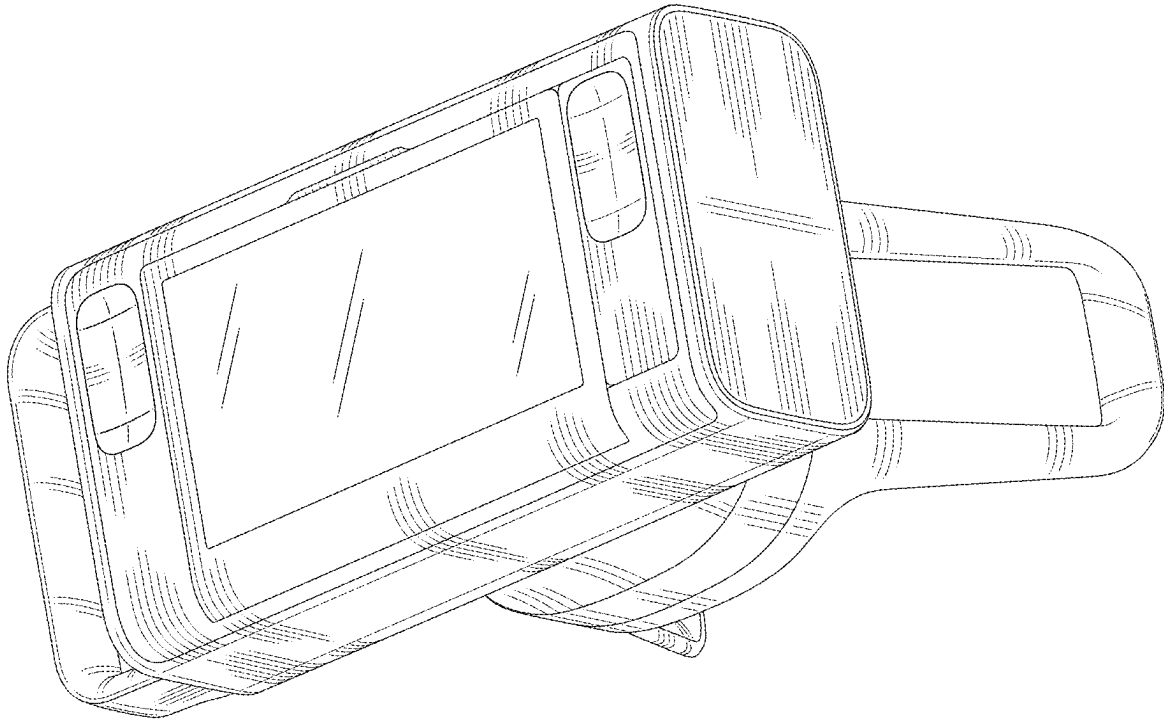


FIG.13

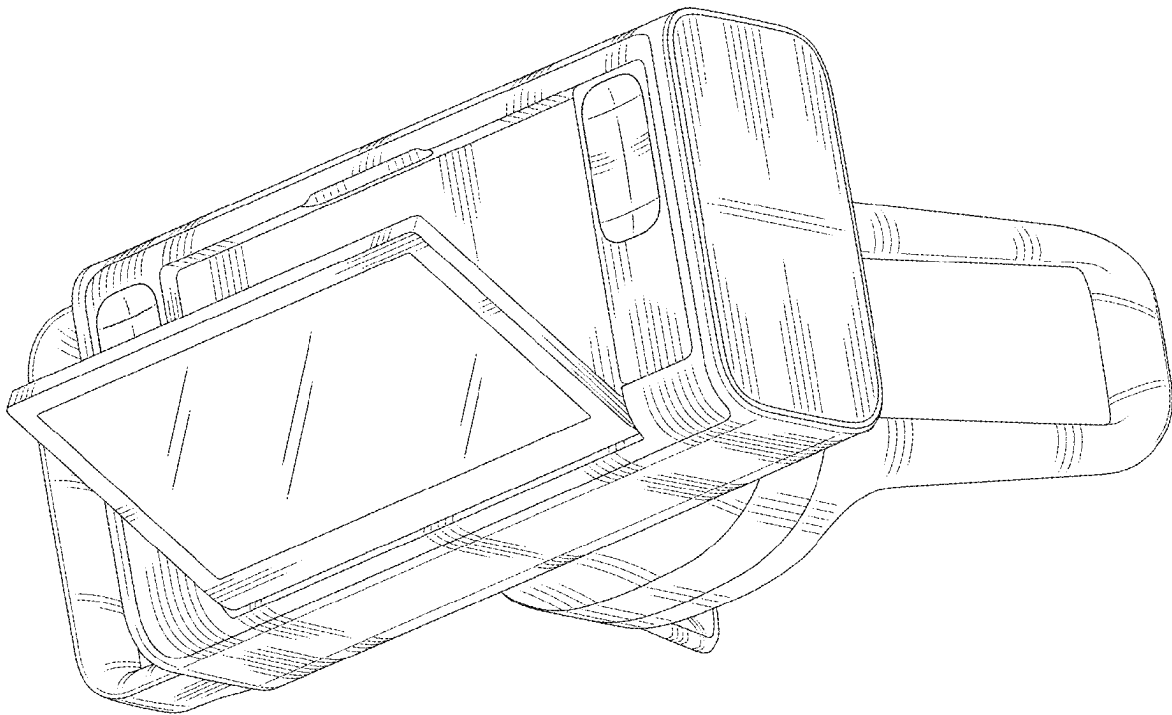


FIG.14

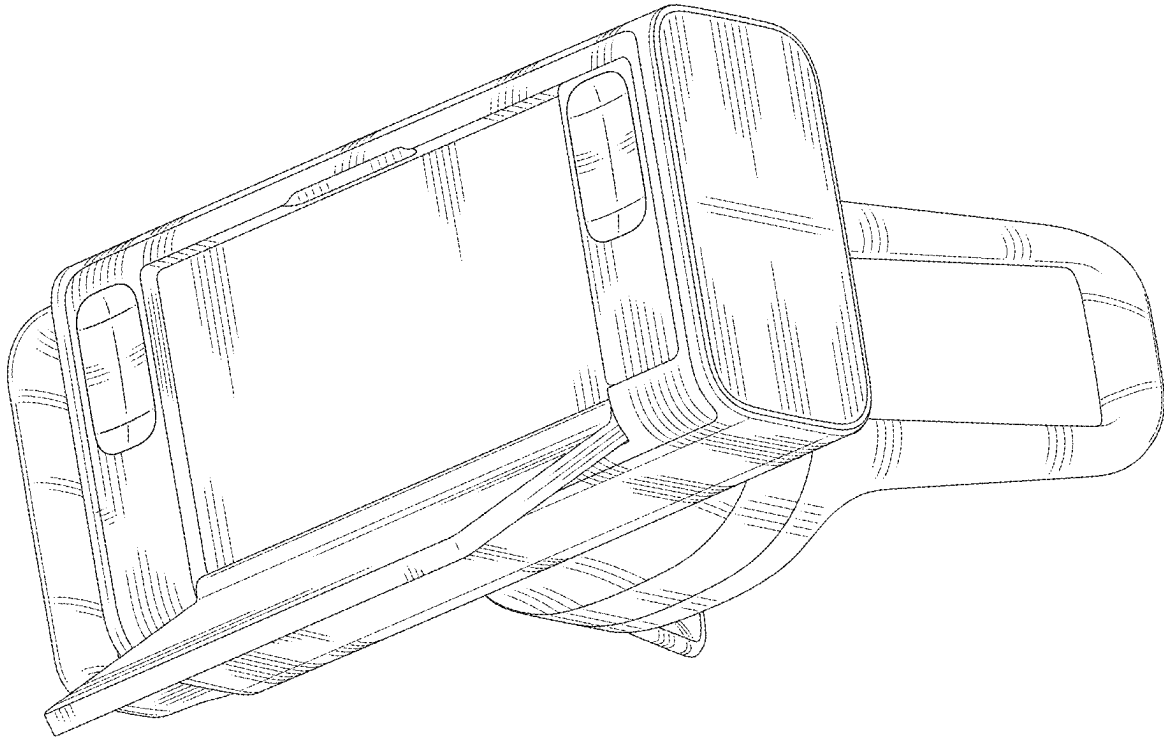


FIG.15