



US0D1093622S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,093,622 S**
Teodorescu et al. (45) **Date of Patent:** **** Sep. 16, 2025**

(54) **SURGICAL SITE ISOLATION DEVICE**

(71) Applicant: **SURGIBOX INC.**, Cambridge, MA
(US)

(72) Inventors: **Debbie Lin Teodorescu**, Cambridge,
MA (US); **Macauley Reardon Dupree**
Kenney, Cambridge, MA (US); **Nathan**
Samuel Phipps, Watertown, MA (US);
Mike Horia Mihail Teodorescu,
Cambridge, MA (US)

(73) Assignee: **SurgiBox Inc.**, Cambridge, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/814,377**

(22) Filed: **Nov. 5, 2021**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/183; D24/217**

(58) **Field of Classification Search**
USPC D24/183, 184, 190, 202, 217;
D29/101.1, 107, 124; D21/834, 835, 837,
D21/838
CPC A61B 6/107; A61B 6/4411; A61B 46/27;
A61B 90/40; G21F 3/00; G21F 3/02;
G21Y 2004/30; A61N 2005/1094; A41D
13/11; A41D 13/1107; A41D 13/1184;
A42B 3/225

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D485,366 S * 1/2004 Hauville D24/234
8,360,084 B1 * 1/2013 Robinson E04H 6/005
135/133
D756,530 S * 5/2016 McAlister D21/834
D950,267 S * 5/2022 Bedard D21/834

D976,414 S * 1/2023 Patmore D24/183
D1,020,344 S * 4/2024 Kandelaar D6/718.29
D1,025,494 S * 4/2024 Campbell-Hill D24/217
2021/0317679 A1 * 10/2021 Hornick E04H 15/48
2022/0008274 A1 * 1/2022 Shih A61B 90/40
2022/0339050 A1 * 10/2022 Ball A47K 3/38
2024/0065794 A1 * 2/2024 Teodorescu A61B 46/27
2024/0123637 A1 * 4/2024 Teodorescu A61B 46/27
2024/0130830 A1 * 4/2024 Teodorescu A61G 10/02

FOREIGN PATENT DOCUMENTS

GB 6187306 * 1/2022

OTHER PUBLICATIONS

Cost-effective canopy protects health workers from COVID-19
infection during ventilation. Online, published date unknown. Retrieved
on Feb. 10, 2025 from URL: <https://www.wsucm.store/?path=page/ggitem&ggpid=822328>.*

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Fish & Richardson P.C.

(57) **CLAIM**


The ornamental design for a surgical site isolation device, as
shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a surgical site isolation
device showing our new design;
FIG. 2 is a top view thereof;
FIG. 3 is a bottom view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a front side view thereof; and,
FIG. 7 is a rear side view thereof.

The broken lines illustrate portions of the surgical site
isolation device and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

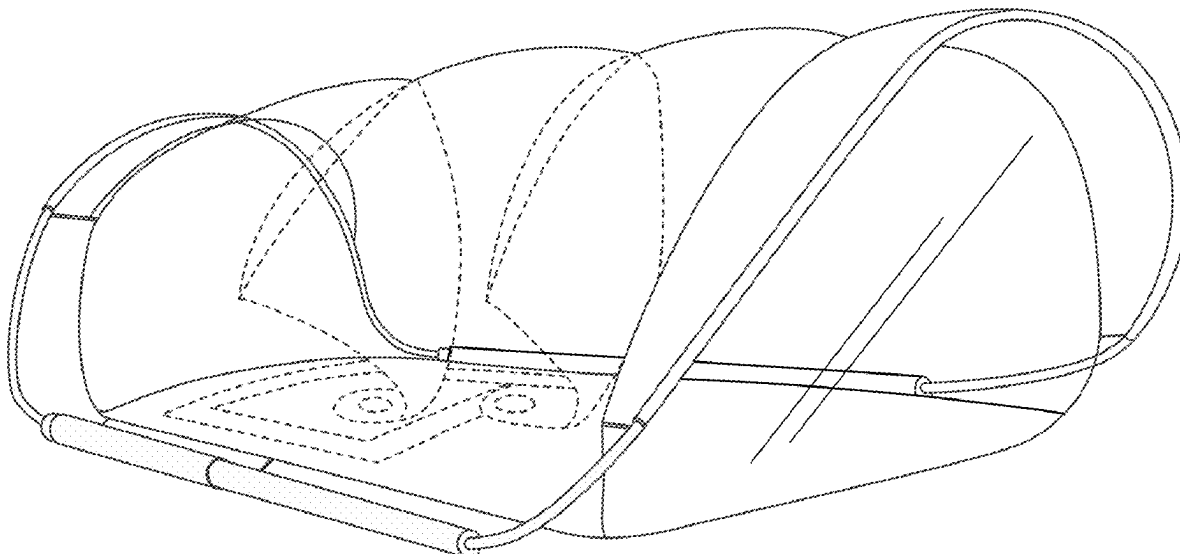

(56)

References Cited

OTHER PUBLICATIONS

SurgiBox's SurgiField System Can Transform from Backpack to Mobile Operating Room in 90-Seconds. Online, published date May 25, 2023. Retrieved on Feb. 10, 2025 from URL: <https://www.techeblog.com/surgibox-surgifield-backpack-operating-room/>.*

Inflatable Operating Room Could Bring Safe Surgery to Front Lines. Online, published date Oct. 11, 2018. Retrieved on Feb. 10, 2025 from URL: <https://www.nationaldefensemagazine.org/articles/2018/10/11/inflatable-operating-room-could-bring-safe-surgery-to-front-lines>.*

* cited by examiner

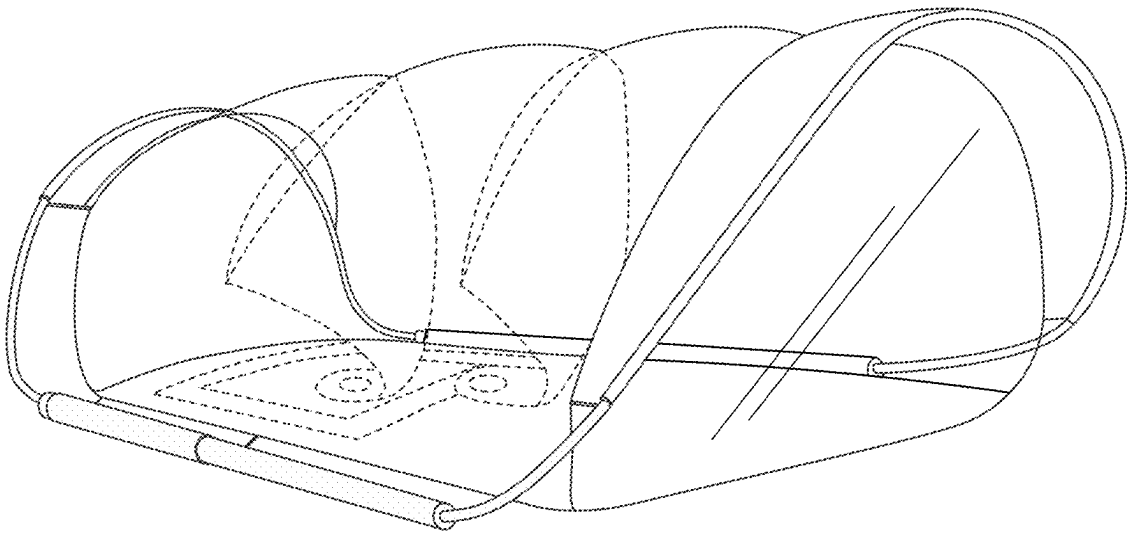


FIG. 1

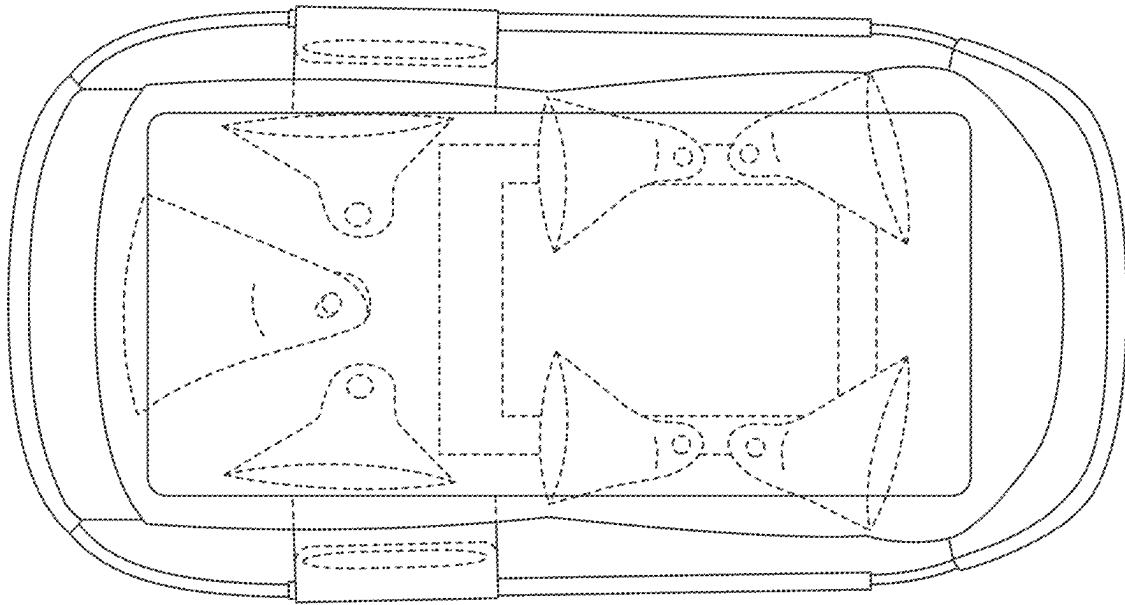


FIG. 2

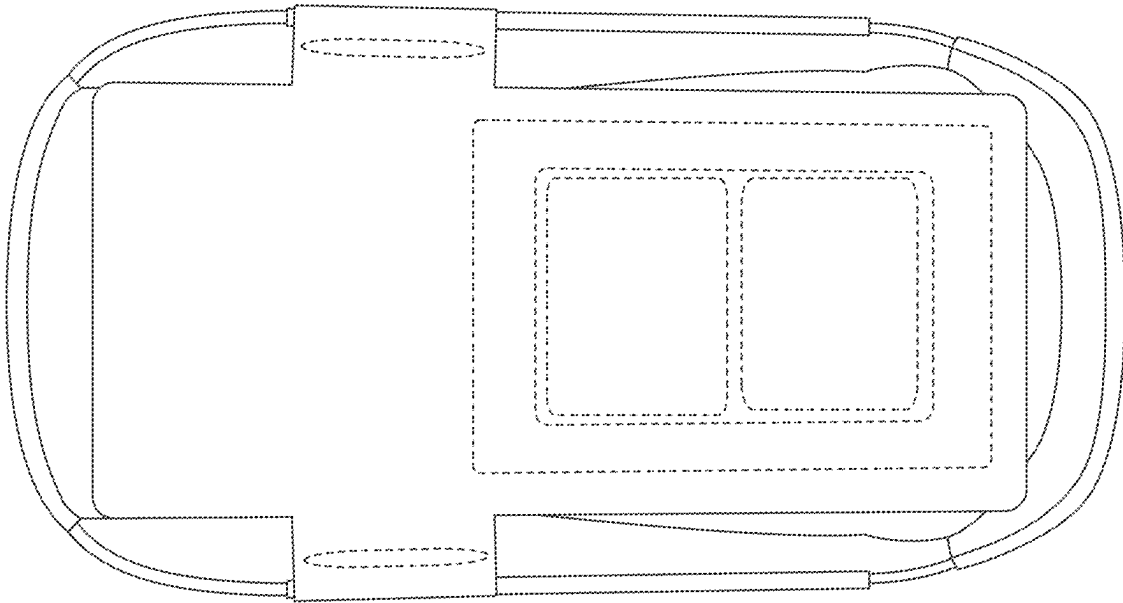


FIG. 3

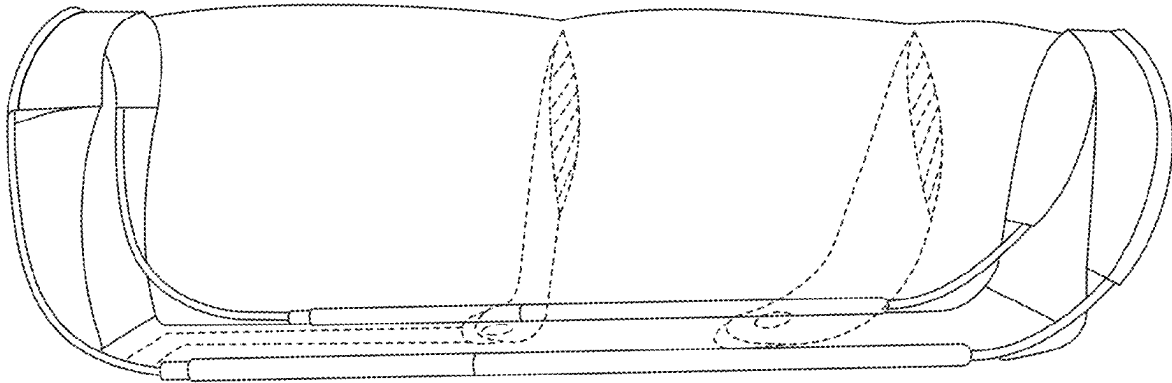


FIG. 4

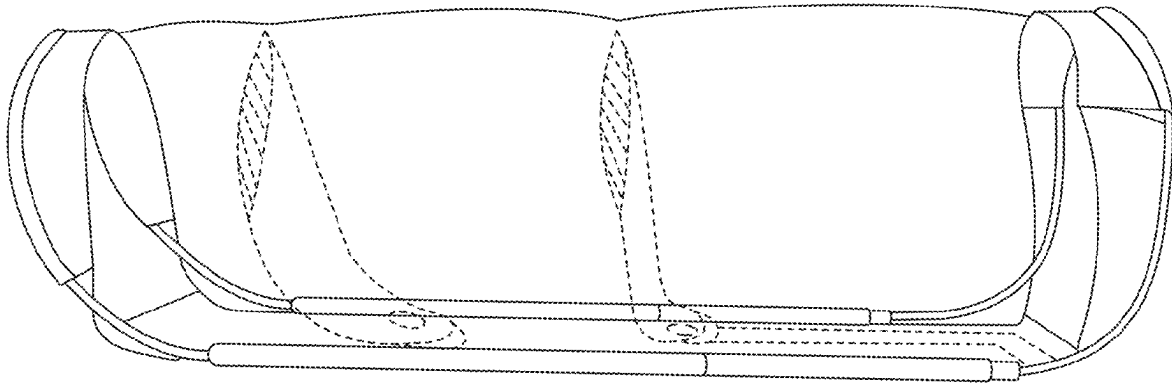


FIG. 5

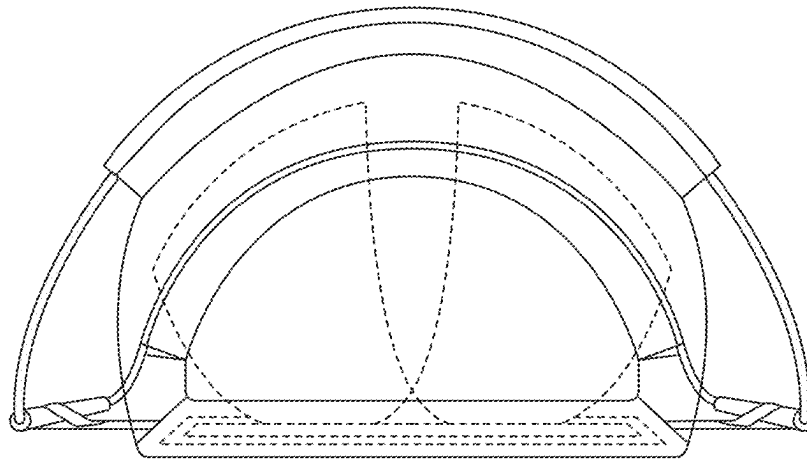


FIG. 6

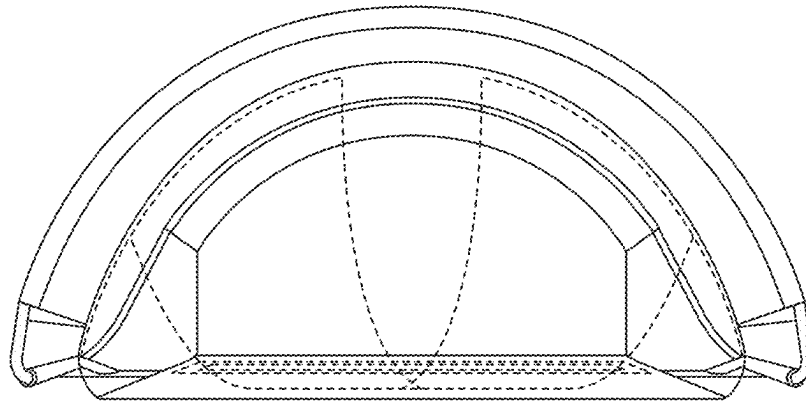


FIG. 7