



US0D1090866S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,090,866 S**
Peng et al. (45) **Date of Patent:** **** Aug. 26, 2025**

(54) **HAND REHABILITATION DEVICE**

(71) Applicants: **Qingjin Peng**, Winnipeg (CA); **Hamid Reza Fazeli**, Richmond Hill (CA)

(72) Inventors: **Qingjin Peng**, Winnipeg (CA); **Hamid Reza Fazeli**, Richmond Hill (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/878,491**

(22) Filed: **Jun. 22, 2023**

(51) **LOC (15) Cl.** **24-04**

(52) **U.S. Cl.**
USPC **D24/190**

(58) **Field of Classification Search**

USPC D24/155, 188, 189, 190, 191, 192, 200,
D24/206, 209; D29/113, 114, 120.1,
D29/120.2, 121.1, 121.2
CPC A61F 5/0123; A61F 5/0125; A61F 5/01;
A61F 5/0585; A61F 13/062; A61F
2007/0042; A61F 2/64; A61F 5/0118;
A61F 5/05866; A61F 13/107; A61F
13/104; A61F 2007/0035; A41D 13/065;
A41D 13/0153;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D228,977 S * 11/1973 Kanicki D29/113
D235,703 S * 7/1975 Birnie 2/163
D294,176 S * 2/1988 Tyo D24/190

(Continued)

FOREIGN PATENT DOCUMENTS

CN 305889539 * 6/2020
CN 308130891 * 7/2023

(Continued)

OTHER PUBLICATIONS

ResearchGate: Commercial device-based hand rehabilitation systems for stroke patients.: Found online Sep. 12, 2024 at researchgate.net. Reference dated Feb. 2023. Retrieved from https://www.researchgate.net/figure/Two-types-of-hand-rehabilitation-robots-a-CyberGrasp-36-and-b-Amadeo-37_fig2_368434785.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) *Attorney, Agent, or Firm* — Kyle R Satterwaite;
Ryan W Dupuis; Ade & Company Inc


(57) **CLAIM**

The ornamental design for a hand rehabilitation device as shown and described.

DESCRIPTION

FIG. 1 is a top front perspective view of a left handed embodiment of the hand rehabilitation device; FIG. 2 is a bottom front perspective view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a front elevational view thereof; FIG. 5 is left side elevational view thereof; FIG. 6 is a right side elevational view thereof; FIG. 7 is a top plan view thereof; FIG. 8 is a bottom plan view thereof; FIG. 9 is a top front perspective view of a right handed embodiment of the hand rehabilitation device, of which each view is a mirror image of the left handed embodiment; FIG. 10 is a bottom front perspective view of the right handed embodiment; FIG. 11 is a rear elevational view thereof; FIG. 12 is a front elevational view thereof; FIG. 13 is left side elevational view thereof; FIG. 14 is a right side elevational view thereof; FIG. 15 is a top plan view thereof; and, FIG. 16 is a bottom plan view thereof. In the drawings, the broken lines depict portions of the hand rehabilitation device that form no part of the claimed design.

1 Claim, 16 Drawing Sheets

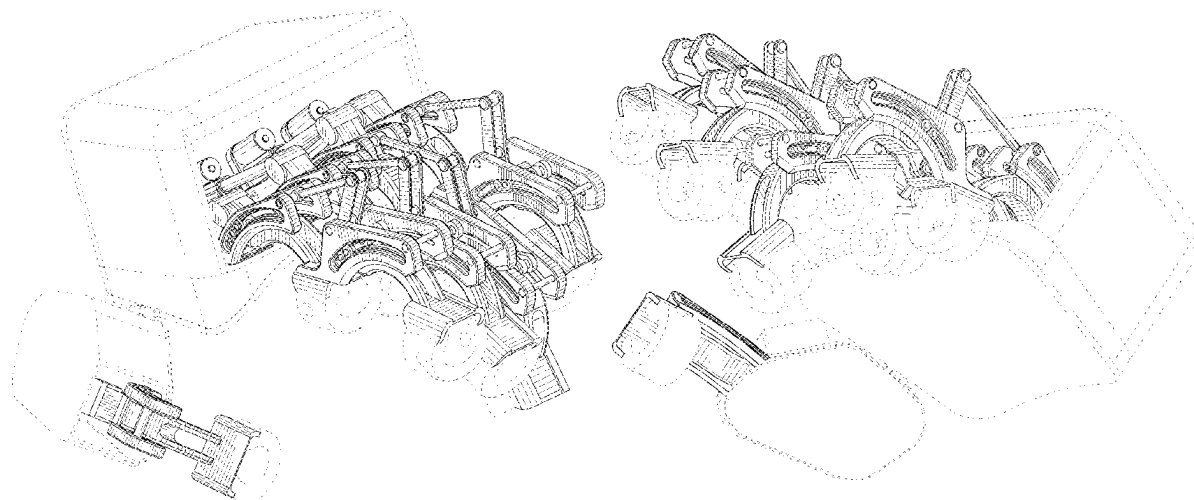

(58) **Field of Classification Search**

CPC A41D 13/088; A61H 1/024; A61H
2201/165; A61H 2205/102; A61H 1/0285
See application file for complete search history.

FOREIGN PATENT DOCUMENTS

CN	308267678	*	10/2023
CN	308824439	*	9/2024
KR	301262342.0000	*	5/2024

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,765,320	A *	8/1988	Lindemann		A61F 5/0118
					D24/190
9,532,916	B2	1/2017	Tsui et al.		
D824,527	S *	7/2018	Fried		D24/190
D881,297	S *	4/2020	Poillucci		D24/190
D881,298	S *	4/2020	Poillucci		D24/190
D883,499	S *	5/2020	Park		D24/190
D942,023	S *	1/2022	Park		D24/188
11,246,786	B2	2/2022	Tsui et al.		
D980,990	S *	3/2023	Zhou		D24/190
2013/0072829	A1 *	3/2013	Fausti		A63B 21/4035
					601/40
2013/0303951	A1 *	11/2013	Liu		A63B 23/16
					601/46
2016/0213978	A1 *	7/2016	Ban		G06F 3/014

OTHER PUBLICATIONS

“Syrebo: Hand Rehabilitation Robot Gloves.” Found online Sep. 12, 2024 at amazon.com. Reference dated Oct. 25, 2022. Retrieved from <https://www.amazon.com/Soft-Rehabilitation-Hand-Glove-Finger/dp/B0BKF78LDK>.*

“MZU: Stroke Recovery Glove.” Found online Sep. 12, 2024 at amazon.com. Reference dated May 18, 2023. Retrieved from <https://www.amazon.com/Recovery-Patients-Exerciser-Rehabilitation-Equipment/dp/B0C5L1S1F5>.*

“MZU: Heated Finger Rehabilitation Robot Glove for Hand Hemiplegia.” Found online Nov. 27, 2024 at amazon.com. Reference dated Oct. 24, 2023. Retrieved from <https://www.amazon.com/dp/B0CLNZPWYQ>.*

* cited by examiner

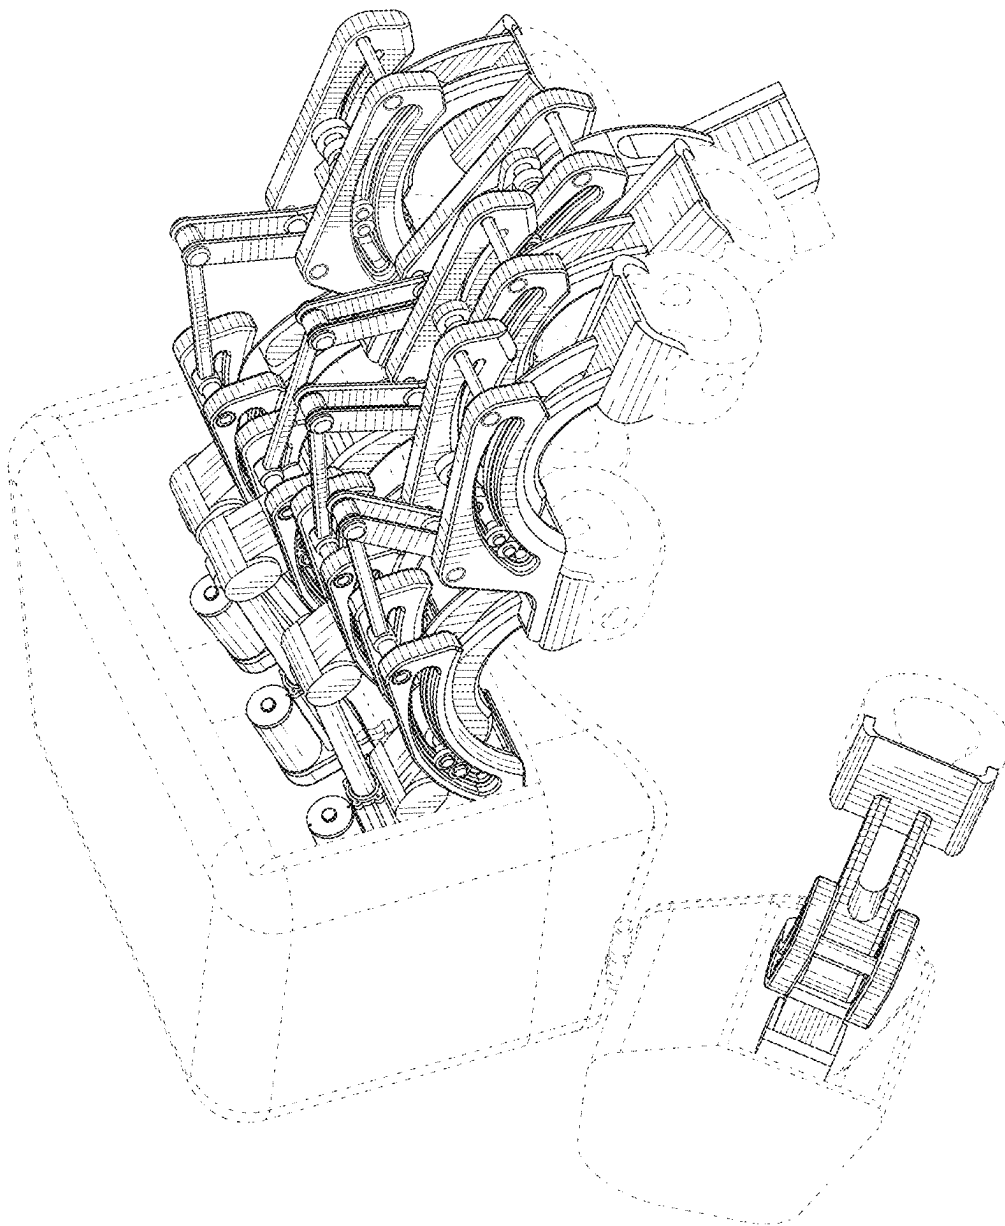


FIG.1

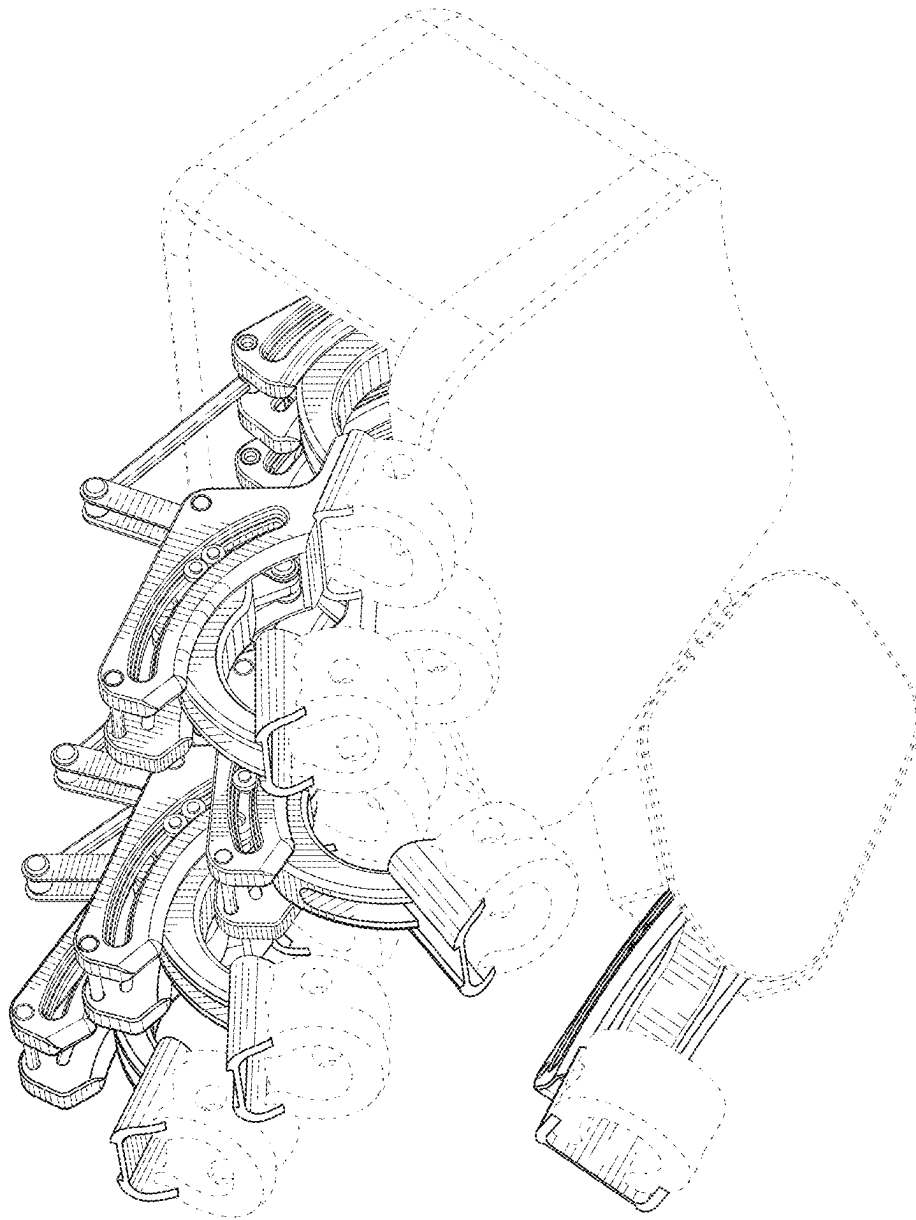


FIG.2

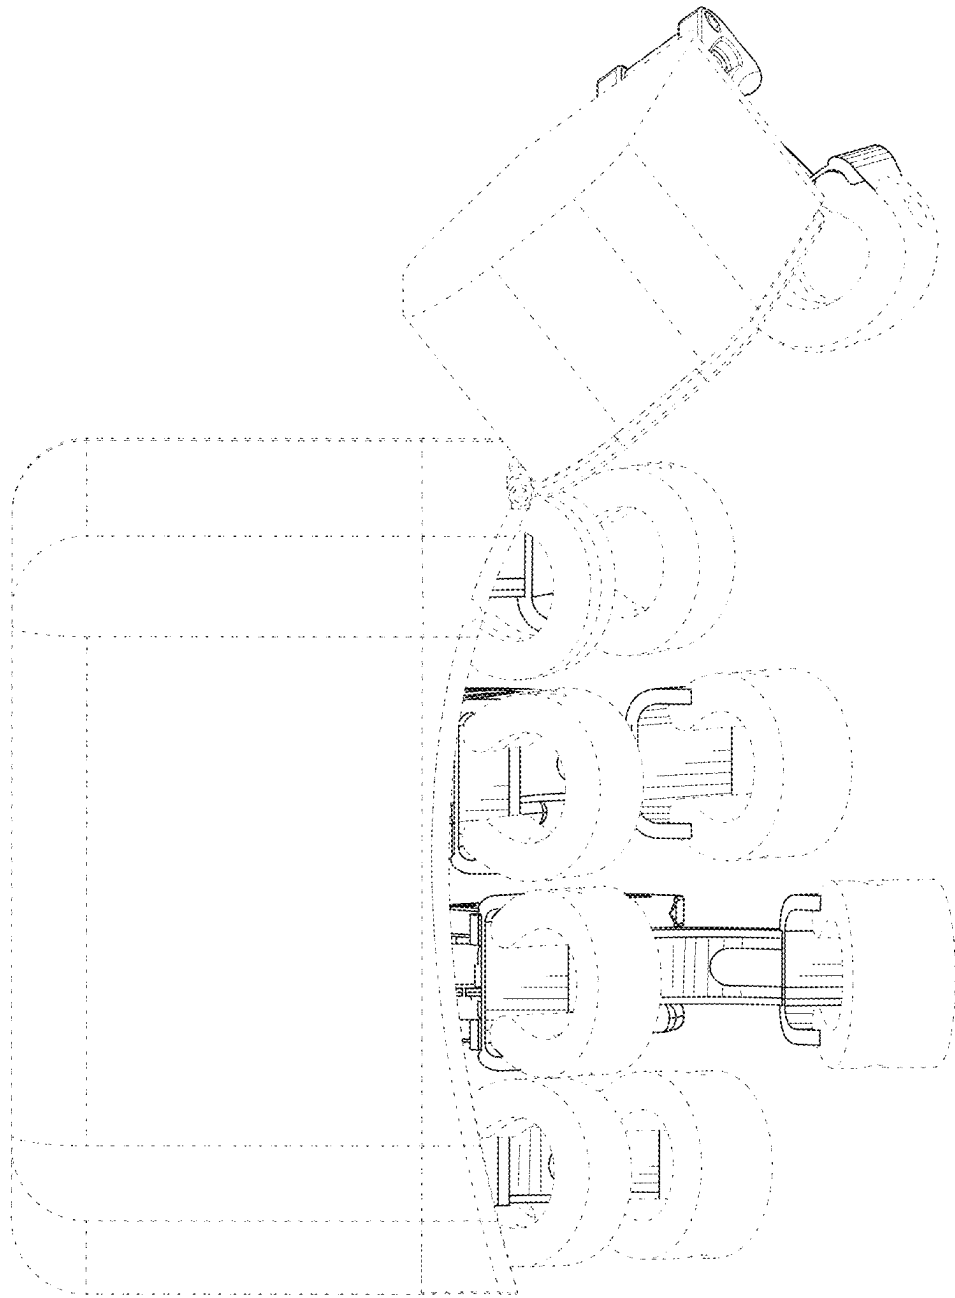


FIG.3

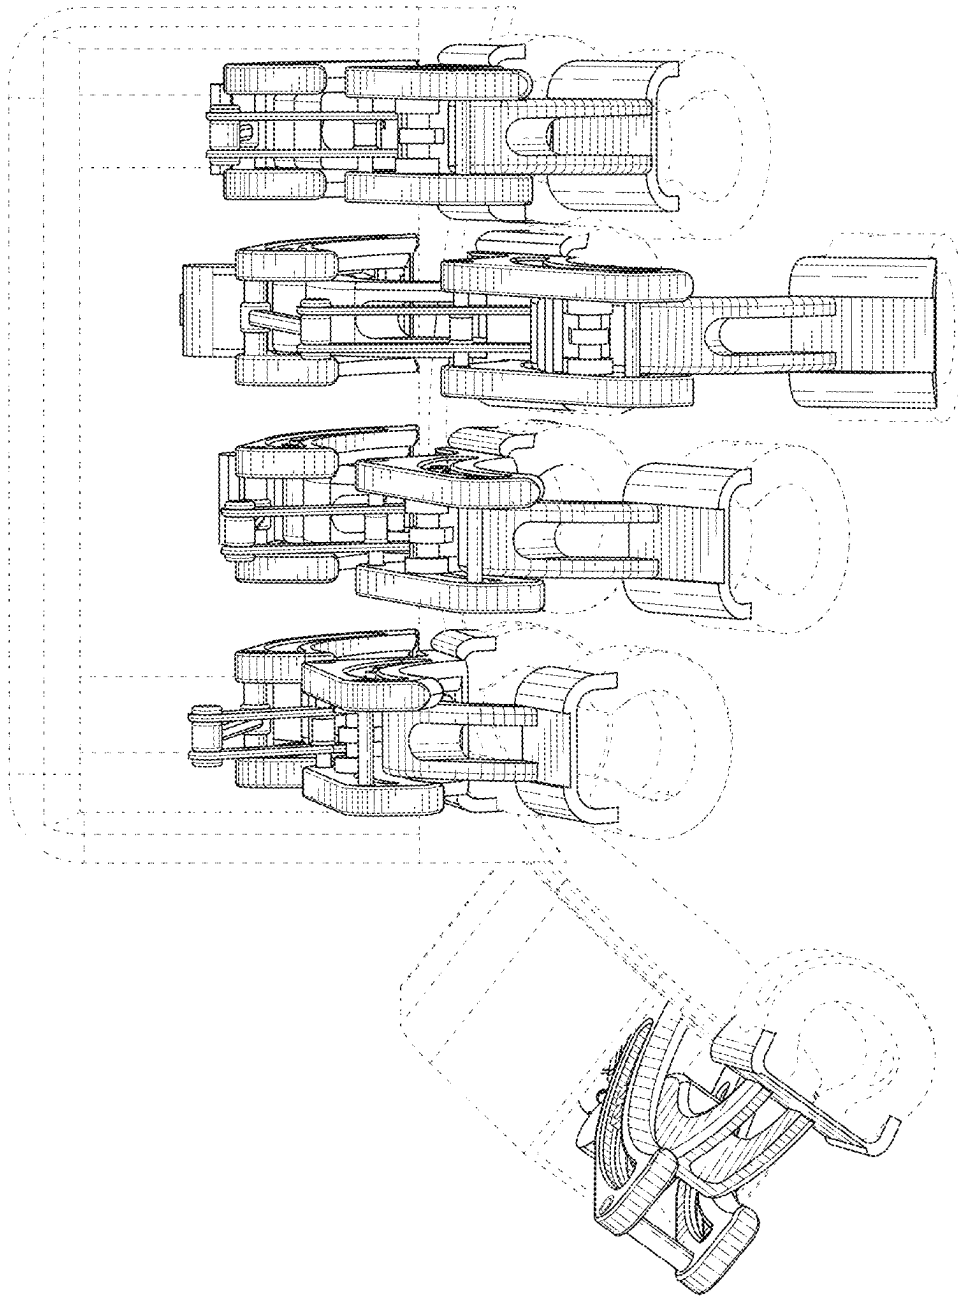


FIG. 4

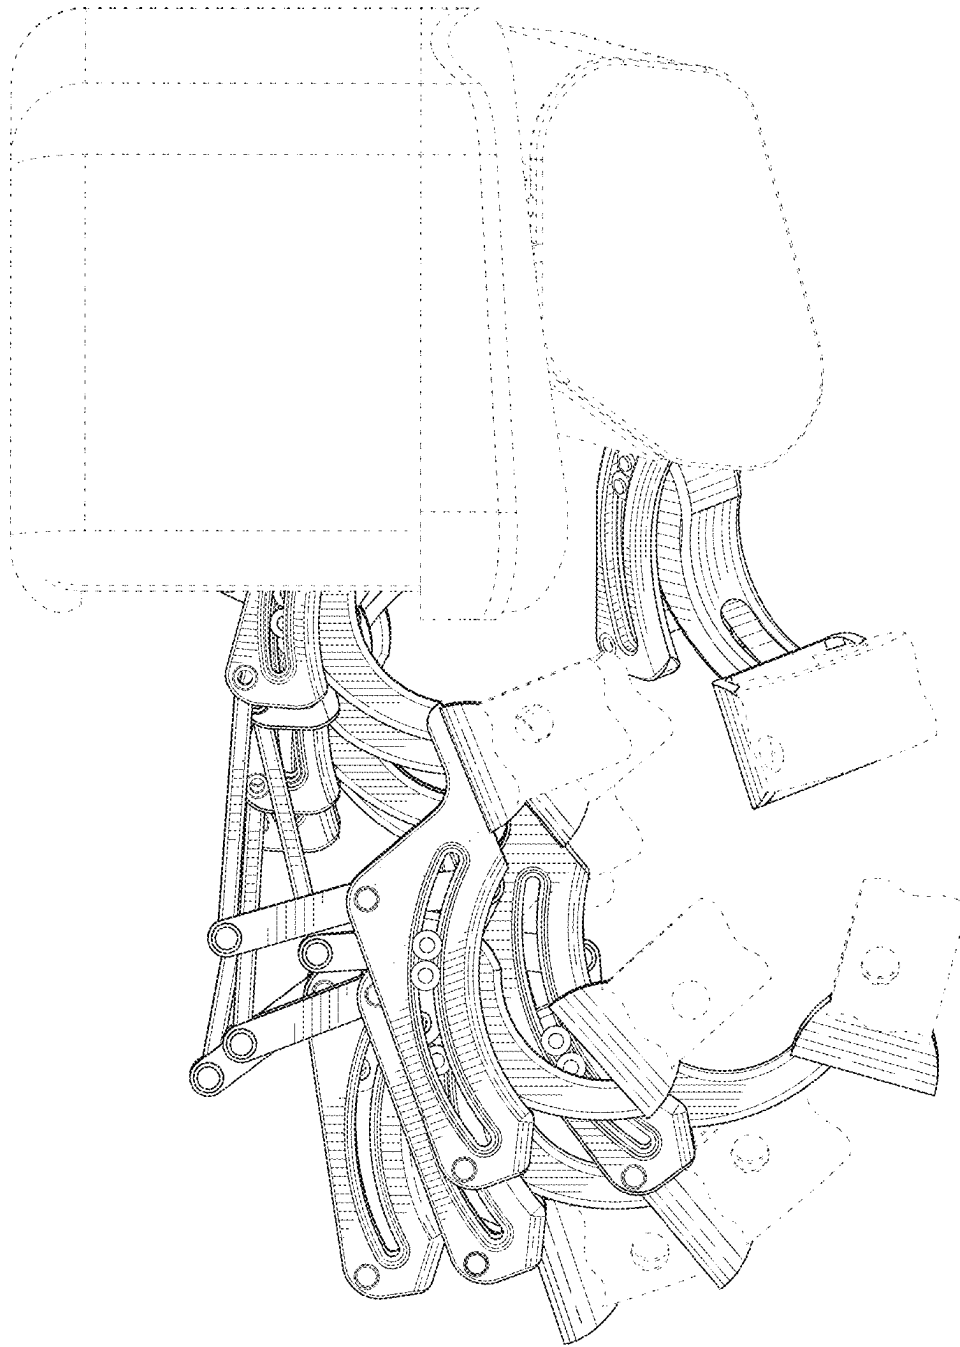


FIG.5

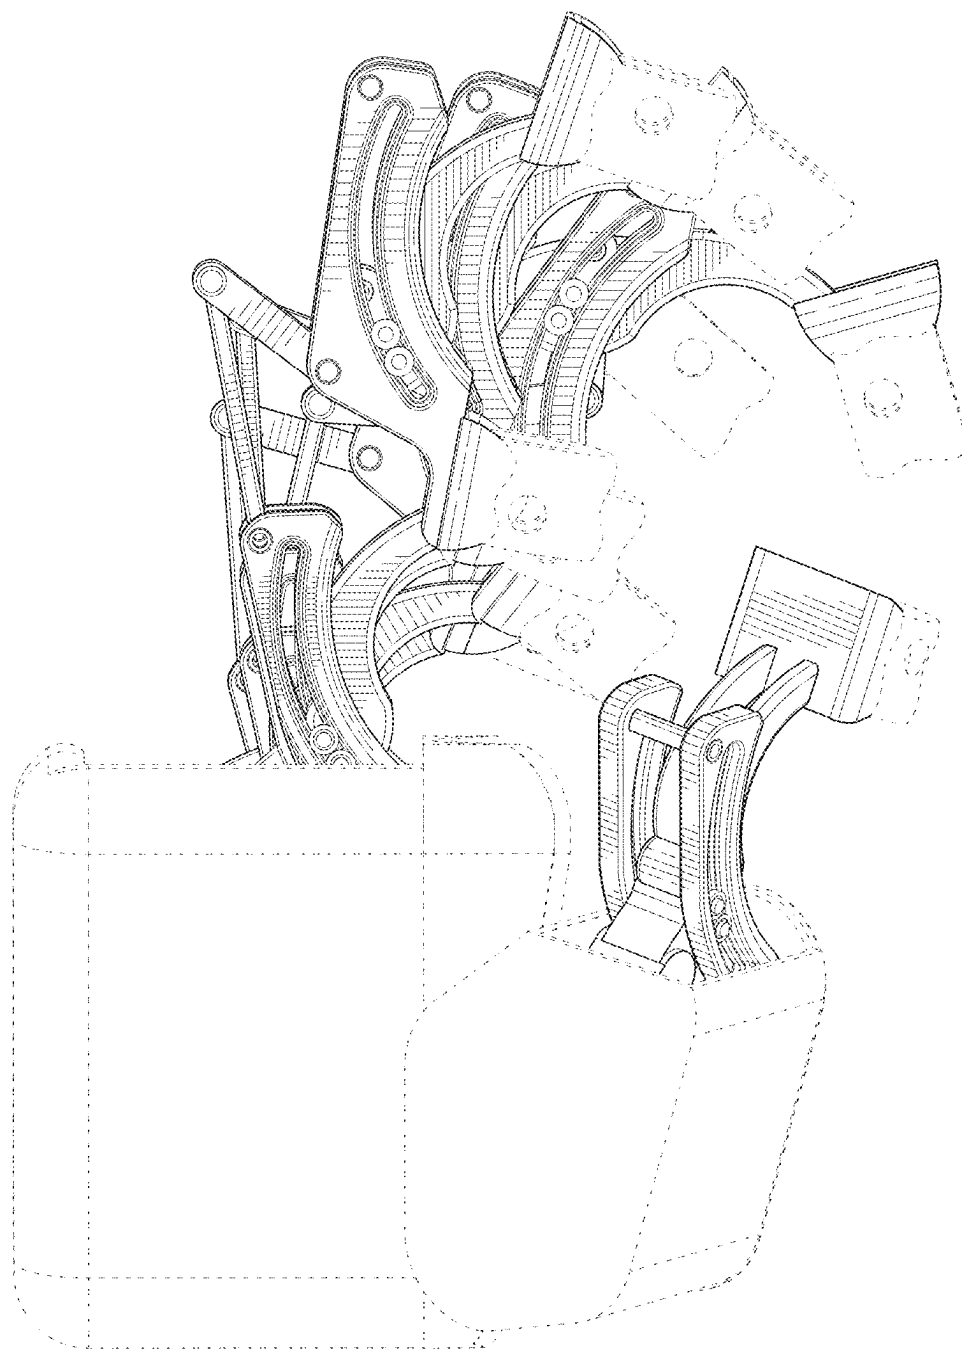


FIG. 6

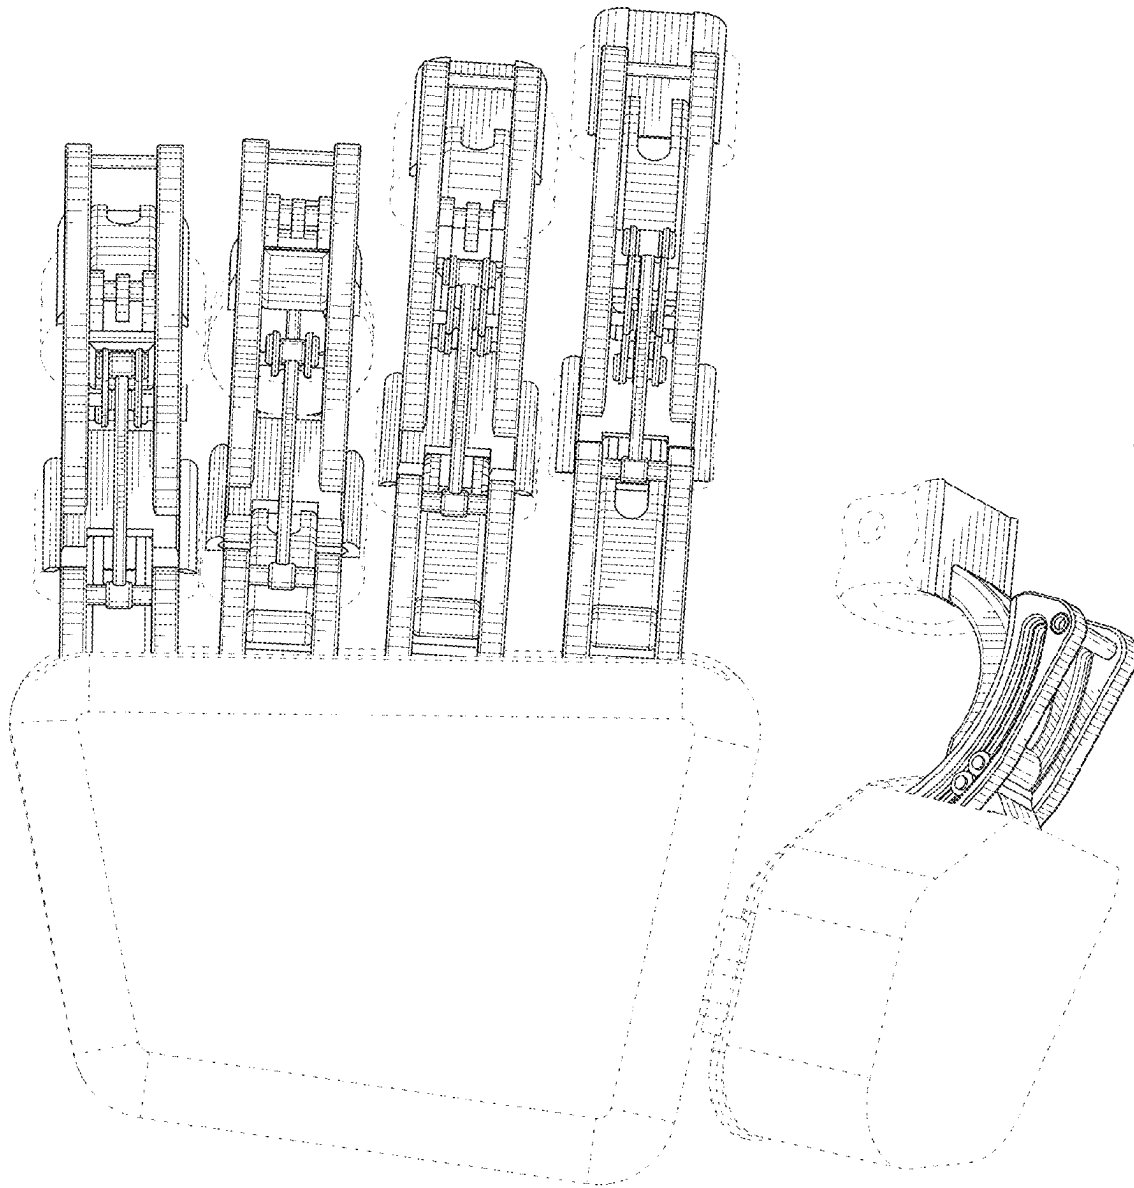


FIG.7

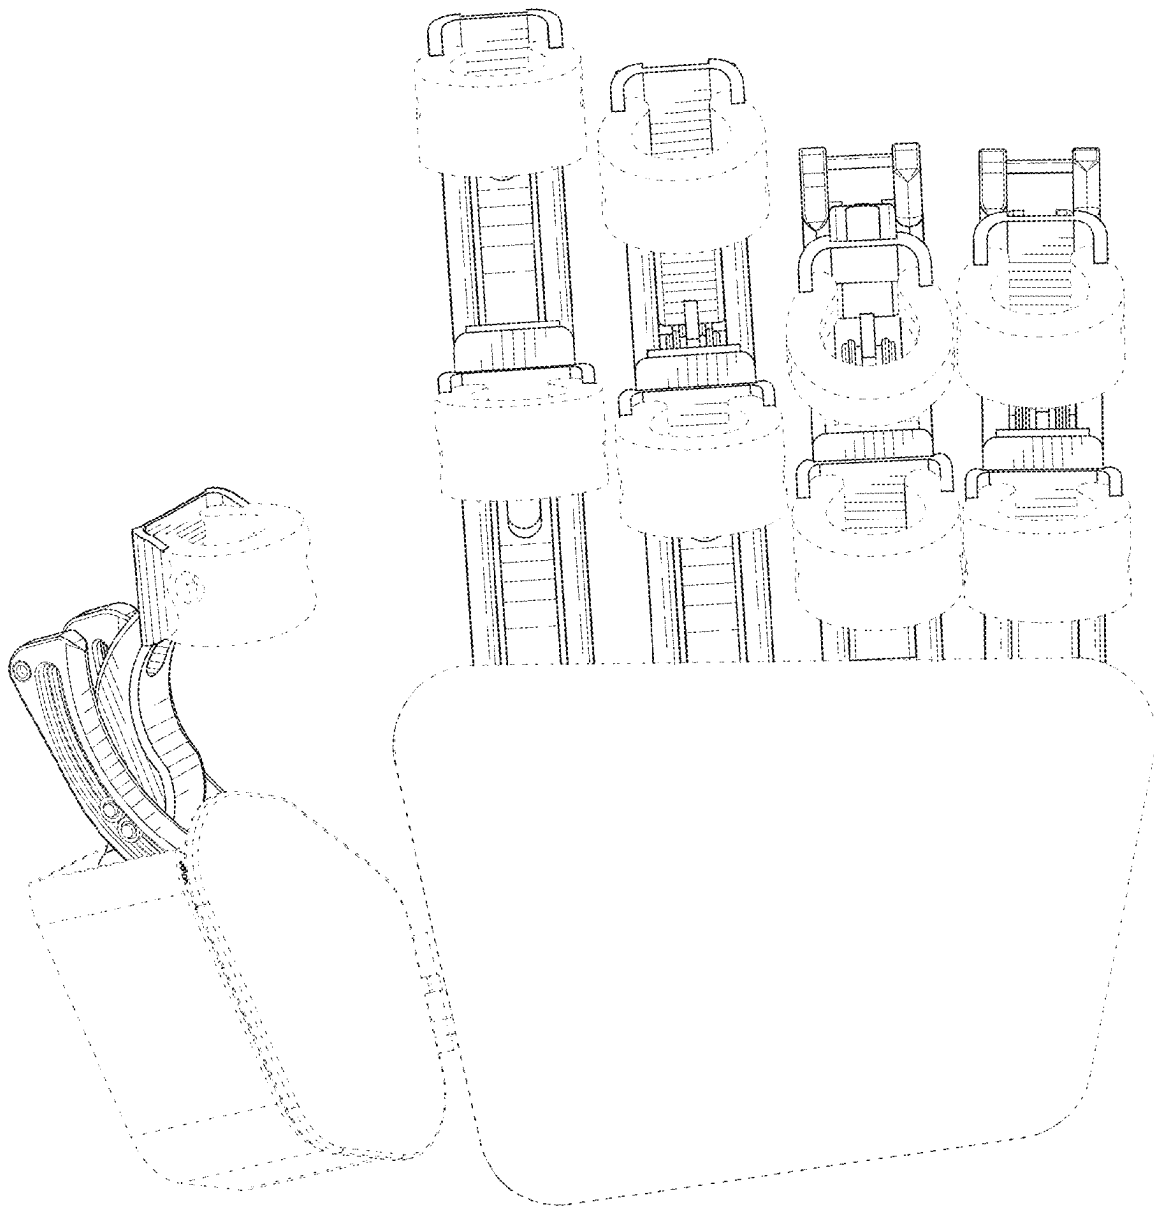


FIG. 8

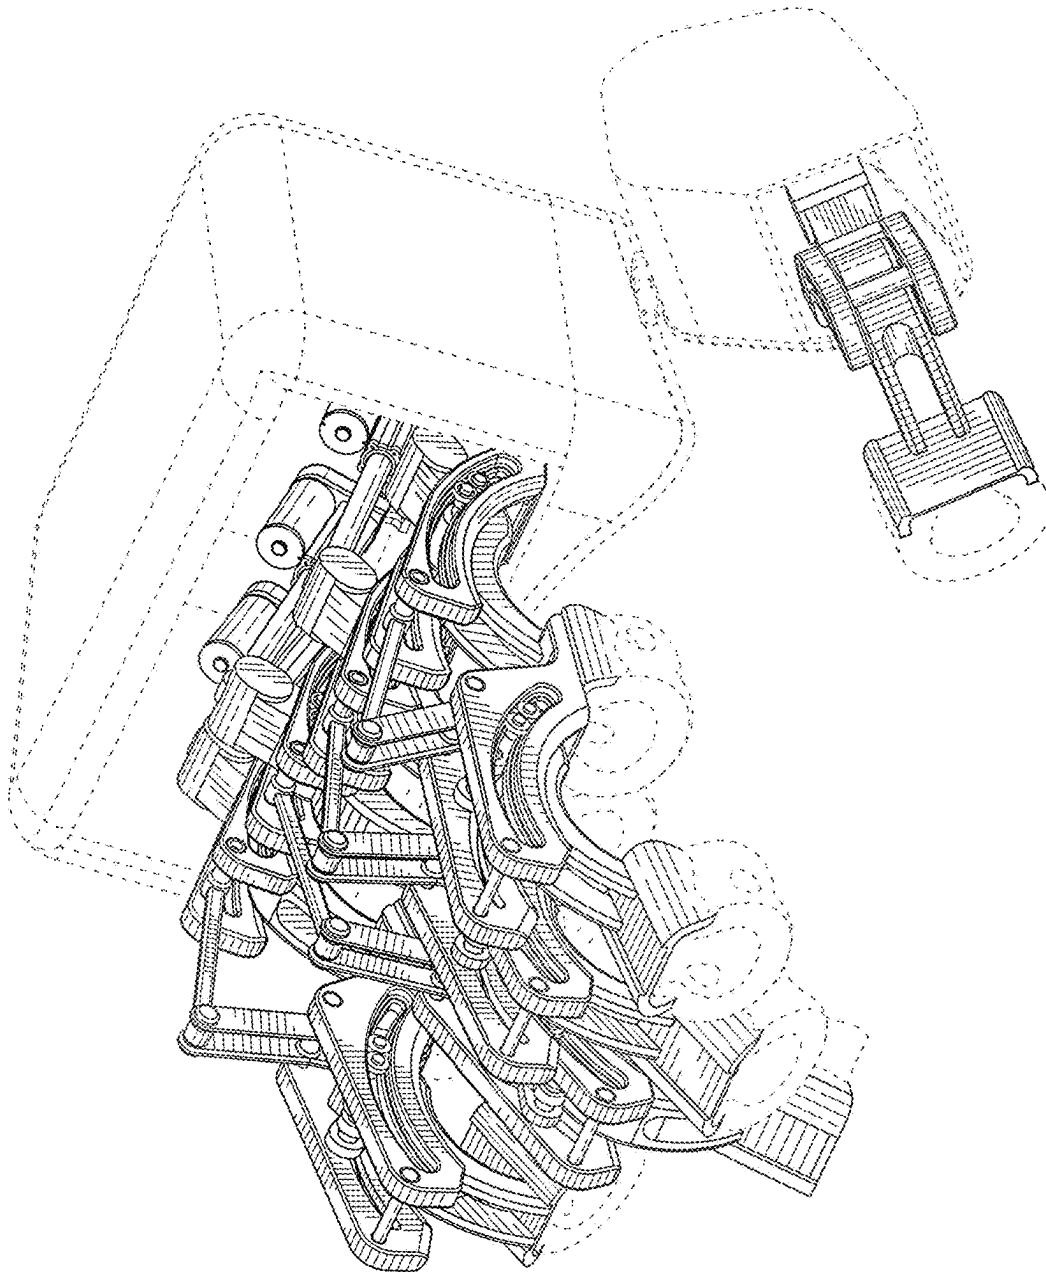


FIG.9

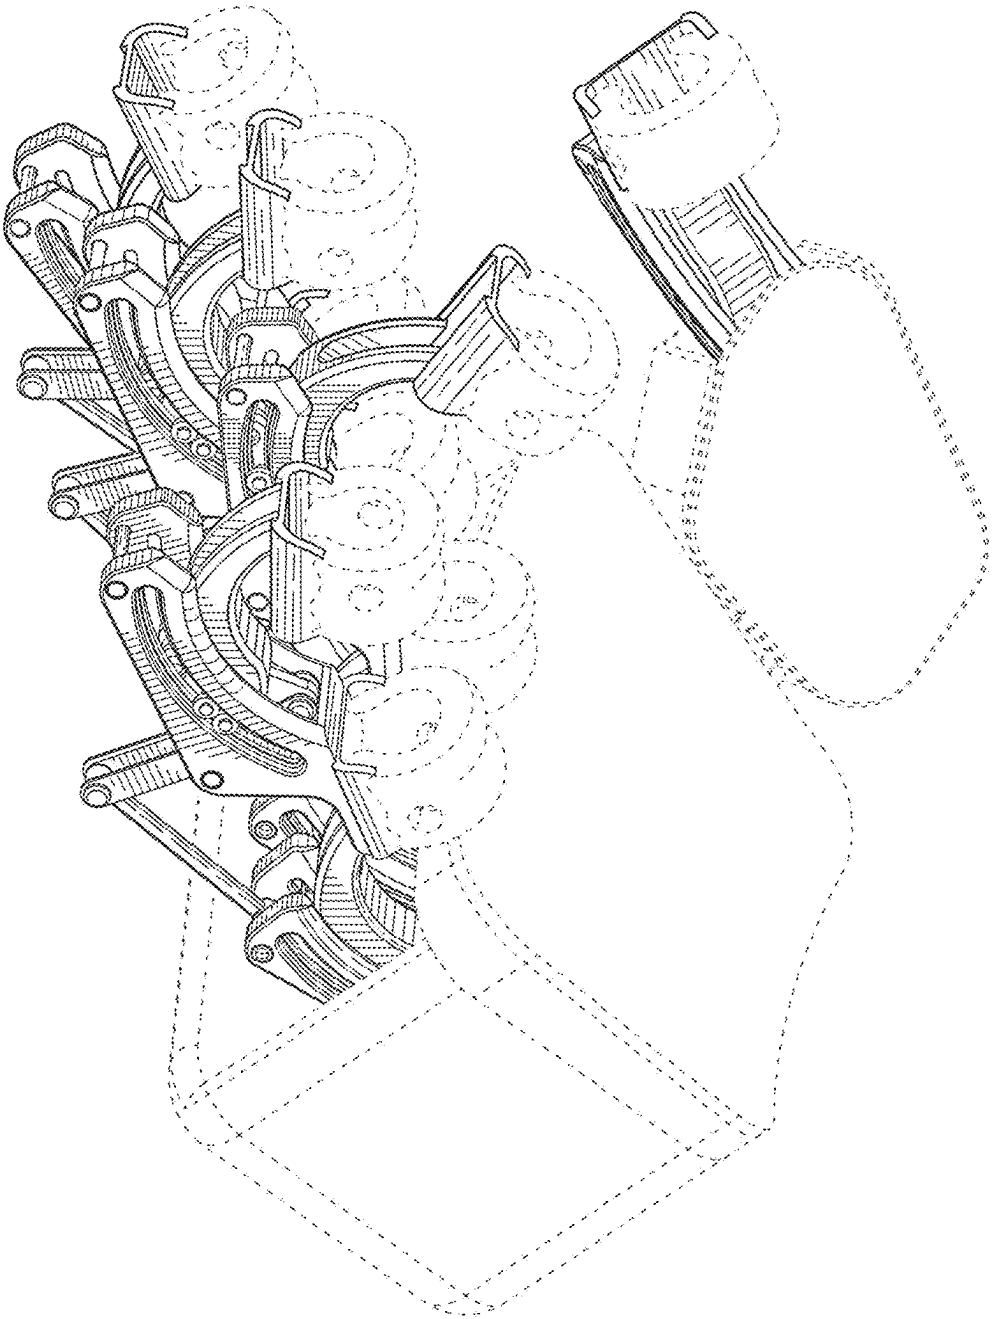


FIG.10

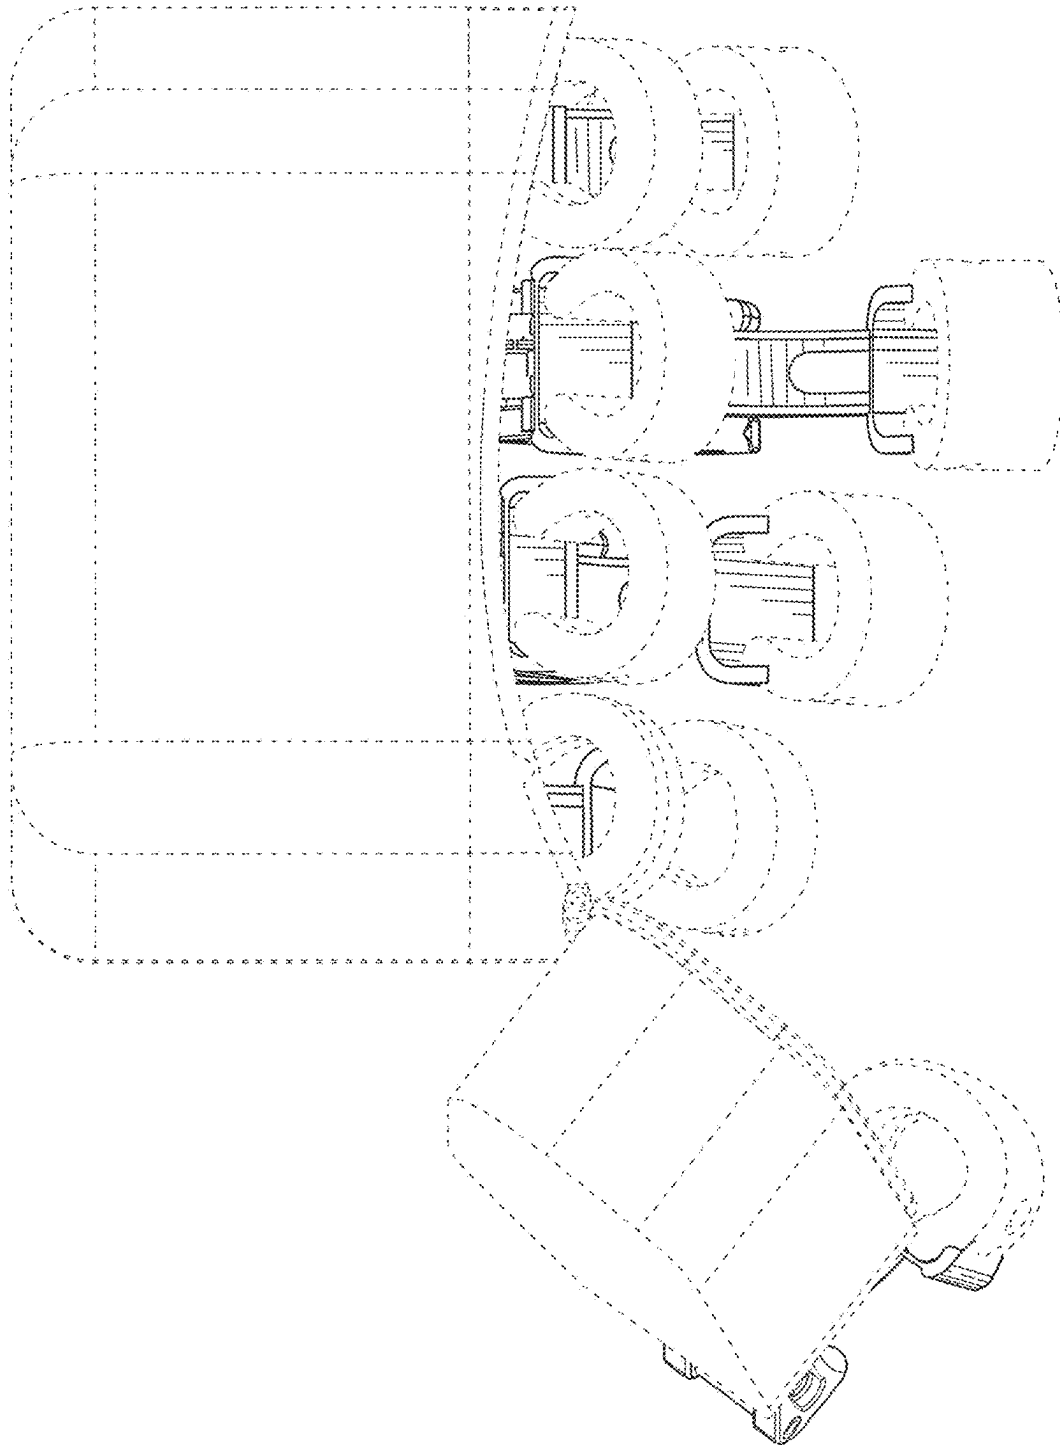


FIG.11

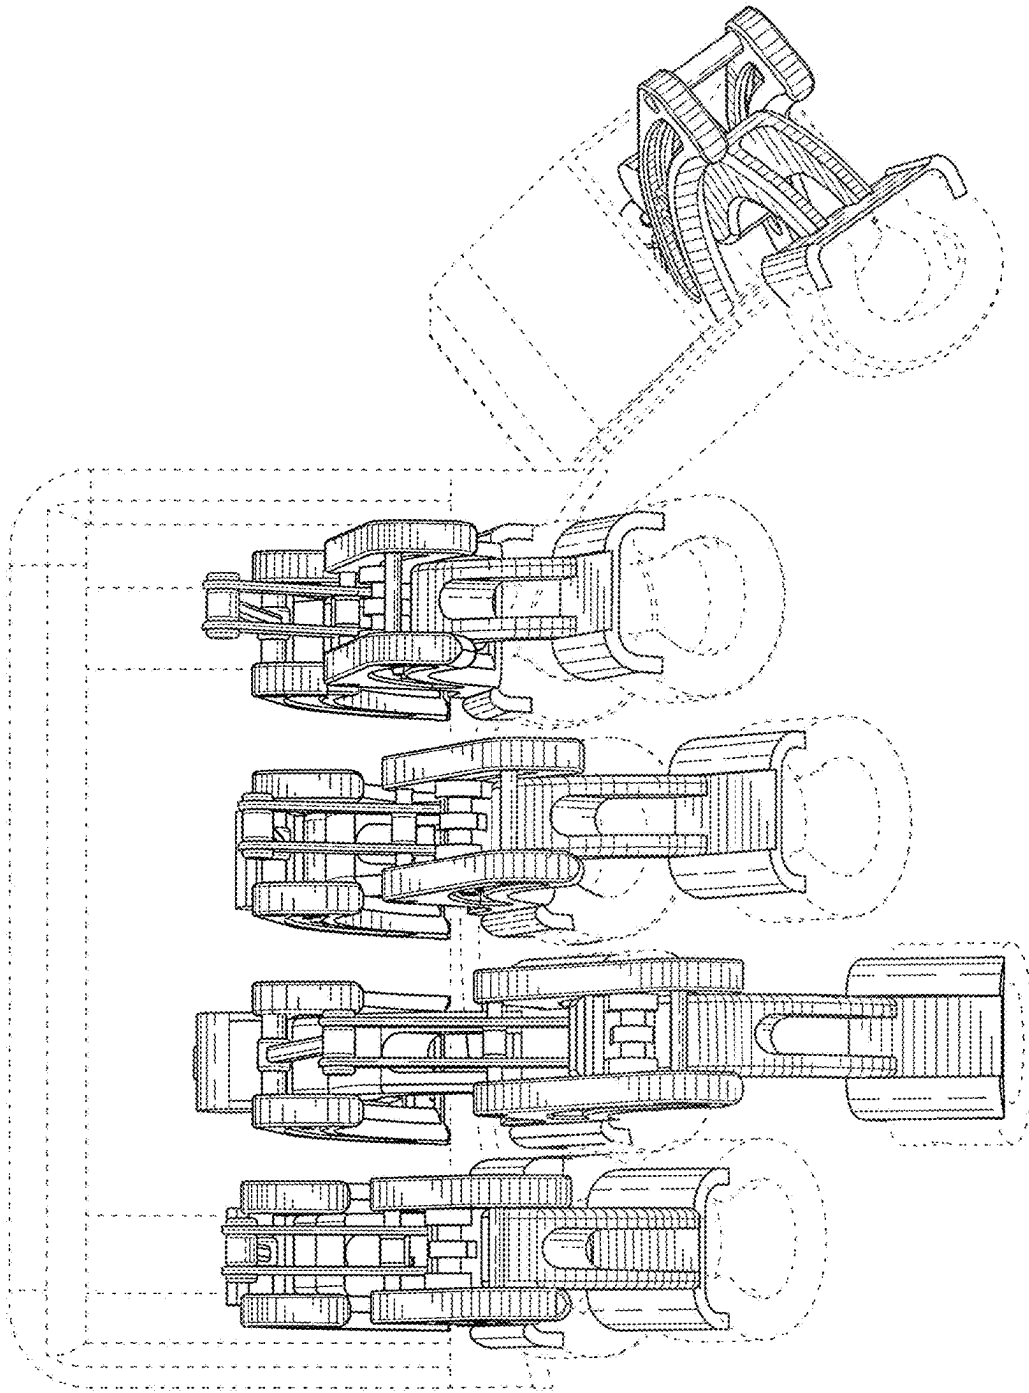


FIG.12

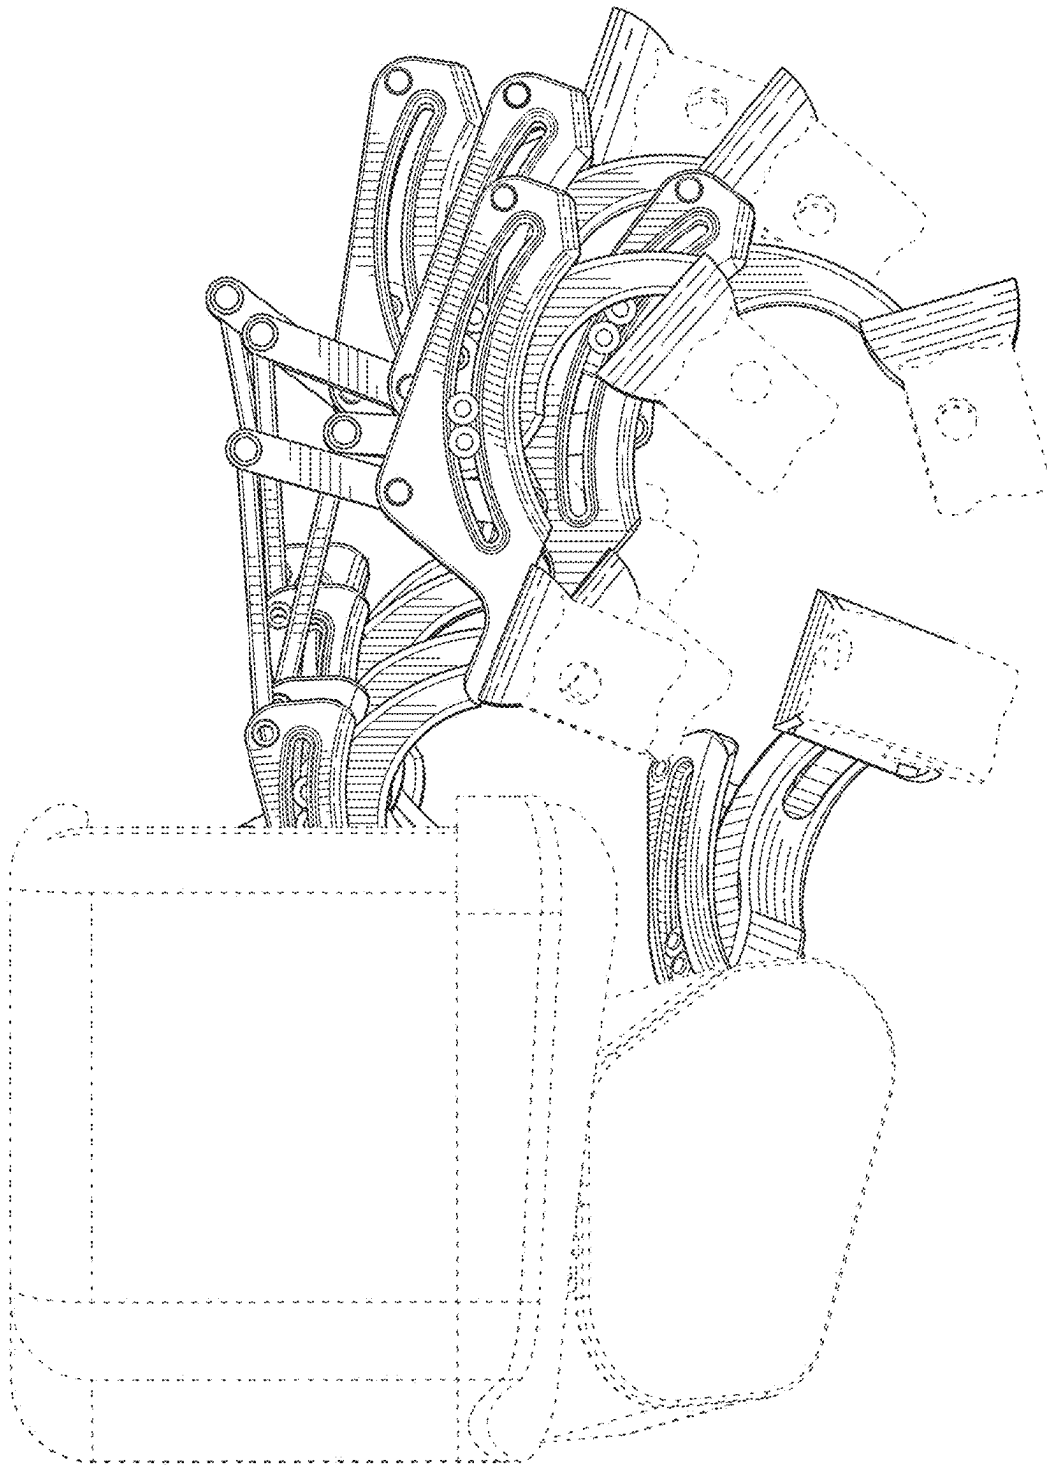


FIG.13

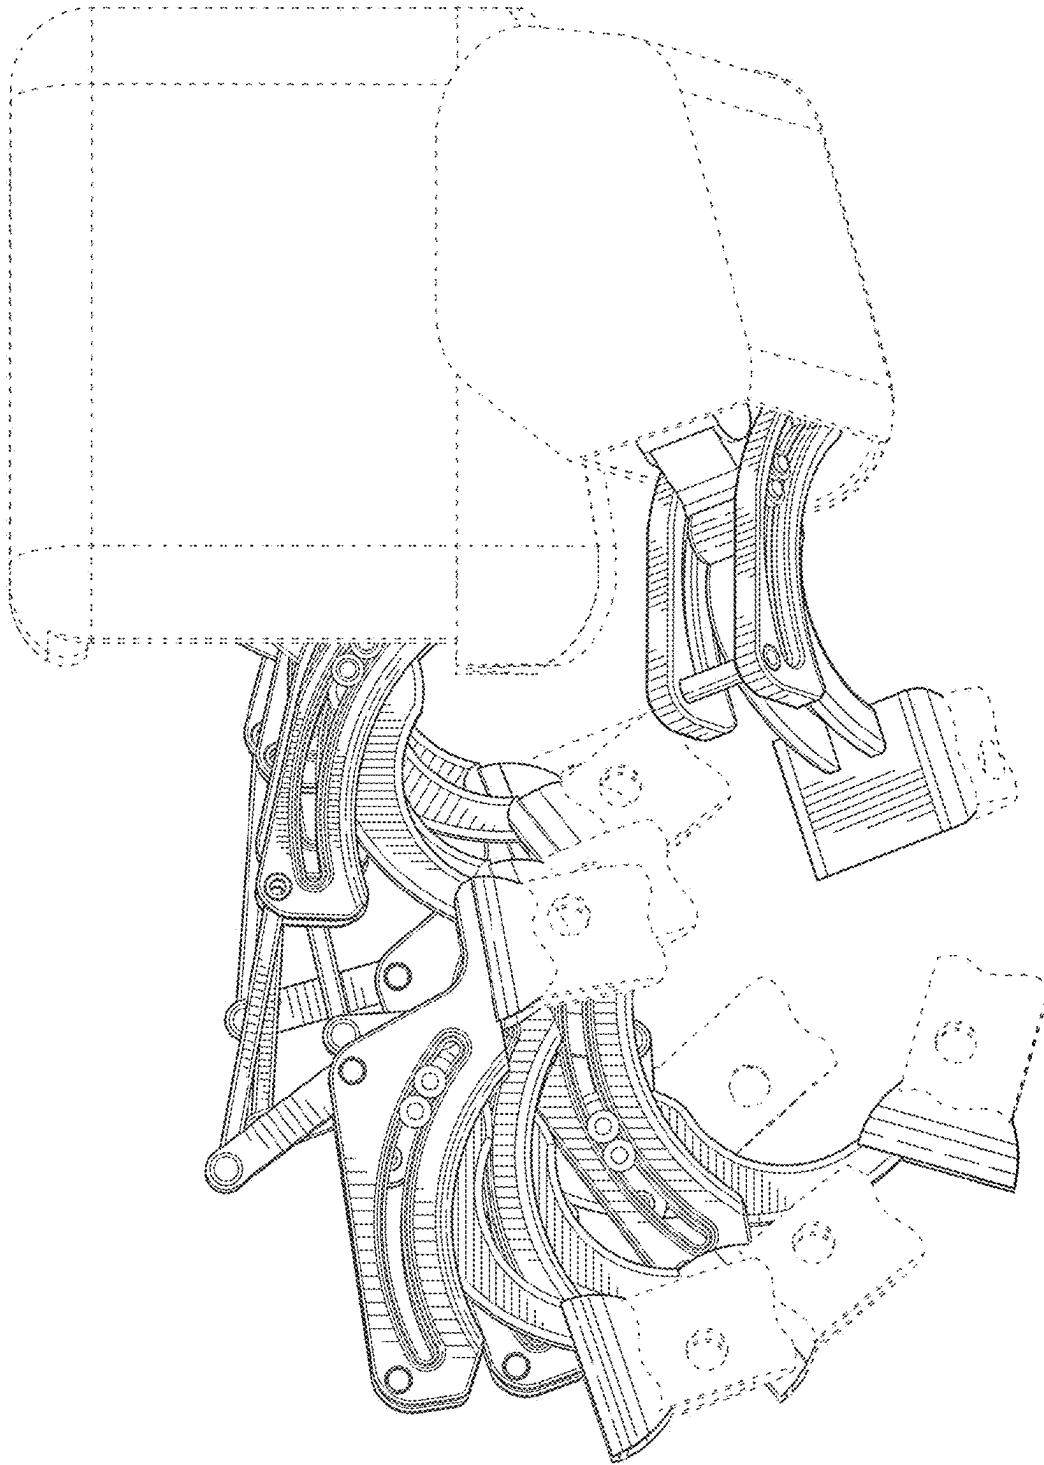


FIG.14

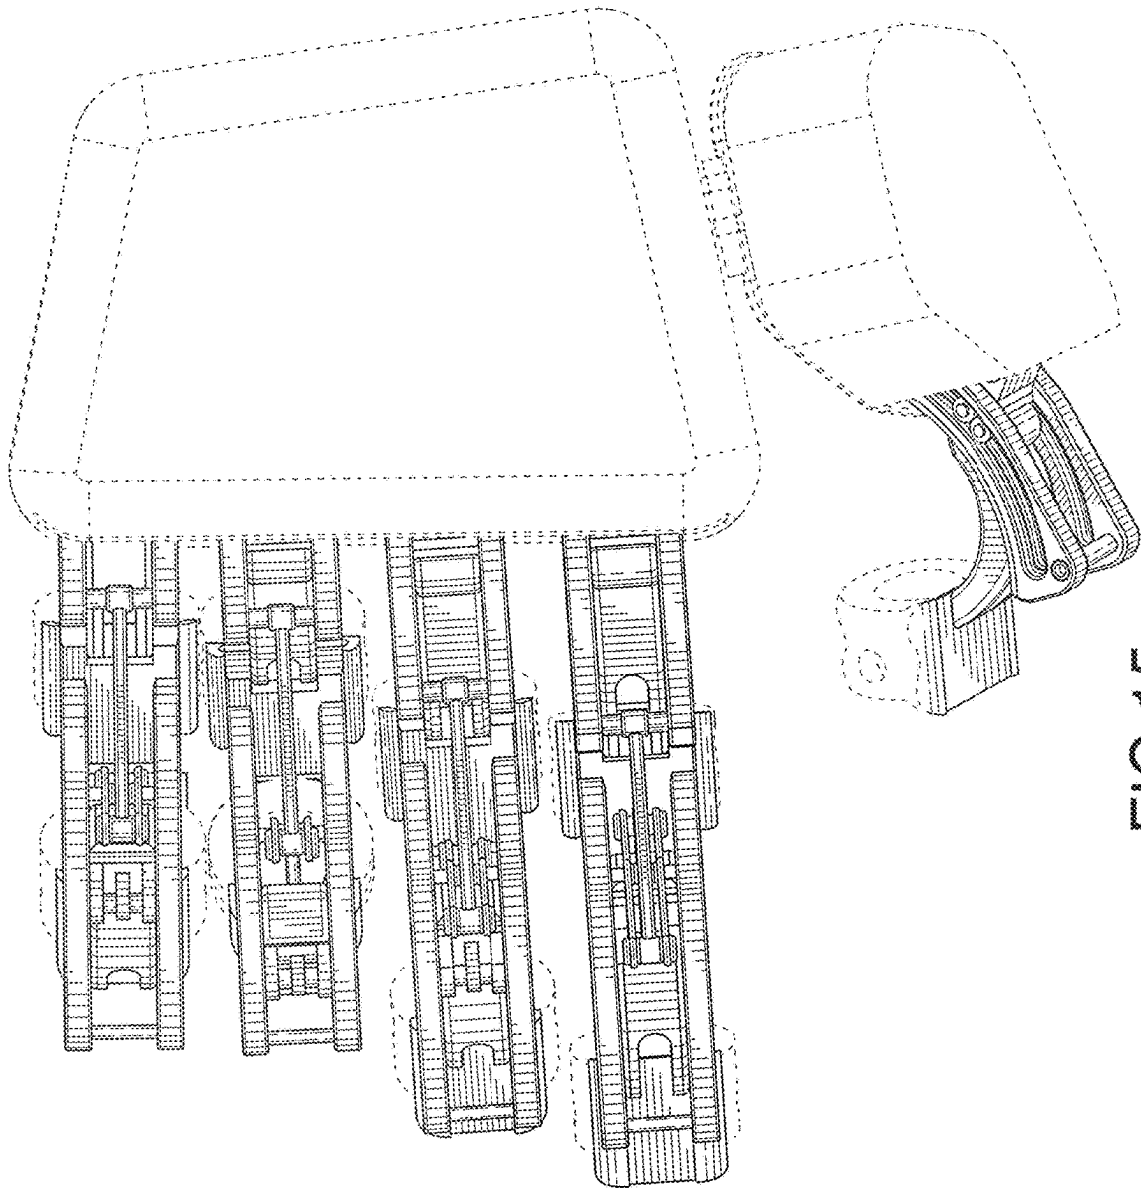


FIG.15

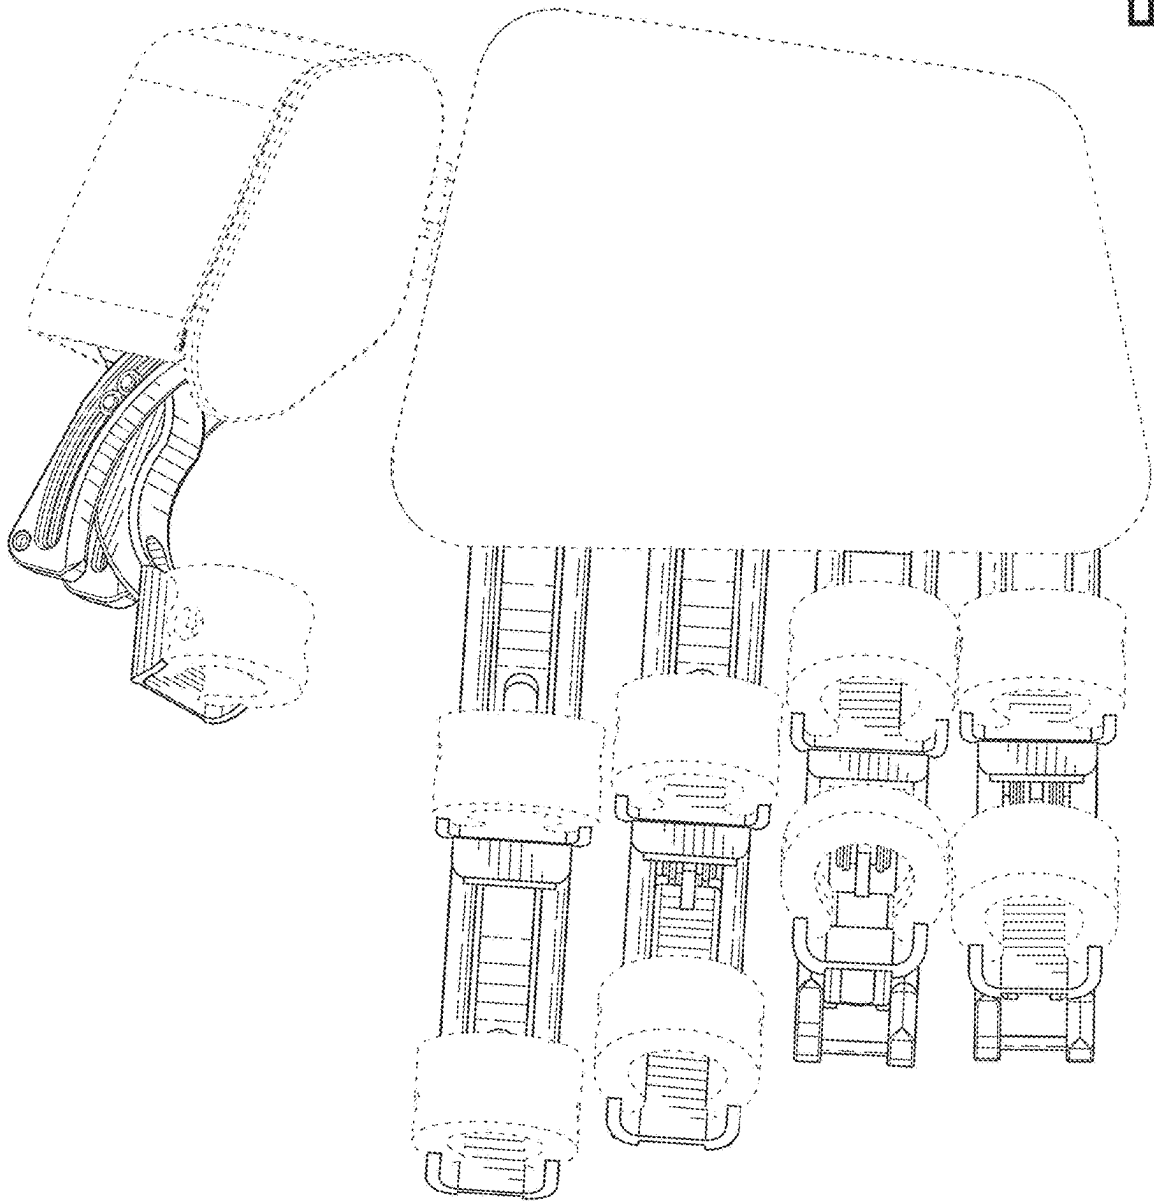


FIG. 16