



US012403313B2

(12) **United States Patent**
Haddock et al.

(10) **Patent No.:** **US 12,403,313 B2**
(45) **Date of Patent:** **Sep. 2, 2025**

(54) **METHODS AND SYSTEMS FOR ESTIMATING NEURAL ACTIVATION BY STIMULATION USING A STIMULATION SYSTEM**

(71) Applicant: **Boston Scientific Neuromodulation Corporation**, Valencia, CA (US)

(72) Inventors: **Andrew James Haddock**, Los Angeles, CA (US); **Tianhe Zhang**, Studio City, CA (US); **Mahsa Malekmohammadi**, Sherman Oaks, CA (US)

(73) Assignee: **Boston Scientific Neuromodulation Corporation**, Valencia, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 558 days.

(21) Appl. No.: **17/838,778**

(22) Filed: **Jun. 13, 2022**

(65) **Prior Publication Data**

US 2022/0395690 A1 Dec. 15, 2022

Related U.S. Application Data

(60) Provisional application No. 63/210,799, filed on Jun. 15, 2021.

(51) **Int. Cl.**
A61N 1/36 (2006.01)
A61B 5/00 (2006.01)
A61B 5/374 (2021.01)

(52) **U.S. Cl.**
CPC **A61N 1/36128** (2013.01); **A61B 5/374** (2021.01); **A61B 5/7246** (2013.01); **A61B 5/748** (2013.01)

(58) **Field of Classification Search**
None

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,999,555	A	12/1976	Person
4,144,889	A	3/1979	Tyers et al.
4,177,818	A	12/1979	De Pedro
4,341,221	A	7/1982	Testerman
4,378,797	A	4/1983	Osterholm
(Continued)			

FOREIGN PATENT DOCUMENTS

EP	813889	12/1997
EP	1048320	11/2000
(Continued)		

OTHER PUBLICATIONS

McIntyre, Cameron C., et al., "Electric Field and Stimulating Influence generated by Deep Brain Stimulation of the Subthalamaic Nucleus," *Clinical Neurophysiology*, 115(3) (Mar. 2004), pp. 589-595.

(Continued)


Primary Examiner — Shirley X Jian

(74) *Attorney, Agent, or Firm* — Branch Partners PLLC; Bruce E. Black

(57) **ABSTRACT**

A method for estimating neural activation arising from stimulation by a stimulation system includes identifying different neural elements stimulated by the stimulation; obtaining a neural response signal resulting from the stimulation by the stimulation system; and decomposing the neural response signal to estimate neural activation of each of the different neural elements.

20 Claims, 10 Drawing Sheets

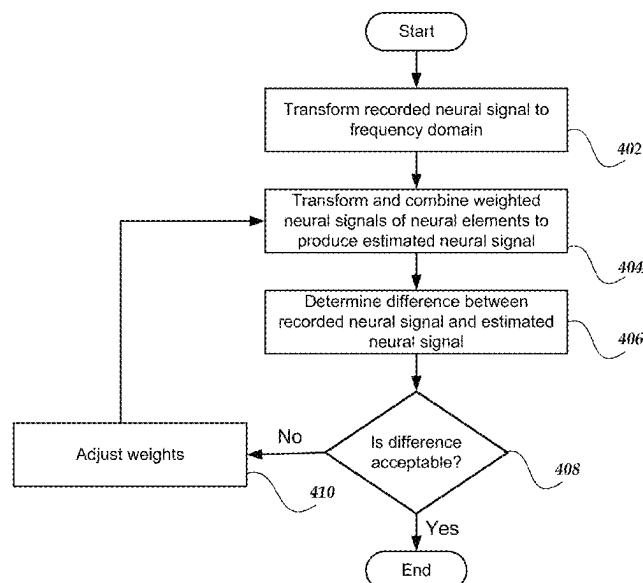

(56)

References Cited

U.S. PATENT DOCUMENTS

4,445,500	A	5/1984	Osterholm	6,442,432	B2	8/2002	Lee
4,735,208	A	4/1988	Wyer et al.	6,463,328	B1	10/2002	John
4,765,341	A	8/1988	Mower et al.	6,491,699	B1	12/2002	Henderson et al.
4,841,973	A	6/1989	Stecker	6,494,831	B1	12/2002	Koritzinsky
5,067,495	A	11/1991	Brehm	6,507,759	B1	1/2003	Prutchi et al.
5,099,846	A	3/1992	Hardy	6,510,347	B2	1/2003	Borkan
5,222,494	A	6/1993	Baker, Jr.	6,516,227	B1	2/2003	Meadows et al.
5,255,693	A	10/1993	Dutcher	6,517,480	B1	2/2003	Krass
5,259,387	A	11/1993	dePinto	6,539,263	B1	3/2003	Schiff
5,304,206	A	4/1994	Baker, Jr. et al.	6,560,490	B2	5/2003	Grill et al.
5,344,438	A	9/1994	Testerman et al.	6,579,280	B1	6/2003	Kovach et al.
5,361,763	A	11/1994	Kao et al.	6,600,956	B2	7/2003	Maschino et al.
5,452,407	A	9/1995	Crook	6,606,523	B1	8/2003	Jenkins
5,560,360	A	10/1996	Filler et al.	6,609,029	B1	8/2003	Mann et al.
5,565,949	A	10/1996	Kasha, Jr.	6,609,031	B1	8/2003	Law et al.
5,593,427	A	1/1997	Gliner et al.	6,609,032	B1	8/2003	Woods et al.
5,601,612	A	2/1997	Gliner et al.	6,622,048	B1	9/2003	Mann et al.
5,607,454	A	3/1997	Cameron et al.	6,631,297	B1	10/2003	Mo
5,620,470	A	4/1997	Gliner et al.	6,654,642	B2	11/2003	North et al.
5,651,767	A	7/1997	Schulmann	6,662,053	B2	12/2003	Borkan
5,711,316	A	1/1998	Elsberry et al.	6,675,046	B2	1/2004	Holsheimer
5,713,922	A	2/1998	King	6,684,106	B2	1/2004	Herbst
5,716,377	A	2/1998	Rise et al.	6,687,392	B1	2/2004	Touzawa et al.
5,724,985	A	3/1998	Snell et al.	6,690,972	B2	2/2004	Conley et al.
5,749,904	A	5/1998	Gliner et al.	6,690,974	B2	2/2004	Archer et al.
5,749,905	A	5/1998	Gliner et al.	6,692,315	B1	2/2004	Soumillion et al.
5,776,170	A	7/1998	MacDonald et al.	6,694,162	B2	2/2004	Hartlep
5,782,762	A	7/1998	Vining	6,694,163	B1	2/2004	Vining
5,843,148	A	12/1998	Gijsbers et al.	6,708,096	B1	3/2004	Frei et al.
5,859,922	A	1/1999	Hoffmann	6,741,892	B1	5/2004	Meadows et al.
5,868,740	A	2/1999	LeVeen et al.	6,748,098	B1	6/2004	Rosenfeld
5,897,583	A	4/1999	Meyer et al.	6,748,276	B1	6/2004	Daignault, Jr. et al.
5,910,804	A	6/1999	Fortenbery et al.	6,778,846	B1	8/2004	Martinez et al.
5,925,070	A	7/1999	King et al.	6,788,969	B2	9/2004	Dupree et al.
5,938,688	A	8/1999	Schiff	6,795,737	B2	9/2004	Gielen et al.
5,938,690	A	8/1999	Law et al.	6,827,681	B2	12/2004	Tanner et al.
5,978,713	A	11/1999	Prutchi et al.	6,830,544	B2	12/2004	Tanner
6,016,449	A	1/2000	Fischell et al.	6,845,267	B2	1/2005	Harrison et al.
6,029,090	A	2/2000	Herbst	6,850,802	B2	2/2005	Holsheimer
6,029,091	A	2/2000	de la Rama et al.	6,895,280	B2	5/2005	Meadows et al.
6,050,992	A	4/2000	Nichols	6,909,913	B2	6/2005	Vining
6,058,331	A	5/2000	King	6,937,891	B2	8/2005	Leinders et al.
6,066,163	A	5/2000	John	6,937,903	B2	8/2005	Schuler et al.
6,080,187	A	6/2000	Alt et al.	6,944,497	B2	9/2005	Stypulkowski
6,083,162	A	7/2000	Vining	6,944,501	B1	9/2005	Pless
6,094,598	A	7/2000	Elsberry et al.	6,950,707	B2	9/2005	Whitehurst
6,096,756	A	8/2000	Crain et al.	6,969,388	B2	11/2005	Goldman et al.
6,106,460	A	8/2000	Panescu et al.	6,993,384	B2	1/2006	Bradley et al.
6,109,269	A	8/2000	Rise et al.	7,003,349	B1	2/2006	Andersson et al.
6,128,538	A	10/2000	Fischell et al.	7,003,352	B1	2/2006	Whitehurst
6,129,685	A	10/2000	Howard, III	7,008,370	B2	3/2006	Tanner et al.
6,146,390	A	11/2000	Heilbrun et al.	7,008,413	B2	3/2006	Kovach et al.
6,161,044	A	12/2000	Silverstone	7,035,690	B2	4/2006	Goetz
6,167,311	A	12/2000	Rezai	7,043,293	B1	5/2006	Baura
6,181,969	B1	1/2001	Gord	7,047,082	B1	5/2006	Schrom et al.
6,192,266	B1	2/2001	Dupree et al.	7,047,084	B2	5/2006	Erickson et al.
6,205,361	B1	3/2001	Kuzma	7,050,857	B2	5/2006	Samuelsson et al.
6,208,881	B1	3/2001	Champeau	7,054,692	B1	5/2006	Whitehurst et al.
6,240,308	B1	5/2001	Hardy et al.	7,058,446	B2	6/2006	Schuler et al.
6,246,912	B1	6/2001	Sluijter et al.	7,082,333	B1	7/2006	Bauhahn et al.
6,253,109	B1	6/2001	Gielen	7,107,102	B2	9/2006	Daignault et al.
6,289,239	B1	9/2001	Panescu et al.	7,126,000	B2	10/2006	Ogawa et al.
6,301,492	B1	10/2001	Zonenshayn	7,127,297	B2	10/2006	Law et al.
6,310,619	B1	10/2001	Rice	7,136,518	B2	11/2006	Griffin et al.
6,319,241	B1	11/2001	King	7,136,695	B2	11/2006	Pless et al.
6,336,899	B1	1/2002	Yamazaki	7,142,923	B2	11/2006	North et al.
6,343,226	B1	1/2002	Sunde et al.	7,146,219	B2	12/2006	Sieracki et al.
6,351,675	B1	2/2002	Tholen et al.	7,146,223	B1	12/2006	King
6,353,762	B1	3/2002	Baudino et al.	7,151,961	B1	12/2006	Whitehurst
6,366,813	B1	4/2002	Dilorenzo	7,155,279	B2	12/2006	Whitehurst
6,368,331	B1	4/2002	Front et al.	7,167,760	B2	1/2007	Dawant et al.
6,389,311	B1	5/2002	Whayne et al.	7,177,674	B2	2/2007	Echaz et al.
6,393,325	B1	5/2002	Mann et al.	7,181,286	B2	2/2007	Sieracki et al.
6,421,566	B1	7/2002	Holsheimer	7,184,837	B2	2/2007	Goetz
6,435,878	B1	8/2002	Reynolds et al.	7,191,014	B2	3/2007	Kobayashi et al.
				7,209,787	B2	4/2007	Dilorenzo
				7,211,050	B1	5/2007	Caplygin
				7,216,000	B2	5/2007	Sieracki et al.
				7,217,276	B2	5/2007	Henderson

(56)

References Cited

U.S. PATENT DOCUMENTS

7,218,968 B2	5/2007	Condie et al.	8,306,627 B2	11/2012	Armstrong
7,228,179 B2	6/2007	Campen et al.	8,326,433 B2	12/2012	Blum et al.
7,231,254 B2	6/2007	DiLorenzo	8,364,278 B2	1/2013	Pianca et al.
7,236,830 B2	6/2007	Gliner	8,369,954 B2	2/2013	Stack et al.
7,239,910 B2	7/2007	Tanner	8,379,952 B2	2/2013	McIntyre et al.
7,239,916 B2	7/2007	Thompson et al.	8,391,985 B2	3/2013	McDonald
7,239,926 B2	7/2007	Goetz	8,429,174 B2	4/2013	Ramani et al.
7,242,984 B2	7/2007	DiLorenzo	8,452,415 B2	5/2013	Goetz et al.
7,244,150 B1	7/2007	Brase et al.	8,473,061 B2	6/2013	Moffitt et al.
7,252,090 B2	8/2007	Goetz	8,483,237 B2	7/2013	Zimmermann et al.
7,254,445 B2	8/2007	Law et al.	8,543,189 B2	9/2013	Paitel et al.
7,254,446 B1	8/2007	Erickson	8,571,665 B2	10/2013	Moffitt et al.
7,257,447 B2	8/2007	Cates et al.	8,589,316 B2	11/2013	Lujan et al.
7,266,412 B2	9/2007	Stypulkowski	8,594,800 B2	11/2013	Butson et al.
7,289,761 B2	10/2007	Mazar et al.	8,594,801 B2	11/2013	Corndorf et al.
7,294,107 B2	11/2007	Simon et al.	8,606,360 B2	12/2013	Butson et al.
7,295,876 B1	11/2007	Erickson	8,620,452 B2	12/2013	King et al.
7,299,096 B2	11/2007	Balzer et al.	8,649,845 B2	2/2014	McIntyre et al.
7,308,302 B1	12/2007	Schuler et al.	8,675,945 B2	3/2014	Barnhorst et al.
7,313,430 B2	12/2007	Urquhart	8,679,038 B1	3/2014	Giuffrida
7,324,851 B1	1/2008	DiLorenzo	8,688,235 B1	4/2014	Pianca et al.
7,346,282 B2	3/2008	Sakanaka et al.	8,744,596 B2	6/2014	Howard
7,346,382 B2	3/2008	McIntyre et al.	8,751,008 B2	6/2014	Carlton et al.
7,385,443 B1	6/2008	Denison	8,774,941 B2	7/2014	Pianca
7,388,974 B2	6/2008	Yanagita	8,792,993 B2	7/2014	Pianca et al.
7,437,193 B2	10/2008	Parramon et al.	8,831,731 B2	9/2014	Blum et al.
7,450,997 B1	11/2008	Pianca et al.	8,831,742 B2	9/2014	Pianca et al.
7,454,245 B2	11/2008	Armstrong et al.	8,845,557 B1	9/2014	Giuffrida et al.
7,463,928 B2	12/2008	Lee et al.	8,849,632 B2	9/2014	Sparks et al.
7,499,048 B2	3/2009	Sieracki et al.	8,855,773 B2	10/2014	Kokones et al.
7,499,752 B2 *	3/2009	Maschino A61N 1/36082 607/40	8,868,199 B2	10/2014	Kaula et al.
7,505,815 B2	3/2009	Lee et al.	8,913,804 B2	12/2014	Blum et al.
7,532,935 B2 *	5/2009	Maschino A61N 1/36082 607/45	8,918,183 B2	12/2014	Carlton et al.
7,548,786 B2	6/2009	Lee et al.	8,918,184 B1	12/2014	Torgerson et al.
7,555,344 B2 *	6/2009	Maschino A61N 1/36082 607/18	8,923,976 B2	12/2014	Johanek
7,565,199 B2	7/2009	Sheffield et al.	8,958,615 B2	2/2015	Blum et al.
7,603,177 B2	10/2009	Sieracki et al.	8,972,023 B2	3/2015	Bradley et al.
7,617,002 B2	11/2009	Goetz	9,020,789 B2	4/2015	Butson et al.
7,623,918 B2	11/2009	Goetz	9,026,317 B2	5/2015	Furukawa et al.
7,650,184 B2	1/2010	Walter	9,050,470 B2	6/2015	Carlton et al.
7,657,319 B2	2/2010	Goetz et al.	9,061,138 B2	6/2015	Pianca
7,672,734 B2	3/2010	Anderson et al.	9,072,905 B2	7/2015	Kokones et al.
7,676,273 B2	3/2010	Goetz et al.	9,081,488 B2	7/2015	Soederstroem
7,680,526 B2	3/2010	McIntyre et al.	9,084,896 B2	7/2015	Kokones et al.
7,734,340 B2	6/2010	De Ridder	9,095,266 B1 *	8/2015	Fu G16H 50/20
7,761,165 B1	7/2010	He et al.	9,135,400 B2	9/2015	McIntyre et al.
7,783,359 B2	8/2010	Meadows	9,149,630 B2	10/2015	Howard et al.
7,792,590 B1	9/2010	Pianca et al.	9,162,056 B2	10/2015	Pianca
7,809,446 B2	10/2010	Meadows	9,220,889 B2	12/2015	Carlton et al.
7,826,902 B2	11/2010	Stone et al.	9,227,074 B2	1/2016	Carcieri et al.
7,848,802 B2	12/2010	Goetz et al.	9,235,685 B2	1/2016	McIntyre et al.
7,860,548 B2	12/2010	McIntyre et al.	9,248,272 B2	2/2016	Romero
7,896,808 B1	3/2011	Koh et al.	9,248,296 B2	2/2016	Carcieri et al.
7,904,134 B2	3/2011	McIntyre et al.	9,254,387 B2	2/2016	Blum et al.
7,945,105 B1	5/2011	Jaenisch	9,272,153 B2	3/2016	Blum et al.
7,949,395 B2	5/2011	Kuzma	9,289,596 B2	3/2016	Leven
7,974,706 B2	7/2011	Moffitt et al.	9,289,600 B2	3/2016	Govea et al.
8,000,794 B2	8/2011	Lozano	9,302,110 B2	4/2016	Kokones et al.
8,019,439 B2	9/2011	Kuzma et al.	9,308,372 B2	4/2016	Sparks et al.
8,150,524 B2 *	4/2012	Maschino A61N 1/36082 607/18	9,310,985 B2	4/2016	Blum et al.
8,175,710 B2	5/2012	He	9,327,111 B2	5/2016	Pianca et al.
8,180,601 B2	5/2012	Butson et al.	9,358,398 B2	6/2016	Moffitt et al.
8,187,209 B1	5/2012	Giuffrida	9,364,665 B2	6/2016	Bokil et al.
8,195,300 B2	6/2012	Gliner et al.	9,381,348 B2	7/2016	Romero et al.
8,209,027 B2	6/2012	Butson et al.	9,387,325 B1	7/2016	Min et al.
8,224,450 B2	7/2012	Brase	9,415,154 B2	8/2016	Leven
8,257,684 B2	9/2012	Covalin et al.	9,474,903 B2	10/2016	Chen et al.
8,262,714 B2	9/2012	Hulvershorn et al.	9,492,655 B2	11/2016	Pianca et al.
8,271,094 B1	9/2012	Moffitt et al.	9,498,620 B2	11/2016	Romero et al.
8,280,514 B2	10/2012	Lozano et al.	9,526,902 B2	12/2016	Blum et al.
8,295,944 B2	10/2012	Howard et al.	9,566,596 B2	2/2017	Kim et al.
			9,572,982 B2	2/2017	Burnes et al.
			9,586,053 B2	3/2017	Moffitt et al.
			9,592,389 B2	3/2017	Moffitt
			9,713,720 B2	7/2017	Zhu
			9,775,988 B2	10/2017	Govea et al.
			9,792,412 B2	10/2017	Moffitt et al.
			9,821,167 B2	11/2017	Carcieri et al.
			9,925,382 B2	3/2018	Carlton et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,959,940 B2	5/2018	Moffitt et al.	2005/0049649 A1	3/2005	Luders et al.
9,974,959 B2	5/2018	Moffitt et al.	2005/0060001 A1	3/2005	Singhal et al.
10,067,659 B2	9/2018	Bokil	2005/0060009 A1	3/2005	Goetz
10,071,249 B2	9/2018	Zottola	2005/0070781 A1	3/2005	Dawant et al.
10,086,205 B2	10/2018	Grill et al.	2005/0075689 A1	4/2005	Toy et al.
10,213,148 B2	2/2019	Min et al.	2005/0085714 A1	4/2005	Foley et al.
10,265,528 B2	4/2019	Carcieri et al.	2005/0165294 A1	7/2005	Weiss
10,265,531 B2	4/2019	Bokil	2005/0171587 A1	8/2005	Daglow et al.
10,286,205 B2	5/2019	Steinke et al.	2005/0228250 A1	10/2005	Bitter et al.
10,300,282 B2	5/2019	Torgerson et al.	2005/0251061 A1	11/2005	Schuler et al.
10,335,607 B2	7/2019	Orinski	2005/0261061 A1	11/2005	Nguyen et al.
10,357,657 B2	7/2019	Moffitt et al.	2005/0261601 A1	11/2005	Schuler et al.
10,369,364 B2	8/2019	Moffitt et al.	2005/0261747 A1	11/2005	Schuler et al.
10,463,860 B2 *	11/2019	Sinclair A61B 5/4842	2005/0267347 A1	12/2005	Oster
10,485,969 B2	11/2019	Govea et al.	2005/0288732 A1	12/2005	Schuler et al.
10,493,269 B2	12/2019	Stoffregen et al.	2006/0004422 A1	1/2006	De Ridder
10,525,257 B2	1/2020	Govea et al.	2006/0017749 A1	1/2006	McIntyre et al.
10,525,266 B2	1/2020	Moffitt et al.	2006/0020292 A1	1/2006	Goetz et al.
10,603,498 B2	3/2020	Blum et al.	2006/0069415 A1	3/2006	Cameron et al.
10,625,072 B2	4/2020	Serrano Carmona	2006/0094951 A1	5/2006	Dean et al.
10,631,937 B2	4/2020	Tyulmankov et al.	2006/0095088 A1	5/2006	De Riddler
10,639,488 B2	5/2020	Kalgren et al.	2006/0155340 A1	7/2006	Schuler et al.
10,653,330 B2	5/2020	Angle et al.	2006/0206169 A1	9/2006	Schuler
10,675,468 B2	6/2020	Torgerson	2006/0218007 A1	9/2006	Bjorner et al.
10,716,505 B2	7/2020	Blum et al.	2006/0224189 A1	10/2006	Schuler et al.
10,780,282 B2	9/2020	Mustakos et al.	2006/0235472 A1	10/2006	Goetz et al.
10,814,127 B2	10/2020	Nageri et al.	2006/0259079 A1	11/2006	King
10,814,140 B2	10/2020	Zhang et al.	2006/0259099 A1	11/2006	Goetz et al.
10,850,101 B2	12/2020	Zhang et al.	2007/0000372 A1	1/2007	Rezai et al.
10,960,203 B2	3/2021	Tyler et al.	2007/0017749 A1	1/2007	Dold et al.
11,020,052 B2	6/2021	Zuckerman-Stark et al.	2007/0027499 A1 *	2/2007	Maschino A61N 1/36096 607/45
11,185,697 B2 *	11/2021	Sinclair A61B 5/6868	2007/0027514 A1	2/2007	Gerber
11,278,726 B2 *	3/2022	Sinclair A61N 1/36167	2007/0043268 A1	2/2007	Russell
11,285,329 B2	3/2022	Carcieri et al.	2007/0049817 A1	3/2007	Preiss et al.
11,298,550 B2	4/2022	Howard et al.	2007/0067003 A1	3/2007	Sanchez et al.
11,357,986 B2	6/2022	Steinke et al.	2007/0078498 A1	4/2007	Rezai et al.
11,517,755 B2	12/2022	Zhang et al.	2007/0083104 A1	4/2007	Butson et al.
11,707,622 B2	7/2023	Juarez Paz et al.	2007/0123953 A1	5/2007	Lee et al.
11,745,010 B2	9/2023	Donega et al.	2007/0129769 A1	6/2007	Bourget et al.
11,890,478 B2 *	2/2024	Sinclair A61B 5/377	2007/0135855 A1	6/2007	Foshee et al.
2001/0031071 A1	10/2001	Nichols et al.	2007/0150036 A1	6/2007	Anderson
2002/0032375 A1	3/2002	Bauch et al.	2007/0156186 A1	7/2007	Lee et al.
2002/0062143 A1	5/2002	Baudino et al.	2007/0162086 A1	7/2007	DiLorenzo
2002/0087201 A1	7/2002	Firlik et al.	2007/0162235 A1	7/2007	Zhan et al.
2002/0099295 A1	7/2002	Gil et al.	2007/0168004 A1	7/2007	Walter
2002/0115603 A1	8/2002	Whitehouse	2007/0168007 A1	7/2007	Kuzma et al.
2002/0116030 A1	8/2002	Rezei	2007/0179557 A1	8/2007	Maschino et al.
2002/0123780 A1	9/2002	Grill et al.	2007/0185544 A1	8/2007	Dawant et al.
2002/0128694 A1	9/2002	Holsheimer	2007/0191887 A1	8/2007	Schuler et al.
2002/0151939 A1	10/2002	Rezai	2007/0191912 A1	8/2007	Ficher et al.
2002/0183607 A1	12/2002	Bauch et al.	2007/0197891 A1	8/2007	Shachar et al.
2002/0183740 A1	12/2002	Edwards et al.	2007/0203450 A1	8/2007	Berry
2002/0183817 A1	12/2002	Van Venrooij et al.	2007/0203532 A1	8/2007	Tass et al.
2003/0097159 A1	5/2003	Schiff et al.	2007/0203537 A1	8/2007	Goetz et al.
2003/0149450 A1	8/2003	Mayberg	2007/0203538 A1	8/2007	Stone et al.
2003/0171791 A1	9/2003	KenKnight et al.	2007/0203539 A1	8/2007	Stone et al.
2003/0212439 A1	11/2003	Schuler et al.	2007/0203540 A1	8/2007	Goetz et al.
2004/0034394 A1	2/2004	Woods et al.	2007/0203541 A1	8/2007	Goetz et al.
2004/0044279 A1	3/2004	Lewin et al.	2007/0203543 A1	8/2007	Stone et al.
2004/0044378 A1	3/2004	Holsheimer	2007/0203544 A1	8/2007	Goetz et al.
2004/0044379 A1	3/2004	Holsheimer	2007/0203545 A1	8/2007	Stone et al.
2004/0054297 A1	3/2004	Wingeier et al.	2007/0203546 A1	8/2007	Stone et al.
2004/0059395 A1	3/2004	North et al.	2007/0213789 A1	9/2007	Nolan et al.
2004/0106916 A1	6/2004	Quaid et al.	2007/0213790 A1	9/2007	Nolan et al.
2004/0133248 A1	7/2004	Frei et al.	2007/0244519 A1	10/2007	Keacher et al.
2004/0152957 A1	8/2004	Stivoric et al.	2007/0245318 A1	10/2007	Goetz et al.
2004/0181262 A1	9/2004	Bauhahn	2007/0255321 A1	11/2007	Gerber et al.
2004/0186532 A1	9/2004	Tadlock	2007/0255322 A1	11/2007	Gerber et al.
2004/0193231 A1	9/2004	David et al.	2007/0260283 A1	11/2007	Li
2004/0199216 A1	10/2004	Lee et al.	2007/0265664 A1	11/2007	Gerber et al.
2004/0267330 A1	12/2004	Lee et al.	2007/0276441 A1	11/2007	Goetz
2005/0003396 A1 *	1/2005	Ozkan C12Q 1/6825 435/7.1	2007/0282189 A1	12/2007	Dan et al.
2005/0021090 A1	1/2005	Schuler et al.	2007/0288064 A1	12/2007	Butson et al.
2005/0033380 A1	2/2005	Tanner et al.	2008/0027514 A1	1/2008	DeMulling et al.
			2008/0039895 A1	2/2008	Fowler et al.
			2008/0046037 A1	2/2008	Haubrich et al.
			2008/0071150 A1	3/2008	Miesel et al.
			2008/0081982 A1	4/2008	Simon et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0086451	A1	4/2008	Torres et al.	2010/0268298	A1	10/2010	Moffitt
2008/0091248	A1	4/2008	Libbus et al.	2010/0324410	A1	12/2010	Paek et al.
2008/0103533	A1	5/2008	Patel et al.	2010/0331883	A1	12/2010	Schmitz et al.
2008/0114233	A1	5/2008	McIntyre et al.	2011/0004267	A1	1/2011	Meadows
2008/0114579	A1	5/2008	McIntyre et al.	2011/0005069	A1	1/2011	Pianca
2008/0123922	A1	5/2008	Gielen et al.	2011/0040351	A1	2/2011	Buston et al.
2008/0123923	A1	5/2008	Gielen et al.	2011/0054559	A1	3/2011	Rosenberg et al.
2008/0133141	A1	6/2008	Frost	2011/0066407	A1	3/2011	Butson et al.
2008/0141217	A1	6/2008	Goetz et al.	2011/0078900	A1	4/2011	Pianca et al.
2008/0154340	A1	6/2008	Goetz et al.	2011/0093045	A1	4/2011	Moffitt
2008/0154341	A1	6/2008	McIntyre et al.	2011/0130803	A1	6/2011	McDonald
2008/0163097	A1	7/2008	Goetz et al.	2011/0130816	A1	6/2011	Howard et al.
2008/0183256	A1	7/2008	Keacher	2011/0130817	A1	6/2011	Chen
2008/0188734	A1	8/2008	Suryanarayanan et al.	2011/0130818	A1	6/2011	Chen
2008/0215101	A1	9/2008	Rezai et al.	2011/0137372	A1	6/2011	Makous et al.
2008/0215118	A1	9/2008	Goetz et al.	2011/0160796	A1	6/2011	Lane et al.
2008/0227139	A1	9/2008	Deisseroth et al.	2011/0172737	A1	7/2011	Davis et al.
2008/0238749	A1	10/2008	Comdorf	2011/0184487	A1	7/2011	Alberts et al.
2008/0242950	A1	10/2008	Jung et al.	2011/0191275	A1	8/2011	Lujan et al.
2008/0261165	A1	10/2008	Steingart et al.	2011/0196253	A1	8/2011	McIntyre et al.
2008/0269588	A1	10/2008	Csavoy et al.	2011/0213440	A1	9/2011	Fowler et al.
2008/0300654	A1	12/2008	Lambert et al.	2011/0224665	A1	9/2011	Crosby et al.
2008/0300797	A1	12/2008	Tabibiazar et al.	2011/0238129	A1	9/2011	Moffitt
2009/0016491	A1	1/2009	Li	2011/0251583	A1	10/2011	Miyazawa et al.
2009/0054947	A1	2/2009	Bourn et al.	2011/0270348	A1	11/2011	Goetz
2009/0054950	A1	2/2009	Stephens	2011/0306845	A1	12/2011	Osorio
2009/0082640	A1	3/2009	Kovach et al.	2011/0306846	A1	12/2011	Osorio
2009/0082829	A1	3/2009	Panken et al.	2011/0307032	A1	12/2011	Goetz et al.
2009/0112289	A1	4/2009	Lee et al.	2011/0313485	A1	12/2011	DeMulling et al.
2009/0118635	A1	5/2009	Lujan et al.	2011/0313500	A1	12/2011	Barker et al.
2009/0118786	A1	5/2009	Meadows et al.	2012/0016378	A1	1/2012	Pianca et al.
2009/0149917	A1	6/2009	Whitehurst et al.	2012/0027272	A1	2/2012	Akinyemi et al.
2009/0163975	A1	6/2009	Gerber et al.	2012/0046710	A1	2/2012	Digiore et al.
2009/0187222	A1	7/2009	Barker	2012/0046715	A1	2/2012	Moffitt et al.
2009/0196471	A1	8/2009	Goetz et al.	2012/0071949	A1	3/2012	Pianca et al.
2009/0196472	A1	8/2009	Goetz et al.	2012/0078106	A1	3/2012	Dentinger et al.
2009/0198306	A1	8/2009	Goetz et al.	2012/0089205	A1	4/2012	Boyden et al.
2009/0198354	A1	8/2009	Wilson	2012/0101552	A1	4/2012	Lazarewicz et al.
2009/0204192	A1	8/2009	Carlton et al.	2012/0116476	A1	5/2012	Kothandaraman
2009/0208073	A1	8/2009	McIntyre et al.	2012/0165898	A1	6/2012	Moffitt
2009/0210208	A1	8/2009	McIntyre et al.	2012/0165901	A1	6/2012	Zhu et al.
2009/0228073	A1	9/2009	Scholten	2012/0165911	A1	6/2012	Pianca
2009/0242399	A1	10/2009	Kamath et al.	2012/0197375	A1	8/2012	Pianca et al.
2009/0270949	A1	10/2009	Kalpin et al.	2012/0203316	A1	8/2012	Moffitt et al.
2009/0276008	A1	11/2009	Lee et al.	2012/0203320	A1	8/2012	Digiore et al.
2009/0276021	A1	11/2009	Meadows et al.	2012/0203321	A1	8/2012	Moffitt et al.
2009/0281595	A1	11/2009	King et al.	2012/0207378	A1	8/2012	Gupta et al.
2009/0281596	A1	11/2009	King et al.	2012/0226138	A1	9/2012	DeSalles et al.
2009/0287271	A1	11/2009	Blum et al.	2012/0229468	A1	9/2012	Lee et al.
2009/0287272	A1	11/2009	Kokones et al.	2012/0239109	A1	9/2012	Lee
2009/0287273	A1	11/2009	Carlton et al.	2012/0239115	A1	9/2012	Lee
2009/0287467	A1	11/2009	Sparks et al.	2012/0265103	A1	10/2012	Pollicker et al.
2009/0299164	A1	12/2009	Singhal et al.	2012/0265262	A1	10/2012	Osorio
2009/0299165	A1	12/2009	Singhal et al.	2012/0265268	A1	10/2012	Blum et al.
2009/0299380	A1	12/2009	Singhal et al.	2012/0271189	A1	10/2012	Nelson et al.
2010/0010387	A1	1/2010	Skelton et al.	2012/0277833	A1	11/2012	Gerber et al.
2010/0010432	A1	1/2010	Skelton	2012/0296396	A1*	11/2012	Moffitt G16H 20/30 607/59
2010/0010566	A1	1/2010	Thacker et al.	2012/0302912	A1	11/2012	Moffitt et al.
2010/0010646	A1	1/2010	Drew et al.	2012/0303087	A1	11/2012	Moffitt et al.
2010/0023103	A1	1/2010	Elborno	2012/0303098	A1	11/2012	Perryman
2010/0023130	A1	1/2010	Henry et al.	2012/0314919	A1	12/2012	Sparks et al.
2010/0030312	A1	2/2010	Shen	2012/0314924	A1	12/2012	Carlton et al.
2010/0049276	A1	2/2010	Blum et al.	2012/0316615	A1	12/2012	Digiore et al.
2010/0049280	A1	2/2010	Goetz	2012/0316619	A1	12/2012	Goetz et al.
2010/0057161	A1	3/2010	Machado et al.	2012/0330374	A1	12/2012	Blum et al.
2010/0064249	A1	3/2010	Groetken	2012/0330622	A1	12/2012	Butson et al.
2010/0076535	A1	3/2010	Pianca et al.	2013/0035740	A1	2/2013	Sharma et al.
2010/0113959	A1	5/2010	Pascual-Leon et al.	2013/0039550	A1	2/2013	Blum et al.
2010/0121409	A1	5/2010	Kothandaraman et al.	2013/0053926	A1	2/2013	Hincapie Ordonez et al.
2010/0135553	A1	6/2010	Joglekar	2013/0060305	A1	3/2013	Bokil
2010/0137944	A1	6/2010	Zhu	2013/0105071	A1	5/2013	Digiore et al.
2010/0152604	A1	6/2010	Kuala et al.	2013/0116744	A1	5/2013	Blum et al.
2010/0152807	A1	6/2010	Grill et al.	2013/0116748	A1	5/2013	Bokil et al.
2010/0179562	A1	7/2010	Linker et al.	2013/0116749	A1	5/2013	Carlton et al.
2010/0211135	A1	8/2010	Caparso et al.	2013/0116929	A1	5/2013	Carlton et al.
				2013/0150922	A1	6/2013	Butson et al.
				2013/0197424	A1	8/2013	Bedenbaugh
				2013/0197602	A1	8/2013	Pianca et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0226261	A1	8/2013	Sparks et al.	2018/0214700	A1	8/2018	Vansickle et al.
2013/0245722	A1	9/2013	Ternes et al.	2018/0264278	A1	9/2018	Laghi
2013/0261684	A1	10/2013	Howard	2018/0272142	A1	9/2018	Zhang et al.
2013/0289380	A1	10/2013	Molnar et al.	2018/0280698	A1	10/2018	Steinke et al.
2013/0289660	A1	10/2013	Molnar et al.	2018/0296828	A1	10/2018	Bradley et al.
2013/0317572	A1	11/2013	Zhu et al.	2018/0369589	A1	12/2018	Schouenborg
2013/0317573	A1	11/2013	Zhu et al.	2018/0369606	A1	12/2018	Zhang et al.
2013/0317587	A1	11/2013	Barker	2018/0369607	A1	12/2018	Zhang et al.
2013/0325091	A1	12/2013	Pianca et al.	2019/0015660	A1	1/2019	Zhang et al.
2014/0039587	A1	2/2014	Romero	2019/0184171	A1	6/2019	Mustakos et al.
2014/0063017	A1	3/2014	Kaula et al.	2019/0209834	A1	7/2019	Zhang et al.
2014/0066999	A1	3/2014	Carcieri et al.	2019/0209849	A1	7/2019	Hershey et al.
2014/0067018	A1	3/2014	Carcieri et al.	2019/0262609	A1	8/2019	Brill et al.
2014/0067022	A1	3/2014	Carcieri et al.	2019/0275331	A1	9/2019	Zhu
2014/0074180	A1	3/2014	Heldman et al.	2019/0329047	A1	10/2019	Moffitt et al.
2014/0107731	A1	4/2014	Stone et al.	2019/0329049	A1	10/2019	Carcieri et al.
2014/0122379	A1	5/2014	Moffitt et al.	2020/0094047	A1	3/2020	Govea et al.
2014/0200633	A1	7/2014	Moffitt	2020/0139127	A1	5/2020	Zhang et al.
2014/0243926	A1	8/2014	Carcieri	2020/0155854	A1	5/2020	Leven et al.
2014/0276707	A1	9/2014	Jaax	2020/0155859	A1	5/2020	Blum et al.
2014/0277282	A1	9/2014	Jaax	2020/0171298	A1	6/2020	Goetz et al.
2014/0277284	A1	9/2014	Chen et al.	2020/0171310	A1	6/2020	Walter et al.
2014/0296953	A1	10/2014	Pianca et al.	2020/0179600	A1	6/2020	Zanos et al.
2014/0343647	A1	11/2014	Romero et al.	2020/0222704	A1	7/2020	Moffitt et al.
2014/0353001	A1	12/2014	Romero et al.	2020/0269053	A1	8/2020	Park
2014/0358207	A1	12/2014	Romero	2020/0353254	A1	11/2020	O Laighin et al.
2014/0358208	A1	12/2014	Howard et al.	2020/0376262	A1	12/2020	Clark et al.
2014/0358209	A1	12/2014	Romero et al.	2020/0376263	A1	12/2020	Zhu
2014/0358210	A1	12/2014	Howard et al.	2020/0398057	A1	12/2020	Esteller et al.
2015/0018915	A1	1/2015	Leven	2021/0008388	A1	1/2021	Vansickle et al.
2015/0021817	A1	1/2015	Romero et al.	2021/0008389	A1	1/2021	Featherstone et al.
2015/0045864	A1	2/2015	Howard	2021/0016111	A1	1/2021	Vansickle et al.
2015/0051681	A1	2/2015	Hershey	2021/0023374	A1	1/2021	Block et al.
2015/0066111	A1	3/2015	Blum et al.	2021/0052893	A1	2/2021	Suri et al.
2015/0066120	A1	3/2015	Govea	2021/0106830	A1*	4/2021	Provenza A61B 5/37
2015/0134031	A1	5/2015	Moffitt et al.	2021/0113844	A1	4/2021	Zhang et al.
2015/0151113	A1	6/2015	Govea et al.	2021/0128920	A1	5/2021	Grill et al.
2015/0246231	A1	9/2015	Martens et al.	2021/0196956	A1	7/2021	Juárez Paz
2015/0360039	A1	12/2015	Lempka et al.	2021/0196964	A1	7/2021	Schnell et al.
2016/0001087	A1	1/2016	Moffitt	2021/0205613	A1	7/2021	Bradley et al.
2016/0022995	A1	1/2016	Kothandaraman et al.	2021/0268268	A1	9/2021	Horn et al.
2016/0023008	A1	1/2016	Kothandaraman	2021/0275820	A1	9/2021	Grill, Jr. et al.
2016/0030749	A1	2/2016	Carcieri et al.	2021/0387002	A1	12/2021	Bourget et al.
2016/0030750	A1	2/2016	Bokil et al.	2022/0007980	A1	1/2022	Single
2016/0045748	A1	2/2016	Astrom et al.	2022/0008729	A1	1/2022	Zhu
2016/0082252	A1	3/2016	Hershey et al.	2022/0040485	A1	2/2022	Li et al.
2016/0096025	A1	4/2016	Moffitt et al.	2022/0062640	A1	3/2022	Raïke et al.
2016/0136429	A1	5/2016	Massoumi et al.	2022/0072329	A1	3/2022	Howard
2016/0136443	A1	5/2016	Kothandaraman et al.	2022/0126100	A1	4/2022	Jackson et al.
2016/0144186	A1	5/2016	Kaemmerer et al.	2022/0257950	A1	8/2022	Moore et al.
2016/0175594	A1	6/2016	Min et al.	2022/0266026	A1	8/2022	Case et al.
2016/0206380	A1	7/2016	Sparks et al.	2022/0296892	A1	9/2022	Esteller et al.
2016/0228692	A1	8/2016	Steinke et al.	2022/0296893	A1	9/2022	Steinke et al.
2016/0256691	A1	9/2016	Cecchi et al.	2022/0339448	A1	10/2022	Jayakumar et al.
2016/0256693	A1	9/2016	Parramon	2022/0347479	A1	11/2022	Esteller et al.
2016/0346557	A1	12/2016	Bokil	2022/0355114	A1	11/2022	Moore et al.
2016/0375248	A1	12/2016	Carcieri et al.	2022/0355115	A1	11/2022	Moore et al.
2016/0375258	A1	12/2016	Steinke	2022/0370808	A1	11/2022	Esteller
2017/0100593	A1	4/2017	Zottola	2022/0387785	A1	12/2022	Huynh et al.
2017/0100601	A1	4/2017	Xiao et al.	2022/0395690	A1	12/2022	Haddock et al.
2017/0106197	A1	4/2017	Wechter et al.	2023/0048571	A1	2/2023	Poltorak
2017/0197086	A1	7/2017	Howard et al.	2023/0064552	A1	3/2023	Moffitt
2017/0225007	A1	8/2017	Orinski	2023/0141183	A1	5/2023	Moore et al.
2017/0252570	A1	9/2017	Serrano Carmona et al.	2023/0181089	A1	6/2023	Zhang et al.
2017/0259078	A1	9/2017	Howard	2023/0181090	A1	6/2023	Juarez Paz
2017/0304610	A1	10/2017	Huibregtse et al.	2023/0181906	A1	6/2023	Moore et al.
2017/0304633	A1	10/2017	Zhang	2023/0248977	A1	8/2023	Esteller et al.
2017/0372039	A1	12/2017	Mustakos et al.	2023/0264025	A1	8/2023	Malekmohammadi et al.
2018/0064930	A1	3/2018	Zhang et al.	2023/0271015	A1	8/2023	Malekmohammadi et al.
2018/0078776	A1	3/2018	Mustakos et al.	2023/0277854	A1	9/2023	Gaviao Kilmar
2018/0104482	A1	4/2018	Bokil	2024/0065620	A1	2/2024	Moore et al.
2018/0104500	A1	4/2018	Blum et al.	2024/0157151	A1	5/2024	Juarez Paz
2018/0110971	A1	4/2018	Serrano Carmona	2024/0198110	A1	6/2024	Moore
2018/0185650	A1	7/2018	Shah	2024/0316346	A1	9/2024	Shah et al.
2018/0193655	A1	7/2018	Zhang et al.				

FOREIGN PATENT DOCUMENTS

EP	1166819	1/2002
EP	1372780	1/2004

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1559369	8/2005
WO	97/39797	10/1997
WO	98/48880	11/1998
WO	01/90876	11/2001
WO	02/26314	4/2002
WO	02/28473	4/2002
WO	02/065896	8/2002
WO	02/072192	9/2002
WO	03/086185	10/2003
WO	2004/019799 A2	3/2004
WO	2004/041080	5/2005
WO	2006/017053	2/2006
WO	2006/113305	10/2006
WO	2007/1097859	8/2007
WO	2007/1097861 A1	8/2007
WO	2007/100427	9/2007
WO	2007/100428	9/2007
WO	2007/112061	10/2007
WO	2009/097224	8/2009
WO	2010/109448	9/2010
WO	2010/120823 A2	10/2010
WO	2011/025865	3/2011
WO	2011/139779 A1	11/2011
WO	2011/159688 A2	12/2011
WO	2012/088482	6/2012
WO	2014/076698	5/2014
WO	2016/025913	2/2016
WO	2016/081099	5/2016
WO	2016/112398	7/2016

OTHER PUBLICATIONS

Mcintyre, Cameron C., et al., "Electric field generated by deep brain stimulation of the subthalamic nucleus," Biomedical Engineering Society Annual Meeting, Nashville TN (Oct. 2003), 16 pages.

Mcintyre, Cameron C., et al., "Excitation of central nervous system neurons by nonuniform electric fields," Biophys. J., 76(2) (1999), pp. 878-888.

McNeal, DR., et al., "Analysis of a model for excitation of myelinated nerve," IEEE Trans Biomed Eng., vol. 23 (1976), pp. 329-337.

Micheli-Tzanakou, E., et al., "Computational Intelligence for target assesment in Parkinson's disease," Proceedings of SPIE vol. 4479, Applications and Science of Neural Networks, Fuzzy Systems, and Evolutionary Computation IV (2001), pp. 54-69.

Miocinovic, S., et al., "Computational analysis of subthalamic nucleus and lenticular fasciculus activation during therapeutic deep brain stimulation," J Neurophysiol., 96(3) (Sep. 2006), pp. 1569-1580.

Miranda, P. C., et al., "The distribution of currents induced in the brain by Magnetic Stimulation: a finite element analysis incorporating OT-MRI-derived conductivity data," Proc. Intl. Soc. Mag. Reson. Med. 9 (2001), p. 1540.

Miranda, P. C., et al., "The Electric Field Induced in the Brain by Magnetic Stimulation: A 3-D Finite-Element Analysis of the Effect of Tissue Heterogeneity and Anisotropy," IEEE Transactions on Biomedical Engineering, 50(9) (Sep. 2003), pp. 1074-1085.

Moffitt, MA., et al., "Prediction of myelinated nerve fiber stimulation thresholds: limitations of linear models," IEEE Transactions on Biomedical Engineering, 51 (2) (2003), pp. 229-236.

Moro, E., et al., "The impact on Parkinson's disease of electrical parameter settings in STN stimulation," Neurology, 59(5) (Sep. 10, 2002), pp. 706-713.

Nowak, LG., et al., "Axons, but not cell bodies, are activated by electrical stimulation in cortical gray matter. I. Evidence from chronaxie measurements," Exp. Brain Res., 118(4) (Feb. 1998), pp. 477-488.

Nowak, LG., et al., "Axons, but not cell bodies, are activated by electrical stimulation in cortical gray matter. II. Evidence from selective inactivation of cell bodies and axon initial segments," Exp. Brain Res., 118(4) (Feb. 1998), pp. 489-500.

O'Suilleabhain, PE., et al., "Tremor response to polarity, voltage, pulsewidth and frequency of thalamic stimulation," Neurology, 60(5) (Mar. 11, 2003), pp. 786-790.

Pierpaoli, C., et al., "Toward a quantitative assessment of diffusion anisotropy," Magn Reson Med., 36(6) (Dec. 1996), pp. 893-906.

Plonsey, R., et al., "Considerations of quasi-stationarity in electrophysiological systems," Bull Math Biophys., 29(4) (Dec. 1967), pp. 657-664.

Ranck, J B., "Specific impedance of rabbit cerebral cortex," Exp. Neurol., vol. 7 (Feb. 1963), pp. 144-152.

Ranck, J B., et al., "The Specific impedance of the dorsal columns of the cat: an anisotropic medium," Exp. Neurol., 11 (Apr. 1965), pp. 451-463.

Ranck, J B., "Which elements are excited in electrical stimulation of mammalian central nervous system: a review," Brain Res., 98(3) (Nov. 21, 1975), pp. 417-440.

Rattay, F., et al., "A model of the electrically excited human cochlear neuron. I. Contribution of neural substructures to the generation and propagation of spikes," Hear Res., 153(1-2) (Mar. 2001), pp. 43-63.

Rattay, F., "A model of the electrically excited human cochlear neuron. II. Influence of the three-dimensional cochlear structure on neural excitability," Hear Res., 153(1-2) (Mar. 2001), pp. 64-79.

Rattay, F., "Arrival at Functional Electrostimulation by modelling of fiber excitation," Proceedings of the Ninth annual Conference of the IEEE Engineering in Medicine and Biology Society (1987), pp. 1459-1460.

Rattay, F., "The influence of intrinsic noise can preserve the temporal fine structure of speech signals in models of electrically stimulated human cochlear neurones," Journal of Physiology, Scientific Meeting of the Physiological Society, London, England, UK Apr. 19-21, 1999 (Jul. 1999), p. 170P.

Rizzone, M., et al., "Deep brain stimulation of the subthalamic nucleus in Parkinson's disease: effects of variation in stimulation parameters," J. Neurol. Neurosurg. Psychiatry., 71(2) (Aug. 2001), pp. 215-219.

Saint-Cyr, J. A., et al., "Localization of clinically effective stimulating electrodes in the human subthalamic nucleus on magnetic resonance imaging," J. Neurosurg., 87(5) (Nov. 2002), pp. 1152-1166.

Sances, A., et al., "In Electroanesthesia: Biomedical and Biophysical Studies," A Sances and SJ Larson, Eds., Academic Press, NY (1975), pp. 114-124.

Si. Jean, P., et al., "Automated atlas integration and interactive three-dimensional visualization tools for planning and guidance in functional neurosurgery," IEEE Transactions on Medical Imaging, 17(5) (1998), pp. 672-680.

Starr, P. A., et al., "Implantation of deep brain stimulators into the subthalamic nucleus: technical approach and magnetic resonance imaging-verified lead locations," J. Neurosurg., 97(2) (Aug. 2002), pp. 370-387.

Sterio, D., et al., "Neurophysiological refinement of subthalamic nucleus targeting," Neurosurgery, 50(1) (Jan. 2002), pp. 58-69.

Struijk, J. J., et al., "Excitation of dorsal root fibers in spinal cord stimulation: a theoretical study," IEEE Transactions on Biomedical Engineering, 40(7) (Jul. 1993), pp. 632-639.

Struijk, J J., et al., "Recruitment of dorsal column fibers in spinal cord stimulation: influence of collateral branching," IEEE Transactions on Biomedical Engineering, 39(9) (Sep. 1992), pp. 903-912.

Tamma, F., et al., "Anatomo-clinical correlation of intraoperative stimulation-induced side effects during HF-DBS of the subthalamic nucleus," Neurol Sci., vol. 23 (Suppl 2) (2002), pp. 109-110.

Tarler, M., et al., "Comparison between monopolar and tripolar configurations in chronically implanted nerve cuff electrodes," IEEE 17th Annual Conference Engineering in Medicine and Biology Society, vol. 2 (1995), pp. 1093-1109.

Testerman, Roy L., "Cortical response to callosal stimulation: A model for determining safe and efficient stimulus parameters," Annals of Biomedical Engineering, 6(4) (1978), pp. 438-452.

Tuch, D.S., et al., "Conductivity mapping of biological tissue using diffusion MRI," Ann NY Acad Sci., 888 (Oct. 30, 1999), pp. 314-316.

(56)

References Cited**OTHER PUBLICATIONS**

- Tuch, D.S., et al., "Conductivity tensor mapping of the human brain using diffusion tensor MRI," *Proc Natl Acad Sci USA*, 98(20) (Sep. 25, 2001), pp. 11697-11701.
- Veraart, C., et al., "Selective control of muscle activation with a multipolar nerve cuff electrode," *IEEE Transactions on Biomedical Engineering*, 40(7) (Jul. 1993), pp. 640-653.
- Vercueil, L., et al., "Deep brain stimulation in the treatment of severe dystonia," *J. Neurol.*, 248(8) (Aug. 2001), pp. 695-700.
- Vilalte, "Circuit Design of the Power-on-Reset," Apr. 2000, pp. 1-25.
- Vitek, J. L., "Mechanisms of deep brain stimulation: excitation or inhibition," *Mov. Disord.*, vol. 17 (Suppl. 3) (2002), pp. 69-72.
- Voges, J., et al., "Bilateral high-frequency stimulation in the subthalamic nucleus for the treatment of Parkinson disease: correlation of therapeutic effect with anatomical electrode position," *J. Neurosurg.*, 96(2) (Feb. 2002), pp. 269-279.
- Wakana, S., et al., "Fiber tract-based atlas of human white matter anatomy," *Radiology*, 230(1) (Jan. 2004), pp. 77-87.
- Alexander, DC., et al., "Spatial transformations of diffusion tensor magnetic resonance images," *IEEE Transactions on Medical Imaging*, 20 (11), (2001), pp. 1131-1139.
- Wu, Y. R., et al., "Does Stimulation of the GPi control dyskinesia by activating inhibitory axons?," *Mov. Disord.*, vol. 16 (2001), pp. 208-216.
- Yelnik, J., et al., "Localization of stimulating electrodes in patients with Parkinson disease by using a three-dimensional atlas-magnetic resonance imaging coregistration method," *J. Neurosurg.*, 99(1) (Jul. 2003), pp. 89-99.
- Yianni, John, et al., "Globus pallidus internus deep brain stimulation for dystonic conditions: a prospective audit," *Mov. Disord.*, vol. 18 (2003), pp. 436-442.
- Zonenshayn, M., et al., "Comparison of anatomic and neurophysiological methods for subthalamic nucleus targeting," *Neurosurgery*, 47(2) (Aug. 2000), pp. 282-294.
- Voghell et al., "Programmable Current Source Dedicated to Implantable Microstimulators" ICM '98 Proceedings of the Tenth International Conference, pp. 67-70.
- Butson, Christopher R., et al., "Patient-specific analysis of the volume of tissue activated during deep brain stimulation," *NeuroImage*, vol. 34. (2007), 661-670.
- Adler, DE., et al., "The tentorial notch: anatomical variation, morphometric analysis, and classification in 100 human autopsy cases," *J. Neurosurg.*, 96(6), (Jun. 2002), pp. 1103-1112.
- Jones et al., "An Advanced Demultiplexing System for Physiological Stimulation", *IEEE Transactions on Biomedical Engineering*, vol. 44 No. 12 Dec. 1997, pp. 1210-1220.
- McIntyre, Cameron, et al., "Finite element analysis of the current-density and electric field generated by metal microelectrodes", *Ann Biomed Eng.* 29(3), (2001), 227-235.
- Foster, K. R., et al., "Dielectric properties of tissues and biological materials: a critical review," *Grit Rev Biomed Eng.* 17(1). {1989}, 25-104.
- Limousin, P., et al., "Electrical stimulation of the subthalamic nucleus in advanced Parkinson's disease", *N Engl J Med.* 339(16), (Oct. 15, 1998), 1105-11.
- Kitagawa, M., et al., "Two-year follow-up of chronic stimulation of the posterior subthalamic white matter for tremor-dominant Parkinson's disease," *Neurosurgery*, 56(2). (Feb. 2005), 281-9.
- Johnson, M. D., et al., "Repeated voltage biasing improves unit recordings by reducing resistive tissue impedances", *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, [see also *IEEE Trans. on Rehabilitation Engineering* (2005)], 160-165.
- Holsheimer, J., et al., "Chronaxie calculated from current-duration and voltage-duration data", *J. Neurosci. Methods*, 97(1). (Apr. 1, 2000), 45-50.
- Hines, M. L., et al., "The Neuron simulation environment", *Neural Comput.* 9(6). (Aug. 15, 1997), 1179-209.
- Herzog, J., et al., "Most effective stimulation site in subthalamic deep brain stimulation for Parkinson's disease", *Mov. Disord.* 19(9). (Sep. 2004), 1050-4.
- Hershey, T., et al., "Cortical and subcortical blood flow effects of subthalamic nucleus stimulation in PD," *Neurology* 61(6). (Sep. 23, 2003), 816-21.
- Hemm, S., et al., "Evolution of Brain Impedance in Dystonic Patients Treated by GPi Electrical Stimulation", *Neuromodulation* 7(2) (Apr. 2004), 67-75.
- Hemm, S., et al., "Deep brain stimulation in movement disorders: stereotactic coregistration of two-dimensional electrical field modeling and magnetic resonance imaging," *J. Neurosurg.* 103(6): (Dec. 2005), 949-55.
- Haueisen, J., et al., "The influence of brain tissue anisotropy on human EEG and MEG", *Neuroimage* 15(1) (Jan. 2002), 159-166.
- Haslinger, B., et al., "Frequency-correlated decreases of motor cortex activity associated with subthalamic nucleus stimulation in Parkinson's disease," *Neuroimage* 28(3). (Nov. 15, 2005), 598-606.
- Hashimoto, T., et al., "Stimulation of the subthalamic nucleus changes the firing pattern of pallidal neurons", *J. Neurosci.* 23(5). (Mar. 1, 2003), 1916-23.
- Hardman, C. D., et al., "Comparison of the basal ganglia in rats, marmosets, macaques, baboons, and humans: volume and neuronal number for the output, internal relay, and striatal modulating nuclei", *J. Comp. Neurol.*, 445(3). (Apr. 8, 2002), 238-55.
- McNaughtan et al., "Electrochemical Issues in Impedance Tomography", 1st World Congress on Industrial Process Tomography, Buxton, Greater Manchester, Apr. 14-17, 1999.
- Grill, Wm., et al., "Electrical properties of implant encapsulation tissue", *Ann Biomed Eng.* vol. 22. (1994), 23-33.
- Grill, W. M., et al., "Deep brain stimulation creates an informational lesion of the stimulated nucleus", *Neuroreport*, 1517t (May 19, 2004), 1137-40.
- International Search Report and Written Opinion for PCT Application No. PCT/US2022/033226 mailed Sep. 20, 2022.
- Pulliam CL, Heldman DA, Orcutt TH, Mera TO, Giuffrida JP, Vitek JL. Motion sensor strategies for automated optimization of deep brain stimulation in Parkinson's disease. *Parkinsonism Relat Disord.* Apr. 2015; 21(4):378-82.
- Benoit M. Dawant et al: "The VU-DBS project: integrated and computer-assisted planning, intra-operative placement, and post-operative programming of deep-brain stimulators", *Proceedings of SPIE*, vol. 6509, Mar. 6, 2007 (Mar. 6, 2007), 11 pages.
- Nowinski, W. L., et al., "Statistical analysis of 168 bilateral subthalamic nucleus implantations by means of the probabilistic functional atlas," *Neurosurgery* 57(4 Suppl) (Oct. 2005), 319-30.
- Obeso, J. A., et al., "Deep-brain stimulation of the subthalamic nucleus or the pars interna of the globus pallidus in Parkinson's disease," *N Engl J Med.*, 345{131. The Deep-Brain Stimulation for Parkinson's Disease Study Group, (Sep. 27, 2001), 956-63.
- Butson et al., "Current Steering to control the volume of tissue activated during deep brain stimulation," vol. 1, No. 1, Dec. 3, 2007, pp. 7-15.
- Patrick, S. K., et al., "Quantification of the UPDRS rigidity scale", *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, [see also *IEEE Trans. on Rehabilitation Engineering* 9(1). (2001), 31-41.
- Phillips, M. D., et al., "Parkinson disease: pattern of functional MR imaging activation during deep brain stimulation of subthalamic nucleus-initial experience", *Radiology* 239(1). (Apr. 2006), 209-16.
- Ericsson, A. et al., "Construction of a patient-specific atlas of the brain: Application to normal aging," *Biomedical Imaging: From Nano to Macro*, ISBI 2008, 5th IEEE International Symposium, May 14, 2008, pp. 480-483.
- Kaikai Shen et al., "Atlas selection strategy using least angle regression in multi-atlas segmentation propagation," *Biomedical Imaging: From Nano to Macro*, 2011, 8th IEEE International Symposium, ISBI 2011, Mar. 30, 2011, pp. 1746-1749.
- Liliane Ramus et al., "Assessing selection methods in the context of multi-atlas based segmentation," *Biomedical Imaging: From Nano to Macro*, 2010, IEEE International Symposium, Apr. 14, 2010, pp. 1321-1324.

(56)

References Cited

OTHER PUBLICATIONS

- Olivier Commowick et al., "Using Frankenstein's Creature Paradigm to Build a Patient Specific Atlas," Sep. 20, 2009, Medical Image Computing and Computer-Assisted Intervention, pp. 993-1000.
- Lotjonen J.M.P. et al., "Fast and robust multi-atlas segmentation of brain magnetic resonance images," NeuroImage, Academic Press, vol. 49, No. 3, Feb. 1, 2010, pp. 2352-2365.
- McIntyre, C. C., et al., "How does deep brain stimulation work? Present understanding and future questions," J Clin Neurophysiol. 21 (1). (Jan.-Feb. 2004),40-50.
- Sanchez Castro et al., "A cross validation study of deep brain stimulation targeting: From experts to Atlas-Based, Segmentation-Based and Automatic Registration Algorithms," IEEE Transactions on Medical Imaging, vol. 25, No. 11, Nov. 1, 2006, pp. 1440-1450.
- Plaha, P., et al., "Stimulation of the caudal zona incerta is superior to stimulation of the subthalamic nucleus in improving contralateral parkinsonism," Brain 129{Pt 7} (Jul. 2006), 1732-47.
- Rattay, F., "Analysis of models for external stimulation of axons", IEEE Trans. Biomed. Eng. vol. 33 (1986), 974-977.
- Rattay, F., "Analysis of the electrical excitation of CNS neurons", IEEE Transactions on Biomedical Engineering 45(6), (Jun. 1998),766-772.
- Rose, T. L., et al., "Electrical stimulation with Pt electrodes. VIII. Electrochemically safe charge injection limits with 0.2ms pulses [neuronal application]", IEEE Transactions on Biomedical Engineering, 37(11), (Nov. 1990), 1118-1120.
- Rubinstein, J. T., et al., "Signal coding in cochlear implants: exploiting stochastic effects of electrical stimulation", Ann Otol Rhinol Laryngol Suppl. 191, (Sep. 2003), 14-9.
- Schwan, H.P., et al., "The conductivity of living tissues," Ann NY Acad Sci., 65(6), (Aug. 1957),1007-13.
- Taylor, R. S., et al., "Spinal cord stimulation for chronic back and leg pain and failed back surgery syndrome: a systematic review and analysis of prognostic factors", Spine 30(1). (Jan. 1, 2005), 152-60.
- Siegel, Ralph M. et al., "Spatiotemporal dynamics of the functional architecture for gain fields in inferior parietal lobule of behaving monkey," Cerebral Cortex, New York, NY, vol. 17, No. 2, Feb. 2007, pp. 378-390.
- Klein, A. et al., "Evaluation of 14 nonlinear deformation algorithms applied to human brain MRI registration," NeuroImage, Academic Press, Orlando, FL, vol. 46, No. 3, Jul. 2009, pp. 786-802.
- Geddes, L. A., et al., "The specific resistance of biological material—a compendium of data for the biomedical engineer and physiologist," Med Biol Eng. 5(3), (May 1967),271-93.
- Gimsa, J., et al., "Choosing electrodes for deep brain stimulation experiments—electrochemical considerations," J Neurosci Methods, 142(2), (Mar. 30, 2005),251-65.
- Vidaillhet, M., et al., "Bilateral deep-brain stimulation of the globus pallidus in primary generalized dystonia", N Engl J Med. 352(5) (Feb. 3, 2005),459-67.
- Izad, Oliver, "Computationally Efficient Method in Predicating Axonal Excitation," Dissertation for Master Degree, Department of Biomedical Engineering, Case Western Reserve University, May 2009.
- Jaccard, Paul, "Elude comparative de la distribution florale dans une portion odes Aples et des Jura," Bulletin de la Societe Vaudoise des Sciences Naturelles (1901), 37:547-579.
- Dice, Lee R., "Measures of the Amount of Ecologic Association Between Species," Ecology 26(3) (1945): 297-302. doi: 10.2307/1932409, <http://jstor.org/stable/1932409>.
- Rand, W.M., "Objective criteria for the evaluation of clustering methods," Journal of the American Statistical Association (American Statistical Association) 66 (336) (1971): 846-850, doi:10.2307/2284239, <http://jstor.org/stable/2284239>.
- Hubert, Lawrence et al., "Comparing partitions," Journal of Classification 21(1) (1985): 193-218, doi:10.1007/BF01908075.
- Cover, T.M. et al., "Elements of information theory," (1991) John Wiley & Sons, New York, NY.
- Meila, Marina, "Comparing Clusterings by the Variation of Information," Learning Theory and Kernel Machines (2003): 173-187.
- Viola, P., et al., "Alignment by maximization of mutual information", International Journal of Computer Vision 24(2). (1997), 137-154.
- Butson et al. "StimExplorer: Deep Brain Stimulation Parameter Selection Software System," Acta Neurochirurgica, Jan. 1, 2007, vol. 97, No. 2, pp. 569-574.
- Butson et al. "Role of Electrode Design on the Volume of Tissue Activated During Deep Brain Stimulation," Journal of Neural Engineering, Mar. 1, 2006, vol. 3, No. 1, pp. 1-8.
- Volkman et al., Introduction to the Programming of Deep Brain Stimulators, Movement Disorders, vol. 17, Suppl. 3, pp. S181-S187 (2002).
- Miocinovic et al. "Cicerone: Stereotactic Neurophysiological Recording and Deep Brain Stimulation Electrode Placement Software System," Acta Neurochirurgica Suppl., Jan. 1, 2007, vol. 97, No. 2, pp. 561-567.
- Schmidt et al. "Sketching and Composing Widgets for 3D Manipulation," Eurographics, Apr. 2008, vol. 27, No. 2, pp. 301-310.
- Volkman, J., et al., "Basic algorithms for the programming of deep brain stimulation in Parkinson's disease", Mov Disord., 21 Suppl 14. (Jun. 2006),S284-9.
- Walter, B. L., et al., "Surgical treatment for Parkinson's disease", Lancet Neurol. 3(12). (Dec. 2004),719-28.
- Wei, X. F., et al., "Current density distributions, field distributions and impedance analysis of segmented deep brain stimulation electrodes", J Neural Eng. 2(4). (Dec. 2005), 139-47.
- Zonenshayn, M., et al., "Location of the active contact within the subthalamic nucleus (STN) in the treatment of idiopathic Parkinson's disease," Surg Neurol., 62(3) (Sep. 2004),216-25.
- Da Silva et al (A primer on diffusion tensor imaging of anatomical substructures. Neurosurg Focus 15(1): p. 1-4, Article 4, 2003.).
- Micheli-Tzanakou, E., et al., "Computational Intelligence for target assessment in Parkinson's disease", Proceedings of SPIE vol. 4479. Applications and Science of Neural Networks, Fuzzy Systems, and Evolutionary Computation IV,(2001),54-69.
- Grill, W. M., "Stimulus waveforms for selective neural stimulation", IEEE Engineering in Medicine and Biology Magazine, 14(4), (Jul.-Aug. 1995), 375-385.
- Miocinovic, S., et al., "Sensitivity of temporal excitation properties to the neuronal element activated by extracellular stimulation", J Neurosci Methods. 132(1). (Jan. 15, 2004), 91-9.
- Hunka, K. et al., Nursing Time to Program and Assess Deep Brain Stimulators in Movement Disorder Patients, J. Neurosci Nurs., 37: 204-10 (Aug. 2005).
- Moss, J., et al., "Electron microscopy of tissue adherent to explanted electrodes in dystonia and Parkinson's disease", Brain, 127{Pt 12}. (Dec. 2004),2755-63.
- Montgomery, E. B., et al., "Mechanisms of deep brain stimulation and future technical developments," Neurol Res. 22(3). (Apr. 2000),259-66.
- Merrill, D. R., et al., "Electrical stimulation of excitable tissue: design of efficacious and safe protocols", J Neurosci Methods. 141(2), (Feb. 15, 2005), 171-98.
- Fisekovic et al., "New Controller for Functional Electrical Stimulation Systems", Med. Eng. Phys. 2001; 23:391-399.
- Butson et al., "Tissue and Electrode Capacitance Reduce Neural Activation Volumes During Deep Brain Stimulation", Clinical Neurophysiology, 116:2490-2500, Oct. 2005.
- Butson et al., "Sources and Effects of Electrode Impedance During Deep Brain Stimulation", Clinical Neurophysiology, 117:447-454, Dec. 2005.
- D'Haese et al., "Computer-Aided Placement of Deep Brain Stimulators: From Planning to Intraoperative Guidance", IEEE Transactions on Medical Imaging, 24:1469-1478, Nov. 2005.
- Gross et al., "Electrophysiological Mapping for the Implantation of Deep Brain Stimulators for Parkinson's Disease and Tremor", Movement Disorders, 21 :S259-S283, Jun. 2006.
- Halpern et al., "Brain Shift During Deep Brain Stimulation Surgery for Parkinson's Disease", Stereotact Funct. Neurosurg., 86:37-43, published online Sep. 2007.

(56)

References Cited**OTHER PUBLICATIONS**

- Herzog et al., "Most Effective Stimulation Site in Subthalamic Deep Brain Stimulation for Parkinson's Disease", *Movement Disorders*, 19:1050-1099, published on line Mar. 2004.
- Jeon et al., "A Feasibility Study of Optical Coherence Tomography for Guiding Deep Brain Probes", *Journal of Neuroscience Methods*, 154:96-101, Jun. 2006.
- Khan et al., "Assessment of Brain Shift Related to Deep Brain Stimulation Surgery", *Stereotact Funct. Neurosurg.*, 86:44-53, published online Sep. 2007.
- Koop et al., "Improvement in a Quantitative Measure of Bradykinesia After Microelectrode Recording in Patients with Parkinson's Disease During Deep Brain Stimulation Surgery", *Movement Disorders*, 21 :673-678, published on line Jan. 2006.
- Lemaire et al., "Brain Mapping in Stereotactic Surgery: A Brief Overview from the Probabilistic Targeting to the Patient-Based Anatomic Mapping", *NeuroImage*, 37:S109-S115, available online Jun. 2007.
- Machado et al., "Deep Brain Stimulation for Parkinson's Disease: Surgical Technique and Perioperative Management", *Movement Disorders*, 21 :S247-S258, Jun. 2006.
- Maks et al., "Deep Brain Stimulation Activation Volumes and Their Association with Neurophysiological Mapping and Therapeutic Outcomes", Downloaded from jnnp.bmj.com, pp. 1-21, published online Apr. 2008.
- Moran et al., "Real-Time Refinement of Subthalamic Nucleus Targeting Using Bayesian Decision-Making on the Root Mean Square Measure", *Movement Disorders*, 21: 1425-1431, published online Jun. 2006.
- Sakamoto et al., "Homogeneous Fluorescence Assays for RNA Diagnosis by Pyrene-Conjugated 2'-O-Methyloligoribonucleotides", *Nucleosides, Nucleotides, and Nuclerics Acids*, 26:1659-1664, on line publication Oct. 2007.
- Winkler et al., "The First Evaluation of Brain Shift During Functional Neurosurgery by Deformation Field Analysis", *J. Neural. Neurosurg. Psychiatry*, 76:1161-1163, Aug. 2005.
- Yelnik et al., "A Three-Dimensional, Histological and Deformable Atlas of the Human Basal Ganglia. I. Atlas Construction Based on Immunohistochemical and MRI Data", *NeuroImage*, 34:618-638, Jan. 2007.
- Ward, H. E., et al., "Update on deep brain stimulation for neuropsychiatric disorders", *Neurobiol Dis* 38 (3) (2010), pp. 346-353.
- Alberts et al., "Bilateral subthalamic stimulation impairs cognitive-motor performance in Parkinson's disease patients." *Brain* (2008), 131, 3348-3360, Abstract.
- Butson, Christopher R., et al., "Sources and effects of electrode impedance during deep brain stimulation", *Clinical Neurophysiology*, vol. 117.(2006),447-454.
- An, et al., "Prefrontal cortical projections to longitudinal columns in the midbrain periaqueductal gray in macaque monkeys," *J Comp Neural* 401 (4) (1998), pp. 455-479.
- Bulson, C. R., et al., "Tissue and electrode capacitance reduce neural activation volumes during deep brain stimulation," *Clinical Neurophysiology*, vol. 116 (2005), pp. 2490-2500.
- Carmichael, S. T., et al., "Connectional networks within the orbital and medial prefrontal cortex of macaque monkeys," *J Comp Neural* 371 (2) (1996), pp. 179-207.
- Croxson, et al., "Quantitative investigation of connections of the prefrontal cortex in the human and macaque using probabilistic diffusion tractography," *J Neurosci* 25 (39) (2005), pp. 8854-8866.
- Frankemolle, et al., "Reversing cognitive-motor impairments in Parkinson's disease patients using a computational modelling approach to deep brain stimulation programming," *Brain* 133 (2010), pp. 746-761.
- Freedman, et al., "Subcortical projections of area 25 (subgenual cortex) of the macaque monkey," *J Comp Neurol* 421 (2) (2000), pp. 172-188.
- Giacobbe, et al., "Treatment resistant depression as a failure of brain homeostatic mechanisms: implications for deep brain stimulation," *Exp Neural* 219 (1) (2009), pp. 44-52.
- Goodman, et al., "Deep brain stimulation for intractable obsessive compulsive disorder: pilot study using a blinded, staggered-onset design," *Biol Psychiatry* 67 (6) (2010), pp. 535-542.
- Greenberg, et al., "Deep brain stimulation of the ventral internal capsule/ventral striatum for obsessive-compulsive disorder: worldwide experience," *Mol Psychiatry* 15 (1) (2010), pp. 64-79.
- Greenberg et al., "Three-year outcomes in deep brain stimulation for highly resistant obsessive-compulsive disorder," *Neuropsychopharmacology* 31 (11) (2006), pp. 2384-2393.
- Gutman, et al., "A tractography analysis of two deep brain stimulation white matter targets for depression," *Biol Psychiatry* 65 (4) (2009), pp. 276-282.
- Haber, et al., "Reward-related cortical inputs define a large striatal region in primates that interface with associative cortical connections, providing a substrate for incentive-based learning," *J Neurosci* 26 (32) (2006), pp. 8368-8376.
- Haber, et al., "Cognitive and limbic circuits that are affected by deep brain stimulation," *Front Biosci* 14 (2009), pp. 1823-1834.
- Hines, M. L., et al., "The Neuron simulation environment," *Neural Comput.*, 9(6) (Aug. 15, 1997), pp. 1179-1209.
- Hua, et al., "Tract probability maps in stereotaxic spaces: analyses of white matter anatomy and tract-specific quantification," *Neuroimage* 39 (1) (2008), pp. 336-347.
- Johansen-Berg, et al., "Anatomical connectivity of the subgenual cingulate region targeted with deep brain stimulation for treatment-resistant depression," *Cereb Cortex* 18 (6) (2008), pp. 1374-1383.
- Kopell, et al., "Deep brain stimulation for psychiatric disorders," *J Clin Neurophysiol* 21 (1) (2004), pp. 51-67.
- Lozano, et al., "Subcallosal cingulate gyrus deep brain stimulation for treatment-resistant depression," *Biol Psychiatry* 64 (6) (2008), pp. 461-467.
- Lujan, et al., "Tracking the mechanisms of deep brain stimulation for neuropsychiatric disorders," *Front Biosci* 13 (2008), pp. 5892-5904.
- Lujan, J.L. et al., "Automated 3-Dimensional Brain Atlas Fitting to Microelectrode Recordings from Deep Brain Stimulation Surgeries," *Stereotact. Funct. Neurosurg.* 87(2009), pp. 229-240.
- Machado, et al., "Functional topography of the ventral striatum and anterior limb of the internal capsule determined by electrical stimulation of awake patients," *Clin Neurophysiol* 120 (11) (2009), pp. 1941-1948.
- Malone, et al., "Deep brain stimulation of the ventral capsule/ventral striatum for treatment-resistant depression," *Biol Psychiatry* 65 (4) (2009), pp. 267-275.
- Mayberg, H. S., et al., "Deep brain stimulation for treatment-resistant depression," *Neuron*, 45(5) (Mar. 3, 2005), pp. 651-660.
- Mayberg, H. S., et al., "Limbic-cortical dysregulation: a proposed model of depression," *J Neuropsychiatry Clin Neurosci.* 9 (3) (1997), pp. 471-481.
- McIntyre, C. C., et al., "Network perspectives on the mechanisms of deep brain stimulation," *Neurobiol Dis* 38 (3) (2010), pp. 329-337.
- Miocinovic, S., et al., "Experimental and theoretical characterization of the voltage distribution generated by deep brain stimulation," *Exp Neural* 216 (i) (2009), pp. 166-176.
- Nuttin, et al., "Electrical stimulation in anterior limbs of internal capsules in patients with obsessive-compulsive disorder," *Lancet* 354 (9189) (1999), p. 1526.
- Saxena, et al., "Cerebral glucose metabolism in obsessive-compulsive hoarding," *Am J Psychiatry*. 161 (6) (2004), pp. 1038-1048.
- Viola, et al., "Importance-driven focus of attention," *IEEE Trans Vis Comput Graph* 12 (5) (2006), pp. 933-940.
- Wakana, S., et al., "Reproducibility of quantitative tractography methods applied to cerebral white matter," *Neuroimage* 36 (3) (2007), pp. 630-644.
- Mayr et al., "Basic Design and Construction of the Vienna FES Implants: Existing Solutions and Prospects for New Generations of Implants", *Medical Engineering & Physics*, 2001; 23:53-60.

(56)

References Cited**OTHER PUBLICATIONS**

- Zhang, Y., et al., "Atlas-guided tract reconstruction for automated and comprehensive examination of the white matter anatomy," *Neuroimage* 52(4) (2010), pp. 1289-1301.
- "BioPSE" The Biomedical Problem Solving Environment, <http://www.sci.utah.edu/cibc/software/index.html>, MCRR Center for Integrative Biomedical Computing, (2004).
- Andrews, R. J., "Neuroprotection trek—the next generation: neuromodulation I. Techniques—deep brain stimulation, vagus nerve stimulation, and transcranial magnetic stimulation," *Ann NY Acad Sci.* 993, (May 2003), 1-13.
- Carnevale, N.T. et al., "The Neuron Book," Cambridge, UK: Cambridge University Press (2006), 480 pages.
- Chaturvedi: "Development of Accurate Computational Models for Patient-Specific Deep Brain Stimulation," Electronic Thesis or Dissertation, Jan. 2012, 162 pages.
- Chaturvedi, A. et al.: "Patient-specific models of deep brain stimulation: Influence of field model complexity on neural activation predictions," *Brain Stimulation*, Elsevier, Amsterdam, NL, vol. 3, No. 2 Apr. 2010, pp. 65-77.
- Frankemolle, et al., "Reversing cognitive-motor impairments in Parkinson's disease patients using a computational modeling approach to deep brain stimulation programming," *Brian* 133 (2010), pp. 746-761.
- McIntyre, C.C., et al., "Modeling the excitability of mammalian nerve fibers: influence of afterpotentials on the recovery cycle," *J Neurophysiol.* 87(2) (Feb. 2002), pp. 995-1006.
- Peterson, et al., "Predicting myelinated axon activation using spatial characteristics of the extracellular field," *Journal of Neural Engineering*, 8 (2011), 12 pages.
- Warman, et al., "Modeling the Effects of Electric Fields on nerver Fibers; Dermination of Excitation Thresholds," *IEEE Transactions on Biomedical Engineering*, vol. 39, No. 12 (Dec. 1992), pp. 1244-1254.
- Wessellink, et al., "Analysis of Current Density and Related Parameters in Spinal Cord Stimulation," *IEEE Transactions on Rehabilitation Engineering*, vol. 6, No. 2 Jun. 1998, pp. 200-207.
- Andrews, R. J., "Neuroprotection trek—the next generation: neuromodulation II. Applications—epilepsy, nerve regeneration, neurotrophins," *Ann NY Acad Sci.* 993 (May 2003), 14-24.
- Astrom, M. , et al., "The effect of cystic cavities on deep brain stimulation in the basal ganglia: a simulation-based study," *J Neural Eng.*, 3(2), (Jun. 2006). 132-8.
- Bazin et al., "Free Software Tools for Atlas-based Volumetric Neuroimage Analysis", *Proc. SPIE* 5747, *Medical Imaging 2005: Image Processing*, 1824 May 5, 2005.
- Back, C. , et al., "Postoperative Monitoring of the Electrical Properties of Tissue and Electrodes in Deep Brain Stimulation", *Neuromodulation*, 6(4), (Oct. 2003), 248-253.
- Baker, K. B., et al., "Evaluation of specific absorption rate as a dosimeter of MRI-related implant heating", *J Magn Reson Imaging.*, 20(2), (Aug. 2004), 315-20.
- Brown, J. "Motor Cortex Stimulation," *Neurosurgical Focus* (Sep. 15, 2001) 11(3):E5.
- Budai et al., "Endogenous Opioid Peptides Acting at m-Opioid Receptors in the Dorsal Horn Contribute to Midbrain Modulation of Spinal Nociceptive Neurons," *Journal of Neurophysiology* (1998) 79(2): 677-687.
- Cesselin, F. "Opioid and anti-opioid peptides," *Fundamental and Clinical Pharmacology* (1995) 9(5): 409-33 (Abstract only).
- Rezai et al., "Deep Brain Stimulation for Chronic Pain" *Surgical Management of Pain*, Chapter 44 pp. 565-576 (2002).
- Xu, Md., Shi-Ang, article entitled "Comparison of Half-Band and Full-Band Electrodes for Intracochlear Electrical Stimulation", *Annals of Otolology, Rhinology & Laryngology* (Annals of Head & Neck Medicine & Surgery), vol. 102(5) pp. 363-367 May 1993.
- Bedard, C. , et al., "Modeling extracellular field potentials and the frequency-filtering properties of extracellular space", *Biophys J ..* 86(3). (Mar. 2004), 1829-42.
- Benabid, A. L., et al., "Future prospects of brain stimulation", *Neurol Res.* 22(3), (Apr. 2000), 237-46.
- Brummer, S. B., et al., "Electrical Stimulation with Pt Electrodes: II—Estimation of Maximum Surface Redox (Theoretical Non-Gassing) Limits", *IEEE Transactions on Biomedical Engineering*, vol. BME-24, Issue 5, (Sep. 1977), 440-443.
- Butson, Christopher R., et al., "Deep Brain Stimulation of the Subthalamic Nucleus: Model-Based Analysis of the Effects of Electrode Capacitance on the Volume of Activation", *Proceedings of the 2nd International IEEE EMBS*, (Mar. 16-19, 2005), 196-197.
- Mcintyre, Cameron C., et al., "Cellular effects of deep brain stimulation: model-based analysis of activation and inhibition," *J Neurophysiol.* 91(4) (Apr. 2004), pp. 1457-1469.
- Chaturvedi, A., et al., "Subthalamic Nucleus Deep Brain Stimulation: Accurate Axonal Threshold Prediction with Diffusion Tensor Based Electric Field Models", *Engineering in Medicine and Biology Society*, 2006. EMBS' 06 28th Annual International Conference of the IEEE, IEEE, Piscataway, NJ USA, Aug. 30, 2006.
- Butson, Christopher et al., "Predicting the Effects of Deep Brain Stimulation with Diffusion Tensor Based Electric Field Models" Jan. 1, 2001, *Medical Image Computing and Computer-Assisted Intervention—Mic CAI 2006 Lecture Notes in Computer Science*; LNCS, Springer, Berlin, DE.
- Butson, C. R., et al., "Deep brainstimulation interactive visualization system", *Society for Neuroscience* vol. 898.7 (2005).
- Hodaie, M., et al., "Chronic anterior thalamus stimulation for intractable epilepsy," *Epilepsia*, 43(6) (Jun. 2002), pp. 603-608.
- Hoekema, R., et al., "Multigrid solution of the potential field in modeling electrical nerve stimulation," *Comput Biomed Res.*, 31(5) (Oct. 1998), pp. 348-362.
- Holsheimer, J., et al., "Identification of the target neuronal elements in electrical deep brain stimulation," *Eur J Neurosci.*, 12(12) (Dec. 2000), pp. 4573-4577.
- Jezernek, S., et al., "Neural network classification of nerve activity recorded in a mixed nerve," *Neurol Res.*, 23(5) (Jul. 2001), pp. 429-434.
- Jones, DK., et al., "Optimal strategies for measuring diffusion in anisotropic systems by magnetic resonance imaging," *Magn. Reson. Med.*, 42(3) (Sep. 1999), pp. 515-525.
- Krack, P., et al., "Postoperative management of subthalamic nucleus stimulation for Parkinson's disease," *Mov. Disord.*, vol. 17(suppl 3) (2002), pp. 188-197.
- Le Bihan, D., et al., "Diffusion tensor imaging: concepts and applications," *J Magn Reson Imaging*, 13(4) (Apr. 2001), pp. 534-546.
- Lee, D. C., et al., "Extracellular electrical stimulation of central neurons: quantitative studies," In: *Handbook of neuroprosthetic methods*, WE Finn and PG Lopresti (eds) CRC Press (2003), pp. 95-125.
- Levy, AL., et al., "An Internet-connected, patient-specific, deformable brain atlas integrated into a surgical navigation system," *J Digit Imaging*, 10(3 Suppl 1) (Aug. 1997), pp. 231-237.
- Liu, Haiying, et al., "Intra-operative MR-guided DBS implantation for treating PD and ET," *Proceedings of SPIE* vol. 4319, Department of Radiology & Neurosurgery, University of Minnesota, Minneapolis, MN 55455 (2001), pp. 272-276.
- Mcintyre, C. C., et al., "Extracellular stimulation of central neurons: influence of stimulus waveform and frequency on neuronal output," *J. Neurophysiol.*, 88(4), (Oct. 2002), pp. 1592-1604.
- Mcintyre, C. C., et al., "Microstimulation of spinal motoneurons: a model study," *Proceedings of the 19th Annual International Conference of the IEEE Engineering in Medicine and Biology society*, vol. 5, (1997), pp. 2032-2034.
- Mcintyre, Cameron C., et al., "Model-based Analysis of deep brain stimulation of the thalamus," *Proceedings of the Second joint EMBS/BM ES Conference*, vol. 3, Annual Fall Meeting of the Biomedical Engineering Society (Cal. No. 02CH37392) IEEE Piscataway, NJ (2002), pp. 2047-2048.
- Mcintyre, C. C., et al., "Model-based design of stimulus trains for selective microstimulation of targeted neuronal populations," *Proceedings of the 23rd Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 1 (2001), pp. 806-809.

(56)

References Cited**OTHER PUBLICATIONS**

- Mcintyre, C. C., et al., Model-based design of stimulus waveforms for selective microstimulation in the central nervous system., Proceedings of the First Joint [Engineering in Medicine and Biology, 1999. 21st Annual Conf. and the 1999 Annual Fall Meeting of the Biomedical Engineering Soc.] BM ES/EMBS Conference, vol. 1 (1999), p. 384.
- Mcintyre, Cameron C., et al., "Modeling the excitability of mammalian nerve fibers: influence of afterpotentials on the recovery cycle," *J Neurophysiol*, 87(2) (Feb. 2002), pp. 995-1006.
- Mcintyre, Cameron C., et al., "Selective microstimulation of central nervous system neurons," *Annals of biomedical engineering*, 28(3) (Mar. 2000), pp. 219-233.
- Mcintyre, C. C., et al., "Sensitivity analysis of a model of mammalian neural membrane," *Biol Cybern.*, 79(1) (Jul. 1998), pp. 29-37.
- Mcintyre, Cameron C., et al., "Uncovering the mechanism(s) of action of deep brain stimulation: activation, inhibition, or both," *Clin Neurophysiol*, 115(6) (Jun. 2004), pp. 1239-1248.
- Mcintyre, Cameron C., et al., "Uncovering the mechanisms of deep brain stimulation for Parkinson's disease through functional imaging, neural recording, and neural modeling," *Crit Rev Biomed Eng.*, 30(4-6) (2002), pp. 249-281.
- Mouine et al. "Multi-Strategy and Multi-Algorithm Cochlear Prostheses", *Biomed. Sci. Instrument*, 2000; 36:233-238.
- Mitra PP, Pesaran B. Analysis of dynamic brain imaging data. *Biophys J*. Feb. 1999;76(2):691-708. doi: 10.1016/S0006-3495(99)77236-X. PMID: 9929474; PMCID: PMC 1300074.
- Hammer N, Glätzner J, Feja C, Kühne C, Meixensberger J, et al. (2015) Human Vagus Nerve Branching in the Cervical Region. *PLoS ONE* 10(2): e0118006. Published: Feb. 13, 2015. <https://doi.org/10.1371/journal.pone.0118006>.
- Trost M, Su S, Su P, Yen RF, Tseng HM, Barnes A, Ma Y, Eidelberg D. Network modulation by the subthalamic nucleus in the treatment of Parkinson's disease. *Neuroimage*. May 15, 2006;31(1):301-7. doi: 10.1016/j.neuroimage.2005.12.024. Epub Feb. 8, 2006.
- Alo, K. M., et al., "New trends in neuromodulation for the management of neuropathic pain," *Neurosurgery*, 50(4), (Apr. 2002), pp. 690-703, discussion pp. 703-704.
- Ashby, P., et al., "Neurophysiological effects of stimulation through electrodes in the human subthalamic nucleus," *Brain*, 122 (Pt 10), (Oct. 1999), pp. 1919-1931.
- Baker, K. B., et al., "Subthalamic nucleus deep brain stimulus evoked potentials: Physiological and therapeutic implications," *Movement Disorders*, 17(5), (Sep./Oct. 2002), pp. 969-983.
- Bammer, R., et al., "Diffusion tensor imaging using single-shot SENSE-EPI", *Magn Reson Med*, 48(1), (Jul. 2002), pp. 128-136.
- Basser, P.J., et al., "MR diffusion tensor spectroscopy and imaging," *Biophys J*, 66(1), (Jan. 1994), pp. 259-267.
- Basser, P.J., et al., "New currents in electrical stimulation of excitable tissues," *Annu Rev Biomed Eng.*, 2, (2000), pp. 377-397.
- Benabid, AL., et al., "Chronic electrical stimulation of the ventralis intermedius nucleus of the thalamus as a treatment of movement disorders," *J. Neurosurg.*, 84(2), (Feb. 1996), pp. 203-214.
- Benabid, AL., et al., "Combined [thalamotomy and stimulation] stereotactic surgery of the VIM thalamic nucleus for bilateral Parkinson disease," *Appl Neurophysiol*, vol. 50, (1987), pp. 344-346.
- Benabid, A.L., et al., "Long-term suppression of tremor by chronic stimulation of the ventral intermediate thalamic nucleus," *Lancet*, 337 (8738), (Feb. 16, 1991), pp. 403-406.
- Butson, C. R., et al., "Predicting the effects of deep brain stimulation with diffusion tensor based electric field models," *Medical Image Computing and Computer-Assisted Intervention—Mic Cai 2006*, Lecture Notes in Computer Science (LNCS), vol. 4191, pp. 429-437, LNCS, Springer, Berlin, DE.
- Christensen, Gary E., et al., "Volumetric transformation of brain anatomy," *IEEE Transactions on Medical Imaging*, 16 (6), (Dec. 1997), pp. 864-877.
- Cooper, S., et al., "Differential effects of thalamic stimulation parameters on tremor and paresthesias in essential tremor," *Movement Disorders*, 17(Suppl. 5), (2002), p. S193.
- Coubes, P., et al., "Treatment of DYT1-generalised dystonia by stimulation of the internal globus pallidus," *Lancet*, 355(9222), (Jun. 24, 2000), pp. 2220-2221.
- Dasilva, A.F. M., et al., "A Primer Diffusion Tensor Imaging of Anatomical Substructures," *Neurosurg. Focus*; 15(1) (Jul. 2003), pp. 1-4.
- Dawant, B. M., et al., "Computerized atlas-guided positioning of deep brain stimulators: a feasibility study," *Biomedical Image registration*, Second International Workshop, WBIR 2003, Revised Papers (Lecture notes in Comput. Sci. vol. (2717), Springer-Verlag Berlin, Germany(2003), pp. 142-150.
- Finnis, K. W., et al., "3-D functional atlas of subcortical structures for image guided stereotactic neurosurgery," *Neuroimage*, vol. 9, No. 6, Iss. 2 (1999), p. S206.
- Finnis, K. W., et al., "3D Functional Database of Subcortical Structures for Surgical Guidance in Image Guided Stereotactic Neurosurgery," *Medical Image Computing and Computer-Assisted Intervention—MICCAI'99*, Second International Conference. Cambridge, UK, Sep. 19-22, 1999, Proceedings (1999), pp. 758-767.
- Finnis, K. W., et al., "A 3-Dimensional Database of Deep Brain Functional Anatomy, and Its Application to Image-Guided Neurosurgery," *Proceedings of the Third International Conference on Medical Image Computing and Computer-Assisted Intervention. Lecture Notes in Computer Science*; vol. 1935 (2000), pp. 1-8.
- Finnis, K. W., et al., "A functional database for guidance of surgical and therapeutic procedures in the deep brain," *Proceedings of the 22nd Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 3 (2000), pp. 1787-1789.
- Finnis, K. W., et al., "Application of a Population Based Electrophysiological Database to the Planning and Guidance of Deep Brain Stereotactic Neurosurgery," *Proceedings of the 5th International Conference on Medical Image Computing and Computer-Assisted Intervention—Part 11*, Lecture Notes in Computer Science; vol. 2489 (2002), pp. 69-76.
- Finnis, K. W., et al., "Subcortical physiology deformed into a patient-specific brain atlas for image-guided stereotaxy," *Proceedings of SPIE—vol. 4681 Medical Imaging 2002: Visualization, Image-Guided Procedures, and Display* (May 2002), pp. 184-195.
- Finnis, Krik W., et al., "Three-Dimensional Database of Subcortical Electrophysiology for Image-Guided Stereotactic Functional Neurosurgery," *IEEE Transactions on Medical Imaging*, 22(1) (Jan. 2003), pp. 93-104.
- Gabriels, L., et al., "Deep brain stimulation for treatment-refractory obsessive-compulsive disorder: psychopathological and neuropsychological outcome in three cases," *Acta Psychiatr Scand.*, 107(4) (2003), pp. 275-282.
- Gabriels, L.A., et al., "Long-term electrical capsular stimulation in patients with obsessive-compulsive disorder," *Neurosurgery*, 52(6) (Jun. 2003), pp. 1263-1276.
- Goodall, E. V., et al., "Modeling study of activation and propagation delays during stimulation of peripheral nerve fibers with a tripolar cuff electrode," *IEEE Transactions on Rehabilitation Engineering*, [see also *IEEE Trans. on Neural Systems and Rehabilitation*], 3(3) (Sep. 1995), pp. 272-282.
- Goodall, E. V., et al., "Position-selective activation of peripheral nerve fibers with a cuff electrode," *IEEE Transactions on Biomedical Engineering*, 43(8) (Aug. 1996), pp. 851-856.
- Goodall, E. V., "Simulation of activation and propagation delay during tripolar neural stimulation," *Proceedings of the 15th Annual International Conference of the IEEE Engineering in Medicine and Biology Society* (1993), pp. 1203-1204.
- Grill, WM., "Modeling the effects of electric fields on nerve fibers: influence of tissue electrical properties," *IEEE Transactions on Biomedical Engineering*, 46(8) (1999), pp. 918-928.
- Grill, W. M., et al., "Neural and connective tissue response to long-term implantation of multiple contact nerve cuff electrodes," *J Biomed Mater Res.*, 50(2) (May 2000), pp. 215-226.

(56)

References Cited**OTHER PUBLICATIONS**

Grill, W. M., "Neural modeling in neuromuscular and rehabilitation research," Proceedings of the 23rd Annual International Conference of the IEEE Engineering in Medicine and Biology Society, vol. 4 (2001), pp. 4065-4068.

Grill, W. M., et al., "Non-invasive measurement of the input-output properties of peripheral nerve stimulating electrodes," *Journal of Neuroscience Methods*, 65(1) (Mar. 1996), pp. 43-50.

Grill, W. M., et al., "Quantification of recruitment properties of multiple contact cuff electrodes," *IEEE Transactions on Rehabilitation Engineering*, [see also *IEEE Trans. on Neural Systems and Rehabilitation*], 4(2) (Jun. 1996), pp. 49-62.

Grill, W. M., "Spatially selective activation of peripheral nerve for neuroprosthetic applications," Ph.D. Case Western Reserve University, (1995), pp. 245 pages.

Grill, W. M., "Stability of the input-output properties of chronically implanted multiple contact nerve cuff stimulating electrodes," *IEEE Transactions on Rehabilitation Engineering* [see also *IEEE Trans. on Neural Systems and Rehabilitation*] (1998), pp. 364-373.

Grill, W. M., "Stimulus waveforms for selective neural stimulation," *IEEE Engineering in Medicine and Biology Magazine*, 14(4) (Jul.-Aug. 1995), pp. 375-385.

Grill, W. M., et al., "Temporal stability of nerve cuff electrode recruitment properties," *IEEE 17th Annual Conference Engineering in Medicine and Biology Society*, vol. 2 (1995), pp. 1089-1090.

Gross, R.E., et al., "Advances in neurostimulation for movement disorders," *Neurol Res.*, 22(3) (Apr. 2000), pp. 247-258.

Guridi et al., "The subthalamic nucleus, hemiballismus and Parkinson's disease: reappraisal of a neurological dogma," *Brain*, vol. 124, 2001, pp. 5-19.

Haberler, C., et al., "No tissue damage by chronic deep brain stimulation in Parkinson's disease," *Ann Neurol.*, 48(3) (Sep. 2000), pp. 372-376.

Hamel, W., et al., "Deep brain stimulation of the subthalamic nucleus in Parkinson's disease: evaluation of active electrode contacts," *J Neurol Neurosurg Psychiatry*, 74(8) (Aug. 2003), pp. 1036-1046.

Hanekom, "Modelling encapsulation tissue around cochlear implant electrodes," *Med. Biol. Eng. Comput.* vol. 43 (2005), pp. 47-55.

Haueisen, J., et al., "The influence of brain tissue anisotropy on human EEG and MEG," *Neuroimage*, 15(1) (Jan. 2002), pp. 159-166.

D'Haese et al. *Medical Image Computing and Computer-Assisted Intervention—MICCAI 2005 Lecture Notes in Computer Science*, 2005, vol. 3750, 2005, 427-434.

Rohde et al. *IEEE Transactions on Medical Imaging*, vol. 22 No. 11, 2003 p. 1470-1479.

Dawant et al., *Biomedical Image Registration. Lecture Notes in Computer Science*, 2003, vol. 2717, 2003, 142-150.

Miocinovic et al., "Stereotactic Neurosurgical Planning, Recording, and Visualization for Deep Brain Stimulation in Non-Human Primates", *Journal of Neuroscience Methods*, 162:32-41, Apr. 5, 2007, XP022021469.


Gemmar et al., "Advanced Methods for Target Navigation Using Microelectrode Recordings in Stereotactic Neurosurgery for Deep Brain Stimulation", 21st IEEE International Symposium on Computer-Based Medical Systems, Jun. 17, 2008, pp. 99-104, XP031284774.

Acar et al., "Safety Anterior Commissure-Posterior Commissure-Based Target Calculation of the Subthalamic Nucleus in Functional Stereotactic Procedures", *Stereotactic Funct. Neurosura.*, 85:287-291, Aug. 2007.

Andrade-Souza, "Comparison of Three Methods of Targeting the Subthalamic Nucleus for Chronic Stimulation in Parkinson's Disease", *Neurosurgery*, 56:360-368, Apr. 2005.

Anheim et al., "Improvement in Parkinson Disease by Subthalamic Nucleus Stimulation Based on Electrode Placement", *Arch Neural.*, 65:612-616, May 2008.

* cited by examiner

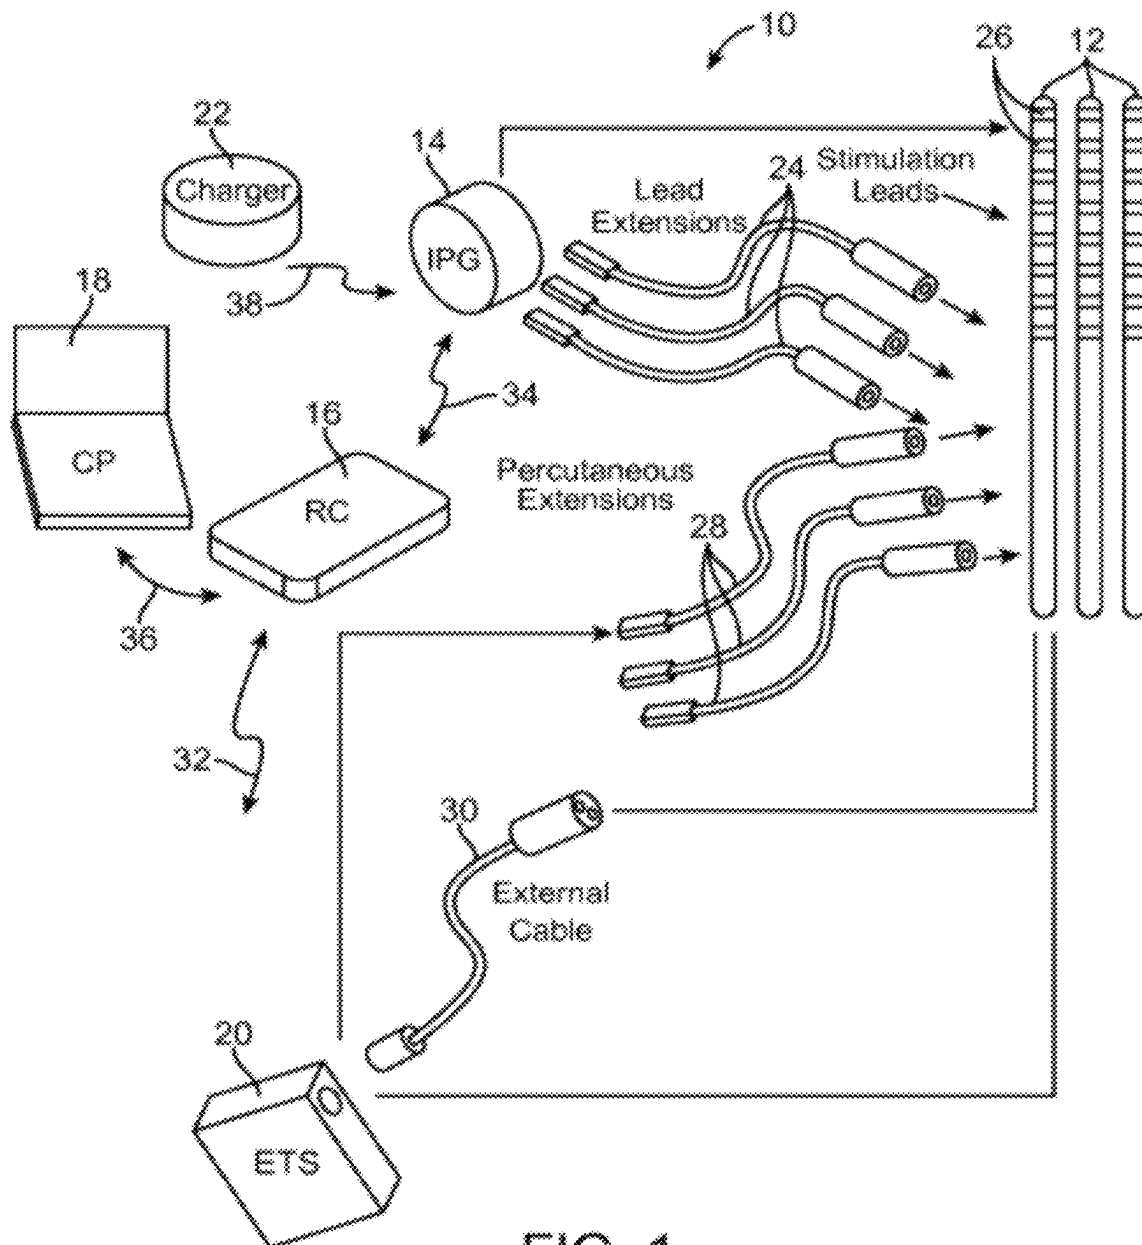

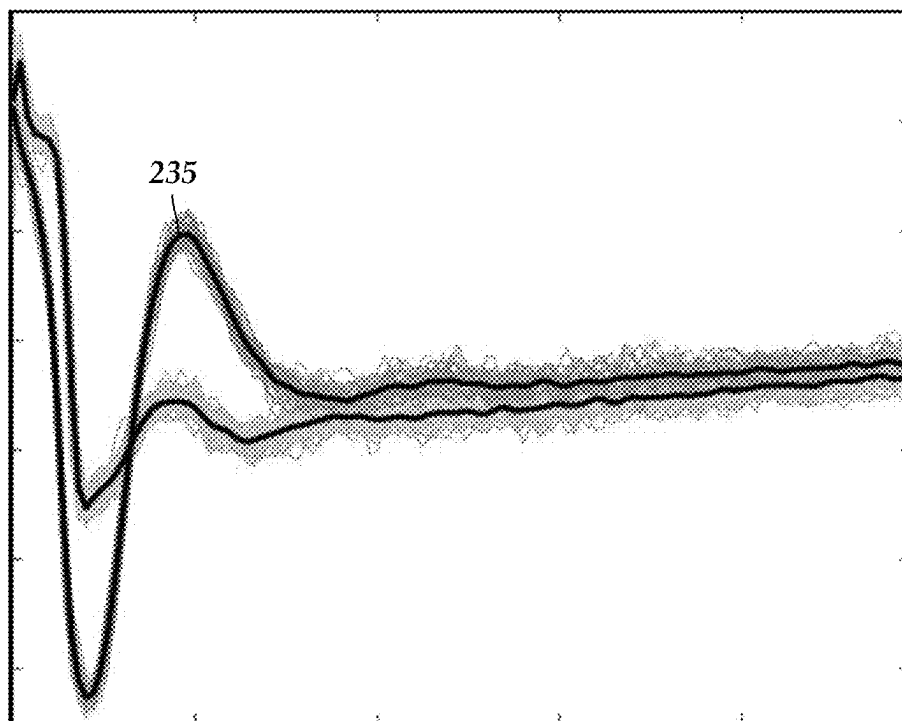


Fig. 2A

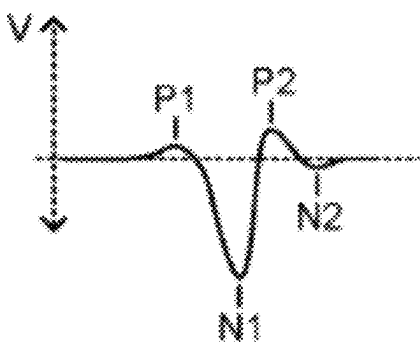
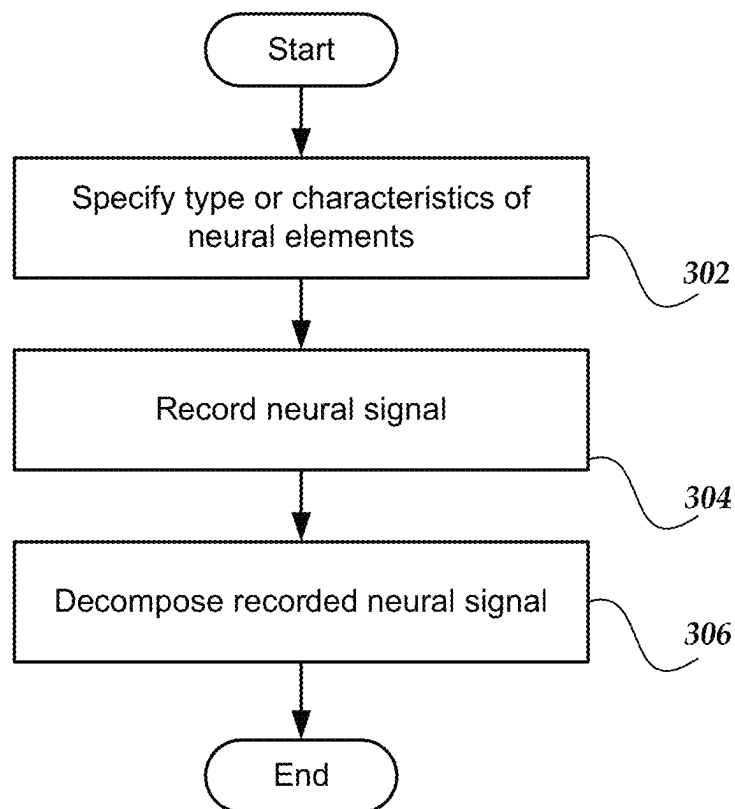
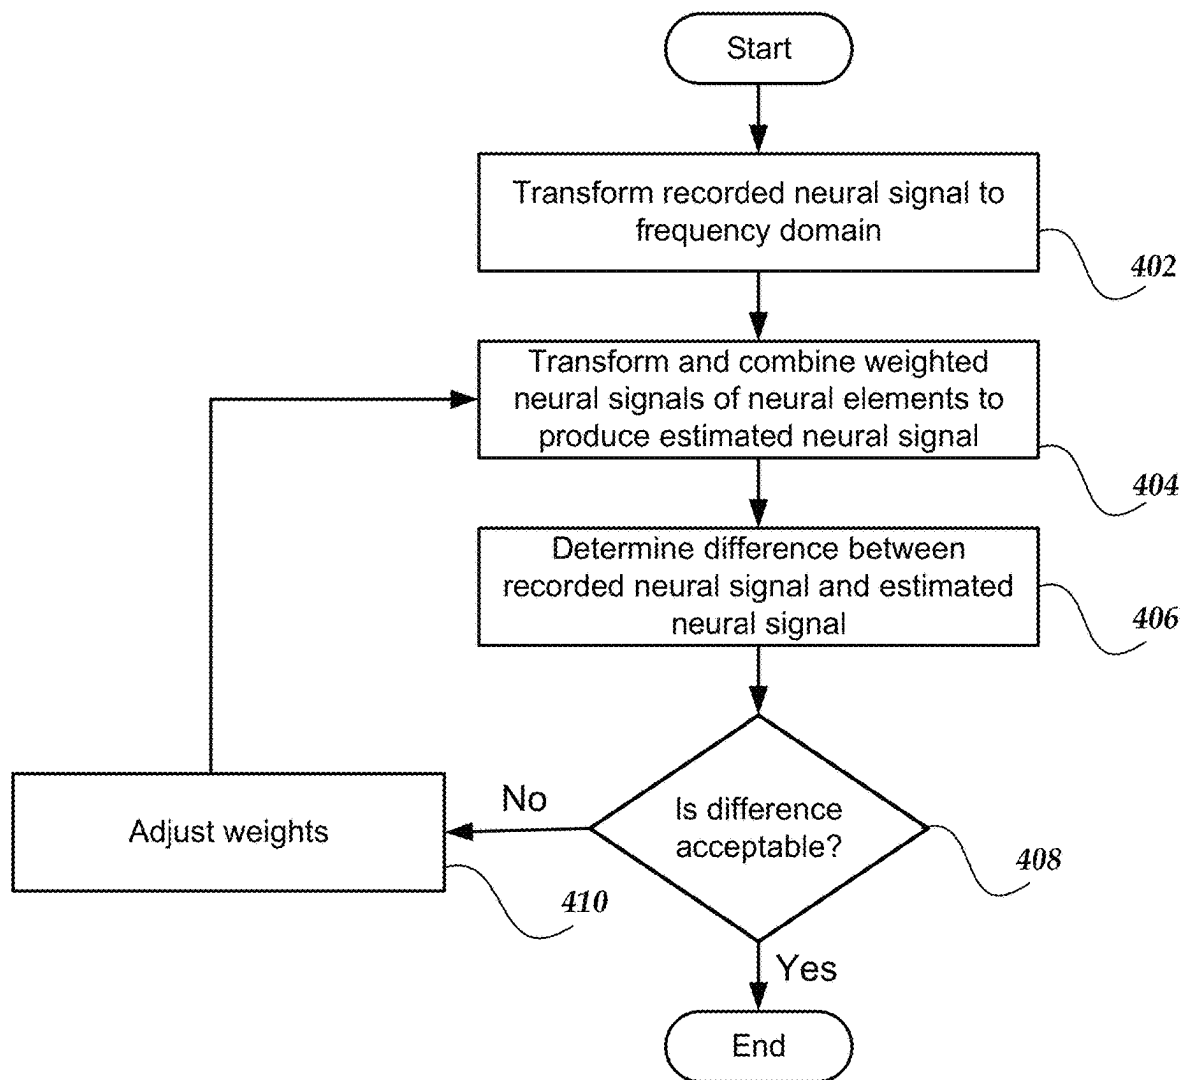
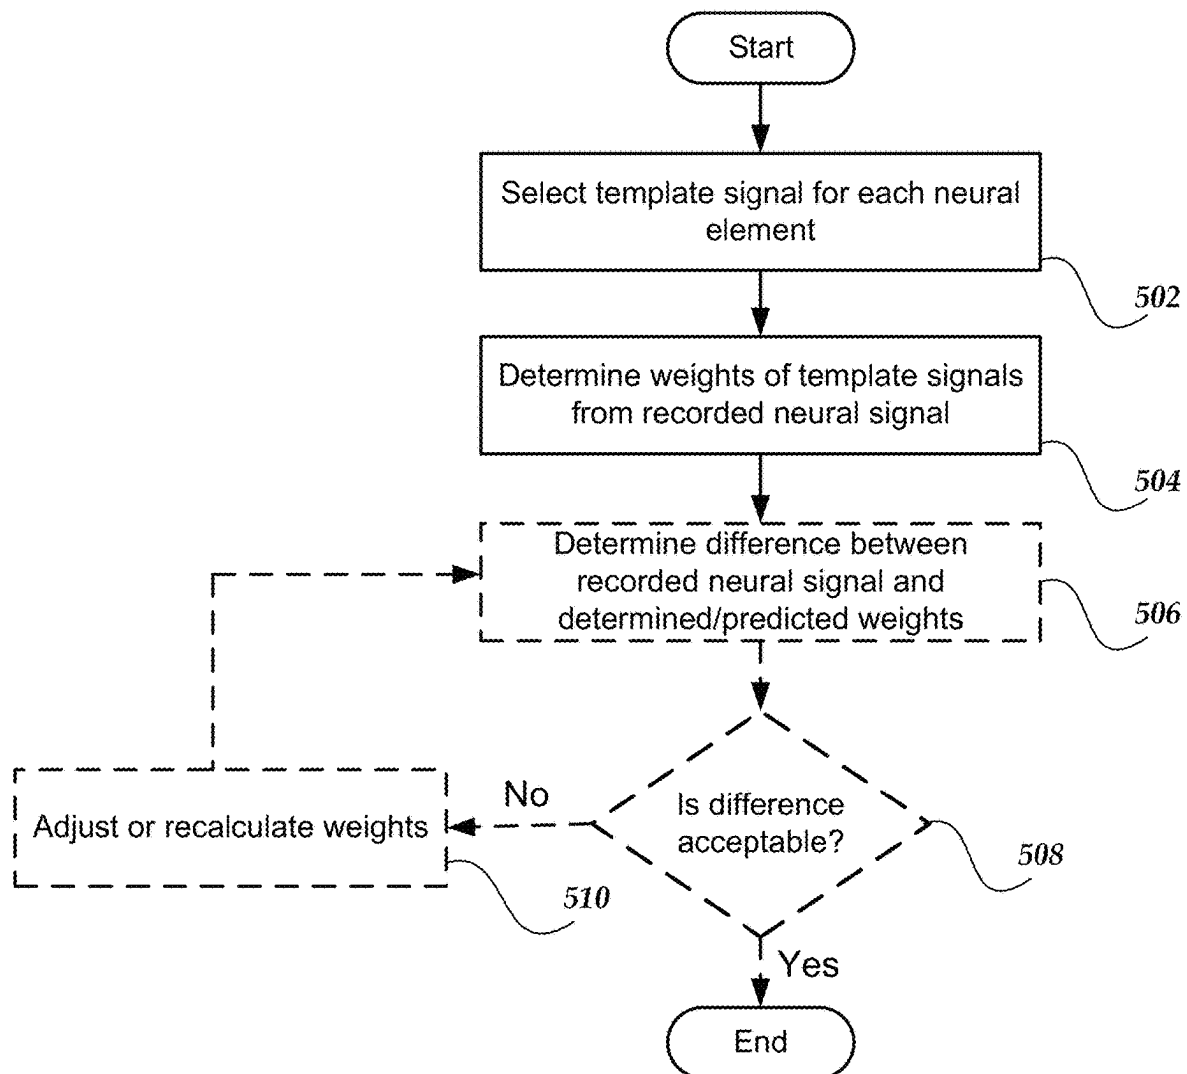
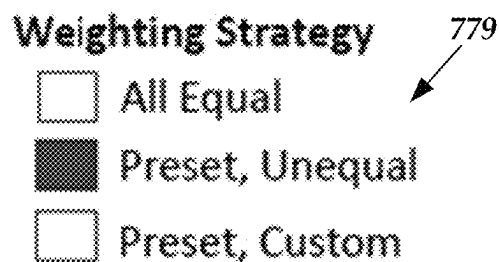
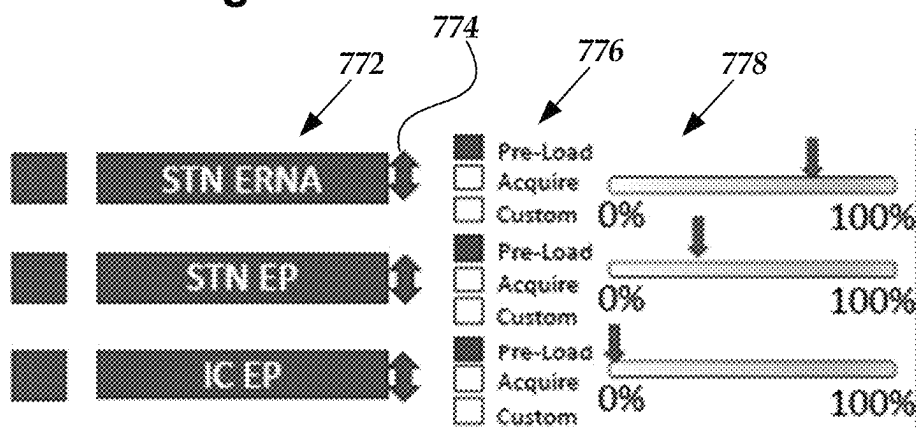
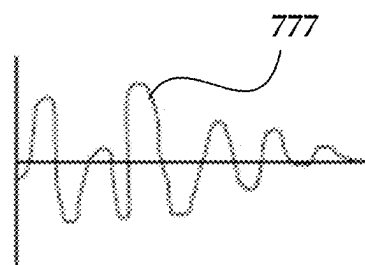
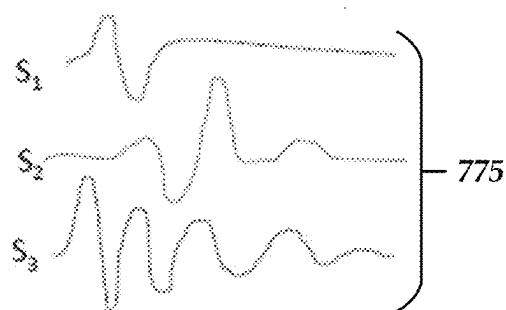
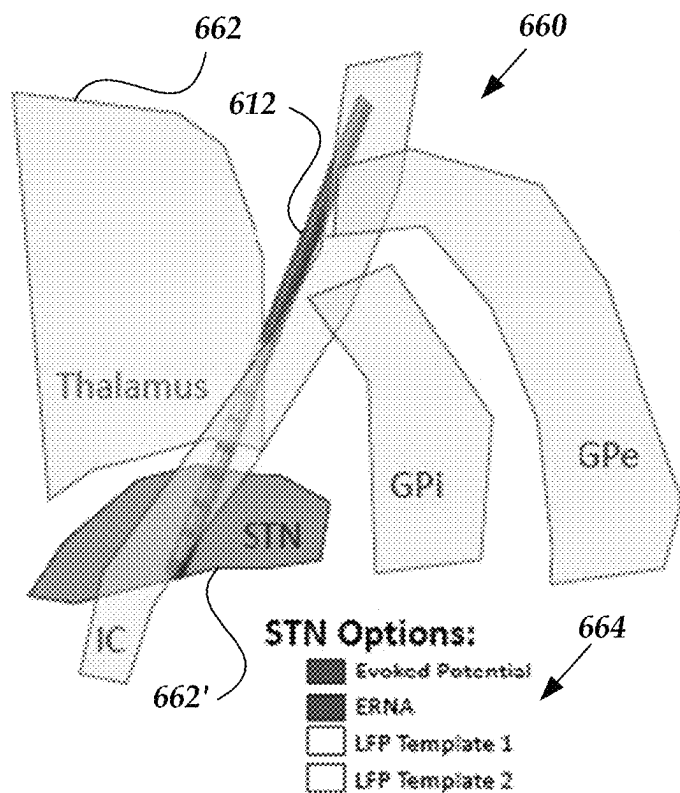


Fig. 2B

**Fig. 3**

**Fig. 4**

**Fig. 5**



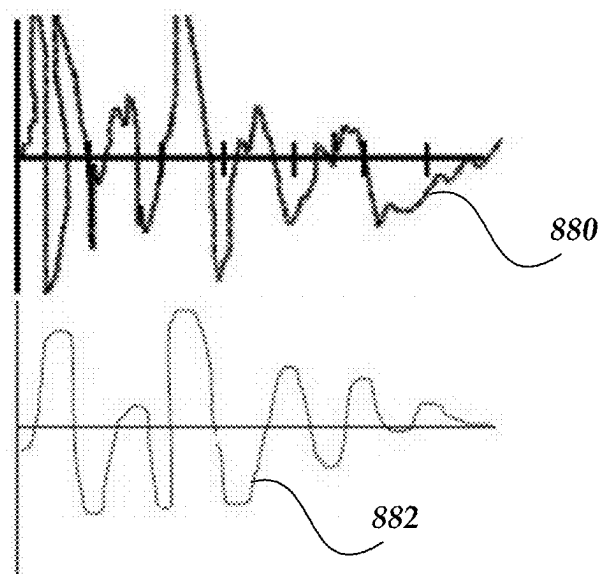


Fig. 8

990

Acquisition and Filter Settings

☒ Artifact Filter: (Add Stim Settings)
PW: 210 μ s Symmetry: Biphasic Filter: Auto

☒ Noise Filter: **BandPass** HPF: 0.5 Hz LPF: 8000 Hz

☐ Lead Encapsulation/Environmental Scaling

☐ Fixed Constant Scaling ☐ Frequency-Dependent Scaling (Specify file)

☒ **Template Signal Properties**

☐ Acquire: N/A Epochs Sampling Rate: 25 kHz

☒ Preload File: ERNA.sig Sampling Duration: 30 ms

Fig. 9

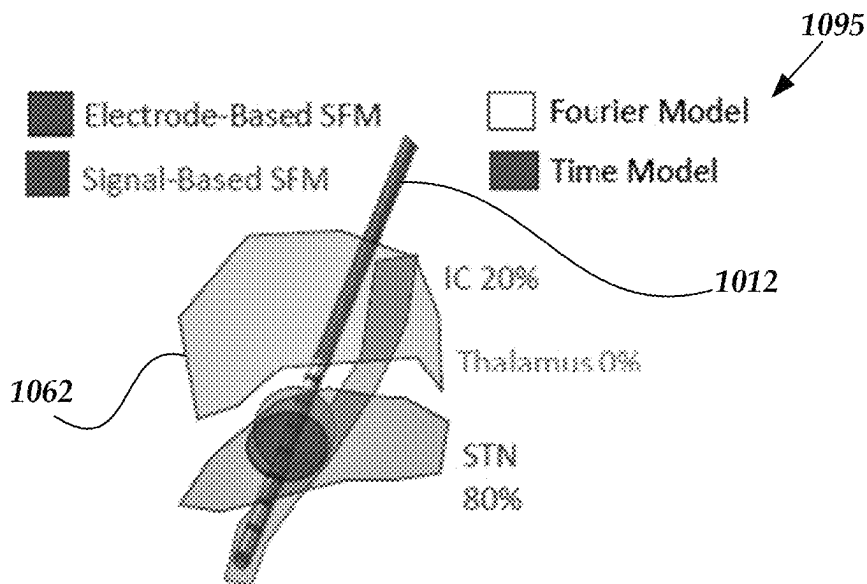


Fig. 10

1196

Amplitude: 2.0 mA $\updownarrow$

PW: 200 μ s $\updownarrow$

Rate: 130 Hz $\uparrow$

Fig. 11

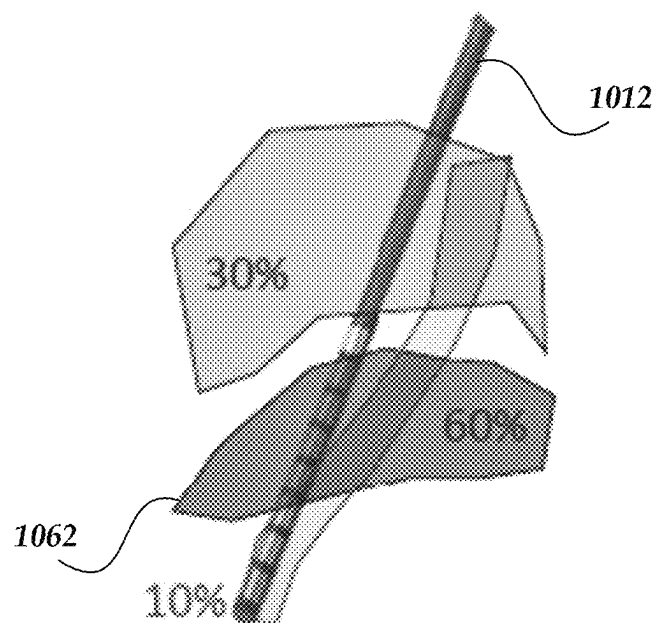
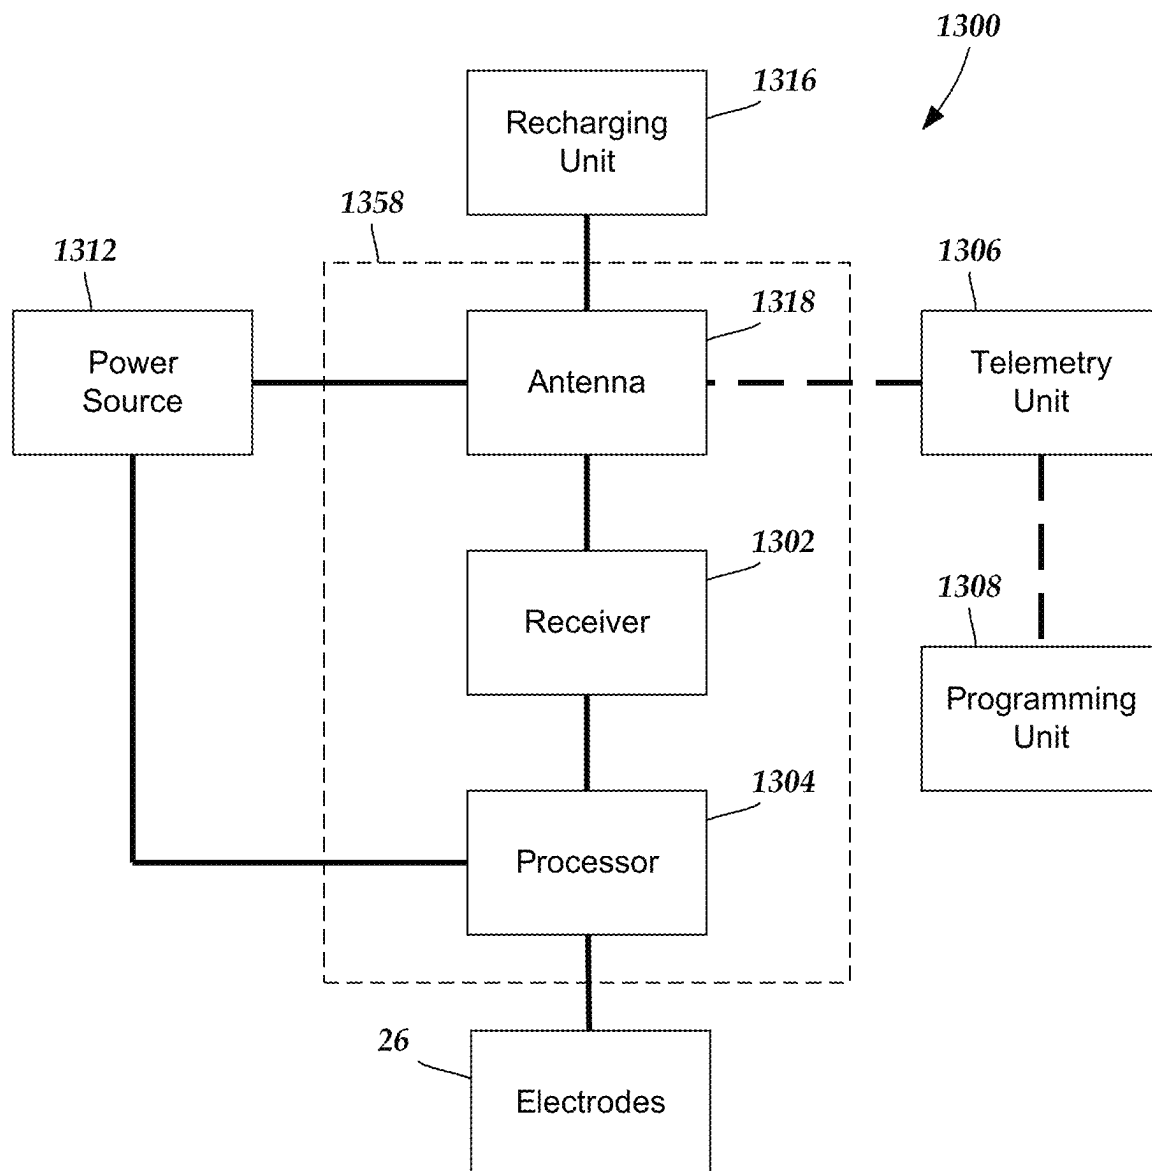
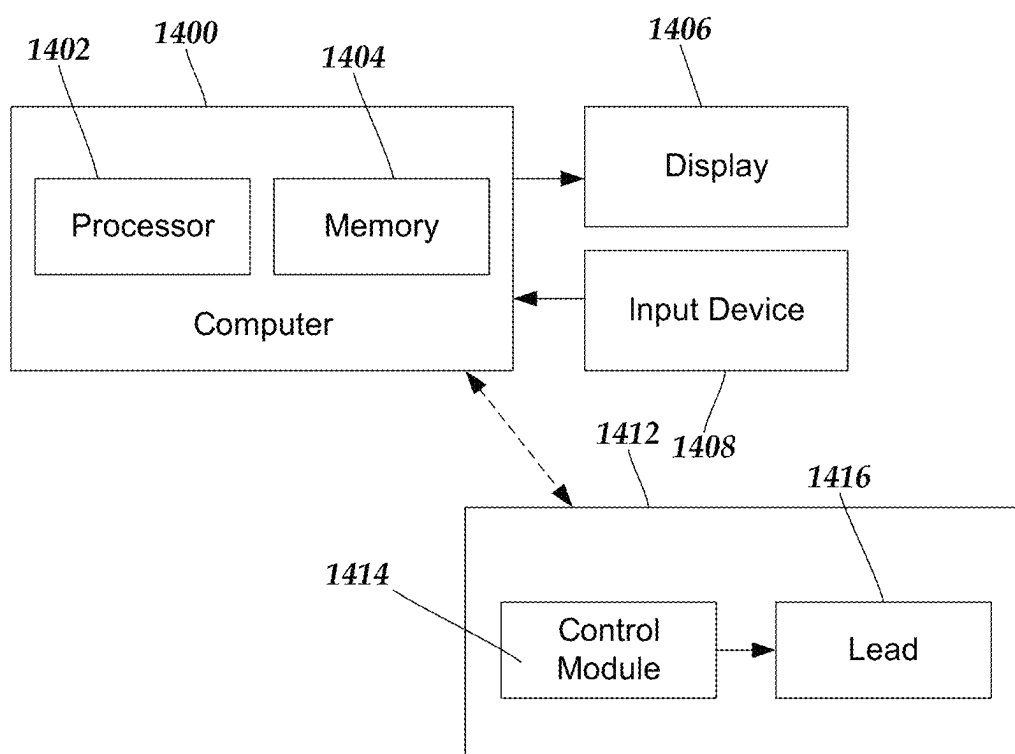


Fig. 12

**Fig. 13**

**Fig. 14**

1

METHODS AND SYSTEMS FOR ESTIMATING NEURAL ACTIVATION BY STIMULATION USING A STIMULATION SYSTEM

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims the benefit under 35 U.S.C. § 119(e) of U.S. Provisional Patent Application Ser. No. 63/210,799, filed Jun. 15, 2021, which is incorporated herein by reference.

FIELD

The present disclosure is directed to the area of implantable electrical stimulation systems and methods of making and using the systems. The present disclosure is also directed to methods and systems for estimating neural activation by stimulation using the implantable electrical stimulation system.

BACKGROUND

Implantable electrical stimulation systems have proven therapeutic in a variety of diseases and disorders. For example, spinal cord stimulation systems have been used as a therapeutic modality for the treatment of chronic pain syndromes. Peripheral nerve stimulation has been used to treat chronic pain syndrome and incontinence, with a number of other applications under investigation. Deep brain stimulation can be used to treat a variety of diseases and disorders.

Stimulators have been developed to provide therapy for a variety of treatments. A stimulator can include a control module (with a pulse generator) and one or more stimulator electrodes. The one or more stimulator electrodes can be disposed along one or more leads, or along the control module, or both. The stimulator electrodes are in contact with or near the nerves, muscles, or other tissue to be stimulated. The pulse generator in the control module generates electrical pulses that are delivered by the electrodes to body tissue.

BRIEF SUMMARY

One aspect is a method for estimating neural activation arising from stimulation by a stimulation system. The method includes identifying a plurality of different neural elements stimulated by the stimulation; obtaining a neural response signal resulting from the stimulation by the stimulation system; and decomposing the neural response signal to estimate neural activation of each of the different neural elements.

In at least some aspects, the method further includes, for each of the different neural elements, providing at least one template signal for the neural element, wherein decomposing the neural response signal includes decomposing the neural response signal using the template signals. In at least some aspects, decomposing the neural response signal using the template signals includes determining weights for each of the template signals as portions of the neural response signal.

In at least some aspects, decomposing the neural response signal includes decomposing the neural response signal in a frequency domain. In at least some aspects, the method further includes transforming the neural response signal into

2

the frequency domain. In at least some aspects, the method further includes determining initial weights for each of the template signals using one or more frequency components in the template signals. In at least some aspects, the method further includes combining the template signals using the weights to generate a composite neural signal. In at least some aspects, the method further includes determining a difference between the neural response signal and the composite neural signal. In at least some aspects, the method further includes determining whether the difference exceeds a predetermined threshold difference and, when so, adjusting the weights.

In at least some aspects, decomposing the neural response signal includes decomposing the neural response signal in a time domain. In at least some aspects, the method further includes combining the template signals using the weights to generate a composite neural signal. In at least some aspects, determining a difference between the neural response signal and the composite neural signal. In at least some aspects, the method further includes determining whether the difference exceeds a predetermined threshold difference and, when so, adjusting the weights. In at least some aspects, the method further includes filtering the neural response signal.

Another aspect is a system for estimating neural activation arising from stimulation by a stimulation system. The system includes at least one processor configured to perform actions, including: receiving an identification of a plurality of different neural elements stimulated by the stimulation; receiving a neural response signal resulting from the stimulation by the stimulation system; and decomposing the neural response signal to estimate neural activation of each of the different neural elements. The actions further include any of the methods described above.

In at least some aspects, the actions further include, for each of the different neural elements, obtaining at least one template signal for the neural element, wherein decomposing the neural response signal includes decomposing the neural response signal using the template signals. In at least some aspects, the system further includes a display and at least one input device coupled to the at least one processor, wherein the actions further include, for each of the different neural elements, receive a selection of a type of signal to be used for the template signal.

In at least some aspects, the system further includes a display and at least one input device coupled to the at least one processor, wherein receiving the identification includes displaying a representation of one or more anatomical regions; receiving a selection by the user of one of the anatomical regions; and identifying one or more of the different neural elements based on the selection of the one of the anatomical regions.

A further aspect is a non-transitory computer-readable medium having processor-executable instructions for estimating neural activation arising from stimulation by a stimulation system, the processor-executable instructions when installed onto a device enable the device to perform actions, the actions including: receiving an identification of a plurality of different neural elements stimulated by the stimulation; receiving a neural response signal resulting from the stimulation by the stimulation system; and decomposing the neural response signal to estimate neural activation of each of the different neural elements. The actions further include any of the methods described above.

In at least some aspects, the actions further include, for each of the different neural elements, obtaining at least one template signal for the neural element, wherein decomposing

ing the neural response signal includes decomposing the neural response signal using the template signals.

BRIEF DESCRIPTION OF THE DRAWINGS

Non-limiting and non-exhaustive embodiments of the present invention are described with reference to the following drawings. In the drawings, like reference numerals refer to like parts throughout the various figures unless otherwise specified.

For a better understanding of the present invention, reference will be made to the following Detailed Description, which is to be read in association with the accompanying drawings, wherein:

FIG. 1 is a schematic view of one embodiment of an electrical stimulation system;

FIG. 2A is a schematic illustration of one embodiment of a neural response or neural signal;

FIG. 2B is a schematic illustration of another embodiment of a neural response or neural signal;

FIG. 3 is a flowchart of one embodiment of a method for estimating neural activation arising from stimulation by a stimulation system;

FIG. 4 is a flowchart of one embodiment of a method for decomposing the recorded neural response signal in the frequency domain;

FIG. 5 is a flowchart of one embodiment of a method for decomposing the recorded neural response signal in the time domain;

FIG. 6 is a schematic representation of one embodiment of a user interface for selection of anatomical regions;

FIG. 7A is a schematic representation of one embodiment of a user interface for selecting which neural signals to use for the neural elements;

FIG. 7B is a schematic representation of one embodiment of three template signals for neural elements;

FIG. 7C is a schematic representation of one embodiment of a composite signal using a weighted combination of the three template signals of FIG. 7B;

FIG. 7D is a schematic representation of one embodiment of a user interface for selecting a weighting strategy;

FIG. 8 is a schematic representation of neural signal before and after filtering;

FIG. 9 is a schematic representation of one embodiment of a user interface for selecting filters or other signal processing;

FIG. 10 is a schematic representation of one embodiment of a user interface for selecting filters or other signal processing;

FIG. 11 is a schematic representation of one embodiment of a user interface for inputting stimulation parameters;

FIG. 12 is a schematic representation of one embodiment of determined weights for a stimulation;

FIG. 13 is a schematic overview of one embodiment of components of a stimulation system, including an electronic subassembly disposed within a control module; and

FIG. 14 is a schematic block diagram of a system for practicing the methods described herein.

DETAILED DESCRIPTION

The present disclosure is directed to the area of implantable electrical stimulation systems and methods of making and using the systems. The present disclosure is also directed to methods and systems for estimating neural activation by stimulation using the implantable electrical stimulation system.

Suitable implantable electrical stimulation systems include, but are not limited to, a least one lead with one or more electrodes disposed on a distal portion of the lead and one or more terminals disposed on one or more proximal portions of the lead. Leads include, for example, percutaneous leads, paddle leads, cuff leads, or any other arrangement of electrodes on a lead. Examples of electrical stimulation systems with leads are found in, for example, U.S. Pat. Nos. 6,181,969; 6,516,227; 6,609,029; 6,609,032; 6,741,892; 7,244,150; 7,450,997; 7,672,734; 7,761,165; 7,783,359; 7,792,590; 7,809,446; 7,949,395; 7,974,706; 8,175,710; 8,224,450; 8,271,094; 8,295,944; 8,364,278; 8,391,985; and 8,688,235; and U.S. Patent Application Publication Nos. 2007/0150036; 2009/0187222; 2009/0276021; 2010/0076535; 2010/0268298; 2011/0005069; 2011/0004267; 2011/0078900; 2011/0130817; 2011/0130818; 2011/0238129; 2011/0313500; 2012/0016378; 2012/0046710; 2012/0071949; 2012/0165911; 2012/0197375; 2012/0203316; 2012/0203320; 2012/0203321; 2012/0316615; 2013/0105071; and 2013/0197602, all of which are incorporated herein by reference. In the discussion below, a percutaneous lead will be exemplified, but it will be understood that the methods and systems described herein are also applicable to paddle leads and other leads.

A percutaneous lead for electrical stimulation (for example, deep brain, spinal cord, or peripheral nerve stimulation) includes stimulation electrodes that can be ring electrodes, segmented electrodes that extend only partially around the circumference of the lead, or any other type of electrode, or any combination thereof. The segmented electrodes can be provided in sets of electrodes, with each set having electrodes circumferentially distributed about the lead at a particular longitudinal position. A set of segmented electrodes can include any suitable number of electrodes including, for example, two, three, four, or more electrodes. For illustrative purposes, the systems and leads are described herein relative to use for deep brain stimulation, but it will be understood that any of the leads can be used for applications other than deep brain stimulation, including spinal cord stimulation, peripheral nerve stimulation, dorsal root ganglion stimulation, sacral nerve stimulation, or stimulation of other nerves, muscles, and tissues.

Turning to FIG. 1, one embodiment of an electrical stimulation system 10 includes one or more stimulation leads 12 and an implantable pulse generator (IPG) 14. The system 10 can also include one or more of an external remote control (RC) 16, a clinician's programmer (CP) 18, an external trial stimulator (ETS) 20, or an external charger 22. The IPG and ETS are examples of control modules for the electrical stimulation system.

The IPG 14 is physically connected, optionally via one or more lead extensions 24, to the stimulation lead(s) 12. Each lead carries multiple electrodes 26 arranged in an array. The IPG 14 includes pulse generation circuitry that delivers electrical stimulation energy in the form of, for example, a pulsed electrical waveform (i.e., a temporal series of electrical pulses) to the electrode array 26 in accordance with a set of stimulation parameters. The implantable pulse generator can be implanted into a patient's body, for example, below the patient's clavicle area or within the patient's buttocks or abdominal cavity or at any other suitable site. The implantable pulse generator can have multiple stimulation channels which may be independently programmable to control the magnitude of the current stimulus from each channel. In some embodiments, the implantable pulse generator can have any suitable number of stimulation channels including, but not limited to, 4, 6, 8, 12, 16, 32, or more

stimulation channels. The implantable pulse generator can have one, two, three, four, or more connector ports, for receiving the terminals of the leads and/or lead extensions.

The ETS 20 may also be physically connected, optionally via the percutaneous lead extensions 28 and external cable 30, to the stimulation leads 12. The ETS 20, which may have similar pulse generation circuitry as the IPG 14, also delivers electrical stimulation energy in the form of, for example, a pulsed electrical waveform to the electrode array 26 in accordance with a set of stimulation parameters. One difference between the ETS 20 and the IPG 14 is that the ETS 20 is often a non-implantable device that is used on a trial basis after the neurostimulation leads 12 have been implanted and prior to implantation of the IPG 14, to test the responsiveness of the stimulation that is to be provided. Any functions described herein with respect to the IPG 14 can likewise be performed with respect to the ETS 20.

The RC 16 may be used to telemetrically communicate with or control the IPG 14 or ETS 20 via a uni- or bi-directional wireless communications link 32. Once the IPG 14 and neurostimulation leads 12 are implanted, the RC 16 may be used to telemetrically communicate with or control the IPG 14 via a uni- or bi-directional communications link 34. Such communication or control allows the IPG 14 to be turned on or off and to be programmed with different stimulation parameter sets. The IPG 14 may also be operated to modify the programmed stimulation parameters to actively control the characteristics of the electrical stimulation energy output by the IPG 14. The CP 18 allows a user, such as a clinician, the ability to program stimulation parameters for the IPG 14 and ETS 20 in the operating room and in follow-up sessions. Alternately, or additionally, stimulation parameters can be programmed via wireless communications (e.g., Bluetooth) between the RC 16 (or external device such as a hand-held electronic device) and the IPG 14.

The CP 18 may perform this function by indirectly communicating with the IPG 14 or ETS 20, through the RC 16, via a wireless communications link 36. Alternatively, the CP 18 may directly communicate with the IPG 14 or ETS 20 via a wireless communications link (not shown). The stimulation parameters provided by the CP 18 are also used to program the RC 16, so that the stimulation parameters can be subsequently modified by operation of the RC 16 in a stand-alone mode (i.e., without the assistance of the CP 18).

For purposes of brevity, the details of the RC 16, CP 18, ETS 20, and external charger 22 will not be further described herein. Details of exemplary embodiments of these devices are disclosed in U.S. Pat. No. 6,895,280, which is expressly incorporated herein by reference. Other examples of electrical stimulation systems can be found at U.S. Pat. Nos. 6,181,969; 6,516,227; 6,609,029; 6,609,032; 6,741,892; 7,949,395; 7,244,150; 7,672,734; and 7,761,165; 7,974,706; 8,175,710; 8,224,450; and 8,364,278; and U.S. Patent Application Publication No. 2007/0150036, as well as the other references cited above, all of which are incorporated herein by reference.

Electrodes of the lead(s) (or electrodes of a sensor or other device) can be used to sense local electrical characteristics of the environment around the lead(s) and electrodes during and between electrical pulses or waveforms (which can be, for example, therapeutic stimulation pulses or waveforms, sub-perception pulses or waveforms, sensing pulses or waveforms, or other electrical pulses or waveforms). Examples of such sensing can include the measurement, recording, or observation of an electrophysiological signal, such as an evoked potential (EP), evoked compound action

potential (ECAP), evoked resonant neural activity (ERNA), local field potential (LFP), ESG (electrospinogram), EEG (electroencephalogram), ECG (electrocardiogram), ECoG (electrocorticogram), or EMG (electromyogram) signal or the like or any combination thereof.

Neural response signals or other neural signals, including, for example, an evoked potential (EP); evoked compound action potential (ECAP); evoked resonant neural activity (ERNA); local field potential (LFP); oscillations within the EEG, ECoG, LFP, or other neural signal; or the like or any combination thereof, can reflect the summed activity of different neural elements. For example, evoked potentials can capture those neurons directly activated by electrical stimulation. Evoked potentials may also reflect the propagation of neural activity across the neural network and may reflect both local and network level activation. FIG. 2A illustrates one example of a neural response 235 or neural signal. When a neural fiber is recruited by electrical stimulation, the neural fiber, in response, will issue an action potential—that is, the neural fiber will “fire.” Should recruitment from electrical stimulation result in the neural fiber’s resting state the neural fiber will depolarize, repolarize, and hyperpolarize before coming to rest again. If electrical stimulation continues, the neural fiber will fire again at some later time. FIG. 2B illustrates one example of an evoked compound action potential (ECAP) which can be a cumulative response of neural fibers recruited and firing within a volume.

Although features of the evoked potentials or other neural response signals can provide information about the neural environment, such features typically do not reveal the type of neural fibers that are activated. As described herein, in at least some embodiments, signal decomposition can be used to, for example, determine or estimate the underlying neural populations activated by stimulation. Use of signal decomposition may assist in improving stimulation targeting procedures.

FIG. 3 illustrates one embodiment of a method for estimating neural activation arising from stimulation by a stimulation system. Such estimations may allow for estimation of which neural elements are activated or the amount of activation within a neural element population. In step 302, a user or a system specifies the types or characteristics of neural elements (for example, neural fibers, neural cells, axons, neural terminals, or other neural structures) that may be stimulated. For example, for deep brain stimulation, the specified neural elements may include anatomical structures such as the subthalamic nucleus (STN), globus pallidus interna (GPi), elements of the basal ganglia-thalamo-cortical loop (BGTC), or the like; specific neural tracts; or specific neural cells or cell groups; or the like or any combination thereof. For spinal cord stimulation, the specified neural elements may include, for example, A-beta or A-delta fibers or other specific neural cells or cell groups or neural structures or the like or any combination thereof. As another example, the different neural elements may be defined by one or more characteristics, such as, for example, the diameter, trajectory, orientation, or the like (or any combination thereof) of the neural fibers or neural cells. In at least some embodiments, the user or system designates the number of distinct neural signals that are expected in a neural response signal.

In at least some embodiments, the user can select some or all of the individual neural elements from a menu or a visual display. In at least some embodiments, the user can indirectly specify some or all of the neural elements by selecting anatomical regions, such as regions in the brain. The system

can then supply one or more specific neural elements based on the user selection of the anatomical region. In at least some embodiments, knowledge about cells, axons, terminals, or other neural structures around the lead can be used to automatically specify some or all of the neural elements.

FIG. 6 illustrates one embodiment of a user interface 660 for selection of anatomical regions 662 or neural elements. In the illustrated embodiment, the STN anatomical region 662' has been selected. In the illustrated embodiment, the thalamus, GPi, globus pallidus externa (GPe), and internal capsule (IC) are also displayed as well as a representation of a lead 612. In at least some embodiments, the user interface 660 also presents a menu 664 for selection of different types of neural signals to allow the user to select the associated neural signal based on the selected anatomical region or neural element (e.g., the STN. In the illustrated embodiment, the menu 664 includes an Evoked Potential (EP), ERNA, LFP Template 1, and LFP Template 2. Other selections may be presented on the menu 664 depending on the selected anatomical region or neural element and on available templates or signals for the anatomical region or neural element. In at least some embodiments, the user or system can select one or more of these neural signals for the neural element. In at least some embodiments, the anatomical regions may be patient-specific based, for example, on patient images. In at least some embodiments, the anatomical regions may be based on an anatomical atlas or generalized model of the brain. In at least some embodiments, the anatomical regions can be a combination of patient-specific anatomical regions and anatomical regions based on an anatomical atlas or generalized model of the brain.

In step 304, a neural response signal is then recorded or otherwise obtained or measured. In step 306, the recorded neural response signal is decomposed into constituent neural signals for the individual neural elements to identify or determine the neural populations activated by stimulation. Examples of methods for decomposing the recorded neural response signal are described below.

In at least some embodiments, the decomposition of the recorded neural response signal includes assumptions that each of the types of neural elements produce a distinctive signal and that these signals from the neural elements can arrive at different periods in time depending, for example, on the distance from the stimulation source, the threshold amount of stimulation needed to produce a response, distance from the recording arrangement or the like or any combination thereof. As an example, in at least some embodiments, each type of neural element can contribute distinctive frequency components at specific timepoints in the signal to generate a composite neural response signal.

FIG. 4 illustrates one embodiment of a method for decomposing the recorded neural response signal in the frequency domain. In step 402, the recorded neural response signal is transformed from the time domain to the frequency domain using any suitable technique, such as, for example, any suitable Fourier transform technique (e.g., a short-time Fourier transform (STFT)), or the like or any combination thereof.

In step 404, one or more neural signals (e.g., template signals) for each of the specified types of neural elements are selected, obtained, or otherwise provided. In at least some embodiments, the neural signals for each neural element are signals that have been previously recorded or extracted for those neural elements or are estimated signals generated from simulations, calculations, or models or any combination thereof.

FIG. 7A illustrates one embodiment of a user interface for selecting which neural signals to use for the neural elements. In section 772, the individual neural signals can be selected. In at least some embodiments, the selection can be made from a menu or using up/down arrows 774. In the illustrated embodiment, the STN ERNA, STN EP, and IC EP signals are selected. In optional section 776, the source for a neural signal can be selected by a user including a pre-loaded (e.g., default or stored) signal, an acquired signal, or a custom (e.g., user-provided) signal. In at least some embodiments, if the custom signal is selected, a prompt appears asking the user to upload the custom signal in an appropriate format (e.g., a .dat format). In at least some embodiments, the user or system may select a portion of the neural signal to use in the composite signal. FIG. 7B illustrates examples of neural signals 775 that can be used as templates for the selected neural signals.

In at least some embodiments, the system may send a warning to a user if two or more of the selected neural signals are of different time lengths or are too similar (which may indicate, for example, that the same neural signal has been selected twice).

Returning to step 404 of FIG. 4, the selected neural signals are transformed (if not already transformed) into the frequency domain. These neural signals can be combined into a composite neural signal using individual weights for each of the neural elements to reflect the strength of the signal expected for the population of the specific neural elements. The combined neural signals form an estimated neural signal. The weights can be relative weights (for example, relative to a weight of 1 for one of the neural signals), absolute weights, or weights that sum to 100 (e.g., 100 percent) or 1 or any other suitable number. The combination, and associated weighting, can utilize linear or non-linear models or combinations.

In at least some embodiments, the distinct frequencies for the neural signal(s) from each neural element may be used to create an a priori estimate of the initial weight for each neural element or neural signal. In at least some embodiments, the user or the system may provide an initial estimate of the weight for each of the neural elements. As an example, in the user interface of FIG. 7A, in section 778 of the user interface the user can select the initial relative weights for each of the signals. In at least some embodiments, the initial estimate of the weights can be based on, for example, literature sources, clinician experience, any other suitable source, or the like or any combination thereof. In at least some embodiments, the system may perform an initial weight estimate using any suitable technique including, but not limited to, least squares fitting, generalized linear model (GLM) regression, other regression techniques, QR factorization, machine learning techniques (for example, fuzzy logic, neural networks, k-nearest neighbor (KNN) techniques, density-based unsupervised clustering, Gaussian mixture models, support vector machine-based supervised methods, hierarchical clustering, or the like), coordinate descent, gradient descent, or the like or any combination thereof.

In at least some embodiments, the system may alert a user if neural signals from two or more of the neural elements have known covariance that exceeds or meets a threshold amount. In other embodiments, the system may alter or select weights based on the known covariance.

FIG. 7D illustrates another embodiment of a user interface 779 that may be provided in addition to, or as an alternative to, section 778 of FIG. 7A. The user interface 779 of FIG. 7D allow the user to select an initial weight for the

neural signals that is equal, preset/unequal, or preset/custom. The “preset, unequal” selection in FIG. 7D may be useful when it is known that activation of a certain neural element will intrinsically produce a larger signal than activation of another neural element (for example, due to more of the first neural element than the second or a larger intrinsic response.) If the “preset, custom” selection in FIG. 7D is made, the user can be prompted to enter weights for one or more of the neural signals. In at least some embodiments, if a weight is not entered for the neural signal, a default value (for example, 0, 1, or 100) is used.

In at least some embodiments, the system can filter the neural response signal or the neural signal(s) for each neural element or any combination thereof. In at least some embodiments, the same filters is applied to both the neural response signal and the individual neural signals. The filtering can be based on, for example, lead impedance, device measurement settings (for example, sampling rate or sample averaging), or the like or any combination thereof. In at least some embodiments, the user can set the filter(s). The filters can include, for example, hardware/analog filters, amplifier gain level, artifact blanking settings, least mean square (LMS) artifact cancellation filters, adaptive filters, or digital FIR filters, or the like or any combination thereof.

FIGS. 8 and 9 illustrate filtering or other signal processing of the recorded response signal or the neural signal(s) for the individual neural elements. In FIG. 8, the acquired response or selected neural signal **880** is illustrated along with a filtered signal **882** obtained by filtering the signal **880**.

FIG. 9 illustrates one embodiment of a user interface **990** for selecting filters or other signal processing. Examples of filters and other signal processing include, but are not limited to, an artifact filter, a noise filter, lead encapsulation/environmental scaling, and template signal properties. The artifact filter can be used, for example, to remove any artifact arising from the stimulation signal that generates the neural response. The artifact filter may include user input such as the pulse width, amplitude, type of stimulation (e.g., biphasic, monophasic, or the like), and the type of filter. The noise filter can be a low pass, high pass, or bandpass filter and may include a user- or system-selected high pass frequency or a user- or system-selected low pass frequency, as appropriate for the type of filter. The lead encapsulation/environmental scaling may account for tissue differences near the lead, such as an encapsulation layer adjacent to the lead, and may provide fixed or frequency-dependent scaling.

The recorded neural response signal may also be filtered based on the properties of the other neural signals such as, for example, sampling rate, sampling duration, or the like or any combination thereof. It will be understood that the filtering or other signal processing can be applied to the recorded neural response signal or the other neural signals or any combination thereof. In at least some embodiments, the same filtering or other signal processing may be applied to both the recorded neural response signal and the other neural signals.

In at least some embodiments, the user may input the lead implant site or estimated distance(s) between the lead and the neural elements. In at least some embodiments, the system may estimate the distance between the lead and the neural elements based on the lead implant site. The system may use the distance information to modify the expected amplitude or other features of any of the neural signal(s) from the individual neural elements.

FIG. 10 illustrates an example of a user interface **1095** with illustrates a lead **1012** and anatomical structures **1062**. The user interface also includes a stimulation field model

(SFM) that is calculated based on stimulation parameters (for example, electrode selection, amplitude, pulse width, pulse duration, or the like or any combination thereof) and illustrates the estimated volume of activation (VOA) of tissue that will be activated by the stimulation. Examples of the SFM or VOA, as well as methods and systems for determining the SFM or VOA, can be found at U.S. Pat. Nos. 8,326,433; 8,379,952; 8,649,845; 8,675,945; 8,831,731; 8,849,632; 8,855,773; 8,913,804; 8,918,183; 8,958,615; 9,026,317; 9,050,470; 9,072,905; 9,081,488; 9,084,896; 9,135,400; 9,227,074; 9,235,685; 9,254,387; 9,272,153; 9,302,110; 9,308,372; 9,310,985; 9,364,665; 9,526,902; 9,586,053; 9,792,412; 9,821,167; 9,925,382; and 9,959,940; U.S. Patent Application Publications Nos. 2009/0287272; 2009/0287273; 2012/0314924; 2013/0116744; 2014/0122379; 2015/0066111; 2016/0375248; 2016/0375258; and 2017/0304633; U.S. patent application Ser. Nos. 15/706,004; 15/864,876; and Ser. No. 15/937,264; and U.S. Provisional Patent Application Ser. Nos. 62/030,655 and 62/532,869, all of which are incorporated herein by reference in their entireties.

In at least some embodiments, the user or system may provide or input stimulation settings such as electrode selection, stimulation rate, stimulation duration, pulse width, amplitude, or the like or any combination thereof. The system may use the stimulation settings to adjust the neural signals that arise in response to the stimulation, for example, if those neural signals are known to be sensitive or dependent on one or more of those stimulation settings. FIG. 11 illustrates one embodiment of a user interface **1196** for inputting stimulation parameters such as amplitude, pulse width (PW), or pulse rate.

In step **406**, the difference between the recorded neural response signal and the estimated neural signal is determined. The difference can be determined using any suitable technique such as, for example, mean squared error, a binned mean squared error, mean rectified error, statistical analyze of features of the signal (for example, comparing a mean and standard deviation of a signal feature from template signals versus the mean and standard deviation for the feature of the recorded signal, or the like or any combination thereof. In at least some embodiments, the feasibility, fitness, or robustness of the determined weights can be compared versus a predictor model that can be based on expected physiological models or the like. If the determined weights are not within a threshold difference from the predictor model, the system may alert the user.

In step **408**, the system determines whether the difference is acceptable or not. For example, the system may determine whether the difference meets or exceeds a threshold amount and, if so, whether the difference is unacceptable. If the difference is acceptable, the process ends. FIG. 12 illustrates one example of determined weights for a stimulation: 60% STN, 30% Thalamus, and 10% IC.

If the difference is not acceptable, the weights are adjusted in step **410** and the process returns to step **404**. In at least some embodiments, the weight adjustment may be requested from the user. In at least some embodiments, the system may perform the weight adjustment using any suitable technique including, but not limited to, least squares fitting, generalize linear model (GLM) regression, other regression techniques, QR factorization, machine learning techniques (for example, fuzzy logic, neural networks, k-nearest neighbor (KNN) techniques, density-based unsupervised clustering, Gaussian mixture models, support vector machine-based supervised methods, hierarchical clustering, or the like or any combination thereof), coordinate descent, gradient descent, or the

like or any combination thereof. The process can continue until acceptable weights are found or the system or user halts the process.

FIG. 5 illustrates one embodiment of a method for decomposing the recorded signal in the time domain. In step 502, template signals for each of the specified types of neural elements are selected. FIG. 7B illustrates examples of neural signals 775 that can be used as templates for the selected neural signals. In at least some embodiments, the template signals for each neural element are signals that have been previously recorded or extracted for those neural elements or are estimated signals generated from simulations, calculations, or models or any combination thereof. The same considerations and options described above with respect to the method illustrated in FIG. 4 are applicable to the method illustrated in FIG. 5, including all of the considerations and options illustrated in FIG. 7A to FIG. 12.

In step 504, weights for the template signals are determined from the recorded neural signal. The system performs a weight determination using any suitable technique including, but not limited to, least squares fitting, generalized linear model (GLM) regression, other regression techniques, QR factorization, machine learning techniques (for example, fuzzy logic, neural networks, k-nearest neighbor (KNN) techniques, density-based unsupervised clustering, Gaussian mixture models, support vector machine-based supervised methods, hierarchical clustering, or the like), coordinate descent, gradient descent, or the like or any combination thereof. FIG. 7C illustrates a composite signal 777 of the three template signals of FIG. 7B combined using weights (for example, 10% of S_1 , 30% of S_2 , and 60% of S_3), as described in more detail below.

In at least some embodiments, the process ends with step 504. In other embodiments, the resulting composite signal may be compared with the neural response signal or a predicted or estimated neural signal. In at least some other embodiments, the user or the system may provide a predicted estimate of the weight for each of the neural elements using, for example, literature sources, clinician experience, any other suitable source, or the like or any combination thereof. In at least some embodiments, the feasibility, fitness, or robustness of the determined weights can be compared versus a predictor model that can be based on expected physiological models or the like.

In optional step 506, the difference between the recorded neural response signal and composite signal generated using the estimated or predicted weights (or the predicted or estimated neural signal) is determined. The difference can be determined using any suitable technique such as, for example, mean squared error, a binned mean squared error, mean rectified error, statistical analysis of features of the signal (for example, comparing a mean and standard deviation of a signal feature from template signals versus the mean and standard deviation for the feature of the recorded signal, or the like or any combination thereof).

In optional step 508, the system determines whether the difference is acceptable or not. For example, the system may determine whether the difference meets or exceeds a threshold amount and, if so, the difference is unacceptable. For example, in at least some embodiments, if the determined weights are not within a threshold difference from the predictor model, the system may alert the user. If the difference is acceptable, the process ends.

If the difference is not acceptable, the weights are adjusted or recalculated in optional step 510 and the process returns to step 506. In at least some embodiments, the weight adjustment may be requested from the user. In at least some

embodiments, the system may perform the weight adjustment using any suitable technique including, but not limited to, least squares fitting, generalized linear model (GLM) regression, other regression techniques, QR factorization, machine learning techniques (for example, fuzzy logic, neural networks, k-nearest neighbor (KNN) techniques, density-based unsupervised clustering, Gaussian mixture models, support vector machine-based supervised methods, hierarchical clustering, or the like), coordinate descent, gradient descent, or the like or any combination thereof. The process can continue until acceptable weights are found or the system or user halts the process.

It will be understood that the methods illustrated in FIGS. 4 and 5 can be modified to apply to either time domain or frequency domain methods or any combination thereof. It will be understood that each block of the flowchart illustration, and combinations of blocks in the flowchart illustration and methods disclosed herein, can be implemented by computer program instructions. These program instructions may be provided to a processor to produce a machine, such that the instructions, which execute on the processor, create means for implementing the actions specified in the flowchart block or blocks disclosed herein. The computer program instructions may be executed by a processor to cause a series of operational steps to be performed by the processor to produce a computer implemented process. The computer program instructions may also cause at least some of the operational steps to be performed in parallel. Moreover, some of the steps may also be performed across more than one processor, such as might arise in a multi-processor computing device. In addition, one or more processes may also be performed concurrently with other processes, or even in a different sequence than illustrated without departing from the scope or spirit of the invention.

The computer program instructions can be stored on any suitable computer-readable medium including, but not limited to, RAM, ROM, EEPROM, flash memory or other memory technology, CD-ROM, digital versatile disks ("DVD") or other optical storage, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, cloud-based storage, or any other medium which can be used to store the desired information and which can be accessed by a computing device.

FIG. 13 is a schematic overview of one embodiment of components of an electrical stimulation system 1300 including an electronic subassembly 1358 disposed within a control module. The electronic subassembly 1358 may include one or more components of the IPG. It will be understood that the electrical stimulation system can include more, fewer, or different components and can have a variety of different configurations including those configurations disclosed in the stimulator references cited herein.

Some of the components (for example, a power source 1312, an antenna 1318, a receiver 1302, and a processor 1304) of the electrical stimulation system can be positioned on one or more circuit boards or similar carriers within a sealed housing of an implantable pulse generator (see e.g., 14 in FIG. 1), if desired. Any power source 1312 can be used including, for example, a battery such as a primary battery or a rechargeable battery. Examples of other power sources include super capacitors, nuclear or atomic batteries, mechanical resonators, infrared collectors, thermally-powered energy sources, flexural powered energy sources, bio-energy power sources, fuel cells, bioelectric cells, osmotic pressure pumps, and the like including the power sources described in U.S. Pat. No. 7,437,193, incorporated herein by reference.

13

As another alternative, power can be supplied by an external power source through inductive coupling via the optional antenna **1318** or a secondary antenna. In at least some embodiments, the antenna **1318** (or the secondary antenna) is implemented using the auxiliary electrically-conductive conductor. The external power source can be in a device that is mounted on the skin of the user or in a unit that is provided near the user on a permanent or periodic basis.

If the power source **1312** is a rechargeable battery, the battery may be recharged using the optional antenna **1318**, if desired. Power can be provided to the battery for recharging by inductively coupling the battery through the antenna to a recharging unit **1316** external to the user. Examples of such arrangements can be found in the references identified above. The electronic subassembly **1358** and, optionally, the power source **1312** can be disposed within a control module (e.g., the IPG **14** or the ETS **20** of FIG. **1**).

In one embodiment, electrical stimulation signals are emitted by the electrodes **26** to stimulate nerve fibers, muscle fibers, or other body tissues near the electrical stimulation system. The processor **1304** is generally included to control the timing and electrical characteristics of the electrical stimulation system. For example, the processor **1304** can, if desired, control one or more of the timing, frequency, strength, duration, and waveform of the pulses. In addition, the processor **1304** can select which electrodes can be used to provide stimulation, if desired. In some embodiments, the processor **1304** selects which electrode(s) are cathodes and which electrode(s) are anodes. In some embodiments, the processor **1304** is used to identify which electrodes provide the most useful stimulation of the desired tissue.

Any processor can be used and can be as simple as an electronic device that, for example, produces pulses at a regular interval or the processor can be capable of receiving and interpreting instructions from an external programming unit **1308** that, for example, allows modification of pulse characteristics. In the illustrated embodiment, the processor **1304** is coupled to a receiver **1302** which, in turn, is coupled to the optional antenna **1318**. This allows the processor **1304** to receive instructions from an external source to, for example, direct the pulse characteristics and the selection of electrodes, if desired.

In one embodiment, the antenna **1318** is capable of receiving signals (e.g., RF signals) from an external telemetry unit **1306** which is programmed by the programming unit **1308**. The programming unit **1308** can be external to, or part of, the telemetry unit **1306**. The telemetry unit **1306** can be a device that is worn on the skin of the user or can be carried by the user and can have a form similar to a pager, cellular phone, or remote control, if desired. As another alternative, the telemetry unit **1306** may not be worn or carried by the user but may only be available at a home station or at a clinician's office. The programming unit **1308** can be any unit that can provide information to the telemetry unit **1306** for transmission to the electrical stimulation system **1300**. The programming unit **1308** can be part of the telemetry unit **1306** or can provide signals or information to the telemetry unit **1306** via a wireless or wired connection. One example of a suitable programming unit is a computer operated by the user or clinician to send signals to the telemetry unit **1306**.

The signals sent to the processor **1304** via the antenna **1318** and the receiver **1302** can be used to modify or otherwise direct the operation of the electrical stimulation system. For example, the signals may be used to modify the

14

pulses of the electrical stimulation system such as modifying one or more of pulse duration, pulse frequency, pulse waveform, and pulse strength. The signals may also direct the electrical stimulation system **1300** to cease operation, to start operation, to start charging the battery, or to stop charging the battery. In other embodiments, the stimulation system does not include the antenna **1318** or receiver **1302** and the processor **1304** operates as programmed.

Optionally, the electrical stimulation system **1300** may include a transmitter (not shown) coupled to the processor **1304** and the antenna **1318** for transmitting signals back to the telemetry unit **1306** or another unit capable of receiving the signals. For example, the electrical stimulation system **1300** may transmit signals indicating whether the electrical stimulation system **1300** is operating properly or not or indicating when the battery needs to be charged or the level of charge remaining in the battery. The processor **1304** may also be capable of transmitting information about the pulse characteristics so that a user or clinician can determine or verify the characteristics.

FIG. **14** illustrates one embodiment of a system for practicing any of the methods described herein. The system can include a computer **1400** or any other similar device that includes at least one processor **1402** and a memory **1404**, a display **1406**, an input device **1408**, and, optionally, the electrical stimulation system **1412**.

The computer **1400** can be a laptop computer, desktop computer, tablet, mobile device, smartphone, or other devices that can run applications or programs, or any other suitable device for processing information and for presenting a user interface. The computer can be, for example, the CP **18** or RC **16** of FIG. **1** or the programming unit **1308** of FIG. **13**. The computer **1400** can be local to the user or can include components that are non-local to the user including one or both of the processor **1402** or memory **1404** (or portions thereof). For example, in some embodiments, the user may operate a terminal that is connected to a non-local computer. In other embodiments, the memory can be non-local to the user. As another example, the computer **1400** may utilize or communicate with a processor in the control module **1414** (such as the IPG **14** or ETS **20** of FIG. **1**).

The computer **1400** can utilize any suitable processor **1402** including one or more hardware processors that may be local to the user or non-local to the user or other components of the computer. The processor **1402** is configured to execute instructions provided to the processor, as described below.

Any suitable memory **1404** can be used for the processor **1402**. The memory **1404** illustrates a type of computer-readable media, namely computer-readable storage media. Computer-readable storage media may include, but is not limited to, nonvolatile, non-transitory, removable, and non-removable media implemented in any method or technology for storage of information, such as computer readable instructions, data structures, program modules, or other data. Examples of computer-readable storage media include RAM, ROM, EEPROM, flash memory, or other memory technology, CD-ROM, digital versatile disks ("DVD") or other optical storage, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, or any other medium which can be used to store the desired information and which can be accessed by a computer.

Communication methods provide another type of computer readable media; namely communication media. Communication media typically embodies computer-readable instructions, data structures, program modules, or other data in a modulated data signal such as a carrier wave, data

15

signal, or other transport mechanism and include any information delivery media. The terms “modulated data signal,” and “carrier-wave signal” includes a signal that has one or more of its characteristics set or changed in such a manner as to encode information, instructions, data, and the like, in the signal. By way of example, communication media includes wired media such as twisted pair, coaxial cable, fiber optics, wave guides, and other wired media and wireless media such as acoustic, RF, infrared, and other wireless media.

The display **1406** can be any suitable display device, such as a monitor, screen, display, or the like, and can include a printer. The input device **1408** can be, for example, a keyboard, mouse, touch screen, track ball, joystick, voice recognition system, or any combination thereof, or the like and can be used by the user to interact with a user interface or clinical effects map.

The electrical stimulation system **1412** can include, for example, a control module **1414** (for example, the IPG **14** or ETS **20** of FIG. 1) and a lead **1416** (for example, the lead **12** illustrated in FIG. 1.) The electrical stimulation system **1412** may communicate with the computer **1400** through a wired or wireless connection or, alternatively or additionally, a user can provide information between the electrical stimulation system **1412** and the computer **1400** using a computer-readable medium or by some other mechanism. In some embodiments, the computer **1400** may include part of the electrical stimulation system. In at least some embodiments, the computer **1400** can program the control module **1414** for delivery of stimulation pulses, charge recovery pulse, charge recovery phases, or the like or any combination thereof.

The above specification and examples provide a description of the manufacture and use of the invention. Since many embodiments of the invention can be made without departing from the spirit and scope of the invention, the invention also resides in the claims hereinafter appended.

What is claimed as new and desired to be protected by Letters Patent of the United States is:

1. A method for estimating neural activation arising from deep brain stimulation by a stimulation system, the method comprising:

- identifying a plurality of different anatomical structures of a brain stimulated by the deep brain stimulation;
- for each of the different anatomical structures of the brain, providing at least one template signal for the anatomical structure of the brain;
- obtaining a neural response signal resulting from the deep brain stimulation by the stimulation system;
- decomposing the neural response signal in a time domain into a plurality of decomposed signals using the template signals to estimate neural activation of each of the different anatomical structures of the brain, wherein decomposing the neural response signal comprises decomposing the neural response signal using the template signals, wherein decomposing the neural response signal comprises determining weights for each of the template signals as portions of the neural response signal;
- combining the template signals using the weights to generate a composite neural signal; and
- using the estimated neural activations of each of the different anatomical structures of the brain to adjust stimulation settings of the stimulation system.

2. The method of claim 1, further comprising determining a difference between the neural response signal and the composite neural signal.

16

3. The method of claim 2, further comprising determining when the difference exceeds a predetermined threshold difference and, when so, adjusting the weights.

4. The method of claim 1, further comprising filtering the neural response signal.

5. The method of claim 1, wherein the plurality of different anatomical structures of the brain comprises at least one of the thalamus, subthalamic nucleus, globus pallidus interna, globus pallidus externa, or internal capsule.

6. The method of claim 1, further comprising displaying a representation of at least a portion of the brain and receiving selections by a user from the representation of the plurality of different anatomical structures of the brain for deep brain stimulation.

7. The method of claim 1, further comprising, for each of the different anatomical structures of the brain, receiving a selection of a type of signal to be used for the template signal.

8. A method for estimating neural activation arising from deep brain stimulation by a stimulation system, the method comprising:

- identifying a plurality of different anatomical structures of a brain stimulated by the deep brain stimulation;
- for each of the different anatomical structures of the brain, providing at least one template signal for the anatomical structure of the brain;
- determining initial weights for each of the template signals using one or more distinctive frequency components in the template signals;
- obtaining a neural response signal resulting from the deep brain stimulation by the stimulation system;
- transforming the neural response signal into a frequency domain;
- decomposing the neural response signal in the frequency domain into a plurality of decomposed signals using the template signals to estimate neural activation of each of the different anatomical structures of the brain, wherein decomposing the neural response signal comprises determining weights for each of the template signals as portions of the neural response signal; and
- using the estimated neural activations of each of the different anatomical structures of the brain to adjust stimulation settings of the stimulation system.

9. The method of claim 8, further comprising displaying a representation of at least a portion of the brain and receiving selections by a user from the representation of the plurality of different anatomical structures of the brain for deep brain stimulation.

10. The method of claim 8, further comprising, for each of the different anatomical structures of the brain, receiving a selection of a type of signal to be used for the template signal.

11. The method of claim 8, further comprising filtering the neural response signal.

12. The method of claim 8, wherein the plurality of different anatomical structures of the brain comprises at least one of the thalamus, subthalamic nucleus, globus pallidus interna, globus pallidus externa, or internal capsule.

13. The method of claim 8, further comprising combining the template signals using the weights to generate a composite neural signal.

14. A method for estimating neural activation arising from deep brain stimulation by a stimulation system, the method comprising:

- identifying a plurality of different anatomical structures of a brain stimulated by the deep brain stimulation;

17

for each of the different anatomical structures of the brain,
 providing at least one template signal for the anatomical
 structure of the brain;
 obtaining a neural response signal resulting from the deep
 brain stimulation by the stimulation system;
 transforming the neural response signal into the frequency
 domain;
 decomposing the neural response signal in the frequency
 domain into a plurality of decomposed signals using the
 template signals to estimate neural activation of each of
 the different anatomical structures of the brain, wherein
 decomposing the neural response signal comprises
 determining weights for each of the template signals as
 portions of the neural response signal;
 combining the template signals using the weights to
 generate a composite neural signal; and
 using the estimated neural activations of each of the
 different anatomical structures of the brain to adjust
 stimulation settings of the stimulation system.

15. The method of claim **14**, further comprising deter-
 mining a difference between the neural response signal and
 the composite neural signal.

18

16. The method of claim **15**, further comprising deter-
 mining when the difference exceeds a predetermined thresh-
 old difference and, when so, adjusting the weights.

17. The method of claim **14**, further comprising display-
 ing a representation of at least a portion of the brain and
 receiving selections by a user from the representation of the
 plurality of different anatomical structures of the brain for
 deep brain stimulation.

18. The method of claim **14**, further comprising, for each
 of the different anatomical structures of the brain, receiving
 a selection of a type of signal to be used for the template
 signal.

19. The method of claim **14**, further comprising filtering
 the neural response signal.

20. The method of claim **14**, wherein the plurality of
 different anatomical structures of the brain comprises at least
 one of the thalamus, subthalamic nucleus, globus pallidus
 interna, globus pallidus externa, or internal capsule.

* * * * *