

(12) **United States Patent**
Welch et al.

(10) **Patent No.:** **US 12,397,129 B2**
(45) **Date of Patent:** **Aug. 26, 2025**

(54) **CORONARY GUIDE CATHETER**

(56) **References Cited**

(71) Applicant: **NorMedix, Inc.**, Eden Prairie, MN
(US)

U.S. PATENT DOCUMENTS

(72) Inventors: **Jeffrey M. Welch**, Maple Grove, MN
(US); **Gregg Stuart Sutton**, Maple
Grove, MN (US)

4,493,329 A 1/1985 Crawford et al.
4,737,153 A * 4/1988 Shimamura A61M 16/0425
138/131

(Continued)

(73) Assignee: **NorMedix, Inc.**, Eden Prairie, MN
(US)

FOREIGN PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 187 days.

CA 2994262 C 9/2023
EP 0810003 A2 12/1997

(Continued)

OTHER PUBLICATIONS

(21) Appl. No.: **17/668,725**

“U.S. Appl. No. 15/224,323, Appeal Brief filed Feb. 15, 2021”, 22
pgs.

(22) Filed: **Feb. 10, 2022**

(Continued)

(65) **Prior Publication Data**

US 2022/0233810 A1 Jul. 28, 2022

Primary Examiner — Bradley J Osinski

(74) *Attorney, Agent, or Firm* — Schwegman Lundberg &
Woessner, P.A.

Related U.S. Application Data

(63) Continuation of application No. 15/224,323, filed on
Jul. 29, 2016, now abandoned.
(Continued)

(51) **Int. Cl.**

A61M 25/00 (2006.01)

A61M 25/06 (2006.01)

(52) **U.S. Cl.**

CPC **A61M 25/005** (2013.01); **A61M 25/0045**
(2013.01); **A61M 25/0041** (2013.01); **A61M**
25/0662 (2013.01)

(58) **Field of Classification Search**

CPC A61M 25/005; A61M 25/0041; A61M
25/0045; A61M 25/0662; A61M
2025/0681; A61M 2025/0047


See application file for complete search history.

(57)

ABSTRACT

Embodiments include an interventional guide catheter, com-
prising: a main tubular shaft with a distal tip and proximal
end; the main tubular shaft comprising: a main inner struc-
tural layer comprising a metallic helically wound multi-filar
wire extending from a proximal tube termination to a distal
end, a braided wire layer covering the main inner structural
layer that extends from the proximal tube termination to the
distal end, an outer layer of polymer jacketing fixedly
attached to the main inner structural layer and braid layer, an
inner layer of polymer jacketing and fixedly attached to the
main inner structural layer, a distal tip made of layers of
polymer, a distal end curve shape for anatomical confor-
mance that is heat processed in the main metal portion of the
structure; and a lamination of the inner layer, main inner
structural layer, braided wire layer and outer layer. Other
embodiments are also included herein.

12 Claims, 5 Drawing Sheets

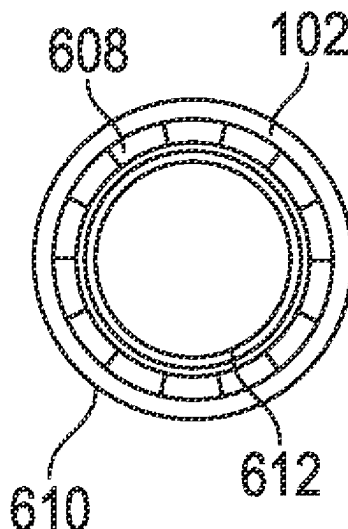

Related U.S. Application Data

- (60) Provisional application No. 62/199,050, filed on Jul. 30, 2015.

References Cited

U.S. PATENT DOCUMENTS

5,106,363	A	4/1992	Nobuyoshi	7,955,313	B2	6/2011	Boismier
5,472,435	A	12/1995	Sutton	7,968,038	B2	6/2011	Dittman et al.
5,558,652	A	9/1996	Henke	8,021,352	B2	9/2011	Slazas et al.
5,573,522	A	11/1996	Houser et al.	8,034,045	B1	10/2011	Lyons
5,658,264	A	8/1997	Samson	8,070,898	B2	12/2011	Eversull et al.
5,695,483	A	12/1997	Samson	8,100,881	B2	1/2012	Hoffa
5,755,704	A	5/1998	Lunn	8,114,144	B2	2/2012	Chow et al.
5,795,341	A	8/1998	Samson	8,142,415	B2	3/2012	Warnock, Jr. et al.
5,846,229	A *	12/1998	Berg A61M 25/0041	8,157,790	B2	4/2012	Kubo
			604/528	8,182,466	B2	5/2012	Stehr et al.
5,853,400	A	12/1998	Samson	8,206,373	B2	6/2012	Zhou
5,876,386	A	3/1999	Samson	8,251,976	B2	8/2012	Zhou
5,891,112	A	4/1999	Samson	8,257,314	B2	9/2012	Agnew
5,891,114	A	4/1999	Chien et al.	8,317,772	B2	11/2012	Jansen et al.
5,947,940	A *	9/1999	Beisel A61M 25/005	8,343,136	B2	1/2013	Howat et al.
			604/526	8,348,925	B2	1/2013	Fischell et al.
5,951,929	A	9/1999	Wilson et al.	8,366,699	B2	2/2013	Jimenez
5,957,910	A	9/1999	Holden, II et al.	8,377,035	B2	2/2013	Zhou et al.
6,042,578	A	3/2000	Dinh et al.	8,431,057	B2	4/2013	Guo et al.
6,053,903	A	4/2000	Samson	8,475,431	B2	7/2013	Howat
6,053,904	A	4/2000	Scribner et al.	8,486,048	B2	7/2013	Kubo et al.
6,103,037	A	8/2000	Wilson	8,529,719	B2	9/2013	Pingleton et al.
6,143,013	A	11/2000	Samson et al.	8,535,293	B2	9/2013	Faherty et al.
6,152,911	A	11/2000	Giannoble	8,535,294	B2	9/2013	Fischell et al.
6,165,163	A	12/2000	Chien et al.	8,540,695	B2	9/2013	Shimogami et al.
6,217,565	B1	4/2001	Cohen	8,591,495	B2	11/2013	Fischell et al.
6,355,027	B1	3/2002	Le et al.	8,636,270	B2	1/2014	Ostrovsky
6,368,316	B1	4/2002	Jansen et al.	8,647,323	B2 *	2/2014	Guo A61M 25/0043
6,374,476	B1	4/2002	Ponzi et al.				604/527
6,451,005	B1	9/2002	Saitou	8,696,699	B2	4/2014	Chomas et al.
6,464,684	B1	10/2002	Galdonik	8,702,679	B2	4/2014	Deckman et al.
6,562,022	B2	5/2003	Hoste et al.	8,702,680	B2	4/2014	Jimenez et al.
6,589,227	B2	7/2003	Sonderskov	8,708,997	B2	4/2014	Parker
6,616,651	B1	9/2003	Stevens	8,721,625	B2	5/2014	Klint
6,626,889	B1	9/2003	Simpson et al.	8,758,326	B2	6/2014	Hennissy
6,629,952	B1	10/2003	Chien et al.	8,858,530	B2	10/2014	Nishigishi et al.
6,635,047	B2	10/2003	Forsberg	8,864,744	B2	10/2014	Howat et al.
6,689,120	B1 *	2/2004	Gerdt A61M 25/005	8,926,560	B2	1/2015	Dinh et al.
			604/526	8,986,284	B2	3/2015	Kuwada et al.
6,702,972	B1	3/2004	Markle	9,114,229	B2	8/2015	Fuentes
6,709,429	B1	3/2004	Schaefer et al.	9,254,374	B2	2/2016	Thorstenenson et al.
6,740,073	B1	5/2004	Saville	9,259,550	B2	2/2016	Schaeffer
6,824,553	B1	11/2004	Samson et al.	9,259,813	B2	2/2016	Heideman
6,866,660	B2	3/2005	Garabedian et al.	9,278,191	B2	3/2016	Nihonmatsu et al.
6,942,654	B1	9/2005	Schaefer et al.	2002/0068899	A1	6/2002	James, Jr. et al.
7,018,372	B2	3/2006	Casey et al.	2002/0095102	A1	7/2002	Winters
7,025,758	B2	4/2006	Klint	2003/0009184	A1	1/2003	Pepin
7,104,979	B2	9/2006	Jansen et al.	2003/0191451	A1	10/2003	Gilmartin
7,117,703	B2	10/2006	Kato et al.	2004/0092844	A1	5/2004	Johnson et al.
7,331,948	B2	2/2008	Skarda	2005/0043713	A1	2/2005	Zhou
7,354,428	B1	4/2008	Gosiengfiao et al.	2005/0090802	A1	4/2005	Connors, III et al.
7,455,739	B2	11/2008	Zhou	2006/0095050	A1 *	5/2006	Hartley A61M 25/0662
7,507,229	B2	3/2009	Hewitt et al.				606/108
7,534,317	B2	5/2009	Brustad et al.	2006/0111649	A1	5/2006	Zhou
7,597,830	B2	10/2009	Zhou	2007/0233040	A1	10/2007	Macnamara et al.
7,615,043	B2	11/2009	Zhou	2010/0217235	A1	8/2010	Thorstenenson et al.
7,637,902	B2	12/2009	Eversull et al.	2012/0109078	A1	5/2012	Schaeffer
7,674,239	B2	3/2010	Sisken et al.	2012/0130217	A1	5/2012	Kauphusman et al.
7,704,245	B2	4/2010	Dittman et al.	2012/0172798	A1	7/2012	Miller et al.
7,713,259	B2	5/2010	Gosiengfiao et al.	2012/0277729	A1	11/2012	Melsheimer
7,744,587	B2	6/2010	Murphy	2013/0018318	A1	1/2013	Ravichandran et al.
7,763,012	B2	7/2010	Petrack et al.	2013/0197481	A1	8/2013	Guo et al.
7,815,762	B2	10/2010	Lentz et al.	2013/0255062	A1	10/2013	Howat
7,824,392	B2	11/2010	Zhou	2013/0289697	A1	10/2013	Baker et al.
7,833,218	B2	11/2010	Lunn et al.	2014/0046138	A1	2/2014	Merk et al.
7,850,623	B2	12/2010	Griffin et al.	2014/0214006	A1	7/2014	Hiroshige et al.
7,909,779	B2	3/2011	Shimogami et al.	2014/0236124	A1	8/2014	Miyata
7,909,812	B2	3/2011	Jansen	2014/0330253	A1	11/2014	Weiss
7,914,515	B2	3/2011	Heideman et al.	2014/0352871	A1	12/2014	Wang et al.
				2015/0051541	A1	2/2015	Kanemasa et al.
				2015/0119859	A1	4/2015	Cajamarca et al.
				2015/0174363	A1	6/2015	Sutermeister et al.
				2015/0217083	A1	8/2015	Richter et al.
				2015/0231360	A1	8/2015	Watanabe et al.
				2015/0258306	A1	9/2015	Plassman et al.
				2015/0335857	A1	11/2015	Ishikawa
				2016/0001040	A1	1/2016	Yamaguchi et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0121075 A1 5/2016 Schaeffer
 2017/0028167 A1 2/2017 Welch et al.

FOREIGN PATENT DOCUMENTS

EP 2687254 A1 1/2014
 EP 3328476 B1 12/2019
 JP H09506541 A 6/1997
 JP 2005537877 A 12/2005
 JP 2018522704 A 8/2018
 WO WO-0166176 A1 9/2001
 WO WO-2006031874 A1 3/2006
 WO WO-2014210427 A1 12/2014
 WO WO-2017020012 A1 2/2017

OTHER PUBLICATIONS

"U.S. Appl. No. 15/224,323, Appeal Decision mailed Dec. 10, 2021", 9 pgs.
 "U.S. Appl. No. 15/224,323, Examiners Answer mailed Mar. 19, 2021", 7 pgs.
 "U.S. Appl. No. 15/224,323, Final Office Action mailed Jun. 7, 2019", 13 pgs.
 "U.S. Appl. No. 15/224,323, Final Office Action mailed Jul. 14, 2020", 14 pgs.
 "U.S. Appl. No. 15/224,323, Non Final Office Action mailed Jan. 8, 2020", 14 pgs.
 "U.S. Appl. No. 15/224,323, Non Final Office Action mailed Mar. 26, 2018", 14 pgs.
 "U.S. Appl. No. 15/224,323, Non Final Office Action mailed Nov. 23, 2018", 13 pgs.
 "U.S. Appl. No. 15/224,323, Reply Brief mailed May 19, 2022", 9 pgs.
 "U.S. Appl. No. 15/224,323, Response filed Jun. 8, 2020 to Non Final Office Action mailed Jan. 8, 2020", 14 pgs.

"U.S. Appl. No. 15/224,323, Response filed Dec. 9, 2019 to Final Office Action mailed Jun. 7, 2019", 15 pgs.

"U.S. Appl. No. 15/224,323, Response to Non Final Office Action mailed Mar. 26, 2018 filed Sep. 26, 2018", 13 pgs.

"U.S. Appl. No. 15/224,323, Response to Non Final Office Action mailed Nov. 23, 2018 filed Mar. 25, 2019", 11 pgs.

"Canadian Application Serial No. 2,994,262, Examiner's Rule 86(2) Requisition mailed Aug. 24, 2022", 6 pgs.

"Canadian Application Serial No. 2,994,262, Response filed Dec. 23, 2022 to Examiner's Rule 86(2) Requisition mailed Aug. 24, 2022", 38 pgs.

"European Application Serial No. 16748030.0, Communication Pursuant to Article 94(3) EPC mailed Nov. 28, 2018", 7 pgs.

"European Application Serial No. 16748030.0, Response filed Apr. 5, 2019 to Communication Pursuant to Article 94(3) EPC mailed Nov. 28, 2018", 35 pgs.

"European Application Serial No. 16748030.0, Response filed Oct. 1, 2018 to Communication Pursuant to Rules 161(1) and 162 EPC mailed Mar. 20, 2018", 22 pgs.

"International Application Serial No. PCT/US2016/044881, International Preliminary Report on Patentability mailed Feb. 8, 2018", 9 pgs.

"International Application Serial No. PCT/US2016/044881, International Search Report mailed Nov. 18, 2016", 6 pgs.

"International Application Serial No. PCT/US2016/044881, Written Opinion mailed Nov. 18, 2016", 7 pgs.

"Japanese Application Serial No. 2018-525532, Notification of Reasons for Refusal mailed Jul. 7, 2020", with English translation, 17 pages.

"Japanese Application Serial No. 2018-525532, Office Action mailed Feb. 9, 2021", with English translation, 14 pages.

"Japanese Application Serial No. 2018-525532, Response filed Jan. 6, 2021 to Notification of Reasons for Refusal mailed Jul. 7, 2020", with English claims, 7 pages.

"Japanese Application Serial No. 2018-525532, Response filed Aug. 6, 2021 to Office Action mailed Feb. 9, 2021", w/ English claims, 7 pgs.

* cited by examiner

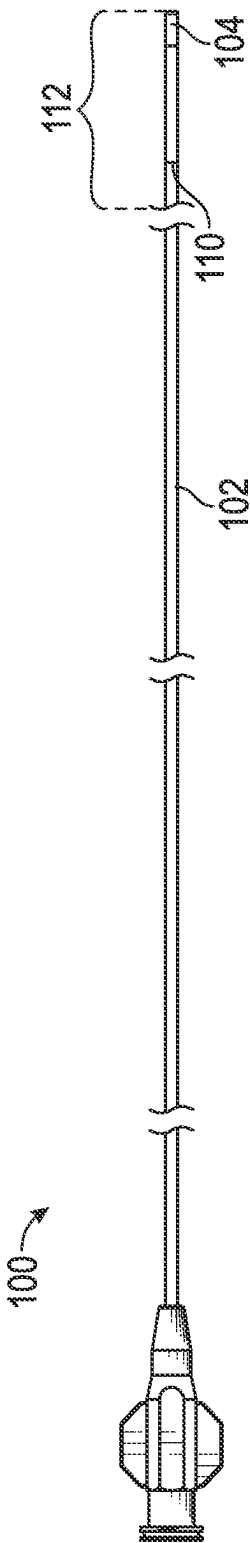


FIG. 1

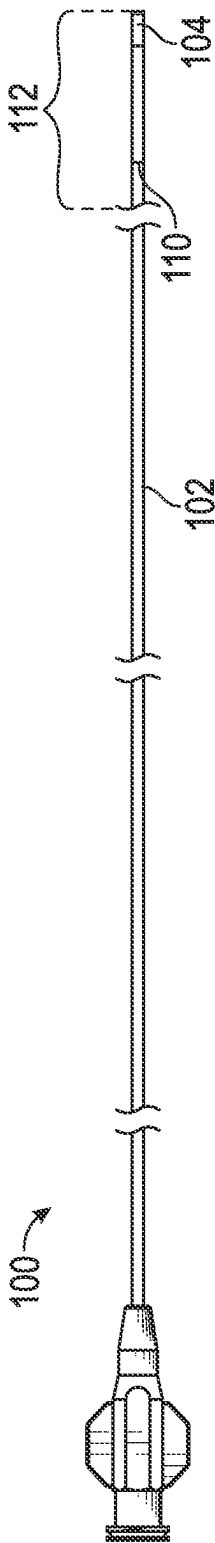


FIG. 2

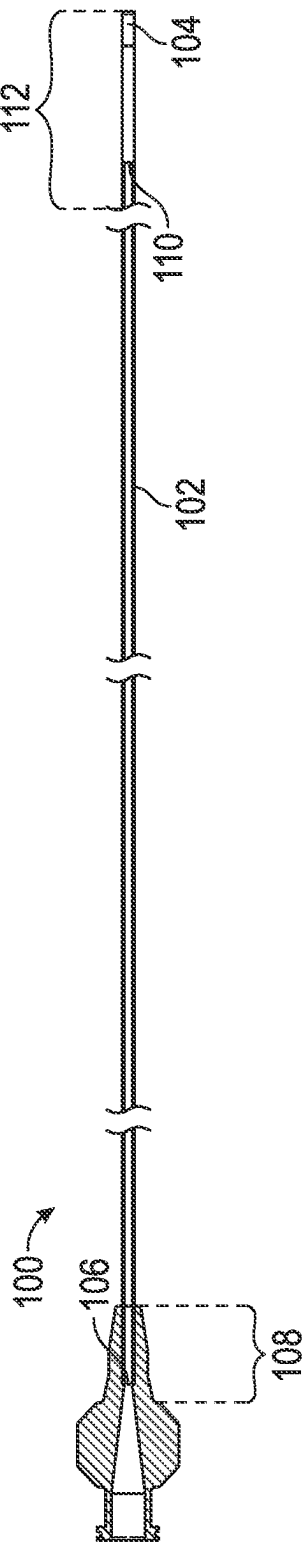


FIG. 3

100

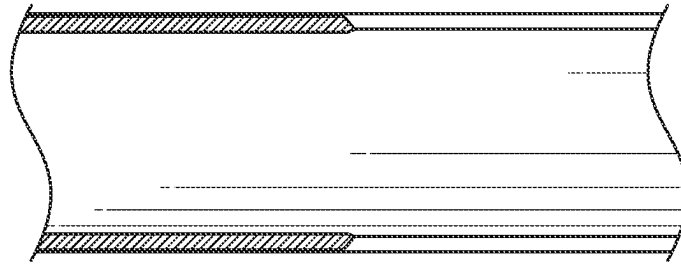


FIG. 4

100

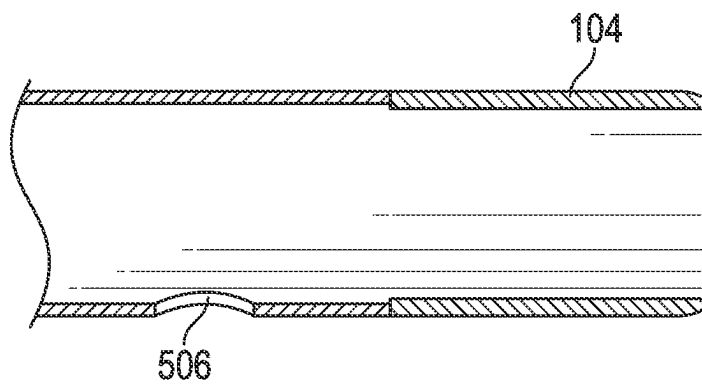


FIG. 5

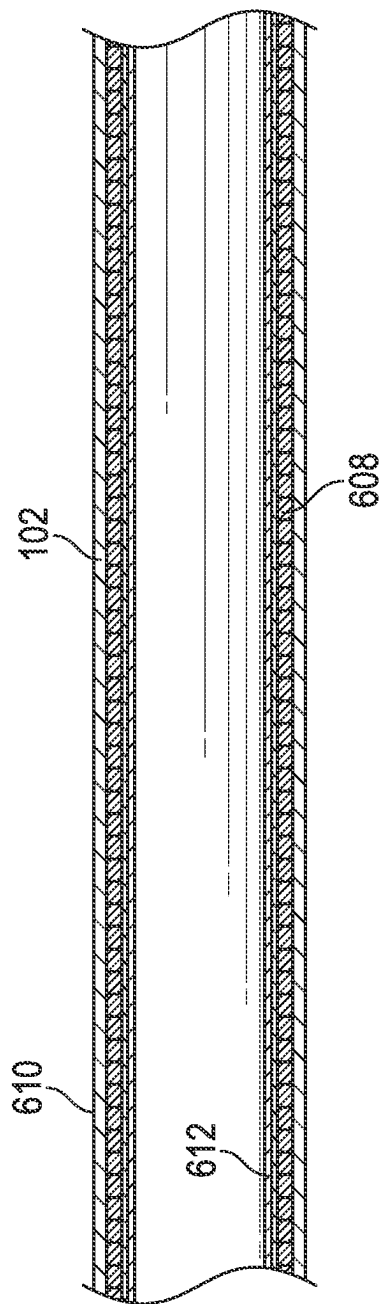


FIG. 6

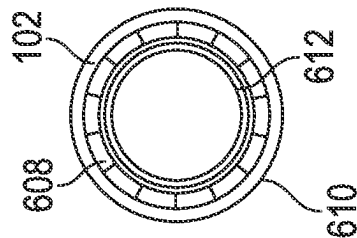


FIG. 7

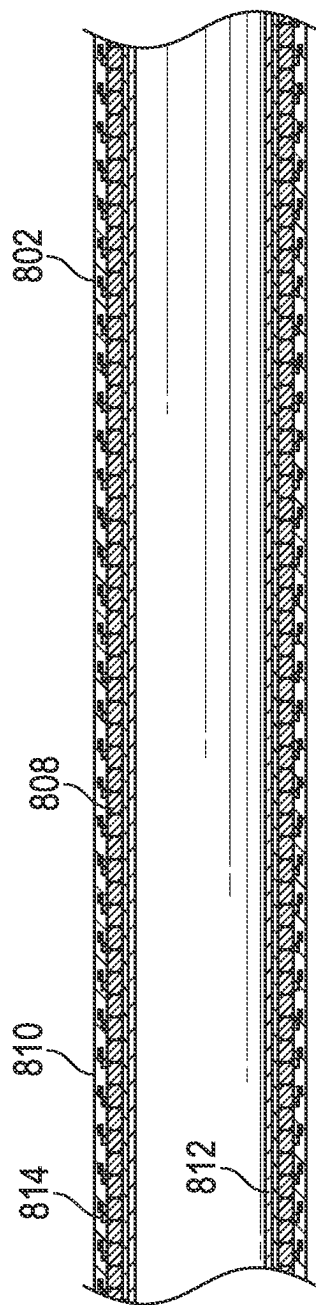


FIG. 8

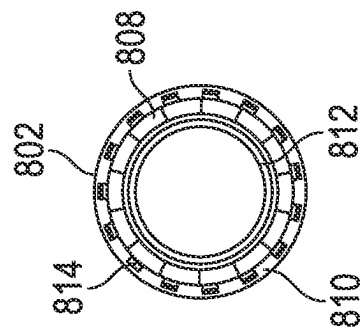


FIG. 9

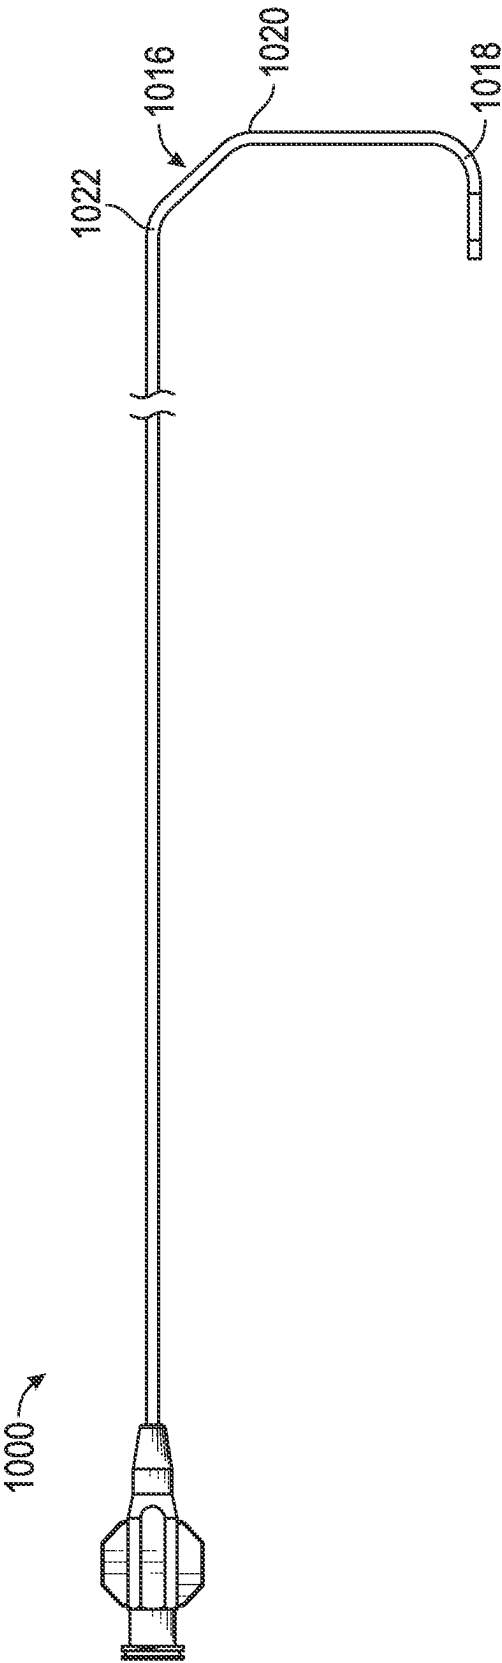


FIG. 10

CORONARY GUIDE CATHETER

CLAIM OF PRIORITY

This application is a continuation of U.S. patent application Ser. No. 15/224,323, filed Jul. 29, 2016, which application claims the benefit of priority to U.S. Provisional Patent Application Ser. No. 62/199,050, filed Jul. 30, 2015, the contents of which are hereby incorporated by reference in their entireties.

FIELD OF THE TECHNOLOGY

The present application relates to coronary guide catheters. More specifically, the present application relates to guide catheters that are used to introduce therapeutic catheters, such as stent delivery systems.

BACKGROUND

Interventional guide catheters are used by physicians to place catheters, electrode leads and other therapeutic interventional devices to desired locations in the patient's body. The guide catheter provides support for device advancement (stents, balloons, etc.) for instance, to the coronary arteries. It is the main conduit for therapeutic device and guide wire transport and provides a means for injecting contrast media. Guide catheters typically have a pre-shaped distal end that is configured to allow access and direction into the arterial branches. In coronary guide catheters, the distal end shapes also provide back-up support for device placement by using shapes made to "back-up" against aortic anatomy.

Guide catheters are made so that the distal shapes as much as possible, retain their shape during the procedure and don't soften in body temperature to any significant or detrimental degree. Guide catheters with distal end shapes also are typically made to provide end-to-end torque to allow "steering" the distal end into the artery. In addition, guide catheter are typically made to be relatively stiff so that there is no stretching and biasing during device passage. To achieve these performance criteria, current guide catheter construction means are usually polymer based with metallic wire braid reinforcement.

The problems associated with current interventional guide catheters include softening at body temperature thereby losing critical performance features like back-up support or torsion. In addition, guide catheters have been prone to kinking, buckling, ovaling and stretching, especially in long procedures or difficult, more tortuous anatomy.

SUMMARY

Embodiments disclosed herein include an interventional guide catheter for introducing interventional catheters into the vasculature, comprising: a main tubular shaft with a distal tip and proximal end; the main tubular shaft comprising: a main inner structural layer comprising a metallic helically wound multi-filar wire (wall thickness (0.0015-0.010")) extending from a proximal tube termination to the distal end, a braided wire layer (0.0005-0.010" thick) covering the metallic helically wound multi-filar layer that extends from the proximal tube termination to the distal end, an outer layer of polymer jacketing covering and fixedly attached to the main metal structure and braid layer with wall thickness of 0.001-0.005", an inner layer of polymer jacketing covering and fixedly attached to the inner metal structure with wall thickness of 0.001-0.0005", a distal tip

made of layers of polymer, the distal tip being 0.05-0.20" in length, an optional distal end curve shape for anatomical conformance that is heat processed in the main metal portion (e.g., one or more of the multi-filar layer, braid or the like) of the structure; and a lamination of the inner layer, metallic helically wound multi-filar layer, braid and outer layer that optionally does not comprise fusion of the outer and inner layers. The main metal portion is separately heat processed (e.g., to provide the distal end curve shape) prior to lamination in one example. In another example, the main metal portion is heat processed while incorporated with the other components of the catheter (e.g., the inner and outer layers, or the like).

In an embodiment, the main helically wound multi-filar layer terminates distally before the primary curve of the distal end. In another embodiment, the main helically wound layer terminates proximal to the distal end curve shape including the primary curve.

In an embodiment, the outer and inner layers are fused together through the main coil structure and braid.

In an embodiment, the metal helically wound multi-filar layer comprises stainless steel.

In an embodiment, the braid layer comprises stainless steel wire.

In an embodiment, the multi-filar structure comprises at least 6 filars and not more than 20 filars.

In an embodiment, the multi-filar structure wire has been swaged.

In an embodiment, the outer diameter of the main tubular shaft is at least 0.060 inches and not more than 0.115 inches.

In an embodiment, the outer layer comprises Pebax.

In an embodiment, the outer layer comprises nylon.

In an embodiment, the outer layer is coated with a hydrophilic polymer.

In an embodiment, the inner layer comprises PTFE.

In an embodiment, the inner layer comprises nylon.

In an embodiment, the inner layer is coated with a hydrophilic polymer.

In an embodiment, the distal tip comprises a PTFE inner layer and a Pebax outer layer.

In an embodiment, the metallic helically wound layer comprises welded terminations.

In an embodiment, the metallic helically wound layer comprises a distal end that comprises a gold coating.

In an embodiment, the gold coating is at least 0.5 mm and not more than 2 mm in length.

In an embodiment, the outer layer comprises at least two layers of Pebax.

In an embodiment, the outer layer is heat shrinkable to allow it to be formed tightly onto the metallic helically wound layer.

In an embodiment, the metallic helically wound wire has a rectangular cross-section.

In an embodiment, the metallic helically wound wire has a circular cross-section.

In an embodiment, the metallic helically wound layer wire has an oval or elliptical cross-section.

In an embodiment, the metallic helically wound layer wire has been coated with PTFE coating prior to forming into the multi-filar configuration.

In an embodiment, the main tubular shaft length is at least 60 cm and not more than 200 cm long.

This summary is an overview of some of the teachings of the present application and is not intended to be an exclusive or exhaustive treatment of the present subject matter. Further details are found in the detailed description and appended claims. Other aspects will be apparent to persons skilled in

3

the art upon reading and understanding the following detailed description and viewing the drawings that form a part thereof, each of which is not to be taken in a limiting sense. The scope of the present application is defined by the appended claims and their legal equivalents.

BRIEF DESCRIPTION OF THE FIGURES

The technology may be more completely understood in connection with the following drawings, in which:

FIG. 1 is a front view of a guide catheter, according to an embodiment.

FIG. 2 is a back view of a guide catheter, according to an embodiment.

FIG. 3 is a cross-section view of a guide catheter, according to an embodiment.

FIG. 4 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 5 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 6 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 7 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 8 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 9 is a cross-section view of a portion of a guide catheter, according to an embodiment.

FIG. 10 is a front view of a guide catheter, according to an embodiment.

While the technology is susceptible to various modifications and alternative forms, specifics thereof have been shown by way of example and drawings, and will be described in detail. It should be understood, however, that the application is not limited to the particular embodiments described. On the contrary, the application is to cover modifications, equivalents, and alternatives falling within the spirit and scope of the technology.

DETAILED DESCRIPTION

The embodiments of the present technology described herein are not intended to be exhaustive or to limit the technology to the precise forms disclosed in the following detailed description. Rather, the embodiments are chosen and described so that others skilled in the art can appreciate and understand the principles and practices of the present technology.

All publications and patents mentioned herein are hereby incorporated by reference. The publications and patents disclosed herein are provided solely for their disclosure. Nothing herein is to be construed as an admission that the inventors are not entitled to antedate any publication and/or patent, including any publication and/or patent cited herein.

The guide catheter as described herein can solve the problems associated with current guide catheter technology by providing a novel design, construction and materials.

The guide catheter, described herein, can be used in interventional cases where significant arterial tortuosity is encountered such as using a radial artery access or using a femoral approach on an obese patient.

In various embodiments, the guide catheter can include a composite built tube that can be fabricated using a specially wound metal inner layer and jacketed with very thin layers of polymer inside and out. The metallic inner layer can be made using a multi-filar (6-20 filars) helically wound wire structure. In some embodiments, the helical structure can be

4

swaged, such that each individual wire strand is partially rectangular in cross-section and therefore can result in a very tight/close fitting wire matrix. The helical structure can also be made using a non-swaged, round, square or rectangular wire.

In various embodiments, the wall thickness of the inner metal structure can range from 1.5 to 10 thousandths of an inch thick.

The helically wound metal structure can improve the mechanical integrity of the catheter tube, such as compared to current guide catheters with respect to kinking, buckling, flexibility, radial strength, and maintaining circularity of the catheter lumen cross-section.

This marked improvement can be achieved by the significant increase in the amount of metal in the catheter. For instance, current guide catheters that are composite built or wire braid reinforced have total cross-sectional metallic component in the range of 5-10%. The guide catheter as described herein can have a total cross-sectional metallic component of 40-60%. The transmission of mechanical energy through this significantly higher modulus composite can result in significantly higher performance.

The guide catheter of this invention also comprises an outer polymer layer and an inner polymer layer. In an embodiment, the outer polymer layer and the inner polymer layer can include one or more polymers, such as PTFE, Pebax, or Polyurethane. The polymer layers can be attached to the metal structure by thermal polymer heat-shrinking or reflow. The resultant wall thickness of the polymer layers can range from 0.5 to 3.0 thousandths of an inch for each layer.

In various embodiments, the guide catheter can include a pre-shaped curve, such as a curved distal end region. The guide catheter can attain the pre-shaped curve configuration by heat-setting the metal in this portion of the catheter. The result can include a curve that retains its shape in body temperature and over time does not substantially soften, such as soften enough to unintentionally change shape.

The guide catheter can further include a soft (low durometer) polymer distal tip, various distal curve shapes, a radiopaque distal marker band, and a proximal luer adapter. The guide catheter range in sizes from 4F to 8F and in lengths from 80 to 125 cm.

In reference now to the figures, FIG. 1 shows a front view of a guide catheter 100, according to an embodiment. FIG. 2 shows a back view of the guide catheter 100. FIG. 3 shows a cross-sectional view of the guide catheter 100. In an embodiment, the guide catheter 100 can be configured for introducing interventional catheters into the vasculature of a patient.

In an embodiment, the catheter 100 can include a main tubular shaft 102 with a distal tip 104 and proximal end 106. The distal tip 104 can be on the opposite end of the tubular shaft 102 from the proximal end 106. The distal tip 104 can include at least one layer of polymer. In an embodiment, the distal tip 104 includes at least two layers of polymer. In an embodiment, the distal tip 104 can include an inner layer and an outer layer. In an embodiment, the inner layer of the distal tip 104 can include PTFE. In an embodiment, the outer layer of the distal tip 104 can include Pebax.

In an embodiment, the distal tip 104 can be at least 0.05 inches long. In an embodiment, the distal tip 104 can be at least 0.02 inches long. In an embodiment, the distal tip 104 can be 0.2 inches long or shorter. In an embodiment, the distal tip 104 can be 0.5 inches long or shorter. In various embodiments, the tubular shaft 102 can include a main inner structural layer.

The main inner structural layer can include a metallic helically wound multi-filar wire extending from a proximal tube termination (e.g., the proximal shaft end **106** or proximal shaft portion **108**) to a distal end **112** including at least the bracketed **112** shown in FIGS. 1-3 (e.g., at the distal location). The main inner structural layer can further include a braided wire layer. In various embodiments, the braided wire layer can cover at least a portion of the outer portion (opposite from the inner lumen) of the metallic helically wound multi-filar layer that extends from the proximal tube termination to the distal end. In other embodiments, the braided wire layer is within the metallic helically wound multi-filar layer.

In various embodiments, the main tubular shaft **102** can include an outer layer. The outer layer can include a polymer. The outer layer can jacket, coat, or cover the outer surface of the main inner structural layer. The outer layer can be fixedly attached to the main inner structural layer.

In various embodiments, the main tubular shaft **102** can include an inner layer. The inner layer can include a polymer. The inner layer can jacket, coat, or cover the inner surface of the main inner structural layer. The inner layer can be fixedly attached to the main inner structural layer.

The main tubular shaft **102** can include a curve, such as on the distal end (shown in FIG. **10**). The curve shape can be configured for anatomical conformance. The shape can be heat processed in the main tubular shaft **102**, such as in the main inner structural layer or another metal portion. In an embodiment, the helically wound multi-filar layer terminates distally prior to the curve of the distal end. In another embodiment the helically wound multi-filar layer terminates proximal a primary curve of the curve (e.g., of the distal end curve shape) and distal to other portions of the curve including, but not limited to secondary and tertiary curves.

In various embodiments, the metallic helically wound multi-filar layer, and the braid can be laminated by the inner layer and the outer layer, such that the lamination does not fuse the outer layer and the inner layer together.

In an embodiment, the main tubular shaft **102** can be at least 60 cm long and not longer than 200 cm. In an embodiment, the main tubular shaft **102** can be at least 10 cm long and not longer than 300 cm. In an embodiment, the main tubular shaft **102** can be at least 30 cm long and not longer than 250 cm. In an embodiment, the main tubular shaft **102** can be at least 50 cm long and not longer than 225 cm.

In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.060 inches and not more than 0.115 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.060 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.040 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.050 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.070 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of at least 0.080 inches.

In an embodiment, the main tubular shaft **102** can have an outer diameter of no greater than 0.115 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of no greater than 0.095 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of no greater than 0.105 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of no greater than 0.125 inches. In an embodiment, the main tubular shaft **102** can have an outer diameter of no greater than 0.135 inches.

FIG. **4** and FIG. **5** show cross-section views of portions of a guide catheter **100**, according to various embodiments. FIG. **5** shows a cross-section of a portion of the distal tip **104**. As seen in FIG. **5**, the guide catheter **100** can define one or more apertures **506**. In various embodiments, the main tubular shaft **102** can define an aperture **506**. In an embodiment, the distal tip **104** can define an aperture **506**.

FIG. **6** shows a cross-section view of a portion of the main tubular shaft **102**, according to an embodiment. FIG. **7** shows a cross-section view from the end of the main tubular shaft **102**. In an embodiment, the main tubular shaft **102**, can include a main inner structural layer **608**. The main inner structural layer **608** can include a metallic helically wound multi-filar wire. In various embodiments, the metallic helically wound multi-filar wire can include stainless steel. In various embodiments, the metallic helically wound multi-filar wire can be swaged.

In various embodiments, the metallic helically wound multi-filar wire can include at least 6 filars and not more than 20 filars. In various embodiments, the metallic helically wound multi-filar wire can include at least 4 filars and not more than 24 filars. In various embodiments, the metallic helically wound multi-filar wire can include at least 8 filars and not more than 18 filars. In various embodiments, the metallic helically wound wire can have a rectangular cross-section, a circular cross-section, an oval cross-section or an elliptical cross-section. In various embodiments, the metallic helically wound wire can have been substantially coated with PTFE coating prior to forming into the multi-filar configuration.

In an embodiment, the main inner structural layer **608** can include welded terminations. In an embodiment, the main inner structural layer **608** can include a distal end that includes a gold coating. In various embodiments, the gold coating can range from 0.5 mm thick to 2 mm in length. In various embodiments, the gold coating can range from 0.4 mm thick to 2.5 mm in length. In various embodiments, the gold coating can range from 0.25 mm thick to 3 mm in length.

In an embodiment, the main inner structural layer **608** can have a thickness that can range from 0.0015 inches to 0.010 inches (e.g., one or more of a consistent thickness or variable thicknesses). In an embodiment, the main inner structural layer **608** can have a thickness of at least 0.0010 inches. In an embodiment, the main inner structural layer **608** can have a thickness of at least 0.0005 inches. In an embodiment, the main inner structural layer **608** can have a thickness of no greater than 0.015 inches. In an embodiment, the main inner structural layer **608** can have a thickness of no greater than 0.020 inches. Optionally, the main inner structural layer **608** includes a varying wall thickness. For instance, the metallic helically wound multi-filar wire is ground so that portions of the layer have varying thickness. The catheter, in some examples includes corresponding reduced diameter based on the grinding of the metallic helically wound multi-filar wire. In still another example, the metallic helically wound multi-filar wire is formed with a varied diameter (e.g., is necked) to accordingly decrease the thickness of the main inner structural layer **608**. In one example, a proximal portion of the main inner structural layer **608** includes a greater thickness relative to a distal portion to enhance pushability of the catheter. In another example, the distal portion of the main inner structural layer **608** has a lesser thickness than the proximal portion to facilitate bending and corresponding navigation through tortuous vasculature. In an embodiment, the main tubular shaft **102** can include an outer layer **610**. The outer layer **610** can include a polymer. The outer layer

610 can jacket or cover at least a portion of the outer portion of the main inner structural layer **608**. In an embodiment, the outer layer **610** can be at least 0.001 inches thick and not more than 0.005 inches thick. In an embodiment, the outer layer **610** can be at least 0.0007 inches thick. In an embodiment, the outer layer **610** can be at least 0.0005 inches thick. In an embodiment, the outer layer **610** can be no more than 0.007 inches thick. In an embodiment, the outer layer can be no more than 0.01 inches thick.

In an embodiment, the outer layer **610** can include Pebax. In an embodiment, the outer layer **610** can include nylon. In an embodiment, the outer layer **610** can be coated with a hydrophilic polymer. In an embodiment, the outer layer **610** can include at least two layers. In an embodiment, each of the two layers included in the outer layer **610** can include Pebax. In various embodiments, the outer layer **610** can be heat shrinkable, such as to allow the outer layer **610** to be formed tightly onto the main inner structural layer **608**.

In an embodiment, the main tubular shaft **102** can include an inner layer **612**. The inner layer **612** can include a polymer. The inner layer **612** can jacket or cover at least a portion of the inner portion of the main inner structural layer **608**. In an embodiment, the inner layer **612** can be at least 0.001 inches thick and not more than 0.005 inches thick. In an embodiment, the inner layer **612** can be at least 0.0007 inches thick. In an embodiment, the inner layer **612** can be at least 0.0005 inches thick. In an embodiment, the inner layer **612** can be no more than 0.007 inches thick. In an embodiment, the inner layer can be no more than 0.01 inches thick.

In an embodiment, the inner layer **612** can include PTFE. In an embodiment, the inner layer **612** can include nylon. In an embodiment, the inner layer **612** can be coated with a hydrophilic polymer.

In an embodiment, the outer layer **610** and the inner layer **612** can be fused together, such as through the main inner structural layer **608** and/or the braid **814** (shown in FIG. 8).

FIG. 8 shows a cross-section view of a portion of the main tubular shaft **802**, according to an embodiment. FIG. 9 shows a cross-section view from the end of the main tubular shaft **802**.

In various embodiments, the main tubular shaft **802** can include a braided wire layer **814**. In an embodiment, the braided wire layer **814** can be disposed between the main inner structural layer **808** and the outer layer **810**. In an embodiment, the braided wire layer **814** can be disposed within a portion of the outer layer **810**. In another embodiment, the braided wire layer **814** is provided within the main inner structural layer **808** (e.g., along the interior of the layer **808**). Optionally, the braided wire layer **814** is between the inner layer **812** and the main inner structural layer **808**.

The braided wire layer **814** can cover at least a portion of the main inner structural layer **808**, such as the helically wound multi-filar layer. In an embodiment, the braided wire can include stainless steel.

In an embodiment, the braided wire layer **814** can be at least 0.0005 inches thick and not more than 0.010 inches thick. In an embodiment, the braided wire layer **814** can be at least 0.005 inches thick and not more than 0.010 inches thick.

In an embodiment, the braided wire layer **814** can be at least 0.0004 inches thick. In an embodiment, the braided wire layer **814** can be at least 0.0003 inches thick. In an embodiment, the braided wire layer **814** can be no more than 0.015 inches thick. In an embodiment, the braided wire layer **814** can be no more than 0.020 inches thick.

FIG. 10 shows a front view of a guide catheter **1000**, according to an embodiment. In an embodiment, the guide catheter **1000** can include a distal end curve **1016**. The distal end curve **1016** can be configured for anatomical conformance. The distal end curve **1016** can be heat processed in the metal portion of the catheter **1000**. In an embodiment, the main helically wound layer can terminate distally before a primary curve (e.g., one or more of curves **1018**, **1020**, **1022** or the like) of the distal end **112**.

In various embodiments, the guide catheter can include a pre-shaped curve, such as a curved distal end region. The guide catheter can attain the pre-shaped curve configuration by heat-setting the metal in this portion of the catheter. The result can include a curve that retains its shape in body temperature and over time does not substantially soften, such as soften enough to unintentionally change shape.

It should be noted that, as used in this specification and the appended claims, the singular forms “a,” “an,” and “the” include plural referents unless the content clearly dictates otherwise. Thus, for example, reference to a composition containing “a compound” includes a mixture of two or more compounds. It should also be noted that the term “or” is generally employed in its sense including “and/or” unless the content clearly dictates otherwise.

It should also be noted that, as used in this specification and the appended claims, the phrase “configured” describes a system, apparatus, or other structure that is constructed or configured to perform a particular task or adopt a particular configuration to. The phrase “configured” can be used interchangeably with other similar phrases such as arranged and configured, constructed and arranged, constructed, manufactured and arranged, and the like.

All publications and patent applications in this specification are indicative of the level of ordinary skill in the art to which this technology pertains. All publications and patent applications are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated by reference.

The technology has been described with reference to various specific and preferred embodiments and techniques. However, it should be understood that many variations and modifications may be made while remaining within the spirit and scope of the technology.

What is claimed is:

1. An interventional guide catheter for introducing interventional catheters into vasculature, comprising:

a main tubular shaft extending between a proximal end and a distal end having a distal tip, the main tubular shaft including a catheter lumen configured for introducing catheters through the distal tip;

wherein the main tubular shaft includes a sidewall having: an outer layer;

an inner layer extending around the catheter lumen;

a metal main inner structural layer including metal interposed between the outer and inner layer; and

a braided wire layer surrounding the metal main inner structural layer, the braided wire layer within the outer layer; and

wherein the outer layer, inner layer, metal main inner structural layer and the braided wire layer are a laminate, and the outer layer and inner layer are isolated from each other by layers consisting of one or more of the metal main inner structural layer or the braided wire layer.

2. The interventional guide catheter of claim 1, wherein the outer layer and inner layer isolated from each other includes the outer layer and inner layer are not fused.

9

3. The interventional guide catheter of claim 2, wherein the main inner structural layer includes a helically wound multi-filar wire.

4. The interventional guide catheter of claim 3, wherein the sidewall has a sidewall thickness including:

an outer layer component thickness of around 0.001 to 0.005 inches;

an inner layer component thickness of around 0.0005 to 0.0007 inches; and

a main inner structural layer component thickness of around 0.0015 to 0.010 inches.

5. The interventional guide catheter of claim 4, wherein the braided wire layer has a braided wire layer thickness of around 0.0005 to 0.010 inches.

6. The interventional guide catheter of claim 5, wherein the braided wire layer thickness is around 0.005 to 0.010 inches.

7. The interventional guide catheter of claim 5, wherein the helically wound multi-filar wire includes distal and proximal edges, and the proximal edges of windings of the

10

helically wound multi-filar wire are engaged with distal edges of proximate windings of the helically wound multi-filar wire.

8. The interventional guide catheter of claim 7, wherein the distal end includes a curve, and the main inner structural layer is absent from the curve of the distal end.

9. The interventional guide catheter of claim 7, wherein the distal end includes a curve, and the main inner structural layer is present in the curve of the distal end.

10. The interventional guide catheter of claim 7, wherein the helically wound multi-filar wire includes a swaged, round, square or rectangular cross-section.

11. The interventional guide catheter of claim 10, wherein a cross section of the main tubular shaft includes a cross-sectional metallic component of around 40 to 60 percent.

12. The interventional guide catheter of claim 11, wherein the braided wire layer includes a cross-sectional metallic component of around 5 to 10 percent of the cross section of the main tubular shaft.

* * * * *