

(12) **United States Design Patent** (10) **Patent No.:** **US D1,091,833 S**
Childress (45) **Date of Patent:** **** Sep. 2, 2025**

(54) **EPIDERMAL ANCHOR**

(71) Applicant: **Christopher Childress**, Bradenton, FL
(US)

(72) Inventor: **Christopher Childress**, Bradenton, FL
(US)

(**) Term: **15 Years**

(21) Appl. No.: **29/898,221**

(22) Filed: **Jul. 25, 2023**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/128; D24/189**

(58) **Field of Classification Search**
USPC D24/100, 107, 185, 186, 187, 188, 209,
D24/210
CPC A61M 25/02; A61M 2025/0206; A61M
2025/0213; A61M 2025/0246; A61M
2025/0253; A61M 2025/0266; A61M
2025/0286; A61M 2209/088; A61F
13/0253; A61F 5/443; A61F 13/82; A61F
13/0246; A61F 13/00995
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D256,162 S * 7/1980 Haerr D24/189
D296,006 S * 5/1988 Asche D24/189
5,604,976 A * 2/1997 Stobie A61N 1/02
264/263
6,571,395 B1 * 6/2003 Korkor A41D 13/1245
2/45
D511,004 S * 10/2005 Masuda D24/187
D555,788 S * 11/2007 Southwell D24/128
D558,882 S * 1/2008 Brady D24/187
D588,274 S * 3/2009 Dent D24/189
D747,455 S * 1/2016 Uematsu D24/100
D932,638 S * 10/2021 McDonough D24/187

D994,894 S * 8/2023 Zhang D24/200
D1,056,229 S * 12/2024 MacGilp D24/209
2007/0071799 A1 * 3/2007 Tacklind A61M 25/02
424/448

FOREIGN PATENT DOCUMENTS

TH 144427 * 12/2015

OTHER PUBLICATIONS

“JFHNMLW: Foley Catheter Stabilization Device.” Found online
Feb. 12, 2025 at amazon.com. Reference dated Jun. 13, 2024.
Retrieved from <https://www.amazon.com/dp/B0D6XTBNLG/>.
“DiaBelt: Peritoneal Dialysis PD Catheter Holder Adhesive Patch.”
Found online Feb. 12, 2025 at amazon.com. Reference dated Jul. 30,
2022. Retrieved from <https://www.amazon.com/Peritoneal-Dialysis-Stabilization-Individually-Non-Woven/dp/B0B84W2VDG?th=1>.

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) *Attorney, Agent, or Firm* — Leon G. Rendeiro, Jr.

(57)


CLAIM

The ornamental design for the epidermal anchor as shown
and described.

DESCRIPTION

FIG. 1 is a perspective view of an epidermal anchor showing
my new design;
FIG. 2 is a top view thereof;
FIG. 3 is a bottom view thereof;
FIG. 4 is a front view thereof;
FIG. 5 is a side view thereof;
FIG. 6 is an opposite side view thereof; and,
FIG. 7 is a second opposite view thereof.
In the drawings, the broken lines depict unclaimed subject
matter only and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

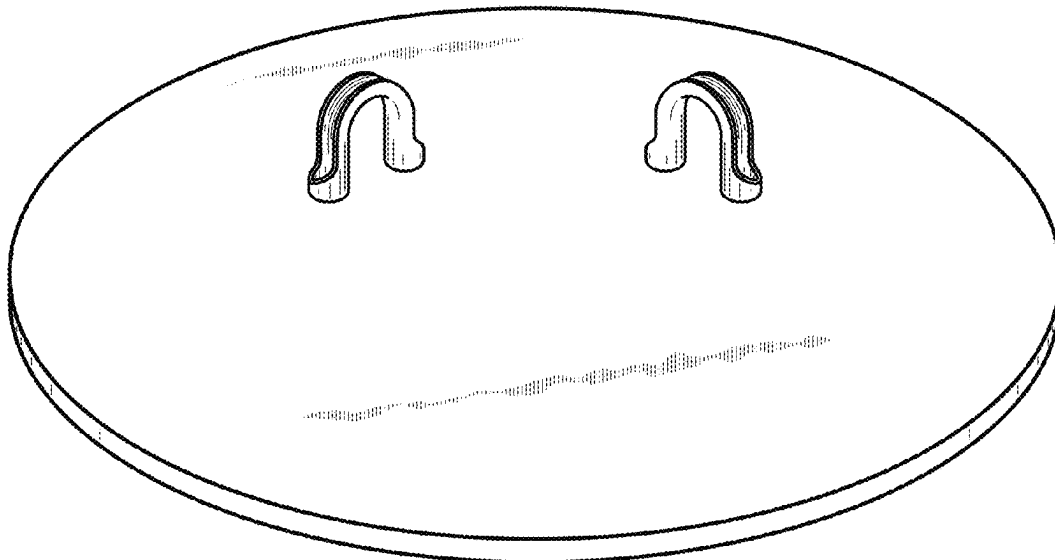

(56)

References Cited

OTHER PUBLICATIONS

“U go Store: Ugo Fix Gentle.” Found online Feb. 12, 2025 at amazon.com. Reference dated Jul. 20, 2018. Retrieved from <https://www.amazon.com/Ugo-Fix-Gentle-Securement-Preparation/dp/B01MS62OKS>.*

“Save Rite Medical: Hollister Feeding Tube Attachment Device.” Found online Feb. 12, 2025 at [saveritemedical.com](https://www.saveritemedical.com). Reference dated Apr. 18, 2019. Retrieved from <https://www.saveritemedical.com/products/feeding-attachment-device-fits-5-fr-to-18-fr>.*

* cited by examiner

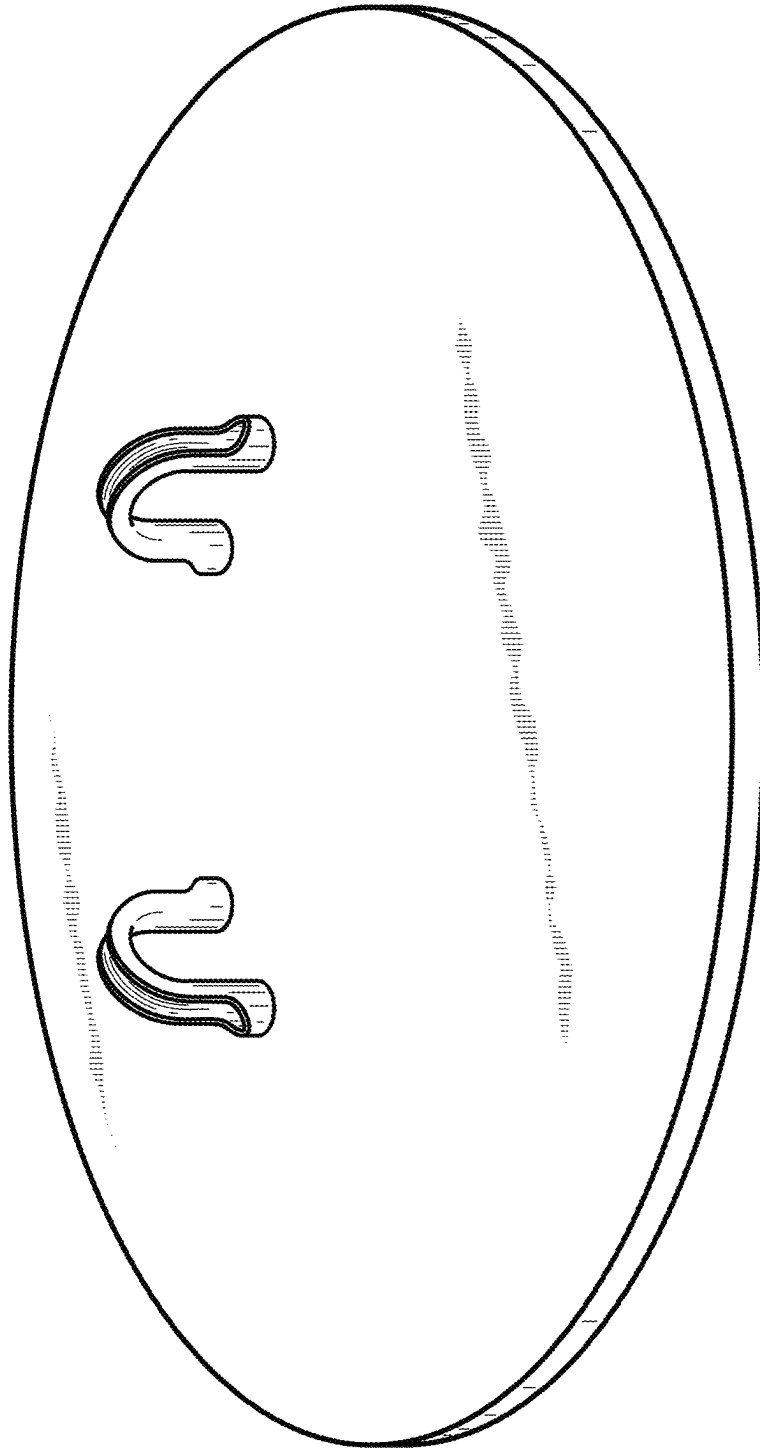


FIG. 1

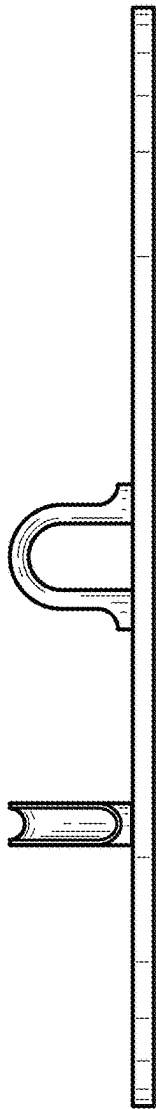


FIG. 2

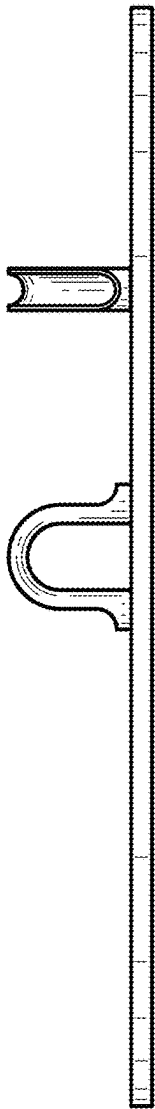


FIG. 3

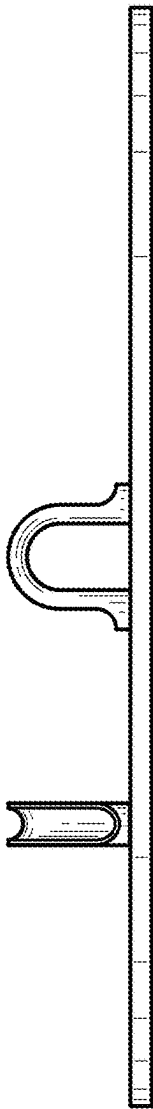


FIG. 4

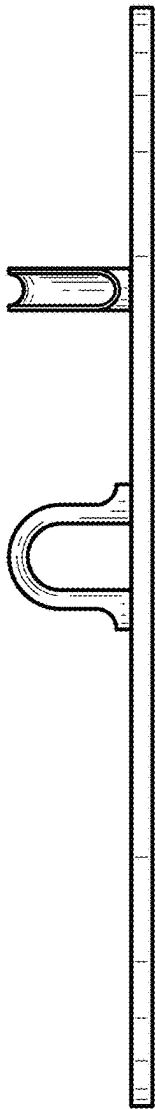


FIG. 5

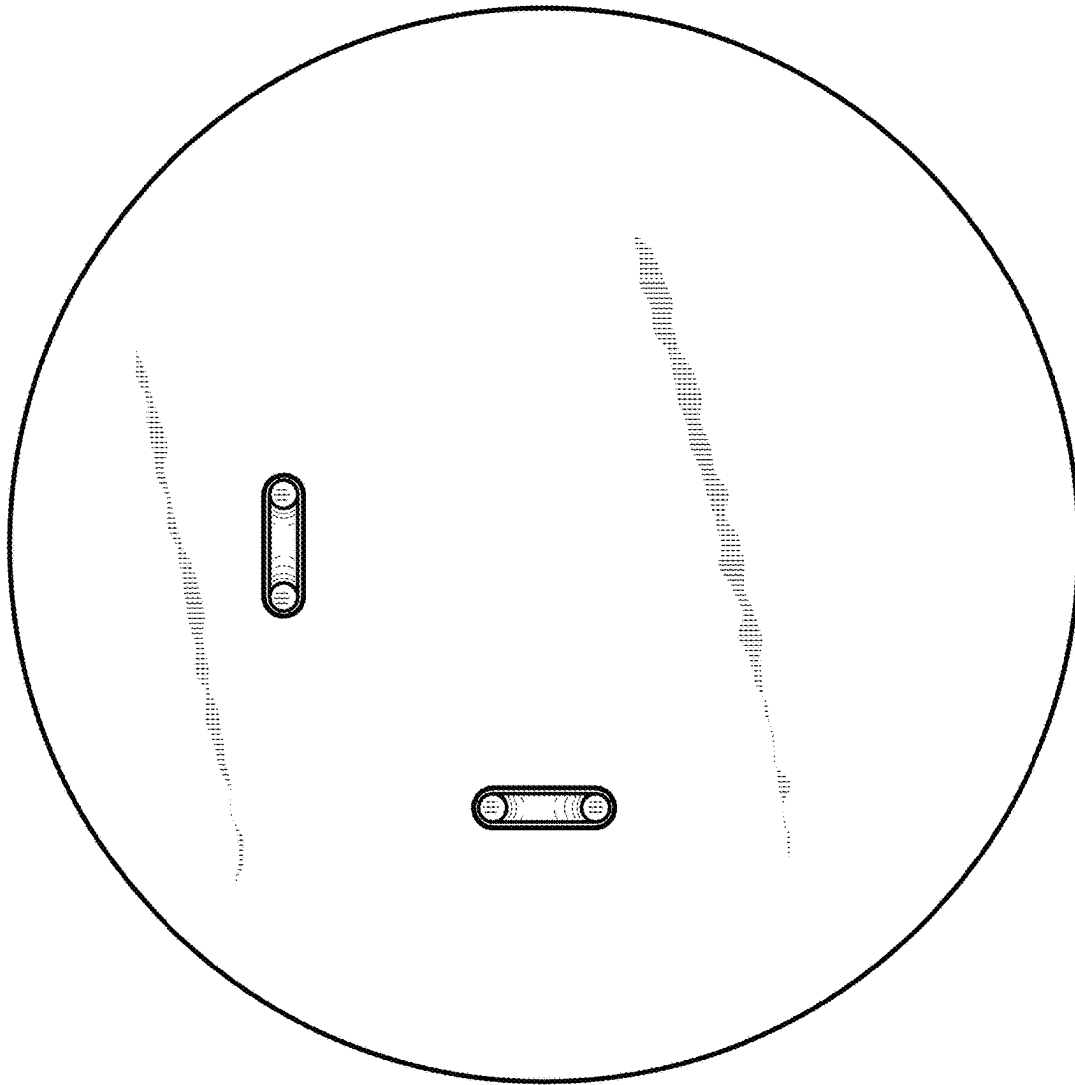


FIG. 6

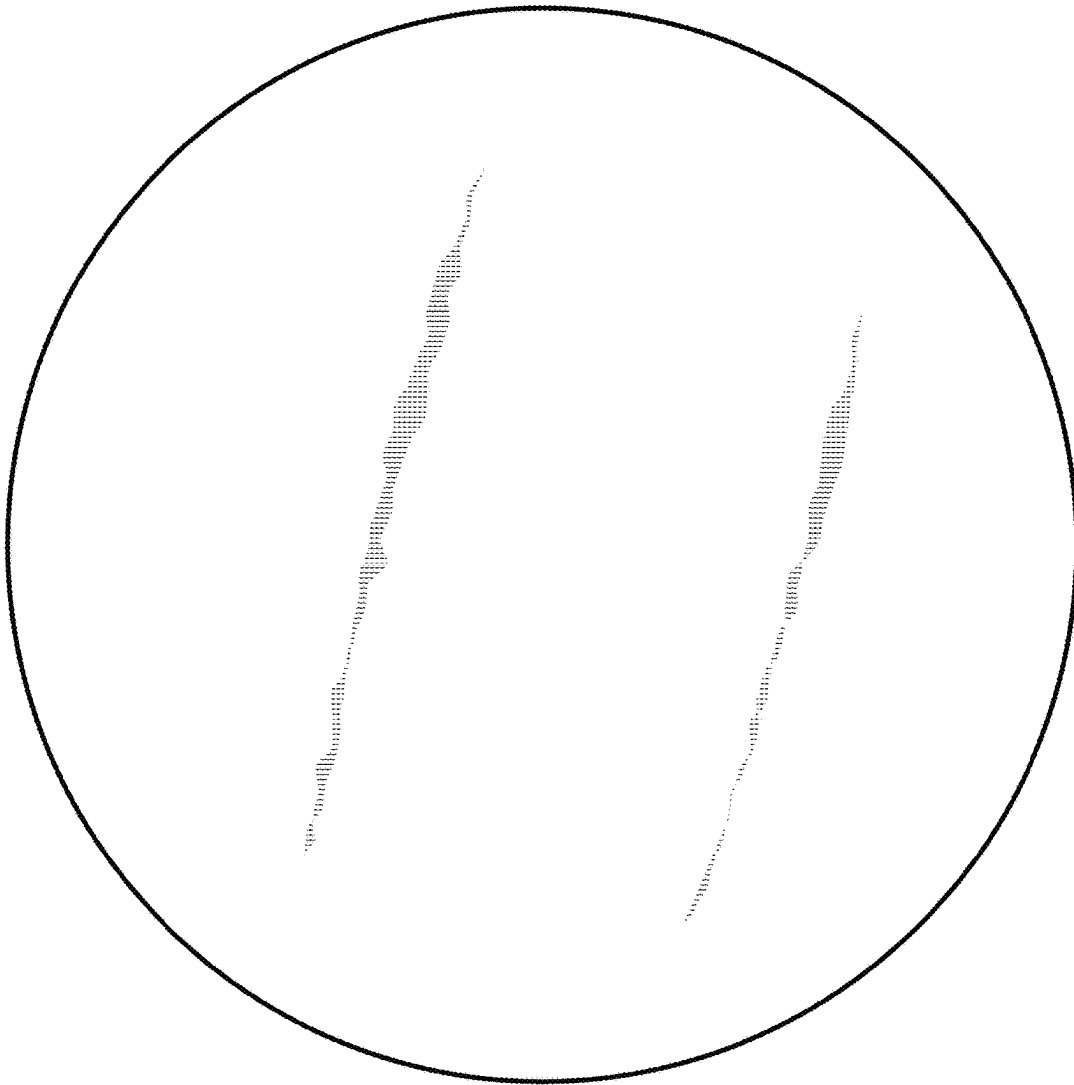


FIG. 7