



US0D1091099S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,091,099 S**
Younger (45) **Date of Patent:** **** Sep. 2, 2025**

(54) **WALKING CANE HANDLE**

(71) Applicant: **Medical Depot, Inc.**, Port Washington,
NY (US)

(72) Inventor: **Max Jefferies Younger**, Roeland Park,
KS (US)

(73) Assignee: **Medical Depot, Inc.**, Port Washington,
NY (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/962,600**

(22) Filed: **Sep. 12, 2024**

(51) **LOC (15) Cl.** **03-03**

(52) **U.S. Cl.**
USPC **D3/12**

(58) **Field of Classification Search**

USPC D3/5, 6, 7, 8, 9, 10, 12, 14, 15, 16, 17
CPC A45B 1/00; A45B 3/00; A45B 7/00; A45B
9/00; A45B 2009/002; A45B 9/02; A45B
9/04

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D515,802	S	*	2/2006	Grierson		D3/7
D518,630	S	*	4/2006	Mival		D3/12
D544,201	S	*	6/2007	Berl		D3/12
D555,892	S	*	11/2007	Carroll		D3/6
D693,565	S	*	11/2013	Chan		D3/7
D722,762	S	*	2/2015	Kroeker		D3/12
D962,629	S	*	9/2022	Fang		D3/7
D982,305	S	*	4/2023	Zou		D3/7
D999,517	S	*	9/2023	Zou		D3/7
D1,011,011	S	*	1/2024	Chen		D3/12
D1,050,053	S	*	11/2024	Chen		D3/12
D1,056,444	S	*	1/2025	Xiong		D3/7
D1,071,534	S	*	4/2025	Li		D3/7
D1,082,285	S	*	7/2025	Psiuk		D3/12

D1,083,353	S	*	7/2025	Pan		D3/7
2002/0129844	A1	*	9/2002	Troyer		A45B 1/00 135/65
2008/0289671	A1	*	11/2008	Chiu		A45B 9/00 135/65
2009/0044847	A1	*	2/2009	Barangan		A45B 9/02 135/72

(Continued)

OTHER PUBLICATIONS

Airgo® Comfort-Plus™ Aluminium Cane | Offset Handle, rehabhire.com, <https://www.rehabhire.com.au/product/airgo-comfort-plus-aluminium-cane-offset-handle/> (Year: 2025).*

(Continued)

Primary Examiner — Steven J Czyz

(74) *Attorney, Agent, or Firm* — Bradley J. Shelowitz

(57) **CLAIM**

The ornamental design for a walking cane handle, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a walking cane handle in accordance with the present design, shown in use attached to a cane;

FIG. 2 is a top perspective view of the walking cane handle of FIG. 1;

FIG. 3 is a bottom perspective view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a left side view thereof;

FIG. 6 is a front view thereof;


FIG. 7 is a rear view thereof;

FIG. 8 is a top view thereof; and,

FIG. 9 is a bottom view thereof.

The broken lines shown in the drawings illustrate portions of the walking cane handle that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

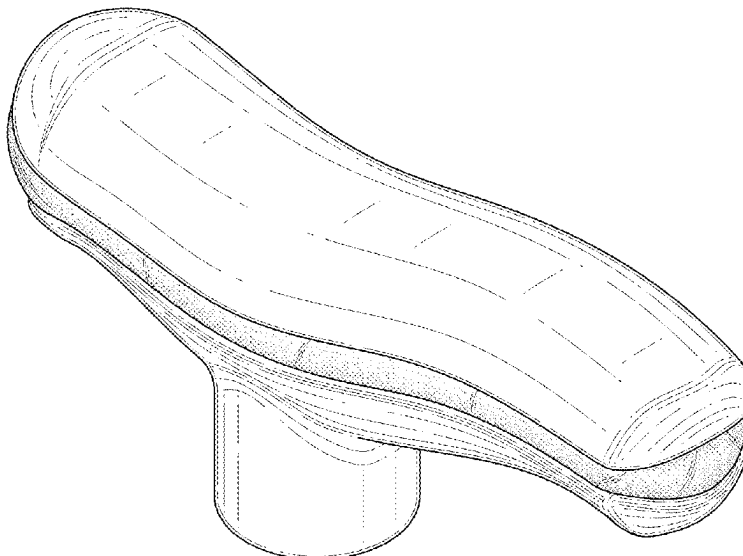

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0271990 A1 * 11/2011 Diamond A45B 3/02
135/65

OTHER PUBLICATIONS

Carex Health Brands Soft Grip Walking Cane—Height Adjustable Cane with Wrist Strap—Latex Free Soft Cushion Handle, Blue Marble, gosupps.com, <https://www.gosupps.com/carex-health-brands-soft-grip-walking-cane-height-adjustable-cane-with-wrist-strap-latex-free-soft-cushion-handle-blue-marble.html> (Year: 2025).*

Walking Stick Folding Cane with LED Light with Cushion T Handle, made-in-china.com, <https://rtmfgltd.en.made-in-china.com/product/FdfGCeWyLAkp/China-Walking-Stick-Folding-Cane-with-LED-Light-with-Cushion-T-Handle.html> (Year: 2025).*

* cited by examiner

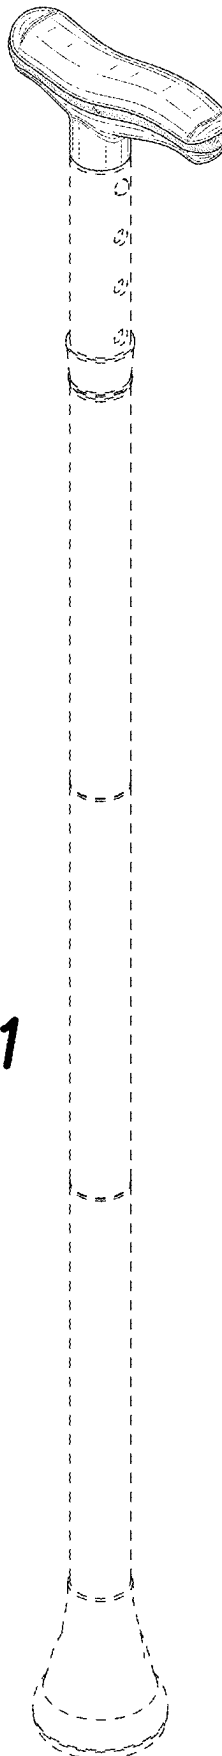


FIG. 1

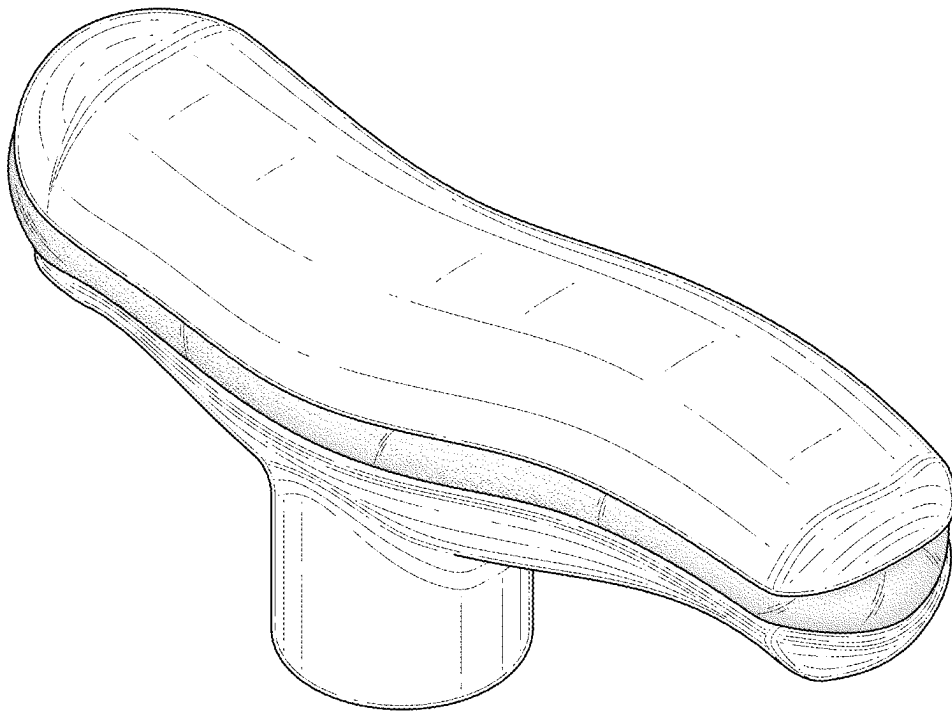


FIG. 2

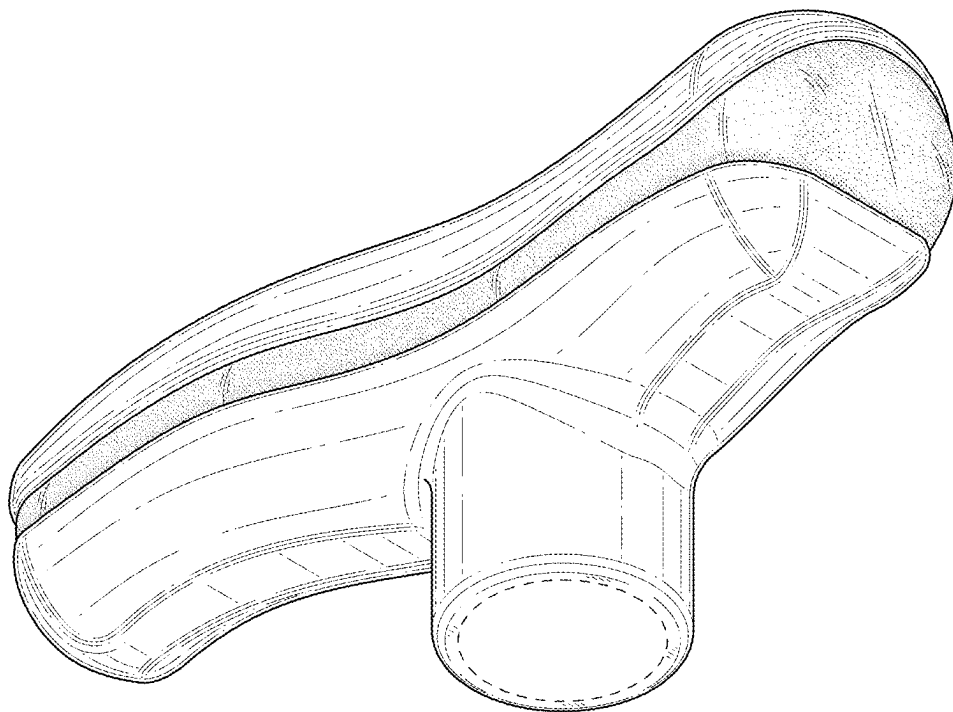


FIG. 3

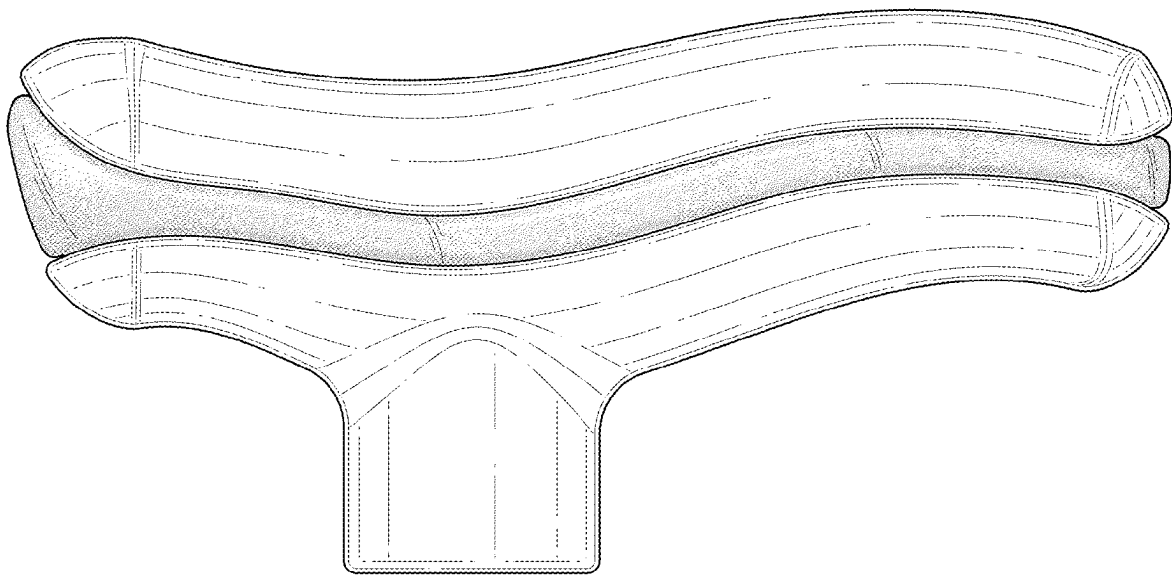


FIG. 4

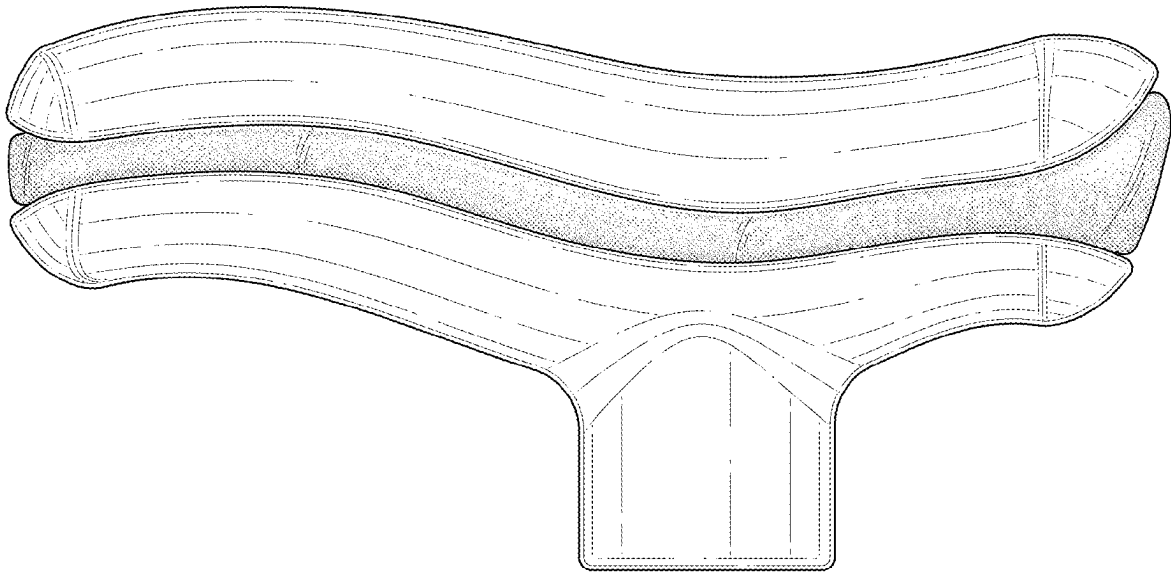


FIG. 5

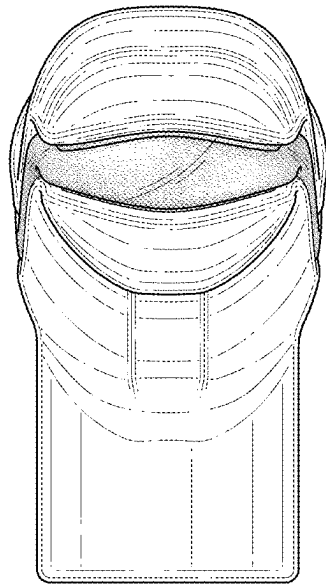


FIG. 6

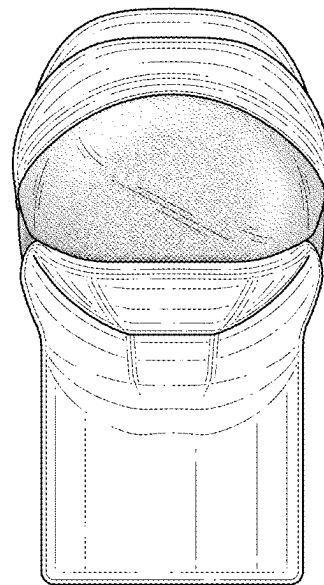


FIG. 7

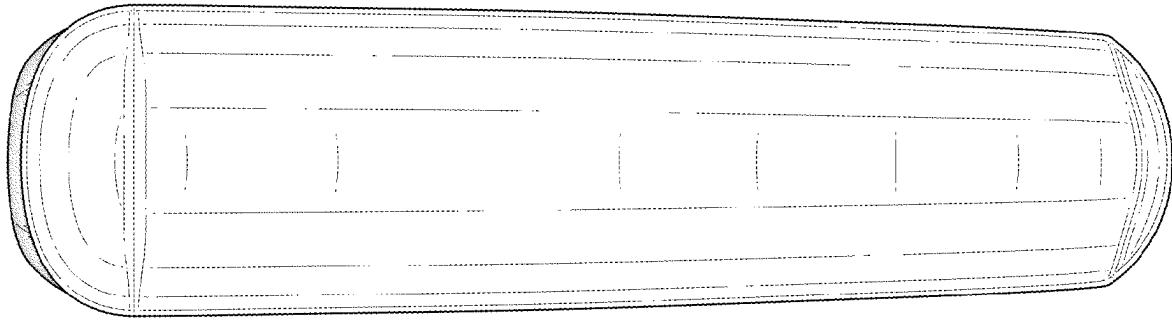


FIG. 8

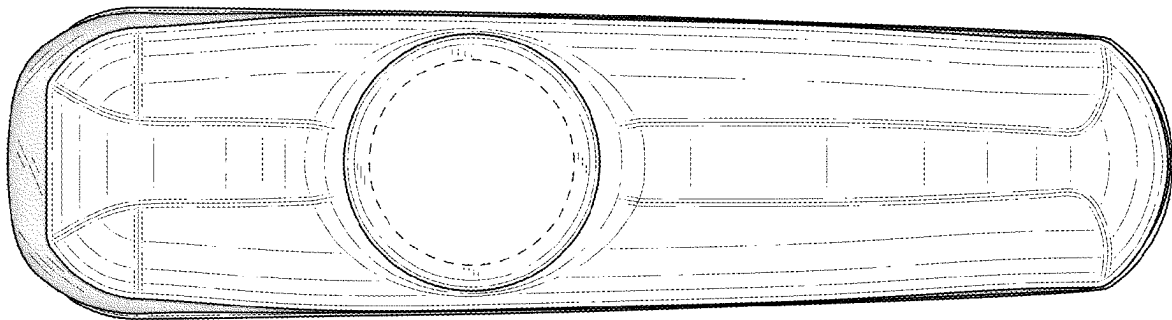


FIG. 9