



US012398176B2

(12) **United States Patent**
Passno et al.

(10) **Patent No.:** **US 12,398,176 B2**
(45) **Date of Patent:** **Aug. 26, 2025**

(54) **USE OF RAMAN SPECTROSCOPY IN
DOWNSTREAM PURIFICATION**

(71) Applicant: **Regeneron Pharmaceuticals, Inc.,**
Tarrytown, NY (US)

(72) Inventors: **Christina Passno**, Tarrytown, NY (US);
Christopher Cowan, Tarrytown, NY
(US); **Andrew Tustian**, Tarrytown, NY
(US)

(73) Assignee: **Regeneron Pharmaceuticals, Inc.,**
Tarrytown, NY (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 765 days.

(21) Appl. No.: **17/742,243**

(22) Filed: **May 11, 2022**

(65) **Prior Publication Data**

US 2022/0340617 A1 Oct. 27, 2022

Related U.S. Application Data

(63) Continuation of application No. 16/550,989, filed on
Aug. 26, 2019, now Pat. No. 11,358,984.
(Continued)

(51) **Int. Cl.**
C07K 1/36 (2006.01)
C07K 1/14 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **C07K 1/36** (2013.01); **C07K 1/145**
(2013.01); **C07K 1/34** (2013.01); **G01N**
1/4044 (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC . C07K 1/145; C07K 1/34; C07K 1/36; C07K
16/00; G01N 1/4044; G01N 1/4077;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

109,819 A 12/1870 Hornbeck et al.
5,675,931 A 10/1997 Wasserman
(Continued)

FOREIGN PATENT DOCUMENTS

AR 113449 A1 5/2020
AU 2004201496 A1 5/2004
(Continued)

OTHER PUBLICATIONS

Abu-Absi et al., Real time monitoring of multiple parameters in
mammalian cell culture bioreactors using an in-line Raman spec-
troscopy probe. Biotechnol Bioeng. May 2011;108(5):1215-21.

(Continued)


Primary Examiner — Jennifer Wecker

(74) *Attorney, Agent, or Firm* — McCarter & English,
LLP

(57) **ABSTRACT**

In situ Raman spectroscopy methods and systems for char-
acterizing or quantifying a protein purification intermediate
and/or final concentrated pool during production or manu-
facture are provided. In one embodiment, in situ Raman
spectroscopy is used to characterize or quantify protein
purification intermediates critical quality attributes during
downstream processing (i.e., after harvest of the protein
purification intermediate). For example, the disclosed in situ
Raman spectroscopy methods and systems can be used to
characterize and quantify protein purification intermediates
as the protein purification intermediates are purified, con-
densed, or otherwise formulated into the final drug product
to be sold or administered.

29 Claims, 20 Drawing Sheets

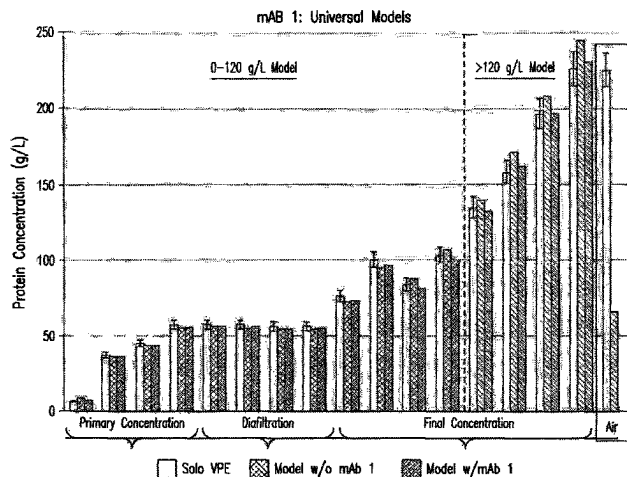

Related U.S. Application Data

- (60) Provisional application No. 62/723,188, filed on Aug. 27, 2018.
- (51) **Int. Cl.**
C07K 1/34 (2006.01)
G01N 1/40 (2006.01)
G01N 21/65 (2006.01)
- (52) **U.S. Cl.**
 CPC **G01N 1/4077** (2013.01); **G01N 21/65** (2013.01); **G01N 2001/4088** (2013.01)
- (58) **Field of Classification Search**
 CPC ... G01N 2001/4088; G01N 2021/8416; G01N 21/65
- See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

5,912,113	A	6/1999	Nakamura et al.
6,156,570	A	12/2000	Hu et al.
6,455,260	B1	9/2002	Muller et al.
6,660,836	B1	12/2003	Anderson et al.
6,780,978	B2	8/2004	Jibu
6,939,686	B2	9/2005	Ling et al.
6,942,968	B1	9/2005	Dickinson et al.
6,979,540	B2	12/2005	Benneteau et al.
6,979,733	B2	12/2005	Zhao et al.
7,101,671	B2	9/2006	Gao
7,129,048	B2	10/2006	Bruchez et al.
7,144,979	B2	12/2006	Maeji et al.
7,169,556	B2	1/2007	Park et al.
7,183,050	B2	2/2007	Krull
7,195,873	B2	3/2007	Filigheddu et al.
7,198,900	B2	4/2007	Woudenberg et al.
7,199,217	B2	4/2007	DiMarchi et al.
7,221,457	B2	5/2007	Jorgenson et al.
7,229,960	B2	6/2007	Pero et al.
7,238,476	B2	7/2007	McKeown et al.
7,258,861	B2	8/2007	Lucas et al.
7,270,951	B1	9/2007	Stemple et al.
7,291,461	B2	11/2007	Welch et al.
7,294,697	B2	11/2007	Xu et al.
7,303,869	B2	12/2007	Stevens et al.
7,309,409	B2	12/2007	Amirkhanian et al.
7,323,319	B2	1/2008	Huang
7,332,586	B2	2/2008	Franzen et al.
7,348,404	B2	3/2008	Holm et al.
7,351,526	B2	4/2008	Soto et al.
7,371,524	B2	5/2008	Dandliker et al.
7,371,834	B2	5/2008	Penninger et al.
7,393,924	B2	7/2008	Vitaliano et al.
7,396,824	B2	7/2008	Sasisekharan et al.
7,402,422	B2	7/2008	Fuchs et al.
7,429,491	B2	9/2008	Luan et al.
7,431,685	B2	10/2008	Frey et al.
7,465,578	B2	12/2008	Berlin et al.
7,482,425	B2	1/2009	Kochendoerfer et al.
7,524,941	B2	4/2009	Olejnik et al.
7,556,815	B2	7/2009	Coleman et al.
7,563,586	B2	7/2009	Okuse et al.
7,572,409	B2	8/2009	Bryning et al.
7,572,603	B2	8/2009	Small et al.
7,572,640	B2	8/2009	Goix et al.
7,585,624	B2	9/2009	Fraser et al.
7,589,079	B2	9/2009	Jonaitis et al.
7,592,434	B2	9/2009	Kerovuo et al.
7,595,198	B2	9/2009	Olejnik et al.
7,642,079	B2	1/2010	Cayouette et al.
7,642,344	B2	1/2010	Van Ness et al.
7,662,566	B2	2/2010	Timms et al.
7,662,644	B2	2/2010	Hahn et al.
7,671,178	B1	3/2010	Phillips et al.
7,692,002	B2	4/2010	Alberto et al.
7,700,277	B2	4/2010	Ambrose et al.
7,727,722	B2	6/2010	Nelson et al.
7,763,649	B2	7/2010	Lockwood et al.
7,771,938	B2	8/2010	Zanni et al.
7,776,528	B2	8/2010	Lakowicz
7,777,011	B2	8/2010	Fishleigh et al.
7,781,572	B2	8/2010	Bartlett et al.
7,803,786	B2	9/2010	McMahon et al.
7,812,137	B2	10/2010	Friedman et al.
7,816,079	B2	10/2010	Fischer
7,824,890	B2	11/2010	Hoser et al.
7,824,895	B2	11/2010	Short et al.
7,824,908	B2	11/2010	Maine et al.
7,838,218	B2	11/2010	Aojula et al.
7,838,237	B2	11/2010	Sampson et al.
7,843,562	B2	11/2010	Chan et al.
7,851,152	B2	12/2010	Chen
7,875,462	B2	1/2011	Gjerde et al.
7,875,465	B2	1/2011	Shiotsuka et al.
7,888,073	B2	2/2011	Densham
7,893,007	B2	2/2011	Ladner et al.
7,893,253	B2	2/2011	Lohse et al.
7,919,249	B2	4/2011	Gelfand et al.
7,927,791	B2	4/2011	Welch et al.
7,939,256	B2	5/2011	Williams
7,939,257	B2	5/2011	Kwitek et al.
7,943,301	B2	5/2011	Sen et al.
7,951,572	B2	5/2011	Kim et al.
7,951,776	B2	5/2011	Gelber
7,960,124	B2	6/2011	Popovic et al.
7,960,516	B2	6/2011	Matheus et al.
7,989,219	B2	8/2011	Shiotsuka et al.
8,003,126	B2	8/2011	Jungles et al.
8,025,883	B2	9/2011	Brooks et al.
8,058,410	B2	11/2011	Jungbauer et al.
8,062,841	B2	11/2011	Su et al.
8,062,883	B2	11/2011	Woudenberg et al.
8,063,184	B2	11/2011	Allawi et al.
8,084,202	B2	12/2011	Castro
8,093,005	B2	1/2012	Jarhede et al.
8,097,421	B2	1/2012	Koo
8,097,442	B2	1/2012	Hitchman et al.
8,110,673	B2	2/2012	Bazan et al.
8,114,587	B2	2/2012	Gite et al.
8,114,596	B2	2/2012	Kaufman
8,133,471	B2	3/2012	Brooks et al.
8,133,984	B2	3/2012	Christensen
8,148,324	B2	4/2012	Greenberg et al.
8,148,516	B2	4/2012	Williams et al.
8,163,566	B2	4/2012	Smith et al.
8,168,399	B2	5/2012	Frutos et al.
8,168,433	B2	5/2012	Gehman et al.
8,173,445	B1	5/2012	Williams et al.
8,173,793	B2	5/2012	Friedman et al.
8,193,430	B2	6/2012	Papadimitrakopoulos et al.
8,198,403	B2	6/2012	Dieckmann et al.
8,212,132	B2	7/2012	Swager et al.
8,216,855	B2	7/2012	Pipper et al.
8,221,719	B2	7/2012	Peuralahti et al.
8,227,428	B2	7/2012	Day et al.
8,227,590	B2	7/2012	Ranga et al.
8,243,267	B2	8/2012	Siegel et al.
8,252,559	B2	8/2012	Fasan et al.
8,263,350	B2	9/2012	Koide et al.
8,263,412	B2	9/2012	Wachter et al.
8,268,981	B2	9/2012	Birkenmeyer et al.
8,273,403	B2	9/2012	Barden et al.
8,273,532	B2	9/2012	Gershow et al.
8,278,085	B2	10/2012	Trotta et al.
8,298,765	B2	10/2012	Luo et al.
8,318,416	B2	11/2012	Tsang et al.
8,318,897	B2	11/2012	Birkenmeyer et al.
8,323,694	B2	12/2012	Hainfeld
8,325,339	B2	12/2012	Ebstein
8,329,647	B2	12/2012	Pfuetzner et al.
8,338,606	B2	12/2012	Perrone et al.
8,350,007	B2	1/2013	Jennings et al.
8,357,505	B2	1/2013	Frommer et al.
8,361,803	B2	1/2013	Fan et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,361,806 B2	1/2013	Gjerde et al.	9,067,962 B2	6/2015	De Paul et al.
8,377,657 B1	2/2013	Shuber	9,068,969 B2	6/2015	Pelligrini
8,383,114 B2	2/2013	Sloey et al.	9,069,700 B2	6/2015	Ishiguro
8,383,585 B2	2/2013	Pfuetzner et al.	9,073,970 B2	7/2015	Muller-Spath et al.
8,414,861 B2	4/2013	Jeong et al.	9,085,598 B2	7/2015	Alaoui-Jamali et al.
8,426,184 B2	4/2013	Blum et al.	9,085,607 B2	7/2015	Phadke et al.
8,426,572 B2	4/2013	Santner et al.	9,085,618 B2	7/2015	Ramasubramanyan et al.
8,436,141 B2	5/2013	Becker	9,085,766 B2	7/2015	Crane et al.
8,445,288 B2	5/2013	Sorensen et al.	9,102,520 B2	8/2015	Han et al.
8,460,471 B2	6/2013	Takeshima et al.	9,102,920 B2	8/2015	Feng et al.
8,460,472 B2	6/2013	Takeshima et al.	9,115,178 B2	8/2015	Gilar et al.
8,476,020 B1	7/2013	Scholl et al.	9,115,189 B2	8/2015	Lou et al.
8,476,033 B2	7/2013	Cheek et al.	RE45,660 E	9/2015	Weiner et al.
8,477,307 B1	7/2013	Yufa et al.	9,120,862 B2	9/2015	Yoshimura et al.
8,481,263 B2	7/2013	Lim et al.	9,121,066 B2	9/2015	Hamamah et al.
8,486,634 B2	7/2013	Lim et al.	9,127,035 B2	9/2015	Auclair et al.
8,486,680 B2	7/2013	Gray et al.	9,133,343 B2	9/2015	Patton et al.
8,501,172 B2	8/2013	Kaplan et al.	9,139,860 B2	9/2015	Chun
8,501,923 B2	8/2013	Rothmund	9,145,575 B2	9/2015	Liu et al.
8,519,031 B2	8/2013	Parker et al.	RE45,763 E	10/2015	Brophy et al.
8,524,450 B2	9/2013	Moon et al.	9,163,283 B2	10/2015	Chee et al.
8,530,626 B1	9/2013	Cardamone	9,169,478 B2	10/2015	Weiner et al.
8,536,324 B2	9/2013	Mohapatra et al.	9,170,197 B2	10/2015	Geddes et al.
8,547,550 B2	10/2013	Carpenter	9,175,275 B2	11/2015	Gray et al.
8,557,956 B2	10/2013	Cheng et al.	9,175,348 B2	11/2015	Korlach et al.
8,563,476 B2	10/2013	Lillard, Jr.	9,186,643 B2	11/2015	Griffiths et al.
8,569,008 B2	10/2013	Choi et al.	9,206,482 B2	12/2015	Davicioni et al.
8,569,468 B2	10/2013	Chen et al.	9,212,379 B2	12/2015	Tsang et al.
8,574,892 B2	11/2013	Su	9,213,027 B2	12/2015	Doranz et al.
8,586,530 B2	11/2013	Ferreira et al.	9,243,017 B2	1/2016	Aslan
8,609,337 B2	12/2013	Pregibon et al.	9,243,275 B1	1/2016	Levon et al.
8,614,057 B2	12/2013	Allen et al.	9,249,400 B2	2/2016	Gray et al.
8,614,086 B2	12/2013	Holt et al.	9,260,494 B2	2/2016	Skerra et al.
8,628,952 B2	1/2014	Stuelpnagel et al.	9,260,505 B2	2/2016	Weir et al.
8,647,821 B2	2/2014	Castro et al.	9,265,815 B2	2/2016	Fraser et al.
8,658,381 B2	2/2014	Mansson et al.	9,265,844 B2	2/2016	Tung et al.
8,658,613 B2	2/2014	Bruno	9,273,089 B2	3/2016	Knutson et al.
8,669,055 B2	3/2014	Bazan et al.	9,279,148 B2	3/2016	Gunderson et al.
8,673,556 B2	3/2014	Akeson et al.	9,279,770 B2	3/2016	Mossoba et al.
8,673,570 B2	3/2014	Shafer	9,290,568 B2	3/2016	Rives et al.
8,679,859 B2	3/2014	Yan et al.	9,296,797 B2	3/2016	Ulijasz et al.
8,697,390 B2	4/2014	Skinderso et al.	9,309,545 B2	4/2016	Medoff
8,697,434 B2	4/2014	Voorhees	9,315,538 B2	4/2016	Carter et al.
8,697,645 B2	4/2014	Acharya et al.	9,315,868 B2	4/2016	Vogelstein et al.
8,697,656 B2	4/2014	Fournial et al.	9,340,568 B2	5/2016	Casteel et al.
8,734,793 B2	5/2014	Tu et al.	9,347,092 B2	5/2016	Roesler et al.
8,747,484 B2	6/2014	Benayahu et al.	9,347,863 B2	5/2016	Mehrpouyan et al.
8,748,696 B2	6/2014	Rathinasabapathi et al.	9,365,623 B2	6/2016	Ulijasz et al.
8,753,870 B2	6/2014	Lee et al.	9,365,883 B2	6/2016	Gannot et al.
8,754,055 B2	6/2014	Allen et al.	9,371,357 B2	6/2016	Sandrock et al.
8,765,367 B2	7/2014	Breidenthal et al.	9,388,047 B2	7/2016	Busnaina et al.
8,765,369 B2	7/2014	Dubus et al.	9,388,373 B2	7/2016	Rao et al.
8,765,373 B2	7/2014	Majda	9,399,059 B2	7/2016	Morrison
8,765,684 B2	7/2014	Jonczyk et al.	9,399,763 B2	7/2016	Weiner et al.
8,765,938 B2	7/2014	Hara et al.	9,399,795 B2	7/2016	Chee et al.
8,771,938 B2	7/2014	Chang et al.	9,410,950 B2	8/2016	Cui et al.
8,779,097 B2	7/2014	Nagarkar et al.	9,439,976 B2	9/2016	Tung et al.
8,785,162 B2	7/2014	De Souza et al.	9,458,225 B2	10/2016	Hassan Abdalla
8,785,608 B2	7/2014	Rigal et al.	9,458,510 B2	10/2016	DePinho et al.
8,796,206 B2	8/2014	Sloey et al.	9,464,109 B2	10/2016	Li et al.
8,815,611 B2	8/2014	Bunch et al.	9,481,908 B2	11/2016	Olasagasti et al.
8,858,770 B2	10/2014	Tan et al.	9,488,660 B2	11/2016	Miao et al.
8,877,478 B2	11/2014	Steer et al.	9,493,513 B2	11/2016	Mehmet et al.
8,883,424 B2	11/2014	Chee et al.	9,493,845 B2	11/2016	Cao et al.
8,889,623 B2	11/2014	Hoepflich et al.	9,506,867 B2	11/2016	Moretto et al.
8,896,829 B2	11/2014	Furusho	9,512,469 B2	12/2016	Seligmann et al.
8,916,154 B2	12/2014	Das et al.	9,517,275 B2	12/2016	Kibbe et al.
8,916,606 B2	12/2014	Tour et al.	9,518,077 B2	12/2016	Halada et al.
8,932,558 B2	1/2015	Madasamy	9,518,280 B2	12/2016	Burke et al.
8,933,197 B2	1/2015	Stemmer et al.	9,518,986 B2	12/2016	Blackburn et al.
8,937,156 B2	1/2015	Qi	9,539,763 B2	1/2017	Houbertz-Krauss et al.
8,945,932 B2	2/2015	Patton et al.	9,540,657 B2	1/2017	Yu et al.
8,975,390 B2	3/2015	Bruno	9,551,025 B2	1/2017	Kim et al.
9,006,458 B2	4/2015	Chang et al.	9,551,667 B2	1/2017	Schmidt et al.
9,051,605 B2	6/2015	Son et al.	9,556,429 B2	1/2017	Mir
			9,579,346 B2	2/2017	McGrath et al.
			9,598,479 B2	3/2017	Rademacher et al.
			9,598,690 B2	3/2017	Sun et al.
			9,603,775 B2	3/2017	Weeks et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,620,727 B2	4/2017	Laaksonen et al.	10,261,020 B2	4/2019	Tedesco et al.
9,624,271 B2	4/2017	Hanko et al.	10,273,530 B2	4/2019	Rimseliene et al.
9,624,307 B2	4/2017	Nahrendorf et al.	10,287,601 B2	5/2019	Anterola
9,624,520 B2	4/2017	Geierstanger et al.	10,294,133 B2	5/2019	Hashim et al.
9,624,547 B2	4/2017	Wong et al.	10,294,515 B2	5/2019	Seligmann et al.
9,637,441 B2	5/2017	Miao et al.	10,308,920 B2	6/2019	Bornscheuer et al.
9,649,383 B2	5/2017	Kashi et al.	10,328,100 B2	6/2019	Bentov et al.
9,657,333 B2	5/2017	Takoh	10,338,078 B2	7/2019	Sodeoka et al.
9,657,360 B2	5/2017	Stewart et al.	10,344,336 B2	7/2019	Bramlett et al.
9,677,107 B2	6/2017	Reitmeir et al.	10,352,945 B2	7/2019	Cohen et al.
9,689,039 B2	6/2017	Wong et al.	10,358,680 B2	7/2019	Vo-Dinh et al.
9,689,801 B2	6/2017	Kho et al.	10,370,698 B2	8/2019	Nolan et al.
9,700,485 B2	7/2017	Weeks et al.	10,385,085 B2	8/2019	Klopp et al.
9,700,486 B2	7/2017	Weeks et al.	10,393,631 B2	8/2019	Hsieh
9,701,709 B2	7/2017	Anderson et al.	10,393,741 B2	8/2019	Rikihisa
9,707,154 B2	7/2017	Weeks et al.	10,413,482 B2	9/2019	Weeks et al.
9,707,155 B2	7/2017	Weeks et al.	10,416,155 B2	9/2019	Dryga et al.
9,708,667 B2	7/2017	Yanai et al.	10,441,667 B2	10/2019	Perfect et al.
9,713,572 B2	7/2017	Weeks et al.	10,538,581 B2	1/2020	Barghorn et al.
9,717,648 B2	8/2017	Weeks et al.	10,548,517 B2	2/2020	Cho et al.
9,717,649 B2	8/2017	Weeks et al.	10,548,953 B2	2/2020	Liu et al.
9,718,894 B2	8/2017	Choi et al.	10,555,930 B2	2/2020	Tang et al.
9,719,079 B2	8/2017	Weiner et al.	10,563,163 B2	2/2020	Berry et al.
9,764,953 B2	9/2017	Zuckermann et al.	10,591,479 B2	3/2020	Gao et al.
9,765,319 B2	9/2017	Steer et al.	10,604,745 B2	3/2020	Darzins et al.
9,782,443 B2	10/2017	Pei et al.	10,625,250 B2	4/2020	Hau
9,808,526 B2	11/2017	Chen	10,640,772 B2	5/2020	Furusuo
9,809,846 B2	11/2017	Willner et al.	10,669,307 B2	6/2020	Villain et al.
9,823,253 B2	11/2017	Weidemaier et al.	10,677,805 B1	6/2020	Chen et al.
9,829,437 B2	11/2017	Chau et al.	10,689,411 B2	6/2020	Migaud et al.
9,844,594 B2	12/2017	Antochshuk et al.	10,689,412 B2	6/2020	Ju et al.
9,849,172 B2	12/2017	Garcia-Sastre et al.	10,711,319 B2	7/2020	Einen et al.
9,856,505 B2	1/2018	Bartko	10,712,310 B2	7/2020	Pleshko et al.
9,862,974 B2	1/2018	Wang et al.	10,716,789 B2	7/2020	Nti-Addae et al.
9,868,937 B2	1/2018	Regnier et al.	10,731,141 B2	8/2020	Iyidogan
9,873,866 B2	1/2018	Darzins et al.	10,736,956 B2	8/2020	Palese et al.
9,879,299 B2	1/2018	Yamakawa et al.	10,745,750 B2	8/2020	Korlach et al.
9,885,716 B2	2/2018	Lee et al.	10,751,423 B2	8/2020	Ghoroghchian et al.
9,889,098 B2	2/2018	Birbara	10,774,304 B2	9/2020	Rao et al.
9,890,208 B2	2/2018	Brooks et al.	10,781,256 B2	9/2020	Weiskopf et al.
9,896,733 B2	2/2018	Kok et al.	10,786,545 B2	9/2020	Kang et al.
9,908,929 B2	3/2018	Smith et al.	10,787,494 B2	9/2020	Struthers et al.
9,913,899 B2	3/2018	Kauvar et al.	10,800,856 B2	10/2020	Barnett et al.
9,914,959 B2	3/2018	Hildebrandt et al.	10,813,980 B2	10/2020	Carelli et al.
9,932,365 B2	4/2018	Kelts et al.	10,844,094 B2	11/2020	Skerra et al.
9,937,152 B2	4/2018	Maeda et al.	10,844,118 B2	11/2020	Winau et al.
9,938,525 B2	4/2018	Carmona Orozco et al.	10,870,875 B2	12/2020	Sutherland et al.
9,944,918 B2	4/2018	Venditti et al.	10,894,121 B2	1/2021	Cheng et al.
9,951,125 B2	4/2018	Barghorn et al.	10,899,803 B2	1/2021	Guerette et al.
9,968,627 B2	5/2018	Stahly et al.	10,913,779 B2	2/2021	Hall et al.
9,980,911 B2	5/2018	Barnett et al.	10,918,126 B2	2/2021	Shchepinov
9,993,590 B2	6/2018	Courtney et al.	10,918,319 B2	2/2021	Lee et al.
10,000,788 B2	6/2018	Straus	10,919,979 B2	2/2021	Magliery et al.
10,040,862 B2	8/2018	Liu et al.	10,953,073 B2	3/2021	Schellenberger et al.
10,040,868 B2	8/2018	Sagi et al.	10,962,512 B2	3/2021	Zografos et al.
10,052,393 B2	8/2018	Park et al.	10,975,427 B2	4/2021	Dambacher et al.
10,059,994 B2	8/2018	Hamamah et al.	10,981,980 B2	4/2021	Hall et al.
10,067,051 B2	9/2018	Diem et al.	11,007,849 B2	5/2021	Csordas et al.
10,071,163 B2	9/2018	Montefeltro et al.	11,015,220 B2	5/2021	Nikiforov et al.
10,088,481 B2	10/2018	Scholl et al.	11,022,611 B2	6/2021	Robinson et al.
10,100,299 B2	10/2018	Slupska et al.	11,026,885 B2	6/2021	Ashton et al.
10,101,209 B2	10/2018	Selker et al.	11,026,963 B2	6/2021	Gallop et al.
10,125,195 B2	11/2018	Depaz et al.	11,034,743 B1	6/2021	Lanquar et al.
10,156,546 B2	12/2018	Trau et al.	11,040,107 B2	6/2021	Grossi et al.
10,174,069 B2	1/2019	Field et al.	11,058,639 B2	7/2021	Dizerega et al.
10,174,329 B2	1/2019	Deng et al.	11,072,797 B1	7/2021	Lanquar et al.
10,179,806 B2	1/2019	Garcia-Sastre et al.	11,073,509 B2	7/2021	Laing et al.
10,183,969 B2	1/2019	Kyhse-Andersen et al.	11,079,388 B2	8/2021	Chen
10,202,428 B2	2/2019	Cary et al.	11,090,385 B2	8/2021	Peyman
10,209,260 B2	2/2019	Oved et al.	11,091,534 B2	8/2021	Chhabra et al.
10,220,098 B2	3/2019	Kim et al.	11,111,603 B2	9/2021	Jackson et al.
10,220,378 B2	3/2019	Rozhkova et al.	11,124,543 B2	9/2021	Berger et al.
10,246,493 B2	4/2019	Demirel et al.	11,130,787 B2	9/2021	Keller et al.
10,246,744 B2	4/2019	Vijayan et al.	11,249,026 B2	2/2022	Moretto et al.
10,253,144 B2	4/2019	Demirel et al.	11,358,984 B2	6/2022	Passno et al.
			2004/0057040 A1	3/2004	Beckenkamp et al.
			2004/0249122 A1	12/2004	Blazyk
			2006/0240489 A1	10/2006	Wei et al.
			2006/0281068 A1	12/2006	Maier et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0122803	A1	5/2007	Moore et al.	2019/0112569	A1	4/2019	Czeterko et al.
2009/0104594	A1	4/2009	Webb	2019/0120824	A1	4/2019	Jaques et al.
2009/0275020	A1	11/2009	Faure	2019/0125859	A1	5/2019	Palese et al.
2010/0136609	A1	6/2010	Clay et al.	2019/0135878	A1	5/2019	Silberg et al.
2010/0203050	A1	8/2010	Weik et al.	2019/0137338	A1	5/2019	Webster et al.
2010/0203651	A1	8/2010	Lim et al.	2019/0142921	A1	5/2019	Delisa et al.
2010/0256336	A1	10/2010	Yuk et al.	2019/0144284	A1	5/2019	Blanford et al.
2010/0291599	A1	11/2010	Tague, Jr. et al.	2019/0153115	A1	5/2019	Schellenberger et al.
2011/0081672	A1	4/2011	Andersen et al.	2019/0153381	A1	5/2019	Angelini et al.
2012/0122076	A1 *	5/2012	Lau C07K 1/14 530/416	2019/0153527	A1	5/2019	Ju et al.
2012/0123688	A1 *	5/2012	Ramasubramanyan G01N 33/6854 702/19	2019/0162726	A1	5/2019	Hawthornthwaite et al.
2012/0275681	A1	11/2012	Honda et al.	2019/0177435	A1	6/2019	Wong et al.
2013/0177919	A1	7/2013	Kaufmann et al.	2019/0194460	A1	6/2019	Ceres et al.
2013/0177972	A1	7/2013	Green et al.	2019/0201556	A1	7/2019	McLeay
2014/0087423	A1	3/2014	Koncilja et al.	2019/0209715	A1	7/2019	Kelly et al.
2014/0150855	A1	6/2014	Inoue et al.	2019/0255106	A1	8/2019	Lande et al.
2014/0335630	A1	11/2014	Cameron et al.	2019/0255173	A1	8/2019	Francis et al.
2015/0110799	A1	4/2015	Ramasubramanyan et al.	2019/0263914	A1	8/2019	Brogdon et al.
2015/0183862	A1	7/2015	Edwards et al.	2019/0270769	A1	9/2019	Milano et al.
2015/0247210	A1	9/2015	Olesberg et al.	2019/0272894	A1	9/2019	Wasalathanthri et al.
2015/0328563	A1	11/2015	Lacki et al.	2019/0275104	A1	9/2019	Lande et al.
2016/0000891	A1	1/2016	Barghorn et al.	2019/0276528	A1	9/2019	Liu et al.
2016/0025633	A1	1/2016	Moretto et al.	2019/0298826	A1	10/2019	Hoos et al.
2016/0069809	A1	3/2016	Bonnier et al.	2019/0309045	A1	10/2019	Yun
2016/0103072	A1	4/2016	Fukutake et al.	2019/0315835	A1	10/2019	Schellenberger et al.
2016/0159888	A1	6/2016	Klingelhoefer et al.	2019/0316208	A1	10/2019	Hanks et al.
2016/0215103	A1	7/2016	Omenetto et al.	2019/0338039	A1	11/2019	Barnett et al.
2016/0251408	A1	9/2016	Chhabra et al.	2019/0339272	A1	11/2019	Campbell et al.
2016/0341667	A1	11/2016	Ramasubramanyan et al.	2019/0352430	A1	11/2019	Demirel et al.
2017/0073393	A1	3/2017	Chhabra et al.	2019/0352598	A1	11/2019	Sabatini et al.
2017/0130186	A1	5/2017	Berry et al.	2019/0374617	A1	12/2019	Hall et al.
2017/0189550	A1	7/2017	Puebla et al.	2019/0375822	A1	12/2019	Seth Chhabra et al.
2017/0299594	A1	10/2017	Depinho et al.	2019/0376020	A1	12/2019	Bickham et al.
2017/0333559	A1	11/2017	Sloey et al.	2019/0381129	A1	12/2019	Grossi et al.
2017/0355947	A9	12/2017	Berry et al.	2019/0381182	A1	12/2019	Dutta et al.
2018/0000146	A1	1/2018	Geremia	2020/0024363	A1	1/2020	Teran et al.
2018/0003712	A1	1/2018	Haam et al.	2020/0031863	A1	1/2020	Muller-Spath et al.
2018/0020956	A1	1/2018	Lee et al.	2020/0032248	A1	1/2020	White
2018/0023111	A1	1/2018	Schutze et al.	2020/0038352	A1	2/2020	Yoon et al.
2018/0034051	A1	2/2018	Whelan et al.	2020/0062832	A1	2/2020	Sun et al.
2018/0051063	A1	2/2018	Cleland et al.	2020/0069717	A1	3/2020	Ju et al.
2018/0071376	A1	3/2018	Bornal et al.	2020/0087379	A1	3/2020	Schellenberger et al.
2018/0087041	A1	3/2018	Venditti	2020/0087632	A1	3/2020	Coffman et al.
2018/0125988	A1	5/2018	Yang et al.	2020/0096448	A1	3/2020	Gillner et al.
2018/0126001	A1	5/2018	Malecki et al.	2020/0108072	A1	4/2020	Honigberg et al.
2018/0127813	A1	5/2018	Haushalter	2020/0116638	A1	4/2020	Duraipandian et al.
2018/0133319	A1	5/2018	Vo-Dinh et al.	2020/0131265	A1	4/2020	Koenig et al.
2018/0135121	A1	5/2018	Ju et al.	2020/0147175	A1	5/2020	Schillaci
2018/0149597	A1	5/2018	Umezaki et al.	2020/0148999	A1	5/2020	Beckers et al.
2018/0155336	A1	6/2018	Mais et al.	2020/0150022	A1	5/2020	Ugawa et al.
2018/0177891	A1	6/2018	McAteer et al.	2020/0157141	A1	5/2020	Sharnes et al.
2018/0180549	A1	6/2018	Lewis	2020/0200763	A1	6/2020	Min et al.
2018/0185518	A1	7/2018	Vitaliano et al.	2020/0231944	A1	7/2020	Budge et al.
2018/0217146	A1	8/2018	Varadarajan et al.	2020/0239852	A1	7/2020	Hiller et al.
2018/0222938	A1	8/2018	Heringstad et al.	2020/0241002	A1	7/2020	Xu
2018/0237501	A1	8/2018	Sloey et al.	2020/0251186	A1	8/2020	Love et al.
2018/0256740	A1	9/2018	Pasqualini et al.	2020/0254093	A1	8/2020	Khandekar et al.
2018/0258484	A1	9/2018	Gros	2020/0254118	A1	8/2020	Bachawal et al.
2018/0284134	A1	10/2018	Basadonna et al.	2020/0255538	A1	8/2020	Magliery et al.
2018/0291329	A1	10/2018	Moretto et al.	2020/0270354	A1	8/2020	Khandekar et al.
2018/0292324	A1	10/2018	Verma et al.	2020/0283506	A1	9/2020	Watters et al.
2018/0305417	A1	10/2018	Spudich et al.	2020/0283713	A1	9/2020	Ball et al.
2018/0327828	A1	11/2018	Ju et al.	2020/0291075	A1	9/2020	Toettcher et al.
2019/0000988	A1	1/2019	Chen	2020/0292538	A1	9/2020	Oliivo et al.
2019/0008965	A1	1/2019	Messersmith et al.	2020/0297855	A1	9/2020	Leach et al.
2019/0009241	A1	1/2019	Prewer	2020/0316163	A1	10/2020	Grossi et al.
2019/0024261	A1	1/2019	Griffiths et al.	2020/0325460	A1	10/2020	Skirgaila et al.
2019/0034597	A1	1/2019	Tsumoto et al.	2020/0347088	A1	11/2020	Jiang et al.
2019/0062419	A1	2/2019	Ramasubramanyan et al.	2020/0352857	A1	11/2020	Gu et al.
2019/0077850	A1	3/2019	Ingber et al.	2020/0354414	A1	11/2020	Zhang et al.
2019/0083402	A1	3/2019	Talley	2020/0354459	A1	11/2020	Pearse et al.
2019/0106461	A1	4/2019	Garcia-Sastre et al.	2020/0361996	A1	11/2020	Pochan et al.
				2020/0362017	A1	11/2020	Popel et al.
				2020/0363416	A1	11/2020	Yang et al.
				2020/0369607	A1	11/2020	Reuveni et al.
				2020/0370133	A1	11/2020	Kim et al.
				2020/0385469	A1	12/2020	Yang et al.
				2020/0385757	A1	12/2020	Kahvejian et al.
				2020/0390908	A1	12/2020	Singh et al.

(56)

References Cited

FOREIGN PATENT DOCUMENTS

U.S. PATENT DOCUMENTS					
2020/0392195	A1	12/2020	Schellenberger et al.	AU	2002363062 B2 3/2007
2020/0392447	A1	12/2020	Berry et al.	AU	2007202906 A1 7/2007
2020/0399398	A1	12/2020	Bangera et al.	AU	2002355997 B2 1/2008
2021/0002335	A1	1/2021	Omenetto et al.	AU	2012200864 A1 3/2012
2021/0002387	A1	1/2021	Geremia et al.	AU	2012201856 A1 4/2012
2021/0002628	A1	1/2021	Federowicz et al.	AU	2012244255 A1 11/2012
2021/0009935	A1	1/2021	Saito et al.	AU	2013201114 A1 3/2013
2021/0015962	A1	1/2021	Shaffner et al.	AU	2013201117 A1 3/2013
2021/0017226	A1	1/2021	Baek	AU	2013201308 B2 5/2013
2021/0017553	A1	1/2021	Hiller et al.	AU	2013202463 A1 5/2013
2021/0024872	A1	1/2021	Martin et al.	AU	2013203326 B2 5/2013
2021/0025004	A1	1/2021	Gleeson et al.	AU	2013204082 A1 5/2013
2021/0025814	A1	1/2021	Stacey et al.	AU	2013204086 B2 5/2013
2021/0025887	A1	1/2021	Broger	AU	2013221356 A1 8/2014
2021/0032289	A1	2/2021	Francois et al.	AU	2017200870 A1 3/2017
2021/0032616	A1	2/2021	Liu et al.	AU	2016334247 A1 4/2018
2021/0040064	A1	2/2021	Fernandez et al.	AU	2018350890 A1 3/2020
2021/0040431	A1	2/2021	Mogi	BR	102012033580 A2 6/2015
2021/0047606	A1	2/2021	Ray et al.	BR	PI1004360 A2 8/2015
2021/0054068	A1	2/2021	Abou-Elkacem et al.	BR	102016017022 B1 2/2018
2021/0054093	A1	2/2021	Wang et al.	BR	132013030798 E2 7/2019
2021/0061854	A1	3/2021	Olmstead et al.	CA	2243943 A1 7/1997
2021/0062133	A1	3/2021	Hassell et al.	CA	2843504 A1 2/2013
2021/0062143	A1	3/2021	Hermiston et al.	CA	2809872 A1 9/2013
2021/0069334	A1	3/2021	Li et al.	CA	2882003 A1 2/2014
2021/0070842	A1	3/2021	Fraser et al.	CA	2849447 A1 10/2014
2021/0071016	A1	3/2021	Zhong et al.	CA	2915653 A1 10/2014
2021/0071249	A1	3/2021	Irani et al.	CA	2884907 A1 5/2015
2021/0077518	A1	3/2021	Poe et al.	CA	2953020 A1 12/2015
2021/0087535	A1	3/2021	Lawrence et al.	CA	2943103 A1 3/2018
2021/0094982	A1	4/2021	Ludemann-Hombourger et al.	CA	3078956 A1 4/2019
2021/0095019	A1	4/2021	Wang et al.	CA	2811493 C 6/2020
2021/0100785	A1	4/2021	Stahly et al.	CN	1218960 A 6/1999
2021/0101974	A1	4/2021	Zhang	CN	101285069 A 10/2008
2021/0106681	A1	4/2021	Duroux et al.	CN	101469333 A 7/2009
2021/0107956	A1	4/2021	Brozik et al.	CN	101482509 A 7/2009
2021/0121504	A1	4/2021	Whitfill	CN	101482554 A 7/2009
2021/0128684	A1	5/2021	Dianzani et al.	CN	101605457 A 12/2009
2021/0130182	A1	5/2021	Vertelova et al.	CN	101208353 B 12/2011
2021/0130294	A1	5/2021	Michael et al.	CN	102875623 A 1/2013
2021/0139533	A1	5/2021	Mearns Spragg	CN	103097411 A 5/2013
2021/0139976	A1	5/2021	Ju et al.	CN	103124738 A 5/2013
2021/0145831	A1	5/2021	Cui et al.	CN	103145777 A 6/2013
2021/0154237	A1	5/2021	Beard et al.	CN	103923169 A 7/2014
2021/0155656	A1	5/2021	Falkenstein et al.	CN	103958491 A 7/2014
2021/0155677	A1	5/2021	Ingber et al.	CN	104152519 A 11/2014
2021/0164011	A1	6/2021	Schellenberger et al.	CN	104297225 A 1/2015
2021/0170012	A1	6/2021	Nizet et al.	CN	104774756 A 7/2015
2021/0188976	A1	6/2021	Chalons-Cottavoz et al.	CN	105273079 A 1/2016
2021/0208139	A1	7/2021	Sasso	CN	105738343 A 7/2016
2021/0220297	A1	7/2021	Reuveni et al.	CN	105899658 A 8/2016
2021/0220483	A1	7/2021	Davis et al.	CN	105934522 A 9/2016
2021/0228619	A1	7/2021	Peyman	CN	106295251 A 1/2017
2021/0230210	A1	7/2021	Olhava	CN	106460069 A 2/2017
2021/0230592	A1	7/2021	Scheinberg et al.	CN	106645079 A 5/2017
2021/0238045	A1	8/2021	Favaro et al.	CN	106674294 A 5/2017
2021/0238259	A1	8/2021	Van Der Flier et al.	CN	106749523 A 5/2017
2021/0246206	A1	8/2021	Liu et al.	CN	106769693 A 5/2017
2021/0246212	A1	8/2021	Salas et al.	CN	107226840 A 10/2017
2021/0260113	A1	8/2021	Kholin et al.	CN	107266569 A 10/2017
2021/0260201	A1	8/2021	Chukly et al.	CN	107383193 A 11/2017
2021/0261607	A1	8/2021	Zhu et al.	CN	107541533 A 1/2018
2021/0261655	A1	8/2021	Bannister et al.	CN	107722109 A 2/2018
2021/0269522	A1	9/2021	Wang et al.	CN	107778336 A 3/2018
2021/0277056	A1	9/2021	Miao et al.	CN	107824800 A 3/2018
2021/0277074	A1	9/2021	Schellenberger et al.	CN	108037107 A 5/2018
2021/0277079	A1	9/2021	Watters et al.	CN	108169203 A 6/2018
2021/0277377	A1	9/2021	Jacky et al.	CN	108239123 A 7/2018
2021/0283233	A1	9/2021	Kurtis et al.	CN	108267437 A 7/2018
2021/0283235	A1	9/2021	Curtiss, III et al.	CN	108459001 A 8/2018
2021/0284684	A1	9/2021	Tustian et al.	CN	108659118 A 10/2018
2021/0299154	A1	9/2021	Gallop et al.	CN	108660185 A 10/2018
2022/0259532	A1	8/2022	Raberg et al.	CN	108699568 A 10/2018
2022/0299370	A1	9/2022	Hu et al.	CN	108727486 A 11/2018
				CN	108732145 A 11/2018
				CN	109266717 A 1/2019
				CN	109342393 A 2/2019

(56)	References Cited			EP	3611495	A1	2/2020
	FOREIGN PATENT DOCUMENTS			EP	3709005	A1	9/2020
				ES	2331781	A1	1/2010
				FR	2964671	A1	3/2012
				GB	2467494	A	8/2010
CN	109342403	A	2/2019	GB	2485479	A	5/2012
CN	109354597	A	2/2019	JP	5-76346	A	3/1993
CN	109536474	A	3/2019	JP	2005-306827	A	11/2005
CN	109553662	A	4/2019	JP	3885054	B2	2/2007
CN	109627328	A	4/2019	JP	2007-302569	A	11/2007
CN	110078734	A	8/2019	JP	2007-530913	A	11/2007
CN	110117575	A	8/2019	JP	2009-517002	A	4/2009
CN	110144330	A	8/2019	JP	4250523	B2	4/2009
CN	110208238	A	9/2019	JP	2009-263273	A	11/2009
CN	110248951	A	9/2019	JP	4502814	B2	7/2010
CN	110286240	A	9/2019	JP	4726196	B2	7/2011
CN	110358739	A	10/2019	JP	4786656	B2	10/2011
CN	209460143	U	10/2019	JP	4881356	B2	2/2012
CN	110441287	A	11/2019	JP	5117191	B2	1/2013
CN	110501319	A	11/2019	JP	2013-537235	A	9/2013
CN	110646401	A	1/2020	JP	2013-541711	A	11/2013
CN	110669147	A	1/2020	JP	2014-516996	A	7/2014
CN	110804089	A	2/2020	JP	2016-512569	A	4/2016
CN	111153990	A	5/2020	JP	2016-156807	A	9/2016
CN	111194221	A	5/2020	JP	2016-531112	A	10/2016
CN	111201434	A	5/2020	JP	6069224	B2	2/2017
CN	111215141	A	6/2020	JP	2018-502090	A	1/2018
CN	111220589	A	6/2020	JP	2018-507180	A	3/2018
CN	111220590	A	6/2020	JP	2018-063131	A	4/2018
CN	111289489	A	6/2020	JP	2018-070626	A	5/2018
CN	111433592	A	7/2020	JP	6348635	B2	6/2018
CN	111454349	A	7/2020	JP	6359559	B2	7/2018
CN	111542507	A	8/2020	JP	2018-138594	A	9/2018
CN	111569939	A	8/2020	JP	2018-143137	A	9/2018
CN	111662879	A	9/2020	JP	6386461	B2	9/2018
CN	111763658	A	10/2020	JP	2018-531398	A	10/2018
CN	111888341	A	11/2020	JP	6402351	B2	10/2018
CN	111912826	A	11/2020	JP	2018-172403	A	11/2018
CN	111944027	A	11/2020	JP	2018-532696	A	11/2018
CN	112014372	A	12/2020	JP	2019-501658	A	1/2019
CN	112138644	A	12/2020	JP	2019-038836	A	3/2019
CN	112279909	A	1/2021	JP	2019-511582	A	4/2019
CN	112375754	A	2/2021	JP	6495256	B2	4/2019
CN	112409933	A	2/2021	JP	2019-513723	A	5/2019
CN	112458062	A	3/2021	JP	6522826	B2	5/2019
CN	112521455	A	3/2021	JP	6525872	B2	6/2019
CN	112639456	A	4/2021	JP	2019-108371	A	7/2019
CN	112725407	A	4/2021	JP	2019-522799	A	8/2019
CN	112834749	A	5/2021	JP	2019-163317	A	9/2019
CN	112979784	A	6/2021	JP	6588039	B2	10/2019
CN	112979814	A	6/2021	JP	2019-208511	A	12/2019
CN	112979815	A	6/2021	JP	2020-500157	A	1/2020
CN	113004392	A	6/2021	JP	6637241	B2	1/2020
CN	113045663	A	6/2021	JP	2020-514278	A	5/2020
CN	113173994	A	7/2021	JP	2020-521443	A	7/2020
CN	113214358	A	8/2021	JP	6722697	B2	7/2020
CN	113214399	A	8/2021	JP	2020-523990	A	8/2020
CN	113234166	A	8/2021	JP	2020-172517	A	10/2020
CN	113286884	A	8/2021	JP	2020-180975	A	11/2020
CN	113354703	A	9/2021	JP	2020-532497	A	11/2020
CN	113444721	A	9/2021	JP	2020-532993	A	11/2020
CN	113454460	A	9/2021	JP	2020-533582	A	11/2020
CZ	299996	B6	1/2009	JP	2020-536497	A	12/2020
CZ	29065	U1	1/2016	JP	2020-536521	A	12/2020
CZ	2015288	A3	11/2016	JP	2020-537126	A	12/2020
CZ	308447	B6	8/2020	JP	6810461	B2	1/2021
DE	10217948	A1	11/2003	JP	2021-048872	A	4/2021
EA	006368	B1	12/2005	JP	6870087	B2	5/2021
EA	007413	B1	10/2006	JP	6873090	B2	5/2021
EA	009294	B1	12/2007	JP	2021-092573	A	6/2021
EA	017887	B1	3/2013	JP	6908605	B2	7/2021
EA	026112	B1	3/2017	JP	2021-518145	A	8/2021
EA	028162	B1	10/2017	JP	2021-521412	A	8/2021
EA	032327	B1	5/2019	JP	6915224	B2	8/2021
EP	2326955	A1	6/2011	JP	2021-524835	A	9/2021
EP	2707030	A1	3/2014	KR	100868248	B1	11/2008
EP	2831587	A1	2/2015	KR	101227434	B1	1/2013
EP	2972238	A1	1/2016	KR	101297667	B1	8/2013
EP	3134104	A1	3/2017	KR	101360405	B1	2/2014
EP	3380825	A1	10/2018				

(56)

References Cited

FOREIGN PATENT DOCUMENTS

KR	101438047	B1	9/2014	WO	WO-2018/188395	A1	10/2018
KR	101496671	B1	3/2015	WO	WO-2018/195134	A1	10/2018
KR	101528440	B1	6/2015	WO	WO-2018/195491	A1	10/2018
KR	101558160	B1	10/2015	WO	WO-2018/237327	A1	12/2018
KR	101669954	B1	10/2016	WO	WO-2019/028285	A2	2/2019
KR	101798295	B1	11/2017	WO	WO-2019/030377	A1	2/2019
KR	20180043835	A	4/2018	WO	WO-2019/032463	A1	2/2019
KR	101860436	B1	5/2018	WO	WO-2019/060685	A1	3/2019
KR	10-2018-0059739	A	6/2018	WO	WO-2019/062689	A1	4/2019
KR	20180094877	A	8/2018	WO	WO-2019/071076	A1	4/2019
KR	101907026	B1	10/2018	WO	WO-2019/079165	A1	4/2019
KR	101919427	B1	11/2018	WO	WO-2019/084512	A1	5/2019
KR	101927864	B1	12/2018	WO	WO-2019/117177	A1	6/2019
KR	20190009512	A	1/2019	WO	WO-2019/148140	A2	8/2019
KR	10-2019-0054746	A	5/2019	WO	WO-2019/157263	A1	8/2019
KR	101974733	B1	5/2019	WO	WO-2019/165105	A1	8/2019
KR	101979000	B1	5/2019	WO	WO-2019/165134	A1	8/2019
KR	102008608	B1	8/2019	WO	WO-2019/185860	A1	10/2019
KR	102012123	B1	8/2019	WO	WO-2019/204508	A1	10/2019
KR	102008609	B1	10/2019	WO	WO-2019/208594	A1	10/2019
KR	20190125891	A	11/2019	WO	WO-2019/211531	A1	11/2019
KR	10-2020-0070218	A	6/2020	WO	WO-2019/216288	A1	11/2019
KR	102169268	B1	10/2020	WO	WO-2019/236447	A1	12/2019
KR	102194995	B1	12/2020	WO	WO-2019/246013	A1	12/2019
KR	102196156	B1	12/2020	WO	WO-2020/007326	A1	1/2020
KR	102196159	B1	12/2020	WO	WO-2020/037117	A1	2/2020
KR	102202082	B1	1/2021	WO	WO-2020/038426	A1	2/2020
KR	102227251	B1	3/2021	WO	WO-2020/041200	A1	2/2020
KR	102227257	B1	3/2021	WO	WO-2020/081598	A1	4/2020
KR	102250446	B1	5/2021	WO	WO-2020/082061	A1	4/2020
KR	102252798	B1	5/2021	WO	WO-2020/086635	A1	4/2020
KR	20210061075	A	5/2021	WO	WO-2020/087040	A1	4/2020
KR	20210073785	A	6/2021	WO	WO-2020/090225	A1	5/2020
RU	2531754	C2	10/2014	WO	WO-2020/092835	A1	5/2020
RU	2589695	C2	7/2016	WO	WO-2020/096965	A1	5/2020
RU	2745511	C1	3/2021	WO	WO-2020/106997	A1	5/2020
SG	183721	A1	9/2012	WO	WO-2020/108735	A1	6/2020
SG	1120201127	T	3/2020	WO	WO-2020/115196	A1	6/2020
TW	201249480	A	12/2012	WO	WO-2020/115661	A1	6/2020
TW	1475209	B	3/2015	WO	WO-2020/124271	A1	6/2020
TW	201529604	A	8/2015	WO	WO-2020/131192	A2	6/2020
TW	201741461	A	12/2017	WO	WO-2020/132074	A1	6/2020
TW	201928042	A	7/2019	WO	WO-2020/150751	A2	7/2020
TW	202033949	A	9/2020	WO	WO-2020/157752	A1	8/2020
TW	202043254	A	12/2020	WO	WO-2020/160462	A1	8/2020
TW	202044131	A	12/2020	WO	WO-2020/162601	A1	8/2020
TW	1734166	B	7/2021	WO	WO-2020/180003	A1	9/2020
TW	202128743	A	8/2021	WO	WO-2020/180534	A1	9/2020
TW	202128745	A	8/2021	WO	WO-2020/186026	A1	9/2020
WO	WO-1997/036540	A1	10/1997	WO	WO-2020/206055	A1	10/2020
WO	WO-2012/037430	A1	3/2012	WO	WO-2020/210476	A1	10/2020
WO	WO-2012/040041	A1	3/2012	WO	WO-2020/210836	A1	10/2020
WO	WO-2014/137291	A1	9/2014	WO	WO-2020/213993	A1	10/2020
WO	WO-2014/170684	A1	10/2014	WO	WO-2020/217895	A1	10/2020
WO	WO-2015/095255	A1	6/2015	WO	WO-2020/218976	A1	10/2020
WO	WO-2015/145149	A1	10/2015	WO	WO-2020/223125	A1	11/2020
WO	WO-2016/004322	A2	1/2016	WO	WO-2020/226513	A1	11/2020
WO	WO-2016/060171	A1	4/2016	WO	WO-2020/227571	A1	11/2020
WO	WO-2016/172350	A1	10/2016	WO	WO-2020/237221	A1	11/2020
WO	WO-2016/196315	A2	12/2016	WO	WO-2020/237304	A1	12/2020
WO	WO-2017/164815	A1	9/2017	WO	WO-2020/238918	A1	12/2020
WO	WO-2018/028634	A1	2/2018	WO	WO-2020/240024	A1	12/2020
WO	WO-2018/031954	A1	2/2018	WO	WO-2020/247730	A1	12/2020
WO	WO-2018/034205	A1	2/2018	WO	WO-2020/247952	A2	12/2020
WO	WO-2018/049372	A1	3/2018	WO	WO-2020/251802	A1	12/2020
WO	WO-2018/058073	A2	3/2018	WO	WO-2020/252266	A1	12/2020
WO	WO-2018/093777	A1	5/2018	WO	WO-2020/252413	A1	12/2020
WO	WO-2018/103038	A1	6/2018	WO	WO-2020/254176	A1	12/2020
WO	WO-2018/111941	A1	6/2018	WO	WO-2020/260073	A1	12/2020
WO	WO-2018/132389	A1	7/2018	WO	WO-2020/260229	A1	12/2020
WO	WO-2018/140041	A1	8/2018	WO	WO-2020/261245	A1	12/2020
WO	WO-2018/156649	A1	8/2018	WO	WO-2021/007111	A1	1/2021
WO	WO-2018/159833	A1	9/2018	WO	WO-2021/007458	A1	1/2021
WO	WO-2018/175346	A1	9/2018	WO	WO-2021/009422	A1	1/2021
WO	WO-2018/183876	A1	10/2018	WO	WO-2021/011927	A1	1/2021
				WO	WO-2021/019167	A1	2/2021
				WO	WO-2021/026172	A1	2/2021
				WO	WO-2021/030672	A1	2/2021
				WO	WO-2021/041759	A1	3/2021

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO-2021/058657	A1	4/2021
WO	WO-2021/059058	A1	4/2021
WO	WO-2021/064219	A1	4/2021
WO	WO-2021/080847	A1	4/2021
WO	WO-2021/081206	A1	4/2021
WO	WO-2021/084538	A1	5/2021
WO	WO-2021/097230	A1	5/2021
WO	WO-2021/099465	A1	5/2021
WO	WO-2021/108809	A1	6/2021
WO	WO-2021/112662	A1	6/2021
WO	WO-2021/123074	A1	6/2021
WO	WO-2021/130390	A1	7/2021
WO	WO-2021/133943	A1	7/2021
WO	WO-2021/137655	A1	7/2021
WO	WO-2021/138676	A1	7/2021
WO	WO-2021/142671	A1	7/2021
WO	WO-2021/145796	A2	7/2021
WO	WO-2021/148488	A2	7/2021
WO	WO-2021/151974	A1	8/2021
WO	WO-2021/163239	A1	8/2021
WO	WO-2021/168083	A1	8/2021
WO	WO-2021/177050	A1	9/2021
WO	WO-2021/195589	A1	9/2021
WO	WO-2022/003359	A1	1/2022

OTHER PUBLICATIONS

Alberts et al., *Molecular Biology of the Cell*, Fourth Edition, Newton Press. pp. 69-70, 107-108, 186-187, 616-619, Dec. 20, 2004.

Ashton et al., The challenge of applying Raman spectroscopy to monitor recombinant antibody production. *Analyst*. Nov. 21, 2013;138(22):6977-85.

Baradez et al., Application of Raman Spectroscopy and Univariate Modelling as a Process Analytical Technology for Cell Therapy Bioprocessing. *Front Med (Lausanne)*. Mar. 5, 2018;5:47, 14 pages.

Berry et al., Quick generation of Raman spectroscopy based in-process glucose control to influence biopharmaceutical protein product quality during mammalian cell culture. *Biotechnol Prog.* Jan.-Feb. 2016;32(1):224-34.

Betty et al., Frequency Response Plots for Savitzky-Golay Filter Functions. *Anal Chem*. Feb. 1977;49(2):351-352.

Buckley et al., Applications of Raman Spectroscopy in Biopharmaceutical Manufacturing: A Short Review. *Appl Spectrosc.* Jun. 2017;71(6):1085-1116.

Carey, Biochemical Applications of Raman and Resonance Raman Spectroscopies. *FEBS Letters*. Jun. 1983;156(1):191.

Culka et al., Acquisition of Raman spectra of amino acids using portable instruments: outdoor measurements and comparison. *Spectrochim Acta A Mol Biomol Spectrosc.* Dec. 2010;77(5):978-83.

Encyclopedia of Cell Biology. Asakura Shoten. pp. 366-367, (2005).

Haberger et al., Assessment of chemical modifications of sites in the CDRs of recombinant antibodies: Susceptibility vs. functionality of critical quality attributes. *MAbs*. Mar.-Apr. 2014;6(2):327-39.

Harada et al., Origin of the doublet at 1360 and 1340 cm in the Raman spectra of tryptophan and related compounds. *Spectrochimica Acta*. 1986;42A(2/3):307-312.

Hodge, Dehydrated Foods. *Chemistry of Browning Reactions in Model Systems. Agricultural and Food Chemistry*. Oct. 14, 1953;1(15):928-943.

Lewis et al., Combined dynamic light scattering and Raman spectroscopy approach for characterizing the aggregation of therapeutic proteins. *Molecules*. Dec. 12, 2014;19(12):20888-905.

Li et al., Cysteine Conformation and Sulfhydryl Interactions in Proteins and Viruses. 1. Correlation of the Raman S-H Band with Hydrogen Bonding and Intramolecular Geometry in Model Compounds. *J Am Chem Soc*. 1991;113:456-462.

Li et al., Cysteine Conformation and Sulfhydryl Interactions in Proteins and Viruses. 2. Normal Coordinate Analysis of the Cysteine Side Chain in Model Compounds. *J Am Chem Soc*. 1992;114:7463-7469.

Li et al., Rapid characterization and quality control of complex cell culture media solutions using Raman spectroscopy and chemometrics. *Biotechnol Bioeng.* Oct. 1, 2010;107(2):290-301.

Milligan et al., Semisynthetic model calibration for monitoring glucose in mammalian cell culture with in situ near infrared spectroscopy. *Biotechnol Bioeng.* May 2014;111(5):896-903.

Miura et al., Tryptophan Raman Bands Sensitive to Hydrogen Bonding and Side-Chain Conformation. *Journal of Raman Spectroscopy*. 1989;20:667-671.

Mungikar et al., Use of In-Line Raman Spectroscopy as a Non-destructive and Rapid Analytical Technique to Monitor Aggregation of a Therapeutic Protein. *American Pharmaceutical Review*. <https://www.americanpharmaceuticalreview.com>. 8 pages, Nov. 1, 2010.

Pitters et al., Raman Spectroscopy as a Real-Time In Situ Analyzer for Cell Culture Bioprocesses. *J Bioanal Biomed*. 2016;8(3 suppl.):51.

Schwartz et al., Diafiltration: A Fast, Efficient Method for Desalting, or Buffer Exchange of Biological Samples. *PALL, Life Sciences*. www.pall.com, Scientific & Technical Report, PN 33289. 6 pages, (2003).

Stoner et al., Protein-solute interactions affect the outcome of ultrafiltration/diafiltration operations. *J Pharm Sci.* Sep. 2004;93(9):2332-42.

Sugeta et al., Vibrational Spectra and Molecular Conformations of Dialkyl Disulfides. *Bulletin of the Chemical Society of Japan*. Nov. 1973;46:3407-3411.

Sugeta, Normal vibrations and molecular conformations of dialkyl disulfides. *Spectrochimica Acta*. 1975;31A:1729-1737.

Van Wart et al., Agreement with the disulfide stretching frequency-conformation correlation of Sugeta, Go, and Miyazawa. *Proc Natl Acad Sci U S A*. May 1986;83(10):3064-7.

Van Wart et al., Disulfide bond dihedral angles from Raman spectroscopy. *Proc Natl Acad Sci U S A*. Sep. 1973;70(9):2619-23.

Wen et al., Application of Raman Spectroscopy in Biopharmaceutical Manufacturing. *American Pharmaceutical Review*. <https://www.americanpharmaceuticalreview.com>. 10 pages, May 1, 2010.

Wen et al., Ultraviolet-resonance Raman spectroscopy of the filamentous virus Pf3: interactions of Trp 38 specific to the assembled virion subunit. *Biochemistry*. Jan. 11, 2000;39(1):146-52.

Wen, Raman spectroscopy of protein pharmaceuticals. *J Pharm Sci*. Nov. 2007;96(11):2861-78.

Whelan et al., In situ Raman spectroscopy for simultaneous monitoring of multiple process parameters in mammalian cell culture bioreactors. *Biotechnol Prog.* Sep.-Oct. 2012;28(5):1355-62.

Yamamoto et al., Development of Raman Optical Activity Spectrometer and Structural Analysis of Proteins in Solution. *Bunseki Kagaku*. 2013;62(5):409-422.

Yang et al., Effects of ammonia on CHO cell growth, erythropoietin production, and glycosylation. *Biotechnol Bioeng.* May 20, 2000;68(4):370-80.

Yuk et al., Controlling glycation of recombinant antibody in fed-batch cell cultures. *Biotechnol Bioeng.* Nov. 2011;108(11):2600-10.

International Preliminary Report on Patentability for Application No. PCT/US2018/055837, dated Apr. 30, 2020, 7 pages.

International Search Report and Written Opinion for Application No. PCT/US2018/055837, dated Jan. 8, 2019, 9 pages.

International Search Report and Written Opinion for Application No. PCT/US2019/048100, dated Nov. 20, 2019, 11 pages.

Japanese Office Action for Application No. 2020-083562, dated Dec. 1, 2022, 10 pages.

Singapore Office Action for Application No. 11202001127T, dated Dec. 4, 2020, 11 pages.

U.S. Appl. No. 16/160,194, filed Oct. 15, 2018, 2019-0112569, Published.

U.S. Appl. No. 16/550,989, filed Aug. 26, 2019, U.S. Pat. No. 11,358,984, Issued.

* cited by examiner

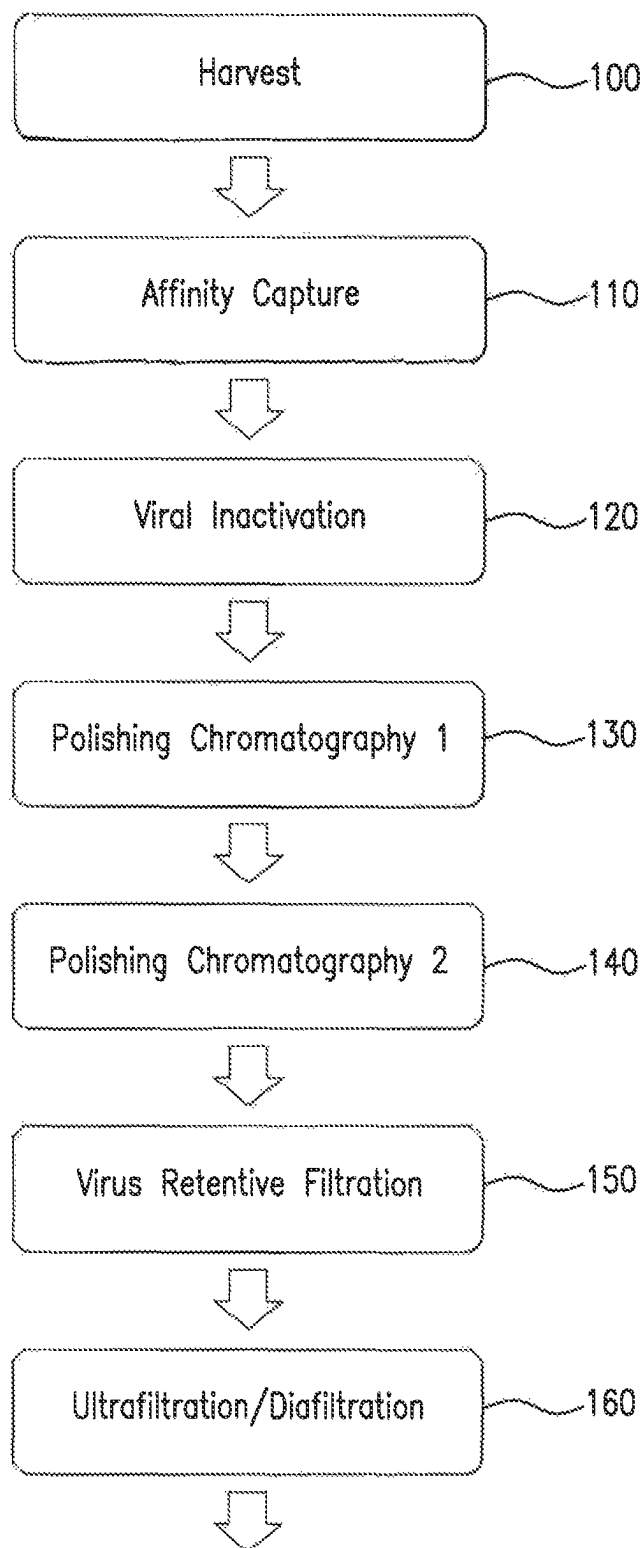


FIG. 1

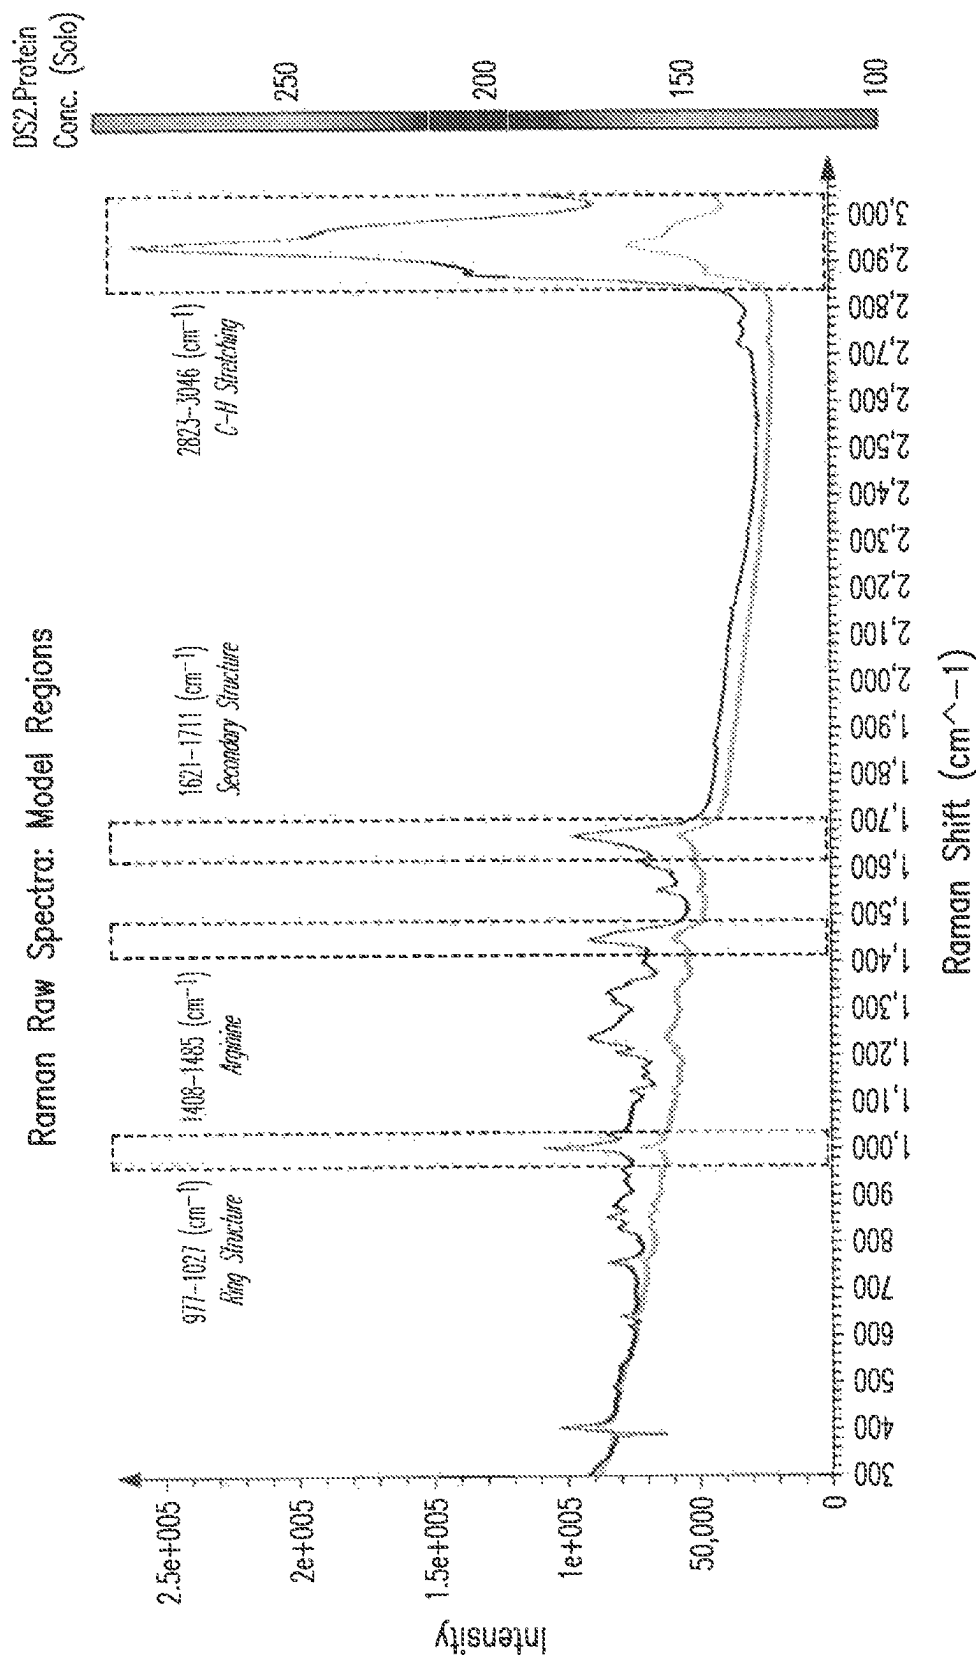


FIG. 2

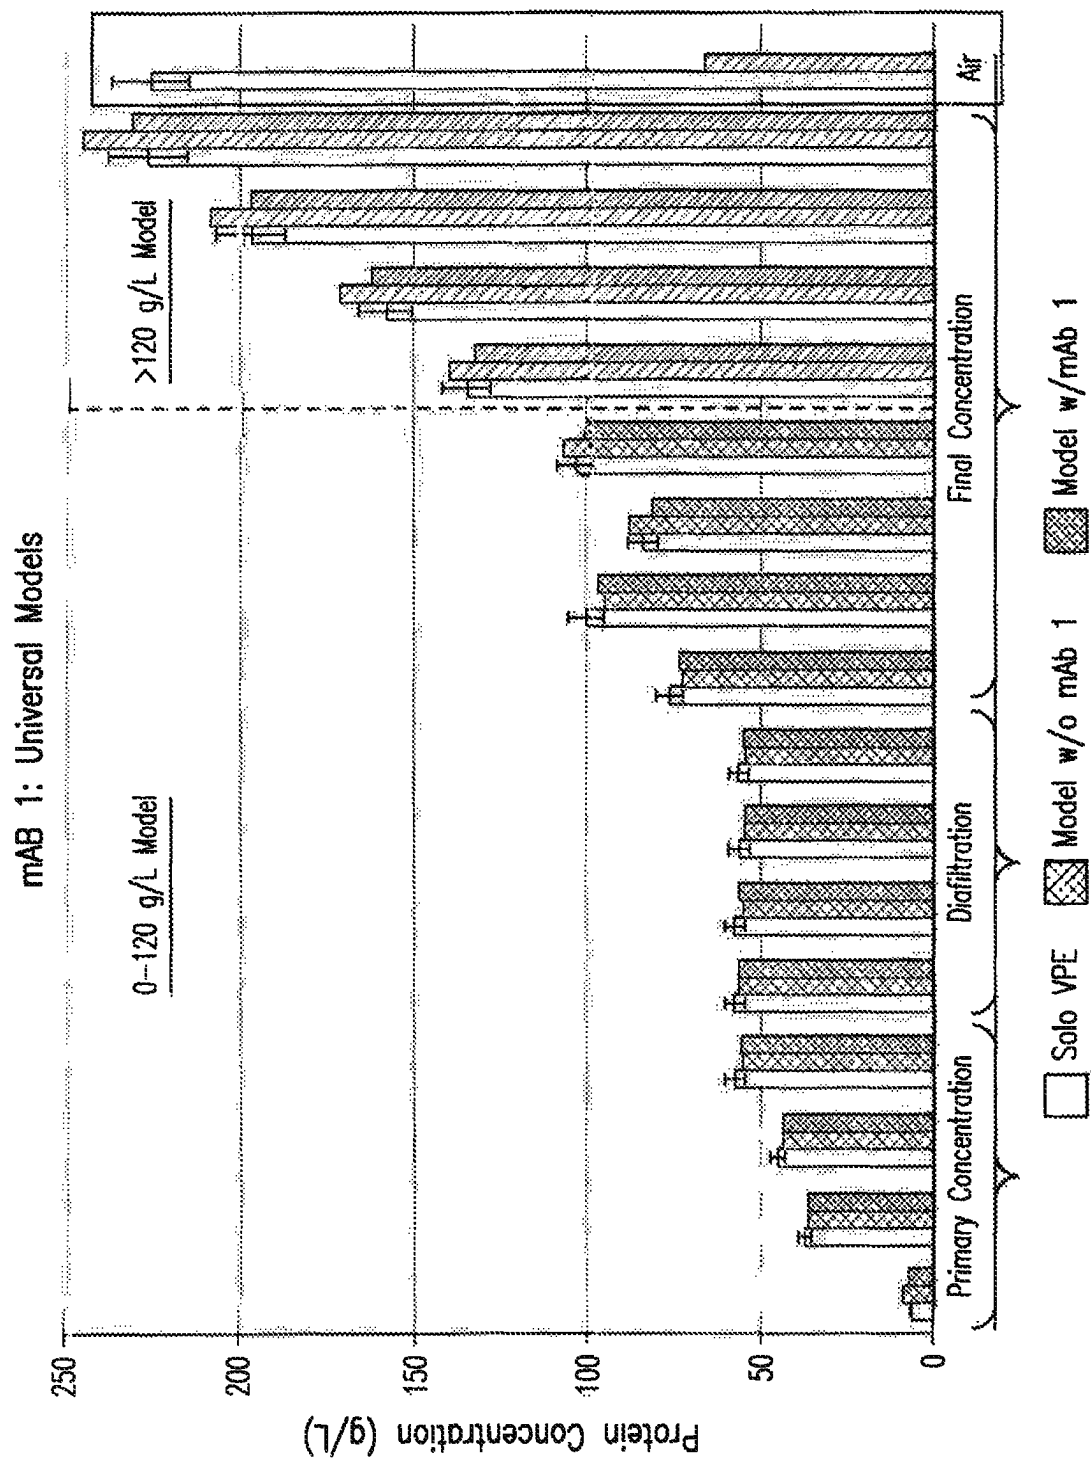


FIG. 3

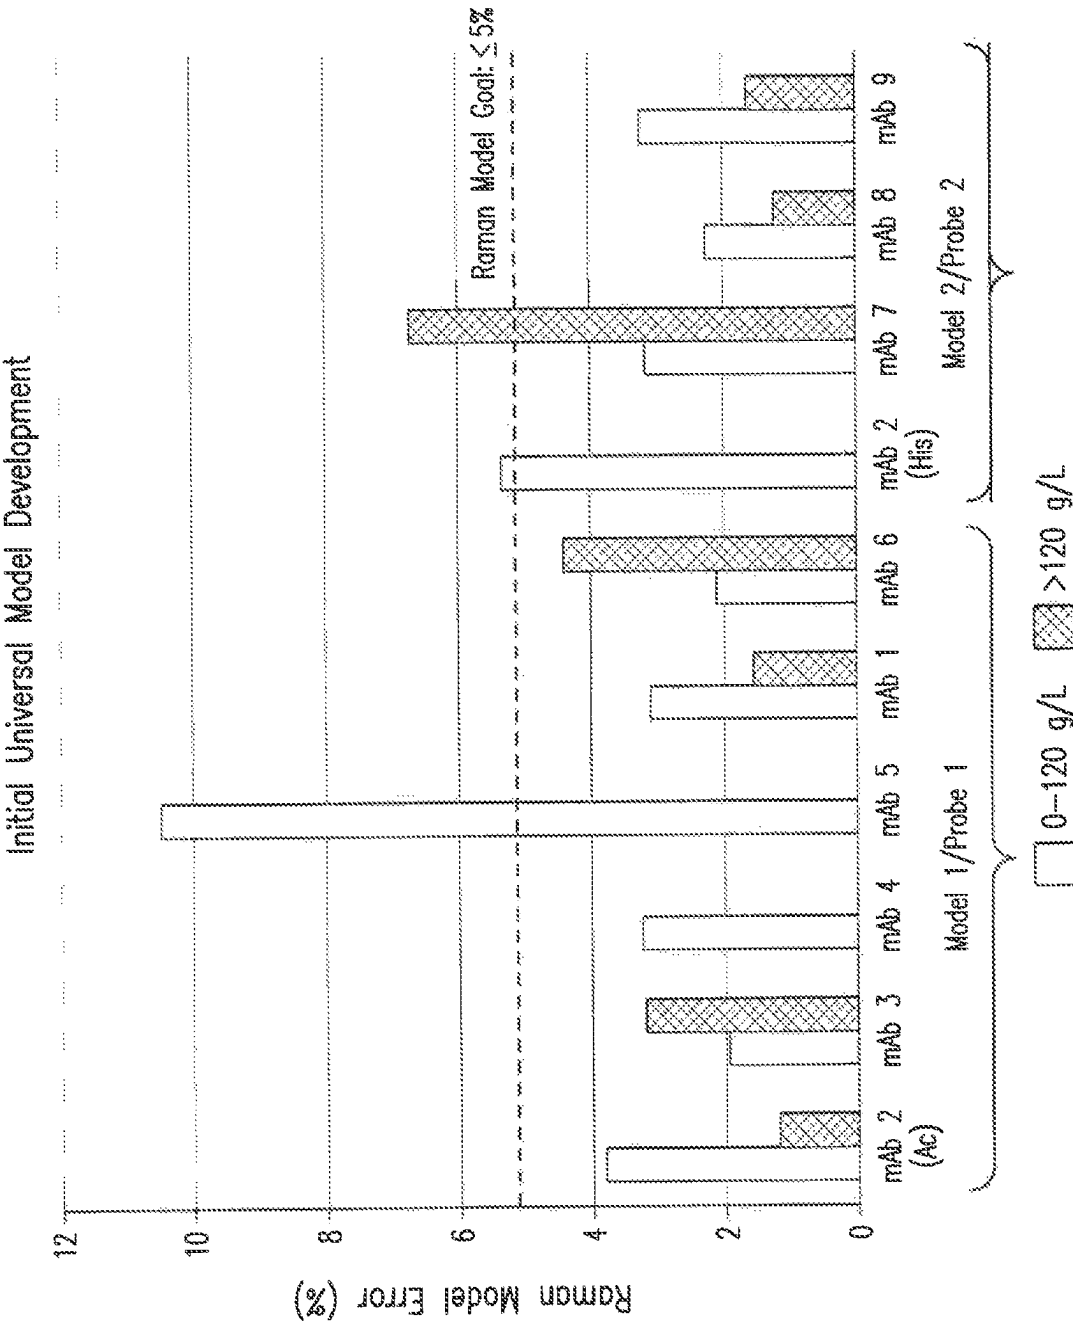


FIG. 4


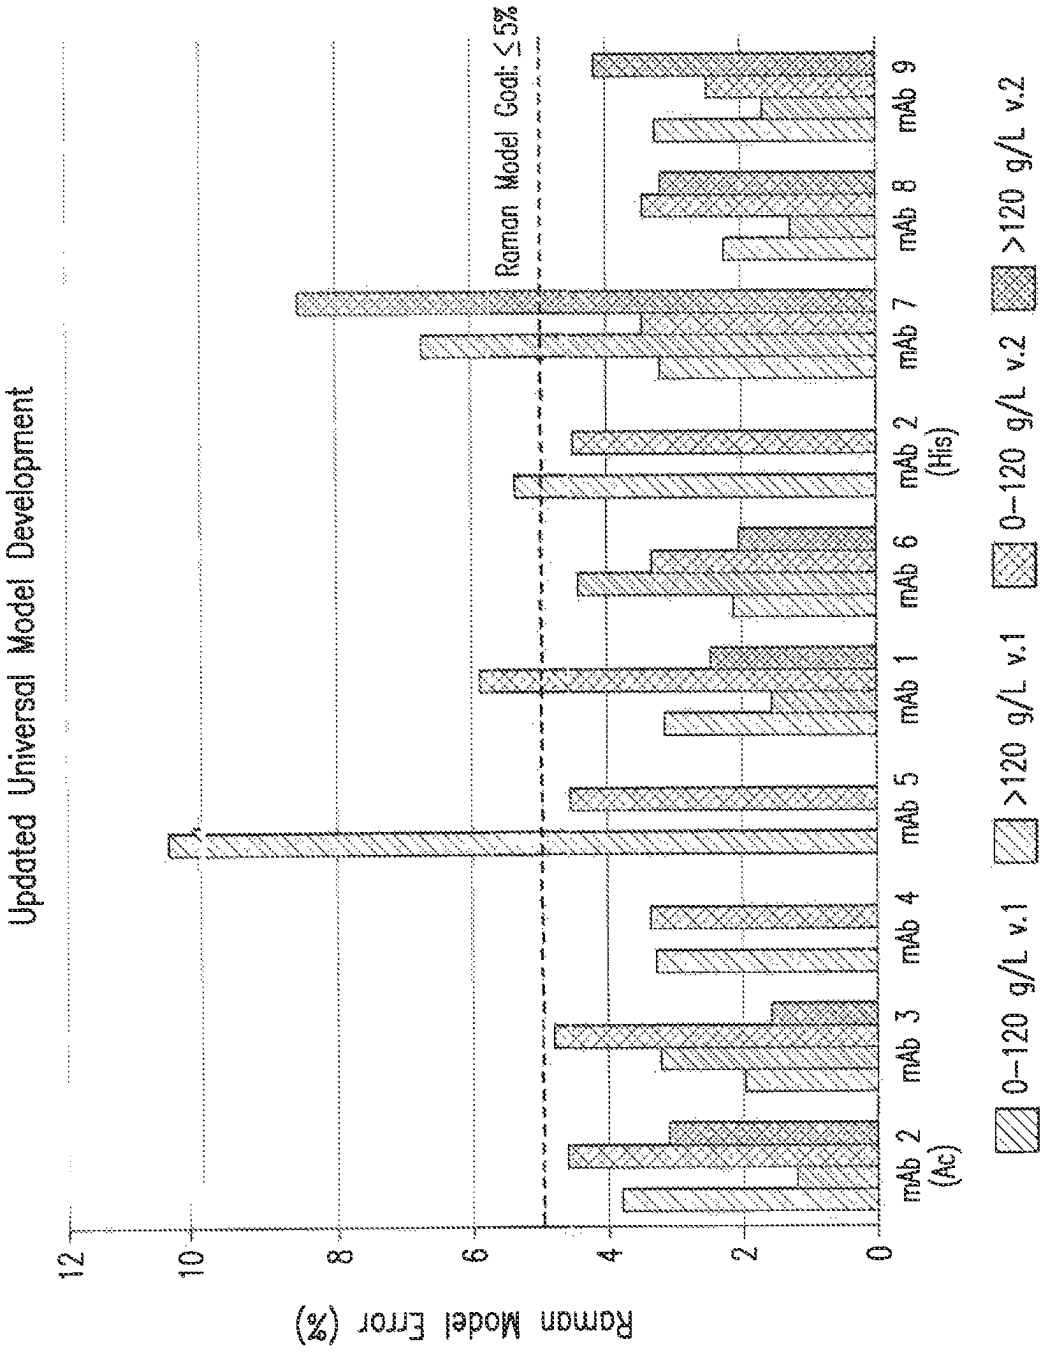


FIG. 5

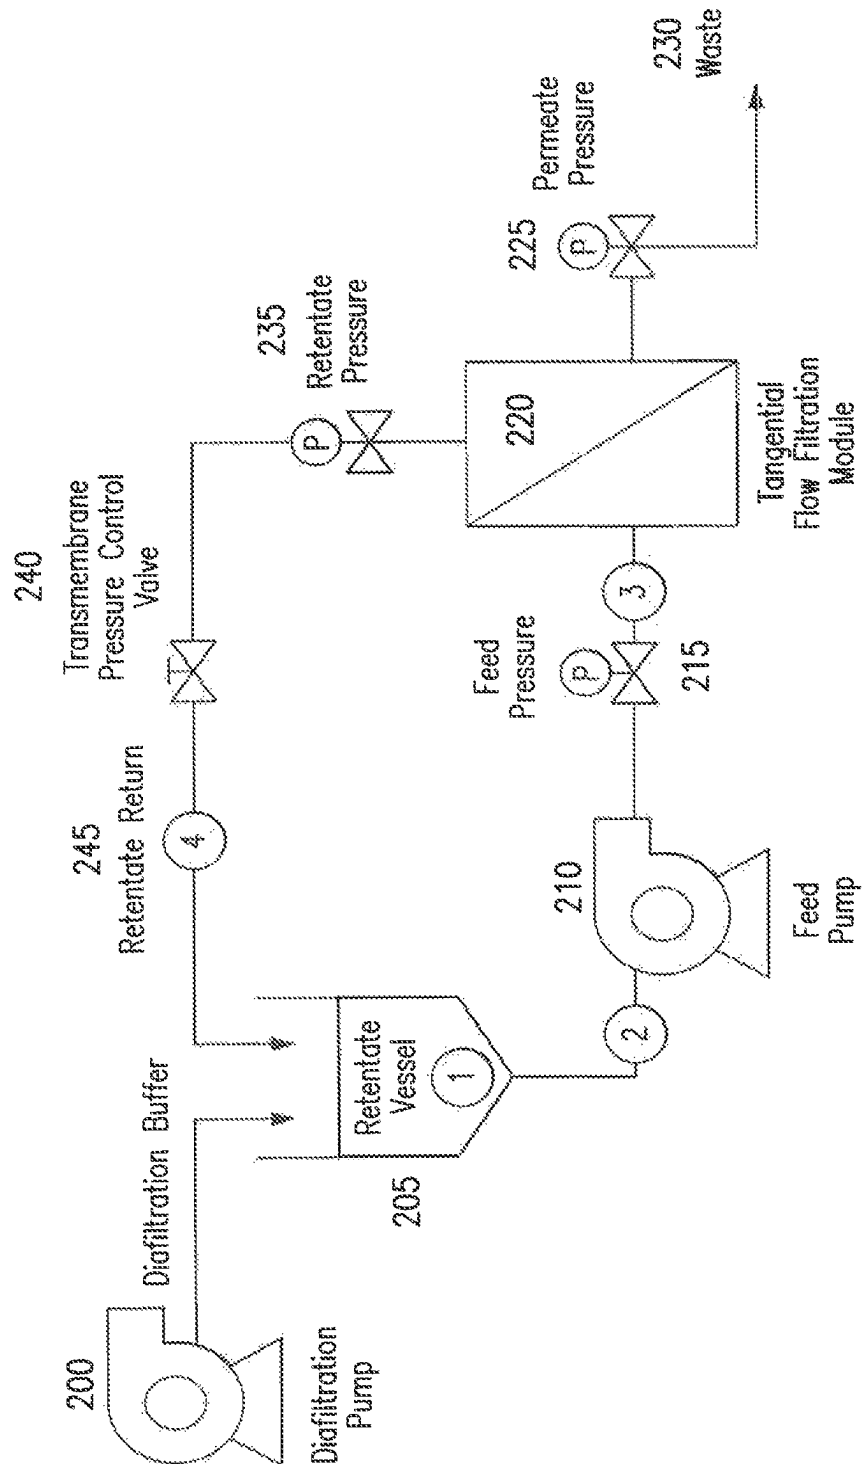

66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891

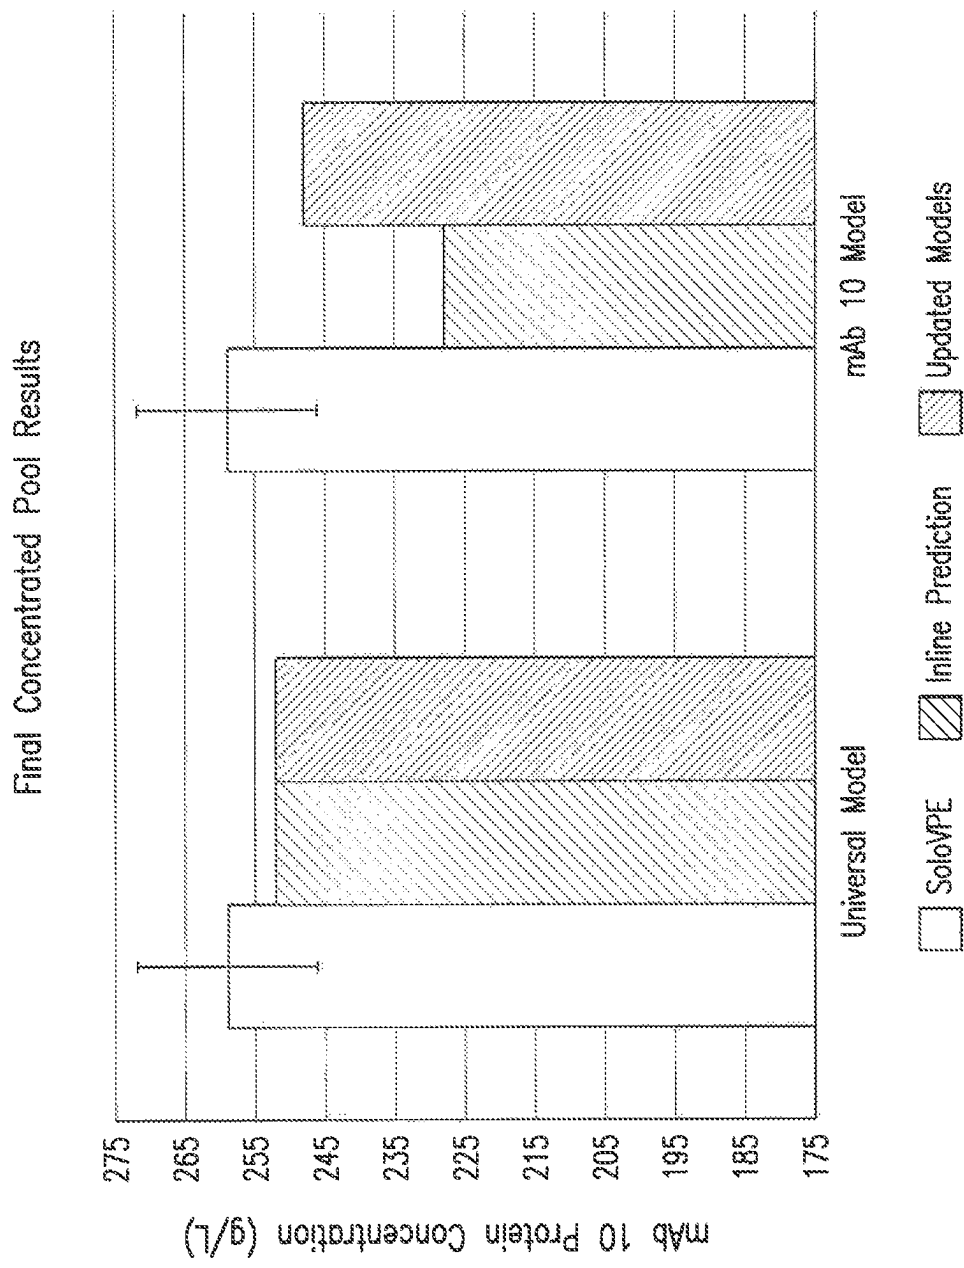


FIG. 7

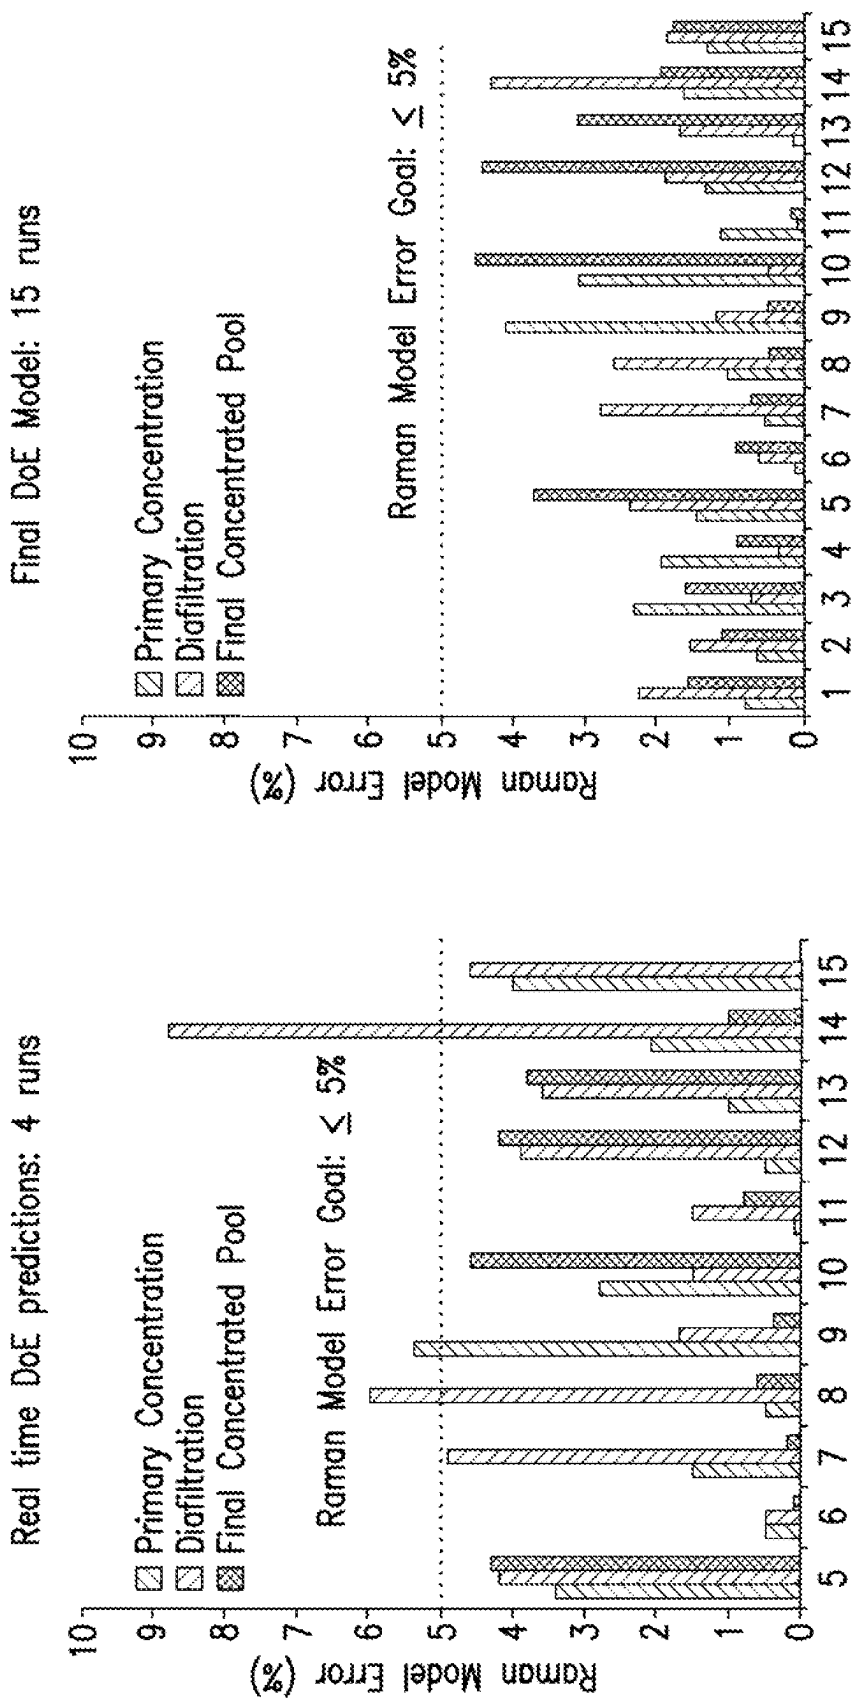


FIG.8A

FIG.8B

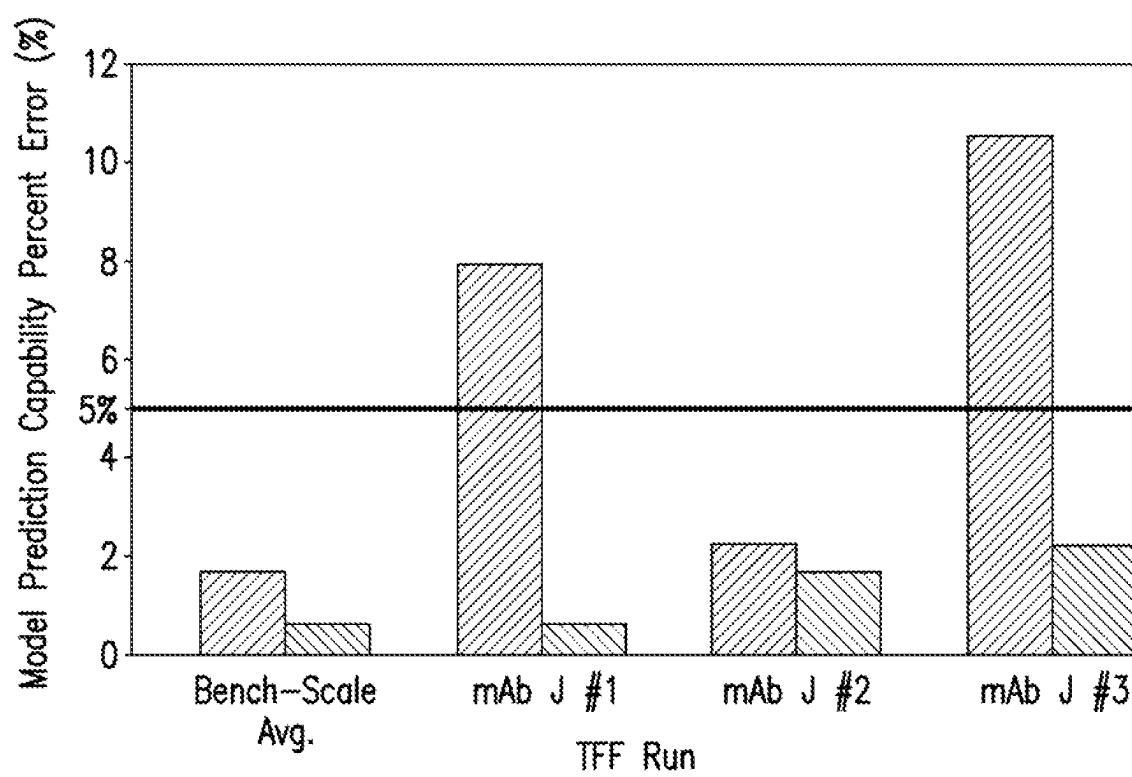


FIG. 9A


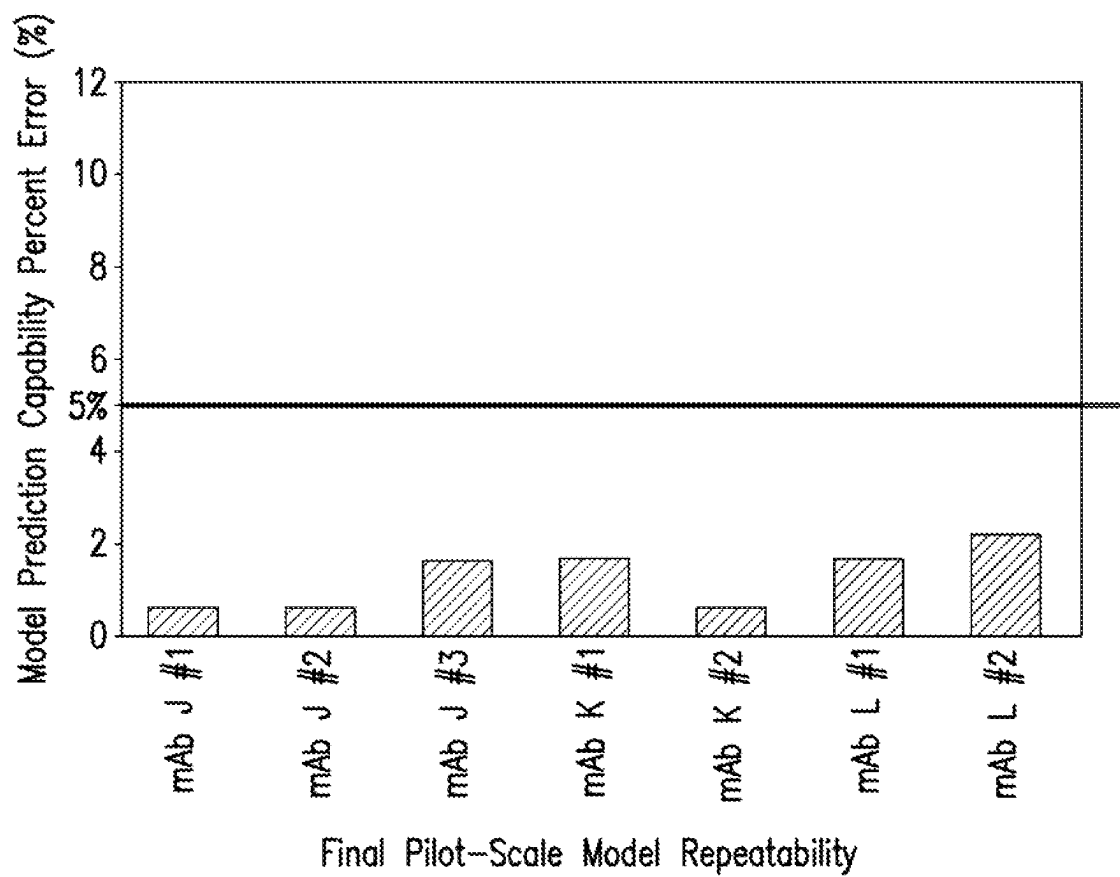


FIG.9B

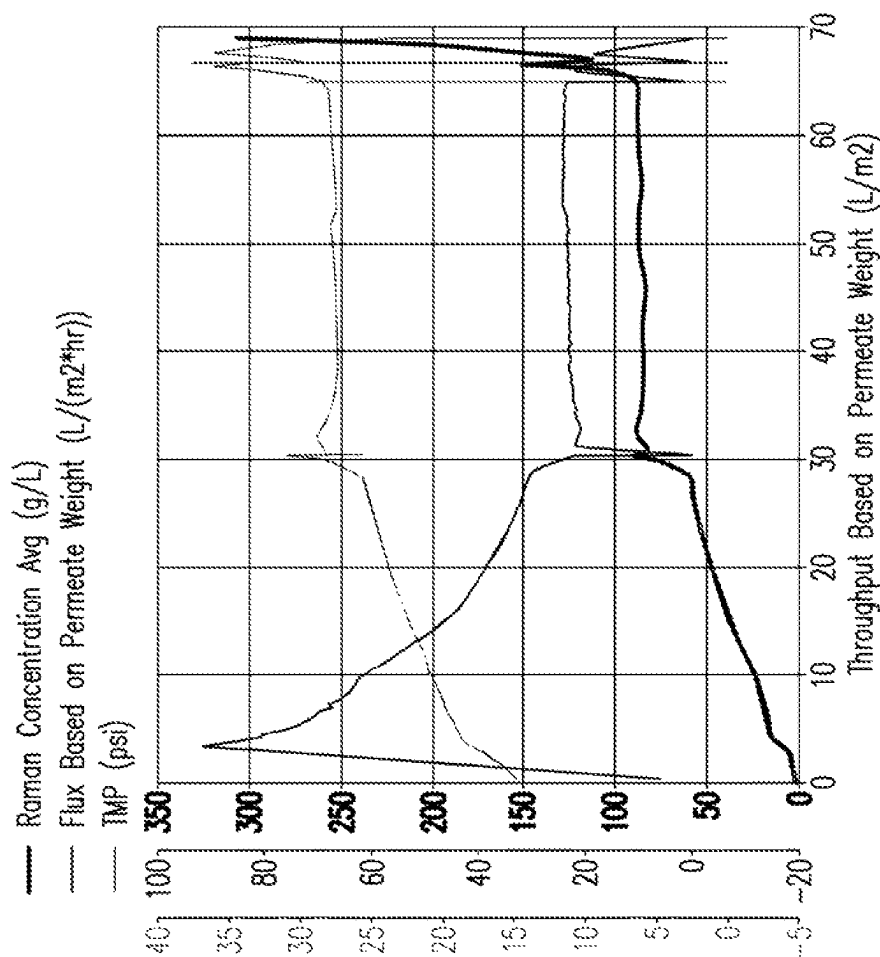

Experiment ID: LVCA2 UFDF 190627
System Status: Ready to Offload
Final Concentration Target: 295 g/L
Raman Concentration Avg: 304.1 g/L
Raman Concentration SD: 1.1 g/L
Processing Time: 160.8 min
Recirculation Time: 20.0 min

System Message: Ready to offload. Switch pump to Manual. Press "Acknowledge" to terminate orchestration

FIG. 10A


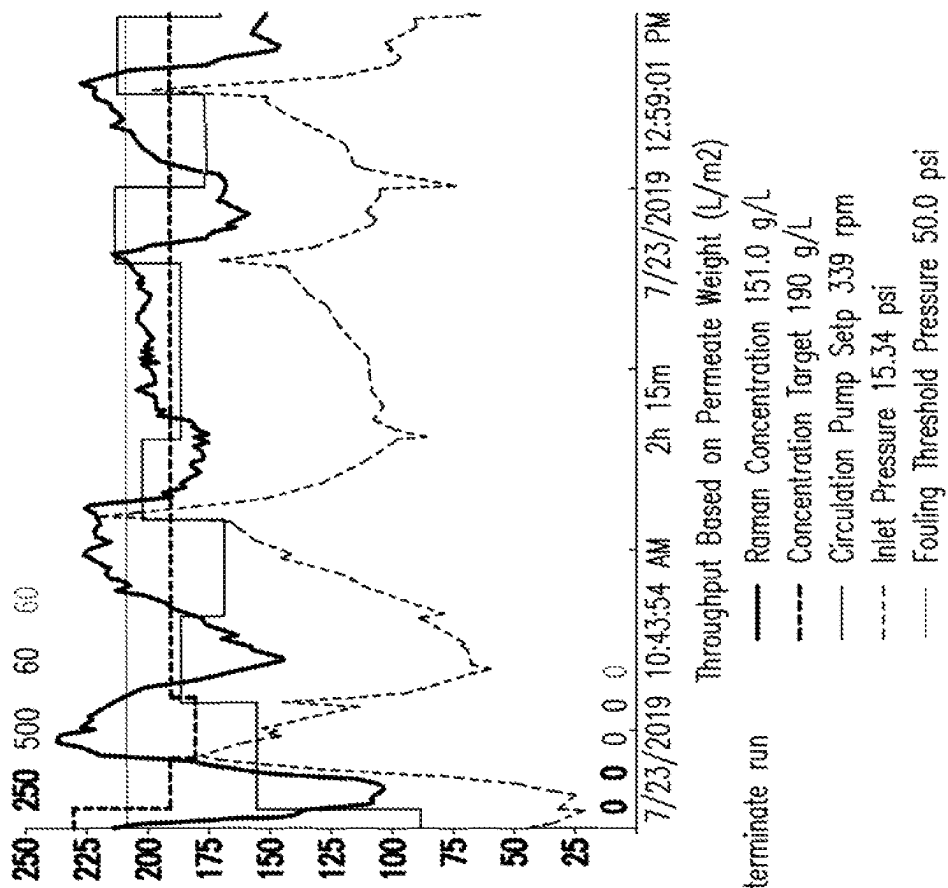


FIG.10B

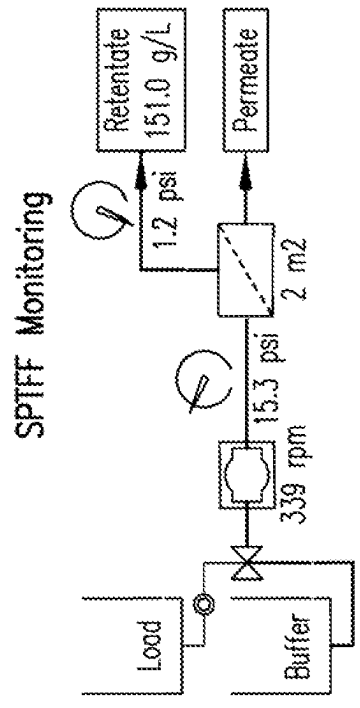

Experiment ID: Automated SPTFF 22July2019
System Status: Post-Use Buffer Flush
Final Concentration Target: 190 g/L
Raman Concentration Avg: 151.0 g/L
Raman Concentration SD: 5.8 g/L

System Message: Buffer flush in progress. Press "Acknowledge" to terminate run

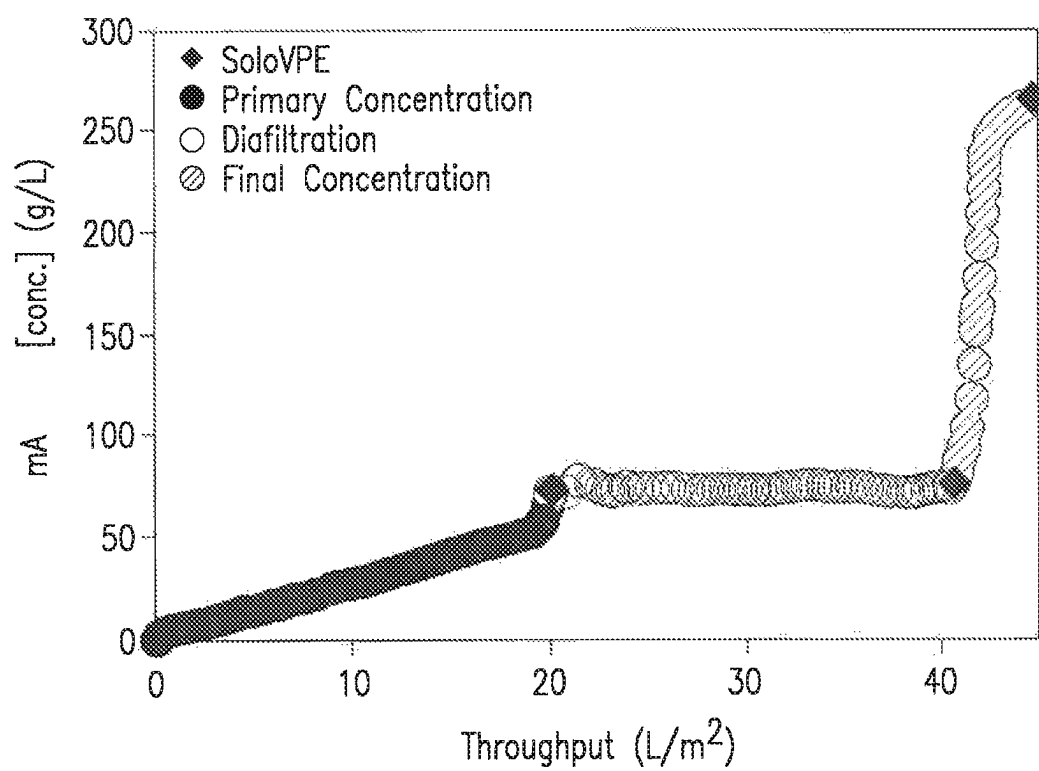


FIG. 11

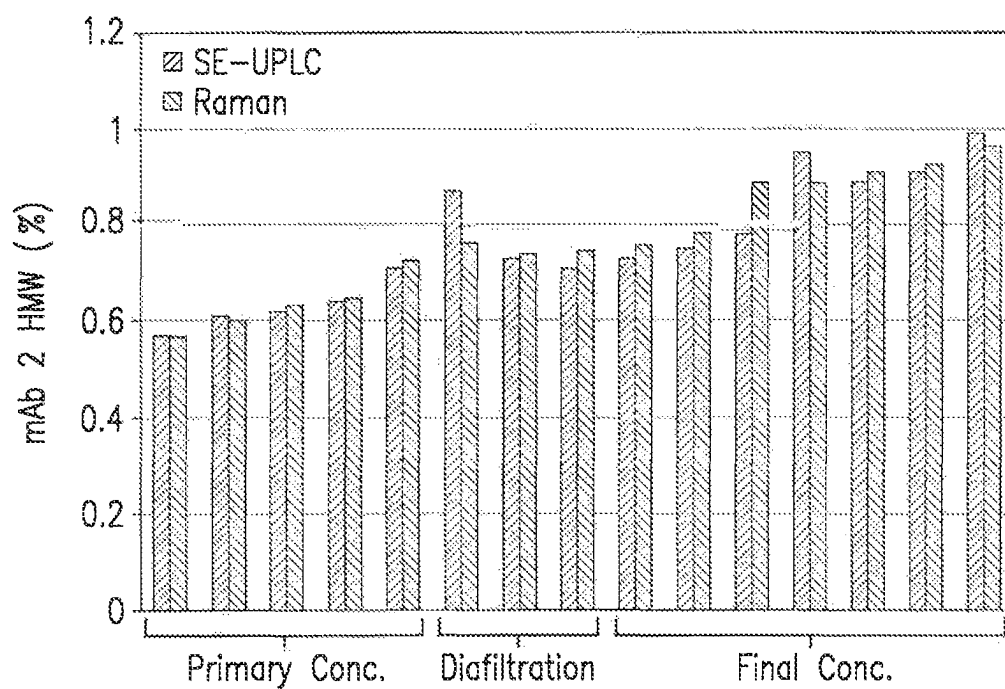


FIG. 12A

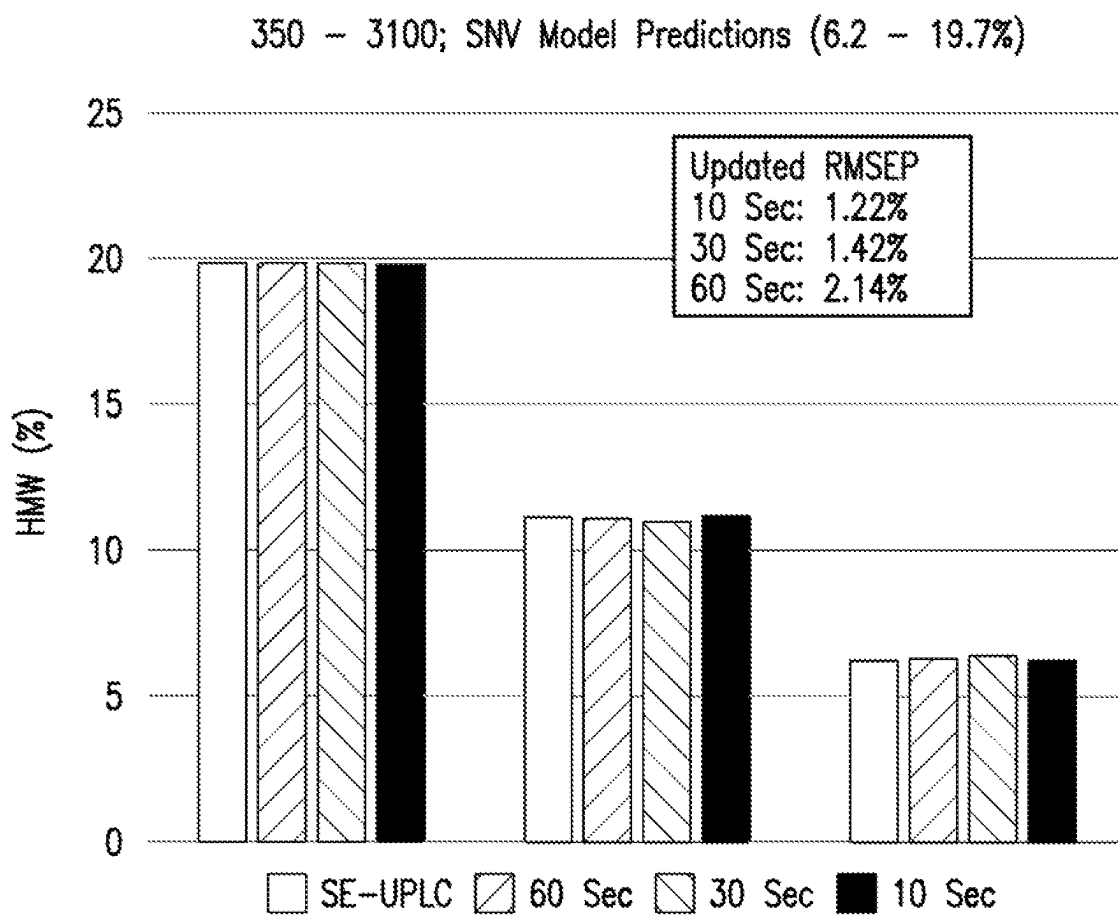


FIG. 12B

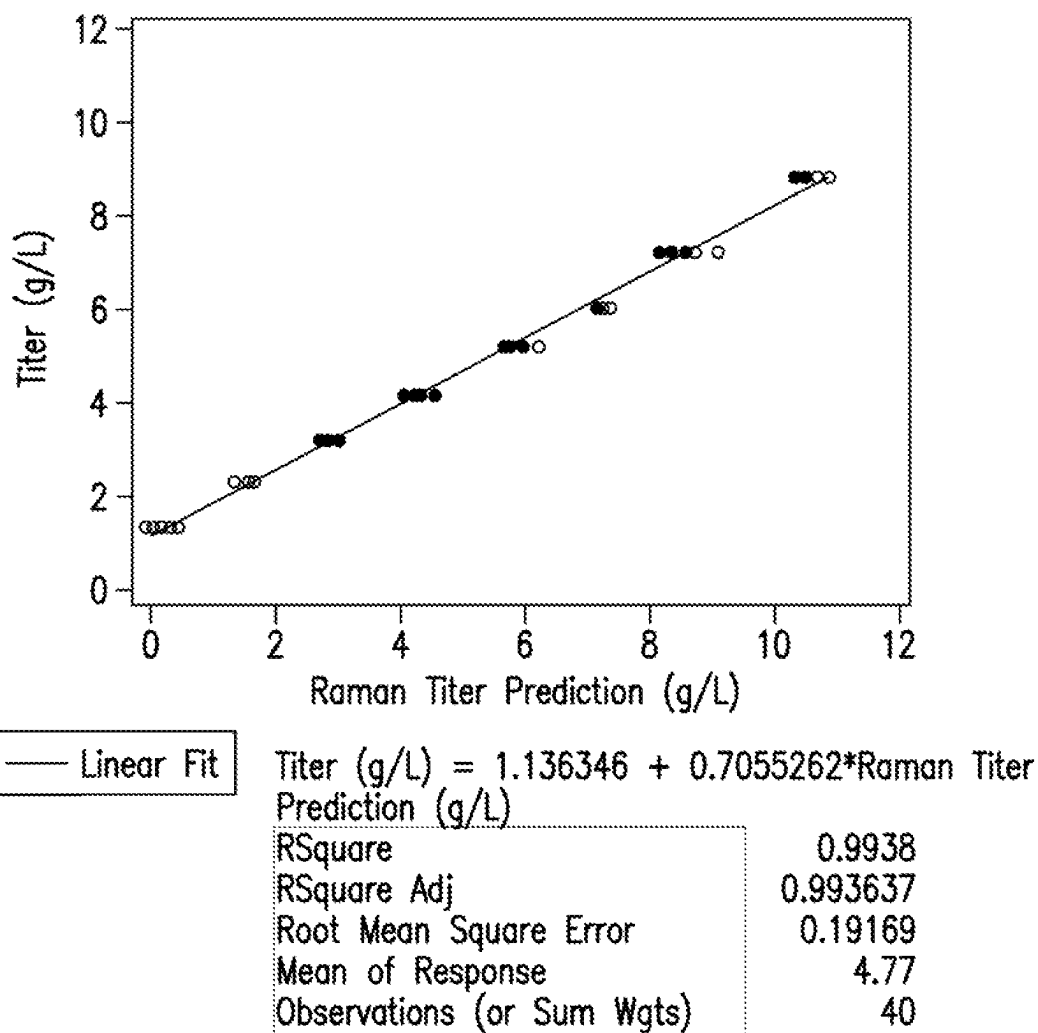


FIG. 13

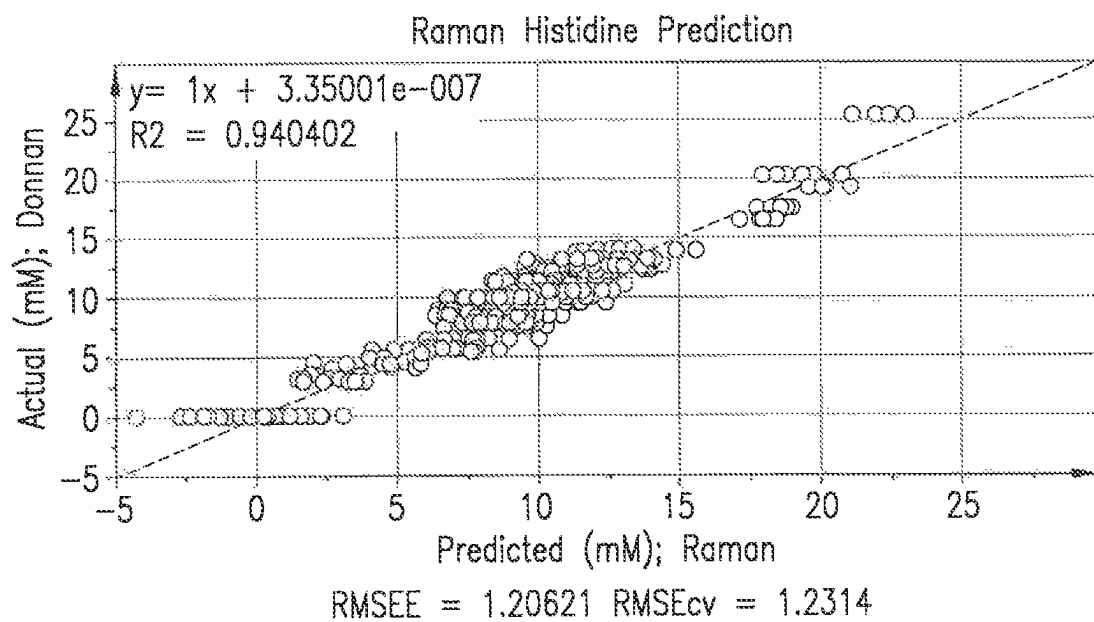
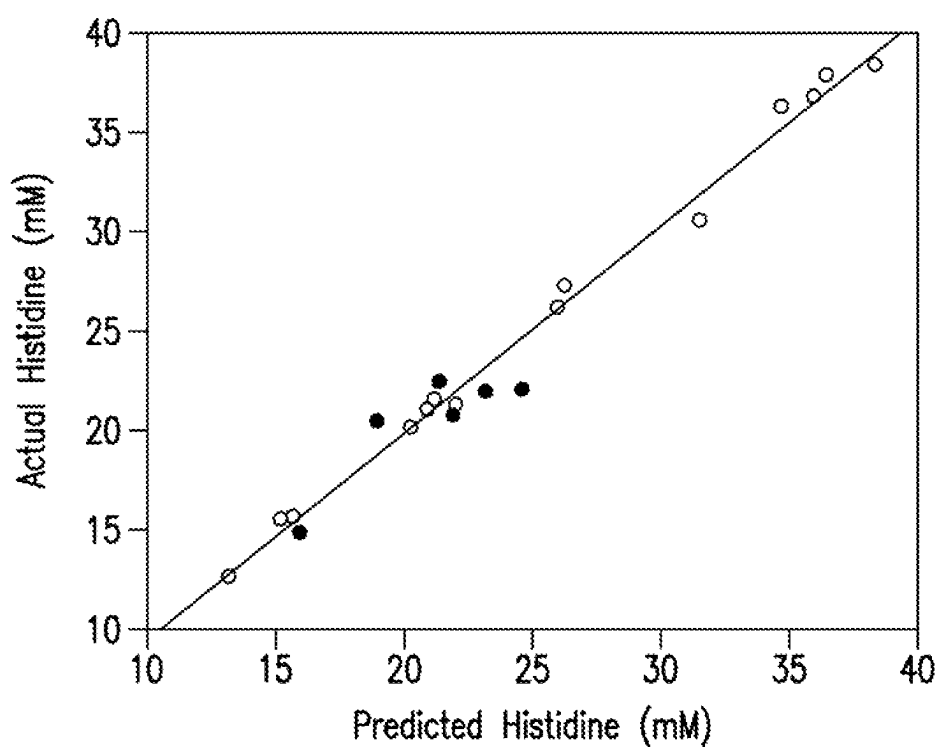


FIG.14A

**FIG.14B**

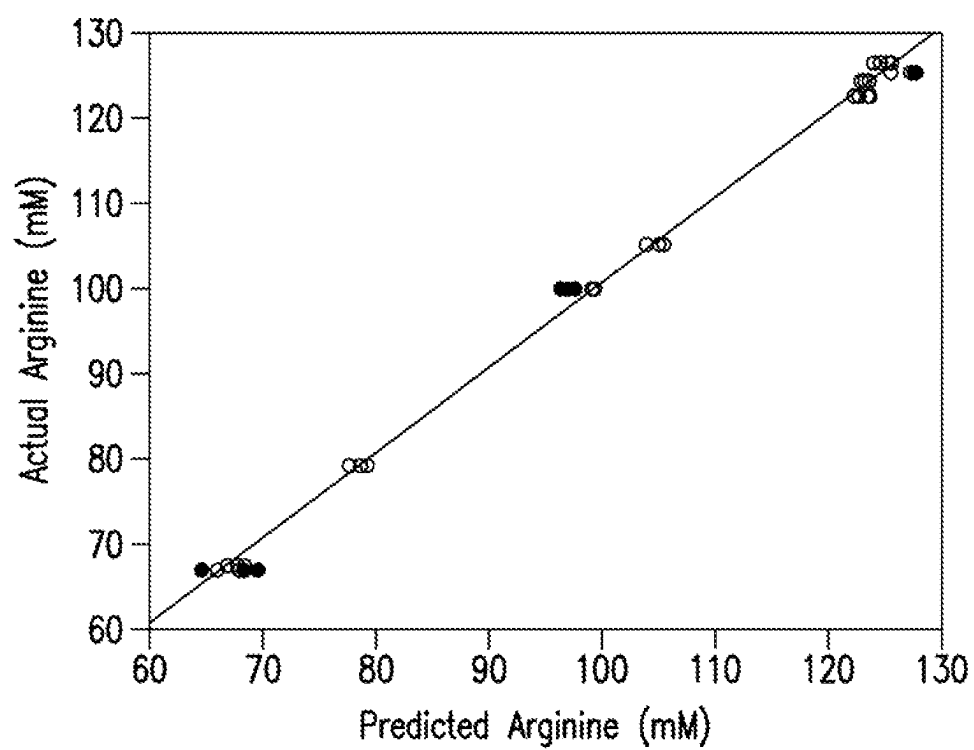


FIG.14C

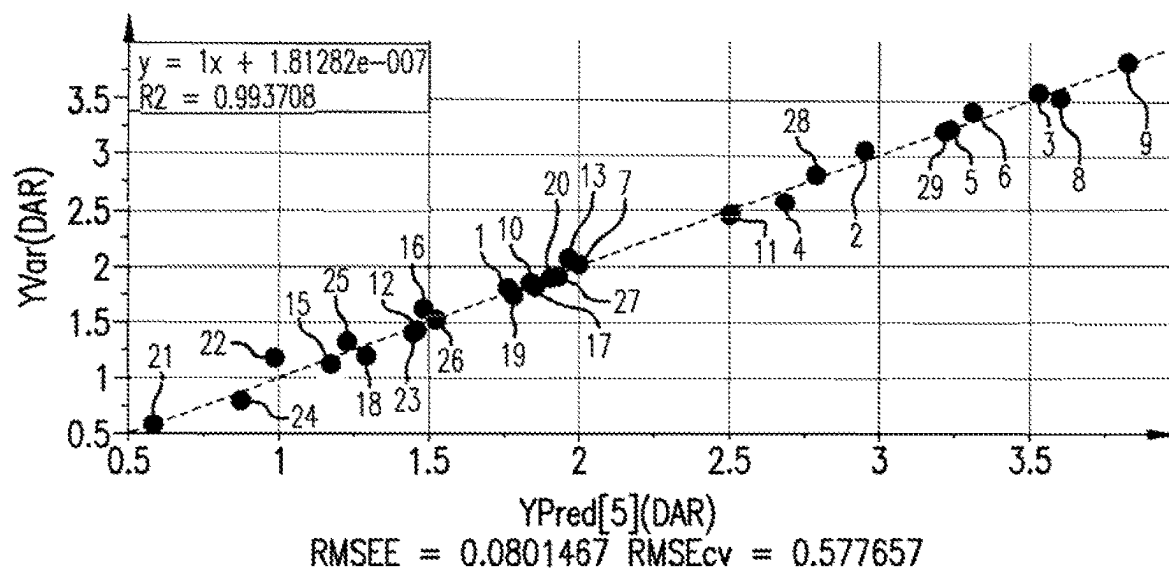


FIG. 15A

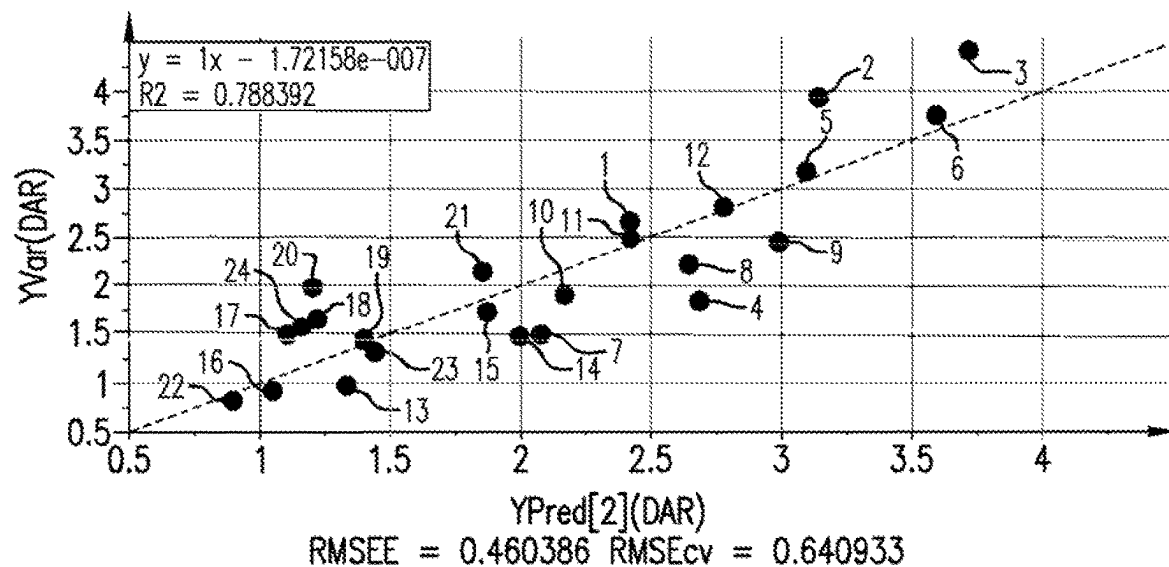


FIG. 15B

USE OF RAMAN SPECTROSCOPY IN DOWNSTREAM PURIFICATION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation application of U.S. patent application Ser. No. 16/550,989, filed on Aug. 26, 2019, which claims benefit of and priority to U.S. Provisional Patent Application No. 62/723,188 filed on Aug. 27, 2018, and where permissible are incorporated by reference in their entirety.

TECHNICAL FIELD OF THE INVENTION

The invention is generally directed to systems and methods for monitoring and controlling one or more critical quality attributes (CQAs) or parameters in downstream protein purification processes.

BACKGROUND OF THE INVENTION

The number of monoclonal antibodies (mAbs) that have been approved for therapeutic use has increased significantly over the past decade. This is due in part to improvements in large scale manufacturing processes which facilitate the production of large quantities of mAbs. In addition, initiatives such as The Process Analytical Technology (PAT) framework of the Food and Drug Administration (FDA) have led to innovative solutions to process development, process analysis, and process control to better understand processes and control the quality of products. Efficient recovery and purification of mAbs from cell culture media is a critical part of the production process. The purification process should reliably produce mAbs that are safe for use in humans. This includes monitoring critical quality attributes (CQAs) that include protein attributes and impurities such as host cell proteins, DNA, viruses, endotoxins, aggregates, concentrations, excipients, and other species that have the potential to impact patient safety, efficacy, or potency. Protein concentration is also often a CQA in purified material, and appropriate protein concentration in process intermediates can be a critical process parameter for unit operation performance. These CQAs need to be monitored throughout production as well as throughout the program lifecycle.

To ensure that the final formulations of mAbs do not contain impurities above determined levels, the mAb products are tested at various stages of the downstream processing. Quality control in the manufacturing of bioproducts such as mAbs is generally accomplished by analyzing purification intermediates and formulated drug substance samples with offline methods for each lot production. The samples are removed from the processing equipment, for example a UF/DF skid, and subjected to offline tests to measure product CQAs such as protein concentration (g/L), buffer excipients, and size variants. Real time monitoring and analysis during manufacturing is not available resulting in increases in processing time and a higher risk of batch failure due to not meeting CQAs. Accordingly, there is a need for rapid, in-line methods of real-time quality control monitoring of mAbs.

Therefore, it is an object of the invention to provide systems and methods for real-time monitoring of critical quality attributes during the downstream purification process.

SUMMARY OF THE INVENTION

In situ Raman spectroscopy methods and systems for characterizing or quantifying a protein purification intermediate during production or manufacture are provided. In one embodiment, in situ Raman spectroscopy is used to characterize or quantify critical quality attributes of a protein drug during downstream processing (i.e., after harvest of the protein purification intermediate from cell culture fluid). For example, the disclosed in situ Raman spectroscopy methods and systems can be used to characterize and quantify protein purification intermediate critical quality attributes as the protein purification intermediates are purified, prior to formulation into the final drug product to be sold or administered. Critical quality attributes include but are not limited to protein concentration, excipients, high molecular weight (HMW) species, antibody titer, and drug-antibody ratio.

One embodiment provides a method of producing a concentrated protein purification intermediate by determining concentrations of a protein purification intermediate in-real time using in situ Raman spectroscopy while concentrating/diafiltering the protein purification intermediate and adjusting parameters of the concentrating step in-real time to obtain the pre-determined concentration targets and excipient levels necessary for formulation of drug substance. The protein purification intermediate product can have a concentration of 5 mg/mL to 300 mg/mL, preferably 50 mg/mL to 300 mg/mL for subsequent formulation steps. In one embodiment, the protein purification intermediate is concentrated to a desired concentration target using ultrafiltration during primary or final concentration. Diafiltration is used during processing following primary concentration as a means for buffer exchange to achieve the desired final formulation components. The protein purification intermediate can be harvested from a bioreactor, a fed-batch culture, or a continuous culture. In another embodiment, determining the concentration of the protein purification intermediate can occur continuously or intermittently in real-time. Quantifying of protein concentration can be performed in intervals from approximately 5 seconds to 10 minutes, hourly, or daily. The protein purification intermediate can be an antibody or antigen binding fragment thereof, a fusion protein, or a recombinant protein. Spectral data can be collected at one or more wavenumber ranges selected from the group consisting of 977-1027 cm^{-1} , 1408-1485 cm^{-1} , 1621-1711 cm^{-1} , 2823-3046 cm^{-1} , and combinations thereof.

Another embodiment provides a method of producing a protein purification intermediate by independently performing Raman Spectroscopy analysis on a plurality of protein purification intermediates to produce a universal model capable of quantifying any one of the plurality of protein purification intermediates. The concentration of a protein purification intermediate can be determined using in situ Raman spectroscopy with the universal model during concentration of the protein purification intermediate from beginning to end of concentrating the protein purification intermediate. Another embodiment provides a method of producing a protein purification intermediate to produce a protein specific model capable of quantifying protein concentrations that would be used for commercial enabling productions of the protein.

The model can be produced using Partial Least Squares Regression Analysis of raw spectral data and using an orthogonal method for offline protein concentration data. Pre-processing techniques such as Standard Normal Variant (SNV) and/or point-smoothing technique can be 1st derivative with 21 cm^{-1} smoothing can be performed on the

Raman spectroscopy data to dampen model variability and prediction error. Further model refinement can be performed to isolate spectral regions that correlate to CQA predictions such as protein concentration. In one embodiment, the model has $\leq 5\%$ error margin, preferably $\leq 3\%$ error margin.

Still another embodiment provides a method for monitoring and controlling the levels of excipients in harvested cell culture fluid and/or protein purification intermediate during downstream purification by determining concentrations of the excipients in-real time using in situ Raman spectroscopy while purifying the cell culture fluid or protein purification intermediate, and adjusting parameters of the purification step in-real time to obtain or maintain predetermined amounts of the excipients in the harvested cell culture fluid and/or protein purification intermediate. The excipient can be acetate, citrate, histidine, succinate, phosphate, hydroxymethylaminomethane (Tris), proline, arginine, sucrose, or combinations thereof. The excipient can be a surface excipient such as polysorbate 80, polysorbate 20, and poloxamer 188.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a flow chart showing an exemplary protein purification process.

FIG. 2 is a representative spectrograph showing the initial model development for in-line Raman spectroscopy. The X axis represents the Raman shift. The Y axis represents intensity. The legend on the right represents protein concentration. Spectral regions used during the initial model development include, from left to right, $977\text{--}1027\text{ cm}^{-1}$ (Ring structure), $1408\text{--}1485\text{ cm}^{-1}$ (Arginine), $1621\text{--}1711\text{ cm}^{-1}$ (Secondary structure), and $2823\text{--}3046\text{ cm}^{-1}$ (C—H stretching).

FIG. 3 is a bar graph showing protein concentration (g/L) for mAb1 during a standard ultrafiltration/diafiltration unit operation. The empty bars are concentrations determined using the UV-Vis based offline method with a SoloVPE system (C-technologies) with error bars of $\pm 5\%$ which is the goal for the inline Raman predictions. The bars with wide hatching represent the model herein referred to as the universal model without mAb1 included in the Raman predictions and the bars with narrow hatching represent the universal model with mAb1. The cross-hatched bars correspond to the predictions from the initial universal model with a range of $0\text{--}120\text{ g/L}$. The hatched bars correspond to the predictions from the initial universal model $>120\text{ g/L}$.

FIG. 4 is a bar graph showing absolute Raman model error for various mAbs from the initial universal model development. The hatched bars represent the initial universal model $0\text{--}120\text{ g/L}$ (Primary concentration and Diafiltration) and the empty bars represent from the initial universal model $>120\text{ g/L}$ (Final Concentration). The horizontal line represents the $\leq 5\%$ error Raman model goal.

FIG. 5 is a bar graph showing absolute Raman model error for various mAbs. The bars with wide hatching represent $0\text{--}120\text{ g/L}$ (Primary concentration and diafiltration) and the bars with narrow hatching represent $>120\text{ g/L}$ (final concentration). The horizontal line represents the $\approx 5\%$ error Raman model goal. Two versions of the universal Raman model are shown. The hatched bars represent the initial universal model and the cross-hatched bars represent the updated universal model.

FIG. 6 is a schematic illustration of an ultrafiltration/diafiltration system, including locations for inline Raman probe placement.

FIG. 7 is a bar graph showing protein concentration for mAb10 using the universal model or the mAb10 specific model for final concentrated pool (FCP) measurements. Protein concentrations are shown for inline real-time Raman predictions (bars with wide hatching), updated models (bars with narrow hatching), and SoloVPE (empty bar). The X axis represents experimental group and the Y axis represents protein concentration.

FIGS. 8A-8B are bar graphs showing Raman model error for bench scale DoE modeling for protein concentration. FIG. 8A shows the Raman model error for real-time predictions in various stages of UF/DF processing (primary concentration, diafiltration, and final concentrated pool). FIG. 8B shows the Raman model error for the final DoE model at various stages of UF/DF processing (primary concentration, diafiltration, and final concentrated pool).

FIG. 9A is a bar graph showing model prediction capability percent error for model scale-up to pilot processing equipment for mAb11. Bench-scale model data is compared to bench-scale model data incorporating the pilot-scale data. The X-axis represents experimental groups and the Y-axis represents model prediction capability percent error (%). FIG. 9B is a bar graph showing model prediction capability for pilot-scale processing for various monoclonal antibodies. The X-axis represents experimental groups and the Y-axis represents model prediction capability percent error (%).

FIG. 10A is a schematic of an exemplary automated batch UF/DF with Raman feedback. FIG. 10B is a schematic of an exemplary automated single pass TFF with Raman feedback.

FIG. 11 is a graph showing mAb14 concentration over the course of UF/DF processing. The X-axis represents throughput (L/m^2) and the Y-axis represents mAb 14 concentration (g/L).

FIG. 12A is a bar graph showing the percent of high molecular weight (HMW) species in mAb2 during various steps of processing (primary concentration, diafiltration, final concentration) determined by either SE-UPLC or Raman modeling. The X-axis represents experimental group and the Y-axis represents mAb2 HMW percent (%). FIG. 12B is a bar graph showing the percent of high molecular weight (HMW) species predicted using various scan times (10 sec, 20 sec, 30 sec) for mAb 15. The X-axis represents experimental group and the Y-axis represents HMW percent (%).

FIG. 13 is a dot plot showing actual titer (g/L) versus Raman predicted titer for monoclonal antibody samples from mAb 14. The X-axis represents Raman predicted titer and the Y-axis represents actual titer (g/L).

FIG. 14A is a scatter plot showing Raman histidine prediction in various monoclonal antibodies. The X-axis represents histidine concentration predicted by Raman modeling and the Y-axis represents actual histidine concentration determined by amino acid analysis. FIG. 14B is a dot plot showing actual histidine concentration versus Raman predicted histidine concentration for monoclonal antibody sample. FIG. 14C is a dot plot showing actual arginine concentration versus Raman predicted arginine concentration for monoclonal antibody sample.

FIG. 15A is a scatter plot showing actual drug-antibody ratio (DAR) versus Raman predicted DAR for monoclonal antibody samples from mAb 3. The X-axis represents Raman predicted DAR and the Y-axis represents actual DAR determined by UV-spectroscopy. FIG. 15B is a scatter plot showing actual drug-antibody ratio (DAR) versus Raman predicted DAR for monoclonal antibody samples from mAb

1. The X-axis represents Raman predicted DAR and the Y-axis represents actual DAR.

DETAILED DESCRIPTION OF THE INVENTION

I. Definitions

It should be appreciated that this disclosure is not limited to the compositions and methods described herein as well as the experimental conditions described, as such may vary. It is also to be understood that the terminology used herein is for the purpose of describing certain embodiments only, and is not intended to be limiting, since the scope of the present disclosure will be limited only by the appended claims.

Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this disclosure belongs. Although any compositions, methods and materials similar or equivalent to those described herein can be used in the practice or testing of the present invention. All publications mentioned are incorporated herein by reference in their entirety.

The use of the terms “a,” “an,” “the,” and similar referents in the context of describing the presently claimed invention (especially in the context of the claims) are to be construed to cover both the singular and the plural, unless otherwise indicated herein or clearly contradicted by context.

Recitation of ranges of values herein are merely intended to serve as a shorthand method of referring individually to each separate value falling within the range, unless otherwise indicated herein, and each separate value is incorporated into the specification as if it were individually recited herein.

Use of the term “about” is intended to describe values either above or below the stated value in a range of approx. $\pm 10\%$; in other embodiments the values may range in value either above or below the stated value in a range of approx. $\pm 5\%$; in other embodiments the values may range in value either above or below the stated value in a range of approx. $\pm 2\%$; in other embodiments the values may range in value either above or below the stated value in a range of approx. $\pm 1\%$. The preceding ranges are intended to be made clear by context, and no further limitation is implied. All methods described herein can be performed in any suitable order unless otherwise indicated herein or otherwise clearly contradicted by context. The use of any and all examples, or exemplary language (e.g., “such as”) provided herein, is intended merely to better illuminate the invention and does not pose a limitation on the scope of the invention unless otherwise claimed. No language in the specification should be construed as indicating any non-claimed element as essential to the practice of the invention.

As used herein, “protein” refers to a molecule comprising two or more amino acid residues joined to each other by a peptide bond. Protein includes polypeptides and peptides and may also include modifications such as glycosylation, lipid attachment, sulfation, gamma-carboxylation of glutamic acid residues, alkylation, hydroxylation and ADP-ribosylation.

Proteins can be of scientific or commercial interest, including protein-based drugs, and proteins include, among other things, enzymes, ligands, receptors, antibodies and chimeric or fusion proteins. Proteins are produced by various types of recombinant cells using well-known cell culture methods, and are generally introduced into the cell by transfection of genetically engineering nucleotide vectors

(e.g., such as a sequence encoding a chimeric protein, or a codon-optimized sequence, an intronless sequence, etc.), where the vectors may reside as an episome or be integrated into the genome of the cell.

“Antibody” refers to an immunoglobulin molecule consisting of four polypeptide chains, two heavy (H) chains and two light (L) chains inter-connected by disulfide bonds. Each heavy chain has a heavy chain variable region (HCVR or VH) and a heavy chain constant region. The heavy chain constant region contains three domains, CH1, CH2 and CH3. Each light chain has a light chain variable region and a light chain constant region. The light chain constant region consists of one domain (CL). The VH and VL regions can be further subdivided into regions of hypervariability, termed complementarity determining regions (CDR), interspersed with regions that are more conserved, termed framework regions (FR). Each VH and VL is composed of three CDRs and four FRs, arranged from amino-terminus to carboxy-terminus in the following order: FR1, CDR1, FR2, CDR2, FR3, CDR3, FR4. The term “antibody” includes reference to both glycosylated and non-glycosylated immunoglobulins of any isotype or subclass. The term “antibody” includes antibody molecules prepared, expressed, created or isolated by recombinant means, such as antibodies isolated from a host cell transfected to express the antibody. The term antibody also includes bispecific antibody, which includes a heterotetrameric immunoglobulin that can bind to more than one different epitope. Bispecific antibodies are generally described in US Patent Application Publication No. 2010/0331527, which is incorporated by reference into this application.

“Secondary structure” refers to local folded structures that form within a polypeptide due to interactions between atoms of the backbone. The most common types of secondary structures are a helix and the β pleated sheet. Both structures are held in shape by hydrogen bonds, which form between the carbonyl O of one amino acid and the amino H of another.

As used herein, “excipient” refers to a pharmacologically inactive substance that is used as a stabilizing agent for long-term storage of the formulated drug substance. Generally, additional excipients are added to the final concentrated pool to produce formulated drug substance. However, during UF/DF processing excipient levels are monitored to ensure the levels will not impact the desired formulation strategy. Excipients provide bulk to the pharmaceutical formulation, facilitate drug absorption or solubility, and provide stability and prevent denaturation. Common pharmaceutical excipients include but are not limited to amino acids, fillers, binders, disintegrants, coatings, sorbents, buffering agents, chelating agents, lubricants, glidants, preservatives, antioxidants, flavoring agents, sweeteners, coloring agents, solvent and co-solvents, and viscosity imparting agents. In one embodiment, the excipient is polyethylene glycol including but not limited to PEG-3550.

“Polyethylene glycol” or “PEG” is a polyether polymer of ethylene oxide commonly used in food, medicine and cosmetics. It is a non-ionic macromolecule that is useful as a molecule that reduces the solubility of a biomolecule. PEG is commercially available in different molecular weights ranging from 300 g/mol to 10,000,000 g/mol. Exemplary types of PEG include but are not limited to PEG 20000, PEG 8000 and PEG 3350. PEG is available in different geometries, including linear, branched (3-10 chains attached to central core), star-shaped (10-100 chains attached to a central core), and combshaped (multiple chains attached to a polymer backbone).

“Raman spectroscopy” is a spectroscopic technique used to measure the wavelength and intensity of in-elastically scattered light from molecules. It is based on the principle that monochromatic incident radiation on materials will be reflected, absorbed, or scattered in a specific manner, which is dependent upon the particular molecule or protein which receives the radiation. The majority of the energy is scattered at the same wavelength, called elastic or Rayleigh scattering. A small amount (<0.001%) is scattered at different wavelengths, called inelastic or Raman scattering. Raman scatter is associated with rotational, vibrational, and electronic level transitions. Raman spectroscopy can reveal the chemical and structural composition of samples.

As used herein, “ultrafiltration” refers to a membrane process that is widely used for protein concentration in the downstream processing of protein therapeutics during the purification of recombinant proteins. Ultrafiltration is a size-based separation, where species larger than the membrane pores are retained and smaller species pass through freely. During processing, the protein solution is pumped tangentially across the surface of a semi-permeable parallel flat sheet membrane. The membrane is permeable to buffer and buffer salts but generally impermeable to monoclonal antibodies. The driving force for permeation is applied transmembrane pressure (TMP) induced by flow restriction at the outlet of the membrane flow channel ($TMP = P_{feed} + P_{retentate} / 2 - P_{permeate}$).

As used herein, “primary concentration” refers to the initial step where transmembrane pressure drives water and salts across the permeable membrane, which reduces the liquid volume and thus increases protein concentration. The extent of concentration in primary concentration may be optimized to balance throughput, protein stability, processing time and buffer consumption.

As used herein, “diafiltration” refers to a technique that uses a semi-permeable membrane to exchange a product of interest from one liquid medium into another. Buffer exchange and de-salting are typically performed using a diafiltration mode in which the small impurities and buffer components are effectively washed away from the product by the continuous addition of a buffer that is intended to condition the protein to a stable pH and excipient concentration that allows high product concentration. This can be performed in a continuous or discontinuous mode based on processing techniques.

Diafiltration is often combined with ultrafiltration to achieve the desired volume reduction while also removing impurities and salts. UF/DF is the final unit operation in downstream purification which conditions the mAb to achieve pH, excipient content, and protein concentration conducive to long term storage and addition of stabilizing excipients to generate Formulated Drug Substance (FDS).

As used herein, “final concentration” refers to the final step where transmembrane pressure drives water and salts across the permeable membrane, which reduces the liquid volume and thus increases protein concentration to the desired target for storage and/or formulation. The resultant pool from the final concentration step is final concentrated pool (FCP). This final concentration step can be performed in a continuous or discontinuous processing mode.

The terms “bioproduct” and “protein purification intermediate” can be used interchangeably and refer to any antibody, antibody fragment, modified antibody, protein, glycoprotein, or fusion protein as well as final drug substances purified from a bioreactor process.

The terms “control” and “controlling” refer to adjusting an amount or concentration level of a critical quality attribute in a harvested cell culture fluid to a predefined set point.

As used herein, the term “upstream processing” refers to the first step in which antibodies or therapeutic proteins are produced, usually by bacterial or mammalian cell lines, in bioreactors. Upstream processing includes media preparation, cell culture, and cell separation and harvest. When the cells have reached the desired density, they are harvested and moved to the downstream section of the bioprocess. The term “downstream processing” refers to the isolation and purification that occurs after the harvest of an antibody or therapeutic protein from a bioreactor. Typically, this means recovery of a product from an aqueous solution via several different modalities. The harvested product is processed to meet purity and critical quality attribute requirements during downstream processing.

As used herein, the term “protein purification intermediate” refers to a protein that has been harvested from a bioreactor and refers to any intermediate during downstream processing.

The term “concentrated protein purification intermediate” refers to a protein purification intermediate with a concentration greater than 5 mg/mL. More preferably the concentration is between 50 mg/mL to 300 mg/mL.

The terms “monitor” and “monitoring” refer to regularly checking an amount or concentration level of a critical quality attribute in a cell culture or a harvested cell culture fluid.

The term “harvested cell culture fluid” refers to fluid that is removed from a bioreactor containing cells that were engineered to secrete proteins of interest. The “harvested cell culture fluid” optimally contains the secreted protein of interest, for example a monoclonal antibody.

As used herein “critical quality attribute (CQA)” refers to a physical, chemical, biological, or microbiological property or characteristic that should be within an appropriate limit, range, or distribution to ensure the desired product quality of a biologic therapeutic drug product. These attributes have the potential to impact safety, efficacy, and/or potency. Critical quality attributes include but are not limited to protein concentration, high molecular weight species, buffer excipients, and pH.

As used herein, “formulated drug substance” refers to an active ingredient that is intended to furnish pharmacological activity, but does not include intermediates used in the synthesis of such ingredient.

As used herein, “universal model” refers to a mathematical correlation of spectral properties of different recombinant proteins used to predict a critical quality attribute.

As used herein, “mAb specific model” refers to a mathematical correlation of spectral properties of one particular protein used to predict a critical quality attribute.

As used herein “titer” refers to the amount of an antibody or protein molecules in a solution.

II. Systems and Methods for Characterization of Downstream Protein Purification Products

Systems and methods for monitoring and controlling protein concentration during protein manufacturing are provided. Concentrated protein solutions are difficult to measure accurately due to high correlated solution viscosities (>10 cP). Accurate quantification requires specialty offline equipment and typically solution dilution. In high concentration UF/DF, final excipient levels are a function of protein concentration due to the Gibbs-Donnan effect. Real time

monitoring and analysis during manufacturing is not available which increases processing time and potential batch failure due to not meeting CQAs. The systems and methods disclosed herein can be used for in-line monitoring of protein concentration and other critical quality attributes.

In one embodiment, the Raman spectroscopy system is an in-line or in situ Raman spectroscopy system used during production of a final concentrated pool, which could be highly concentrated (≥ 150 g/L). Typically, the Raman spectroscopy system is employed downstream of production of the protein purification intermediate, for example during processing of the protein purification intermediate after harvest from a bioreactor or fed-batch culture system and subsequent purification. FIG. 1 shows an exemplary protein purification process. Typically, the protein purification intermediate is harvested from cell culture (100) and processed through various purification steps such as affinity capture (110), viral inactivation (120), polishing chromatography (130 and 140), virus retentive filtration (150), and ultrafiltration/diafiltration (160), to produce the final concentrated pool which is then formulated to drug substance. In one embodiment, the monitoring of protein concentration in a harvested cell culture fluid is performed by in situ Raman spectroscopy.

A. Raman Spectroscopy

In one embodiment, monitoring and controlling protein concentration in a harvested cell culture fluid is performed by Raman spectroscopy. Raman spectroscopy is a form of vibrational spectroscopy that provides information about molecular vibrations that can be used for sample identification and critical quality attribute quantitation. In situ Raman analysis is a method of analyzing a sample in its original location without having to extract a portion of the sample for analysis in a Raman spectrometer. In situ Raman analysis is advantageous in that the Raman spectroscopy analyzers are noninvasive and nondestructive which reduces the risk of contamination and loss of protein quality. In-line Raman analysis can be implemented to enable continuous processing while monitoring protein concentration of harvested cell culture fluid, protein purification intermediates, and/or final concentrated pool.

The in situ Raman analysis can provide real-time assessments of protein concentration in protein purification intermediates. For example, the raw spectral data provided by in situ Raman spectroscopy can be used to obtain and monitor the current protein concentration in protein purification intermediates. In this aspect, to ensure that the raw spectral data is continuously up to date, the spectral data from the Raman spectroscopy should be acquired about every 5 seconds to 10 hours. In another embodiment, the spectral data should be acquired about every 15 minutes to 1 hour. In still another embodiment, the spectral data should be acquired about every 20 minutes to 30 minutes.

The monitoring of the protein concentration in the protein purification intermediate can be analyzed by any commercially available Raman spectroscopy analyzer that allows for in situ Raman analysis. The in situ Raman analyzer should be capable of obtaining raw spectral data within the protein purification intermediate. For example, the Raman analyzer should be equipped with a probe that may be inserted inline of the fluid circuit. Suitable Raman analyzers include, but are not limited to, RamanRXN2 and RamanRXN4 analyzers (Kaiser Optical Systems, Inc. Ann Arbor, MI).

The raw spectral data obtained by in situ Raman spectroscopy may be compared to offline protein concentration measurements in order to correlate the peaks within the spectral data to the protein concentration. Offline protein

concentration measurements may be used to determine which spectral regions exhibit the protein signal. The offline measurement data may be collected through any appropriate analytical method. In the case of protein concentration, for example, the offline measurement can be collected using SoloVPE (C-technologies). Additionally, any type of multivariate software package, for example, SIMCA 13 (MKS Data Analytic Solutions, Umea, Sweden), may be used to correlate the peaks within the raw spectral data to offline measurements of protein concentration. However, in some embodiments, it may be necessary to pretreat the raw spectral data with spectral filters to remove any varying baselines. For example, the raw spectral data may be pretreated with any type of point smoothing technique or normalization technique. Normalization may be needed to correct for any probe, optic, laser power variation and exposure time by the Raman analyzer. In one embodiment, the raw spectral data may be treated with point smoothing, such as 1st derivative with 21 cm^{-1} point smoothing, and normalization, such as Standard Normal Variate (SNV) normalization. These pre-processing techniques may be combined for certain spectral regions to improve the model predictions.

Chemometric modeling may also be performed on the obtained spectral data. In this aspect, one or more multivariate methods including, but not limited to, Partial Least Squares (PLS), Principal Component Analysis (PCA), Orthogonal Partial least squares (OPLS), Multivariate Regression, Canonical Correlation, Factor Analysis, Cluster Analysis, Graphical Procedures, and the like, can be used on the spectral data. In one embodiment, the obtained spectral data is used to create a PLS regression model. A PLS regression model may be created by projecting predicted variables and observed variables to a new space. In this aspect, a PLS regression model may be created using the measurement values obtained from the Raman analysis and the offline measurement values. The PLS regression model provides predicted process values, for example, predicted protein concentration value. In one embodiment, the model provides predicted protein concentration values with $\leq 5\%$ error compared to off-line protein concentration values. In a preferred embodiment, the model provides predicted protein concentration values with $\leq 3\%$ error compared to off-line protein concentration values.

After chemometric modeling, a signal processing technique may be applied to the predicted protein concentration values. In one embodiment, the signal processing technique will dampen model variability and prediction error. In this aspect, one or more of the pre-processing techniques may be applied to the predicted protein concentration values. Any pre-processing techniques known to those skilled in the art may be utilized. For example, the noise reduction technique may include data smoothing and/or signal rejection. Smoothing is achieved through a series of smoothing algorithms and filters while signal rejection uses signal characteristics to identify data that should not be included in the analyzed spectral data. In one embodiment, the predicted protein concentration values are noise mitigated by a noise reduction filter. The noise reduction filter provides final predicted protein concentration values. In this aspect, the noise reduction technique combines raw measurements with a model-based estimate for what the measurement should yield according to the model. In one embodiment, the noise reduction technique combines a current predicted protein concentration value with its uncertainties. Uncertainties can be determined by the repeatability of the predicted protein concentration values and the current protein concentration

values. Once the next predicted protein concentration value is observed, the estimate of the predicted protein concentration value is updated using a weighted average where more weight is given to the estimates with higher certainty. Using an iterative approach, the final protein concentration values may be updated based on the previous measurement and the current measurement. In this aspect, the algorithm should be recursive and able to run in real time so as to utilize the current predicted protein concentration value, the previous value, and experimentally determined constants. The noise reduction technique improves the robustness of the measurements received from the Raman analysis and the PLS predictions by reducing noise upon which the automated feedback controller will act.

B. Methods of Use

The disclosed methods can be used to monitor and control protein concentration in harvested cell culture and/or protein purification intermediates fluids during downstream protein purification processes. Common downstream purification processes include but are not limited to centrifugation, direct depth filtration, protein A affinity purification, viral inactivation steps, ion-exchange chromatography, hydrophobic interaction chromatography, size-exclusion chromatography, ultrafiltration/diafiltration, viral retentive filtration, and combinations thereof. These unit operations are used in a defined sequential combination to isolate the protein of interest and ensure impurities and/or critical quality attributes are monitored prior to the production of formulated drug substance. In one embodiment, the disclosed methods include a Raman probe in-line of the fluid circuit. In another embodiment, the disclosed methods can be used to produce a concentrated protein purification intermediate or final concentrated pool.

1. Antibody Titer and Protein Concentration

Both antibody titer and protein concentration are important factors in the purification of bioproducts. Antibody titer measured after the initial harvest of the cell culture fluid is important to determine column loadings and ensure a robust purification process for removal of impurities. Monitoring protein concentration throughout purification steps is important to ensure both the proper concentration of end product, and proper performance of the purification unit operations performed. Improper protein concentration can lead to ineffective drug products or production of formulated drug substance.

In one embodiment, harvested cell culture fluid is subjected to Raman spectral analysis immediately after being harvested, but before any additional purification has begun. Raman spectral data can be used after harvest to quantify antibody titer in the harvested cell culture fluid. Protein concentration can be measured using the disclosed methods at multiple steps during the protein purification process, for example, during affinity capture, during polishing chromatography, during virus retentive filtration, or during ultrafiltration/diafiltration. Inline Raman probes can detect Raman scattering in the harvested cell culture fluid and/or protein purification intermediate within the fluid circuit without removing sample from the system providing analytical characterizations that are normally determined in an offline fashion.

In one embodiment, if the protein concentration is not within the pre-determined concentration during ultrafiltration/diafiltration, the system is notified and the protein purification intermediate is altered accordingly. For example, if the protein concentration in the protein purification intermediate is below the predetermined protein con-

centration the protein purification intermediate can be further concentrated by performing ultrafiltration/diafiltration.

In one embodiment, the concentration step is performed by Protein A affinity chromatography.

2. Drug-to-Antibody Ratio

In another embodiment, the disclosed methods can be used to monitor and control drug-to-antibody ratio (DAR). DAR is a quality attribute that is monitored during development of antibody-drug conjugates (ADC), antibody-radionuclide conjugates (ARC), and general protein conjugates (potent steroids, non-cytotoxic payloads, etc.) to ensure consistent product quality and to facilitate subsequent labeling with payloads. DAR is the average number of drugs or other therapeutic molecules conjugated to antibodies, and is an important quality attribute in the production of therapeutic conjugates. The DAR value affects the efficacy of the conjugated drug as low drug loading reduces the drug potency while high loading can negatively affect the pharmacokinetics and safety.

In one embodiment, antibody-radionuclide conjugates are subjected to Raman spectral analysis immediately after being conjugated, but before any additional purification occurs. Raman spectral data can be used after conjugation to determine the DAR.

In one embodiment, if the DAR is not within the predetermined concentration during processing, the system is notified and the ADC intermediate is altered accordingly. For example, if the DAR in the ADC intermediate is below the predetermined DAR the conjugation reaction components can be altered, for example reactant concentrations can be optimized, the type of linker can be altered, temperature, or other manufacturing variables can be optimized.

3. Buffer Excipients

The disclosed methods can be used to monitor and control the levels of buffer excipients in harvested cell culture fluid and/or protein purification intermediate during downstream purification. Buffer excipients that are commonly used in monoclonal antibody productions include but are not limited to acetate, citrate, histidine, succinate, phosphate, and hydroxymethylaminomethane (Tris), proline, and arginine. Surfactant excipients include but are not limited to polysorbate 80 (Tween 80), polysorbate 20 (Tween 20), and poloxamer 188. Polyol/disaccharide/polysaccharide excipients include but are not limited to mannitol, sorbitol, sucrose, and dextran 40. Antioxidant excipients include but are not limited to ascorbic acid, methionine, and ethylenediaminetetraacetic acid (EDTA). Two commonly used amino acid excipients are histidine and arginine. In a preferred embodiment, the excipient that is monitored and controlled is histidine and arginine.

Final concentrated pool excipient concentrations differ from the composition of the diafiltration buffer due to the combination of the excluded volume and Donnan effects. The Donnan effect is a phenomenon that arises due to retention of the net positively charged protein by the membrane during UF/DF combined with the requirement for charge neutrality in both the retentate and permeates. To balance the positively charged protein, negatively charged buffer components are enriched in the retentate relative to the diafiltration buffer, while positively charged buffer components are expelled. This effect can lead to FCP pH and buffer excipient concentrations differing substantially from the diafiltration buffer composition (Stoner, et al., *J Pharm Sci*, 93:2332-2342 (2004)).

Volume exclusion describes the behavior of highly concentrated samples in which protein occupies a significant fraction of the solution volume. Buffer is excluded from the

volume occupied by the protein, causing the buffer solute concentrations to decrease as protein concentration increases expressed as moles (or mass) of solute per solution volume. Buffer is excluded from the volume occupied by the protein, causing the buffer solute concentrations to decrease as protein concentration increases when expressed as moles (or mass) of solute per solution volume.

Based on both of these principles and buffer excipient levels being critical quality attributes, inline Raman probes will minimize offline analytical characterization and provide further process understanding to ensure excipient levels are sufficient prior to formulation.

4. High Molecular Weight Impurities

In production of monoclonal antibodies, low levels of products-related impurities often exist even after extensive purification steps. High molecular weight (HMW) species (e.g., antibody dimer species) are a product-related impurity that contributes to size heterogeneity of mAb products. The formation of HMW species within a therapeutic mAb drug product as a result of protein aggregation can potentially compromise both drug efficacy and safety. HMW species are considered a CQA that are routinely monitored during drug development and as part of release testing of purified protein drug products during manufacturing.

In one embodiment, the disclosed methods can be used to identify protein drug products that contain HMW species. HMW species can be detected by Raman spectroscopy at various steps during the purification process including but not limited to during affinity capture, during viral inactivation, during polishing chromatography, during virus retentive filtration, during ultrafiltration/diafiltration, or combinations thereof.

In one embodiment, the disclosed methods detect HMW species in the harvested cell culture fluid and the fluid is further processed to remove the HMW species. Methods of removing HMW species for cell culture fluid include additional polishing steps including but not limited to cation exchange chromatography and anion exchange chromatography.

C. UF/DF Systems

FIG. 6 illustrates an ultrafiltration/diafiltration processing system, including various locations for in-line Raman probes (circled numbers 1-4). Protein purification intermediate is pumped into a retentate vessel **205** by a diafiltration pump **200** which may be a peristaltic, rotary lobe, pressure transfer, or diaphragm pump. Fluid from retentate vessel **205** flows to feed pump **210** which may be either a rotary lobe, peristaltic or diaphragm pump, past feed pressure valve **215** and into tangential flow filtration module (TFFM) **220**. In TFFM **220** the protein purification intermediate is subjected to ultrafiltration across a membrane. The bioproduct of interest is retained in the fluid (retentate) while water and low molecular weight solutes including buffer excipients pass through the membrane in the permeate (filtrate) which exits the system by passing through permeate pressure valve **225** into waste tank **230**. The retentate exits TFFM **220** and passes through retentate pressure valve **235**, transmembrane pressure control valve **240**, and retentate return channel **245** wherein it flows back into retentate vessel **205**. The process can be repeated as necessary to concentrate the bioproduct, remove impurities, and ensure CQAs are within acceptable limits. During diafiltration the same flow path described above is followed where permeable solutes are replaced as new buffer is washed into the product stream. When new buffer is added at the same rate as permeate is removed from the system, the sum of the retentate tank and skid hold-up volume defines the system volume. One turn-over volume

(TOV) is defined as an amount of diafiltration buffer added to the UF/DF process equal to the system volume. Typically, replacement of 8-times system volume (8 TOV) assures >99.9% buffer exchange (Schwartz, L., *Scientific and Technical Report*, PN 33289).

Additionally, during the UF/DF process, it is necessary to mix the protein solution in the retentate vessel **205**. Differences in density between the diafiltration buffer, the retentate return, and bulk retentate during diafiltration require that agitation in the tank should be sufficient to ensure adequate buffer exchange, yet sufficiently moderate to avoid shear, as this has been observed to result in protein aggregation and subvisible particle (SVP) generation in certain products. Additionally, it is important to ensure adequate mixing of retentate return during concentration stages to prevent protein concentration polarization in the retentate tank resulting in higher protein concentrations being delivered to the UF/DF membranes.

In one embodiment the Raman probe is placed at location **1**, downstream of diafiltration pump **200** in retentate vessel **205**. The Raman probe could alternatively be placed at location **2** downstream of retentate vessel **205** inline before feed pump **210**. In another embodiment, the Raman probe is placed inline at location **3** between feed pressure pump **215** and tangential flow filtration module **220**. In yet another embodiment, the Raman probe is placed inline in retentate return **245**. The location of the Raman probe is critical to ensure accurate inline measurements in a complicated system that has engineering and processing constraints.

D. Cell Culture

The harvested cell culture fluid can be harvested from a bioreactor containing cells engineered to produce monoclonal antibodies. The term "cell" includes any cell that is suitable for expressing a recombinant nucleic acid sequence. Cells include those of prokaryotes and eukaryotes, such as bacterial cells, mammalian cells, human cells, non-human animal cells, avian cells, insect cells, yeast cells, or cell fusions such as, for example, hybridomas or quadromas. In certain embodiments, the cell is a human, monkey, ape, hamster, rat or mouse cell. In other embodiments, the cell is selected from the following cells: Chinese Hamster Ovary (CHO) (e.g. CHO K1, DXB-11 CHO, Veggie-CHO), COS (e.g. COS-7), retinal cell, Vero, CV1, kidney (e.g. HEK293, 293 EBNA, MSR 293, MDCK, HaK, BHK21), HeLa, HepG2, WI38, MRC 5, Colo25, HB 8065, HL-60, lymphocyte, e.g. Jurkat (T lymphocyte) or Daudi (B lymphocyte), A431 (epidermal), U937, 3T3, L cell, C127 cell, SP2/0, NS-0, MMT cell, stem cell, tumor cell, and a cell line derived from an aforementioned cell. In some embodiments, the cell comprises one or more viral genes, e.g. a retinal cell that expresses a viral gene (e.g. a PER.C6® cell). In some embodiments, the cell is a CHO cell. In other embodiments, the cell is a CHO K1 cell.

In protein production, a "fed-batch cell culture" or "fed-batch culture" refers to a batch culture wherein the cells and culture medium are supplied to the culturing vessel initially, and additional culture nutrients are slowly fed, in discrete increments, to the culture during culturing, with or without periodic cell and/or product harvest before termination of culture. Fed-batch culture includes "semi-continuous fed-batch culture" wherein periodically whole culture (which may include cells and medium) is removed and replaced by fresh medium. Fed-batch culture is distinguished from simple "batch culture" whereas all components for cell culturing (including the animal cells and all culture nutrients) are supplied to the culturing vessel at the start of the culturing process in batch culture. Fed-batch culture may be

different from “perfusion culture” insofar as the supernatant is not removed from the culturing vessel during a standard fed-batch process, whereas in perfusion culturing, the cells are restrained in the culture by, e.g., filtration, and the culture medium is continuously or intermittently introduced and removed from the culturing vessel. However, removal of samples for testing purposes during fed-batch cell culture is contemplated. The fed-batch process continues until it is determined that maximum working volume and/or protein production is reached, and protein is subsequently harvested.

The phrase “continuous cell culture” relates to a technique used to grow cells continually, usually in a particular growth phase. For example, if a constant supply of cells is required, or the production of a particular protein of interest is required, the cell culture may require maintenance in a particular phase of growth. Thus, the conditions must be continually monitored and adjusted accordingly in order to maintain the cells in that particular phase.

The terms “cell culture medium” and “culture medium” refer to a nutrient solution used for growing mammalian cells that typically provides the necessary nutrients to enhance growth of the cells, such as a carbohydrate energy source, essential (e.g. phenylalanine, valine, threonine, tryptophan, methionine, leucine, isoleucine, lysine, and histidine) and nonessential (e.g. alanine, asparagine, aspartic acid, cysteine, glutamic acid, glutamine, glycine, proline, serine, and tyrosine) amino acids, trace elements, energy sources, lipids, vitamins, etc. Cell culture medium may contain extracts, e.g. serum or peptones (hydrolysates), which supply raw materials that support cell growth. Media may contain yeast-derived or soy extracts, instead of animal-derived extracts. Chemically defined medium refers to a cell culture medium in which all of the chemical components are known (i.e. have a known chemical structure). Chemically defined medium is entirely free of animal-derived components, such as serum- or animal-derived peptones. In one embodiment, the medium is a chemically defined medium.

The solution may also contain components that enhance growth and/or survival above the minimal rate, including hormones and growth factors. The solution may be formulated to a pH and salt concentration optimal for survival and proliferation of the particular cell being cultured.

E. Proteins of Interest

Any protein of interest suitable for expression in prokaryotic or eukaryotic cells can be monitored using the disclosed methods. For example, the protein of interest includes, but is not limited to, an antibody or antigen-binding fragment thereof, a chimeric antibody or antigen-binding fragment thereof, an ScFv or fragment thereof, an Fc-fusion protein or fragment thereof, a growth factor or a fragment thereof, a cytokine or a fragment thereof, or an extracellular domain of a cell surface receptor or a fragment thereof. Proteins of interest may be simple polypeptides consisting of a single subunit, or complex multisubunit proteins comprising two or more subunits. The protein of interest may be a biopharmaceutical product, food additive or preservative, or any protein product subject to purification and quality standards.

In some embodiments, the antibody is selected from the group consisting of an anti-Programmed Cell Death 1 antibody (e.g., an anti-PD1 antibody as described in U.S. Pat. No. 9,987,500), an anti-Programmed Cell Death Ligand-1 (e.g., an anti-PD-L1 antibody as described in U.S. Pat. No. 9,938,345), an anti-D114 antibody, an anti-Angiopoietin-2 antibody (e.g., an anti-ANG2 antibody as described in U.S. Pat. No. 9,402,898), an anti-Angiopoietin-Like 3 antibody (e.g., an anti-AngPt13 antibody as described in U.S. Pat. No. 9,018,356), an anti-platelet derived growth factor

receptor antibody (e.g., an anti-PDGFR antibody as described in U.S. Pat. No. 9,265,827), an anti-Erb3 antibody, an anti-Prolactin Receptor antibody (e.g., anti-PRLR antibody as described in U.S. Pat. No. 9,302,015), an anti-Complement 5 antibody (e.g., an anti-C5 antibody as described in U.S. Pat. No. 9,795,121), an anti-TNF antibody, an anti-epidermal growth factor receptor antibody (e.g., an anti-EGFR antibody as described in U.S. Pat. No. 9,132,192 or an anti-EGFRvIII antibody as described in U.S. Pat. No. 9,475,875), an anti-Proprotein Convertase Subtilisin Kexin-9 antibody (e.g., an anti-PCSK9 antibody as described in U.S. Pat. No. 8,062,640 or U.S. Pat. No. 9,540,449), an anti-Growth And Differentiation Factor-8 antibody (e.g. an anti-GDF8 antibody, also known as anti-myostatin antibody, as described in U.S. Pat. No. 8,871,209 or 9,260,515), an anti-Glucagon Receptor (e.g., anti-GCGR antibody as described in U.S. Pat. No. 9,587,029 or 9,657,099), an anti-VEGF antibody, an anti-IL1R antibody, an interleukin 4 receptor antibody (e.g., an anti-IL4R antibody as described in U.S. Pat. Appin. Pub. No. US2014/0271681A1 or U.S. Pat. No. 8,735,095 or 8,945,559), an anti-interleukin 6 receptor antibody (e.g., an anti-IL6R antibody as described in U.S. Pat. Nos. 7,582,298, 8,043,617 or 9,173,880), an anti-IL1 antibody, an anti-IL2 antibody, an anti-IL3 antibody, an anti-IL4 antibody, an anti-IL5 antibody, an anti-IL6 antibody, an anti-IL7 antibody, an anti-interleukin 33 (e.g., anti-IL33 antibody as described in U.S. Pat. No. 9,453,072 or 9,637,535), an anti-Respiratory syncytial virus antibody (e.g., anti-RSV antibody as described in U.S. Pat. Appin. Pub. No. 9,447,173), an anti-Cluster of differentiation 3 (e.g., an anti-CD3 antibody, as described in U.S. Pat. Nos. 9,447,173 and 9,447,173, and in U.S. Application No. 62/222,605), an anti-Cluster of differentiation 20 (e.g., an anti-CD20 antibody as described in U.S. Pat. No. 9,657,102 and US20150266966A1, and in U.S. Pat. No. 7,879,984), an anti-CD19 antibody, an anti-CD28 antibody, an anti-Cluster of Differentiation-48 (e.g. anti-CD48 antibody as described in U.S. Pat. No. 9,228,014), an anti-Fel d1 antibody (e.g. as described in U.S. Pat. No. 9,079,948), an anti-Middle East Respiratory Syndrome virus (e.g. an anti-MERS antibody as described in U.S. Pat. No. 9,718,872), an anti-Ebola virus antibody (e.g., as described in U.S. Pat. No. 9,771,414), an anti-Zika virus antibody, an anti-Lymphocyte Activation Gene 3 antibody (e.g., an anti-LAG3 antibody, or an anti-CD223 antibody), an anti-Nerve Growth Factor antibody (e.g., an anti-NGF antibody as described in U.S. Pat. Appin. Pub. No. US2016/0017029 and U.S. Pat. Nos. 8,309,088 and 9,353,176) and an anti-Activin A antibody.

In some embodiments, the bispecific antibody is selected from the group consisting of an anti-CD3×anti-CD20 bispecific antibody (as described in U.S. Pat. No. 9,657,102 and U.S. Pat. Appin. Pub. No. US20150266966A1), an anti-CD3×anti-Mucin 16 bispecific antibody (e.g., an anti-CD3×anti-Muc16 bispecific antibody), and an anti-CD3×anti-Prostate-specific membrane antigen bispecific antibody (e.g., an anti-CD3×anti-PSMA bispecific antibody). In some embodiments, the protein of interest is selected from the group consisting of abciximab, adalimumab, adalimumab-atto, ado-trastuzumab, alemtuzumab, alirocicab, atezolizumab, avelumab, basiliximab, belimumab, benralizumab, bevacizumab, bezlotoxumab, blinatumomab, brentuximab vedotin, brodalumab, canakinumab, capromab penodetide, certolizumab pegol, cemiplimab, cetuximab, denosumab, dinutuximab, dupilumab, durvalumab, eculizumab, elotuzumab, emicizumab-kxwh, emtansinealirocicab, evinacumab, evolocumab, fasinumab, golimumab, guselkumab, ibritumomab tiuxetan, idarucizumab, infliximab,

17

infiximab-abda, infiximab-dyyb, ipilimumab, ixekizumab, mepolizumab, necitumumab, nesvacumab, nivolumab, obil-toxaximab, obinutuzumab, ocrelizumab, ofatumumab, olaratumab, omalizumab, panitumumab, pembrolizumab, pertuzumab, ramucirumab, ranibizumab, raxibacumab, reslizumab, rinucumab, rituximab, sarilumab, secukinumab, siltuximab, tocilizumab, tocilizumab, trastuzumab, trevogrumab, ustekinumab, and vedolizumab.

EXAMPLES

Example 1: Universal In-line Protein Concentration Model for UF/DF Applications

Materials and Methods

The data collection for the model included spectral data from Raman Rxn2 and Rxn 4 analyzers (Kaiser Optical Systems, Inc. Ann Arbor, MI) utilizing MR-Probe-785 and RamanRxn Probehead-758 (Kaiser Optical Systems, Inc. Ann Arbor, MI). Additionally, several different optics were used throughout development based on availability. Raman analyzers operating parameters were set to a 10 second scan time for 6 accumulations, repeated 5 times. SIMCA 13 (MKS Data Analytic Solutions, Umea, Sweden) was used to correlate peaks within the spectral data to offline protein concentration measurements. Inline measurements were made throughout different points of UF/DF unit operation including primary concentration, diafiltration, and final concentration. Offline protein concentrations were determined using SoloVPE (C Technologies, Inc.). SoloVPE measurements were made in triplicate.

FIG. 2 shows the spectral regions that were used for making the chemometric models. The regions included region 1—977-1027 cm^{-1} (Ring structure), region 2—1408-1485 cm^{-1} (Arginine), region 3—1621-1711 cm^{-1} (Secondary structure), and region 4—2823-3046 cm^{-1} (C—H stretching). The following spectral filtering was performed on the raw spectral data: 1st derivative with 21 cm^{-1} point smoothing to remove varying baselines

Results

To determine the feasibility of a universal inline protein concentration model for ultrafiltration/diafiltration (UF/DF) applications mAb1 was analyzed using Raman spectroscopy. Protein concentration was measured before diafiltration (primary concentration), during diafiltration (diafiltration), and after diafiltration (final concentration). The calculated concentrations from the model were compared to the protein concentration determined by SoloVPE (FIG. 3). The model error for 0-120 g/L (primary concentration and diafiltration) was 3.1% and the model error for >120 g/L (final concentration) was 1.8% when the training set data was included (mAb 1 spectra incorporated into PLS model).

Processing errors can be detected by Raman spectroscopy. FIG. 3 shows that air entrainment in the system during final recirculation through the UF/DF system was detected by the Raman spectral data. The bars bounded by the rectangle show that the predicted concentration of mAb1 by SoloVPE was >200 g/L while the Raman prediction was ~65 g/L.

FIG. 4 shows absolute Raman model error for ten representative mAbs. This data showed the successful development of models for the mAbs shown which included different mAb isotypes (IgG1 and IgG4) as well as bispecific molecules. 14 out of 17 model predictions met $\leq 5\%$ error. However, specific models (0-120 g/L and >120 g/L) were

18

created for each probe that was used during development as tested in line with multiple mAbs. Model refinement was performed where only one spectral region was the focus of the updated universal model: 2823-3046 cm^{-1} (C—H stretching) with a spectral filtering of Standard Normal Variant (SNV) to correct for laser power variation and probe variability as a baseline correction. A comparison of the two model components developed is summarized in Table 1.

To optimize the model, different probes and lasers were tested in line with multiple mAbs. Model refinement was performed where only one spectral region was the focus of the updated universal model: 2823-3046 cm^{-1} (C—H stretching) with a spectral filtering of Standard Normal Variant (SNV) to correct for laser power variation and probe variability as a baseline correction. A comparison of the two model components developed is summarized in Table 1. Partial Least Squares (PLS) regression models were created with corresponding offline SoloVPE measurements performed in triplicate. The Partial Least Squares Regression Model details are shown in Table 2. The updated dataset predicted with an optimized laser/probe universal model showed 15 out of 17 model predictions meeting $\leq 5\%$ error compared to previous 14 out of 17 (FIG. 5).

TABLE 1

Universal Model Components Comparison		
Component Description	Universal Model (v. 1)	Universal Model (v. 2)
Laser	1	3
Optics	2	6
Preprocessing filter	1 st Derivative with 21 cm^{-1} point smoothing	Standard Normal Variant (SNV)
Spectral Regions	977-1027 cm^{-1} 1408-1485 cm^{-1} 1621-1711 cm^{-1} 2823-3046 cm^{-1}	2823-3046 cm^{-1}

TABLE 2

Protein Concentration Partial Least Squares Regression Universal Model (v. 2) Details		
Final Models	0-120 g/L	>120 g/L
Sample Size	1412	879
R ² X	0.993	0.987
Q ²	0.984	0.958
RMSECV	3.34	7.77

R²X-Percent of variation explained by the model, Target: R² > 0.9

Q²-Percent of variation predicted by the model during cross-validation, Target: Q² > 0.8

RMSECV: Root mean square error of cross-validation

Example 2: Scale-up Performance of Protein Concentration Models

Materials and Methods

The optimized Universal models (v. 2) (see Table 1) were tested with a scale-up 1/2" Single Use Tangential Flow Filtration System (Pall Corporation) experiment with mAb10. The mAb10 load material was formulated drug substance, rather than typical processing load material. The FDS material was diluted to representative UF/DF load source including protein concentration and buffer excipients. However, due to the presence of additional excipients in load source that had not been tested during the universal model development, mAb 10 specific models were created. Refer to example 1 for methods for Raman data collection and scan length information. The mAb specific model for >120 g/L used the same spectral regions and pre-processing

techniques as the Universal model (v. 2). However, the 0-120 g/L mAb specific model used the four spectral regions as shown in FIG. 2 with Standard Normal Variant pre-processing. The differences in the 0-120 g/L model can be attributed to the additional excipients in the load source. Results

The model goal of $\leq 5\%$ error was met for $\frac{3}{4}$ updated models when the training set was included in the model predictions as shown in Table 3. Based on the notable differences such as the load source, laser and scale (bench scale vs. scale-up) during the preliminary experimentation at TOPS a second run was performed. Prior to the second experiment, a change was made to the 0-120 g/L mAb 10 specific model. All four regions were included using SNV pre-processing but the three regions; 977-1027 cm^{-1} , 1408-1485 cm^{-1} , and 1621-1711 cm^{-1} additionally used 1st derivative with 21 cm^{-1} point smoothing. A summary of the compiled experimental results is summarized in Table 3. During the second experiment, the model goal of $\leq 5\%$ error was met for $\frac{3}{4}$ updated models when the training set was included in the model predictions as shown in Table 3. An additional observation made during data analysis was the load source being the main contributing factor to increased error. If the load sample is removed, the universal model error is reduced from 8.6% to 5.7%. In FIG. 7, the results for the inline predictions (real-time, bars with wide hatching) and updated models (bars with narrow hatching) for the final concentrated pool are shown comparing the protein concentration to the offline measurement of the SoloVPE (empty bars). The universal model inline and updated model had an error of 2.7% whereas the mAb 10 model inline and updated model was 12.0% and 4.2%, respectively for final concentrated pool. The increased error observed in the mAb 10 model can be attributed to limited data in the ~ 250 g/L range whereas the universal model has a larger data set. An additional contributing factor to the increased error is the inability of models to extrapolate outside the characterized range (i.e. >250 g/L in the mAb 10 model).

TABLE 3

Average Model Error for Protein Concentration Predictions in Scale Up				
	IOPS Experiment # 1		IOPS Experiment # 2	
	Inline	Updated	Inline	Updated ¹
Universal 0-120 g/L	13.8%	8.9%	9.9%	8.6%
Universal >120 g/L	8.8%	2.8%	5.1%	5.0%
mAb 11 0-120 g/L	6.0%	5.5%	4.1%	3.5%
mAb 11 >120 g/L	12.0%	1.5%	8.8%	3.6%

¹Removal of load sample reduces error; Universal (0-120 g/L): 8.6% to 5.7% and mAb11 (0-120 g/L): 3.5% to 2.7%

Example 3: Protein Concentration Model Scale-Up to Pilot Processing Equipment

Materials and Methods

During process development of commercially enabled processes, the UF/DF is characterized as unit operation following Quality by Design principles to understand critical process parameters as well as critical quality attributes. Raman and model development was included during mAb 11 development to enhance process understanding and propose a streamlined approach to model development. Refer to example 1 for method information for Raman data collection with the exception of scan time length which was adjusted

from 10 seconds to 5 seconds. The developed mAb 11 model used SNV pre-processing for all four spectral regions but the three regions; 977-1027 cm^{-1} , 1408-1485 cm^{-1} , and 1621-1711 cm^{-1} . additionally used 1st derivative with 21 cm^{-1} point smoothing.

Results:

The bench-scale model was generated using four DoE experiments and 4 spectral regions. FIG. 8A shows the Raman model error for real time predictions from four DoE experiments. FIG. 8B shows the Raman model error for 15 additional experiments using the bench scale model. mAb specific protein concentration models were generated for 0-120 g/L and >120 g/L with $\leq 5\%$ error.

Using bench-scale model (n=15), pilot-scale runs (n=3) have a prediction error of 0.6%-10.6% for mAb11 (FIG. 9A). Pilot-scale prediction error decreased to 0.6-2.2% when pilot-scale data was incorporated into the bench-scale model (n=18). Increased bench-scale model error is likely a result of temperature impact on Raman spectral shifts due to heat dissipation associated with scale-up equipment. Temperature will be a factor considered during future Raman development and model verification claims.

In seven pilot scale experiments with three different monoclonal antibodies (mAb J, mAb K, and mAb L) final model prediction error was 0.6-2.2%; well within the 5% goal (FIG. 9B).

Example 4: Use of Raman Models for Real-time Concentration Determination Allowing Processing Decisions

Materials and Methods

Refer to example 3 for further information as the same protocol for Raman spectral collection and modeling was used for Raman automations. An automated control strategy was developed to use Raman spectral data to achieve final protein concentration targets. Using the generated predictive models, data was filtered, and was used to provide input to instrumentation on the UF/DF to terminate the unit operation upon achieving the protein concentration target. SoloVPE measurements were made in triplicate.

Results:

FIGS. 10A and 10B show exemplary screen setup for automated monitoring of batch UF/DF and single-pass TFF protein concentration. FIG. 11 shows that predictive modeling can be used to monitor real-time concentration of mAb14 throughout various processing steps and trigger the concentration unit operation to stop when a desired concentration target has been met. The final concentrated pool was predicted by Raman to be 260 g/L compared to the offline SoloVPE measurement of 262 g/L resulting in a 0.8% error meeting the $\leq 5\%$ error goal. Raman is a suitable application to be used to make automated processing decisions verifying the desired protein concentration target is met.

Example 5: Proof of Concept for High Molecular Weight (HMW) Species Modeling in UF/DF

Materials and Methods

The data collection for the HMW species model included spectral data from Raman Rxn2 analyzers (Kaiser Optical Systems, Inc. Ann Arbor, MI) RamanRxn Probehead-758 (Kaiser Optical Systems, Inc. Ann Arbor, MI). Additionally, several different optics were used throughout development based on availability. Raman analyzers operating parameters

21

were set to a 72 second scan time for 1 accumulation, repeated 25 times. Inline measurements were made throughout different points of UF/DF unit operation including primary concentration, diafiltration, and final concentration. The spectral range was 110-3415 cm^{-1} . The raw spectral data was pre-processed using SNV and additionally filtered using 1st derivative with 21 cm^{-1} smoothing. Offline HMW species measurements were determined using size-exclusion ultra performance liquid chromatography.

Results:

HMW species are another attribute that are deemed a preliminary critical quality attribute in protein purification. Current technologies cannot monitor HMW species in real-time during processing. FIG. 12A shows that the disclosed Raman modeling method can be used to monitor HMW species during protein purification. HMW species predictions by Raman modeling were compared to measurements collected using SE-UPLC throughout purification (primary concentration, diafiltration, and final concentration). Raman modeling effectively predicted the percent of high molecular species in real-time during protein processing. The model was generated with an average error of 3.4%.

Example 6. Proof of Concept for High Molecular Weight (HMW) Species Modeling in Polishing Chromatography

Materials and Methods

The data collection for the HMW species model included spectral data from Raman Rxn2 analyzers (Kaiser Optical Systems, Inc. Ann Arbor, MI) utilizing MR-Probe-785. Raman analyzer operating parameters were set to either 10, 30, or 60 second scan times for 1 accumulations with 5 repetitive measurements. Offline measurements were made with anion exchange chromatography (AEX) pools with 6.2%-76.2% total HMW. The spectral ranges used for modeling and pre-processing techniques used are described in Table 4. Offline HMW species measurements were determined using size-exclusion ultra-performance liquid chromatography.

Results:

The disclosed Raman modeling method can be used to monitor HMW species during polishing chromatography protein purification. HMW species predictions by Raman modeling were compared to measurements collected using SE-UPLC from the generated AEX pools. As summarized in Table 4, the RMSEP of the evaluated methods ranged from 3.2-7.6%. In FIG. 12B, a condensed data set of 6.2%-19.7% HMW was used to evaluate a model generated with a spectral region of 350-3100 cm^{-1} and SNV pre-processing techniques. By reducing the HMW range, the RMSEP was reduced to 1.2%, 1.4%, and 2.1% for 10, 30, and 60 seconds respectively. Based on these results HMW content can be determined with Raman in AEX pools.

TABLE 4

HMW Model Predicted Error (RMSEP) for HMW content of 6.2%-76.2%.			
	10 Sec.	30 Sec.	60 Sec.
1550-1725 cm^{-1}	7.62%	5.31%	3.21%
1 st Der.			
350-3100 cm^{-1}	3.48%	3.37%	4.63%
SNV			
990-1020, 1550-1725 cm^{-1}	7.12%	7.48%	4.98%
1 st Der.			

22

Example 7. Proof of Concept for Titer Modeling

Materials and Methods

The training set model was 35 protein A flow through samples spiked with FCP (265 g/L) to achieve titers ranging from 0.36-9.8 g/L. The model was evaluated on diluted depth filtrate samples with titers ranging from 1.3-8.8 g/L. The data collection for the titer model included spectral data from Raman Rxn2 (Kaiser Optical Systems, Inc. Ann Arbor, MI) utilizing MR-Probe-785. An immersion probe was used in an offline fashion to generate spectral data with operating parameters set to a 20 second scan time for 1 accumulation, repeated 5 times. The spectral ranges were 977-1027, 1408-1485, 1621-1711, and 2823-3046 cm^{-1} . The raw spectral data was pre-processed using SNV and additionally filtered using 1st derivative with 21 cm^{-1} smoothing. Model characteristics are described in Table 5.

TABLE 5

Antibody Titer Model Characteristics.	
Spectral Regions (cm^{-1})	3046-2823, 1711-1621, 1485-1408, 1027-977
Preprocessing techniques	1 st derivative and SNV
Accumulations and Length	5 x 20 seconds
Average Model Error	25.7%

Results:

Antibody titer is a process attribute in protein purification that is needed to inform subsequent downstream purification unit operations including affinity column loading, production consistency, as well as in-process intermediate volume constraints. Inaccurate column loading can impact subsequent preliminary critical quality attributes hence the desire for a monitoring technique such as Raman spectroscopy. FIG. 13 shows actual antibody titer versus Raman predicted antibody titer for a monoclonal antibody. In this experiment, the model error was 26% which is higher than a desired goal of $\leq 5\%$. Increasing scan lengths as well as developing a model using diluted and non-diluted depth filtrate will reduce the model error.

Example 8: Raman Models for Buffer Excipient Measurements that Meet Current Orthogonal Assay Error of about 10%

Materials and Methods

Data was collected from previous concentration model development runs for various antibodies. Refer to example 1 for method information for Raman data collection. Table 6 shows the model components for detecting histidine and arginine in the samples. The spectral regions were based on known histidine/arginine peaks (Zhu, et al., *Spectrochim Acta A Mol Biomol Spectrosc*, 78(3):1187-1195 (2011)). Following initial model development of histidine and arginine, further model characterization was performed with mAb 14. Using a non-contact optic probe, Raman analyzer operating parameters were set to a 20 second scan time for 5 accumulations. The spectral range for histidine was 1200-1480 cm^{-1} and for arginine 860-1470 cm^{-1} were used. For both buffer excipients the raw spectral data was pre-processed using SNV and additionally filtered using 1st derivative with 21 cm^{-1} smoothing. Offline histidine and arginine

species measurements were determined using an ultra-performance liquid chromatography (UPLC) amino acid quantification-based method.

Results:

To determine if the disclosed Raman modeling method and system could be used to measure buffer excipients in a processed antibody sample, data collected from previous concentration model development runs were analyzed for histidine and arginine. Predicted values using Raman modeling were compared to values calculated based on the UPLC based amino acid method as can be seen in FIG. 14A. The predicted values and average model error for the preliminary histidine/arginine Raman modeling are presented in Table 6. In FIG. 14B a dot plot for predicted histidine versus actual histidine model is shown for mAb 14 with an average model error of 8.2% meeting the $\leq 10\%$ goal for buffer excipients. The $\leq 10\%$ goal is based on the current UPLC orthogonal method assay variability. In FIG. 14C a dot plot for predicted arginine versus actual arginine model is shown for mAb 14 with an average model error of 2.9% meeting the $\leq 10\%$ goal.

This data shows that Raman modeling can be used to predict the levels of buffer excipients from in-process UF/DF and FCP material. Successful quantification of these excipients ensures that UF/DF provides a final concentrated pool that will enable subsequent formulation.

TABLE 6

Model components and data collected for histidine/arginine from universal concentration model (example 1) processing.		
	Histidine	Arginine
Spectral Region (cm ⁻¹)	1200-1480	970-1100, 1300-1500
Preprocessing technique	1 st derivative and SNV	1 st derivative and SNV
R ² Y	0.940	0.964
Q ²	0.938	0.963
RMSEP	1.20 mM	6.19 mM
Average Model Error	10.4%	7.39%

Histidine Range: 0-25 mM; Arginine Range: 0-81 mM

SNV-Standard Normal Variate-mean centered and normalized

R²-Percent of variation in the training set explained by the model, R² > 0.9

Q²-Percent of variation in the training set predicted by the model during cross-validation, Q² > 0.8

(RMSEP) Root Mean Square Error Prediction

Example 9: Raman Models for Drug-to-antibody Ratio Measurements

Materials and Methods

DAR is a quality attribute that is monitored during development of antibody-drug conjugates (ADC), antibody-radionuclide conjugates (ARC), and general protein conjugates (potent steroids, non-cytotoxic payloads, etc.) to ensure consistent product quality and to facilitate subsequent labeling with payloads. Raman was evaluated as technology to monitor DAR levels which could then be used a control strategy for the reaction. Two different mAbs that were under development (mAb 1 and mAb 3) were assessed for DAR determination feasibility using Raman. Using a non-contact optic probe, Raman analyzer operating parameters were set to a 10 second scan time for 10 accumulations. The spectral range of 350-3100 cm⁻¹ was used with the raw spectral data pre-processed using SNV and additionally filtered using 2nd derivative with 21 cm⁻¹ smoothing. Table 7 shows the model components for determining DAR in the

samples. Offline DAR measurements were determined using a UV spectroscopy-based method.

TABLE 7

Model components for drug-antibody ratio measurements.		
Model Name	REGN2810 UV-DAR	REGN910 UV-DAR
Y Range	0.81-4.39	0.79-3.57
Best Model	2 nd Derivative	2 nd Derivative
	R2Y = 0.788	R2Y = 0.994
	Q2 = 0.548	Q2 = 0.776
	RMSECV = 0.64	RMSECV = 0.58

Results:

FIGS. 15A-15B show that Raman modeling can be used to measure drug-to-antibody ratio for an iPET drug conjugates for mAb 1 and mAb 3. For both models the root mean square error of cross validation was 0.6 DAR. The current orthogonal UV based assay has variability associated with 0.3 DAR (one standard deviation). The initial Raman prediction is within two standard deviations and suggests with further model refinement DAR can be successfully predicted with Raman.

While in the foregoing specification this invention has been described in relation to certain embodiments thereof, and many details have been put forth for the purpose of illustration, it will be apparent to those skilled in the art that the invention is susceptible to additional embodiments and that certain of the details described herein can be varied considerably without departing from the basic principles of the invention.

All references cited herein are incorporated by reference in their entirety. The present invention may be embodied in other specific forms without departing from the spirit or essential attributes thereof and, accordingly, reference should be made to the appended claims, rather than to the foregoing specification, as indicating the scope of the invention.

We claim:

1. A method of producing a protein purification intermediate, comprising:

providing a universal model produced using a plurality of protein purification intermediates;

quantifying one or more impurities in the protein purification intermediate using in situ Raman spectroscopy; and

adjusting parameters of the process to obtain or maintain the protein purification intermediate at a predetermined purity.

2. The method of claim 1, wherein the parameters of the process are adjusted in-real time.

3. The method of claim 1, wherein the process is a downstream process.

4. The method of claim 1, further comprising removing the one or more impurities from the protein purification intermediate, wherein the one or more impurities impact the protein purification intermediate's safety, efficacy, potency, pharmacokinetics, or pharmacological activity, or a combination thereof.

5. The method of claim 1, wherein the one or more impurities is selected from the group consisting of a product-related impurity, a high molecular weight (HMW) species, a host cell protein, a DNA, a virus, an endotoxin, an aggregate, a concentration, an excipient, and combinations thereof.

25

6. The method of claim 1, further comprising quantifying one or more critical quality attributes in the protein purification intermediate using in situ Raman spectroscopy; and adjusting parameters of the process to obtain or maintain the protein purification intermediate at a predetermined critical quality attribute level,

wherein the critical quality attributes is selected from the group consisting of antibody titer, protein concentration, high molecular weight species, drug-antibody ratio, excipients, pH, salts, and combinations thereof.

7. The method of claim 3, wherein the downstream process comprises at least one selected from the group consisting of cell harvest, centrifugation, direct depth filtration, affinity capture, protein A affinity purification, viral inactivation, polishing chromatography, ion-exchange chromatography, cation exchange chromatography, anion exchange chromatography, hydrophobic interaction chromatography, size-exclusion chromatography, virus retentive filtration, ultrafiltration/diafiltration, and combinations thereof.

8. The method of claim 1, further comprising determining the concentration of the protein purification intermediate in-real time using in situ Raman spectroscopy with the universal model while processing the protein purification intermediate.

9. The method of claim 8, wherein determining the concentration of the protein purification intermediate occurs continuously or intermittently in real-time.

10. The method of claim 1, further comprising providing a protein specific model produced using the protein purification intermediate.

11. The method of claim 10, further comprising determining the concentration of the protein purification intermediate in-real time using in situ Raman spectroscopy with the protein specific model while processing the protein purification intermediate.

12. The method of claim 1, further comprising producing the protein purification intermediate when the concentration reaches a predetermined concentration.

13. The method of claim 1, wherein the concentration of the protein purification intermediate is at least 150 mg/mL.

14. The method of claim 1, wherein the concentration of the protein purification intermediate is between about 150 mg/mL to about 300 mg/mL.

15. The method of claim 1, wherein the protein purification intermediate is concentrated using ultrafiltration, buffer exchange, or both.

16. The method of claim 1, wherein the protein purification intermediate is harvested from a bioreactor, a fed-batch culture, or a continuous culture.

26

17. The method of claim 1, wherein the protein purification intermediate is selected from the group consisting of an antibody, an antigen binding fragment, a fusion protein, and a recombinant protein.

18. The method of claim 1, further comprising performing a normalization technique or point-smoothing on the Raman spectroscopy data.

19. The method of claim 1, wherein the model provides predicted protein concentration values for a plurality of protein purification intermediates with $\leq 5\%$ error compared to off-line protein concentration values.

20. The method of claim 1, wherein the protein purification intermediate is further concentrated using at least one selected from the group consisting of ultrafiltration and diafiltration.

21. The method of claim 6, wherein the excipient comprises a buffer excipient, wherein the buffer excipient comprises at least one selected from the group consisting of acetate, citrate, histidine, succinate, phosphate, tris(hydroxymethyl)aminomethane (Tris), proline, arginine, sucrose, and combinations thereof.

22. The method of claim 6, wherein the excipient comprises a surfactant excipient, wherein the surfactant excipient comprises at least one selected from the group consisting of polysorbate 80, polysorbate 20, poloxamer 188, and combinations thereof.

23. The method of claim 6, wherein the excipient comprises at least one selected from the group consisting of polyethylene glycol, sucrose, and combinations thereof.

24. The method of claim 1, wherein spectral data is collected at one or more wavenumber ranges.

25. The method of claim 24, wherein spectral data is collected at one or more wavenumber ranges selected from the group consisting of 977-1027 cm^{-1} , 1408-1485 cm^{-1} , 1621-1711 cm^{-1} , 2823-3046 cm^{-1} , and combinations thereof.

26. The method of claim 1, wherein the protein purification intermediate comprises at least one selected from the group consisting of an extracellular domain of a cell surface receptor, a fragment thereof, and combinations thereof.

27. The method of claim 1, wherein the protein purification intermediate comprises at least one selected from the group consisting of a Fc-fusion protein, a fragment thereof, and combinations thereof.

28. The method of claim 1, wherein the protein purification intermediate comprises at least one selected from the group consisting of an antibody, an antigen binding fragment thereof, and combinations thereof.

29. The method of claim 1, further comprising at least one selected from the group consisting of determining and adjusting chromatography column loadings.

* * * * *