



US0D1092718S

(12) **United States Design Patent**
Formica et al.

(10) **Patent No.:** **US D1,092,718 S**
(45) **Date of Patent:** **** Sep. 9, 2025**

(54) **HUMIDIFIER TUB FOR POSITIVE AIRWAY PRESSURE DELIVERY CONSOLE**

D1,010,130 S 1/2024 Bath
12,083,284 B2 * 9/2024 Lin A61M 16/0816
12,102,769 B2 * 10/2024 Bath A61M 16/021

(Continued)

(71) Applicant: **ResMed Pty Ltd**, Bella Vista (AU)

(72) Inventors: **Justin John Formica**, Sydney (AU);
Sung Hoon Mun, Sydney (AU)

(73) Assignee: **ResMed Pty Ltd**, Bella Vista (AU)

(**) Term: **15 Years**

(21) Appl. No.: **29/982,357**

(22) Filed: **Jan. 6, 2025**

Related U.S. Application Data

(62) Division of application No. 29/731,572, filed on Apr. 16, 2020, now Pat. No. Des. 1,061,869.

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.** **D24/110**
USPC **D24/110**

(58) **Field of Classification Search**
USPC D24/110, 108, 110.6, 111, 164
CPC A61M 16/0057; A61M 16/006; A61M 16/0063; A61M 16/0072; A61M 16/0075; A61M 16/0081; A61M 16/0066; A61M 16/109

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D738,489 S	9/2015	Formica	
D744,108 S	11/2015	Verma	
D791,329 S *	7/2017	Verma	D24/164
D798,428 S	9/2017	Cork	
D809,124 S	1/2018	Bertinetti	
D889,659 S	7/2020	Bath	
D892,303 S	8/2020	Formica	
D921,900 S	6/2021	Verma	

FOREIGN PATENT DOCUMENTS

EM	015025278-0005	6/2023
WO	WO 2014/138804 A1	9/2014
WO	WO 2015/089582 A1	6/2015

OTHER PUBLICATIONS

“ResMed AirSense 11: Get to know your sleep therapy device,” posted by Resmed. Youtube. Posting date: Sep. 14, 2021. Retrieval date: Mar. 23, 2024. Retrieved from internet: <https://www.youtube.com/watch?v=c-35CQaSkcs> (Year: 2021).

(Continued)

Primary Examiner — Daniel J Domino

Assistant Examiner — Lee D. Starr

(74) *Attorney, Agent, or Firm* — Nixon & Vanderhye P.C.

(57) **CLAIM**

The ornamental design for a humidifier tub for positive airway pressure delivery console, as shown and described.

DESCRIPTION

FIG. 1 is a rear perspective view of a humidifier tub for positive airway pressure delivery console showing our new design;

FIG. 2 is a left side view thereof;

FIG. 3 is a right side view thereof;

FIG. 4 is a top view thereof;

FIG. 5 is a bottom view thereof;


FIG. 6 is a front view thereof;

FIG. 7 is a rear view thereof; and,

FIG. 8 is another rear perspective view thereof.

The broken lines represent portions of the humidifier tub for positive airway pressure delivery console and do not form a portion of the claimed design.

1 Claim, 8 Drawing Sheets

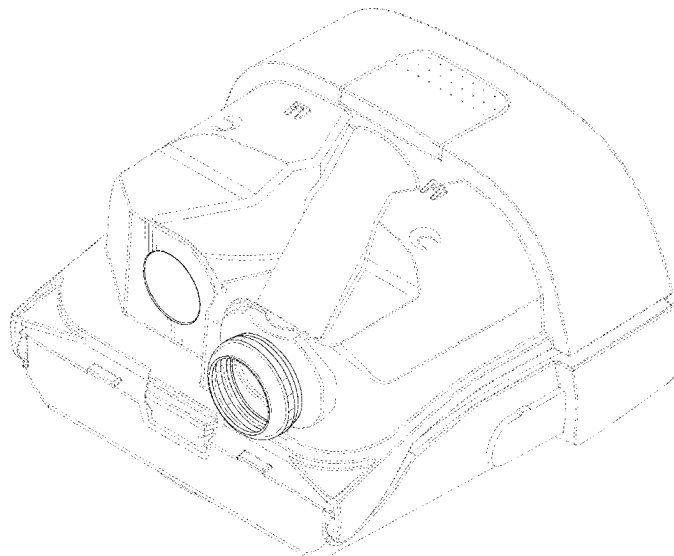

(56)

References Cited

U.S. PATENT DOCUMENTS

D1,054,547	S *	12/2024	Formica	D24/110
12,168,100	B2 *	12/2024	Tang	A61M 16/16
D1,061,869	S *	2/2025	Formica	D24/110
2008/0009835	A1	1/2008	Kriesel	
2014/0264975	A1	9/2014	Bath	
2015/0273167	A1	10/2015	Feldhahn	
2016/0022954	A1	1/2016	Bath	
2016/0199612	A1 *	7/2016	Foote	A61M 16/0875 128/202.27
2016/0310691	A1 *	10/2016	Bath	G16H 20/40
2018/0043125	A1	2/2018	Bencke	
2018/0333556	A1	11/2018	Ormrod	
2019/0298964	A1	10/2019	Bayer	
2020/0330720	A1	10/2020	Formica	
2021/0093825	A1	4/2021	Lin	
2021/0379322	A1	12/2021	Maurer	
2022/0016383	A1	1/2022	Workman	
2022/0265954	A1	8/2022	Tyke	
2022/0339395	A1	10/2022	Hattori	
2023/0075277	A1	3/2023	Cork	
2023/0256181	A1	8/2023	Hartono	
2024/0189530	A1 *	6/2024	Doudkine	A61M 16/024

OTHER PUBLICATIONS

Formica et al., U.S. Appl. No. 29/731,572, filed Apr. 16, 2020, for "Humidifier Tub for Positive Airway Pressure Delivery Console," (parent application).

* cited by examiner

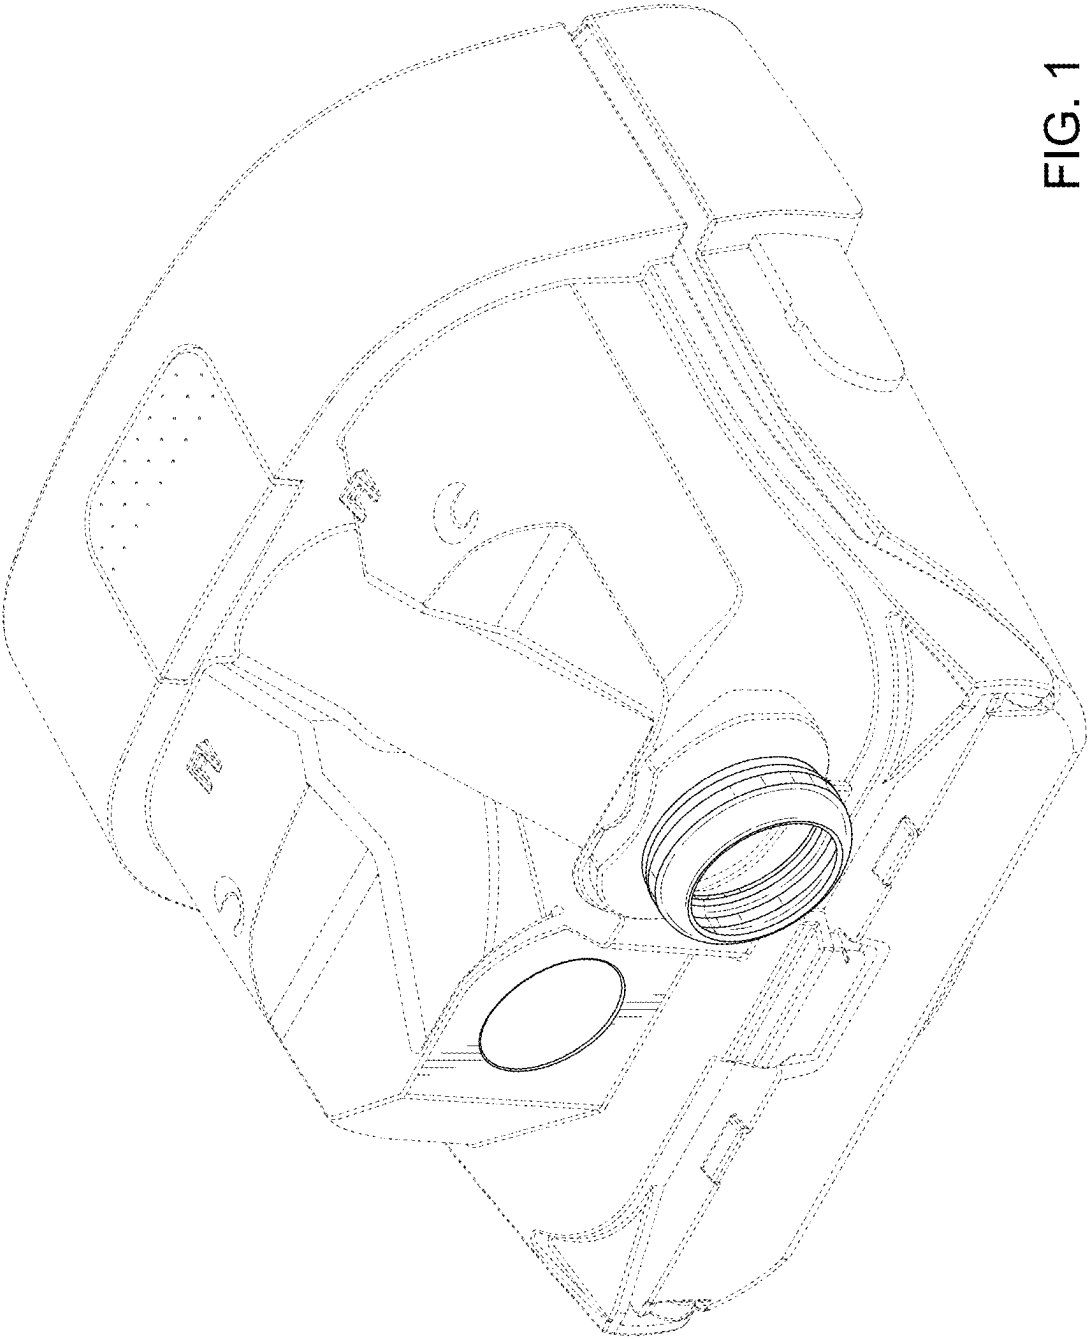


FIG. 1

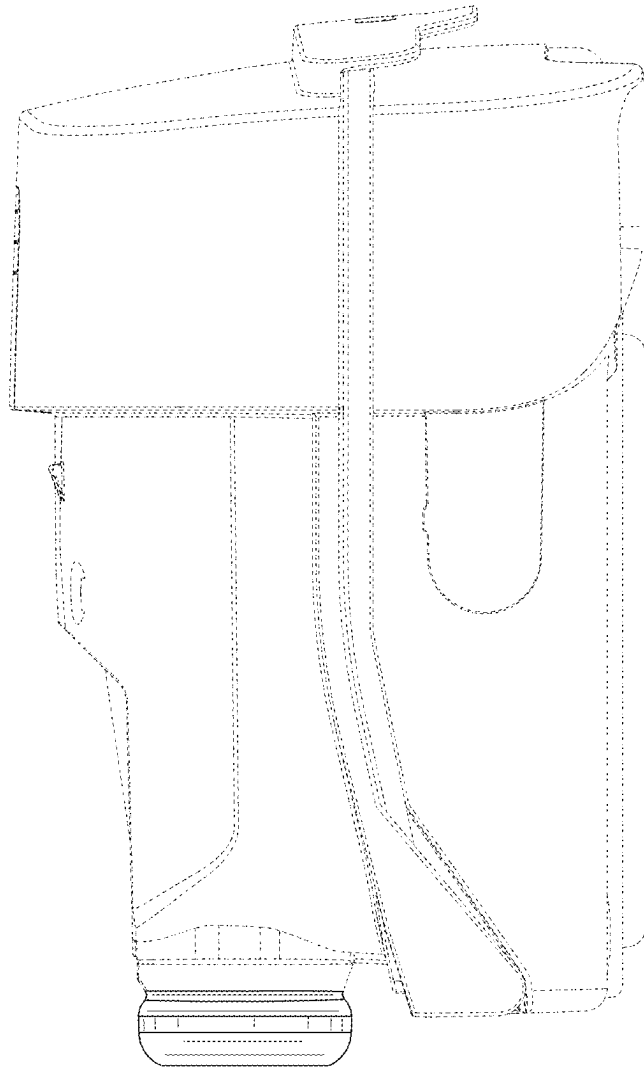


FIG. 2

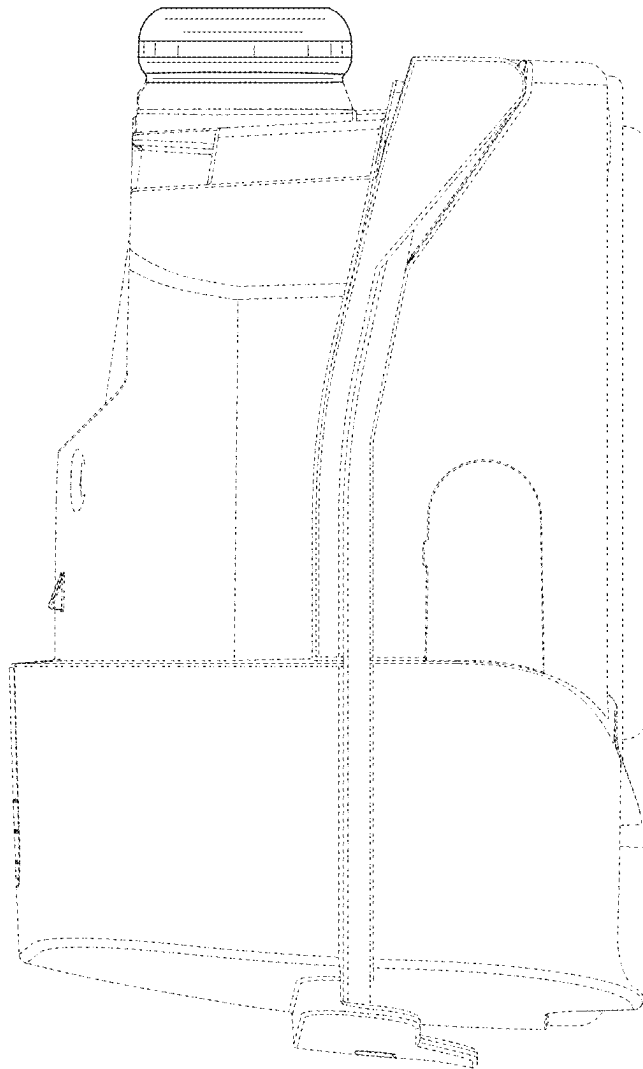


FIG. 3

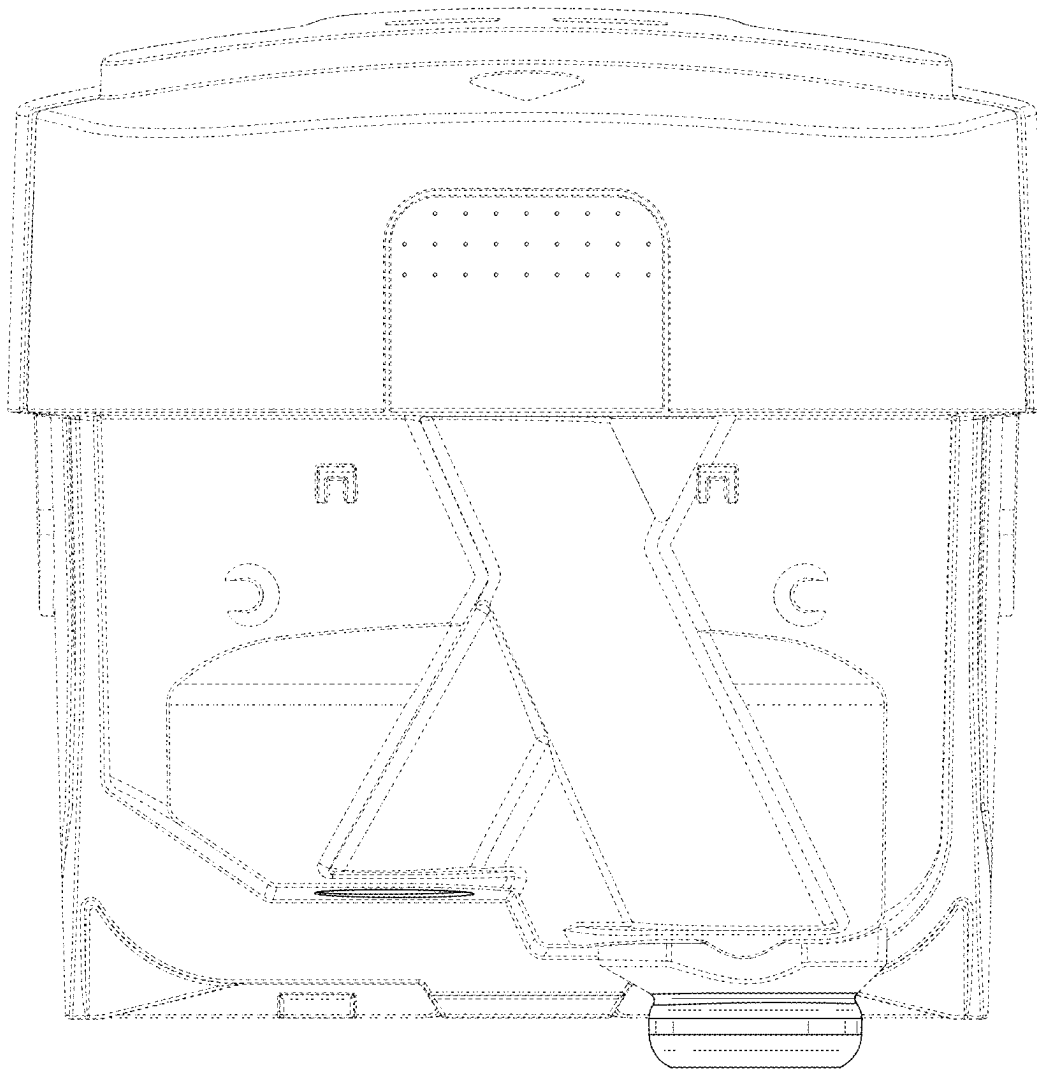


FIG. 4

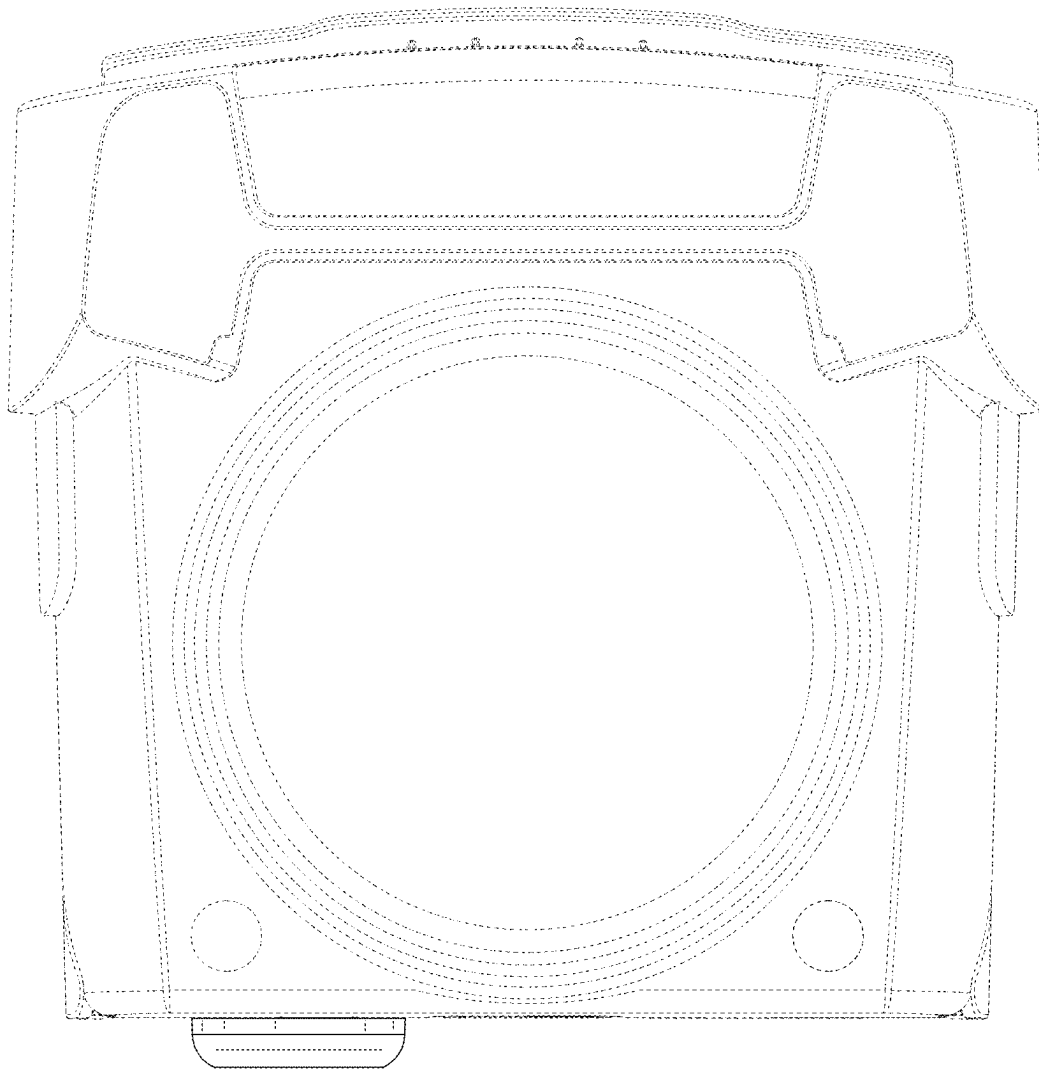


FIG. 5

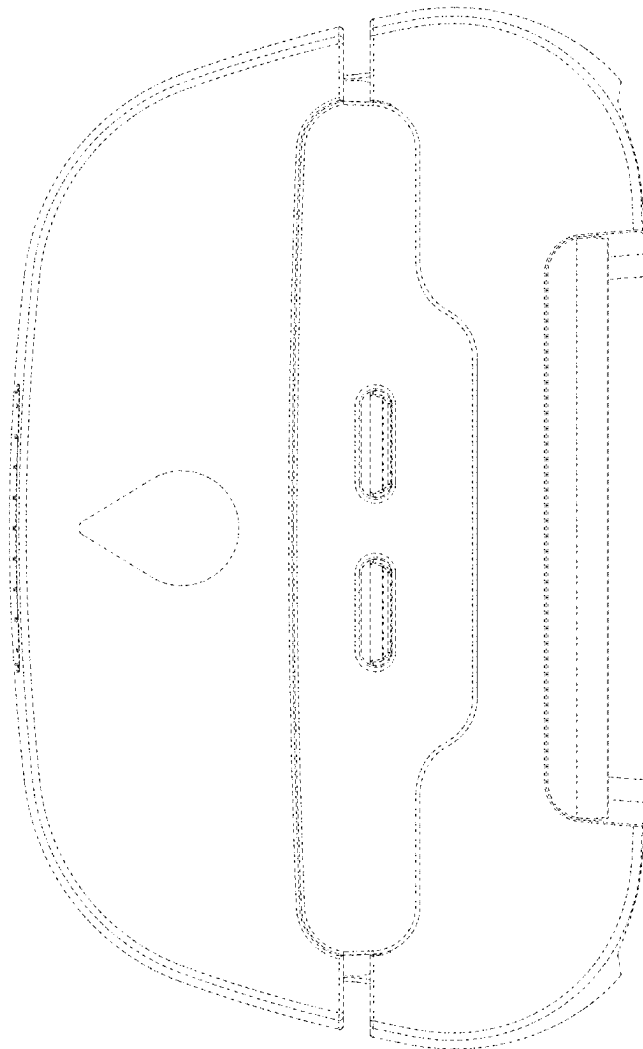


FIG. 6

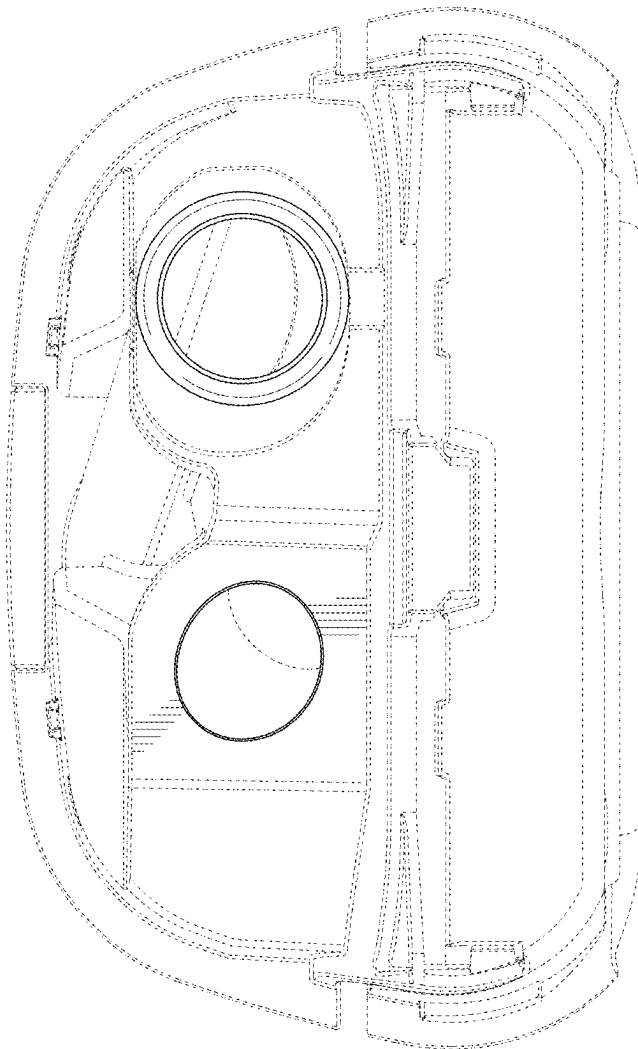


FIG. 7

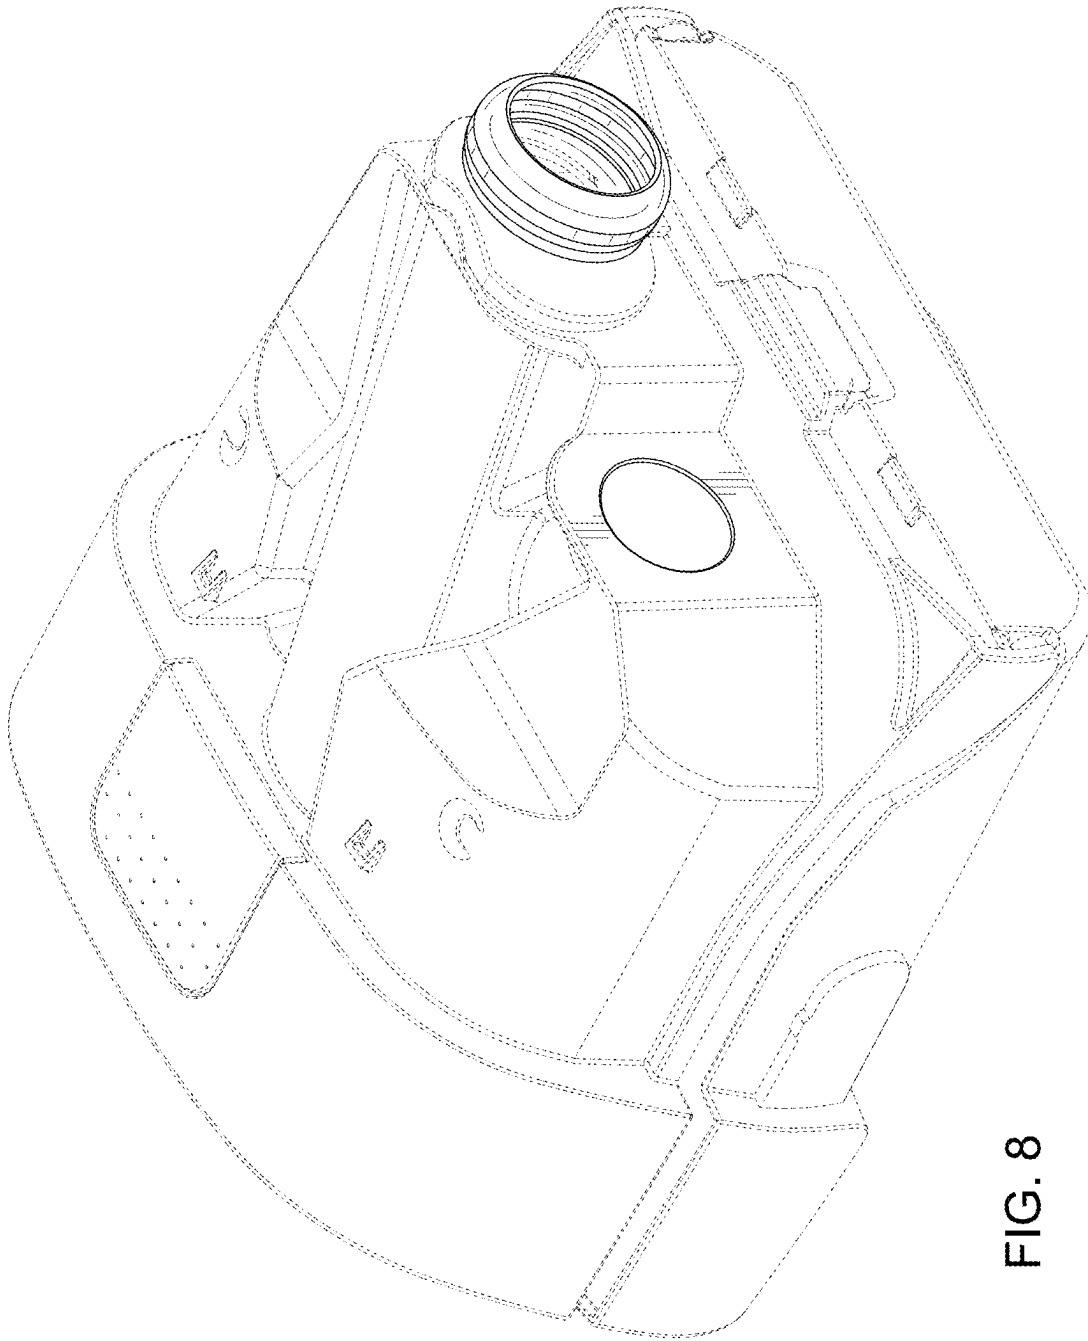


FIG. 8