



US0D1092758S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,092,758 S**  
**White et al.** (45) **Date of Patent:** **\*\* Sep. 9, 2025**

(54) **TRANSCRANIAL ELECTRO-STIMULATION  
DEVICE**

(71) Applicant: **Nexalin Technology, Inc.**, Houston, TX  
(US)

(72) Inventors: **Mark H. White**, Houston, TX (US);  
**John Patrick Claude**, Redwood City,  
CA (US)

(73) Assignee: **NEXALIN TECHNOLOGY, INC.**,  
Houston, TX (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/994,229**

(22) Filed: **Mar. 19, 2025**

**Related U.S. Application Data**

(62) Division of application No. 29/917,241, filed on Nov.  
17, 2023, now Pat. No. Des. 1,073,092.

(51) **LOC (15) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/200; D24/231**

(58) **Field of Classification Search**

USPC ..... D24/133, 141, 144, 155, 170, 187, 188,  
D24/190, 191, 200, 211.214, 215, 231

CPC ..... A61H 39/002; A61H 2201/10; A61H  
2205/02; A61N 1/36; A61N 1/36014;  
A61N 1/36017; A61N 1/36021

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

|          |   |   |        |            |       |         |
|----------|---|---|--------|------------|-------|---------|
| D456,908 | S | * | 5/2002 | Cunningham | ..... | D24/200 |
| D749,746 | S | * | 2/2016 | Guarraia   | ..... | D24/200 |
| D750,794 | S | * | 3/2016 | Guarraia   | ..... | D24/200 |
| D908,230 | S | * | 1/2021 | Chu        | ..... | D24/200 |
| D922,592 | S | * | 6/2021 | Chu        | ..... | D24/200 |

|              |    |   |         |         |       |             |
|--------------|----|---|---------|---------|-------|-------------|
| D922,593     | S  | * | 6/2021  | Chu     | ..... | D24/200     |
| D930,162     | S  | * | 9/2021  | Cremer  | ..... | D24/231     |
| D1,058,938   | S  | * | 1/2025  | Wilson  | ..... | D29/102     |
| D1,066,700   | S  | * | 3/2025  | Roman   | ..... | D24/200     |
| D1,073,092   | S  | * | 4/2025  | White   | ..... | D24/231     |
| 2016/0367804 | A1 | * | 12/2016 | Peng    | ..... | A61N 1/0456 |
| 2019/0022372 | A1 | * | 1/2019  | Dar     | ..... | A61N 1/0484 |
| 2022/0054864 | A1 | * | 2/2022  | Baldoni | ..... | A61N 7/02   |

**OTHER PUBLICATIONS**

Brain Spa Insomnia Relief Device, found online Jul. 10, 2025 at  
<https://www.amazon.com/dp/B0861V6FK2?> Reference dated Jun.  
4, 2024.\*

(Continued)

*Primary Examiner* — Kendra Leslie Hamilton

*Assistant Examiner* — Jameson P Carey

(74) *Attorney, Agent, or Firm* — STETINA GARRED  
BRUCKER & NEWBOLES

(57) **CLAIM**


The ornamental design for a transcranial electro-stimulation  
device as shown and described.

**DESCRIPTION**

FIG. 1 is bottom perspective view of our new design for a  
transcranial electro-stimulation device;  
FIG. 2 is top perspective view thereof;  
FIG. 3 is top plan view thereof;  
FIG. 4 is front elevation view thereof;  
FIG. 5 is right side elevation view thereof;  
FIG. 6 is left side elevation view thereof;  
FIG. 7 is bottom plan view thereof; and,  
FIG. 8 is rear elevation view thereof.

The portions of the transcranial electro-stimulation device  
shown in broken lines in FIGS. 1-8 form no part of the  
claimed design. The drawings are shaded to indicate con-  
trasting surfaces.

**1 Claim, 4 Drawing Sheets**

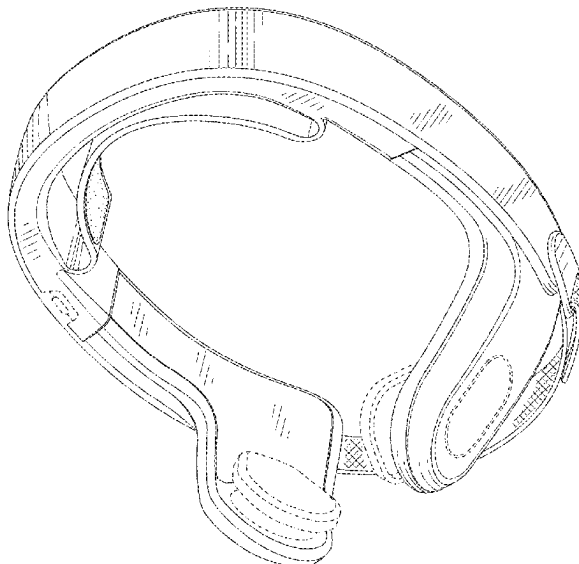

(56)

**References Cited**


OTHER PUBLICATIONS

Capotron Brain Stimulator, found online Jul. 10, 2025 at <https://www.amazon.ca/dp/B07HL2S9JQ/?th=1> Reference dated Oct. 15, 2020.\*


Interaxon Muse 2 Brain Detection Headband, found online Jul. 10, 2025 at <https://www.amazon.ae/dp/B08KHNRMYS> Reference dated Nov. 3, 2018.\*

Piyuda Smart Brain Helmet, found online Jul. 10, 2025 at <https://www.amazon.com/dp/B0D62H9FX1> Reference dated Mar. 23, 2020.\*


\* cited by examiner

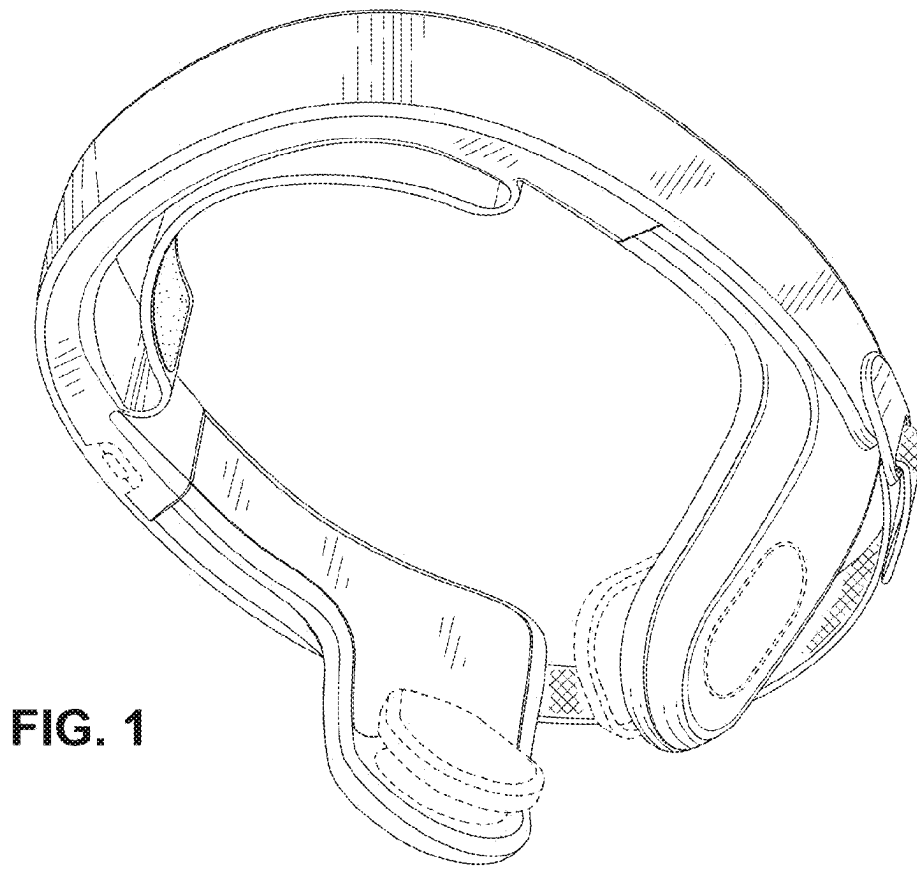


**FIG. 1**

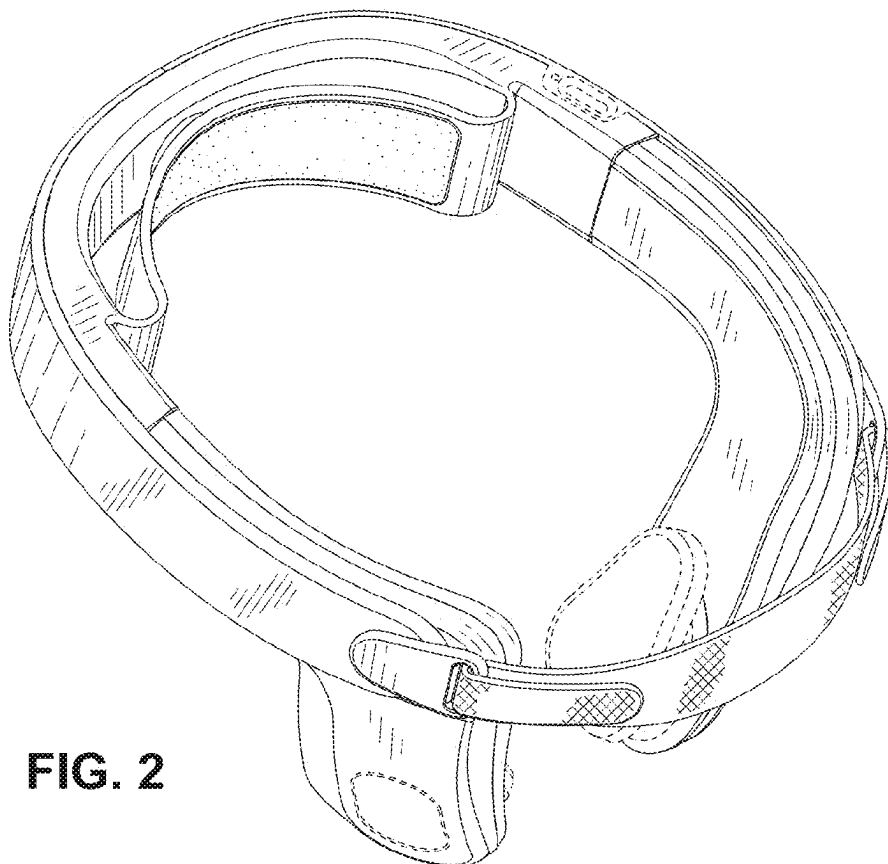


**FIG. 2**

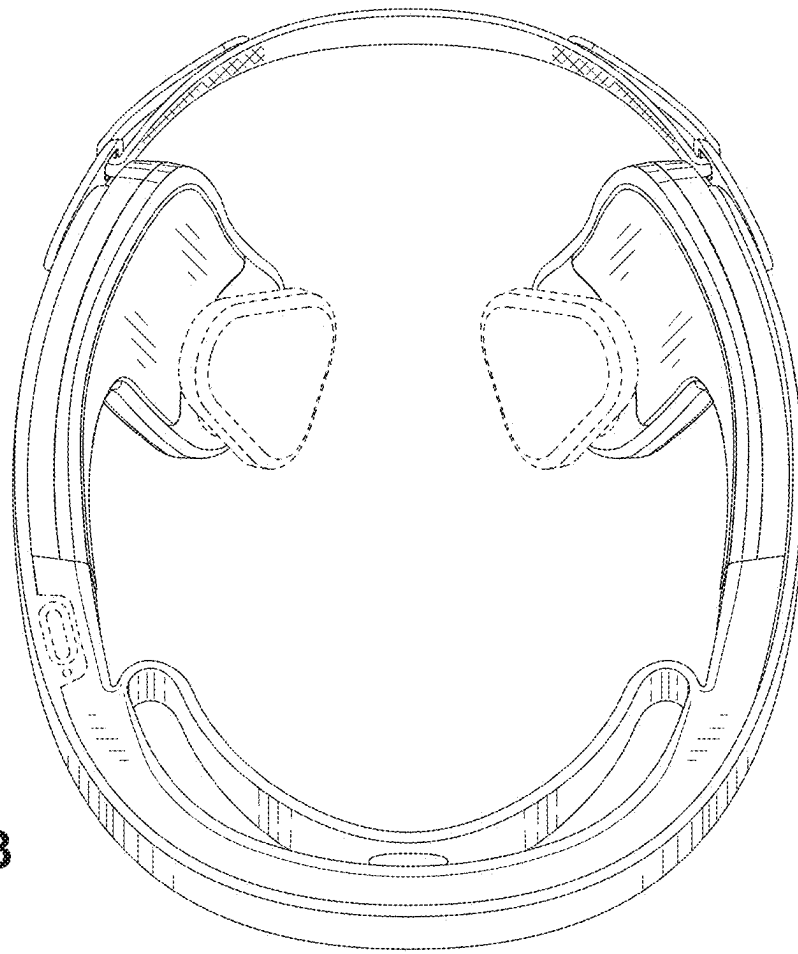


**FIG. 3**

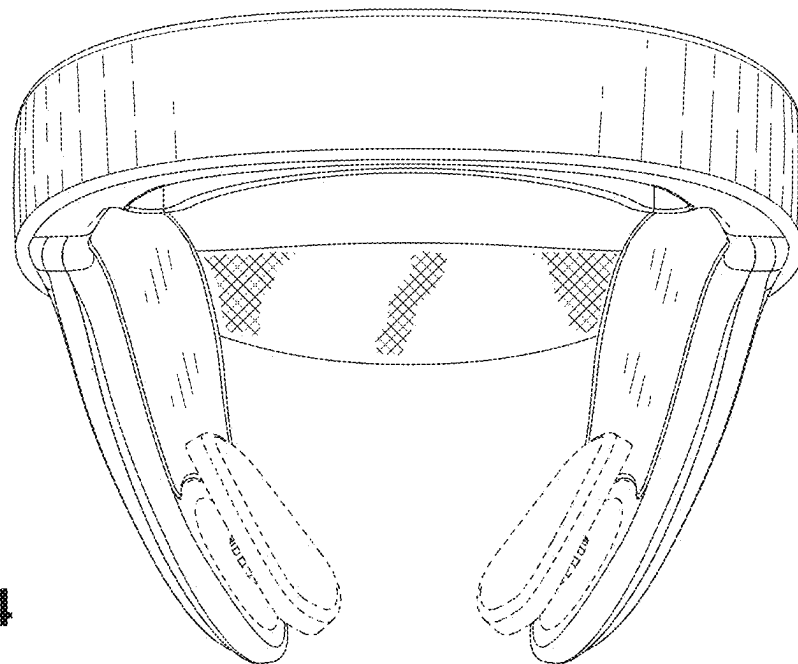


**FIG. 4**

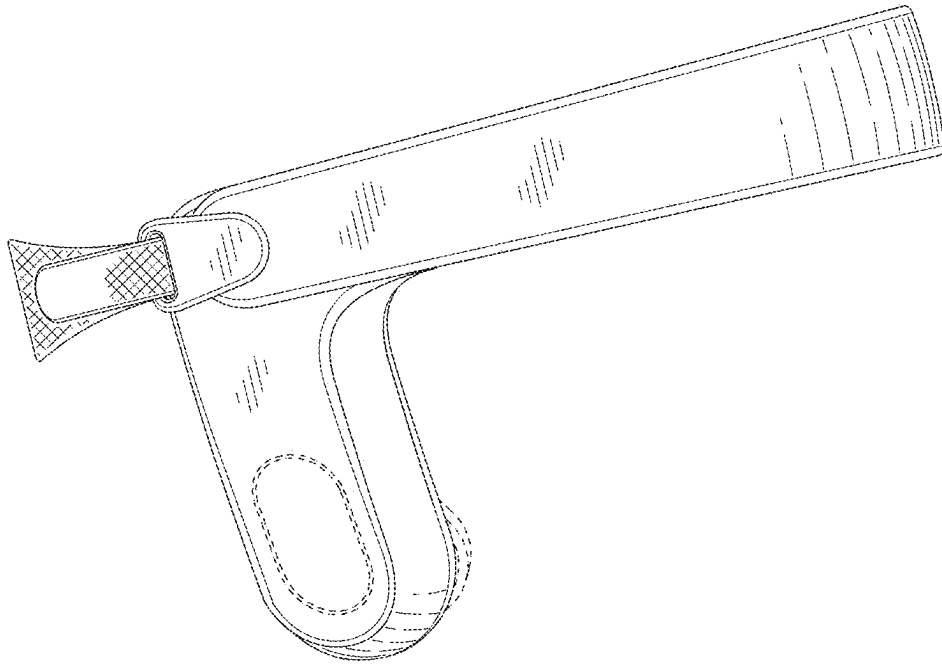


**FIG. 5**

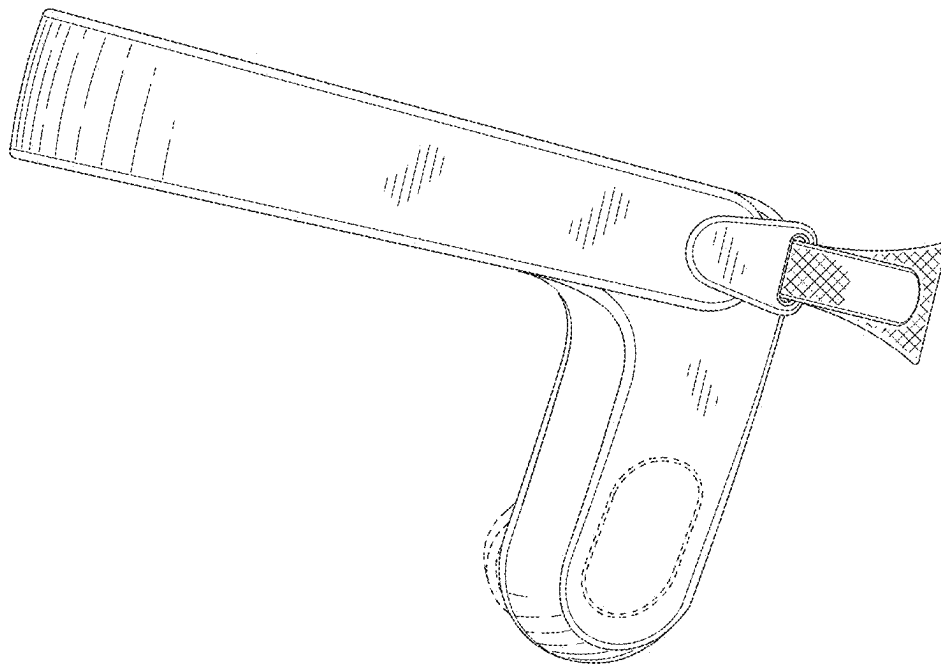

**FIG. 6**

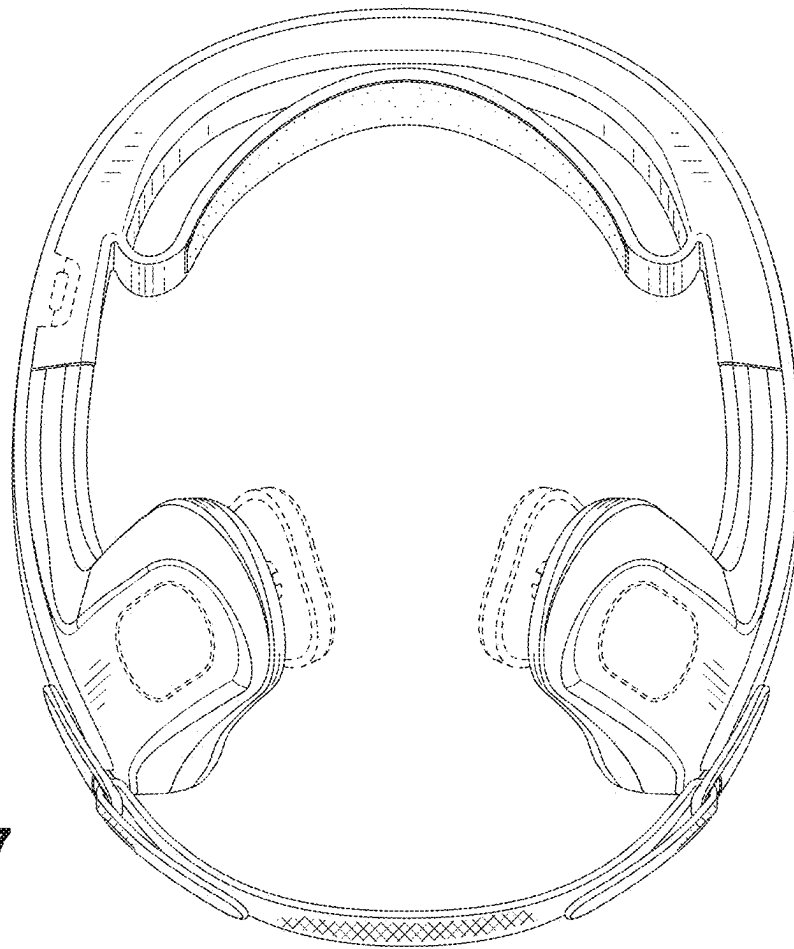

**FIG. 7**

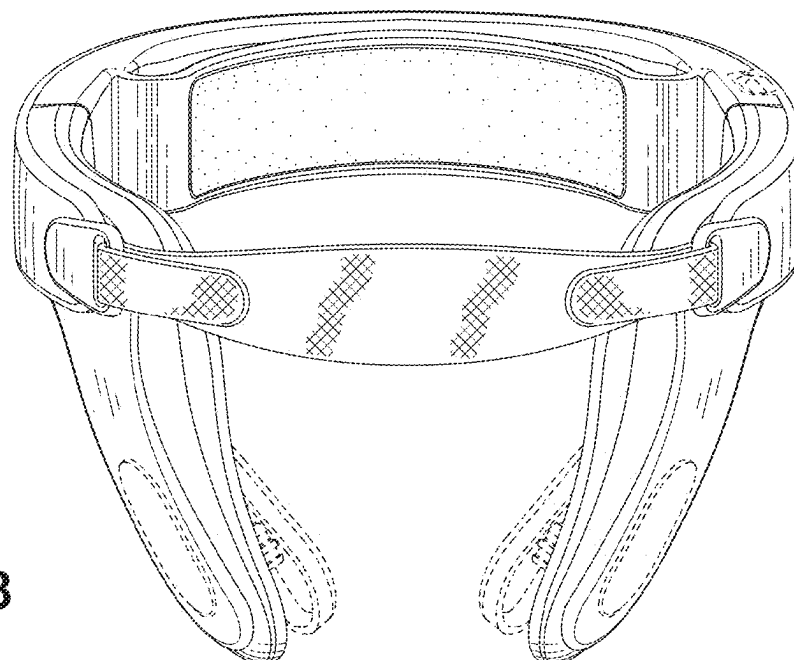

**FIG. 8**