



US0D1092774S

(12) **United States Design Patent**
Wu et al.

(10) **Patent No.: US D1,092,774 S**

(45) **Date of Patent: ** Sep. 9, 2025**

(54) **LIQUID SAMPLE TEST DEVICE**

(56) **References Cited**

(71) Applicant: **Hangzhou Biotest Biotech Co., LTD.**,
Hangzhou (CN)

U.S. PATENT DOCUMENTS

(72) Inventors: **Shujiang Wu**, Hangzhou (CN); **Qihui Zhao**, Hangzhou (CN); **Hui Geng**,
Hangzhou (CN); **Liang Hong**,
Hangzhou (CN)

4,943,522 A * 7/1990 Eisinger G01N 33/54388
436/514
D328,136 S * 7/1992 Hayakawa D24/225
D341,663 S * 11/1993 Coulter D24/224
5,384,264 A * 1/1995 Chen G01N 33/54366
436/805
D361,842 S * 8/1995 Nazareth D24/223
D369,868 S * 5/1996 Nazareth D24/224
D379,662 S * 6/1997 Pearson D24/223

(73) Assignee: **Hangzhou Biotest Biotech Co., LTD.**,
Hangzhou (CN)

(Continued)

(**) Term: **15 Years**

OTHER PUBLICATIONS

(21) Appl. No.: **29/992,609**

The Asahi Shimbun, "Test kit to detect COVID-19 and flu simultaneously to be sold soon", Dec. 6, 2022. Available from Internet.
URL: <https://www.asahi.com/ajw/articles/14785982> (Year: 2022).*

(22) Filed: **Mar. 10, 2025**

Related U.S. Application Data

(62) Division of application No. 29/880,233, filed on Jul. 19, 2023.

Primary Examiner — T Chase Nelson

Assistant Examiner — Kelly L Gross

(74) *Attorney, Agent, or Firm* — Muncy, Geissler, Olds & Lowe, P.C.

(30) **Foreign Application Priority Data**

Jun. 26, 2023 (CN) 202330393919.1

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/186, 216, 234, 108, 107, 225, 169,
D24/223; D10/71, 78, 81, 46, 75, 77, 70,
D10/106.2

CPC G01N 33/66; G01N 33/49; G01N 33/493;
G01N 21/01; G01N 21/75; A61B
5/14532; A61B 2560/0412; A61B
2560/0443; A61B 2560/0462; B01L
3/5027; B01L 3/50273; B01L 3/502738;
B01L 2300/0609; B01L 2300/0672; B01L
2300/0829; B01L 2200/025; B01L
2200/026; B01L 2200/028; B01L 2200/16

See application file for complete search history.


(57) **CLAIM**

The ornamental design for a liquid sample test device as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a liquid sample test device showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIG. 8 is another perspective view thereof.

1 Claim, 8 Drawing Sheets

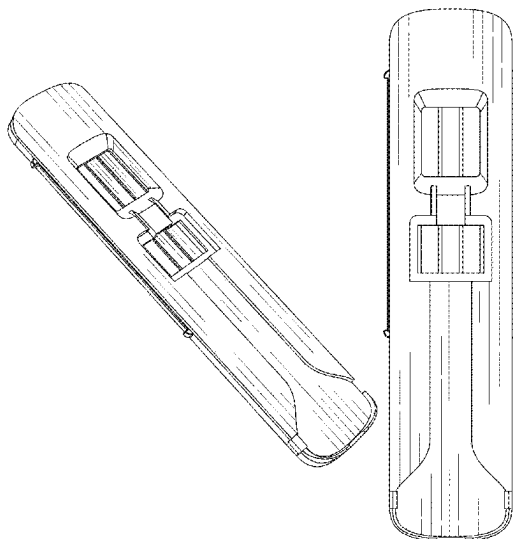

(56)

References Cited

U.S. PATENT DOCUMENTS

D429,527 S *	8/2000	Bolam	D24/169	D898,921 S *	10/2020	DaCosta	D24/186
D432,244 S *	10/2000	Anderson	D24/223	D899,604 S *	10/2020	DaCosta	D24/186
D456,082 S *	4/2002	Bouse	D24/223	D903,853 S *	12/2020	Wiegerinck	D24/107
D471,280 S *	3/2003	Jaeck	D24/169	D907,243 S *	1/2021	Sekiguchi	D24/225
D491,274 S *	6/2004	Dubniczki	D24/223	D910,871 S *	2/2021	Johnson	D24/224
D499,813 S *	12/2004	Wu	D24/223	D921,219 S *	6/2021	Johnson	D24/224
D500,142 S *	12/2004	Crisanti	D24/223	D928,980 S *	8/2021	Fang	D24/223
D509,901 S *	9/2005	Phelan	D24/186	D938,607 S *	12/2021	Lamble	D24/216
D512,512 S *	12/2005	Bell	D24/225	D952,860 S *	5/2022	Lin	D24/169
D523,964 S *	6/2006	Phelan	D24/186	D954,982 S *	6/2022	Ye	D24/223
D530,825 S *	10/2006	Lee	D24/223	D954,983 S *	6/2022	Ye	D24/223
D531,321 S *	10/2006	Godfrey	D24/225	D959,015 S *	7/2022	Fang	D24/223
D531,735 S *	11/2006	Lee	D24/223	D959,693 S *	8/2022	Lamble	D24/223
D536,798 S *	2/2007	Lee	D24/223	D977,673 S *	2/2023	Lei	D24/223
D557,815 S *	12/2007	Lee	D24/223	D980,449 S *	3/2023	Fang	D24/223
D576,737 S *	9/2008	Lee	D24/216	D983,402 S *	4/2023	Fang	D24/223
D590,063 S *	4/2009	Garthoff	D24/186	D983,403 S *	4/2023	Fang	D24/223
D606,664 S *	12/2009	Jacono	D24/225	D983,992 S *	4/2023	Buenning	G01N 33/56983
D631,556 S *	1/2011	Shi	D24/225				D24/223
D639,975 S *	6/2011	Doyle	D24/225	D990,704 S *	6/2023	Li	D24/223
D655,424 S *	3/2012	Castanon	D24/225	D999,931 S *	9/2023	Fang	D24/223
D660,977 S *	5/2012	Wagner	D24/223	D1,013,536 S *	2/2024	Hewitt	D24/223
D660,978 S *	5/2012	Wagner	D24/223	D1,013,537 S *	2/2024	Hewitt	D24/223
D663,845 S *	7/2012	Delaey	D24/169	D1,025,392 S *	4/2024	Cai	D24/223
D668,350 S *	10/2012	Rowley	D24/225	D1,028,278 S *	5/2024	Fang	D24/223
D676,570 S *	2/2013	Chance	D24/223	D1,032,873 S *	6/2024	Ling	D24/223
D742,524 S *	11/2015	Yao	D24/169	D1,035,906 S *	7/2024	Diller	D24/223
D765,264 S *	8/2016	Zin	D24/223	D1,040,369 S *	8/2024	Fang	D24/223
D772,428 S *	11/2016	Fumito	D24/225	D1,041,025 S *	9/2024	Fang	D24/223
D784,551 S *	4/2017	Todd	D24/224	D1,044,024 S *	9/2024	Fischl	D24/216
D791,952 S *	7/2017	Florescu	D24/186	D1,052,106 S *	11/2024	Lei	D24/223
D800,332 S *	10/2017	Snider	D24/223	D1,052,755 S *	11/2024	Lei	D24/223
D800,333 S *	10/2017	Snider	D24/223	D1,053,378 S *	12/2024	Lei	D24/223
D827,837 S *	9/2018	Pascal	D24/186	D1,053,379 S *	12/2024	Shen	D24/223
D834,721 S *	11/2018	Klein	D24/225	D1,054,036 S *	12/2024	Zenil	D24/186
D837,388 S *	1/2019	DaCosta	D24/186	D1,058,852 S *	1/2025	Numbers	D24/223
D837,998 S *	1/2019	Schaff	D24/219	2007/0092401 A1 *	4/2007	Liao	B01L 3/5023
D855,825 S *	8/2019	Parsons	D24/223				422/68.1
D859,684 S *	9/2019	Edwards	D24/223	2015/0064800 A1 *	3/2015	Chance	G01N 33/6854
D884,919 S *	5/2020	Parsons	D24/223				436/501
D894,422 S *	8/2020	Johnson	D24/224	2018/0164242 A1 *	6/2018	Virtanen	G01N 33/5438
D895,140 S *	9/2020	Heron	D24/225	2018/0356393 A1 *	12/2018	Piasio	G01N 27/3272
				2022/0323047 A1 *	10/2022	Berros	A61B 10/0096

* cited by examiner

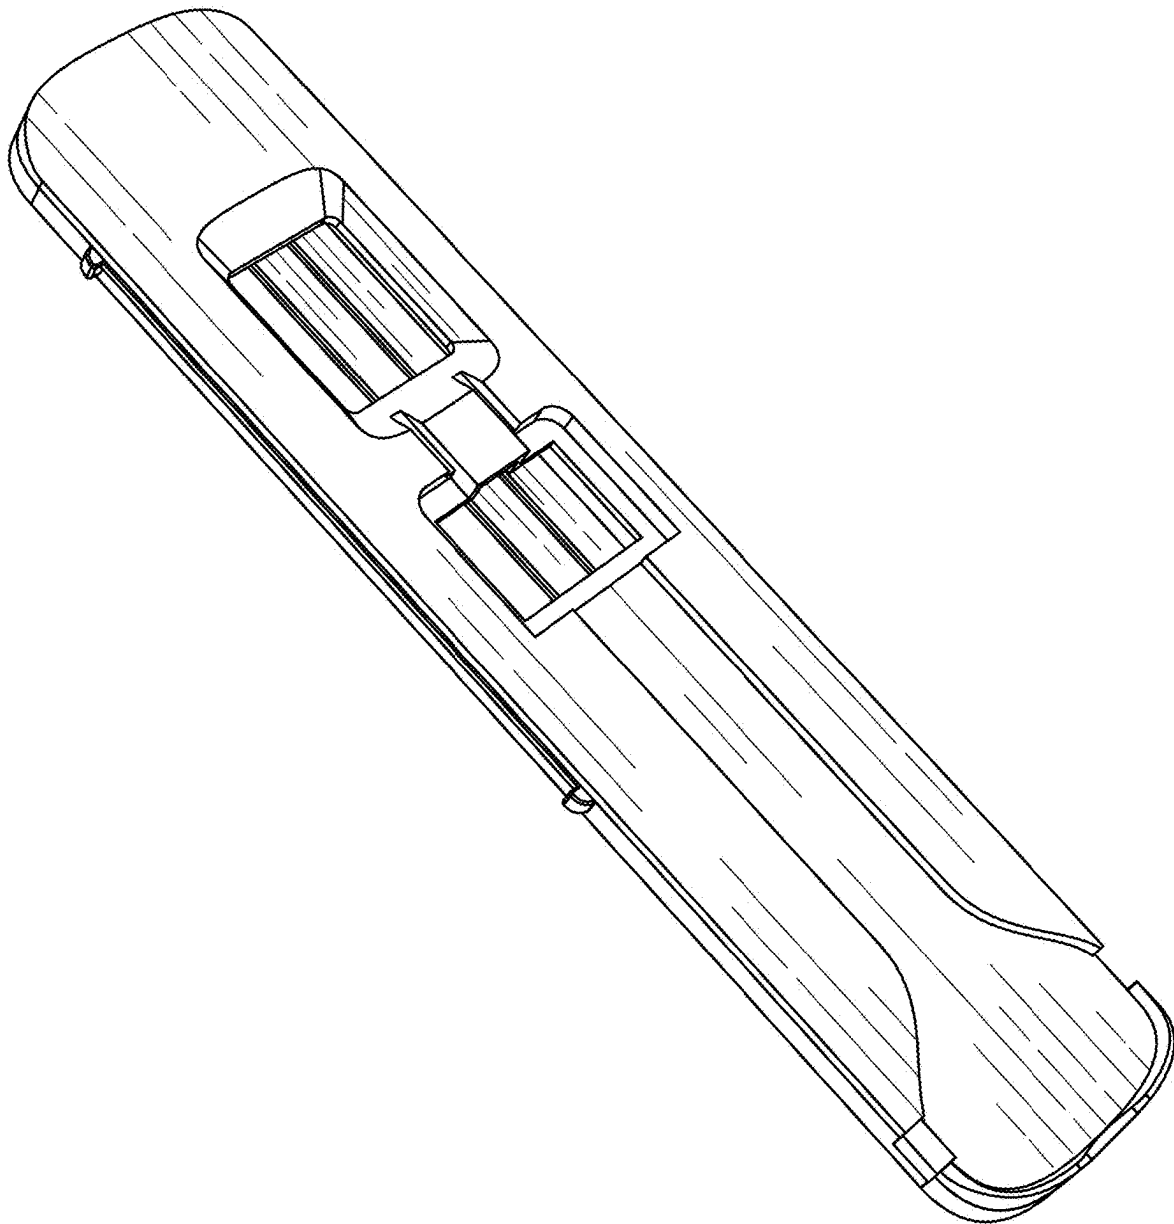


Fig.1

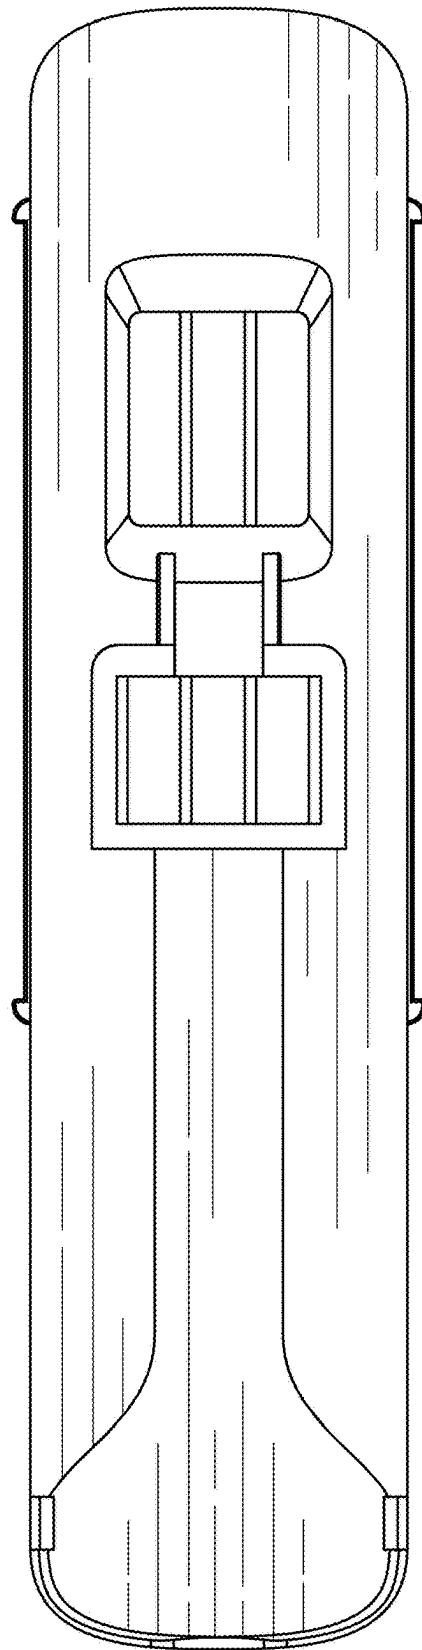


Fig.2

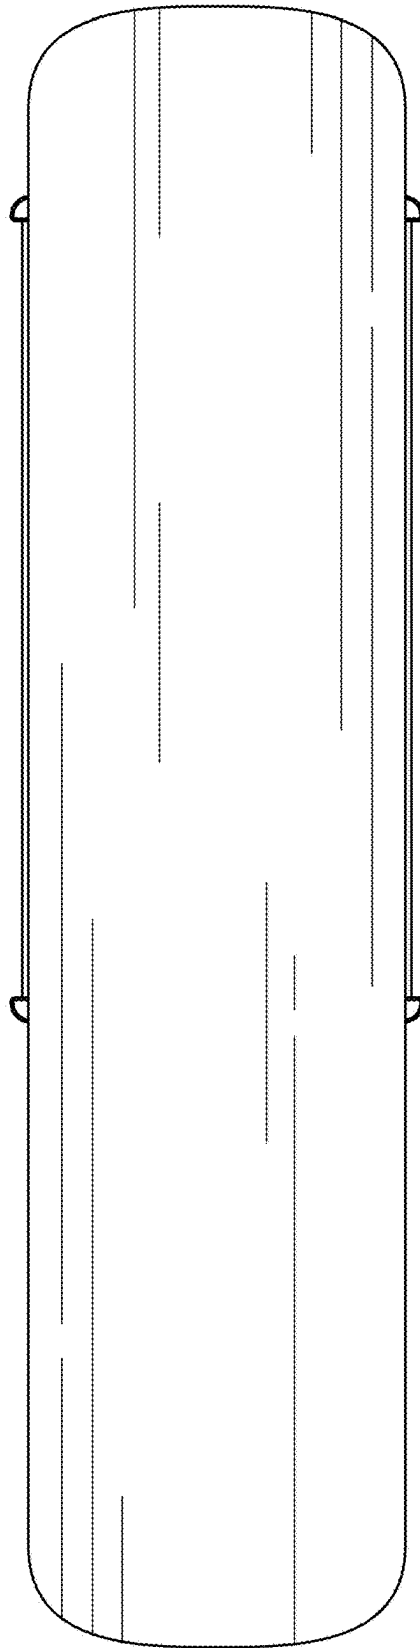


Fig.3



Fig.4




Fig.5




Fig.6




Fig.7

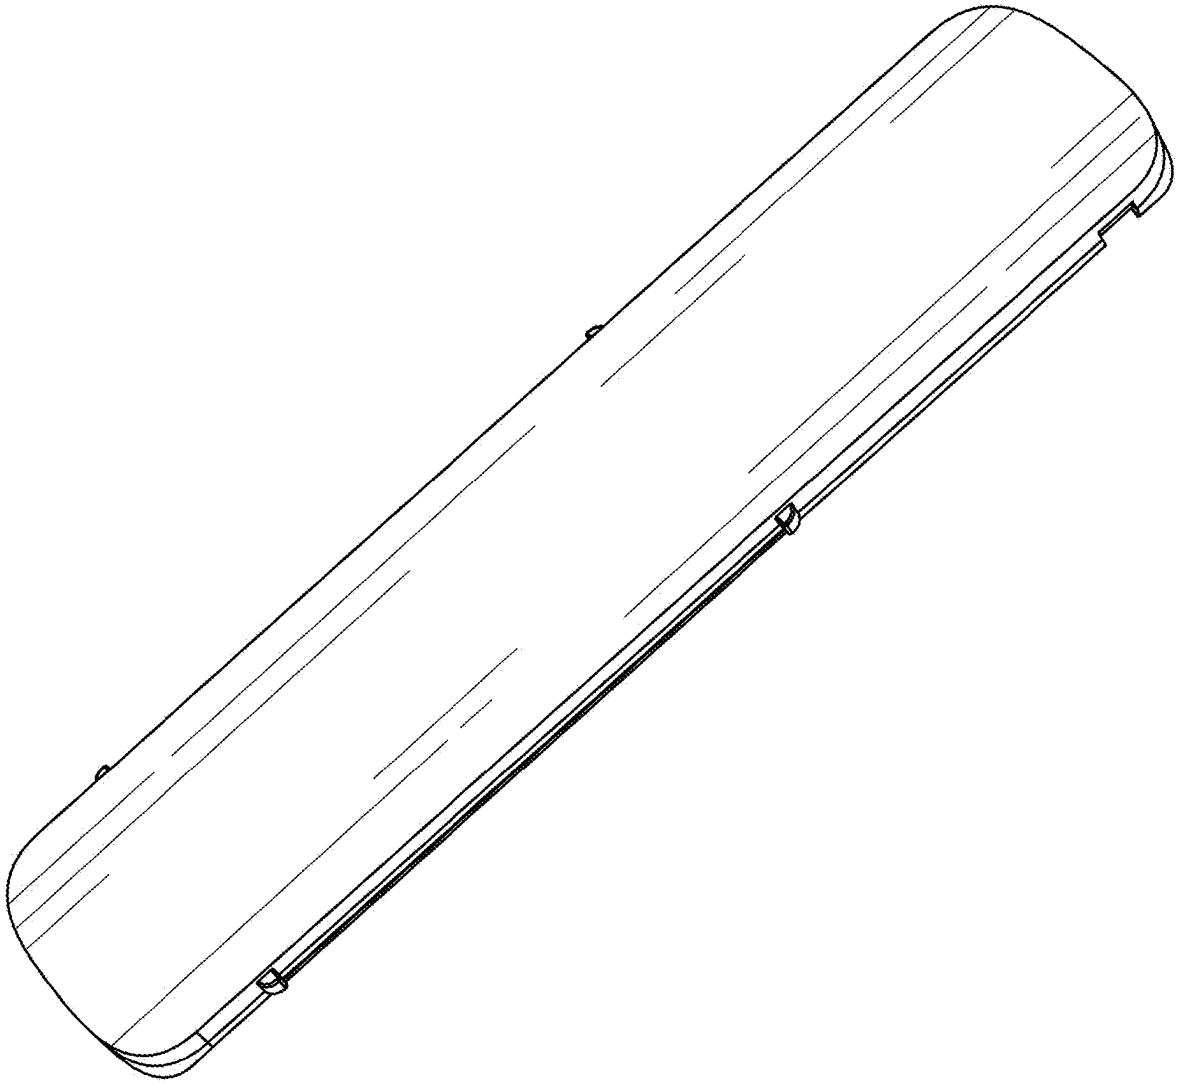


Fig.8