



US012402804B2

(12) **United States Patent**
Hacking et al.

(10) **Patent No.:** **US 12,402,804 B2**

(45) **Date of Patent:** **Sep. 2, 2025**

(54) **WEARABLE DEVICE FOR COUPLING TO A USER, AND MEASURING AND MONITORING USER ACTIVITY**

(71) Applicant: **ROM TECHNOLOGIES, INC.**, Las Vegas, NV (US)

(72) Inventors: **S. Adam Hacking**, Nashua, NH (US);
Sucheta Tamragouri, Nashua, NH (US); **Jeff Cote**, Raymond, NH (US);
Daniel Lipszyc, Glasgow, MT (US);
Mikael Taveras, Boston, MA (US)

(73) Assignee: **ROM Technologies, Inc.**, Brookfield, CT (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 551 days.

(21) Appl. No.: **17/017,062**

(22) Filed: **Sep. 10, 2020**

(65) **Prior Publication Data**

US 2021/0076981 A1 Mar. 18, 2021

Related U.S. Application Data

(60) Provisional application No. 62/991,295, filed on Mar. 18, 2020, provisional application No. 62/911,515, (Continued)

(51) **Int. Cl.**
A61B 5/107 (2006.01)
A61B 5/00 (2006.01)
A61B 5/11 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 5/1071** (2013.01); **A61B 5/1121** (2013.01); **A61B 5/6801** (2013.01); **A61B 2562/166** (2013.01)

(58) **Field of Classification Search**
CPC ... **A61B 5/1071**; **A61B 5/1121**; **A61B 5/6801**;
A61B 5/4585; **A61B 5/742**;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

59,915 A 11/1866 Lalletment
363,522 A 5/1887 Knous
(Continued)

FOREIGN PATENT DOCUMENTS

CA 2698078 A1 3/2010
CA 3193419 A1 3/2022
(Continued)

OTHER PUBLICATIONS

International Searching Authority, Search Report and Written Opinion for International Application No. PCT/US2021/038617, Date of Mailing Oct. 15, 2021, 12 pages.

(Continued)

Primary Examiner — Jennifer Robertson


Assistant Examiner — Nidhi N Patel

(74) *Attorney, Agent, or Firm* — Dickinson Wright PLLC; Jonathan H. Harder; Stephen A. Mason

(57) **ABSTRACT**

A system for measuring an angle of a joint of a user includes a center hub, a first arm, a second arm, a magnet, and a sensor. The center hub includes a first hub and a second hub. The first arm is configured for attachment to a first limb portion of the user at a first outer end and to the first hub at a first inner end. The second arm is configured for attachment to a second limb portion of the user at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub. The magnet is coupled to the second hub. The sensor is disposed in the center hub and configured to detect a rotation of the magnet.

5 Claims, 29 Drawing Sheets

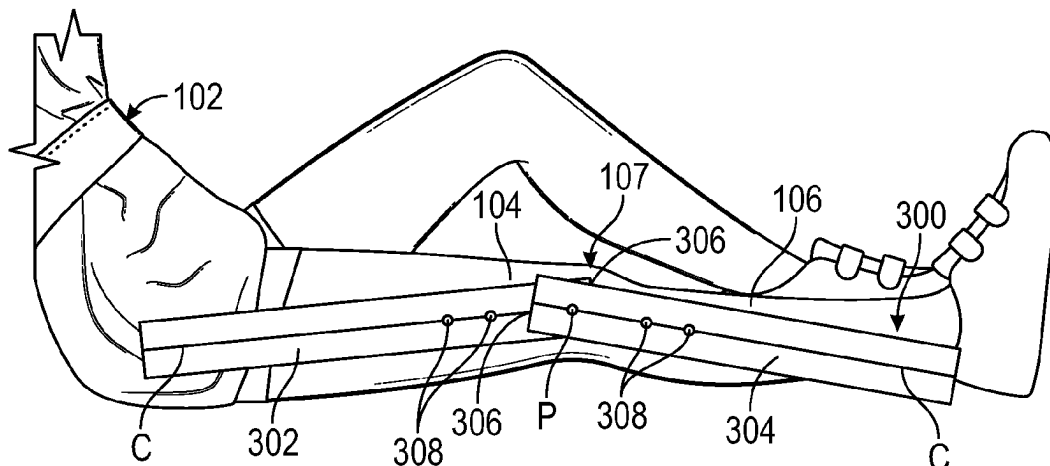

Related U.S. Application Data

filed on Oct. 7, 2019, provisional application No. 62/904,013, filed on Sep. 23, 2019, provisional application No. 62/901,464, filed on Sep. 17, 2019, provisional application No. 62/901,411, filed on Sep. 17, 2019.

(58) Field of Classification Search

CPC ... A61B 5/4528; A61B 5/6842; A61B 5/6828;
A61B 5/6833; A61B 2562/166; A61B
2562/0233; A61B 2562/164; A61B
2560/0223

See application file for complete search history.

(56) References Cited**U.S. PATENT DOCUMENTS**

446,671 A 2/1891 Elliott
610,157 A 8/1898 Campbell
631,276 A 8/1899 Bulova
823,712 A 6/1906 Uhlmann
1,149,029 A 8/1915 Clark
1,227,743 A 5/1917 Burgedorfp
1,784,230 A 12/1930 Freeman
3,081,645 A 3/1963 Bergfors
3,100,640 A 8/1963 Weitzel
3,137,014 A 6/1964 Meucci
3,143,316 A 8/1964 Shapiro
3,713,438 A 1/1973 Knutsen
3,744,480 A 7/1973 Gause et al.
3,888,136 A 6/1975 Lapeyre
4,079,957 A 3/1978 Blease
4,408,613 A 10/1983 Relyea
4,436,097 A 3/1984 Cunningham
4,446,753 A 5/1984 Nagano
4,477,072 A 10/1984 DeCloux
4,499,900 A 2/1985 Petrofsky et al.
4,509,742 A 4/1985 Cones
4,606,241 A 8/1986 Fredriksson
4,611,807 A 9/1986 Castillo
4,616,823 A 10/1986 Yang
4,648,287 A 3/1987 Preskitt
4,673,178 A 6/1987 Dwight
4,824,104 A 4/1989 Bloch
4,850,245 A 7/1989 Feamster et al.
4,858,942 A 8/1989 Rodriguez
4,869,497 A 9/1989 Stewart et al.
4,915,374 A 4/1990 Watkins
4,930,768 A 6/1990 Lapcevic
4,961,570 A 10/1990 Chang
5,161,430 A 11/1992 Febey
5,202,794 A 4/1993 Schnee et al.
5,247,853 A 9/1993 Dalebout
5,282,748 A 2/1994 Little
5,316,532 A 5/1994 Butler
5,318,487 A 6/1994 Golen
5,324,241 A 6/1994 Artigues et al.
5,336,147 A 8/1994 Sweeney, III
5,338,272 A 8/1994 Sweeney, III
5,356,356 A 10/1994 Hildebrandt
5,361,649 A 11/1994 Slocum, Jr.
D359,777 S 6/1995 Hildebrandt
5,458,022 A 10/1995 Mattfeld et al.
5,487,713 A 1/1996 Butler
5,566,589 A 10/1996 Buck
5,580,338 A 12/1996 Scelta et al.
5,676,349 A 10/1997 Wilson
5,685,804 A 11/1997 Whan-Tong et al.
5,860,941 A 1/1999 Saringer et al.
5,950,813 A 9/1999 Hoskins et al.
6,007,459 A 12/1999 Burgess
D421,075 S 2/2000 Hildebrandt
6,053,847 A 4/2000 Stearns et al.
6,077,201 A 6/2000 Cheng
6,102,834 A 8/2000 Chen
6,155,958 A 12/2000 Goldberg

6,162,189 A 12/2000 Girone et al.
6,182,029 B1 1/2001 Friedman
6,253,638 B1 7/2001 Bermudez
6,371,891 B1 4/2002 Speas
6,413,190 B1 7/2002 Wood et al.
6,430,436 B1 8/2002 Richter
6,450,923 B1 9/2002 Vatti
6,474,193 B1 11/2002 Farney
6,491,649 B1 12/2002 Ombrellaro
6,514,085 B2 2/2003 Slattery et al.
6,543,309 B2 4/2003 Heim
6,589,139 B1 7/2003 Butterworth
6,601,016 B1 7/2003 Brown et al.
6,613,000 B1 9/2003 Reinkensmeyer et al.
6,626,800 B1 9/2003 Casler
6,640,122 B2* 10/2003 Manoli A61B 5/6804
607/139
6,640,662 B1 11/2003 Baxter
6,820,517 B1 11/2004 Farney
6,865,969 B2 3/2005 Stevens
6,890,312 B1 5/2005 Priester et al.
6,895,834 B1 5/2005 Baatz
6,902,513 B1 6/2005 McClure
7,058,453 B2 6/2006 Nelson et al.
7,063,643 B2 6/2006 Arai
7,169,085 B1 1/2007 Killin et al.
7,204,788 B2 4/2007 Andrews
7,209,886 B2 4/2007 Kimmel
7,226,394 B2 6/2007 Johnson
7,594,879 B2 9/2009 Johnson
7,628,730 B1 12/2009 Watterson et al.
D610,635 S 2/2010 Hildebrandt
7,815,551 B2 10/2010 Merli
7,969,315 B1 6/2011 Ross et al.
7,974,689 B2 7/2011 Volpe et al.
8,012,107 B2 9/2011 Einav et al.
8,021,270 B2 9/2011 D'Eredita
8,038,578 B2 10/2011 Olrik et al.
8,113,991 B2 2/2012 Kutliroff
8,177,732 B2 5/2012 Einav et al.
8,298,123 B2 10/2012 Hickman
8,371,990 B2 2/2013 Shea
8,515,777 B1 8/2013 Rajasenan
8,607,465 B1* 12/2013 Edwards G01B 3/56
33/471
8,751,264 B2 6/2014 Beraja et al.
8,823,448 B1 9/2014 Shen
8,845,493 B2 9/2014 Watterson et al.
8,849,681 B2 9/2014 Hargrove et al.
8,893,287 B2 11/2014 Gjonej et al.
8,911,327 B1 12/2014 Boyette
9,004,598 B2 4/2015 Weber
9,311,789 B1 4/2016 Gwin
9,312,907 B2 4/2016 Auchinleck et al.
9,474,935 B2 10/2016 Abbondanza et al.
9,480,873 B2 11/2016 Chuang
9,514,277 B2 12/2016 Hassing et al.
9,629,558 B2 4/2017 Yuen et al.
9,640,057 B1 5/2017 Ross
9,707,147 B2 7/2017 Levital et al.
D794,142 S 8/2017 Zhou
9,757,612 B2 9/2017 Weber
9,802,081 B2 10/2017 Ridgel et al.
9,813,239 B2 11/2017 Chee et al.
9,827,445 B2 11/2017 Marcos et al.
9,849,337 B2 12/2017 Roman et al.
9,868,028 B2 1/2018 Shin
9,919,198 B2 3/2018 Romeo et al.
9,939,784 B1 4/2018 Berardinelli
9,977,587 B2 5/2018 Mountain
9,993,181 B2 6/2018 Ross
10,004,946 B2 6/2018 Ross
D826,349 S 8/2018 Oblamski
10,055,550 B2 8/2018 Goetz
10,058,473 B2 8/2018 Oshima et al.
10,089,443 B2 10/2018 Miller et al.
10,111,643 B2 10/2018 Shulhauser et al.
10,130,298 B2 11/2018 Mokaya et al.
10,137,328 B2 11/2018 Baudhuin

References Cited

2005/0020411	A1	1/2005	Andrews	
2005/0085346	A1	4/2005	Johnson	
2005/0085353	A1	4/2005	Johnson	
2005/0115561	A1	6/2005	Stahmann	
2005/0274220	A1	12/2005	Reboullet	
2006/0003871	A1	1/2006	Houghton	
2006/0058648	A1	3/2006	Meier	
2006/0064136	A1	3/2006	Wang	
2006/0064329	A1	3/2006	Abolfathi et al.	
2006/0247095	A1	11/2006	Rummerfield	
2007/0118389	A1	5/2007	Shipon	
2007/0184414	A1	8/2007	Perez	
2007/0194939	A1	8/2007	Alvarez et al.	
2007/0219059	A1	9/2007	Schwartz	
2008/0082356	A1	4/2008	Friedlander et al.	
2008/0161166	A1	7/2008	Lo	
2008/0161733	A1	7/2008	Einav et al.	
2008/0221485	A1*	9/2008	Lissek	A61B 5/1071 600/595
2008/0281633	A1	11/2008	Burdea et al.	
2009/0011907	A1	1/2009	Radow et al.	
2009/0058635	A1	3/2009	LaLonde et al.	
2009/0070138	A1	3/2009	Langheier et al.	
2009/0211395	A1	8/2009	Mul'e	
2009/0287503	A1	11/2009	Angell et al.	
2009/0299766	A1	12/2009	Friedlander et al.	
2010/0076786	A1	3/2010	Dalton et al.	
2010/0121160	A1	5/2010	Stark et al.	
2010/0216168	A1	8/2010	Heinzman et al.	
2010/0248905	A1	9/2010	Lu	
2010/0268304	A1	10/2010	Matos	
2010/0326207	A1	12/2010	Topel	
2011/0010188	A1	1/2011	Yoshikawa et al.	
2011/0119212	A1	5/2011	De Bruin et al.	
2011/0172059	A1	7/2011	Watterson et al.	
2011/0218814	A1	9/2011	Coats	
2011/0306846	A1	12/2011	Osorio	
2012/0041771	A1	2/2012	Cosentino et al.	
2012/0065987	A1	3/2012	Farooq et al.	
2012/0167709	A1	7/2012	Chen et al.	
2012/0190502	A1	7/2012	Paulus et al.	
2012/0259648	A1	10/2012	Mallon et al.	
2012/0296455	A1	11/2012	Ohnemus et al.	
2012/0310667	A1	12/2012	Altman et al.	
2013/0123667	A1	5/2013	Komatireddy et al.	
2013/0211281	A1	8/2013	Ross et al.	
2013/0253943	A1	9/2013	Lee et al.	
2013/0274069	A1	10/2013	Watterson et al.	
2013/0296987	A1	11/2013	Rogers et al.	
2013/0332616	A1	12/2013	Landwehr	
2014/0006042	A1	1/2014	Keefe et al.	
2014/0089836	A1	3/2014	Damani et al.	
2014/0113261	A1	4/2014	Akiba	
2014/0172442	A1	6/2014	Broderick	
2014/0188009	A1	7/2014	Lange et al.	
2014/0194250	A1	7/2014	Reich et al.	
2014/0228649	A1	8/2014	Rayner et al.	
2014/0246499	A1	9/2014	Proud et al.	
2014/0257837	A1	9/2014	Walker et al.	
2014/0303540	A1	10/2014	Baym	
2014/0315689	A1	10/2014	Vauquelin et al.	
2014/0322686	A1	10/2014	Kang	
2014/0371816	A1	12/2014	Matos	
2015/0025816	A1	1/2015	Ross	
2015/0073814	A1	3/2015	Linebaugh	
2015/0088544	A1	3/2015	Goldberg	
2015/0099458	A1	4/2015	Weisner et al.	
2015/0099952	A1	4/2015	Lain et al.	
2015/0112230	A1	4/2015	Iglesias	
2015/0130830	A1	5/2015	Nagasaki	
2015/0141200	A1	5/2015	Murray et al.	
2015/0149217	A1	5/2015	Kaburagi	
2015/0161331	A1	6/2015	Oleynik	
2015/0196805	A1	7/2015	Koduri	
2015/0257679	A1	9/2015	Ross	
2015/0265209	A1	9/2015	Zhang	
2015/0339442	A1	11/2015	Oleynik	
2015/0351664	A1	12/2015	Ross	
2015/0351665	A1	12/2015	Ross	

(56)	References Cited						
U.S. PATENT DOCUMENTS							
2015/0379430	A1	12/2015	Dirac et al.	2018/0318122	A1	11/2018	LeCursi et al.
2016/0023081	A1	1/2016	Popa-Simil	2018/0330810	A1	11/2018	Garnarnik
2016/0045170	A1	2/2016	Migita	2018/0330824	A1	11/2018	Athey et al.
2016/0096073	A1	4/2016	Rahman et al.	2018/0353812	A1	12/2018	Lannon et al.
2016/0140319	A1	5/2016	Stark	2019/0009135	A1	1/2019	Wu
2016/0143593	A1	5/2016	Fu et al.	2019/0019163	A1	1/2019	Batey et al.
2016/0166833	A1	6/2016	Bum	2019/0019573	A1	1/2019	Lake et al.
2016/0166881	A1	6/2016	Ridgel et al.	2019/0019578	A1	1/2019	Vaccaro
2016/0193306	A1	7/2016	Rabovsky et al.	2019/0046794	A1	2/2019	Goodall et al.
2016/0213924	A1	7/2016	Coleman	2019/0060708	A1	2/2019	Fung
2016/0275259	A1	9/2016	Nolan et al.	2019/0065970	A1	2/2019	Bonutti et al.
2016/0287166	A1	10/2016	Tran	2019/0066832	A1	2/2019	Kang et al.
2016/0302721	A1	10/2016	Wiedenhoefer et al.	2019/0080802	A1	3/2019	Ziobro et al.
2016/0322078	A1	11/2016	Bose et al.	2019/0090744	A1	3/2019	Mahfouz
2016/0354636	A1	12/2016	Jang	2019/0117128	A1 *	4/2019	Chen A61B 5/1121
2016/0373477	A1	12/2016	Moyle	2019/0118038	A1	4/2019	Tana et al.
2017/0004260	A1	1/2017	Moturu et al.	2019/0126099	A1	5/2019	Hoang
2017/0095692	A1	4/2017	Chang et al.	2019/0134454	A1	5/2019	Mahoney et al.
2017/0095693	A1	4/2017	Chang et al.	2019/0167988	A1	6/2019	Shahriari et al.
2017/0100637	A1	4/2017	Princen et al.	2019/0200920	A1	7/2019	Tien et al.
2017/0113092	A1	4/2017	Johnson	2019/0209891	A1	7/2019	Fung
2017/0132947	A1	5/2017	Maeda et al.	2019/0223797	A1	7/2019	Tran
2017/0136296	A1	5/2017	Barrera et al.	2019/0228856	A1	7/2019	Leifer
2017/0143261	A1	5/2017	Wiedenhoefer et al.	2019/0244540	A1	8/2019	Errante et al.
2017/0147752	A1	5/2017	Toru	2019/0251456	A1	8/2019	Constantin
2017/0147789	A1	5/2017	Wiedenhoefer et al.	2019/0262084	A1	8/2019	Roh
2017/0148297	A1	5/2017	Ross	2019/0269343	A1	9/2019	Ramos Murguialday et al.
2017/0181698	A1	6/2017	Wiedenhoefer et al.	2019/0314681	A1	10/2019	Yang
2017/0202724	A1	7/2017	De Rossi	2019/0344123	A1	11/2019	Rubin et al.
2017/0220751	A1	8/2017	Davis	2019/0362242	A1	11/2019	Pillai et al.
2017/0235882	A1	8/2017	Orlov et al.	2020/0034665	A1	1/2020	Ghanta
2017/0235906	A1	8/2017	Dorris et al.	2020/0038703	A1	2/2020	Cleary et al.
2017/0243028	A1	8/2017	LaFever et al.	2020/0143922	A1	5/2020	Chekroud et al.
2017/0262604	A1	9/2017	Francois	2020/0151595	A1	5/2020	Jayalath et al.
2017/0265800	A1	9/2017	Auchinleck et al.	2020/0152339	A1	5/2020	Pulitzer et al.
2017/0270260	A1	9/2017	Shetty	2020/0160198	A1	5/2020	Reeves et al.
2017/0278209	A1	9/2017	Olsen et al.	2020/0170876	A1	6/2020	Kapure et al.
2017/0281390	A1 *	10/2017	Abdul-Hafiz A61F 5/013	2020/0176098	A1	6/2020	Lucas et al.
2017/0282015	A1	10/2017	Wicks et al.	2020/0237291	A1	7/2020	Raja
2017/0283508	A1	10/2017	Demopulos et al.	2020/0275886	A1	9/2020	Mason
2017/0286621	A1	10/2017	Cox	2020/0289045	A1	9/2020	Hacking et al.
2017/0300654	A1	10/2017	Stein et al.	2020/0289046	A1	9/2020	Hacking et al.
2017/0304024	A1	10/2017	Nobrega	2020/0289879	A1	9/2020	Hacking et al.
2017/0312614	A1	11/2017	Tran et al.	2020/0289880	A1	9/2020	Hacking et al.
2017/0323481	A1	11/2017	Tran et al.	2020/0289881	A1	9/2020	Hacking et al.
2017/0329917	A1	11/2017	McRaith et al.	2020/0289889	A1	9/2020	Hacking et al.
2017/0329933	A1	11/2017	Brust	2020/0293712	A1	9/2020	Potts et al.
2017/0344726	A1	11/2017	Duffy et al.	2020/0303063	A1	9/2020	Sharma et al.
2017/0347923	A1	12/2017	Roh	2020/0365256	A1	11/2020	Hayashitani et al.
2017/0360586	A1	12/2017	Dempers et al.	2020/0401224	A1	12/2020	Cotton
2017/0368413	A1	12/2017	Shavit	2020/0410385	A1	12/2020	Otsuki
2018/0052962	A1	2/2018	Van Der Koijk et al.	2020/0411162	A1	12/2020	Lien et al.
2018/0056104	A1	3/2018	Cromie et al.	2021/0005224	A1	1/2021	Rothschild et al.
2018/0060494	A1	3/2018	Dias et al.	2021/0005319	A1	1/2021	Otsuki et al.
2018/0071565	A1	3/2018	Gomberg et al.	2021/0008413	A1	1/2021	Asikainen et al.
2018/0071566	A1	3/2018	Gomberg et al.	2021/0077860	A1	3/2021	Posnack et al.
2018/0071569	A1	3/2018	Gomberg et al.	2021/0101051	A1	4/2021	Posnack et al.
2018/0071570	A1	3/2018	Gomberg et al.	2021/0113890	A1	4/2021	Posnack et al.
2018/0071571	A1	3/2018	Gomberg et al.	2021/0127974	A1	5/2021	Mason et al.
2018/0071572	A1	3/2018	Gomberg et al.	2021/0128080	A1	5/2021	Mason et al.
2018/0078843	A1	3/2018	Tran et al.	2021/0128255	A1	5/2021	Mason et al.
2018/0102190	A1	4/2018	Hogue et al.	2021/0134412	A1	5/2021	Guaneri et al.
2018/0116741	A1 *	5/2018	Garcia Kilroy G01L 3/1428	2021/0134425	A1	5/2021	Mason et al.
2018/0140927	A1	5/2018	Kito	2021/0134428	A1	5/2021	Mason
2018/0146870	A1	5/2018	Shemesh	2021/0134430	A1	5/2021	Mason et al.
2018/0177612	A1	6/2018	Trabish et al.	2021/0134432	A1	5/2021	Mason et al.
2018/0220935	A1	8/2018	Tadano et al.	2021/0134456	A1	5/2021	Posnack et al.
2018/0240552	A1	8/2018	Tuyl et al.	2021/0134457	A1	5/2021	Mason et al.
2018/0263530	A1	9/2018	Jung	2021/0134458	A1	5/2021	Mason et al.
2018/0263535	A1	9/2018	Cramer	2021/0134463	A1	5/2021	Mason et al.
2018/0263552	A1	9/2018	Graman et al.	2021/0138304	A1	5/2021	Mason et al.
2018/0271432	A1	9/2018	Auchinleck et al.	2021/0142875	A1	5/2021	Mason et al.
2018/0280784	A1	10/2018	Romeo et al.	2021/0142893	A1	5/2021	Guaneri et al.
2018/0290017	A1	10/2018	Fung	2021/0142898	A1	5/2021	Mason et al.
2018/0296143	A1	10/2018	Anderson et al.	2021/0142903	A1	5/2021	Mason et al.
				2021/0144074	A1	5/2021	Guaneri et al.
				2021/0244998	A1	8/2021	Hacking et al.
				2021/0251562	A1	8/2021	Jain
				2021/0272677	A1	9/2021	Barbee

(56)

References Cited

U.S. PATENT DOCUMENTS

2021/0338469 A1 11/2021 Dempers
 2021/0343384 A1 11/2021 Purushothaman et al.
 2021/0345879 A1 11/2021 Mason et al.
 2021/0345975 A1 11/2021 Mason et al.
 2021/0350888 A1 11/2021 Guaneri et al.
 2021/0350898 A1 11/2021 Mason et al.
 2021/0350899 A1 11/2021 Mason et al.
 2021/0350901 A1 11/2021 Mason et al.
 2021/0350902 A1 11/2021 Mason et al.
 2021/0350914 A1 11/2021 Guaneri et al.
 2021/0350926 A1 11/2021 Mason et al.
 2021/0361514 A1 11/2021 Choi et al.
 2021/0366587 A1 11/2021 Mason et al.
 2021/0383909 A1 12/2021 Mason et al.
 2021/0391091 A1 12/2021 Mason
 2021/0398668 A1 12/2021 Chock et al.
 2021/0407670 A1 12/2021 Mason et al.
 2021/0407681 A1 12/2021 Mason et al.
 2022/0000556 A1 1/2022 Casey et al.
 2022/0015838 A1 1/2022 Posnack
 2022/0016480 A1 1/2022 Bissonnette et al.
 2022/0016482 A1 1/2022 Bissonnette
 2022/0016485 A1 1/2022 Bissonnette et al.
 2022/0016486 A1 1/2022 Bissonnette
 2022/0020469 A1 1/2022 Tanner
 2022/0044806 A1 2/2022 Sanders et al.
 2022/0047921 A1 2/2022 Bissonnette
 2022/0080265 A1 3/2022 Watterson
 2022/0105390 A1 4/2022 Yuasa
 2022/0118218 A1 4/2022 Bense et al.
 2022/0133576 A1 5/2022 Choi et al.
 2022/0176039 A1 6/2022 Intereur et al.
 2022/0181004 A1 6/2022 Zilca et al.
 2022/0193491 A1 6/2022 Mason
 2022/0238223 A1 7/2022 Mason
 2022/0262504 A1 8/2022 Bratty et al.
 2022/0273985 A1 9/2022 Jeong et al.
 2022/0300787 A1 9/2022 Wall et al.
 2022/0304881 A1 9/2022 Choi et al.
 2022/0304882 A1 9/2022 Choi
 2022/0305328 A1 9/2022 Choi et al.
 2022/0323826 A1 10/2022 Khurana
 2022/0327714 A1 10/2022 Cook et al.
 2022/0327807 A1 10/2022 Cook et al.
 2022/0330823 A1 10/2022 Janssen
 2022/0338761 A1 10/2022 Maddahi et al.
 2022/0339052 A1 10/2022 Kim
 2022/0395232 A1 12/2022 Locke
 2022/0401783 A1 12/2022 Choi
 2023/0001268 A1 1/2023 Bissonnette et al.
 2023/0029639 A1 2/2023 Roy
 2023/0119461 A1 4/2023 Mason
 2023/0190100 A1 6/2023 Stump
 2023/0197240 A1 6/2023 Rosenberg
 2023/0201656 A1 6/2023 Hacking et al.
 2023/0207097 A1 6/2023 Mason
 2023/0207124 A1 6/2023 Walsh et al.
 2023/0215539 A1 7/2023 Rosenberg et al.
 2023/0215552 A1 7/2023 Khotilovich et al.
 2023/0245747 A1 8/2023 Rosenberg et al.
 2023/0245748 A1 8/2023 Rosenberg et al.
 2023/0245750 A1 8/2023 Rosenberg et al.
 2023/0245751 A1 8/2023 Rosenberg et al.
 2023/0253089 A1 8/2023 Rosenberg et al.
 2023/0255555 A1 8/2023 Sundaram et al.
 2023/0263428 A1 8/2023 Hull et al.
 2023/0274813 A1 8/2023 Rosenberg et al.
 2023/0282329 A1 9/2023 Mason et al.
 2023/0364472 A1 11/2023 Posnack
 2023/0368886 A1 11/2023 Rosenberg
 2023/0377711 A1 11/2023 Rosenberg
 2023/0377712 A1 11/2023 Rosenberg
 2023/0386639 A1 11/2023 Rosenberg
 2023/0395231 A1 12/2023 Rosenberg

2023/0395232 A1 12/2023 Rosenberg
 2024/0029856 A1 1/2024 Rosenberg
 2024/0203580 A1 6/2024 Mason

FOREIGN PATENT DOCUMENTS

CN 2885238 Y 4/2007
 CN 101964151 A 2/2011
 CN 201889024 U 7/2011
 CN 102670381 A 9/2012
 CN 103263336 A 8/2013
 CN 103390357 A 11/2013
 CN 103473631 A 12/2013
 CN 103501328 A 1/2014
 CN 103721343 A 4/2014
 CN 203677851 U 7/2014
 CN 103136447 B 8/2016
 CN 205626871 U 10/2016
 CN 106236502 A 12/2016
 CN 106621195 A 5/2017
 CN 107551475 A 1/2018
 CN 107930021 A 4/2018
 CN 207220817 U 4/2018
 CN 208224811 A 12/2018
 CN 109191954 A 1/2019
 CN 109363887 A 2/2019
 CN 110201358 A 9/2019
 CN 110322957 A 10/2019
 CN 110808092 A 2/2020
 CN 110931103 A 3/2020
 CN 110993057 A 4/2020
 CN 111111110 A 5/2020
 CN 111460305 A 7/2020
 CN 112071393 A 12/2020
 CN 212141371 U 12/2020
 CN 112289425 A 1/2021
 CN 212624809 U 2/2021
 CN 112603295 A 4/2021
 CN 213190965 U 5/2021
 CN 113384850 A 9/2021
 CN 113499572 A 10/2021
 CN 215136488 U 12/2021
 CN 113885361 A 1/2022
 CN 114049961 A 2/2022
 CN 114203274 A 3/2022
 CN 216258145 U 4/2022
 CN 114694824 A 7/2022
 CN 114898832 A 8/2022
 CN 114983760 A 9/2022
 CN 217472652 U 9/2022
 CN 110270062 B 10/2022
 CN 218420859 U 2/2023
 CN 115954081 A 4/2023
 DE 4330269 A1 3/1995
 EP 1159989 A1 12/2001
 EP 1968028 9/2008
 EP 1909730 B1 4/2014
 EP 2815242 A4 12/2014
 EP 2869805 A 5/2015
 EP 2997951 A1 3/2016
 EP 2688472 B1 4/2016
 EP 3264303 A1 1/2018
 EP 3984508 A1 4/2022
 EP 3984509 A1 4/2022
 EP 3984510 A1 4/2022
 EP 3984511 A1 4/2022
 EP 3984512 A1 4/2022
 EP 3984513 A1 4/2022
 EP 4054699 A1 9/2022
 EP 4112033 A1 1/2023
 FR 3127393 A1 3/2023
 GB 2591542 B 3/2022
 IN 201811043670 A 7/2018
 JP 2000005339 A 1/2000
 JP 2005227928 A 8/2005
 JP 2005227928 A1 8/2005
 JP 2009011517 A 1/2009
 JP 2009112336 A 5/2009
 JP 3193662 U 10/2014

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP 5804063 B2 11/2015
 JP 2018102842 A 7/2018
 JP 2019028647 A 2/2019
 JP 6871379 B2 5/2021
 JP 2022521378 A 4/2022
 JP 3238491 U 7/2022
 JP 7198364 B2 12/2022
 JP 7202474 B2 1/2023
 JP 7231750 B2 3/2023
 JP 7231751 B2 3/2023
 JP 7231752 B2 3/2023
 KR 200276919 Y1 5/2002
 KR 100582596 B1 5/2006
 KR 101042258 B1 6/2011
 KR 20110099953 A 9/2011
 KR 101258250 B1 4/2013
 KR 101325581 B1 11/2013
 KR 20140128630 A 11/2014
 KR 20150078191 A 7/2015
 KR 101580071 B1 12/2015
 KR 101647620 B1 8/2016
 KR 20180004928 A 1/2018
 KR 20190029175 A 3/2019
 KR 101988167 B1 6/2019
 KR 101969392 B1 8/2019
 KR 102055279 B1 12/2019
 KR 102088333 B1 3/2020
 KR 20200029180 A 3/2020
 KR 102097190 B1 4/2020
 KR 102121586 B1 6/2020
 KR 20200119665 A 10/2020
 KR 102246049 B1 4/2021
 KR 102246050 B1 4/2021
 KR 102246051 B1 4/2021
 KR 102246052 B1 4/2021
 KR 102352602 B1 1/2022
 KR 102352603 B1 1/2022
 KR 102352604 B1 1/2022
 KR 20220004639 A 1/2022
 KR 102387577 B1 4/2022
 KR 102421437 B1 7/2022
 KR 20220102207 A 7/2022
 KR 102427545 B1 8/2022
 KR 102467495 B1 11/2022
 KR 102467496 B1 11/2022
 KR 102469723 B1 11/2022
 KR 102471990 B1 11/2022
 KR 20220145989 A 11/2022
 KR 20220156134 A 11/2022
 KR 102502744 B1 2/2023
 KR 20230019349 A 2/2023
 KR 20230019350 A 2/2023
 KR 20230026556 A 2/2023
 KR 20230026668 A 2/2023
 KR 20230040526 3/2023
 KR 20230050506 A 4/2023
 KR 20230056118 A 4/2023
 KR 102528503 B1 5/2023
 KR 102531930 B1 5/2023
 KR 102532766 B1 5/2023
 KR 102539190 B1 6/2023
 RU 2014131288 A 2/2016
 RU 2607953 C2 1/2017
 TW M474545 U 3/2014
 TW M638437 U 3/2023
 WO 2001056465 A1 8/2001
 WO 02093312 A2 11/2002
 WO 2005018453 A1 3/2005
 WO 2007102709 A1 9/2007
 WO 2011025322 A2 3/2011
 WO 2012128801 A1 9/2012
 WO 2013002568 A2 1/2013
 WO 2023164292 A1 3/2013
 WO 2013122839 A1 8/2013
 WO 2014011447 A1 1/2014

WO 2015026744 A1 2/2015
 WO 2015065298 A1 5/2015
 WO 2015082555 A1 6/2015
 WO 2017030781 A1 2/2017
 WO 2017091691 A1 6/2017
 WO 2017165238 A1 9/2017
 WO 2018081795 A1 5/2018
 WO 2019204876 A1 4/2019
 WO 2019143940 A1 7/2019
 WO 2020185769 A1 3/2020
 WO 2020256577 A1 12/2020
 WO 2021055427 A1 3/2021
 WO 2021055491 A1 3/2021
 WO 2021081094 A1 4/2021
 WO 2021090267 A1 5/2021
 WO 2021216881 A1 10/2021
 WO 2021236542 A1 11/2021
 WO 2021236961 A1 11/2021
 WO 2021262809 A1 12/2021
 WO 2022047006 A1 3/2022
 WO 2022092493 A1 5/2022
 WO 2022092494 A1 5/2022
 WO 2022212883 A1 10/2022
 WO 2022212921 A1 10/2022
 WO 2023008680 A1 2/2023
 WO 2023008681 A1 2/2023
 WO 2023022319 A1 2/2023
 WO 2023022320 A1 2/2023
 WO 2023052695 A1 4/2023
 WO 2023091496 A1 5/2023
 WO 2023215155 A1 11/2023
 WO 2023230075 A1 11/2023
 WO 2024107807 A1 5/2024

OTHER PUBLICATIONS

Claris Healthcare Inc.; Claris Reflex Patient Rehabilitation System Brochure, <https://clarisreflex.com/>, retrieved from internet on Oct. 2, 2019; 5 pages.

International Search Report and Written Opinion for PCT/US2023/014137, dated Jun. 9, 2023, 13 pages.

Website for "Esino 2022 Physical Therapy Equipments Arm Fitness Indoor Trainer Leg Spin Cycle Machine Exercise Bike for Elderly," <https://www.made-in-china.com/showroom/esinogroup/product-detailYdZtwGhCMKVR/China-Esino-2022-Physical-Therapy-Equipments-Arm-Fitness-Indoor-Trainer-Leg-Spin-Cycle-Machine-Exercise-Bike-for-Elderly.html>, retrieved on Aug. 29, 2023, 5 pages.

Abedtash, "An Interoperable Electronic Medical Record-Based Platform For Personalized Predictive Analytics", ProQuest LLC, Jul. 2017, 185 pages.

Alcaraz et al., "Machine Learning as Digital Therapy Assessment for Mobile Gait Rehabilitation," 2018 IEEE 28th International Workshop on Machine Learning for Signal Processing (MLSP), Aalborg, Denmark, 2018, 6 pages.

Androutsou et al., "A Smartphone Application Designed to Engage the Elderly in Home-Based Rehabilitation," Frontiers in Digital Health, Sep. 2020, vol. 2, Article 15, 13 pages.

Silva et al., "SapoFitness: A mobile health application for dietary evaluation," 2011 IEEE 13th International Conference on U e-Health Networking, Applications and Services, Columbia, MO, USA, 2011, 6 pages.

Wang et al., "Interactive wearable systems for upper body rehabilitation: a systematic review," Journal of NeuroEngineering and Rehabilitation, 2017, 21 pages.

Marzolini et al., "Eligibility, Enrollment, and Completion of Exercise-Based Cardiac Rehabilitation Following Stroke Rehabilitation: What Are the Barriers?," Physical Therapy, vol. 100, No. 1, 2019, 13 pages.

Nijjar et al., "Randomized Trial of Mindfulness-Based Stress Reduction in Cardiac Patients Eligible for Cardiac Rehabilitation," Scientific Reports, 2019, 12 pages.

Lara et al., "Human-Robot Sensor Interface for Cardiac Rehabilitation," IEEE International Conference on Rehabilitation Robotics, Jul. 2017, 8 pages.

(56)

References Cited

OTHER PUBLICATIONS

Ishraque et al., "Artificial Intelligence-Based Rehabilitation Therapy Exercise Recommendation System," 2018 IEEE MIT Undergraduate Research Technology Conference (URTC), Cambridge, MA, USA, 2018, 5 pages.

Zakari et al., "Are There Limitations to Exercise Benefits in Peripheral Arterial Disease?," *Frontiers in Cardiovascular Medicine*, Nov. 2018, vol. 5, Article 173, 12 pages.

You et al., "Including Blood Vasculature into a Game-Theoretic Model of Cancer Dynamics," *Games* 2019, 10, 13, 22 pages.

Jeong et al., "Computer-assisted upper extremity training using interactive biking exercise (iBike) platform," Sep. 2012, 34th Annual International Conference of the IEEE EMBS, 5 pages.

Gerbild et al., "Physical Activity to Improve Erectile Dysfunction: A Systematic Review of Intervention Studies," *Sexual Medicine*, 2018, 15 pages.

Chrif et al., "Control design for a lower-limb paediatric therapy device using linear motor technology," Article, 2017, pp. 119-127, Science Direct, Switzerland.

Robben et al., "Delta Features From Ambient Sensor Data are Good Predictors of Change in Functional Health," Article, 2016, pp. 2168-2194, vol. 21, No. 4, *IEEE Journal of Biomedical and Health Informatics*.

Kantoch et al., "Recognition of Sedentary Behavior by Machine Learning Analysis of Wearable Sensors during Activities of Daily Living for Telemedical Assessment of Cardiovascular Risk," Article, 2018, 17 pages, *Sensors*, Poland.

Warburton et al., "International Launch of the PAR-•Q+ and ePARmed-•X+ Validation of the PAR-•Q+ and ePARmed-•X+," *Health & Fitness Journal of Canada*, 2011, 9 pages, vol. 4, No. 2.

* cited by examiner

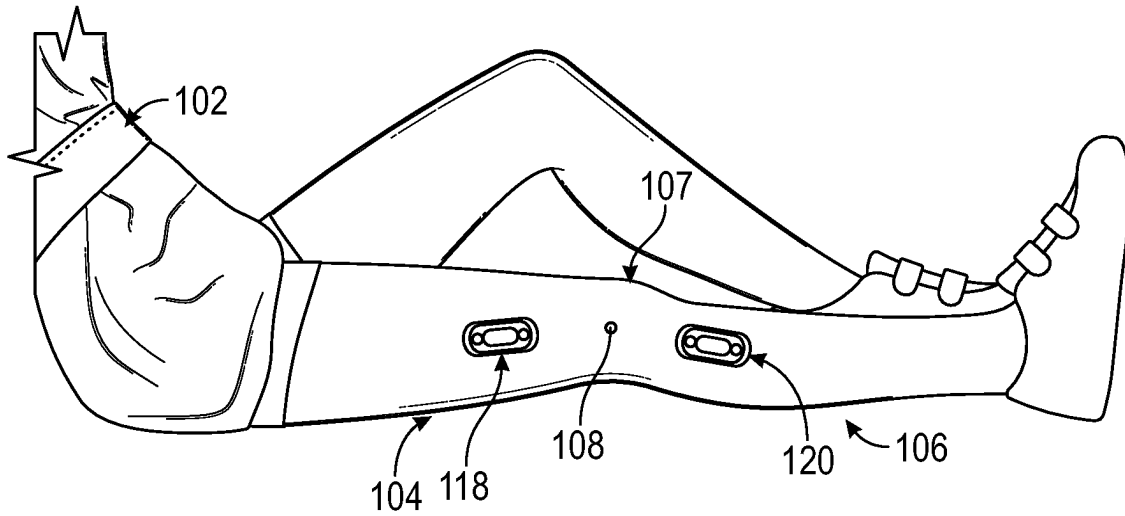


FIG. 1A

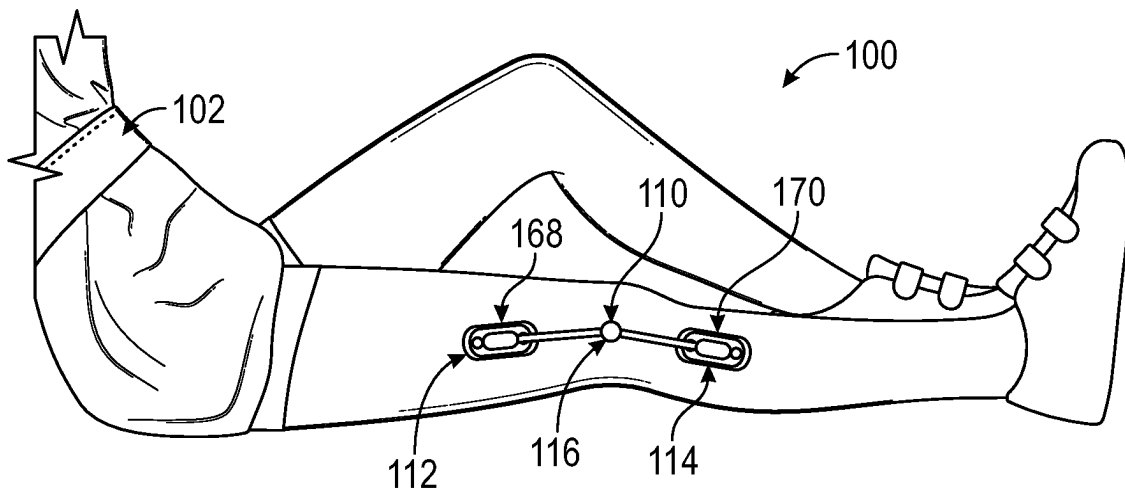


FIG. 1B

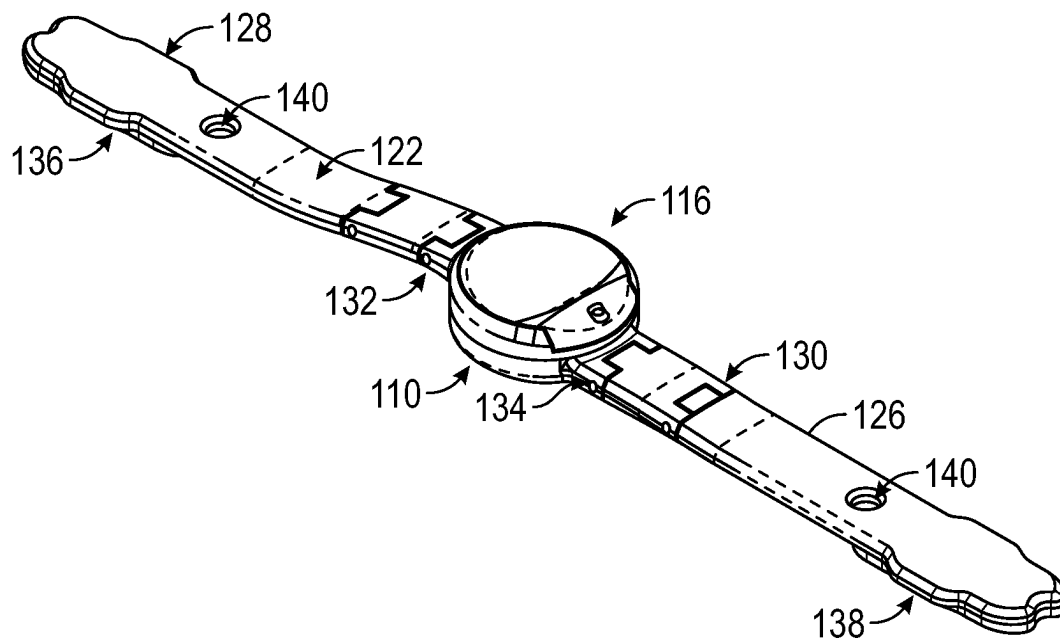


FIG. 2A

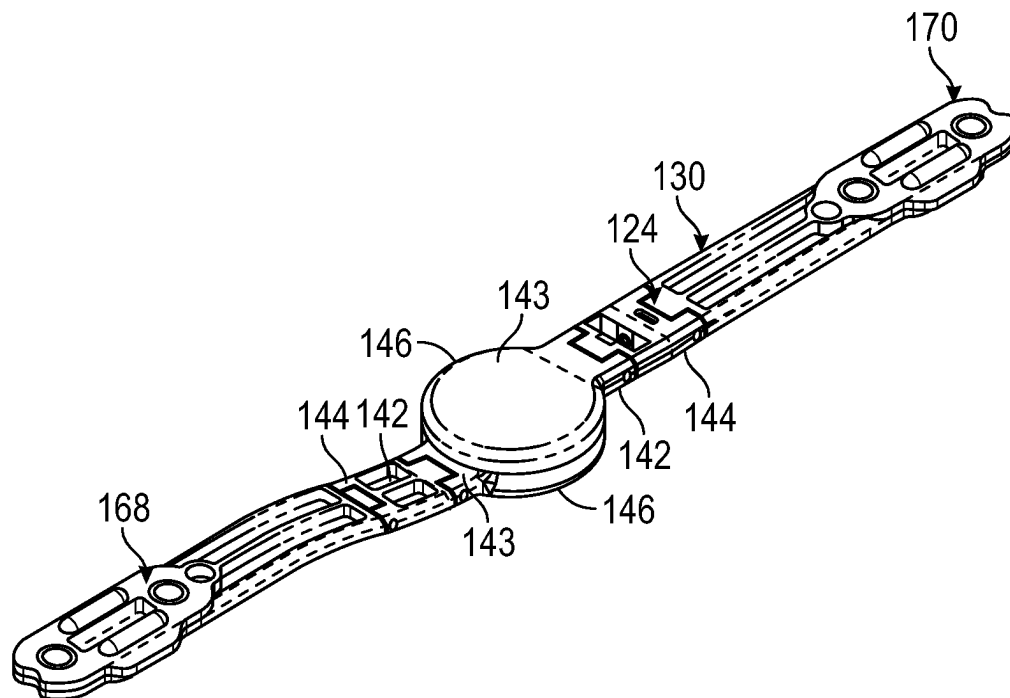


FIG. 2B

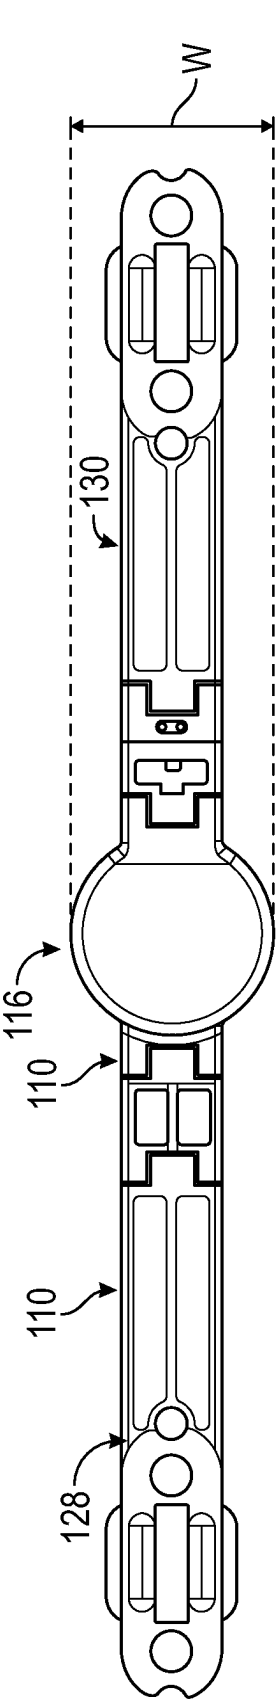


FIG. 3A

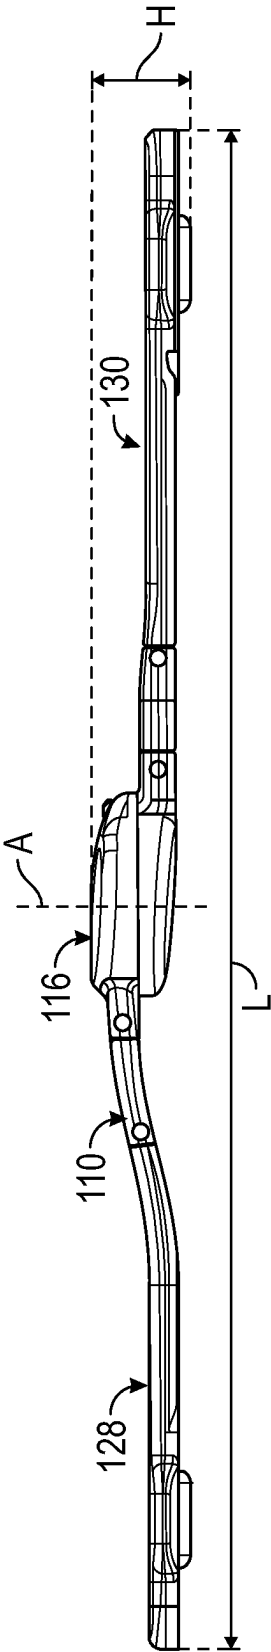


FIG. 3B

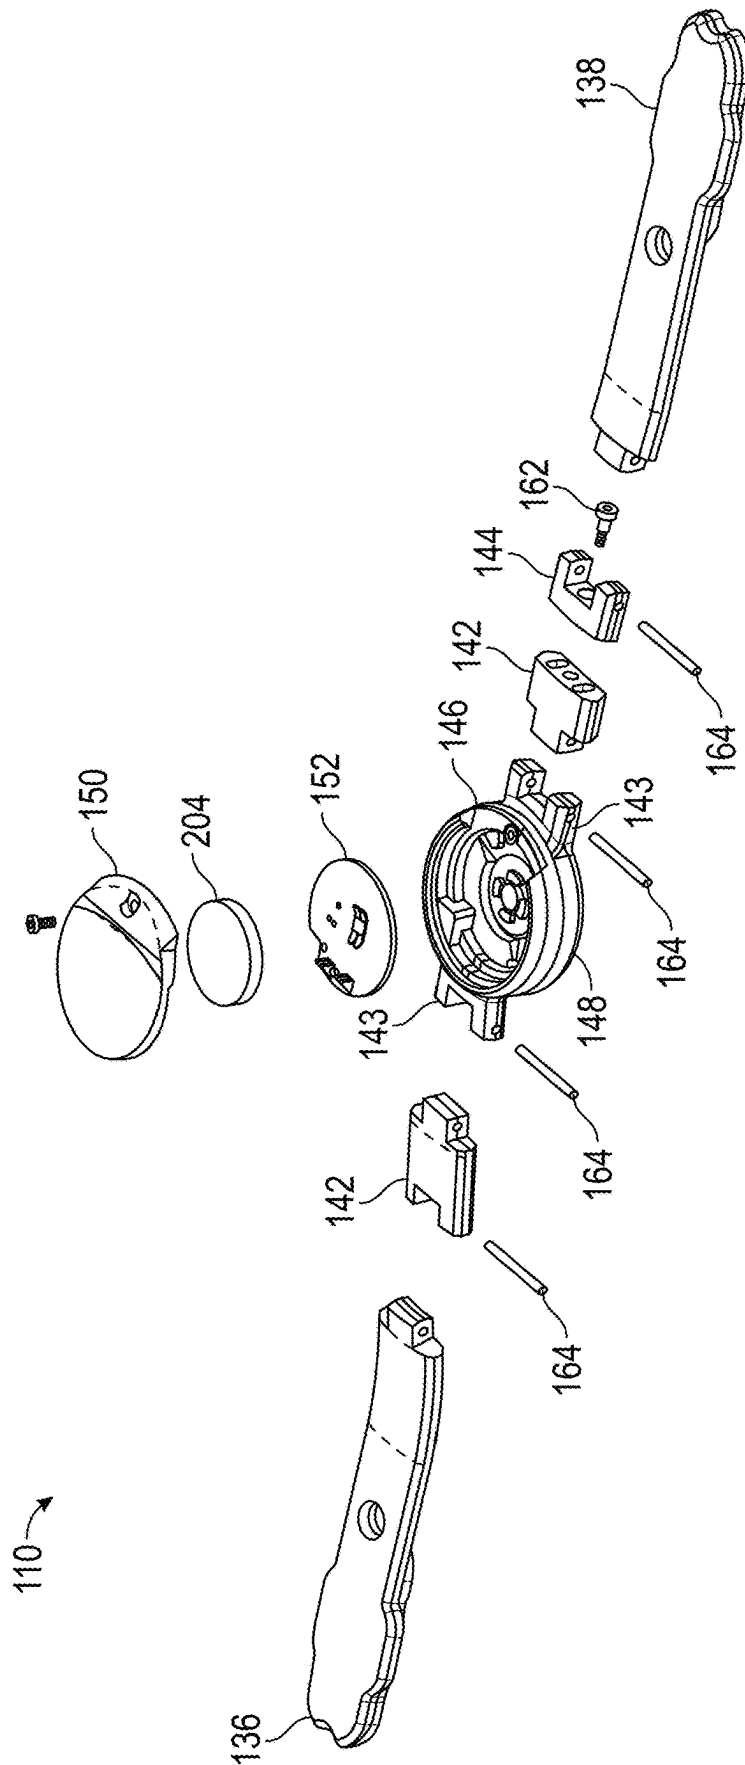


FIG. 4

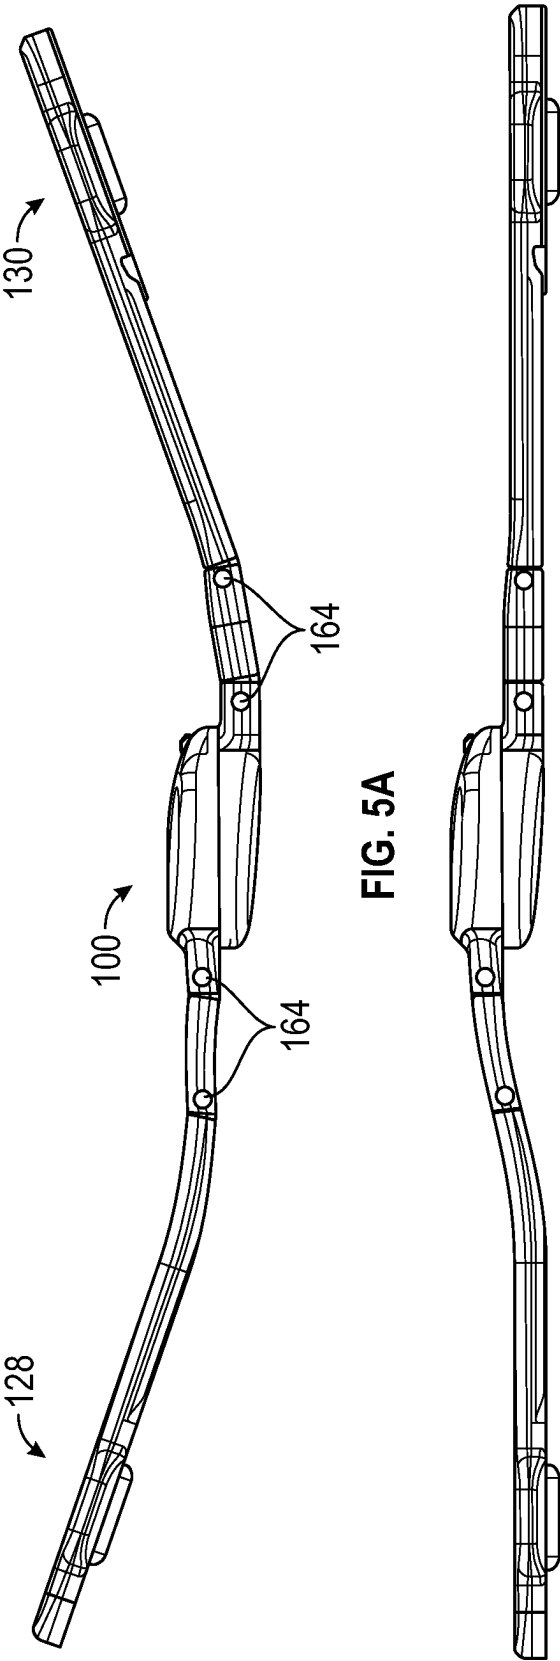


FIG. 5A



FIG. 5B

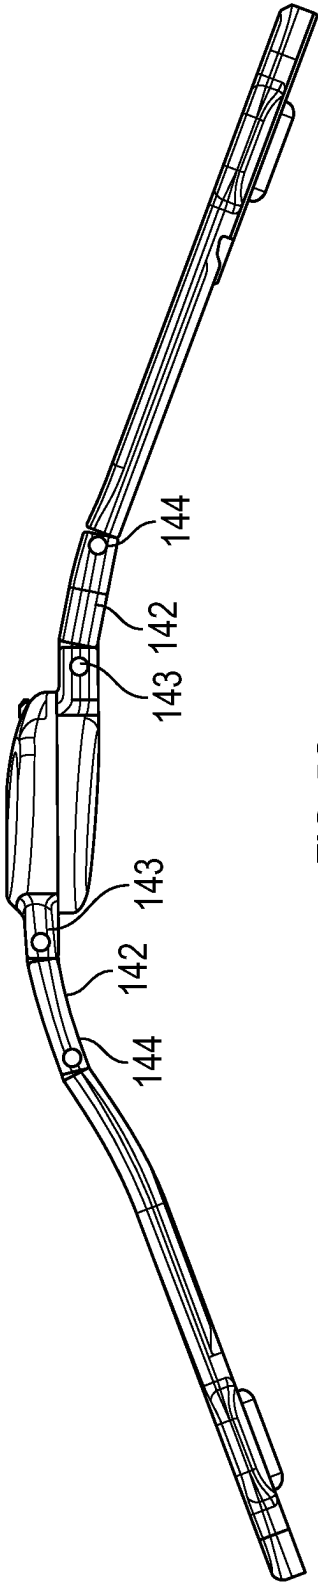


FIG. 5C

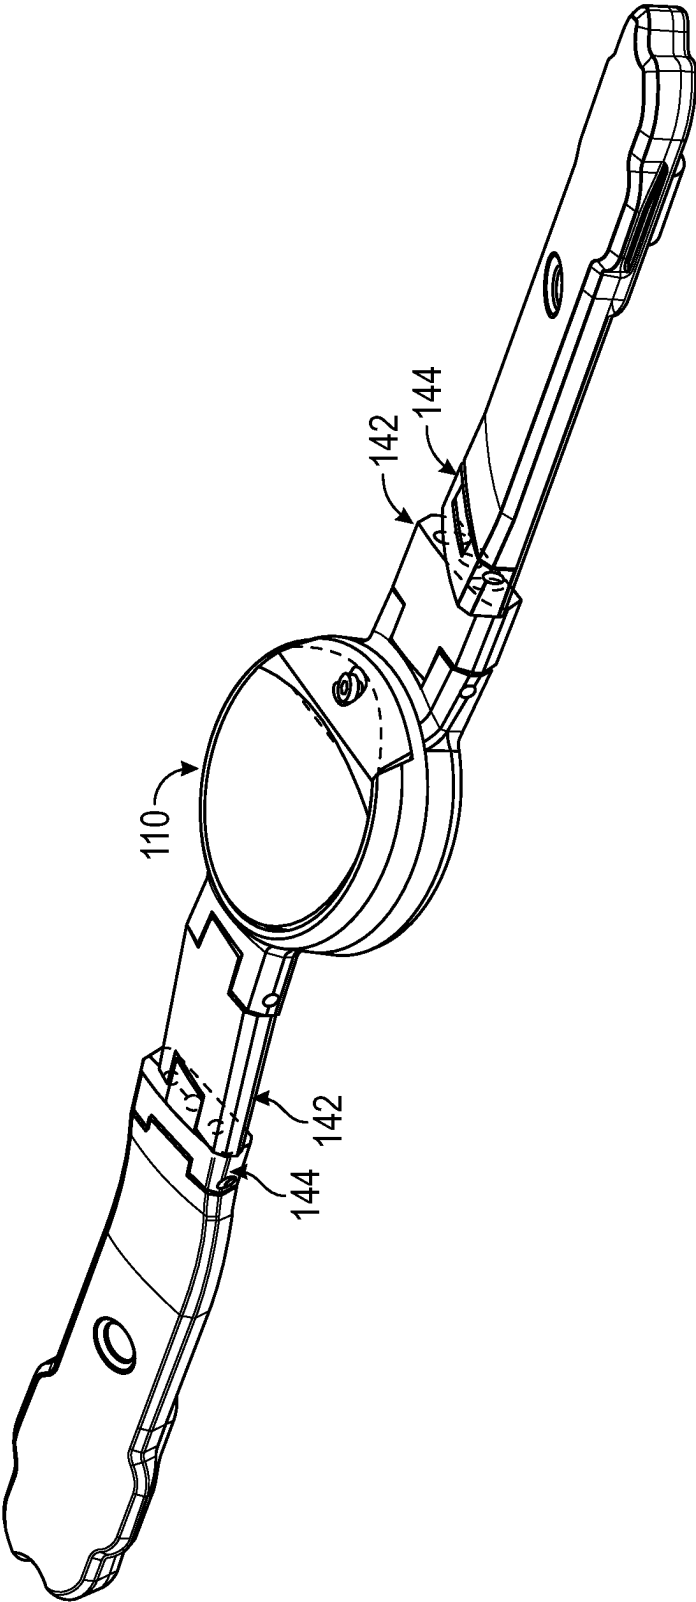


FIG. 6

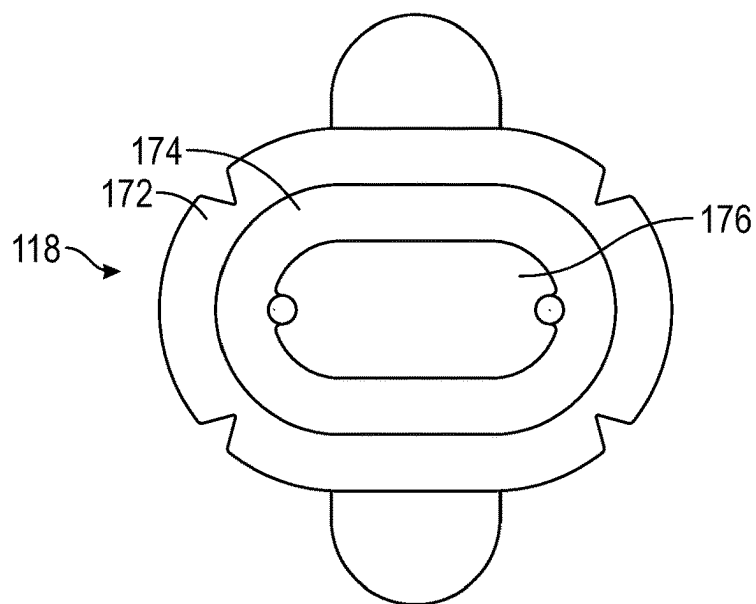


FIG. 7A

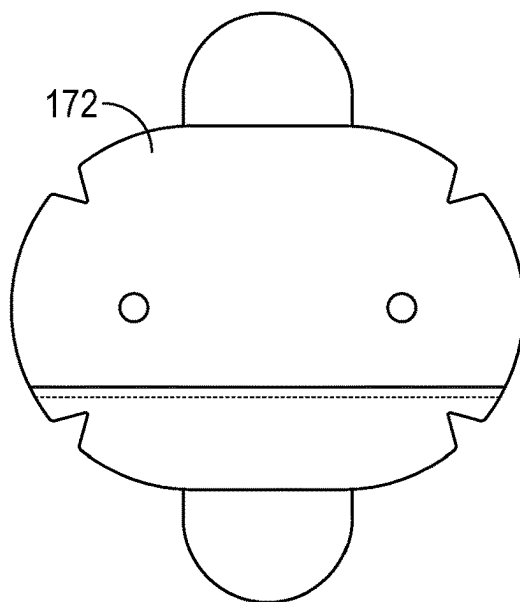


FIG. 7B

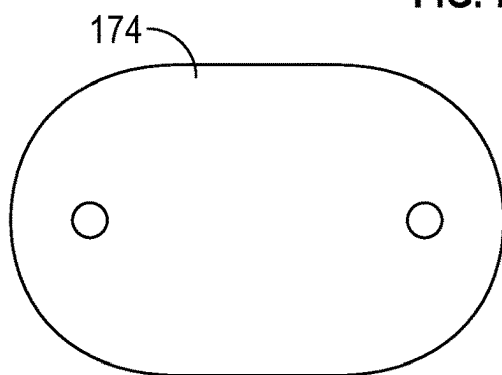


FIG. 7C

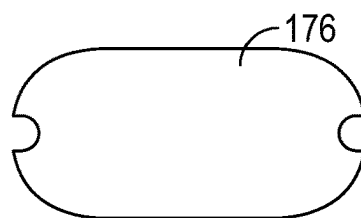


FIG. 7D

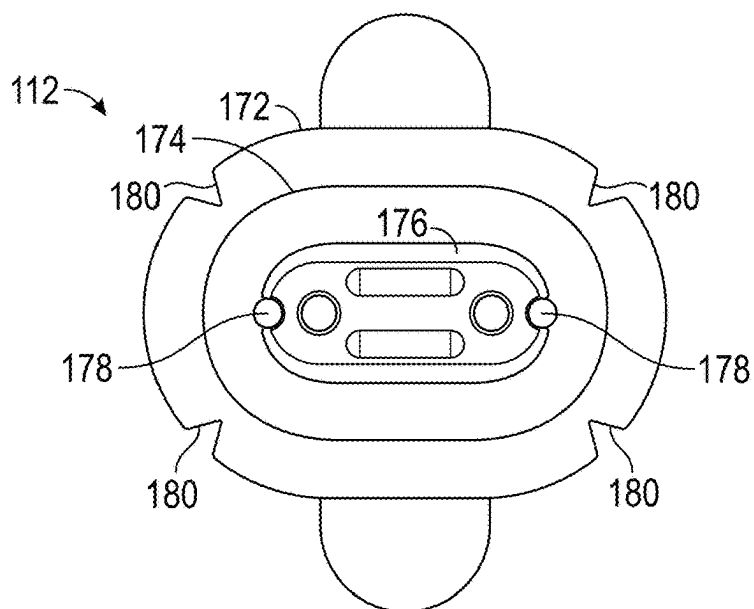


FIG. 8A

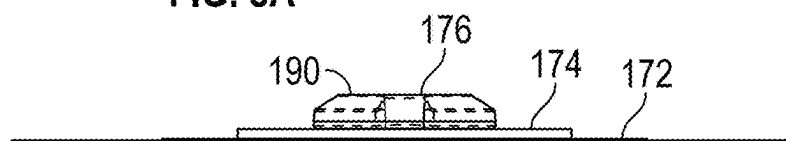


FIG. 8B

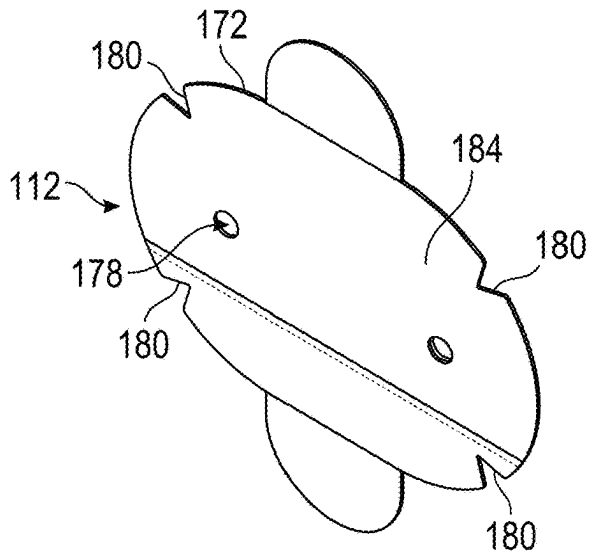


FIG. 8C

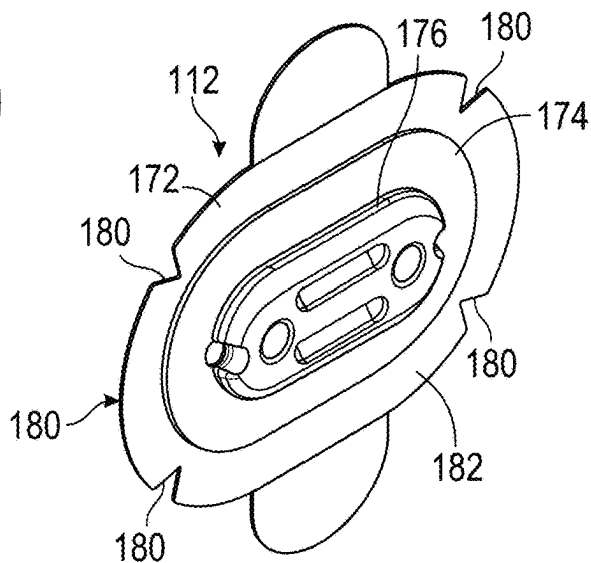


FIG. 8D

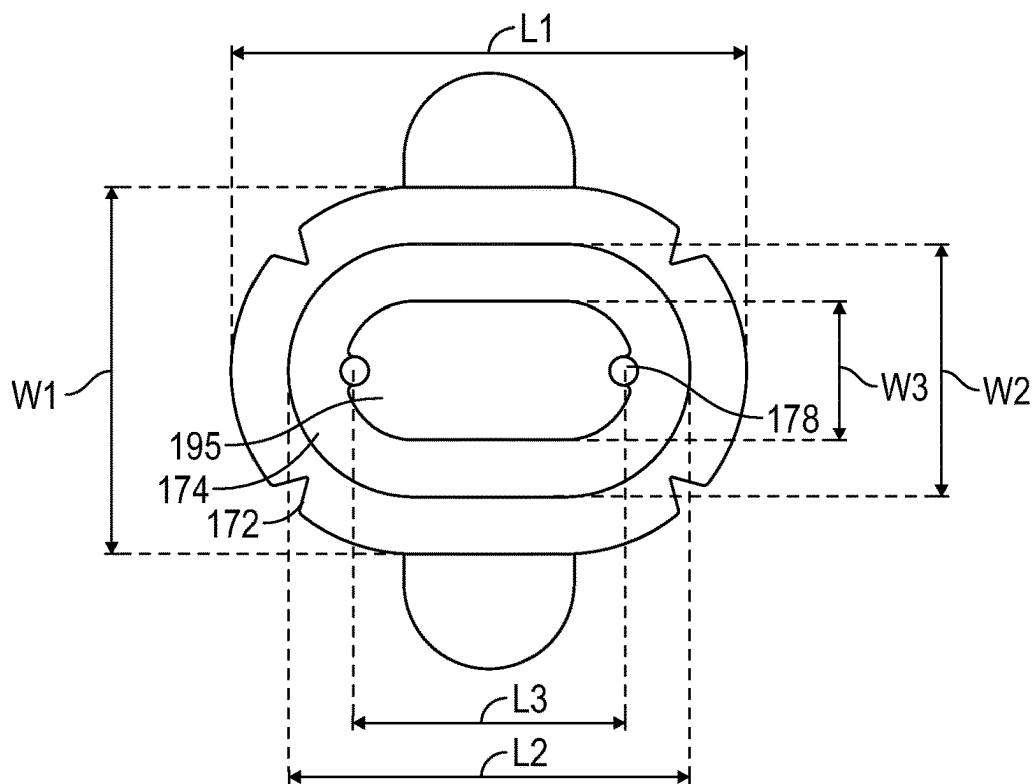


FIG. 9A

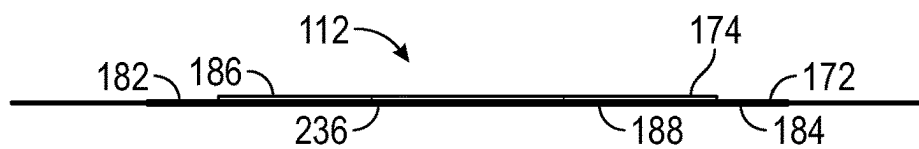


FIG. 9B

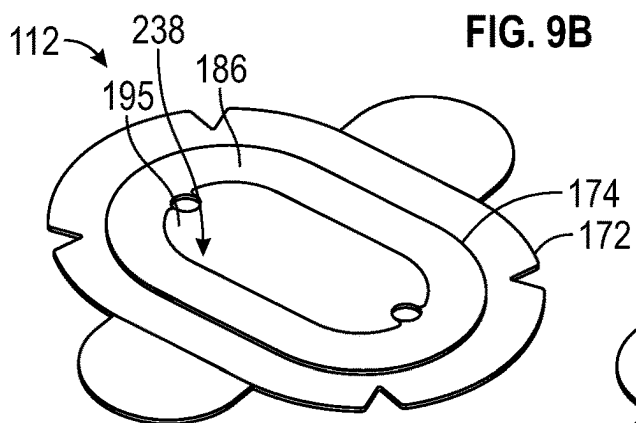


FIG. 9C

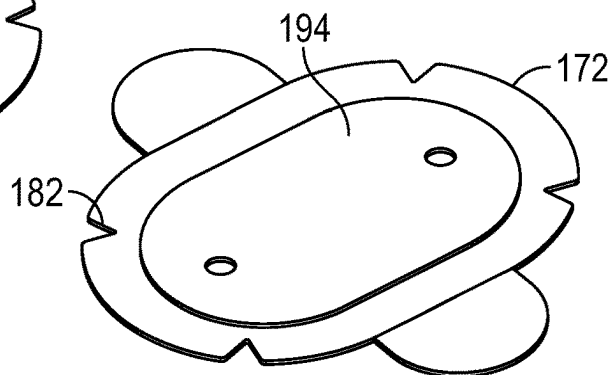


FIG. 9D

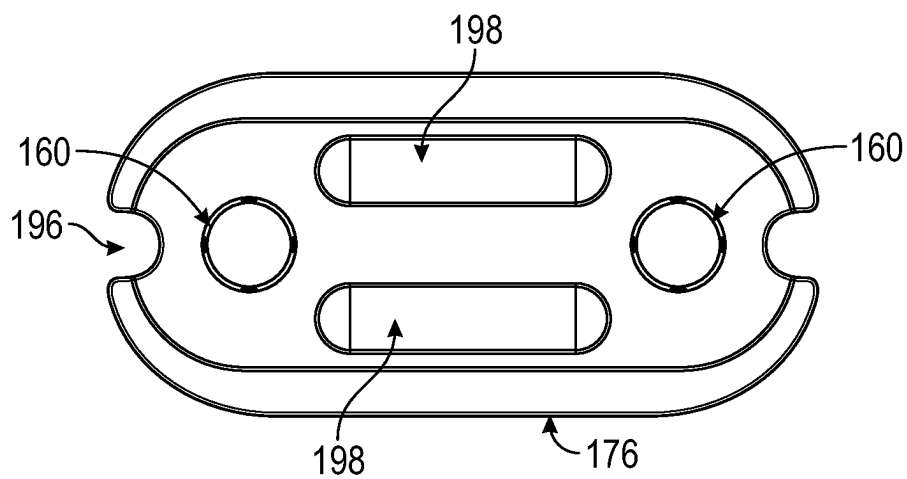


FIG. 10A



FIG. 10B

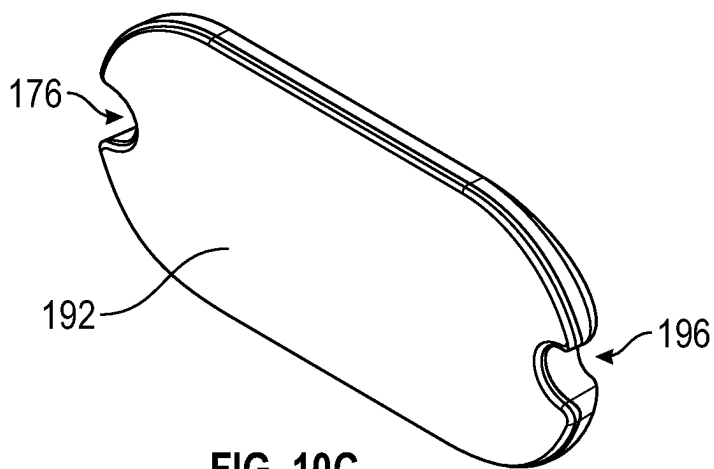


FIG. 10C

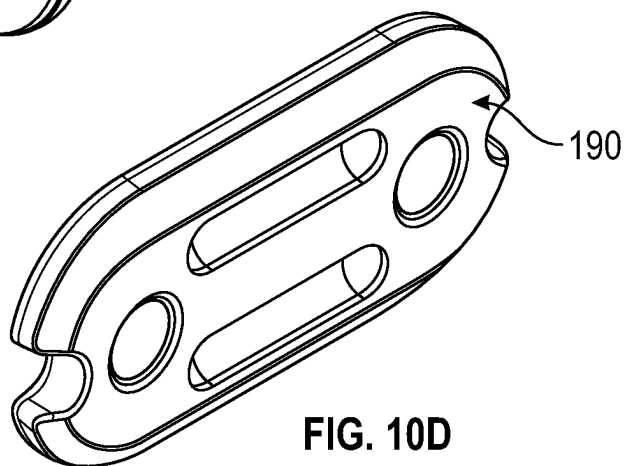


FIG. 10D

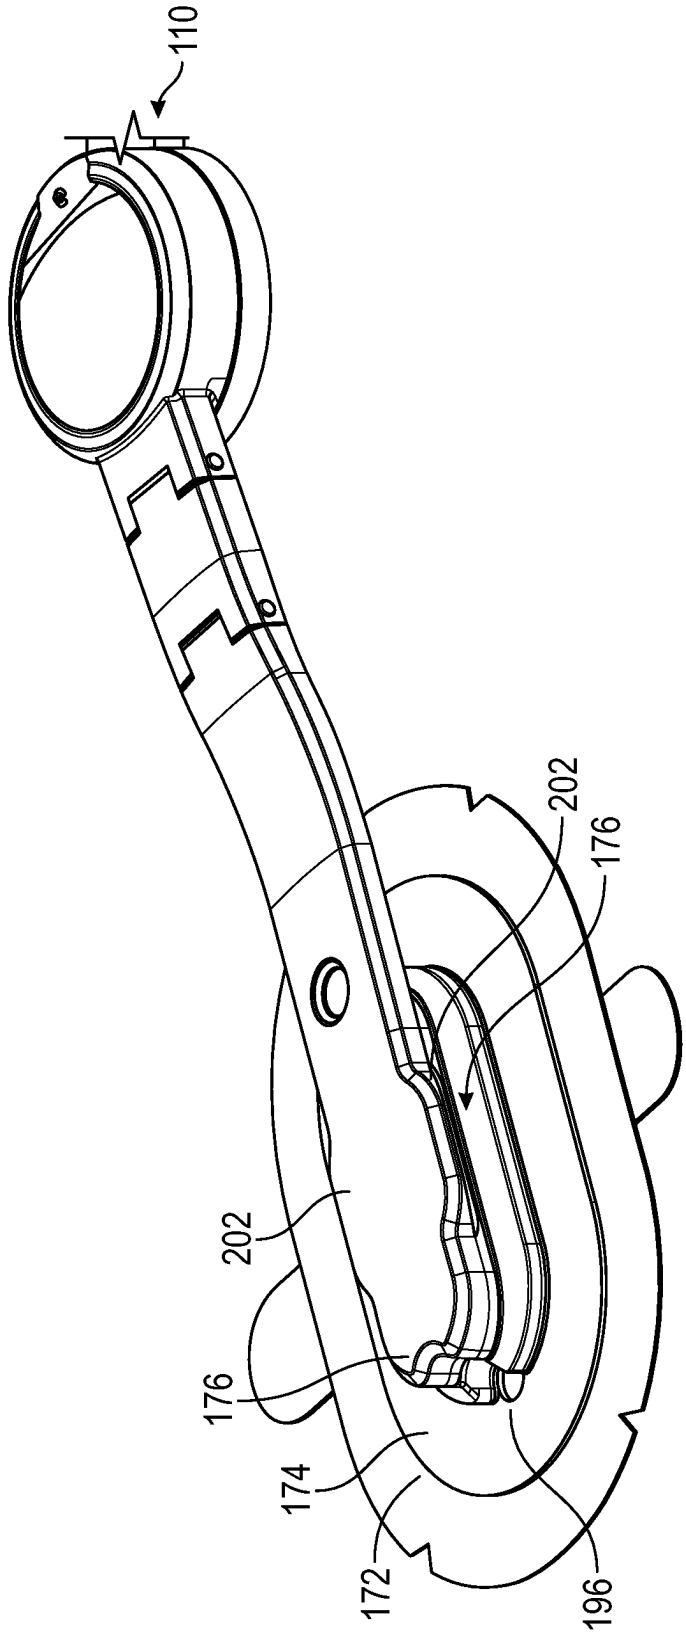


FIG. 11A

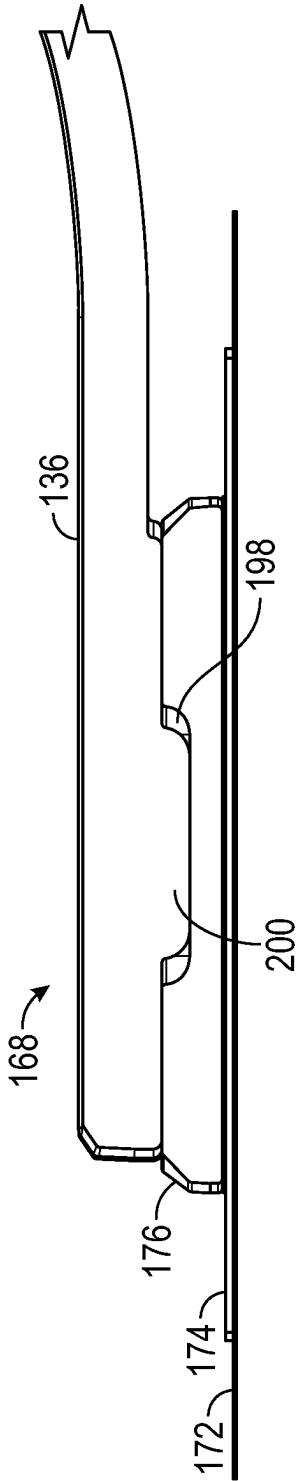


FIG. 11B

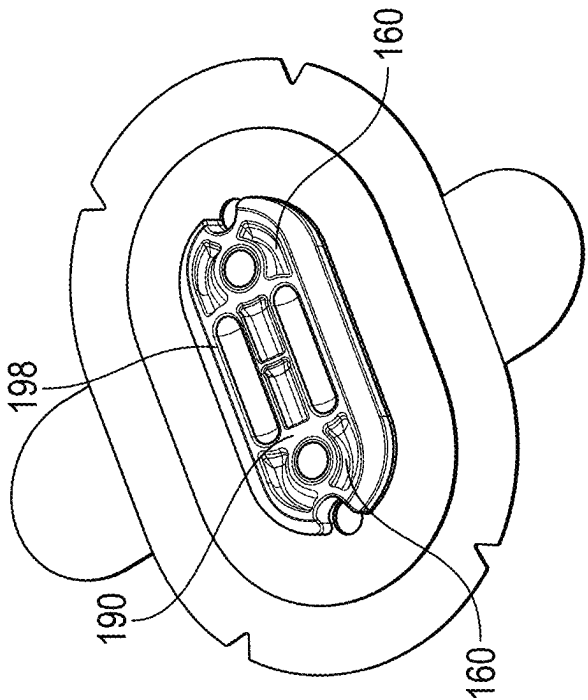


FIG. 12A

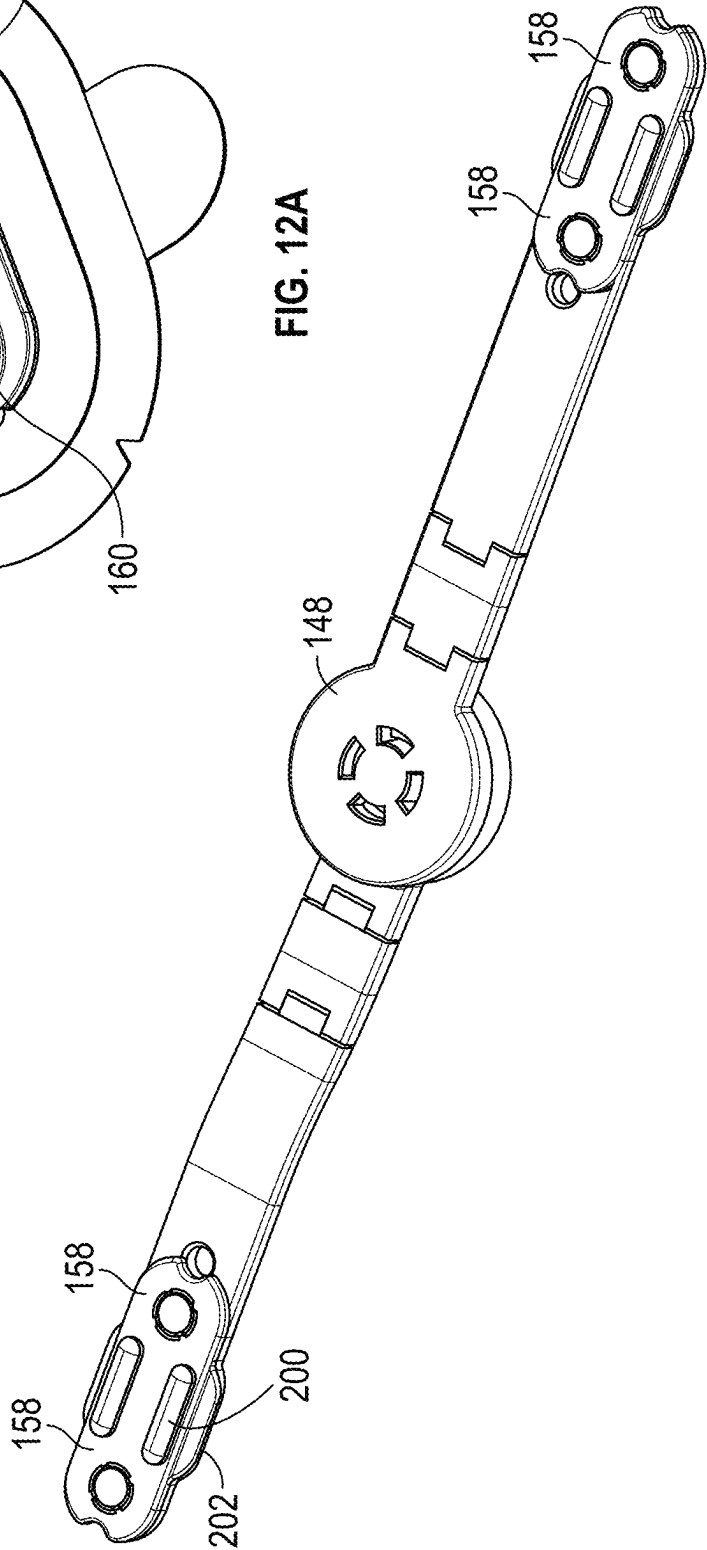


FIG. 12B

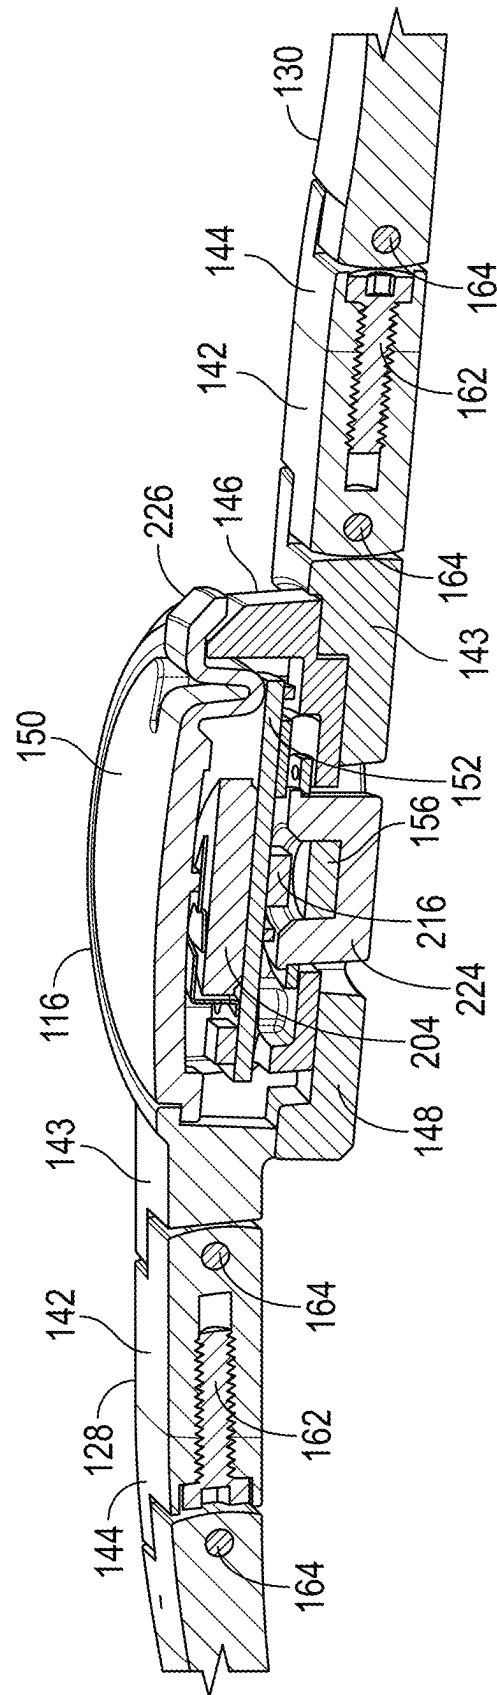


FIG. 13

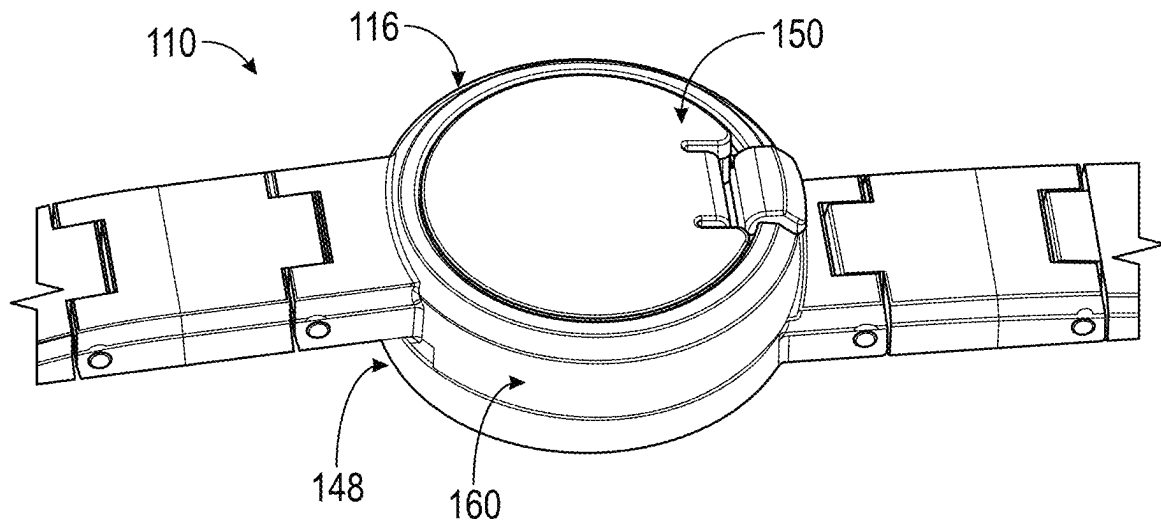


FIG. 14A

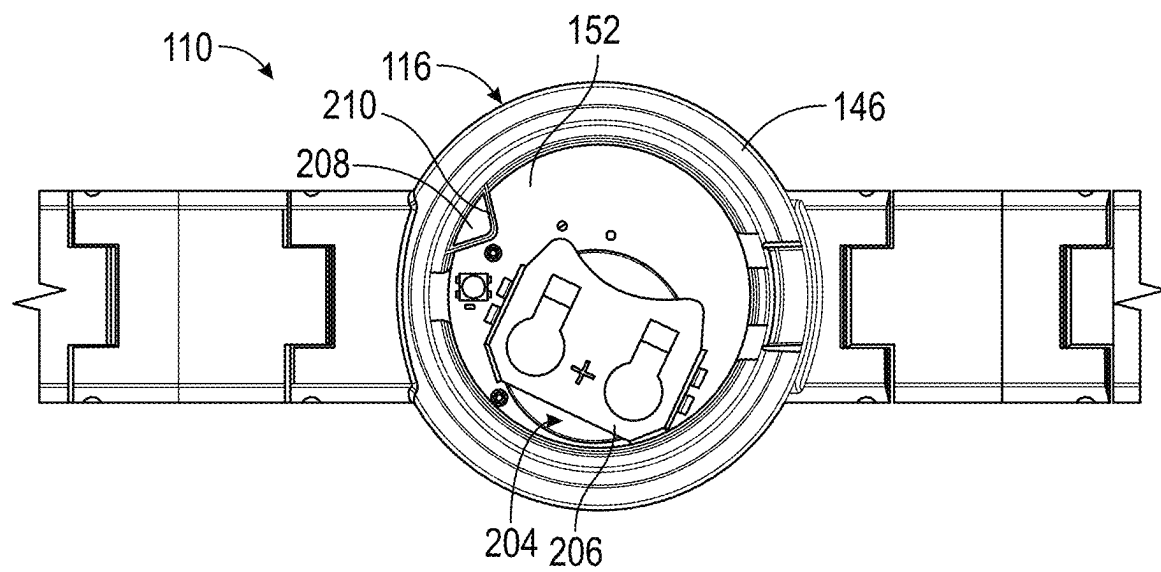


FIG. 14B

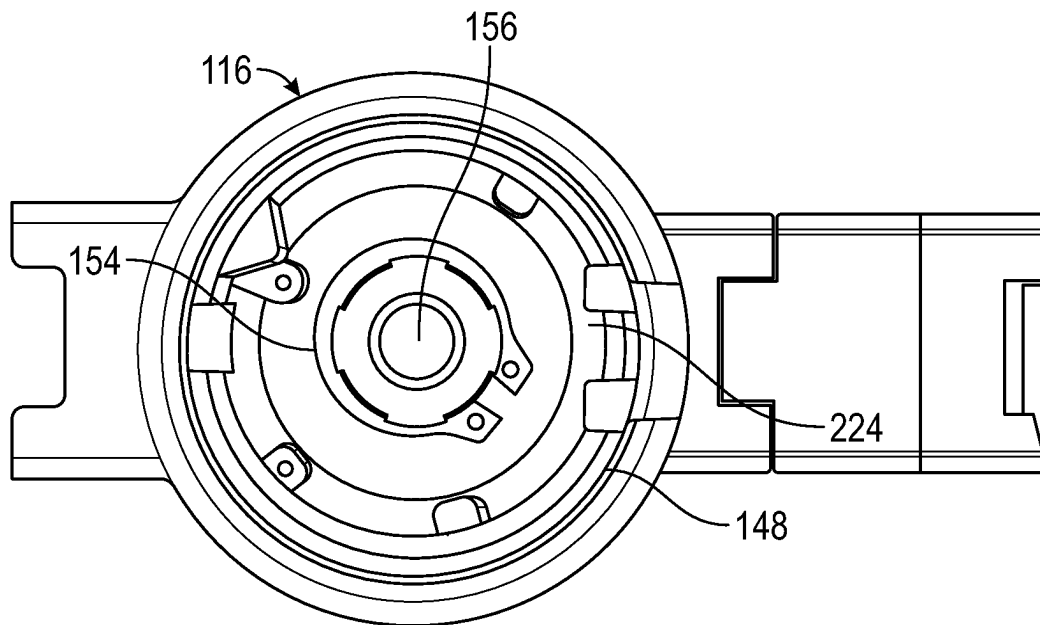


FIG. 14C

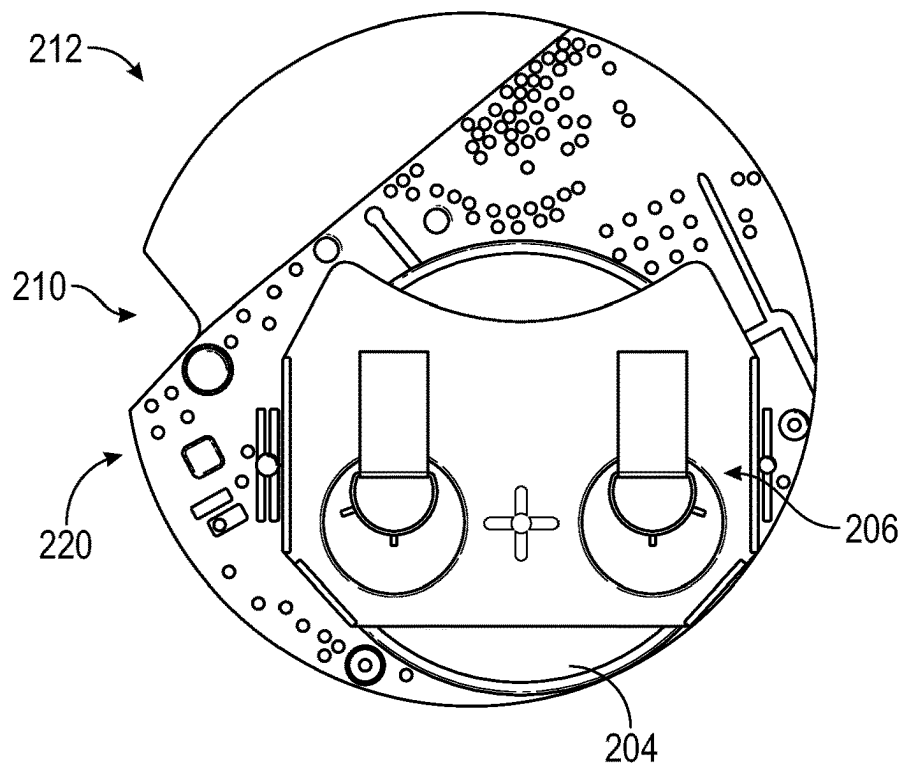


FIG. 15A

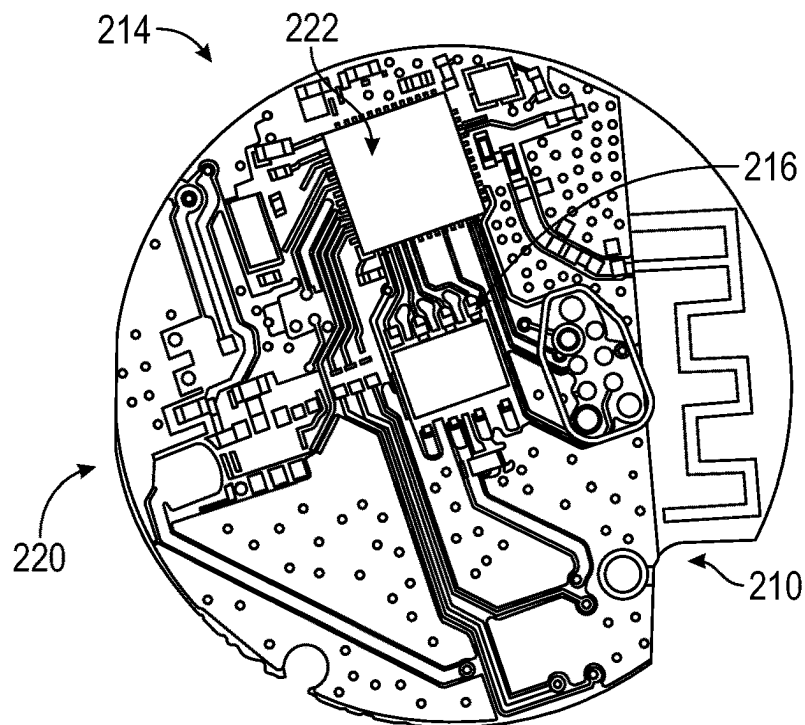


FIG. 15B

228 → **Range of Motion and Standard Deviation using Adhesive Based Goniometer Fixation**

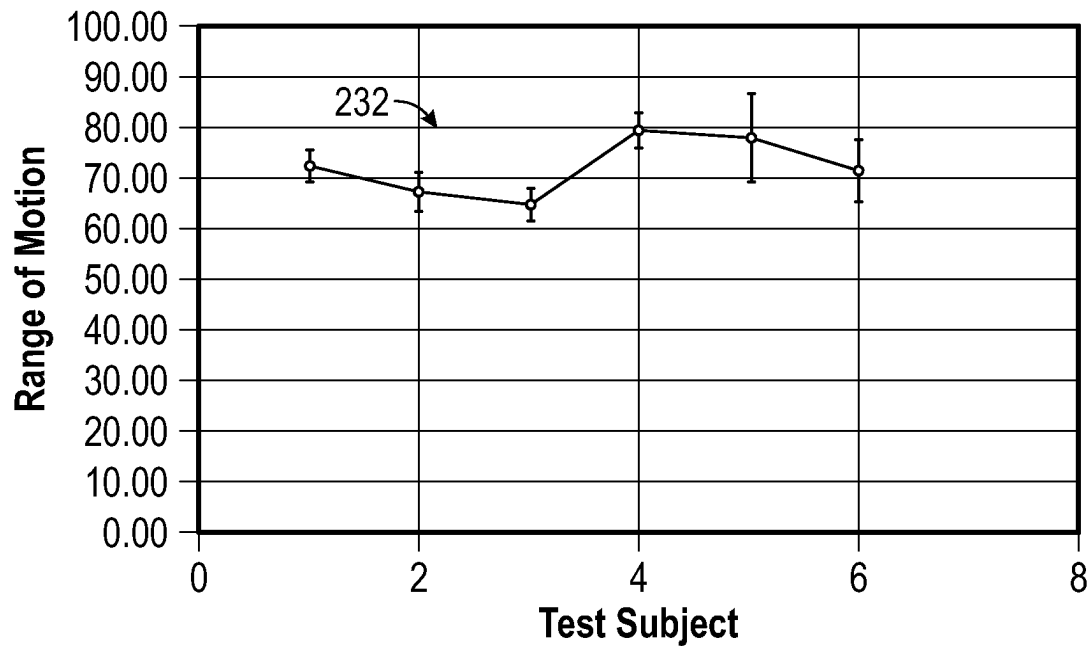


FIG. 16A

230 → **Range of Motion and Standard Deviation using Strap Based Goniometer Fixation**

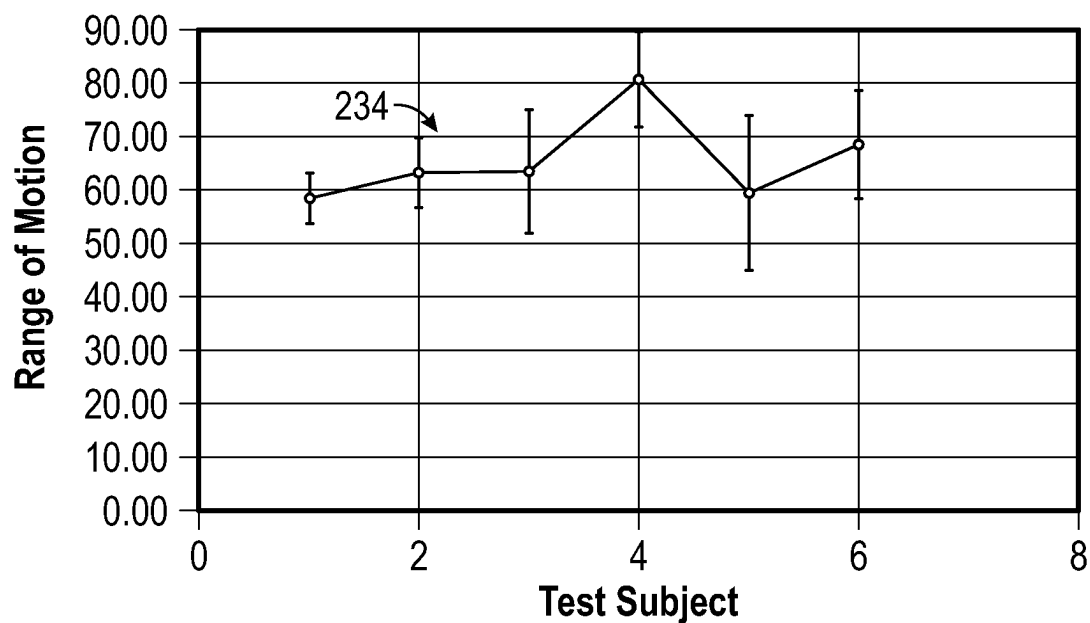


FIG. 16B

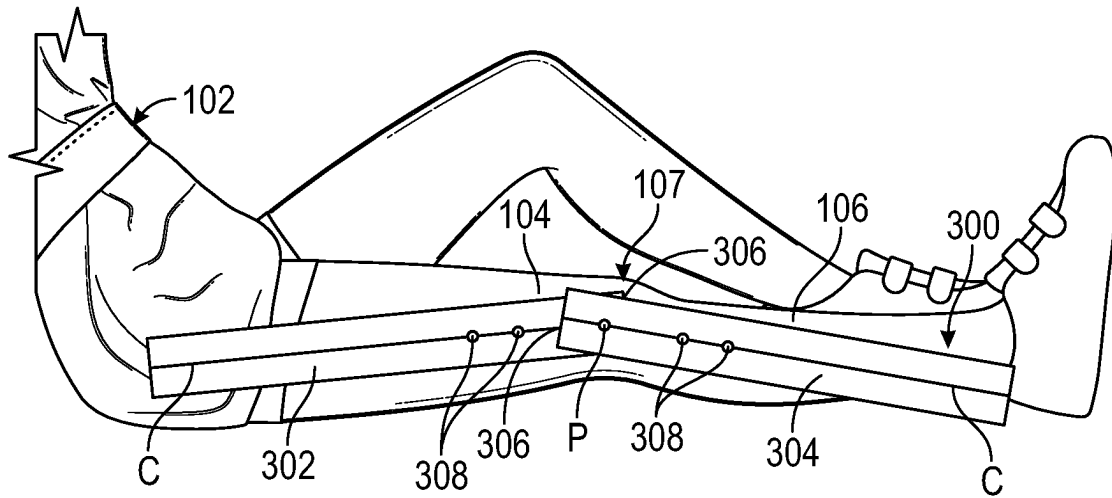


FIG. 17

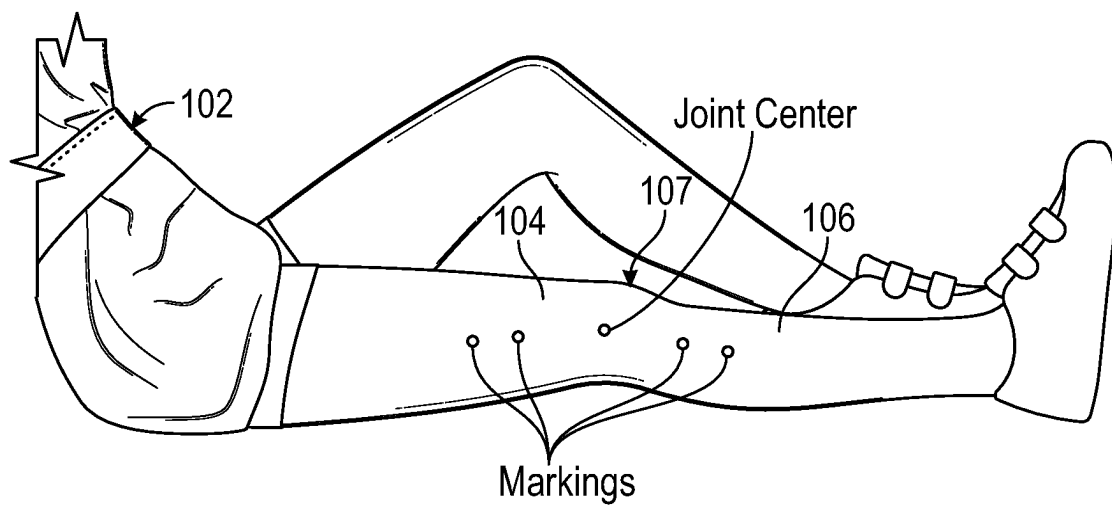


FIG. 18

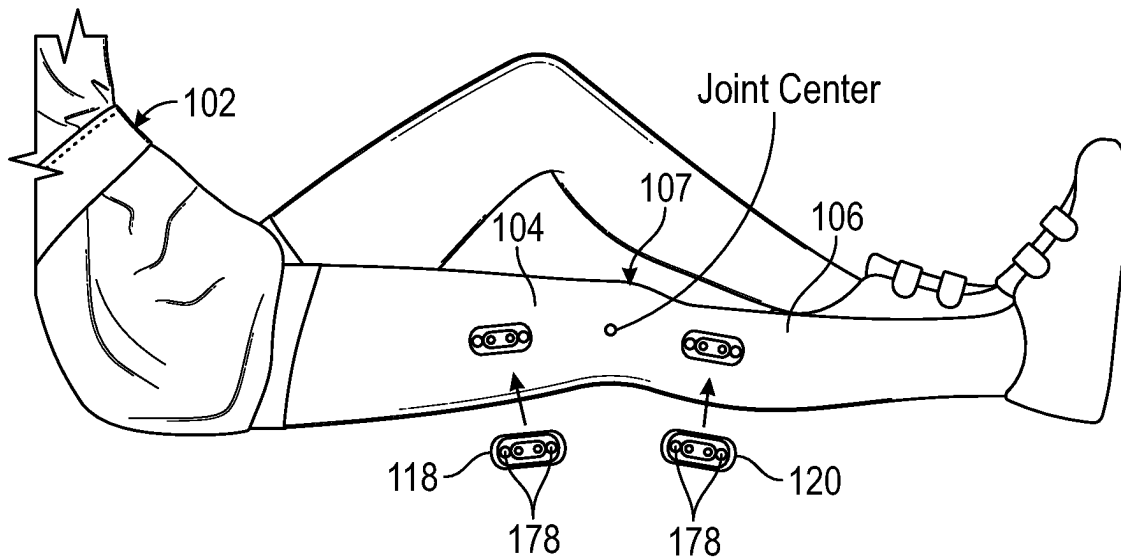


FIG. 19

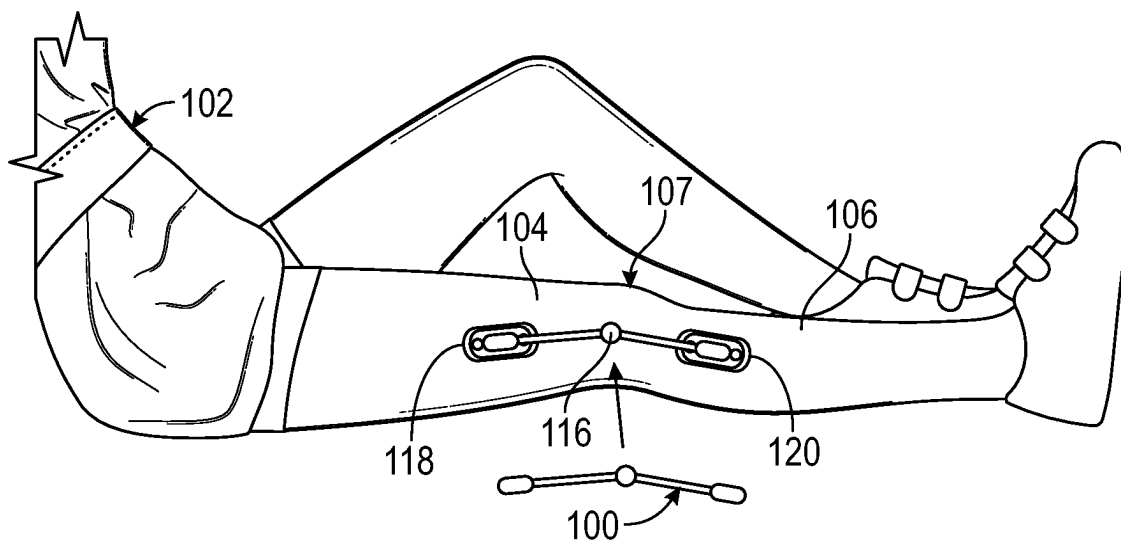


FIG. 20

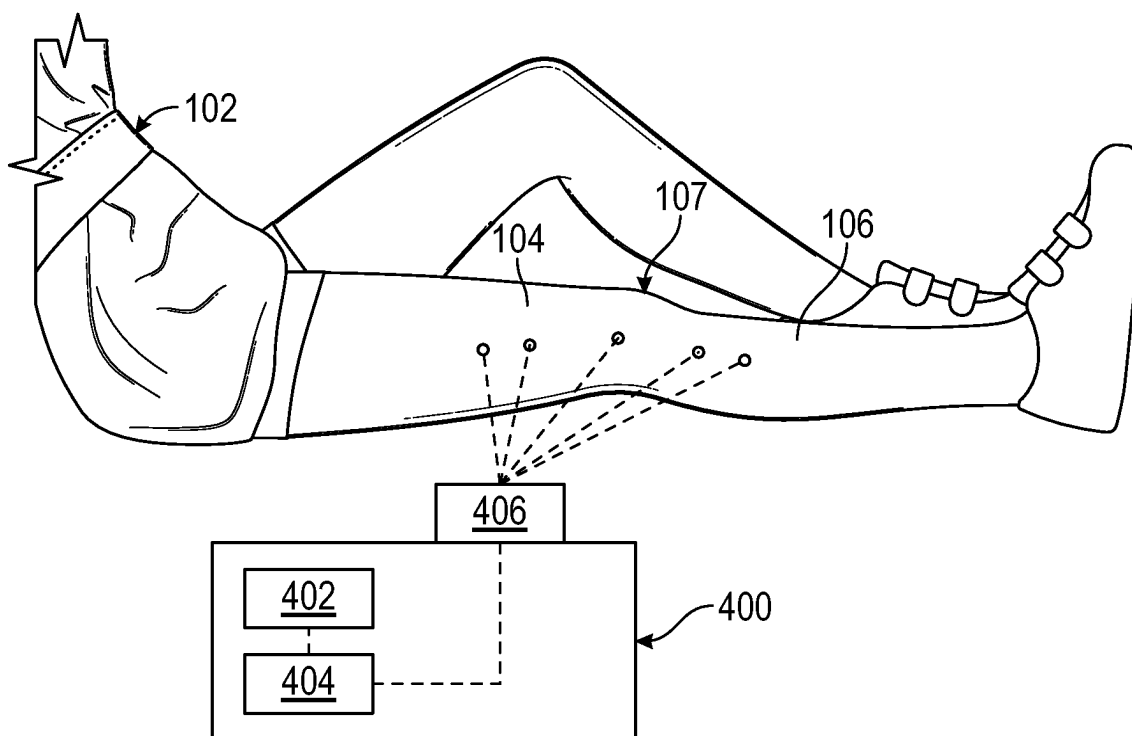


FIG. 21

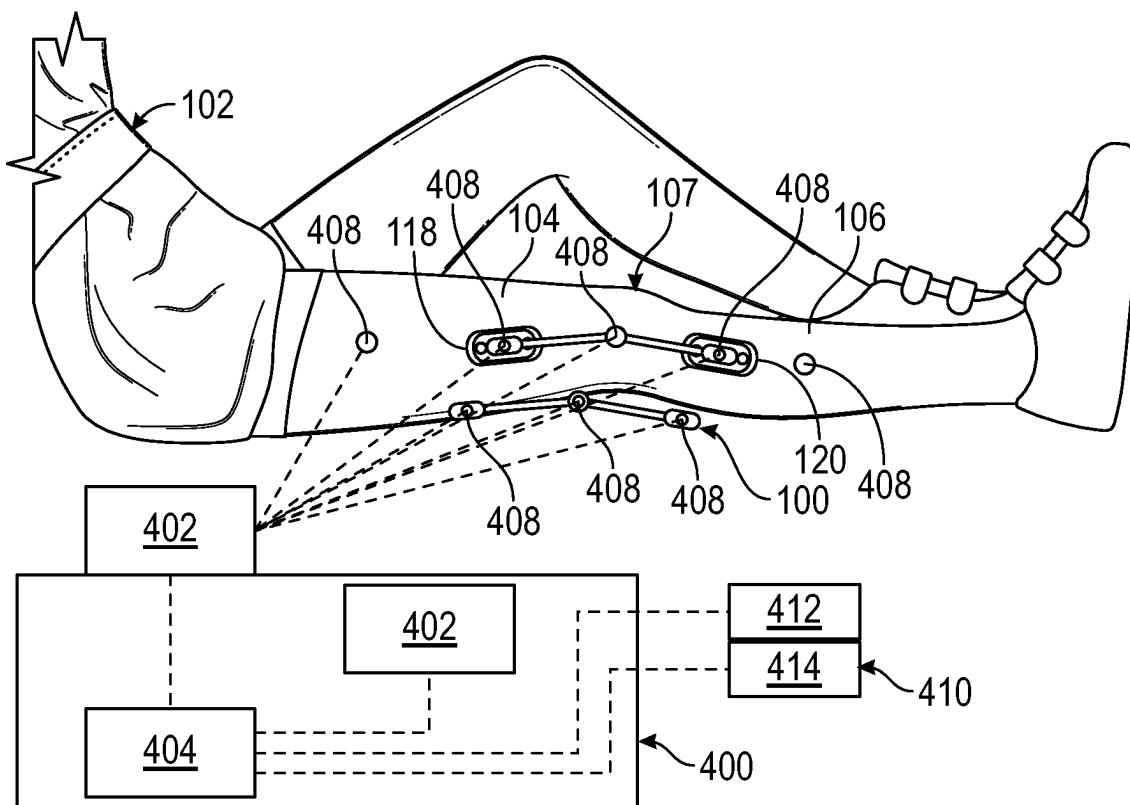


FIG. 22

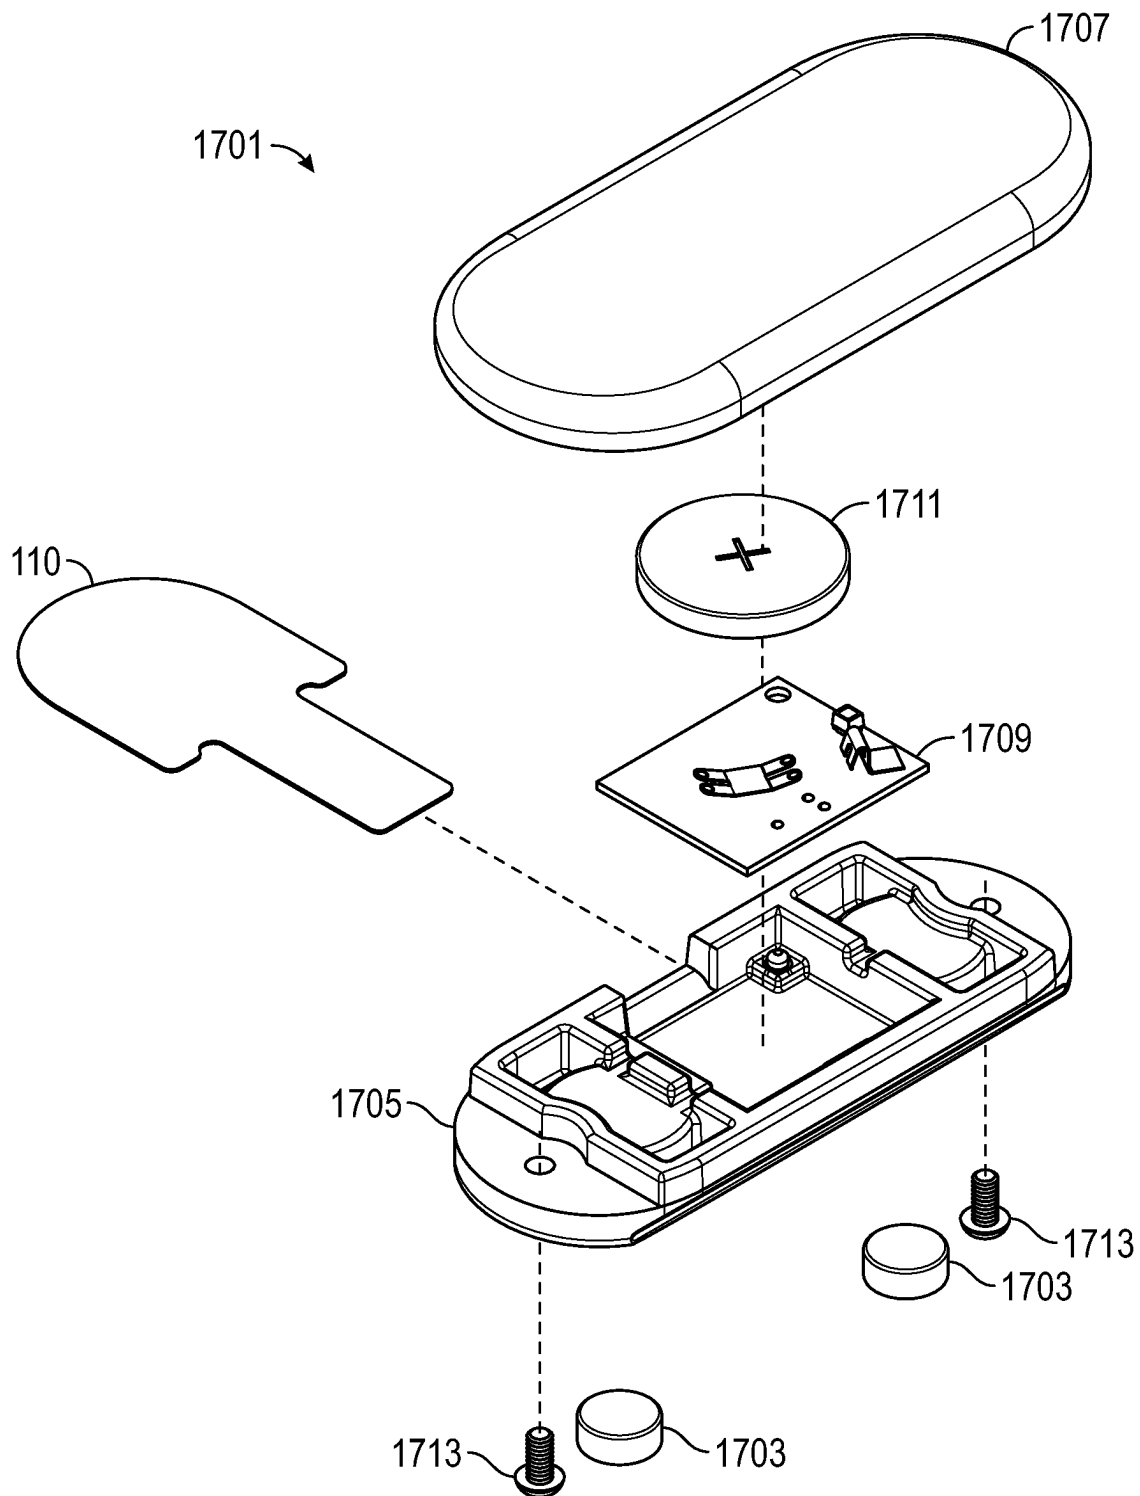


FIG. 23A

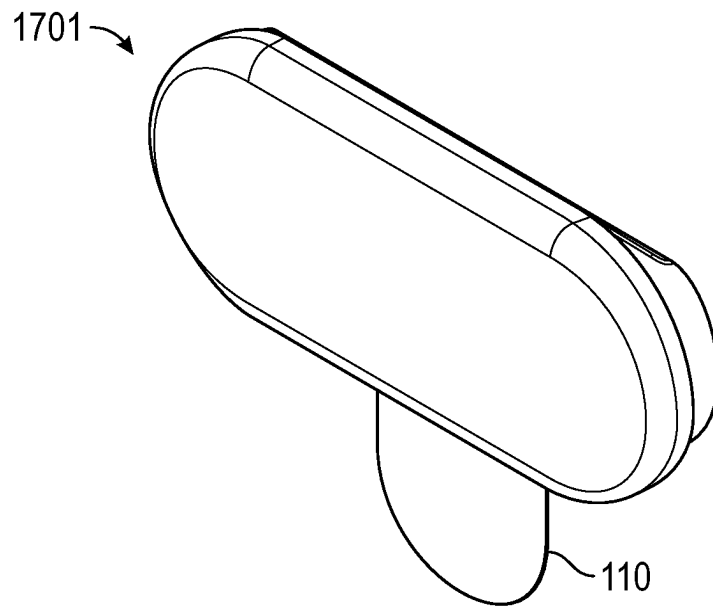


FIG. 23B

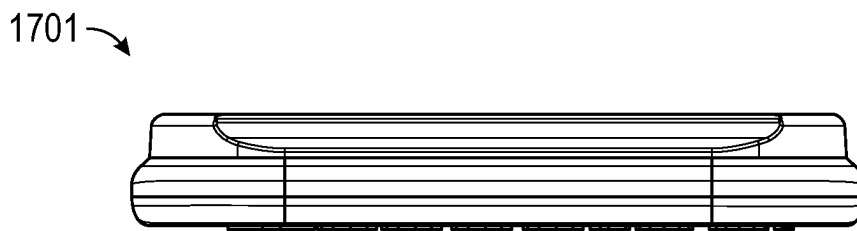


FIG. 23C

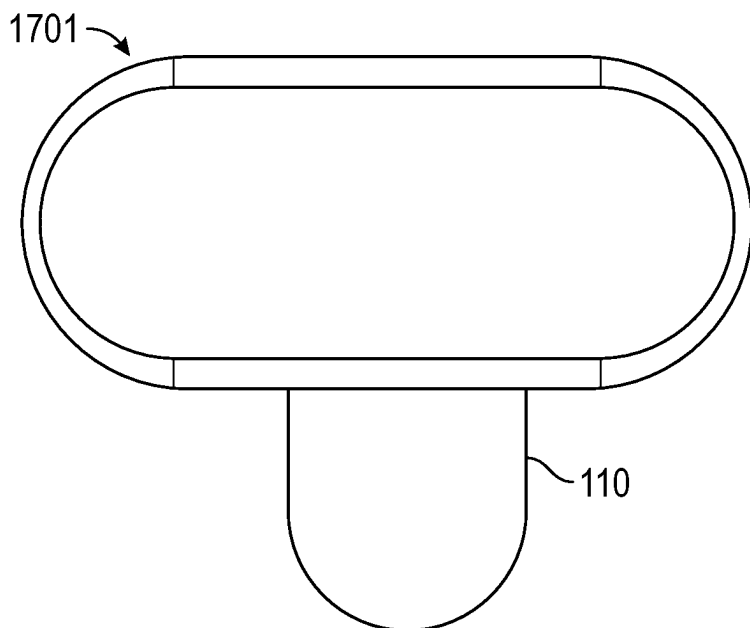


FIG. 23D

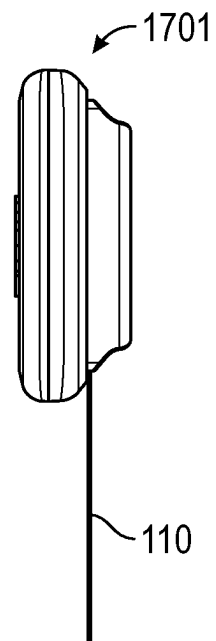


FIG. 23E

1300 ↗

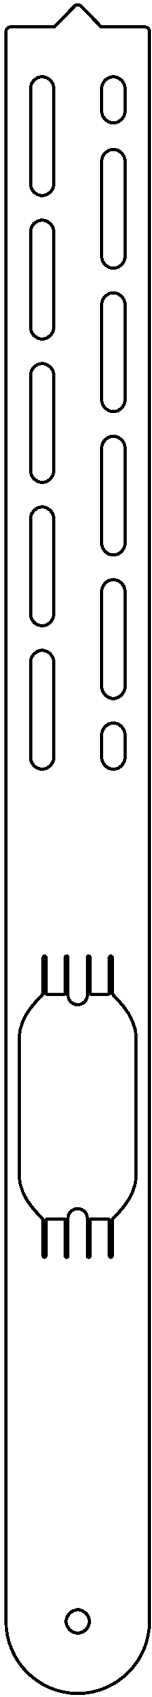


FIG. 24

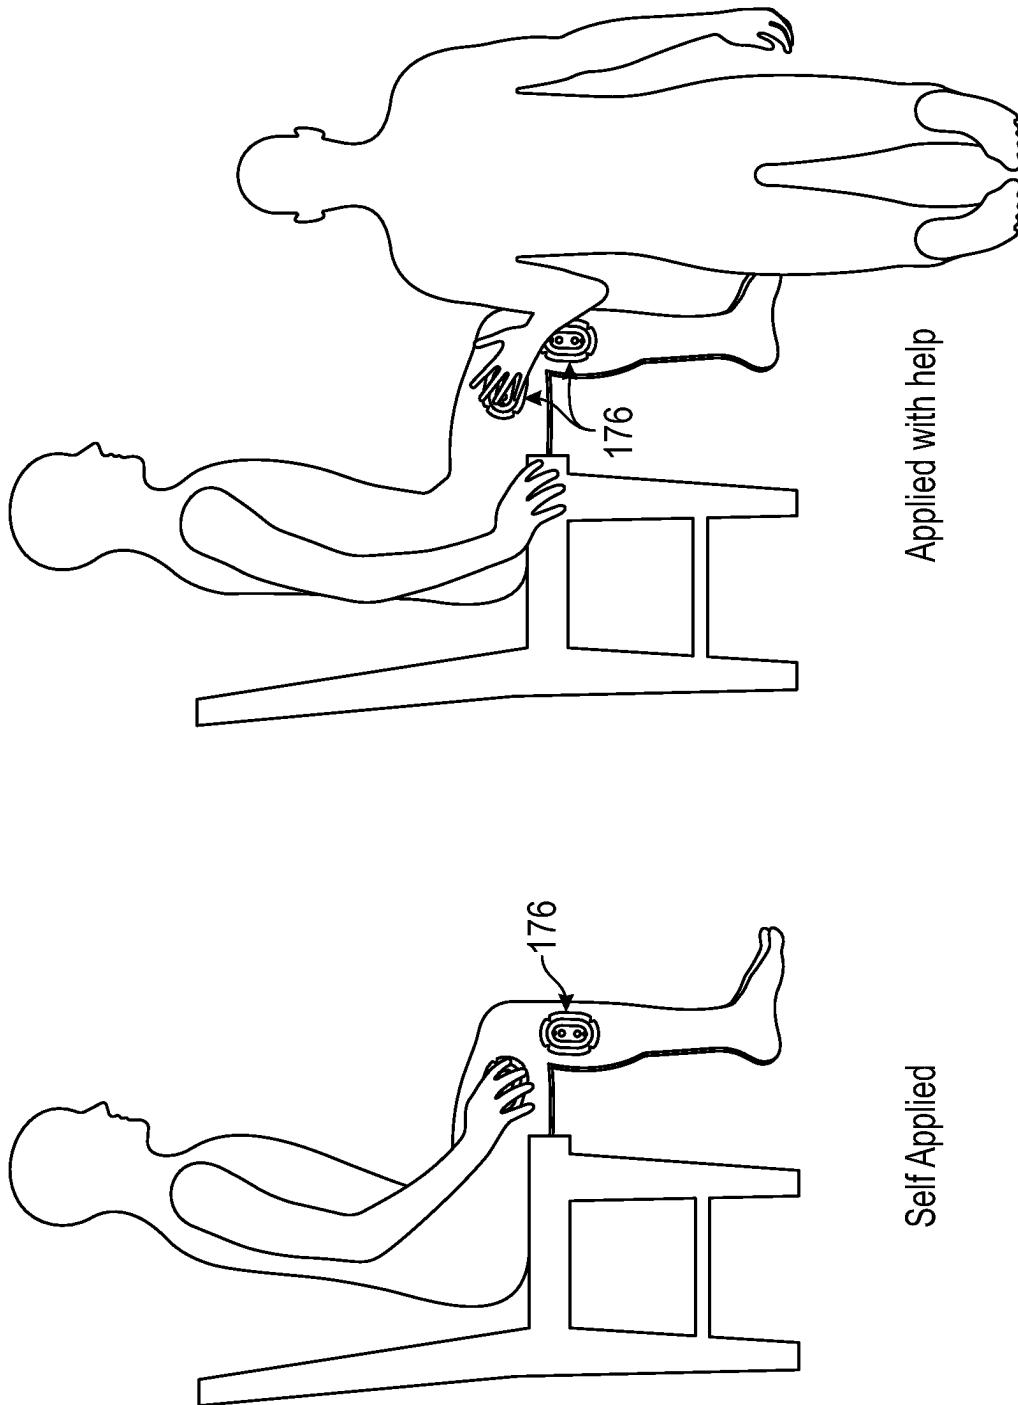


FIG. 25

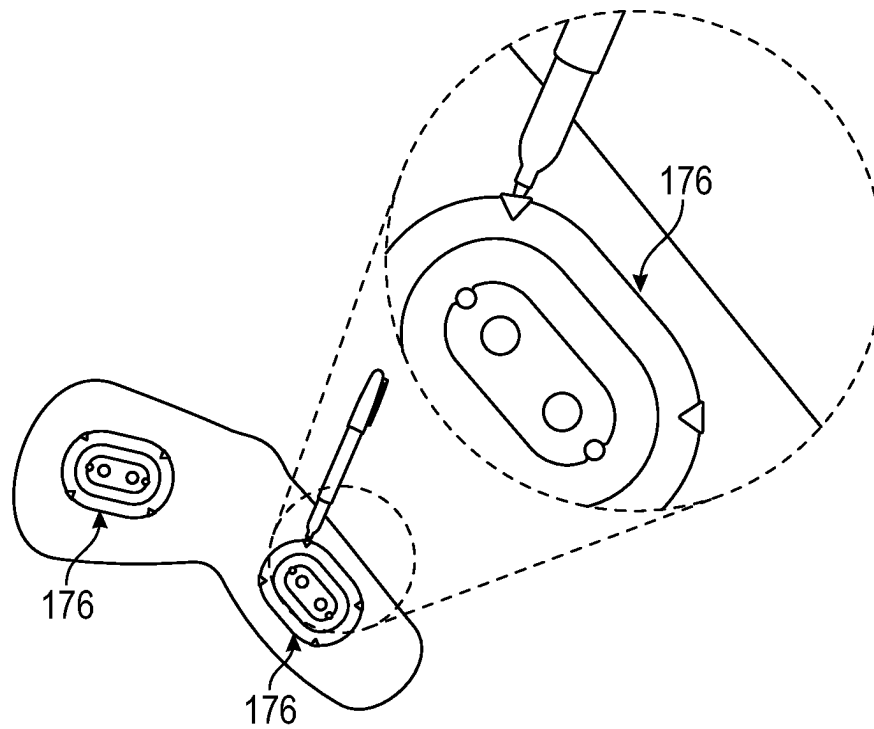


FIG. 26

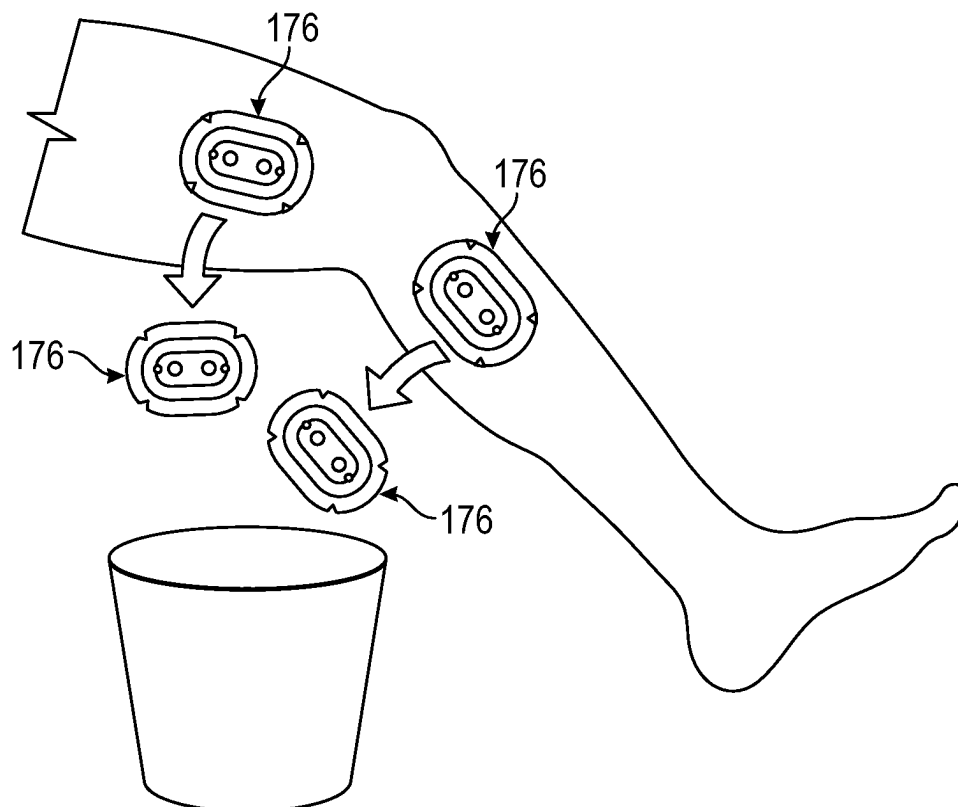


FIG. 27

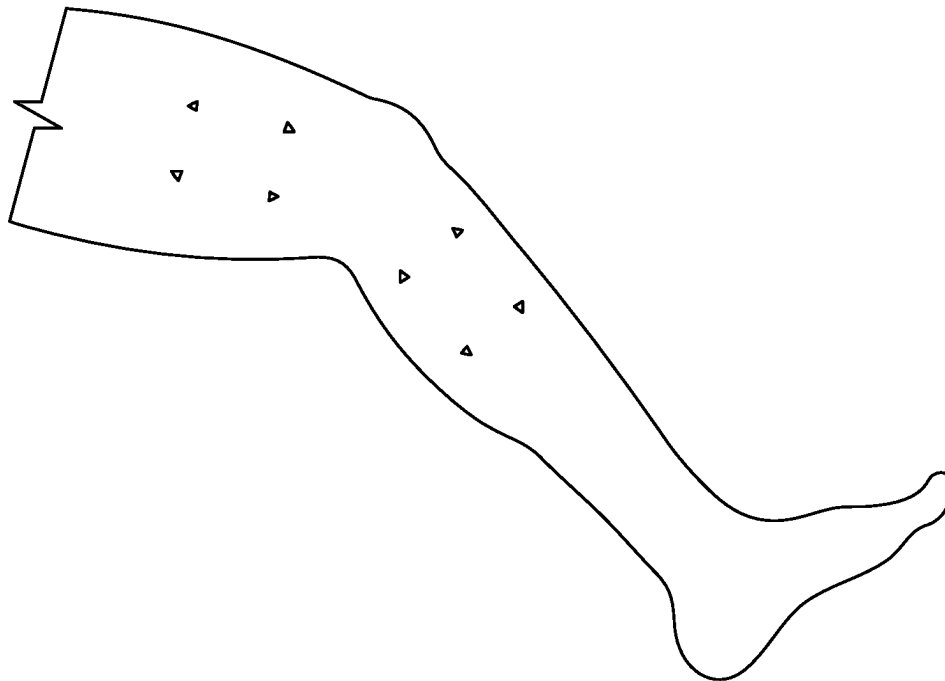


FIG. 28

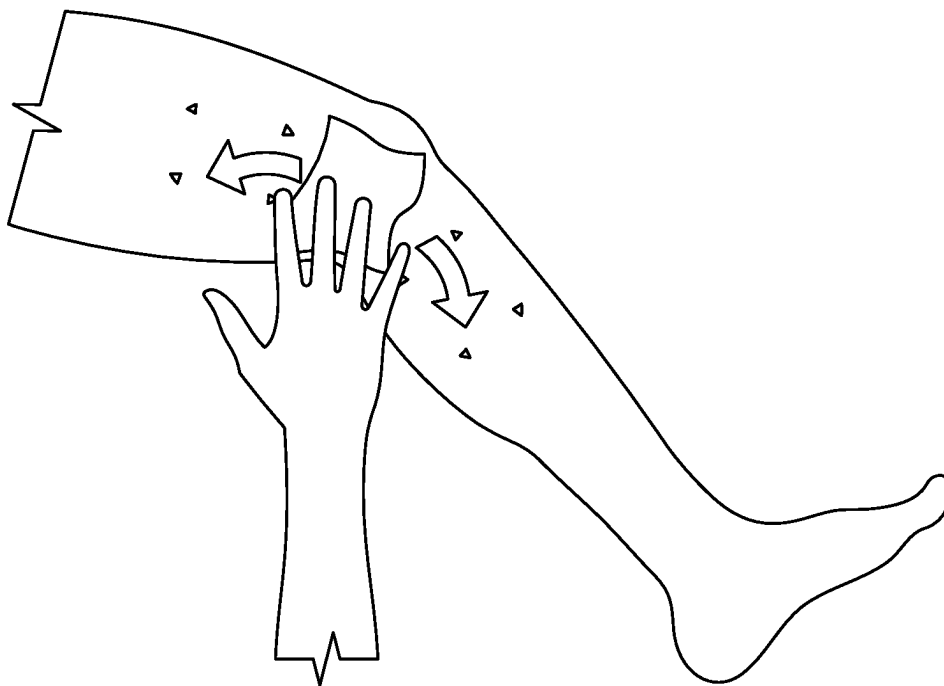


FIG. 29

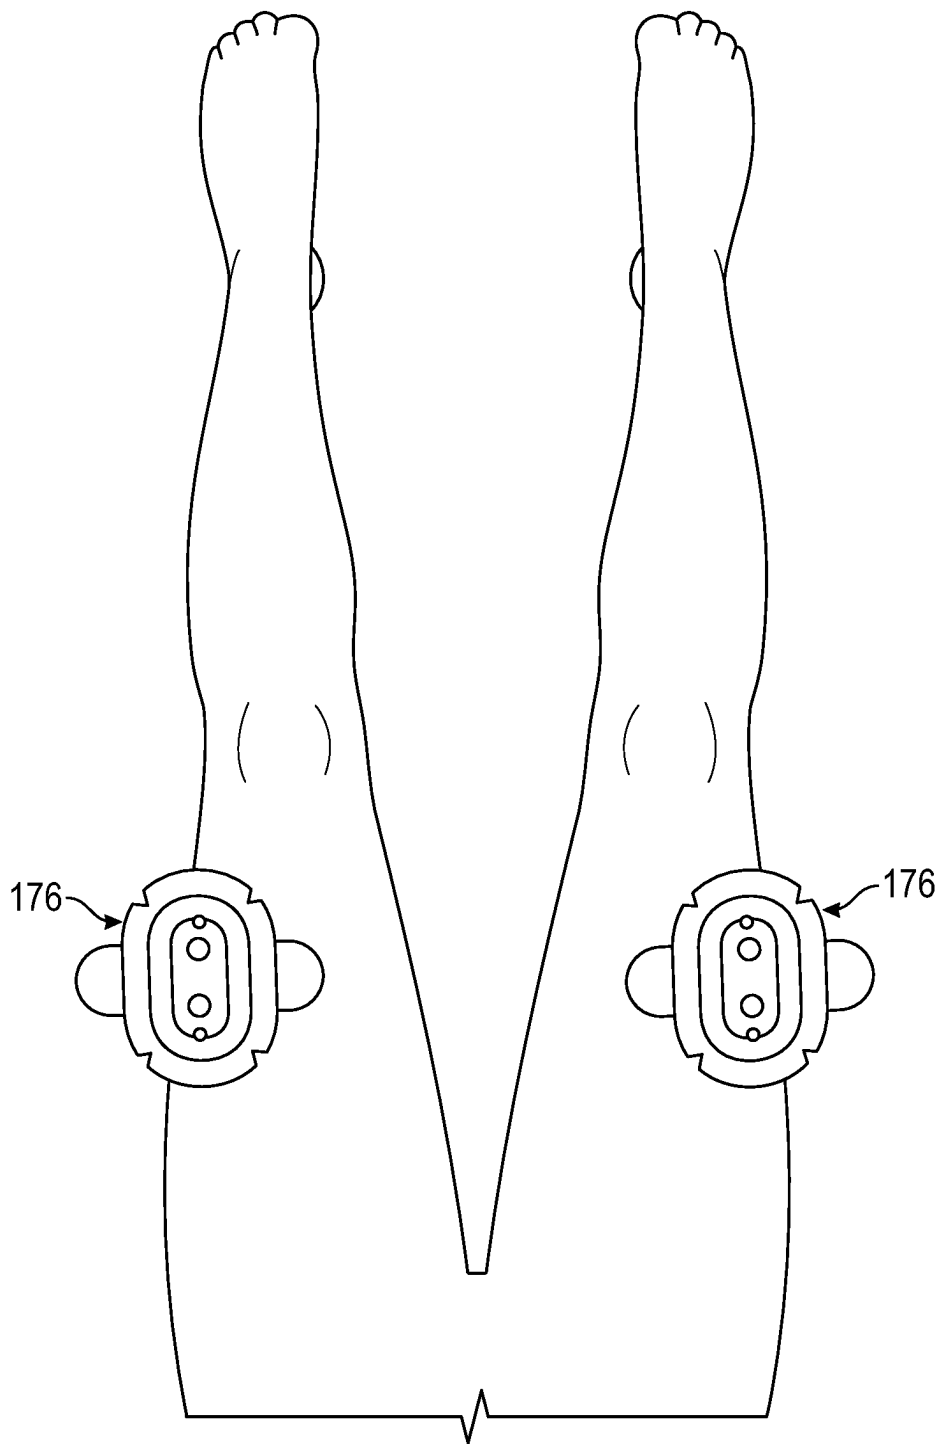


FIG. 30

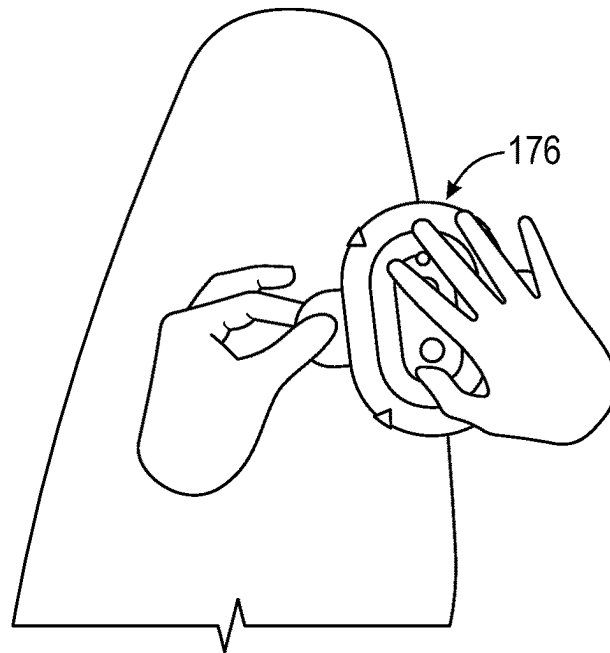


FIG. 31

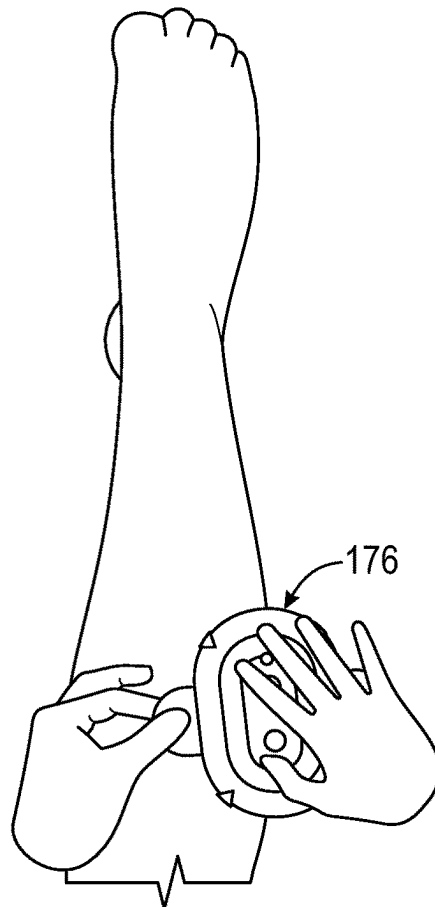


FIG. 32

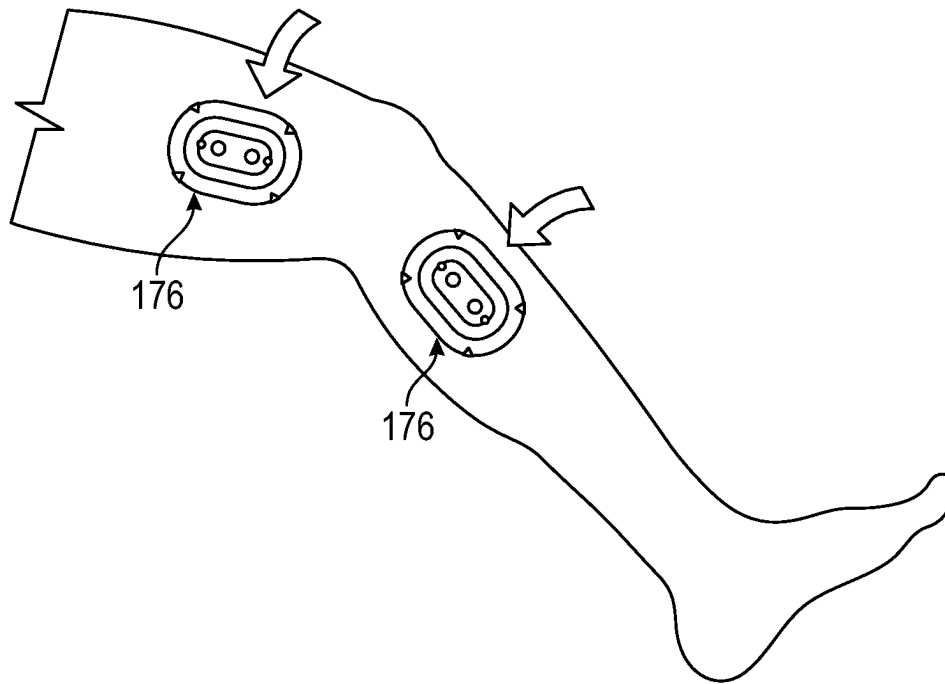


FIG. 33

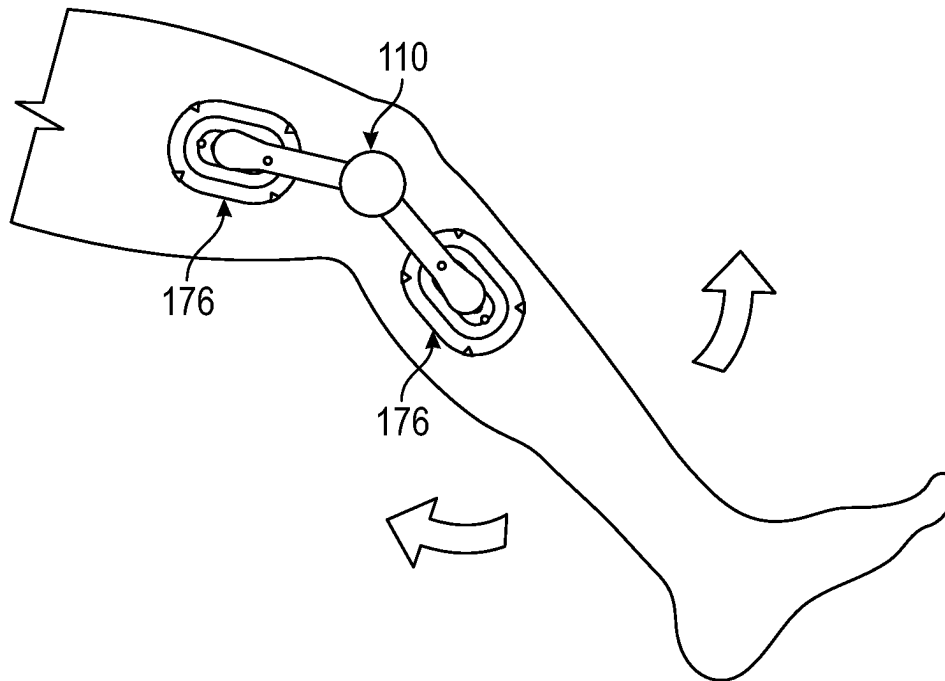


FIG. 34

1

WEARABLE DEVICE FOR COUPLING TO A USER, AND MEASURING AND MONITORING USER ACTIVITY

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority to and the benefit of: U.S. Prov. Pat. App. No. 62/991,295, filed Mar. 18, 2020, U.S. Prov. Pat. App. No. 62/911,515, filed Oct. 7, 2019, U.S. Prov. Pat. App. No. 62/904,013, filed Sep. 23, 2019, U.S. Prov. Pat. App. No. 62/901,464, filed Sep. 17, 2019, and U.S. Prov. Pat. App. No. 62/901,411, filed Sep. 17, 2019, each of which is incorporated herein by reference in its entirety.

TECHNICAL FIELD

This disclosure generally relates to wearable devices and, in particular, to coupling a wearable device to a user and measuring and monitoring activity of the user.

BACKGROUND

A patient often requires physical therapy to recover from surgery, such as a knee replacement surgery. The physical therapy can include exercise to increase the patient's strength, flexibility and stability. If a patient over-extends his or her muscles or joints, the muscles or joints, surrounding tissues or repaired tissues may become further injured. If a patient does not exercise his or her muscles or joints to gain the appropriate range of motion, the joint may become stiff and require additional surgery. Measuring and monitoring the range of motion during physical therapy can help prevent further injury to the patient and result in a faster recovery time.

A goniometer is an instrument that can be used to measure ranges of motion or joint angles of a patient's body. A standard goniometer consists of a stationary arm that cannot move independently, a moving arm attached to a fulcrum in the center of a body, and the body being a protractor of which 0 to 180 or 360 degrees are drawn. The stationary arm is attached to one limb or part of the patient's body (e.g., a thigh) and the moving arm is attached to another limb or part of the patient's body (e.g., a lower leg). The fulcrum can be a rivet or screw-like device at the center of the body that allows the moving arm to move freely on the body of the device in order for a clinician to obtain a measurement of the angle of movement of the patient's joint (e.g., a knee). The measurements can be used to track progress in a rehabilitation program. Each time a patient has a rehabilitation session, the clinician places and hold, or attaches the goniometer device onto the patient, for example, using straps. The patient may have different clinicians setting up the goniometer device and measuring the joint movement. Based on the experience of the clinician, or other person, the goniometer device may be attached onto different locations on the patient, which can affect the accuracy and reproducibility of the measurements. The accuracy of the repeated measurements may also be compromised due to issues with or the sensitivity of the device.

SUMMARY

Exemplary implementations of a system for measuring an angle of a joint of a user are disclosed. The system can

2

include a center hub, a first arm, a second arm, a magnet, and a sensor. The center hub includes a first hub and a second hub. The first arm is configured for attachments to a first limb portion of the user at a first outer end and to the first hub at a first inner end. The second arm is configured for attachments to a second limb portion of the user at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub. The magnet is coupled to the second hub. The sensor is disposed in the center hub and configured to detect a rotation of the magnet.

Other implementations of a system for measuring an angle of a joint of a user can include a center hub, first and second coupling apparatuses, and first and second arms. The center hub has a first hub and a second hub. The first arm is configured for attachment to a first limb portion of the user at a first outer end and to the first hub at a first inner end. The second arm is configured for attachment to a second limb portion of the user at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub and configured to rotate 360 degrees about an axis. The system further comprises a magnet, a printed circuit board (PCB), and a sensor. The magnet is coupled to the second hub. The PCB is removably disposed in the center hub. The sensor is coupled to the PCB and configured to detect a rotation of the magnet.

BRIEF DESCRIPTION OF THE DRAWINGS

The disclosure is best understood from the following detailed description when read in conjunction with the accompanying drawings. It is emphasized that, according to common practice, the various features of the drawings are not to scale. On the contrary, the dimensions of the various features are arbitrarily expanded or reduced for clarity.

For a detailed description of example embodiments, reference will now be made to the accompanying drawings in which:

FIGS. 1A and 1B are perspective views of a wearable device for measuring and recording movement in accordance with aspects of the present disclosure.

FIGS. 2A and 2B are top and bottom perspective views of a goniometer in accordance with aspects of the present disclosure.

FIGS. 3A and 3B are top and side views of a goniometer in accordance with aspects of the present disclosure.

FIG. 4 is an exploded view of a goniometer in accordance with aspects of the present disclosure.

FIGS. 5A-C are side views of the goniometer with its arms rotating in accordance with aspects of the present disclosure.

FIG. 6 is a perspective view of the goniometer with its arms twisting in accordance with aspects of the present disclosure.

FIGS. 7A-D are top schematic views of the attachment in accordance with aspects of the present disclosure.

FIGS. 8A-D are views of an attachment in accordance with aspects of the present disclosure.

FIGS. 9A-D are views of first and second layers of the attachment in accordance with aspects of the present disclosure.

FIGS. 10A-D are views of a pod of the attachment in accordance with aspects of the present disclosure.

FIGS. 11A and 11B are perspective and cross-sectional views of a coupling apparatus in accordance with aspects of the present disclosure.

FIGS. 12A and 12B are perspective views of the attachment and a goniometer attachment in accordance with aspects of the present disclosure.

FIG. 13 is a cross sectional view of the goniometer in accordance with aspects of the present disclosure.

FIGS. 14A-C are perspective and top views of a center hub of the goniometer closed, open, and with components removed in accordance with aspects of the present disclosure.

FIGS. 15A and 15B are top and bottom views of a printed circuit board (PCB) in accordance with aspects of the present disclosure.

FIGS. 16A and 16B are graphs illustrating test data in accordance with aspects of the present disclosure.

FIG. 17 is a perspective view of the alignment device, with the alignment device shown aligned relative to the center of the joint of the user.

FIG. 18 is a perspective view of the user illustrating the markings on the skin of the user at the center of the joint, and on the opposing limb portions.

FIG. 19 is a perspective view illustrating the attachments being aligned with the markings on the opposing limb portions.

FIG. 20 is a perspective view illustrating the wearable device being coupled to the attachment, and aligned relative to the center of the joint.

FIG. 21 is a perspective view illustrating an alternative embodiment of the alignment device, and illustrating the light beams at the center of the joint and on the opposing limb portions, which are configured to assist the clinician in aligning the attachments and wearable device relative to the center of the joint.

FIG. 22 is a perspective view illustrating yet another alternative embodiment of the alignment device, and illustrating the diodes at the center of the joint, on the opposing limb portions, and on the wearable device.

FIGS. 23A-23E are various views of an embodiment of a pedometer that may be coupled to the goniometer.

FIG. 24 is a plan view of another embodiment of an alignment device.

FIGS. 25-34 are schematic sequential images of an embodiment of alignment and installation method.

NOTATION AND NOMENCLATURE

Various terms are used to refer to particular system components. Different companies may refer to a component by different names—this document does not intend to distinguish between components that differ in name but not function. In the following discussion and in the claims, the terms “including” and “comprising” are used in an open-ended fashion, and thus should be interpreted to mean “including, but not limited to . . .” Also, the term “couple” or “couples” is intended to mean either an indirect or direct connection. Thus, if a first device couples to a second device, that connection may be through a direct connection or through an indirect connection via other devices and connections.

The terminology used herein is for the purpose of describing particular example embodiments only, and is not intended to be limiting. As used herein, the singular forms “a,” “an,” and “the” may be intended to include the plural forms as well, unless the context clearly indicates otherwise. The method steps, processes, and operations described herein are not to be construed as necessarily requiring their performance in the particular order discussed or illustrated,

unless specifically identified as an order of performance. It is also to be understood that additional or alternative steps may be employed.

The terms first, second, third, etc. may be used herein to describe various elements, components, regions, layers and/or sections; however, these elements, components, regions, layers and/or sections should not be limited by these terms. These terms may be only used to distinguish one element, component, region, layer or section from another region, layer or section. Terms such as “first,” “second,” and other numerical terms, when used herein, do not imply a sequence or order unless clearly indicated by the context. Thus, a first element, component, region, layer or section discussed below could be termed a second element, component, region, layer or section without departing from the teachings of the example embodiments. The phrase “at least one of,” when used with a list of items, means that different combinations of one or more of the listed items may be used, and only one item in the list may be needed. For example, “at least one of: A, B, and C” includes any of the following combinations: A, B, C, A and B, A and C, B and C, and A and B and C. In another example, the phrase “one or more” when used with a list of items means there may be one item or any suitable number of items exceeding one.

Spatially relative terms, such as “inner,” “outer,” “beneath,” “below,” “lower,” “above,” “upper,” “top,” “bottom,” and the like, may be used herein. These spatially relative terms can be used for ease of description to describe one element’s or feature’s relationship to another element(s) or feature(s) as illustrated in the figures. The spatially relative terms may also be intended to encompass different orientations of the device in use, or operation, in addition to the orientation depicted in the figures. For example, if the device in the figures is turned over, elements described as “below” or “beneath” other elements or features would then be oriented “above” the other elements or features. Thus, the example term “below” can encompass both an orientation of above and below. The device may be otherwise oriented (rotated 90 degrees or at other orientations) and the spatially relative descriptions used herein interpreted accordingly.

DETAILED DESCRIPTION

The following discussion is directed to various embodiments of the invention. Although one or more of these embodiments may be preferred, the embodiments disclosed should not be interpreted, or otherwise used, as limiting the scope of the disclosure, including the claims. In addition, one skilled in the art will understand that the following description has broad application, and the discussion of any embodiment is meant only to be exemplary of that embodiment, and not intended to intimate that the scope of the disclosure, including the claims, is limited to that embodiment.

In accordance with aspects of the present disclosure, FIGS. 1A and 1B illustrate an exemplary system or wearable device 100 for measuring and recording flexion and extension at a joint 107 of a user 102. The wearable device 100 comprises first and second coupling apparatuses, or attachments, 112, 114, 118, 120 (hereinafter referred to as first and second attachments 118, 120) and may be configured to be removably coupled to the user 102 at opposing limb portions 104, 106 of the joint 107. For example, and as illustrated in FIGS. 1A and 1B, the first and second attachments 118, 120 may be coupled to a leg of a user at opposing limb portions 104, 106, e.g., thigh 104, and calf 106, of the knee or joint 107 of the user 102. As will be appreciated by those of skill

5

in the art, the first and second attachments **118, 120** may be coupled to the user at opposing limb portions of any other joint of a patient or user **102**. It is further contemplated that the wearable device **100** may be utilized for measuring flexion and extension of joints in animals, a joint of a robot, or any other desired joint or joint equivalent.

To position the wearable device **100** relative to the joint **107**, a person, such as a clinician, may identify a joint center **108**, where the joint center **108** may be used to align the wearable device **100** to the joint **107**. The clinician may use an alignment device **300** to identify and mark the joint center **108**. For example, the alignment device **300** may be used to mark the skin of the user **102** at the joint center **108** with a marker, pen, or any other desired tool. Further, the alignment device **300** may be used to identify and mark positions at opposing limb portions **104, 106** for the first and second attachments **118, 120** relative to the joint center.

With reference to FIGS. 2A-6, the wearable device **100** comprises an exemplary device or apparatus **110**, such as a goniometer. Hereinafter, the device or apparatus **110** may be referred to as a goniometer **110**. The goniometer **110** is configured to measure the angular flexion and extension at the joint **107** of the user **102**. The goniometer **110** has a top **122**, a bottom **124**, and opposing sides **126**. The goniometer **110** may comprise a center hub **116** aligned coaxially with an axis A, and first and second arms **128, 130**, wherein the arms **128, 130** couple to, and are rotatable about, the axis A and the center hub **116**. More specifically, first and second inner ends **132, 134** of the respective arms **128, 130** couple to the center hub **116**. The arms **128, 130** extend outwardly from the center hub **116** to respective first and second outer ends **168, 170**. In an alternative embodiment, the arms **128, 130** may be integrally formed with the center hub **116**. Embodiments of the goniometer can enable various rotational or pivotal motions, such as with an axle, a rack and pinion system, etc.

With reference to FIGS. 3A and 3B, the goniometer **110** can have a length L that extends from the first outer end **136** to the second outer end **138**. The length L can vary depending on the relative position of the first and second arms **128, 130**. For example, a maximum length L of the goniometer **110** may be measured when the arms **128, 130** are positioned opposing one another. Whereas, when the arms **128, 130** are positioned parallel, and respectively directly above and below one another, a minimum length L of the goniometer **110** may be measured between the outer ends **136, 138** to an opposite side of the center hub **116**. A width W of the goniometer may be measured as a diameter of the center hub **116**. Further, a height H of the goniometer **110** may be measured from a bottom of the second arm **130** to a top of the first arm **128**, or to a top of the center hub **116**, whichever is greater.

In an exemplary embodiment, the center hub **116** comprises a first or upper hub **146** and a second or lower hub **148**. The hubs **146, 148** are coaxially aligned with one another, and with axis A. Moreover, the hubs **146, 148** may be configured to rotate about the axis A for 360 degrees, and relative to one another. Further, each of the hubs **146, 148** may have a link arm **143** for coupling between the hubs **146, 148** and the respective arms **128, 130**. For example, the first arm **128** may be coupled to the link arm **143** of the first hub **146**, and the second arm **130** may be coupled to the link arm **143** of the second hub **148**.

In operation, embodiments of the arms **128, 130** may rotate, pivot, flex or extend relative to the center hub **116**. This design can account for the complex motion of a joint, slippage of the joint, and the broad range of shapes and sizes

6

of the patient's joint **107**. In addition, this design can maintain the position of the center hub relative to the joint center **108**. Embodiments of the device can enable freedom of motion in many planes but not in the rotational plane of the joint. This enables the device to fit many different people but still make accurate measurements.

More specifically, and as best illustrated in FIG. 4, the first and second arms **128, 130** may each include an inner link **142** disposed adjacent to the respective inner ends **132, 134**, and an outer link **144** disposed between the inner link **142** and the outer ends **168, 170**. With reference to FIGS. 5A-C, the inner link **142** may couple to the link arm **143** in order to couple between respective arms **128, 130** and hubs **146, 148**. The inner link **142** may be configured to facilitate the pivot, flex, or extension of the respective arm **128, 130** relative to the center hub **116**. A pin **164** may be used to couple the inner link **142** and the link arm **143** of each arm **128, 130** to allow for the pivot, flexion, or extension of the respective arms **128, 130**. The pin **164** may be disposed perpendicular to the length of the arms **128, 130**.

The outer link **144** may couple to the inner link **142** and respective outer ends **136, 138**. With reference to FIG. 6, the outer link **144** may be configured to couple to the inner link **142** to facilitate rotation of the respective arms **128, 130** relative to the center hub **116**. A screw **162** may be configured to couple the outer link **144** to the inner link **142** to facilitate rotation of the respective arms **128, 130** about the screw **162**, all relative to the center hub **116**. The screw **162** may align parallel with the length of the respective arm **128, 130**. It is to be appreciated that the first and second arms **128, 130** may rotate $\pm$ -eighteen degrees, or any other desired amount, in one or more directions. Further yet, and with reference to FIGS. 5A-C, the outer link **144** may be configured to couple to the respective outer ends **136, 138** to facilitate further pivot, flexion, or extension of the respective arms **128, 130** relative to the center hub **116**. A pin **164** may be used to couple the outer link **144** and the respective outer ends **136, 138** to allow for further pivot, flexion, or extension, of the respective arms **128, 130** relative to the center hub **116**. The pin **164** may be disposed perpendicular to the length of the respective arms **128, 130**.

The first and second outer ends **136, 138** may comprise first and second goniometer attachments **168, 170**, which may be integral with, or coupled to the respective outer ends **136, 138**. It is to be appreciated the goniometer attachments **168, 170** may couple, or be integral with, the arms **128, 130** at any desired location, or in any desired configuration. The first and second goniometer attachments **168, 170** may be configured to removably couple with the attachments **118, 120**. Further, each goniometer attachment **168, 170** can comprise one or more bosses **200**, and one or more magnets **158** positioned next to the bosses **200** to facilitate the coupling and alignment of the goniometer attachments **168, 170** and the attachments **118, 120**. The bosses **200** and magnets **158** further facilitate the alignment of the goniometer **110** relative to the attachments **118, 120**. The arms **128, 130** may also include one or more arm alignment holes **140** configured to align with the attachments **118, 120**, or an alignment mark on a user **102**. The arms **128, 130** may further have one or more wings **202** that extend from a side **126** of the goniometer **110**, such as from the first or second goniometer attachments **168, 170**. The wings **202** can be formed from or coupled to the first or second goniometer attachments **168, 170**. The wings **202** can be a tab or have any other desired shape. The wings **202** may be configured to assist a user in moving the arms **128, 130** of the goniometer perpendicularly relative to the attachments to facili-

tate uncoupling the goniometer 110 from the attachments 118, 120 without uncoupling the attachments 118, 120 from the user 102.

With reference to FIGS. 7-9, the attachments 118, 120 may comprise first and second layers 172, 174 and a pod 176 coupled together with one another. When coupled to one another, each of the layers 172, 174 and the pod 176 may be concentric with one another. The first attachment 118 may be the same as and interchangeable with the second attachment 120. The first layer 172, the second layer 174, and the pod 176 may be generally oval-shaped or any other desired shape. The first layer 172 may be larger than the second layer 174, and the second layer 174 may be larger than the pod 176. Further, the first layer 172 may be thinner than the second layer 174, and the pod 176 can be thicker than the first and second layers 172, 174.

The first layer 172 may have a top 182 and a bottom 184, and may be formed from a pad, coated paper, plastic, woven fabric, latex, or any other desired material. For example, the top 182 may be formed from a pad and the bottom 184 may comprise an adhesive material 236, such as a medical-grade adhesive or other suitable material. The adhesive material 236 couples to the skin of the user 102 to couple the attachments 118, 120 to the user 102. Further, the top 182 may also have an adhesive layer 194, which may be smaller in area than the first layer 172. Further, the adhesive layer 194 can be less than or equal to the area of the second layer 174. The adhesive layer 194 may be ovular in shape, and define one or more notches or voids in an outer periphery. Further, the first layer 172 can define notches 180 in an outer periphery for assisting in aligning the first attachment 118 relative to a predetermined location, or mark, on the user 102. The notches 180 can be v-shaped or have any other desired shape. Further yet, the first layer 172 may define a pair of voids or alignment holes 178, which may assist in the alignment of the first attachment 118 relative to a predetermined location, or mark, on the user 102. The alignment holes 178 and notches 180 of the first layer 172 may be the same as, or aligned with, the notches or voids of the adhesive layer 194.

The second layer 174 may have a top 186 and a bottom 188, and may be formed of a foam material or any other desired material. The second layer 174 may couple to the adhesive layer 194 of the first layer 172. To prevent uncoupling, the foam material of the second layer 174 may dampen forces between the goniometer 110 and the attachments 118, 120. The top 186 of the second layer 174 may also have an adhesive layer 195 on an upper surface 238 of the top 186, which may be smaller in area than the area of the pod 176. The adhesive layer 195 may have an ovular shape, or any other desired shape. Further, the adhesive layer 195 and the second layer 174 may have one or more holes, or one or more cutouts that may be aligned with the alignment hole 178 of the first layer 172 to align the adhesive layer 195 and the second layer 174 with the first layer 172. The adhesive layers 194, 195 can be formed of an adhesive material or any other desired coupling material, such as a hook- or a loop-type material. The first layer 172 can have a length L1 and a width W1. The second layer 174 can have a length L2 and a width W2. The adhesive layer 195 can have a length L3 and a width W3.

As illustrated in FIGS. 10A-D, the pod 176 has a top 190 and a bottom 192. The pod 176 can include one or more notches 196. For example, notches 196 can be located at opposing ends of the pod 176. The notches 196 can be used for alignment of the first coupling apparatus 112, the pod 176, or any other desired feature of the wearable device 100.

The pod 176 can include one or more magnets 160. The magnet 160 may be a neodymium magnet or any other desired magnet. The pod 176 can have a recess for housing the magnet 160. The magnet 160 can be circular or any other desired shape. Two magnets 160 can be disposed in the pod 176 at opposing ends of the pod 176. The pod 176 can be sized to be received by and detachably coupled to the upper surface 238 of the second layer 174.

More specifically, the pod 176 has an underside, such as the bottom 192, which may couple to the upper surface 238 of the second layer 174. The bottom 192 can have one or more hooks or loops, to couple to the upper surface 238. Alternatively, the upper surface 238 and the bottom 192 may comprise an adhesive material to facilitate the detachable coupling between the upper surface 238 and the pod 176. The top 190 of the pod 176 may have one or more recesses 198. The recess 198 may be ovular in shape or have any other desired shape. The recesses 198 may also have tapered edges to assist a user 102 in uncoupling from the pod 176 by moving the arms 128, 130 perpendicularly relative to the pod 176. Two recesses 198 may be formed in the pod 176 at opposing ends or sides of the pod 176.

With reference to FIGS. 11-12, the recesses 198 are sized to receive the bosses 200 to align the goniometer 110 relative to the attachments 118, 120. Moreover, the recesses 198 are sized to allow slight movement of the bosses 200 to compensate for slight translational movement of the joints 128, 130 while the goniometer 110 is worn by the user 102. This movement may reduce the stress between, and prevent uncoupling of, the attachments 118, 120 to the skin, clothing, brace, or any other desired location on the user 102.

When the user 102 moves the first or second limb portions 104, 106, the first or second arms 128, 130 move or rotate with the first and second hubs 146, 148. The goniometer 110 can measure the rotation of joint 107 by measuring the angle between the first and second hubs 146, 148. To achieve this, and with reference to FIGS. 4, 13-15, the center hub 116 defines an opening for receiving and containing a printed circuit board (PCB) 152, a sensor 216, a retaining ring 154, a magnet 156, or any other components of the goniometer 110 which cooperate with one another to measure relative angular movement between the arms 128, 130. More specifically, the first and second hubs 146, 148 may define the opening of the center hub 116.

For enclosing the opening, a cover 150 may be attached to the center hub 116, and more specifically to the first hub 146. The cover 150 can be detachably coupled to the first hub 146 or any other desired location. The cover 150 can also be configured to inhibit movement of the PCB 152 and other components located within the center hub 116. For example, when the cover is closed, a bottom portion of the cover 150 may apply direct or indirect pressure to the PCB 152. The cover 150 may have a snap mechanism 226, such as a finger snap or any other desired mechanism, configured to attach and detach the cover to the center hub 116.

The magnet 156 may couple to the second hub 148, and the sensor 216 also disposed in the center hub 116 is configured to detect rotation of the magnet 156. The sensor 216 can be configured to measure the rotation of the magnet 156 to a sensitivity up to one-hundredth of a degree, or to any other desired sensitivity.

As illustrated in FIGS. 13-14C, the center hub 116 includes the first hub 146 positioned rotatably above the second hub 148. An outward notch 208 may be coupled to the first hub 146, or any other desired location. The outward notch 208 may be formed with the first hub 146 or attached to the first hub 146. The PCB 152 may be removably

disposed in the center hub **116**. The PCB **152** may have an inward notch **210**. The outward notch **208** may be configured to couple with the inward notch **210** to align the sensor **216** and the magnet **156**. The alignment can restrict movement of the PCB **152** within the center hub **116**.

When the cover **150** is removed, the PCB **152** may be accessed. FIG. **14B** illustrates a battery housing **206** coupled to the PCB **152**. The battery housing **206** may be attached to a top side **212** of the PCB **152**. The battery housing **206** may be formed of conductive metal or any other desired material. When the cover **150** is attached to the first hub **146**, the cover **150** may apply pressure to the battery housing **206**, which may secure PCB **152** within the center hub **116**. A battery **204** may be detachably coupled to the battery housing **206**. The battery **204** may be a lithium ion battery or any other desired battery or power source. The battery housing **206** may have tabs or any other desired contact points for conduction with the battery **204**. The battery **204** may be removed from the battery housing **206** to turn the goniometer **110** off or for replacement of the battery **204**. For example, when the cover **150** is opened or removed from the first hub **146**, the PCB **152** may be removed from the center hub **116** and the battery **204** may be replaced. To maintain calibration of the goniometer **110** after a battery replacement, the inward notch **210** of the PCB **152** is configured for receiving the outward notch **208** of the first hub **146**.

In FIG. **14C**, the cover **150** and the PCB **152** are removed from the center hub **116**. As shown, the second hub **148** may include a magnet housing **224**. The magnet housing **224** may be located in the center of the second hub **148** or any other desired location. The magnet housing **224** may be coupled to the PCB **152** using a weld, an adhesive, a tack, or any other desired attachment. The magnet housing **224** may be configured to receive the magnet **156**. The magnet **156** may be configured to have north and south polarity within the center hub **116** or any other desired polarity. The magnet housing **224** may include a lip at a top of the magnet housing **224** or have any other desired configuration. The retaining ring **154** may be configured to couple the magnet **156** to the second hub **148**. The retaining ring **154** may be coupled to the second hub **148** around the magnet housing **224**. For example, the retaining ring **154** may be positioned between the lip or top of the magnet housing **224** and the second hub **148**. The retaining ring **154** may secure the magnet within the magnet housing **224**. The retaining ring **154** may move with the second hub **148** and the magnet **156** as the second hub **148** rotates with the second arm **130**.

FIG. **15A** illustrates the top side **212** of the PCB **152**. As described above, the battery housing **206** may be attached to the top side **212**. FIG. **15B** illustrates a bottom side **214** of the PCB **152** in accordance with aspects of the present disclosure. The PCB **152** includes components coupled to the bottom side **214**. The components may comprise a circuit **220** including resistors, LEDs, transistors, capacitors, inductors, transducers, diodes, switches, the sensor **216**, a transmitter **222**, or any other desired component. The components may be attached to the PCB **152** using a surface mount method, a through-hole method, or any other desired method. The PCB **152** may include additional and/or fewer components and is not limited to those illustrated in FIGS. **15A** and **B**.

The circuit **220** may be configured to generate an electrical signal based on the rotation of the magnet **156**. The circuit **220** may be configured to transmit the electrical signal in real time. The circuit **220** may transmit the electrical signal. For example, a transmitter **222** may be coupled to the PCB **152** and configured to transmit an electrical

signal based on the rotation of the magnet **156** to an external device. The transmitter **222** may include wired or wireless transmission, such as Bluetooth™, WiFi, NFC or any other means or method of desired transmission. The external device may be a mobile phone, a computer, a tablet, or any other desired device. The external device may have a user interface. The user interface may be configured to receive the electrical signal and display data obtained from the electrical signal. The data may include the angle of the joint **107**, or any other desired information.

The user interface may include an app that receives the data, manipulates the data, records the data, and displays aspects of the data. For example, the app may display the angle of the joint **107** of a user **102**, a history of the angle of the joint **107**, duration of the angle, or any other desired information, such as a measurement of the angle in real time.

The sensor **216** may be a Hall Effect sensor, or any other desired sensor (e.g., a magnetic position sensor AS5601 using internal MEMS Hall Effect sensors). The sensor **216** may be coupled to the PCB **152** or any other desired device. The sensor **216** may be coupled to the bottom side **214** of the PCB **152** at a location directly above the magnet **156** when the PCB **152** is disposed within the center hub **116**. The PCB **152** and the sensor **216** may rotate with the first hub **146** and the first arm **128**. The magnet **156** may rotate with the second hub **148** and the second arm **130**. The design of the wearable device **100**, including the configuration of the sensor **216** and the magnet **156**, may improve the accuracy of the measurements of the angle of the joint **107**.

FIG. **16A** is an exemplary graph **228** with line **232** depicting, while the wearable device **100** is attached to the user **102**, the accuracy of measurements of angles of the joint **107** by the wearable device **100**. FIG. **16B** is an exemplary graph **230** with line **234** depicting the accuracy of measurements of angles of the joint **107** by a different measurement device attached to a user using Velcro™ straps. The standard deviation of the measurements made by the different measurement device shown by line **234** is greater than the standard deviation of the measurements made by the wearable device **100** shown by line **232**. Users, such as clinicians or patients, are able to more accurately initially place and realign the first and second attachments **118** and **120** of the wearable device **100** as compared to using the Velcro™ straps. The configuration of the first and second arms **128**, **130** of the wearable device **100** to fit different users may increase accuracy of the measurements. The configuration of the components, including the PCB **152**, the sensor **216**, and the magnet **156** within the center hub **116** of the wearable device **100** may further increase accuracy of the measurements. The wearable device **100** may be configured to measure the angle of the joint **107** up to an accuracy of measurement up to a one hundredth degree. The different measurement device may have an accuracy up to five degrees. In other words, the measurements taken by the different measurement device may have an accuracy of about $\pm$ five degrees, such as about $\pm$ 11 degree, or even $\pm$ about 0.01 degree from the actual angle of the joint **107**.

With reference to FIGS. **17** and **18**, the alignment device **300** may be used to assist a clinician to align the wearable device **100** (see FIG. **20**) on opposing limb **104**, **106** portions of the joint **107** of the user **102** relative to a center of the joint **107**. Properly aligning the wearable device **100** relative to the joint **107** facilitates greater accuracy and precision of the measurements made with the wearable device **100**. Hence,

11

the need for a device, such as alignment device **300**, to assist in aligning the wearable device **100** relative to the joint **107** of a patient **102**.

The alignment device **300** comprises a first segment **302** and a second segment **304** pivotably coupled to the first segment **302** at a pivot point **P**. More specifically, the segments **302**, **304** each have a coupling end **306** where the segments **302**, **304** pivotably couple to one another at the pivot point **P**. Moreover, the pivot point **P** is spaced adjacently and equidistant from each coupling end **306** of the segments **302**, **304**. Further yet, when the segments **302**, **304** are pivotally coupled, center axes **C** of each segment **302**, **304** intersect at the pivot point **P**.

The alignment device **300** further includes voids **308** defined by each segment **302**, **304**, and the voids **308** facilitate the marking of the skin of the user **102** during use of the alignment device **300**. The voids **308** are spaced equidistant on each segment **302**, **304** from the pivot point **P**, and the spacing between, and size, of each void **308** is commensurate with the spacing between, and size, of each alignment hole **178** of the attachments **118**, **120** (see FIGS. **19** and **20**). Further yet, when the attachments **118**, **120** are coupled to the goniometer attachments **168**, **170**, the spacing between, and position of, each void **308** and the pivot point **P** is commensurate with the spacing between the center hub **116** and the alignment holes **178** of the attachments **118**, **120**.

Using the alignment device **300**, the clinician may locate the center of the joint **107** of the user **102**, and then position the pivot point **P** at the center of the joint **107**. When the joint **107** of the user **102** is a knee, the clinician may locate the lateral epicondyle of the knee, and position the pivot point **P** adjacent to the lateral epicondyle. With the pivot point **P** positioned adjacent to the lateral epicondyle, the clinician may centrally position each segment **302**, **304** adjacent to the opposing limb portions **104**, **106** of the joint **107**. The clinician may rely on the center axes **C** of each segment **302**, **304** to assist in centrally aligning with the segments **302**, **304** to the opposing limb portions **104**, **106**. With reference to FIGS. **17** and **18**, with the segments **302**, **304** centrally aligned with the opposing limb portions **104**, **106**, the clinician may use the voids **308** to mark the skin of the user **102**. Thereafter, and with reference to FIGS. **19** and **20**, the clinician may coaxially align the alignment holes **178** of the attachments **118**, **120** with the markings on the skin of the user **102** to facilitate the alignment, and coupling to the user **102**, of the wearable device **100** relative to the center of the joint **107**. Further, the clinician may use pegs to assist in aligning with the attachments **118**, **120** coaxially with the marks.

Alternatively, and with reference to FIGS. **21** and **22**, an alignment device **400** may be used to assist a clinician to facilitate the alignment of the wearable device **100** relative to a center of the joint **107** of the user. More specifically, alignment device **400** may rely on data from an imaging device **402** of the joint **107** to assist the clinician in positioning the wearable device **100** on the user **102**. The imaging device **402** may be an x-ray, ultrasound, any other imaging device capable of providing image data in 2D, 3D or 4D to the alignment device **400**, or any other imaging device. A processor **404** of the alignment device **400** receives and processes the image data from the imaging device **402**, and the processor **404** facilitates communication from the alignment device **400** to the clinician for the proper positioning of the attachments **118**, **120**, or the wearable device **100**.

In one embodiment, and with reference to FIG. **21**, the alignment device **400** may include one or more lasers **406**

12

that produce a light beam. In this embodiment, the processor **404** may communicate with the lasers **406** to cause the lasers **406** to be positioned such that light beams causes spots of light on the skin of the user **102** on the center of the joint **107** and on opposing limb portion **104**, **106**. The spacing between, and size of, the spots of light are commensurate with the spacing between, and size of, each alignment hole **178** of the attachments **118**, **120**. The clinician may rely on the spots to align the wearable device **100** to center of the joint **107**. Alternatively, the clinician may mark the locations of the spots of light on the skin, similar to the markings used with alignment device **300**, and rely on the markings to align the wearable device **100** to the center of the joint **107**. Further yet, the wearable device **100** may have indicia which the clinician may align with the light beams to facilitate alignment of the wearable device **100**. In yet another alternative, the light beam may create an outline of the wearable device **100** on the skin of the user **102**, where the outline may be commensurate to a perimeter of the wearable device, and may be used to properly align the wearable device **100** to the center of the joint **107**.

In another embodiment of the alignment device **400**, and with reference to FIG. **22**, to assist the clinician in aligning the wearable device **100** relative to a center of the joint **107** of the user **102**, the imaging device **402** may communicate with diodes **408** positioned on the user **102** and/or the wearable device **100**. The diodes **408** may provide position data to the processor **404** such that the processor **404** may communicate with, and position, the lasers **406** to assist the clinician in the positioning of the attachments **118**, **120**. Alternatively, with the position data of the diodes **408**, the processor **404** may communicate, to the clinician, with a clinician communication device **410**, to assist in the alignment of the wearable device **100**. Further yet, the wearable device **100** may also have diodes **408**, which may communicate with the imaging device **402**. Relying on position data of the diodes **408** from the imaging device **402**, the processor **404** may cause the speaker **412** or the display **414** to provide respective audio or image outputs to communicate instructions, to the clinician, to facilitate the alignment of the wearable device **100**. For example, the speaker **412** may provide audio guidance to the clinician, such as "move wearable device 5 mm to the left," to assist in the positioning of the wearable device **100**. In another example, the display **414** may provide visual guidance to the user **102** on the location of the wearable device **100**, and instructions for adjusting its position to achieve proper alignment. The display **414** may be a monitor, or iPad, or any other device for providing an image to the user, such as 3D googles. Of course, any of the above techniques could be used in combination with one another to assist the clinician to properly align the wearable device **100**.

FIGS. **23A-23E** depict an embodiment of an ambulation monitor or pedometer **1701**. Versions of the pedometer **1701** can count the number of steps that a user takes, such as a daily count of steps post-operatively. Such a device can be carried by the user or attached to the user or to a peripheral of the user, such as the goniometer **110**. The pedometer **1701** is operational to track steps of the user even if the user requires a walker or other assistance device.

In some versions, the pedometer **1701** can include the ability to attach to the magnets of the goniometer **110** to ensure accurate tracking of all steps of the user. The pedometer **1701** can include metallic elements that are magnetically attracted to the magnets of the goniometer **110**. Alternatively, additional magnets **1703** mounted to the pedometer **1701**. Embodiments of the pedometer **1701** can further

13

include a body 1705, a removable cap 1707, a circuit board 1709 including one or more sensors (e.g., a motion sensor such as an accelerometer, mechanical sensor or other electromechanical sensor), a battery 1711 and fasteners 1713.

FIG. 24 is a plan view of another embodiment of an alignment device 1300. Alignment device 1300 can be used in manners that are similar to the previously described alignment devices.

FIGS. 25-34 are schematic sequential images of an embodiment of alignment and installation method. As shown in FIG. 25, the patient or user can change their own pods 176. Alternatively, another person can help the user change their pods 176. Although these images are shown for the user's right leg, the actions are mirrored for the user's left leg.

Before either pod 176 is removed (FIG. 26), a permanent ink marker can be used to mark the user's skin with four marks (e.g., triangles) inside the four V-shaped notches on each of the user's current pods 176. A total of eight triangular marks can be made, including four marks on the pod attached to the user's upper leg and four marks on the pod attached to the user's lower leg. These marks can be used to correctly position the new pods 176.

Starting at the edge of one of the pods 176 (FIG. 27), the adhesive portion of the pod can be gently peeled away and off of the user's skin. Repeat for the second pod 176, and discard both of the old pods 176. After removing both old pods 176 from the user's skin (FIG. 28), the user can wait 24 hours before putting on new pods 176. This gives the skin time to "air out" and restore itself after being covered for a week. The area may be cleaned with mild soap to avoid removal of the ink markings. If one or more of the markings are fading, they can be re-marked before they disappear entirely.

In FIG. 29, the area is cleansed with a simple hand soap, rinsed and dried. In FIG. 30, two new pods 176 are removed from their packaging and correctly oriented such that the "1" tab is pointing toward the center of the user, and the "2" tab is pointing outward away from the user. In FIG. 31, the V-notches in the pod are aligned with the triangles drawn on the user's upper leg. The same hand as the leg working on is used to hold the center of the pod 176 onto the leg so that the V-notches are aligned with the triangle marks. With the other hand, the tab "1" is gently pulled to expose the adhesive on the back of the pod 176. The center of the pod 176 is kept in place as the backing paper is removed. Once the "1" backing paper is removed, the adhesive flap is rolled down so that it sticks to the skin smoothly and without getting wrinkled. The V-notches should still be aligned with the triangle marks. The adhesive is gently pressed onto the skin, making sure it has fully adhered to the skin. Next, the "2" tab is removed from the rest of the backing paper. The rest of the adhesive is rolled onto the skin. The entire adhesive can be smoothed to make sure it has fully adhered to the skin.

In FIG. 32, another pod 176 is oriented on the lower leg so that the "1" tab is pointing toward the center of the body and the "2" tab is pointing away from the body. Next, the V-notches in the pod are aligned with the triangle marks drawn on the lower leg. Using the same hand as the leg being worked on, the center of the pod 176 is held onto the leg so that the V-notches are aligned with the triangle marks. With the other hand, the "1" tab is removed to expose the adhesive on the back of the pod 176. The center of the pod 176 should be held in place as the backing paper is removed. Once the "1" tab backing paper is removed, the adhesive flap is rolled down so that it sticks to the skin smoothly and without

14

getting wrinkled. The V-notches should still be aligned with the triangle marks. Gently press the adhesive onto the skin, making sure it has fully adhered to the skin. The "2" tab is gently removed to roll the rest of the adhesive onto the skin. Smooth down the entire adhesive to make sure it has fully adhered to the skin.

The fingertips can be used to flatten the edges of the adhesive fully against the skin (FIG. 33). Rub gently to increase adhesion for both pods 176. The pods 176 are now changed and the goniometer 110 is ready to attach to the user. Hold the goniometer 110 close to the magnets on the pods 176 and let them snap into place via the magnets. Positioning of the pods 176 can be checked by attaching the goniometer 110 and flexing the leg (FIG. 34). If the goniometer 110 pops off of one or both of the pods 176, the detached pod 176 has been re-applied too far from the correct position. Check to see if any V-notches are not well aligned with the triangle marks on the skin. If this is the case, remove that pod 176 and reapply a new pod 176, making sure it is aligned more closely to the triangle marks on the skin.

Pod Function

A pair of truncated pull tab pod assemblies, one adhered to the upper leg, and one to the lower leg, act as anchors to the ends of the goniometer, which measures the angle of the knee over the course of the patient's sessions. Although the goniometer is removed between sessions, the pair of pods are to be left in place for about a week. Once a week, the patient or caregiver replaces the first set of pod assemblies with new pod assemblies. Repeat weekly. Location targets marked on the legs can be "refreshed" by the patient to provide for repeatable placement locations for each new pair of pod assemblies. The "semi-continuous" measurement anchor points provided by the pods allow for a reliable assessment of range of motion over the duration of the therapy.

Pod Description

The pod assembly can include three basic layers. The bottom layer can be highly compliant, hypoallergenic, breathable, and adheres to the skin. The middle layer can be a thin foam that is moderately compliant. The top layer can be a rigid plastic molded part that has locating features and a pair of magnets and is adhered to the middle layer with an adhesive.

Four location notches in the bottom layer can provide for reliable marking of initial pod locations such that subsequent pods can be placed accurately in the same location and orientation. The middle layer can act as a transitional material between the larger, compliant layer and the smaller pod with snaps. Features in the rigid pod can include the top layer as location features to assemble to the goniometer and to the pod template. The magnets, mating with similar magnets in the goniometer, provide the retention force to allow use of the goniometer during a session. Before assembly to the body, the pod comes from the package with two release papers with large pull tabs that cover the adhesive of the bottom layer.

Pod Design Aspects

The pods can be consistent anchor points for the goniometer. When the goniometer is not in place during a session, either the pods can act as attachment points for the goniometer or a pedometer. For the goniometer to provide relevant and reliable range of motion information for clinical use, the pods can be initially located accurately with respect to physiological landmarks and reliably replaced. The pod assembly allows for accurate initial placement and reliable replacement. A combination of novel features and functions

15

in the pod assembly and the alignment assembly allow for these features. Within the pod assembly, the V-notches in allow for accurate replacement of subsequent pods. The asymmetric release paper adhesive backing and large numbered pull tabs allow for the easy location and highly reliable placement and adhesion to the skin. Once the skin is marked with the four targets triangles, the patient can easily locate and orient a new pod by aligning the V-notches to the marked triangles. This “peel-in-place” feature allows for targeting and adhering to be decoupled. Once the first section of the adhesive is revealed and adhered to the skin it acts as an anchor for the following steps. The patient or caregiver can pull the second pull tab and reveal the rest of the adhesive, and can simply smooth the rest of the pod onto the skin with little concern it will be out of place.

Alignment Assembly Function

The alignment assembly allows physiological landmarks of the patient to be used for accurate pods placements for use with the goniometer. The skin over the lateral epicondyle is located and a circular sticker is placed on the patient’s skin or clothing over both the greater trochanter and lateral malleolus. A knee pivot anchor of the alignment assembly can be accurately placed over the lateral epicondyle. The pod is placed with the alignment assembly such that it “points” to either the greater trochanter or lateral malleolus target sticker. Once aligned, the assembly is stabilized and affixed. The process is repeated for other pods as described herein.

Alignment Assembly Description

The alignment arm can be a long chipboard part that has a hole to accept the knee pivot anchor, “pointing” features at the far end to help align with the physiological landmarks, and a hole in the mid-section that aligns to and snaps to features on pods. The distance between these two holes in the template assists in final placement of the pods, and corresponds to hard dimensions in the goniometer. The knee pivot anchor can be a plastic part with a pad of adhesive that snaps into a hole in the end of the template and allows for rotation such that it can be used for both segments of the leg. The center of the anchor can be hollow so that a mark can be placed over the lateral epicondyle. The “skin-side” of the anchor is designed to be flexible, such that the adhesive pad assembled to it can conform to the side of the knee and provide a good adhesion point for use. This part can be removed.

These designs provide accuracy, repeatability, and ease of use for both the patient and the caregiver. The “peel-in-place” release paper design can be superior to the conventional “peel then place” method for the pods. The “mark after placement” method for initial alignment rather than conventional “mark (with a template) then place” method also is an advantage. The release paper can be asymmetric to allow for holding during the first release paper pull. The release paper can use pull tabs to number the release paper in the order of release. In addition to being an ergonomic aid (a “third hand”) for stabilizing the assembly to the leg, the locked pivot point, used for both pod placements insures that the pod-to-pod distance will be well controlled, and within the tolerances of use with the corresponding and highly repeatable goniometer geometry.

Other embodiments can include one or more of the following items or components.

900

A system for measuring an angle of a joint of a user, comprising:

a center hub, the center hub having a first hub and a second hub;

16

a first arm configured for attachment to a first limb portion of the user at a first outer end and to the first hub at a first inner end;

a second arm configured for attachment to a second limb portion of the user at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub;

a magnet coupled to the second hub; and

a sensor disposed in the center hub and configured to detect a rotation of the magnet.

The system further comprising a printed circuit board (PCB) removably disposed in the center hub, the PCB having an inward notch; and an outward notch coupled to the first hub, wherein the outward notch is configured to couple with the inward notch to align the sensor and the magnet.

The system further comprising a cover detachably coupled to the first hub, wherein the cover is configured to inhibit movement of the PCB within the center hub.

The system wherein the sensor is a Hall Effect sensor coupled to the PCB.

The system wherein the sensor is configured to measure the rotation of the magnet up to a precision of about ± 0.01 degree.

The system further comprising a retaining ring configured to couple the magnet to the second hub.

The system wherein the magnet is configured with north and south polarity within the center hub.

The system further comprising a circuit configured to generate an electrical signal based on the rotation of the magnet and to transmit the electrical signal in real time.

The system further comprising a user interface configured to receive the electrical signal and display data obtained from the electrical signal.

The system wherein the data includes the angle of the joint of the user.

The system wherein the first hub and the second hub are configured to rotate 360 degrees about an axis.

A system for measuring an angle of a joint of a user, comprising:

a center hub, the center hub having a first hub and a second hub;

a first arm configured for attachment to a first limb portion of the user at a first outer end and to the first hub at a first inner end;

a second arm configured for attachment to a second limb portion of the user at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub and configured to rotate 360 degrees about an axis;

a magnet coupled to the second hub;

a printed circuit board (PCB) removably disposed in the center hub; and

a sensor coupled to the PCB and configured to detect a rotation of the magnet.

The system further comprising a battery housing coupled to the PCB; and a battery detachably coupled to the battery housing.

The system further comprising a transmitter coupled to the PCB and configured to transmit an electrical signal based on the rotation of the magnet.

The system further comprising a user interface configured to receive the electrical signal and display data obtained from the electrical signal, wherein the data has the angle of the joint of the user.

The system wherein the first and second arms are adhesively attached to respective ones of the first and second limb portions of the user.

17

A system for measuring an angle of a joint of a user, comprising:

- a center hub, the center hub having a first hub and a second hub, wherein the first hub has an outward notch;
- a first and second coupling apparatus configured to be adhesively attached to first and second limb portions proximal to the joint of the user;
- a first arm configured for attachment to a first coupling apparatus at a first outer end and to the first hub at a first inner end;
- a second arm configured for attachment to a second coupling apparatus at a second outer end and to the second hub at a second inner end, wherein the first hub is pivotally coupled to the second hub;
- a magnet coupled to the second hub;
- a printed circuit board (PCB) having an inward notch and removably disposed in the center hub;
- a sensor coupled to the PCB and configured to detect a rotation of the magnet, wherein the outward notch is configured to fit within the inward notch to align the sensor and the magnet; and
- a transmitter coupled to the PCB and configured to transmit an electrical signal based on the rotation of the magnet, wherein the electrical signal has data of the angle of the joint of the user.

The system further comprising a cover coupled to the center hub, wherein the cover has a snap mechanism configured to attach and detach the cover.

The system wherein the first and second arms have sections configured to rotate the first and second arms about $\pm$ -ten degrees.

The system wherein the first and second arms have sections configured to twist the first and second arms about $\pm$ -eighteen degrees.

1000

An apparatus for coupling a device to a user, the apparatus comprising:

- a first layer having a top and a bottom, wherein the bottom comprises an adhesive material configured to couple the device to the user;
- a second layer concentric with the first layer and coupled to the top of the first layer, and the second layer is smaller in size than the first layer and has an upper surface area;
- a pod concentric with the second layer and sized to be received by and detachably coupled to the upper surface area, and the pod is configured to detachably couple the pod to the device.

The apparatus wherein, to prevent the apparatus from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between the device and the apparatus and caused by relative movement between the device and the apparatus.

The apparatus wherein the adhesive material is a medical grade adhesive.

The apparatus wherein the upper surface area comprises one of hooks and loops, wherein the pod has an underside comprised of one of hooks and loops, and wherein the upper surface and the underside are detachably coupled by the hooks and loops.

The apparatus wherein the first layer defines a notch for assisting in aligning the apparatus relative to a predetermined location on the user.

The apparatus wherein the notch is V-shaped.

The apparatus wherein the first layer defines a pair of alignment holes.

18

The apparatus wherein, to facilitate alignment of the apparatus relative to a predetermined location on the user, the upper surface of the second layer comprises an adhesive material to enable detachable coupling between the upper surface and the pod.

The apparatus wherein, when the device couples to the apparatus, the pod defines a recess for positioning and aligning the device relative to the apparatus.

The apparatus wherein the pod comprises a magnet positioned adjacent to the recess to detachably couple the pod to the apparatus.

An apparatus for coupling a device to a user, the apparatus comprising:

- a first layer with a first periphery, and the first layer has a top and a bottom, wherein the bottom comprises an adhesive material configured to couple the apparatus to the user, and the first layer defines a plurality of notches spaced apart from one another and disposed about the first periphery of the first layer, and the first layer defines a pair of alignment holes, and the notches and the alignment holes align the apparatus relative to a predetermined location on the user;
- a second layer smaller in size than, and concentric with, the first layer, and the second layer has a lower surface that couples to the first layer and an upper surface, wherein the upper surface presents an area that comprises an adhesive material;
- a pod concentric with the second layer and sized to be received by and detachably coupled to the area of the upper surface area, and the pod has a magnet to allow the pod to be detachably coupled to the device, and the pod defines a recess for positioning and aligning the device relative to the apparatus when the device couples to the pod.

The apparatus wherein, to prevent the apparatus from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between and caused by relative movement between the device and the apparatus.

An apparatus for measuring flexion and extension of a joint of a user, said apparatus comprising:

- a first attachment and a second attachment, each comprising:
- a first layer with a top and a bottom, wherein the bottom comprises an adhesive material for coupling, on opposite sides of the joint, the attachments to the user;
- a second layer concentric with the first layer, and the second layer has a lower surface that couples to the first layer and an upper surface; and
- a pod concentric with the second layer and detachably coupled to the upper surface; and
- a goniometer for measuring flexion and extension of the joint of the user, and the goniometer is detachably coupled to, and spans between, the pods of the attachments.

The apparatus wherein, to prevent the attachments from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between the goniometer and the attachments and caused by relative movement between the goniometer and the attachments.

The apparatus wherein the goniometer has a pair of arms rotatably coupled to and about a center hub, and each arm has a boss for aligning and coupling each arm to a respective pod.

19

The apparatus wherein each pod defines a recess for receiving and detachably coupling to one of the bosses of the goniometer, and for positioning the goniometer relative to each attachment.

The apparatus wherein, to prevent the goniometer from uncoupling from the attachments, the bosses are sized to be movable within the recesses to allow movement of the bosses in the recesses.

The apparatus wherein, to detachably couple the goniometer to the attachments, magnets are disposed adjacent to each boss and each recess.

The apparatus wherein wings extend outwardly from the sides of each arm of the goniometer configured to enable a user to move the arms of the goniometer perpendicularly relative to the attachments, and to uncouple the goniometer from the attachments.

The apparatus wherein the edges of the pod are tapered, such configuration enabling a user to further move the arms of the goniometer perpendicularly relative to the attachments, and to uncouple the goniometer from the attachments.

1010

An apparatus for coupling a device to a user, the apparatus comprising:

a first layer having a top and a bottom, wherein the bottom comprises an adhesive material configured to couple the device to the user;

a second layer concentric with the first layer and coupled to the top of the first layer, and the second layer is smaller in size than the first layer and has an upper surface area;

a pod concentric with the second layer and sized to be received by and detachably coupled to the upper surface area, and the pod is configured to detachably couple the pod to the device; and

a pedometer configured to count steps of the user and configured to be removably attached to the apparatus.

The apparatus wherein, to prevent the apparatus from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between the device and the apparatus and caused by relative movement between the device and the apparatus.

The apparatus wherein the adhesive material is a medical grade adhesive.

The apparatus wherein the upper surface area comprises one of hooks and loops, wherein the pod has an underside comprised of one of hooks and loops, and wherein the upper surface and the underside are detachably coupled by the hooks and loops.

The apparatus wherein the first layer defines a notch for assisting in aligning the apparatus relative to a predetermined location on the user.

The apparatus wherein the notch is V-shaped.

The apparatus wherein the first layer defines a pair of alignment holes.

The apparatus wherein, to facilitate alignment of the apparatus relative to a predetermined location on the user, the upper surface of the second layer comprises an adhesive material to enable detachable coupling between the upper surface and the pod.

The apparatus wherein, when the device couples to the apparatus, the pod defines a recess for positioning and aligning the device relative to the apparatus.

The apparatus wherein the pod comprises a magnet positioned adjacent to the recess to detachably couple the pod to the apparatus.

20

An apparatus for coupling a device to a user, the apparatus comprising:

a first layer with a first periphery, and the first layer has a top and a bottom, wherein the bottom comprises an adhesive material configured to couple the apparatus to the user, and the first layer defines a plurality of notches spaced apart from one another and disposed about the first periphery of the first layer, and the first layer defines a pair of alignment holes, and the notches and the alignment holes align the apparatus relative to a predetermined location on the user;

a second layer smaller in size than, and concentric with, the first layer, and the second layer has a lower surface that couples to the first layer and an upper surface, wherein the upper surface presents an area that comprises an adhesive material;

a pod concentric with the second layer and sized to be received by and detachably coupled to the area of the upper surface area, and the pod has a magnet to allow the pod to be detachably coupled to the device, and the pod defines a recess for positioning and aligning the device relative to the apparatus when the device couples to the pod; and

a pedometer configured to count steps of the user and configured to be removably attached to the apparatus.

The apparatus wherein, to prevent the apparatus from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between and caused by relative movement between the device and the apparatus.

An apparatus for measuring flexion and extension of a joint of a user, said apparatus comprising:

a first attachment and a second attachment, each comprising:

a first layer with a top and a bottom, wherein the bottom comprises an adhesive material for coupling, on opposite sides of the joint, the attachments to the user;

a second layer concentric with the first layer, and the second layer has a lower surface that couples to the first layer and an upper surface; and

a pod concentric with the second layer and detachably coupled to the upper surface; and

a goniometer for measuring flexion and extension of the joint of the user, and the goniometer is detachably coupled to, and spans between, the pods of the attachments; and

a pedometer configured to count steps of the user and configured to be removably attached to the apparatus.

The apparatus wherein, to prevent the attachments from uncoupling from the user, the second layer comprises a material configured to dampen forces acting between the goniometer and the attachments and caused by relative movement between the goniometer and the attachments.

The apparatus wherein the goniometer has a pair of arms rotatably coupled to and about a center hub, and each arm has a boss for aligning and coupling each arm to a respective pod.

The apparatus wherein each pod defines a recess for receiving and detachably coupling to one of the bosses of the goniometer, and for positioning the goniometer relative to each attachment.

The apparatus wherein, to prevent the goniometer from uncoupling from the attachments, the bosses are sized to be movable within the recesses to allow movement of the bosses in the recesses.

21

The apparatus wherein, to detachably couple the goniometer to the attachments, magnets are disposed adjacent to each boss and each recess.

The apparatus wherein wings extend outwardly from the sides of each arm of the goniometer configured to enable a user to move the arms of the goniometer perpendicularly relative to the attachments, and to uncouple the goniometer from the attachments.

The apparatus wherein the edges of the pod are tapered, such configuration enabling a user to further move the arms of the goniometer perpendicularly relative to the attachments, and to uncouple the goniometer from the attachments.

1500

An apparatus for measuring flexion and extension at a joint of a user, the apparatus comprising:

- a center hub having a first hub, and a second hub coaxially aligned with and rotatably coupled to the first hub;
- a first arm coupled to and rotatable with the first hub; and
- a second arm coupled to and rotatable with the second hub wherein, to maintain a position of the center hub relative to the joint of the user, the first and second arms pivotably and rotatably couple to a respective first and second hub such that rotation, flexion, and extension of the first and second arms are allowed.

The apparatus of claim 1, wherein each of the first and second arms comprise an inner link for pivotably coupling the first and second arms to the first and second hubs, and the inner links are configured to allow the first and second arms to flex and extend relative to the center hub.

The apparatus wherein each of the first and second arms comprise an outer link coupled to the inner link, and the outer links are configured to rotate the first and second arms relative to the center hub.

The apparatus further comprising a screw configured to couple one of the inner and one of the outer links, wherein the screw is aligned parallel to a length of a respective one of the first and second arms, and wherein, to allow the rotation of the first and second arms relative to the center hub, the screw provides for rotation of the inner and outer links.

The apparatus wherein each of the first and second arms comprises an outer end coupled to the outer link, and the outer end is configured to flex and extend relative to the center hub such that further flexion and extension of the first and second arms relative to the center hub are enabled.

The apparatus further comprising link arms extending outwardly from each of the first and second hubs, wherein the link arms couple to respective ones of the first and second arms.

The apparatus further comprising pins configured to couple between a respective outer link and a respective outer end, and between a respective inner link and a respective link arm, and wherein the pins are aligned perpendicular to a length of a respective arm, and wherein the pins provide for the flexion and extension of the first and second arms relative to the center hub.

The apparatus wherein the arms include a magnet and a boss.

An apparatus for measuring flexion and extension at a joint of a user, the apparatus comprising:

- a center hub that has an upper hub, and a lower hub coaxially aligned with and rotatably coupled to the upper hub;
- an arm coupled to, and rotatable with, each of the upper and lower hubs, and the arms pivotably and rotatably couple to the hubs to allow rotation, flexion, and

22

extension of the arms, and to restrict movement of the center hub relative to the joint of the user.

The apparatus further comprising link arms that extend outwardly from each of the upper and lower hubs, and the arms couple to a respective hub at a respective link arm.

The apparatus wherein pins couple each of the link arms and each of the arms, and the pins are aligned perpendicular to the length of a respective arm and configured to allow flexion and extension of the arms, and a screw couples between each of the link arms and each of the arms, and each screw is aligned parallel with the length of a respective arm configured to allow rotation of each arm about each screw.

The apparatus wherein the arms include a magnet and a boss for aligning and coupling the arms to attachments.

An apparatus for measuring flexion and extension at a joint of a user, the apparatus comprising:

- a center hub comprising:
 - an upper hub and a first link arm that extends outwardly from the upper hub;
 - a lower hub coaxially aligned with and rotatably coupled to the upper hub, and a second link arm extends outwardly from the lower hub;
 - an arm pivotably coupled to each of the first and second link arms, and each arm comprises:
 - an inner link for pivotably coupling the arm to a respective first and second link arm and for allowing the arm to flex and extend relative to the center hub;
 - an outer link rotatably coupled to the inner link to allow the arm to rotate relative to the center hub;
 - an outer end pivotably coupled to the outer link to allow the outer end of the arm to flex and extend relative to the outer link and the center hub.

The apparatus wherein the link arms are integrally formed with the hubs.

The apparatus wherein the link arms are coupled to the respective hubs, and the link arms are configured to allow flexion and extension of the arms relative to the center hub.

The apparatus wherein the link arms couple to the respective hubs and are configured to allow rotation of the arms relative to the center hub.

The apparatus wherein a pin couples the inner link and the link arm, and the pin is aligned perpendicular to the length of the arm, and the pin provides for the pivotable coupling between the inner links and link arm.

The apparatus wherein a pin couples the outer link and the outer end, and the pin is aligned perpendicular to the length of the arm, and the pin provides for the pivotable coupling between the outer link and the outer end.

The apparatus wherein a screw couples the inner and outer link, and the screw is aligned parallel with the length of the arm, and the screw provides for the rotatable coupling between the inner link and outer link.

The apparatus wherein the arms include a magnet and a boss.

1700

An apparatus for assisting a person in aligning, relative to a center of a joint of a user, a wearable device on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and the alignment holes have a size, the apparatus comprising:

- a first segment;
- a second segment coupled to the first segment at a pivot point, and when positioned adjacent the center of the joint, the pivot point aligns the apparatus relative to the center of the joint;

23

the first and second segments each defining voids, the voids are spaced on each of the first and second segments equidistant from the pivot point, and the spacing between, and size of, the voids is commensurate with the spacing between, and size of, the alignment holes of the respective attachments; and

whereby the person pivots the segments to centrally align the segments relative to the respective opposing limb portions of the user, and the person marks locations on the respective opposing limb portions through the voids, wherein the alignment holes of the attachments are aligned with respective marks to align the attachments and to couple the wearable device to the user.

The apparatus wherein the first and second segments each have center axes, the center axes intersect at the pivot point, and prior to marking locations on the respective opposing limb portions, the person pivots each segment to centrally align the center axes with the respective centers of the opposing limb portions.

The apparatus wherein the second segment pivotably couples to the first segment at the pivot point.

The apparatus wherein the second segment couples to the first coupling end at a pivot point by overlaying with the first segment.

The apparatus wherein the pivot point is spaced adjacent to and equidistant from first and second coupling ends of the respective first and second segments.

The apparatus wherein the alignment holes of the attachments are aligned coaxially with respective marks to align the attachments, and enable the wearable device to be mounted on the user.

A method for assisting a person in aligning a wearable device relative to a center of a joint of a user, on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and each alignment hole has a size, the method comprising:

providing an apparatus having a first segment and a second segment pivotably coupled to the first segment at a pivot point;

providing voids defined in each of the first and second segments, the voids are spaced an equidistant from the pivot point on each of the first and second segments, and the spacing between, and size of, the voids is commensurate with the spacing between, and size of, the alignment holes of the respective attachments;

locating the center of the joint;

aligning the pivot point of the apparatus with the center of the joint;

pivoting each segment to centrally align the segments relative to respective opposing limb portions;

marking locations on the respective opposing limb portions through the voids;

positioning the alignment holes of the attachments with respective marks to align the attachments and the wearable device on the user; and

coupling the attachments and the wearable device to the user.

The method further comprising:

providing center axes of the first and second segments, and the center axes intersect at the pivot point;

pivoting each segment to centrally align the center axes with the center of the respective opposing limb portion.

The method further comprising:

providing pegs; and

24

coaxially aligning the pegs with the markings to facilitate alignment of the alignment holes of the attachments with each mark.

The method wherein the step of locating the center of the joint is further defined as locating the lateral epicondyle of a knee joint.

An apparatus for assisting a person in aligning a wearable device relative to a center of a joint of a user, on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and the alignment holes have a size, the apparatus comprising:

an imaging device for locating a position of the joint of the user and the opposing limb portions;

a laser configured to provide a beam of light;

a processor in communication with the imaging device and the laser; and

the processor is configured to receive and process data from the imaging device representative of the position of the joint of the user and the opposing limb portions, the processor communicates with the lasers to position the laser such that the light beam forms spots of light on the user at the center of the joint and on the opposing limb portions of the user commensurate with the spacing between, and size of, the alignment holes of the respective attachments, and wherein the alignment holes of the attachments are aligned with respective alignment holes of the attachments to couple the wearable device on the user.

A method for assisting a person in aligning a wearable device relative to a center of a joint of a user, on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and each alignment hole has a size, the method comprising:

providing an imaging device;

providing a laser configured to provide a beam of light;

providing a processor configured to communicate with the imaging device and the laser;

locating with the imaging device positions of the joint and the opposing limb portions;

communicating data from the imaging device to the processor, the data being representative of the positions of the joint and the opposing limb portions;

processing the data with the processor;

calculating with the processor positions of the laser to provide the laser beam to form spots of light on the user at the center of the joint and the opposing limb portions, and the foregoing is commensurate with the spacing between, and size of, the alignment holes of the respective attachments;

communicating instructions to the laser;

moving the laser to the positions; and

aligning the alignment holes of the attachments with the respective spots of light to align the attachments and to couple the wearable device to the user.

The method further comprising the step of marking on the opposing limb portions the location of the laser beam, and aligning the alignment holes of the attachments coaxial with respective marks to align the attachments and to couple the wearable device to the user.

An apparatus for assisting a person in aligning a wearable device relative to a center of a joint of a user and on opposing limb portions of the joint of the user, the apparatus comprising:

diodes coupled to the wearable device, the joint, and the opposing limb portions;

25

an imaging device for locating positions of the diodes;
 a personal communication device configured to commu-
 nicate with a person;
 a processor in communication with the imaging device
 and the personal communication device; and
 the processor is configured to receive and process data
 from the imaging device representative of the positions
 of the diodes, and the processor communicates with the
 personal communication device to provide instructions
 representative of action to be taken by the person to
 align the wearable device relative to the center of joint
 of the user.

The apparatus wherein the personal communication
 device is a display.

The apparatus wherein the personal communication
 device is a speaker.

A method for assisting a person in aligning a wearable
 device on opposing limb portions of a joint of a user relative
 to a center of the joint of the user, the method comprising:

providing a diode coupled to the wearable device, the
 joint, and the opposing limb portions of the user;
 providing an imaging device for locating a position of the
 diodes;

providing a personal communication device configured to
 communicate with a person;

providing a processor configured to communicate with the
 imaging device and the personal communication
 device;

locating with the imaging device the position of the
 diodes;

communicating, from the imaging device to the processor,
 data representative of the position of the diodes;

processing of the data by the processor;

calculating by the processor a position of the wearable
 device relative to the joint and the opposing limb
 portions;

calculating by the processors a position of the wearable
 device, and instructions for the person to align the
 wearable device relative to the center of the joint of the
 patient;

communicating by the processors to the personal com-
 munication device the instructions to be provided to the
 person for aligning the wearable device relative to the
 center of the joint of the user; and

communicating to the person with the personal commu-
 nication device.

The method wherein the step of communicating to the
 person with the personal communication device further
 comprises providing audio instruction through a speaker to
 the personal communication device.

The method wherein the step of communication to the
 person with the communication device further comprises
 providing visual instruction through a display to the personal
 communication device.

An apparatus for assisting a person in aligning, relative to
 a center of a joint of a user, a wearable device on opposing
 limb portions of the joint of the user, the wearable device has
 attachments, each attachment defines alignment holes
 spaced from each other, and the alignment holes have a size,
 the apparatus comprising:

a first segment;

a second segment coupled to the first segment at a pivot
 point, and when positioned adjacent the center of the
 joint, the pivot point aligns the apparatus relative to the
 center of the joint;

the first and second segments each defining voids, the
 voids are spaced on each of the first and second

26

segments equidistant from the pivot point, and the
 spacing between, and size of, the voids is commensu-
 rate with the spacing between, and size of, the align-
 ment holes of the respective attachments; and

whereby the person pivots the segments to centrally align
 the segments relative to the respective opposing limb
 portions of the user, and the person marks locations on
 the respective opposing limb portions through the
 voids, wherein the alignment holes of the attachments
 are aligned with respective marks to align the attach-
 ments and to couple the wearable device to the user.

The apparatus wherein the first and second segments each
 have center axes, the center axes intersect at the pivot point,
 and prior to marking locations on the respective opposing
 limb portions, the person pivots each segment to centrally
 align the center axes with the respective centers of the
 opposing limb portions.

The apparatus wherein the second segment pivotably
 couples to the first segment at the pivot point.

The apparatus wherein the second segment couples to the
 first coupling end at a pivot point by overlaying with the first
 segment.

The apparatus wherein the pivot point is spaced adjacent
 to and equidistant from first and second coupling ends of the
 respective first and second segments.

The apparatus wherein the alignment holes of the attach-
 ments are aligned coaxially with respective marks to align
 the attachments, and enable the wearable device to be
 mounted on the user.

A method for assisting a person in aligning a wearable
 device relative to a center of a joint of a user, on opposing
 limb portions of the joint of the user, the wearable device has
 attachments, each attachment defines alignment holes
 spaced from each other, and each alignment hole has a size,
 the method comprising:

providing an apparatus having a first segment and a
 second segment pivotably coupled to the first segment
 at a pivot point;

providing voids defined in each of the first and second
 segments, the voids are spaced an equidistant from the
 pivot point on each of the first and second segments,
 and the spacing between, and size of, the voids is
 commensurate with the spacing between, and size of,
 the alignment holes of the respective attachments;

locating the center of the joint;

aligning the pivot point of the apparatus with the center of
 the joint;

pivoting each segment to centrally align the segments
 relative to respective opposing limb portions;

marking locations on the respective opposing limb por-
 tions through the voids;

positioning the alignment holes of the attachments with
 respective marks to align the attachments and the
 wearable device on the user; and

coupling the attachments and the wearable device to the
 user.

The method further comprising:

providing center axes of the first and second segments,
 and the center axes intersect at the pivot point;

pivoting each segment to centrally align the center axes
 with the center of the respective opposing limb portion.

The method further comprising:

providing pegs; and

coaxially aligning the pegs with the markings to facilitate
 alignment of the alignment holes of the attachments
 with each mark.

27

The method wherein the step of locating the center of the joint is further defined as locating the lateral epicondyle of a knee joint.

An apparatus for assisting a person in aligning a wearable device relative to a center of a joint of a user, on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and the alignment holes have a size, the apparatus comprising:

- an imaging device for locating a position of the joint of the user and the opposing limb portions;
- a laser configured to provide a beam of light;
- a processor in communication with the imaging device and the laser; and
- the processor is configured to receive and process data from the imaging device representative of the position of the joint of the user and the opposing limb portions, the processor communicates with the lasers to position the laser such that the light beam forms spots of light on the user at the center of the joint and on the opposing limb portions of the user commensurate with the spacing between, and size of, the alignment holes of the respective attachments, and wherein the alignment holes of the attachments are aligned with respective alignment holes of the attachments to couple the wearable device on the user.

A method for assisting a person in aligning a wearable device relative to a center of a joint of a user, on opposing limb portions of the joint of the user, the wearable device has attachments, each attachment defines alignment holes spaced from each other, and each alignment hole has a size, the method comprising:

- providing an imaging device;
- providing a laser configured to provide a beam of light;
- providing a processor configured to communicate with the imaging device and the laser;
- locating with the imaging device positions of the joint and the opposing limb portions;
- communicating data from the imaging device to the processor, the data being representative of the positions of the joint and the opposing limb portions;
- processing the data with the processor;
- calculating with the processor positions of the laser to provide the laser beam to form spots of light on the user at the center of the joint and the opposing limb portions, and the foregoing is commensurate with the spacing between, and size of, the alignment holes of the respective attachments;
- communicating instructions to the laser;
- moving the laser to the positions; and
- aligning the alignment holes of the attachments with the respective spots of light to align the attachments and to couple the wearable device to the user.

The method further comprising the step of marking on the opposing limb portions the location of the laser beam, and aligning the alignment holes of the attachments coaxial with respective marks to align the attachments and to couple the wearable device to the user.

An apparatus for assisting a person in aligning a wearable device relative to a center of a joint of a user and on opposing limb portions of the joint of the user, the apparatus comprising:

- diodes coupled to the wearable device, the joint, and the opposing limb portions;
- an imaging device for locating positions of the diodes;
- a personal communication device configured to communicate with a person;

28

a processor in communication with the imaging device and the personal communication device; and
the processor is configured to receive and process data from the imaging device representative of the positions of the diodes, and the processor communicates with the personal communication device to provide instructions representative of action to be taken by the person to align the wearable device relative to the center of joint of the user.

The apparatus wherein the personal communication device is a display.

The apparatus wherein the personal communication device is a speaker.

A method for assisting a person in aligning a wearable device on opposing limb portions of a joint of a user relative to a center of the joint of the user, the method comprising:

- providing a diode coupled to the wearable device, the joint, and the opposing limb portions of the user;
- providing an imaging device for locating a position of the diodes;
- providing a personal communication device configured to communicate with a person;
- providing a processor configured to communicate with the imaging device and the personal communication device;
- locating with the imaging device the position of the diodes;
- communicating, from the imaging device to the processor, data representative of the position of the diodes;
- processing of the data by the processor;
- calculating by the processor a position of the wearable device relative to the joint and the opposing limb portions;
- calculating by the processors a position of the wearable device, and instructions for the person to align the wearable device relative to the center of the joint of the patient;
- communicating by the processors to the personal communication device the instructions to be provided to the person for aligning the wearable device relative to the center of the joint of the user; and
- communicating to the person with the personal communication device.

The method wherein the step of communicating to the person with the personal communication device further comprises providing audio instruction through a speaker to the personal communication device.

The method wherein the step of communication to the person with the communication device further comprises providing visual instruction through a display to the personal communication device.

The above discussion is meant to be illustrative of the principles and various embodiments of the present invention. Numerous variations and modifications will become apparent to those skilled in the art once the above disclosure is fully appreciated. It is intended that the following claims be interpreted to embrace all such variations and modifications.

The various aspects, embodiments, implementations or features of the described embodiments may be used separately or in any combination. The embodiments disclosed herein are modular in nature and may be used in conjunction with or coupled to other embodiments.

Benefits, other advantages, and solutions to problems have been described above with regard to specific embodiments. However, the benefits, advantages, solutions to problems, and any feature(s) that can cause any benefit, advan-

29

tage, or solution to occur or become more pronounced are not to be construed as a critical, required, sacrosanct or an essential feature of any or all of the claims.

Consistent with the above disclosure, the examples of assemblies enumerated in the following clauses are specifically contemplated and are intended as a non-limiting set of examples.

What is claimed:

1. A system for positioning a wearable device for measuring an angle of a joint of a user, the system comprising: the wearable device;

an alignment device separate from the wearable device and including a first segment and a second segment pivotally coupled to the first segment at a pivot point, wherein each of the first segment and the second segment of the alignment device defines first and second voids, and wherein the first voids of the first segment and the second segment are equidistant from the pivot point and the second voids of the first and second segment are equidistant from the pivot point; and

first and second attachment portions separate from the wearable device and the alignment device and configured to adhesively couple to the user, wherein each of the attachment portions defines at least one alignment hole, wherein each of the attachment portions is configured for securing the wearable device to a corresponding limb portion of the user adjacent to the joint, and wherein the alignment device is configured to facilitate alignment of the first and second attachment portions to the joint,

wherein the first and second voids of each of the first segment and the second segment have a spacing and a size that is commensurate with the at least one alignment hole in a corresponding attachment portion of the

30

first and second attachment portions to facilitate alignment of the first and second attachment portions to the joint,

wherein the wearable device includes

a first hub pivotally coupled to a second hub, a first arm attached to the first hub at a first inner end and defining a first outer end opposite the first inner end, and a second arm attached to the second hub at a second inner end and defining a second outer end opposite the second inner end, and

wherein each of the first and second attachment portions includes a pod configured to be selectively coupled to a corresponding one of the first outer end of the first arm and the second outer end of the second arm.

2. The system of claim 1, wherein the first and second voids in each of the first segment and the second segment define a straight line with the pivot point.

3. The system of claim 1, wherein the wearable device defines an axis of rotation about which the first hub is pivotally coupled to the second hub, and

wherein the first and second voids of each of the first segment and the second segment are configured for positioning the first and second attachment portions at specific locations on the corresponding limb portions of the user to cause the axis of rotation to be aligned with a pivot axis of the joint.

4. The system of claim 1, wherein the pods are each selectively coupled to the corresponding one of the first arm and the second arm using magnets.

5. The system of claim 1, wherein at least one of the first arm and the second arm defines a boss, and wherein the pods each define a recess configured to receive the boss of a corresponding one of the one of the first arm and the second arm.

* * * * *