



US0D1090897S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,090,897 S**
Norell (45) **Date of Patent:** **** Aug. 26, 2025**

(54) **TUBE RACK** D995,815 S * 8/2023 Knight B01L 9/06
D24/230
(71) Applicant: **Norell, Inc.**, Morganton, NC (US) D1,028,275 S * 5/2024 Suchocki D24/226
D1,049,422 S * 10/2024 Norell D24/229
(72) Inventor: **Gregory B. Norell**, Morganton, NC D1,053,380 S * 12/2024 Allegoren D24/224
(US) 2004/0265186 A1 * 12/2004 Clark B01L 3/50255
422/400

(Continued)

(73) Assignee: **Norell, Inc.**

(**) Term: **15 Years**

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **29/887,354**

JP D2022-06671 * 10/2022

(22) Filed: **Mar. 20, 2023**

OTHER PUBLICATIONS

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.** **D24/229**
USPC **D24/229**

(58) **Field of Classification Search**
USPC D24/216, 217, 219, 220, 224–227, 229,
D24/232, 233; D9/424, 425, 732, 735,
D9/755, 758; D7/550.1, 553.1–553.5,
D7/554.3; D3/294–295; D18/43, 44
CPC A47G 23/06; A16B 50/20; A61B 50/30;
A61J 1/00; C07K 1/26; B01L 3/52; B01L
7/00
See application file for complete search history.

Rack with 96 sample tubes for use with SampleJet. Online, published date unknown. Retrieved on Feb. 18, 2025 from URL: https://store.bruker.com/products/96-sample-tubes-for-samplejet-with-code.*

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — The Belles Group, P.C.

(57) **CLAIM**

The ornamental design for a tube rack, as shown and described.

(56) **References Cited**


DESCRIPTION

U.S. PATENT DOCUMENTS

D624,196 S 9/2010 Himmelsbach et al.
D624,660 S 9/2010 Himmelsbach et al.
D624,661 S 9/2010 Himmelsbach et al.
D628,306 S * 11/2010 Blanc D24/230
8,312,781 B2 11/2012 Himmelsbach et al.
D808,540 S * 1/2018 Johns D24/227
D812,243 S * 3/2018 Johns D24/227
D840,053 S * 2/2019 Kamees D24/230
D865,215 S * 10/2019 Dangelo D24/224
D932,052 S * 9/2021 Zergiebel D24/229
11,179,726 B2 * 11/2021 Knight B01L 3/527
D965,815 S * 10/2022 Watts D24/227
D968,644 S * 11/2022 Schatilov D24/230
D981,591 S * 3/2023 Jeffrey-Coker D24/226

FIG. 1 is a top, front perspective view of a tube rack showing my new design;
FIG. 2 is a bottom, rear perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a left side view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.
The broken lines illustrating portions of the tube rack form no part of the claimed design.

1 Claim, 8 Drawing Sheets

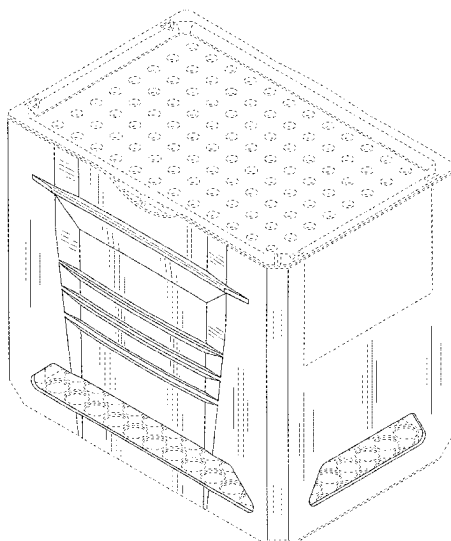

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0124250 A1 * 5/2008 Yang G01N 35/1065
422/400
2011/0306118 A1 * 12/2011 Belz G01N 35/00732
422/68.1
2015/0174579 A1 * 6/2015 Iten B65D 25/108
422/560
2016/0249995 A1 * 9/2016 Ritchey A61B 50/33
53/425
2017/0043346 A1 * 2/2017 Welch B65D 25/24
2017/0297027 A1 * 10/2017 Knight B01L 3/50853
2024/0316565 A1 * 9/2024 Chao B31B 50/20

OTHER PUBLICATIONS

Fisher scientific website “Norell Inc 3mm, 4” (103.5mm) Long NMR Tubes for Automated Sample Tube System, 96PK, Includes Open Port Sample Vault Caps, Includes Sample Vault™ NMR Sample Tube Rack”, <https://www.fishersci.com/shop/products/nmr-tubes-4in-3mm-caps-96pk/NC1196108>, Retrieved Mar. 20, 2023; pp. 1-3.

Secure nmrtubes website “Sample Vault™ NMR Sample Tube Rack from Norell® Available With Superior Sample Vault™ NMR Tube Caps”, <https://secure.nmrtubes.com/nmr-epr-tubes/sample-vault-tm-nmr-sample-tube-rack>, Retrieved Mar. 20, 2023; pp. 1-3.

* cited by examiner

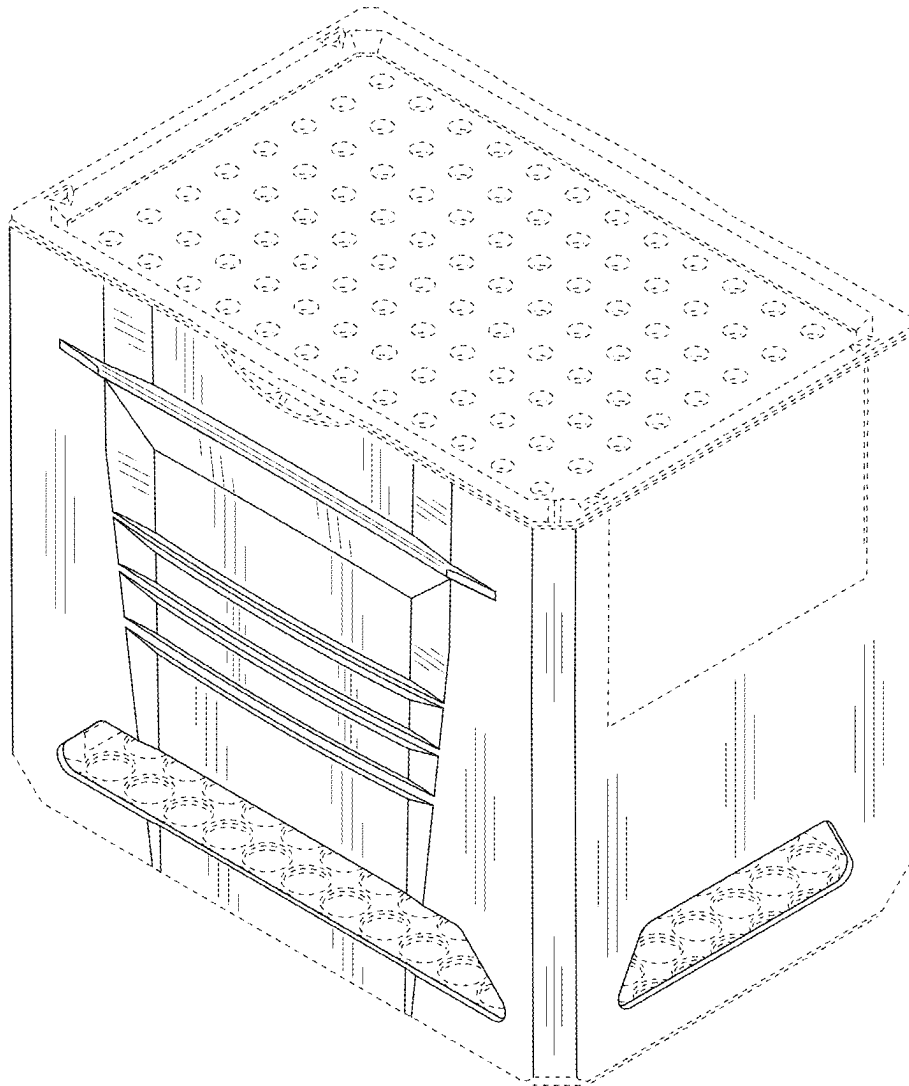


FIG. 1

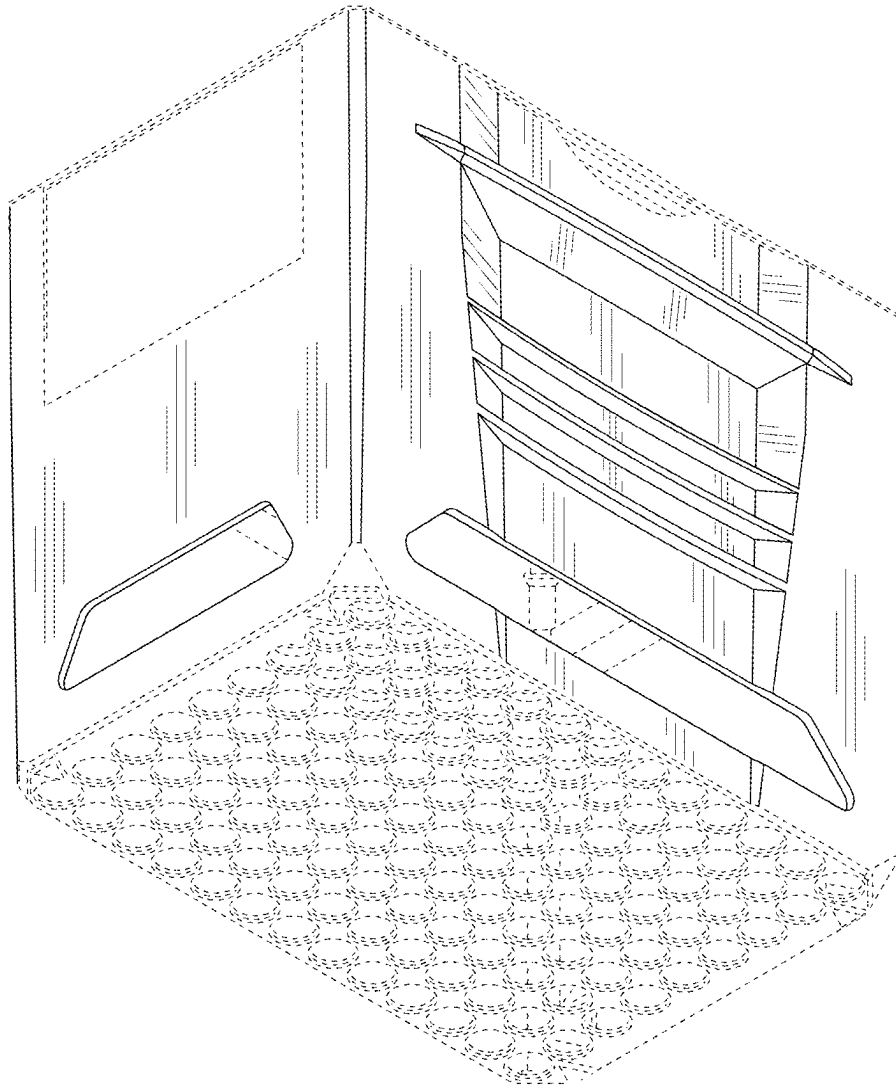


FIG. 2

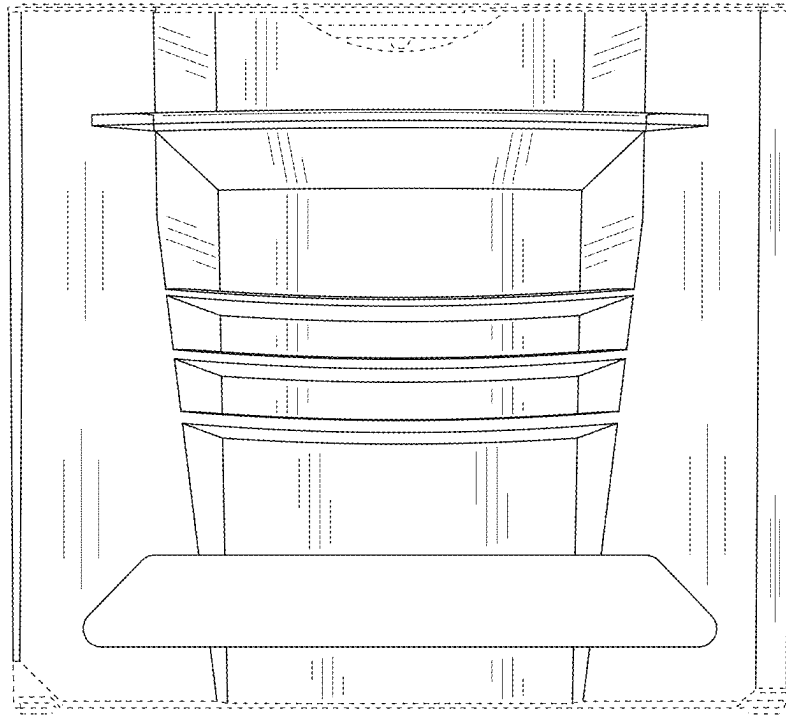


FIG. 3

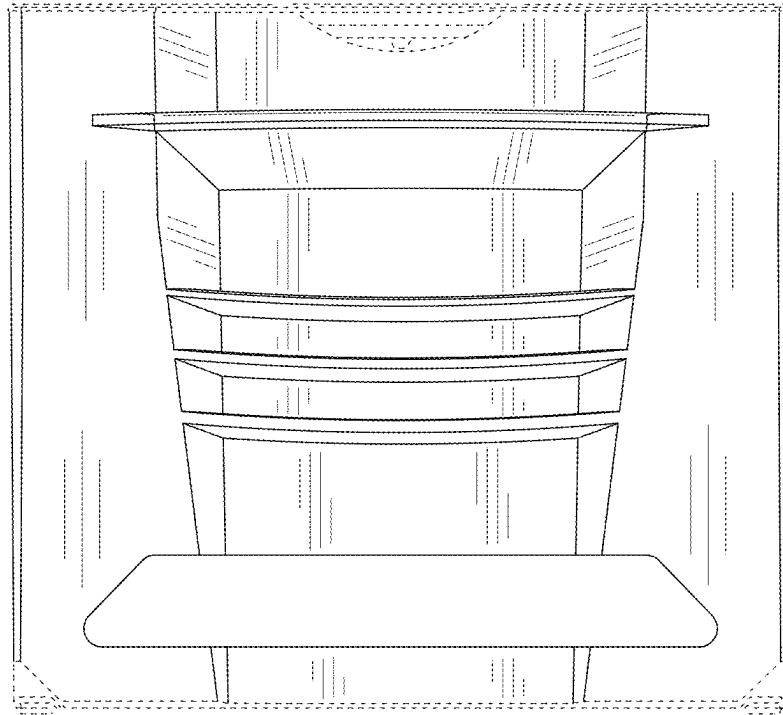


FIG. 4

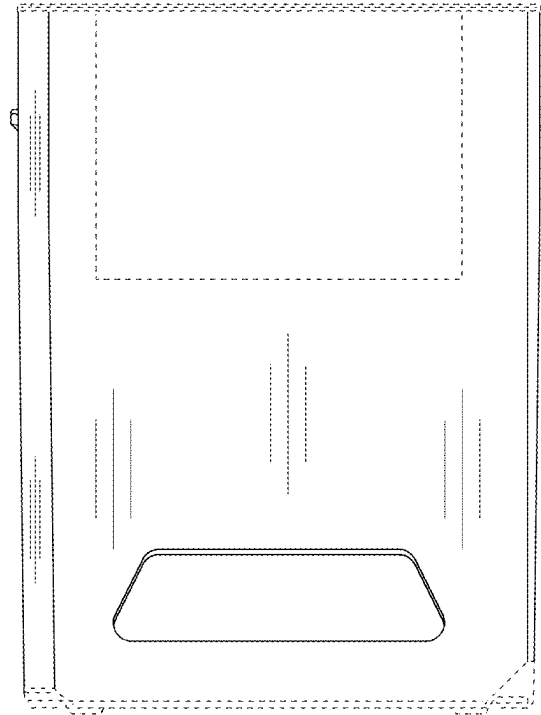


FIG. 5

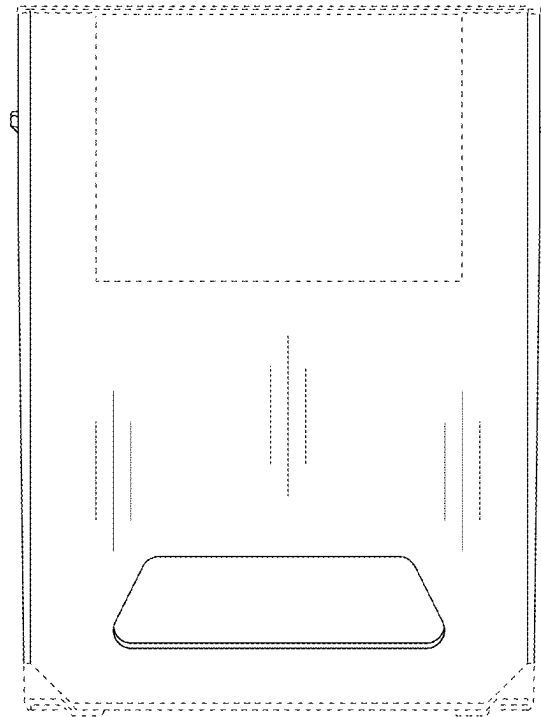


FIG. 6

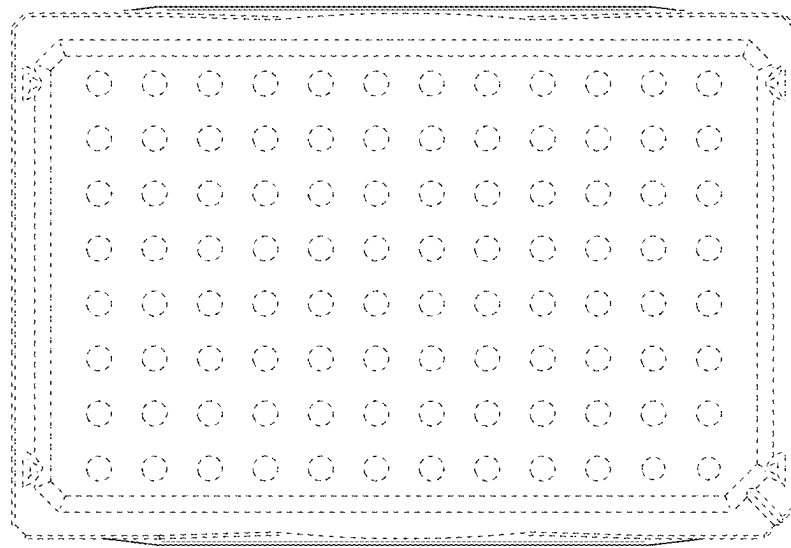


FIG. 7

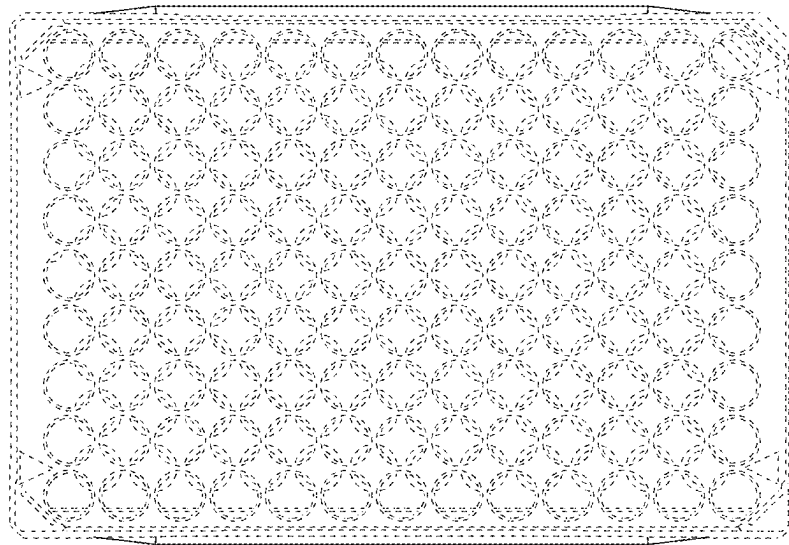


FIG. 8