



US0D1092749S

(12) **United States Design Patent**
Hahn et al.

(10) **Patent No.:** **US D1,092,749 S**
(45) **Date of Patent:** **** Sep. 9, 2025**

(54) **MOLDED SINGLE PIECE PATIENT
REPOSITIONING WEDGE**

(71) Applicant: **Medline Industries, LP**, Northfield, IL
(US)

(72) Inventors: **Vincent Hahn**, Chicago, IL (US);
Jeremy Fogel, Evanston, IL (US);
Drew Phalen, Skokie, IL (US)

(73) Assignee: **Medline Industries, LP**, Northfield, IL
(US)

(**) Term: **15 Years**

(21) Appl. No.: **29/898,407**

(22) Filed: **Jul. 27, 2023**

Related U.S. Application Data

(63) Continuation of application No. 29/757,192, filed on
Nov. 4, 2020, now Pat. No. Des. 997,364, which is a
continuation of application No. 29/676,199, filed on
Jan. 9, 2019, now Pat. No. Des. 907,777.

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/183; D24/190**

(58) **Field of Classification Search**
USPC D24/183–184, 188, 190–191, 200, 211,
D24/215; D6/392, 596, 601; D29/101.3
CPC A61B 34/71; A61B 90/14; A61G 13/0036;
A61G 13/0054; A61G 13/1285; A61G
13/1295; A61G 13/12; A47C 21/00;
A47C 21/003

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D215,536 S	10/1969	Larsen
4,048,681 A	9/1977	Baulch
4,635,306 A	1/1987	Wiley

D288,632 S	3/1987	Grimsrud
4,686,719 A	8/1987	Johnson
4,770,466 A	9/1988	Pesterfield
4,802,249 A	2/1989	Bills
D336,134 S	6/1993	Kalatsky

(Continued)

OTHER PUBLICATIONS

Medline Comfort Glide 30° Foam Wedge. Online, published date
unknown. Retrieved on Apr. 3, 2025 from URL:<https://www.healthproductsforyou.com/p-medline-comfort-glide-30-foam-wedge.html>.*

(Continued)

Primary Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Fitch, Even, Tabin &
Flannery LLP

(57) **CLAIM**

The ornamental design for a molded single piece patient
repositioning wedge, as shown and described.

DESCRIPTION

FIG. 1 is a top, front perspective view of a molded single
piece patient repositioning wedge in accordance with our
new design;

FIG. 2 is a bottom, rear perspective view thereof;

FIG. 3 is a front elevation view thereof;

FIG. 4 is a rear elevation view thereof;

FIG. 5 is a top plan view thereof;

FIG. 6 is a bottom plan view thereof;


FIG. 7 is a right elevation view thereof; and,

FIG. 8 is a left elevation view thereof.

The broken lines represent portions of the molded single
piece patient repositioning wedge that form no part of the
claimed design.

The stippling represents a contrasting texture to that of the
non-stippled areas of the molded single piece patient repositioning wedge.

1 Claim, 7 Drawing Sheets

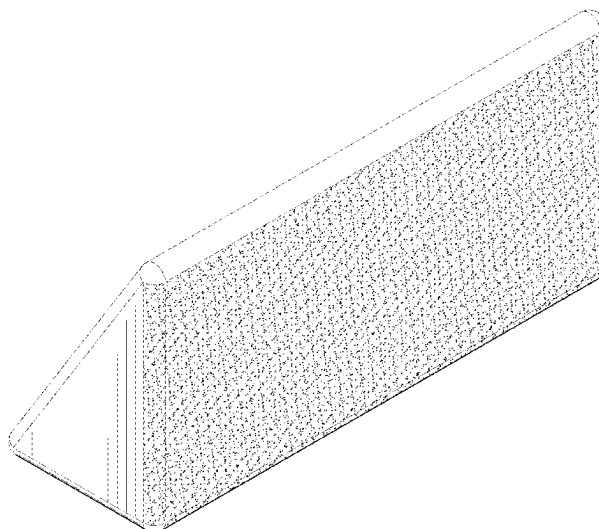

(56)

References Cited

U.S. PATENT DOCUMENTS

D366,527	S	1/1996	Paterson	
D369,054	S *	4/1996	Straub	D24/183
5,526,543	A	6/1996	Dimatteo	
D406,718	S	3/1999	Jacobs	
5,943,839	A	8/1999	Miller	
6,073,291	A	6/2000	Davis	
6,230,350	B1	5/2001	Goldstein	
6,684,425	B2	2/2004	Davis	
6,931,683	B1	8/2005	Elkin	
7,028,350	B1	4/2006	Davis	
7,168,115	B2	1/2007	Davis	
7,240,384	B2	7/2007	Dudonis	
7,328,471	B1	2/2008	Stohr	
7,475,441	B1	1/2009	Soberal	
D610,852	S	3/2010	Rothschild	
7,681,262	B2	3/2010	Weedling	
D652,715	S	1/2012	Quinter	
8,152,749	B2	4/2012	Ponsi	
8,435,199	B2	5/2013	Ponsi	
D690,424	S	9/2013	Ponsi	
8,535,255	B2	9/2013	Ponsi	
8,789,533	B2	7/2014	Steffens	
8,850,634	B2	10/2014	Ponsi	
8,984,681	B2	3/2015	Ponsi	
D733,897	S	7/2015	Rossouw	
9,414,977	B2	8/2016	Ponsi	
D778,373	S	2/2017	Gossett	
D781,429	S *	3/2017	Westdyk	D24/190
9,693,920	B2	7/2017	Fowler	
9,820,902	B2	11/2017	Ponsi	
9,820,903	B2	11/2017	Steffens	
D805,325	S	12/2017	Chan	
9,849,053	B2	12/2017	Rigoni	
9,861,544	B2	1/2018	Rigoni	
10,064,773	B2	9/2018	Rigoni	
D837,566	S	1/2019	Connors	
D868,500	S	12/2019	Rowe	
D871,593	S	12/2019	Rossouw	
D872,504	S	1/2020	Toft	
D876,860	S	3/2020	Swanson	
D880,901	S	4/2020	Raad	
D882,296	S *	4/2020	Huang	D6/601
D907,777	S	1/2021	Hahn	
D941,060	S *	1/2022	Kong	D6/601
D944,906	S	3/2022	Che	
D950,979	S *	5/2022	Rifelj	D6/601
D970,257	S	11/2022	Klerer	
11,559,153	B2 *	1/2023	Mani	A47G 9/1045
D997,364	S	8/2023	Hahn	
D1,006,495	S *	12/2023	Zhu	D6/601
D1,008,386	S *	12/2023	Wu	D21/686
D1,015,452	S *	2/2024	Pasquale	D21/686
D1,021,474	S *	4/2024	Huang	D6/601
D1,046,500	S *	10/2024	Wu	D6/601
2001/0044968	A1	11/2001	Schmitter	
2005/0005358	A1	1/2005	Dudonis	
2009/0192028	A1	7/2009	Shank	
2010/0262050	A1	10/2010	Gasparovich	
2012/0186012	A1	7/2012	Ponsi	
2012/0186587	A1	7/2012	Steffens	
2013/0205495	A1	8/2013	Ponsi	

2013/0205504	A1 *	8/2013	Ratner	A61G 13/121 5/622
2014/0189956	A1	7/2014	Sosi	
2016/0095776	A1	4/2016	Batiste	
2016/0331611	A1	11/2016	Ponsi	
2017/0042339	A1	2/2017	Monderine	
2017/0049647	A1	2/2017	Rigoni	
2017/0049648	A1	2/2017	Kennedy	
2017/0051851	A1	2/2017	Kennedy	
2017/0119608	A1	5/2017	Rigoni	
2017/0216117	A1	8/2017	Rigoni	
2017/0296414	A1	10/2017	Fowler	
2018/0049935	A1	2/2018	Rigoni	

OTHER PUBLICATIONS

Acello, Barbara; Nursing Assisting: Essentials of Long Term Care; 2nd Edition, Thomson/Delmar Learning; Chapter 8, p. 164, "Moving and Positioning Devices for Comfort and Pressure Relief", Aug. 4, 2004; 1 page.

Aktiverings—og forflytningshjælpemidler Forflytningsssystemer catalog (in Danish); Positioning Wedge pp. 26-27; Etac A/S; publicly available at least as of 2009; 32 pages.

Aktiverings—og forflytningshjælpemidler Mindre forflytningshjælpemidler catalog (in Danish); Positioning Wedge pp. 18-19; Etac Sveridge AB; publicly available at least as of 2009; 24 pages.

AliMed® Safe Patient Handling catalog; "In-Bed Patient Positioning System" p. 11; AliMed® inc.; publicly available at least as of 2011; 24 pages.

Comfort Glide Foam Wedges from <https://www.medline.com/product/Comfort-Glide-Foam-Wedges/Wedges/Z05-PF80217?question=wedge&index=P2&indexCount=2#>; Medline Industries, Inc.; publicly available at least as of Mar. 2015; 4 pages.

Etac 4Way Glide Bed Management System product brochure; Etac®; presently believed to be publicly available at least as of 2005; 4 pages.

In-Bed Patient Positioning System product brochure from Skil-Care™ Corporation; presently believed to be publicly available at least as of Oct. 2013; 2 pages.

National Guideline Clearinghouse: Prevention of Pressure Ulcers from <http://www.guideline.gov/syntheses/printView.aspx?id=25078>, retrieved Sep. 5, 2013; U.S. Department of Health & Human Services, Agency for Healthcare Research and Quality; 9 pages.

No-Slip Wedge™ Positioning Cushion Instruction Sheet; Intensive Therapeutics, Inc.; publicly available at least as of 2005; 1 page.

PrevalonTurn and Position System 2.0 by Sage Products. Online, published date unknown. Retrieved on Apr. 3, 2020 from URL: <https://www.medline.com/product/PrevalonTurn-and-Position-System-20-by-Sage-Products/Positioners/Z05-PF90858?question=position&index=P4&indexCount=4>; 1 page.

Skil-Care™ Corporation; Long-Term/Acute Care & Rehab Product Catalog—Bed Positioning; 2012-2013; 8 pages.

Top 10 Best Wedge Pillows in 2020. Online, published date Mar. 13, 2018. Retrieved on Apr. 3, 2020 from URL: <https://www.youtube.com/watch?v=gJqFhpx17sQ>; 1 page.

Turnwedge™ The Ultimate Body Positioner, product instructions; CarePlus Medical, Inc.; from <https://web.archive.org/web/20100327/http://turnwedge.com/>; presently believed to be publicly available at least as of Mar. 27, 2010; 1 page.

* cited by examiner

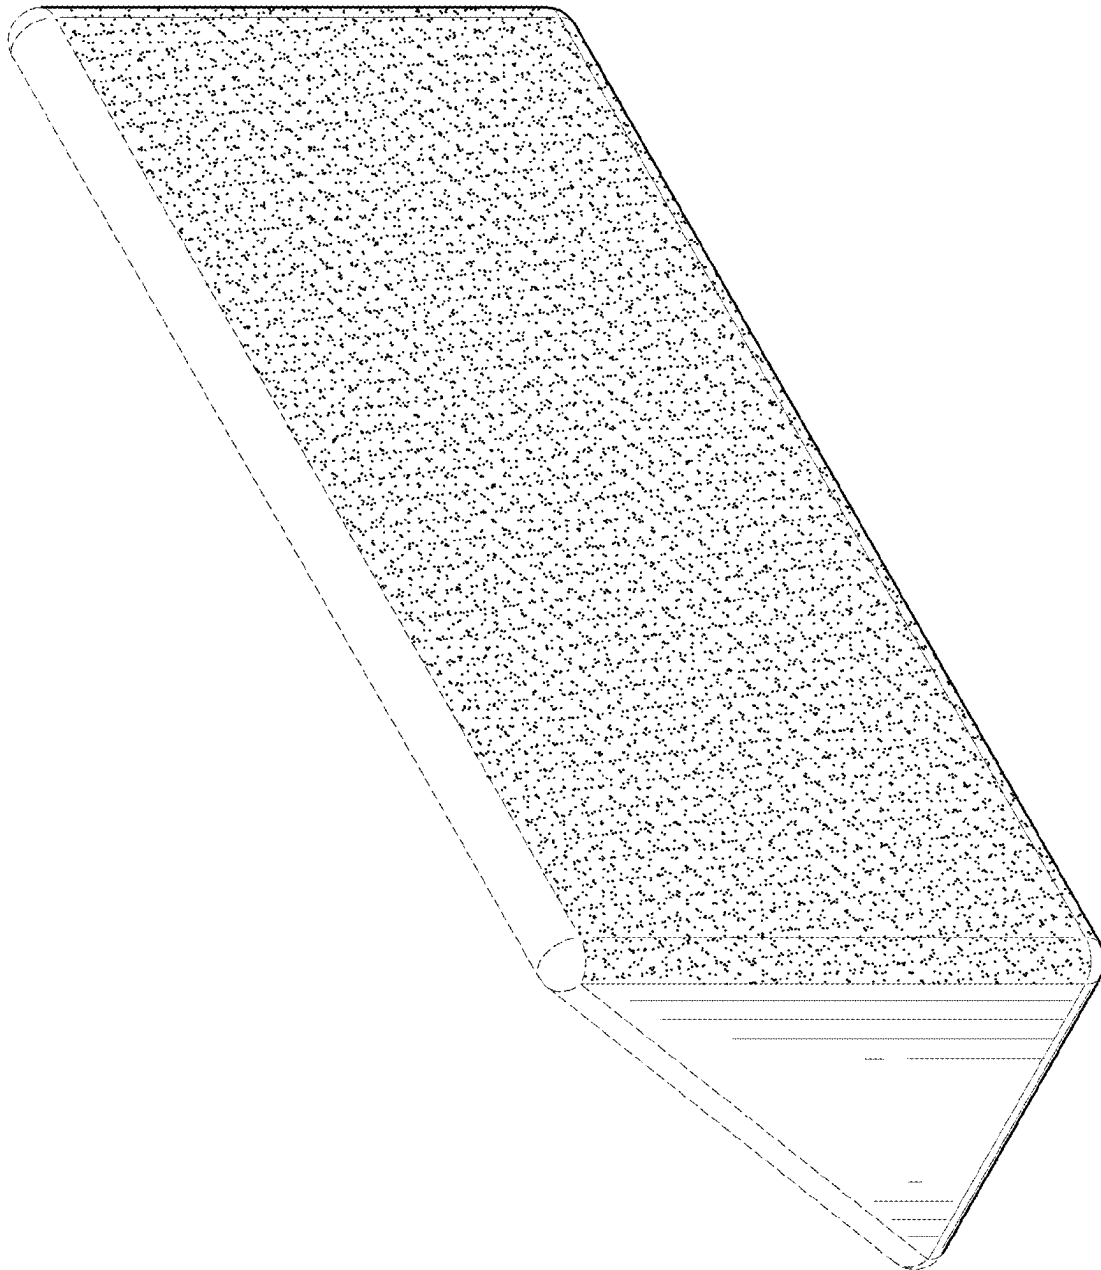


FIG. 1

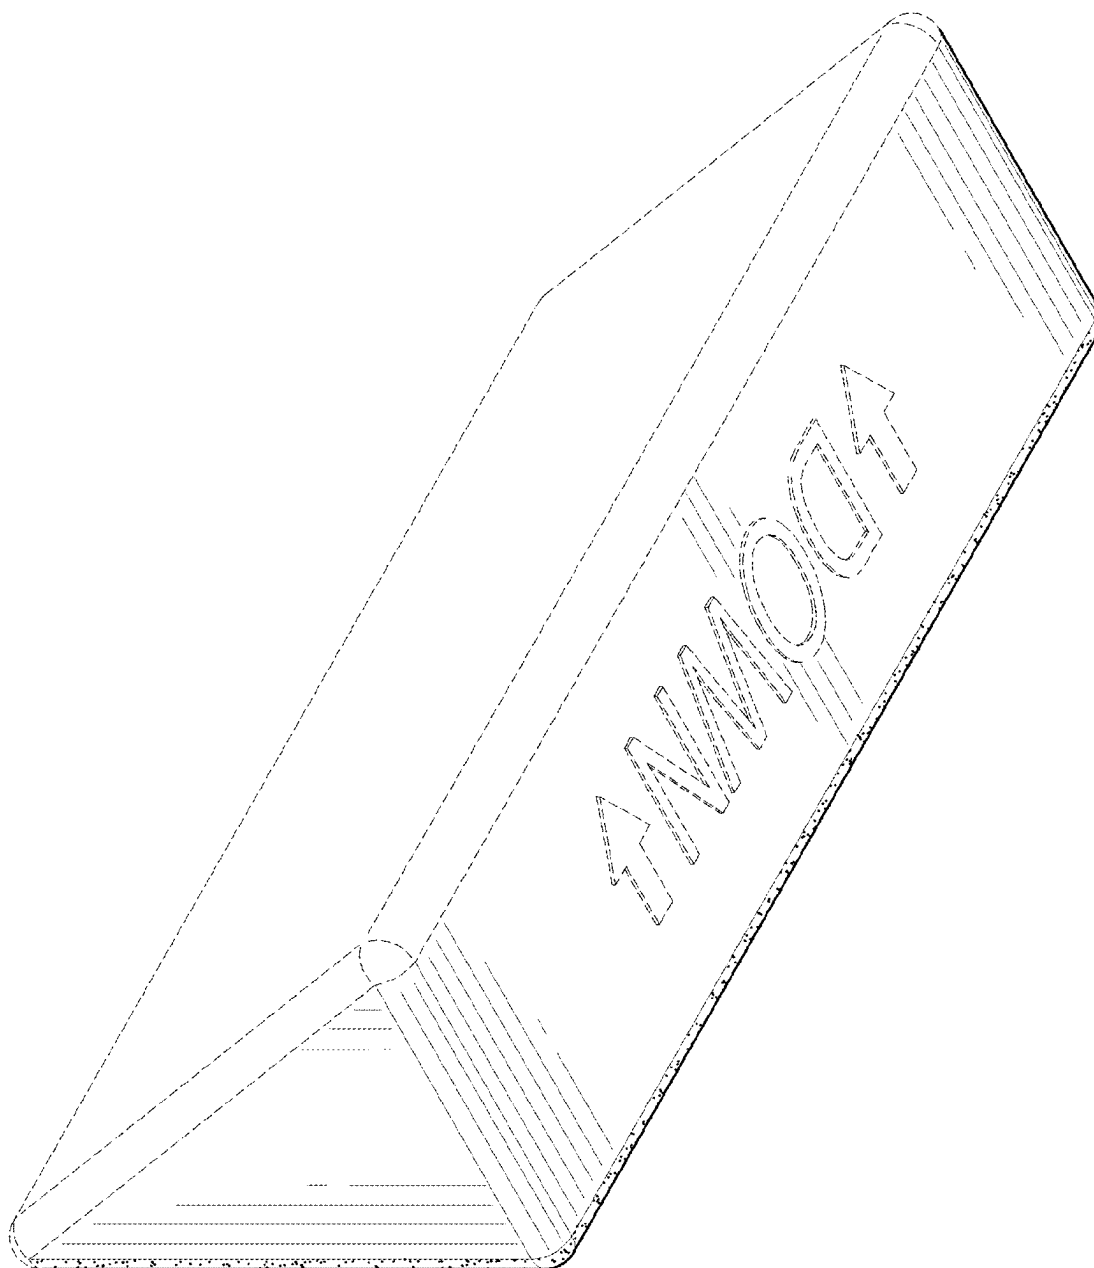


FIG. 2

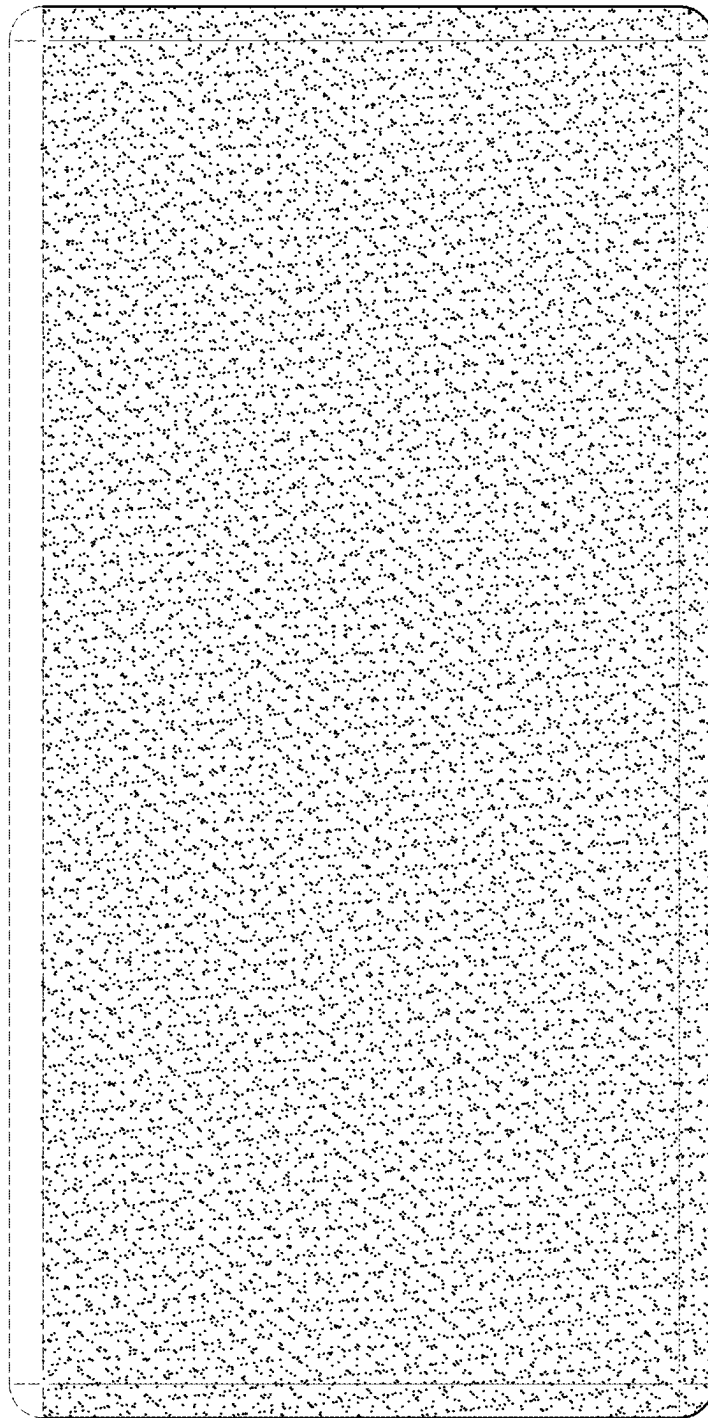


FIG. 3

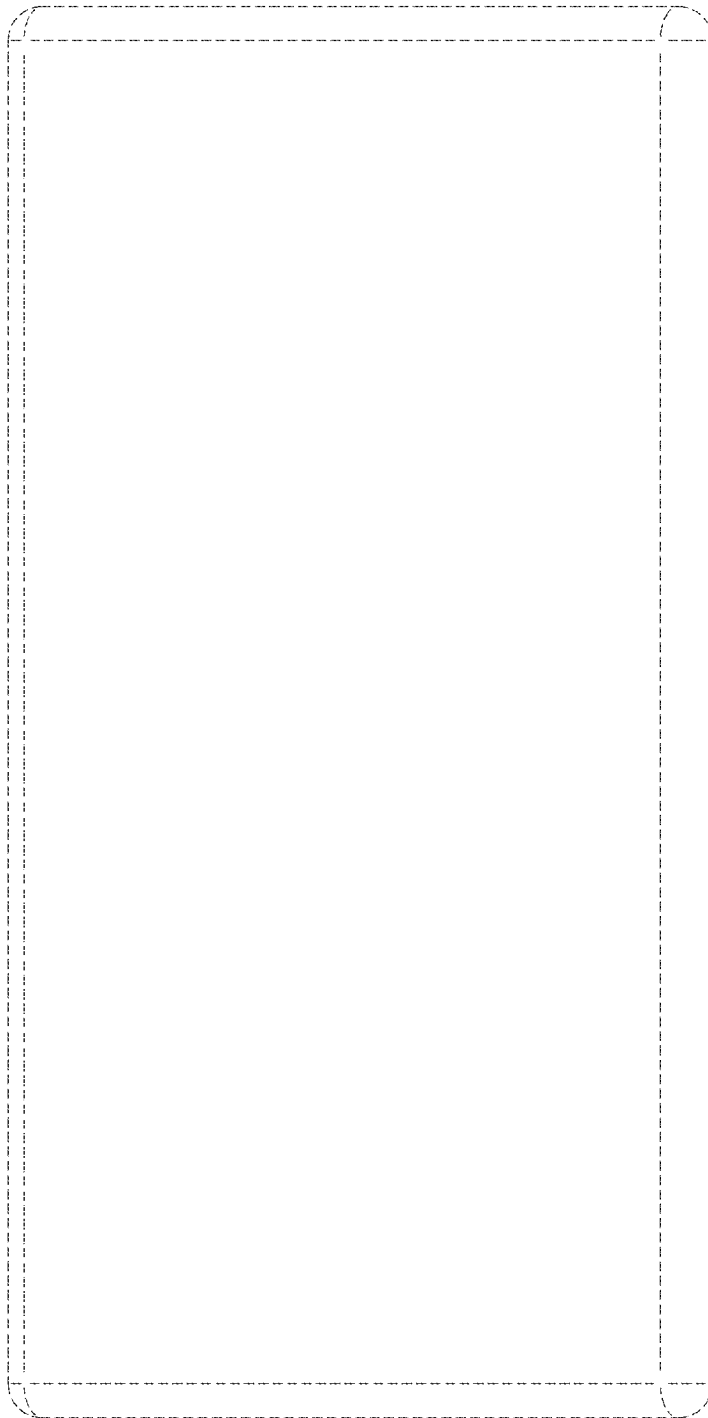


FIG. 4

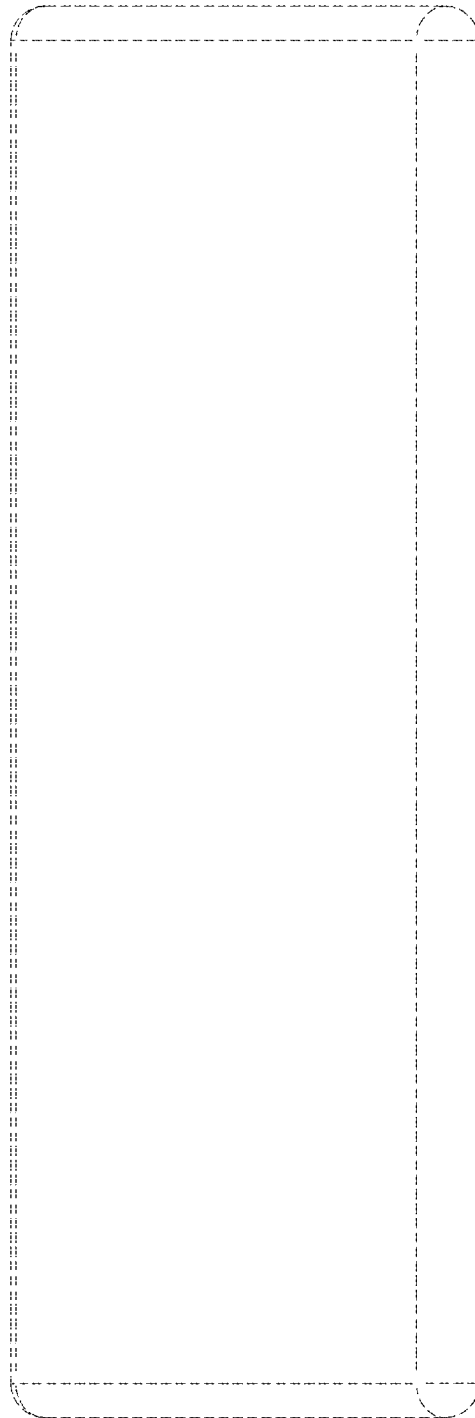


FIG. 5

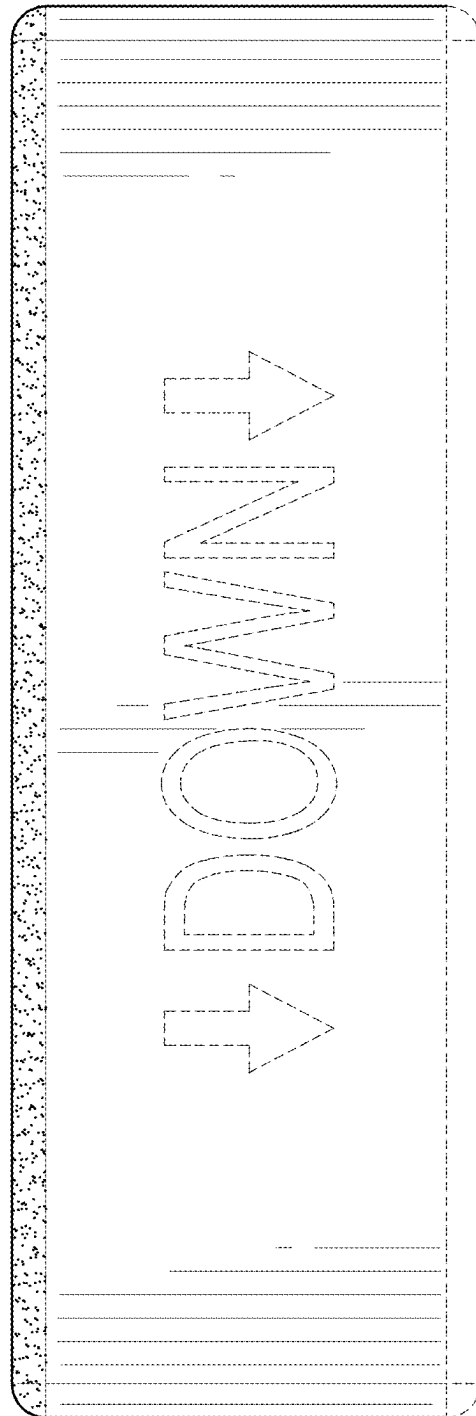


FIG. 6

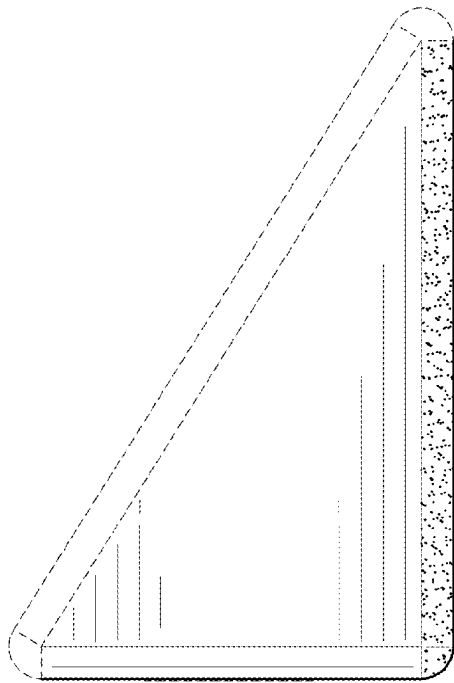


FIG. 7

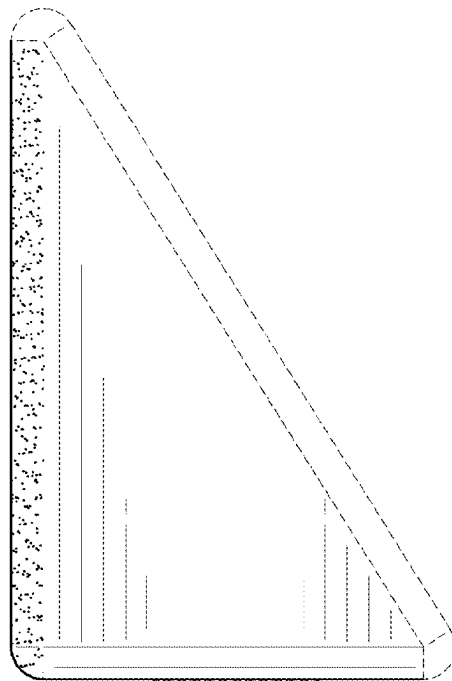


FIG. 8