



US0D1090871S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,090,871 S**
Shah et al. (45) **Date of Patent:** **** Aug. 26, 2025**

(54) **NERVE STIMULATION DEVICE** D1,015,552 S * 2/2024 Bao D24/200
2015/0018634 A1 * 1/2015 Zhu A61N 1/36135
(71) Applicant: **ElectroCore, Inc.**, Rockaway, NJ (US) 2016/0001067 A1 * 1/2016 Pereira A61L 24/00
600/301
(72) Inventors: **Jeckin Shah**, Flemington, NJ (US); 2021/0244940 A1 * 8/2021 Liberatore A61N 1/3603
Tanja Martin, Rockaway, NJ (US) 2022/0096832 A1 * 3/2022 Peterson A61N 1/3754
607/116

(73) Assignee: **Electrocore, Inc.**, Rockaway, NJ (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/901,333**

(22) Filed: **Aug. 31, 2023**

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/200**

(58) **Field of Classification Search**

USPC D24/200, 141, 206–207, 135, 119, 133,
D24/211–215, 167, 155, 185–186;
D30/160; D14/344; D11/3; D28/44.1
CPC A61M 29/00; A61B 1/00148; A61B 1/32;
A61B 1/00085; A61B 1/31; A61B 1/303;
A61B 18/1485; A61B 2017/00513; A61H
7/001; A61H 7/007; A61H 19/32; A61H
2205/087; A61H 19/50; A61H 7/003;
A61H 19/40; A63B 23/20; A63B 23/00;
A61N 1/403; A61N 1/40524; A61N
5/045; A61N 5/0603; A61N 5/0601;
A61N 2005/0611; A61N 1/0558; A61L
24/00; A61L 24/10; A61F 7/00; A61F
7/007; A61F 2007/0001; A61F
2007/0029; A61F 2007/0078; A61F
2007/0087; A61F 2007/0036; A61F
2007/0037

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D338,731 S * 8/1993 Byland D24/155
D437,938 S * 2/2001 Ko D24/200

OTHER PUBLICATIONS

The 5 Best Vagus Nerve Stimulation Devices on the Market in 2024, first available Aug. 28, 2024, healthnews.com, [online], [site visited Oct. 18, 2024], Available from internet URL: <https://healthnews.com/longevity/biohacking/best-vagus-nerve-stimulation-device/> (Year: 2024).*

Truvaga Plus, first available May 11, 2024, truvaga.com, [online], [site visited Oct. 18, 2024], Available from internet URL: <https://www.truvaga.com/product/truvaga-plus/> (Year: 2024).*

Verelief Reset, hooolest.com, [online], [site visited Oct. 18, 2024], Available from internet URL: <https://hooolest.com/> (Year: 2024).*

* cited by examiner

Primary Examiner — Justin M Jonaitis

Assistant Examiner — Holly M Rodriguez

(74) *Attorney, Agent, or Firm* — Farber LLC


(57) **CLAIM**

The ornamental design for a nerve stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a front view of the nerve stimulation device; FIG. 2 is a back view of the nerve stimulation device; FIG. 3 is a right side view of the nerve stimulation device; FIG. 4 is a left side view of the nerve stimulation device; FIG. 5 is a bottom view of the nerve stimulation device; and, FIG. 6 is a top view of the nerve stimulation device. The broken line shown in FIG. 4 is for the purpose of illustrating portions of the nerve stimulation device and forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

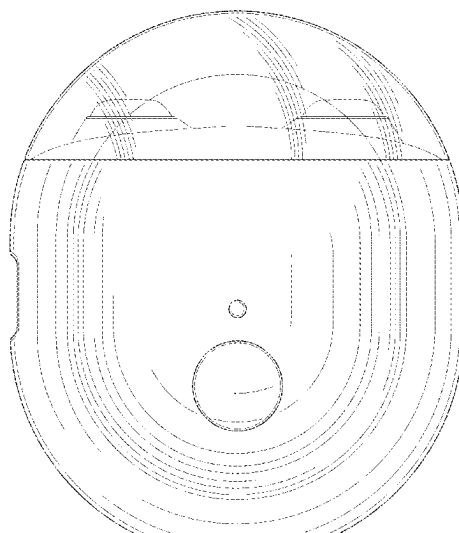

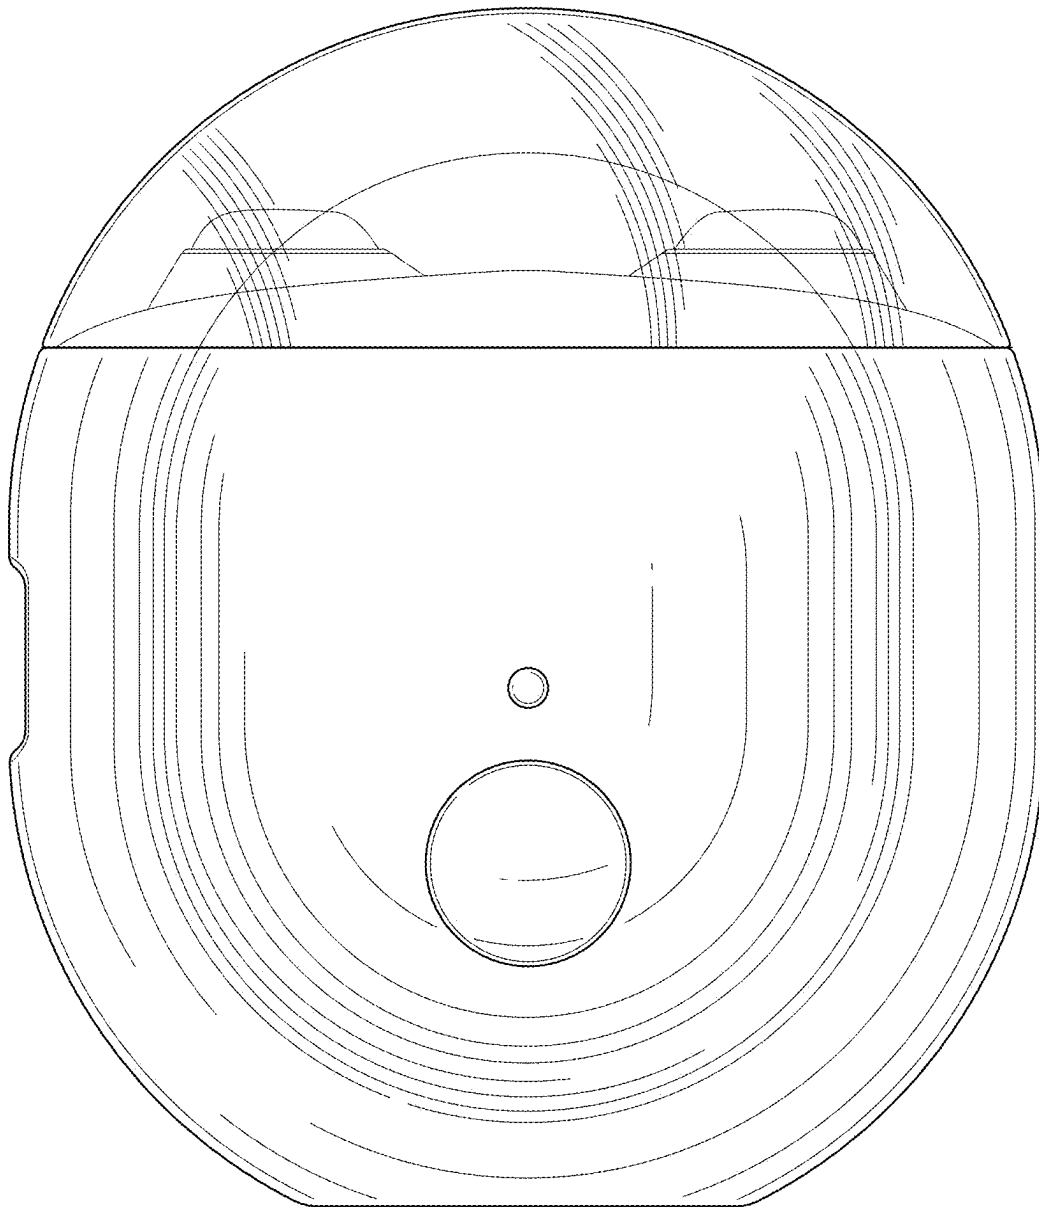


FIG. 1

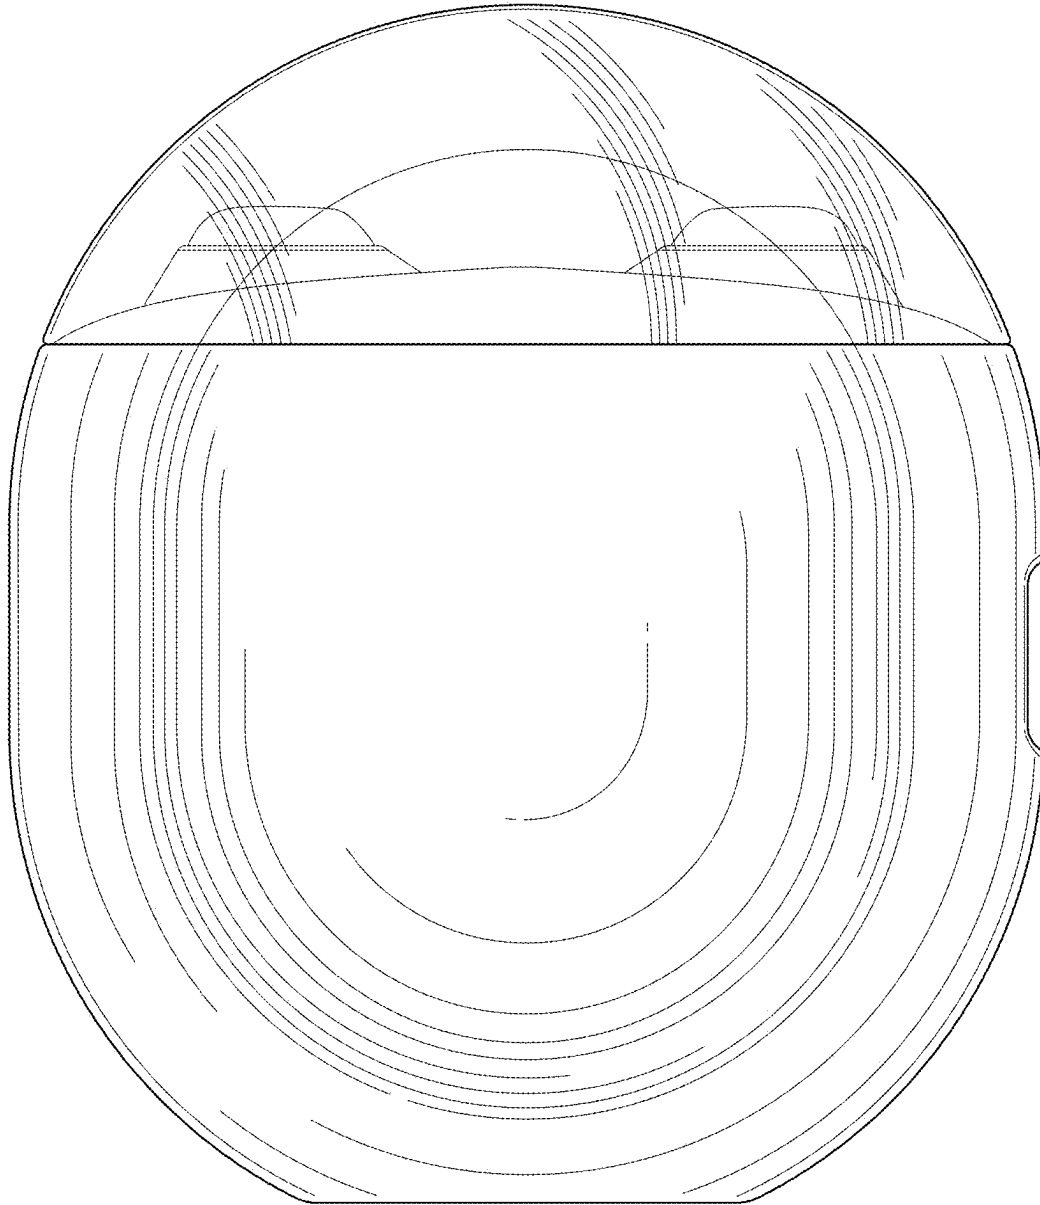


FIG. 2

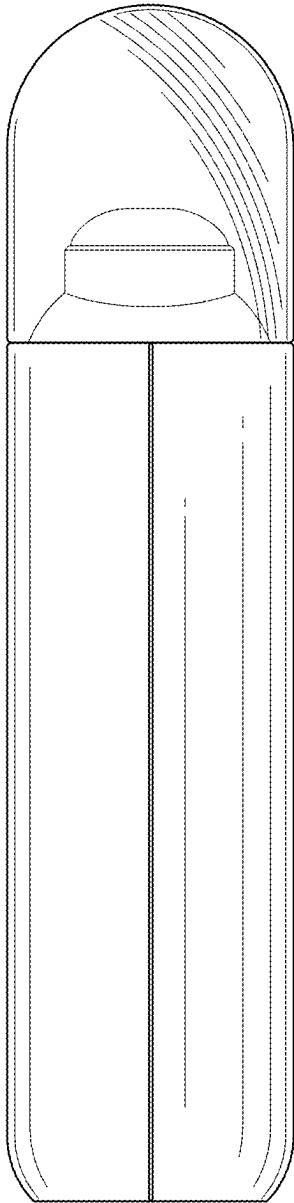


FIG. 3

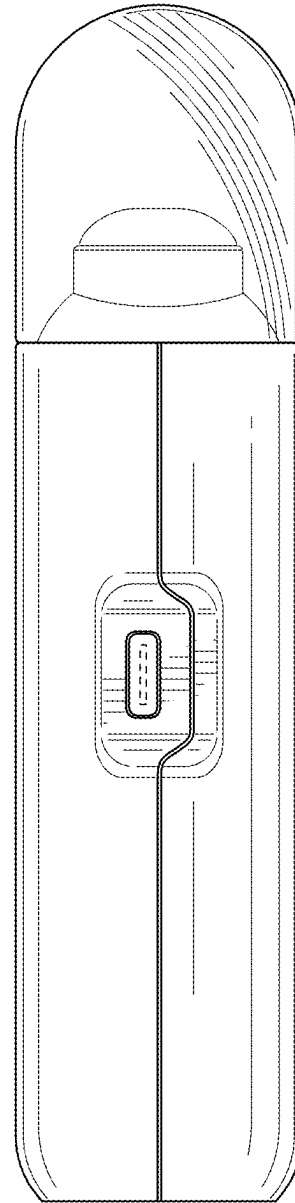


FIG. 4

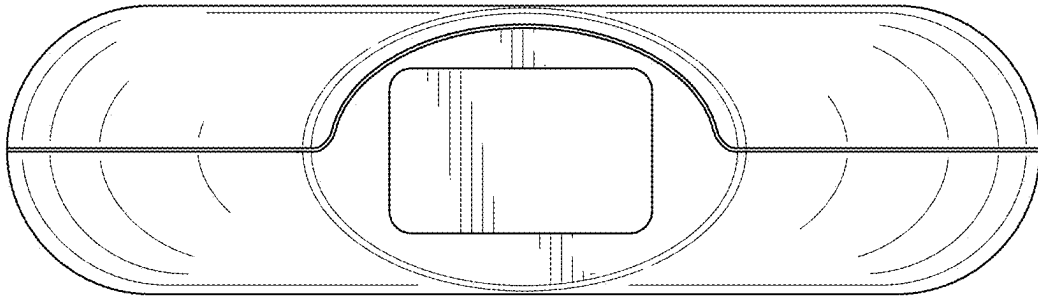


FIG. 5

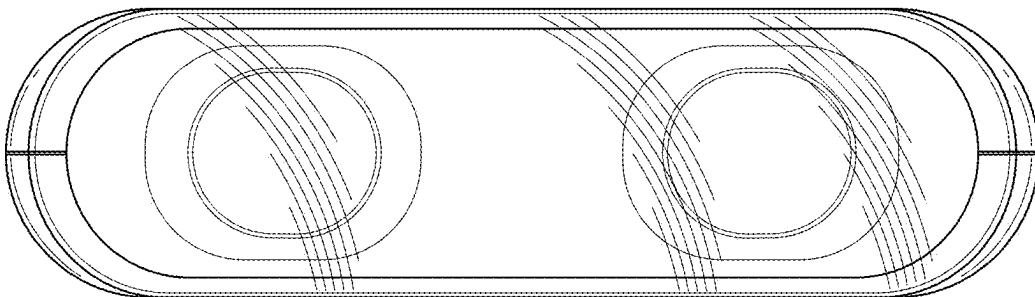


FIG. 6