



US012402902B2

(12) **United States Patent**
Vale et al.

(10) **Patent No.:** **US 12,402,902 B2**

(45) **Date of Patent:** **Sep. 2, 2025**

(54) **DEVICES AND METHODS FOR REMOVAL OF ACUTE BLOCKAGES FROM BLOOD VESSELS**

(71) Applicant: **Neuravi Limited**, Galway (IE)

(72) Inventors: **David Vale**, Barna (IE); **Eamon Brady**, Loughrea (IE); **Michael Gilvarry**, Headford (IE); **David Hardiman**, Dublin (IE); **Brendan Casey**, Barna (IE)

(73) Assignee: **Neuravi Limited**, Galway (IE)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 840 days.

(21) Appl. No.: **17/409,424**

(22) Filed: **Aug. 23, 2021**

(65) **Prior Publication Data**

US 2021/0378695 A1 Dec. 9, 2021

Related U.S. Application Data

(60) Division of application No. 16/248,539, filed on Jan. 15, 2019, now Pat. No. 11,103,264, which is a (Continued)

(51) **Int. Cl.**
A61B 17/221 (2006.01)
A61L 31/02 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 17/221** (2013.01); **A61L 31/022** (2013.01); **B05D 1/322** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC A61F 2/91; A61B 17/0057; A61B 17/221; B23K 26/38

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,070,791 A 12/1962 Ferrera et al.
4,455,717 A 6/1984 Gray
(Continued)

FOREIGN PATENT DOCUMENTS

CN 2557083 Y 6/2003
CN 101172051 A 5/2008
(Continued)

OTHER PUBLICATIONS

US 6,348,062 B1, 02/2002, Hopkins et al. (withdrawn)
US 6,348,062, 7/2003, Hopkins, et al. (withdrawn)

Primary Examiner — Dah-Wei D. Yuan


Assistant Examiner — Andrew J Bowman

(74) *Attorney, Agent, or Firm* — Troutman Pepper Locke LLP

(57) **ABSTRACT**

Manufacturing an expandable body of a clot retrieval device having a first coating of radiopaque material defining a plurality of micro-columns and a second coating, the method including applying the first coating to strut elements, removing at least a portion of the first coating from at least one area of the strut elements, and cutting away regions of both the first coating and the strut elements to form an interconnected pattern of coated and uncoated regions.

13 Claims, 12 Drawing Sheets

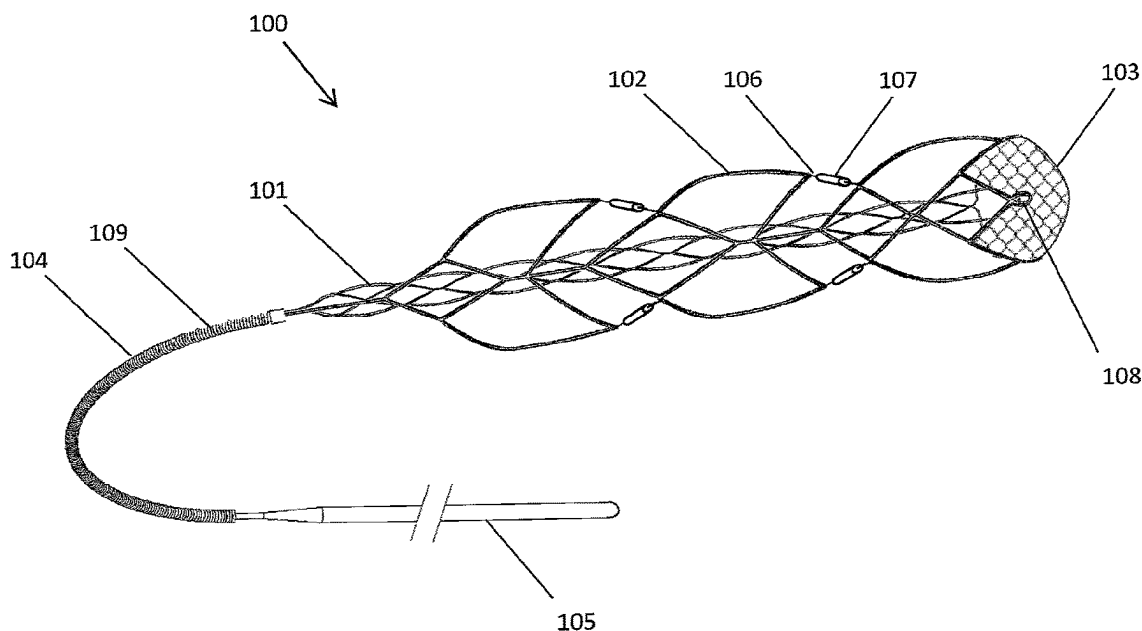

Related U.S. Application Data

continuation of application No. 14/207,069, filed on Mar. 12, 2014, now Pat. No. 10,201,360.

- (60) Provisional application No. 61/784,940, filed on Mar. 14, 2013.

(51) **Int. Cl.**

B05D 1/32 (2006.01)

B05D 3/12 (2006.01)

A61B 17/00 (2006.01)

A61B 17/22 (2006.01)

A61B 90/00 (2016.01)

(52) **U.S. Cl.**

CPC **B05D 3/12** (2013.01); **A61B 2017/00526** (2013.01); **A61B 2017/00867** (2013.01); **A61B 2017/00942** (2013.01); **A61B 2017/00951** (2013.01); **A61B 2017/22034** (2013.01); **A61B 2017/2212** (2013.01); **A61B 2017/2217** (2013.01); **A61B 2090/3966** (2016.02)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,611,594 A 9/1986 Grayhack et al.
4,612,931 A 9/1986 Dormia
4,643,184 A 2/1987 Mobin-Uddin
4,727,873 A 3/1988 Mobin-Uddin
4,793,348 A 12/1988 Palmaz
4,873,978 A 10/1989 Ginsburg
5,011,488 A 4/1991 Ginsburg
5,084,065 A 1/1992 Macgregor et al.
5,092,839 A 3/1992 Kipperman
5,100,423 A 3/1992 Fearnot
5,102,415 A 4/1992 Guenther et al.
5,108,419 A 4/1992 Reger et al.
5,122,136 A 6/1992 Guglielmi et al.
5,163,951 A 11/1992 Pinchuk et al.
5,171,233 A 12/1992 Amplatz et al.
5,171,259 A 12/1992 Inoue
5,217,441 A 6/1993 Shichman
5,234,437 A 8/1993 Sepetka
5,236,447 A 8/1993 Kubo et al.
5,330,482 A 7/1994 Gibbs et al.
5,383,887 A 1/1995 Nadal
5,387,219 A 2/1995 Rappe
5,387,226 A 2/1995 Miraki
5,449,372 A 9/1995 Schmaltz et al.
5,499,985 A 3/1996 Hein et al.
5,538,512 A 7/1996 Zenzon et al.
5,538,515 A 7/1996 Kafry et al.
5,549,626 A 8/1996 Miller et al.
5,558,652 A 9/1996 Henke
5,609,627 A 3/1997 Goicoechea et al.
5,624,461 A 4/1997 Mariant
5,639,277 A 6/1997 Mariant et al.
5,639,278 A 6/1997 Dereume et al.
5,645,558 A 7/1997 Horton
5,653,605 A 8/1997 Woehl et al.
5,658,296 A 8/1997 Bates et al.
5,665,117 A 9/1997 Rhodes
5,695,519 A 12/1997 Summers et al.
5,709,704 A 1/1998 Nott et al.
5,713,853 A 2/1998 Clark et al.
5,733,325 A 3/1998 Robinson et al.
5,769,871 A 6/1998 Mers Kelly et al.
5,769,884 A 6/1998 Solovay
5,779,686 A 7/1998 Sato et al.
5,779,716 A 7/1998 Cano et al.
5,800,519 A 9/1998 Sandock
5,810,874 A 9/1998 Lefebvre
5,814,064 A 9/1998 Daniel et al.
5,824,041 A 10/1998 Lenker et al.
5,827,304 A 10/1998 Hart

5,853,422 A 12/1998 Huebsch et al.
5,855,598 A 1/1999 Pinchuk
5,893,869 A 4/1999 Barnhart et al.
5,895,398 A 4/1999 Wensel et al.
5,897,567 A 4/1999 Ressemann et al.
5,904,698 A 5/1999 Thomas et al.
5,911,702 A 6/1999 Romley et al.
5,911,725 A 6/1999 Boury
5,919,126 A 7/1999 Armini
5,931,509 A 8/1999 Bartholomew
5,935,139 A 8/1999 Bates
5,947,995 A 9/1999 Samuels
6,063,113 A 5/2000 Kavteladze et al.
6,066,149 A 5/2000 Samson et al.
6,066,158 A 5/2000 Engelson et al.
6,093,196 A 7/2000 Okada
6,093,199 A 7/2000 Brown et al.
6,096,053 A 8/2000 Bates
6,099,534 A 8/2000 Bates et al.
6,099,559 A 8/2000 Nolting
6,102,932 A 8/2000 Kurz
6,106,548 A 8/2000 Roubin et al.
6,129,739 A 10/2000 Khosravi
6,143,022 A 11/2000 Shull et al.
6,146,404 A 11/2000 Kim et al.
6,156,064 A 12/2000 Chouinard
6,165,194 A 12/2000 Denardo
6,165,199 A 12/2000 Barbut
6,168,604 B1 1/2001 Cano
6,168,622 B1 1/2001 Mazzocchi
6,174,318 B1 1/2001 Bates et al.
6,174,329 B1 * 1/2001 Callo A61F 2/91
606/198
6,179,861 B1 1/2001 Khosravi et al.
6,203,561 B1 3/2001 Ramee et al.
6,214,026 B1 4/2001 Lepak et al.
6,221,006 B1 4/2001 Dubrul et al.
6,221,096 B1 4/2001 Aiba et al.
6,231,597 B1 5/2001 Deem et al.
6,238,412 B1 5/2001 Dubrul et al.
6,245,012 B1 6/2001 Kleshinski
6,245,087 B1 6/2001 Addis
6,251,122 B1 6/2001 Tsukernik
6,254,571 B1 7/2001 Hart
6,264,663 B1 7/2001 Cano
6,267,777 B1 7/2001 Bosma et al.
6,290,710 B1 9/2001 Cryer et al.
6,312,444 B1 11/2001 Barbut
6,315,778 B1 11/2001 Gambale et al.
6,325,815 B1 12/2001 Kusleika et al.
6,325,819 B1 12/2001 Pavcnik et al.
6,334,864 B1 1/2002 Amplatz et al.
6,336,934 B1 1/2002 Gilson et al.
6,346,116 B1 2/2002 Brooks et al.
6,348,056 B1 2/2002 Bates et al.
6,355,057 B1 3/2002 DeMarais et al.
6,361,545 B1 3/2002 Macoviak et al.
6,364,895 B1 4/2002 Greenhalgh
6,375,668 B1 4/2002 Gifford et al.
6,375,670 B1 4/2002 Greenhalgh
6,383,205 B1 5/2002 Samson et al.
6,383,206 B1 5/2002 Gillick et al.
6,391,037 B1 5/2002 Greenhalgh
6,402,771 B1 6/2002 Palmer et al.
6,416,541 B2 7/2002 Denardo
6,425,909 B1 7/2002 Dieck et al.
6,428,558 B1 8/2002 Jones et al.
6,432,122 B1 8/2002 Gilson et al.
6,436,112 B2 8/2002 Wensel et al.
6,458,139 B1 10/2002 Palmer et al.
6,485,497 B2 11/2002 Wensel et al.
6,485,501 B1 11/2002 Green
6,485,502 B2 11/2002 Don Michael et al.
6,488,701 B1 12/2002 Nolting et al.
6,511,492 B1 1/2003 Rosenbluth et al.
6,530,935 B2 3/2003 Wensel et al.
6,530,939 B1 3/2003 Hopkins et al.
6,537,294 B1 3/2003 Boyle et al.
6,540,768 B1 4/2003 Diaz et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,544,279 B1	4/2003	Hopkins et al.	7,288,112 B2	10/2007	Denardo et al.
6,551,341 B2	4/2003	Boylan et al.	7,300,458 B2	11/2007	Henkes et al.
6,551,342 B1	4/2003	Shen et al.	7,306,618 B2	12/2007	Demond et al.
6,575,996 B1	6/2003	Denison et al.	7,314,483 B2	1/2008	Landau et al.
6,575,997 B1	6/2003	Palmer et al.	7,316,692 B2	1/2008	Huffmaster
6,582,448 B1	6/2003	Boyle et al.	7,323,001 B2	1/2008	Clubb et al.
6,585,756 B1	7/2003	Strecker	7,331,976 B2	2/2008	McGuckin, Jr. et al.
6,589,265 B1	7/2003	Palmer et al.	7,344,550 B2	3/2008	Carrison et al.
6,592,607 B1	7/2003	Palmer et al.	D568,476 S	5/2008	Cottone, Jr. et al.
6,592,614 B2	7/2003	Lenker et al.	D569,976 S	5/2008	Raj D. et al.
6,592,616 B1	7/2003	Stack et al.	7,399,308 B2	7/2008	Borillo et al.
6,602,265 B2	8/2003	Dubrul et al.	7,410,491 B2	8/2008	Hopkins et al.
6,602,271 B2	8/2003	Adams et al.	7,425,215 B2	9/2008	Boyle et al.
6,602,272 B2	8/2003	Boylan et al.	7,452,496 B2	11/2008	Brady et al.
6,605,102 B1	8/2003	Mazzocchi et al.	7,491,215 B2	2/2009	Vale et al.
6,610,077 B1	8/2003	Hancock et al.	7,491,216 B2	2/2009	Brady
6,616,679 B1	9/2003	Khosravi et al.	7,510,565 B2	3/2009	Gilson et al.
6,632,241 B1	10/2003	Hancock et al.	7,534,252 B2	5/2009	Sepetka et al.
6,638,245 B2	10/2003	Miller et al.	7,556,636 B2	7/2009	Mazzocchi et al.
6,638,293 B1	10/2003	Makower et al.	D597,671 S	8/2009	Cottone, Jr. et al.
6,641,590 B1	11/2003	Palmer et al.	7,582,111 B2	9/2009	Krolik et al.
6,656,218 B1	12/2003	Denardo et al.	7,594,926 B2	9/2009	Linder et al.
6,660,021 B1	12/2003	Palmer et al.	7,604,649 B2	10/2009	McGuckin, Jr. et al.
6,663,650 B2	12/2003	Sepetka et al.	7,604,650 B2	10/2009	Bergheim
D484,979 S	1/2004	Fontaine	7,618,434 B2	11/2009	Santra et al.
6,673,089 B1	1/2004	Yassour et al.	7,662,165 B2	2/2010	Gilson et al.
6,685,722 B1	2/2004	Rosenbluth et al.	D612,499 S	3/2010	Ondracek et al.
6,692,504 B2	2/2004	Kurz et al.	7,670,356 B2	3/2010	Mazzocchi et al.
6,692,508 B2	2/2004	Wensel et al.	7,678,123 B2	3/2010	Chanduszko
6,692,509 B2	2/2004	Wensel et al.	7,691,121 B2	4/2010	Rosenbluth et al.
6,695,858 B1	2/2004	Dubrul et al.	7,691,124 B2	4/2010	Balgobin
6,702,782 B2	3/2004	Miller et al.	7,708,770 B2	5/2010	Linder et al.
6,702,834 B1	3/2004	Boylan et al.	7,717,929 B2	5/2010	Fallman
6,709,465 B2	3/2004	Mitchell et al.	7,736,385 B2	6/2010	Agnew
6,712,834 B2	3/2004	Yassour et al.	7,749,246 B2	7/2010	McGuckin, Jr. et al.
6,726,701 B2	4/2004	Gilson et al.	7,758,606 B2	7/2010	Streeter et al.
6,726,703 B2	4/2004	Broome et al.	7,758,611 B2	7/2010	Kato
6,730,104 B1	5/2004	Sepetka et al.	D622,387 S	8/2010	Igaki
6,783,528 B2	8/2004	Vincent-Prestigiacomo	D622,388 S	8/2010	Igaki
6,783,538 B2	8/2004	McGuckin, Jr. et al.	7,766,934 B2	8/2010	Pal et al.
6,824,545 B2	11/2004	Sepetka et al.	7,771,452 B2	8/2010	Pal et al.
6,855,155 B2	2/2005	Denardo et al.	7,780,694 B2	8/2010	Palmer et al.
6,878,163 B2	4/2005	Denardo et al.	7,780,700 B2	8/2010	Frazier et al.
6,890,340 B2	5/2005	Duane	7,811,305 B2	10/2010	Balgobin et al.
6,913,612 B2	7/2005	Palmer et al.	7,815,659 B2	10/2010	Conlon et al.
6,913,618 B2	7/2005	Denardo et al.	7,819,893 B2	10/2010	Brady et al.
6,939,361 B1	9/2005	Kleshinski	7,828,815 B2	11/2010	Mazzocchi et al.
6,953,472 B2	10/2005	Palmer et al.	7,828,816 B2	11/2010	Mazzocchi et al.
6,989,019 B2	1/2006	Mazzocchi et al.	7,833,240 B2	11/2010	Okushi et al.
6,989,021 B2	1/2006	Bosma et al.	7,842,053 B2	11/2010	Chanduszko et al.
6,994,718 B2	2/2006	Groothuis et al.	7,846,175 B2	12/2010	Bonnette et al.
7,004,954 B1	2/2006	Voss et al.	7,846,176 B2	12/2010	Gilson et al.
7,004,955 B2	2/2006	Shen et al.	7,850,708 B2	12/2010	Pal
7,004,956 B2	2/2006	Palmer et al.	7,883,516 B2	2/2011	Huang et al.
7,008,434 B2	3/2006	Kurz et al.	7,887,560 B2	2/2011	Kusleika
7,033,376 B2	4/2006	Tsukernik	D635,261 S	3/2011	Rossi
7,041,116 B2	5/2006	Goto et al.	D635,262 S	3/2011	Rossi
7,048,758 B2	5/2006	Boyle et al.	7,901,426 B2	3/2011	Gilson et al.
7,052,500 B2	5/2006	Bashiri et al.	7,914,549 B2	3/2011	Morsi
7,058,456 B2	6/2006	Pierce	7,922,732 B2	4/2011	Mazzocchi et al.
7,063,707 B2	6/2006	Bose et al.	7,927,784 B2	4/2011	Simpson
7,083,633 B2	8/2006	Morrill et al.	7,931,659 B2	4/2011	Bose et al.
7,083,822 B2	8/2006	Brightbill	7,998,165 B2	8/2011	Huffmaster
7,094,249 B1	8/2006	Broome et al.	8,002,822 B2	8/2011	Glocker et al.
7,097,653 B2	8/2006	Freudenthal et al.	8,021,379 B2	9/2011	Thompson et al.
7,101,380 B2	9/2006	Khachin et al.	8,021,380 B2	9/2011	Thompson et al.
7,172,614 B2	2/2007	Boyle et al.	8,043,326 B2	10/2011	Hancock et al.
7,175,655 B1	2/2007	Molaei	8,048,151 B2	11/2011	O'Brien et al.
7,179,273 B1	2/2007	Palmer et al.	8,052,640 B2	11/2011	Fiorella et al.
7,185,922 B2	3/2007	Takayanagi et al.	8,057,497 B1	11/2011	Raju et al.
7,220,271 B2	5/2007	Clubb et al.	8,057,507 B2	11/2011	Horan et al.
7,226,464 B2	6/2007	Garner et al.	8,066,757 B2	11/2011	Ferrera et al.
7,229,472 B2	6/2007	DePalma et al.	D652,927 S	1/2012	Braido et al.
7,241,304 B2	7/2007	Boyle et al.	D653,341 S	1/2012	Braido et al.
7,241,308 B2	7/2007	Andreas et al.	8,088,140 B2	1/2012	Ferrera et al.
			8,100,935 B2	1/2012	Rosenbluth et al.
			8,109,941 B2	2/2012	Richardson
			8,118,829 B2	2/2012	Carrison et al.
			8,118,856 B2	2/2012	Schreck et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,123,769 B2	2/2012	Osborne	9,161,766 B2	10/2015	Slee et al.
8,137,376 B2	3/2012	Clubb et al.	9,173,668 B2	11/2015	Ulm, III
8,137,377 B2	3/2012	Palmer et al.	9,186,487 B2	11/2015	Dubrul et al.
8,142,422 B2	3/2012	Makower et al.	9,198,687 B2	12/2015	Fulkerson et al.
8,142,442 B2	3/2012	Palmer et al.	9,204,887 B2	12/2015	Cully et al.
D660,433 S	5/2012	Braido et al.	9,211,132 B2	12/2015	Bowman
D660,967 S	5/2012	Braido et al.	9,232,992 B2	1/2016	Heidner et al.
8,182,508 B2	5/2012	Magnuson et al.	9,254,371 B2	2/2016	Martin et al.
8,187,298 B2	5/2012	Pal	9,301,769 B2	4/2016	Brady et al.
8,246,641 B2	8/2012	Osborne et al.	9,332,999 B2	5/2016	Ray et al.
8,246,672 B2	8/2012	Osborne	9,402,707 B2	8/2016	Brady et al.
8,252,017 B2	8/2012	Paul, Jr. et al.	9,445,829 B2	9/2016	Brady et al.
8,252,018 B2	8/2012	Valaie	9,456,834 B2	10/2016	Folk
8,262,689 B2	9/2012	Schneiderman et al.	9,532,792 B2	1/2017	Galdonik et al.
8,282,668 B2	10/2012	McGuckin, Jr. et al.	9,532,873 B2	1/2017	Kelley
8,298,257 B2	10/2012	Sepetka et al.	9,533,344 B2	1/2017	Monetti et al.
RE43,882 E	12/2012	Hopkins et al.	9,539,011 B2	1/2017	Chen et al.
8,357,178 B2	1/2013	Grandfield et al.	9,539,022 B2	1/2017	Bowman
8,357,179 B2	1/2013	Grandfield et al.	9,539,122 B2	1/2017	Burke et al.
8,357,180 B2	1/2013	Feller, III et al.	9,539,382 B2	1/2017	Nelson
8,357,893 B2	1/2013	Xu et al.	9,549,830 B2	1/2017	Bruszewski et al.
8,361,095 B2	1/2013	Osborne	9,554,805 B2	1/2017	Tompkins et al.
8,361,110 B2	1/2013	Chanduszko	9,561,125 B2	2/2017	Bowman et al.
8,366,663 B2	2/2013	Fiorella et al.	9,572,982 B2	2/2017	Burnes et al.
8,409,215 B2	4/2013	Sepetka et al.	9,579,104 B2	2/2017	Beckham et al.
8,414,482 B2	4/2013	Belson	9,579,484 B2	2/2017	Barnell
8,414,543 B2	4/2013	McGuckin, Jr. et al.	9,585,642 B2	3/2017	Dinsmoor et al.
8,419,748 B2	4/2013	Valaie	9,615,832 B2	4/2017	Bose et al.
8,460,312 B2	6/2013	Bose et al.	9,615,951 B2	4/2017	Bennett et al.
8,460,313 B2	6/2013	Huffmaster	9,622,753 B2	4/2017	Cox
8,486,104 B2	7/2013	Samson et al.	9,636,115 B2	5/2017	Henry et al.
8,512,352 B2	8/2013	Martin	9,636,439 B2	5/2017	Chu et al.
8,529,596 B2	9/2013	Grandfield et al.	9,642,639 B2	5/2017	Brady et al.
8,545,526 B2	10/2013	Martin et al.	9,642,675 B2	5/2017	Werneth et al.
8,574,262 B2	11/2013	Ferrera et al.	9,655,633 B2	5/2017	Leynov et al.
8,579,915 B2	11/2013	French et al.	9,655,645 B2	5/2017	Staunton
8,585,713 B2	11/2013	Ferrera et al.	9,655,989 B2	5/2017	Cruise et al.
8,608,761 B2	12/2013	Osborne et al.	9,662,129 B2	5/2017	Galdonik et al.
8,679,142 B2	3/2014	Slee et al.	9,662,238 B2	5/2017	Dwork et al.
8,690,907 B1	4/2014	Janardhan et al.	9,662,425 B2	5/2017	Lilja et al.
8,696,622 B2	4/2014	Fiorella et al.	9,668,898 B2	6/2017	Wong
8,702,652 B2	4/2014	Fiorella et al.	9,675,477 B2	6/2017	Thompson
8,702,704 B2	4/2014	Shelton, IV et al.	9,675,782 B2	6/2017	Connolly
8,702,724 B2	4/2014	Olsen et al.	9,676,022 B2	6/2017	Ensign et al.
8,777,976 B2	7/2014	Brady et al.	9,692,557 B2	6/2017	Murphy
8,777,979 B2	7/2014	Shrivastava et al.	9,693,852 B2	7/2017	Lam et al.
8,784,434 B2	7/2014	Rosenbluth et al.	9,700,262 B2	7/2017	Janik et al.
8,784,441 B2	7/2014	Rosenbluth et al.	9,700,399 B2	7/2017	Acosta-Acevedo
8,795,305 B2	8/2014	Martin et al.	9,717,421 B2	8/2017	Griswold et al.
8,795,317 B2	8/2014	Grandfield et al.	9,717,500 B2	8/2017	Tieu et al.
8,795,345 B2	8/2014	Grandfield et al.	9,717,502 B2	8/2017	Teoh et al.
8,814,892 B2	8/2014	Galdonik et al.	9,724,103 B2	8/2017	Cruise et al.
8,814,925 B2	8/2014	Hilaire et al.	9,724,526 B2	8/2017	Strother et al.
8,852,205 B2	10/2014	Brady et al.	9,750,565 B2	9/2017	Bloom et al.
8,870,941 B2	10/2014	Evans et al.	9,757,260 B2	9/2017	Greenan
8,900,265 B1	12/2014	Ulm, III	9,764,111 B2	9/2017	Gulachenski
8,920,358 B2	12/2014	Levine et al.	9,770,251 B2	9/2017	Bowman et al.
8,939,991 B2	1/2015	Krolik et al.	9,770,577 B2	9/2017	Li et al.
D723,165 S	2/2015	Chanduszko	9,775,621 B2	10/2017	Tompkins et al.
D723,166 S	2/2015	Igaki et al.	9,775,706 B2	10/2017	Peterson et al.
8,945,143 B2	2/2015	Ferrera et al.	9,775,732 B2	10/2017	Khenansho
8,945,160 B2	2/2015	Krolik et al.	9,788,800 B2	10/2017	Mayoras, Jr.
8,945,169 B2	2/2015	Pal	9,795,391 B2	10/2017	Saatchi et al.
8,945,172 B2	2/2015	Ferrera et al.	9,801,651 B2	10/2017	Harrah et al.
8,956,399 B2	2/2015	Cam et al.	9,801,980 B2	10/2017	Karino et al.
8,968,330 B2	3/2015	Rosenbluth et al.	D802,765 S	11/2017	Erzberger et al.
9,011,481 B2	4/2015	Aggerholm et al.	9,808,599 B2	11/2017	Bowman et al.
9,039,749 B2	5/2015	Shrivastava et al.	9,833,252 B2	12/2017	Sepetka et al.
9,072,537 B2	7/2015	Grandfield et al.	9,833,304 B2	12/2017	Horan et al.
9,095,342 B2	8/2015	Becking et al.	9,833,604 B2	12/2017	Lam et al.
9,113,936 B2	8/2015	Palmer et al.	9,833,625 B2	12/2017	Waldhauser et al.
9,119,656 B2	9/2015	Bose et al.	9,901,434 B2	2/2018	Hoffman
9,138,307 B2	9/2015	Valaie	9,918,720 B2	3/2018	Marchand et al.
9,155,552 B2	10/2015	Ulm, III	10,016,206 B1	7/2018	Yang
9,161,758 B2	10/2015	Figulla et al.	10,070,878 B2	9/2018	Ma
			10,098,651 B2	10/2018	Marchand et al.
			D834,193 S	11/2018	Erzberger et al.
			10,201,360 B2	2/2019	Vale et al.
			10,231,751 B2	3/2019	Sos

(56)

References Cited

U.S. PATENT DOCUMENTS

10,292,723 B2	5/2019	Brady et al.	2003/0153944 A1	8/2003	Phung et al.
10,299,811 B2	5/2019	Brady et al.	2003/0163064 A1	8/2003	Vrba et al.
10,363,054 B2	7/2019	Vale et al.	2003/0163158 A1	8/2003	White
10,376,274 B2	8/2019	Farin et al.	2003/0171769 A1	9/2003	Barbut
10,390,850 B2	8/2019	Vale et al.	2003/0171771 A1	9/2003	Anderson et al.
10,524,811 B2	1/2020	Marchand et al.	2003/0176884 A1	9/2003	Berrada et al.
10,531,942 B2	1/2020	Eggers	2003/0187495 A1	10/2003	Cully et al.
D875,250 S	2/2020	Hillukka	2003/0195537 A1	10/2003	Dubrul et al.
D875,935 S	2/2020	Erzberger et al.	2003/0195554 A1	10/2003	Shen et al.
D881,396 S	4/2020	Qiu et al.	2003/0199917 A1	10/2003	Knudson et al.
10,617,435 B2	4/2020	Vale et al.	2003/0204202 A1	10/2003	Palmer et al.
D883,485 S	5/2020	Carpenter et al.	2003/0208224 A1	11/2003	Broome
D887,003 S	6/2020	Garza et al.	2003/0212430 A1*	11/2003	Bose A61B 17/221 606/200
D889,653 S	7/2020	Erzberger et al.	2003/0236533 A1	12/2003	Wilson et al.
10,722,257 B2	7/2020	Skillrud et al.	2004/0044399 A1	3/2004	Ventura
D910,852 S	2/2021	Zeng et al.	2004/0064179 A1	4/2004	Linder et al.
11,439,418 B2	9/2022	O'Malley	2004/0068288 A1	4/2004	Palmer et al.
D965,787 S	10/2022	Park et al.	2004/0073243 A1	4/2004	Sepetka et al.
11,517,340 B2	12/2022	Casey	2004/0079429 A1	4/2004	Miller et al.
D977,101 S	1/2023	Armer et al.	2004/0082962 A1	4/2004	Demarais et al.
D987,080 S	5/2023	Thomas et al.	2004/0082967 A1	4/2004	Broome et al.
D1,039,153 S	8/2024	Armer et al.	2004/0088001 A1	5/2004	Bosma et al.
D1,039,700 S	8/2024	Spenser et al.	2004/0093065 A1	5/2004	Yachia et al.
D1,046,151 S	10/2024	Park et al.	2004/0098050 A1	5/2004	Foerster et al.
D1,078,039 S	6/2025	Tegg et al.	2004/0133231 A1	7/2004	Maitland et al.
2001/0001315 A1	5/2001	Bates et al.	2004/0133232 A1	7/2004	Rosenbluth et al.
2001/0016755 A1	8/2001	Addis	2004/0138692 A1	7/2004	Phung et al.
2001/0037141 A1	11/2001	Yee et al.	2004/0153117 A1	8/2004	Clubb et al.
2001/0041909 A1	11/2001	Tsugita et al.	2004/0153118 A1	8/2004	Clubb et al.
2001/0044632 A1	11/2001	Daniel et al.	2004/0199201 A1	10/2004	Kellett et al.
2001/0049554 A1	12/2001	Ruiz et al.	2004/0204749 A1	10/2004	Gunderson
2001/0051810 A1	12/2001	Dubrul et al.	2004/0215318 A1	10/2004	Kwitkin
2002/0004667 A1	1/2002	Adams et al.	2004/0220663 A1	11/2004	Rivelli
2002/0016609 A1	2/2002	Wensel et al.	2005/0010245 A1	1/2005	Wasicek
2002/0022859 A1	2/2002	Hogendijk	2005/0033348 A1	2/2005	Sepetka et al.
2002/0026211 A1	2/2002	Khosravi et al.	2005/0038447 A1	2/2005	Huffmaster
2002/0042627 A1	4/2002	Brady et al.	2005/0038468 A1	2/2005	Panetta et al.
2002/0049468 A1	4/2002	Streeter et al.	2005/0043759 A1	2/2005	Chanduszeko
2002/0052620 A1	5/2002	Barbut	2005/0049619 A1	3/2005	Sepetka et al.
2002/0058911 A1	5/2002	Gilson et al.	2005/0049669 A1	3/2005	Jones et al.
2002/0068954 A1	6/2002	Foster	2005/0049670 A1	3/2005	Jones et al.
2002/0072764 A1	6/2002	Sepetka et al.	2005/0055033 A1	3/2005	Leslie et al.
2002/0082558 A1	6/2002	Samson et al.	2005/0055047 A1	3/2005	Greenhalgh
2002/0091407 A1	7/2002	Zadno-Azizi et al.	2005/0059995 A1	3/2005	Sepetka et al.
2002/0095171 A1	7/2002	Belef	2005/0085849 A1	4/2005	Sepetka et al.
2002/0123765 A1	9/2002	Sepetka et al.	2005/0090779 A1	4/2005	Osyepka
2002/0128680 A1	9/2002	Pavlovic	2005/0090857 A1	4/2005	Kusleika et al.
2002/0138094 A1	9/2002	Borillo et al.	2005/0125024 A1	6/2005	Sepetka et al.
2002/0143349 A1	10/2002	Gifford, III et al.	2005/0171566 A1	8/2005	Kanamaru
2002/0143362 A1	10/2002	Macoviak et al.	2005/0192627 A1	9/2005	Whisenant et al.
2002/0156455 A1	10/2002	Barbut	2005/0215942 A1	9/2005	Abrahamson et al.
2002/0161393 A1	10/2002	Demonet et al.	2005/0216030 A1	9/2005	Sepetka et al.
2002/0165576 A1	11/2002	Boyle et al.	2005/0216050 A1	9/2005	Sepetka et al.
2002/0173819 A1	11/2002	Leefflang et al.	2005/0228417 A1	10/2005	Teitelbaum et al.
2002/0183787 A1	12/2002	Wahr et al.	2005/0251206 A1	11/2005	Maahs et al.
2002/0188276 A1	12/2002	Evans et al.	2005/0251209 A1	11/2005	Saadat et al.
2002/0188314 A1	12/2002	Anderson et al.	2005/0267491 A1	12/2005	Kellett et al.
2002/0193824 A1	12/2002	Boylan et al.	2005/0273135 A1	12/2005	Chanduszeko et al.
2002/0198588 A1	12/2002	Armstrong et al.	2005/0283186 A1	12/2005	Berrada et al.
2003/0004536 A1	1/2003	Boylan et al.	2005/0288686 A1	12/2005	Sepetka et al.
2003/0004538 A1	1/2003	Secrest et al.	2006/0009798 A1	1/2006	Callister et al.
2003/0004540 A1	1/2003	Linder et al.	2006/0009799 A1	1/2006	Kleshinski et al.
2003/0004542 A1	1/2003	Wensel et al.	2006/0020285 A1	1/2006	Niermann
2003/0009146 A1	1/2003	Muni et al.	2006/0020286 A1	1/2006	Niermann
2003/0009191 A1	1/2003	Wensel et al.	2006/0030877 A1	2/2006	Martinez et al.
2003/0038447 A1	2/2003	Cantele	2006/0041228 A1	2/2006	Vo et al.
2003/0040772 A1	2/2003	Hyodoh et al.	2006/0058836 A1	3/2006	Bose et al.
2003/0050663 A1	3/2003	Khachin et al.	2006/0058837 A1	3/2006	Bose et al.
2003/0069520 A1	4/2003	Skujins et al.	2006/0058838 A1	3/2006	Bose et al.
2003/0114879 A1	6/2003	Euteneuer et al.	2006/0064151 A1	3/2006	Guterman et al.
2003/0125798 A1	7/2003	Martin	2006/0069424 A1	3/2006	Acosta et al.
2003/0130682 A1	7/2003	Broome et al.	2006/0074477 A1	4/2006	Berthiaume et al.
2003/0144687 A1	7/2003	Brady et al.	2006/0142838 A1	6/2006	Molaei et al.
2003/0144688 A1	7/2003	Brady et al.	2006/0149313 A1	7/2006	Arguello et al.
2003/0153943 A1	8/2003	Michael et al.	2006/0155305 A1	7/2006	Freudenthal et al.
			2006/0161187 A1	7/2006	Levine et al.
			2006/0195137 A1	8/2006	Sepetka et al.
			2006/0224176 A1	10/2006	Fung et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2006/0224177 A1	10/2006	Finitis	2009/0069828 A1	3/2009	Martin et al.
2006/0224179 A1	10/2006	Kucharczyk et al.	2009/0076539 A1	3/2009	Valaie
2006/0229638 A1	10/2006	Abrams et al.	2009/0088793 A1	4/2009	Bagaoisan et al.
2006/0235501 A1	10/2006	Igaki	2009/0088795 A1	4/2009	Cahill
2006/0241677 A1	10/2006	Johnson et al.	2009/0105722 A1	4/2009	Fulkerson et al.
2006/0282111 A1	12/2006	Morsi	2009/0105737 A1	4/2009	Fulkerson et al.
2006/0287668 A1	12/2006	Fawzi et al.	2009/0105747 A1	4/2009	Chanduszko et al.
2006/0287701 A1	12/2006	Pal	2009/0149881 A1	6/2009	Vale et al.
2006/0293706 A1	12/2006	Shimon	2009/0163851 A1	6/2009	Holloway et al.
2007/0010857 A1	1/2007	Sugimoto et al.	2009/0177206 A1	7/2009	Lozier et al.
2007/0032879 A1	2/2007	Levine et al.	2009/0182336 A1	7/2009	Brenzel et al.
2007/0088382 A1	4/2007	Bei et al.	2009/0281610 A1	11/2009	Parker
2007/0088383 A1	4/2007	Pal et al.	2009/0281619 A1	11/2009	Le et al.
2007/0100348 A1	5/2007	Cauthen, III et al.	2009/0287229 A1	11/2009	Ogdahl
2007/0118173 A1	5/2007	Magnuson et al.	2009/0292297 A1	11/2009	Ferrere
2007/0135826 A1	6/2007	Zaver et al.	2009/0292307 A1	11/2009	Razack
2007/0149997 A1	6/2007	Muller	2009/0299393 A1	12/2009	Martin et al.
2007/0156170 A1	7/2007	Hancock et al.	2009/0299403 A1	12/2009	Chanduszko et al.
2007/0165170 A1	7/2007	Fukuda	2009/0306702 A1	12/2009	Miloslavski et al.
2007/0173921 A1	7/2007	Wholey et al.	2009/0326636 A1	12/2009	Hashimoto et al.
2007/0179527 A1	8/2007	Eskuri et al.	2010/0004607 A1	1/2010	Wilson et al.
2007/0191866 A1	8/2007	Palmer et al.	2010/0076482 A1	3/2010	Shu et al.
2007/0198028 A1	8/2007	Miloslavski et al.	2010/0087850 A1	4/2010	Razack
2007/0198051 A1	8/2007	Clubb et al.	2010/0087908 A1	4/2010	Hilaire et al.
2007/0198075 A1	8/2007	Levy	2010/0114017 A1	5/2010	Lenker et al.
2007/0208367 A1	9/2007	Fiorella et al.	2010/0125326 A1	5/2010	Kalstad et al.
2007/0208371 A1	9/2007	French et al.	2010/0125327 A1	5/2010	Agnew
2007/0219612 A1	9/2007	Andreas et al.	2010/0191272 A1	7/2010	Keating
2007/0225749 A1	9/2007	Martin et al.	2010/0211094 A1	8/2010	Sargent, Jr.
2007/0233175 A1	10/2007	Zaver et al.	2010/0268264 A1	10/2010	Bonnette et al.
2007/0244505 A1	10/2007	Gilson et al.	2010/0268265 A1	10/2010	Krolik et al.
2007/0270902 A1	11/2007	Slazas et al.	2010/0274277 A1	10/2010	Eaton
2007/0288054 A1	12/2007	Tanaka et al.	2010/0318178 A1	12/2010	Rapaport et al.
2008/0045881 A1	2/2008	Teitelbaum et al.	2010/0324649 A1	12/2010	Mattsson et al.
2008/0077227 A1	3/2008	Ouellette et al.	2010/0331949 A1	12/2010	Habib
2008/0082107 A1	4/2008	Miller et al.	2011/0009875 A1	1/2011	Grandfield et al.
2008/0086190 A1	4/2008	Ta	2011/0009940 A1	1/2011	Grandfield et al.
2008/0091223 A1	4/2008	Pokorney et al.	2011/0009950 A1	1/2011	Grandfield et al.
2008/0097386 A1	4/2008	Osyepka	2011/0015718 A1	1/2011	Schreck
2008/0109031 A1	5/2008	Sepetka et al.	2011/0022149 A1	1/2011	Cox et al.
2008/0109032 A1	5/2008	Sepetka et al.	2011/0040319 A1	2/2011	Fulton, III
2008/0119886 A1	5/2008	Greenhalgh et al.	2011/0054287 A1	3/2011	Schultz
2008/0125798 A1	5/2008	Osborne et al.	2011/0054504 A1	3/2011	Porter
2008/0177296 A1	7/2008	Sepetka et al.	2011/0054514 A1	3/2011	Arcand et al.
2008/0178890 A1	7/2008	Townsend et al.	2011/0054516 A1	3/2011	Keegan et al.
2008/0183197 A1	7/2008	Sepetka et al.	2011/0060212 A1	3/2011	Slee et al.
2008/0183198 A1	7/2008	Sepetka et al.	2011/0060359 A1	3/2011	Hannes et al.
2008/0183205 A1	7/2008	Sepetka et al.	2011/0106137 A1	5/2011	Shimon
2008/0188876 A1	8/2008	Sepetka et al.	2011/0125181 A1	5/2011	Brady et al.
2008/0188885 A1	8/2008	Sepetka et al.	2011/0152920 A1	6/2011	Eckhouse et al.
2008/0188887 A1	8/2008	Batiste	2011/0160763 A1	6/2011	Ferrera et al.
2008/0200946 A1	8/2008	Braun et al.	2011/0166586 A1	7/2011	Sepetka et al.
2008/0200947 A1	8/2008	Kusleika et al.	2011/0172678 A1	7/2011	Behl et al.
2008/0215077 A1	9/2008	Sepetka et al.	2011/0184456 A1	7/2011	Grandfield et al.
2008/0221600 A1	9/2008	Dieck et al.	2011/0196414 A1	8/2011	Porter et al.
2008/0228209 A1	9/2008	DeMello et al.	2011/0202088 A1	8/2011	Eckhouse et al.
2008/0234706 A1	9/2008	Sepetka et al.	2011/0208233 A1	8/2011	McGuckin, Jr. et al.
2008/0243170 A1	10/2008	Jenson et al.	2011/0213297 A1	9/2011	Aklog et al.
2008/0255596 A1	10/2008	Jenson et al.	2011/0213393 A1	9/2011	Aklog et al.
2008/0262410 A1	10/2008	Jenson et al.	2011/0213403 A1	9/2011	Aboytes
2008/0262528 A1	10/2008	Martin	2011/0224707 A1	9/2011	Miloslavski et al.
2008/0262532 A1	10/2008	Martin	2011/0270374 A1	11/2011	Orr et al.
2008/0262590 A1	10/2008	Murray	2011/0276120 A1	11/2011	Gilson et al.
2008/0269871 A1	10/2008	Eli	2011/0319917 A1	12/2011	Ferrera et al.
2008/0275488 A1	11/2008	Fleming	2012/0022572 A1	1/2012	Braun et al.
2008/0275493 A1	11/2008	Farmiga	2012/0041449 A1	2/2012	Eckhouse et al.
2008/0281350 A1	11/2008	Sepetka et al.	2012/0041469 A1	2/2012	Fischell et al.
2008/0296274 A1*	12/2008	Bialas	2012/0041474 A1	2/2012	Eckhouse et al.
		B23K 26/38 219/121.72	2012/0059356 A1	3/2012	di Palma et al.
2008/0312681 A1	12/2008	Ansel et al.	2012/0065660 A1	3/2012	Ferrera et al.
2009/0005853 A1	1/2009	Osman	2012/0083823 A1	4/2012	Shrivastava et al.
2009/0005858 A1	1/2009	Young et al.	2012/0083868 A1	4/2012	Shrivastava et al.
2009/0024157 A1	1/2009	Anukhin	2012/0089216 A1	4/2012	Rapaport et al.
2009/0030443 A1	1/2009	Buser et al.	2012/0101510 A1	4/2012	Lenker et al.
2009/0062841 A1	3/2009	Amplatz et al.	2012/0116440 A1	5/2012	Leynov et al.
			2012/0123466 A1	5/2012	Porter et al.
			2012/0143230 A1	6/2012	Sepetka et al.
			2012/0143237 A1	6/2012	Cam et al.
			2012/0143317 A1	6/2012	Cam et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0150147	A1	6/2012	Leynov et al.	2015/0313617	A1	11/2015	Grandfield et al.
2012/0165858	A1	6/2012	Eckhouse et al.	2015/0320431	A1	11/2015	Ulm
2012/0165859	A1	6/2012	Eckhouse et al.	2015/0352325	A1	12/2015	Quick
2012/0209312	A1	8/2012	Aggerholm et al.	2015/0359547	A1	12/2015	Vale et al.
2012/0215250	A1	8/2012	Grandfield et al.	2015/0366650	A1	12/2015	Zi et al.
2012/0277788	A1	11/2012	Cattaneo	2015/0374391	A1	12/2015	Quick et al.
2012/0283768	A1	11/2012	Cox et al.	2015/0374393	A1	12/2015	Brady et al.
2012/0296362	A1	11/2012	Cam et al.	2015/0374479	A1	12/2015	Vale
2012/0316600	A1	12/2012	Ferrera et al.	2016/0015402	A1	1/2016	Brady et al.
2012/0330350	A1	12/2012	Jones et al.	2016/0022296	A1	1/2016	Brady et al.
2013/0030460	A1	1/2013	Marks et al.	2016/0045298	A1	2/2016	Thinnes, Jr. et al.
2013/0030461	A1	1/2013	Marks et al.	2016/0066921	A1	3/2016	Seifert et al.
2013/0046330	A1	2/2013	McIntosh et al.	2016/0100928	A1	4/2016	Lees et al.
2013/0046333	A1	2/2013	Jones et al.	2016/0106448	A1	4/2016	Brady et al.
2013/0046334	A1	2/2013	Jones et al.	2016/0106449	A1	4/2016	Brady et al.
2013/0116774	A1	5/2013	Strauss et al.	2016/0113663	A1	4/2016	Brady et al.
2013/0131614	A1	5/2013	Hassan et al.	2016/0113664	A1	4/2016	Brady et al.
2013/0144311	A1	6/2013	Fung et al.	2016/0113665	A1	4/2016	Brady et al.
2013/0144326	A1	6/2013	Brady et al.	2016/0120558	A1	5/2016	Brady et al.
2013/0158591	A1	6/2013	Koehler	2016/0143653	A1	5/2016	Vale et al.
2013/0158592	A1	6/2013	Porter	2016/0192953	A1	7/2016	Brady et al.
2013/0184739	A1	7/2013	Brady et al.	2016/0192954	A1	7/2016	Brady et al.
2013/0197567	A1	8/2013	Brady et al.	2016/0192955	A1	7/2016	Brady et al.
2013/0226146	A1	8/2013	Tekulve	2016/0192956	A1	7/2016	Brady et al.
2013/0268050	A1	10/2013	Wilson et al.	2016/0256180	A1	9/2016	Vale et al.
2013/0281788	A1	10/2013	Garrison	2016/0303381	A1	10/2016	Pierce et al.
2013/0325051	A1	12/2013	Martin et al.	2016/0317168	A1	11/2016	Brady et al.
2013/0325055	A1	12/2013	Eckhouse et al.	2017/0007264	A1	1/2017	Cruise et al.
2013/0325056	A1	12/2013	Eckhouse et al.	2017/0007265	A1	1/2017	Guo et al.
2013/0325107	A1	12/2013	Wu	2017/0020542	A1	1/2017	Martin et al.
2013/0345739	A1	12/2013	Brady et al.	2017/0020670	A1	1/2017	Murray et al.
2014/0005712	A1	1/2014	Martin	2017/0020700	A1	1/2017	Bienvenu et al.
2014/0005713	A1	1/2014	Bowman	2017/0027640	A1	2/2017	Kunis et al.
2014/0046359	A1	2/2014	Bowman et al.	2017/0027692	A1	2/2017	Bonhoeffer et al.
2014/0088678	A1	3/2014	Wainwright et al.	2017/0027725	A1	2/2017	Argentine
2014/0121672	A1	5/2014	Folk	2017/0035436	A1	2/2017	Morita
2014/0128905	A1	5/2014	Molaei	2017/0035567	A1	2/2017	Duffy
2014/0134654	A1	5/2014	Rudel et al.	2017/0042548	A1	2/2017	Lam
2014/0135812	A1	5/2014	Divino et al.	2017/0049596	A1	2/2017	Schabert
2014/0142598	A1	5/2014	Fulton, III	2017/0056061	A1	3/2017	Ogle et al.
2014/0163367	A1	6/2014	Eskuri	2017/0071614	A1	3/2017	Vale et al.
2014/0180122	A1	6/2014	Stigall et al.	2017/0071737	A1	3/2017	Kelley
2014/0180377	A1	6/2014	Bose et al.	2017/0072452	A1	3/2017	Monetti et al.
2014/0180397	A1	6/2014	Gerberding et al.	2017/0079671	A1	3/2017	Morero et al.
2014/0194911	A1	7/2014	Johnson et al.	2017/0079680	A1	3/2017	Bowman
2014/0194919	A1	7/2014	Losordo et al.	2017/0079766	A1	3/2017	Wang et al.
2014/0200607	A1	7/2014	Sepetka et al.	2017/0079767	A1	3/2017	Leon-Yip
2014/0200608	A1	7/2014	Brady et al.	2017/0079812	A1	3/2017	Lam et al.
2014/0236220	A1	8/2014	Inoue	2017/0079817	A1	3/2017	Sepetka et al.
2014/0243881	A1	8/2014	Lees et al.	2017/0079819	A1	3/2017	Pung et al.
2014/0257362	A1	9/2014	Eidenschink	2017/0079820	A1	3/2017	Lam et al.
2014/0276922	A1	9/2014	McLain et al.	2017/0086851	A1	3/2017	Wallace et al.
2014/0277079	A1	9/2014	Vale et al.	2017/0086862	A1	3/2017	Vale et al.
2014/0303667	A1	10/2014	Cox et al.	2017/0086863	A1	3/2017	Brady et al.
2014/0309657	A1	10/2014	Ben-Ami	2017/0086996	A1	3/2017	Peterson et al.
2014/0309673	A1	10/2014	Dacuyucuy et al.	2017/0095259	A1	4/2017	Tompkins et al.
2014/0330302	A1	11/2014	Tekulve et al.	2017/0100126	A1	4/2017	Bowman et al.
2014/0343585	A1	11/2014	Ferrera et al.	2017/0100141	A1	4/2017	Morero et al.
2014/0371769	A1	12/2014	Vale et al.	2017/0100143	A1	4/2017	Grandfield
2014/0371779	A1	12/2014	Vale et al.	2017/0100183	A1	4/2017	Iaizzo et al.
2014/0371780	A1	12/2014	Vale et al.	2017/0105743	A1	4/2017	Vale et al.
2014/0379023	A1	12/2014	Brady et al.	2017/0112515	A1	4/2017	Brady et al.
2015/0018859	A1	1/2015	Quick et al.	2017/0112647	A1	4/2017	Sachar et al.
2015/0018860	A1	1/2015	Quick et al.	2017/0113023	A1	4/2017	Steingisser et al.
2015/0032144	A1	1/2015	Holloway	2017/0119409	A1	5/2017	Ma
2015/0080937	A1	3/2015	Davidson	2017/0143465	A1	5/2017	Ulm, III
2015/0112376	A1	4/2015	Molaei et al.	2017/0147765	A1	5/2017	Mehta
2015/0133990	A1	5/2015	Davidson	2017/0150979	A1	6/2017	Ulm
2015/0150672	A1	6/2015	Ma	2017/0151032	A1	6/2017	Loisel
2015/0164523	A1	6/2015	Brady et al.	2017/0165062	A1	6/2017	Rothstein
2015/0224133	A1	8/2015	Ohri et al.	2017/0165065	A1	6/2017	Rothstein et al.
2015/0250497	A1	9/2015	Marks et al.	2017/0165454	A1	6/2017	Tuohy et al.
2015/0257775	A1	9/2015	Gilvarry et al.	2017/0172581	A1	6/2017	Bose et al.
2015/0272716	A1	10/2015	Pinchuk et al.	2017/0172766	A1	6/2017	Vong et al.
2015/0297252	A1	10/2015	Miloslavski et al.	2017/0172772	A1	6/2017	Khenansho
				2017/0189033	A1	7/2017	Sepetka et al.
				2017/0189035	A1	7/2017	Porter
				2017/0189041	A1	7/2017	Cox et al.
				2017/0215902	A1	8/2017	Leynov et al.

(56)	References Cited			CN	208582467	U	3/2019
	U.S. PATENT DOCUMENTS			DE	202009001951	U1	3/2010
				DE	102009056450	A1	6/2011
				DE	102010010849	A1	9/2011
				DE	102010014778	A1	10/2011
				DE	102010024085	A1	12/2011
				DE	102011014586	B3	9/2012
2017/0216484	A1	8/2017	Cruise et al.	EP	1153581	A1	11/2001
2017/0224350	A1	8/2017	Shimizu et al.	EP	2301450	A1	3/2011
2017/0224355	A1	8/2017	Bowman et al.	EP	2438891	A1	4/2012
2017/0224467	A1	8/2017	Piccagli et al.	EP	2628455	A1	8/2013
2017/0224511	A1	8/2017	Dwork et al.	EP	3156004	A1	4/2017
2017/0224953	A1	8/2017	Tran et al.	EP	3593742	A1	1/2020
2017/0231749	A1	8/2017	Perkins et al.	EP	3669802	A1	6/2020
2017/0252064	A1	9/2017	Staunton	EP	3858291	A1	8/2021
2017/0265983	A1	9/2017	Lam et al.	ES	2210456	T3	7/2004
2017/0281192	A1	10/2017	Tieu et al.	GB	2427554	A	1/2007
2017/0281331	A1	10/2017	Perkins et al.	GB	2494820	A	3/2013
2017/0281344	A1	10/2017	Costello	JP	09-19438	A	1/1997
2017/0281909	A1	10/2017	Northrop et al.	JP	2014-511223	A	5/2014
2017/0281912	A1	10/2017	Melder et al.	JP	2014-525796	A	10/2014
2017/0290593	A1	10/2017	Cruise et al.	JP	2015-505250	A	2/2015
2017/0290654	A1	10/2017	Sethna	JP	2016-513505	A	5/2016
2017/0296324	A1	10/2017	Argentine	JP	2019-072504	A	5/2019
2017/0296325	A1	10/2017	Marrocco et al.	JP	2019-526365	A	9/2019
2017/0303939	A1	10/2017	Greenhalgh et al.	JP	2019-536552	A	12/2019
2017/0303942	A1	10/2017	Greenhalgh et al.	WO	WO 94/24926	A1	11/1994
2017/0303947	A1	10/2017	Greenhalgh et al.	WO	WO 97/27808	A1	8/1997
2017/0303948	A1	10/2017	Wallace et al.	WO	WO 97/38631	A1	10/1997
2017/0304041	A1	10/2017	Argentine	WO	WO 99/20335	A1	4/1999
2017/0304097	A1	10/2017	Corwin et al.	WO	WO 99/56801	A2	11/1999
2017/0304595	A1	10/2017	Nagasrinivasa et al.	WO	WO 99/60933	A1	12/1999
2017/0312109	A1	11/2017	Le	WO	WO 01/21077	A1	3/2001
2017/0312484	A1	11/2017	Shipley et al.	WO	WO 02/02162	A2	1/2002
2017/0316561	A1	11/2017	Helm et al.	WO	WO 02/11627	A2	2/2002
2017/0319826	A1	11/2017	Bowman et al.	WO	WO 02/43616	A2	6/2002
2017/0333228	A1	11/2017	Orth et al.	WO	WO 02/070061	A1	9/2002
2017/0333236	A1	11/2017	Greenan	WO	WO 02/094111	A2	11/2002
2017/0333678	A1	11/2017	Bowman et al.	WO	WO 03/002006	A1	1/2003
2017/0340383	A1	11/2017	Bloom et al.	WO	WO 03/030751	A1	4/2003
2017/0348014	A1	12/2017	Wallace et al.	WO	WO 03/051448	A2	6/2003
2017/0348514	A1	12/2017	Guyon et al.	WO	WO 2004/028571	A2	4/2004
2018/0140315	A1	5/2018	Bowman et al.	WO	WO 2004/056275	A1	7/2004
2018/0206865	A1	7/2018	Martin et al.	WO	WO 2005/000130	A1	1/2005
2018/0207399	A1	7/2018	Chou et al.	WO	WO 2005/027779	A2	3/2005
2018/0256177	A1	9/2018	Cooper et al.	WO	WO 2006/021407	A2	3/2006
2018/0263650	A1	9/2018	Iwanami et al.	WO	WO 2006/031410	A2	3/2006
2018/0325537	A1	11/2018	Shamay et al.	WO	WO 2006/107641	A2	10/2006
2018/0326024	A1	11/2018	Prochazka et al.	WO	WO 2006/135823	A2	12/2006
2018/0344338	A1	12/2018	Brady et al.	WO	WO 2007/054307	A2	5/2007
2019/0000492	A1	1/2019	Casey et al.	WO	WO 2007/068424	A2	6/2007
2019/0015061	A1	1/2019	Liebeskind et al.	WO	WO 2008/034615	A2	3/2008
2019/0021750	A1	1/2019	Heilman et al.	WO	WO 2008/051431	A1	5/2008
2019/0167284	A1	6/2019	Friedman et al.	WO	WO 2008/131116	A1	10/2008
2019/0239907	A1	8/2019	Brady et al.	WO	WO 2008/135823	A1	11/2008
2019/0292273	A1	9/2019	Hanotin et al.	WO	WO 2009/031338	A1	3/2009
2019/0374239	A1	12/2019	Martin et al.	WO	WO 2009/076482	A1	6/2009
2019/0380723	A1	12/2019	Grandfield et al.	WO	WO 2009/086482	A1	7/2009
2019/0388097	A1	12/2019	Girdhar et al.	WO	WO 2009/105710	A1	8/2009
2020/0000483	A1	1/2020	Brady et al.	WO	WO 2010/010545	A1	1/2010
2020/0009150	A1	1/2020	Chamorro Sanchez	WO	WO 2010/046897	A1	4/2010
2020/0085444	A1	3/2020	Vale et al.	WO	WO 2010/075565	A2	7/2010
2020/0085454	A1	3/2020	Gogoussis et al.	WO	WO 2010/102307	A1	9/2010
2020/0100804	A1	4/2020	Casey et al.	WO	WO 2010/146581	A1	12/2010
2020/0297364	A1	9/2020	Choe et al.	WO	WO 2011/013556	A1	2/2011
2020/0390459	A1	12/2020	Casey et al.	WO	WO 2011/066961	A1	6/2011
2021/0005321	A1	1/2021	Hwang	WO	WO 2011/082319	A1	7/2011
2021/0007757	A1	1/2021	Casey et al.	WO	WO 2011/095352	A1	8/2011
2021/0228223	A1	7/2021	Casey et al.	WO	WO 2011/106426	A1	9/2011
2022/0192739	A1	6/2022	Deen et al.	WO	WO 2011/110316	A1	9/2011
	FOREIGN PATENT DOCUMENTS			WO	WO 2011/135556	A1	11/2011
CN	102307613	A	1/2012	WO	WO 2012/052982	A1	4/2012
CN	102316809	A	1/2012	WO	WO 2012/064726	A1	5/2012
CN	102596098	A	7/2012	WO	WO 2012/081020	A1	6/2012
CN	103764049	A	4/2014	WO	WO 2012/110619	A1	8/2012
CN	104042304	A	9/2014	WO	WO 2012/120490	A2	9/2012
CN	105208950	A	12/2015	WO	WO 2012/156924	A1	11/2012
CN	105662532	A	6/2016	WO	WO 2013/016435	A1	1/2013
CN	205359559	U	7/2016	WO	WO 2013/072777	A2	5/2013
CN	107530090	A	1/2018				

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2013/105099	A2	7/2013
WO	WO 2013/109756	A2	7/2013
WO	WO 2013/187927	A1	12/2013
WO	WO 2014/047650	A1	3/2014
WO	WO 2014/081892	A1	5/2014
WO	WO 2014/139845	A1	9/2014
WO	WO 2014/169266	A1	10/2014
WO	WO 2014/178198	A1	11/2014
WO	WO 2015/061365	A1	4/2015
WO	WO 2015/103547	A1	7/2015
WO	WO 2015/134625	A1	9/2015
WO	WO 2015/179324	A2	11/2015
WO	WO 2015/189354	A1	12/2015
WO	WO 2016/010995	A1	1/2016
WO	WO 2016/089451	A1	6/2016
WO	WO 2017/089424	A1	6/2017
WO	WO 2017/090473	A1	6/2017
WO	WO 2017/103686	A2	6/2017
WO	WO 2017/161204	A1	9/2017
WO	WO 2020/039082	A1	2/2020
WO	WO 2021/113302	A1	6/2021

* cited by examiner

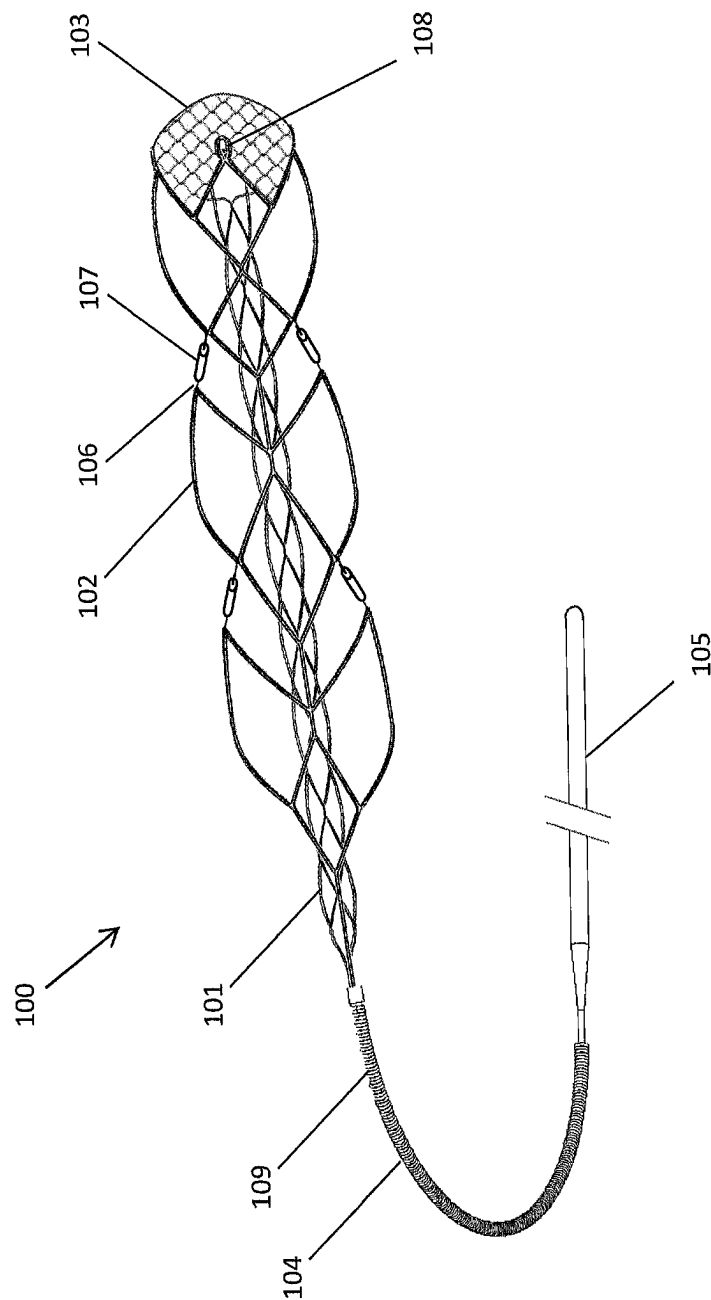


Fig 1

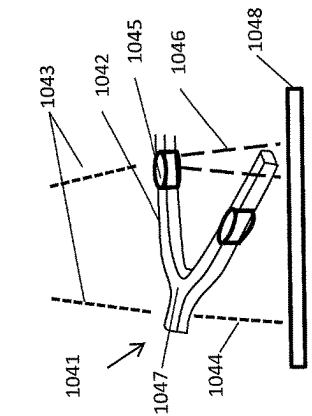


Fig 3a

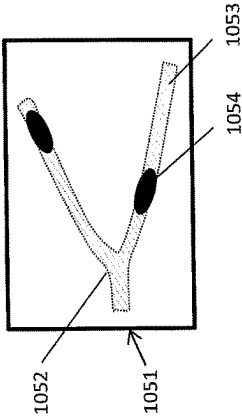


Fig 3b

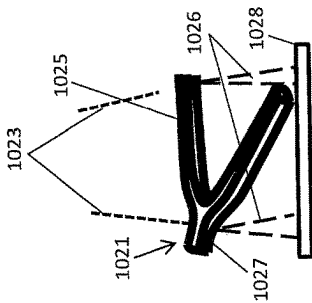


Fig 2c

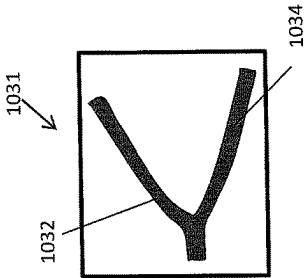


Fig 2d

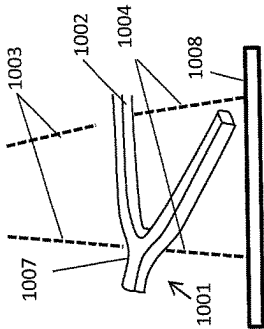


Fig 2a

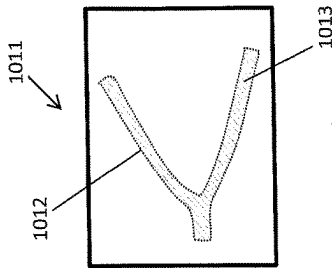


Fig 2b

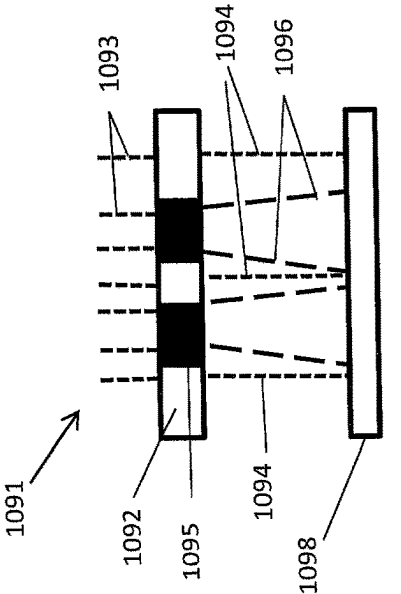


Fig 6a

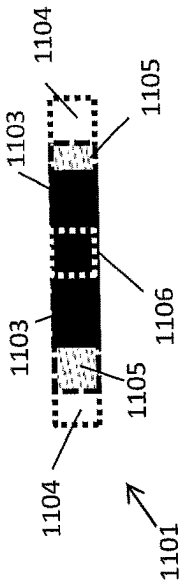


Fig 6b

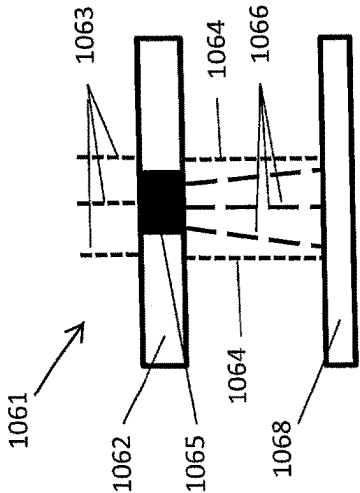


Fig 4a

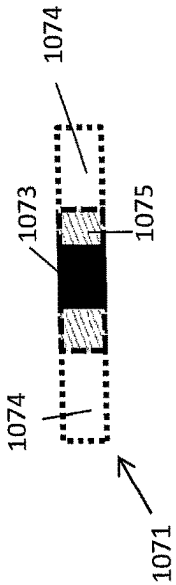


Fig 4b

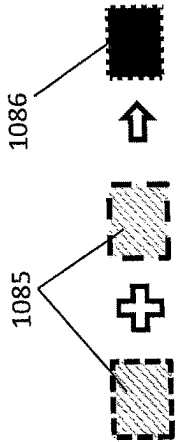


Fig 5

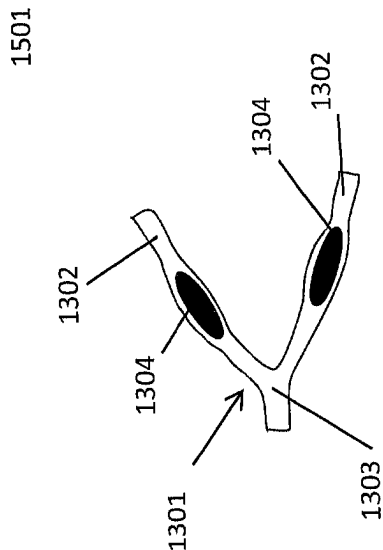


Fig 8

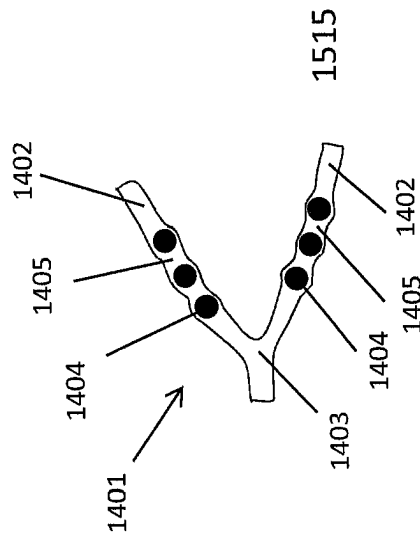


Fig 9

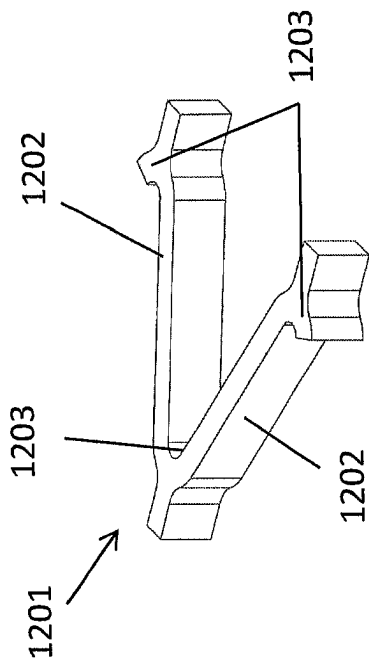


Fig 7a

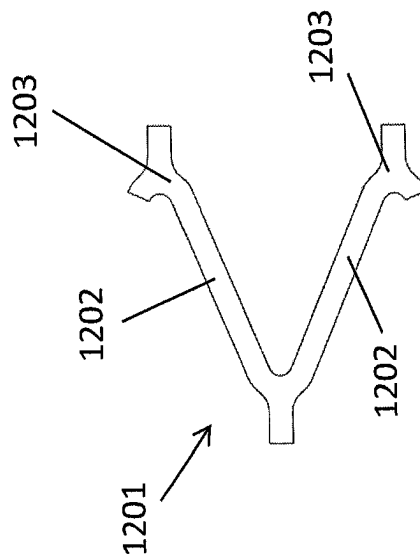
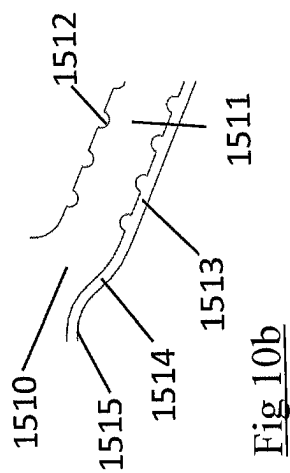
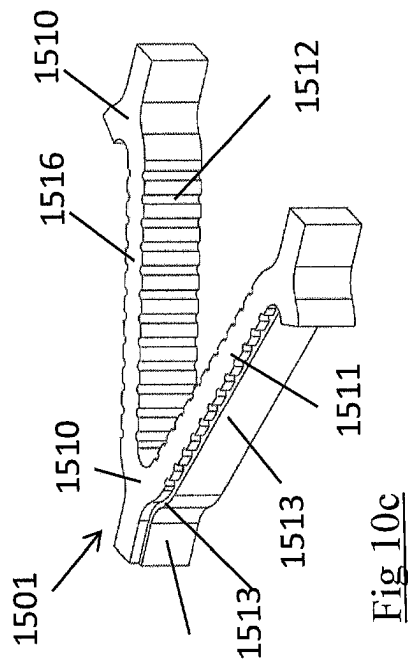
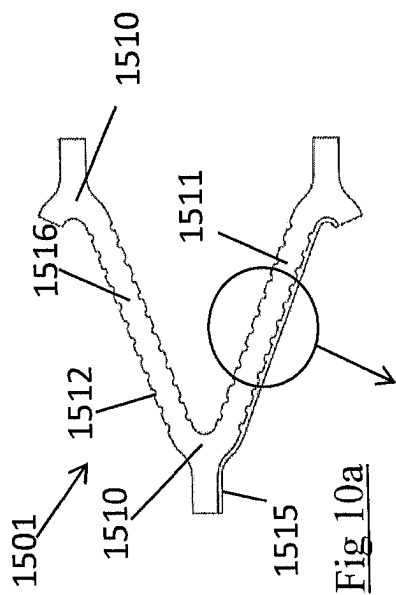


Fig 7b



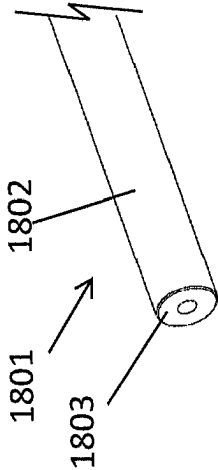


Fig 13a

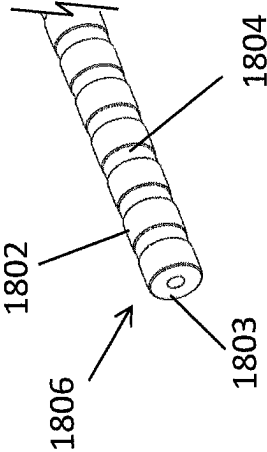


Fig 13b

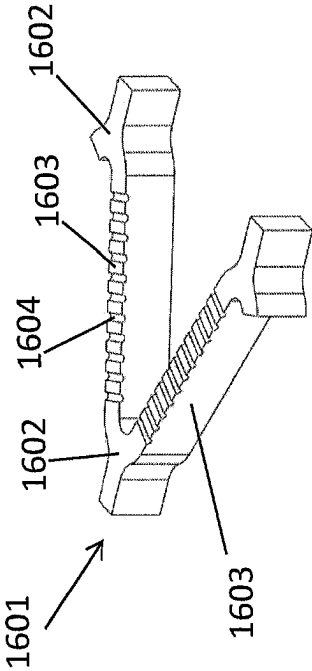


Fig 11

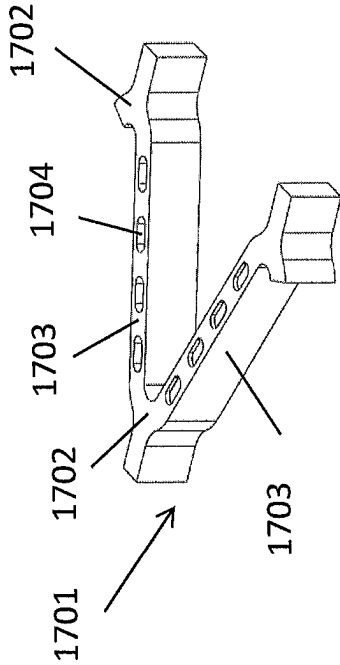


Fig 12

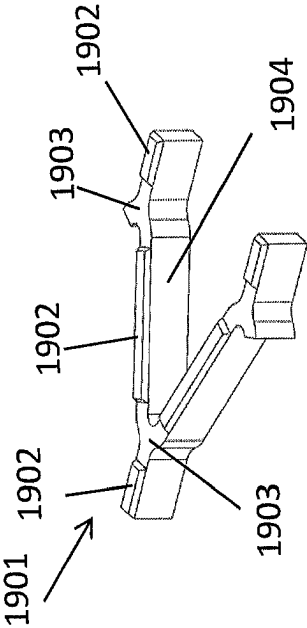


Fig 14

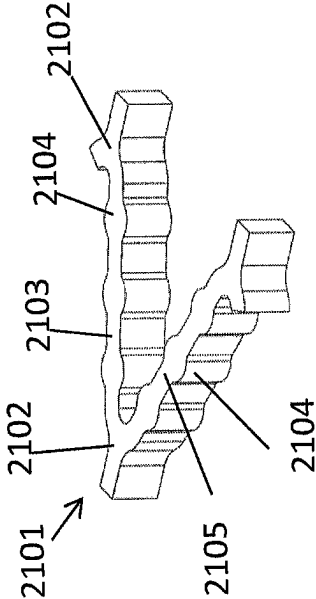


Fig 16

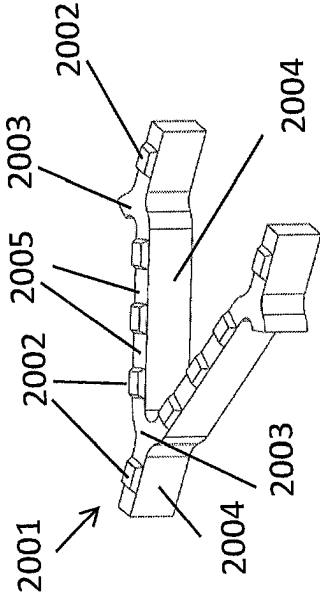


Fig 15

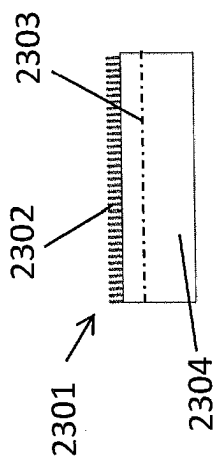


Fig 17a

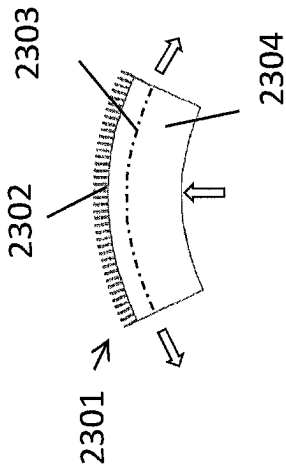


Fig 17b

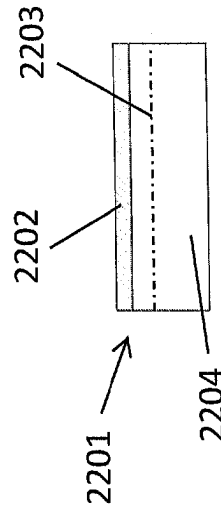


Fig 18a

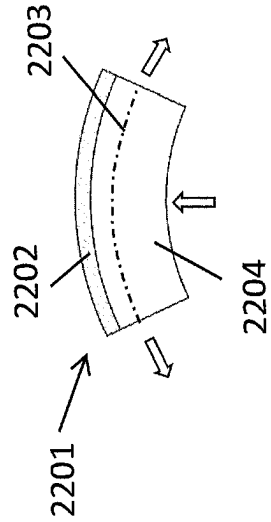


Fig 18b

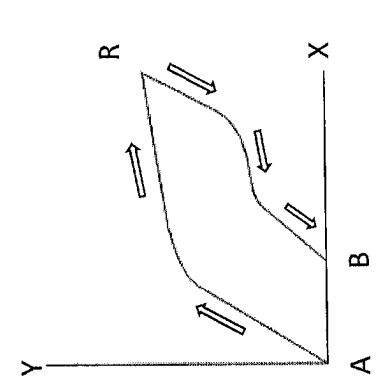


Fig 19a

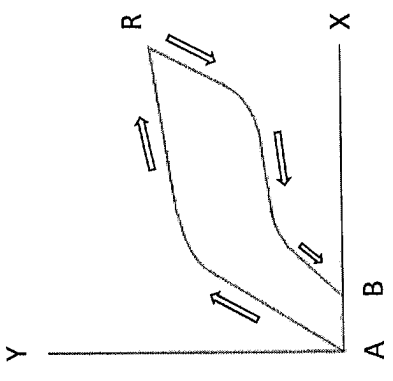


Fig 19b

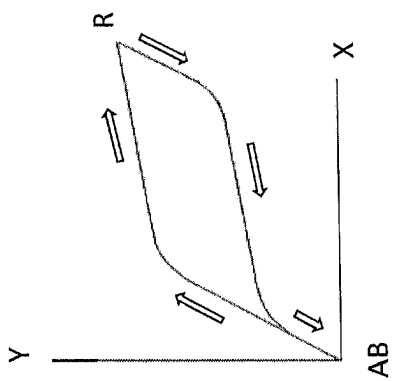


Fig 19c

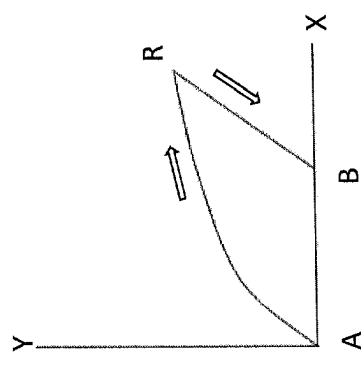
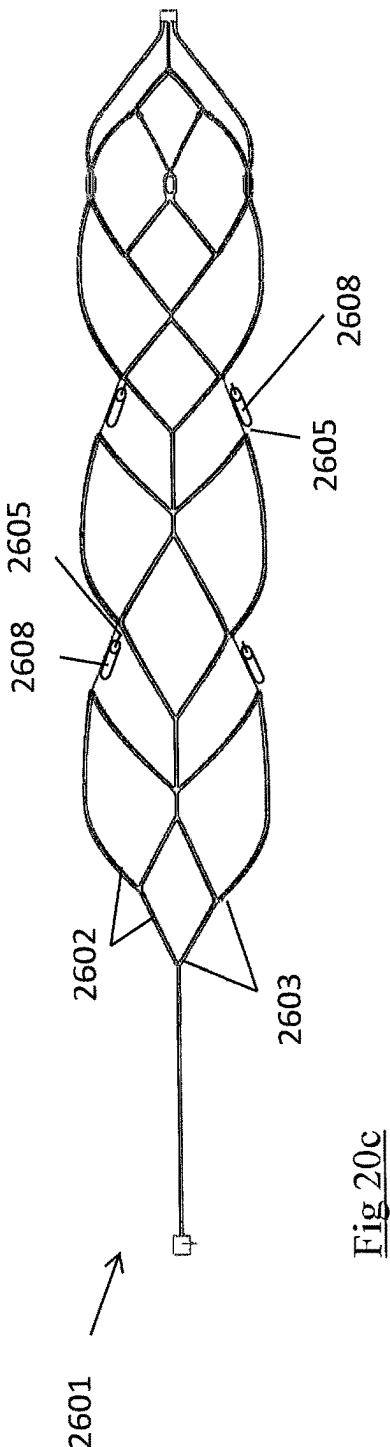
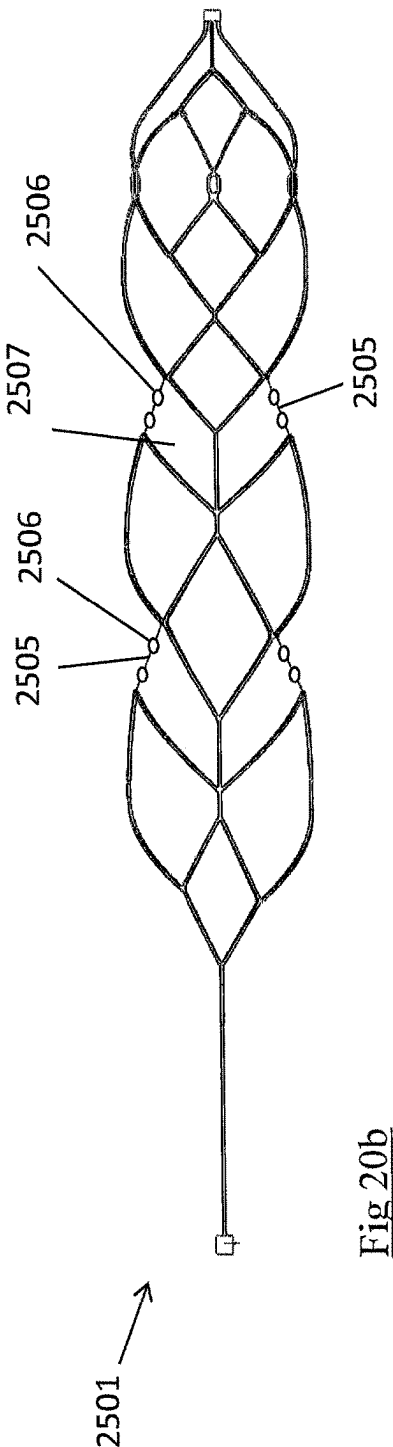
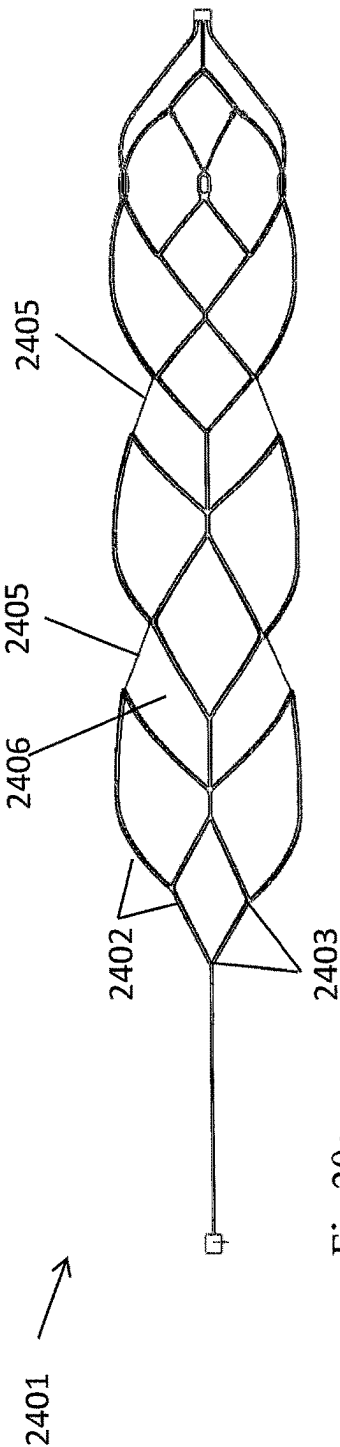


Fig 19d



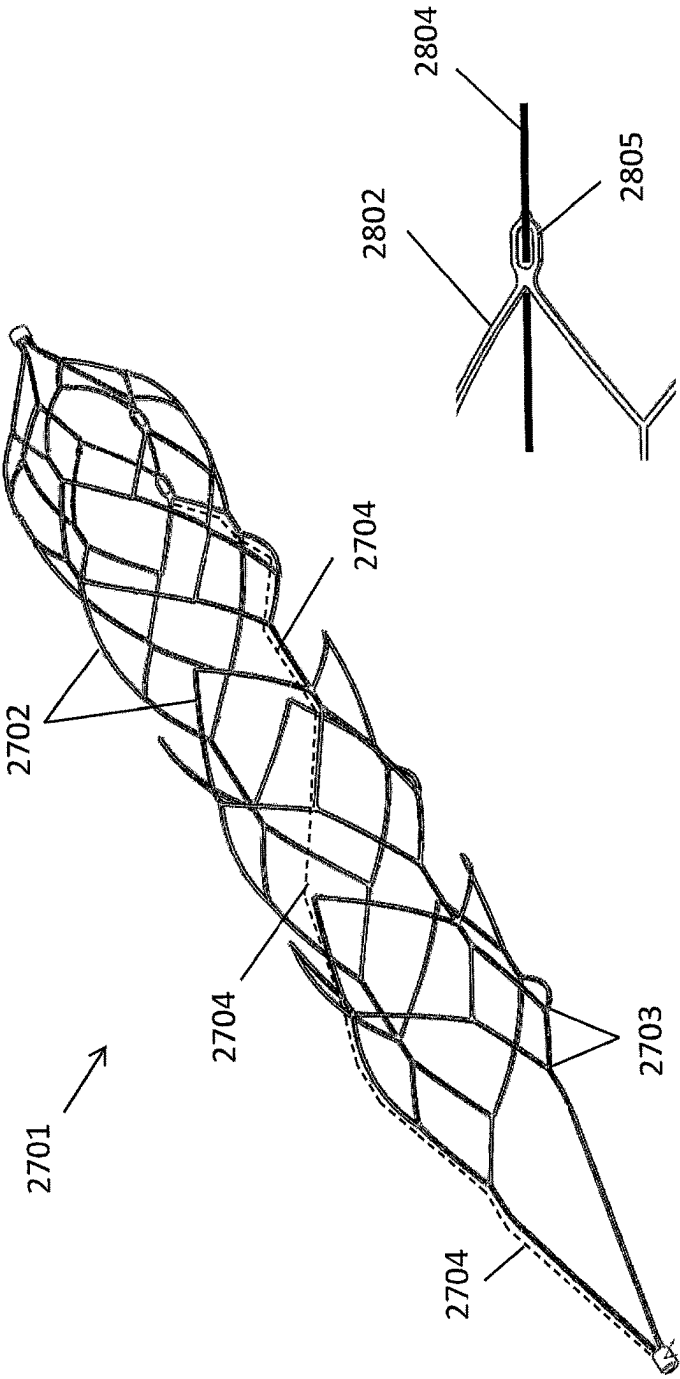


Fig 21a

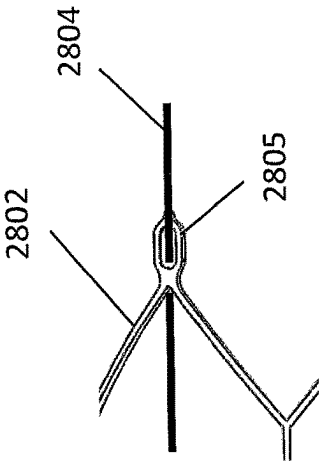


Fig 21b

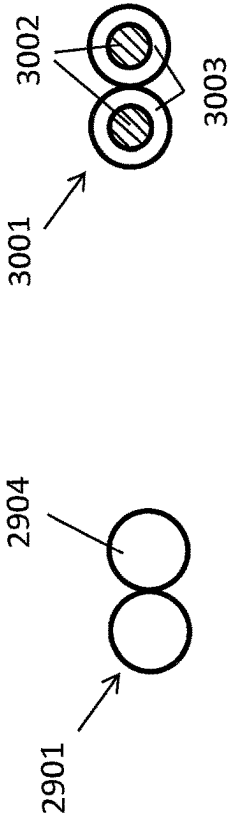


Fig 21c






Fig 21d

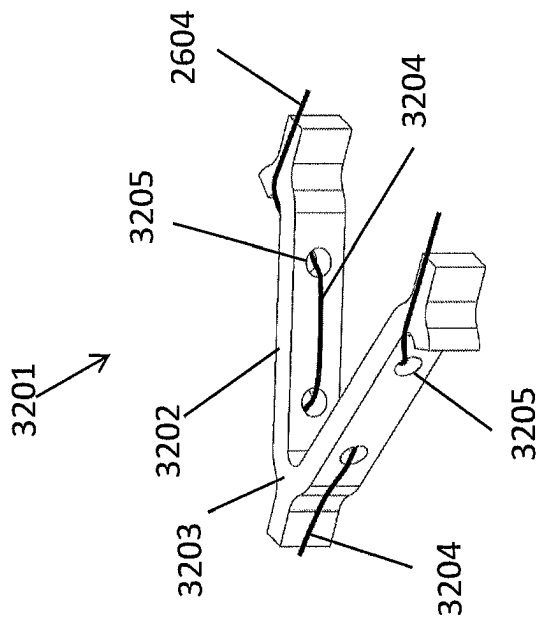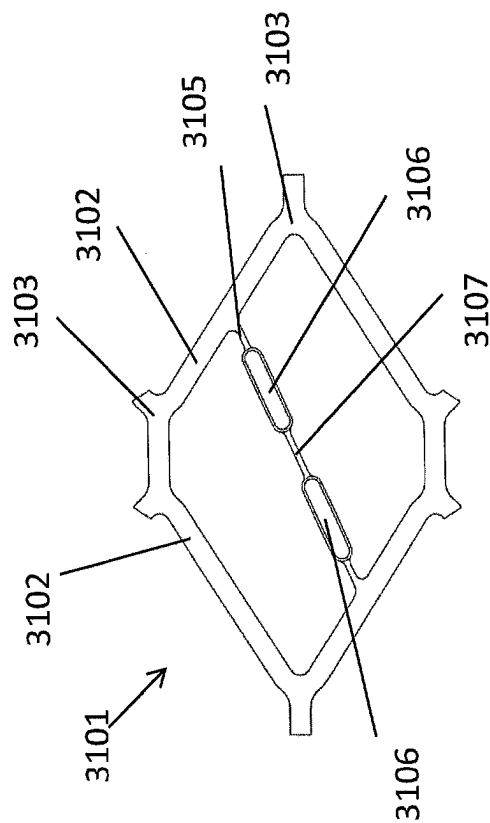

1

DEVICES AND METHODS FOR REMOVAL OF ACUTE BLOCKAGES FROM BLOOD VESSELS

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a divisional application of U.S. patent application Ser. No. 16/248,539 filed Jan. 15, 2019, which is a continuation application of U.S. patent application Ser. No. 14/207,069 filed Mar. 12, 2014, now U.S. Pat. No. 10,201,360 issued Feb. 12, 2019, which claims the benefit of U.S. Provisional Application No. 61/784,940 filed Mar. 14, 2013, each of which is incorporated herein by reference in their entirety.

FIELD OF THE INVENTION

This invention relates to devices intended for removing acute blockages from blood vessels. The invention especially relates to means of rendering such devices visible under x-ray or fluoroscopy. Acute obstructions may include clot, misplaced devices, migrated devices, large emboli and the like. Thromboembolism occurs when part or all of a thrombus breaks away from the blood vessel wall. This clot (now called an embolus) is then carried in the direction of blood flow. An ischemic stroke may result if the clot lodges in the cerebral vasculature. A pulmonary embolism may result if the clot originates in the venous system or in the right side of the heart and lodges in a pulmonary artery or branch thereof. Clots may also develop and block vessels locally without being released in the form of an embolus--this mechanism is common in the formation of coronary blockages. The invention is particularly suited to removing clot from cerebral arteries in patients suffering acute ischemic stroke (AIS), from coronary native or graft vessels in patients suffering from myocardial infarction (MI), and from pulmonary arteries in patients suffering from pulmonary embolism (PE) and from other peripheral arterial and venous vessels in which clot is causing an occlusion.

BACKGROUND

Clot retrieval devices comprising a self-expanding Nitinol stent-like member disposed at the end of a long shaft are commonly used to remove clot from blood vessels, particularly from patients suffering from acute ischemic stroke. These devices are typically provided with small marker bands at either end of the self-expanding member which help to indicate the device's position. It would be very beneficial to a physician to be able to see the full expandable body of such a device under fluoroscopy, and thus receive visual information on the device's condition as rather than simply its position. Clot retrieval procedures are conducted under an x-ray field in order to allow the user to visualize the anatomy and at a minimum the device position during a procedure. It is desirable and enhances the user experience to be able to visualize the device state as well as position structure during a procedure, for example if the device is in an expanded configuration or a collapsed configuration. This means that the radiopaque sections must move closer to the device axis in a collapsed configuration and further from a device axis in an expanded configuration. It is generally desirable to make interventional devices such as clot retrieval devices more flexible and lower profile to improve deliverability in interventional procedures. This may be achieved by reducing the dimensions for device features,

2

and the level of contrast seen under x-ray is generally reduced as the device dimensions are reduced. Radiopaque materials generally comprise noble metals such as gold, tantalum, tungsten, platinum, iridium and the like, and generally have poor elastic recovery from a strained condition and are therefore not optimal material for devices, particularly for the regions of these devices undergoing high strain in moving from a collapsed to an expanded state and vice versa. Radiopaque materials may be added through coating a structure comprising a highly recoverable elastic material such as Nitinol, but coating the entire structure has a dampening effect that inhibits device performance.

This invention overcomes limitations associated with the dampening effect of adding radiopaque material to an expandable clot retrieval device, while making the structure sufficiently radiopaque to allow full visualization of the device condition as well as position.

STATEMENT OF THE INVENTION

Various devices and method are described in our PCT/IE2012/000011 which was published under the number WO2012/120490A. This PCT application claims the benefit of U.S. Provisional 61/450,810, filed Mar. 9, 2011 and U.S. Provisional 61/552,130 filed Oct. 27, 2011. The corresponding U.S. National stage is U.S. application Ser. No. 13/823,060 filed on Mar. 13, 2013 and issued as U.S. Pat. No. 9,301,769, on Apr. 5, 2016. The entire contents of all of the above-listed applications are herein incorporated by reference. In addition, we hereby incorporate by reference in its entirety our U.S. Provisional Application No. 61/785,213 entitled "A Clot Retrieval Device for Removing Occlusive Clot from a Blood Vessels" filed on Mar. 14, 2013.

This invention is particularly applicable to clot retrieval devices comprising expandable bodies made from a metallic framework. Such a framework might be a Nitinol framework of interconnected struts, formed by laser (or otherwise) cutting a tube or sheet of material, and may thus comprise a structure with a pattern of strut features and connector features. In some embodiments the clot retrieval device may comprise an inner expandable member and an outer expandable member, which may define a flow lumen through a clot and engage a clot.

In order to go from a collapsed to an expanded configuration, portions of the device undergo recoverable deformation and varying levels of strain. Some portions require a higher level of recoverable strain than others in order to work effectively. Where the framework or expandable member comprises a pattern of strut features and connector features, the struts typically comprise inflection regions or connection regions generally referred to as crowns, which typically experience higher strain than the struts or connectors when the device is collapsed or expanded.

The term detector is generally referred to as the part of the equipment which collects the beam for processing into useful images and can include for example flat panel detectors or image intensifiers. X-ray beams are filtered through an anti-scatter grid during processing. This filters out scattered beams which deflect significantly from the trajectory of the source beam and beams less significantly deflected off the original trajectory pass through the anti-scatter grid creating areas of overlap between non-scattered photon beams and scattered photon beams, referred to herein as shadow areas.

In an embodiment of this invention discrete markers are placed in low strain regions of the clot retrieval device

members, and high strain regions comprise a super elastic material with little or no radiopaque material.

In use, it is desirable to maximize visibility and therefore maximize the area and volume of radiopaque markers located in the clot retrieval device. Increasing the ratio of radiopaque material to Nitinol generally improves radiopa-
city. For the effective operation of the device in moving
between expanded and collapsed configurations, it is desir-
able to maintain a ratio of Nitinol to radiopaque material
such that strain levels from an expanded to a collapsed
configuration are substantially in the elastic region. This
creates a conflict of requirements, and the solutions provided
herein overcome this conflict.

Discrete markers placed in close proximity create over-
lapping shadow areas, referred to as intersection zones
herein, which give the illusion under x-ray imaging of a
continuous marker thereby providing fuller visual informa-
tion to the user in an x-ray image.

Various embodiments of the invention are described in
more detail below. Within these descriptions various terms
for each portion of the devices may be interchangeably used.
Each of the described embodiments are followed by a list of
further qualifications (preceded by the word "wherein") to
describe even more detailed versions of the preceding head-
line embodiment. It is intended that any of these qualifica-
tions may be combined with any of the headline embodi-
ments, but to maintain clarity and conciseness not all of the
possible permutations have been listed.

One embodiment of a device of this invention comprises
a clot retrieval device comprising an elongate shaft and an
expandable section, the expandable section comprising a
framework of interconnected strut elements, the connection
region between adjacent strut elements comprising crown
elements, said framework formed from a substrate material,
at least a portion of a plurality of said strut elements coated
with a coating material, and at least a portion of a plurality
of said crown elements not coated with said coating mate-
rial.

Wherein the substrate material has a density of less than
10 g/cm³.

Wherein the substrate material has a density of less than
8 g/cm³.

Wherein the coating material has a density of more than
10 g/cm³.

Wherein the coating material has a density of more than
15 g/cm³.

Wherein the coating material has a density of more than
18 g/cm³.

Wherein the substrate material is a superelastic material
such as Nitinol or other super or pseudo elastic metallic
alloy.

Wherein the coating material is Gold, Tantalum, Tung-
sten, Platinum, or an alloy of one of these elements or other
dense element or alloy containing one or more radiodense
elements.

Wherein the coating material comprises a polymer or
adhesive filled with a dense or high atomic number material
such as Barium Sulphate, Bismuth SubCarbonate, Barium
OxyChloride, Gold, Tungsten, Platinum or Tantalum.

Wherein the coating material is applied using an electro-
plating process, a dipping process, a plasma deposition
process, an electrostatic process, a dip or spray coating
process, a sputtering process, a soldering process, a cladding
process, or a drawing process.

Another aspect of this invention comprises a method of
manufacturing the expandable body of a clot retrieval

device, the expandable body comprising a substrate material
and a coating material, the method comprising:

a first step of applying the coating material to the substrate
material,

a second step of removing at least a portion of said coating
material from at least one area of said substrate mate-
rial,

and a third step of cutting away regions of both coating
and substrate material to form an interconnected pattern
of coated and uncoated regions.

Wherein the first step comprises an electroplating process,
a dipping process, a plasma deposition process, an electro-
static process, a dip or spray coating process, a sputtering
process, a soldering process, a cladding process or a drawing
process.

Wherein the second step comprises a grinding process, a
polishing process, a buffing process, an etching process, a
laser cutting or laser ablation process.

Wherein the third step comprises a laser cutting process,
a wire cutting process, a water jet cutting process, a machin-
ing process or an etching process.

Wherein the coating material is Gold, Tantalum, Tung-
sten, Platinum or an alloy of one of these elements or other
dense element or alloy containing one or more radiodense
elements.

Wherein the coating material comprises a polymer or
adhesive filled with a dense or high atomic number material
such as Barium Sulphate, Bismuth SubCarbonate, Barium
OxyChloride, Gold, Tungsten, Platinum or Tantalum.

Wherein the substrate material comprises Nitinol, or an
alloy of Nitinol or another super or pseudo elastic alloy.

Wherein the interconnected pattern comprises a plurality
of strut elements and connector elements.

Wherein the interconnected pattern of the Clot Retrieval
device comprises an expanded state and a collapsed state.

Wherein the second step removes at least a portion of the
coating from those areas of the interconnected pattern which
experience the highest strain in moving from the expanded
state to the collapsed state, and/or from the collapsed state
to the expanded state.

Wherein the strut elements terminate in crown elements,

Wherein the second step removes some or all of the
coating from the crown elements.

Wherein the second step removes some or all of the
coating from discrete sections of the strut elements; in one
embodiment these discrete sections comprising stripes
across the width of the struts.

Another embodiment of a device of this invention com-
prises a clot retrieval device comprising an elongate shaft
and an expandable section, the expandable section formed
from a substrate material, at least a portion of the substrate
material coated with a first coating material and at least a
portion of the first coating material coated with a second
coating material;

Wherein the substrate material is a superelastic material
such as Nitinol or other super or pseudo elastic metallic
alloy.

Wherein the first coating material is Gold, Tantalum,
Tungsten, Platinum or an alloy of one of these elements or
other dense element or alloy containing one or more
radiodense elements.

Wherein the first coating material is applied by a plasma
deposition process, an electrostatic process, a dip or spray
coating process, a sputtering process, a sputtering process
using a cylindrical magnetron, a soldering process, a clad-
ding process or a drawing process.

5

Wherein the first coating material comprises a porous or non-porous columnar structure.

Wherein the first coating material comprises a porous columnar structure, comprising generally independent columns of the coating material which extend substantially 5 perpendicularly to the substrate surface.

Wherein said columns have a first end and a second end, said first end being adjacent the substrate surface, and the spacing between the second ends of adjacent columns varying with deformation of the substrate material/expandable 10 body.

Wherein the second ends of the first coating material define an outer surface, and said outer surface is a rough surface.

Wherein the second coating material comprises a smooth 15 surface, and/or a soft surface.

Wherein the second coating material is a polymeric material.

Wherein the elastic modulus of the second coating material is lower than that of the first coating material.

Wherein the elastic modulus of the second coating material is lower than that of the substrate material.

Wherein the elastic modulus of the second coating material is less than 50% of that of the first coating material and/or substrate material.

Wherein the elastic modulus of the second coating material is less than 40% of that of the first coating material and/or substrate material.

Wherein the elastic modulus of the second coating material is less than 30% of that of the first coating material and/or substrate material.

Wherein the elastic modulus of the second coating material is less than 20% of that of the first coating material and/or substrate material.

Wherein the elastic modulus of the second coating material is less than 10% of that of the first coating material and/or substrate material.

Wherein the second coating material is a hydrophilic material or a hydrogel.

Wherein the coefficient of friction of the first coating 40 material is greater than 0.2.

Wherein the coefficient of friction of the first coating material is greater than 0.3.

Wherein the coefficient of friction of the first coating material is greater than 0.4.

Wherein the coefficient of friction of the first coating material is greater than 0.5.

Wherein the coefficient of friction of the second coating material is less than 0.2.

Wherein the coefficient of friction of the second coating material is less than 0.15.

Wherein the coefficient of friction of the second coating material is less than 0.1.

Wherein the coefficient of friction of the second coating material is less than 0.08.

Another embodiment of a device of this invention comprises a clot retrieval device comprising an elongate shaft and an expandable member, the expandable member comprising a proximal section, a body section and a distal section, the body section comprising a metallic framework of a first (or substrate) material, the metallic framework comprising a plurality of strut elements, said strut elements comprising an outer surface, an inner surface and side wall surfaces, at least one of said surfaces comprising a smooth surface and recessed features, at least some of said recessed 65 features at least partially filled with a second coating material.

6

Wherein the recessed features comprise grooves or slots in the top surface of a strut element.

Wherein the recessed features comprise holes in the top surface of a strut element.

Wherein the recessed features comprise holes through a strut element.

Wherein the above holes are circular, or oblong, or square or rectangular.

Wherein the recessed features comprise grooves or slots in the side wall of a strut element.

Wherein all of the recessed features are filled with the second coating material.

Wherein at least one of the smooth surfaces are coated with the second coating material.

Wherein all of the smooth surfaces are coated with the second coating material.

Wherein the thickness of coating material in the recessed features is greater than the thickness of coating material on the smooth surfaces.

Another aspect of this invention comprises a method of manufacturing the expandable body of a clot retrieval device, the expandable body comprising a substrate material and a coating material, the method comprising: a first step of removing material from discrete areas of the substrate material to form recesses, a second step of applying the coating material to the substrate material and recesses, and a third step of removing some or all of the coating from the non-recessed areas of the substrate.

Another aspect of this invention comprises a method of applying a radiopaque coating to selective areas of the expandable body of a clot retrieval device, the method involving a masking material and comprising:

a first step of applying a masking material to selective areas of the expandable body,

a second step of applying a coating material to the expandable body, and a third step of removing the masking material from the expandable body.

Another aspect of this invention comprises a method of manufacturing the expandable body of a clot retrieval device, the expandable body comprising a substrate material and a coating material, the method involving a masking material and comprising:

a first step of applying the masking material to the substrate material,

a second step of removing at least a portion of said masking material from at least one area of said substrate material,

a third step of cutting away regions of both masking and substrate material to form an expandable body with masked and unmasked regions,

a fourth step of applying a coating material to the expandable body, such that the coating material adheres to the unmasked areas but does not adhere to the masked areas of the expandable body,

and a fifth step of removing the masking material from the expandable body.

Wherein the fourth step comprises an electroplating process, a dipping process, a plasma deposition process, an electrostatic process, a dip or spray coating process, a sputtering process, a soldering process, a cladding process or a drawing process.

Wherein the second step comprises a grinding process, a polishing process, a buffing process, an etching process, a laser cutting or laser ablation process.

Wherein the third step comprises a laser cutting process, a wire cutting process, a water jet cutting process, a machining process or an etching process.

Wherein the coating material is Gold, Tantalum, Tungsten, Platinum or an alloy of one of these elements or other dense element or alloy containing one or more radiodense elements. Wherein the coating material comprises a polymer or adhesive filled with a dense or high atomic number material such as Barium Sulphate, Bismuth SubCarbonate, Barium OxyChloride, Gold, Tungsten, Platinum or Tantalum.

Wherein the substrate material comprises Nitinol, or an alloy of Nitinol or another super or pseudo elastic alloy.

Wherein the expandable body comprises a plurality of strut elements and connector elements.

Wherein the expandable body of the Clot Retrieval device comprises an expanded state and a collapsed state.

Wherein the third step results in the masking material being positioned on those areas of the expandable body which experience the highest strain in moving from the expanded state to the collapsed state, and/or from the collapsed state to the expanded state.

Another embodiment of a device of this invention comprises a clot retrieval device comprising an expandable body and an elongate shaft, the expandable body comprising a proximal section, a body section and a distal section, the body section comprising a framework of strut elements and at least one fiber assembly, the fiber assembly comprising a radiodense material.

Wherein the distal section comprises a clot capture scaffold.

Wherein the clot capture scaffold comprises a net.

Wherein the fiber assembly comprises at least one fiber and at least one floating element, the floating element comprising a radiodense material.

Wherein the fiber comprises a polymer monofilament, or plurality of polymer filaments. Wherein the polymer filament is of LCP, Aramid, PEN, PET, or UHMWPE.

Wherein the fiber comprises at least one metallic filament.

Wherein the metallic filament is a nitinol wire, or plurality of such wires

Wherein the metallic filament comprises a nitinol outer layer with an inner core of a radiodense material such as Gold, Platinum, Tantalum or Tungsten.

Wherein the floating element is a coil, a tube, or a bead.

Wherein the material of the floating element comprises Gold, Tantalum, Tungsten, Platinum or an alloy of one of these elements or other dense element or alloy containing one or more radiodense elements.

Wherein the material of the floating element comprises a polymer filled with a dense and/or high atomic number material such as Barium Sulphate, Bismuth SubCarbonate, Barium OxyChloride or Tantalum.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a side view of a clot retrieval device of this invention;

FIG. 2a is an isometric view of a portion of a clot retrieval device comprising standard material under x-ray imaging;

FIG. 2b is a representation of an x-ray image of FIG. 2a;

FIG. 2c is an isometric view of a portion of another clot retrieval device comprising a radiopaque material under x-ray imaging;

FIG. 2d is a representation of an x-ray image of FIG. 2c;

FIG. 3a is an isometric view of a portion of another clot retrieval device comprising standard material and radiopaque material under x-ray imaging;

FIG. 3b is a representation of an X-ray image;

FIG. 4a is a cross section view of a strut feature of a clot retrieval device comprising standard material and radiopaque material;

FIG. 4b is a representation of an x-ray image of FIG. 4a;

FIG. 5 schematically represents the resulting x-ray image from two adjacent shadow zones;

FIG. 6a is a cross section of a strut feature of a clot retrieval device comprising standard material and spaced apart radiopaque material features;

FIG. 6b is a representation of an x-ray image from FIG. 6a;

FIG. 7a is an isometric view of a portion of a clot retrieval device;

FIG. 7b is a developed plan view of the portion of a clot retrieval device from FIG. 7a;

FIG. 8 is a developed plan view of a portion of another clot retrieval device;

FIG. 9 is a developed plan view of a portion of another clot retrieval device;

FIG. 10a is a view of a portion of a clot retrieval device;

FIG. 10b is a detail view of a region of the device shown in FIG. 10a;

FIG. 10c is an isometric view of the device shown in FIG. 10a;

FIG. 11 is an isometric view of a portion of a clot retrieval device;

FIG. 12 is an isometric view of a portion of a clot retrieval device;

FIG. 13a is an isometric view of a tube used to form a part of a clot retrieval device;

FIG. 13b is an isometric view of a tube used to form a part of a clot retrieval device;

FIG. 14 is an isometric view of a portion of a clot retrieval device;

FIG. 15 is an isometric view of a portion of a clot retrieval device;

FIG. 16 is an isometric view of a portion of a clot retrieval device;

FIG. 17a is a side view of an element of a clot retrieval device;

FIG. 17b is a view of the element shown in FIG. 17a in bending;

FIG. 18a is a side view of an element of a clot retrieval device;

FIG. 18b is a view of the element shown in FIG. 18a in bending;

FIG. 19a is a stress-strain curve of a material used in the construction of a clot retrieval device;

FIG. 19b is a stress-strain curve of another material used in the construction of a clot retrieval device;

FIG. 19c is a stress-strain curve of an element of a clot retrieval device;

FIG. 19d is a stress-strain curve of another element of a clot retrieval device;

FIG. 20a is a side view of part of a clot retrieval device of this invention;

FIG. 20b is a side view of part of a clot retrieval device of this invention;

FIG. 20c is a side view of part of a clot retrieval device of this invention;

FIG. 21a is an isometric view of part of a clot retrieval device of this invention;

FIG. 21b is a detail view of a region of the device of FIG. 21a;

FIG. 21c is a section through one embodiment of a part of FIG. 21a

9

FIG. 21*d* is a section through another embodiment of a part of FIG. 21*a*;

FIG. 22 is a view of a portion of a clot retrieval device of this invention; and

FIG. 23 is an isometric view of part of a clot retrieval device of this invention.

DETAILED DESCRIPTION

Specific embodiments of the present invention are now described in detail with reference to the figures, wherein identical reference numbers indicate identical or functionality similar elements. The terms “distal” or “proximal” are used in the following description with respect to a position or direction relative to the treating physician. “Distal” or “distally” are a position distant from or in a direction away from the physician. “Proximal” or “proximally” or “proximate” are a position near or in a direction toward the physician.

The following detailed description is merely exemplary in nature and is not intended to limit the invention or the application and uses of the invention. Although the description of the invention is in the context of treatment of intracranial arteries, the invention may also be used in other body passageways as previously described.

FIG. 1 is an isometric view of a clot retrieval device 100 with an inner expandable member 101 and outer member 102. In use, inner member 101 creates a flow channel through a clot and its freely expanded diameter is less than that of outer member 102. The inner and outer members are connected at their proximal ends to an elongate shaft 104, whose proximal end 105 extends outside of the patient in use. A distal fragment capture net 103 may be attached to the distal end of the device.

Positional visualization of this device may be provided by proximal Radiopaque coil 109 and distal radiopaque markers 108. User visualization of device 100 would be enhanced by providing visual information to the user on device expansion in a vessel or clot. This information may allow the user to visualize the profile of a clot and provide a fuller map of the luminal space created upon device deployment. As the device is withdrawn, the user will see the device response as it tracks through the anatomy with clot incorporated. It is therefore desirable to add radiopaque materials to outer member 102 and/or to inner tubular member 101 to provide the highest quality information to the user. One of the challenges with incorporating radiopaque material in such a manner is the dampening effect such materials have on superelastic Nitinol. The inventions disclosed in this document facilitate incorporation of radiopaque material and therefore product visualization without compromising the superelastic response of the outer member or inner tubular member. It is intended that any of the designs and inventions disclosed may be adopted to enhance the radiopacity of a clot retrieval device such as shown in FIG. 1, or any clot retrieval device comprising an expandable body.

In the embodiment shown the radiopacity of the outer member is enhanced by the presence of Radiopaque elements 107, which are attached to the outer member by supporting fibers 106. These fibers may be connected to the framework of the outer member by a variety of means, including threading the fibers through eyelets or attachment features. Radiopaque elements 107 may comprise tubes, beads, or coils of a radiodense material such as Gold, Tungsten, Tantalum, Platinum or alloy containing these or other high atomic number elements. Polymer materials

10

might also be employed, containing a Radiopaque filler such as Barium Sulphate, Bismuth SubCarbonate, Barium Oxy-Chloride or Tantalum.

FIG. 2*a* is an isometric view of a portion of a clot retrieval device 1001 with strut feature 1002 and crown feature 1007 comprising a superelastic material such as Nitinol. The portion of the clot retrieval device is shown in an expanded configuration. It can be appreciated that in the collapsed configuration, for clot retrieval device delivery, the struts 1002 may move to a position adjacent each other. During an interventional procedure, such as a neurothrombectomy procedure, the patient anatomy and device location in visualized with the aid of x-ray equipment such as a fluoroscope. Source x-ray beam 1003 originates at a photon beam source and targets device 1001. Partially scattered x-ray beam 1004 is the photon beam deflected by device 1001 which passes to detector 1008. Partially scattered x-ray beam generically refers to a photon beam which may be absorbed or scattered by a material (e.g. photoelectric absorption or Compton scattering). For materials, such as Nitinol that is relatively non-radiopaque relative to the treatment environment, source photon beams 1004 may pass through the device relatively uninterrupted, without being absorbed, changing trajectory, or without a significant wavelength change.

FIG. 2*b* is a representation of resulting image 1011 captured by detector 1008 in FIG. 2*a*. Low contrast image 1013 represents the outline of device 1012 under x-ray. Device 1012 may not be visible or barely visible if it comprises standard material such as Nitinol and/or if device strut feature dimensions are small enough to be below a detectable range. This is due to the level of scattering of the x-ray or photon beam being relatively uninterrupted by device 1012 relative to the tissue environment in which it is placed.

FIG. 2*c* is an isometric view of a portion of a clot retrieval device 1021 with strut feature 1022 and crown feature 1027 comprising a radiopaque material, or a superelastic material such as Nitinol fully covered with radiopaque material through a process such as electroplating or sputtering. Source x-ray beam 1023 is a source photon beam between and x-ray source and device 1021. Highly scattered x-ray beam 1025 is the photon beam between device 1001 and detector 1008. As a source x-ray beam 1023 passes through radiopaque materials, such as noble metals such as gold, platinum, and the like, the level of scattering of a beam is relatively much greater than the level of scattering of either an adjacent non-radiopaque device comprising Nitinol or relative to the treatment environment where source x-ray beams 1023 pass through relatively uninterrupted.

FIG. 2*d* is a representation of resulting image 1031 captured by detector 1028 in FIG. 2*c*. High contrast image 1034 represents the outline of device 1032 under x-ray. Device 1032 is highly visible as it comprises a radiopaque material or material combination such as Nitinol coated with a radiopaque material. This is due to the difference high level of scattering of the x-ray or photon beam, highly uninterrupted by device 1032 relative to the tissue environment in which it is placed.

FIG. 3*a* is an isometric view of a portion of a clot retrieval device 1041 with strut feature 1042 and crown feature 1047. The device structure substantially comprises superelastic Nitinol material, especially at crown feature 1047 where a high level of elastic recovery is desirable for effective device operation. Discrete radiopaque marker 1045 is located on strut feature 1042 as an example of a location on a structural feature of the device which deflects less and requires less elastic recovery than other features of the device, for

11

example crown feature **1047**. Several embodiments of devices incorporating discrete radiopaque marker **1045** are disclosed later. Source x-ray beam **1043** is used to image device **1041** and in this example a mixture of highly scattered x-ray beam **1046** and partially scattered x-ray beam **1044** reach detector **1048**.

FIG. **3b** is a representation of x-ray image **1051** of device **1052** captured by detector **1048** (FIG. **3a**). Low contrast image **1053** represents areas of device **1041** in FIG. **3a** comprising superelastic materials such as Nitinol and high contrast image **1054** represents the location of discrete radiopaque marker **1045** in FIG. **3a** which interrupts the path of x-ray source beam **1043**. Device **1052** is partially visible to the user as it comprises sections of a radiopaque material and non-radiopaque material. This is due to the difference level of scattering of the x-ray or photon beam, highly uninterrupted by discrete radiopaque marker **1045** relative to the tissue environment and strut feature **1042** and crown feature **1047** comprising superelastic material such as Nitinol which has a partially scattered x-ray beam.

FIG. **4a** and FIG. **4b** further represent the scattering of x-ray beams and interruption of beam patterns as they pass through a medical device such as a clot retrieval device. FIG. **4a** is a cross section view of clot retrieval device **1061** comprising strut feature **1062** with discrete radiopaque marker **1065**. Source x-ray beam **1063** passes through the device, and the photon beam reaches x-ray detector **1068** to image device **1061**. The wavelength and trajectory of partially scattered photon beam **1066** passed through strut feature **1062** comprising nitinol material without significant disruption. The wavelength and trajectory of highly scattered photon beam **1066** passed through discrete radiopaque marker **1065** is significantly changed or absorbed by said discrete radiopaque marker.

FIG. **4b** is an illustration of x-ray image **1071** with low contrast image **1074**, high contrast image **1073**, and shadow zone **1075**. Shadow zone **1075** in FIG. **4b** occurs as a result of a mixture of partially scattered photon beams **1064** and highly scattered photon beams **1066** reaching the same area of detector **1068** in FIG. **4a**.

FIG. **5** is a graphical representation of an x-ray image resulting from of two adjacent shadow zones **1085** combining to create Intersection Zone **1086**.

FIG. **6a** is a cross section view of a portion of a clot retrieval device **1091** with strut feature **1092** and a plurality of discrete radiopaque markers **1095**. The device structure substantially comprises superelastic Nitinol material, especially strut feature **1092** and especially areas where a high level of elastic recovery is desirable for effective device operation such as crown features not shown in this drawing. A plurality of discrete radiopaque markers **1095** are located on strut feature **1092** as an example of a location on a structural feature of the device which deflects less and requires less elastic recovery than other features of the device. Source x-ray beam **1093** is used to image device **1091** and in this example a mixture of highly scattered x-ray beams **1096** and partially scattered x-ray beam **1094** reach detector **1098** after filtration through an anti-scatter grid.

FIG. **6b** is a representation of x-ray image **1101** of device **1092** (FIG. **3a**) captured by detector **1098** (FIG. **3a**). Low contrast image **1104** represents areas of device **1091** in FIG. **3a** comprising superelastic materials such as Nitinol and high contrast image **1104** represents the location of discrete radiopaque markers **1095** in FIG. **3a** which interrupts the path of x-ray source beam **1043**. Shadow Zone **1105** in FIG. **3a** corresponds with, referring back to FIG. **3a**, a location where a mixture of highly scattered x-ray beams **1096** and

12

partially scattered x-ray beams **1094** reach the same location of x-ray detector **1098**. Intersection Zone **1106** in FIG. **3b** represents a zone where, referring back to FIG. **3a**, a mixture of highly scattered x-ray beams **1096** and partially scattered x-ray beams **1094** reach the same location of x-ray detector **1098** in a region where discrete radiopaque markers **1095** are located in relatively close proximity. The configuration has the advantage of creating the illusion for the user of a continuous marker under x-ray imaging, thereby providing fuller information on the geometry of the device.

FIG. **7a** and FIG. **7b** are respective isometric and developed plan views of a repeating pattern of clot retrieval device **1201**, comprising strut features **1202** and crown features **1203**. Clot retrieval device has an expanded configuration as shown in FIGS. **7a** and **7b** and a collapsed configuration for delivery. In the collapsed configuration areas of high strain, preferably high elastic strain, are concentrated at crown features **1203**. Force is transmitted to crown features **1203** via structural strut features **1202**. Low strain, preferably low elastic strain, regions are concentrated in strut features **1202**.

FIG. **8** is a developed plan view of a portion of another clot retrieval device **1301**, comprising strut features **1302** and crown features **1303**. In this embodiment, discrete elongate radiopaque markers **1304** are located in strut features **1302** and undergo low levels of strain as clot retrieval device **1301** moves from a collapsed to an expanded configuration. As described previously, radiopaque markers generally comprise noble metals which have lower yield points and therefore reduced elastic recovery in contrast to a superelastic material such as Nitinol.

FIG. **9** is developed plan view of another clot retrieval device **1401** comprising crown features **1403**, strut features **1402**, discrete radiopaque markers **1404**, and inter-marker strut region **1405**. In this embodiment, limitations associated with conflicting requirements of highly recoverable elastic strain and incorporating radiopaque features to optimize visibility are overcome. The location of discrete radiopaque markers **1404** in low strain strut features **1402** away from high strain location crown features **1403** reduces overall plastic strain and spacing discrete radiopaque markers apart in a strut to create inter-marker strut regions **1405** further reduces accumulated plastic strain to optimize device operation, particularly in moving from a collapsed configuration to an expanded configuration and transmission of force by clot retrieval device **1401** in a radial direction, which is desirable for effective clot retrieval. Referring back to FIGS. **6a** and **6b**, it will be appreciated that spacing marker bands apart will provide high quality visual information to the user due as high contrast regions are created both from radiopaque markers and from combined shadow zones where radiopaque markers are located adjacent each other.

FIG. **10a** is a sectioned plan view of a portion of partially coated clot retrieval device **1501** having crown feature **1510**, uncoated strut feature **1516**, and partially coated strut feature **1511** partially covered in a radiopaque coating **1515**. The strut and crown features may comprise a highly elastic material such as Nitinol, and the radiopaque material may comprise noble metals such as gold or platinum or the like or a polymer material such as polyurethane, Pebax, nylon, polyethylene, or the like, filled with radiopaque filler such as tungsten, barium sulphate, bismuth SubCarbonate, bismuth oxychloride or the like or an adhesive filled with radiopaque filler. Strut features and crown features may comprise Nitinol material with strut sidewall recess feature **1512**. In the example shown, strut sidewall recess feature comprises a series of grooves in the sidewall of the strut. Grooves may

13

be incorporated in a sidewall using cutting process such as laser cutting or other cutting means of incorporated through mechanical abrasion, cutting, grinding, or selective chemical etching. Other recess features may be incorporated such as dimples, knurls, or highly roughened surface to achieve a non-planar, textured, or rough surface. The coating can be applied as a single step (a partially coated device is shown for illustration purposes) through a process such as electroplating, sputtering, dipping, spraying, cladding, physical deposition, or other means.

FIG. 10b is a detailed view of partially coated strut feature 1511 showing uncoated groove 1512 for illustration purposes on one side and coating 1515 on the other side. Device 1501 has strut sidewall recess feature 1512 and device 1501 is preferentially coated in these areas with thick coating section 1513 resulting, which is located in a low-strain area for effective operation. The elastic recovery dampening effect of coating material 1515 has less impact on low strain strut features. Crown feature 1510 has a thin coating 1514 and is less preferentially coated because of its non-recessed, non-textured, or smooth surface, so potential dampening effect of radiopaque coating is minimized in parts of the clot retrieval device 1501 features requiring more elastic recovery such as crown feature 1510.

FIG. 10c is a partially cut isometric view of clot retrieval device 1501. The device is shown with coating 1515 partially cut away for illustration purposes. Clot retrieval device 1501 has crown features 1510, uncoated strut feature 1516 with strut sidewall recess feature 1512 to promote thick coating layer 1513 in on low strain parts of the device and thin coating layer 1514 on high strain parts of the device.

FIG. 11 is an isometric view of a repeating cell of clot retrieval device 1601 comprising crown feature 1602 and strut feature 1603. Strut feature 1603 has top surface grooves 1604 to promote preferential radiopaque coating adherence now on the top surface in a similar manner to preferential coating deposition or adherence described previously.

FIG. 12 is an isometric view of a repeating cell of clot retrieval device 1701 comprising crown feature 1702 and strut feature 1703. Strut feature 1703 has top surface dimples 1704 to promote preferential radiopaque coating adherence on the top surface in a similar manner to preferential coating deposition or adherence described previously. Grooves 1604 or dimples 1704 in FIG. 11 and FIG. 12 respectively may be added through processing techniques such as laser ablation, laser cutting, mechanical abrasion such as grinding, mechanical deformation process such as knurling or indentation and the radiopaque covering described previously.

FIG. 13a is an isometric view of tubing 1801 comprising Nitinol material 1803 and radiopaque cladding 1802 comprising a radiopaque material such as a gold, platinum, iridium or tantalum. This material may be processed by means such as electroplating, sputtering, or a mechanical compression process such as crimping or drawing.

FIG. 13b is an isometric view of tubing 1806 with comprising Nitinol material 1803 and cladding 1302 comprising rings of radiopaque material, with intermittent gaps 1304 between cladding rings 1302. Tubing 1806 may be manufactured from applying a secondary process to tubing 1801 in FIG. 13a by removing annular sections of radiopaque material through a process such as laser ablation, laser cutting, or mechanical removal such as grinding or cutting for example on a lathe.

FIG. 14 is an isometric view of clot retrieval device 1901. Clot retrieval device 1901 may be constructed of tubing 1806 as shown in FIG. 14. Device 1901 may be made through a series of processing steps wherein tubing 1806 is cut to form

14

strut and crown patterns, deburred, expanded and heat treated, and electropolished. Crown features 1903, which are areas requiring high elastic recovery, are located in areas in which cladding 1902 is absent, and strut feature 1904, which undergoes less strain and requiring less elastic recovery, is located in areas where cladding 1902 remains.

FIG. 15 is an isometric view of clot retrieval device 2001 with radiopaque material free crowns 2003 as in device 1901 of FIG. 14 but the spacing of cladding rings in device 2001 is such that strut 2004 also has clad-free areas 2005 to further promote elastic behavior of strut feature 2004. In transitioning from collapsed configuration to expanded configuration or vice versa, areas of high strain are located at crown feature 2003 and elastic recovery is less of a requirement for strut features 2004. It may however be desirable in use, particularly if a device is required to conform to a tortuous vessel such in use, for strut feature 2004 to deflect in bending and recover elastically. Device 2001 with radiopaque-material-free areas 2005 has the advantage of facilitating more recoverable strain. Devices 2001 and 1901 may be manufactured from clad tubing 1806 and cutting a pattern whereby crown features and strut features are located in clad-free and clad areas respectively, they may also be constructed from tubing 1801 and cladding removed during or subsequent to the laser cutting process.

FIG. 16 is an isometric view of clot retrieval device 2101 comprising crown features 2102 and strut features 2105. Strut 2105 comprises thick strut sections 2104 and regular strut sections 2103, which respectively provide enhanced radiopacity and flexibility. Radiopacity of device 2101 is enhanced by the addition of thickened strut sections 2104 in strut feature 2105. The increased material volume in thickened strut section 2104 blocks x-ray/photon beams in contrast to crown feature 2102 and regular strut section 2103 without compromising device flexibility performance.

FIG. 17a is a cross section of a structural element 2204 in a non-strained condition of clot retrieval device 2201 comprising Nitinol material, with radiopaque material coating 2202. Line 2203 represents a line or plane within structural element 2204 away from the neutral axis of bending.

FIG. 17b is a cross section of structural element 2204 in a strained configuration through a bending load.

FIG. 18a is a cross section of structural element 2304 of clot retrieval device 2301 comprising superelastic material such as Nitinol and discontinuous radiopaque coating 2302. Line 2303 is a reference line close to device surface away from the neutral axis of structural element 2304. In FIG. 18b, structural element 2304 is shown in the deformed or bent configuration with line 2303, which is between the neutral axis and the outer surface, representing a line or plane of constant strain. Discontinuous radiopaque coating 2302 may be deposited through means such as a sputter coating process, growing single crystals on the surface in a discrete fibre-like micro or nano-structure or columnar structure. Other means of achieving discontinuous radiopaque coating include micro-laser ablation of layers or mechanical separation such as slicing. One advantage of such a coating structure is that a high strain (or deformation) can be induced in the substrate material without a high strain being induced in the coating material. This is because the discrete micro-fibers or micro-columns from which the coating is composed have minimal connectivity between each other. Thus, the outer ends of the micro-fibers or micro-columns simply move further apart when the a convex bend is applied to the substrate material as shown in FIG. 18b. A smooth surface may subsequently be achieved on the device by coating with

15

a polymer coating, such as a layer of Pebax for example, or Parylene, or a hydrophilic material and/or a hydrogel.

Deformation, such as the applied bending load shown in FIG. 17 by way of example, causes material to deform in tension along line **2203**. For materials such as Nitinol, the stress-strain or force-deflection deformation generally follows a curve shown in FIG. 19a where material along line **2204** starts at point A in and follows the arrows to generate a typical flag-shaped stress-strain curve. Stress or force is shown on the y-axis and strain or deflection is shown along the x-axis of FIG. 19. When an applied load or deflection is removed, for nitinol, the load is reversed at point R and the material follows the unloading curve shown until it reaches point B. For a perfectly elastic or pseudoelastic material, point A and point B are coincident and there is no residual or plastic strain in the material, and therefore no permanent deformation.

Referring now to FIG. 19b, a pattern of stress-strain is shown which is more typical of a radiopaque material such as gold, where loading begins at point A and the stress-strain behavior follows the loading pattern shown until the load is removed and the strain reduces to point B. Since point A and point B are not coincident, plastic or permanent deformation results, which is quantified as the distance between point B and point A. Considering the structural element **2201** comprising material such as Nitinol combined with radiopaque material such as Gold, the loading and unloading pattern is illustrated in FIG. 19c wherein load or strain is applied, and when the load is removed at point R, the internal material stress-strain response follows the curve from point R to point B. The combined material properties are such that plastic strain, defined by the distance between B and A along the x-axis, results. In this configuration the plastic strain is less than that of pure radiopaque material but more than that of pure Nitinol. The dampening effect on device recovery is generally not desirable for effective operation of clot retrieval device performance.

FIG. 19d is a stress-strain curve of structural element **2301M** bending, taking line **2303** as an example, where the device is loaded from point A to point R and when the load is removed the device unloads from point R to point B. The magnitude of plastic strain is reduced (reduced distance between point B and A when comparing FIGS. 19c and 19d) as the coating becomes more discontinuous and approaches zero as the number of discontinuities increases.

FIG. 20a is a side view of Clot Retrieval Device Outer Member **2401** comprising strut features **2402** and crown features **2403**. Radiopaque filaments **2405** are connected between crown features or strut features to enhance device radiopacity. Radiopaque filaments are located along the outer circumference of clot retrieval device outer member **2401** in order to enhance fluoroscopic visualization of the expanded or collapsed configuration of the device. The circumferential location of the filaments may also aid visualization of device interaction with a clot during use. The filaments may run parallel to the axis of the device, or in a helical path from crown to crown, crown to strut, or strut to strut in order to maintain clot reception space **2406** for clot retrieval. Radiopaque filaments may comprise single or multiple strands of radiopaque wire such as tungsten, platinum/iridium or gold, or similar materials.

FIG. 20b is a side view of Clot Retrieval Device Outer Member **2501** comprising strut features **2502** and crown features **2503**. Filaments **2505** incorporating radiopaque beads **2506** are connected between crown features or strut features to enhance device radiopacity. Sequenced radiopaque beads **2505** along filaments **2505** do not con-

16

tribute to the mechanical stiffness of the device or contribute to or detract from radial force in any way, and in a collapsed configuration wrap into inter-strut spaces in a versatile manner. The filaments may run parallel to the axis of the device, or in a helical path from crown to crown, crown to strut, or strut to strut in order to maintain clot reception space **2507** for clot retrieval as in FIG. 20a. While radiopaque beads are spaced apart to maintain beaded-filament flexibility, adjacent beads create the illusion of a continuous radiopaque member, providing high quality visual information to the user. Filaments may comprise high ultimate tensile strength monofilament or multifilament polymers such as UHMWPE, Kevlar, aramid, LCP, PEN or wire such as Nitinol and radiopaque beads may comprise polymer filled with radiopaque filler such as tungsten powder, barium sulphate, or solid radiopaque material such as gold or platinum.

FIG. 20c is a side view of clot retrieval device outer member **2601** comprising strut features **2602** and crown features **2603**. Filaments **2605** are incorporated in device outer member **2601** in a similar matter detailed in FIG. 20b, with radiopaque coils **2608** located on filament **2605**. Radiopaque coils may comprise wound wire such as platinum/iridium or platinum/tungsten or similar radiopaque wire wound into a spring-like coil structure. Filaments **2605** incorporating radiopaque coils **2608** maintain flexibility in bending so device performance characteristics such as flexibility, trackability, radial force, deliverability, etc. are not compromised.

FIG. 21a is an isometric view of clot retrieval device outer member **2701** comprising strut features **2702** and crown features **2703**. An elongate radiopaque thread **2405** is incorporated in the structural elements, i.e. struts or crowns, of clot retrieval device outer member. Elongate radiopaque thread **2704** threads the perimeter of outer member **2704** to define the outer boundary of device in an axial and circumferential direction under fluoroscopic imaging. A plurality of radiopaque threads may be incorporated to further define the boundary of the outer member.

FIG. 21b illustrates a means of incorporating elongate thread **2804** in strut **2802** through eyelet **2805**. Elongate radiopaque thread may be incorporated through other means such as surface adhesion.

FIG. 21c and FIG. 21d are cross section views of bifilar elongate radiopaque threads **2901** and **3001** respectively incorporated in outer member **2701** in FIG. 21a. Thread **2904** is a single material radiopaque thread such as platinum/iridium, platinum/tungsten, or gold. Thread **3001** in FIG. 21d comprises Nitinol outer material **3003** with inner radiopaque core such as a gold core. The coaxial configuration of radiopaque thread **3001** part retains the elasticity/elastic recovery, in particular at low strains, and has the advantage of contributing to the structural integrity of clot retrieval device **2701**, for example it may be used to enhance the radial force of the device. The bifilar configuration of thread **2901** enhances radiopacity by increasing the effective area or volume of material scattering the x-ray field while maintaining good flexibility.

FIG. 22 is a plan view of clot retrieval device cell **3101** comprising structural strut **3102** and structural crown **3102** with radiopaque markers **3106** traversing cell **3101**, connected via non-structural struts **3107**. Non-structural struts **3107** are connected to structural struts **3102** at connection crown **3105** and have minimal structural integrity and therefore minimal contribution to the structural rigidity in bending and in the radial direction. The cell may comprise a

17

Nitinol material with radiopaque markers incorporated in eyelets using a crimping process.

FIG. 23 is an isometric view of clot retrieval device cell 3201 comprising crown features 3203 and strut features 3202. A radiopaque filament 3204 is threaded through side holes 3205 in strut 3202. Side holes 3205 facilitate incorporation of radiopaque filament in inter-strut space, therefore not adding to the outer or inner profile of the device. Radiopaque filament may comprise radiopaque material, or polymer or wire monofilaments or yarns with radiopaque beads or coils described previously.

It will be apparent from the foregoing description that, while particular embodiments of the present invention have been illustrated and described, various modifications can be made without parting from the spirit and scope of the invention. Accordingly, it is not intended that the present invention be limited and should be defined only in accordance with the appended claims and their equivalents.

What is claimed is:

1. A method of manufacturing an expandable body of a clot retrieval device, the expandable body comprising:
 - a framework of interconnected strut elements distal of an elongate shaft, the strut elements forming an outer expandable body and an inner expandable body, at least a portion of the strut elements comprising:
 - a first coating of radiopaque material defining a plurality of micro-columns, wherein each micro-column includes a length extending between a first end coupled to at least one of the strut elements and a second free end opposite the first end, the length of each micro-column is longer than a width of each micro-column; wherein the second free ends of the micro-columns are capable of moving further apart when a convex bend is applied to at least a portion of the strut elements during use; and
 - a second coating,
- the method comprising:
 - applying the first coating to the strut elements,
 - removing at least a portion of the first coating from at least one area of the strut elements, and
 - cutting away regions of both the first coating and the strut elements to form an interconnected pattern of coated and uncoated regions.

18

2. The method according to claim 1, wherein the step of applying comprises an electroplating process, a dipping process, a plasma deposition process, an electrostatic process, a dip or spray coating process, a sputtering process, a soldering process, a cladding process or a drawing process.

3. The method according to claim 1, wherein the step of removing comprises a grinding process, a polishing process, a buffing process, an etching process, a laser cutting or laser ablation process.

4. The method according to claim 1, wherein the step of cutting away comprises a laser cutting process, a wire cutting process, a water jet cutting process, a machining process or an etching process.

5. The method according to claim 1, wherein the first coating is Gold, Tantalum, Tungsten, or Platinum.

6. The method according to claim 1, wherein the interconnected pattern comprises a plurality of strut elements and connector elements.

7. The method according to claim 1, wherein the removing step removes at least a portion of the first coating from those areas of the interconnected pattern which experience the highest strain in moving from the expanded state to the collapsed state, and/or from the collapsed state to the expanded state.

8. The method according to claim 1, wherein the strut elements terminate in crown elements.

9. The method according to claim 1, wherein the micro-columns are porous.

10. The method according to claim 1, wherein the framework is formed from a superelastic material.

11. The method according to claim 1, wherein the micro-columns of the first coating are generally independent columns that extend substantially perpendicular to a substrate of at least a portion of the strut elements.

12. The method according to claim 1, wherein the second coating is a hydrophilic material or a hydrogel.

13. The method according to claim 1, further comprising applying the second coating to fill adjacent recesses of at least a portion of the strut elements.

* * * * *