



(12) **United States Patent**
Tanis et al.

(10) **Patent No.:** **US 12,403,331 B2**
(45) **Date of Patent:** **Sep. 2, 2025**

(54) **MEDICAL DEVICE**

(71) Applicant: **Smith & Nephew, Inc.**, Memphis, TN (US)

(72) Inventors: **Kevin J. Tanis**, Collierville, TN (US); **Jin Zhang**, Memphis, TN (US); **Kelly Ann Umstead**, Raleigh, NC (US)

(73) Assignee: **Smith & Nephew, Inc.**, Memphis, TN (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 116 days.

(21) Appl. No.: **18/102,044**

(22) Filed: **Jan. 26, 2023**

(65) **Prior Publication Data**

US 2023/0166130 A1 Jun. 1, 2023

Related U.S. Application Data

(63) Continuation of application No. 16/863,820, filed on Apr. 30, 2020, now Pat. No. 11,565,134, which is a (Continued)

(51) **Int. Cl.**
A61N 7/00 (2006.01)
A61B 5/1172 (2016.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61N 7/00** (2013.01); **A61B 5/1172** (2013.01); **A61B 34/25** (2016.02); **G16H 40/63** (2018.01);
(Continued)

(58) **Field of Classification Search**
CPC A61N 7/00; A61N 2007/0013; A61N 2007/0078; A61B 5/1172; A61B 34/25;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

695,270 A 3/1902 Beringer
3,194,239 A 7/1965 Sullivan et al.
(Continued)

FOREIGN PATENT DOCUMENTS

CA 2819475 A1 6/2012
CN 1797418 A 7/2006
(Continued)

OTHER PUBLICATIONS

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. EP2627277, dated Mar. 16, 2021, 3 pages.

(Continued)


Primary Examiner — Sanjay Cattungal

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A medical device includes a treatment module configured to apply a treatment to a patient. The medical device includes an interface configured to operatively connect to a removable storage device storing authorization data that identifies a level of treatment authorization. The medical device includes a processing device configured to perform operations in response to receiving user input indicating a treatment should be initiated. The operations include determining whether the removable storage device is valid for use with the medical device. If the removable storage device is determined to be valid, the authorization data is accessed. The processing device determines whether the treatment is authorized based on the accessed authorization data. If the treatment is determined to be authorized, the treatment module is controlled to apply the treatment. If the treatment is determined to not be authorized, the treatment module is controlled such that the treatment is not applied.

20 Claims, 20 Drawing Sheets

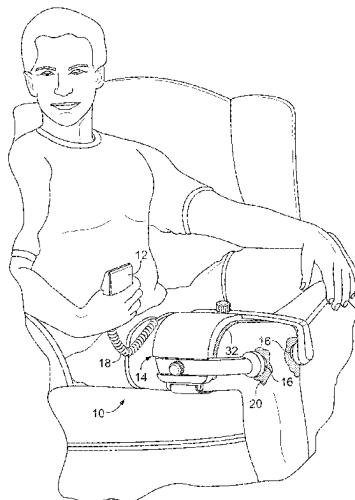

Related U.S. Application Data

continuation of application No. 15/482,449, filed on Apr. 7, 2017, now Pat. No. 10,639,502, which is a continuation of application No. 15/357,883, filed on Nov. 21, 2016, now Pat. No. 10,086,216, which is a continuation of application No. 13/271,870, filed on Oct. 12, 2011, now Pat. No. 9,526,920.

- (60) Provisional application No. 61/483,445, filed on May 6, 2011, provisional application No. 61/405,757, filed on Oct. 22, 2010, provisional application No. 61/405,405, filed on Oct. 21, 2010, provisional application No. 61/392,154, filed on Oct. 12, 2010.

(51) **Int. Cl.**

A61B 34/00 (2016.01)

G16H 40/63 (2018.01)

G16H 40/67 (2018.01)

A61B 90/00 (2016.01)

A61B 90/90 (2016.01)

(52) **U.S. Cl.**

CPC *G16H 40/67* (2018.01); *A61B 2034/258* (2016.02); *A61B 2090/0803* (2016.02); *A61B 90/90* (2016.02); *A61M 2205/6009* (2013.01); *A61N 2007/0013* (2013.01); *A61N 2007/0078* (2013.01)

(58) **Field of Classification Search**

CPC *A61B 90/90*; *A61B 2034/258*; *A61B 2090/0803*; *G16H 40/63*; *G16H 40/67*; *A61M 2205/6009*; *H04L 67/12*
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,642,769 A 2/1987 Petrofsky
4,832,299 A 5/1989 Gorton et al.
4,899,839 A 2/1990 Dessertine et al.
5,016,172 A 5/1991 Dessertine
5,158,528 A 10/1992 Walker et al.
5,174,533 A 12/1992 Pryor et al.
5,215,523 A 6/1993 Williams et al.
5,219,428 A 6/1993 Stern
5,419,768 A 5/1995 Kayser
5,449,347 A 9/1995 Preen et al.
5,466,229 A 11/1995 Elson et al.
5,473,536 A 12/1995 Wimmer
5,556,372 A 9/1996 Talish et al.
5,582,601 A 12/1996 Wortrich et al.
5,584,824 A 12/1996 Gillette et al.
5,590,658 A 1/1997 Chiang et al.
5,599,308 A 2/1997 Krupa
5,622,429 A 4/1997 Heinze
5,634,939 A 6/1997 Kuster et al.
5,656,027 A 8/1997 Ellingboe
5,669,892 A 9/1997 Keogh et al.
5,687,717 A 11/1997 Halpern et al.
5,693,013 A 12/1997 Geuder
5,748,103 A 5/1998 Flach et al.
5,779,207 A 7/1998 Danby
D408,625 S 4/1999 Barker
5,933,136 A 8/1999 Brown
5,956,023 A 9/1999 Lyle et al.
5,960,403 A 9/1999 Brown
5,989,234 A 11/1999 Valerio et al.
6,018,289 A 1/2000 Sekura et al.
6,055,506 A 4/2000 Frasca et al.
6,161,095 A 12/2000 Brown
6,174,306 B1 1/2001 Fleischmann
6,228,056 B1 5/2001 Boehringer et al.
6,241,739 B1 6/2001 Waldron

6,250,482 B1 6/2001 Want et al.
6,261,249 B1 7/2001 Talish et al.
6,270,460 B1 8/2001 McCartan et al.
6,308,089 B1 10/2001 Von Der Ruhr et al.
6,336,900 B1 1/2002 Alleckson et al.
6,353,445 B1 3/2002 Babula et al.
6,375,614 B1 4/2002 Braun et al.
6,385,622 B2 5/2002 Bouve et al.
6,387,092 B1 5/2002 Burnside et al.
6,406,426 B1 6/2002 Reuss et al.
6,413,213 B1 7/2002 Essenpreis et al.
6,434,572 B2 8/2002 Derzay et al.
6,460,041 B2 10/2002 Lloyd
6,572,530 B1 6/2003 Araki et al.
6,574,518 B1 6/2003 Lounsberry et al.
6,577,893 B1 6/2003 Besson et al.
6,605,032 B2 8/2003 Benkowski et al.
6,640,145 B2 10/2003 Hoffberg et al.
6,640,246 B1 10/2003 Gary et al.
6,675,131 B2 1/2004 Hahn
6,681,003 B2 1/2004 Linder et al.
6,723,046 B2 4/2004 Lichtenstein et al.
6,738,052 B1 5/2004 Manke et al.
6,747,556 B2 6/2004 Medema et al.
6,766,218 B2 7/2004 Rosenblum
6,779,024 B2 8/2004 DeLaHueraga
6,782,285 B2 8/2004 Birkenbach et al.
6,792,306 B2 9/2004 Henley et al.
6,811,533 B2 11/2004 Lebel et al.
6,868,528 B2 3/2005 Roberts
6,871,211 B2 3/2005 Labounty et al.
6,909,974 B2 6/2005 Yung et al.
6,912,481 B2 6/2005 Breunissen et al.
6,961,731 B2 11/2005 Holbrook
7,004,915 B2 2/2006 Boynton et al.
7,022,113 B2 4/2006 Lockwood et al.
7,048,687 B1 5/2006 Reuss et al.
7,051,012 B2 5/2006 Cole et al.
7,066,883 B2 6/2006 Schmidt et al.
7,103,578 B2 9/2006 Beck et al.
7,108,683 B2 9/2006 Zamierowski
7,120,488 B2 10/2006 Nova et al.
7,128,735 B2 10/2006 Weston
7,133,869 B2 11/2006 Bryan et al.
7,167,858 B2 1/2007 Naeymi-Rad et al.
7,212,829 B1 5/2007 Lau et al.
7,264,591 B2 9/2007 Brown
7,273,483 B2 9/2007 Wiener et al.
7,304,573 B2 12/2007 Postma
7,311,665 B2 12/2007 Hawthorne et al.
7,333,002 B2 2/2008 Bixler et al.
D565,177 S 3/2008 Locke et al.
7,353,179 B2 4/2008 Ott et al.
7,361,184 B2 4/2008 Joshi
7,364,554 B2 4/2008 Bolze et al.
7,384,267 B1 6/2008 Franks et al.
7,395,214 B2* 7/2008 Shillingburg G16H 20/13
705/2
7,430,598 B2 9/2008 Raden et al.
D581,042 S 11/2008 Randolph et al.
D581,522 S 11/2008 Randolph et al.
7,448,265 B2 11/2008 Smyser et al.
7,451,002 B2 11/2008 Choubey
7,457,804 B2 11/2008 Uber et al.
7,460,872 B2 12/2008 Millard et al.
7,492,278 B2 2/2009 Zigmond et al.
7,505,815 B2 3/2009 Lee et al.
D590,934 S 4/2009 Randolph et al.
7,534,240 B1 5/2009 Johnson
7,553,306 B1 6/2009 Hunt et al.
7,569,742 B2 8/2009 Haggstrom et al.
7,594,901 B2 9/2009 Hopkins et al.
D602,582 S 10/2009 Pidgeon et al.
D602,583 S 10/2009 Pidgeon et al.
7,598,855 B2 10/2009 Scalisi et al.
7,611,500 B1 11/2009 Lina et al.
7,615,036 B2 11/2009 Joshi et al.
7,627,334 B2 12/2009 Cohen et al.
7,639,120 B2 12/2009 Sekura

(56)

References Cited

U.S. PATENT DOCUMENTS

7,649,449 B2	1/2010	Fenske et al.	8,334,768 B2	12/2012	Eaton et al.
7,670,323 B2	3/2010	Hunt et al.	8,337,482 B2	12/2012	Wood et al.
7,671,733 B2	3/2010	McNeal et al.	8,360,975 B1	1/2013	Schwieterman et al.
7,684,999 B2	3/2010	Brown	8,366,692 B2	2/2013	Weston et al.
7,699,823 B2	4/2010	Haggstrom et al.	8,377,016 B2	2/2013	Argenta et al.
7,723,560 B2	5/2010	Lockwood et al.	8,377,018 B2	2/2013	Bendele et al.
7,734,764 B2	6/2010	Weiner et al.	8,400,295 B1	3/2013	Khaira
7,749,164 B2	7/2010	Davis	8,403,902 B2	3/2013	Locke et al.
7,753,894 B2	7/2010	Blott et al.	8,409,170 B2	4/2013	Locke et al.
7,770,855 B2	8/2010	Locke et al.	8,422,377 B2	4/2013	Weiner et al.
7,776,028 B2	8/2010	Miller et al.	8,424,517 B2	4/2013	Sutherland et al.
7,779,153 B2	8/2010	Van Den Heuvel et al.	8,436,871 B2	5/2013	Alberte
7,785,277 B2	8/2010	Babaev et al.	8,439,882 B2	5/2013	Kelch
7,789,828 B2	9/2010	Clapp	8,444,392 B2	5/2013	Turner et al.
D625,801 S	10/2010	Pidgeon et al.	8,457,740 B2	6/2013	Osche
7,827,148 B2	11/2010	Mori et al.	8,480,641 B2	7/2013	Jacobs
7,846,141 B2	12/2010	Weston	8,494,349 B2	7/2013	Gordon
7,857,806 B2	12/2010	Karpowicz et al.	8,515,776 B2	8/2013	Schoenberg
7,865,375 B2	1/2011	Lancaster et al.	8,532,764 B2	9/2013	Duke
7,889,069 B2	2/2011	Fifolt et al.	8,540,688 B2	9/2013	Eckstein et al.
7,890,887 B1	2/2011	Linardos et al.	8,545,483 B2	10/2013	Schwabe et al.
7,912,823 B2	3/2011	Ferrari et al.	8,552,880 B2	10/2013	Kopp et al.
D635,588 S	4/2011	Sprules	8,554,195 B2	10/2013	Rao
7,925,603 B1	4/2011	Laidig et al.	8,558,964 B2	10/2013	Bedingfield
7,927,319 B2	4/2011	Lawhorn	8,560,082 B2	10/2013	Wei
7,933,817 B2	4/2011	Radl et al.	8,577,694 B2	11/2013	Kanaan
7,945,452 B2	5/2011	Fathallah et al.	8,595,553 B2	11/2013	Goertler et al.
7,955,281 B2	6/2011	Pedersen et al.	8,604,265 B2	12/2013	Locke et al.
7,956,727 B2	6/2011	Loncar	8,617,129 B2	12/2013	Hartwell
7,976,519 B2	7/2011	Bubb et al.	8,622,981 B2	1/2014	Hartwell et al.
7,981,098 B2	7/2011	Boehringer et al.	8,626,342 B2	1/2014	Williams et al.
D644,250 S	8/2011	Barber et al.	8,626,526 B2	1/2014	Lemke et al.
7,988,850 B2	8/2011	Roncadi et al.	8,628,258 B2	1/2014	Vogt
8,007,481 B2	8/2011	Schuessler et al.	8,632,485 B2	1/2014	Schlaeper et al.
8,015,443 B2	9/2011	Adachi	8,641,693 B2	2/2014	Locke et al.
8,015,972 B2	9/2011	Pirzada	8,652,111 B2	2/2014	Pratt et al.
8,019,618 B2	9/2011	Brown	8,659,420 B2	2/2014	Salvat et al.
8,048,046 B2	11/2011	Hudspeth et al.	8,668,677 B2	3/2014	Eckstein et al.
8,054,950 B1	11/2011	Hung et al.	8,676,597 B2	3/2014	Buehler et al.
8,061,360 B2	11/2011	Locke et al.	8,689,008 B2	4/2014	Rangadass et al.
8,066,243 B2	11/2011	Svedman et al.	8,694,600 B2	4/2014	Gaines et al.
8,094,009 B2	1/2012	Allen et al.	8,747,376 B2	6/2014	Locke et al.
8,096,515 B2	1/2012	Locke et al.	8,756,078 B2	6/2014	Collins, Jr. et al.
8,100,873 B2	1/2012	Jaeb et al.	8,768,441 B2	7/2014	De Zwart et al.
8,105,295 B2	1/2012	Blott et al.	8,771,259 B2	7/2014	Karpowicz et al.
8,126,735 B2	2/2012	Dicks et al.	8,781,847 B2	7/2014	Simms et al.
8,130,095 B2	3/2012	Allen et al.	8,795,171 B2	8/2014	Adamczyk
8,131,472 B2	3/2012	Chow et al.	8,795,244 B2	8/2014	Randolph et al.
8,180,750 B2	5/2012	Wilmering et al.	8,798,284 B2	8/2014	Cartwright et al.
8,190,445 B2	5/2012	Kuth et al.	8,814,841 B2	8/2014	Hartwell
8,190,448 B2	5/2012	Bajars et al.	8,814,842 B2	8/2014	Coulthard et al.
8,216,198 B2	7/2012	Heagle et al.	8,827,983 B2	9/2014	Braga et al.
8,228,188 B2	7/2012	Key et al.	8,843,327 B2	9/2014	Vernon-Harcourt et al.
8,235,955 B2	8/2012	Blott et al.	8,845,603 B2	9/2014	Middleton et al.
8,240,470 B2	8/2012	Pidgeon et al.	8,845,604 B2	9/2014	Croizat et al.
8,246,606 B2	8/2012	Stevenson et al.	8,852,149 B2	10/2014	Weston et al.
8,246,607 B2	8/2012	Karpowicz et al.	8,858,517 B2	10/2014	Pan et al.
8,249,894 B2	8/2012	Brown	8,862,393 B2	10/2014	Zhou et al.
8,255,241 B2	8/2012	Cafer	8,868,794 B2	10/2014	Masoud et al.
8,257,328 B2	9/2012	Augustine et al.	8,870,812 B2	10/2014	Alberti et al.
8,260,630 B2	9/2012	Brown	8,874,035 B2	10/2014	Sherman et al.
8,267,918 B2	9/2012	Johnson et al.	8,887,100 B1	11/2014	Cook et al.
8,280,682 B2	10/2012	Vock et al.	8,890,656 B2	11/2014	Pendse
8,284,024 B2	10/2012	Toleti et al.	8,897,198 B2	11/2014	Gaines et al.
8,284,046 B2	10/2012	Allen et al.	8,902,278 B2	12/2014	Pinter et al.
8,290,792 B2	10/2012	Sekura	8,905,959 B2	12/2014	Basaglia
8,291,337 B2	10/2012	Gannin et al.	8,905,985 B2	12/2014	Allen et al.
8,294,586 B2	10/2012	Pidgeon et al.	8,909,595 B2	12/2014	Gandy et al.
8,298,200 B2	10/2012	Vess et al.	8,926,574 B2	1/2015	Croizat et al.
8,308,714 B2	11/2012	Weston et al.	8,943,168 B2	1/2015	Wiesner et al.
8,317,752 B2	11/2012	Cozmi et al.	8,945,030 B2	2/2015	Weston
8,317,774 B2	11/2012	Adahan	8,945,073 B2	2/2015	Croizat et al.
8,323,263 B2	12/2012	Wood et al.	8,945,074 B2	2/2015	Buan et al.
8,332,233 B2	12/2012	Ott et al.	8,947,237 B2	2/2015	Margon et al.
8,333,744 B2	12/2012	Hartwell et al.	8,961,497 B2	2/2015	Ryu et al.
			8,974,429 B2	3/2015	Gordon et al.
			8,978,026 B2	3/2015	Charlton et al.
			8,996,393 B2	3/2015	Sobie
			9,017,286 B2	4/2015	Kamen et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,019,681	B2	4/2015	Locke et al.	2004/0019464	A1	1/2004	Martucci et al.
9,023,002	B2	5/2015	Robinson et al.	2004/0039255	A1	2/2004	Simonsen et al.
9,047,648	B1	6/2015	Lekutai et al.	2004/0049172	A1	3/2004	Root et al.
9,058,634	B2	6/2015	Buan et al.	2004/0054338	A1	3/2004	Bybordi et al.
9,067,003	B2	6/2015	Buan et al.	2004/0054775	A1	3/2004	Poliac et al.
9,084,845	B2	7/2015	Adie et al.	2004/0059284	A1	3/2004	Nash et al.
9,098,114	B2	8/2015	Potter et al.	2004/0064132	A1	4/2004	Boehringer et al.
9,105,006	B2	8/2015	Williamson	2004/0078223	A1	4/2004	Sacco et al.
9,135,398	B2	9/2015	Kaib et al.	2004/0102743	A1	5/2004	Walker
9,215,581	B2	12/2015	Julian et al.	2004/0120825	A1	6/2004	Bouton et al.
9,268,827	B2	2/2016	Fernandez	2004/0143458	A1	7/2004	Pulkkinen et al.
9,286,443	B2	3/2016	Ford et al.	2004/0158193	A1	8/2004	Bui et al.
9,323,893	B2	4/2016	Berry et al.	2004/0167802	A1	8/2004	Takada et al.
9,408,954	B2	8/2016	Gordon et al.	2004/0167804	A1	8/2004	Simpson et al.
9,436,800	B2	9/2016	Forrester	2004/0171982	A1	9/2004	Danchin
9,526,920	B2	12/2016	Tanis et al.	2004/0172301	A1	9/2004	Mihai et al.
9,539,373	B2	1/2017	Jones et al.	2004/0176983	A1	9/2004	Birkett et al.
9,658,066	B2	5/2017	Yuen et al.	2004/0181314	A1	9/2004	Zaleski
9,662,438	B2	5/2017	Kamen et al.	2004/0181433	A1	9/2004	Blair
9,741,084	B2	8/2017	Holmes et al.	2004/0193449	A1	9/2004	Wildman et al.
9,792,660	B2	10/2017	Cannon et al.	2004/0204962	A1	10/2004	Howser et al.
9,818,164	B2	11/2017	Nolte et al.	2004/0227737	A1	11/2004	Novak et al.
9,878,081	B2	1/2018	Leiendecker et al.	2004/0249673	A1	12/2004	Smith
9,990,466	B2	6/2018	DeBusk et al.	2005/0011282	A1	1/2005	Voegel et al.
10,061,894	B2	8/2018	Sethumadhavan et al.	2005/0022274	A1	1/2005	Campbell et al.
10,173,008	B2	1/2019	Simpson et al.	2005/0027311	A1	2/2005	Wiener et al.
10,231,878	B2	3/2019	Hartwell et al.	2005/0033124	A1	2/2005	Kelly et al.
10,639,502	B2	5/2020	Tanis et al.	2005/0055225	A1	3/2005	Mehl
2001/0013822	A1	8/2001	Nazarian et al.	2005/0055242	A1	3/2005	Bello et al.
2001/0031944	A1	10/2001	Peterson et al.	2005/0055244	A1	3/2005	Mullan et al.
2001/0041831	A1	11/2001	Starkweather et al.	2005/0060211	A1	3/2005	Xiao et al.
2001/0049609	A1	12/2001	Girouard et al.	2005/0065471	A1	3/2005	Kuntz
2002/0002326	A1	1/2002	Causey et al.	2005/0065817	A1	3/2005	Mihai et al.
2002/0002368	A1	1/2002	Tomita et al.	2005/0097200	A1	5/2005	Denning, Jr. et al.
2002/0013516	A1	1/2002	Freyre et al.	2005/0102167	A1	5/2005	Kapoor
2002/0015034	A1	2/2002	Malmberg	2005/0108046	A1	5/2005	Craft
2002/0026160	A1	2/2002	Takahashi et al.	2005/0108057	A1	5/2005	Cohen et al.
2002/0049562	A1	4/2002	Hahn	2005/0108190	A1	5/2005	Conkel
2002/0065685	A1	5/2002	Sasaki et al.	2005/0114176	A1	5/2005	Dominick et al.
2002/0082568	A1	6/2002	Yam	2005/0116126	A1	6/2005	Ugent et al.
2002/0087360	A1	7/2002	Pettit	2005/0119914	A1	6/2005	Batch
2002/0120467	A1	8/2002	Buanes	2005/0124966	A1	6/2005	Karpowicz et al.
2002/0128804	A1	9/2002	Geva	2005/0187528	A1	8/2005	Berg
2002/0128869	A1	9/2002	Kuth	2005/0209560	A1	9/2005	Boukhny et al.
2002/0135336	A1	9/2002	Zhou et al.	2005/0222873	A1	10/2005	Nephtin et al.
2002/0161317	A1	10/2002	Risk et al.	2005/0230575	A1	10/2005	Zelenski et al.
2002/0177757	A1	11/2002	Britton	2005/0240111	A1	10/2005	Chung
2002/0184055	A1	12/2002	Naghavi et al.	2005/0246416	A1	11/2005	Blomquist
2002/0193679	A1	12/2002	Malave et al.	2005/0256447	A1	11/2005	Richardson et al.
2002/0198505	A1	12/2002	Want et al.	2005/0261805	A1	11/2005	Mori et al.
2003/0009244	A1	1/2003	Engleson et al.	2005/0283382	A1	12/2005	Donoghue et al.
2003/0018395	A1	1/2003	Crnkovich et al.	2006/0004604	A1	1/2006	White
2003/0018736	A1	1/2003	Christ et al.	2006/0020161	A1	1/2006	Mageras et al.
2003/0023460	A1	1/2003	Ackermann et al.	2006/0029675	A1	2/2006	Ginther
2003/0028175	A1	2/2003	D'Antonio	2006/0064323	A1	3/2006	Alleckson et al.
2003/0036683	A1	2/2003	Kehr et al.	2006/0064491	A1	3/2006	Ebert et al.
2003/0093041	A1	5/2003	Risk, Jr. et al.	2006/0085393	A1	4/2006	Modesitt
2003/0093181	A1*	5/2003	Rosenblum	2006/0089539	A1	4/2006	Miodownik et al.
			G06V 20/66	2006/0089544	A1	4/2006	Williams, Jr. et al.
			700/232	2006/0095853	A1	5/2006	Amyot et al.
2003/0095648	A1	5/2003	Kaib et al.	2006/0132283	A1	6/2006	Eberhart et al.
2003/0105389	A1	6/2003	Noonan et al.	2006/0144440	A1	7/2006	Merkle
2003/0105649	A1	6/2003	Sheiner et al.	2006/0149171	A1	7/2006	Vogel et al.
2003/0128125	A1	7/2003	Burbank et al.	2006/0155584	A1	7/2006	Aggarwal
2003/0130567	A1	7/2003	Mault et al.	2006/0161460	A1	7/2006	Smitherman et al.
2003/0164600	A1	9/2003	Dunn et al.	2006/0190130	A1	8/2006	Fedor et al.
2003/0176183	A1	9/2003	Drucker et al.	2006/0195843	A1	8/2006	Hall
2003/0182158	A1	9/2003	Son	2006/0224051	A1	10/2006	Teller et al.
2003/0199794	A1	10/2003	Sakurai et al.	2006/0229557	A1	10/2006	Fathallah et al.
2003/0214412	A1	11/2003	Ho et al.	2006/0246922	A1	11/2006	Gasbarro et al.
2003/0221687	A1	12/2003	Kaigler	2006/0255935	A1	11/2006	Scalisi et al.
2003/0229518	A1	12/2003	Abraham-Fuchs et al.	2007/0005029	A1	1/2007	Hopkins et al.
2003/0233071	A1	12/2003	Gillespie et al.	2007/0016152	A1	1/2007	Karpowicz et al.
2003/0236450	A1	12/2003	Kocinski	2007/0032741	A1	2/2007	Hibner et al.
2004/0006492	A1	1/2004	Watanabe	2007/0032762	A1	2/2007	Vogel
2004/0015132	A1	1/2004	Brown	2007/0032763	A1	2/2007	Vogel
				2007/0038044	A1	2/2007	Dobbles et al.
				2007/0052683	A1	3/2007	Knott et al.
				2007/0055209	A1	3/2007	Patel et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0078444	A1	4/2007	Larsson	2009/0048492	A1	2/2009	Rantala et al.
2007/0100403	A1	5/2007	Felice et al.	2009/0048865	A1	2/2009	Breazeale, Jr.
2007/0118096	A1	5/2007	Smith et al.	2009/0082741	A1	3/2009	Hu
2007/0118397	A1	5/2007	Williams et al.	2009/0097623	A1	4/2009	Bharadwaj
2007/0136099	A1	6/2007	Neligh et al.	2009/0099866	A1	4/2009	Newman
2007/0138069	A1	6/2007	Roncadi et al.	2009/0099867	A1	4/2009	Newman
2007/0156186	A1	7/2007	Lee et al.	2009/0101219	A1	4/2009	Martini et al.
2007/0156456	A1	7/2007	McGillin et al.	2009/0112769	A1	4/2009	Dicks et al.
2007/0173708	A9	7/2007	Dobbles et al.	2009/0115663	A1	5/2009	Brown et al.
2007/0179460	A1	8/2007	Adahan	2009/0118591	A1	5/2009	Kim et al.
2007/0180904	A1	8/2007	Gao	2009/0118751	A1	5/2009	Wiener et al.
2007/0197881	A1	8/2007	Wolf et al.	2009/0125055	A1	5/2009	Larkin et al.
2007/0219480	A1	9/2007	Kamen et al.	2009/0125331	A1	5/2009	Pamsgaard et al.
2007/0219826	A1	9/2007	Brodsky et al.	2009/0125389	A1	5/2009	Dunko et al.
2007/0227360	A1	10/2007	Atlas et al.	2009/0136909	A1	5/2009	Asukai et al.
2007/0227537	A1	10/2007	Bemister et al.	2009/0144091	A1	6/2009	Rago
2007/0233022	A1	10/2007	Henley et al.	2009/0157429	A1	6/2009	Lee et al.
2007/0250009	A1	10/2007	Barak	2009/0163774	A1	6/2009	Thatha et al.
2007/0255114	A1	11/2007	Ackermann et al.	2009/0171166	A1	7/2009	Amundson et al.
2007/0255116	A1	11/2007	Mehta et al.	2009/0171288	A1	7/2009	Wheeler
2007/0260226	A1	11/2007	Jaeb et al.	2009/0171289	A1	7/2009	Davis et al.
2007/0271298	A1	11/2007	Juang et al.	2009/0177495	A1	7/2009	Abousy et al.
2007/0276309	A1	11/2007	Xu et al.	2009/0182266	A1	7/2009	Gordon et al.
2007/0282249	A1	12/2007	Quisenberry et al.	2009/0182594	A1	7/2009	Choubey
2008/0004818	A1	1/2008	Zaleski	2009/0187424	A1	7/2009	Grabowski
2008/0009681	A1	1/2008	Al Hussiny	2009/0204434	A1	8/2009	Breazeale, Jr.
2008/0015526	A1	1/2008	Reiner et al.	2009/0204435	A1	8/2009	Gale
2008/0039761	A1	2/2008	Heaton et al.	2009/0205042	A1	8/2009	Zhou et al.
2008/0041401	A1	2/2008	Casola et al.	2009/0206017	A1	8/2009	Rohde et al.
2008/0051708	A1	2/2008	Kumar et al.	2009/0224889	A1	9/2009	Aggarwal et al.
2008/0071209	A1	3/2008	Moubayed et al.	2009/0227910	A1	9/2009	Pedersen et al.
2008/0071216	A1	3/2008	Locke et al.	2009/0248448	A1	10/2009	Zakay et al.
2008/0071234	A1	3/2008	Kelch et al.	2009/0248578	A1*	10/2009	Pollock G06Q 30/06 705/64
2008/0071235	A1	3/2008	Locke et al.	2009/0254362	A1	10/2009	Choubey et al.
2008/0077091	A1	3/2008	Mulligan	2009/0259220	A1	10/2009	Appling et al.
2008/0082040	A1	4/2008	Kubler et al.	2009/0270833	A1	10/2009	DeBelser et al.
2008/0082077	A1	4/2008	Williams	2009/0276008	A1	11/2009	Lee et al.
2008/0086357	A1	4/2008	Choubey et al.	2009/0281464	A1*	11/2009	Cioanta A61B 90/96 601/2
2008/0091175	A1	4/2008	Frikart et al.	2009/0281822	A1	11/2009	Warner et al.
2008/0091659	A1	4/2008	McFaul	2009/0281830	A1	11/2009	McNames et al.
2008/0097550	A1	4/2008	Dicks et al.	2009/0281867	A1	11/2009	Sievenpiper et al.
2008/0119705	A1	5/2008	Patel et al.	2009/0282192	A1	11/2009	Maus et al.
2008/0125697	A1	5/2008	Gao	2009/0292264	A1	11/2009	Hudspeth et al.
2008/0125698	A1	5/2008	Gerg et al.	2009/0299306	A1	12/2009	Buan
2008/0126126	A1	5/2008	Ballai	2009/0326339	A1	12/2009	Horvitz
2008/0140160	A1	6/2008	Goetz et al.	2009/0327102	A1	12/2009	Maniar et al.
2008/0147431	A1	6/2008	Walneck et al.	2010/0001838	A1	1/2010	Miodownik et al.
2008/0167534	A1	7/2008	Young et al.	2010/0010646	A1	1/2010	Drew et al.
2008/0177224	A1	7/2008	Kelly et al.	2010/0017471	A1	1/2010	Brown et al.
2008/0177579	A1	7/2008	Dehaan	2010/0020021	A1	1/2010	Mills et al.
2008/0180268	A1	7/2008	Nissels et al.	2010/0022848	A1	1/2010	Lee et al.
2008/0200868	A1	8/2008	Alberti et al.	2010/0022990	A1	1/2010	Karpowicz et al.
2008/0200905	A1	8/2008	Heaton et al.	2010/0030302	A1	2/2010	Blowers et al.
2008/0200906	A1	8/2008	Sanders et al.	2010/0036333	A1	2/2010	Schenk, III et al.
2008/0201174	A1	8/2008	Ramasubramanian et al.	2010/0042021	A1	2/2010	Hu et al.
2008/0208147	A1	8/2008	Argenta et al.	2010/0042059	A1	2/2010	Pratt et al.
2008/0209357	A1	8/2008	Vasta et al.	2010/0056875	A1	3/2010	Schoenberg et al.
2008/0221396	A1	9/2008	Garces et al.	2010/0069829	A1	3/2010	Hutchinson et al.
2008/0228526	A1	9/2008	Locke et al.	2010/0081971	A1	4/2010	Allison
2008/0234641	A1	9/2008	Locke et al.	2010/0090004	A1	4/2010	Sands et al.
2008/0242945	A1	10/2008	Gugliotti et al.	2010/0106528	A1	4/2010	Brackett et al.
2008/0243035	A1	10/2008	Crunkilton	2010/0113908	A1	5/2010	Vargas et al.
2008/0243096	A1	10/2008	Svedman	2010/0114026	A1	5/2010	Karratt et al.
2008/0249377	A1	10/2008	Molducci et al.	2010/0121257	A1	5/2010	King
2008/0272254	A1	11/2008	Harr et al.	2010/0126268	A1	5/2010	Baily et al.
2008/0300572	A1	12/2008	Rankers et al.	2010/0137775	A1	6/2010	Hu et al.
2008/0307353	A1	12/2008	Molducci et al.	2010/0139120	A1	6/2010	Manz et al.
2008/0312953	A1	12/2008	Claus	2010/0145161	A1	6/2010	Niyato et al.
2008/0319510	A1*	12/2008	Simpson A61N 1/37235 607/59	2010/0145289	A1	6/2010	Lina et al.
2009/0005746	A1	1/2009	Nielsen et al.	2010/0150991	A1	6/2010	Bernstein
2009/0023432	A1	1/2009	MacInnis et al.	2010/0152624	A1	6/2010	Tanis et al.
2009/0037216	A1	2/2009	Bluemler et al.	2010/0168687	A1	7/2010	Yu
2009/0037220	A1	2/2009	Chambers et al.	2010/0169111	A1*	7/2010	Brue G16H 40/67 340/541
2009/0043268	A1	2/2009	Eddy et al.	2010/0169120	A1	7/2010	Herbst et al.
				2010/0191178	A1	7/2010	Ross et al.
				2010/0191199	A1	7/2010	Evans et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0198142	A1	8/2010	Sloan et al.	2011/0288878	A1	11/2011	Blair
2010/0200486	A1	8/2010	Guenther et al.	2011/0290979	A1	12/2011	Henault et al.
2010/0204663	A1	8/2010	Wudyka	2011/0313789	A1	12/2011	Kamen et al.
2010/0211030	A1	8/2010	Turner et al.	2011/0319813	A1	12/2011	Kamen et al.
2010/0222645	A1	9/2010	Nadler et al.	2012/0001762	A1	1/2012	Turner et al.
2010/0228205	A1	9/2010	Hu et al.	2012/0029312	A1	2/2012	Beaudry et al.
2010/0234708	A1	9/2010	Buck et al.	2012/0029313	A1	2/2012	Burdett et al.
2010/0250697	A1	9/2010	Hansen et al.	2012/0032819	A1	2/2012	Chae et al.
2010/0251114	A1	9/2010	Wehba et al.	2012/0035427	A1	2/2012	Friedman et al.
2010/0255876	A1	10/2010	Jordan et al.	2012/0035560	A1	2/2012	Eddy et al.
2010/0268179	A1	10/2010	Kelch et al.	2012/0035561	A1	2/2012	Locke et al.
2010/0274177	A1	10/2010	Rybski et al.	2012/0046624	A1	2/2012	Locke et al.
2010/0280435	A1	11/2010	Raney et al.	2012/0046625	A1	2/2012	Johannison
2010/0280536	A1	11/2010	Hartwell	2012/0071845	A1	3/2012	Hu et al.
2010/0282834	A1	11/2010	Devergne et al.	2012/0077605	A1	3/2012	Nakagaito et al.
2010/0305490	A1	12/2010	Coulthard et al.	2012/0081225	A1	4/2012	Waugh et al.
2010/0305523	A1	12/2010	Vess	2012/0089369	A1	4/2012	Abuzeni et al.
2010/0313958	A1	12/2010	Patel et al.	2012/0123323	A1	5/2012	Kagan et al.
2010/0314517	A1	12/2010	Patzer	2012/0123358	A1	5/2012	Hall et al.
2010/0317933	A1	12/2010	Colman et al.	2012/0123796	A1	5/2012	McFaul
2010/0318043	A1	12/2010	Malhi et al.	2012/0157889	A1	6/2012	Tanis et al.
2010/0318071	A1	12/2010	Wudyka	2012/0157941	A1	6/2012	Luckemeyer et al.
2010/0331673	A1	12/2010	Maschke et al.	2012/0176394	A1	7/2012	Vik et al.
2010/0331741	A9	12/2010	Cioanta et al.	2012/0181405	A1	7/2012	Zlatic et al.
2011/0003610	A1	1/2011	Key et al.	2012/0182143	A1	7/2012	Gaines et al.
2011/0004188	A1	1/2011	Shekalim	2012/0184930	A1	7/2012	Johannison
2011/0006876	A1	1/2011	Moberg et al.	2012/0184932	A1	7/2012	Giezendanner et al.
2011/0009824	A1	1/2011	Yodfat et al.	2012/0191475	A1	7/2012	Pandey
2011/0015585	A1	1/2011	Svedman et al.	2012/0197196	A1	8/2012	Halbert et al.
2011/0015587	A1	1/2011	Tumey et al.	2012/0197580	A1	8/2012	Vij et al.
2011/0015590	A1	1/2011	Svedman et al.	2012/0209228	A1	8/2012	Croizat et al.
2011/0015593	A1	1/2011	Svedman et al.	2012/0212434	A1	8/2012	Bluemler et al.
2011/0021952	A1	1/2011	Vallone	2012/0212455	A1	8/2012	Kloeffel
2011/0028881	A1	2/2011	Basaglia	2012/0215136	A1	8/2012	Schneider et al.
2011/0028882	A1	2/2011	Basaglia	2012/0215455	A1	8/2012	Patil et al.
2011/0028921	A1	2/2011	Hartwell et al.	2012/0220960	A1	8/2012	Ruland
2011/0034861	A1	2/2011	Schaefer	2012/0226247	A1	9/2012	Danei et al.
2011/0038741	A1	2/2011	Lissner et al.	2012/0226768	A1	9/2012	Gaines et al.
2011/0040288	A1	2/2011	Eckstein et al.	2012/0259283	A1	10/2012	Haase
2011/0046521	A1	2/2011	Farrelly	2012/0259651	A1	10/2012	Mallon et al.
2011/0054810	A1	3/2011	Turner et al.	2012/0271256	A1	10/2012	Locke et al.
2011/0063117	A1	3/2011	Turner et al.	2012/0289895	A1	11/2012	Tsoukalis
2011/0066096	A1	3/2011	Svedman	2012/0289913	A1	11/2012	Eckstein et al.
2011/0066110	A1	3/2011	Fathallah et al.	2012/0289914	A1	11/2012	Eckstein et al.
2011/0066123	A1	3/2011	Tout et al.	2012/0290217	A1	11/2012	Shoval et al.
2011/0071415	A1	3/2011	Karwoski et al.	2012/0293322	A1	11/2012	Ray et al.
2011/0071844	A1	3/2011	Cannon et al.	2012/0295566	A1	11/2012	Collins et al.
2011/0073107	A1	3/2011	Rodman et al.	2012/0302976	A1	11/2012	Locke et al.
2011/0073644	A1*	3/2011	Sarkis, Jr. G07F 17/0014 235/382	2012/0310205	A1	12/2012	Lee et al.
2011/0077605	A1	3/2011	Karpowicz et al.	2013/0018355	A1	1/2013	Brand et al.
2011/0092927	A1	4/2011	Wilkes et al.	2013/0019744	A1	1/2013	Hu
2011/0106028	A1	5/2011	Giezendanner et al.	2013/0023719	A1	1/2013	Bennett
2011/0106561	A1	5/2011	Eaton, Jr. et al.	2013/0028788	A1	1/2013	Gronau et al.
2011/0107251	A1	5/2011	Guaitoli et al.	2013/0030394	A1	1/2013	Locke et al.
2011/0112492	A1	5/2011	Bharti et al.	2013/0035615	A1	2/2013	Hsieh
2011/0112857	A1	5/2011	Yurko et al.	2013/0045764	A1	2/2013	Vik et al.
2011/0130712	A1	6/2011	Topaz	2013/0053692	A1	2/2013	Barron et al.
2011/0133948	A1	6/2011	Ervin	2013/0062265	A1	3/2013	Balschat et al.
2011/0137759	A1	6/2011	Wellington et al.	2013/0066285	A1	3/2013	Locke et al.
2011/0145018	A1	6/2011	Fotsch et al.	2013/0066301	A1	3/2013	Locke et al.
2011/0152739	A1	6/2011	Roncadi et al.	2013/0073303	A1	3/2013	Hsu
2011/0173028	A1	7/2011	Bond	2013/0076528	A1	3/2013	Boettner et al.
2011/0184754	A1	7/2011	Park et al.	2013/0087609	A1	4/2013	Nichol et al.
2011/0190703	A1	8/2011	Pratt et al.	2013/0088452	A1	4/2013	Glaser-Seidnitzer et al.
2011/0196321	A1	8/2011	Wudyka	2013/0090613	A1	4/2013	Kelch et al.
2011/0225008	A1	9/2011	Elkhouh et al.	2013/0090949	A1	4/2013	Tibebu
2011/0237981	A1	9/2011	Voss	2013/0102836	A1	4/2013	Millman
2011/0245682	A1	10/2011	Robinson et al.	2013/0103419	A1	4/2013	Beaudry
2011/0246219	A1	10/2011	Smith et al.	2013/0123755	A1	5/2013	Locke et al.
2011/0251569	A1	10/2011	Turner et al.	2013/0124227	A1	5/2013	Ellis
2011/0257572	A1	10/2011	Locke et al.	2013/0133036	A1	5/2013	Wang et al.
2011/0275353	A1	11/2011	Liu	2013/0144227	A1	6/2013	Locke et al.
2011/0285244	A1	11/2011	Lewis et al.	2013/0144230	A1	6/2013	Wu et al.
2011/0288511	A1	11/2011	Locke et al.	2013/0150686	A1	6/2013	Fronterhouse et al.
				2013/0159456	A1	6/2013	Daoud et al.
				2013/0160082	A1	6/2013	Miller
				2013/0165821	A1	6/2013	Freedman et al.
				2013/0165854	A1	6/2013	Sandhu et al.
				2013/0165877	A1	6/2013	Leeson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0169432 A1 7/2013 Ozgul et al.
 2013/0176230 A1 7/2013 Georgiev et al.
 2013/0186405 A1 7/2013 Krzyzanowski et al.
 2013/0190717 A1 7/2013 Dollar et al.
 2013/0190903 A1 7/2013 Balakrishnan et al.
 2013/0196703 A1 8/2013 Masoud et al.
 2013/0198685 A1 8/2013 Bernini et al.
 2013/0204106 A1 8/2013 Bennett
 2013/0204210 A1 8/2013 Pratt et al.
 2013/0211854 A1 8/2013 Wagstaff
 2013/0212168 A1 8/2013 Bonasera et al.
 2013/0214925 A1 8/2013 Weiss
 2013/0218053 A1 8/2013 Kaiser et al.
 2013/0223979 A1 8/2013 Locke et al.
 2013/0226607 A1 8/2013 Woody et al.
 2013/0227128 A1 8/2013 Wagstaff
 2013/0231596 A1 9/2013 Hornbach et al.
 2013/0245387 A1 9/2013 Patel
 2013/0245580 A1 9/2013 Locke et al.
 2013/0253952 A1 9/2013 Burke et al.
 2013/0254717 A1 9/2013 Al-Ali et al.
 2013/0262730 A1 10/2013 Al-Ali et al.
 2013/0267917 A1 10/2013 Pan et al.
 2013/0267918 A1 10/2013 Pan et al.
 2013/0267919 A1 10/2013 Caso et al.
 2013/0268283 A1 10/2013 Vann et al.
 2013/0271556 A1 10/2013 Ross et al.
 2013/0275145 A1 10/2013 Moore et al.
 2013/0285837 A1 10/2013 Uchida
 2013/0289536 A1 10/2013 Croizat et al.
 2013/0293570 A1 11/2013 Dolgos et al.
 2013/0297350 A1 11/2013 Gross et al.
 2013/0303975 A1 11/2013 Gvodas, Jr.
 2013/0310631 A1 11/2013 Lee et al.
 2013/0310726 A1 11/2013 Miller et al.
 2013/0310778 A1 11/2013 Locke et al.
 2013/0317420 A1 11/2013 Wehmeyer
 2013/0317463 A1 11/2013 Yao et al.
 2013/0325508 A1 12/2013 Johnson et al.
 2013/0327326 A1 12/2013 Brennan
 2013/0331822 A1 12/2013 Patel et al.
 2013/0332197 A1 12/2013 Hinkel
 2013/0335233 A1 12/2013 Kamar et al.
 2013/0345524 A1 12/2013 Meyer et al.
 2014/0031884 A1 1/2014 Elghazzawi
 2014/0032231 A1 1/2014 Semen et al.
 2014/0052202 A1 2/2014 Daynes
 2014/0055588 A1 2/2014 Bangera et al.
 2014/0058344 A1 2/2014 Toth
 2014/0100516 A1 4/2014 Hunt et al.
 2014/0108033 A1 4/2014 Akbay et al.
 2014/0108034 A1 4/2014 Akbay et al.
 2014/0108035 A1 4/2014 Akbay et al.
 2014/0114236 A1 4/2014 Gordon
 2014/0114237 A1 4/2014 Gordon
 2014/0129250 A1 5/2014 Daniel et al.
 2014/0136218 A1 5/2014 Bolene et al.
 2014/0148138 A1 5/2014 Chou
 2014/0163490 A1 6/2014 Locke et al.
 2014/0163493 A1 6/2014 Weston et al.
 2014/0194835 A1 7/2014 Ehler
 2014/0236106 A1 8/2014 Locke et al.
 2014/0303551 A1 10/2014 Germain et al.
 2014/0323906 A1 10/2014 Peatfield et al.
 2015/0012290 A1 1/2015 Inciardi et al.
 2015/0025482 A1 1/2015 Begin et al.
 2015/0025486 A1 1/2015 Hu et al.
 2015/0051560 A1 2/2015 Askem
 2015/0073363 A1 3/2015 Kelch et al.
 2015/0094673 A1 4/2015 Pratt et al.
 2015/0094674 A1 4/2015 Pratt et al.
 2015/0133829 A1 5/2015 DeBusk et al.
 2015/0174304 A1 6/2015 Askem et al.
 2016/0080365 A1 3/2016 Baker et al.
 2016/0110507 A1 4/2016 Abbo

2016/0151015 A1 6/2016 Condurso et al.
 2016/0203275 A1 7/2016 Benjamin et al.
 2017/0065837 A1 3/2017 Tanis et al.
 2018/0158545 A1 6/2018 Blomquist
 2018/0233016 A1 8/2018 Daniel et al.
 2018/0233221 A1 8/2018 Blomquist

FOREIGN PATENT DOCUMENTS

CN 201921164 U 8/2011
 CN 102805894 A 12/2012
 CN 102961815 A 3/2013
 CN 104721892 A 6/2015
 DE 102010036405 A1 1/2012
 DE 202014101752 U1 6/2014
 EP 0403294 A1 12/1990
 EP 0526166 A3 2/1994
 EP 0829228 A1 3/1998
 EP 1034734 A1 9/2000
 EP 1064053 A1 1/2001
 EP 0566381 B1 7/2002
 EP 1231965 A2 8/2002
 EP 0809470 B1 10/2002
 EP 1291802 A2 3/2003
 EP 1309960 A1 5/2003
 EP 1176909 A4 7/2003
 EP 0904788 B1 11/2003
 EP 0814864 B1 12/2003
 EP 1407624 A2 4/2004
 EP 1011420 B1 12/2004
 EP 1199046 A3 1/2005
 EP 1495713 A1 1/2005
 EP 1524619 A2 4/2005
 EP 1540557 A2 6/2005
 EP 1566201 A2 8/2005
 EP 1566201 A3 9/2005
 EP 1579367 A2 9/2005
 EP 1587017 A2 10/2005
 EP 1633241 A1 3/2006
 EP 1684146 A2 7/2006
 EP 1702649 A1 9/2006
 EP 1788503 A2 5/2007
 EP 1797918 A1 6/2007
 EP 1839244 A1 10/2007
 EP 1839615 A1 10/2007
 EP 1857950 A2 11/2007
 EP 1870068 A1 12/2007
 EP 1904964 A1 4/2008
 EP 1934852 A1 6/2008
 EP 1975828 A2 10/2008
 EP 1993435 A2 11/2008
 EP 1610861 B1 3/2009
 EP 2038786 A2 3/2009
 EP 2040604 A2 4/2009
 EP 2092470 A2 8/2009
 EP 2146297 A1 1/2010
 EP 2172859 A1 4/2010
 EP 2214552 A1 8/2010
 EP 2218478 A1 8/2010
 EP 2246079 A1 11/2010
 EP 2248545 A1 11/2010
 EP 1668556 B1 2/2011
 EP 2279028 A2 2/2011
 EP 1404213 B1 3/2011
 EP 1247229 B1 4/2011
 EP 1970098 A3 5/2011
 EP 1406540 B1 6/2011
 EP 1812094 B1 8/2011
 EP 2384472 A1 11/2011
 EP 2226002 B1 1/2012
 EP 1610494 B1 3/2012
 EP 1248660 B1 4/2012
 EP 2023800 B1 4/2012
 EP 2451513 A1 5/2012
 EP 1248661 B1 8/2012
 EP 2488977 A1 8/2012
 EP 2503478 A2 9/2012
 EP 2505169 A3 12/2012
 EP 2529765 A2 12/2012

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	2389961	B1	3/2013
EP	2619723	A2	7/2013
EP	1881784	B1	10/2013
EP	2664194	A2	11/2013
EP	2674845	A1	12/2013
EP	2650027	A3	1/2014
EP	1565219	B1	2/2014
EP	2745204	A1	6/2014
EP	2562665	A3	7/2014
EP	2066365	B1	4/2015
EP	2563437	B1	3/2017
EP	2556650	B1	5/2017
EP	2632407	B1	8/2017
EP	2320971	B1	5/2018
EP	2335173	B1	5/2018
EP	2440112	B1	10/2018
EP	3219340	B1	1/2019
EP	3246054	B1	5/2019
GB	2235877	A	3/1991
GB	2279784	A	1/1995
GB	2342584	A	4/2000
GB	2409951	A	7/2005
GB	2436160	A	9/2007
GB	2449400	A	11/2008
GB	2456708	A	7/2009
GB	2423178	B	5/2010
GB	2475091	A	5/2011
GB	2488904	A	9/2012
GB	2446923	B	5/2013
GB	2491946	B	8/2014
JP	H1085288	A	4/1998
JP	2003116796	A	4/2003
JP	2005027798	A	2/2005
JP	2005071314	A	3/2005
JP	2007289481	A	11/2007
WO	WO-9619335	A1	6/1996
WO	WO-9625112	A1	8/1996
WO	WO-9627163	A1	9/1996
WO	WO-9744745	A1	11/1997
WO	WO-9924927	A1	5/1999
WO	WO-9935588	A1	7/1999
WO	WO-9947209	A1	9/1999
WO	WO-9963886	A1	12/1999
WO	WO-0032088	A1	6/2000
WO	WO-0060522	A2	10/2000
WO	WO-0061003	A1	10/2000
WO	WO-0114048	A1	3/2001
WO	WO-0133457	A1	5/2001
WO	WO-0136027	A1	5/2001
WO	WO-0181829	A1	11/2001
WO	WO-0217075	A2	2/2002
WO	WO-0228477	A1	4/2002
WO	WO-0233577	A1	4/2002
WO	WO-02078594	A2	10/2002
WO	WO-02101713	A1	12/2002
WO	WO-02093301	A3	5/2003
WO	WO-03054668	A2	7/2003
WO	WO-03055432	A1	7/2003
WO	WO-03060650	A2	7/2003
WO	WO-03101508	A2	12/2003
WO	WO-2004057514	A2	7/2004
WO	WO-03094090	A3	9/2004
WO	WO-2004074457	A2	9/2004
WO	WO-2004093983	A1	11/2004
WO	WO-2004100779	A1	11/2004
WO	WO-2005022349	A2	3/2005
WO	WO-2005031632	A2	4/2005
WO	WO-2005036447	A2	4/2005
WO	WO-2005045461	A1	5/2005
WO	WO-2005053793	A1	6/2005
WO	WO-2005057466	A2	6/2005
WO	WO-2005101282	A2	10/2005
WO	WO-2005120097	A2	12/2005
WO	WO-2005109297	A3	3/2006
WO	WO-2006021154	A1	3/2006

WO	WO-2006066583	A1	6/2006
WO	WO-2006066585	A2	6/2006
WO	WO-2006071711	A2	7/2006
WO	WO-2006099120	A2	9/2006
WO	WO-2006108858	A1	10/2006
WO	WO-2006111109	A1	10/2006
WO	WO-2007027490	A2	3/2007
WO	WO-2007035646	A2	3/2007
WO	WO-2007056734	A1	5/2007
WO	WO-2007127879	A2	11/2007
WO	WO-2007133478	A2	11/2007
WO	WO-2007137869	A2	12/2007
WO	WO-2008010012	A2	1/2008
WO	WO-2008036344	A1	3/2008
WO	WO-2008036360	A2	3/2008
WO	WO-2008039314	A2	4/2008
WO	WO-2008062382	A2	5/2008
WO	WO-2008104609	A1	9/2008
WO	WO-2008116295	A1	10/2008
WO	WO-2008132215	A1	11/2008
WO	WO-2008157017	A1	12/2008
WO	WO-2009021523	A1	2/2009
WO	WO-2009023432	A3	4/2009
WO	WO-2009047524	A2	4/2009
WO	WO-2009089390	A2	7/2009
WO	WO-2009093116	A1	7/2009
WO	WO-2009117549	A1	9/2009
WO	WO-2009137699	A2	11/2009
WO	WO-2009140669	A2	11/2009
WO	WO-2009151645	A2	12/2009
WO	WO-2010017484	A2	2/2010
WO	WO-2010025166	A1	3/2010
WO	WO-2010025467	A1	3/2010
WO	WO-2010039481	A1	4/2010
WO	WO-2010078558	A1	7/2010
WO	WO-2010085033	A2	7/2010
WO	WO-2010089368	A2	8/2010
WO	WO-2010126668	A1	11/2010
WO	WO-2010132617	A2	11/2010
WO	WO-2010145780	A1	12/2010
WO	WO-2011022330	A1	2/2011
WO	WO-2011023275	A1	3/2011
WO	WO-2011023384	A1	3/2011
WO	WO-2011039676	A2	4/2011
WO	WO-2011046860	A2	4/2011
WO	WO-2011047334	A1	4/2011
WO	WO-2011089270	A1	7/2011
WO	WO-2011107972	A1	9/2011
WO	WO-2011123933	A1	10/2011
WO	WO-2011124388	A1	10/2011
WO	WO-2011137230	A1	11/2011
WO	WO-2012009869	A1	1/2012
WO	WO-2012027342	A1	3/2012
WO	WO-2012027912	A1	3/2012
WO	WO-2012027913	A1	3/2012
WO	WO-2012027914	A1	3/2012
WO	WO-2012027915	A1	3/2012
WO	WO-2012027916	A1	3/2012
WO	WO-2012051278	A1	4/2012
WO	WO-2012054863	A1	4/2012
WO	WO-2012100624	A1	8/2012
WO	WO-2012107430	A1	8/2012
WO	WO-2012127281	A1	9/2012
WO	WO-2012156655	A1	11/2012
WO	WO-2012160164	A1	11/2012
WO	WO-2012172818	A1	12/2012
WO	WO-2013014278	A1	1/2013
WO	WO-2013025815	A1	2/2013
WO	WO-2013026999	A1	2/2013
WO	WO-2013029330	A1	3/2013
WO	WO-2013036853	A2	3/2013
WO	WO-2013054217	A1	4/2013
WO	WO-2013063848	A1	5/2013
WO	WO-2013066775	A1	5/2013
WO	WO-2013078214	A1	5/2013
WO	WO-2013089712	A1	6/2013
WO	WO-2013102855	A1	7/2013
WO	WO-2013109517	A1	7/2013
WO	WO-2013119978	A1	8/2013

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO-2013123022	A1	8/2013
WO	WO-2013126049	A1	8/2013
WO	WO-2013141870	A1	9/2013
WO	WO-2013150025	A1	10/2013
WO	WO-2013175076	A1	11/2013
WO	WO-2013182218	A1	12/2013
WO	WO-2014012802	A1	1/2014
WO	WO-2014151930	A2	9/2014
WO	WO-2014009876	A3	12/2014
WO	WO-2015023515	A1	2/2015
WO	WO-2015091070	A1	6/2015
WO	WO-2015197462	A1	12/2015

OTHER PUBLICATIONS

Brief Communication—Letter from the Proprietor, re the Opposition of European Patent No. EP2627277, dated Apr. 7, 2021, 13 pages.

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. 2627277, dated Feb. 9, 2022, 4 pages.

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. 2630601, dated Sep. 22, 2021, 5 pages.

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. EP2627277, dated Dec. 10, 2021, 4 pages.

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. EP2630601, dated Jan. 19, 2021, 3 pages.

Brief Communication—Letter from the Opponent, re the Opposition of European Patent No. EP3581244, mailed on Jun. 22, 2022, 5 pages.

Brief Communication—Letter from the Proprietor for Opposition proceedings of the European Patent No. 2630601, mailed on Oct. 16, 2020, 43 pages.

Brief Communication—Letter from the Proprietor for Reply to the notice(s) of opposition of European Patent No. 2630601, mailed on Oct. 29, 2020, 15 pages.

Brief Communication—Letter from the Proprietor of the Patent, re the Opposition for Simmons & Simmons for European Patent No. 2630601, dated Sep. 21, 2021, 2 pages.

Brief Communication—Letter from the Proprietor of the Patent, re the Opposition of European Patent No. EP3581244, dated May 13, 2022, 47 pages.

Brief Communication—Letter from the Proprietor, re the Opposition of European Patent No. EP2627277, dated Dec. 9, 2021, 2 pages.

Brief communication in opposition procedure—time limit, letter from the Proprietor for European Patent No. 2630601, mailed on Oct. 27, 2020, 2 pages.

Brief Communication of Letter from the Opponent for Opposition against of the European Patent No. 2630601, mailed on Nov. 11, 2020, 6 pages.

Cinterion., “Cinterion PHS8-P 3G HSPA+,” retrieved from http://www.cinterion.com/tl_files/cinterion/downloads/cinterion_datasheet_PHS8_web.pdf, 2012, 2 pages.

Communication of a Notice of Opposition including Statement of Facts and Arguments for European Patent No. 3581244, dated Dec. 22, 2021, 26 pages.

Communication of further notices of opposition pursuant to Rule 79(2) EPC for European Application No. 11776953.9, mailed on Sep. 1, 2020, 2 pages.

Communication to the parties concerning termination of opposition proceedings for European Patent No. 2627277, dated May 25, 2022, 1 page.

Decision of Rejection for Japanese Patent Application No. 2015254568, mailed on Jul. 3, 2017, 4 pages.

Discussion between Lesley Fenton and Kevin Cordina regarding Opponent’s name, mailed on Dec. 12, 2019, 3 pages.

Discussion between Mr. Kevin Cordina and Mr. Nadeem Bridi regarding Opponent’s name, mailed on Dec. 11, 2019, 2 pages.

Extract from the Register of European Patents No. EP2731564 on Jan. 12, 2021, 4 pages.

First Examination Report for Australian Application No. 2011316883, mailed on Feb. 29, 2016, 3 pages.

Forwarding of submissions to parties of a letter of the Opponent for European Patent No. EP2630601, dated Oct. 12, 2022, 17 pages.

Forwarding of submissions to parties of a letter of the patent proprietor for European Patent No. EP2630601, dated Oct. 14, 2022, 11 pages.

Grounds for the Decision, the Opposition of European Patent No. 2630601, mailed Feb. 17, 2022, 77 pages.

Hartmann Vivano., “Vivano—Product Application Description,” retrieved from <http://www.vivanosystem.info/20809.php>, accessed on Feb. 28, 2013, 3 pages.

Huntleigh Healthcare, “Negative Pressure Positive Outcomes,” WoundASSIST TNP Console and Canister Brochure, 2007, 6 pages.

Information about the Result of Oral Proceedings, the Opposition of European Patent No. 2630601, dated Nov. 18, 2021, 4 pages.

International Preliminary Report on Patentability Application No. PCT/US2011/057337, mailed on May 2, 2013, 8 pages.

International Preliminary Report on Patentability for Application No. PCT/US2011/055937, mailed on Apr. 25, 2013, 8 pages.

International Preliminary Report on Patentability for Application No. PCT/US2014/026692, mailed on Sep. 24, 2015, 16 pages.

International Preliminary Report on Patentability for International Application No. PCT/US2011/057332, mailed May 2, 2013, 8 pages.

International Search Report and Written Opinion for Application No. PCT/US2011/055937, mailed on Dec. 23, 2011, 11 pages.

International Search Report and Written Opinion for Application No. PCT/US2011/057332, mailed on Mar. 23, 2012, 8 pages.

International Search Report and Written Opinion for Application No. PCT/US2011/057337, mailed on Feb. 23, 2012, 9 pages.

International Search Report and Written Opinion for Application No. PCT/US2014/026692, mailed on Mar. 2, 2015, 26 pages.

Invitation to Pay and Partial International Search Report for Application No. PCT/US2014/026692, mailed on Sep. 26, 2014, 9 pages.

Japanese Office Action, re JP Application No. 2015-254568, dated Feb. 21, 2017, 6 pages.

Letter from the Proprietor for Opposition proceedings of the European Patent No. 2630601, mailed on Dec. 7, 2020, 4 pages.

Notice of Communication of amended entries concerning the representative (R. 143(1)(h) EPC) and enclosed letter from the proprietor of the patent dated Jan. 11, 2021 for European Patent No. 2627277, mailed on Jan. 20, 2021, 21 pages.

Notice of Decision to Discontinue the Opposition Proceedings for European Patent No. 2627277, dated Feb. 10, 2022, 3 pages.

Notice of Opposition—Statement of Facts and Evidence for the European Patent No. 2731564, mailed on Jan. 22, 2020, 12 pages.

Notice of Opposition for the European Patent No. 2630601, mailed on May 7, 2020, 37 pages.

Notice of Reasons for Rejection for Japanese Patent Application No. 2013533968, mailed Jul. 14, 2015, 6 pages.

Oddsson L.I.E., et al., “A Robotic Home Telehealth Platform System for Treatment Adherence, Social Assistance and Companionship—an Overview,” 31st Annual international Conference of the IEEE EMBS, Sep. 2009, pp. 6437-6440.

Office Action mailed Dec. 11, 2017 for Canadian Application No. 2814657, 4 pages.

Office Action mailed Nov. 14, 2017 for Australian Application No. 2017201192, 3 pages.

Office Action mailed Jul. 19, 2017 for Canadian Application No. 2815474, 5 pages.

Office Action mailed Jan. 9, 2015 for Australian Application No. 2011316599, 5 pages.

Opponent’s Statement of Facts and Arguments for the European Patent No. 2627277, mailed on Aug. 20, 2020, 5 pages.

Patentee’s letter for Opposition proceedings of the European Patent No. 2731564, dated Jun. 16, 2020, 5 pages.

(56)

References Cited**OTHER PUBLICATIONS**

Proprietor's Written Submission in Preparation for the Oral Proceedings for the Opposition of European Patent No. 2627277, dated Feb. 3, 2022, 2 pages.

Second Examination Report for Australian Application No. 2011316883, mailed on Feb. 2, 2017, 5 pages.

State on Oath of Kevin Cronin submitted in the Opposition against European Patent No. 2630601, signed on Nov. 4, 2020, 1 page.

State on Oath of Nadeem Bridi submitted in the Opposition against European Patent No. 3246054, signed on Dec. 14, 2020, 1 page.

Statement of Grounds of Appeal for the European Patent No. 2630601, mailed on Jun. 8, 2022, 63 pages.

Statement of Grounds of Appeal for the European Patent No. 2630601, mailed on Jun. 14, 2022, 4 pages.

Summons to Attend Oral Proceedings Pursuant to Rule 115(1) EPC for European Patent No. 2627277, mailed on Apr. 28, 2021, 10 pages.

Summons to Attend Oral Proceedings Pursuant to Rule 115(1) EPC for European Patent No. 3581244, mailed on Nov. 29, 2022, 16 pages.

Summons to Attend Oral Proceedings pursuant to rule 115(1) EPC for Patent No. 2630601, mailed on Jan. 18, 2021, 18 pages.

Termination of the Opposition Proceedings with Maintenance of European Patent No. 2627277, dated May 20, 2022, 1 page.

Brief Communication—Letter from the Opponent of Apr. 12, 2023, for the European Patent No. 3581244, dated Apr. 17, 2023, 4 pages.

Brief Communication—Letter from the Proprietor of the Patent of Apr. 6, 2023, for the European Patent No. 3581244, dated Apr. 13, 2023, 33 pages.

Communication of the Board of Appeal pursuant to Article 15(1) of the Rules of Procedure filed in the Opposition against European Patent No. 2630601, mailed on Aug. 2, 2024, 9 pages.

Decision to maintain the European patent in amended form (Art. 101(3)(a) EPC) for European Patent No. 3581244, mailed on Dec. 7, 2023, 1 page.

Maintenance of the Patent with the Documents specified in the Final Decision filed in the Opposition against European Patent No. 2630601, mailed on Sep. 18, 2024, 1 page.

Maintenance of the patent with the documents specified in the final decision, re the opposition of European patent No. EP3581244, mailed on Oct. 4, 2023, 1 page.

Notification of Cancellation Postponing of Oral Proceedings filed in the Opposition against European Patent No. 2630601, mailed on Sep. 13, 2024, 1 page.

Transmittal of Decision Summons for the Opposition of European Patent No. 3581244, mailed on Jun. 23, 2023, 66 pages.

* cited by examiner

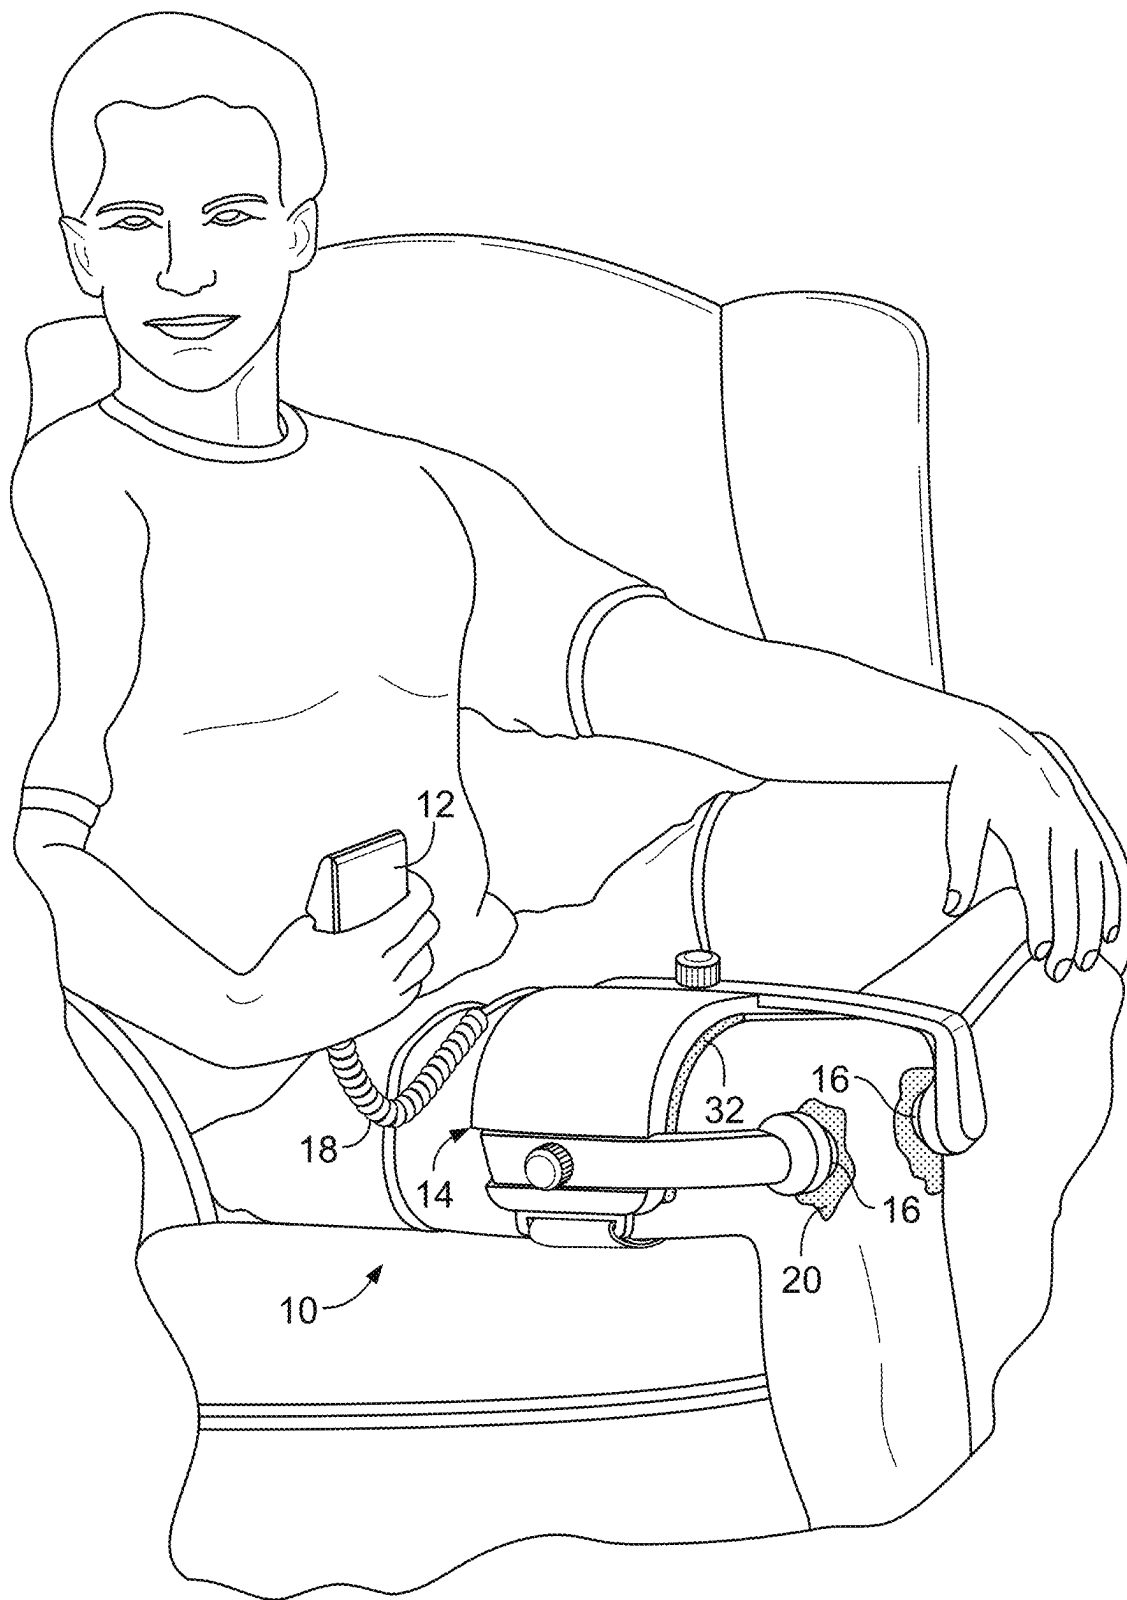


FIG. 1

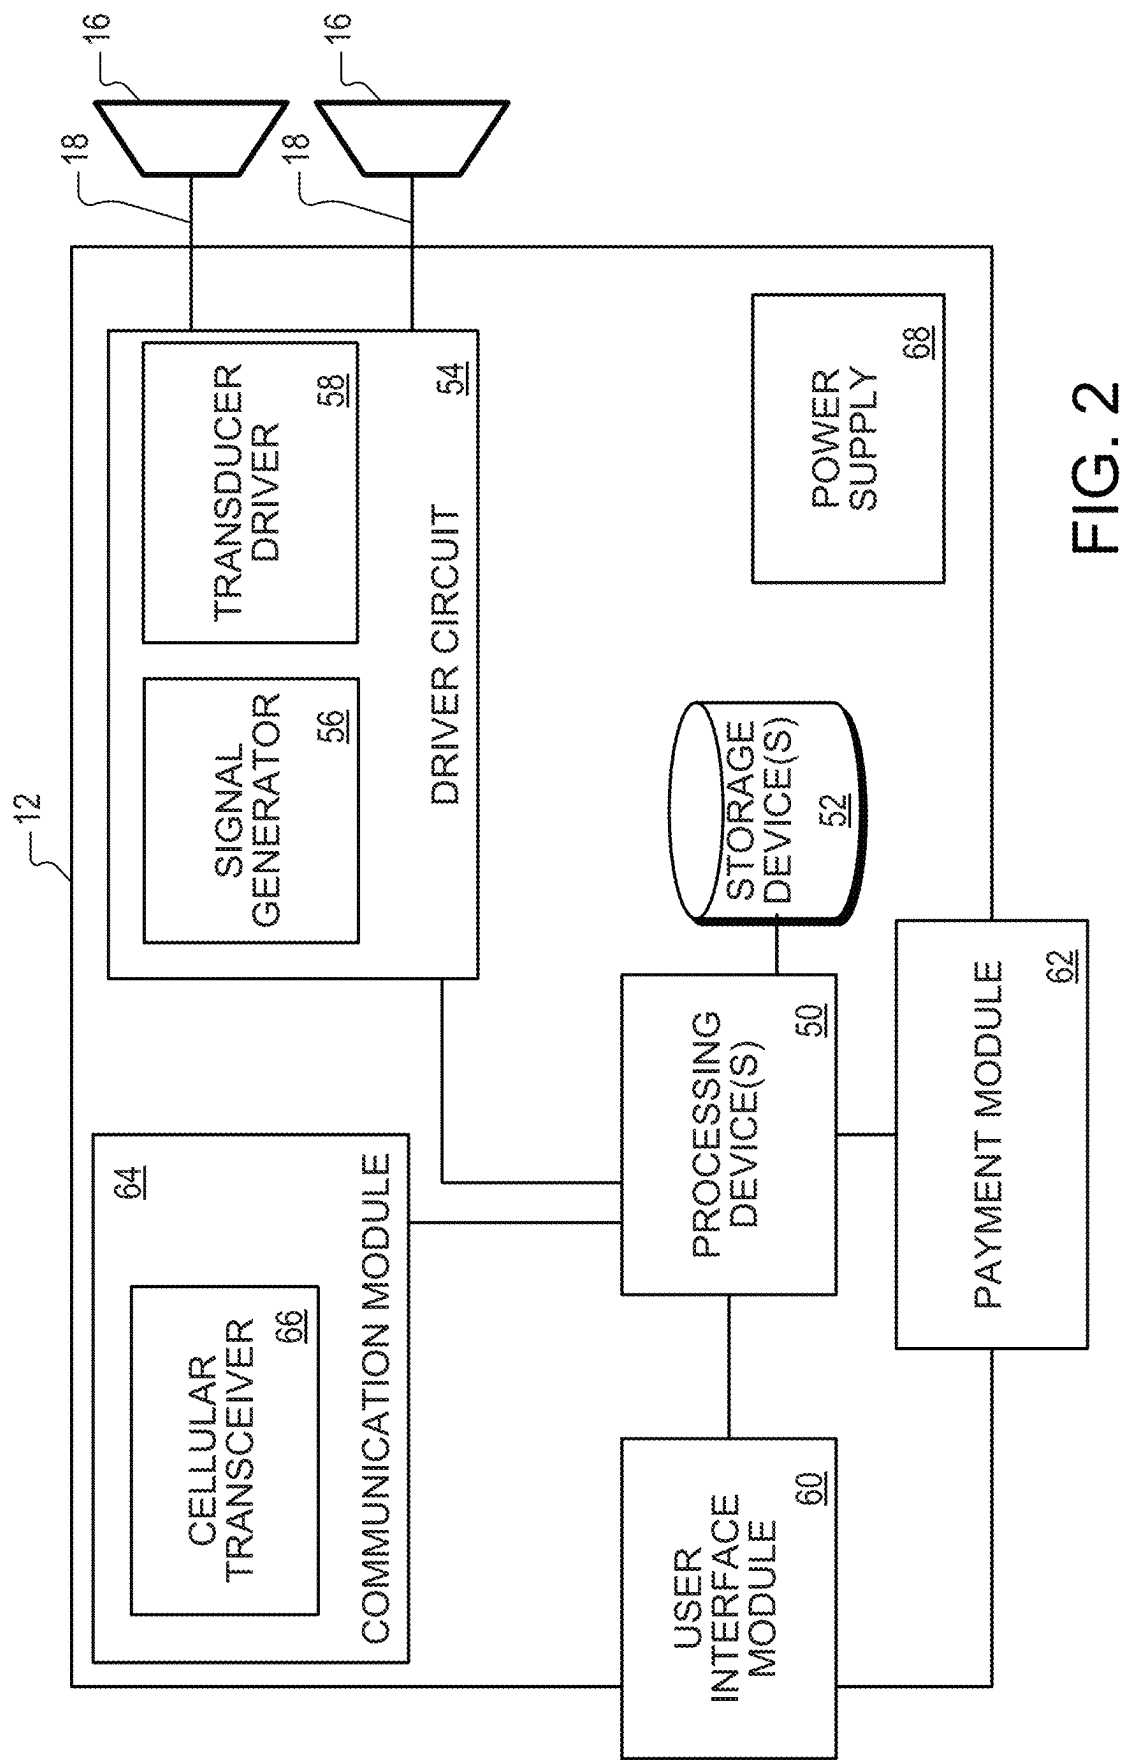


FIG. 2

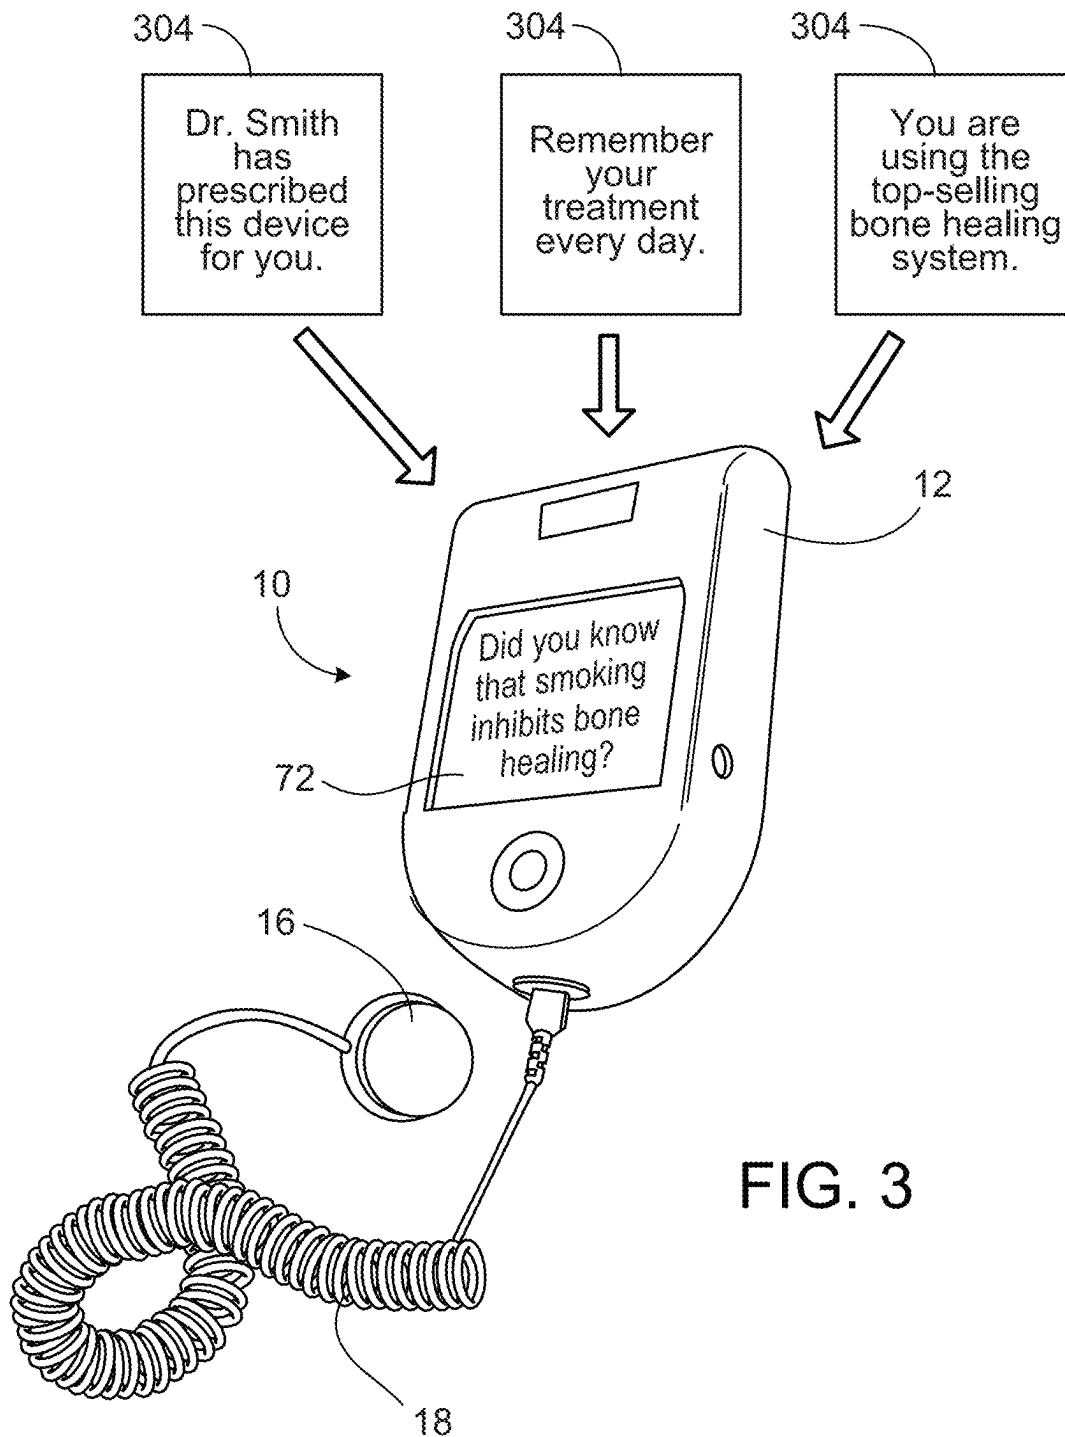


FIG. 3

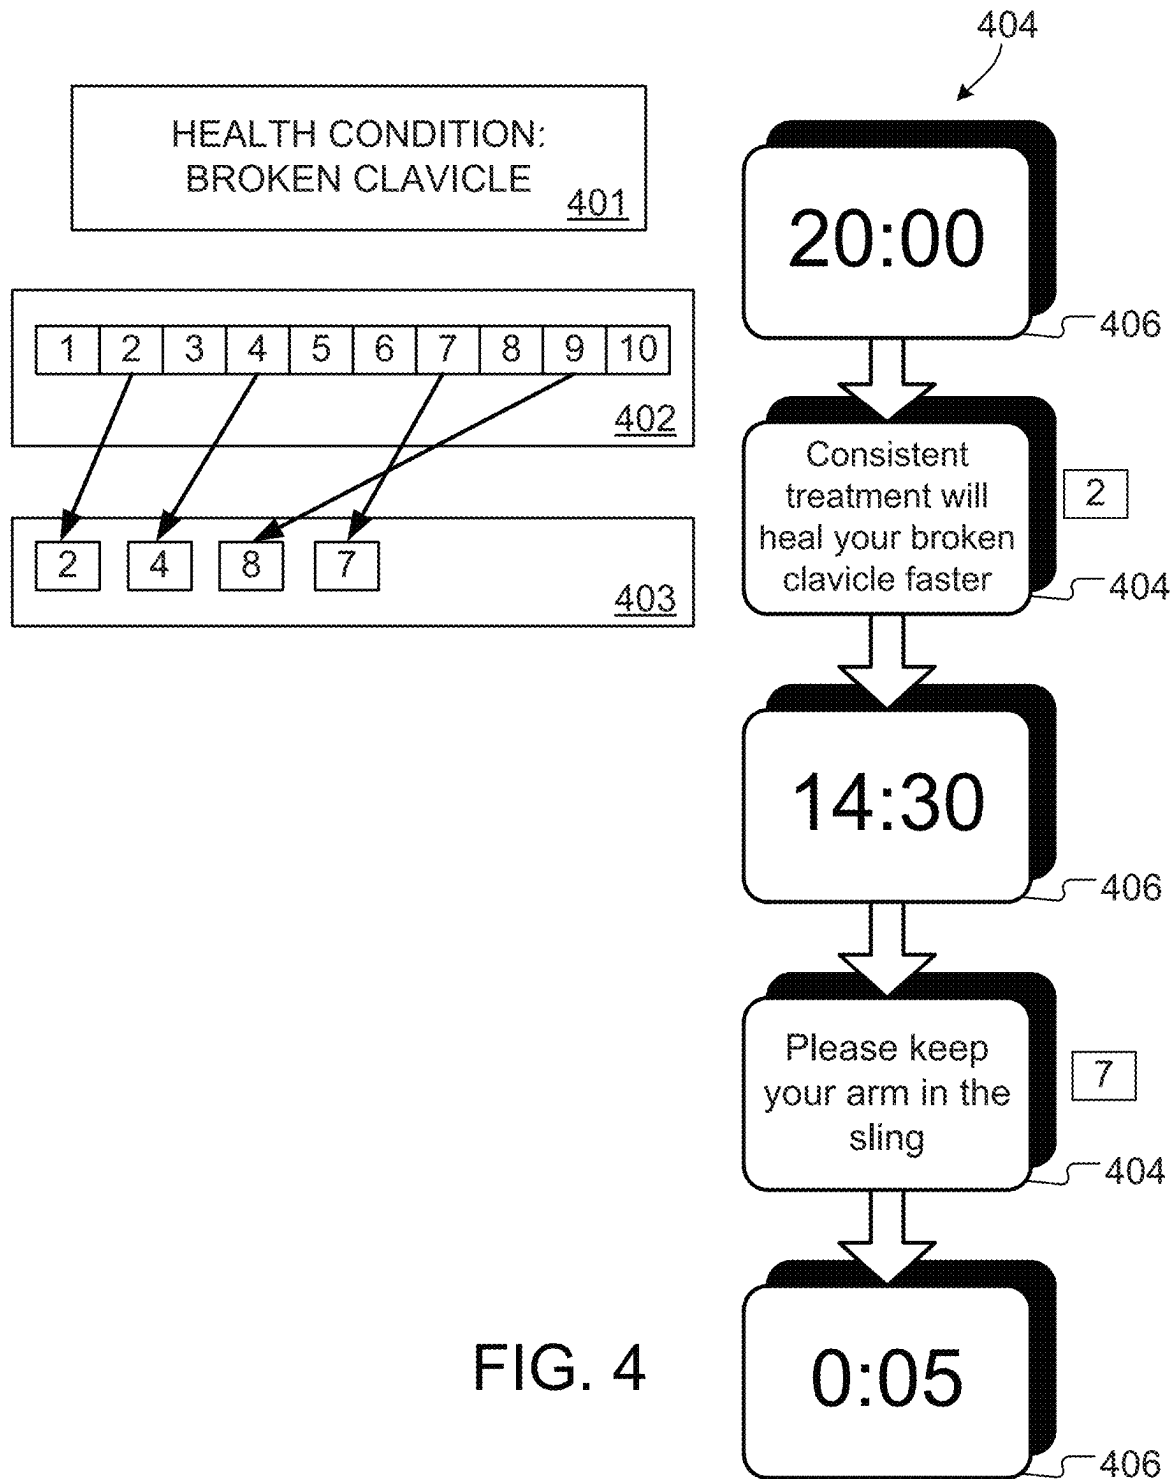


FIG. 4

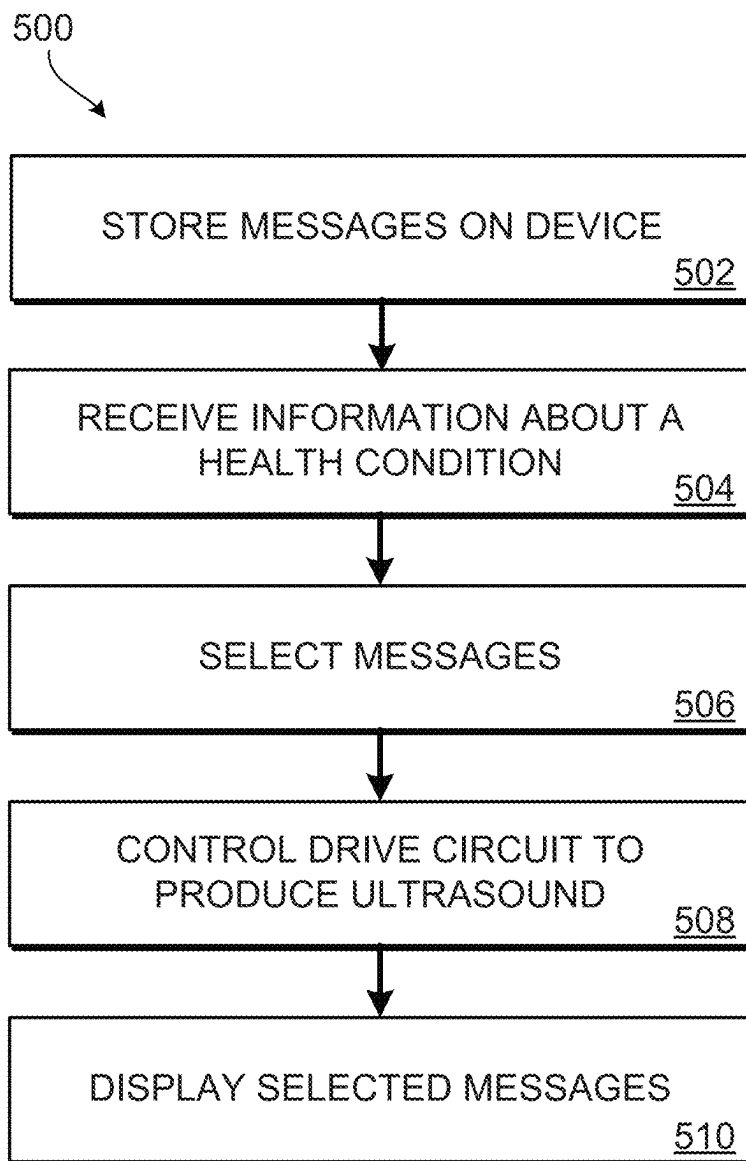


FIG. 5

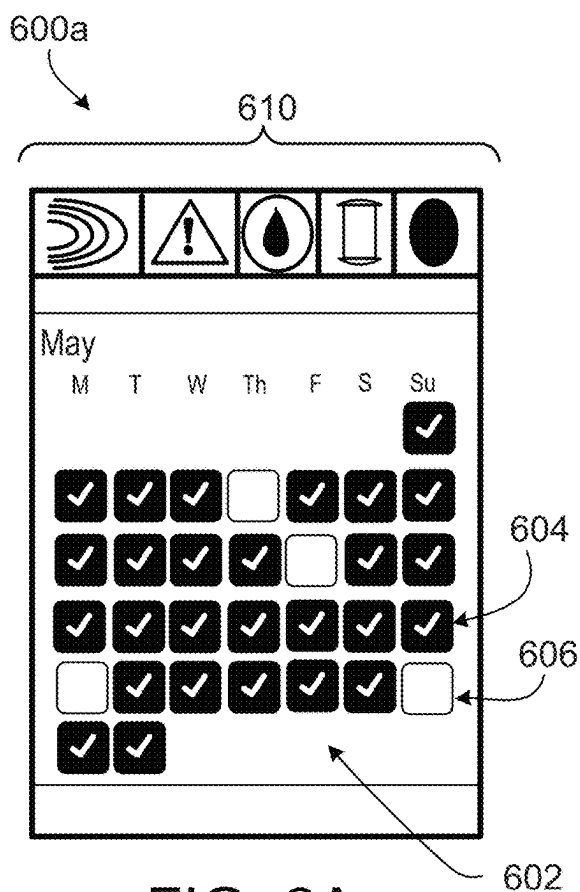


FIG. 6A

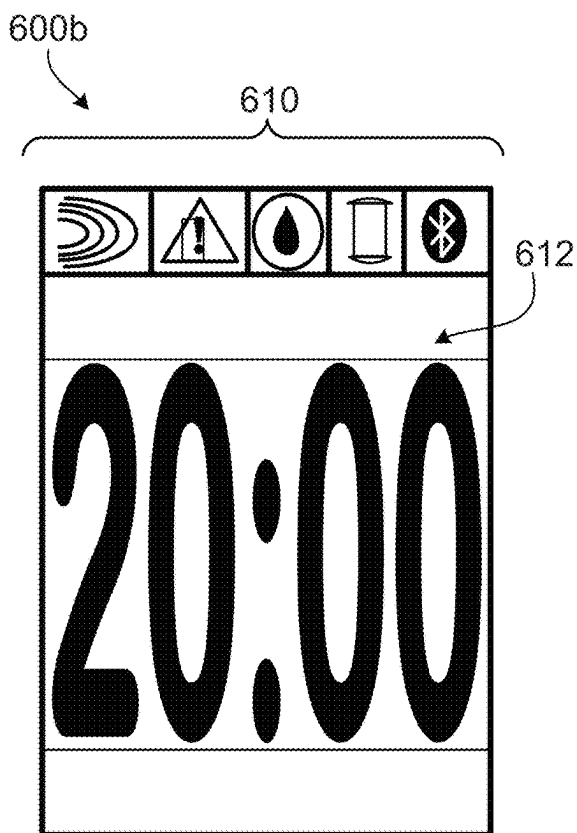


FIG. 6B

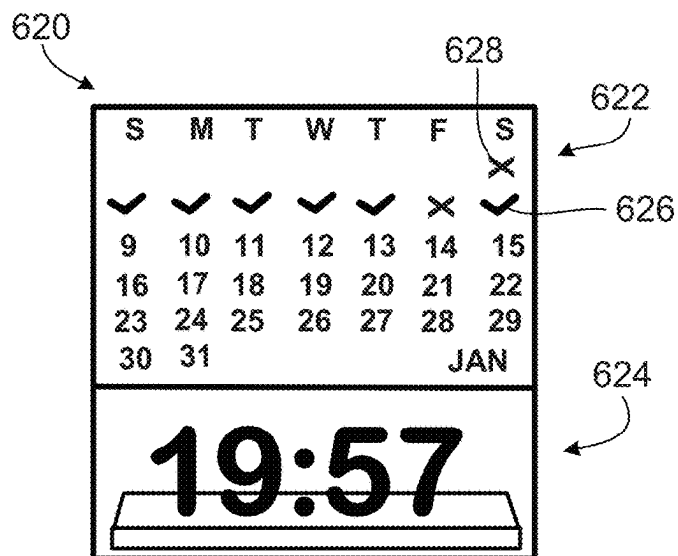


FIG. 6C

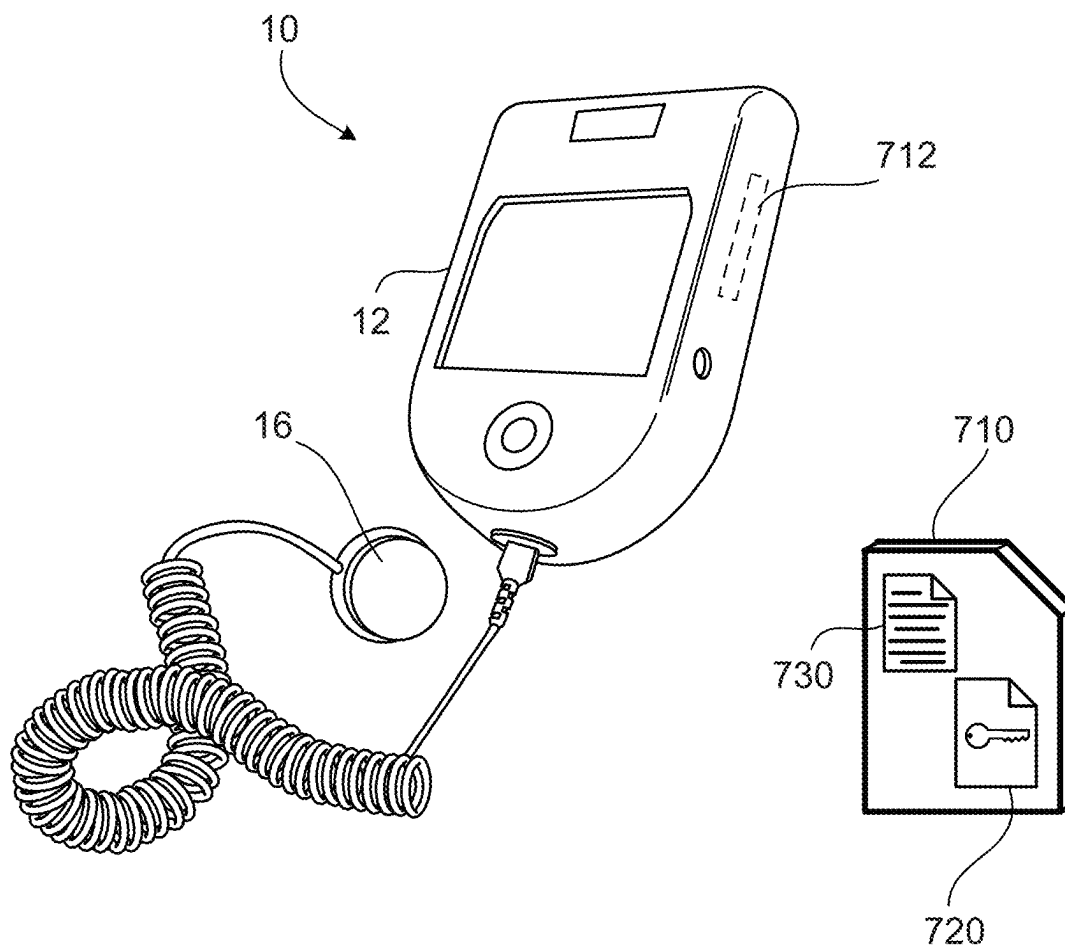


FIG. 7

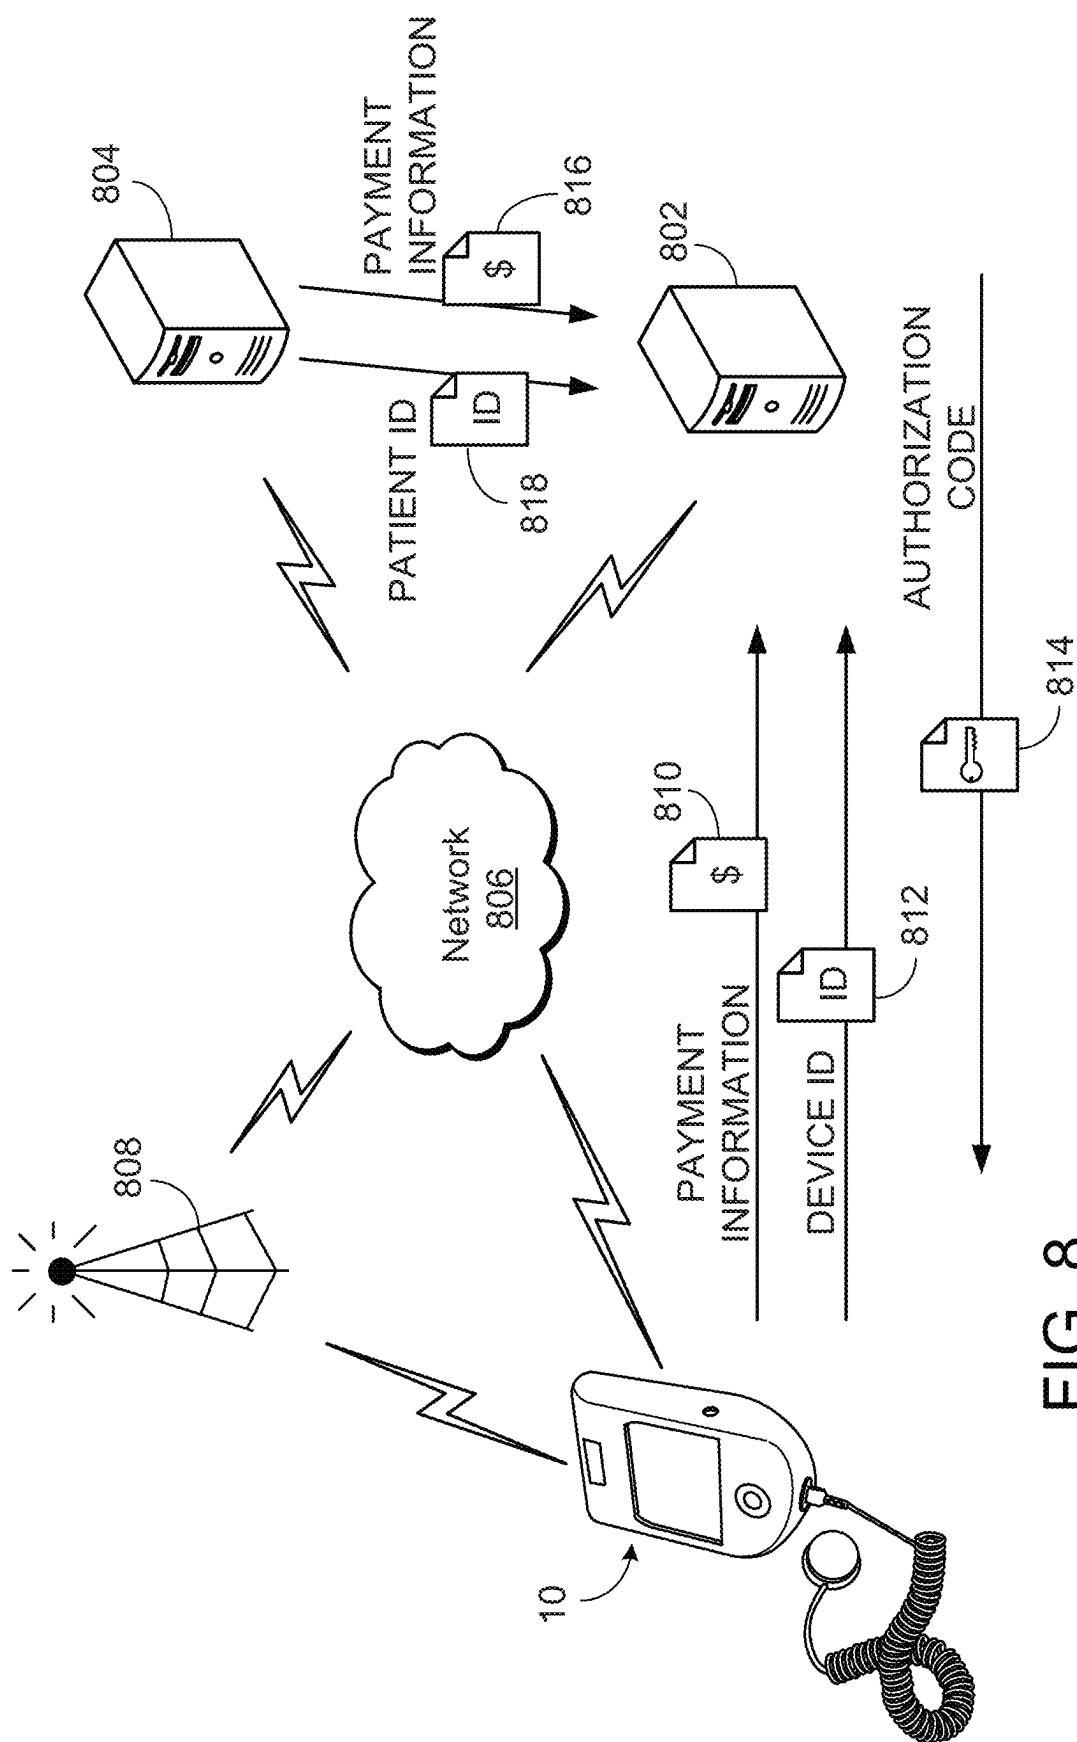


FIG. 8

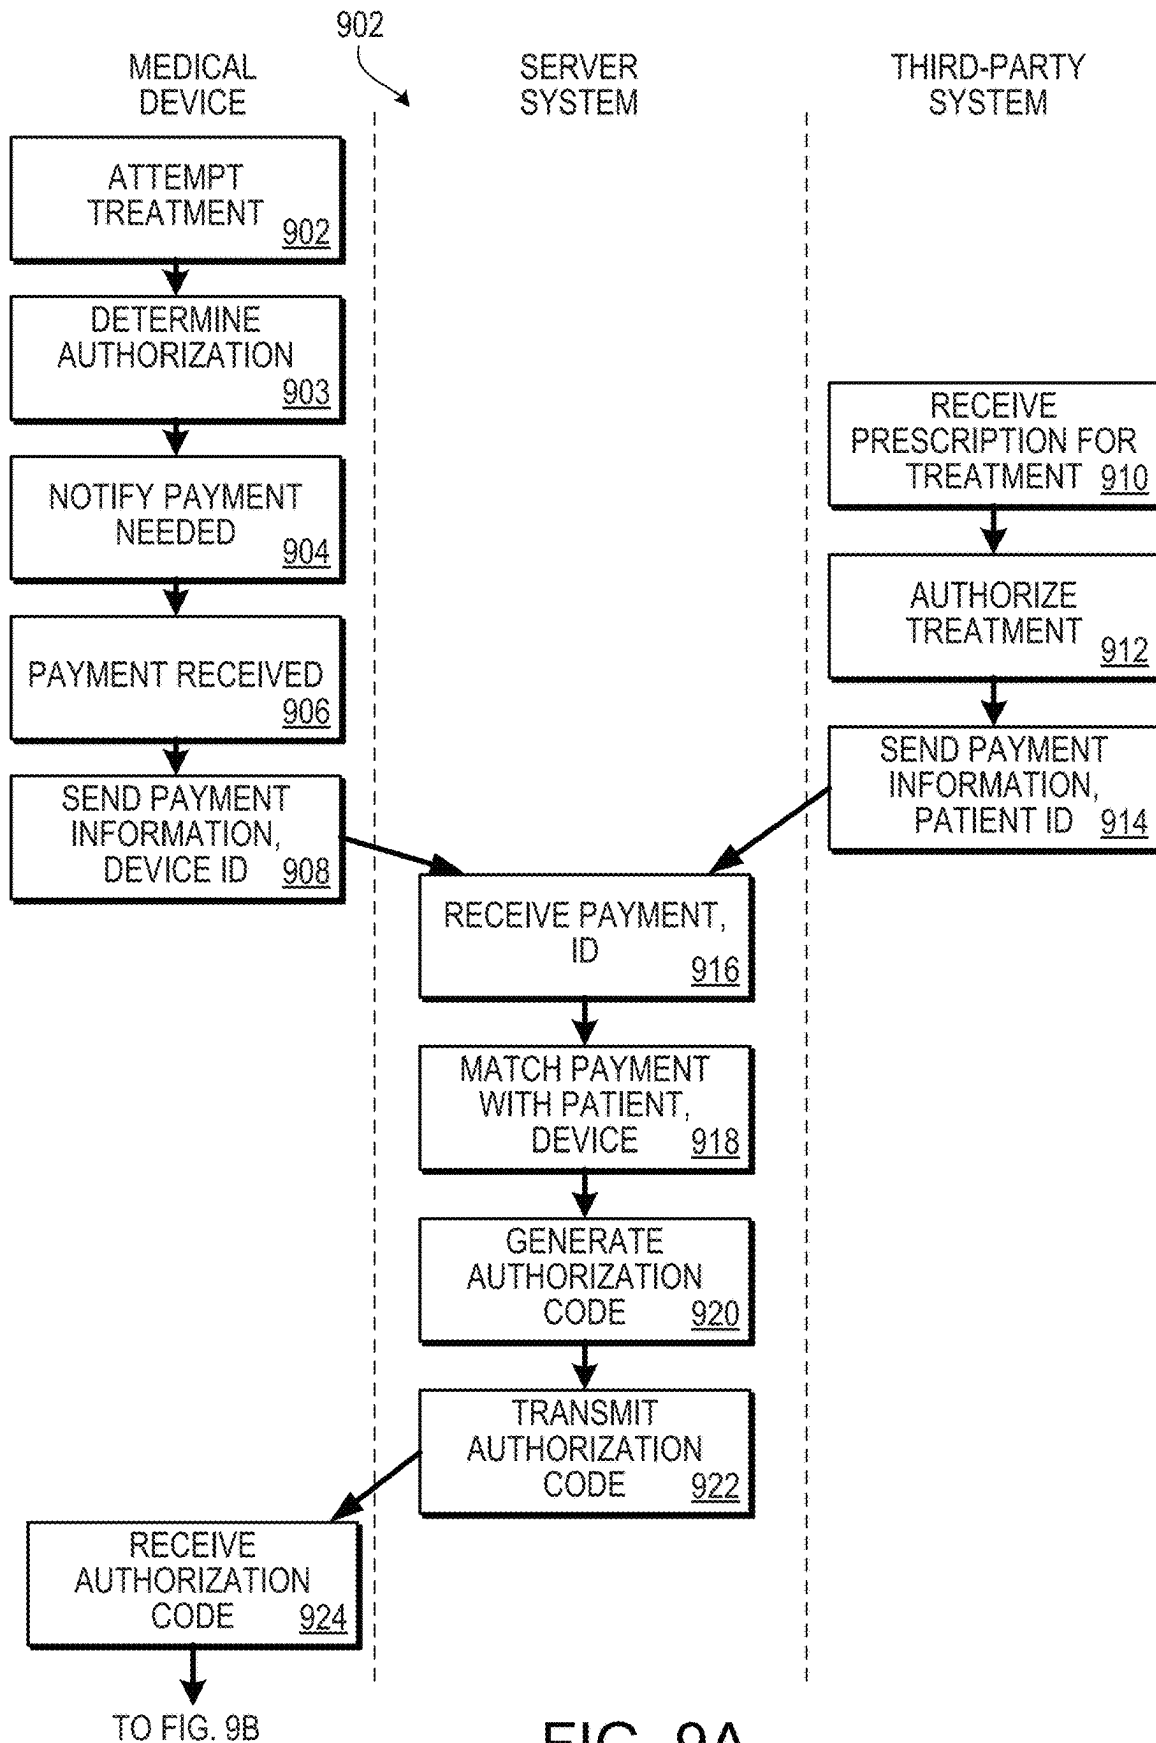


FIG. 9A

FROM FIG. 9A

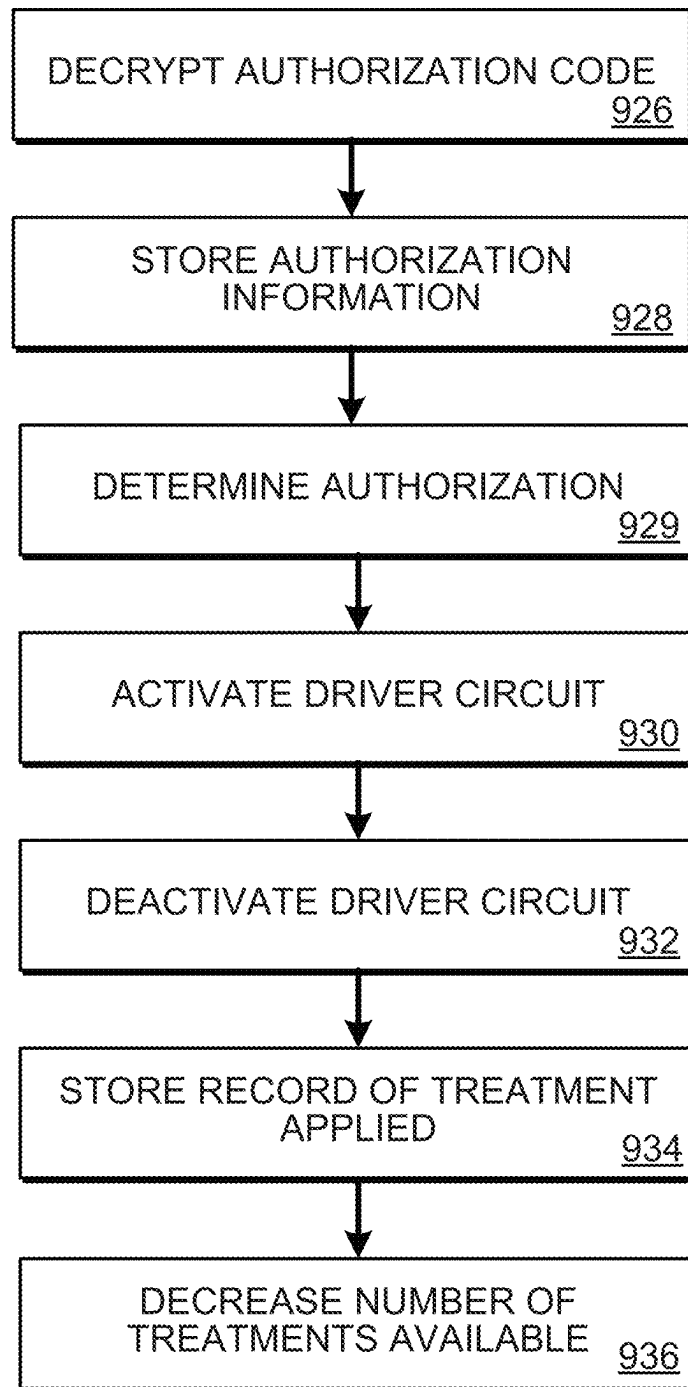
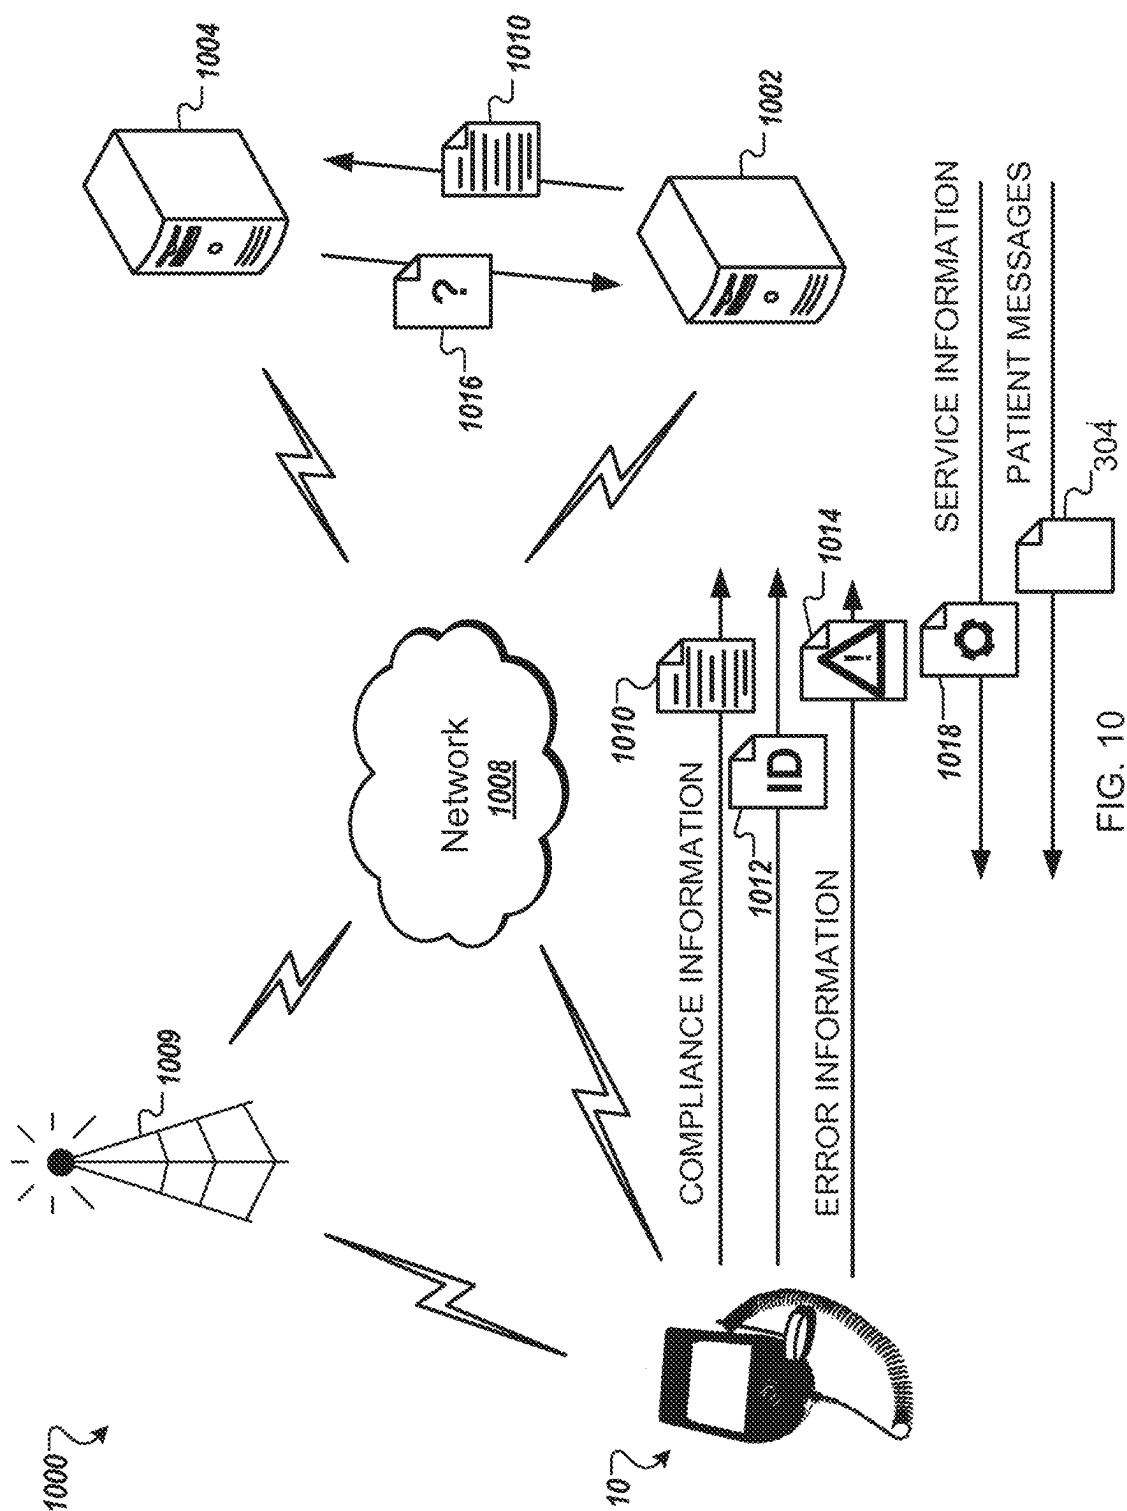


FIG. 9B



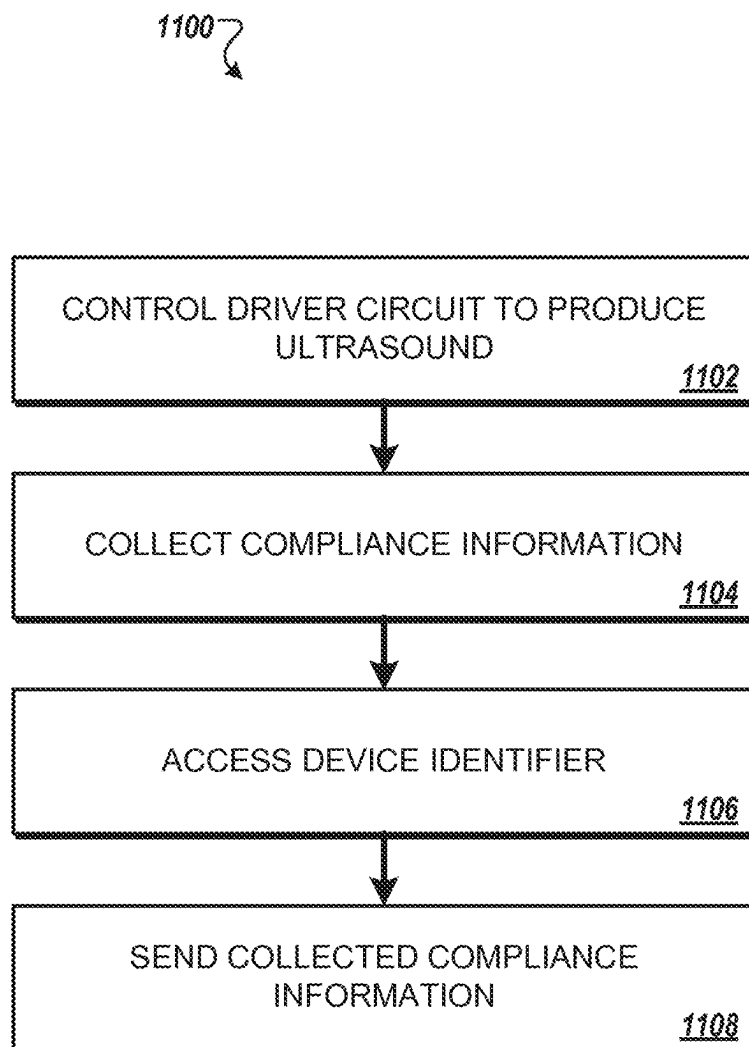


FIG 11

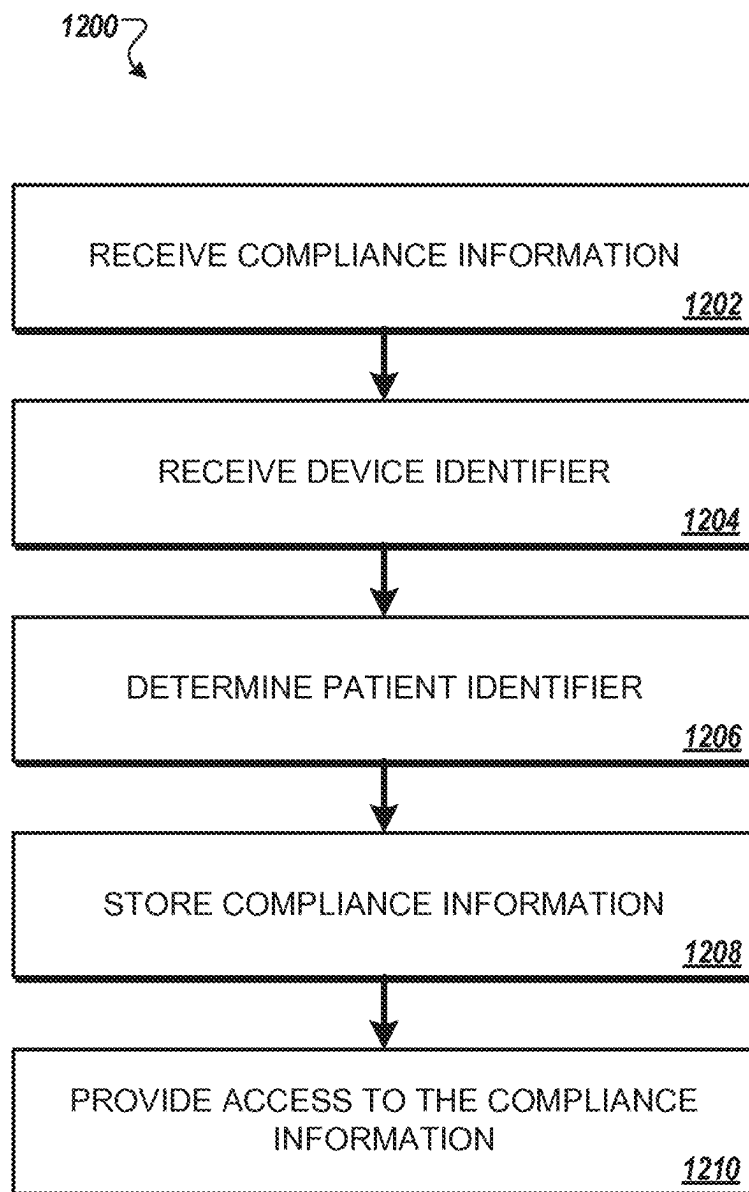
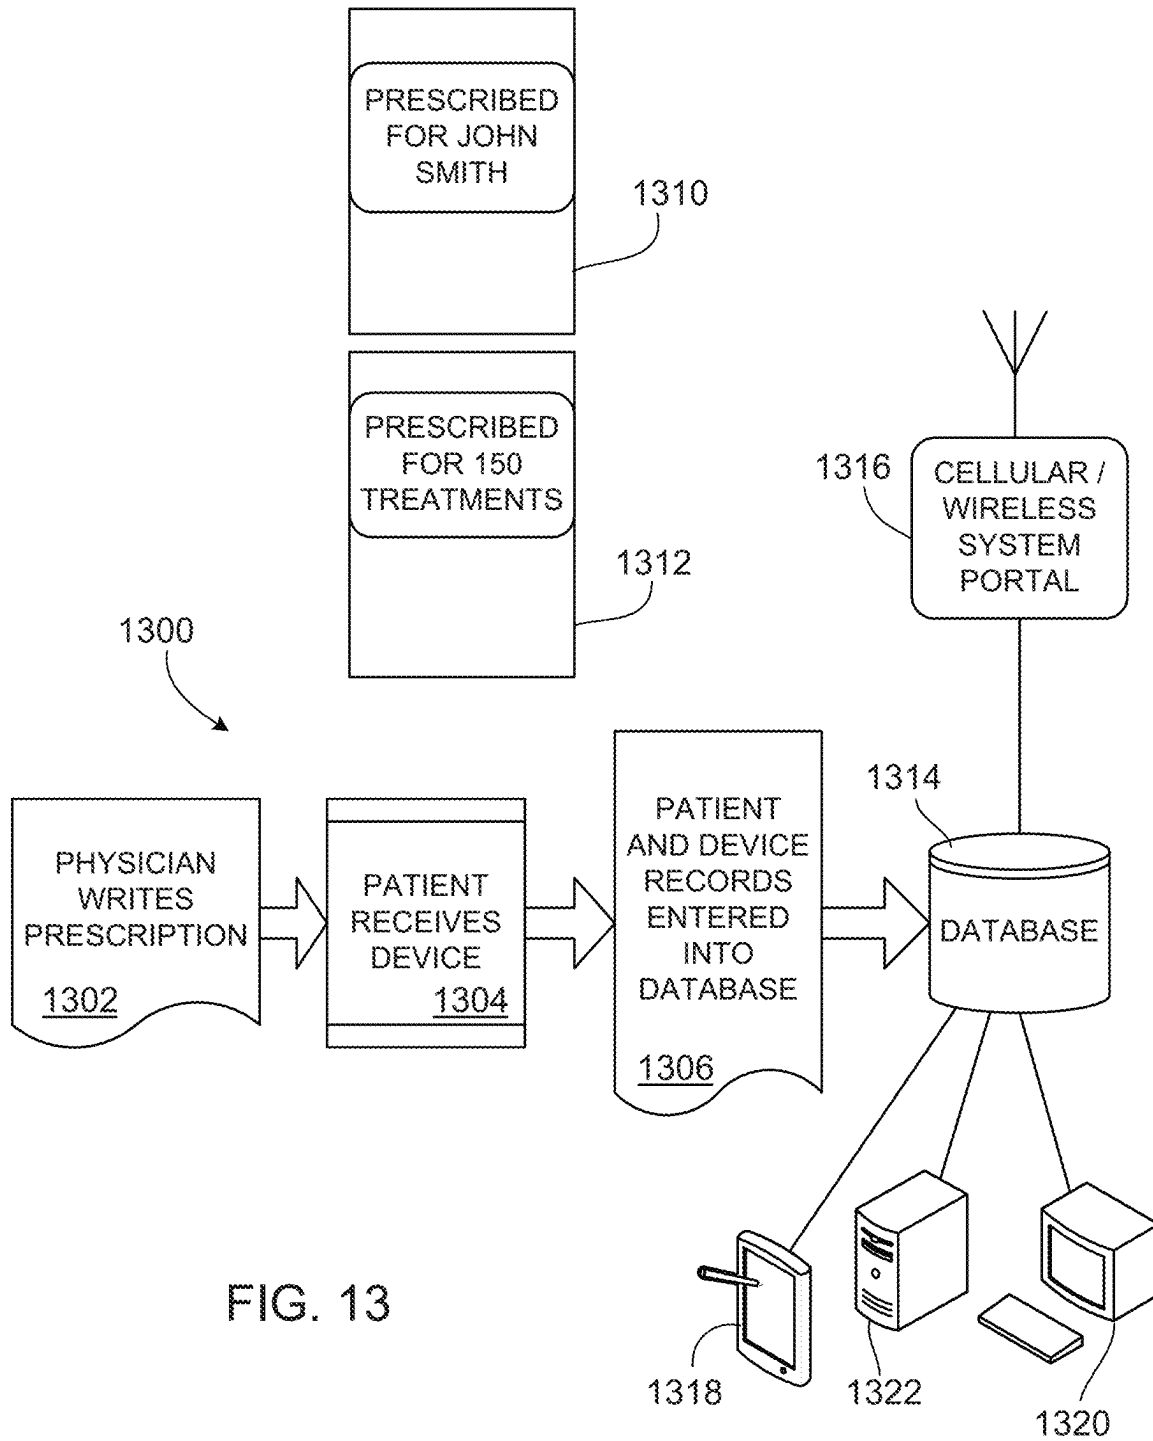


FIG 12



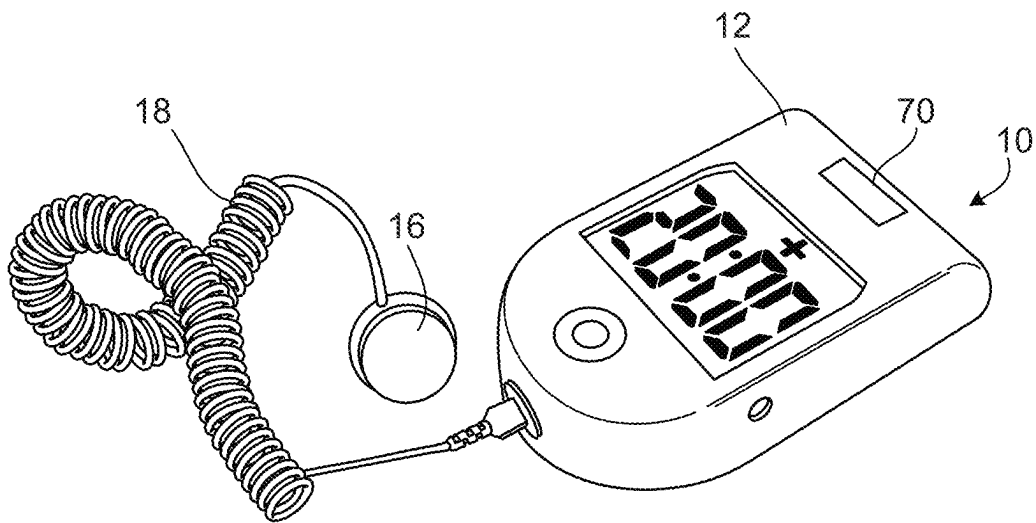


FIG. 14

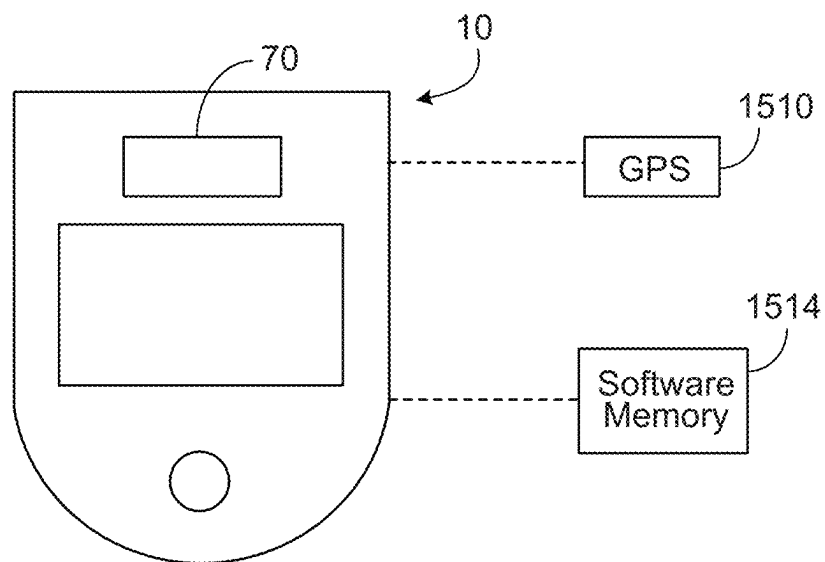


FIG. 15

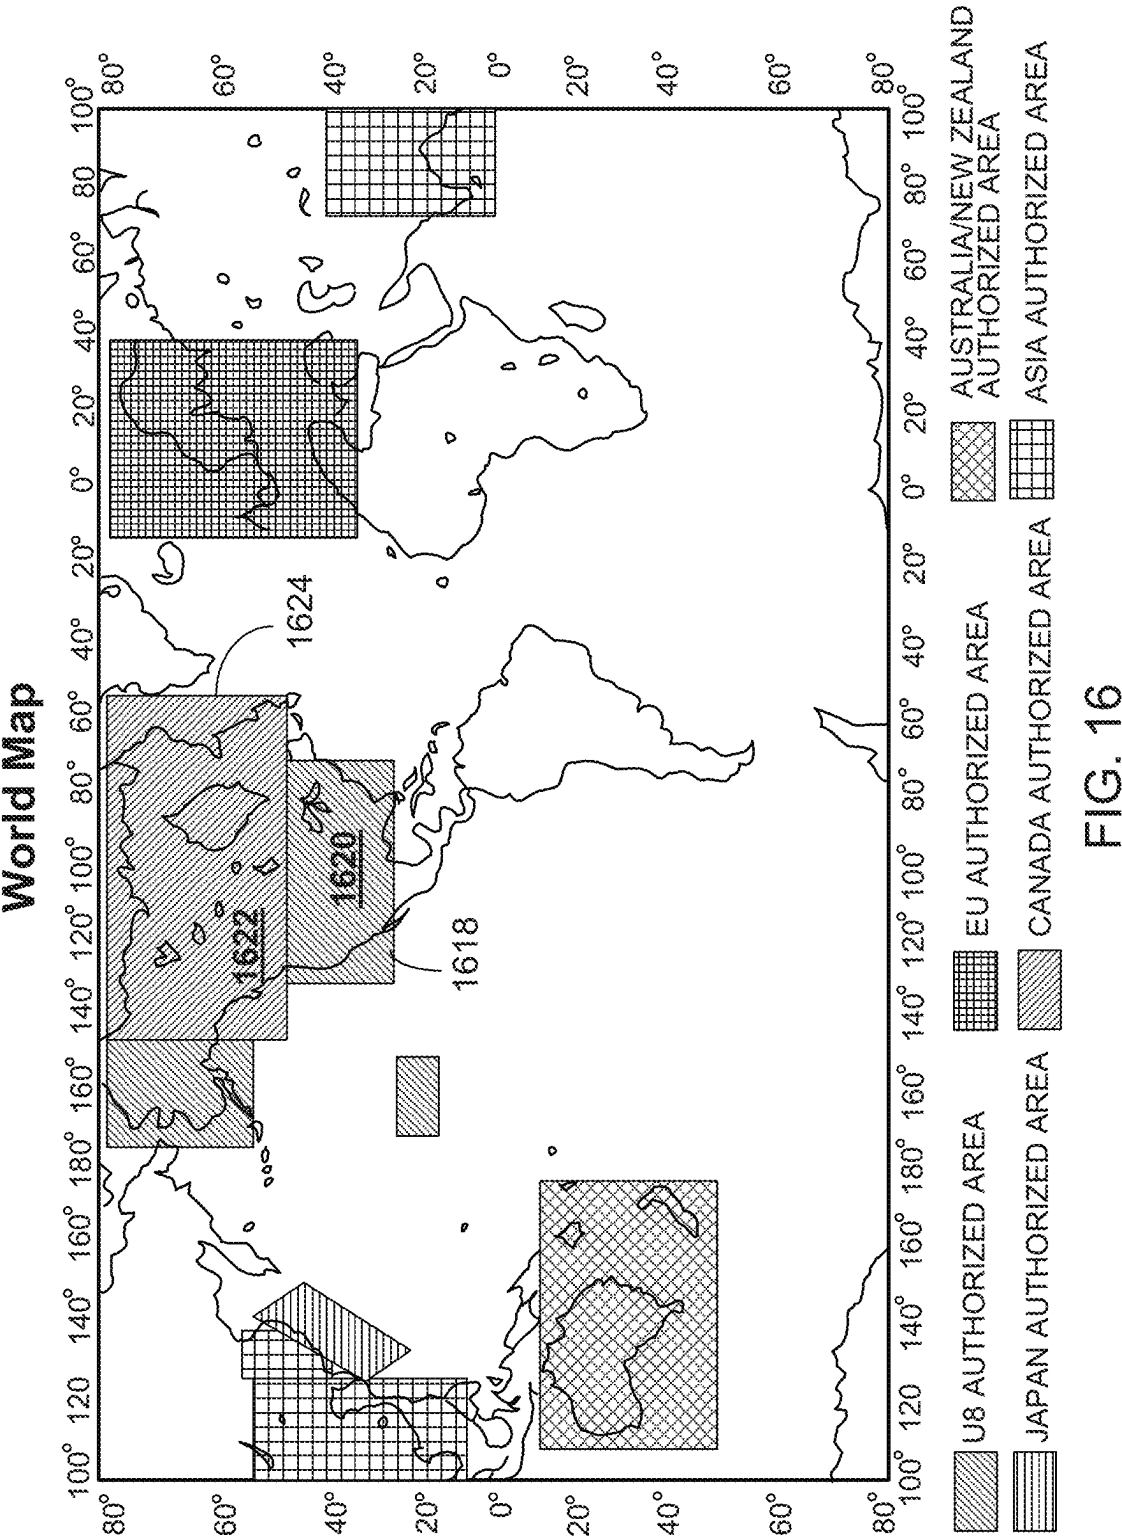


FIG. 16

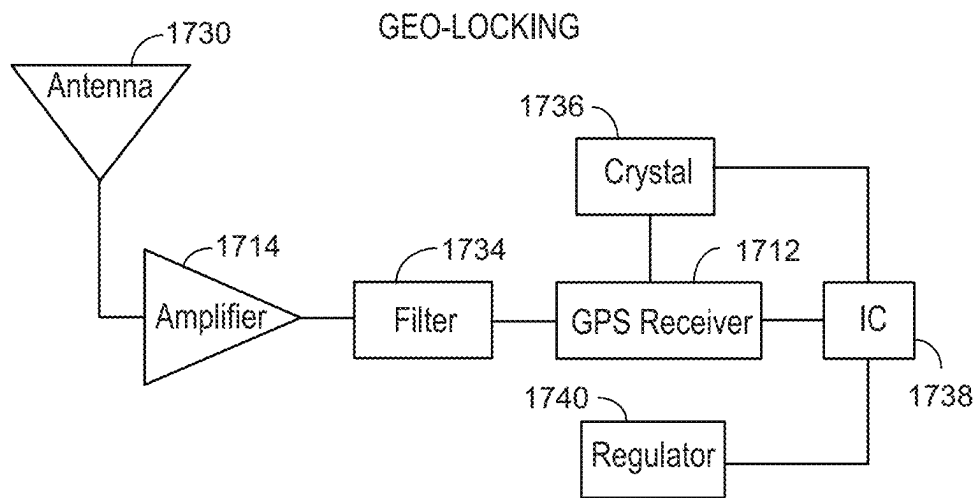


FIG. 17

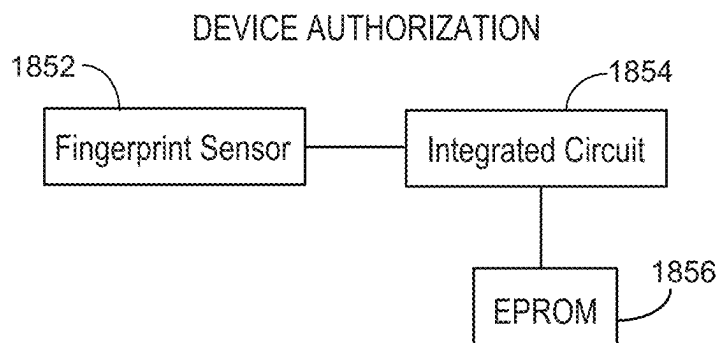


FIG. 18



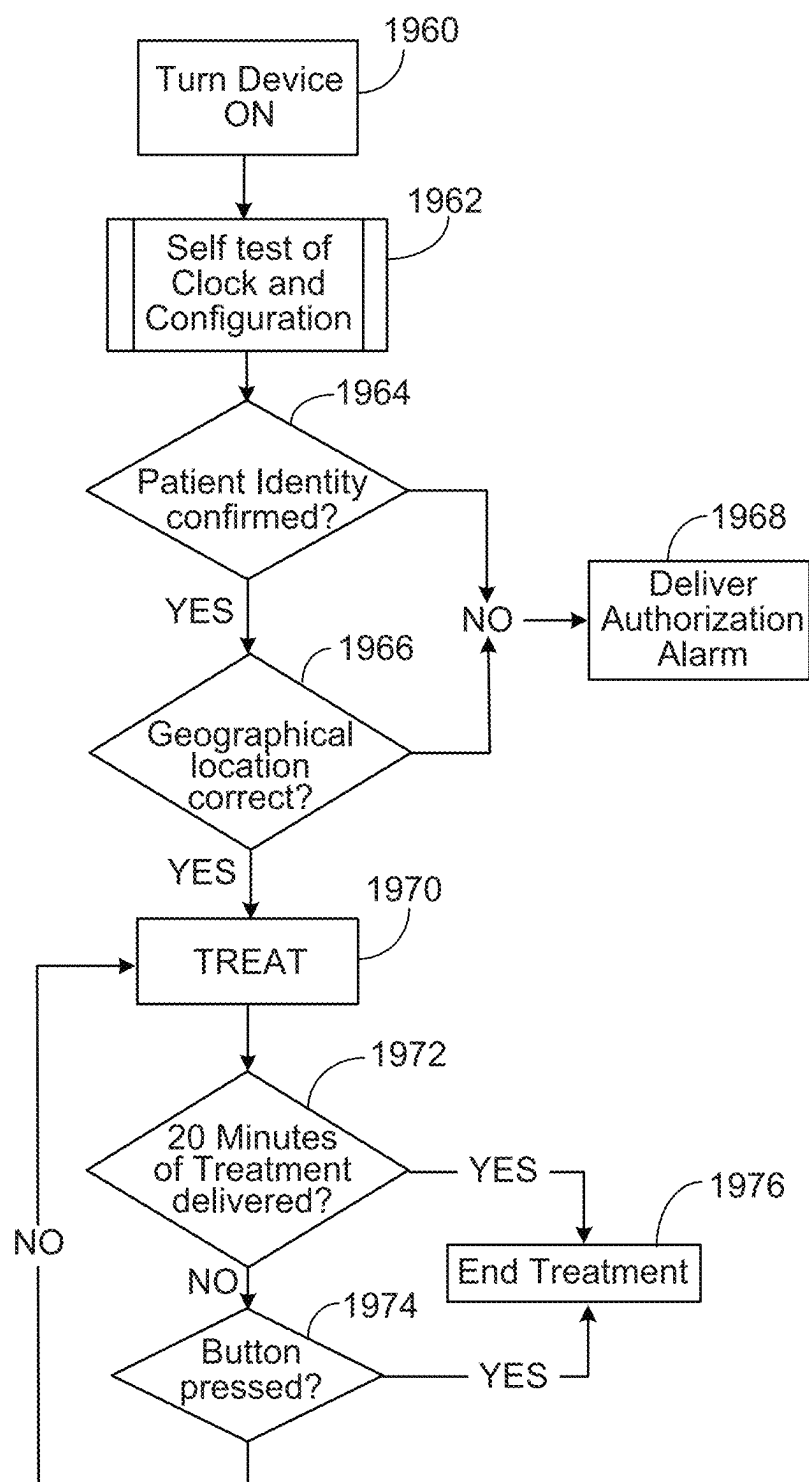


FIG. 19

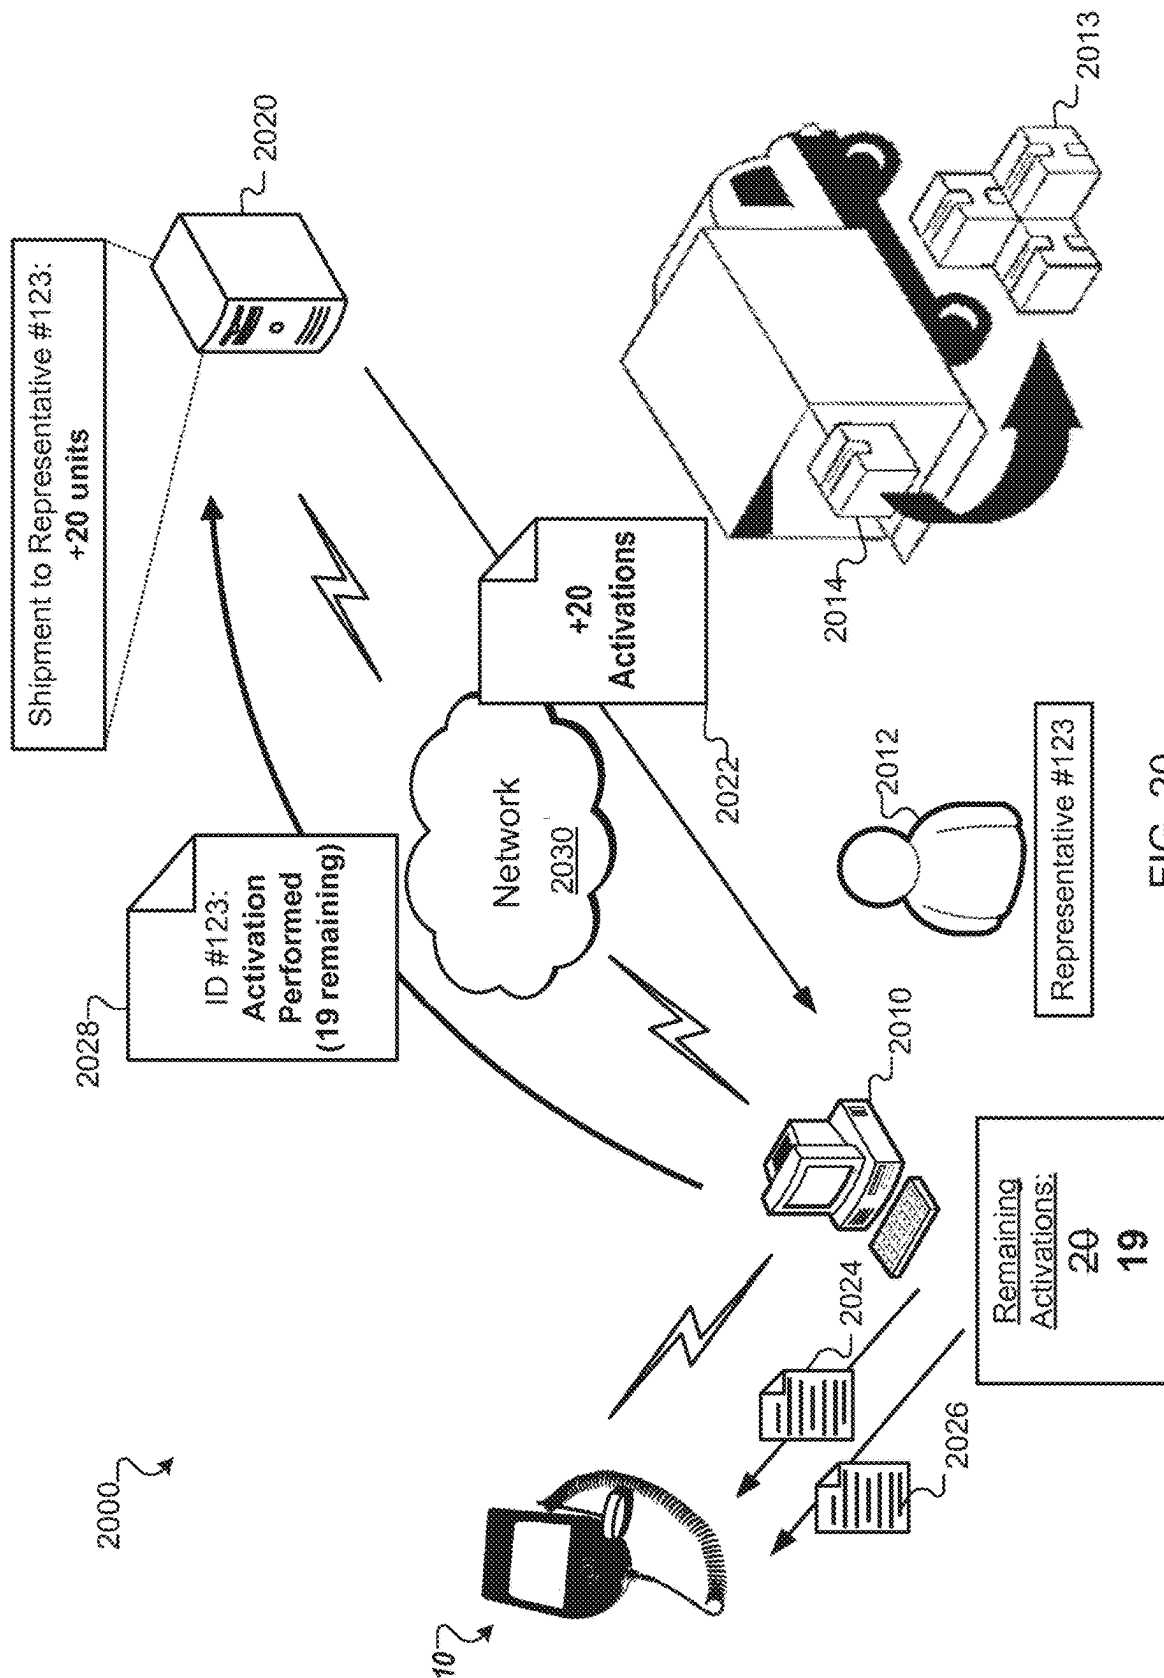

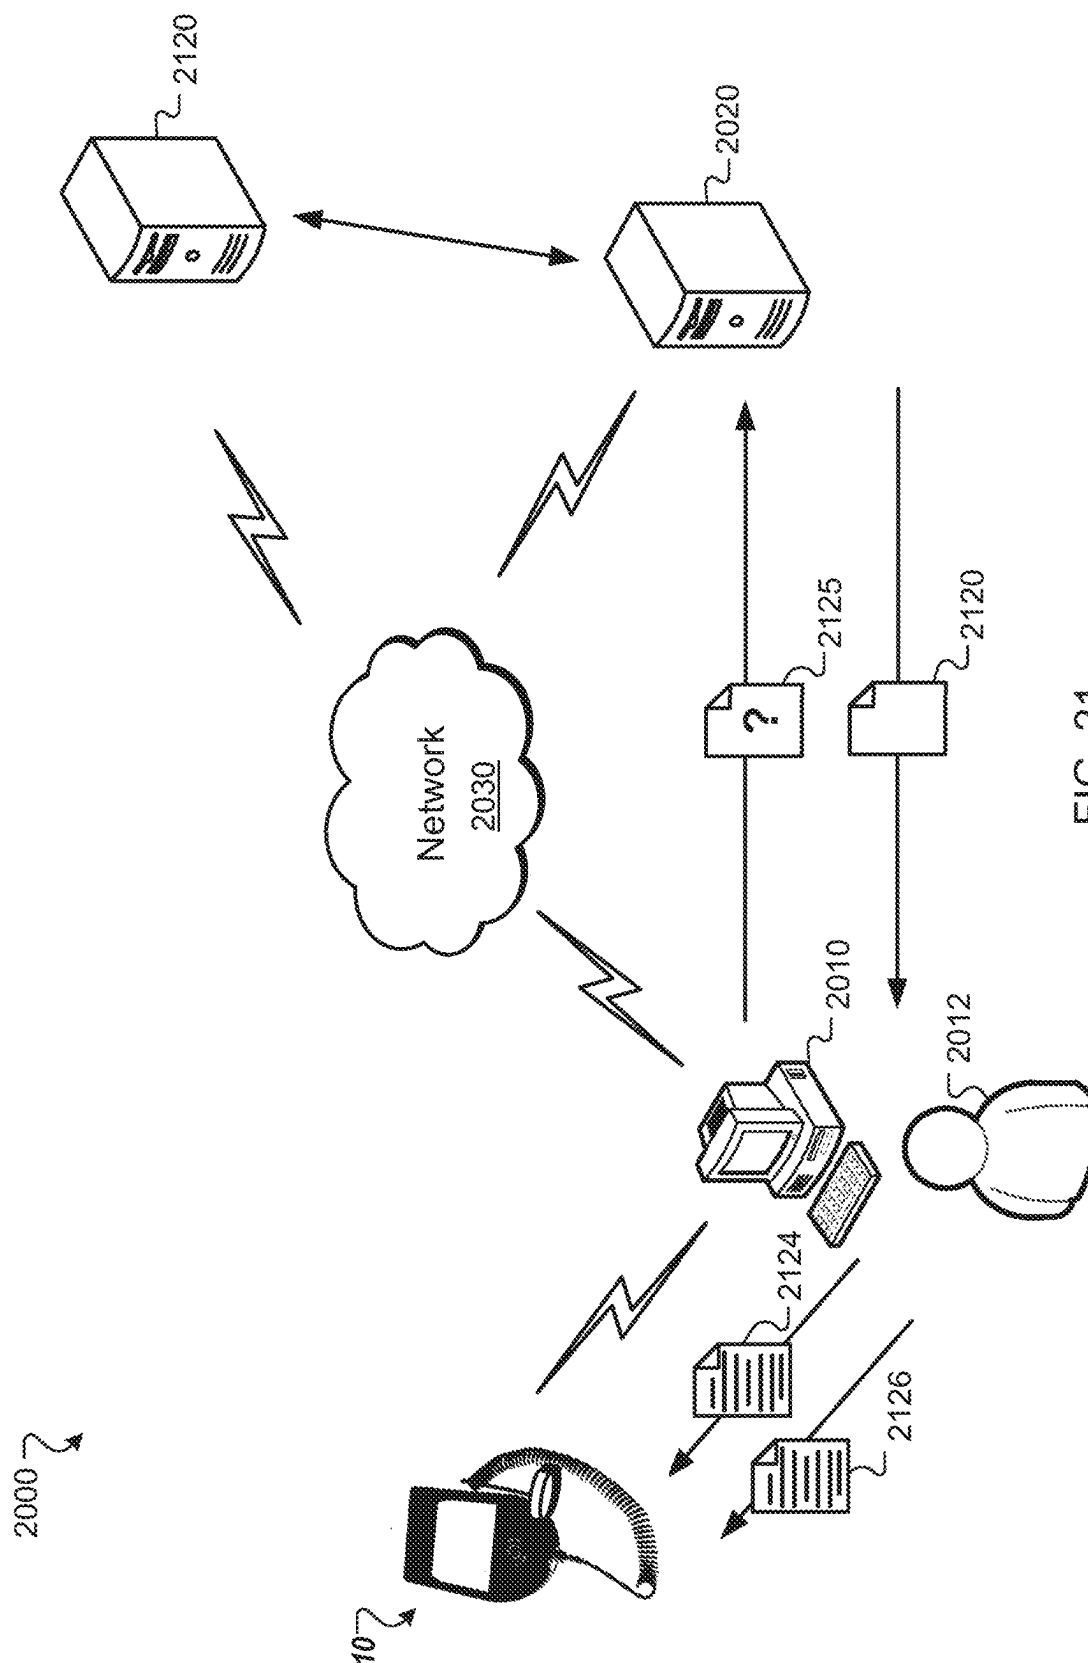

1

MEDICAL DEVICE**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation of U.S. application Ser. No. 16/863,820, filed on Apr. 30, 2020, which is a continuation of U.S. application Ser. No. 15/482,449, filed on Apr. 7, 2017, now U.S. Pat. No. 10,639,502, issued on May 5, 2020, which is a continuation of U.S. application Ser. No. 15/357,883, filed on Nov. 21, 2016, now U.S. Pat. No. 10,086,216, issued on Oct. 2, 2018, which is a continuation of U.S. application Ser. No. 13/271,870, filed on Oct. 12, 2011, now U.S. Pat. No. 9,526,920, issued on Dec. 27, 2016, which claims the benefit of U.S. Provisional Application No. 61/392,154, filed Oct. 12, 2010, U.S. Provisional Application No. 61/405,405, filed Oct. 21, 2010, U.S. Provisional Application No. 61/405,757, filed Oct. 22, 2010, and U.S. Provisional Application No. 61/483,445, filed May 6, 2011, each of which is incorporated herein in its entirety for all purposes.

FIELD

This description relates to a medical device.

BACKGROUND

Medical devices can provide treatment for a variety of health conditions. In some instances, a patient has a degree of control over treatment with a medical device. For example, a patient may be able to initiate treatment with a medical device. The capabilities of a medical device determine to a large degree the way that the patient and others interact with the medical device. In particular, it is important that a medical device be capable of providing effective treatment and a positive patient experience.

SUMMARY

In one aspect, a medical device includes: a treatment module configured to apply a treatment to a patient; one or more processing devices configured to: disallow treatment using the treatment module until treatment authorization occurs; determine that treatment authorization occurs; and in response to determining that treatment authorization occurs, permit treatment to be applied using the treatment module.

Implementations may include one or more of the following features. For example, treatment authorization occurs via payment. Treatment authorization occurs via patient identification. Treatment authorization is linked to geographic location. Treatment authorization occurs via authorization data stored on a removable medium.

Implementations may include one or more of the following features. For example, the medical device includes a wireless communication module operable to receive the activation code over a wireless communication link. The wireless communication link is a Bluetooth or cellular communication link. The medical device is configured to receive the activation code from an enabling device configured to activate a limited number of medical devices and to not activate more than the limited number of medical devices. The one or more processing devices being configured to receive the activation code includes the one or more processing devices being configured to access the activation code from a removable medium. The activation code

2

includes authorization information indicating a number of treatments authorized using the medical device.

In another general aspect, an enabling device includes: a communication module operable to wirelessly transmit one or more activation codes to a medical device, the one or more activation codes being capable of activating the medical device; one or more data storage devices storing authorization information indicating a number of authorized activations of medical devices that the enabling device is authorized to perform; one or more processing devices configured to: receive user input indicating that a medical device should be activated; determine, based on the authorization information, whether activation of the medical device is authorized; if the determination indicates that the activation of the medical device is authorized: control the wireless communication module to transmit the one or more activation codes, and update the authorization information to decrease the number of authorized activations remaining for the enabling device; if the determination indicates that the treatment is not authorized, control the treatment module such that the one or more activation codes are not transmitted.

Implementations may include one or more of the following features. For example, the enabling device is associated with an inventory of medical devices, and the number of authorized activations of medical devices is based on the associated inventory. The communication module is further configured to receive, over a network, second authorization information altering the number of authorized activations the enabling device is authorized to perform, and the one or more processors are further configured to update the information indicating the number of authorized activations to alter the number of authorized activations by the additional number indicated by the second authorization information. The communication module is further configured to receive, over a network, second authorization information indicating an additional number of authorized activations the enabling device is authorized to perform, and the one or more processors are further configured to update the information indicating the number of authorized activations to increase the number of authorized activations by the additional number indicated by the second authorization information.

In another general aspect, a medical device includes: at least one treatment module configured to apply a treatment to a patient, the treatment module including at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer; one or more data storage devices; an interface configured to operatively connect to a removable storage device storing authorization data that identifies a level of treatment authorization; and at least one processing device configured to perform the following in response to receiving user input indicating a treatment should be initiated: determine whether the removable storage device is valid for use with the medical device; if the removable storage device is determined to be valid, access the authorization data; determine whether the treatment is authorized based on the accessed authorization data; if the treatment is determined to be authorized, control the treatment module to apply the treatment; and if the treatment is determined to not be authorized, control the treatment module such that the treatment is not applied.

Implementations of any of the aspects may include one or more of the following features. For example, to determine whether the removable storage device is valid for use with the medical device, the at least one processing device is configured to: access a serial number of the removable medium; and determine that the removable medium is valid

if the serial number is within a predetermined range of values. The at least one processing device is configured to record compliance data for the treatment on the removable storage device if the treatment is applied. The compliance data indicates a time, date, and duration of the treatment. The treatment module includes at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer. To control the treatment module to apply the treatment, the processing device is configured to control the driver circuit such that the driver circuit causes the ultrasound transducer to produce ultrasound with therapeutic properties. To control the treatment module such that the treatment is not applied, the processing device is configured to control the driver circuit such that ultrasound with therapeutic properties is not produced. The driver circuitry includes a signal generator and an ultrasound transducer driver.

The authorization data indicates a number of authorized treatments, and the at least one processing device is configured to decrease the number of authorized treatments indicated by the authorization data after a treatment is applied. The authorization data indicates an authorized amount of treatment time, and the at least one processing device is configured to decrease the amount of authorized treatment time indicated by the authorization data after a treatment is applied. The medical device includes a communication module. The at least one processing device is configured to: receive authorization data that indicates a level of treatment authorization through the communication module; store the received authorization data on the removable storage device or a second storage device of the medical device; and in response to receiving the user input indicating a treatment should be initiated, determine whether the treatment is authorized based on the received authorization data. The communication module is a wireless communication module. The wireless communication module is a cellular communication module.

The authorization data is received from a server system configured to: determine that payment has been made for a number of treatments; determine that the payment is associated with the medical device; generate the authorization data; and transmit the authorization data to the medical device. The processing device is further configured to provide, if the treatment is determined to not be authorized, an indication to the patient that more treatments need to be purchased. The processing device is configured to receive new authorization data after providing the indication to the patient that more treatments need to be purchased, the new authorization data identifying a number of additional treatments for which payment has been received. The authorization data is encrypted, and the processing device is further configured to decrypt the authorization data. The medical device includes a second storage device. The second storage device stores a device identifier that uniquely identifies the medical device, the authorization data is encrypted, the at least one processing device is further configured to decrypt the authorization data; and the device identifier is used to decrypt the authorization data. The medical device includes a payment module configured to receive payment for a number of treatments. The payment module is configured to receive payment through a code, a credit card, or a SIM card. The at least one processing device is configured to: record on the removable storage device or an internal storage device information indicating occurrences of treatment applied by the medical device; and indicate, on a display of the medical device, days during which treatment was applied and days during which treatment was not applied. The medical device

stores information about a treatment regimen for use of the medical device; and the at least one processing device is configured to indicate compliance with the treatment regimen by displaying a calendar that indicates the days during which treatment was applied and the days during which treatment was not applied.

Implementations may include one or more of the following features. For example, the enabling device is configured to activate the medical device by transmitting an activation code over a wireless communication link between the enabling device and the medical device, and the medical device is configured to allow treatments using the treatment module in response to receiving the activation code.

In another general aspect, a medical device includes: a treatment module configured to apply a treatment to a patient, the treatment module including at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer, a display, one or more data storage devices, and one or more processing devices. The one or more processing devices are configured to: receive user input that a treatment should be initiated using the treatment module; in response to receiving the user input, apply a treatment using the treatment module; record on the one or more data storage devices information indicating occurrences of treatment using the treatment module; and indicate on the display days during which treatment was applied and days during which treatment was not applied.

Implementations of any of the aspects may include one or more of the following features. For example, the days during which treatment was applied and days during which treatment was not applied are indicated on a calendar. Days of the calendar during which one or more treatments are applied are marked with a check mark and days of the calendar during which one or more treatments were not applied are unchecked. The one or more storage devices store information about a treatment regimen for use of the medical device, and the one or more processing devices are configured to indicate compliance with the treatment regimen on the calendar. The one or more processing devices being configured to indicate on the display days during which treatment was applied and days in which treatment was not applied includes the one or more processing devices being configured to automatically indicate on the display, in response to the medical device being powered on, days during which treatment was applied and days during which treatment was not applied.

In another general aspect, a medical device includes: a treatment module operable to apply a treatment to a patient, the treatment module including at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer; a primary or rechargeable battery configured to supply power to the medical device; a color display configured to display information to a user of the medical device; a wireless communication module; one or more data storage devices; one or more processing devices configured to: disallow treatment using the treatment module until an activation code is received; receive an activation code received by the wireless communication module over a wireless communication link; in response to receiving the activation code, permit treatment to be applied using the treatment module; store on the one or more data storage devices authorization information indicating a number of authorized treatments remaining for the medical device; receive user input indicating a treatment should be initiated; determine whether the treatment is authorized; if the determination indicates that the treatment is authorized, control the treatment module to apply the treatment and update the

5

authorization information to decrease the number of authorized treatments remaining for the medical device; if the determination indicates that the treatment is not authorized, control the treatment module such that the treatment is not applied; record, on the one or more storage devices, compliance information indicating dates during which treatment was performed using the treatment module; cause the wireless communication module to transmit the recorded compliance information over the wireless communication link; and display on the color display a calendar indicating days during which treatment was performed and days during which treatment was not performed.

In another general aspect, a medical device includes: a treatment module operable to apply a treatment to a patient, the treatment module including at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer; a primary or rechargeable battery configured to supply power to the medical device; a color display configured to display information to a user of the medical device; one or more data storage devices including a removable memory card and a non-removable storage device; one or more processing devices configured to cause the medical device to: access from the removable memory card information indicating a number of authorized treatments for the medical device; based on the accessed information, store authorization information indicating the number of authorized treatments for the medical device on the non-removable storage; receive user input indicating a treatment should be initiated; determine, based on the authorization information, whether the treatment is authorized; if the determination indicates that the treatment is authorized, control the treatment module to apply the treatment and update the authorization information to decrease the number of authorized treatments remaining for the medical device; if the determination indicates that the treatment is not authorized, control the treatment module such that the treatment is not applied; record on the one or more storage devices compliance information indicating dates during which treatment was performed using the treatment module; automatically display on the color display, in response to the medical device being powered on, a calendar indicating days during which treatment was performed and days during which treatment was not performed; access, from a second removable memory card, second authorization information indicating a second number of authorized treatments using the medical device; and based on the second authorization information, increase the number of authorized treatments remaining for the medical device stored on the one or more storage devices.

The medical device includes means for determining the geographic location of the medical device, and treatment is not allowed to commence if the determined geographic location is outside an authorized geographic location. The medical device includes means for determining user identity, and treatment is not allowed to commence if the determined user identity does not match an authorized identity. The treatment module is configured to produce a pulsed ultrasound signal having a frequency in the range of 1 MHz to 2 MHz, consisting of pulses generated at a rate in the range of 100 Hz to 10 KHz with each pulse having a duration in the range of 10 microseconds to 2,000 microseconds. The pulsed ultrasound signal has a power intensity of 100 milliwatts per square centimeter or less. The medical device is a hand-held device configured to accelerate bone healing.

In another general aspect a computer-implemented method includes: receiving user input through a user interface of a medical device, the user input indicating a treat-

6

ment should be administered by the medical device, and the medical device includes a treatment module configured to apply a treatment to a patient; determining whether a removable storage device coupled to the medical device is valid for use with the medical device; in response to determining that the removable storage device is valid for use with the medical device, accessing authorization data stored on the removable storage device; determining that the treatment is authorized based on the accessed authorization data; and controlling the treatment module to apply the treatment in response to determining that the treatment is authorized based on the accessed authorization data.

Implementations of any of the above aspects may include one or more of the following features. For example, the activation code includes the authorization information. The wireless communication link is a Bluetooth or cellular communication link. The one or more storage devices include a removable memory card; and the one or more processing devices configured to: record the compliance information to the removable memory card; and access an activation code stored on the removable memory card or another memory card.

The removable memory card and the second removable memory cards are Secure Digital memory cards. The one or more processing devices being configured to record on the one or more storage devices compliance information indicating dates during which treatment was performed using the treatment module includes the one or more processing devices being configured to record, on the removable memory card and on the non-removable storage, compliance information indicating dates during which treatment was performed using the treatment module. The one or more processing devices being configured to indicate on the display days during which treatment was performed and days in which treatment was not performed includes the one or more processing devices being configured to automatically indicate on the display, in response to the medical device being powered on, days during which treatment was performed and days in which treatment was not performed. The one or more processing devices are further configured to receive an authorization code indicating a number of treatments that are authorized for the medical device and update the authorization information such that the number of treatments indicated by authorization code are added. The one or more processing devices are configured to determine whether the treatment is authorized by determining if the authorization information indicates that at least one treatment is authorized for the medical device. The one or more processing devices are further configured to: access an identifier from the one or more storage devices; and cause the compliance information and the accessed identifier to be transmitted to a server system that is configured to receive the compliance information and the identifier.

Implementations of any of the aspects may include one or more of the following features. For example, determining whether the removable storage device coupled to the medical device is valid for use with the medical device includes accessing a serial number of the removable medium and determining that the removable medium is valid if the serial number is within a predetermined range of values. Recording compliance data for the treatment on the removable storage device if the treatment is applied. The treatment module includes at least one ultrasound transducer and at least one driver circuit. Controlling the treatment module to apply the treatment includes controlling the driver circuit such that the driver circuit causes an ultrasound transducer to produce ultrasound with therapeutic properties. Control-

ling the treatment module such that the treatment is not applied includes controlling the driver circuit such that ultrasound with therapeutic properties is not produced. Receiving the authorization data, and storing the received authorization data on the removable device.

Receiving the authorization data includes receiving the authorization data with a wireless communication module. The wireless communication module is a cellular communication module. The authorization data indicates a number of authorized treatments, and the computer-implemented method further includes decreasing the number of authorized treatments indicated by the authorization data after a treatment is applied. The authorization data indicates an authorized amount of treatment time, and the computer-implemented method further includes decreasing the amount of authorized treatment time indicated by the authorization data after a treatment is applied. Storing a device identifier that uniquely identifies a medical device. The authorization data is encrypted, accessing the authorization code includes decrypting the authorization data, and the device identifier is used to decrypt the authorization data. Recording on the removable storage device or an internal storage device information indicating occurrences of treatment applied by the medical device. Indicating, on a display of the medical device, days during which treatment was applied and days during which treatment was not applied. Indicating compliance with a treatment regimen by displaying a calendar that indicates the days during which treatment was applied and the days during which treatment was not applied. Receiving payment for a number of treatments. Receiving payment for a number of treatments includes receiving payment at the medical device for a number of treatments, the payment being entered with a code, a credit card, or a SIM card.

In another general aspect, a computer-implemented method includes: receiving user input that a treatment should be initiated using a treatment module of a medical device; in response to receiving the user input, controlling the treatment module to apply a treatment; recording on one or more data storage devices information indicating occurrences of treatment using the treatment module; and indicating, on a display of the medical device, days during which treatment was applied and days during which treatment was not applied.

Implementations of any of the aspects may include one or more of the following features. For example, indicating days during which treatment was applied and days during which treatment was not applied includes indicating the days during which treatment was applied and the days during which treatment was not applied on a calendar. Indicating the days during which treatment was applied and the days during which treatment was not applied on a calendar includes marking days of the calendar during which treatment was applied with a check mark and displaying days of the calendar during which one or more treatments were not applied as unchecked. Storing information about a treatment regimen for use of the medical device, and indicating compliance with the treatment regimen on the calendar. Indicating the days during which treatment was applied and the days during which treatment was not applied occurs in response to the medical device being powered on.

Determining the geographic location of the medical device, and disallowing commencement of treatment using the treatment module if the determined geographic location is outside an authorized geographic location. Determining user identity, and disallowing commencement of treatment using the treatment module if the determined user identity does not match an authorized identity. Controlling the treat-

ment module to apply a treatment includes controlling the treatment module to produce a pulsed ultrasound signal having a frequency in the range of 1 MHz to 2 MHz, consisting of pulses generated at a rate in the range of 100 Hz to 10 KHz with each pulse having a duration in the range of 10 microseconds to 2,000 microseconds. The pulsed ultrasound signal has a power intensity of 100 milliwatts per square centimeter or less.

According to another general aspect, a computer-readable storage medium storing instructions that, when executed by one or more processing devices, cause the one or more processing devices to perform the operations of the computer-implemented methods.

According to another general aspect, a medical device includes: at least one treatment module configured to apply a treatment to a patient, the treatment module including at least one ultrasound transducer and at least one driver circuit coupled to the ultrasound transducer; an interface configured to operatively connect to a removable storage device storing authorization data that identifies a level of treatment authorization; and at least one processing device. The at least one processing device is configured to perform the following in response to receiving user input indicating a treatment should be initiated: determine whether the removable storage device is valid for use with the medical device; if the removable storage device is determined to be valid, access the authorization data; determine whether the treatment is authorized based on the accessed authorization data; if the treatment is determined to be authorized, control the treatment module to apply the treatment by producing ultrasound with therapeutic properties; and if the treatment is determined to not be authorized, control the treatment module such that the treatment is not applied.

The one or more processing devices are further configured to: identify a treatment regimen that identifies a prescribed use of the medical device; compare the information about a recorded use to the prescribed use of the medical device; and generate information indicating the degree that the recorded use matches the prescribed use.

The details of one or more implementations are set forth in the accompanying drawings and the description below. Other features and advantages will become apparent from the description, the drawings, and the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a medical device.

FIG. 2 is a block diagram of the medical device.

FIG. 3 is a diagram of the medical device configured to display information.

FIG. 4 is a chart illustrating examples of information that may be displayed.

FIG. 5 is a flow diagram illustrating a process for displaying information.

FIGS. 6A to 6C are diagrams illustrating user interfaces for the medical device.

FIG. 7 is a diagram illustrating a medium for authorizing treatment using the medical device.

FIG. 8 is a diagram of a system for authorizing medical treatments.

FIGS. 9A and 9B are flow diagrams of a process for authorizing medical treatments.

FIG. 10 is a diagram illustrating a system for collecting information related to a medical device.

FIG. 11 is a flow diagram illustrating a process for sending information from a medical device.

FIG. 12 is a flow diagram illustrating a process for collecting information.

FIG. 13 is a diagram of a process for storing patient information.

FIG. 14 is a diagram of the medical device.

FIG. 15 is a diagram of a main operating unit of the medical device.

FIG. 16 shows authorized geographic areas.

FIG. 17 is a block diagram of geo-locking components of the medical device.

FIG. 18 is a block diagram of device authorization components of the medical device.

FIG. 19 is a flowchart depicted use of the medical device.

FIGS. 20 and 21 are diagrams illustrating a system for activating a medical device.

DETAILED DESCRIPTION

In some implementations, a medical device can control its operation to apply treatments that have been purchased and to not apply treatments that have not been purchased. For instance, the medical device can be authorized to provide a particular number of treatments purchased for a patient. When the purchased treatments are exhausted, the medical device can be authorized to perform additional treatments based on additional payment. For example, a user can purchase a card or other removable medium that authorizes a number of additional, prepaid treatments with the medical device. The medical device can access authorization data stored on the removable medium, determine that treatment is authorized, and perform the appropriate treatment.

In addition, or as an alternative, to the above-mentioned features, the medical device can also store information and provide information to a patient. For example, the medical device may provide instructions for using the medical device or information about a particular health condition. The medical device can select the information to provide based a particular health condition of the patient or other information about the patient.

In addition, or as an alternative, to the above-mentioned features, the medical device can record compliance information that indicates occurrences of treatments using the medical device. For example, the compliance information can indicate days and/or times that a patient has performed treatments using the medical device. The compliance information can also indicate the degree to which a patient has complied with a particular treatment regimen. The compliance information can be collected at a server system, and the information can be accessed by multiple parties. The level of access that a party receives can be limited based on the party's relationship to the patient. The server system can receive, store, and provide access to compliance information from multiple medical devices operated by different patients. The medical device can also record errors in the operation of the medical device, send the errors to a server system, and receive service information to address the errors.

In addition, or as an alternative, to the above-mentioned features, the medical device can display information to a patient that indicates the recorded compliance information. The medical device can display a calendar indicating days on which treatment was performed and days on which treatment was not performed. The calendar can also indicate whether or not the treatments that were performed occurred according to the scheduled treatments indicated by a particular treatment regimen for the patient.

In addition, or as an alternative, to the above-mentioned features, the medical device can limit restrict unauthorized use based on an identity of a user or the geographical location of the medical device. The medical device can determine the geographic location of the medical device and not allow treatment to commence if the determined geographic location is outside an authorized geographic region. The medical device can also determine the identity of a user and not allow treatment if the determined identity is not any authorized identity.

Some implementations of the medical device may provide the following advantages. For example, rather than incur a large initial expense by purchasing a medical device with unlimited treatments, in some instances, a patient or third-party payer may pay for only the treatments that are prescribed to the patient. By purchasing treatments as needed, patients and third-party payers may also spread expenses over time. Also, when treatments can be authorized after an initial set of treatments is exhausted, the additional use of the medical device can be easily added. Additional treatments can generally be authorized without service, repair, or reconditioning of the medical device. In some instances, the patient may enter payment directly at the medical device and receive treatment with minimal delay after payment is complete. In addition, by providing only treatments that have been purchased, excessive treatment and misuse of the medical device can be deterred.

Some implementations of the medical device may provide the following additional advantages. Information can be displayed to the patient during treatment, including, for example, information about a health condition of the patient, instructions for using the medical device, and information about the patient's compliance with a treatment regimen. Messages may, for example, encourage, motivate, inform, entertain, and instruct the patient.

Some implementations of the medical device may provide the following additional advantages. Compliance information may be collected and sent to a server system. Security measures can be implemented so that insurance companies, physicians, and caretakers can receive access to the compliance information based on their relationship to the patient. The server system may receive information about errors that occur during operation of the medical device, and the server system may send service information to address the errors.

Some implementations of the medical device may provide the following additional advantages. Medical devices can be maintained in a deactivated state until activated in a controlled process, reducing incentive for theft and misuse. The ability of devices to activate medical devices and authorize medical treatments can be controlled. The number of medical device activations that can be performed by a device can be limited to the inventory associated with the device.

Some implementations of the medical device may provide the following additional advantages. Information indicating a patient's usage of a medical device over time and compliance with a treatment regimen can be displayed. The patient's compliance with a treatment regimen can be easily discernable from a calendar display indicating days on which treatment occurred.

Some implementations of the medical device can limit use by unauthorized users.

Some implementations of the medical device can also limit use outside an authorized geographical area.

Referring to FIG. 1, a patient is shown using a medical device 10 that includes a treatment module for applying a treatment to the patient. In the example illustrated, the

11

medical device 10 is a portable ultrasonic treatment device. The treatment module may include, for example, one or more ultrasound transducers 16 and at least one driver circuit coupled to the ultrasound transducers 16.

The medical device 10 can include a control unit 12 that controls the operation of the transducers 16. The control unit 12 can include the transducer driver circuit. The medical device 10 can also include cables 18 that can carry power, data, and control signals between the control unit 12 and the transducers 16.

The medical device 10 can include a placement module 14 that couples the transducers at a location of the patient's body where treatment is needed, for example, over a fractured bone or next to damaged connective tissue. The placement module 14 can include a band, sleeve, applicator, or other connector to fasten the one or more transducers to a treatment site. An ultrasound conducting gel 20 can be applied to the skin of the patient to enable the ultrasound to propagate effectively to the patient's tissue.

The medical device 10 can use low intensity, high-frequency acoustic energy (ultrasound) to treat injuries, defects, or pathologies. For instance, the ultrasonic treatment device can be designed to treat injuries, defects, or pathologies of bones or connective tissue, and, in some instances, can increase cellular level activity that leads to healing of ischaemic or grafted tissue. The medical device 10 may be used as an adjunct to surgical repair, in order to speed healing, or in some cases can be used alone to heal tissue injuries without surgery (e.g., for degenerative diseases such as osteoarthritis, tendinosis, and tendonitis). The medical device 10 can be suitable for use in treatment of bone fractures and/or connective tissues associated with joints, such as those in the hand, foot, wrist, ankle, knee, elbow, hip, shoulder, back, and neck.

For example, following surgery, the medical device 10 can be applied non-invasively to the outside of the body (e.g., coupled to the skin with coupling media, such as a gel) in the region of the repaired tissue. The medical device 10 can be operated to transmit ultrasound (for example, in the form of pulses) into the tissue in need of treatment, or at the interface with the uninjured tissues. Exposure to the ultrasound can stimulate a faster, better quality repair of the tissue. At a bone interface, the ultrasound can also stimulate bone repair and bone ingrowth into repair or graft tissue. This can give rise to a faster, stronger repair and improved integration of the interface between, for example, tendon, ligament, and bone. The ultrasonic treatment device may also be used to non-invasively treat pathologies of connective tissues, such as osteoarthritis, ligament and tendon conditions, without the need for a surgical procedure.

Referring to FIG. 2, the control unit 12 of the medical device 10 can include a processing device 50 that executes instructions stored on a storage device 52. The processing device 50 can include one or more processing devices. The storage device 52 can include one or more storage devices, one or more of which may be removable. The control unit 12 can also include a driver circuit 54, a user interface module 60, a payment module 62, a communication module 64, and a power supply 68.

By executing the instructions stored on the storage device 52, the processing device 50 can, for example, determine whether a treatment is authorized. If treatment is authorized, the processing device 50 can control the treatment module (for example, driver circuit 54 and transducers 16) to apply the treatment. Applying the treatment can include controlling the driver circuit 54 to produce ultrasound with therapeutic properties. Controlling the driver circuit 54 to pro-

12

duce ultrasound can include activating the driver circuit 54, for example, supplying power to the driver circuit 54, sending control signals to the driver circuit 54, or causing the driver circuit 54 to produce a particular output. If the treatment is not authorized, the processing device 50 can control the treatment module such that the treatment is not applied. For example, the processing device 50 can control the driver circuit 54 such that ultrasound with therapeutic properties is not produced. Controlling the driver circuit to not apply treatment can include not activating the driver circuit 54, deactivating the driver circuit 54, setting the output of the driver circuit 54 (for example, setting the amplitude to zero), and/or otherwise limiting or preventing treatment. The processing device 50 can also be configured to control other components described below, for example through instructions stored on the storage device 52.

The processing device 50 can determine whether a treatment is authorized by, for example, accessing authorization data. If, for example, accessed authorization data is invalid, is for a different medical device 10, has expired or all treatments associated with the code have been expended, or if no authorization data can be accessed, the processing device 50 can determine that treatment is not authorized. On the other hand, if valid authorization data can be accessed, the processing device 50 determines whether at least one treatment using the medical device 10 is authorized. The authorization data may or may not include an authorization code that indicates that payment for treatments has occurred. The authorization data can be stored in the storage device 52, for example, or, as described further below, in a removable medium.

The storage device 52 can store a device identifier, such as a serial number, that identifies the particular medical device 10. The device identifier can uniquely identify the medical device 10 and distinguish it from all other ultrasonic treatment devices, even those of the same type or model. The storage device 52 can also store information about the treatments that are authorized for the medical device 10, for example, a number of treatments that are authorized or an authorization code that authorizes treatments.

The driver circuit 54 can be configured to send drive signals that cause the transducers 16 to generate ultrasound with therapeutic properties. The driver circuit 54 can include a signal generator 56 that generates a signal and a transducer driver 58 that drives the transducers 16 according to the generated signal. In an implementation, the ultrasound generated by the transducers 16 can include low intensity ultrasound (for example, 100 mW/cm² or less) having a frequency ranging between about 1 and 2 MHz, more particularly about 1.5 MHz. The ultrasound can be pulsed, with a pulse width ranging from about 10 to 2,000 microseconds, more particularly about 200 microseconds, with a repetition frequency ranging from about 100 Hz to about 10 KHz, more particularly about 1 KHz.

The user interface module 60 can provide information to the patient and enable treatment to be initiated. The user interface module 60 may include one or more input devices or controls, for example, buttons, a keypad, or a touch-sensitive screen. The user interface module 60 may be used by a patient or other person, for example, to enter user input that indicates that a treatment should be administered by the medical device. When the processing device 50 determines that treatment is not authorized, the processing device 50 can provide an indication to the patient on the user interface module 60 that more treatments need to be purchased.

The user interface module 60 may also include one or more output devices, for example a screen, a liquid crystal

13

display, or lights. For example, the interface module 60 can include a screen 72, for example, a liquid crystal display (LCD), a thin-film transistor (TFT) display, a field sequential display, or an organic light-emitting diode (OLED) display. The interface module 60 can also include light-emitting diodes (LEDs) and other indicators. The interface module 60 may include a speaker or other device that can produce sound (not shown), or other output devices. The user interface module 60 may also include input capabilities or input devices (not shown), for example, buttons, one or more keypads, and other controls. The screen 72 may be touch-sensitive to receive input from a user. The user interface module 60 can also include an interface to access a removable storage medium, such as a subscriber identity module (SIM) card, a Secure Digital (SD) card, or other types of removable storage media.

The payment module 62 can enable a patient to enter payment at the control unit 12, or to receive information indicating prior payment. Payment can be enabled through one or more methods. The payment module 62 can include a credit card reader that reads a card and charges treatment to a credit card, debit card, or similar card that is swiped at the control unit 12. The payment module can include a SIM card reader, and a patient may purchase a SIM card that includes information that represents one or more payments made for treatment with the ultrasonic treatment device. The payment module can include a reader for reading other types of removable media, for example, a SD card or other flash memory device. The control unit 12 can be configured to receive payment in the form of a code or other user input that may be entered on the interface module 60. Some implementations may exclude the payment module 62. For instance, in some implementations, provisions may be made to allow payment remotely from the device 10, for example, at a computer connected to a network.

The communication module 64 can be configured to send payment information to a remote system and/or receive authorization information that authorizes additional treatments using the medical device 10.

In some implementations, the processing device 50 is configured to receive an authorization code or other authorization data through the communication module 64 and to store the received authorization code in the storage device 52. The communication module 64 can enable communication with a server system, client system, or other computer system over a wired or wireless connection. The communication module 64 may enable a communication link that is wired or wireless. The communication module may enable communication over, for example, Ethernet, Universal Serial Bus, 502.11, Bluetooth, Zigbee, cellular networks, and other communication links. In one implementation, the communication module 64 can include a cellular transceiver 66 to receive and/or transmit information over a cellular network. The communication module 64 may also enable communication through multiple communication links.

The communication module 64 can be configured to send payment information to a remote system and/or receive authorization information that authorizes additional treatments using the medical device 10. The processing device 50 can be configured to receive an authorization code through the communication module 64 and to store the received authorization code in the storage device 52.

A power supply 68 can provide power to the components of the medical device 10, including the driver circuit 54, the processing device 50, the storage device 52, the payment module 62, the communication module 64, and the user interface module 60. The power supply 68 can include a

14

battery that is integrated into the control unit 12 or is removable. The battery can be primary battery or a rechargeable battery, and the power supply 68 can include a detachable power adapter that can charge a rechargeable battery.

When a user performs treatment using the medical device 10, the medical device 10 can collect and store compliance information. Collecting compliance information can include recording information about use of the medical device 10, for example recording the number of treatments that are performed. Compliance information can include a number of treatments provided by the medical device 10, a date and time that a treatment was provided by the medical device 10, and/or a duration that a treatment was provided by the medical device 10. Information about multiple uses or treatments with the medical device 10 can be collected.

A treatment regimen that identifies a prescribed use of the medical device 10 can be identified. For example, the treatment regimen may be entered on the device after the health condition has been diagnosed or after the medical device 10 has been prescribed to the patient. Information about a treatment regimen may be entered on the medical device 10 or received from a network, which may include a cellular network. The information about the recorded use of the medical device 10 can be compared to the information about the prescribed use of the medical. Information indicating the degree that the recorded use matches the prescribed use can be generated.

Compliance information can be stored on the storage device 52, on a removable medium, or both the storage device 52 and a separate removable medium. The compliance information may, but is not required to, include one or more results of a comparison between the recorded use of the medical device 10 and the treatment regimen of the patient.

Referring to FIG. 3, the medical device 10 can display information to the patient. For example, the medical device 10 can display information that relates to the particular patient using the medical device 10, for example, information about a health condition of the patient, a treatment regimen of the patient, or a physician of the patient. The information displayed on the medical device 10 can thus be personalized to the particular patient that receives the medical device 10 and a particular health condition of the patient. In some instances, the information displayed may be selected to instruct, encourage, or entertain the patient. In addition, the information can provide advertisements and personalize treatment using the name or brand of, for example a particular physician, hospital, or insurance company.

The information displayed on the medical device 10 may be organized into a plurality of messages 304. Messages 304 can include a variety of media, including text, images, video, and sound. Messages 304 can be stored on the storage device 52 of the control unit 12. Some messages 304 may be entered onto medical device 10 during manufacturing. For example, an initial set of predetermined messages 304 may be loaded onto a storage device 52 before it is shipped. Messages 304 may also be entered at other times to supplement the initially loaded messages 304, including before a medical device 10 is dispensed to a patient and after a patient begins use of the medical device 10. Messages 304 may be received with, for example, the communication module 64 and may be stored on the storage device 52.

Messages 304 can include information related to specific health conditions. For example, some messages 304 may relate to treatment of broken bones of the foot, and others may relate to treatment of broken bones of the arm. The

15

medical device 10 can store messages 304 that relate to a wide variety of health conditions. To ensure that the messages 304 displayed to the patient are useful, the processing device 50 can access information that identifies a health condition of the patient, which can be stored on the storage device 52.

Based on the identified health condition, the processing device 50 can select one or more messages out of the set of messages 304 that are stored on the storage device 52. For example, if the processing device 50 determines that the patient has a broken foot, the processing device 50 can select one or more messages 304 related to broken bones of the foot and treatment of a broken foot. The selected messages 304 can be displayed to the patient on the screen 72. In some implementations, the screen 72 may be part of the interface module 60, while in others the 72 screen may be integrated into the control unit 12.

Selected messages 304 can be displayed to the patient during treatment. For example, while a treatment is applied, the medical device 304 can display information to instruct the patient about proper use of the medical device 10. In many instances, a patient receives only minimal instruction about the proper use of the medical device 10 when the medical device 10 is dispensed to the patient. A patient may forget the proper use of medical device and the details of a treatment regimen, especially when the medical device 10 is new. By providing messages 304 that instruct the patient how to use the medical device 10, the patient may be more likely to perform treatment correctly. The instructive messages 304 can be selected based on the health condition of the patient and the associated treatment regimen for the health condition.

The medical device 10 can select and display a variety of other messages 304 during treatment. For example, messages 304 can also provide general health information, such as, "smoking inhibits bone healing" or "tell your doctor if you use blood thinners."

Messages 304 can also be selected based on a patient's compliance to a treatment regimen. The medical device 10 can store information that indicates when the patient should receive treatment. The medical device 10 can also record information indicating when treatment is actually performed. The medical device 10 can compare the planned or prescribed use of the medical device with the actual use of the device and determine how well the patient has complied with the prescribed treatment regimen. The medical device 10 can display messages 304 to the patient that directly or indirectly provide compliance information. For example, messages can provide direct feedback about a patient's compliance. Messages 304 can also be displayed that motivate, encourage, and remind the patient to follow a consistent treatment schedule. Messages 304 can also describe the benefits of continuing treatment or provide information about how the medical device 10 operates.

Messages 304 can also provide physicians and others an opportunity to provide a personalized message. For example, one or more messages 304 may include the name of a patient's physician, the name of the patient's insurance company, or the logo for a hospital. Customized messages 304 can enable physicians and organizations to reinforce their brands and enhance the patient's experience during treatment. Messages 304 can also include contact information, for example, the phone number for the patient's primary physician. Messages 304 can include advertisements and paid content.

Messages 304 can also be provided to entertain a patient during treatment and thus encourage the patient to complete

16

the treatment. In some implementations, the medical device may enable the patient to acquire or input additional content to display on the medical device.

Referring to FIG. 4, a diagram illustrates the selection and display of messages 304 on a screen 72 of the medical device 10.

The processing device 50 of the medical device 10 can access information identifying a health condition of a patient. As illustrated, a health condition record 401 indicates that the health condition of the patient is a broken clavicle. Based on the identified health condition, the processing device 50 can select one or more messages from a plurality of messages 304. The plurality of messages 304 may include a set 402 of predetermined messages 304. Each message 304 in the set 402 may be associated with an identifier, as represented by the numbers from one to ten. From the set 402, a subset 403 of messages 304 may be selected. The selected messages 304 can include messages 304 that relate to the particular health condition of the patient. The selected messages 304 can be ordered into a sequence 404 for display on the medical device 10.

The sequence 404 of messages 304 may be displayed on the screen 72 of the medical device 10. In one implementation, the sequence 404 of messages 304 may begin to be displayed when treatment begins, and the sequence 404 may end roughly when treatment ends. In addition to the messages 304, other information can be included, for example, information that describes the treatment being performed. For example, notifications 406 that indicate the time remaining until treatment is completed may be interspersed between other messages 304.

The messages 304 selected and the sequence 404 of the selected messages 304 can vary according to the needs of the patient and to limit unnecessary repetition. For example, instructions about how to use the medical device 10 may be selected and displayed for an initial set of treatments using the medical device 10, but instructions may be omitted after many treatments have successfully been performed.

Referring to FIG. 5, an example of a process 500 for providing information is illustrated. The processing device 50 of the medical device 10 can be configured to perform the process 500, for example, by executing instructions stored on the storage device 52.

A plurality of messages is stored on the medical device (502). For example, the storage device may store the plurality of messages. Messages may be entered on the storage device by a manufacturer of the medical device before the medical device is sold. Messages can also be entered on the storage device by sales representatives, physicians, and others at other times.

The medical device receives information about a health condition of a patient (504).

For example, after a patient is diagnosed with a particular health condition, the health condition can be entered on the medical device. A physician, assistant, sales representative, or other person may enter information that indicates the health condition of the patient on the medical device. In addition, or alternately, the medical device may receive information about a health condition of the patient through the communication module. For example, the medical device may receive information about a prescription or diagnosis automatically over a network, without requiring any manual input. The medical device can store the information about the patient's health condition for later access. The health condition can be, for example, a health condition that is treatable by the medical device.

The medical device selects messages for the patient (506). For example, the messages can be selected from the stored messages stored on the storage device. One or more messages can be selected based on the identified health condition of the patient. For example, if the patient has a broken ankle, messages can be selected that describe treatment of a broken ankle. The selected messages can include messages related to multiple health conditions. The selected messages can include instructions for using the medical device. The selected messages can include one or more messages that include information about a doctor that treated the patient or a medical office where the patient was treated. The selected messages can include one or more messages about the medical device or information about the provider of the medical device. The selected messages can include advertisements. The selected messages can include image data or video data.

In some implementations, the medical device can store records indicating use of the medical device. For example, the medical device can record the number of treatments that have been performed using the medical device, the date and time that each treatment is performed, and/or the duration of each treatment. The information in these records, referred to generally as compliance information, indicates the manner in which treatments were performed using the device, from which a patient's compliance with a particular treatment regimen can be determined.

Compliance information can be stored on the one or more storage devices 52. For example, the compliance information can be stored on internal memory of the medical device 10 and can also be stored on a removable medium, such as an SD memory card. Recording the compliance information on internal memory and the removable medium provides a backup in case one of the storage devices should fail. Additionally, the removable medium may be removed and used to transfer compliance information to other systems.

The medical device can also identify a treatment regimen that corresponds to the health condition. For example, the medical device may receive the information from a prescription, a treatment regimen that is entered directly on the medical device, or the medical device may store a number of treatment regimens on the storage device. The medical device can access the records indicating use of the device. The medical device can compare the records indicating use of the medical device to the treatment regimen identified for the health condition of the patient.

The medical device can provide an indication of compliance with the treatment regimen. For example, the medical device may provide an indication of compliance in one or more messages that are selected to be later displayed to the patient. The selected messages can also encourage compliance to a treatment regimen, for example, by praising the patient for past compliance or assuring the patient that continued treatment will bring good results. The selection of messages, including the selection of messages about compliance to the treatment regimen, can be based on the number of uses of the medical device indicated in the records that indicate use of the medical device.

The medical device can also identify the language of the patient and select one or more messages in the language of the patient. The plurality of messages stored on the medical device can include messages in at least two languages. For example, some or all of the stored messages can be included in multiple languages. The medical device can identify the language of the user, for example, based on user input, messages input on the medical device, information received by the communication module, or other information.

The medical device can begin treatment (508). For example, a patient may enter input indicating that treatment should begin, and the medical device may control a driver circuit to drive an ultrasound transducer so that the ultrasound transducer produces ultrasound with therapeutic properties. The medical device can store and update records indicating use of the medical device.

The medical device can display the selected messages (510). The selected messages can be displayed during treatment, for example, while the ultrasound with therapeutic properties is applied to the patient. The messages can be displayed on a liquid crystal display or other screen.

Referring to FIG. 6A, the medical device 10 can display information about a patient's compliance with a treatment regimen on a user interface 600a. The user interface 600a can be displayed on the screen 72 of the user interface module 60. The user interface 600a includes a calendar view 602 that indicates whether treatment was performed each day of, for example, the current month, or the current month and previous months. In the calendar space corresponding to each day that treatment was performed, a compliance indicator 604 can be displayed, for example, a colored square, a check mark, or other image or icon. In the space corresponding to each day in which treatment was not performed, a noncompliance indicator 606 can be displayed, for example, a different image or icon, such as a blank square or a red "X." Thus the user interface 600a can visually distinguish the days during which treatment was performed from days during which treatment was not performed, providing an easily-understandable indication of recent compliance with the treatment regimen.

In some implementations, information about the particular treatment regimen prescribed for the user of the medical device 10 is stored on the medical device 10, and the compliance indicator 604 is displayed to indicate that a treatment performed on a particular day complies with the particular treatment regimen prescribed. In other words, rather than assuming that the treatment regimen requires one treatment each day, the medical device 10 compares times that treatments were performed to times that treatments were scheduled to be performed, as dictated by a treatment regimen. If a treatment regimen involves treatment every other day, for example, a neutral indicator can be displayed to represent days in which treatment was not scheduled and was not performed. The neutral indicator may be, for example, the day of the month that the day occurs. The noncompliance indicator 606 may be displayed, for example, only when treatment was scheduled to be performed on a day and treatment did not occur on that day. If treatment was performed on a day that treatment was not scheduled, an improper treatment indicator different from the noncompliance indicator 606 may be displayed for that day, distinguishing noncompliance by omitted treatment from noncompliance by performance of an unscheduled treatment. As a result, compliance relative to a treatment regimen can be accurately indicated when scheduled treatments are not scheduled every day.

Similarly, compliance can be indicated for treatment regimens that dictate treatment multiple times in a day. For example, multiple compliance indicators 604 or multiple noncompliance indicators 606 can be displayed to indicate each treatment that was completed or missed that day.

In other implementations, the medical device 10 displays the compliance indicator 604 for days that treatment was performed and displays the noncompliance indicator 606 for days that treatments were not performed, without regard to times that treatments were dictated by a prescribed treatment

regimen. Thus even when the medical device **10** does not have access to information indicating a treatment regimen, the calendar view **602** indicates when treatments were performed, permitting the user or others to determine compliance with an appropriate treatment regimen.

The user interface **600a** may display patient compliance for time period longer or shorter than a month, and for previous periods of time rather than, for example, the most recent weeks or months.

The medical device **10** can automatically display the calendar view **602** as the medical device **10** is powered on or at other times. For example, each time the medical device **10** is powered on, while the medical device **10** is initializing and for a period of time afterward, the calendar view **602** showing compliance can be displayed. The calendar view **602** can also be displayed to physicians, caretakers, and others. The calendar view **602** can be displayed automatically after particular functions of the medical device **10** are accessed, or in response to a request that the calendar view **602** be displayed.

The medical device **10** can automatically display a total compliance to-date indication. For example, if ten days have elapsed since the start of a daily treatment regimen and the patient only used the device for eight out of the ten days, then the total compliance indicator can display 8/10 or 80% to indicate the overall level of compliance.

The user interface **600a** can also display notification icons **610**. The notification icons **610** can vary in appearance according to the current status of the medical device **10**. The notification icons **610** can indicate, for example, the status and availability of communication links such as wireless connections, whether service is needed, that error or notification messages are available, the types or quality of connections with various modules, the remaining battery charge of the medical device, and other notifications.

Referring to FIG. 6B, after the calendar view **602** is displayed, or after receiving user input, the medical device **10** can display a treatment timer **612** on a user interface **600b**. The treatment timer **612** can indicate the time remaining before a treatment is completed. For example, for a twenty-minute treatment, the treatment timer **612** can initially indicate the duration of treatment, twenty minutes. While a treatment is in progress, the treatment timer **612** can count down toward zero, reaching zero when the treatment ends. The notification icons **610** can also be displayed.

Referring to FIG. 6C, an alternative user interface **620** includes a calendar view **622** indicating daily compliance with the treatment regimen and a treatment timer **624**. Days for which treatment was performed as indicated in the treatment regimen are indicated with a first marking **626**, while days for which planned treatment failed to be performed are indicated with a different marking **628**. Days in the future can be marked with their corresponding calendar numbers.

Referring to FIG. 7, a removable medium **710**, for example, an SD card, USB device, or other removable memory device, can be used to authorize use of the medical device **10**. The removable medium **710** can store authorization data **720** that indicates a level of treatment authorization, for example, a number of treatments authorized or an amount of treatment time authorized using the medical device **10**.

The medical device **10** can include an interface **712** that operatively connects to the removable medium **710**, permitting the processing device **50** to access the authorization data **720**. The interface **712** can include a slot that receives the removable medium **710** within the medical device **10**. The

slot can be accessible to a user, permitting the user to replace the removable medium **710** with a different removable medium. The control unit **12** of the medical device **10** can define the slot and can include a cover that covers the slot.

To obtain treatment authorization, the patient can obtain the removable medium **710**, which can be a prepaid medium that represents that payment has been made by or for the user. Removable media can store differing levels of treatment authorization. Different removable media may be sold with authorization data **720** that permits, for example, 50, 25, or 10 treatments. Treatment authorization may additionally or alternatively be indicated as an amount of time, for example, 1000, 500, or 100 minutes of treatment. In some implementations, the removable medium **710** can be purchased from a retail store or a physician's office. The fact that the patient obtained the removable medium **710** indicates that payment was made, and no additional verification of payment may be necessary to use the medical device **10**.

The removable medium **710** may be a secure mode of communicating that a particular number of treatments are authorized. The removable medium can include a copy-protection or anti-counterfeiting feature that can be used to determine whether the removable medium is genuine. For example, the removable medium can store an encoded value in a manner that the value is not easily duplicated or copied from one removable medium to another. The encoded value can be hardware-encoded or factory-set with a physical setting such that similar removable media cannot be altered to mimic the encoded value. In some implementations, the encoded value is a serial number that is embedded in non-writable storage of the removable medium. Each valid removable medium can have a unique serial number. Only removable media that have a serial number within a predetermined range of values can be considered genuine.

In use, a user interacts with the medical device **10** to indicate that treatment should be initiated, for example, by pressing a button or entering other input. In response, the processing device **50** determines whether a removable medium is present. If no removable medium is present, the processing device **50** disallows treatment.

If a removable medium such as the removable medium **710** is present, the processing device **50** determines whether the removable medium **710** is valid for use with the medical device **10**. For example, the processing device **50** determines whether a serial number or other value encoded in the removable medium meets predetermined criteria. In some implementations, the processing device **50** determines whether the value is within a predetermined set or range of values. The serial number can be a value that is not modifiable by a user, for example, a value that is fixed in the hardware configuration of the removable medium and cannot be copied onto a similar removable medium. Thus the processing device **50** can verify that the physical medium is valid. If a removable medium is not genuine, or is not compatible with or intended for the medical device **10**, the processing device **50** disallows treatment.

If the removable medium **710** is genuine, the processing device **50** accesses authentication data **720** stored on the removable medium **710**. The authentication data **720** can indicate a number of treatments authorized or a number of treatment minutes that treatment is authorized. For example, when each treatment has a duration of twenty minutes, the authorization data **720** may indicate that ten treatments are authorized, or may indicate that two hundred minutes of treatments are authorized. If the authorization data **720** indicates that at least one treatment is authorized, or that one or more treatment minutes are authorized, the processing

device **50** controls the treatment module to provide ultrasound with therapeutic properties. If the authorization data **720** indicates that no treatments are authorized, the processing device **50** disallows treatment.

After the medical device **10** applies a treatment, the processing device **50** alters the authorization data **720** to indicate an updated level of authorization. For example, the medical device **10** can decrease the number of authorized treatments or decrease the number of authorized treatment minutes remaining. Modified authorization data that indicates an updated level of authorization can be stored on the removable medium **710**, for example, by overwriting the authorization data **720** that was stored before treatment began.

The medical device **10** can also store compliance data **730** on the removable medium **710**. When the medical device **10** applies a treatment, the processing device **50** can store information about the treatment performed. For example, the compliance data **730** can indicate the time, date, and duration of the treatment applied, along with other treatment information. The removable medium **710** can thus include a compliance log that indicates use of the medical device **10** over time. The compliance data **730** can also indicate, for example, the degree that the use of the medical device **10** corresponds to planned or prescribed use of the medical device **10**. For example, the compliance data **730** can indicate days or times at which treatment was scheduled and whether treatment occurred at those days or times. Compliance data **730** can additionally or alternatively be stored on an internal storage device of the medical device, such as the storage device **52**.

In some implementations, the authentication data **720** is encrypted, which can discourage tampering. In such implementations, the processing device **50** decrypts the authentication data **720** before determining whether treatment is authorized. Also, after modifying the authentication data to indicate a decreased level of authorization, the processing device **50** encrypts the modified data and stores the encrypted data on the removable medium **710**.

When additional treatments are desired, for example, after the treatment authorization of the authorization data **720** is depleted, a user can obtain a different removable medium that includes authorization data for additional treatments.

In some implementations, the authorization data **720** directly authorizes the treatments, without the medical device **10** needing additional information or confirmation from another system. In some implementations, as described below, the medical device **10** verifies the authenticity of authorization data **720** by communicating with a server system or other device.

Referring to FIG. 8, a system **800** for authorizing medical treatments includes the medical device **10** connected to a server system **802** via a network **806**. The system **800** can also include a third-party server system **804** and a cellular network **808**. After payment is made by or for a patient, authorization data can be entered at or received by the medical device **10**. The authorization data indicates a level of treatment authorization, and can include an authorization code.

A patient may desire to authorize medical treatments using the ultrasonic treatment device **10**. For example, the patient may receive the ultrasonic treatment device **10** in a condition in which treatments have not yet been authorized. As another example, the patient may have used treatments authorized for the ultrasonic treatment device **10** so that an insufficient number of treatments are currently authorized to complete treatment.

To purchase additional treatments of the medical device **10**, the patient may provide payment information **810** at the medical device **10**. Payment information **810** includes payment entered or authorized at the medical device **10** and also information that indicates that payment has been made in another manner. For example, the patient may enter a credit card, a debit card, or another payment device into an appropriate reader of the medical device **10** and authorize a charge to an account owned by the patient. The patient may also enter an account number on the user interface module **60** of the medical device **10** to authorize payment. The patient may also purchase a prepaid medium, for example, a SIM card, a Secure Digital (SD) card, or a prepaid card with a magnetic strip, an optical code, or a printed code, from a store or physician's office. In one implementation, the prepaid medium may be a secure mode of communicating an amount of payment that has been paid. The patient may enter the prepaid medium at the ultrasonic treatment device **10** to indicate that payment has been made. The patient may also purchase treatments in a store or through a web site, may receive a confirmation code for the transaction, and may enter the confirmation code at the ultrasonic treatment device **10**. The system **800** can also be used to verify the validity of an authorization code received from a prepaid medium.

The medical device **10** can send the payment information **810** to a server system **802**. The payment information **810** can be associated with a device identifier **812** that identifies the medical device **10**, which can also be sent to the server system **802**. In addition to, or instead of, sending a device identifier **812**, the medical device **10** may send a patient identifier that identifies the patient, together with the payment information. As will be described in greater detail below, the server system **802** can send an authorization code to the medical device **10** after receiving the payment information **810** and the device identifier **812**.

The medical device **10** may send the payment information **810** and the device identifier **812** to the server system **802** through the network **806**. Alternatively, or additionally, the medical device **10** may initiate a communication using the cellular network **808** to send the payment information **810** and the device identifier **812** to the server system **802**. Payment information **810** can also be received through a removable medium, token, code or other indication that treatment is authorized.

In one implementation, a prepaid medium can store an authorization code that can directly authorize treatments, so that the ultrasonic treatment device **10** is not required to transmit any information to the server system **802**. A prepaid medium can include an authorization code that can enable treatments of the ultrasonic treatment device **10**, independent of a server system **802**. For example, a patient may purchase a SIM card or other device that stores an authorization code compatible with the ultrasonic treatment device **10**. The SIM card containing the authorization code can be entered at the ultrasonic treatment device **10** and the treatments authorized by the authorization code can be enabled on the ultrasonic treatment device **10**. Payment is received by the retail store or physician's office where the prepaid medium was obtained. The fact that the patient obtained the prepaid medium proves that payment was made, and no additional verification may be necessary. In some implementations, the ultrasonic treatment device **10** may verify that the authentication code included with the prepaid medium is authentic, and may ensure that the authentication code of the prepaid medium is not used multiple times (for example, by altering the data on the prepaid medium). In

another implementation, a mechanical device or key may also be used to indicate authorization of additional treatments of the ultrasonic treatment device **10**.

Treatments can also be purchased for a patient by a third-party payer, for example, an insurance company. A third-party server system **804** can transfer payment information **816** to the server system **802** with a patient identifier **818** that identifies the patient. The payment information **816** can include the information that completes the act of payment or indicates that payment has been made. The patient identifier **818** can include a name, prescription number, insurance policy number, or other identifier.

The server system **802** can receive the payment information **810** and the device identifier **812** from the medical device **10**, or can receive the payment information **816** and the patient identifier **818** from the third-party server system **804**.

The server system **802** can determine that payment has been made for a number of treatments, for example, using the payment information **810**, **816**. The server system **802** can also determine that patient is associated with the medical device, for example, using the patient identifier **818** or device identifier **812** associated with the payment information **810**, **816**. The server system **802** can use the received information and stored records to associate the payment with the patient to be treated with the medical device **10**. The server system **802** may store records that associate patient identifiers **818** and device identifiers **812** with particular patients and medical devices **10** so that payment can be applied for the correct patient and medical device **10**.

The server system **802** can also generate an authorization code **814** that enables the medical device **10** to provide a number of treatments. The number of treatments authorized can be based on the amount of payment received. The server system **802** can send the authorization code **814** to the medical device **10** through the network **806** and/or through the cellular network **808**.

The authorization code **814** can be encrypted or encoded so that the authorization code **814** enables treatments only for the particular medical device **10** associated with a particular payment received. In one implementation, the authorization code **814** can be encrypted so that the unique device identifier **812** or another unique decryption key is necessary to decrypt or decode the authorization code **814**. For example, the authorization code **814** can be encrypted using a symmetric-key or asymmetric-key encryption scheme.

Using a symmetric-key or shared-key encryption system, a key may be used as both the encryption and decryption key. The key can be stored on both the server system **802** and the medical device **10**, for example, by the manufacturer of the medical device **10**. To prevent interception, the key may not be transmitted. The medical device **10** can send a patient identifier or a device identifier **812** unrelated to the key to identify the medical device **10**. The server system **802** can send the encrypted data to the medical device **10**, which can decrypt the data with the stored key.

Using an asymmetric-key cryptography system, for example, a public key private key pair encryption system, the server system **802** can store an encryption key and the medical device **10** can store a corresponding decryption key. The server system **802** may encrypt the authorization code **814** using the encryption key and send the encrypted data to the medical device **10**. The medical device **10** can include a stored decryption key that can decrypt the encrypted data. The decryption key can include the device identifier **812** or another key. In an implementation, the encryption key that

encrypts messages for a particular medical device **10** may be known only to the server system **802**.

Because the server system **802** can store records associating patients, medical devices **10**, and corresponding encryption keys, the system **800** may not require that the decryption key be sent to the server system **802**. If the device identifier **812** is used to decrypt an authorization code **814**, instead of sending the device identifier **812**, the medical device **10** can send another identifier, such as a patient identifier or a device identifier unrelated to the encryption scheme. The device identifier **812** can be independent of the encryption scheme so that interception of the device identifier does not compromise the encryption scheme.

The medical device **10** can receive the encrypted authorization code **814** through the network **806** or the cellular network **808** and can decrypt the authorization code **814**. The medical device **10** can use the authorization code **814** to authorize a number of treatments of the medical device **10**. The authorization code **814** or information determined based on the authorization code **814** can be stored to indicate the number of treatments authorized. When the patient attempts to initiate treatment with the medical device **10**, the processing device of the medical device **10** can determine that authorized treatments remain for the medical device **10** and initiate treatment.

The medical device **10** may also use the authorization code **814** to determine a change in treatment. For example, an authorization code **814** may indicate that treatment should be disallowed after a particular period of time has elapsed or if the patient does not apply a treatment for a period of time. The authorization code **814** may indicate that the number of treatments that are available each day should be changed, for example, from one treatment each day to two treatments each day. The authorization code **814** may indicate that the intensity of ultrasound produced by the medical device **10** should be changed, for example, that the intensity should be reduced if the patient is healing well.

Referring to FIG. 9A, a process **900** for authorizing medical treatments can include actions by a medical device, a server system, and/or a third-party system. The medical device can be an ultrasonic treatment device as described above.

As illustrated, the process **900** can include payment for treatment by a patient at the medical device, payment by a third-party at a remote system, or both sources of payment. The actions performed by the medical device can be performed by one or more processing devices of the medical device configured to perform those actions. The server system can include one or more processing devices and one or more storage devices that store instructions that, when executed by the one or more processing devices, cause the processing devices to perform the various functions of the server system described below.

A patient can attempt to initiate treatment with the medical device (**902**). For example, the medical device can receive user input indicating that a treatment should be administered by the medical device.

The medical device can determine whether treatment is authorized (**903**). For example, the medical device can determine whether at least one treatment is authorized based on stored information that indicates the number of treatments that are authorized. The medical device can access an authorization code that has been received, for example, and determine whether treatment is authorized based on the accessed authorization code. The determination whether the attempted treatment is authorized can be performed in response to the attempt to initiate treatment in (**902**).

If the determination indicates that treatment by the medical device is authorized, the medical device can control a treatment module to apply the treatment that the patient attempted. If the determination indicates that treatment is not authorized, the medical device can control the treatment module so that the treatment attempted by the patient is not applied. No treatment may be authorized for a medical device if, for example, all of the previously authorized treatments have already been used or if the medical device has not received an initial authorization code to enable treatments.

When treatment is not authorized for the medical device, the medical device can notify the patient that payment is needed to purchase additional treatments (904). The example illustrated in FIG. 9A shows a scenario in which the medical device is not initially authorized to perform a treatment attempted by a patient, so additional payment and authorization of the medical device is needed.

Payment can be received at the medical device (906). The patient can then enter payment in one or more ways, including entering payment at the medical device using, for example, a credit card or a debit card to purchase additional treatments. The patient may also complete payment at a location other than the medical device, and enter proof of payment at the medical device. The patient may purchase treatments for example, at a store, at a medical office, or over the Internet. The patient may then enter proof of payment at the medical device in the form of, for example, a computer file, a code, or a SIM card.

The medical device can then send payment information for the payment received and an identifier to the server system (908). The identifier may be a device identifier that uniquely identifies the particular medical device used by the patient. In other words, the device identifier can identify not merely a model or type of medical device, but a single, particular medical device. The identifier may be a patient identifier that identifies a particular patient associated with the medical device.

Treatments can also be purchased for a patient by a third-party, for example, an insurance company. The third-party system can receive, for example, a prescription for treatment of the patient using the medical device (910). The third-party system can authorize one or more treatments using the medical device (912). For example, the third-party system can authorize the treatments identified in the received prescription.

The third party system can send payment information and an identifier to the server system (914). The payment information can include information that enables a transaction to occur, for example, an authorization to charge an account or otherwise cause funds to be transferred, and can include information that indicates that payment has been performed. The identifier can identify the patient associated with the prescription that was received in action (910). For example, the identifier can include a name of the patient, an insurance policy number for the patient, a prescription identifier, or other information relating to the patient. The identifier may also identify the medical device for the patient.

The server system can receive payment information and an associated identifier from either the medical device or the third party system (916). The associated identifier can be a device identifier that uniquely identifies the medical device. The server system can match the payment described in the payment information with the patient and the medical device of the patient (918). The server system can store one or more associations between a patient and the medical device configured to apply a medical treatment to the patient. For

example, the server system can store records that associate patients with particular medical devices, patient identifiers, and medical device identifiers.

The server system may use one or more received identifiers to determine which patient and device are associated with a payment. Specifically, the server system can determine that payment has been made for the patient for a particular number of treatments by the medical device. The determination can be made based on the received information that payment has been made for the patient. The server system can identify the medical device associated with the patient based on the stored association between the patient and the medical device and, for example, based on a received device identifier that uniquely identifies the medical device. The server system may also record the determination that payment has been made for the user and the identification of the medical device associated with the patient.

The server system can generate an authorization code that can authorize the medical device associated with the patient to perform the purchased treatments (920). The authorization code can enable the number of treatments purchased by the patient or third-party payer. The authorization code can be generated so that the code only enables treatments of the particular medical device associated with the patient for whom payment was received. For example, the authorization code may be encoded or encrypted so that only the particular medical device associated with the payment can decode or decrypt the authorization code. The authorization code may include or be transmitted with a unique device identifier, and a medical device can be configured to enter an authorization code only when a device identifier of the medical device matches the device identifier received with an authorization code.

The server system can transmit the authorization code to the medical device (922).

The authorization code may be transmitted, for example, over a cellular communication link to the medical device that the server system identified as being associated with the patient.

The medical device can receive the authorization code (924). The authorization code may be a new authorization code that is received after an initial or prior authorization code that authorized different treatments. The new authorization code can be received after the medical device has provided an indication to the patient that more treatments need to be purchased, and the new authorization code can identify a number of additional treatments for which payment has been received.

Referring to FIG. 9B, the medical device can decrypt or decode the authorization code (926). In one implementation, the medical device may decrypt the authorization code using a unique device identifier or decryption key stored on the medical device. The medical device may determine that an authorization code is authentic or intended for the particular medical device that received it. The medical device may determine, using decrypted or decoded data, what treatments are authorized. For example, the medical device may determine that a particular number of treatments are authorized. The medical device may also determine that treatment using the medical device should be modified in some way, for example, that two treatments are authorized each day instead of one treatment each day, or that the intensity of ultrasound produced should be changed.

The medical device can store authorization information (928). For example, the medical device can store the number of treatments that the authorization code indicates should be

authorized. The medical device can also store the authorization code received, the authorization information extracted from the received data, and other authorization information. In some instances, treatments using the medical device can be authorized without any input or action by the patient. For example, when a third-party payer sends payment to the server system, the medical device can be authorized without involvement from the patient.

The medical device can determine whether treatment is authorized (929). For example, the medical device can determine whether treatment is authorized based on the authorization code that was accessed by the medical device. The medical device can determine whether treatment authorized in response to receiving user input that treatment should be provided, in (902) or through later inputs. In the situation that the patient has attempted treatment with the medical device in (902), and subsequently entered payment needed to authorize treatment in (906), the medical device can proceed to apply the treatment after the determination is made that treatment is authorized. For example, the payment and authorization process may occur quickly so that the patient perceives very little delay between entering payment and the initiation of treatment. In one implementation, treatment may begin automatically when the patient has previously attempted to initiate treatment. Treatment may alternatively be delayed until the patient imitates treatment again or confirms that treatment should proceed.

If the determination indicates that treatment is authorized, the medical device can control a driver circuit to apply treatment (930). For example, the medical device may control an ultrasound transducer driver circuit in a manner that causes one or more ultrasound transducers to produce ultrasound with therapeutic properties. For example, the driver circuit can be activated to drive one or more ultrasound transducers. The driver circuit may continue to drive the ultrasound transducers until treatment is complete. Of course, if the determination indicates that treatment is not authorized based on the authorization code (for example, if the authorization code is for a different medical device, or if the treatments authorized by that code have already been expended), the medical device can control the driver circuit so that treatment is not applied, for example, by not activating the driver circuit so that treatment is prevented.

The driver circuit can be deactivated when treatment is finished (932). The medical device can store a record of the treatment applied (934). The medical device can also decrease the number of treatments authorized for the medical device (936). For example, if the medical device had received an authorization code that authorized twenty treatments of the medical device, after one treatment is completed, the medical device may update the number of authorized treatments to reflect that only nineteen treatments are currently authorized for the medical device.

Referring to FIG. 10, an example of a system 1000 for collecting compliance information includes the medical device 10, a server system 1002, and a third-party system, all connected by a network 1008. The medical device 10 and the server system 1002 may, additionally or alternatively, communicate through a cellular network 1009.

The medical device 10 can record use of the medical device 10, for example, by recording the date, time, and duration that treatment occurs using the medical device 10. The recorded use of the medical device 10 can be collected as compliance information 1010. For example, the medical device 10 can collect information about multiple treatments performed or multiple aspects of treatment.

As described above, in some implementations, the medical device 10 may receive information about the treatment regimen for the patient. For example, the treatment regimen may be entered on the device after the health condition has been diagnosed or after the medical device 10 has been prescribed to the patient. The compliance information 1010 may, but is not required to, include one or more results of a comparison between the recorded use of the medical device 10 and the treatment regimen of the patient.

To distinguish the medical device 10 from other medical devices 10, the medical device 10 may store a device identifier 1012 that enables the medical device 10 to be identified. For example, the device identifier 1012 may uniquely identify a particular medical device 10.

The medical device 10 can send the compliance information 1010 to the server system 1002. Compliance information 1010 can be sent automatically, for example, after a predefined number of treatments are performed, after a particular amount of time has elapsed, or after a treatment regimen has been completed. The medical device 10 may send the compliance information 1010 over the network 1008. Additionally, or alternatively, medical device 10 may send the compliance information 1010 over a cellular network 1009. The medical device 10 can also send the device identifier 1012 to the server system 1002 with the compliance information 1010, enabling the server system 1002 to associate the compliance information 1010 with the particular device. In addition to a device identifier, or alternatively, the medical device 10 may send a patient identifier with the compliance information 1010.

The server system 1002 can be configured to receive the compliance information 1010 and the device identifier 1012 from the medical device 10. The server system 1002 can determine a patient identifier using the device identifier 1012. For example, the server system 1002 may store records that associate device identifiers 1012 for multiple medical devices 10 with patient identifiers. The server system 1002 can compare the received device identifier 1012 to stored device identifiers to determine a patient identifier and identify the patient that uses the medical device 10. The server system can store the compliance information 1010 in association with the determined patient identifier.

The server system 1002 can be configured to receive compliance information from multiple medical devices 10 operated by different patients. For example, the server system 1002 may include a compliance database of many patients and information about the prescriptions and medical devices 10 that correspond to each patient. The server system 1002 can receive and record compliance information from each or any of patients or medical devices 10 described in the compliance database. The server system 1002 can add information about additional patients and medical devices 10 to the compliance database records.

The server system 1002 can provide access to the stored compliance information 1010 to one or more parties that have a relationship with the patient. For example, an insurance company for the patient may use the compliance information 1010 to determine whether the patient is using the medical device 10 that the insurance company paid for. A physician or a caretaker of the patient may use compliance information 1010 to determine if the patient is complying with a treatment regimen that has been prescribed. To obtain compliance information 1010 for the patient, a third-party system 1004 may submit an inquiry requesting the compliance information 1010 to the server system 1002. For example, the inquiry 1016 may include one or more patient

identifiers to identify one or more patients. The server system **1002** can provide access to the compliance information **1010** for one or more users in response to receiving the inquiry from the third-party system **1004**.

Because the server system **1002** can store compliance information about multiple patients and multiple medical devices **10**, the server system **1002** can provide aggregate information about multiple patients and medical devices **10**. For example, the server system **1002** may provide an insurance provider with a summary of the treatments performed for all patients covered by the insurance provider. As another example, a physician may receive compliance information for each of his patients from the server system **1002**, without being required to interface with each of the prescribed medical devices **10** individually.

Summaries, reports, graphs, and comparisons can be provided based on compliance data for multiple patients, including, for example, information about a set or subset of patients. For example, the compliance of patients that have a particular health condition can be provided.

Access to the compliance information **1010** can be limited based on the relationship of the third party to the patient. The server system **1002** can store records that associate various third parties with various patients. The third party system **1004** may be required to be authenticated or comply with other security measures before access to compliance information **1010** is provided. Access to compliance information **1010** can also be limited by restricting the quantity or detail of information available. For example, one third party may receive more detailed compliance information **1010** than a different third party may receive for the same patient. For example, an insurance company for the patient may be provided access only to the number of treatments performed with the medical device **10**, but the physician of the patient may be provided access to the particular dates and times that treatments occurred in addition to the total number of treatments.

The medical device **10** can also detect and record information about errors of the medical device **10**. During treatment or during other operation of the medical device **10**, one or more errors may occur. The medical device can store information about the errors as error information **1014**, and can send the error information **1014** to the server system **1002** with the device identifier **1012**. In one implementation, error information **1014** can be sent soon after the error is detected. Examples of errors that can be detected, and for which information can be recorded and sent, include a gel error indicating that there is insufficient ultrasound conductive gel on a transducer, a battery error that indicates that remaining power of the battery is low, and a connectivity error that indicates that a wire to a transducer is disconnected or broken.

The server system **1002** can be configured to receive the error information **1014** and the device identifier **1012**. The server system **1002** can store the received error information **1014** and can associate error information **1014** with the device identifier **1012**. The received error information **1014** may quickly and accurately indicate which medical devices **10** and which types of medical devices **10** experience errors and at what frequency errors occur.

The received error information may also enable the server system **1002** to provide information to the medical device **10** to address the errors. For example, the server system **1002** may use error information **1014** to determine a possible cause of an error. The server system **1002** may select service information **1018** that addresses the error. For example, the server system **1002** may select information to store on the

medical device **10**, which may include information to restore or replace outdated or incorrect information. The server system **1002** may select control instructions to be executed on the medical device **10**, for example, control instructions to clear an error or to reinitialize the medical device **10**. The server system **1002** can send the selected service information **1018** that addresses one or more errors to the medical device **10**. The service information **1018** can include, for example, software or firmware updates, instructions to the user of the medical device **10**, instructions to trained service personnel, and/or control instructions to alter the functioning of the medical device **10** and modules coupled to the medical device **10**.

The medical device **10** can send information including one or more messages **304** to the medical device **10**. The messages **304** may be stored on the medical device **10** and displayed to the patient during treatment. The messages **304** can include updated information or additional information to add to the variety of messages **304** already stored on the medical device **10**. In addition, one or more messages **304** can be provided to instruct the patient how to correct an error of the medical device **10**, or to inform the patient that an error has been corrected.

Referring to FIG. **11**, a medical device **10** may collect and send information as illustrated in the process **1100**. The processing device **50** of the medical device **10** may, for example, execute instructions stored on the storage device **52** to perform the process **1100**.

A driver circuit is controlled to produce ultrasound with therapeutic properties (**1102**).

Compliance information is collected (**1104**). Collecting compliance information can include recording information about use of the medical device, for example recording the number of treatments that are performed. Compliance information can include a number of treatments provided by the medical device, a date and time that a treatment was provided by the medical device, and/or a duration that a treatment was provided by the medical device. Information about multiple uses or treatments with the medical device can be collected.

A treatment regimen that identifies a prescribed use of the medical device can be identified. For example, information about a treatment regimen may be entered on the medical device or received from a network, which may include a cellular network. The information about the recorded use of the medical device can be compared to the information about the prescribed use of the medical. Information indicating the degree that the recorded use matches the prescribed use can be generated.

A device identifier can be accessed (**1106**). The device identifier can be stored on the medical device. The compliance information can be sent (**1108**). The accessed device identifier can be sent with the compliance information. For example, the compliance information can be sent to a server system configured to receive the compliance information. Compliance information can be sent automatically after a predetermined number of treatments have been performed. Compliance information may be sent using a wireless module, and the wireless module can include a cellular transceiver. For example, compliance information may be sent to a server system over a cellular network using the cellular transceiver. The medical device can include a SIM card that associates a particular telephone number with the medical device.

One or more errors of the medical device can be detected. Information about the detected errors can be sent with the

31

accessed device identifier to a server system. Service information to address the detected errors can be received from the server system.

Referring to FIG. 12, a server system can process information according to the illustrated process 1200. For example, one or more storage devices can store instructions that, when executed by one or more processing devices, cause the server system to perform the process 1200.

Compliance information can be received (1202). For example, compliance information can be received over a network or cellular network from one or more medical devices. Compliance information for multiple medical devices operated by different patients can be received. For example, the server system may be configured to receive compliance information from each of a plurality of patients, and each patient can be associated with at least one of a plurality of medical devices. The compliance information can include a number of treatments provided by a medical device, a date and time that a treatment was provided by the medical device, and/or a duration that a treatment was provided by the medical device. Compliance information can be received for multiple medical devices operated by different patients.

A device identifier can be received (1204). The device identifier can be received with the compliance information. A patient identifier can be determined (1206). For example, the received device identifier can be used to determine the patient identifier. The server system can store records that associate device identifiers with one or more patient identifiers. The recorded device identifiers can be compared to the received device identifier to determine a recorded device identifier that matches the received device identifier.

The compliance information can be stored (1208). The compliance information can be stored in association with the patient identifier that was determined to correspond to the compliance information. For example, the server system may be configured to store compliance information for each of a plurality of patients, and each patient can be associated with at least one of a plurality of medical devices. Compliance information for each patient can be stored in association with one or more device identifiers and/or patient identifiers.

Access to the compliance information can be provided (1210). For example, access may be provided to one or more users of the server system. Users may submit an inquiry to the server system, and the inquiry can be associated with a patient identifier. Users can include, for example, one or more of a representative of an insurance provider of the patient, a physician of the patient, and a caretaker of the patient. Access to the compliance information for a particular patient can be provided to the users in response to receiving the inquiry that is associated with the patient identifier for the particular patient. Access to the compliance information can be limited based on the relationship of the user to the patient.

For example, a physician of the patient may receive access to only a portion of the compliance information, such as only the number of times the medical device was used. A physician, on the other hand, may receive access to more detailed compliance information, such as the date, time, and duration that the medical device was used.

Because compliance information for multiple patients and multiple medical devices can be stored, access to compliance information for multiple patients and multiple medical devices can be provided. For example, compliance information can be provided to a third party for treatment performed by multiple medical devices operated by multiple patients.

32

Users that can receive access to the compliance information can include, for example, one or more caretakers, physicians, and representatives of insurance providers for any of the multiple patients whose compliance information is stored. Access can be provided to compliance information for each of a plurality of patients, where each patient is associated with at least one of a plurality of medical devices. Access to the compliance information for a particular patient can be provided to the users in response to receiving the inquiry that is associated with the patient identifier for the particular patient.

Information about one or more errors of the medical device can be received. Based on the information about the errors, service information to address the errors can be selected and transmitted to the medical device. One or more messages for the patient can be transmitted to the medical device.

Referring to FIG. 13, a process 1300 for storing patient information can begin with a physician writing a prescription for a patient for treatment using a medical device (1302). To carry out the prescribed treatment, a medical device can be dispensed to the patient (1304). The medical device can be authorized at the time the medical device is dispensed or at a later time.

Records for the patient and the dispensed medical device can be entered into a database 1314 (1306). For example, the database 1314 may store a patient record 1310 that associates a particular medical device or treatment with a particular patient, in the example, a patient named "John Smith." The database 1314 may also store a prescription record 1312 that indicates the number of treatments that can be purchased for the patient. The number of treatments indicated in a prescription record 1312 may be authorized for application by the medical device after payment has been received for the prescribed treatments. For example, the treatments can be enabled after a third-party payer agrees to pay for the treatments or after the patient enters payment at the medical device. The database 1314 may also store other records including records that identify patient identifiers and medical device identifiers. The information in the database can be accessed by one or more client devices 1318, 1320, a server system 1322, or other systems. For example, the server system 1322 may use the patient record 1310 to match payment to a particular medical device or patient. The records stored in the database 1314 may also be used to inform a third-party payer or patient the number of treatments that should be purchased to enable a treatment plan to be carried out.

Referring to FIG. 14, the authorized use of the medical device 10 can be limited to a particular patient and/or geographic area. In some instances, it is desirable by an automated method to limit the use of a medical device by an unauthorized person or in an unauthorized geographic area, such as in a country where the device has not received regulatory approval or in which an unauthorized sale of the device circumvents the chain of distribution of the device. Other examples where "geolocking" of a medical device may be desirable is where devices are sold at different price points in different regions and it is desirable to limit the ability of a lower priced device to be sold in a higher priced region, where device have region specific chargers, include specific languages, or are designed for single patient use or multiple patient use such as in some hospitals.

It is also desirable to limit a single patient use device from being shared with other than the intended patient by, for example, resale or shared use with friends or family members, particularly where the device is a prescription device.

The desire to limit such use is particularly applicable to medical devices such as the Exogen™ Ultrasound Bone Healing System sold by Smith & Nephew, Inc. that is easily transported.

To limit, and preferably prevent, the use of a medical device **10** (FIG. **14**) in an unauthorized geographic area, the medical device **10** includes hardware and software that determine the geographical location of the medical device **10** upon start-up and compare the determined geographical location to an authorized geographical location. The authorized geographical location can be, for example, programmed in the medical device **10** during the manufacturing process. Referring to FIG. **15**, the medical device **10** include a GPS receiver **1510** to determine geographical location, and memory **1514** to store authorized operating areas for the medical device **10**. Alternatively, the medical device **10** can use cell phone networks or Wi-Fi to determine geographical location.

Referring to FIG. **16**, the location of the medical device **10** is compared to an approved area **1618** in which treatment is authorized. If the geographical location **1620** of the device **10** is within the authorized area **1618**, treatment begins. If the geographical location **1622** of the device **10** is in an unauthorized area **1624**, no treatment is delivered. The device can include two-way communication, such as cellular, internet or wireless communication. To accommodate patient travel, the medical device **10** can be configured to accept over-the-air-updates to the authorized geographical location.

As illustrated in FIG. **17**, for “geolocking” purposes, the medical device **10** includes the GPS receiver **1712**, an antenna **1730** connected to the GPS receiver **1712** via an amplifier **1732** and a filter **1734**, and a crystal **1736**, an integrated circuit **1738**, and a regulator **1740**.

Advantageously, a medical device can be designed for use within only a specific geographical area, for example, a country or region as illustrated in FIG. **16**, such that use of the device in unintended markets is limited or prevented.

To limit, and preferably prevent, the use of the medical device **10** by an unauthorized person, the medical device **10** requires proof of patient identity using, for example, a key card or token issued to the user, a password, or physical evidence. For example, referring to FIG. **2**, the medical device **10** includes hardware and software and a user interface **70** implemented on the device to identify the patient using a fingerprint, retinal scan, or voice recognition.

The identity of the user is compared to the stored patient identity and treatment is only authorized when the user is confirmed to be the patient.

As illustrated in FIG. **18**, for device authorization purposes, the medical device **10** includes, for example, a fingerprint sensor **1852**, control electronics such as an integrated circuit **1854**, and an EPROM **1856**.

Advantageously, the use of a fingerprint, retinal scan, or voice recognition ensures that the patient is at least present during the treatment. In situations where the patient is, for example, young or elderly, the identity of a supervising individual can alternatively or additionally be required. The fingerprint, voice or retinal scan of the authorized user is saved into the memory of the device when the device is prescribed and fitted by a responsible party, for example, a doctor, pharmacist or sales representative.

Referring to FIG. **19**, a method for limiting unauthorized use of the medical device **10** includes determining the geographic location of the medical device **10** and not allowing treatment to commence if the determined geographic location is outside an authorized geographic loca-

tion, and/or includes determining user identity and not allowing treatment to commence if the determined user identity does not match an authorized identity. The medical device **10** includes means for determining the geographic location of the medical device **10** and means for determining user identity. Treatment is not allowed to commence if either the determined geographic location is outside an authorized geographic location or the determined user identity does not match an authorized identity.

In use, the patient turns the device **10** on at step **1960**, the device performs a self-test of the clock and configuration at step **1962**, the patient, for example, scans his or her index finger over the fingerprint sensor **1852**, and the device confirms the patient identity at step **1964**. If the patient is the authorized user, the geographical location of the device is checked at step **1966**. If the patient is not the authorized user, an authorization alarm is delivered at step **1968** and treatment will not commence. If the patient is the authorized user and the device **10** is within its authorized geographical location treatment can be started at step **1970**. If the device **10** is not within its authorized geographical location, an authorization alarm is delivered at step **1968** and treatment will not commence.

At steps **1972**, **1974** and **1976**, the device **10** monitors the time of use, allowing up to 20 minutes of treatment to be delivered before ending treatment.

Referring to FIG. **20**, an inventory tracking and medical device activation system **2000** can be used to control the distribution of medical devices **10**. The system **2000** includes an enabling device **2010** that communicates with the medical device **10**. The enabling device **2010** also communicates with a server **2020** over a network **2030**.

Each medical device **10** can be provided to a distributor or physician in a disabled or deactivated state. For example, the medical device **10** can be provided in a state in which no treatments are authorized. Additionally, the medical device **10** can be provided in a state in which treatments cannot be purchased or authorized, until the medical device **10** is activated and thus made operative by an enabling device. Because the medical devices **10** are shipped and stored in inventory in an inoperative state, the potential for unauthorized use is very low.

The enabling device **2010** includes the capability to activate medical devices **10**. For example, the enabling device **2010** can include an activation module including a wireless or wired communication system to transmit activation information. The server **2020**, however, can limit the enabling device **2010**. For example, the server **2020** can authorize the enabling device **2010** to activate only a limited number of medical devices **10**. The total number of medical device activations that the enabling device can be performed can be limited (e.g., no more than 10 activations, until further authorization is received). Additionally, or alternatively, the number of activations that can be performed over a particular period of time can be limited (e.g., no more than 10 activations per month). As described in further detail below, the server **2020** can limit the number of medical device activations that the enabling device **2010** can perform so that, at any given time, the enabling device **2010** is authorized to perform a number of medical device activations no greater than the number of medical devices in a particular inventory **2013** of a particular sales representative **2012**. The enabling device **2010** is associated with the sales representative **2012**, and a unique identifier for the enabling device **2010** or for the representative **2012** associates the enabling device **2010** with the inventory **2013** of the representative **2012**.

35

The server **2020** tracks the inventories of multiple representatives. The server **2020** can identify changes in inventories using information from reliable sources, for example, information that is verifiable or outside the control of the representatives. For example, the server **2020** receives information from manufacturers or distributors of medical devices about shipments of products to the representatives.

Based on the inventory **2013** for the representative **2012**, the server **2020** adjusts the ability of the enabling device **2010** to activate medical devices **10**. For example, the server **2020** authorizes the enabling device **2010** to activate as many medical devices **10** as are in the official inventory **2013** for the representative **2012**. For example, when the medical devices **10** are shipped to the representative **2012**, the server **2020** receives information about the shipment **2014** from the manufacturer or distributor. In response to determining that the inventory **2013** for the representative **2012** has increased, the server **2020** transmits to the representative's enabling device **2010** an authorization code **2022** permitting a number of medical device **10** activations corresponding to the size of the shipment **2014**. If twenty medical devices **10** are shipped to the representative **2012**, the server **2020** sends an authorization code **2022** permitting the enabling device **2010** to activate up to twenty medical devices **10**.

When the medical device **10** is purchased or dispensed to a patient, the sales representative **2012** can activate the medical device **10** using the enabling device **2010**. The enabling device **2010** communicates with the medical device **10** over a wired link or a wireless link, such as Bluetooth. For example, the enabling device **2010** supplies an activation code **2024** to the medical device **10** that unlocks the functionality of the medical device **10**. The enabling device **2010** can also supply an authorization code **2026** that authorizes a particular number of treatments to be performed with the medical device **10**. The activation code **2024** and the authorization code **2026** can be combined in a single message or code. After the medical device **10** receives the activation code **2024**, the medical device **10** determines whether the activation code **2024** is valid to activate the medical device **10** and/or one or more of its treatment modules. In response to determining that the activation code **2024** is valid, the medical device **10** may send an activation confirmation message (not shown) to the enabling device **2010** to indicate that activation was successful.

After the enabling device **2010** activates the medical device **10**, the enabling device **2010** automatically decreases the number of activations that the enabling device **2010** can provide. For example, the number of activations permitted is decreased by one, from twenty to nineteen. The number of activations can be decreased in response to receiving the activation confirmation message from the medical device **10** so that the number is decreased only after successful activation attempts.

Once the activations allowed by the authorization code **2022** are exhausted, the enabling device **2010** is restricted from activating additional medical devices **10**. The representative **2012** is thus restricted from activating medical devices **10** beyond those legitimately in the representative's inventory **2013**. When a new shipment of medical devices **10** is sent to the representative **2012**, the server **2020** transmits a new authorization code that permits the enabling device **2010** to activate the medical devices **10** in the new shipment.

In some implementations, the server **2020** can also communicate with the enabling device **2010** to reduce the number of activations allowed, for example, if the inventory

36

2013 of the representative **2012** decreases due to returning unused medical devices to the manufacturer. Accordingly, the number of activations that can be provided by the enabling device **2010** is maintained according to the current inventory **2013** of the representative **2012**.

In some implementations, the enabling device **2010** sends a message **2028** to the server **2020** that indicates when an activation of a medical device **10** has occurred, allowing the server **2020** to monitor activations. The remaining number of activations currently allowed by the enabling device **2010** can also be included in the message **2028**.

In some implementations, after the medical device **10** expends all of the treatments authorized by the authorization code **2026**, a second authorization code can be received to permit additional treatments to be performed. As described above, the second authorization code can be received in response to payment by a patient or a patient's insurance provider. The second authorization code can be received, for example, over the network **2030**, from the enabling device **2010**, or from a removable medium.

By contrast, in some implementations, the medical device **10** returns to an inoperative, deactivated state after the treatments authorized by the authorization code **2026** are exhausted. Thus the medical device **10** must be activated with an activation code from the enabling device **2010** before further treatments are permitted.

The medical device **10** can be configured to transmit information indicating usage of the medical device **10**, including compliance with a treatment regimen, to the enabling device **2010** over the same communication link used to receive the activation code. Thus, as part of the exchange, the medical device **10** receives a new activation code from the enabling device **2010**, and the enabling device **2010** receives usage information from the medical device **10**. The enabling device **2010** can then transmit the usage information to the server **2020**, with identifiers to identify, for example, the patient, prescription, and medical device **10** associated with the usage information.

In some implementations, rather than being enabled by a transmission of an activation code from an enabling device, a medical device can be activated by a code accessed from a removable medium, such as an SD memory card.

Referring to FIG. 21, the system **2000** can also control medical device activations and treatment authorizations based on prescriptions and insurance payment authorizations. For example, the enabling device **2010** can be limited to activating a medical device when a valid prescription for the medical device is received, or when an insurance company authorizes payment for a prescribed medical device.

The enabling device **2010** can be configured to require an authorization code before performing each activation. Each time a medical device is activated, a new authorization code is required. The server **2020** provides authorization codes over the network **2030**. The server **2020** can provide an authorization code allowing the activation of a single medical device based on a particular prescription for the medical device. If no prescription is submitted to the server **2020**, the server **2020** does not send an authorization code to the enabling device **2010**, and the enabling device **2010** is unable to activate medical devices.

For example, after a physician issues a prescription for treatment using the medical device **10**, the prescription can be entered on the enabling device **2010**, which transmits identifying information **2115** identifying the prescription to the server **2020**. For example, the enabling device **2010** transmits a representative identifier and a prescription identifier in the identifying information **2115**. The identifying

information **2115** may be additionally or alternatively transmitted by the medical device **10**, a physician's computer system, an insurance company computer system, or other system. In some implementations, the identifying information **2115** can identify the prescription, the patient receiving the prescription, the doctor or office issuing the prescription, an insurance company for the patient, an insurance policy for the patient, the representative **2012**, the medical device **10** to be activated, and/or the enabling device **2010**, and the information can be stored by the server **2020**.

The server **2020** verifies the prescription information, for example, by comparing the prescription information to other prescription records or by verifying an authentication signature in the received information. The server **2020** can also communicate with another server system **2110**, such as a server for an insurance company of the patient, to determine whether payment has been authorized for the prescription.

If the prescription is determined to be valid, and/or if payment has been authorized, the server **2020** transmits an authorization code **2120** to the enabling device **2010**. The authorization code **2120** permits the enabling device **2010** to activate a single medical device **10** for the patient and prescription that were verified. The enabling device **2010** transmits an activation code **2124** to the medical device **10**. The enabling device **2010** also transmits an authorization code **2126** to the medical device **10**, permitting the medical device **10** to apply the number of treatments indicated in the prescription, or the number of treatments for which payment was authorized by the insurance company.

The enabling device **2010** can transmit information to the server **2020** indicating that the activation of the medical device **10** was performed. Based on the initial identifying information **2115** and/or information received subsequent to the activation, the server **2020** can record the transaction identifying, for example, the patient, the prescription, the medical device **10**, the representative **2012**, the enabling device **2010**, and the authorization code **2120** associated with the activation.

When no prescription is submitted to the server **2020**, the server **2020** does not send an authorization code to the enabling device **2010**, and the enabling device **2010** cannot activate the medical device **10**. Similarly, if the prescription information sent to the server **2020** is invalid or is not verifiable, or if payment is refused by an insurance provider, the server **2020** can withhold the authorization code, disallowing the activation of the medical device **10**.

In a similar manner, the system **2000** can be used to track and/or evaluate passes for unpaid treatments. In some implementations, the enabling device **2010** can be authorized to provide a limited number of complimentary medical device activations or treatment authorizations for previously activated medical devices **10**. Each time a pass is provided, the enabling device **2010** transmits information to the server **2020** identifying, for example, the physician, representative **2012**, medical device **10**, and insurance provider associated with the pass. The information may also identify the patient and prescription associated with the pass. The server **2020** can thus maintain a database tracking the issuance of complimentary passes for different representatives **2012**, physicians, and insurance providers.

In some implementations, the enabling device **2010** can be limited to providing passes when the server **2020** provides authorization for each pass individually. For example, the server **2020** can evaluate the circumstances of a particular patient and a particular prescription to determine whether the patient qualifies for complimentary or reduced cost treatment.

The enabling device **2010** transmits a request to the server **2020** that indicates the circumstances of the desired pass. The request can indicate, for example, the medical condition to be treated, the identity of the patient, an associated prescription, the patient's income or other financial status, whether and to what degree treatment is covered by insurance, and what insurance provider covers the treatment. The request can also identify the physician, representative **2012**, enabling device **2010**, and medical device **10** associated with the request.

The server **2020** receives and evaluates the request for the pass. For example, the server **2020** uses the information in the request to evaluate the patient's medical needs, economic circumstances, and other circumstances to determine whether to authorize the activation and treatment authorization of a medical device for the patient. If the patient's circumstances meet the criteria for complimentary treatment, the server **2020** sends an authorization code to the enabling device **2010** permitting the enabling device **2010** to provide a pass for the particular patient. If the patient does not qualify for a pass, the server system **2020** withholds the authorization code necessary to activate a medical device or authorize additional treatments for the medical device. The server **2020** can record each request for a pass, each pass granted, and activations and treatments that occur based on the pass.

The techniques described above are not limited to any particular hardware or software configuration. Rather, they may be implemented using hardware, software, or a combination of both. The methods and processes described may be implemented as computer programs that are executed on programmable computers comprising at least one processor and at least one data storage system. The programs may be implemented in a high-level programming language and may also be implemented in assembly or other lower level languages, if desired.

Any such program will typically be stored on a computer-usable storage medium or device (e.g., CD-ROM, RAM, or magnetic disk). When read into the processor of the computer and executed, the instructions of the program cause the programmable computer to carry out the various operations described above.

A number of implementations have been described. Nevertheless, it will be understood that various modifications may be made. For example, the described features of presentation of messages selected for a particular patient, the collection and display of compliance information, and treatment authorization, and medical device locking based on identity or geographical location may be implemented for a single medical device. In addition, any subset of the features described can be implemented. Each of the message presentation, compliance information collection and display, treatment authorization, and medical device locking features may be implemented individually, separate from the other features described, or together in any combination.

Accordingly, other implementations are within the scope of the following claims.

The invention claimed is:

1. A method of operating a medical therapy system, the method comprising:
 - by a medical therapy device that includes electronic processing circuitry:
 - causing provision of a therapy to a wound of a patient;
 - generating a compliance data reflecting a degree to which a duration of provision of the therapy has complied with a therapy prescription; and

39

communicating the compliance data to one or more remote computing device; and

by the one or more remote computing devices that include at least one processor:

at a first time:

determining that the compliance data does not satisfy a compliance threshold; and

responsive to determining that the compliance data does not satisfy the compliance threshold, causing provision of an indication that the compliance data does not satisfy the compliance threshold.

2. The method of claim 1, wherein provision of the indication is performed on a user interface of the medical therapy device.

3. The method of claim 1, wherein the indication is provided to the patient via a cellular network.

4. The method of claim 1, further comprising, by the one or more remote computing devices:

receiving the therapy prescription from a physician; and

transmitting the therapy prescription to the medical therapy device.

5. The method of claim 4, wherein receiving the therapy prescription from the physician is responsive to the physician diagnosing the patient with a particular health condition.

6. The method of claim 4, further comprising, by the medical therapy device, activating provision of the therapy to the wound of the patient in response to receiving the therapy prescription, wherein provision of the therapy is performed according to the therapy prescription.

7. The method of claim 1, further comprising, by the one or more remote computing devices, transmitting an indication to the patient to contact a physician of the patient.

8. The method of claim 1, wherein the compliance threshold comprises 80%.

9. A medical therapy system comprising:

a medical therapy device including:

a driving circuitry configured to cause provision of a therapy to a wound of a patient;

a transmission circuitry configured to transmit data to one or more remote computing devices; and

an electronic processing circuitry configured to:

generate a compliance data reflecting a degree to which a duration of provision of the therapy has complied with a therapy prescription; and

cause the transmission circuitry to communicate the compliance data to the one or more remote computing devices; and

the one or more remote computing devices including at least one processor configured to:

responsive to a determination that the compliance data does not satisfy a compliance threshold, cause provision of an indication that the compliance data does not satisfy the compliance threshold.

10. The medical therapy system of claim 9, wherein the medical therapy device further comprises a user interface, and wherein the indication is provided to the patient via the user interface.

40

11. The medical therapy system of claim 9, wherein the indication is provided by the electronic processing circuitry responsive to a communication received from the one or more remote computing devices.

12. The medical therapy system of claim 9, wherein the indication is provided to the patient via a cellular network.

13. The medical therapy system of claim 9, wherein the one or more remote computing devices are further configured to:

receive the therapy prescription from a physician; and

transmit the therapy prescription to the transmission circuitry.

14. The medical therapy system of claim 13, wherein receipt of the therapy prescription from the physician is responsive to the physician diagnosing the patient with a particular health condition.

15. The medical therapy system of claim 13, wherein the electronic processing circuitry is further configured to activate provision of the therapy to the wound of the patient in response to receipt of the therapy prescription, and wherein provision of the therapy is performed according to the therapy prescription.

16. The medical therapy system of claim 9, wherein the one or more remote computing devices are further configured to transmit an indication to the patient to contact a physician of the patient.

17. The medical therapy system of claim 9, wherein the compliance threshold comprises 80%.

18. The medical therapy system of claim 9, wherein the medical therapy device comprises an ambulatory medical device.

19. The medical therapy system of claim 10, wherein the at least one processor of the one or more remote computing devices is further configured to:

responsive to the determination that the compliance data does not satisfy the compliance threshold, cause the medical therapy device to provide the indication as a first graphical object on the user interface; and

responsive to a determination that the compliance data satisfies the compliance threshold, cause the medical therapy device to provide an indication that the compliance data satisfies the compliance threshold as a second graphical object on the user interface.

20. The method of claim 1, further comprising, by the one or more remote computing devices:

at the first time:

causing the medical therapy device to provide the indication as a first graphical object on a user interface of the medical therapy device; and

at a second time:

determine that the compliance data satisfies the compliance threshold; and

responsive to determining that the compliance data satisfies the compliance threshold, causing the medical therapy device to provide an indication that the compliance data satisfies the compliance threshold as a second graphical object on the user interface.

* * * * *