



US0D1091829S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,091,829 S**
Kurihara et al. (45) **Date of Patent:** **** Sep. 2, 2025**

(54) **COMPUTING DEVICE FOR A SURGICAL SYSTEM**

wordpress.com/wp-content/uploads/2016/06/davinci-si-system-users-manual.pdf (Year: 2012).*

(Continued)

(71) Applicant: **Verb Surgical Inc.**, Santa Clara, CA (US)

Primary Examiner — Jennifer L Rempfer

Assistant Examiner — Edward P Jones

(72) Inventors: **Junnosuke Kurihara**, Milpitas, CA (US); **Berk Gonenc**, San Jose, CA (US); **Bernhard A. Fuerst**, Munich (DE); **Benjamin A. Sanker**, San Jose, CA (US); **Rose Y. Huang**, Quincy, MA (US)

(74) *Attorney, Agent, or Firm* — FROST BROWN TODD LLP

(73) Assignee: **VERB SURGICAL INC.**, Santa Clara (CA)

The ornamental design for a computing device for a surgical system as shown and described.

(**) Term: **15 Years**

(21) Appl. No.: **29/810,313**

(22) Filed: **Oct. 4, 2021**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search**
USPC D24/186, 107, 138, 144, 158, 160, 170, D24/185, 231–232, 216

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D567,381 S * 4/2008 Olivera D24/185
D687,023 S * 7/2013 Jung D14/242

(Continued)

FOREIGN PATENT DOCUMENTS

IN 361626-001 * 6/2022
JP D1752323 * 9/2023
KR 3012011800004 * 1/2023

OTHER PUBLICATIONS

Intuitive Surgical, da Vinci Si User Manual, Published: 2012; mercyor.wordpress.com, Retrieved from Internet: <https://mercyor.wordpress.com/wp-content/uploads/2016/06/davinci-si-system-users-manual.pdf> (Year: 2012).*

DESCRIPTION

FIG. 1 is a front top perspective view of a computing device for a surgical system, showing our new design;

FIG. 2 is a rear top perspective view of the computing device for a surgical system of FIG. 1;

FIG. 3 is a front bottom perspective view of the computing device for a surgical system of FIG. 1;

FIG. 4 is a front elevational view of the computing device for a surgical system of FIG. 1;

FIG. 5 is a rear elevational view of the computing device for a surgical system of FIG. 1;

FIG. 6 is a side elevational view of the computing device for a surgical system of FIG. 1;


FIG. 7 is a side elevational view of the computing device for a surgical system of FIG. 1, the side elevational view of FIG. 7 being opposite to the side elevational view of FIG. 6;

FIG. 8 is a top plan view of the computing device for a surgical system of FIG. 1; and,

FIG. 9 is a bottom plan view of the computing device for a surgical system of FIG. 1.

The evenly-spaced broken lines in the drawings are included for purpose of illustrating portions of the computing device for a surgical system that form no part of the claimed design. The dot-dash-dot broken lines in the drawings are included for the purpose of defining the boundary of the claim, it being understood that the region between the dot-dash-dot

(Continued)

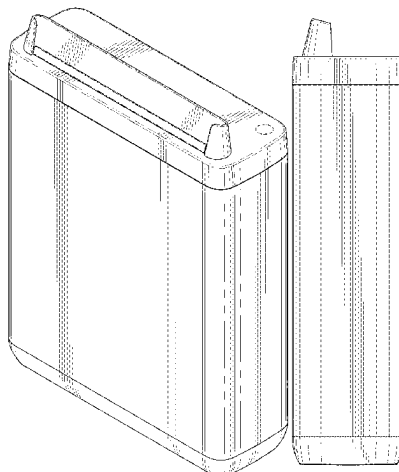

broken lines and the dot-dash-dot broken lines themselves
form no part of the claimed design.

1 Claim, 7 Drawing Sheets

(58) Field of Classification Search

CPC ... A61B 2034/101; A61B 34/00; A61B 34/10;
A61B 34/101; A61B 34/30; A61B 34/32;
A61B 34/37

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D689,195	S *	9/2013	Nelsen		D24/232
D748,803	S *	2/2016	Zhang		D24/170
D837,380	S *	1/2019	Hulford		D24/185
D861,167	S *	9/2019	Emery		D24/158
D877,140	S *	3/2020	Little		D14/314
D902,412	S *	11/2020	Angeles		D24/185

D976,257	S *	1/2023	Zhang		D14/363
D981,570	S *	3/2023	Shi		D24/185
D1,010,090	S *	1/2024	Campbell		D23/365
D1,056,896	S *	1/2025	Villar		D14/314
D1,062,720	S *	2/2025	Wu		D14/314
2017/0290704	A1 *	10/2017	Mercado		A61F 9/00736
2020/0316778	A1 *	10/2020	Desai		G16H 20/40
2024/0407869	A1 *	12/2024	Troxell		A61B 17/1655

OTHER PUBLICATIONS

Hale, Trans Enterix nets FDA clearance for AI vision-guided surgery, Fierce Biotech, Published: Mar. 13, 2020, fiercebiotech.com, Retrieved from Internet: <https://www.fiercebiotech.com/medtech/transenterix-nets-fda-clearance-for-ai-vision-guided-surgery> (Year: 2020).*

Pedersen, Leading Robotic Surgeon Spills the Tea on Medtronic's Hugo, Published: Oct. 6, 2022, mddionline.com, Retrieved from Internet: <https://www.mddionline.com/robotics/leading-robotic-surgeon-spills-the-tea-on-medtronic-s-hugo> (Year: 2022).*

* cited by examiner

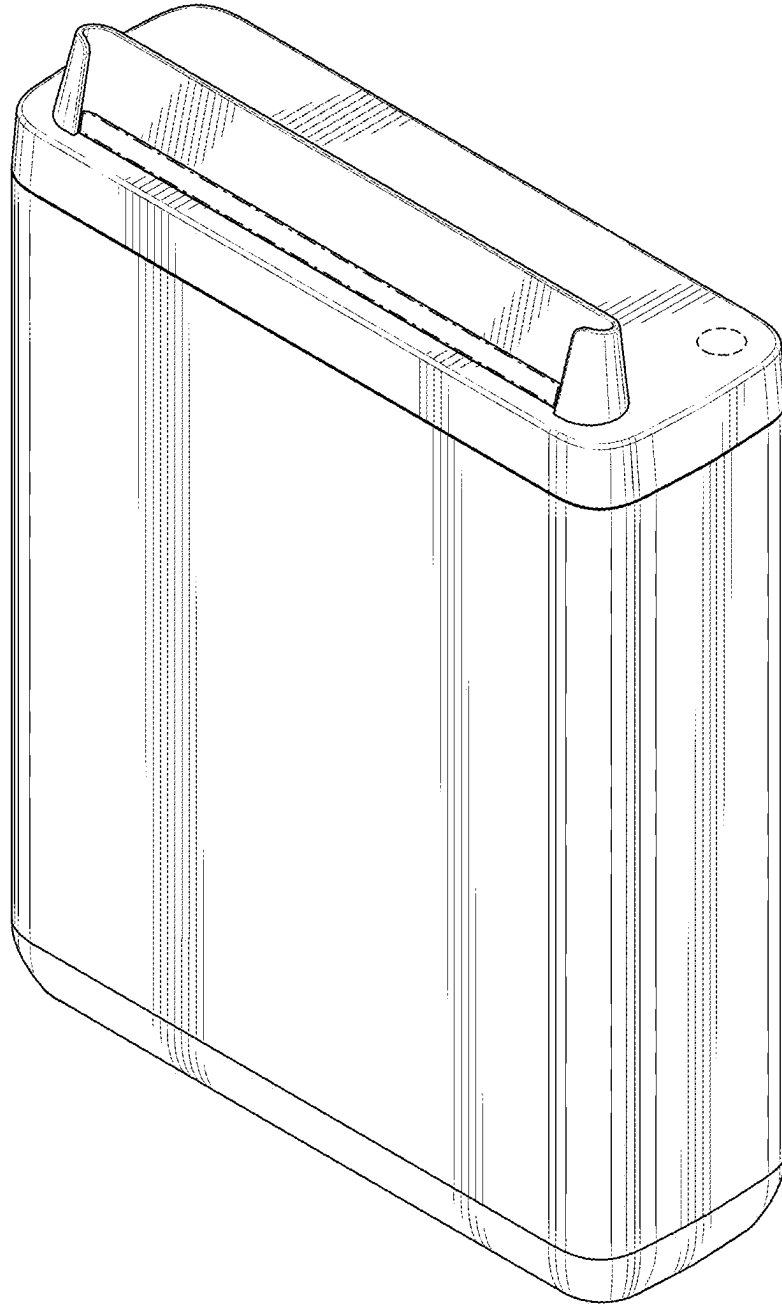


FIG. 1

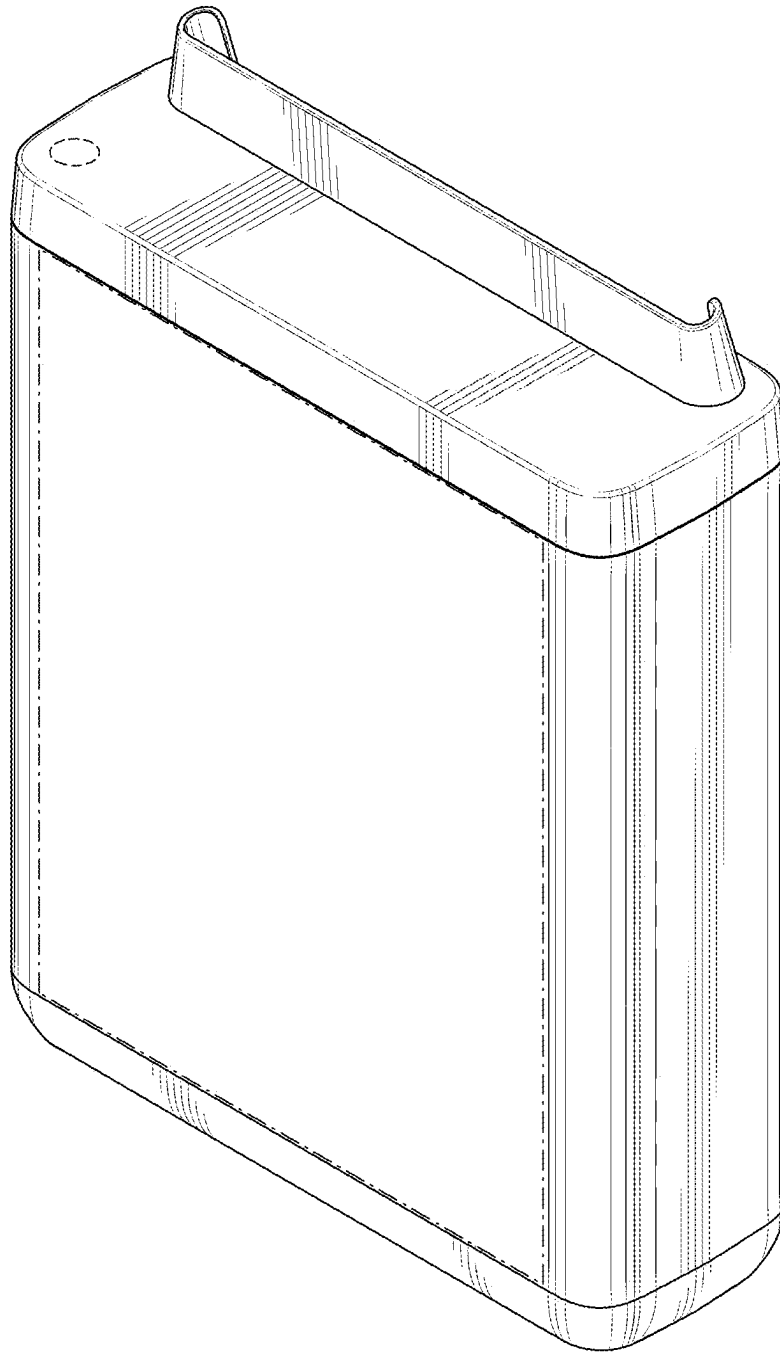


FIG. 2

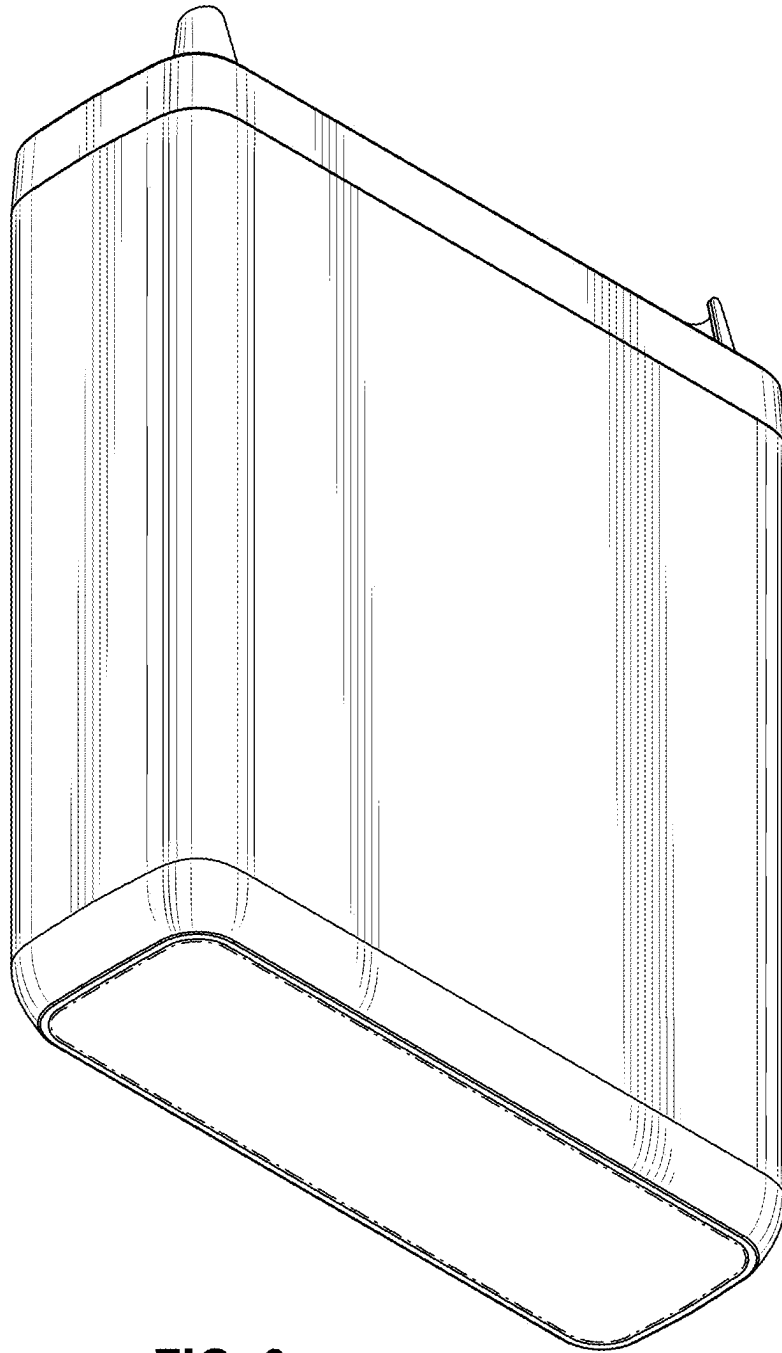


FIG. 3

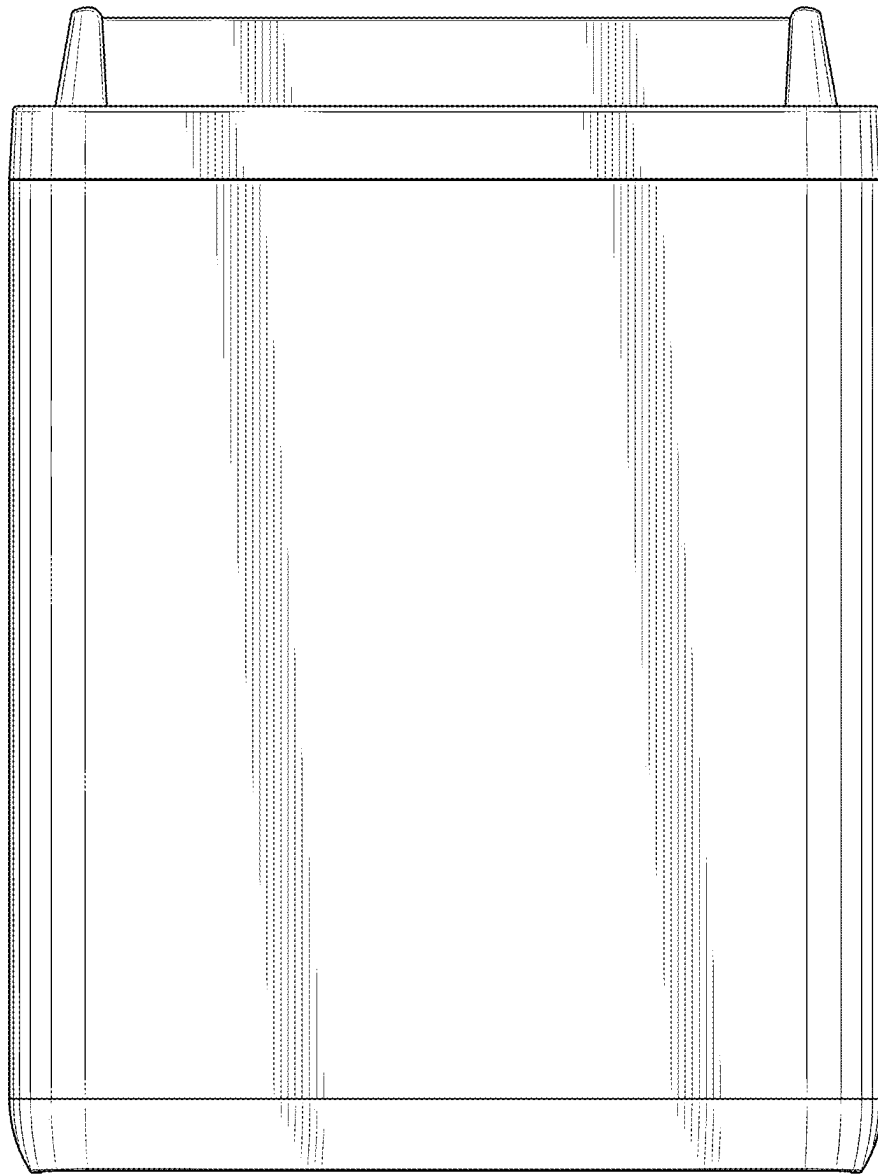


FIG. 4

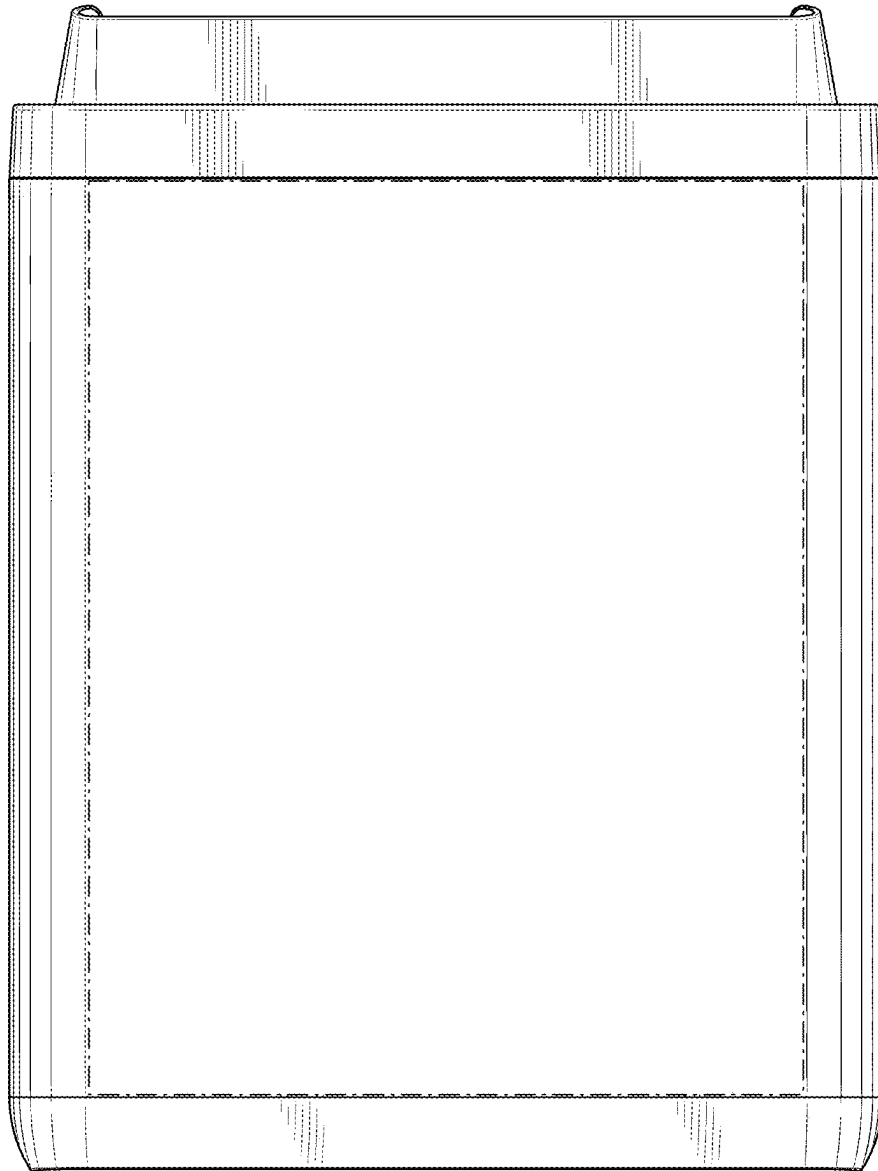


FIG. 5

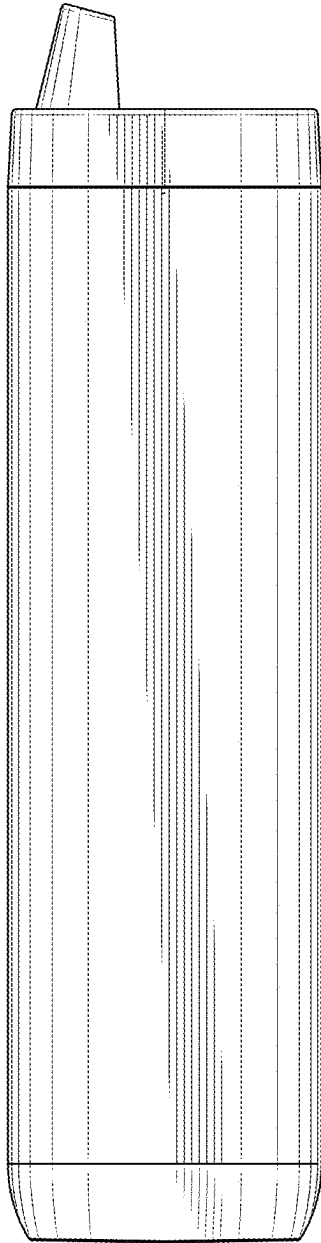


FIG. 6

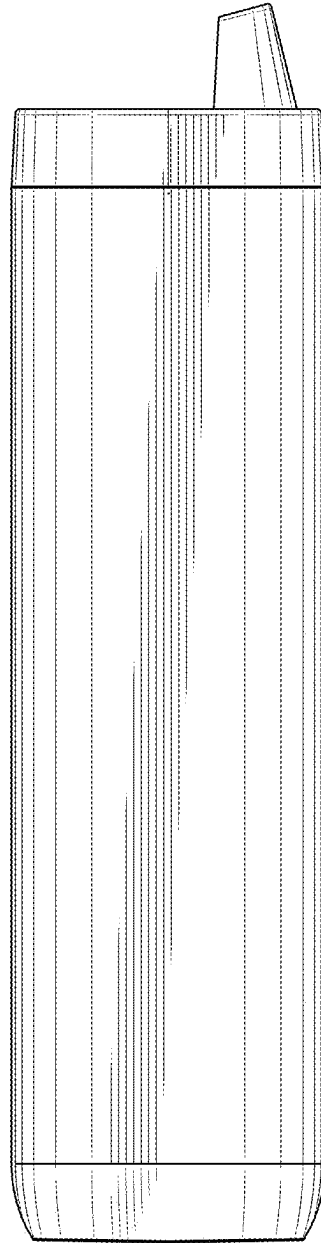


FIG. 7

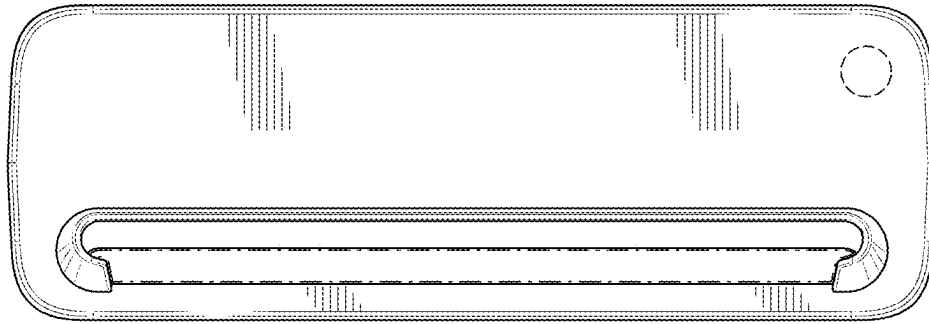


FIG. 8

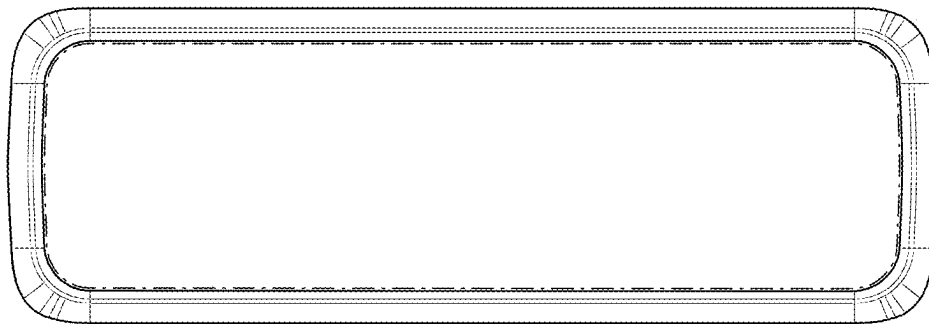


FIG. 9