



US0D1091831S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,091,831 S**  
**Xu et al.** (45) **Date of Patent:** **\*\* Sep. 2, 2025**

(54) **SINGLE LEAD ELECTROCARDIOGRAPH  
DETECTOR**

(71) Applicant: **Wuhan United Imaging Surgical Co.,  
Ltd., Wuhan (CN)**

(72) Inventors: **Ting Xu, Hubei (CN); Junqiang  
Xiong, Hubei (CN)**

(\*\*) Term: **15 Years**

(21) Appl. No.: **35/522,808**

(22) Filed: **Oct. 27, 2023**

(80) **Hague Agreement Data**

Int. Filing Date: **Oct. 27, 2023**

Int. Reg. No.: **DM/233398**

Int. Reg. Date: **Oct. 27, 2023**

Int. Reg. Pub. Date: **Nov. 1, 2024**

(30) **Foreign Application Priority Data**

Apr. 28, 2023 (CN) ..... 202330245921.4

(51) **LOC (15) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187; D24/168**

(58) **Field of Classification Search**

USPC ..... D24/107, 168, 186, 187, 189, 200  
CPC ... A61B 5/0404; A61B 5/0416; A61B 5/0422;  
A61B 5/0424; A61B 5/04012; A61B  
5/04082; A61B 5/04085; A61B 5/04087;  
A61B 5/6841; A61N 1/046; A61N  
1/0472; A61N 1/0476

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D746,993 S \* 1/2016 Lewis, Jr. .... D24/187  
D775,361 S \* 12/2016 Vosch ..... D24/187

D905,253 S \* 12/2020 Hubelbank ..... D24/189  
D907,219 S \* 1/2021 Neri ..... D24/189  
D981,571 S \* 3/2023 Keeman ..... D24/187  
D985,127 S \* 5/2023 Hubelbank ..... D24/168  
D1,027,189 S \* 5/2024 Peremen ..... D24/187  
D1,029,277 S \* 5/2024 Huang ..... D24/168  
D1,036,677 S \* 7/2024 Peremen ..... D24/187  
D1,037,464 S \* 7/2024 Kubik ..... D24/187  
D1,039,704 S \* 8/2024 Chen ..... D24/187  
D1,055,290 S \* 12/2024 Wasserman ..... D24/187  
2023/0045240 A1 \* 2/2023 Park ..... A61N 1/36

\* cited by examiner

Primary Examiner — Jennifer L Rempfer

Assistant Examiner — Michelle Marquart Christeon

(57) **CLAIM**

The ornamental design for a single lead electrocardiograph detector as shown and described.

## DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

1. Single lead electrocardiograph detector

1.1 : Perspective

1.2 : Front

1.3 : Back

1.4 : Left


1.5 : Right

1.6 : Top


1.7 : Bottom

The product is used for sticking to the body surface and collecting human electrocardiograph signals.


**1 Claim, 7 Drawing Sheets**  
**(7 of 7 Drawing Sheet(s) Filed in Color)**

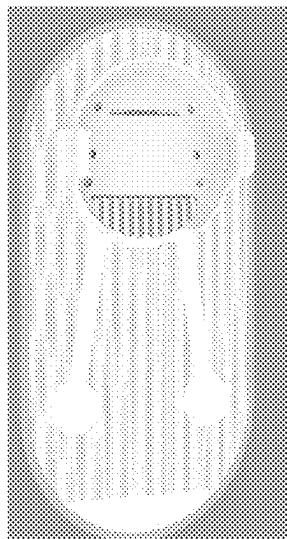


1.1

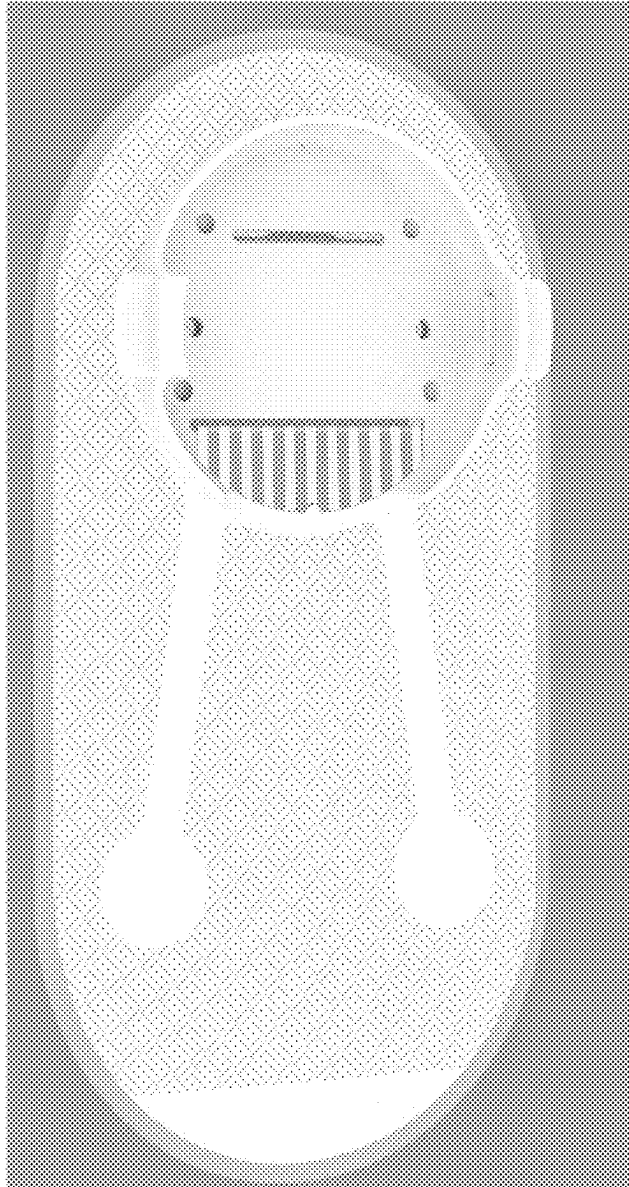


1.2

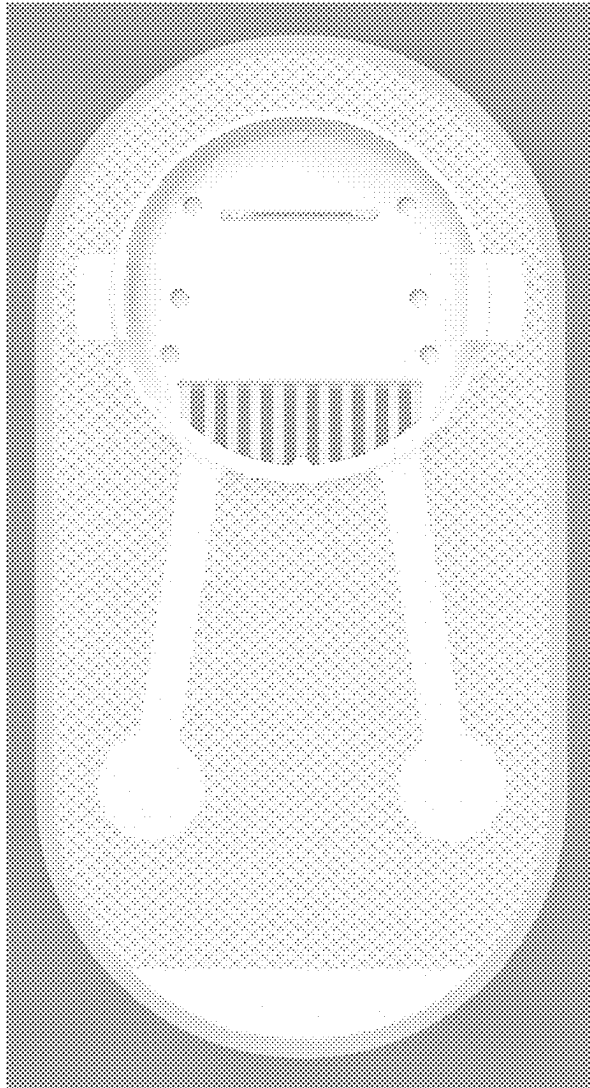


1.3

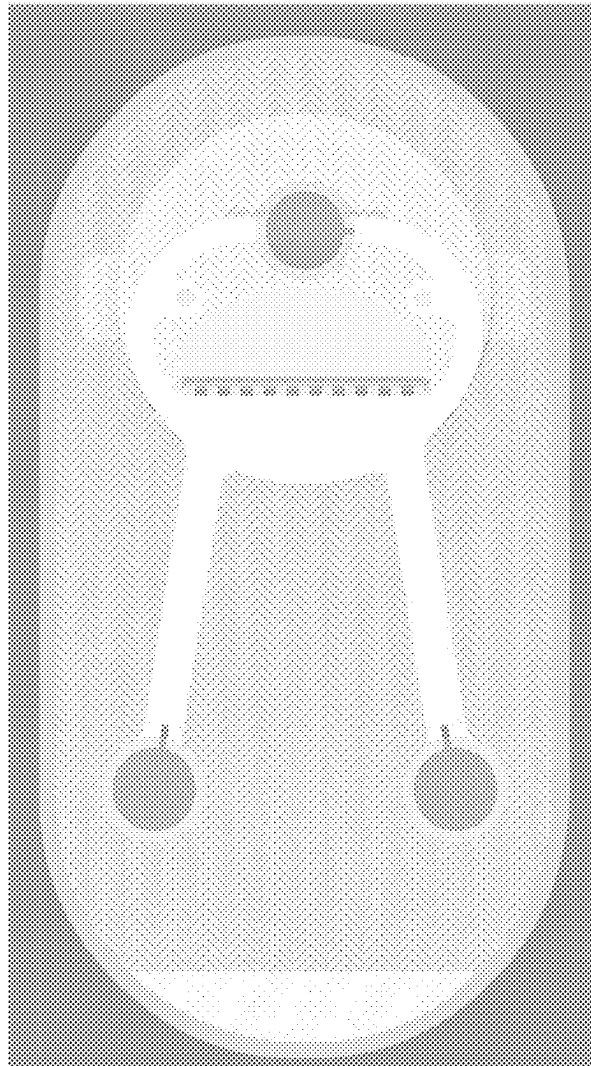


**1.4**

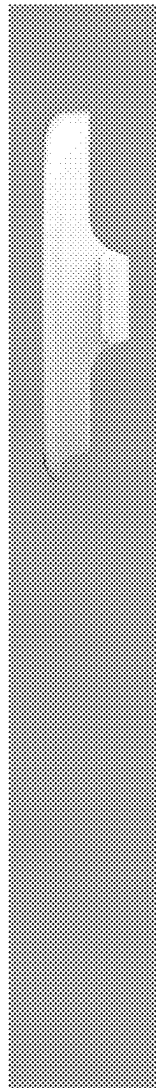

**1.5**

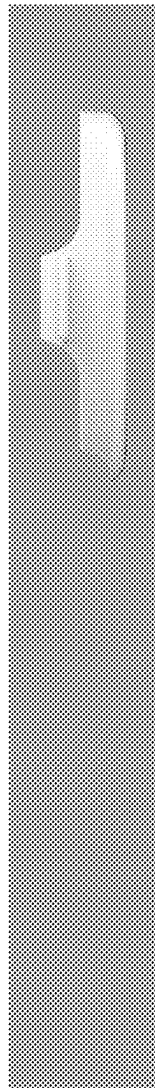

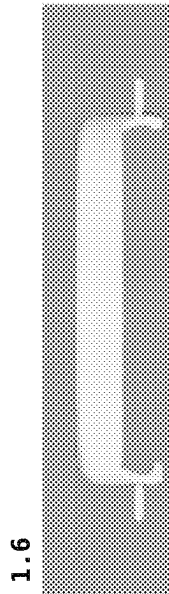

1.7

