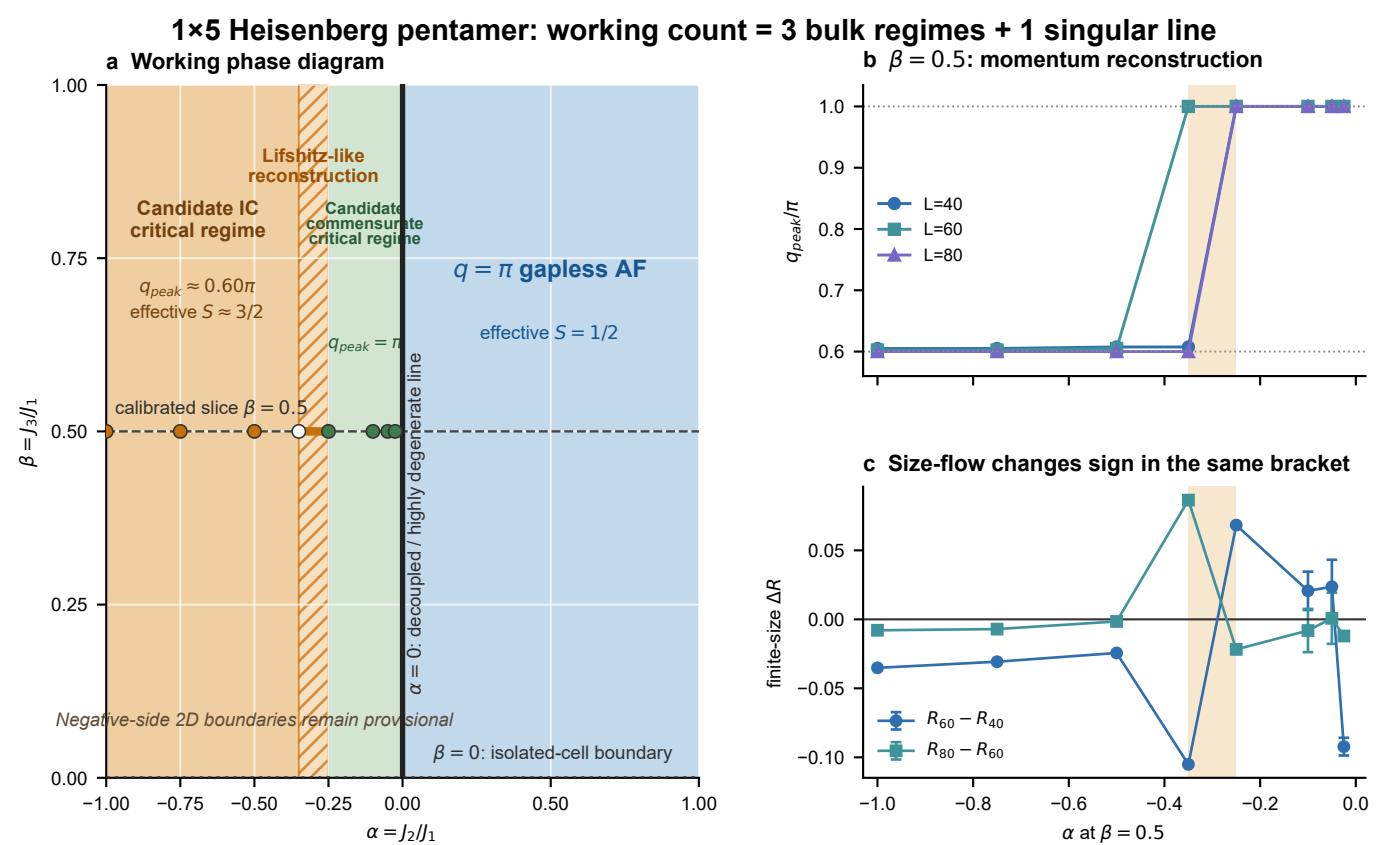


Interpretive labels are intentionally permissive. Only the beta=0.5 bracket is calibrated; Stage B/C must establish its beta dependence and thermodynamic status.