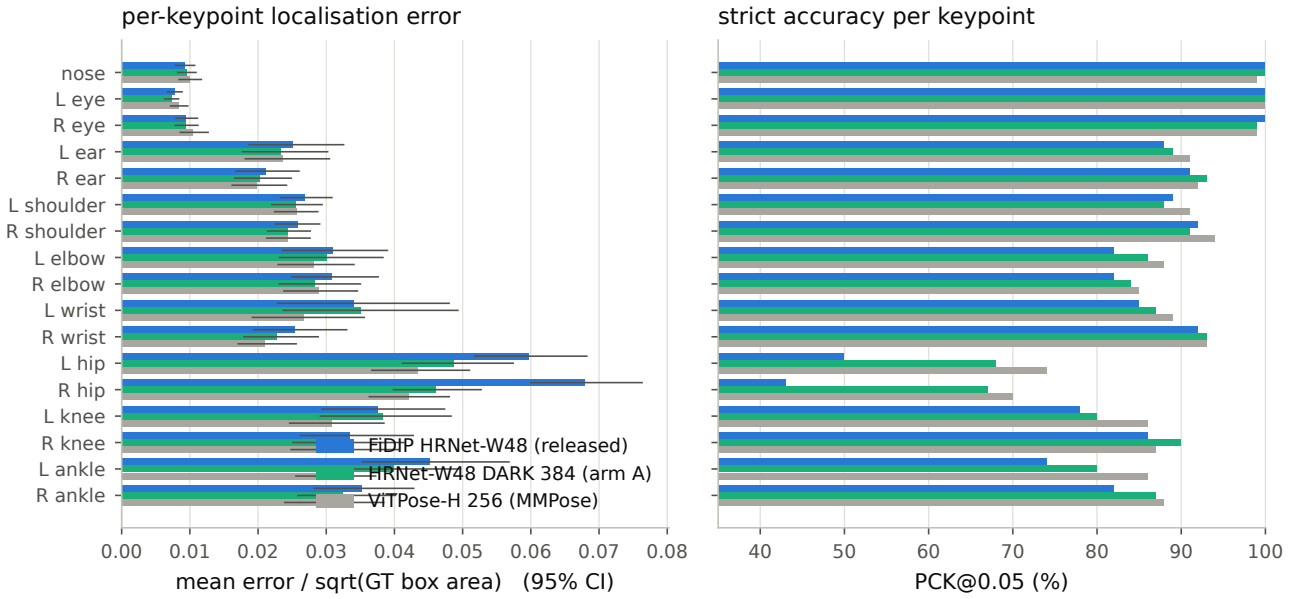
per-keypoint localisation error
strict accuracy per keypoint
nose
L eye
R eye
L ear
R ear
L shoulder
R shoulder
L elbow
R elbow
L wrist
R wrist
L hip
R hip
L knee
R knee
L ankle
R ankle
FiDIP HRNet-W48 (released)
HRNet-W48 DARK 384 (arm A)
ViTPose-H 256 (MMPose)
0.00
0.01
0.02
0.03
0.04
0.05
0.06
0.07
0.08
mean error / sqrt(GT box area) (95% CI)
40
50
60
70
80
90
100
PCK@0.05 (%)