

## ***Fragment Analyzer Run Summary:***

**Filename and Data Path:** C:\AATI\Data\2025 01 22\Schwartz RNA repeat 12-39-23\2025 01 22 12H 39M.raw

**Created:** Wednesday, January 22, 2025 1:01:31 PM

**# of Capillaries:** 3

**Array Serial #:** 010622-30USFS

**Effect Length:** 33 cm

**Array Usage Count:** 197

**FA Version #:** 1.2.0.11

**Device Serial #:** 2689

### **METHOD INFORMATION**

**Method Name:** DNF-472T33 - HS Total RNA 15nt.mthds

**Gel Prime:** No

**Full Conditioning:** Yes

**Gel Prime to Buffer:** Yes

**Gel Selection:** Gel 2

**Perform Prerun:** 8.0 kV, 30 sec.

**Rinse:** No

**Marker 1:** No

**Rinse:** Tray: 3, Row: A, # Dips: 2

**Sample Injection:** 7.0 kV, 150 sec.


**Separation:** 8.0 kV, 40.0 min.

**Tray Name:** Tray-1

**Analysis Mode:** RNA (Eukaryotic)


### **NOTES**

## Gel Image

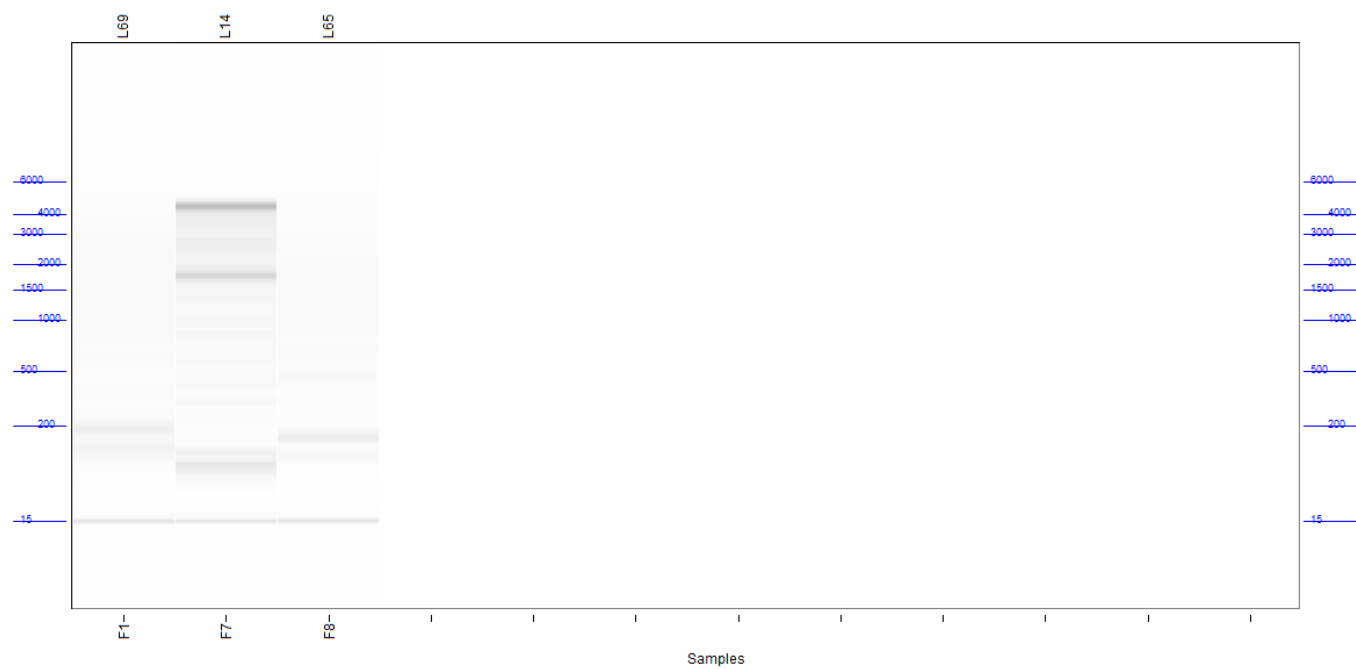


**Filename and Data Path:** C:\AATI\Data\2025 01 22\Schwartz RNA repeat 12-39-23\2025 01 22 12H 39M.raw


**F1: L69**  
RON: 4.3

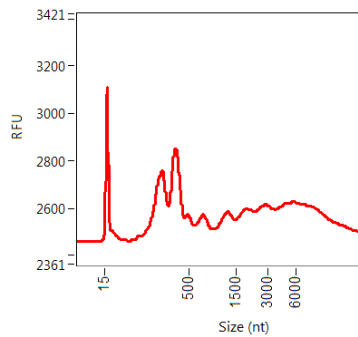


**F7: L14**  
RON: 7.2

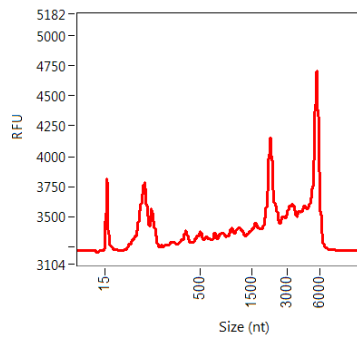

**F8: L65**  
RON: 4.0

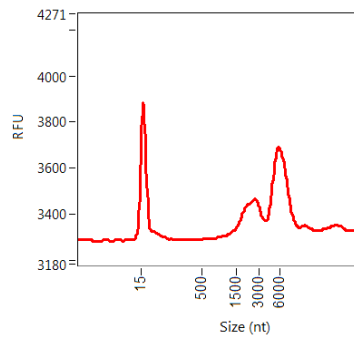

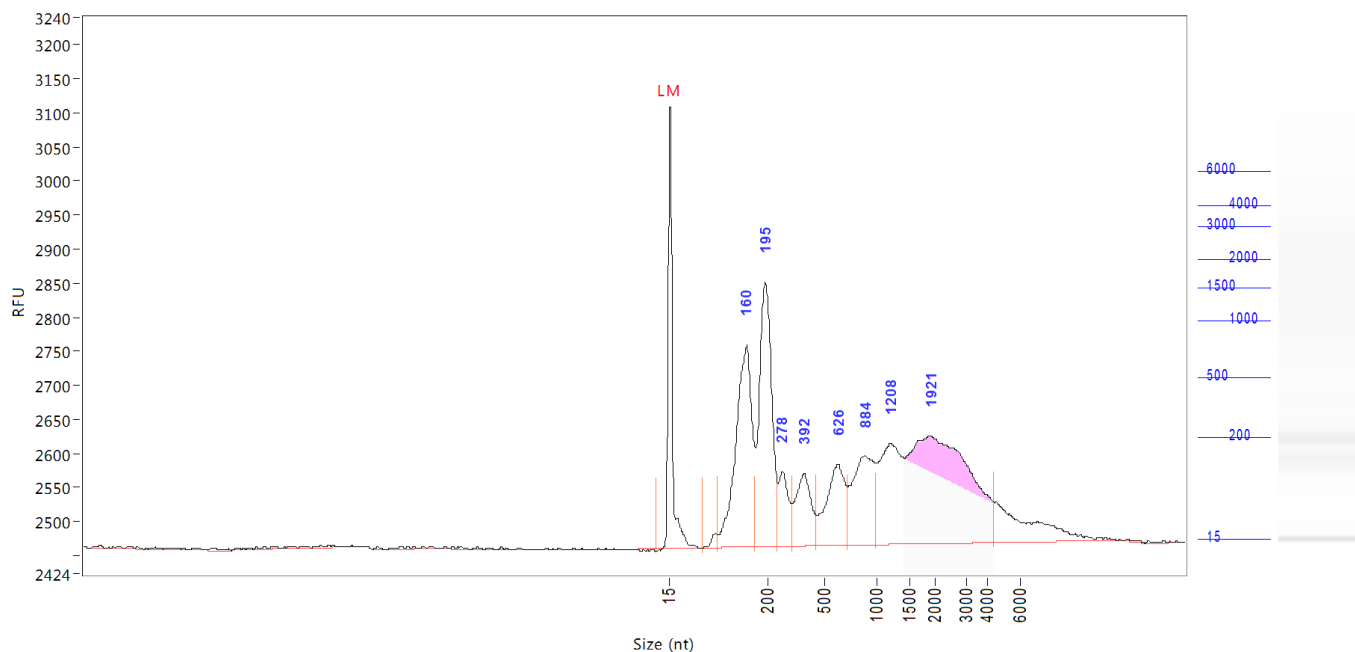
**Sample:** L69**Well Location:** F1**Created:** Wednesday, January 22, 2025 1:01:31 PM

| Peak | Size<br>(nt) | Conc.<br>(ng/uL) | From<br>(nt) | To<br>(nt) | RFU |
|------|--------------|------------------|--------------|------------|-----|
| 1    | 15 (LM)      | 0.0237           | 0            | 76         | 647 |
| 2    | 160          | 0.3867           | 106          | 177        | 294 |
| 3    | 195          | 0.3810           | 177          | 254        | 386 |
| 4    | 278          | 0.0814           | 254          | 325        | 108 |
| 5    | 392          | 0.1201           | 325          | 455        | 105 |
| 6    | 626          | 0.1583           | 455          | 720        | 117 |
| 7    | 884          | 0.1949           | 720          | 996        | 128 |
| 8    | 1208         | 0.2160           | 996          | 1429       | 147 |
| 9    | 1921         | 0.5895           | 1429         | 4439       | 157 |

TIC: 2.1279 ng/uL  
 TIM: 18.5597 nmole/L  
 Total Conc.: 2.2320 ng/uL

28S/18S: 0.0  
 RQN 4.3

Sample Peak Width (sec): 6    Sample Min Peak Height: 20    Sample Baseline V to V?: Y    Sample Baseline V to V pts: 3  
 Sample Filter: Binomial    # of Pts for Filter: 9    Sample Start Region (min): 0    Sample End Region (min): 40  
 Manual Baseline Start (min): 18    Manual Baseline End (min): 38  
 Marker Peak Width (sec): 6    Marker Min Peak Height: 100    Marker Baseline V to V?: Y    Marker Baseline V to V pts: 3  
 Lower Marker Selection: First Peak > 100 RFU    Upper Marker Selection: Last Peak > 100 RFU  
 Ladder Size (nt) 15, 200, 500, 1000, 1500, 2000, 3000, 4000, 6000  
 Quantification Using: Ladder    Final Concentration (ng/uL): 0.2000    Dilution Factor: 10.0  
 Min. RFU for Data Processing: 2

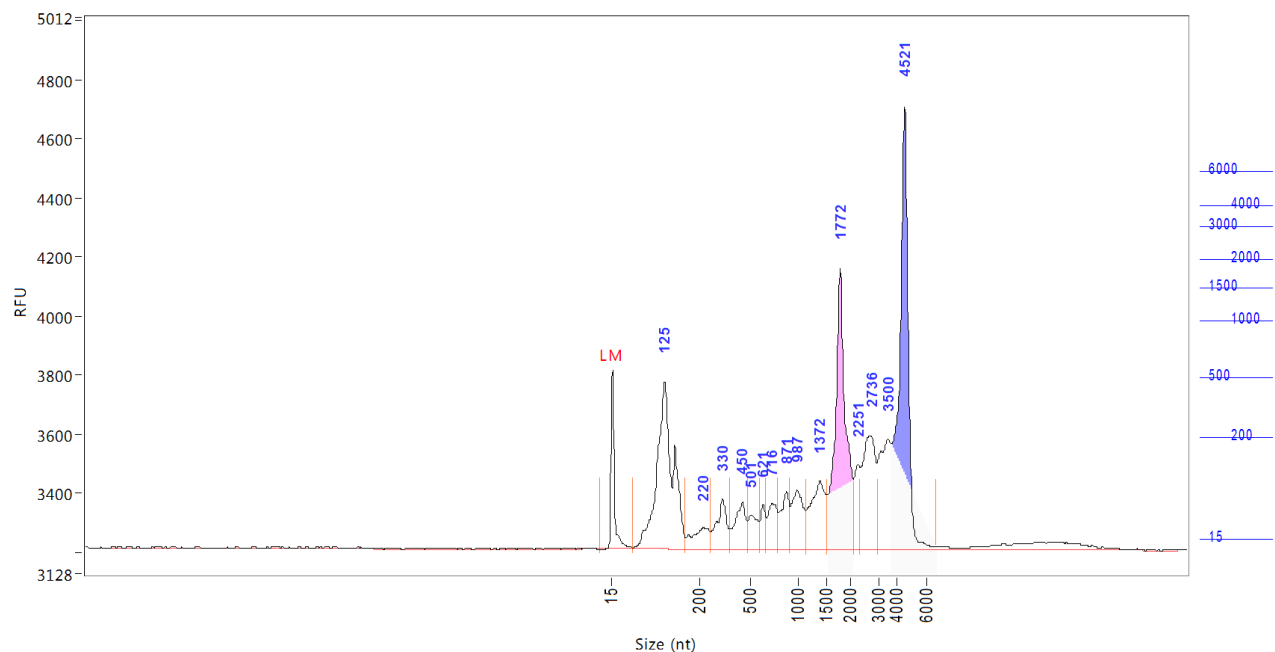
**Sample:** L14**Well Location:** F7**Created:** Wednesday, January 22, 2025 1:01:31 PM

| Peak | Size (nt) | Conc. (ng/uL) | From (nt) | To (nt) | RFU  |
|------|-----------|---------------|-----------|---------|------|
| 1    | 15 (LM)   | 0.0237        | 0         | 59      | 604  |
| 2    | 125       | 1.0033        | 59        | 170     | 565  |
| 3    | 220       | 0.1234        | 170       | 261     | 70   |
| 4    | 330       | 0.1691        | 261       | 371     | 169  |
| 5    | 450       | 0.1698        | 371       | 478     | 157  |
| 6    | 501       | 0.1068        | 478       | 583     | 113  |
| 7    | 621       | 0.0778        | 583       | 660     | 149  |
| 8    | 716       | 0.1374        | 660       | 789     | 152  |
| 9    | 871       | 0.1518        | 789       | 914     | 192  |
| 10   | 987       | 0.2041        | 914       | 1122    | 198  |
| 11   | 1372      | 0.3118        | 1122      | 1501    | 229  |
| 12   | 1772      | 0.8550        | 1501      | 2089    | 947  |
| 13   | 2251      | 0.1521        | 2089      | 2354    | 285  |
| 14   | 2736      | 0.4130        | 2354      | 2956    | 384  |
| 15   | 3500      | 0.3526        | 2956      | 3705    | 372  |
| 16   | 4521      | 1.0526        | 3705      | 6678    | 1498 |

TIC: 5.2807 ng/uL  
 TIM: 36.4799 nmole/L  
 Total Conc.: 5.3383 ng/uL

28S/18S: 1.4  
 RQN 7.2

Sample Peak Width (sec): 6 Sample Min Peak Height: 20 Sample Baseline V to V?: Y Sample Baseline V to V pts: 3  
 Sample Filter: Binomial # of Pts for Filter: 9 Sample Start Region (min): 0 Sample End Region (min): 40  
 Manual Baseline Start (min): 18 Manual Baseline End (min): 38  
 Marker Peak Width (sec): 6 Marker Min Peak Height: 100 Marker Baseline V to V?: Y Marker Baseline V to V pts: 3  
 Lower Marker Selection: First Peak > 100 RFU Upper Marker Selection: Last Peak > 100 RFU  
 Ladder Size (nt) 15, 200, 500, 1000, 1500, 2000, 3000, 4000, 6000  
 Quantification Using: Ladder Final Concentration (ng/uL): 0.2000 Dilution Factor: 10.0  
 Min. RFU for Data Processing: 2

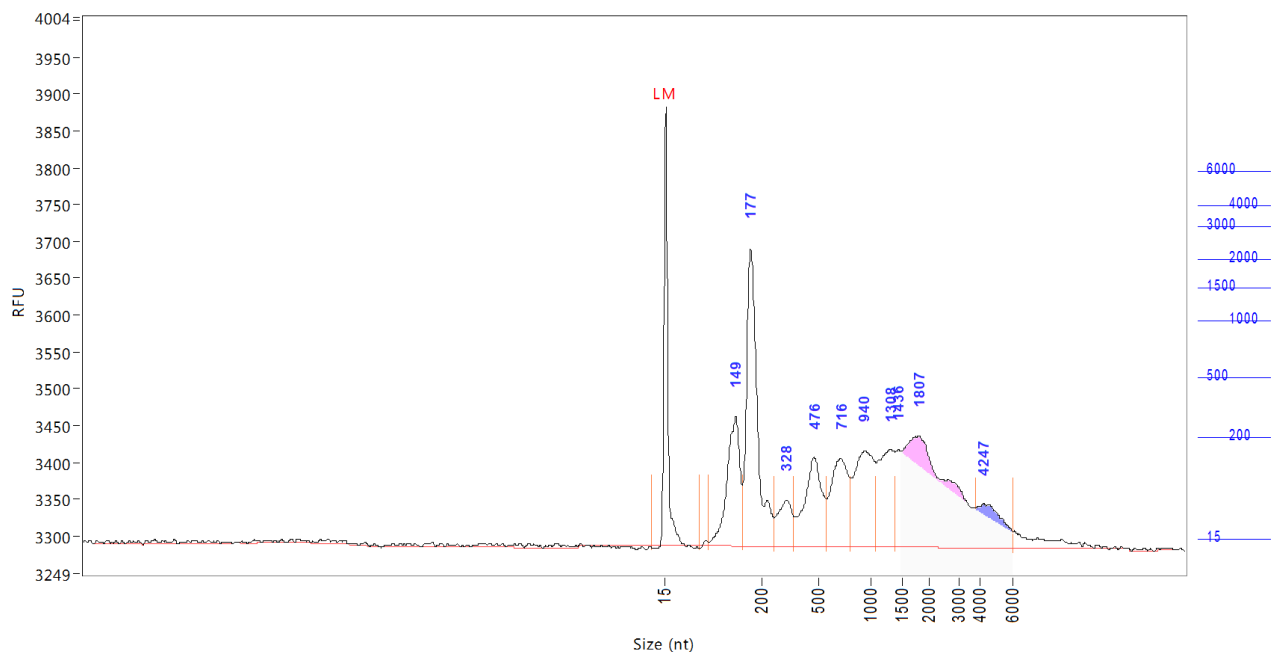**Sample:** L65**Well Location:** F8**Created:** Wednesday, January 22, 2025 1:01:31 PM

| Peak | Size<br>(nt) | Conc.<br>(ng/uL) | From<br>(nt) | To<br>(nt) | RFU |
|------|--------------|------------------|--------------|------------|-----|
| 1    | 15 (LM)      | 0.0237           | 0            | 80         | 594 |
| 2    | 149          | 0.2118           | 99           | 163        | 173 |
| 3    | 177          | 0.4029           | 163          | 263        | 400 |
| 4    | 328          | 0.0751           | 263          | 368        | 61  |
| 5    | 476          | 0.1765           | 368          | 574        | 119 |
| 6    | 716          | 0.1664           | 574          | 802        | 118 |
| 7    | 940          | 0.2038           | 802          | 1079       | 128 |
| 8    | 1308         | 0.1609           | 1079         | 1386       | 130 |
| 9    | 1436         | 0.0502           | 1386         | 1471       | 130 |
| 10   | 1807         | 0.4856           | 1471         | 3818       | 149 |
| 11   | 4247         | 0.0981           | 3818         | 6027       | 58  |

TIC: 2.0315 ng/uL  
TIM: 16.0269 nmole/L  
Total Conc.: 2.0494 ng/uL

28S/18S: 0.3  
RQN 4.0

Sample Peak Width (sec): 6    Sample Min Peak Height: 20    Sample Baseline V to V?: Y    Sample Baseline V to V pts: 3  
Sample Filter: Binomial    # of Pts for Filter: 9    Sample Start Region (min): 0    Sample End Region (min): 40  
Manual Baseline Start (min): 18    Manual Baseline End (min): 38  
Marker Peak Width (sec): 6    Marker Min Peak Height: 100    Marker Baseline V to V?: Y    Marker Baseline V to V pts: 3  
Lower Marker Selection: First Peak > 100 RFU    Upper Marker Selection: Last Peak > 100 RFU  
Ladder Size (nt) 15, 200, 500, 1000, 1500, 2000, 3000, 4000, 6000  
Quantification Using: Ladder    Final Concentration (ng/uL): 0.2000    Dilution Factor: 10.0  
Min. RFU for Data Processing: 2

**Sample:** DNA Size Ladder

**Well Location:** A12

**Created:** Wednesday, January 22, 2025 1:01:31 PM

**Import From:** c:\users\aatl\desktop\ladders\columbia\_directrna\_hs-rna-ladder.scal

**Fit Type:** Point to Point

Calibration Curve

