




## 3 Phase Analysis.vi

C:\Users\Public\Desktop\LabVIEW\_Applications\_2018\3 Phase Analysis.exe\3 Phase Analysis.vi

Last modified on 2022-09-21 at 9:49 AM

Printed on 2022-09-21 at 9:49 AM

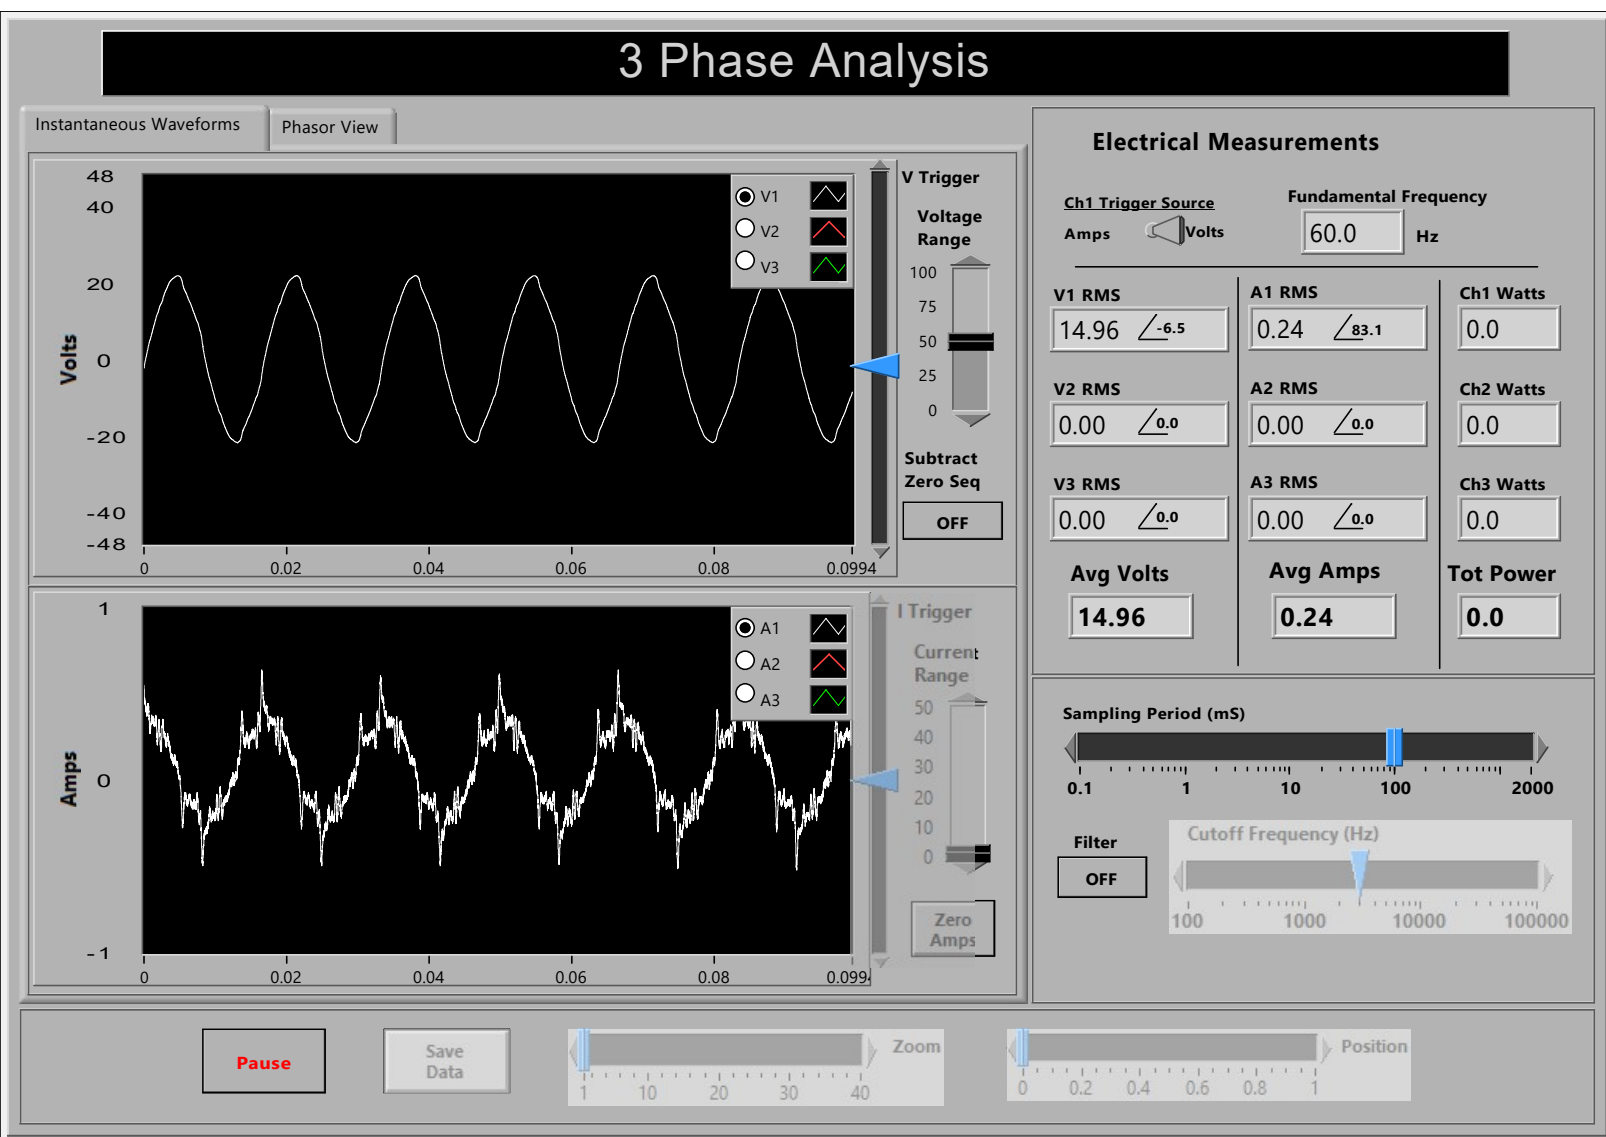

Pause

Save Data

Zoom

1

10

20

30

40

Position

0

0.2

0.4

0.6

0.8

1

Ch1 Trigger Source

Amps

Volts

Fundamental Frequency

60.0

Hz

V1 RMS

14.96

$\angle -6.5$

A1 RMS

0.24

$\angle 83.1$

Ch1 Watts

0.0

V2 RMS

0.00

$\angle 0.0$

A2 RMS

0.00

$\angle 0.0$

Ch2 Watts

0.0

V3 RMS

0.00

$\angle 0.0$

A3 RMS

0.00

$\angle 0.0$

Ch3 Watts

0.0

Avg Volts

14.96

Avg Amps

0.24

Tot Power

0.0

Sampling Period (mS)

0.1

1

10

100

2000

Filter

OFF

Cutoff Frequency (Hz)

100

1000

10000

100000