



Isotonic calibration

MAE 0.0805 against 0.1752 for the mean

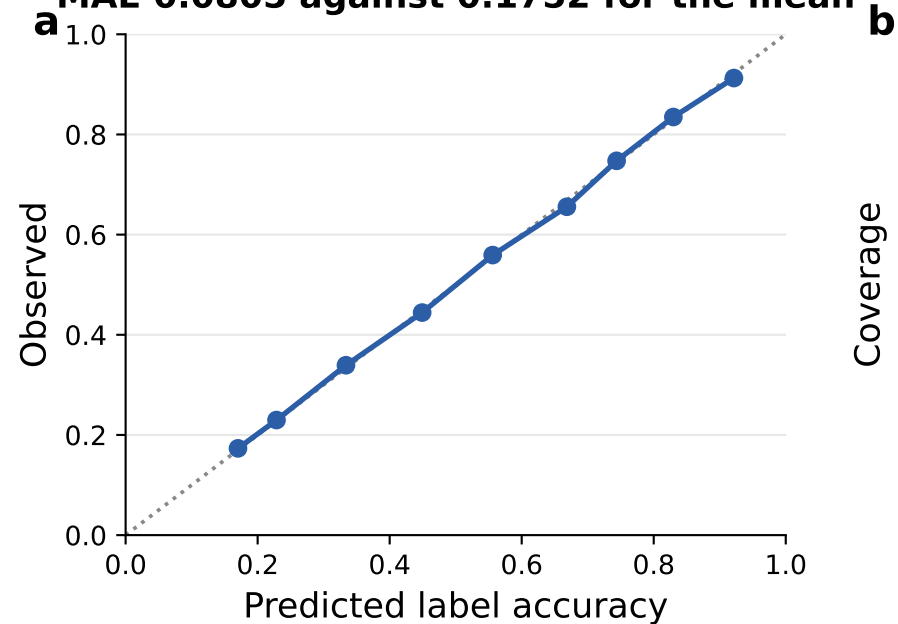

Split-conformal coverage

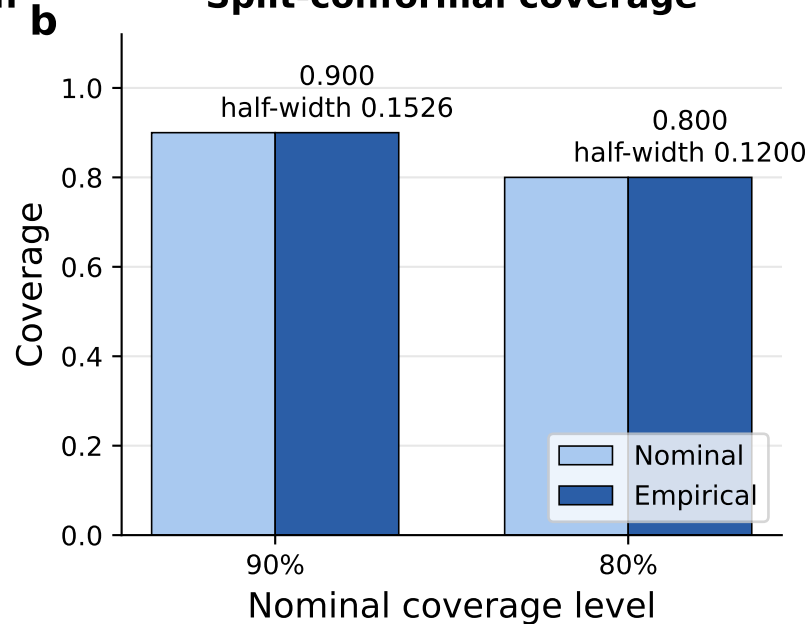

Fold-quality tier separation

