



Isotonic calibration

MAE 0.0814 against 0.1734 for the mean

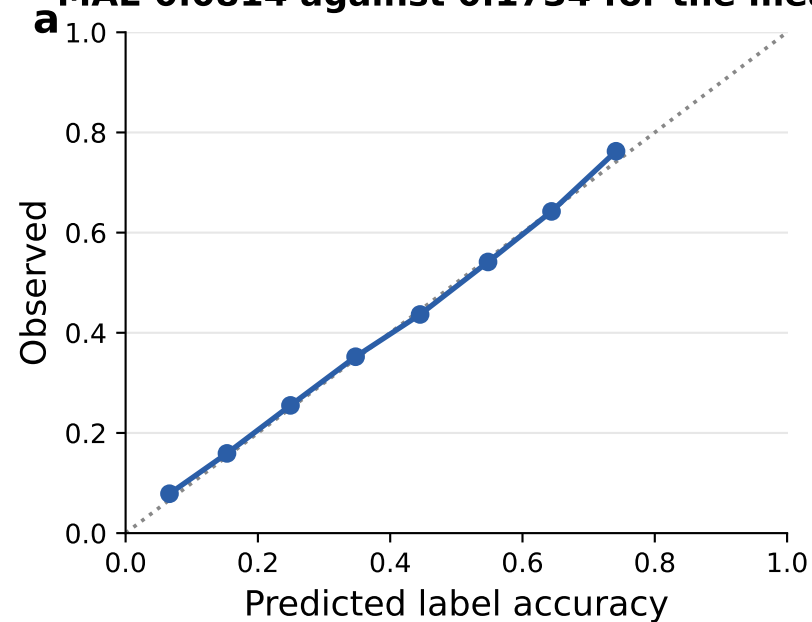

Split-conformal coverage

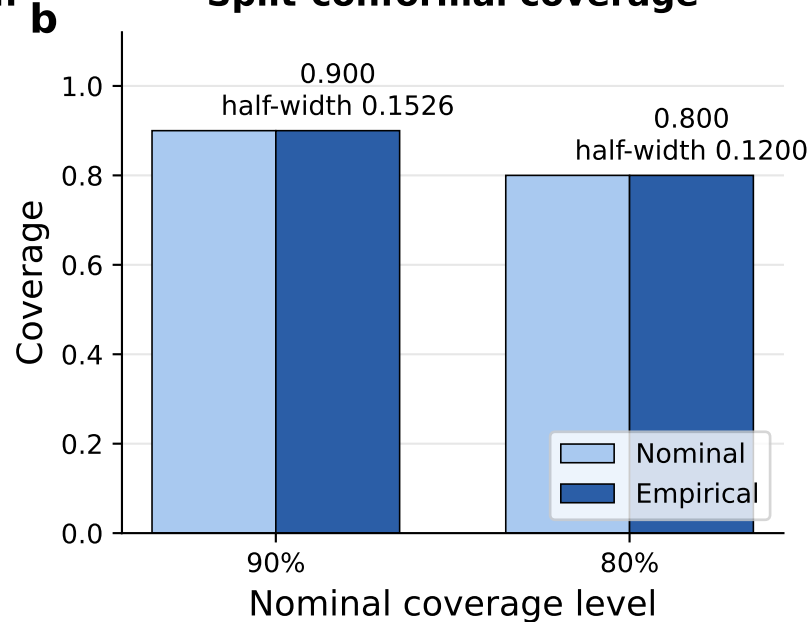

Fold-quality tier separation

