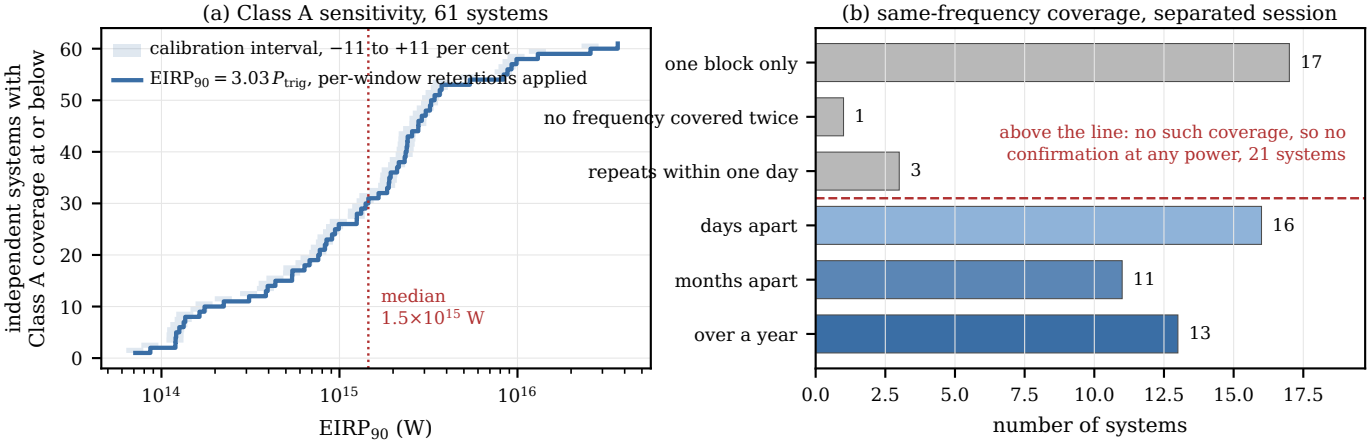
(a) Class A sensitivity, 61 systems
calibration interval, −11 to +11 per cent
EIRP90 = 3.03 Ptrig, per-window retentions applied
independent systems with Class A coverage at or below
median
1.5×10^15 W
EIRP90 (W)
(b) same-frequency coverage, separated session
one block only
17
no frequency covered twice
1
repeats within one day
3
above the line: no such coverage, so no confirmation at any power, 21 systems
days apart
16
months apart
11
over a year
13
number of systems