


End-to-end OCT glaucoma classification

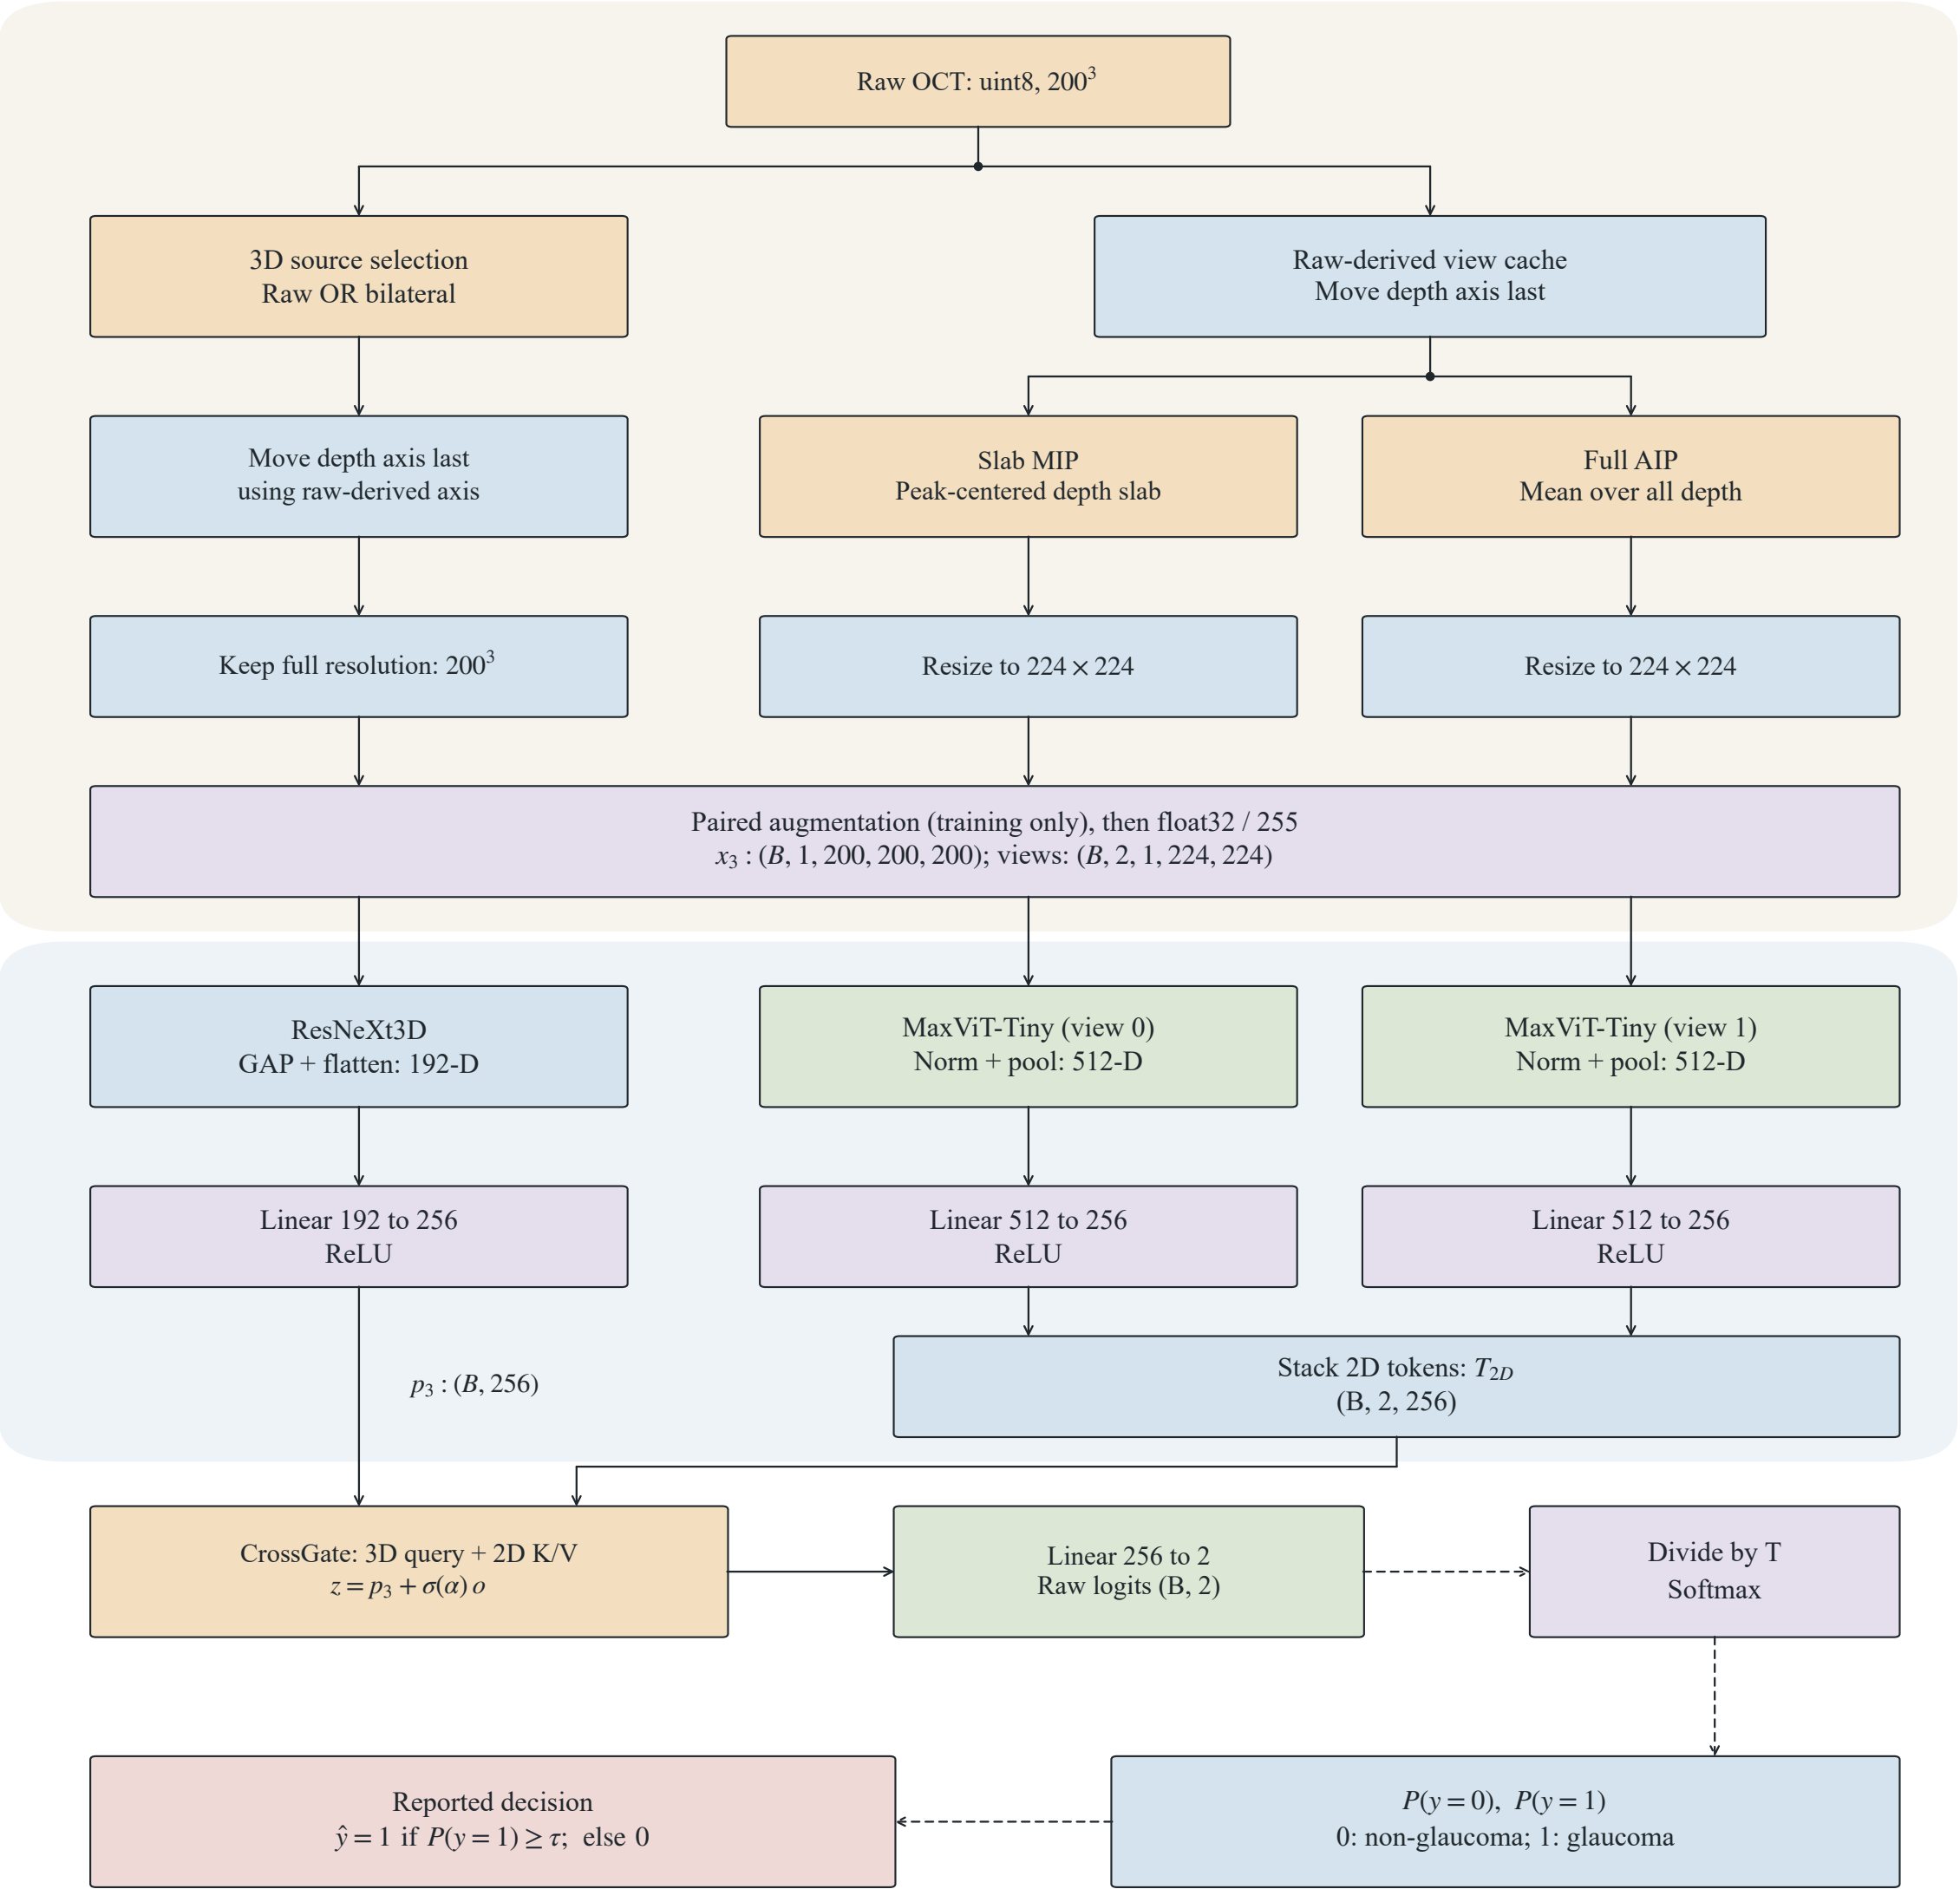

Bilateral affects only the 3D input; both 2D views remain raw-derived. Two MaxViT encoders have independent weights.
Dashed arrows: notebook test-time processing. T is fitted on validation logits; tau is selected on uncalibrated validation probabilities.
The current notebook applies tau after test calibration (a protocol mismatch). Training uses weighted cross-entropy on raw logits.