Statmatic Set Maintenance Time

LED 1 **LED 2** **LED 3**

LED
Standby

Start Button
Instrument
and Turbine
Maintenance

Start Button
Chuck
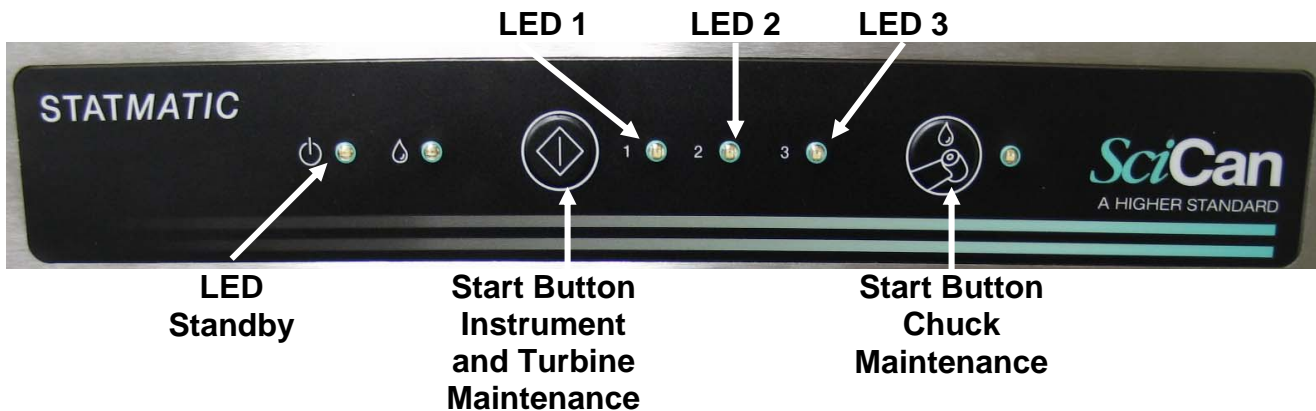**Maintenance**

To change maintenance time, switch on power while ⬥ is pressed.

The LED ⏻ Standby then flashes at .3-second intervals.

Maintenance time is set as follows:

15S	LED 1 illuminates
20S	LED 2 illuminates
30S	LED 3 illuminates
40S	LED 1, 2 & 3 illuminate

The 💧 button is used to change the setting. The most recently set valve is automatically

saved after 5 seconds. After saving the unit assumes normal operation (LED ⏻ illuminates).