


Progeny®—the leader in intraoral x-ray systems in the U.S. and the preferred choice of dentists around the world.

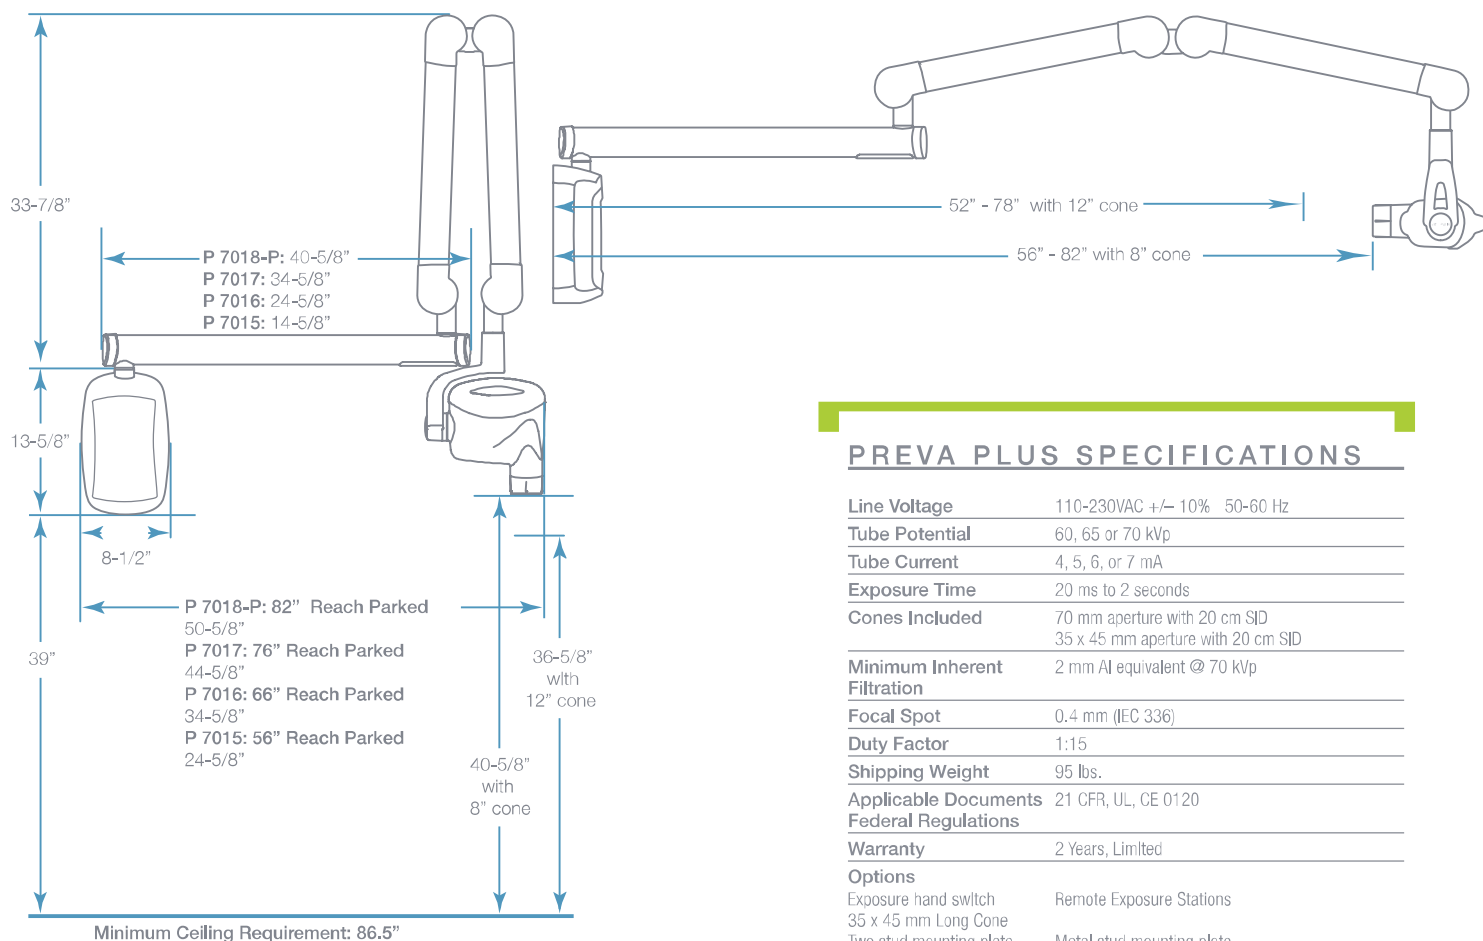

Cabinet Pass Through

66" Arm: 31" W x 47.5" H

76" Arm: 41" W x 47.5" H

Cabinet Pass Through (Alternate)

66" Arm: 26.75" W x 47.5" H

76" Arm: 36.75" W x 47.5" H

Mobile

Base: 26.9" W x 36" L

Height: 76.9"

Arm reach: 44"

PREVA PLUS SPECIFICATIONS

| | |
|-----------------------------|--|
| Line Voltage | 110-230VAC +/- 10% 50-60 Hz |
| Tube Potential | 60, 65 or 70 kVp |
| Tube Current | 4, 5, 6, or 7 mA |
| Exposure Time | 20 ms to 2 seconds |
| Cones Included | 70 mm aperture with 20 cm SID 35 x 45 mm aperture with 20 cm SID |
| Minimum Inherent Filtration | 2 mm Al equivalent @ 70 kVp |
| Focal Spot | 0.4 mm (IEC 336) |
| Duty Factor | 1:15 |
| Shipping Weight | 95 lbs. |
| Applicable Documents | 21 CFR, UL, CE 0120 |
| Federal Regulations | |
| Warranty | 2 Years, Limited |
| Options | Exposure hand switch Remote Exposure Stations 35 x 45 mm Long Cone Two stud mounting plate Metal stud mounting plate Choice of 56", 66", 76", or 82" (total reach) and Mobile |
| Sensor | |
| Film Size equivalent | Size 1 Size 2 |
| Dimensions | 37 x 24 x 5.5 mm 43 x 32 x 5.5 mm |
| Active Area | 30 x 20 mm 36 x 26 mm |
| Sensor Cable | 90 cm 90 cm |
| Computer Interface | High Speed USB 2.0 High Speed USB 2.0 |

Computer Requirements

Please see www.progeny dental.com for operating system and hardware requirements

Contact your Midmark representative for additional system requirement information.

midmark.com

675 Heathrow Drive Lincolnshire, IL 60069
847-415-9800 Toll-free 888-924-3800

©Midmark 2013 All Rights Reserved Printed in the USA
ML-00041 Rev. D

