

Labcyte Echo 550

Device Driver User Guide



Agilent Technologies

Notices

© Agilent Technologies, Inc. 2008-2009

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

User Guide Part Number

G5415-90026

July/2007

Contact Information

Agilent Technologies Inc.
Automation Solutions
5301 Stevens Creek Blvd.
Santa Clara, CA 95051
USA

Technical Support: 1.800.979.4811
or +1.408.345.8011
service.automation@agilent.com

Customer Service: 1.866.428.9811
or +1.408.345.8356
orders.automation@agilent.com

European Service: +44 12081443513
euroservice.automation@agilent.com

Documentation feedback:
documentation.automation@agilent.com

Web: <http://www.agilent.com>

Acknowledgements

Microsoft and Windows are registered trademarks of the Microsoft Corporation in the United States and other countries.

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses


The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or sub-contract, Software is delivered and licensed as “Commercial computer software” as defined in DFAR 252.227-7014 (June 1995), or as a “commercial item” as defined in FAR 2.101(a) or as “Restricted computer software” as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Agilent Technologies’ standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14

(June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

 A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

Letter to our Customers

Dear Customer,

The Agilent Technologies acquisition of Velocity11 resulted in the following changes:

- Creation of Agilent Technologies Automation Solutions, formerly Velocity11
- Renaming of some Velocity11 products
- New Customer Service and Technical Support contact information
- New website address for product information

Please make a note of the following changes as they impact this user guide.

Velocity11 product name changes

Velocity11 product name	Changes to ...
Access2 Automated Microplate Loader	Automated Centrifuge Loader
Element Automation System	BioCel 900 System
IWorks Device Driver Programming Interface	VWorks DCL Interface
PlatePierce Seal Piercing Station	Microplate Seal Piercer
VCode Barcode Print and Apply Station	Microplate Barcode Labeler
Velocity11 Robot	3-Axis Robot
VHooks Integration Interface	VWorks Hooks Interface
VPrep Pipetting System	Vertical Pipetting Station
VSpin Microplate Centrifuge	Microplate Centrifuge
VStack Labware Stacker	Labware Stacker

New contact information

Documentation feedback: documentation.automation@agilent.com

Technical Support: 1.800.979.4811 or +1.408.345.8011
service.automation@agilent.com

Customer Service: 1.866.428.9811 or +1.408.345.8356
orders.automation@agilent.com

European Service: +44 12081443513
euroservice.automation@agilent.com

Web: <http://www.agilent.com>

Contents

Chapter 1. Introduction	1
Who should read this guide	2
About Velocity11 user guides	3
What this guide covers	5
About devices	6
About device drivers	7
Installing device drivers	9
Adding devices	10
About diagnostics	11
Opening diagnostics	12
About profiles	15
Setting the properties for a device	16
Adding and linking Sub Process tasks	19
Using JavaScript to set task parameters	21
About reader output files	22
About device initialization	25
 Chapter 2. Labcyte Echo 550	 27
Workflow for configuring Labcyte Echo 550 devices	28
Creating a Labcyte Echo 550 profile	29
Setting Labcyte Echo 550 task parameters	31
Operating the Labcyte Echo 550 with diagnostics	36
Managing Labcyte Echo 550 profiles	38

Introduction

1

This chapter introduces Velocity11 device drivers and provides some basic procedures that are needed to use them.

A Velocity11 device driver is software that plugs into VWorks or BenchWorks software to allow them to control a specific device.

Before reading this guide, you should be familiar with the VWorks or BenchWorks software user interface. Information about using VWorks or BenchWorks software can be found in the *VWorks Version 3 Automation Control User Guide* or *BenchWorks Automation Control User Guide*.

To set up and use Velocity11 device drivers, become familiar with the content in this guide as well as the guides for the devices that use VWorks or BenchWorks software.

This chapter contains the following topics:

- ☐ “Who should read this guide” on page 2
- ☐ “About Velocity11 user guides” on page 3
- ☐ “What this guide covers” on page 5
- ☐ “About devices” on page 6
- ☐ “About device drivers” on page 7
- ☐ “Installing device drivers” on page 9
- ☐ “Adding devices” on page 10
- ☐ “About diagnostics” on page 11
- ☐ “Opening diagnostics” on page 12
- ☐ “About profiles” on page 15
- ☐ “Setting the properties for a device” on page 16
- ☐ “Adding and linking Sub Process tasks” on page 19
- ☐ “Using JavaScript to set task parameters” on page 21
- ☐ “About reader output files” on page 22
- ☐ “About device initialization” on page 25

Who should read this guide

Job roles

This user guide is for people with the following job roles:


Job role	Responsibilities
Integrator	Someone who writes software and configures hardware controlled by device drivers.
Lab manager, administrator, or technician	Someone who is responsible for: <ul style="list-style-type: none"><input type="checkbox"/> Installing device drivers<input type="checkbox"/> Managing device drivers<input type="checkbox"/> Developing the applications that are run using device drivers<input type="checkbox"/> Solving the more challenging problems that might arise<input type="checkbox"/> Developing training materials and standard operating procedures for operators
Operator	Someone who performs the daily production work using the device driver and solves routine problems. Your organization may choose to create its own procedures for operators including the procedures in this guide.

Related topics

For information about...	See...
Contacting Velocity11	http://www.velocity11.com/contact.html
Accessing online help	"About Velocity11 user guides" on page 3
Device drivers	"About device drivers" on page 7

About Velocity11 user guides

About this topic	<p>This topic describes the different formats of Velocity11 user information and explains how to access the user information.</p>
Formats available	<p>Velocity11 user information is provided to you as:</p> <ul style="list-style-type: none"><input type="checkbox"/> Online help<input type="checkbox"/> A PDF file<input type="checkbox"/> A printed book <p>The information in each format is the same but each format has different benefits.</p>
Where to find user information	<p>Online help</p> <p>The online help is added to your computer with the Velocity11 lab automation system software installation.</p> <p>PDF file</p> <p>The PDF file of the user guide is on the software CD that is supplied with the product.</p> <p>Velocity11 website</p> <p>You can search the online help or download the latest version of any PDF file from the Velocity11 website at www.velocity11.com.</p> <p><i>Note:</i> All Velocity11 user information can be searched from the website at www.velocity11.com.</p>
Online help	<p>The online help is the best format to use when you are working at the computer and when you want to perform fast or advanced searches for information.</p> <p>To open the online help:</p> <ol style="list-style-type: none">1. In the Velocity11 lab automation software, press F1. The online help window opens. <p>Main features</p> <p>The online help window contains the following:</p> <ul style="list-style-type: none"><input type="checkbox"/> <i>Navigation pane.</i> Consists of four tabs. The Contents, Index, and Search tabs provide different ways to locate information. The Using tab contains information about using the help system.<input type="checkbox"/> <i>Content pane.</i> Displays the online help topics.<input type="checkbox"/> <i>Navigation buttons.</i> Enables you to navigate through the pages. The online help includes a navigation pane, content pane, and navigation buttons.

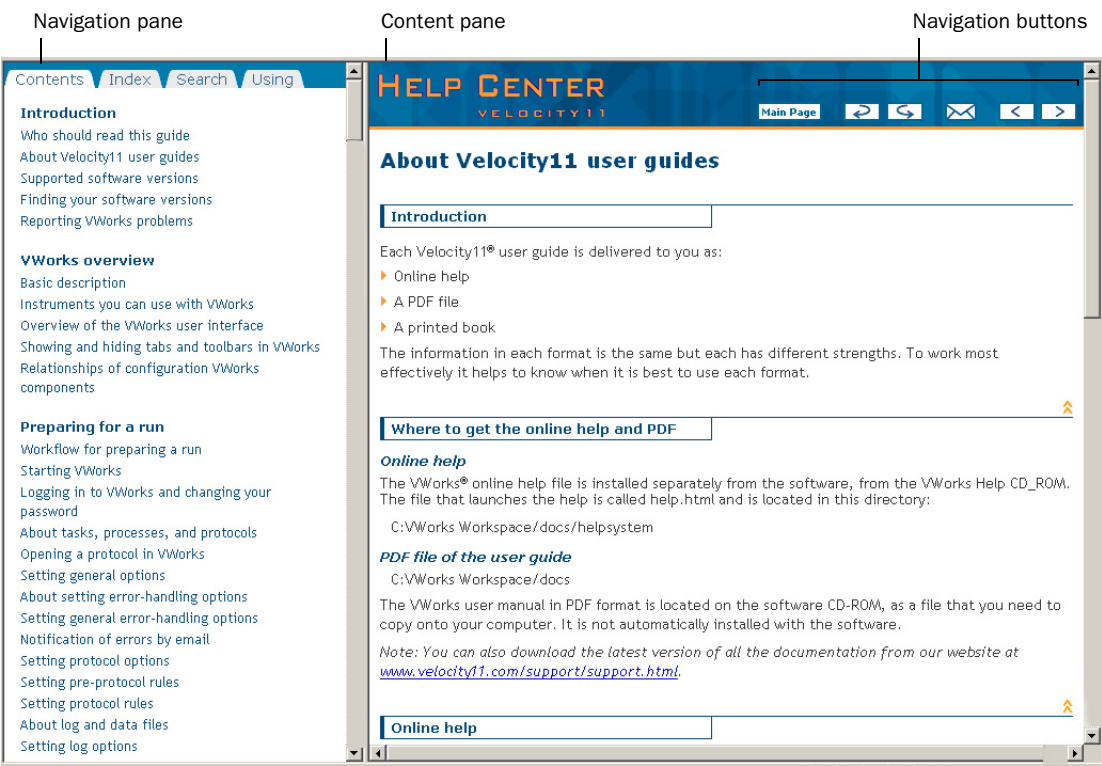

PDF user guides

Computer requirements

To open a user guide in PDF format, you need a PDF viewer. You can download a free PDF viewer from the internet.

Printing and searching

The user guides in PDF format are mainly for printing additional copies. You can perform simple searches in the PDF file, although these searches are much slower than online help searches.

More information

For more information about using PDF documents, see the user documentation for the PDF viewer.

Related topics

For information about...	See...
Who this guide is for	“Who should read this guide” on page 2
What’s in this guide	“What this guide covers” on page 5
Device driver plug-ins	“About device drivers” on page 7

What this guide covers

About this topic

This topic presents an overview of what procedures and information are provided in this user guide.

This guide explains how to:

- ☐ Install the driver for the device
- ☐ Configure the device in the device manager
- ☐ Set and use the tasks associated with the device
- ☐ Use *Device Diagnostics*

Also read

Information about device drivers not covered in this guide and about running VWorks or BenchWorks software can be found in the *VWorks Version 3 Automation Control User Guide* or the *BenchWorks Automation Control User Guide*.

Driver version

To find version information for a driver in VWorks:

1. Start VWorks.
2. Click **Help** and select **About VWorks**.

The **About VWorks** dialog box lists the version numbers of all the current software for all the devices and plug-ins.

To find version information for a driver in BenchWorks:

1. Start BenchWorks.
2. Click **Help** and select **About BenchWorks**.

The **About BenchWorks** dialog box lists the version numbers of all the current software for all the devices and plug-ins.

Firmware version

Some devices have firmware installed on them. Because each device is different, the version number may not be the same for all devices.

To find version information for device firmware:

1. Open **Device Diagnostics** dialog box.
2. Click **About**.

The **About Device Control** message box appears displaying the current version of firmware.

What this guide does not cover

This guide does not cover the following:

- ☐ The operation of the device
- ☐ The operation of VWorks or BenchWorks software
- ☐ Velocity11 devices, such as the PlateLoc Sealer, VCode Microplate Labeler, and VPrep Pipettor when used in stand-alone mode

VWorks or BenchWorks compatibility

If you have purchased a device driver plug-in and are installing it yourself, check with the Velocity11 Technical Support to be sure your version of VWorks or BenchWorks software and the device driver plug-in are using the same version of IWorks software.

BenchWorks versions

Device driver plug-ins used with BenchWorks software may not include some newer features that were specifically added for use with VWorks software and that are described in this manual.

Related topics

For information about...	See...
Who this guide is for	"Who should read this guide" on page 2
User documentation	"About Velocity11 user guides" on page 3
Device driver plug-ins	"About device drivers" on page 7

About devices

About this topic

This topic presents a definition of a Velocity11 device and the device file.

Read this topic if you are unfamiliar with Velocity11 devices and VWorks or BenchWorks software.

Device defined

A device is an item on your lab automation system that has an entry in the device manager. A device can be a robot, an instrument, or a location on the lab automation system that can hold a piece of labware.

Examples of devices:

- ☐ Velocity11 robot
- ☐ Human robot
- ☐ PlateLoc Thermal Plate Sealer
- ☐ Labcyte Echo550
- ☐ Platepad
- ☐ VPrep shelf
- ☐ Waste

Device file defined

The data entered into the device manager and saved as a device file contains the configuration information for your devices.

Device file location Device files have the file name format *file name.dev* and are stored in the folder location that you specify when saving the file.

Related topics

For information about...	See...
Device diagnostics	"About diagnostics" on page 11
Device profiles	"About profiles" on page 15
Adding a device to the device manager	"Adding devices" on page 10

About device drivers

About this topic This topic describes what device drivers are and what they do. Velocity11 device drivers enable mechanical devices or software programs to work with VWorks or BenchWorks software. Read this topic if you are:

- ☐ An administrator in charge of installing device drivers and managing Velocity11 devices
- ☐ A lab automation system integrator who writes software and configures hardware controlled by VWorks or BenchWorks software

Device driver defined A Velocity11 device driver enables VWorks or BenchWorks software to control and communicate with the specific type of device. Each type of device that you operate with VWorks or BenchWorks software requires a device driver. For example, VWorks software uses the:

- ☐ VPrep Pipettor device driver to communicate with the Velocity11 VPrep Pipettor device
- ☐ Softmax Reader device driver to communicate with Molecular Devices readers

Plug-in defined A plug-in is a software program that when added to another program extends it.

Plug-in device drivers Some device drivers are incorporated directly into the VWorks or BenchWorks software application. Other device drivers are distributed as plug-ins. All the device drivers covered in this guide are the plug-in type.

Advantages of distributing device drivers as plug-ins are:

- ☐ You only need to install the plug-ins for the devices you use
- ☐ When new plug-ins become available, they can be easily added. There is no need to re-install the VWorks or BenchWorks software application

IWorks interface

The device driver plug-ins and VWorks or BenchWorks software use IWorks software as a common interface to communicate with each other. Using a common interface allows the creation of a device driver plug-in without the necessity of changing the software.

!! IMPORTANT !! Both VWorks or BenchWorks software and the device driver must be using the same version of IWorks to work properly.

Writing your own device driver

If you are a lab automation system integrator who writes software and configures hardware controlled by VWorks or BenchWorks software, you can write your own driver plug-in for a new device. Contact the Velocity11 Technical Support for information about how to do this.

What functions do the device drivers provide?

Once installed, the following items are enabled:

- ☐ Tasks associated with the device.
Device-specific tasks appear in the Protocol Tasks list and are available for use in protocol editor processes.
- ☐ Task parameters associated with the device.
Device-specific task parameters appear in the Protocol Task Parameters toolbar. These determine the conditions with which to execute the tasks of the device.
- ☐ Diagnostic commands specific to the device.
Device-specific diagnostic commands and options appear in the *Device* Diagnostics dialog box. These commands enable direct control of the device.

Related topics

For information about...	See...
Adding a device to the device manager	"Adding devices" on page 10
Opening diagnostics	"Opening diagnostics" on page 12
Installing a device driver	"Installing device drivers" on page 9
Devices	"About devices" on page 6

Installing device drivers

About this topic

Devices are integrated into VWorks or BenchWorks software using device driver plug-ins. Plug-ins need to be installed before the device can be configured and used.

This topic describes how to install device drivers if they are not already installed on your system. Read this topic if you are an administrator in charge of managing Velocity11 devices.

Procedure

To install device drivers:

1. Insert the device driver installation disc into the CD-ROM of the computer running VWorks or BenchWorks software.
2. Follow the on-screen instructions for installation, selecting the default values when available.
3. When finished, exit VWorks or BenchWorks software.
4. Log off Windows and restart your computer.
5. Start VWorks or BenchWorks software.

For this application...	The default location for the device driver is...
VWorks software	C:\VWorks Workspace\bin\plugins
BenchWorks software	C:\Program Files\Velocity11\BenchWorks\plugins

Related topics

For information about...	See...
Device drivers	"About device drivers" on page 7
Opening diagnostics	"Opening diagnostics" on page 12

Adding devices

About this topic

To configure your lab automation system to use a device, you need to add it to a device file in VWorks or BenchWorks software. The VWorks or BenchWorks software device manager uses the information in the device file to communicate and operate the device within the automation system.

This topic describes how to:

- ☐ Create a new device file (if one does not already exist)
- ☐ Add devices
- ☐ Save the device file


Read this topic if you are an administrator in charge of managing Velocity11 devices.

Procedure

To add devices to a device file:

1. Make sure that the devices are physically networked to the VWorks or BenchWorks software computer and turned on.
2. Start VWorks or BenchWorks software and login as an Administrator.
3. Do one of the following:
 - ◆ If you have an existing device file that you want to add to, select **File > Device File**, click **Open**, and select your device file.
 - ◆ If you are creating a new device file, select **File > Device File** and click **New**.
4. Click the **Device Manager** tab.
5. Click **New device** in the **Device List** toolbar and enter a name for the device you are adding.
6. In the device manager, set the **Device type**.

The default type is **Plate Pad, Standard**.

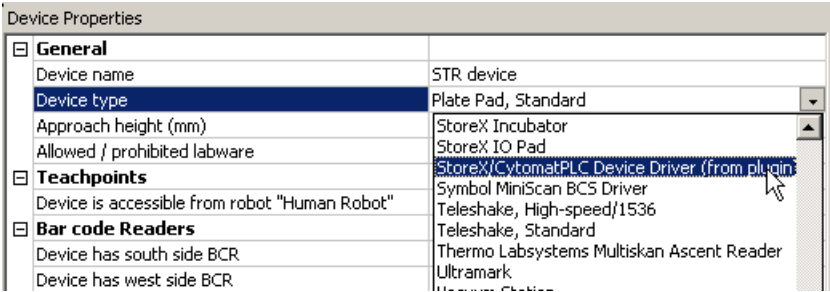

7. Repeat step 5 and step 6 for each device.

8. Select **File > Device File > Save**.

If you are creating a new device file, you are prompted to enter a name for your device file.

Alternatively, you can select **File > Save All**. This saves the device file and the current protocol file at the same time.

Related topics

For information about...	See...
Device drivers	"About device drivers" on page 7
Setting generic device properties	"Setting the properties for a device" on page 16
Adding a sub-process to a protocol	"Adding and linking Sub Process tasks" on page 19
Opening diagnostics	"Opening diagnostics" on page 12

About diagnostics

About this topic

This topic presents an overview of diagnostics software.

Read this topic if you need to set up or troubleshoot a device running VWorks or BenchWorks software.

Background

Devices can be controlled in real time directly through the VWorks or BenchWorks software Diagnostics using simple commands.

Diagnostics software is used for:

- ☐ Troubleshooting
- ☐ Setting teachpoints
- ☐ Performing manual operations outside a protocol
- ☐ Creating and editing profiles

For example, if an error occurs during a run that leaves a plate and the robot where they should not be, you can use robot diagnostics to move the plate and return the robot to its home position.

Types of diagnostics software

Devices and robots manufactured by Velocity11 include their own diagnostics software. You can find instructions for using this software in the relevant user guide.

Related topics

For information about...	See...
Opening diagnostics	"Opening diagnostics" on page 12
Adding a device to the device manager	"Adding devices" on page 10
Device drivers	"About device drivers" on page 7
The definition of devices	"About devices" on page 6

Opening diagnostics

About this topic

Every device has diagnostics software to assist you with troubleshooting and setting up the device. This topic describes how to open a device's diagnostics in VWorks or BenchWorks software.

Read this topic if you need to access a device's diagnostics to perform a device setup task or manually operate a device.

Procedure 1


If you are using VWorks4 software

To open Diagnostics:

1. Click **Diagnostics** on the Control toolbar.



2. In the device file's window, select the device. Expand the general name of the device, if necessary.

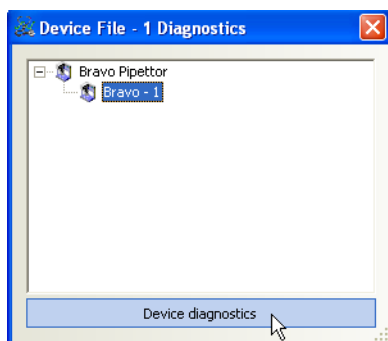

3. Click **Device diagnostics** located at the bottom of the window. The device's diagnostics dialog box opens.


If you are using VWorks3 or BenchWorks software

To open Diagnostics:

1. Click **Diagnostics** on the Control toolbar.



2. In the **Diagnostics** window, select the device. Expand the general name of the device, if necessary.

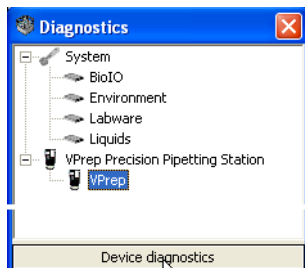


3. Click **Device diagnostics**. The device's diagnostics dialog box opens.

Procedure 2


If you are using VWorks4 software

To open Diagnostics:

1. Click the **Device File** tab.
2. Select the device from the **Devices** toolbar.
Expand the general name of the device, if necessary.

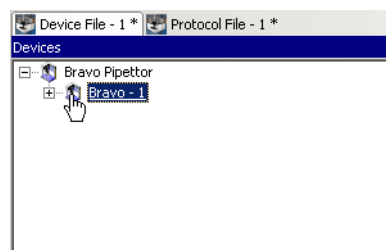

3. Click **Device diagnostics** located at the bottom of the **Devices** toolbar.

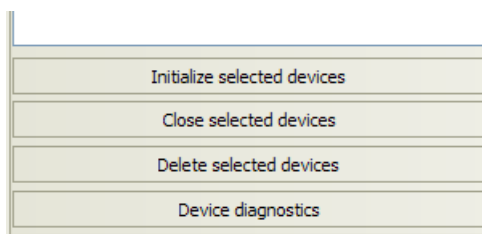


The device's diagnostics dialog box opens.


If you are using VWork3 or BenchWorks software

To open Diagnostics:

1. Click the **Device Manager** tab.
2. Select the device from the **Device List** toolbar. Expand the general name of the device, if necessary.

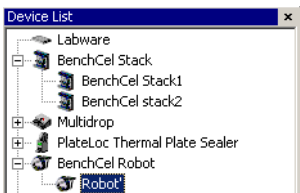

- Click **Device diagnostics** located at the bottom of the **Device List** toolbar.

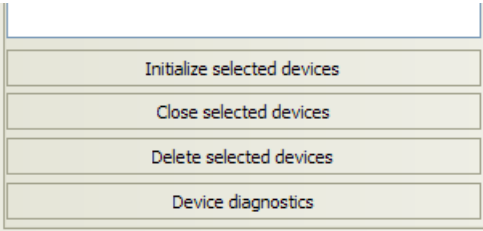

The device’s diagnostics dialog box opens.

Related topics

For information about...	See...
Diagnostics	“About diagnostics” on page 11
About device drivers	“About device drivers” on page 7
Adding a device to the device manager	“Adding devices” on page 10
Setting generic device properties	“Setting the properties for a device” on page 16

About profiles

About this topic

This topic describes what profiles are and what they do.

Read this topic if you are an administrator in charge of managing Velocity11 devices.

Profiles defined

A profile contains the initialization settings needed for communication between a device and device driver. The data in a profile is used by VWorks or BenchWorks software to identify each device on the network.

A profile can also contain other basic settings that you are unlikely to change once set up.

Because profiles identify device driver devices on the network, each device driver device must have its own profile.

You can create, modify, and delete profiles as needed.

Stored settings

Profiles are stored in the Windows registry.

The settings stored in a device driver profile include:

- ☐ Whether the device is connected using serial or Ethernet
- ☐ If the device is connected using Ethernet, the Device ID of the device on the network
- ☐ If the device is connected using serial, the COM port that the controlling computer uses for communication
- ☐ Configuration of accessories

Related topics

For information about...	See...
Device drivers	"About device drivers" on page 7
Adding a device to the device manager	"Adding devices" on page 10
Opening device diagnostics	"Opening diagnostics" on page 12

Setting the properties for a device

About this topic

The device properties provide VWorks or BenchWorks software with additional information about the device’s current configuration, such as which profile to use, and stores the information in the device file. The device file is automatically loaded when you open a protocol.

The device properties need to be set when configuring the device. Typically, these properties only need to be set once. This topic describes how to set the following device properties:

☐ General

☐ Teachpoint

☐ Barcode

☐ Location (for devices with multiple teachpoints)

☐ Device Properties

Read this topic if you are an administrator in charge of managing Velocity11 devices.

Before you start

Make sure that you have installed the device driver plug-in and have added the device to the device manager.

See “Related information” for procedures on how to do these tasks.

Setting general properties

To set the general properties for a device:

1. Click the **Device Manager** tab.

2. Select the device from the **Device List** toolbar. (Expand the device name, if necessary.)

Note: For devices with **Locations**, see “Setting location properties” on page 17. If no Locations, continue with step 3.

3. In the **General** group, set the following:

a. **Approach height.** This is the height to raise the robot gripper above the teachpoint when the robot moves the plate horizontally towards or away from it.

General	
Device name	VCode
Device type	VCode (3k) Bar Code Print and Apply Station
Approach height (mm)	11
Allowed / prohibited labware	
Teachpoints	
Bar code Readers	
"VCode (3k) Bar Code Print and Apply Station"	

b. **Allowed/prohibited labware.** Click the adjacent field to open the dialog box. Move the labware classes by selecting them and clicking one of the arrow buttons.

4. In the **Device Properties**, select the desired profile if it is not already selected.

5. Select **File > Device File > Save** to save the changes to the device file.

Setting teachpoints

Teachpoints are the coordinates in space that a robot travels to in order to interact with a device. Only the devices that are accessible by robots are able to have teachpoints.

To set the teachpoint properties:

1. Open the **Device Properties** page.
2. In the **Teachpoints** property group, set the following:
 - a. **Device is accessible from robot *robot's name***. Choose **Yes** or **No**.

Teachpoints	
Device is accessible from robot "robot"	Yes
Teachpoint for robot "robot"	No
Bar code Readers	
Device has south side BCR	No
Device has west side BCR	No

- b. **Teachpoint for robot *robot's name***. Choose a file.

Teachpoints	
Device is accessible from robot "Robot"	Yes
Teachpoint for robot "Robot"	Teachpoint 1
Bar code Readers	
Device has south side BCR	No
Device has west side BCR	No

Setting barcode location

If your device has a barcode reader, indicate where the reader is located.

To set the barcode readers property:

1. In the **Barcode Readers** property group, set the side that has the barcode to **Yes**.

Bar code Readers	
Device has south side BCR	Yes
South side BCR COM port	
Device has west side BCR	No
Device has north side BCR	No
Device has east side BCR	No

2. Enter the number of the COM port to which the device is connected.

Setting location properties

Note: The options available under Location groups might differ for software and hardware device drivers. Software devices do not have robot-accessible labware positions.

For hardware devices that have more than one robot-accessible labware position, the approach height, allowable/prohibited labware, teachpoint, and barcode properties are located under Location groups.

To set the Location properties:

1. *Hardware device drivers only.* Set the **Use linked location**. Follow the procedure in "Setting the Use linked location" on page 18.
2. *Hardware device drivers only.* Set the **Teachpoints**. Follow the procedure in "Setting teachpoints" on page 17.

3. *Some software device drivers only.* Set the **Approach height** and **Allowed/prohibited labware**. Follow the procedure in “Setting general properties” on page 16.
4. Set the **Barcode Readers** location. Follow the procedure in “Setting barcode location” on page 17.
5. Assign the **Labware** used by the location by selecting the correct labware type from the list.

Location 'Stage1'	
Use linked location	No
Location is accessible from robot 'StaubliRobot'	Yes
Teachpoint for robot 'StaubliRobot'	
Approach height (mm)	9
Allowed / prohibited labware	
Location 'Stage1' has south side BCR	No
Location 'Stage1' has west side BCR	No
Location 'Stage1' has north side BCR	No
Location 'Stage1' has east side BCR	No
Labware	1536 Greiner 783092 P5 blk clr btm LoBase
Location 'Stage2'	

6. In the **Device Properties**, select the desired profile if it is not already selected.
7. Select **File > Device File > Save** to save the changes to the device file.

Setting the Use linked location

Currently, this feature is enabled for the special situations in which there is a storage device such as a PlateHub Carousel, StoreX, or Cytomat and a robot, such as the Velocity11 Translator robot that is shuttling plates between systems.

To use this feature, select yes and then select the device location to which you want to link. This tells the software that the current device location is the same physical location as the device selected from the Device to use list.

Note: Selecting this option when it is not enabled will have no effect on the system.

Location 'Stage1'	
Use linked location	Yes
Device to use	Staubli
Location is accessible from robot 'Staubli'	Staubli
Approach height (mm)	TecanEvo

Related topics

For information about...	See...
Device drivers	“About device drivers” on page 7
Installing a device driver plug-in	“Installing device drivers” on page 9
Profiles	“About profiles” on page 15
Adding a device to the device manager	“Adding devices” on page 10
Opening diagnostics	“Opening diagnostics” on page 12

Adding and linking Sub Process tasks

About this topic

This topic describes how to add a sub-process to a protocol and configure it. Read this topic if you are an administrator or technician and are responsible for creating protocols in VWorks or BenchWorks software.

Before you read this


Before you read this topic, become familiar with the topics in the *VWorks Version 3 Automation Control User Guide* or *BenchWorks Automation Control User Guide* describing what a protocol is and how it is created.

Sub Process task defined

Sub Process tasks indicate the existence of a subroutine within a protocol. Sub-processes typically contain a series of liquid handling tasks used by devices such as the VPrep Pipettor or Multimek dispenser.


Adding a Sub Process task

The first step in creating a pipette process is to add a Sub Process task to the protocol editor. Drag the Sub Process icon into the process.

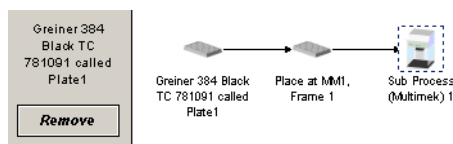

Setting Sub Process task parameters


When you add the Sub Process task, a new sub-process is started in the pipette process editor. This process is identified by its sub-process link icon.



Because you can have more than one sub-process in a protocol, you must link the Sub Process task to the correct sub-process.

To link the Sub Process task to the correct sub-process:

1. In the **Protocol Editor**, add a Sub Process task to the protocol and then select it in the protocol sequence.
2. In the **Protocol Task Parameters** toolbar, select the sub-process that you want to use for this pipetting task from the **Use Sub Process** list.

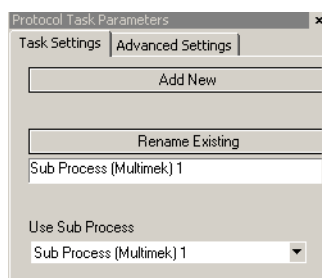

3. If there is only one sub-process and you need to create a second one, click **Add New**.

Associating the sub-process to a device


Because you can have more than one device that uses sub-processes on a lab automation system, you must link each sub-process link icon with one or more devices that you want the sub-process to be able to use. You do this by setting the parameter for the sub-process link icon.

To link a Sub Process task to a device:

1. In the **Pipette Process Editor**, select the **Sub Process** link icon.



2. In the **Available devices** list of the **Pipette Task Parameters** toolbar, select one or more pipettors to link to and click **Add**.

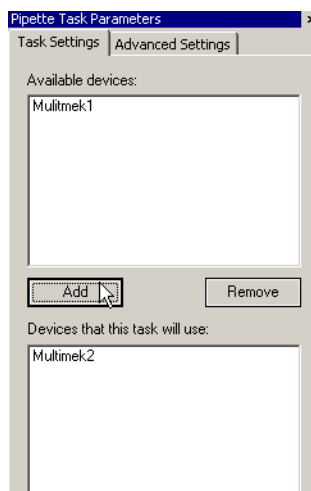

The selected pipettors move to the lower box and become available for use.

Related topics

For information about...	See...
Device drivers	"About device drivers" on page 7
Setting common device properties	"Setting the properties for a device" on page 16
Adding a device to the device manager	"Adding devices" on page 10
Creating protocols	<input type="checkbox"/> <i>VWorks Version 3 Automation Control User Guide</i> <input type="checkbox"/> <i>BenchWorks Automation Control User Guide</i>

Using JavaScript to set task parameters

About this topic

JavaScript programs (scripts) can be used to change the parameters of a protocol task immediately before it is scheduled. This extends the capability of VWorks or BenchWorks software because the parameters can be changed dynamically during a run, based on the following:

- ☐ Information passed from an external source, such as a database
- ☐ The number of times the protocol has cycled
- ☐ Feedback on changing conditions during the run

This topic describes the use of JavaScript to set task parameters in a protocol.

Read this topic if you are an administrator or technician responsible for creating VWorks or BenchWorks software protocols and want to add functionality to a task using JavaScript.


Where scripts are written

Scripts can be written in two ways:

- ☐ Directly into the box in the Advanced Settings tab of the Task Parameters toolbar
- ☐ As an external file that is located by clicking Browse in the Advanced Settings tab and navigating to its location on the hard drive

Note: You can also call an external file by embedding the "open () " function in the box.

The following screenshot displays a short script that prints the parameters of a task to the log toolbar, just before the task runs. In this case, the script is written directly in the Advanced Settings box.

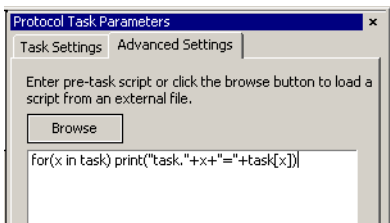

For more information about using JavaScript, refer to the *VWorks Version 3 Automation Control User Guide* or the *BenchWorks Automation Control User Guide*.

Related topics

For information about...	See...
Using JavaScript in protocols	<div><input type="checkbox"/> <i>VWorks Version 3 Automation Control User Guide</i></div> <div><input type="checkbox"/> <i>BenchWorks Automation Control User Guide</i></div>
Adding tasks to protocols	<div><input type="checkbox"/> <i>VWorks Version 3 Automation Control User Guide</i></div> <div><input type="checkbox"/> <i>BenchWorks Automation Control User Guide</i></div>

About reader output files

About this topic

Plug-in device drivers that are written for plate readers have a common way of naming their output files. This topic explains the concepts related to output file naming. By reading this topic, you will learn how to prevent data in the reader output files from being overwritten by newer data.

Read this topic if you are an operator who wants to make changes to the task parameters for one of these readers:

- ☐ VR4000
- ☐ Analyst GT
- ☐ Fusion
- ☐ Viewlux
- ☐ Tecan readers

Plug-in default output file

When you first install a reader device driver plug-in, all data recorded during a protocol or by a manual read using diagnostics software is written to a single file stored in the C: drive.

The exact name of the file is specific to the device. For example, the RVSI VR4000 device driver creates a file with the name vialreaderresults.txt.

This file can only store data for one read, which means that the set of data for each read overwrites the last set in the file. To avoid this problem you must set up an output file naming convention.

Profile default output file name

Some device drivers allow more than one device of that type to be used in the lab automation system. In this case, each device must have its own profile. Even if you have only one device, you can still set up multiple profiles for it, with each storing different settings.

In these cases, you probably want each profile to have a separate default output filename to prevent the data from runs using one profile overwriting those of another.

Filename suffixes


To prevent the data from one read overwriting the data from another, you need to append a variable suffix to the file name. You can append a date/time stamp and one or more bar codes on the rack or plate.

Append the following to the output filename:

- ☐ Date/timestamp
- ☐ South bar code
- ☐ West bar code
- ☐ North bar code
- ☐ East bar code

Example

The example output file folder below shows that a profile default file name of output.txt was created at one time. At another time, a suffix was appended in the profile for the device driver, which added a barcode identifier to the file name (for example output_C100040329.txt).

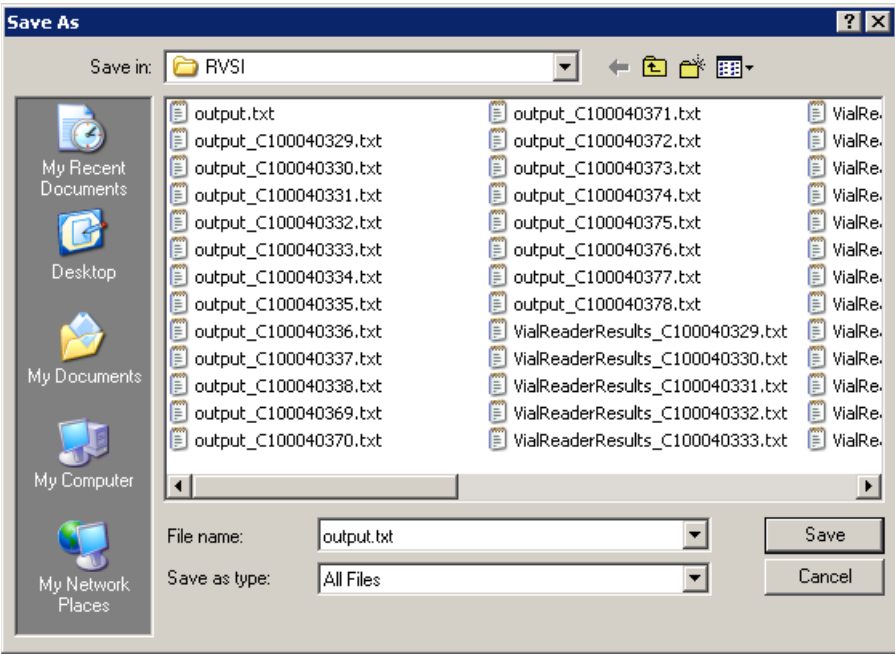

Overriding output file names with tasks

You can override the default output file name that is set in the profile using the Output filename property of the Read task parameters.

"Read tubes" properties	
Use tubes expected parameter	No
Tubes expected (0-96)	96
Output filename	

This allows you to use different output file names for every task. The suffix used for the file name that you set in the task parameters is taken from the suffix specified in the device diagnostics profile. So if you select date/time stamp in the profile, the date/time stamp will also be appended during a run in which you have specified a different file name.

Related topics

For more information about...	See...
Opening diagnostics	"Opening diagnostics" on page 12
Profiles	"About profiles" on page 15

About device initialization

About this topic	When working in device diagnostics software, you are often required to initialize the device. This topic explains why device initialization is necessary.
Opening communications	Initializing a device opens communications with it. For example, if the device is connected with a serial cable, the COM port is opened, and if the device is connected with an Ethernet cable, the TCP/IP socket is connected.
Homing motors	<p>Initializing a device homes motors that do not track their position along their line of travel. Homing a motor moves it until it triggers an event, called a home flag. This tells the motor its location.</p> <p>The motors on some devices automatically move to their home positions when the device is turned on. The motors on other devices must be initialized to be homed.</p>
Setting profile parameters	Initializing a device applies relevant parameters set in the device's profile.
Setting state and memory variables	Most devices store variables in software or firmware. Initializing a device sets these variables to their initial values.

Related topics

For information about...	See...
Using Diagnostics	<input type="checkbox"/> "About diagnostics" on page 11 <input type="checkbox"/> "Opening diagnostics" on page 12
Workflow for configuring devices	"Adding devices" on page 10

Labcyte Echo 550

2

The Labcyte Echo 550 is a liquid handler optimized for transferring volumes as low as 2.5 nL of DMSO/water solutions between microplates with any-well to any-well capability, coupled with any volume transfers. It can be configured to work in lab automation systems running VWorks or BenchWorks software.

- ☐ “Workflow for configuring Labcyte Echo 550 devices” on page 28
- ☐ “Creating a Labcyte Echo 550 profile” on page 29
- ☐ “Setting Labcyte Echo 550 task parameters” on page 31
- ☐ “Operating the Labcyte Echo 550 with diagnostics” on page 36
- ☐ “Managing Labcyte Echo 550 profiles” on page 38

Workflow for configuring Labcyte Echo 550 devices

About this topic

This topic gives the workflow for configuring the Labcyte Echo 550 device driver.

Read this topic if you are an administrator responsible for setting up devices in VWorks or BenchWorks software.

Before you start

Before you can configure the Labcyte Echo 550 device driver it must be installed.

!! IMPORTANT !! To launch the Labcyte client software from Velocity11 Labcyte Echo 550 Diagnostics, the Labcyte client software must be installed on the computer that is running VWorks or BenchWorks software.

Workflow

Step	Topic
1	"Adding devices" on page 10
2	"Creating a Labcyte Echo 550 profile" on page 29
3	"Setting the properties for a device" on page 16

Related information

For information about...	See...
Device drivers	"About device drivers" on page 7
Device driver installation	"Installing device drivers" on page 9
Opening diagnostics	"Opening diagnostics" on page 12
Setting Labcyte Echo 550 task parameters	"Setting Labcyte Echo 550 task parameters" on page 31
Using Labcyte Echo 550 Diagnostics	"Operating the Labcyte Echo 550 with diagnostics" on page 36

Creating a Labcyte Echo 550 profile

About this topic

This topic describes how to create a profile for the Labcyte Echo 550 in VWorks or BenchWorks software.


Before you start

Before you can create a profile, you need to have installed the device driver and added the Labcyte Echo 550 to the device manager.

Procedure


To create a Labcyte Echo 550 profile:

1. Open **Labcyte Echo 550 Diagnostics**.
2. Click the **Profiles** tab.
3. In the **Profile Management** area, click **Create a new profile**.

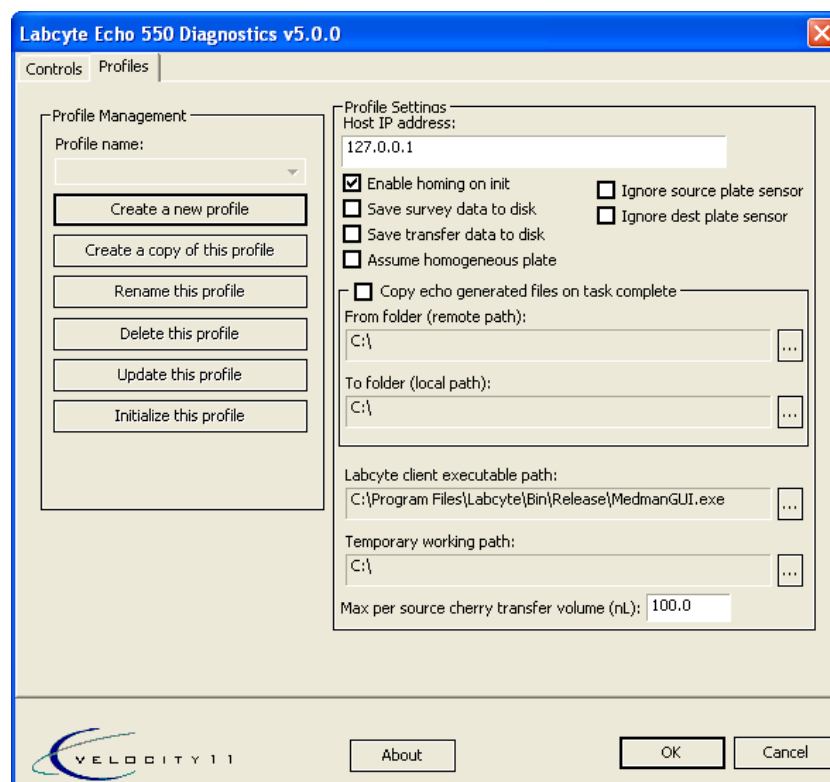

4. In the **New Profile** dialog box, enter a name for the profile and click **OK**. The name appears in the **Profile name** list.
5. In the **Profile Settings** area, set the following:

Setting	Comment
Host IP address	Input for the IP address of the Labcyte Echo 550 computer.
Enable homing on init	Homes the source and destination stages when initializing the device.

Setting	Comment
Save survey data to disk	Saves survey data collected prior to each transfer.
Save transfer data to disk	Saves transfer data, specifying which wells have failed transfer.
Assume homogeneous plate	Select if all plate wells are known to have consistent fluid fill volumes and solvent concentrations.
Ignore source plate sensor	Bypasses the source plate present sensor. This may be useful when an individual source plate does not fit correctly and you want to run a protocol without triggering a “no source plate loaded” error message.
Ignore dest plate sensor	Bypasses the destination plate present sensor. This may be useful when an individual destination plate does not fit correctly, or droplets are being transferred to a microplate lid or other substrate that does not fit like a microplate and you want to run a protocol without triggering a “no destination plate loaded” error message.
Copy echo generated files on task complete	<p>Copies files generated by transfer or survey to a user designated location. Enter the remote and local paths.</p> <p>Click the ellipsis () to open the Browse for folder dialog box and locate a directory.</p>
Labcyte client executable path	Designates the path to the Labcyte client software or any other user specified application launched with the Launch Labcyte client command on the Controls tab.
Temporary working path	Designates an empty directory to hold the temporary files created when one .csv file is split into multiple files in order to override the maximum liquid transfer volume cap.
Max per source cherry transfer volume (nL)	<p>Sets the maximum transfer volume in order to control the maximum volume dispensed to each well. This cap can be overridden by using multiple transfers.</p> <p>The generated data in multiple files is sent to the Temporary working path.</p>

6. Click **Update this profile** to save the profile.

Related information

For information about...	See...
Adding the Labcyte Echo 550 to the device manager	"Adding devices" on page 10
Profiles	"About profiles" on page 15
The next step	"Setting Labcyte Echo 550 task parameters" on page 31
The workflow to which this procedure belongs	"Workflow for configuring Labcyte Echo 550 devices" on page 28
Adding, deleting, and editing Labcyte Echo 550 profiles	"Managing Labcyte Echo 550 profiles" on page 38
Opening diagnostics	"Opening diagnostics" on page 12
Using Labcyte Echo 550 Diagnostics	"Operating the Labcyte Echo 550 with diagnostics" on page 36

Setting Labcyte Echo 550 task parameters

About this topic

When you add an Labcyte Echo 550 task to a protocol, you need to set the parameters for the task. This topic describes how to set Labcyte Echo 550 device driver task parameters. Read this topic if you are:

- ☐ An administrator or technician responsible for creating protocols in VWorks or BenchWorks software
- ☐ An operator who wants to make changes to the Labcyte Echo 550 task parameters in a protocol


Note: Only the administrator can save changes made to the task parameters.

About Labcyte Echo 550 tasks

There are four tasks and a pipetting sub-process associated with Velocity11 Labcyte Echo 550 device driver:

- ☐ Retract And Close (Labcyte Echo 550)
- ☐ Survey (Labcyte Echo 550)
- ☐ Cherry Transfer (Labcyte Echo 550)
- ☐ Standard Transfer (Labcyte Echo 550)
- ☐ Sub Process (Labcyte Echo 550)

These tasks are represented by the following icons in the Protocol Tasks toolbar.

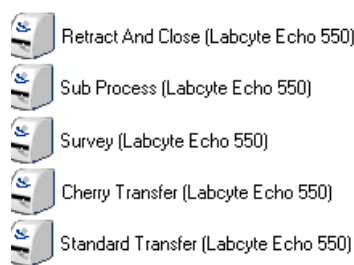


Task	Function	VWorks or BenchWorks Editor
Retract And Close	Retracts the source or destination stage into the instrument and closes the door.	Pre-Protocol Post-Protocol
Sub Process	Inserts a subroutine containing liquid handling tasks into the protocol,	Protocol
Survey	Records reflection amplitudes from the microplate and fluid surfaces, the results of which are used to optimize the delivered acoustic transfer wave.	Protocol
Cherry Transfer	Selects single or multiple liquid transfers.	Pipette Process
Standard Transfer	Transfers liquids from all plate wells in a single task execution.	Pipette Process

Before you start

Before you start, you must have created a protocol in the software that runs the Labcyte Echo 550. For information about setting up a protocol, see the Labcyte Echo 550 user documents.


- Configuring task settings
- To set the Retract And Close (Labcyte Echo 550) task parameters:**
 1. Add the Retract And Close (Labcyte Echo 550) task to the Pre- or Post-Protocol Editor.
 2. Click the **Task Settings** tab from the **Pre/Post Protocol Task Parameters** toolbar.
 3. In the left-hand field, select the Labcyte Echo 550 stage that you want to retract.
 4. Click **Add**. The selected Labcyte Echo 550 stage moves to the right-hand field and is chosen for protocol execution.

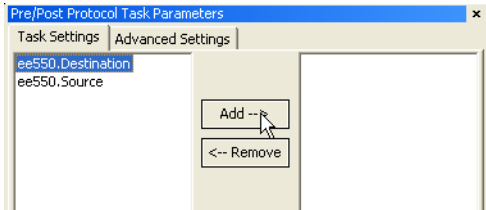

To set the Sub Process (Labcyte Echo 550) task parameters:


Note: Adding a Sub Process task to the Protocol Editor enables you to create a fluid transfer process.

1. Add the Sub Process (Labcyte Echo 550) to the **Protocol Editor**.
2. Click the **Task Settings** tab from the **Protocol Task Parameters** toolbar.
3. Click **Add new process** to create a new Sub Process task.
4. Click **Rename process** to assign a name to a Sub Process task.
5. Select the desired Sub Process task from the **Use Sub Process** list.

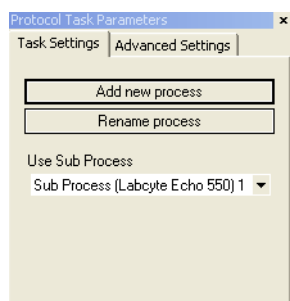


To set the Survey (Labcyte Echo 550) task parameters:

1. Add the Survey task to the **Protocol Editor**.
2. Click the **Task Settings** tab from the **Protocol Task Parameters** toolbar.
3. In the left-hand field, select the Labcyte Echo 550 stage that you want to survey.
4. Click **Add**. The selected Labcyte Echo 550 stage moves to the right-hand field and is chosen for protocol execution.

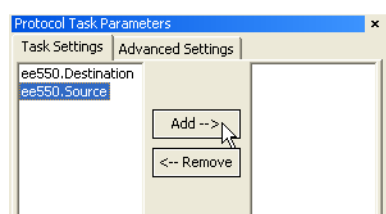


5. Set the **“Survey”** properties.

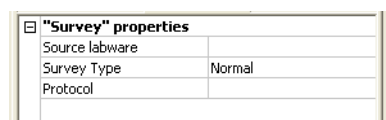

Property	Setting
Source labware	Select the plate to be accessed.
Survey Type	Select the mode of survey (Normal, Fast, or For Transfer).
Protocol	Select a Labcyte Echo 550 protocol.

To set the Cherry Transfer (Labcyte Echo 550) task parameters:


1. Add the Cherry Transfer task to the **Pipette Process Editor**.
Note: This task is only available in the Pipette Process Editor.
2. Click the **Task Settings** tab from the **Pipette Task Parameters** toolbar.
3. Set **“Cherry Transfer”** properties.

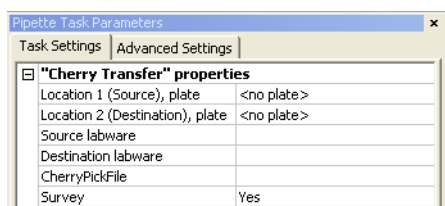

Property	Setting
Location 1 (Source)	Select the stage with the plate with fluids to be transferred.
Location 2 (Destination)	Select the stage with the plate receiving the fluids.
Source labware	Select the type of plate holding the fluids. <i>Note:</i> This parameter is populated after communication with the Labcyte server.
Destination labware	Select the type of plate receiving the fluids. <i>Note:</i> This parameter is populated after communication with the Labcyte server.
CherryPickFile	Select the file containing the locations of the wells for fluid transfer.
Survey	Select whether to execute a survey or not.

To set the Standard Transfer (Labcyte Echo 550) task parameters:

1. Add the Standard Transfer task to the **Pipette Process Editor**.
Note: This task is only available in the Pipette Process Editor.
2. Click the **Task Settings** tab from the **Pipette Task Parameters** toolbar.
3. Set **“Standard Transfer”** properties.

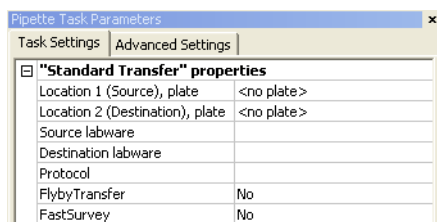

Property	Setting
Location 1 (Source)	Select the location of plate from where the samples are accessed.
Location 2 (Destination)	Select the location of plate to where samples are to be transferred.
Source labware	Select the type of plate used for the source samples. <i>Note:</i> This parameter is available after communication with the Labcyte server.
Destination labware	Select the type of plate used for the destination. <i>Note:</i> This parameter is available after communication with the Labcyte server.
Protocol	Select a protocol. <i>Note:</i> This parameter is available after communication with the Labcyte server.
FlybyTransfer	Select this to perform fluid transfers without stopping beneath each well. The acoustic pulse will be generated, and the droplet ejected while the acoustic transducer continues to move. This type of fluid transfer can improve throughput, but it is dependent on a consistent well volume and DMSO/ water ratio.
FastSurvey	Select this option to survey a representative sample of wells and to use that data to estimate the other wells.

Related information

For information about...	See...
Configuring the Labcyte Echo 550	"Workflow for configuring Labcyte Echo 550 devices" on page 28
Adding the Labcyte Echo 550 to the device manager	"Adding devices" on page 10
Using Labcyte Echo 550 Diagnostics	"Operating the Labcyte Echo 550 with diagnostics" on page 36

Operating the Labcyte Echo 550 with diagnostics

About this topic


This topic describes how to:

- ☐ Perform a manual transfer
- ☐ Perform a manual survey
- ☐ Launch the Labcyte client software (from Vworks or BenchWorks software)
- ☐ Manage profiles


Procedures

To perform a manual transfer:

1. Open the Labcyte Echo 550 Diagnostics.
2. Click the **Controls** tab
3. Place a source plate on the Labcyte Echo 550.
 - a. In the **Source Stage** area, select an Labcyte Echo 550 plate definition from the **Select plate definition** list.
 - b. Click **Extend stage**.
 - c. Place a plate on the stage that matches the selected definition.
 - d. Click **Retract stage**.

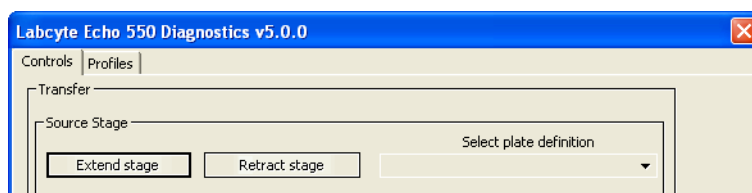


4. Place a destination plate on the Labcyte Echo 550.
 - a. In the **Destination Stage** area, select a Labcyte Echo 550 plate definition from the **Select plate definition** list.
 - b. Click **Extend stage**.
 - c. Place a plate on the stage that matches the selected definition.
 - d. Click **Retract stage**.



5. At the bottom of the **Transfer** area, select an existing protocol from the **Select transfer protocol** list.

Note: Select **Flyby transfer** to scan across the plate without stopping. See “FlybyTransfer” on page 35.

6. Click **Execute protocol**.




To perform a plate survey:

1. Open the **Labcyte Echo 550 Diagnostics**.
2. Click the **Controls** tab
3. Place a source plate on the Labcyte Echo 550.
4. Click **Retract Stages and Close Door**.
5. Click **Survey source plate**.

Note: Use **Fast Survey** to analyze a representative sample of source microplate wells.

During a **Fast Survey**, data for unsurveyed wells is interpolated. For a fast survey to be accurate, the microplate contents must be homogenous in nature: that is, all wells must have consistent fluid fill volumes and solvent concentrations.




To launch the Labcyte client:

1. Open the **Labcyte Echo 550 Diagnostics**.

Note: To launch the Labcyte client from Velocity11 Labcyte Echo 550 Diagnostics, the Labcyte Echo 550 device driver and the Labcyte client software must be installed on the same computer.

2. Click the **Controls** tab
3. Click **Launch Labcyte client** to open the Labcyte Echo 550 software.

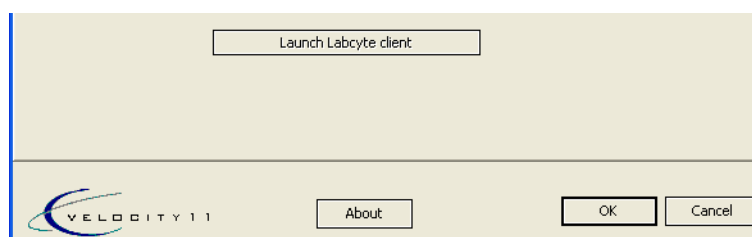

Related information

For information about...	See...
Opening Labcyte Echo 550 Diagnostics	"Opening diagnostics" on page 12
Configuring the Labcyte Echo 550	"Workflow for configuring Labcyte Echo 550 devices" on page 28

For information about...	See...
Setting up devices	“Setting the properties for a device” on page 16
Setting Labcyte Echo 550 task parameters	“Setting Labcyte Echo 550 task parameters” on page 31

Managing Labcyte Echo 550 profiles


About this topic

This topic describes how administrators and technicians can manage Labcyte Echo 550 profiles.

Managing profiles

To manage Labcyte Echo 550 profiles:

1. Open **Labcyte Echo 550 Diagnostics**.
2. Click the **Profiles** tab.

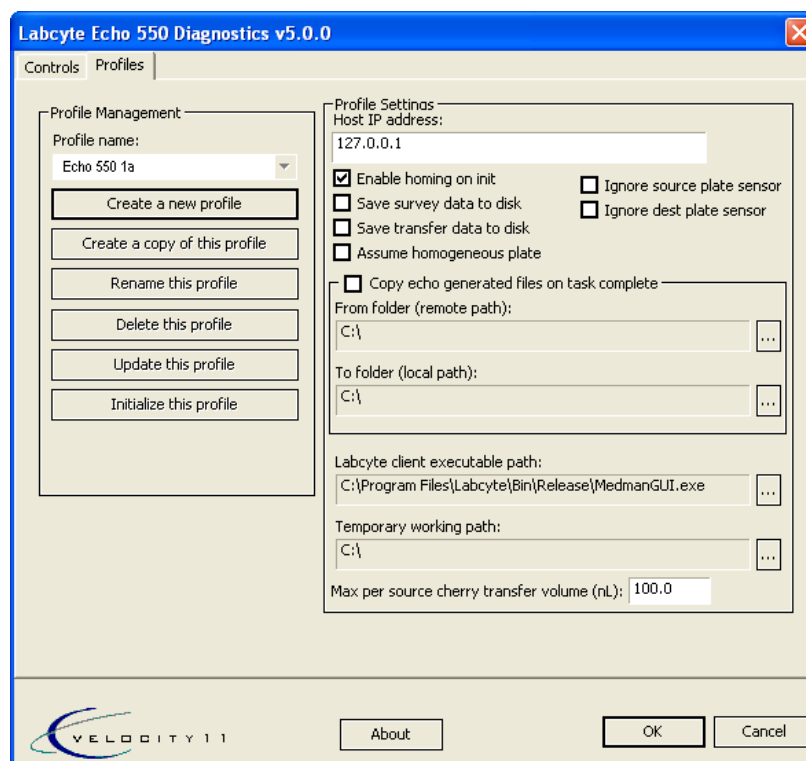

3. Select a profile from the **Profile name** list.
4. Perform management tasks.

Management tasks include the following:

- ◆ Updating the profile

- ◆ Copying a profile
- ◆ Renaming a profile
- ◆ Deleting a profile
- ◆ Saving changes to a profile

Note: Click **Update this profile** to save edits.

Related topics

For more information about...	See...
Opening diagnostics	"Opening diagnostics" on page 12
The workflow for configuring the Labcyte Echo 550	"Workflow for configuring Labcyte Echo 550 devices" on page 28
Creating an Labcyte Echo 550 profile	"Creating a Labcyte Echo 550 profile" on page 29
Operating the Labcyte Echo 550	"Operating the Labcyte Echo 550 with diagnostics" on page 36



User Guide
G5415-90026