


De-risk probe: Soft posterior stays calibrated under real Tigress obfuscation (GO)

Calibration survives — raw stays low, fully recalibratable



Discrimination holds — no collapse toward chance

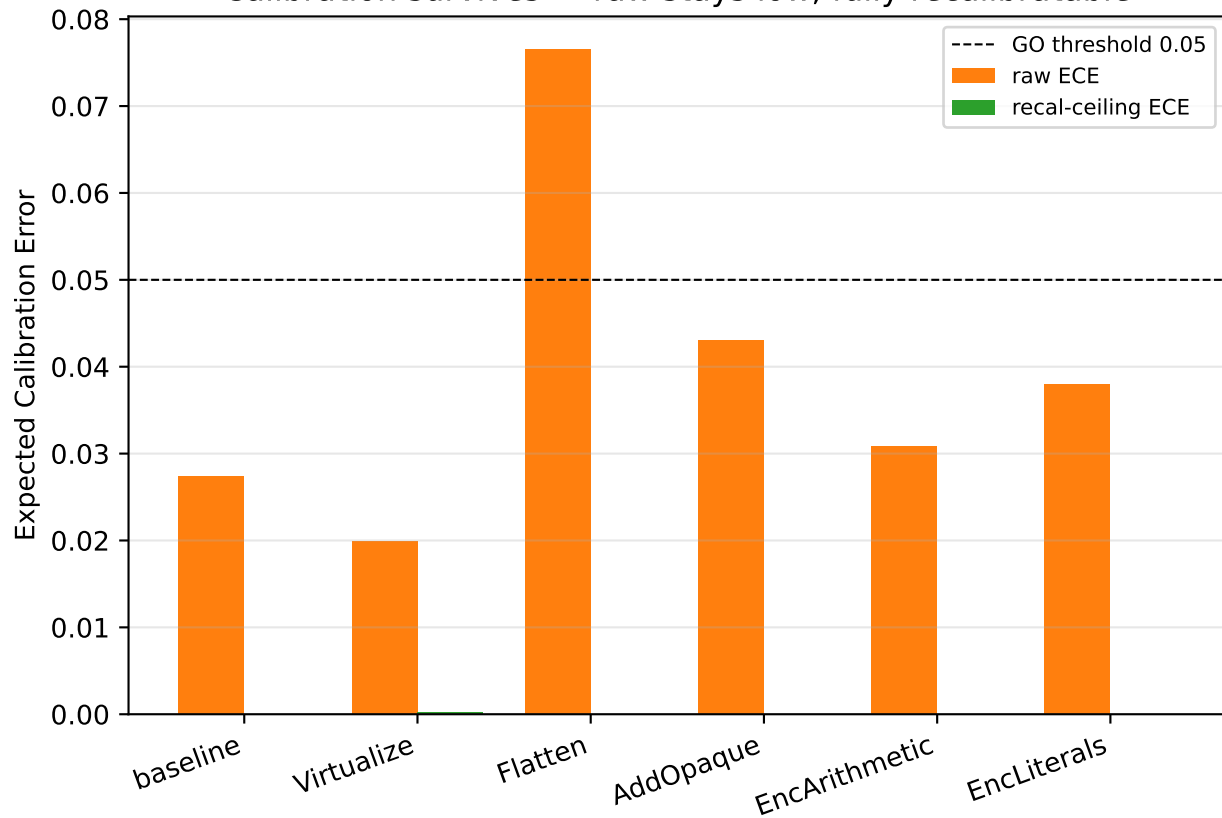