

Internal Volume Measurement Device

Tym Pakulski - University of Bath

September 2013 - August 2014

Contents

0.1	Introduction	1
0.1.1	Theory	2
0.1.2	Specifications	3
0.1.3	State of the Project	3
0.2	Instrumentation and DAQ	5
0.2.1	Bronkhorst Flow Controllers	5
0.3	Problems with Flow Controllers	6
0.3.1	DAQ	6
0.4	Analysis tools	7
0.5	Recommendations	7

0.1 Introduction

Leak testing of the various CMS cooling systems is a regular exercise that currently relies on a 'rule of thumb' approach to test specifications. True allowable leak rates are defined in terms of a percent of total internal volume per unit time, but exact numbers for the internal volumes of the various subsystems are difficult to establish. A device that can measure the internal volume of existing systems would be useful to quantify allowable leak rates and streamline the leak testing process. This report documents the proof-of-concept phase of a rig that will be used to measure internal volumes by injecting them with gas and measuring the rate of pressure change.

Useful Contacts

- Norbert Frank: +41764873618, Norbert.Frank@cern.ch
- Patrick Carrier (for instrumentation): +41764870415, Patrick.Carrie@cern.ch
- Roberto Guida (for theory): +41764872146, Roberto.Guida@cern.ch
- Tym Pakulski: tsp26@bath.ac.uk

0.1.1 Theory

The volume measurement concept comes from the ideal gas law (1), and the equation for molar volume (2). It assumes constant temperature and volume. All units are S.I.

$$PV = nRT \quad (1)$$

$$V_{mol} = \frac{RT}{P} \quad (2)$$

$$\begin{aligned} n &= \frac{PV}{RT} \\ \frac{dn}{dt} &= \frac{V}{RT} \frac{dP}{dt} \\ \frac{dV_{in}}{dt} &= \frac{RT}{P} \frac{V}{RT} \frac{dP}{dt} \\ V &= \dot{V}_{in} dt \frac{P_1}{P_2 - P_1} \end{aligned} \quad (3)$$

An alternative derivation supplied by Roberto Guida assumes standard conditions to calculate the molar volume. While slightly more complex, this formulation has the advantage of taking flow controller readings directly as input, as it corrects for ambient temperature different from the flow controller calibration. See 0.2.1.

$$\begin{aligned} PV &= nRT \\ V_{mol} &= 22.4 \text{ [L]} \end{aligned} \quad (4)$$

$$\begin{aligned} n &= \frac{PV}{RT} \\ \frac{dn}{dt} &= \frac{V}{RT} \frac{dP}{dt} \\ \frac{dV_{in}}{dt} &= \frac{22.4 V}{R} \frac{dP}{T dt} \\ \dot{V}_{in} [\text{l}] &= 2.69 \frac{V}{T} \frac{P_2 - P_1}{dt} \\ V &= \frac{\dot{V}_{in}}{2.69} \frac{T}{P_2 - P_1} \\ V [\text{cm}^3] &= \frac{\dot{V}_{in} [\text{l}/\text{hour}]}{3600} \frac{dt [\text{s}]}{P_2 - P_1 [\text{bar}]} \frac{T [\text{°C}] + 273}{269} 1000 \end{aligned} \quad (5)$$

The concept can be implemented by moving gas from a high-pressure volume to the test volume at a known constant rate and measuring the change in pressure over time. The minimum apparatus to achieve this involves a pressurised gas bottle connected to a flow controller and a downstream pressure sensor, as shown in Figure 1.

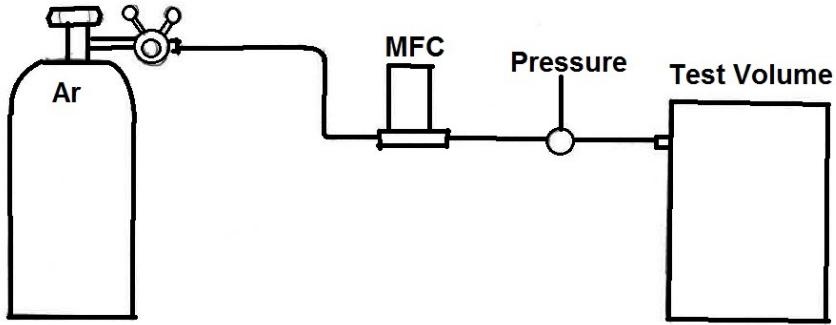


Figure 1: Schematic of the volume estimation concept

0.1.2 Specifications

The final product should be:

- Compact and transportable
- Simply designed and accessible for untrained users
- Sufficiently accurate to meet the leak test specification accuracy
- Usable without a laptop or expensive data logging equipment
- Self-sufficient in DAQ and practical for automated data analysis.

Accuracy Specification

The accuracy of the device is constrained by the allowable errors in the devices used. An error in the calculated volume will affect the accuracy of both the *allowable leak rate* and the *measured leak rate*.[1].

0.1.3 State of the Project

So far, the volume estimation concept has been tested using a pressure transmitter and DAQ of Norbert Frank's pressure decay measurement rig in building 27, shown in Figure 2. Two different flow meters have been used to measure the volume of a dive bottle.

Using the Building 27 Rig

DAQ is handled by a labVIEW module on the local PC. The .vi, saved to the desktop, is called *MAIN_ScanChannels.vi*. Tests can be run from the *Stand1*



Figure 2: The test rig in building 27.

tab on the front panel. The data for each test is saved to a .txt file in a folder at *C:/Project/PressureTest/Data/*. The useful channels are the time and the first pressure signal: *absSysPressure*. The PC also has installed Bronkhorst's Flow DDE and Flow Plot software, which can be used to change the flow controller set point and log its 3 channels through RS232. The current flow controller is connected to a local display for adjusting the set point. The password for the display is *abc*.

The rig is connected to the 15 L (true volume) dive bottle with 1/4" VCR fittings. The bottle's volume was confirmed by filling it with water and measuring its change in weight.

The rigs gas inlet, purge line and fluid connection are controlled by valves shown in Figure 3.

Valve 4 connects to an unused part of the rig and is kept close to minimise pipe volume.

To run a test, open the *Stand1* tab of *MAIN_ScanChannels.vi* . Type in a name for the test and a start pressure. And click run. Open the valve on the gas bottle, and adjust the pressure reducer to match the calibration pressure of the flow controller. Then, adjust the set point of the flow controller. Ensure the valve between the pressure reducer and the flow controller is open, and the purge and differential valves on the rig are closed. Click the green button *Start DAQ*.

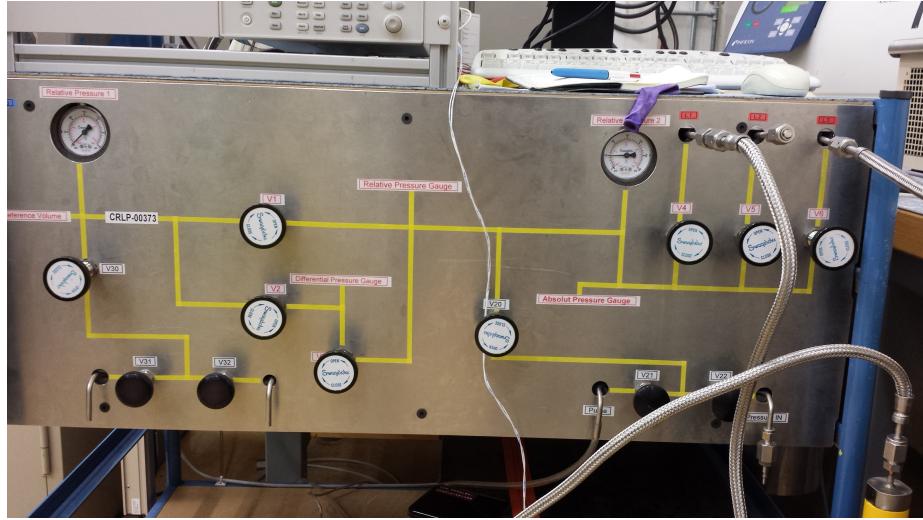


Figure 3: V6: fluid inlet, V4: Test volume, V20 and V21: Purge, V1 and V3: keep closed

0.2 Instrumentation and DAQ

0.2.1 Bronkhorst Flow Controllers

The first iterations of the rig have used Bronkhorst EL FLOW flow controllers. These were borrowed from Patrick Carier of the Gas Group in building 155.

Operating Principles

The controllers operate on the thermal mass flow principle, and measure the mass of fluid passing through their regulation valve as a function of the power needed to heat a temperature probe a set distance away in the flow. See appendix. The instruments take a L_n per minute set point via RS232 bus, which they convert for their grams per second control logic using equation (2). In other words, the instruments are calibrated for a specific fluid, inlet pressure and fluid temperature. **It is essential that these parameters are respected.**

In practice, this means using the correct fluid and adjusting the downstream pressure of the reducer to match the value specified in the controller firmware and typically marked on the side of the device. Ambient temperature is more difficult to adjust. Instead, it is good practice to check the calibration temperature, which is typically 273 K, and multiply the volumetric flow rate by a 'temperature gain', as shown in (6)

$$\dot{V}_{true} = \dot{V}_{setpoint} \frac{T_{true}[K]}{T_{calibrated}[K]} \quad (6)$$

Alternatively, the temperature gain can be applied to the calculated volume itself. If the derivation supplied by Roberto Guida is used, the temperature difference can be ignored.

0.3 Problems with Flow Controllers

Two major problems were encountered during early iterations of the project. The first version of the instrumentation seemed to exhibit random errors in calculated volume in the order of 10%, well beyond those predicted by theory. Second, an unexpected correlation between injection flow set point and calculated volume was observed. Both problems were resolved by a change of flow controller.

It appears the most likely explanation for the systematic error is a leak in the instrumentation section. In general, a faster flow rate means a larger integral of pressure with respect to time, which causes a higher net leak flow out of the system. Thus the higher the flow rate, the greater the error due to leaks. No leaks were found in several sniffer tests conducted with both CO_2 and helium. However, pressure drops in the instrumentation section consistent with a leak were observed. The random error in calculated volume was most likely due to temperature variations. Minor temperature variations first appeared trivial. While the temperature term is eliminated in the first formulation of the derivation used for data analysis, it can be expressed as a pressure error using the ideal gas law. The linear error implies that the typical 3 degree temperature fluctuations observed were insignificant.

However, the derivation itself rests on the assumption of constant temperature, and the 1 percent error is enough to invalidate the concept.

The new controller, with 10 times the maximum flow of the old one, eliminated the systematic error with leak tight connections, and led to fast-flow tests too short for significant temperature fluctuations. While the old controller required 8-14 hour tests for the 15 L volume, the new one could achieve 1 bar of dP in 30 minutes.

0.3.1 DAQ

Estimating volume requires, at a minimum, two data points of time and pressure and the flow set point. A temperature reading is useful to eliminate a minor systematic error if temperature is constant, or to detect a change in temperature that would void the test. More time and pressure data reduce random errors. The current rig measure pressure through a 4-20 mA current loop connected to a *LabVIEW* module. The software can log pressure and time in this way. Future iterations of the project will probably simplify the DAQ process by saving the current loop readings with time stamps to a USB storage device. This will allow the test to be run without a laptop.

0.4 Analysis tools

0.5 Recommendations

The next iteration of the product should evaluate its accuracy for smaller test volumes of 2-3 litres. If the system's performance meets accuracy specifications, focus can shift to selecting permanent components with the correct parameters. Future iterations should respect the following findings about the instrumentation

- The inlet pressure on the flow meter must match the calibration pressure in the firmware.
- The test volume temperature must be kept constant.
- Tests should be kept short to minimise temperature variation.
- A temperature gain should be applied to the calculated volume if rig temperature differs from the calibrated temperature.
- A fast flow meter in the order of 1 l/min appears to offer a good balance of short test duration and flexibility for test volumes of interest.
- The rig must be leak tight.
- The project will require a deeper understanding of the theory, especially the conversion between moles per second and $l_n s^{-1}$ made by the mass flow controllers. To decide which equation will be implemented in the future and how temperature deviations will be handled.

With instrumentation ordered, final design development should focus on the user experience, specifically the software. With 4-20 mA current readings saved to the USB drive, a simple program should be written to fetch the data. Once a minimum viable product has been established, two further developments are worth investigating:

Monitoring temperature

A temperature measurement is useful to be able to quantify the temperature gain that should be applied to the volume calculation to account for the difference in gas temperature and calibration temperature. Further, a running temperature measurement can be used to check whether significant temperature changes occur during the test, which would void the data.

The former could be achieved with something as simple as an analogue thermometer somewhere on the rig, assuming a constant temperature throughout the test. The latter would require dedicated hardware and DAQ to store the signals, which would likely be incompatible with the 4-20 mA pressure signals. With short tests, it can be argued that it is safe to assume constant temperature throughout the test.

Pressure decay test capability

The rig could also be used for pressure decay testing. By adding a valve upstream of the pressure sensor as shown in Figure 4, the pressurised test volume can be sealed, and the pressure transducer can be used to record pressure drop over time. This would prove particularly convenient in the CMS, as it

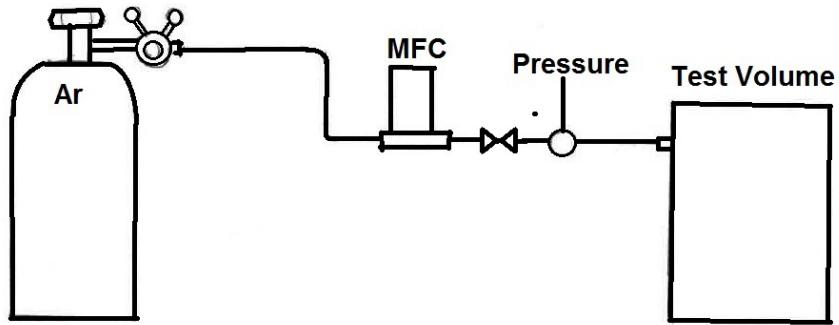


Figure 4: The volume estimation instrumentation with an added valve for pressure decay testing.

would allow both the volume estimation and the pressure decay test without purging the system or disconnecting the fittings. The device would first be connected to the pressure reducer and the test volume. Argon would be injected and pressure measured to calculate the volume. Then, the valve would be closed and pressure drop measured. With the pressure drop, the time, and the calculated volume, the leak rate can be calculated.

Bibliography

- [1] Paola Tropea *Procedures for the Construction and Testing of the Cooling Plants Built by the TS/CV/DC Section* 2006: TS Department, CERN