



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000


Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Interpretive Summary

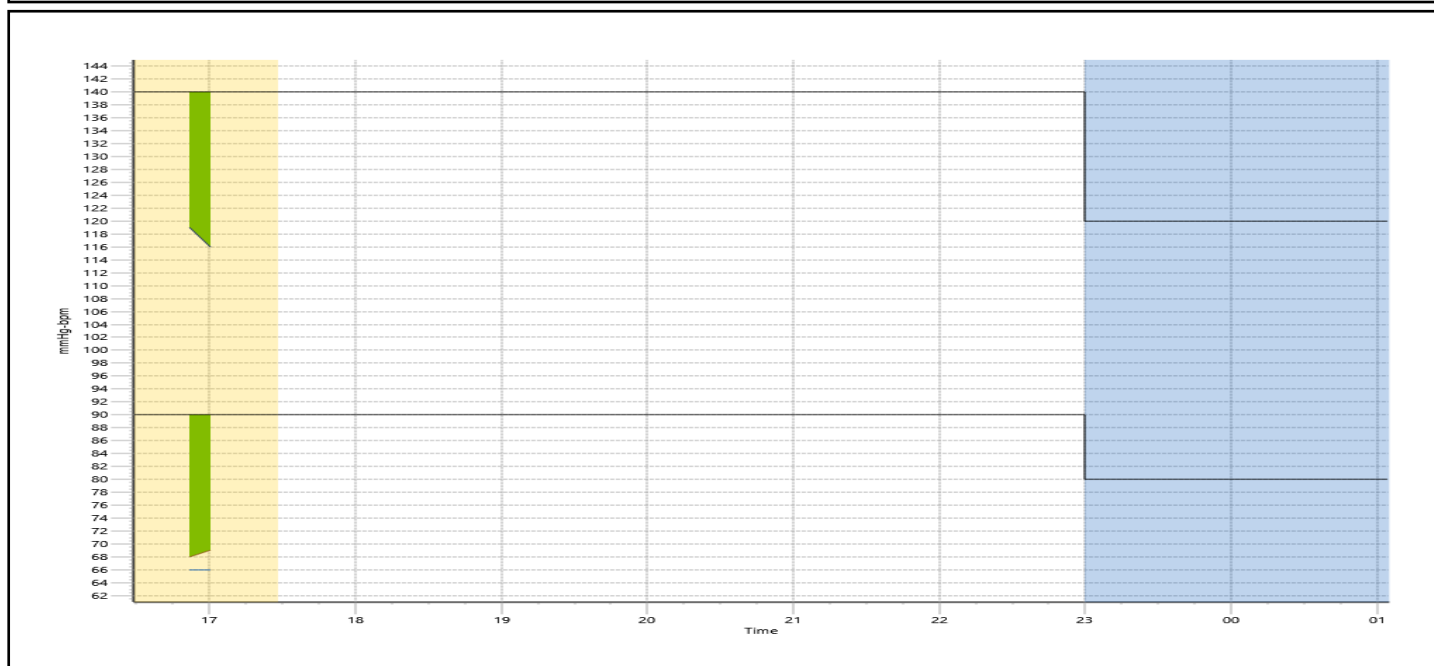

Brachial BP Results

Period	Time	Samples	Mean SYS mmHg (+/- Std.Dev)	Mean DIA mmHg (+/- Std.Dev)	Mean HR BPM (+/- Std.Dev)	BP Load Sys (%)	BP Load Dia (%)
Overall	16:29-19:04 (2:35)	2	118 (+/-2.1)	69 (+/-0.7)	66 (--)	0	0
Awake Period	07:00-23:00	2	118 (+/-2.1)	69 (+/-0.7)	66 (--)	0	0
Asleep Period	23:00-07:00	0	-- (--)	-- (--)	-- (--)	0	0
White Coat Period	16:29-17:28 (1st Hr.)	2				0	0
Max			119	69	66		
Mean			118	69	66		
Asleep Dip:	--/--						

Referring physician Dr.

Interpreting physician Dr.

Signature

Date

Signature

Date



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Patient Information

Weight : 177

Height : 6'1

Race :

Telephone :

Address :

Patient History

Current Medication

Physician Interpretation

Reason for Test



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

ABPM Statistics

Overall Period: Time: 16:29 - 19:04 Duration: 2:35 Samples: 2 of 10 (20%)

	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	118	+/-2.1	119 (16:51)	116 (17:00)		1.8%
DIA (mmHg)	69	+/-0.7	69 (17:00)	68 (16:51)		1.0%
HR (bpm)	66	--	66 (16:51)	66 (16:51)		--
MAP (mmHg)	85	--	85 (16:51)	85 (16:51)		--
PP (mmHg)	49	+/-2.8	51 (16:51)	47 (17:00)		5.7%
BP Load :	0% of SYS readings > 140 mmHg awake and > 120 mmHg asleep 0% of DIA readings > 90 mmHg awake and > 80 mmHg asleep					
Asleep Dip:	--/--					
AASI:	Unable to report					
Morning Surge:	Insufficient data to calculate					
Smoothness Index:						

Awake Period: Time: 07:00 - 23:00 Samples: 2 of 10 (20%)

	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	118	+/-2.1	119 (16:51)	116 (17:00)		1.8%
DIA (mmHg)	69	+/-0.7	69 (17:00)	68 (16:51)		1.0%
HR (bpm)	66	--	66 (16:51)	66 (16:51)		--
MAP (mmHg)	85	--	85 (16:51)	85 (16:51)		--
PP (mmHg)	49	+/-2.8	51 (16:51)	47 (17:00)		5.7%
BP Load :	0% of SYS readings > 140 mmHg 0% of DIA readings > 90 mmHg					

Asleep Period: Time: 23:00 - 07:00 Samples: 0 of 0 (0%)

	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	--	--	-- (---)	-- (---)		--
DIA (mmHg)	--	--	-- (---)	-- (---)		--
HR (bpm)	--	--	-- (---)	-- (---)		--
MAP (mmHg)	--	--	-- (---)	-- (---)		--
PP (mmHg)	--	--	-- (---)	-- (---)		--
BP Load :	0% of SYS readings > 120 mmHg 0% of DIA readings > 80 mmHg					

White Coat Period: Time: 16:29 - 17:28 Samples: 2 of 4 (50%)

	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	118	+/-2.1	119 (16:51)	116 (17:00)		1.8%
DIA (mmHg)	69	+/-0.7	69 (17:00)	68 (16:51)		1.0%
HR (bpm)	66	--	66 (16:51)	66 (16:51)		--
MAP (mmHg)	85	--	85 (16:51)	85 (16:51)		--
PP (mmHg)	49	+/-2.8	51 (16:51)	47 (17:00)		5.7%
BP Load :	0% of SYS readings > 140 mmHg 0% of DIA readings > 90 mmHg					



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Additional Time Periods

Time Period-1 Time: 07:00 - 23:00 Duration: 16:00 Samples: 2 of 10 (20%)						
	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	118	+/-2.1	119 (16:51)	116 (17:00)		1.8%
DIA (mmHg)	69	+/-0.7	69 (17:00)	68 (16:51)		1.0%
HR (bpm)	66	--	66 (16:51)	66 (16:51)		--
MAP (mmHg)	85	--	85 (16:51)	85 (16:51)		--
PP (mmHg)	49	+/-2.8	51 (16:51)	47 (17:00)		5.7%
BP Load : 0% of SYS readings > 140 mmHg awake and > 120 mmHg asleep 0% of DIA readings > 90 mmHg awake and > 80 mmHg asleep						
Time Period-2 Time: 23:00 - 07:00 Duration: 8:00 Samples: 0 of 0 (0%)						
	Mean	Std. Dev.	Max (time)	Min (time)	Above Threshold	CV
SYS (mmHg)	--	--	-- (--:--)	-- (--:--)		--
DIA (mmHg)	--	--	-- (--:--)	-- (--:--)		--
HR (bpm)	--	--	-- (--:--)	-- (--:--)		--
MAP (mmHg)	--	--	-- (--:--)	-- (--:--)		--
PP (mmHg)	--	--	-- (--:--)	-- (--:--)		--
BP Load : 0% of SYS readings > 140 mmHg awake and > 120 mmHg asleep 0% of DIA readings > 90 mmHg awake and > 80 mmHg asleep						



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Reviewed ABP Data

#	Time	SYS/DIA (mmHg)	HR (BPM)	MAP (mmHg)	Comment
3+	16:51	119/68	66	85	
4	17:00	116/69	66	85	
	17:11				Event marked
	15:23				Event marked
	15:23				Low battery
	15:23				Low battery
	15:57				Low battery
	15:57				Low battery



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Omitted ABP Data

#	Time	SYS/DIA (mmHg)	HR (BPM)	MAP (mmHg)	EC
1	16:29	--/--	--	--	87
2	16:33	--/--	--	--	87
5	18:00	--/--	--	--	87
6	18:04	--/--	--	--	87
7	18:30	--/--	--	--	87
8	18:34	--/--	--	--	86
9	19:00	--/--	--	--	87
10	19:04	--/--	--	--	86

Events Marked

#	Time	Event Code	Comment
1	17:11	107	Study End
2	15:23	107	Study End
3	15:23	94	Low battery
4	15:23	94	Low battery
5	15:57	94	Low battery
6	15:57	94	Low battery



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

Monitor System Configuration

Device Model :	Oscar2 M250	Serial Number :	00168743
Firmware Version BP :	O22731	Firmware Version CBP :	CBPERR
Firmware Version UI :	UI3612	AccuWin Pro™ 4 Version :	4.0.4.230
Start Study in 5 Min :	OFF	Max Pressure :	220
Intervals :	Fixed	Minimum time between readings :	1
Retry Attempts :	ON	Manual Readings :	OFF
Brachial BP Only :	OFF	Selected Measurement	Brachial
Audible Alerts :	ON	Button Configuration	OFF
Display Results :	OFF	Day / Night button :	OFF

Number of time periods : 2

#	Start Time	End Time	Brachial BP Interval (min)
1	07:00	23:00	30
2	23:00	07:00	60

Dose response sequences (configured) :

#	Name	Time	Duration	Samples

Quality Control

QC Review Period Start :	QC Review Period End :
Scheduled Readings Captured :	Readings Captured Per Hour :
Hours Containing Readings :	

Error Code Definitions (EC)

1 = No signal	93 =
2 = Artifact/Erratic signal	94 = Low battery
3 = Retries exceeded	95 = Mosfet failure
4 = Time limit exceeded	96 = Calibration error
5 = Out of range	97 = Transducer failed
6 = BP not allowed	98 = ADC failure
7 = Reading unusable	99 = CRC failure
50 = BP not allowed	100 = Study event marker
85 = Blocked valve	101 =
86 = User abort	102 =
87 = Air leak	103 =
88 = Safety timeout	104 =
89 = Cuff overpressure	105 = Start Study
90 = Low batteries	106 = Monitor turned off
91 = Auto-zero failed	107 = Study End



Ambulatory Blood Pressure Report

Patient Name : Almustafa Qusai

Date of Birth : 7/3/2000

Gender : Male

Patient ID : 00168743

Study Reference : Test

Test Date: 7/8/2024

92 = BP comm error

See Operations Manual for AccuWin Pro™ 4 for further details on code description