PARTICLEMETRIX
www.particle-metrix.de

Electrophoresis & Brownian Motion Video Analysis Laser Scattering Microscopy

Operator (Report): sop_kabanovlab.inst

Video Operator: sop_kabanovlab.inst

Sample Parameters

Sample Name: G104_F1
Comment: Sens=80, Sample Remarks0:
Sample Remarks1:
Sample Remarks2:
Electrolyte:
Temperature: 24.64 °C sensed
pH 7.0 entered
Conductivity: 9241.01 µS/cm sensed

Instrument Parameters

Laser Wavelength: 488 nm
Filter Wavelength: Scatter

Measurement Parameters

Cell S/N: ZNTA

Measurement Mode: Size Distribution 2 Cycles

11 Positions, 3 Removed for Analysis

Result (sizes in nm)

	Number	Concentration	Volume
Median (X50)	174.9	174.9	283.6
Span	80.0	79.9	116.6

Concentration: 4.3E+7 Particles / mL
Dilution Factor: 200
Original Concentration: 8.6E+9 Particles / mL

Quality

Average Counted Particles per Frame: 94
Number of Traced Particles: 745

Analysis Parameters

Max Area: 1000, Min Area: 10, Min Brightness: 20

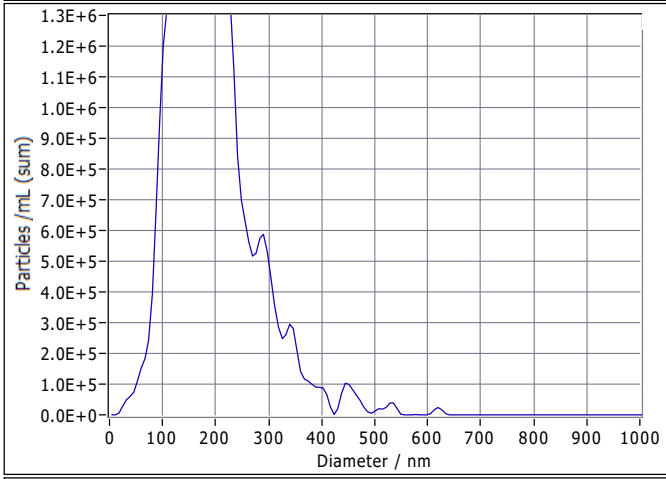

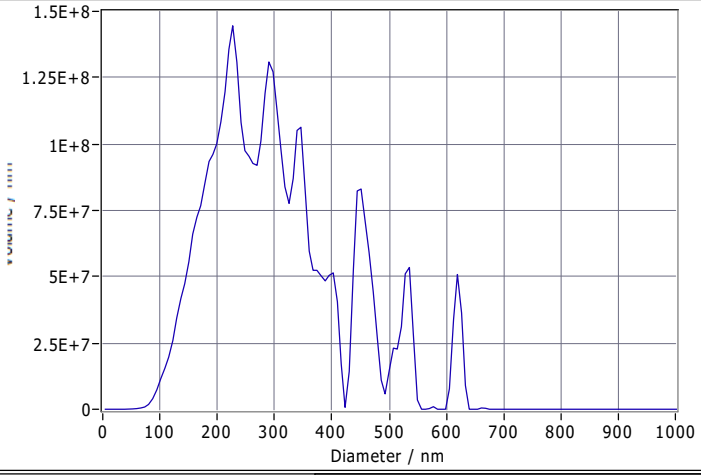

Peak Analysis (Concentration)

Diameter / nm	Particles/mL	FWHM / nm	Percentage
150.3	1.8E+6	145.5	85.6
284.8	5.8E+5	41.2	14.4

X Values (all sizes are given in nm)

	Number	Concentration	Volume
X10	102.7	102.7	168.0
X50	174.9	174.9	283.6
X90	292.9	293.0	463.2
Span	1.1	1.1	1.0
Mean	191.8	191.8	305.3
StdDev	80.0	79.9	116.6

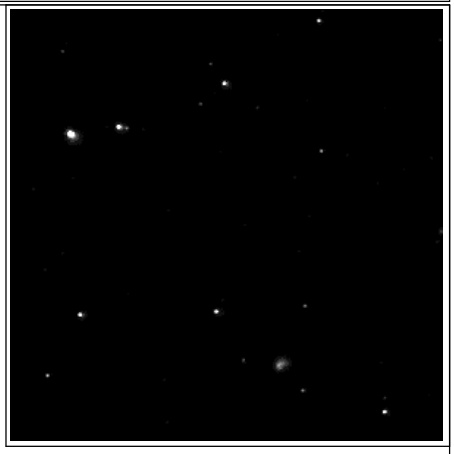

Comment

(Signature)

Analyzed Video: C:\Zetaview Data\Nancy\2023_02_14\20230214_0002_G104_F1_size_488.avi

ZetaVIEW S/N 19-490, Software ZetaView (version 8.05.12 SP2), Camera 0.713 mum/px

Experiment: 2023-02-14 14:47, Report: 2023-02-14 14:50